



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100400

Report Issue Date: 04/25/2024
Date Received: 2024-02-21
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG217902	0.019	0.019	0.019	0.019	0.019	0.019
0.080	0.078	AG310901	0.076	0.076	0.075	0.075	0.076	0.076
0.300	0.293	AG327804	0.288	0.287	0.287	0.288	0.288	0.288

As Found - Evaluation Analyst: Carlie Glaister
 As Found Conditions - Barometric Pressure (inHg): 29.49 Barometer Used: Fisher S/N 230307229 Temperature (C): 22.1 Relative Humidity (%): 17
 As-Found Lab Activity Date Range: 02/22/2024 - 02/22/2024

Replaced o-ring.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.019	0.020	0.020	0.019	0.019	0.019	+/- 0.002
0.040	0.040	AG217904	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.079	AG310901	0.076	0.076	0.076	0.076	0.077	0.076	+/- 0.004
0.100	0.099	AG333401	0.098	0.098	0.097	0.097	0.097	0.097	+/- 0.004
0.150	0.148	AG332004	0.143	0.144	0.144	0.144	0.144	0.144	+/- 0.005
0.300	0.297	AG327804	0.292	0.291	0.292	0.292	0.292	0.292	+/- 0.011

As Left Conditions - Barometric Pressure (inHg): 29.60 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.1 Relative Humidity (%): 25
 As-Left Lab Activity Date Range: 03/28/2024 - 03/29/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Carlie Glaister on 03/29/2024

carlie.glaister@alaska.gov

Technically and administratively reviewed by Brandi Barnett on 04/25/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100400 Analyst or Technician Name: Kaija Swisher
DataMaster DMT Calibration Start Date: 3/28/24 Supervised by Carla Glaister

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: 5/2/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.60 Temperature(C) 20.1 Relative Humidity(%) 25
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20290214C03 Expiration Date: 5/14/24
Simulator S/N: SD1088 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240214C03 Expiration Date: 5/14/24
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 224P41201 Expiration Date: 8/24/24
Simulator S/N: SD177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 9/19/2025

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 3/28/24
Data Interpretation Date (Technician): 3/29/24 KS (if applicable)
Data Interpretation Date (Analyst): supervised by CKG 3/29/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100400

Date: 03/28/2024
Time: 08:59:25

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.69 V PASSED
(1.00 V - 2.32 V)
Cooler Voltage = 1.67 V PASSED
(1.00 V - 2.34 V)
Bias Voltage = 79 V PASSED
(47 V - 111 V)
Chopper Freq = 526 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.7 in

PUMP INFO

Flow Rate = 4.965 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.108 1.07% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100400

Date: 03/28/2024
Time: 9:18 AM

Temperatures (°C)
Sample Cell: 49.2°C
Breath Tube: 47.4°C

Current Barometer 29.6 in
Volume (Ltr) 1.49

Settings
Lamp: 1.74 V
Bias: 79 V
Cooler: 1.72 V
Chopper: 518 Hz

Voltages (V)
Flow: 1.05 V
Detector: -0.055 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100400

Date: 12/16/2019
Time: 10:36:49

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca = 0.1000
CAL = 0.968246 0.800 <= CAL < 1.200
b1 = 0.0003 0.0000 <= b1 < 0.0040
b2 = 0.0047 0.0010 <= b2 < 0.0100
b3 = 0.0002 0.0000 <= b3 < 0.0040
Xq = 0.1066 0.0500 <= Xq < 0.2000
a21 = 1.177357 1.050 <= a21 < 1.300
a31 = 0.464721 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100400

Date: 03/28/2024

Time: 09:32:17

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.60: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	09:33
BLANK TEST	0.000
INTERNAL STANDARD	0.076
EXTERNAL STANDARD	0.000
BLANK TEST	0.000
SUBJECT SAMPLE (Vol=1.56L)	0.000
BLANK TEST	0.000
EXTERNAL STANDARD	0.077
BLANK TEST	0.000

Alcohol (g/210L)
Flow Rate (L/M)
Min. Flow Rate (L/M)

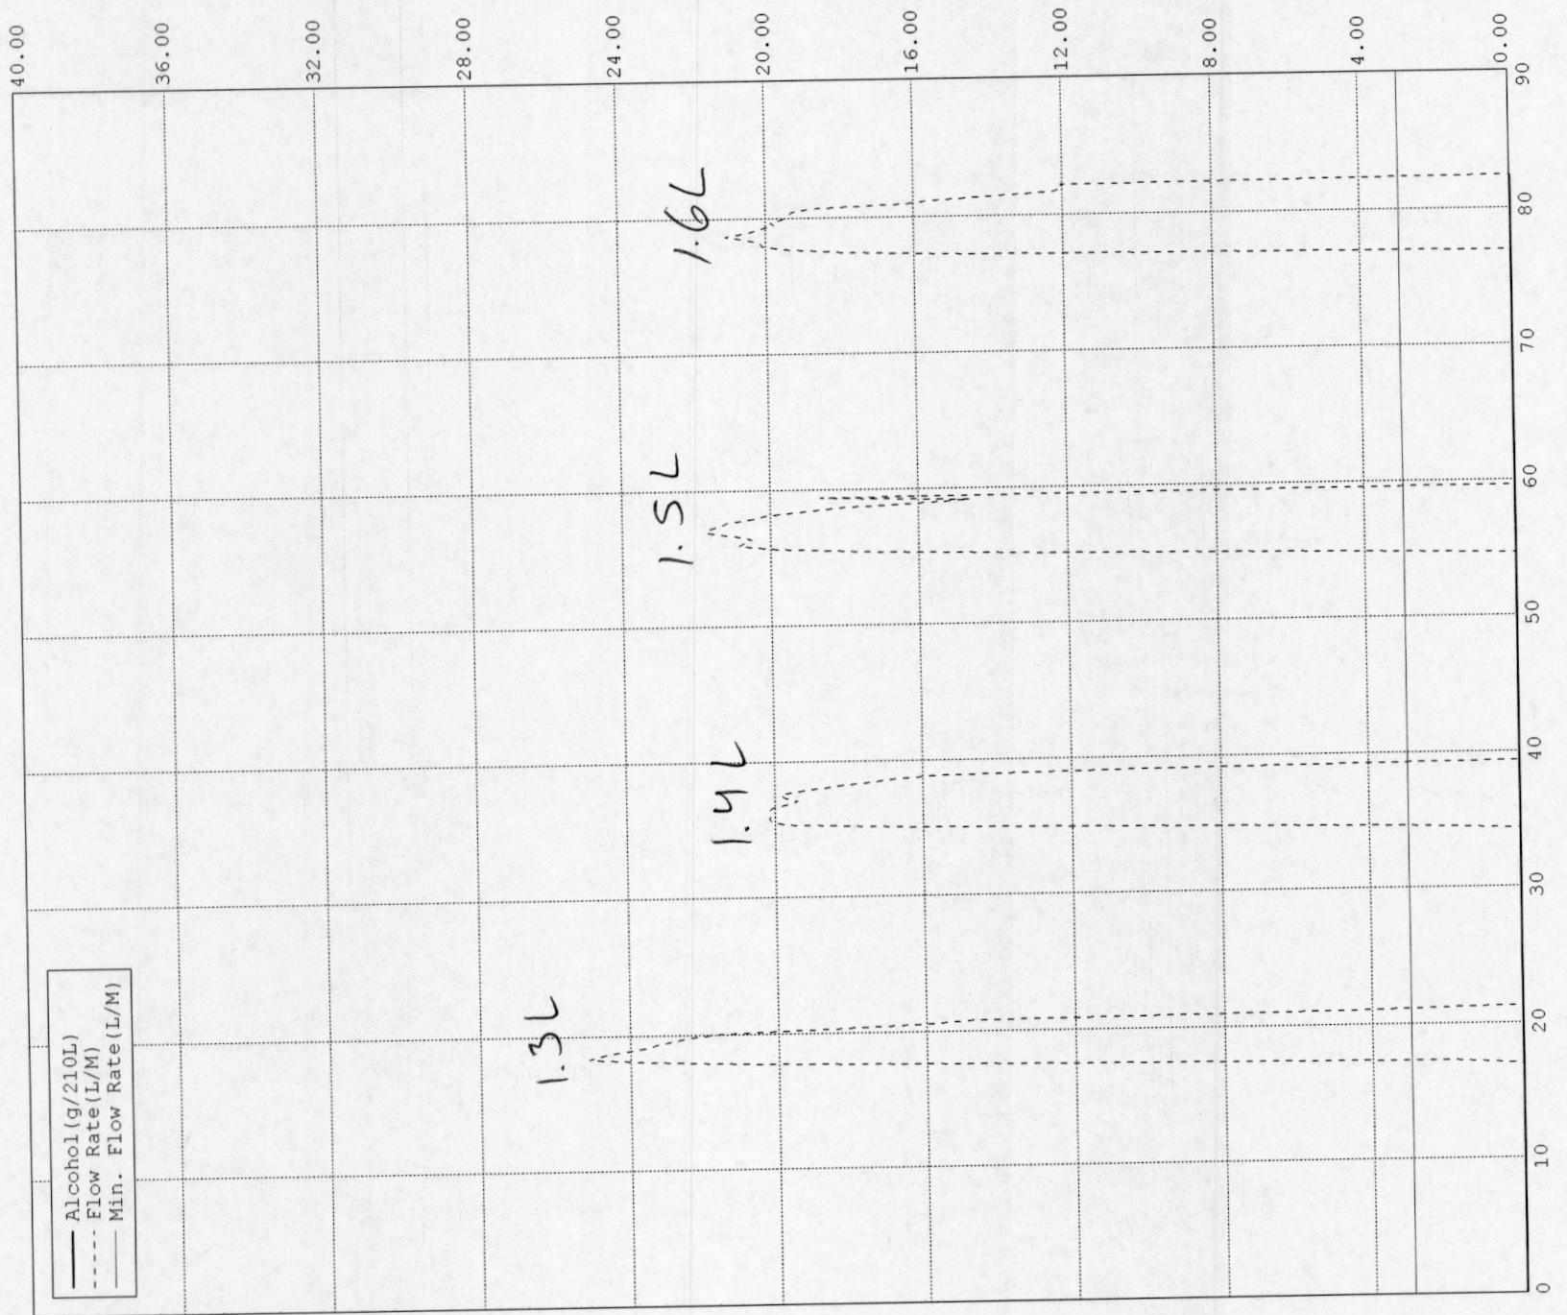

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100400

Date: 03/28/2024
 Time: 09:46:32

SUPERVISOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.020	0.0194	0.0005
0.040	0.0390	0.0000
0.079	0.0762	0.0004
0.099	0.0974	0.0005
0.148	0.1438	0.0004
0.297	0.2918	0.0004

SLOPE = 0.983245
 R² = 0.999943

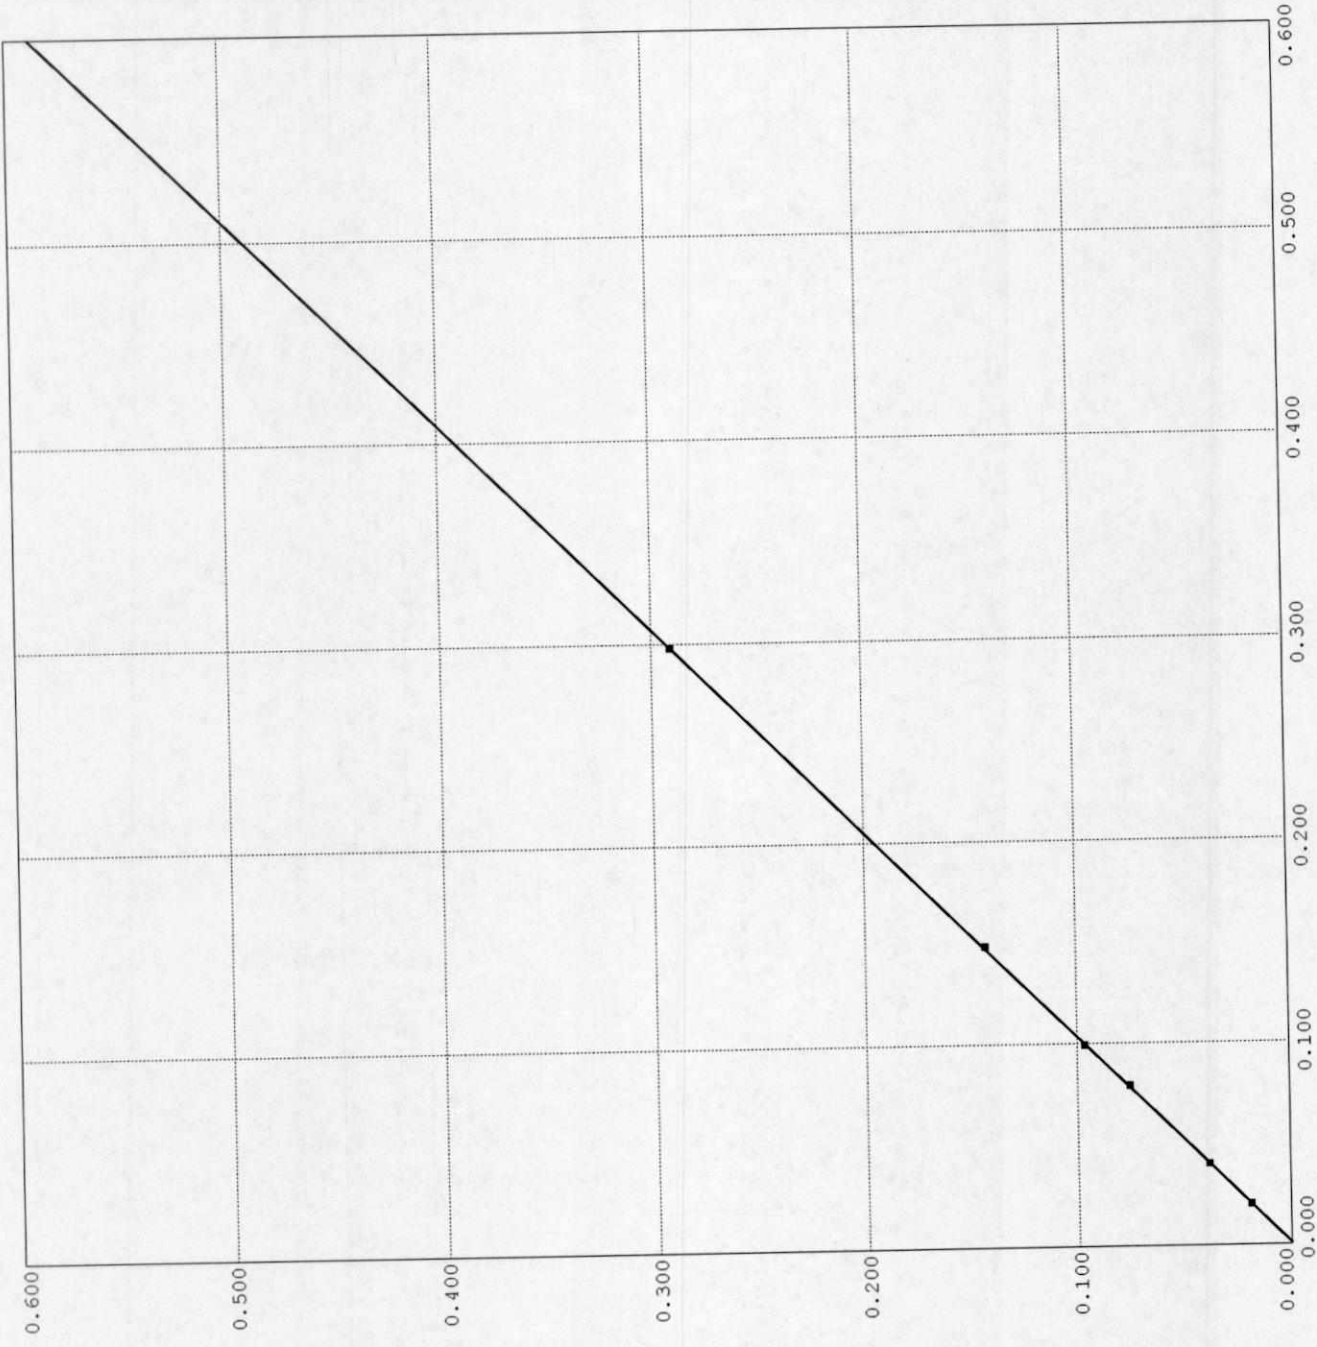

KS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100400






Date: 03/28/2024
 Time: 09:46:35

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.61: 0.020
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 206 psi

BLANK TEST	0.000	09:48
INTERNAL STANDARD	VERIFIED	09:48
EXTERNAL STANDARD	0.019	09:48
BLANK TEST	0.000	09:49
EXTERNAL STANDARD	0.020	09:49
BLANK TEST	0.000	09:50
EXTERNAL STANDARD	0.020	09:50
BLANK TEST	0.000	09:51
EXTERNAL STANDARD	0.019	09:51
BLANK TEST	0.000	09:52
EXTERNAL STANDARD	0.019	09:52
BLANK TEST	0.000	09:53

Average = 0.0194
 Std Dev = 0.0005

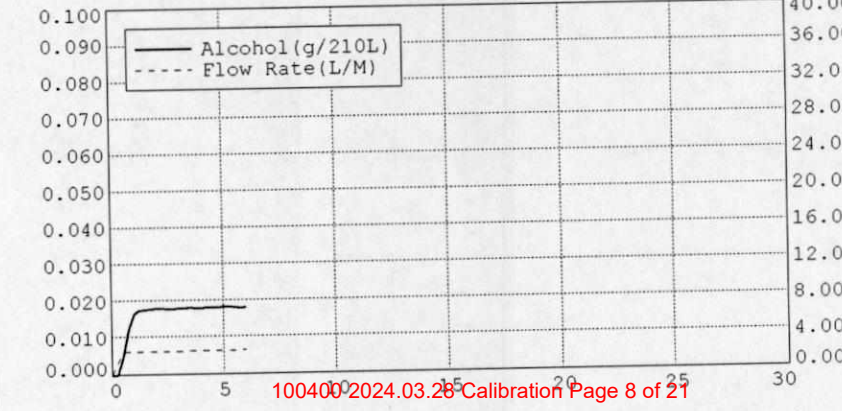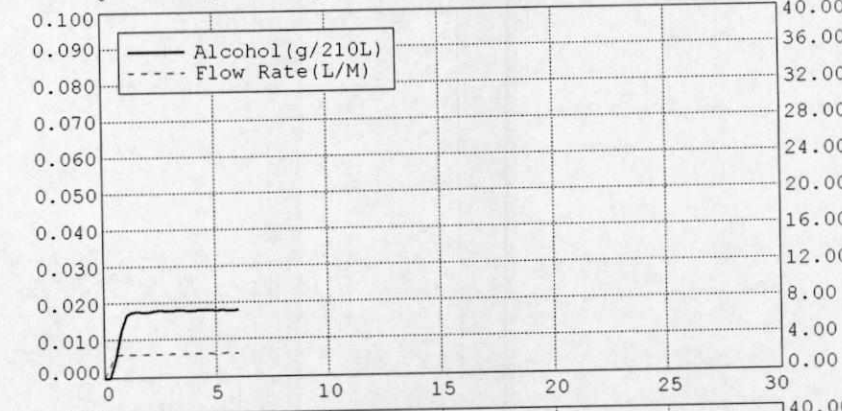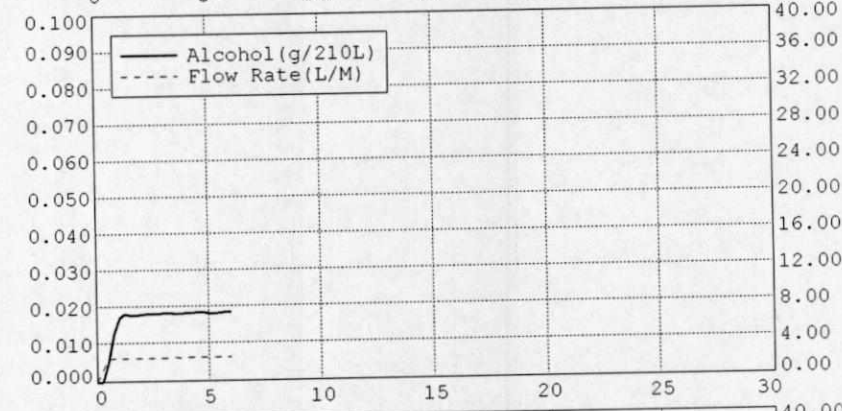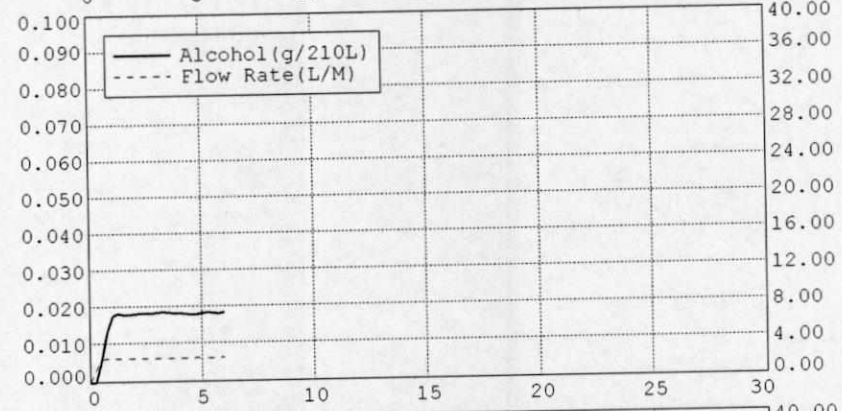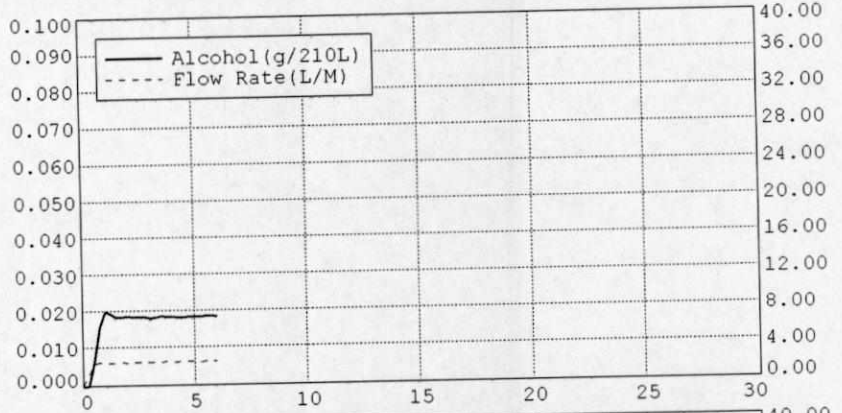

LINEARITY CHECK: Control Test 2






Alaska Department of Public Safety
 DATAMASTER dmt: 100400

Date: 03/28/2024
 Time: 09:54:51

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.040
 TARGET AT 29.61: 0.040
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 756 psi

BLANK TEST	0.000	09:55
INTERNAL STANDARD	VERIFIED	09:56
EXTERNAL STANDARD	0.039	09:56
BLANK TEST	0.000	09:57
EXTERNAL STANDARD	0.039	09:57
BLANK TEST	0.000	09:58
EXTERNAL STANDARD	0.039	09:58
BLANK TEST	0.000	09:59
EXTERNAL STANDARD	0.039	09:59
BLANK TEST	0.000	10:00
EXTERNAL STANDARD	0.039	10:00
BLANK TEST	0.000	10:01

Average = 0.0390
 Std Dev = 0.0000

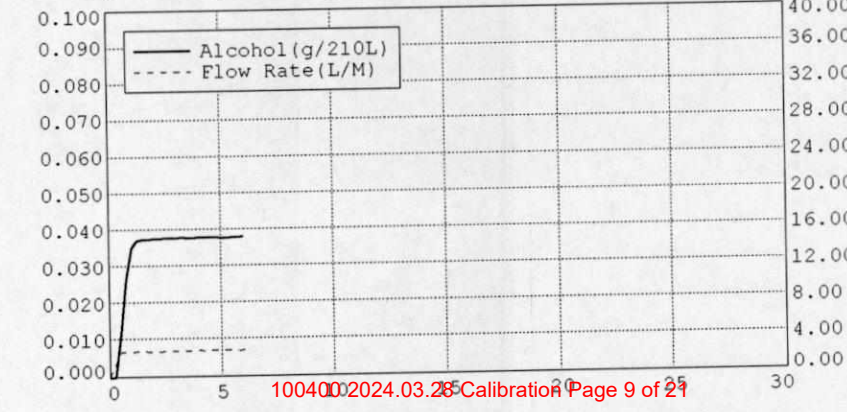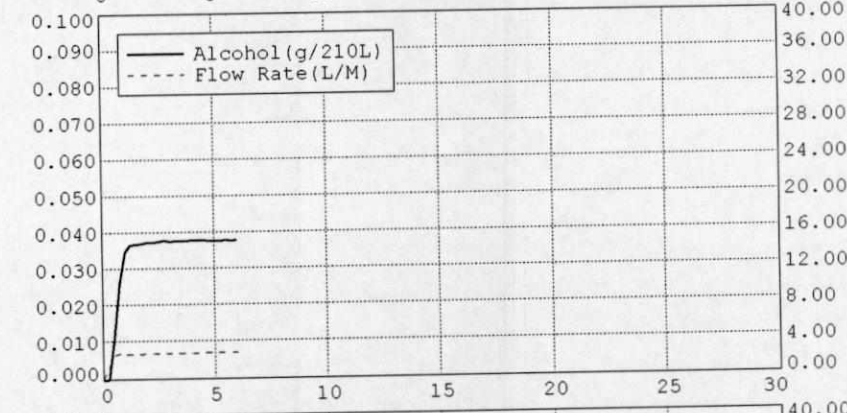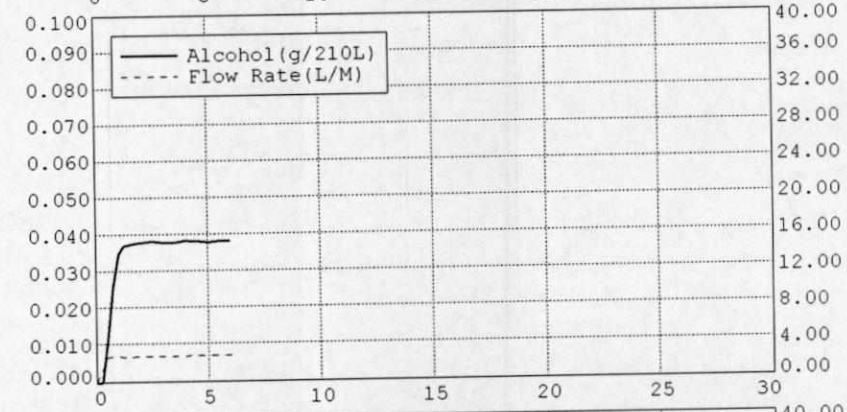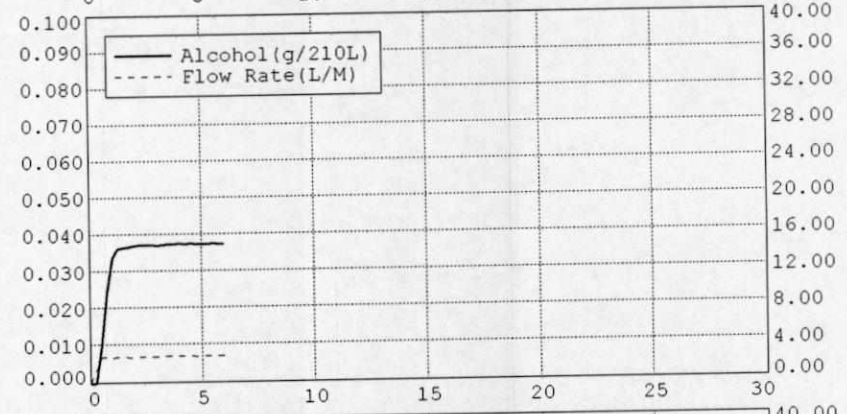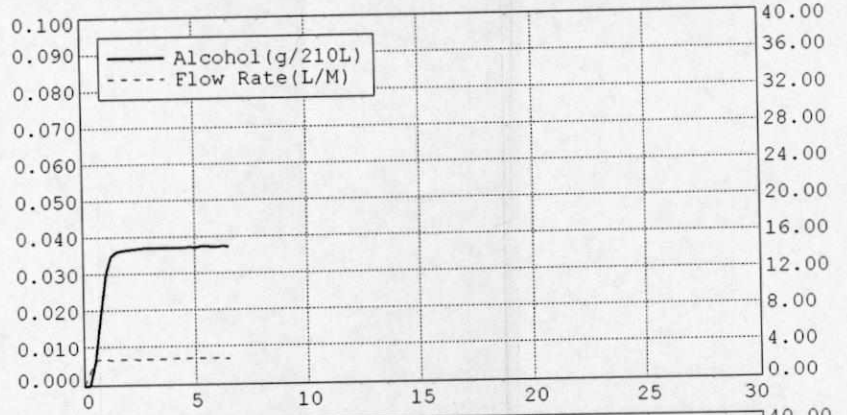

LINEARITY CHECK: Control Test 3






Alaska Department of Public Safety
 DATAMASTER dmt: 100400

Date: 03/28/2024
 Time: 10:03:05

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.61: 0.079
 LOT #: AG310901
 EXPIRATION: 04/19/2025
 TANK PRESSURE: 220 psi

BLANK TEST	0.000	10:04
INTERNAL STANDARD	VERIFIED	10:04
EXTERNAL STANDARD	0.076	10:04
BLANK TEST	0.000	10:05
EXTERNAL STANDARD	0.076	10:05
BLANK TEST	0.000	10:06
EXTERNAL STANDARD	0.076	10:06
BLANK TEST	0.000	10:07
EXTERNAL STANDARD	0.076	10:07
BLANK TEST	0.000	10:08
EXTERNAL STANDARD	0.077	10:08
BLANK TEST	0.000	10:09

Average = 0.0762
 Std Dev = 0.0004

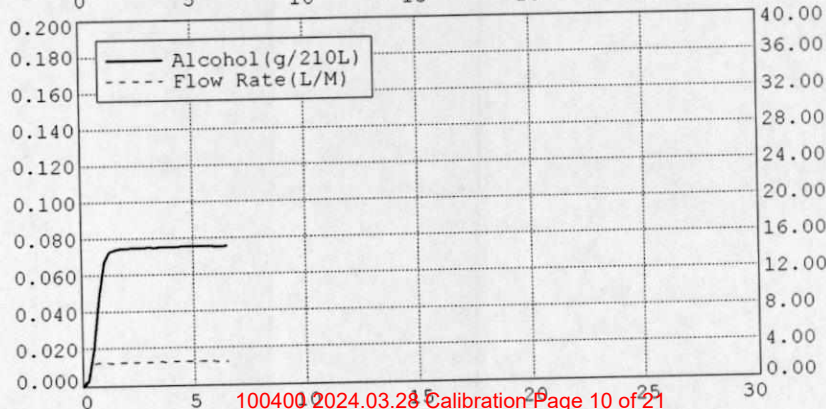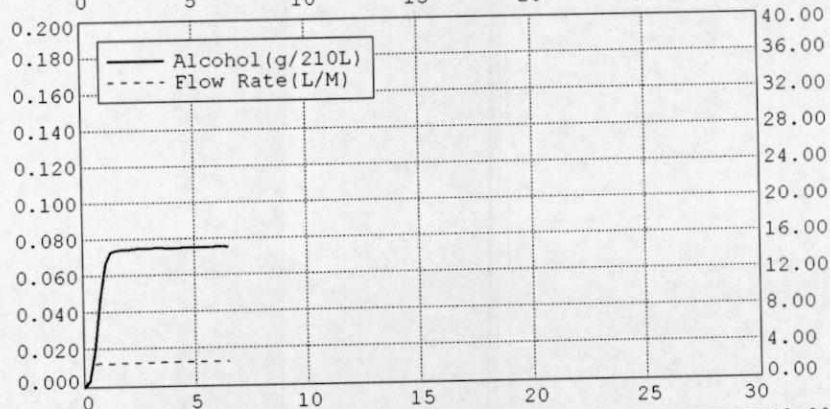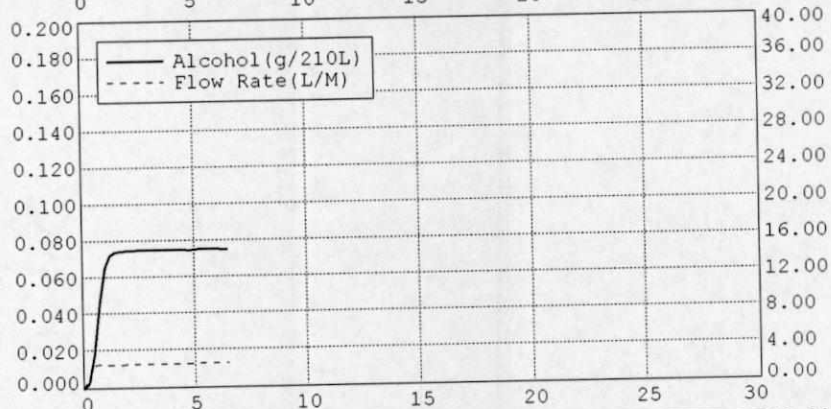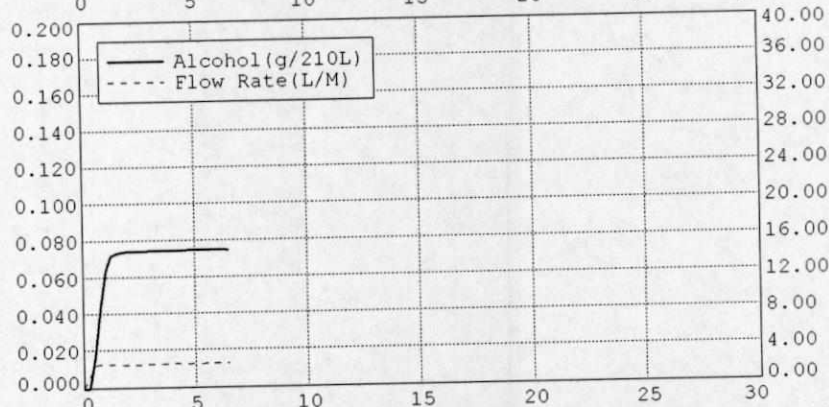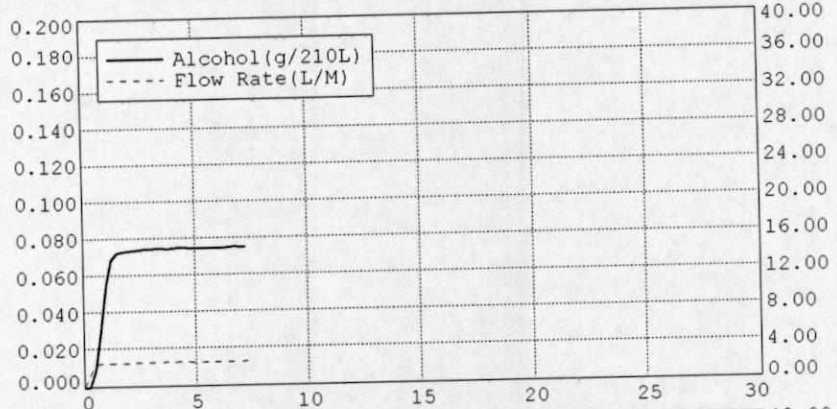

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100400






Date: 03/28/2024
 Time: 10:11:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.62: 0.099
 LOT #: AG333401
 EXPIRATION: 11/30/2025
 TANK PRESSURE: 1131 psi

BLANK TEST	0.000	10:12
INTERNAL STANDARD	VERIFIED	10:12
EXTERNAL STANDARD	0.098	10:13
BLANK TEST	0.000	10:14
EXTERNAL STANDARD	0.098	10:14
BLANK TEST	0.000	10:15
EXTERNAL STANDARD	0.097	10:15
BLANK TEST	0.000	10:16
EXTERNAL STANDARD	0.097	10:16
BLANK TEST	0.000	10:17
EXTERNAL STANDARD	0.097	10:17
BLANK TEST	0.000	10:18

Average = 0.0974
 Std Dev = 0.0005

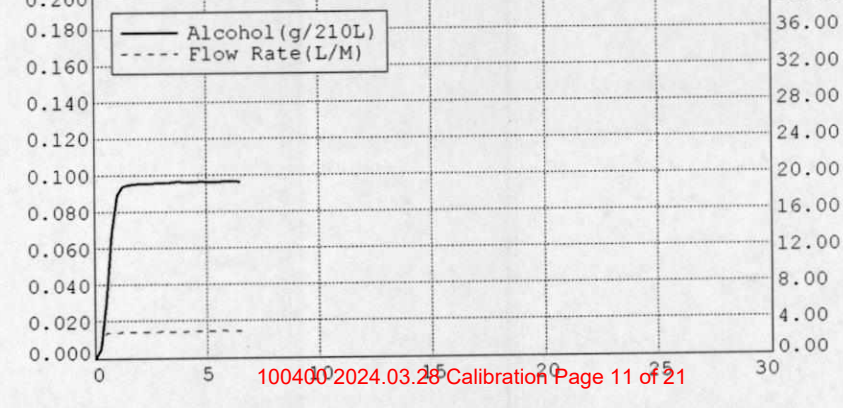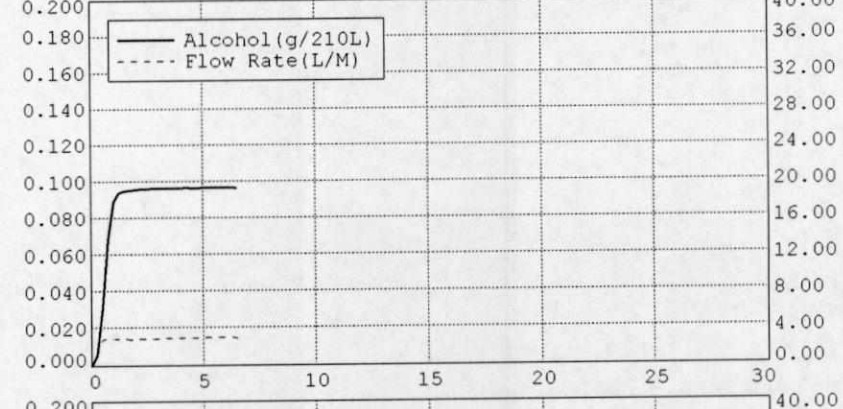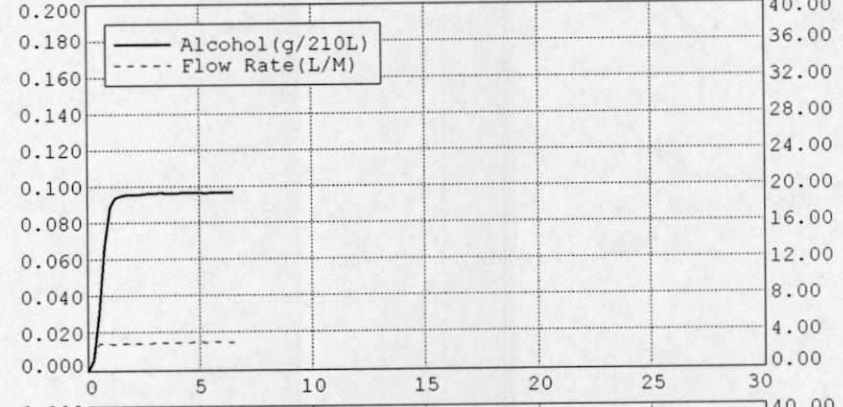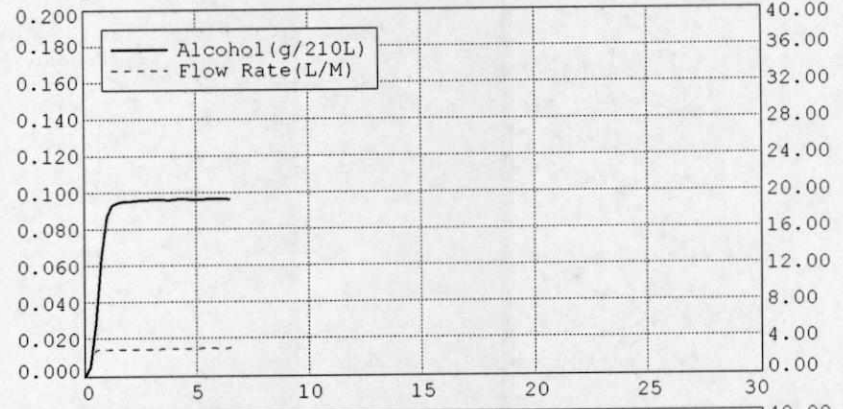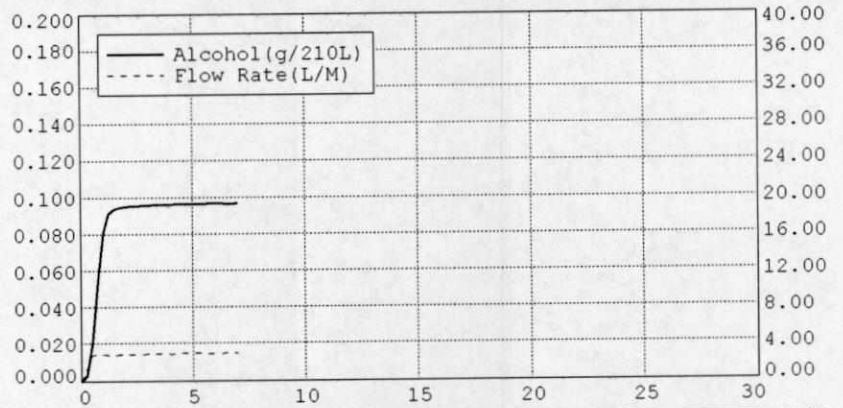

LINEARITY CHECK: Control Test 5






Alaska Department of Public Safety
 DATAMASTER dmt: 100400

Date: 03/28/2024
 Time: 10:23:07

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.150
 TARGET AT 29.61: 0.148
 LOT #: AG332004
 EXPIRATION: 11/16/2025
 TANK PRESSURE: 666 psi

BLANK TEST	0.000	10:24
INTERNAL STANDARD	VERIFIED	10:24
EXTERNAL STANDARD	0.143	10:24
BLANK TEST	0.000	10:25
EXTERNAL STANDARD	0.144	10:25
BLANK TEST	0.000	10:26
EXTERNAL STANDARD	0.144	10:26
BLANK TEST	0.000	10:27
EXTERNAL STANDARD	0.144	10:28
BLANK TEST	0.000	10:28
EXTERNAL STANDARD	0.144	10:29
BLANK TEST	0.000	10:30

Average = 0.1438
 Std Dev = 0.0004

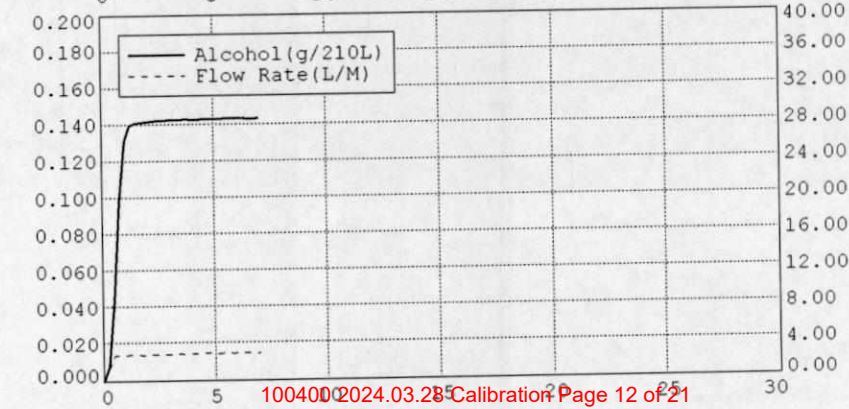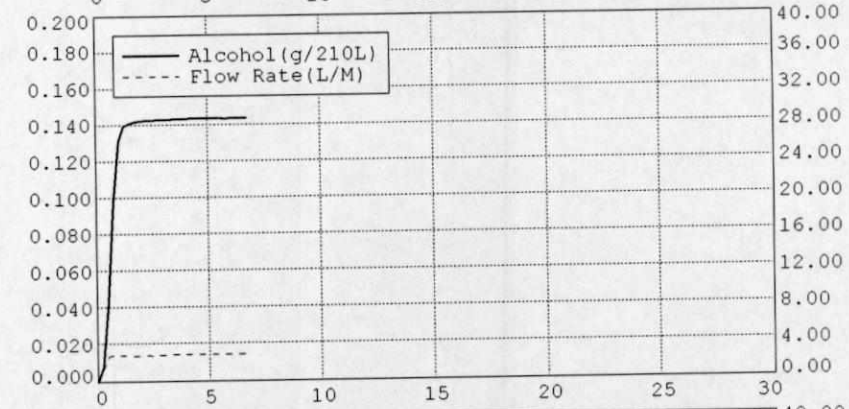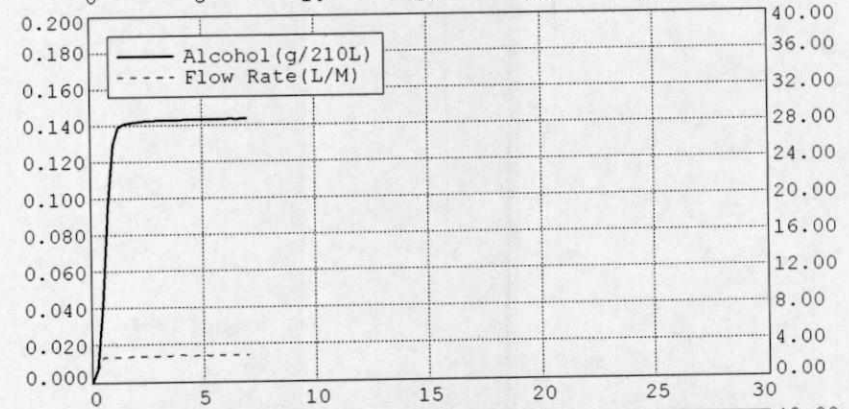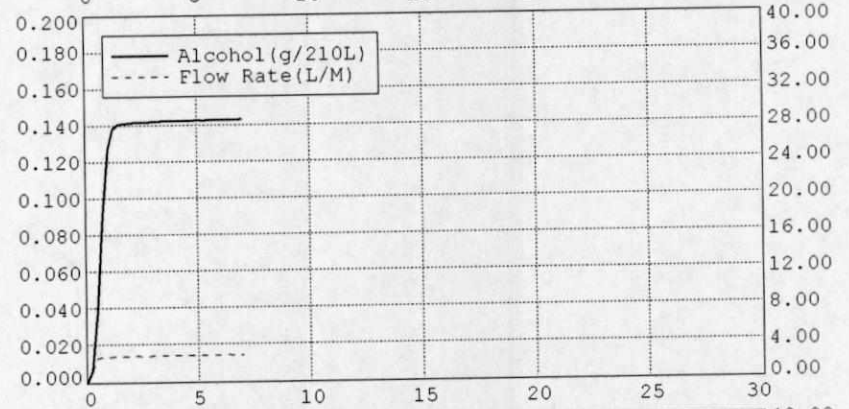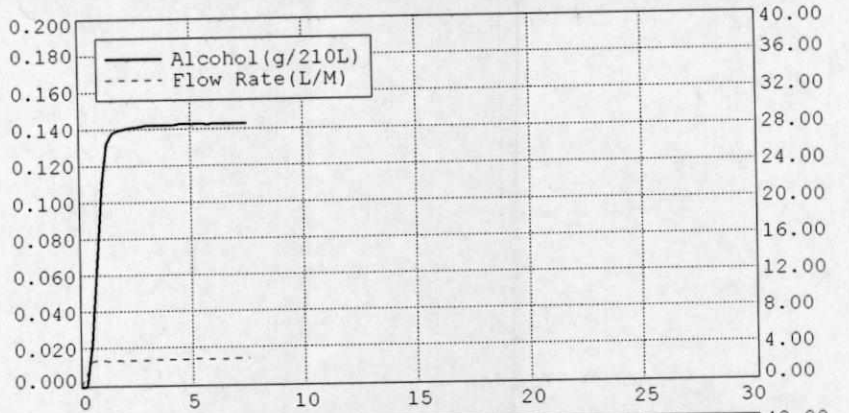

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100400






Date: 03/28/2024
 Time: 10:30:42

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.61: 0.297
 LOT #: AG327804
 EXPIRATION: 10/05/2025
 TANK PRESSURE: 261 psi

BLANK TEST	0.000	10:32
INTERNAL STANDARD	VERIFIED	10:32
EXTERNAL STANDARD	0.292	10:32
BLANK TEST	0.000	10:33
EXTERNAL STANDARD	0.291	10:33
BLANK TEST	0.000	10:34
EXTERNAL STANDARD	0.292	10:34
BLANK TEST	0.000	10:35
EXTERNAL STANDARD	0.292	10:35
BLANK TEST	0.000	10:36
EXTERNAL STANDARD	0.292	10:37
BLANK TEST	0.000	10:38

Average = 0.2918
 Std Dev = 0.0004

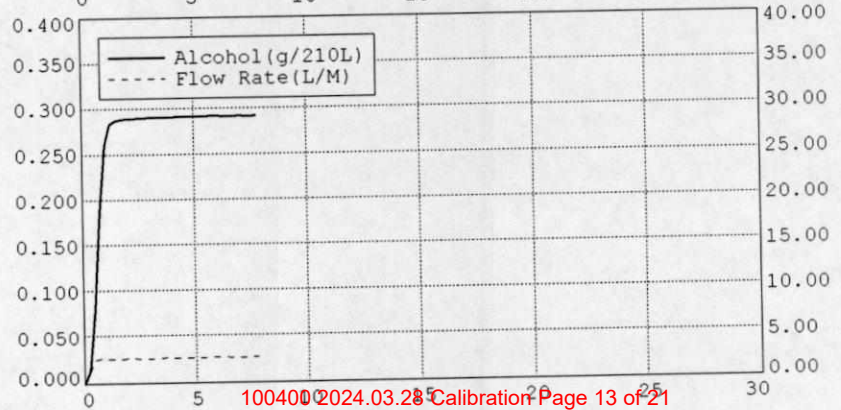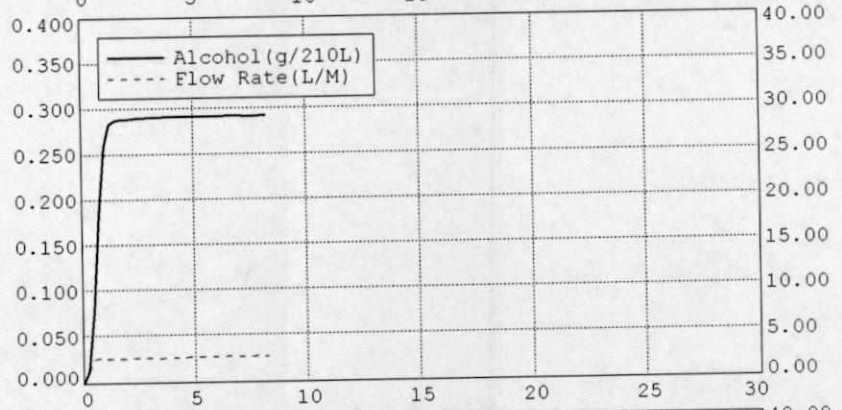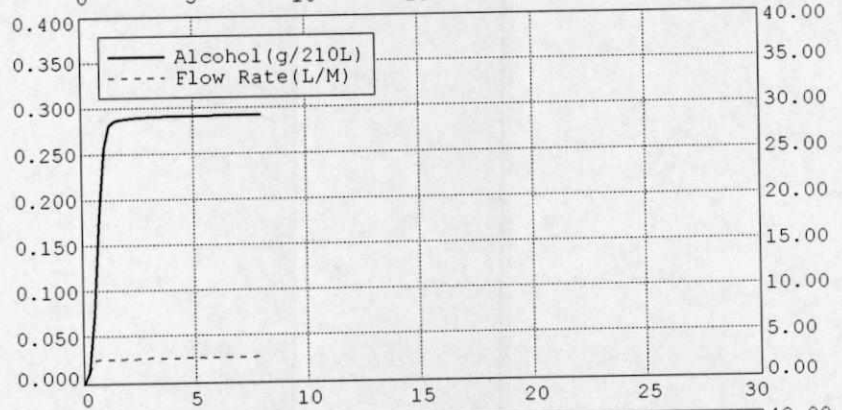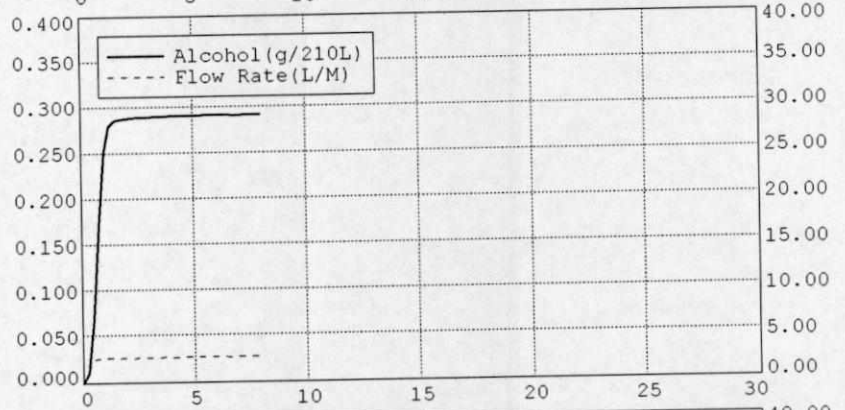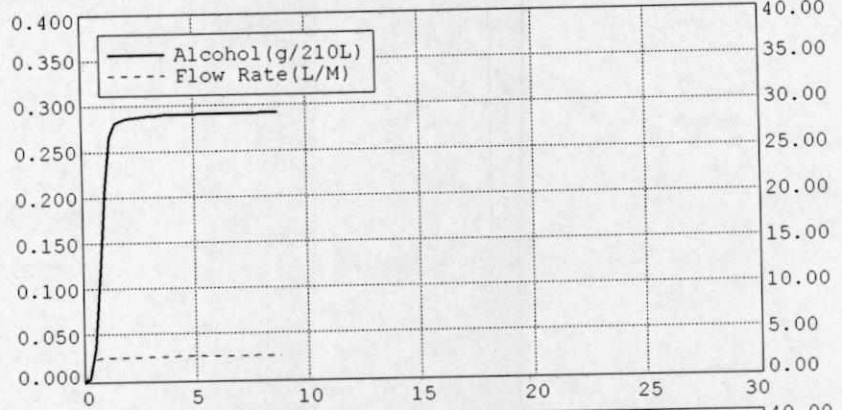

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100400

Date: 03/28/2024

Time: 10:44:57

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

INCOMPLETE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.62: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

PASSED 10:46

BLANK TEST

0.000 10:46

INTERNAL STANDARD

VERIFIED 10:46

0.076 10:46

BLANK TEST

0.000 10:47

SUBJECT SAMPLE

INCOMPLETE 10:49



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100400

Date: 03/28/2024
Time: 10:52:18

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
MAX ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.61: 0.079
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	10:53
BLANK TEST	0.000	10:53
INTERNAL STANDARD	VERIFIED	10:53
EXTERNAL STANDARD	0.077	10:53
BLANK TEST	0.000	10:54
SUBJECT SAMPLE	XXX	10:55

Maximum Attempts Exceeded

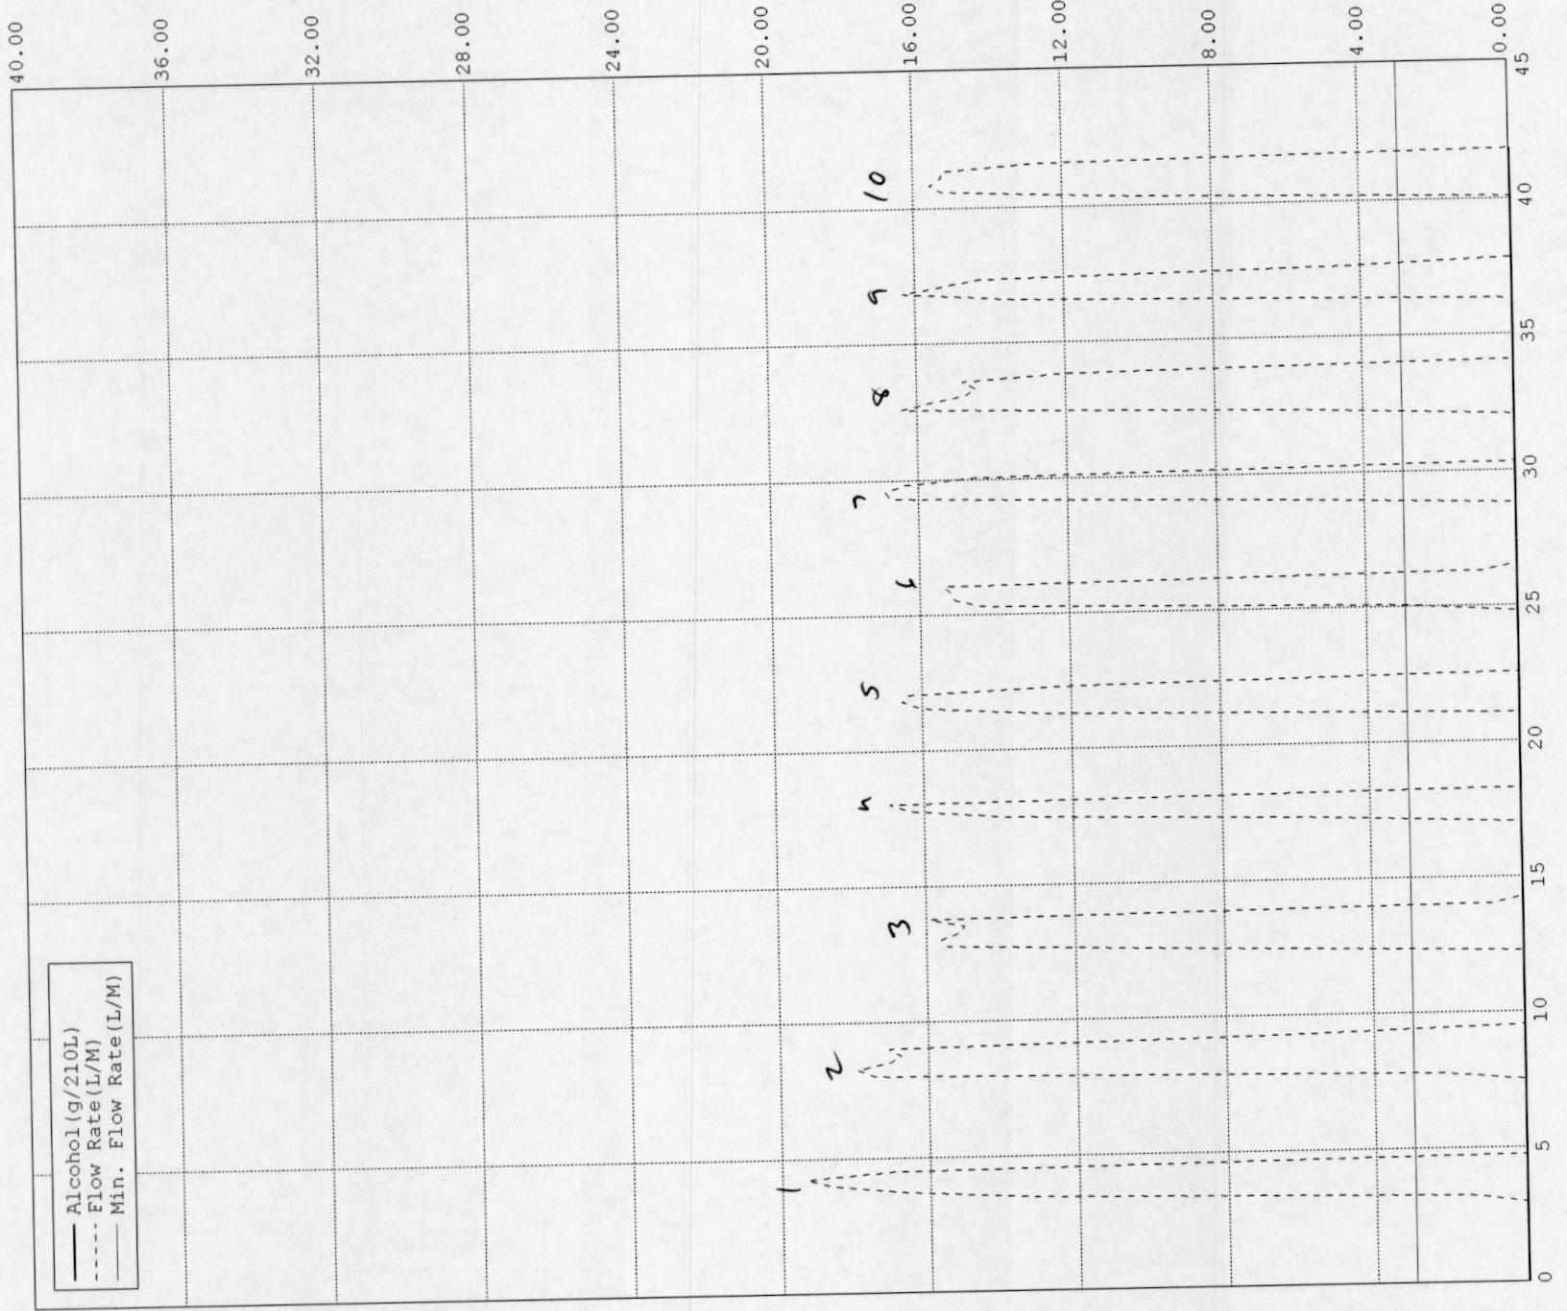

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100400

Date: 03/28/2024

Time: 11:11:27

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

INVALID

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.62: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 11:13
0.000 11:13
VERIFIED 11:13
0.077 11:13
0.000 11:14
INVALID 11:14

Alcohol (g/210L)
Flow Rate (L/M)
Min. Flow Rate (L/M)

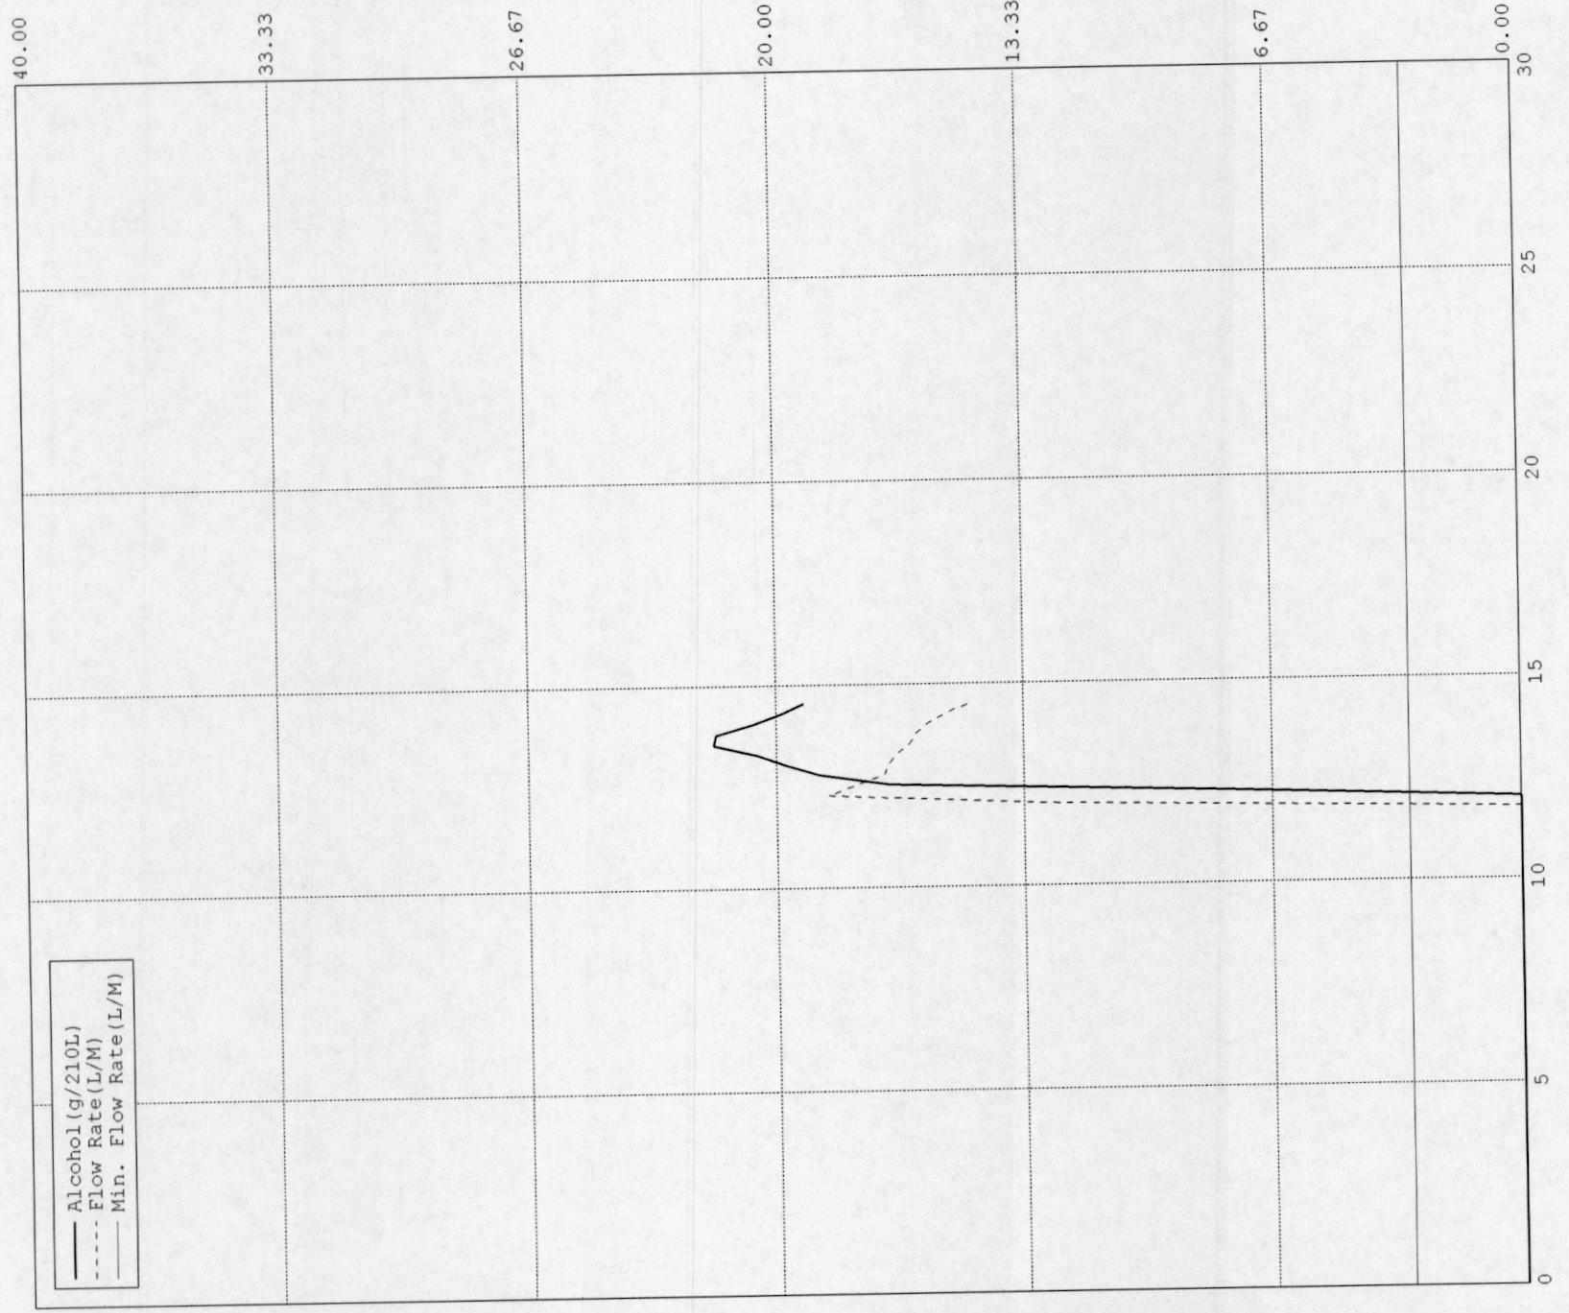

SUBJECT TEST

 Alaska Department of Public Safety
 DATAMASTER dmt: 100400

Date: 03/28/2024
 Time: 11:16:53

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

DEPT/AGENCY:
 RFI
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.63: 0.079
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	11:17
BLANK TEST	0.000	11:18
INTERNAL STANDARD	VERIFIED	11:18
EXTERNAL STANDARD	0.076	11:18
BLANK TEST	0.000	11:19

RFI DETECTED



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100400

Date: 03/28/2024

Time: 13:29:14

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

INTERFERENCE ACETONE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.63: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	13:30
BLANK TEST	0.000	13:30
INTERNAL STANDARD	VERIFIED	13:30
Xq = 0.108 (1.07%)		
EXTERNAL STANDARD	0.077	13:30
X[1] = 0.0766 (-0.0009)	(0.0027)	
BLANK TEST	0.000	13:31
SUBJECT SAMPLE	XXX	13:32
X[1] = 0.1050 (-0.0191)	(0.0006)	

Interference Detected

Filter 2 average = -6.0010

Filter 3 average = 0.0623

ics 3/29/24

QMB 3/29/24



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100400

Date: 03/28/2024
Time: 13:19:49

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.63: 0.079
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 13:21
BLANK TEST 0.000 13:21
INTERNAL STANDARD VERIFIED 13:21
Xq = 0.107 (0.58%) 0.076 13:21
EXTERNAL STANDARD X[1] = 0.0764 (-0.0010) (0.0026)
BLANK TEST 0.000 13:22
SUBJECT SAMPLE XXX 13:23
X[1] = 0.1171 (-0.0256) (0.0016)

Interference Detected

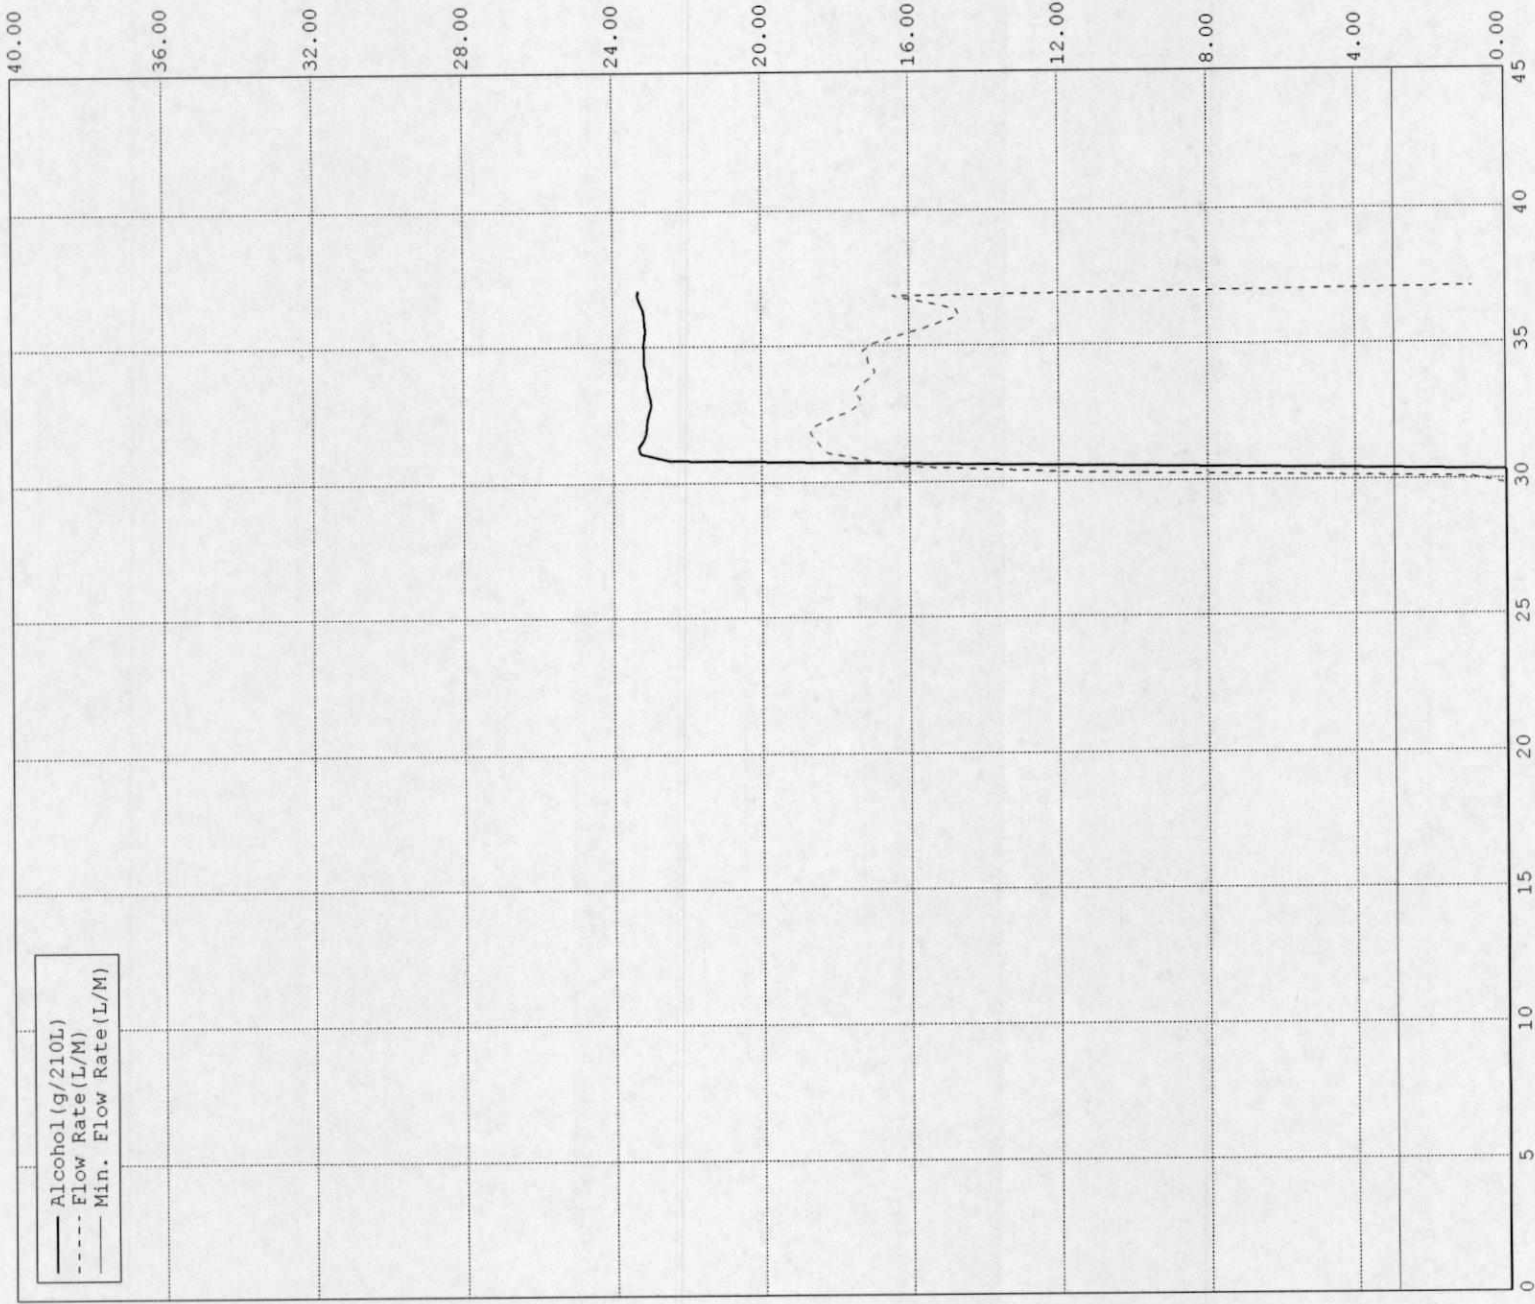

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100400

Date: 03/28/2024
 Time: 13:35:03

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

DEPT/AGENCY:
 INTERFERENCE NEGATIVE
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.63: 0.079
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	13:36
BLANK TEST	0.000	13:36
INTERNAL STANDARD	VERIFIED	13:36
EXTERNAL STANDARD	0.077	13:36
$X_q = 0.108$ (0.91%)	$X[1] = 0.0769$ (-0.0007)	(0.0023)
BLANK TEST	0.000	13:37
SUBJECT SAMPLE (Vol=1.93L)	0.093	13:37
$X[1] = 0.0936$ (-0.0006)	(0.0008)	
BLANK TEST	0.000	13:38
EXTERNAL STANDARD	0.076	13:39
$X[1] = 0.0763$ (-0.0013)	(0.0017)	
BLANK TEST	0.000	13:40



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100400

Date: 03/28/2024
Time: 14:00:19

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.63: 0.079
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:01
BLANK TEST	0.000	14:01
INTERNAL STANDARD	VERIFIED	14:01
EXTERNAL STANDARD	0.077	14:01
BLANK TEST	0.000	14:02
SUBJECT SAMPLE (Vol=2.63L)	0.000	14:03
BLANK TEST	0.000	14:03
EXTERNAL STANDARD	0.077	14:04
BLANK TEST	0.000	14:05

KS

