

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument
State of Alaska

Serial #: 100669

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 02/24/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.33: 0.081
LOT #: 11313080A1
EXPIRATION: 06/01/2015
TANK PRESSURE: 777 psi

BLANK TEST	0.000	09:12
INTERNAL STANDARD	VERIFIED	09:12
EXTERNAL STANDARD	0.078	09:13
BLANK TEST	0.000	09:14
EXTERNAL STANDARD	0.078	09:14
BLANK TEST	0.000	09:15
EXTERNAL STANDARD	0.078	09:15
BLANK TEST	0.000	09:16
EXTERNAL STANDARD	0.078	09:16
BLANK TEST	0.000	09:17
EXTERNAL STANDARD	0.078	09:17
BLANK TEST	0.000	09:18

Average = 0.0780
Std Dev = 0.0000

Diagnostic Check

VERSIONS

DMT: 3.00
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
Breath Tube = 47.1°C PASSED

PUMP INFO

Flow Rate = 4.628 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO


Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

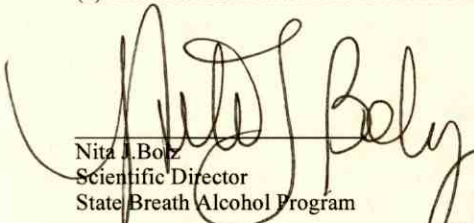
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

3/13/2015

Subscribed and sworn before me this 13th day of Mar., 2015


Nikki Roth, Notary Public
My Commission Expires With Office

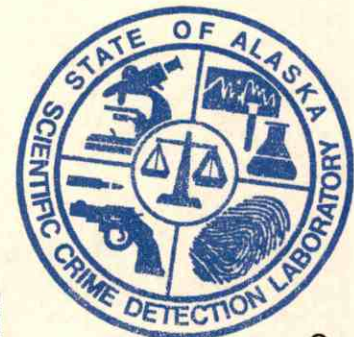

BMB
3/2/15