



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100361

**Report Issue Date:** 09/04/2024  
**Date Received:** 2024-07-26  
**Condition of Item:** Damaged

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG408002	0.020	0.020	0.020	0.019	0.019	0.020	
0.080	0.079	AG335202	0.079	0.078	0.078	0.078	0.078	0.078	
0.300	0.297	AG327804	0.296	0.295	0.296	0.296	0.295	0.296	

As Found - Evaluation Analyst: Colleen O'Bryant  
 As Found Conditions - Barometric Pressure (inHg): 29.88 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.1 Relative Humidity (%): 56  
 As-Found Lab Activity Date Range: 07/26/2024 - 07/29/2024

Plastic end of breath hose where the mouth piece attaches was removed and thrown away. New breath hose needed.

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG408002	0.020	0.020	0.020	0.019	0.019	0.020	+/- 0.002	
0.040	0.039	AG407908	0.040	0.038	0.039	0.039	0.039	0.039	+/- 0.003	
0.080	0.078	AG335202	0.078	0.078	0.078	0.078	0.078	0.078	+/- 0.004	
0.100	0.098	AG333401	0.097	0.098	0.098	0.098	0.098	0.098	+/- 0.004	
0.150	0.147	AG332004	0.145	0.144	0.145	0.144	0.144	0.144	+/- 0.006	
0.300	0.294	AG327804	0.294	0.294	0.294	0.294	0.294	0.294	+/- 0.012	

As Left Conditions - Barometric Pressure (inHg): 29.32 Barometer Used: Fisher S/N 230307229 Temperature (C): 22.0 Relative Humidity (%): 50  
 As-Left Lab Activity Date Range: 07/30/2024 - 07/30/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

*Megan Carlock*

Results authorized by Megan Carlock on 09/03/2024

[megan.crouse@alaska.gov](mailto:megan.crouse@alaska.gov)

Technically and administratively reviewed by Carlie Glaister on 09/04/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100361 Analyst or Technician Name: Megan Carlock  
DataMaster DMT Calibration Start Date: 7/30/24

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 230307229  
Calibration Due Date: 5/27/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.32 Temperature(C) 22.0 Relative Humidity(%) 50  
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20240501KS Expiration Date: 8/1/2024  
Simulator S/N: SD1088 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240501MNC Expiration Date: 8/1/2024  
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 22HP41201 Expiration Date: 8/1/2024 8/24/2024  
Simulator S/N: SD1177 Thermometer Verification Performed?  MNC 9/3/24

Calibrated External Thermometer S/N: 230631106  
Calibration Due Date: 9/19/2025

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 7/30/24  
Data Interpretation Date (Technician): N/A (if applicable)  
Data Interpretation Date (Analyst): 7/30/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100361  
-----

Date: 07/30/2024  
Time: 11:17:02

VERSIONS

DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 45.3°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.87 V PASSED  
(1.17 V - 2.73 V)  
Cooler Voltage = 1.89 V PASSED  
(1.01 V - 2.35 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 526 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.4 in

PUMP INFO

Flow Rate = 4.531 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.003 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.087 0.40% (0.00% - 4.00%) PASSED

Technician Screen

-----  
DATAMASTER dmt: 100361  
-----

Date: 07/30/2024  
Time: 11:27 AM

Temperatures (°C)  
Sample Cell: 50.0°C  
Breath Tube: 43.9°C

Current Barometer 29.3 in  
Volume (Ltr) 1.55

Settings  
Lamp: 1.87 V  
Bias: 80 V  
Cooler: 1.94 V  
Chopper: 525 Hz

Voltages (V)  
Flow: 1.04 V  
Detector: -0.005 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100361  
-----

Date: 04/23/2021  
Time: 09:19:31

OPERATOR NAME:  
NPAS TECH  
CERTIFICATE #: G12921/20490

Ca = 0.1000  
CAL = 0.999458    0.800 <= CAL < 1.200  
b1 = 0.0003    0.0000 <= b1 < 0.0040  
b2 = 0.0060    0.0010 <= b2 < 0.0100  
b3 = 0.0001    0.0000 <= b3 < 0.0040  
Xq = 0.0877    0.0500 <= Xq < 0.2000  
a21 = 1.187326    1.050 <= a21 < 1.300  
a31 = 0.501823    0.300 <= a31 < 0.800



SUBJECT TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361

Date: 07/30/2024  
 Time: 11:30:53

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXX

OPERATOR NAME:  
 MEGAN CARLOCK  
 OPERATOR'S #: 10747


DEPT/AGENCY:  
 MINIMUM VOLUME TEST  
 CASE/REPORT: XXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.31: 0.078  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:31
BLANK TEST	0.000	11:32
INTERNAL STANDARD	VERIFIED	11:32
EXTERNAL STANDARD	0.079	11:32
BLANK TEST	0.000	11:33
SUBJECT SAMPLE (Vol=1.55L)	0.000	11:34
BLANK TEST	0.000	11:35
EXTERNAL STANDARD	0.078	11:36
BLANK TEST	0.000	11:36

MNC

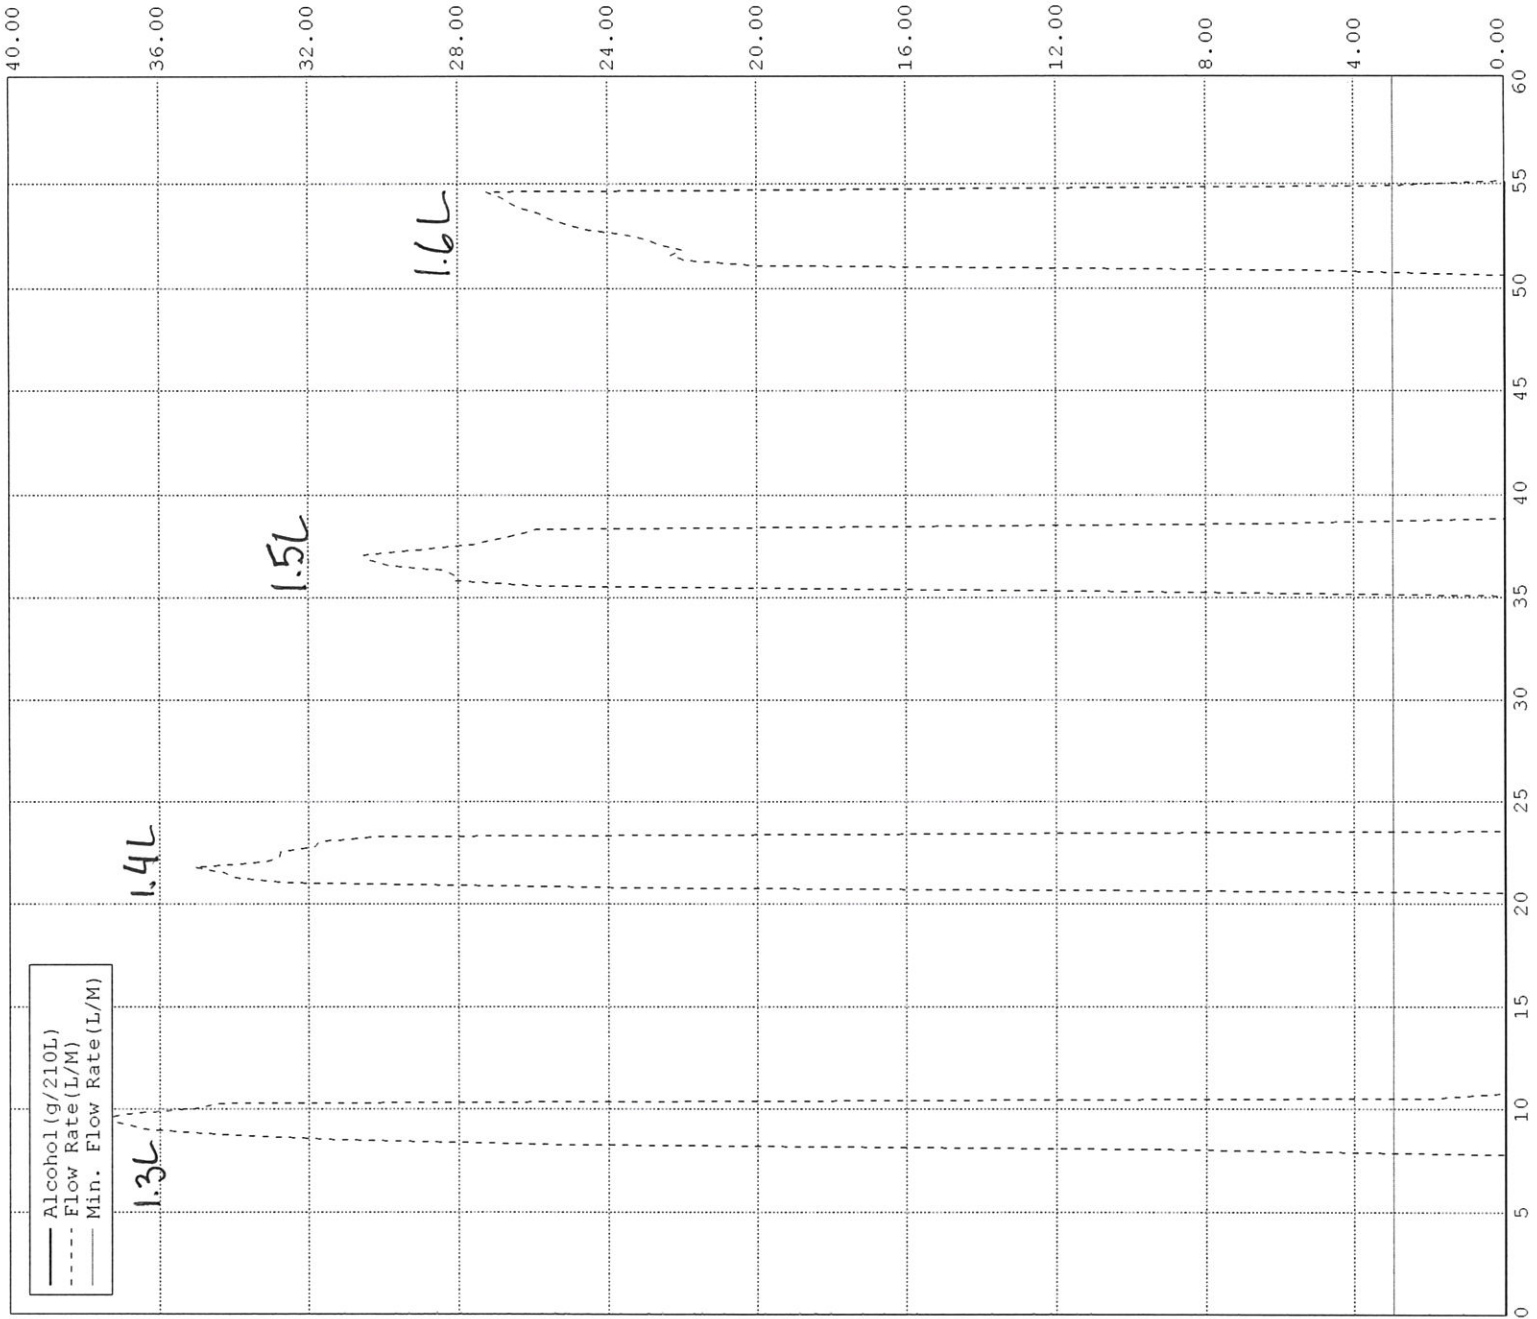



LINEARITY CHECK


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100361  
 -----

Date: 07/30/2024  
 Time: 11:40:52

SUPERVISOR NAME:  
 MEGAN CARLOCK  
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.020	0.0196	0.0005
0.039	0.0390	0.0007
0.078	0.0780	0.0000
0.098	0.0978	0.0004
0.147	0.1444	0.0005
0.294	0.2940	0.0000

SLOPE = 0.999005  
 R<sup>2</sup> = 0.999895

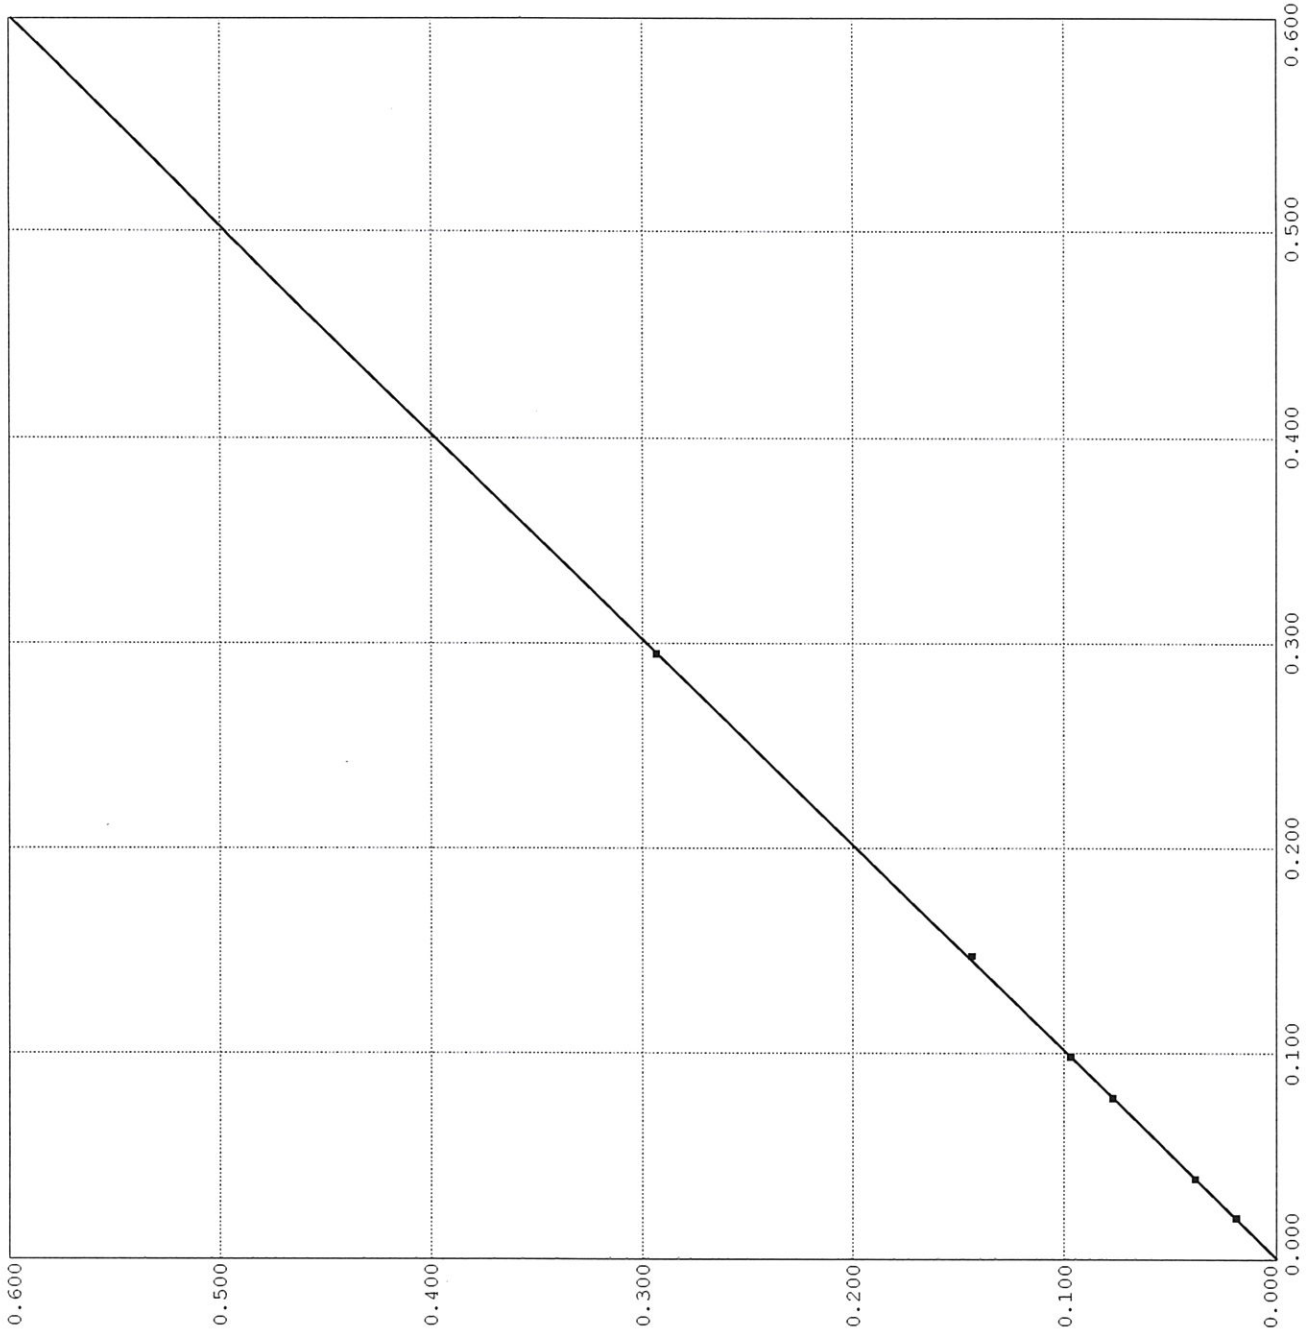

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 07/30/2024  
 Time: 11:43:39

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.31: 0.020  
 LOT #: AG408002  
 EXPIRATION: 03/20/2026  
 TANK PRESSURE: 510 psi

BLANK TEST	0.000	11:45
INTERNAL STANDARD	VERIFIED	11:45
EXTERNAL STANDARD	0.020	11:45
BLANK TEST	0.000	11:46
EXTERNAL STANDARD	0.020	11:46
BLANK TEST	0.000	11:47
EXTERNAL STANDARD	0.020	11:47
BLANK TEST	0.000	11:48
EXTERNAL STANDARD	0.019	11:48
BLANK TEST	0.000	11:49
EXTERNAL STANDARD	0.019	11:49
BLANK TEST	0.000	11:50

Average = 0.0196  
 Std Dev = 0.0005

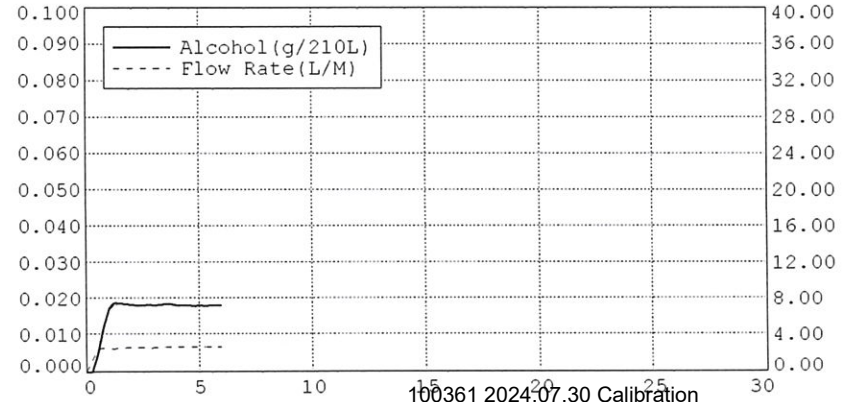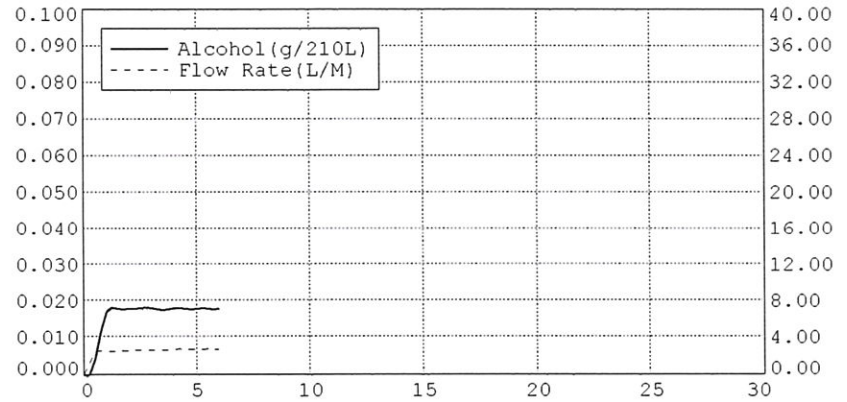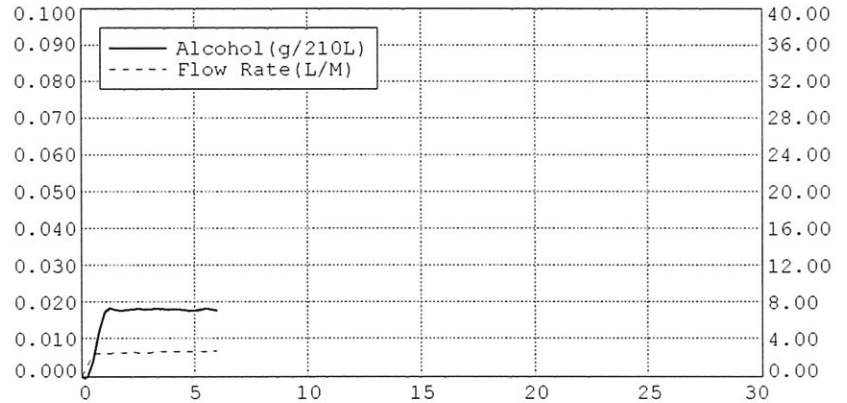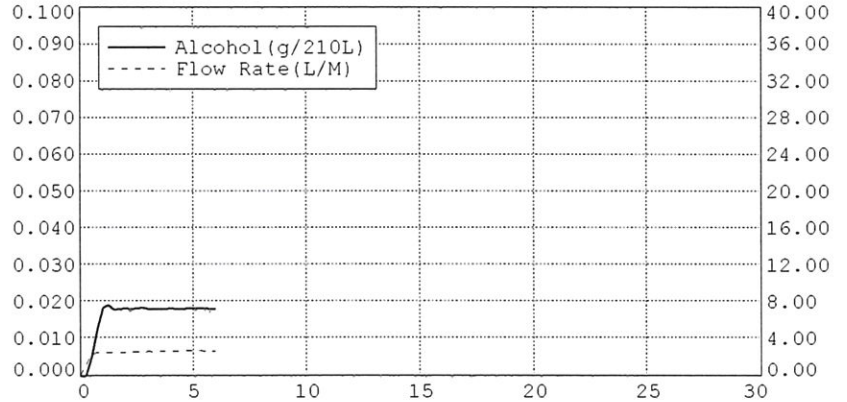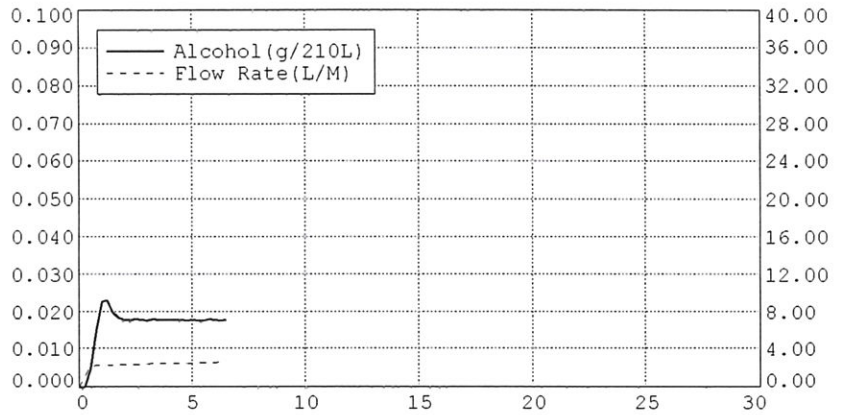



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 07/30/2024  
 Time: 11:51:22

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.31: 0.039  
 LOT #: AG407908  
 EXPIRATION: 03/19/2026  
 TANK PRESSURE: 1059 psi

BLANK TEST	0.000	11:52
INTERNAL STANDARD	VERIFIED	11:52
EXTERNAL STANDARD	0.040	11:52
BLANK TEST	0.000	11:53
EXTERNAL STANDARD	0.038	11:54
BLANK TEST	0.000	11:54
EXTERNAL STANDARD	0.039	11:55
BLANK TEST	0.000	11:56
EXTERNAL STANDARD	0.039	11:56
BLANK TEST	0.000	11:57
EXTERNAL STANDARD	0.039	11:57
BLANK TEST	0.000	11:58

Average = 0.0390  
 Std Dev = 0.0007

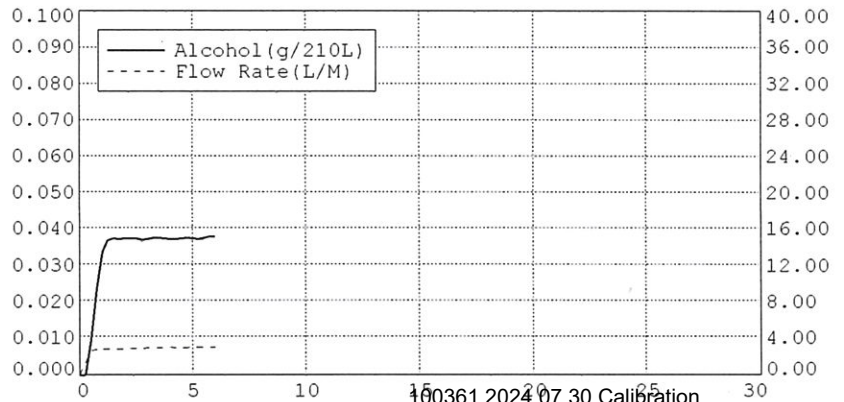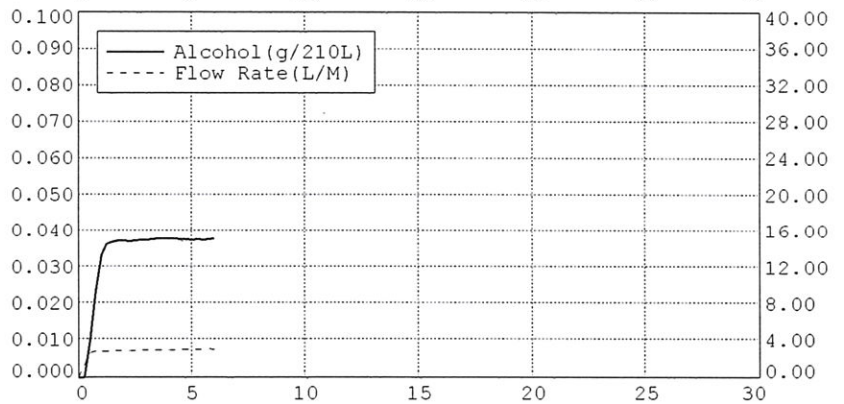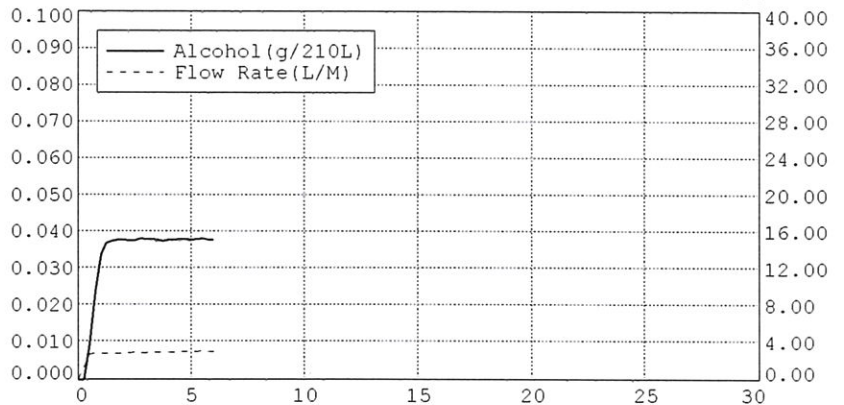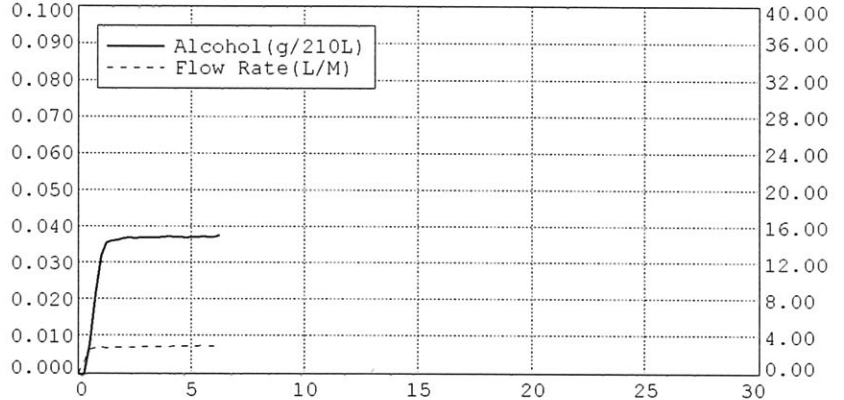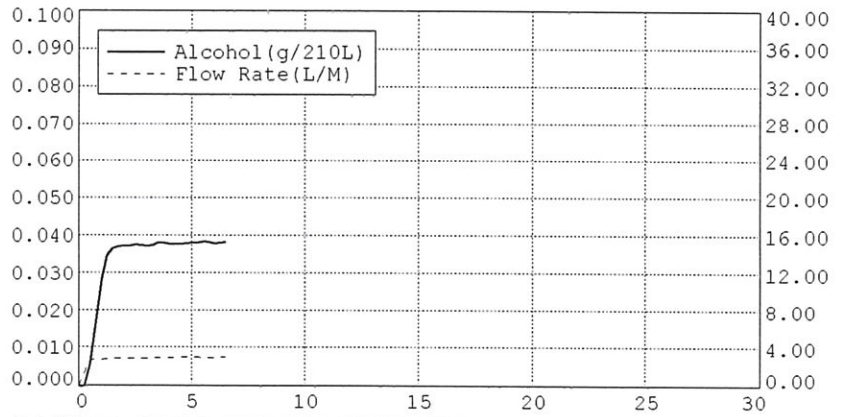

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 07/30/2024  
 Time: 11:59:30

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.31: 0.078  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025  
 TANK PRESSURE: 1102 psi

BLANK TEST	0.000	12:00
INTERNAL STANDARD	VERIFIED	12:00
EXTERNAL STANDARD	0.078	12:01
BLANK TEST	0.000	12:02
EXTERNAL STANDARD	0.078	12:02
BLANK TEST	0.000	12:03
EXTERNAL STANDARD	0.078	12:03
BLANK TEST	0.000	12:04
EXTERNAL STANDARD	0.078	12:04
BLANK TEST	0.000	12:05
EXTERNAL STANDARD	0.078	12:05
BLANK TEST	0.000	12:06

Average = 0.0780  
 Std Dev = 0.0000

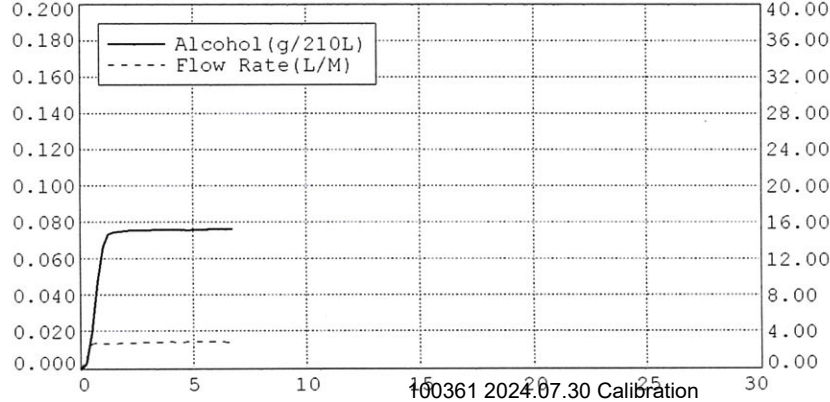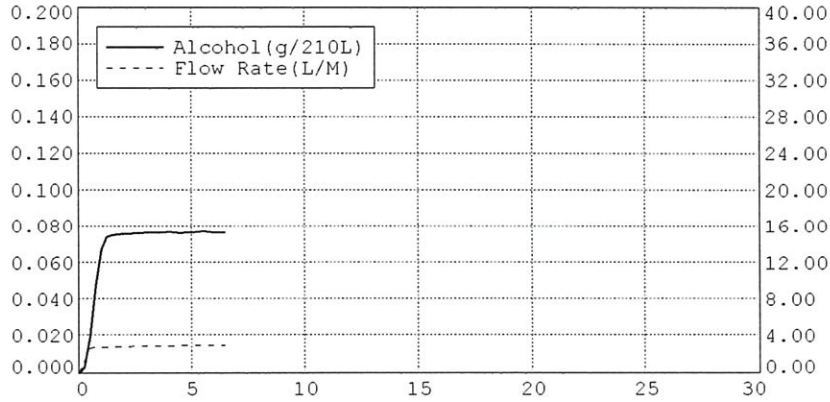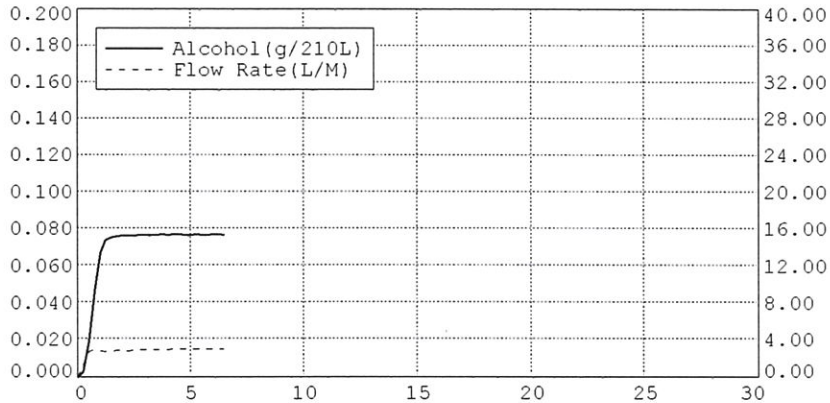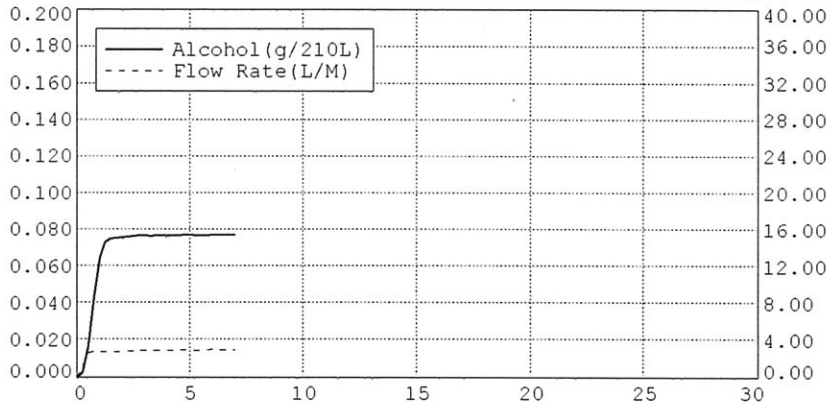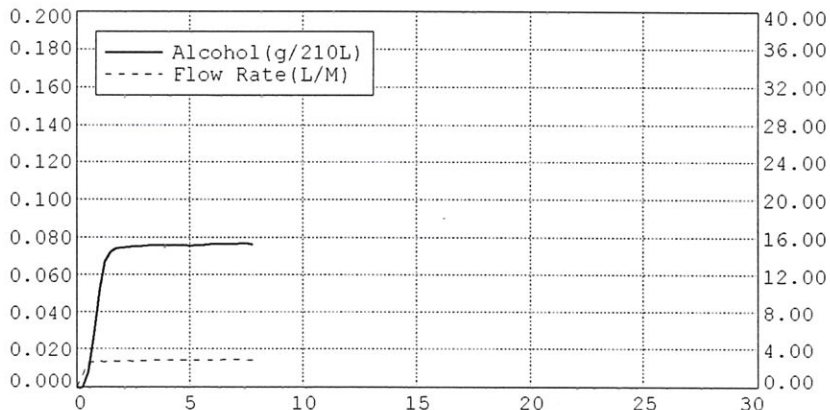



LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 07/30/2024  
 Time: 12:33:04

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.33: 0.098  
 LOT #: AG333401  
 EXPIRATION: 11/30/2025  
 TANK PRESSURE: 856 psi

BLANK TEST	0.000	12:34
INTERNAL STANDARD	VERIFIED	12:34
EXTERNAL STANDARD	0.097	12:34
BLANK TEST	0.000	12:35
EXTERNAL STANDARD	0.098	12:35
BLANK TEST	0.000	12:36
EXTERNAL STANDARD	0.098	12:36
BLANK TEST	0.000	12:37
EXTERNAL STANDARD	0.098	12:38
BLANK TEST	0.000	12:38
EXTERNAL STANDARD	0.098	12:39
BLANK TEST	0.000	12:40

Average = 0.0978  
 Std Dev = 0.0004

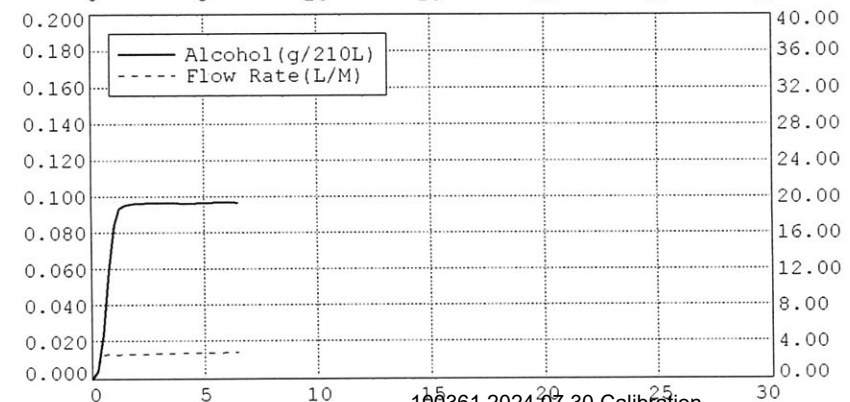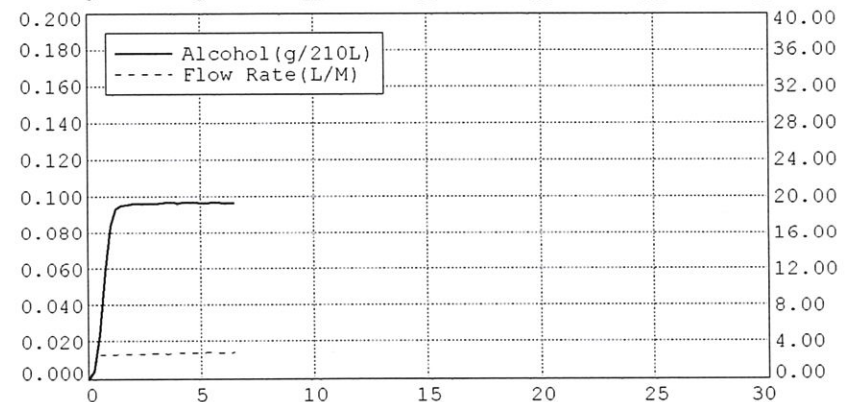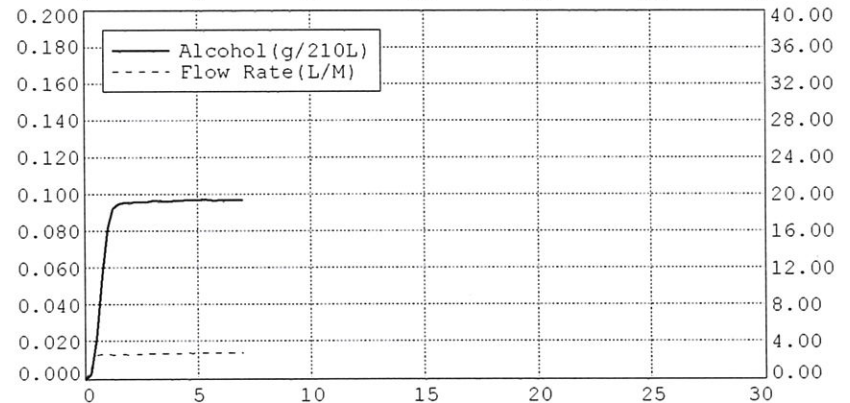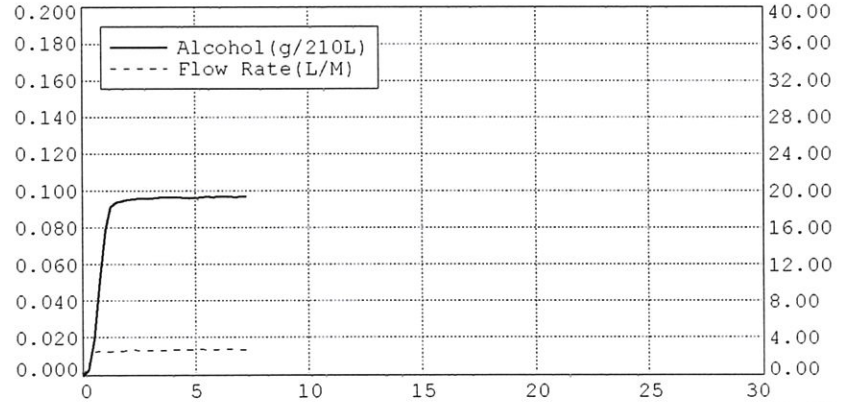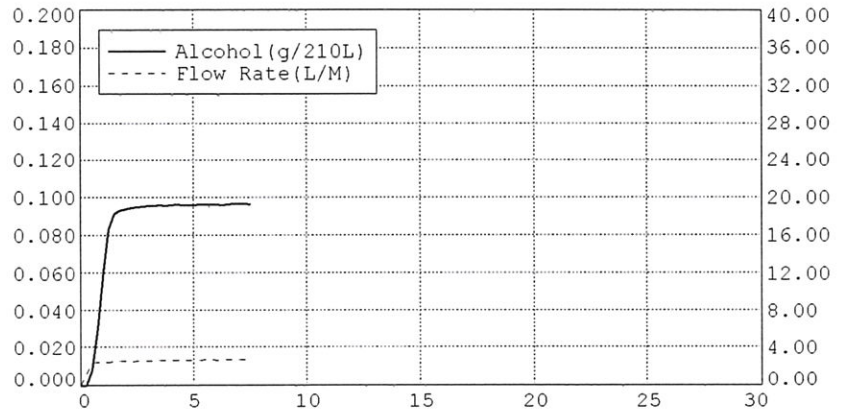

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 07/30/2024  
 Time: 12:47:40

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.33: 0.147  
 LOT #: AG332004  
 EXPIRATION: 11/16/2025  
 TANK PRESSURE: 477 psi

BLANK TEST	0.000	12:48
INTERNAL STANDARD	VERIFIED	12:49
EXTERNAL STANDARD	0.145	12:49
BLANK TEST	0.000	12:50
EXTERNAL STANDARD	0.144	12:50
BLANK TEST	0.000	12:51
EXTERNAL STANDARD	0.145	12:51
BLANK TEST	0.000	12:52
EXTERNAL STANDARD	0.144	12:52
BLANK TEST	0.000	12:53
EXTERNAL STANDARD	0.144	12:53
BLANK TEST	0.000	12:54

Average = 0.1444  
 Std Dev = 0.0005

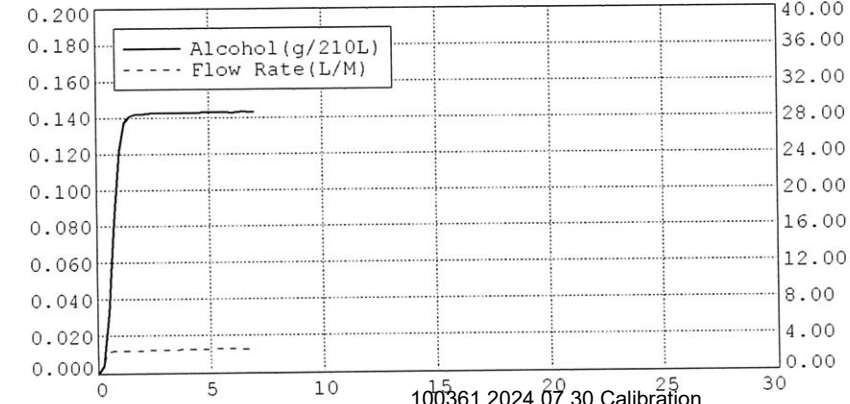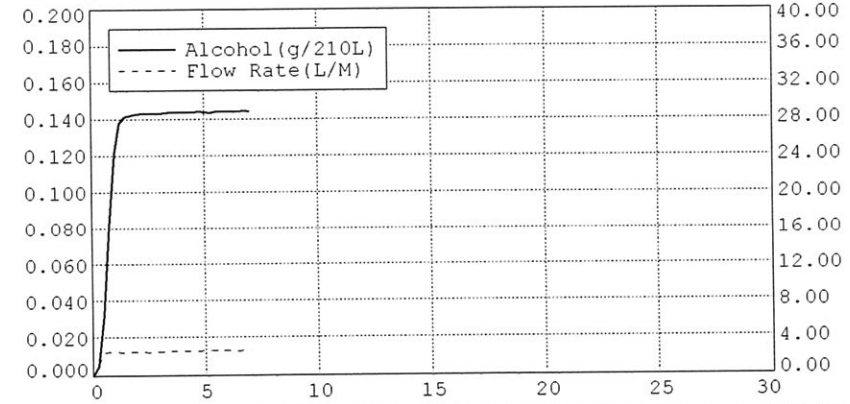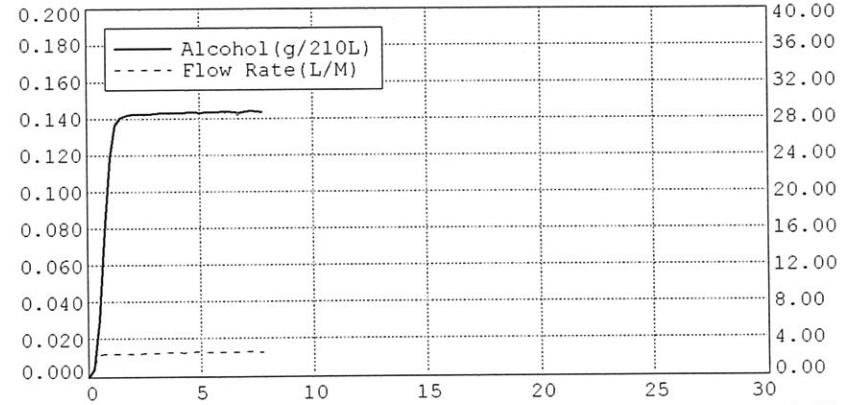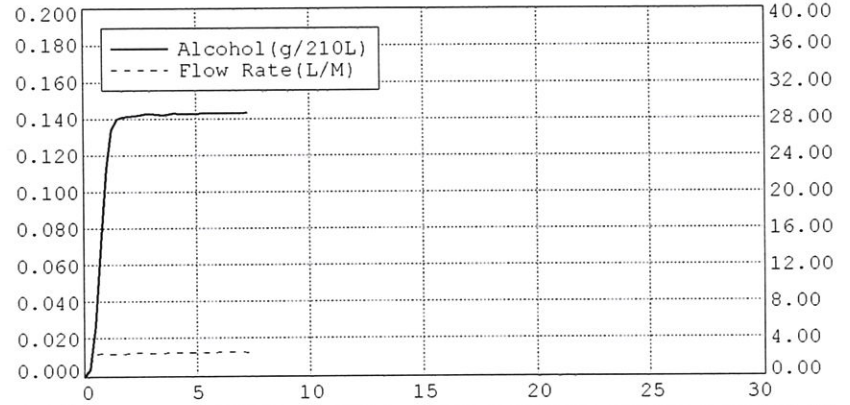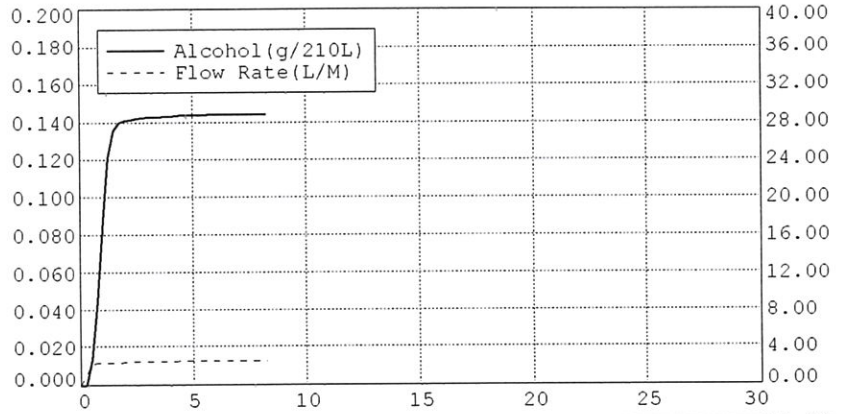



LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 07/30/2024  
 Time: 12:55:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.33: 0.294  
 LOT #: AG327804  
 EXPIRATION: 10/05/2025  
 TANK PRESSURE: 280 psi

BLANK TEST	0.000	12:56
INTERNAL STANDARD	VERIFIED	12:56
EXTERNAL STANDARD	0.294	12:56
BLANK TEST	0.000	12:57
EXTERNAL STANDARD	0.294	12:57
BLANK TEST	0.000	12:58
EXTERNAL STANDARD	0.294	12:59
BLANK TEST	0.000	12:59
EXTERNAL STANDARD	0.294	13:00
BLANK TEST	0.000	13:01
EXTERNAL STANDARD	0.294	13:01
BLANK TEST	0.000	13:02

Average = 0.2940  
 Std Dev = 0.0000

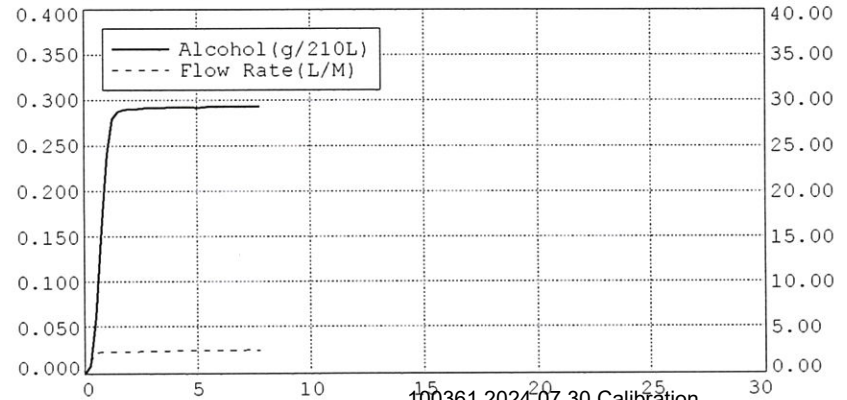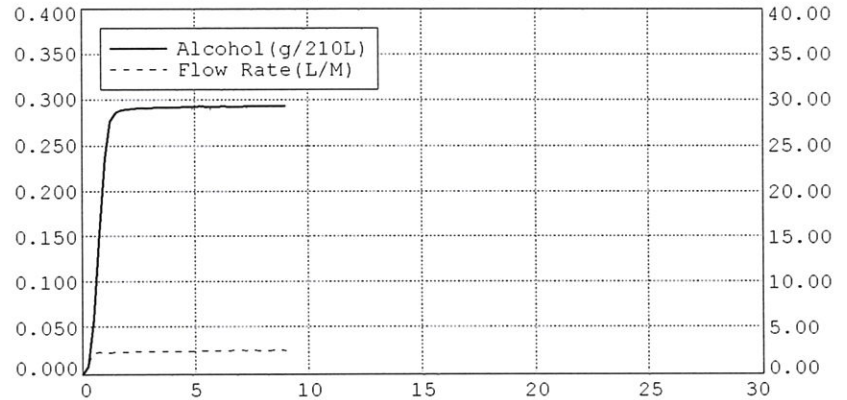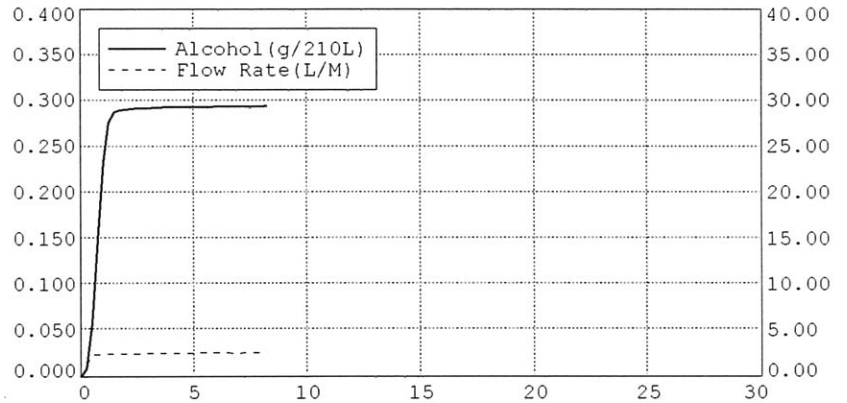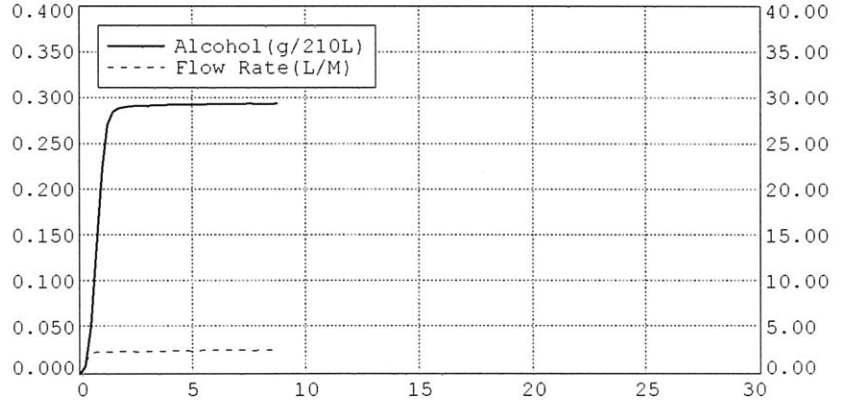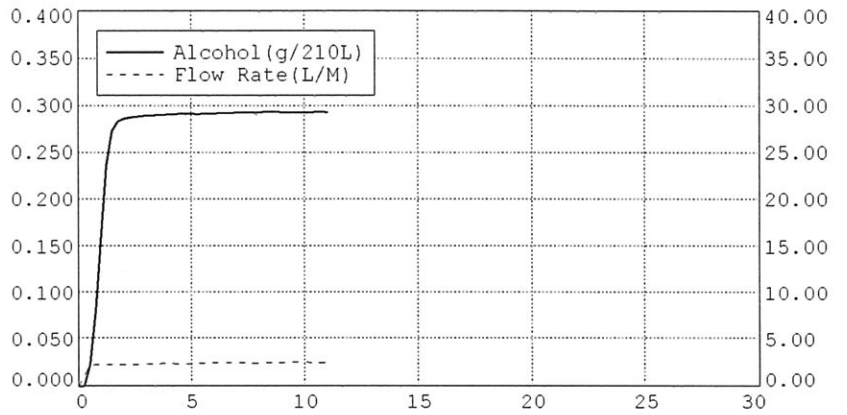



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100361

Date: 07/30/2024  
Time: 13:06:28

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
MEGAN CARLOCK  
OPERATOR'S #: 10747

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.34: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:07  
BLANK TEST 0.000 13:07  
INTERNAL STANDARD VERIFIED 13:07  
EXTERNAL STANDARD 0.079 13:07  
BLANK TEST 0.000 13:08  
SUBJECT SAMPLE INCOMPLETE 13:10

MNC

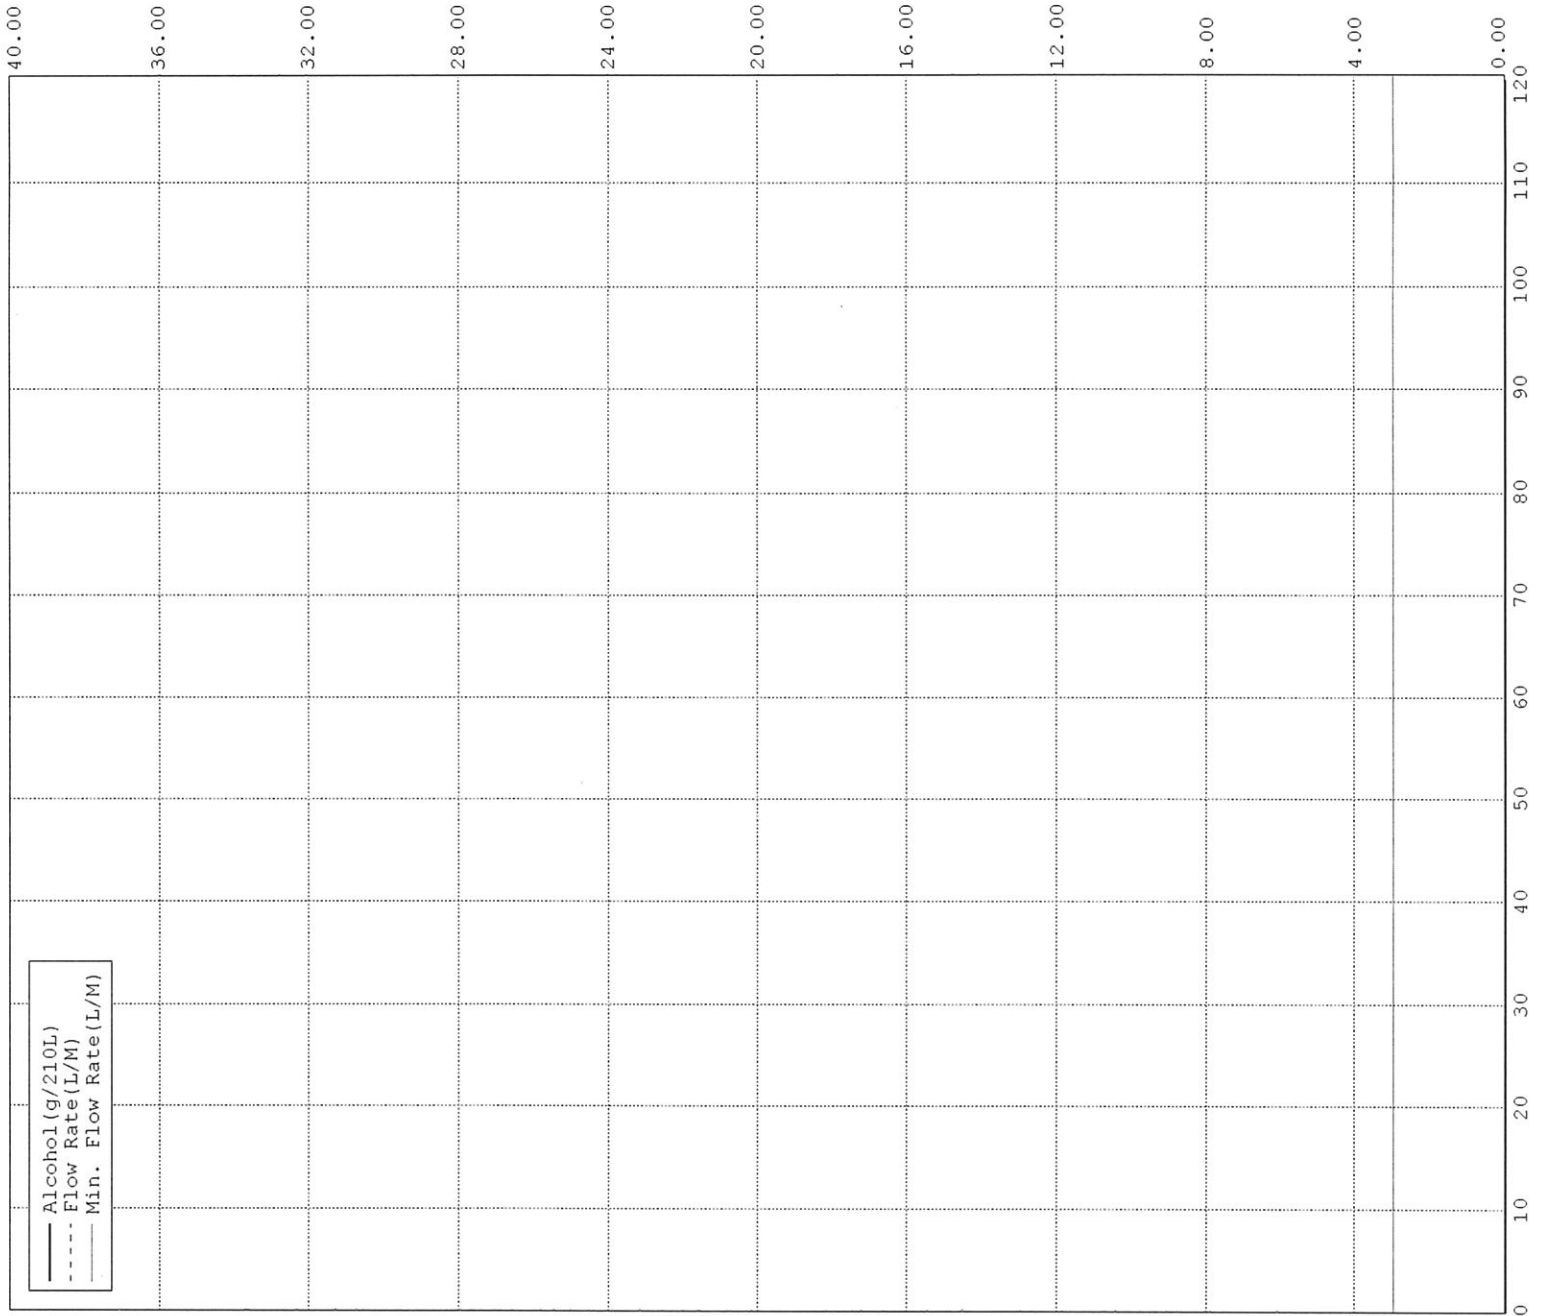

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100361

Date: 07/30/2024  
Time: 13:12:52

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CARLOCK  
OPERATOR'S #: 10747


DEPT/AGENCY:  
MAXIMUM ATTEMPTS EXCEEDED  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.34: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:14  
BLANK TEST 0.000 13:14  
INTERNAL STANDARD VERIFIED 13:14  
EXTERNAL STANDARD 0.078 13:14  
BLANK TEST 0.000 13:15  
SUBJECT SAMPLE XXX 13:16

Maximum Attempts Exceeded

MNC

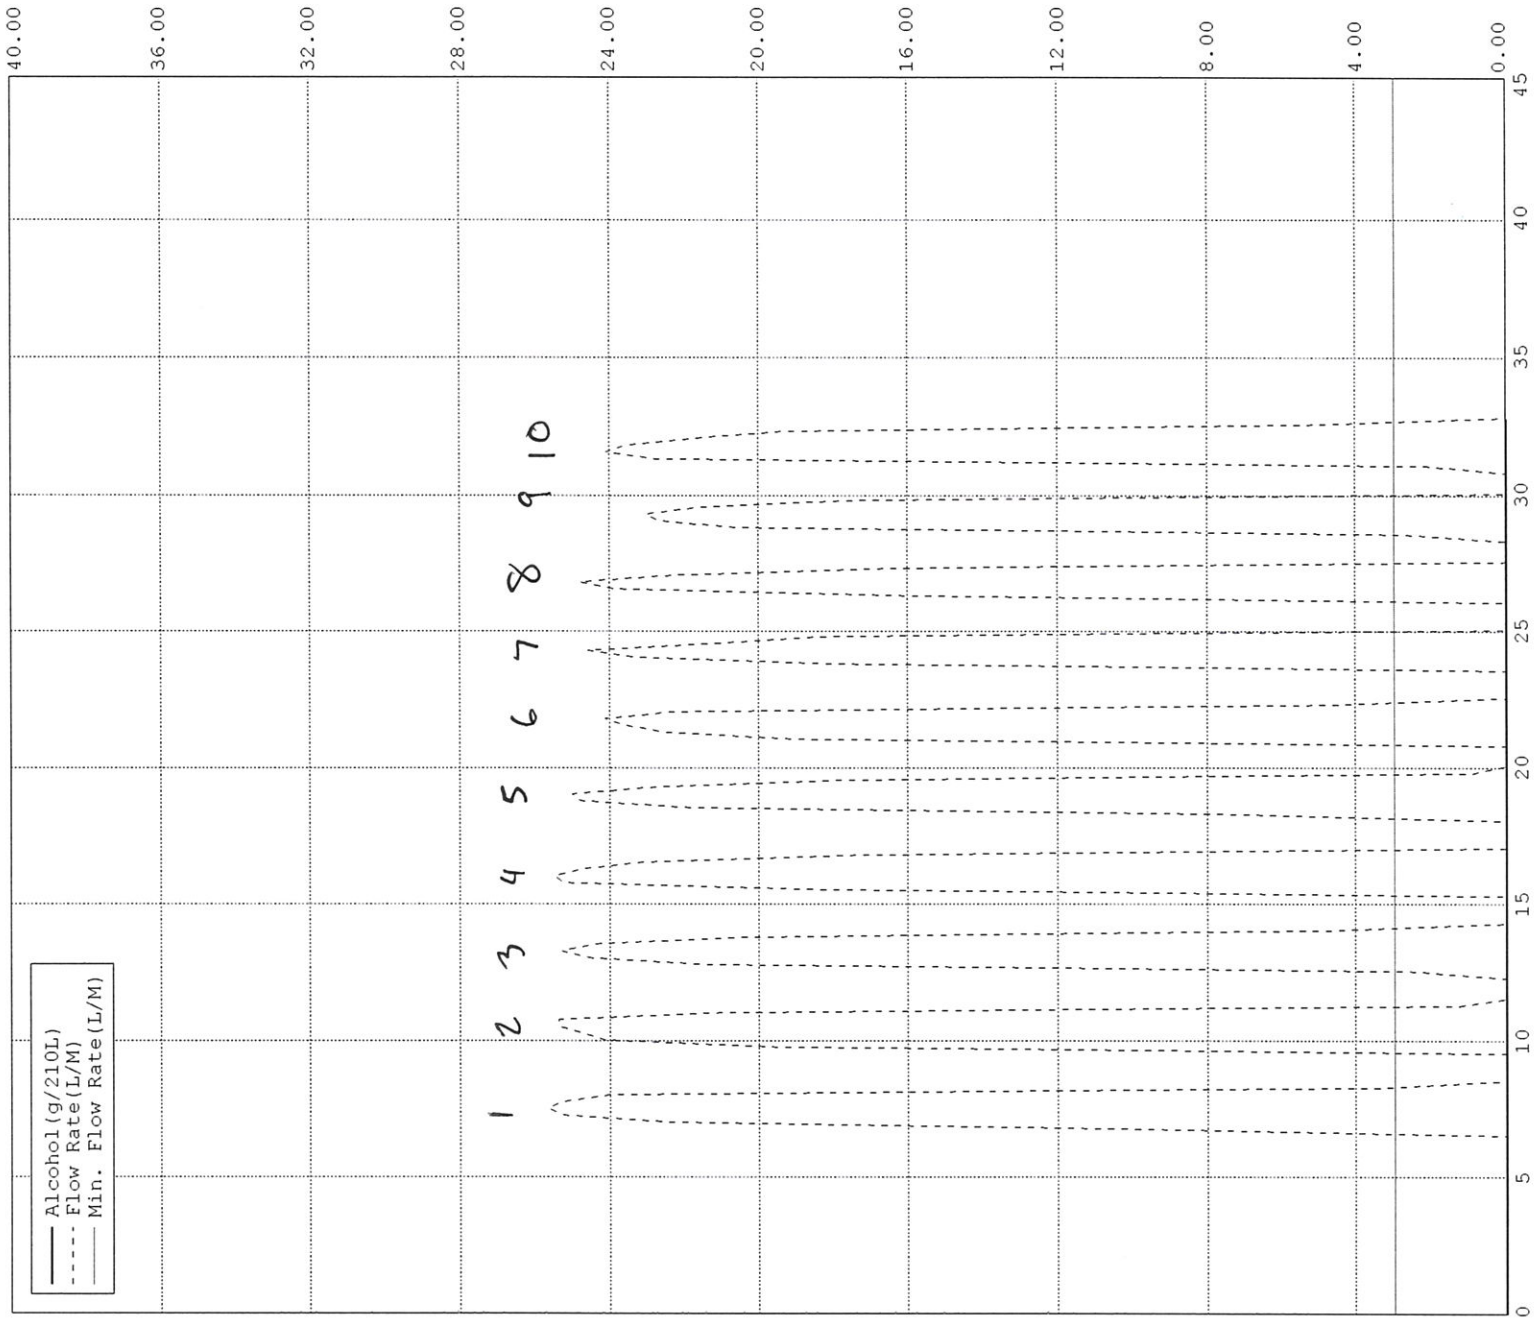

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100361

Date: 07/30/2024

Time: 13:29:18

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INVALID

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.34: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

PASSED 13:33

BLANK TEST 0.000 13:33

INTERNAL STANDARD

VERIFIED 13:33


EXTERNAL STANDARD

0.078 13:33

BLANK TEST 0.000 13:34

SUBJECT SAMPLE INVALID 13:34

Alcohol (g/210L)  
Flow Rate (L/M)  
Min. Flow Rate (L/M)

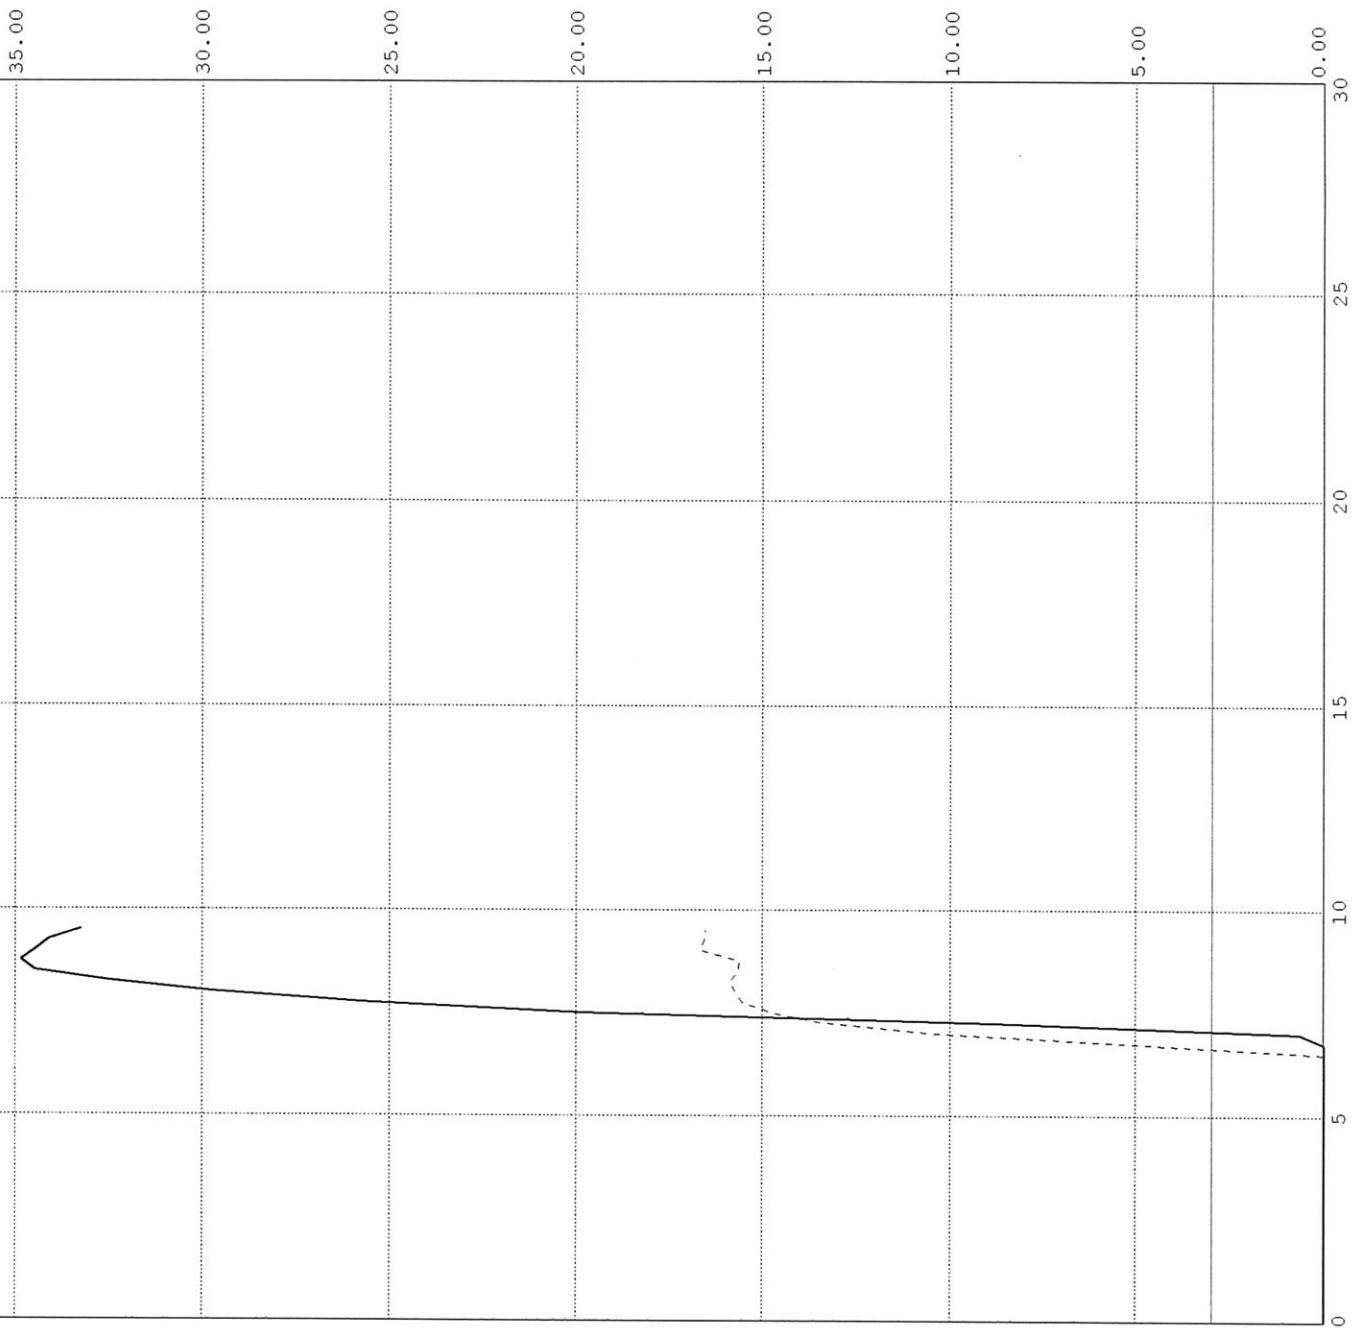

MNC

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100361

Date: 07/30/2024

Time: 13:19:00

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

RFI

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.34: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

PASSED 13:23

0.000 13:23


VERIFIED 13:23

0.080 13:23

0.000 13:24

RFI DETECTED

MNC

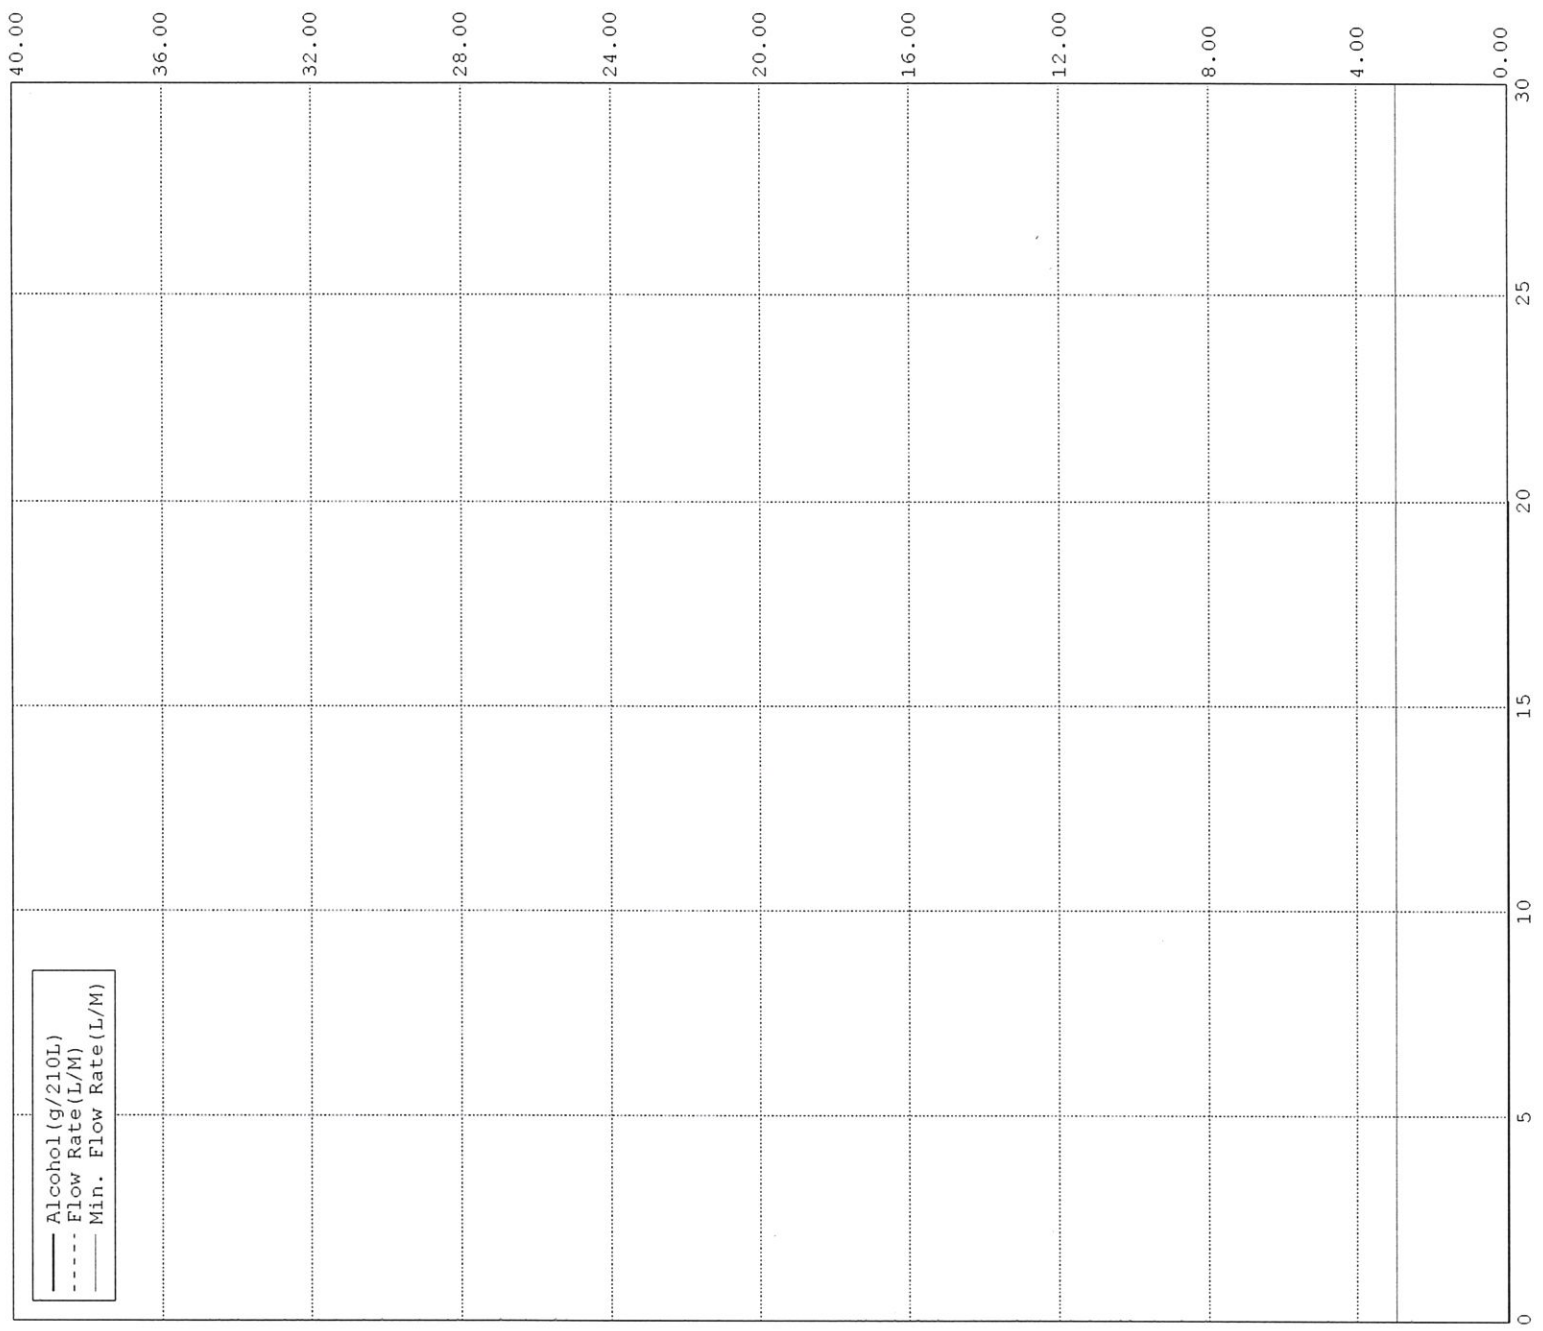



SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100361

Date: 07/30/2024

Time: 13:46:37

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INTERFERENCE- ACETONE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.35: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:47

BLANK TEST 0.000 13:47

INTERNAL STANDARD VERIFIED 13:47

Xq = 0.088 (0.70%)

EXTERNAL STANDARD 0.078 13:48

X[1] = 0.0776 (-0.0005) (0.0033)

BLANK TEST 0.000 13:49

SUBJECT SAMPLE XXX 13:49

X[1] = 0.1003 (-0.0165) (-0.0004)


Interference Detected

Filter 2 Average: -0.0003

Filter 3 Average: 0.0026

MNC 7/30/24

MNC

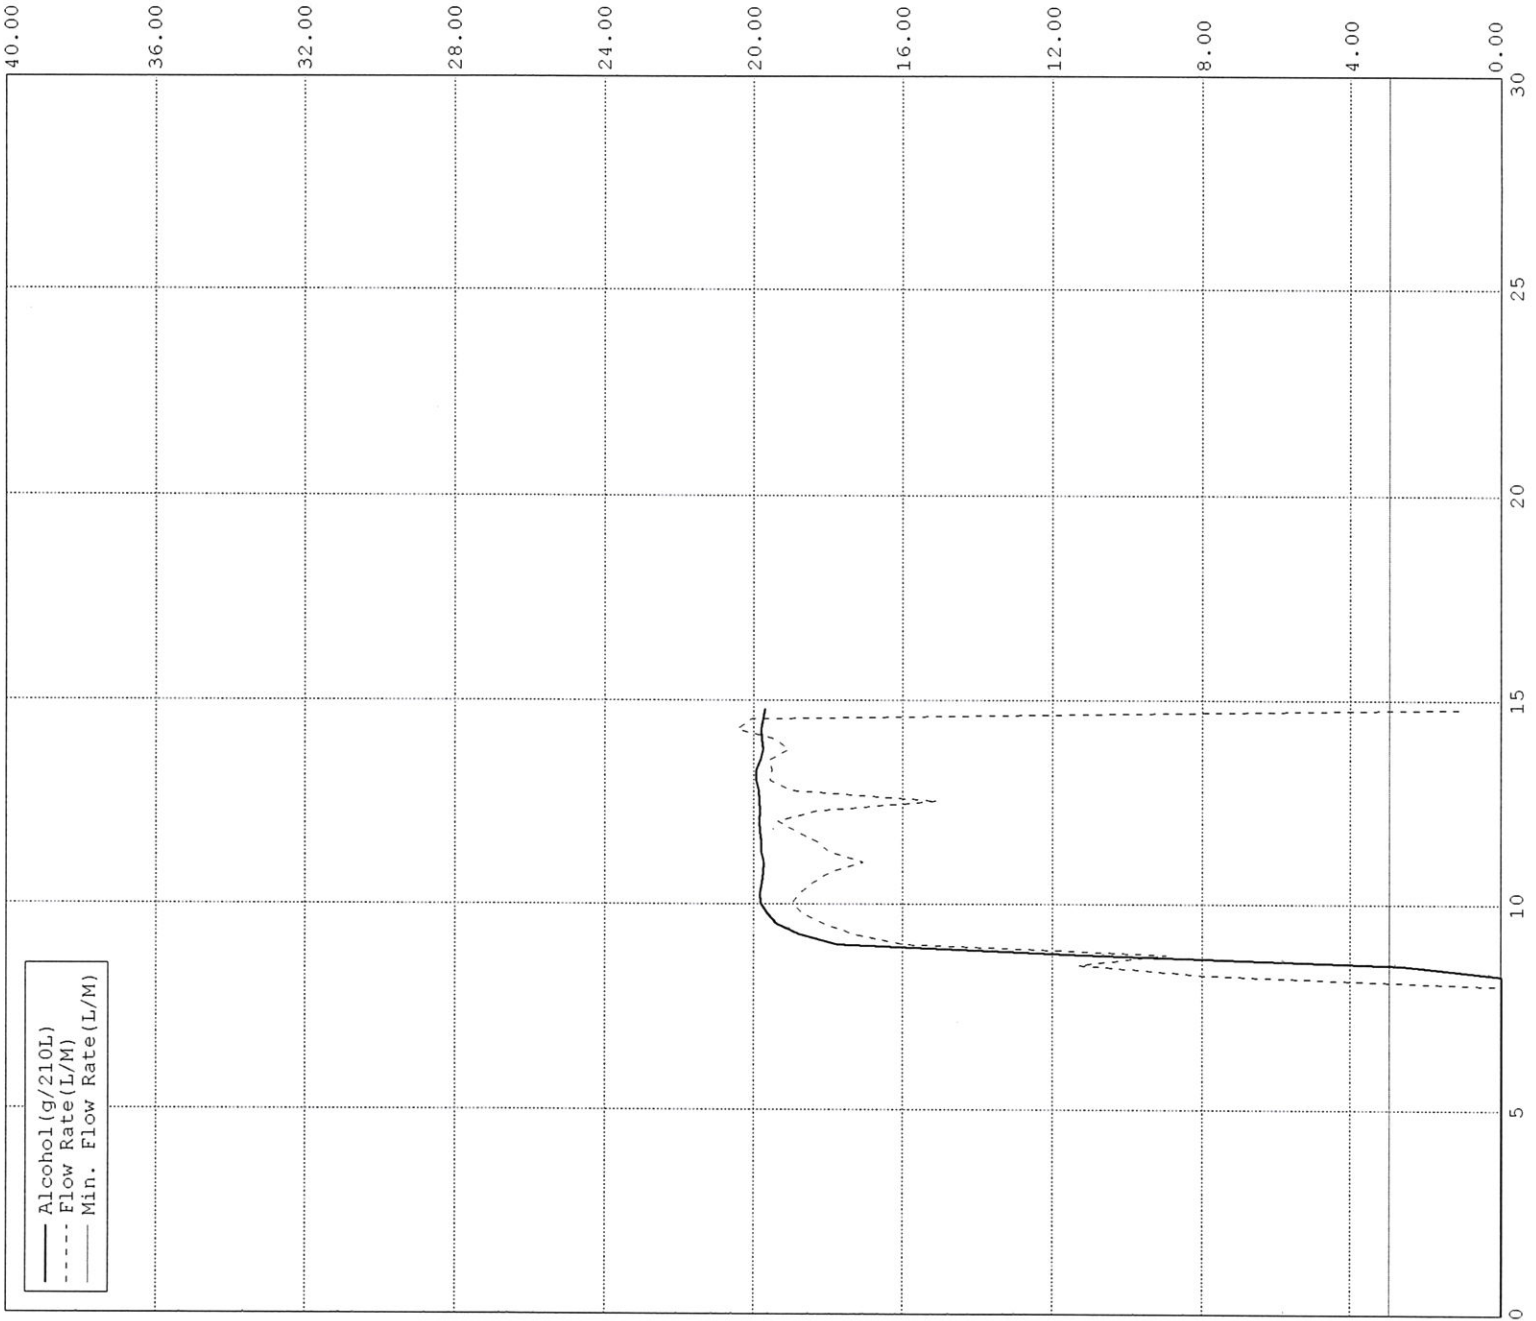



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100361

Date: 07/30/2024  
Time: 13:51:43

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CARLOCK  
OPERATOR'S #: 10747

DEPT/AGENCY:  
INTERFERENCE- IPA  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 13:52  
BLANK TEST 0.000 13:52  
INTERNAL STANDARD VERIFIED 13:53  
Xq = 0.088 (0.50%)  
EXTERNAL STANDARD 0.078 13:53  
X[1] = 0.0785 (-0.0004) (0.0022)  
BLANK TEST 0.000 13:54  
SUBJECT SAMPLE XXX 13:54  
X[1] = 0.1097 (-0.0222) (0.0023)

Interference Detected

MNC

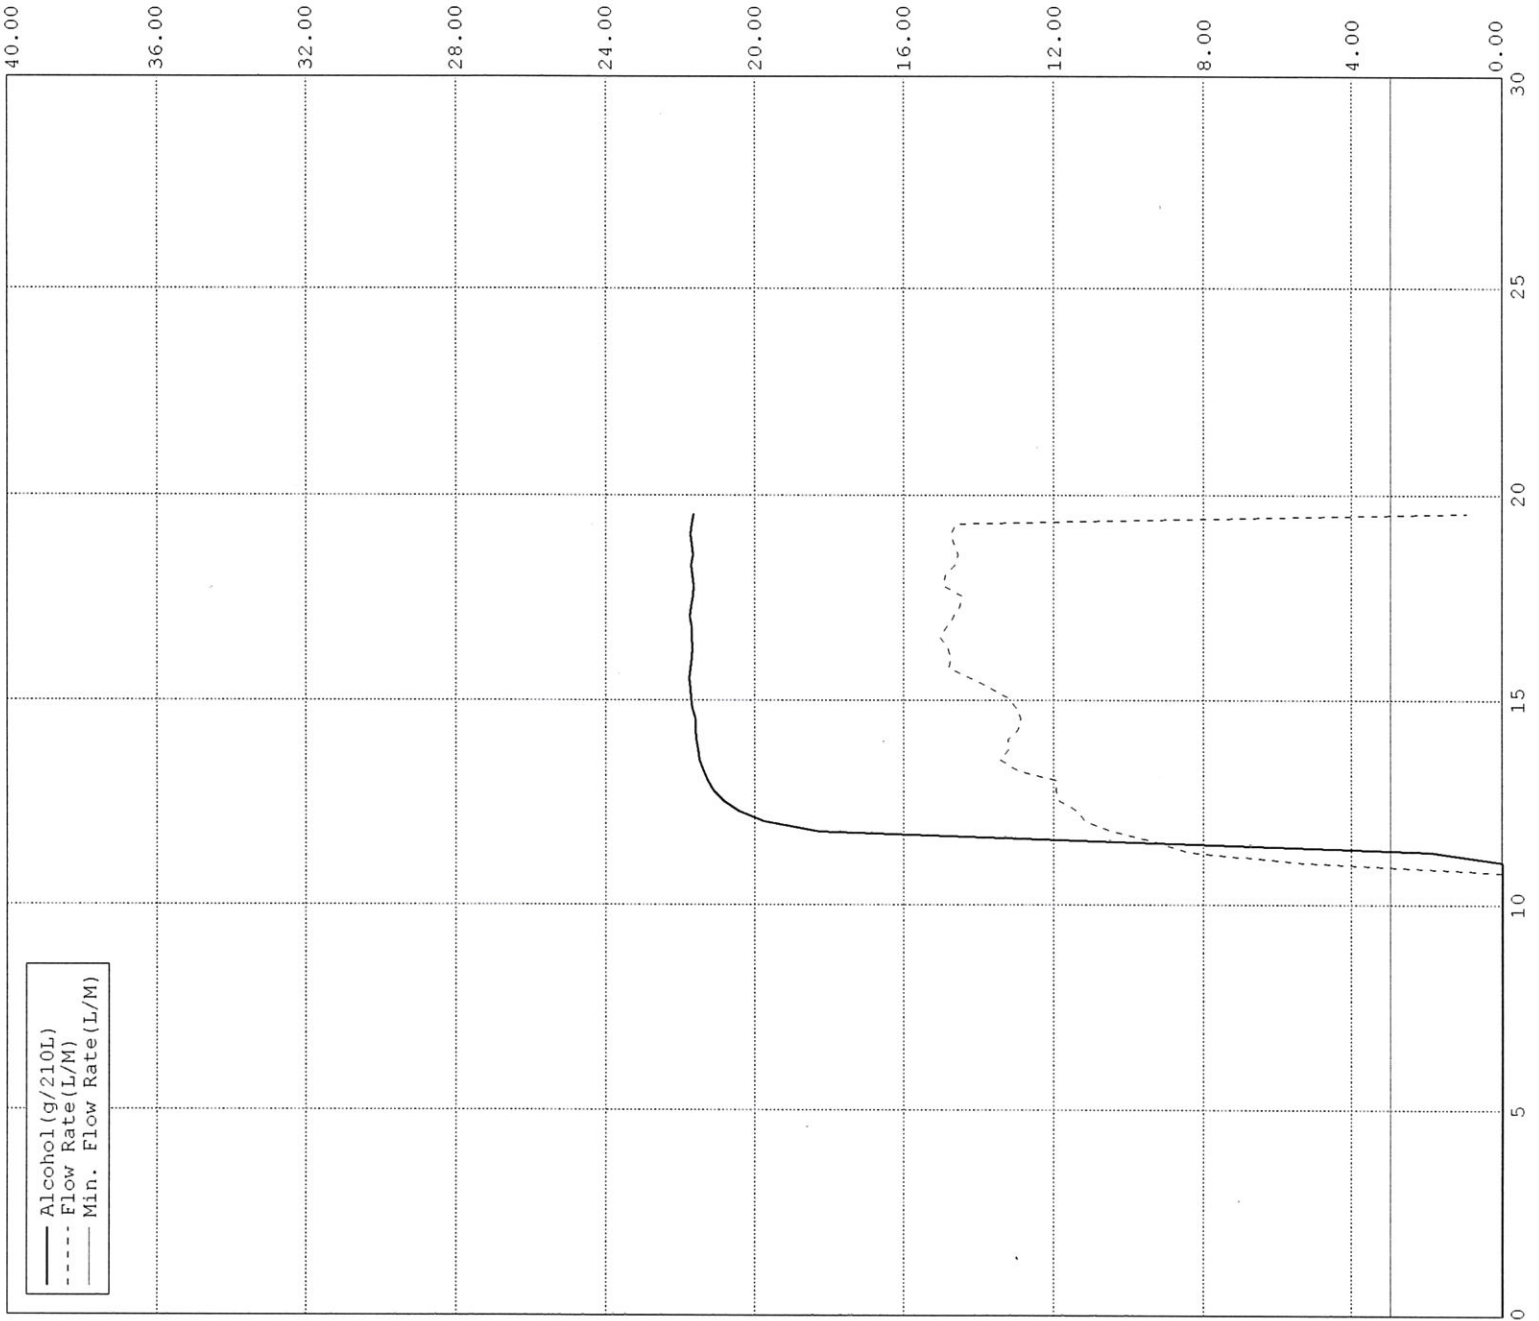

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100361

Date: 07/30/2024  
Time: 13:37:04

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
MEGAN CARLOCK  
OPERATOR'S #: 10747

DEPT/AGENCY:  
INTERFERENCE - NEGATIVE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:41
BLANK TEST	0.000	13:41
INTERNAL STANDARD	VERIFIED	13:41
$X_q = 0.088$ (0.80%)		
EXTERNAL STANDARD	0.078	13:41
$X[1] = 0.0782$ (0.0006)	(0.0032)	
BLANK TEST	0.000	13:42
SUBJECT SAMPLE (Vol=1.94L)	0.086	13:42
$X[1] = 0.0861$ (0.0005)	(0.0001)	
BLANK TEST	0.000	13:43
EXTERNAL STANDARD	0.078	13:44
$X[1] = 0.0776$ (-0.0010)	(0.0017)	
BLANK TEST	0.000	13:44

MNJC

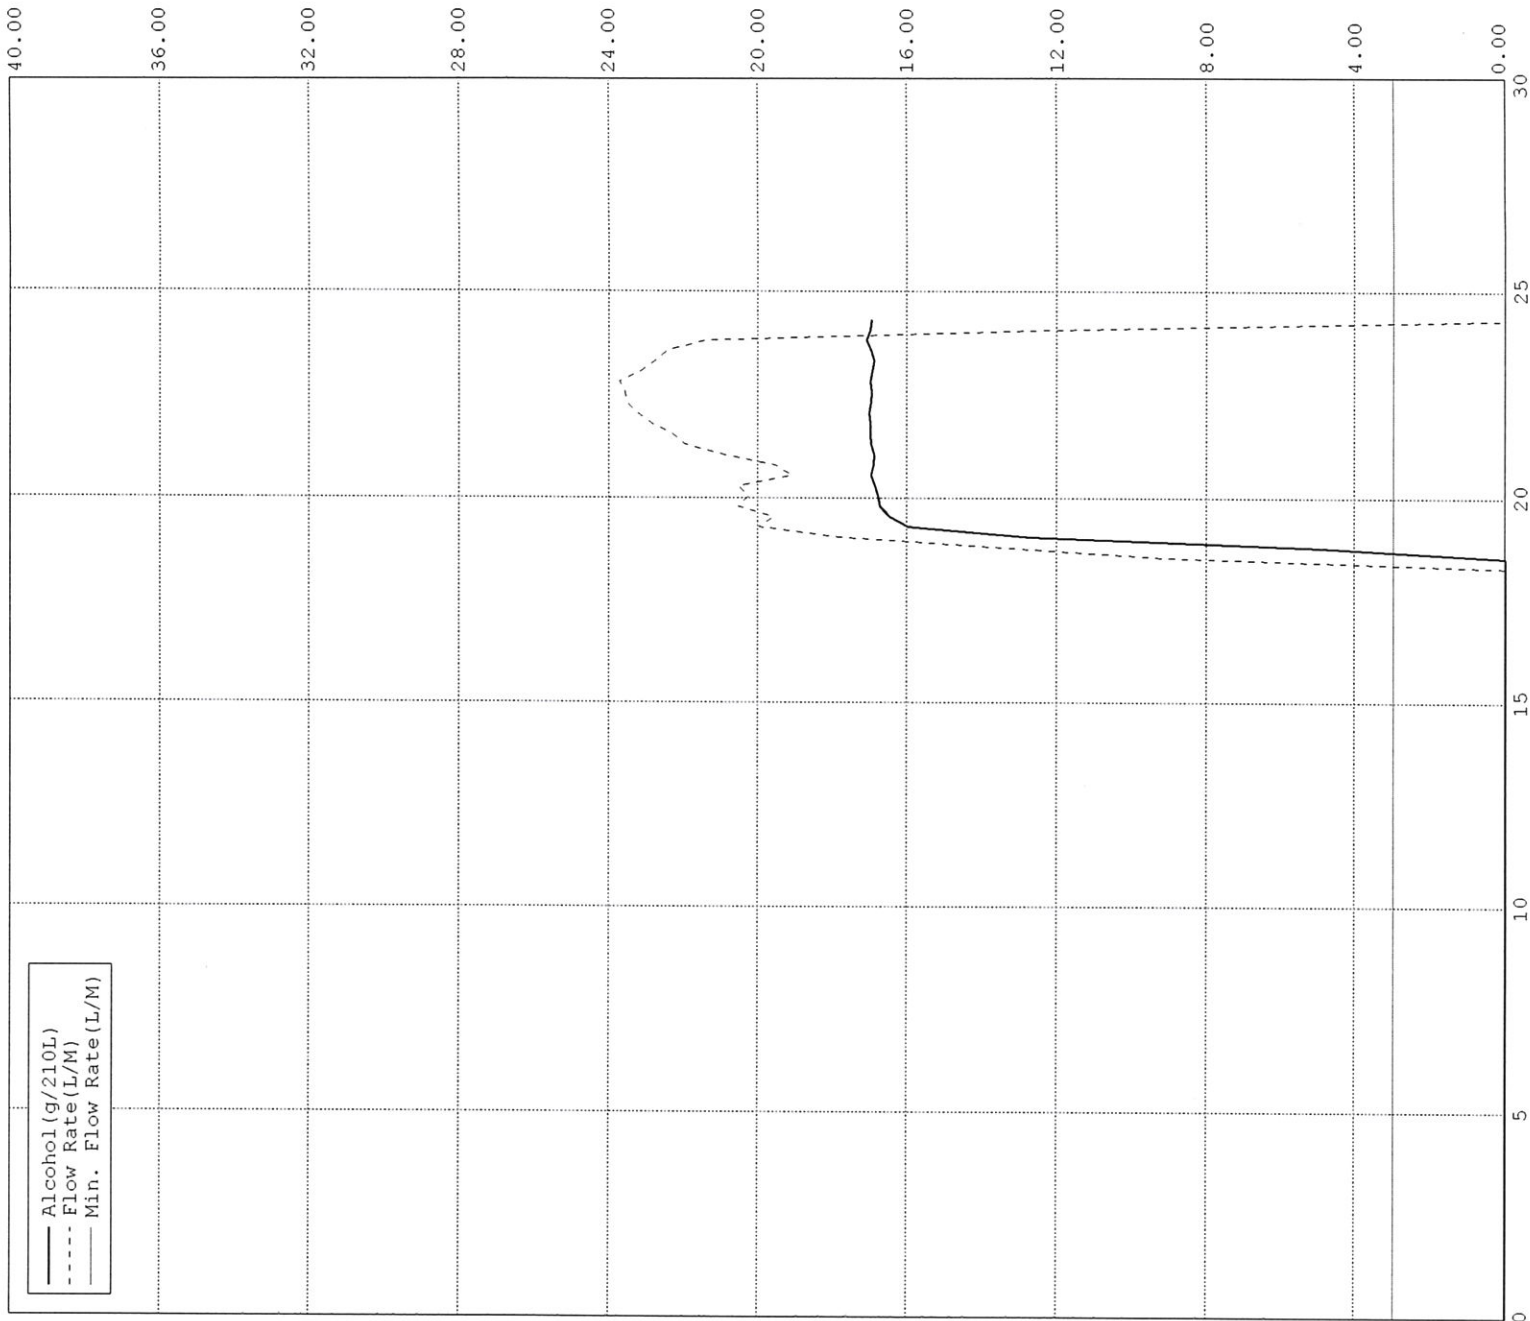

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100361

Date: 07/30/2024  
Time: 14:09:26

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CARLOCK  
OPERATOR'S #: 10747

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:10
BLANK TEST	0.000	14:10
INTERNAL STANDARD	VERIFIED	14:10
EXTERNAL STANDARD	0.078	14:10
BLANK TEST	0.000	14:11
SUBJECT SAMPLE (Vol=2.50L)	0.000	14:12
BLANK TEST	0.000	14:13
EXTERNAL STANDARD	0.079	14:13
BLANK TEST	0.000	14:14

MNC

