



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100695

**Report Issue Date:** 04/25/2024  
**Date Received:** 2023-07-18  
**Condition of Item:** Good

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.021	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.080	AG310901	0.080	0.080	0.080	0.080	0.080	0.080	0.080
0.300	0.299	AG217903	0.302	0.301	0.301	0.301	0.301	0.301	0.301

As Found - Evaluation Analyst: Tatiana Malnoske  
 As Found Conditions - Barometric Pressure (inHg): 29.81 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.7 Relative Humidity (%): 51%  
 As-Found Lab Activity Date Range: 07/18/2023 - 07/18/2023

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002	
0.040	0.040	AG217904	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003	
0.080	0.079	AG310901	0.079	0.079	0.079	0.079	0.078	0.079	+/- 0.004	
0.100	0.099	AG211003	0.099	0.099	0.099	0.099	0.099	0.099	+/- 0.004	
0.150	0.148	AG332004	0.146	0.146	0.146	0.146	0.146	0.146	+/- 0.005	
0.300	0.297	AG327804	0.298	0.297	0.297	0.297	0.297	0.297	+/- 0.011	

As Left Conditions - Barometric Pressure (inHg): 29.60 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.4 Relative Humidity (%): 25  
 As-Left Lab Activity Date Range: 03/28/2024 - 03/29/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Carlie Glaister on 03/29/2024

[carlie.glaister@alaska.gov](mailto:carlie.glaister@alaska.gov)

Technically and administratively reviewed by Brandi Barnett on 04/25/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100695 Analyst or Technician Name: Megan C.  
DataMaster DMT Calibration Start Date: 3/28/24 Supervised by Carlie Glaister

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 230307229  
Calibration Due Date: 5/2/2025
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.60 Temperature(C) 20.4 Relative Humidity(%) 25  
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20240214COR Expiration Date: 5/14/24  
Simulator S/N: SD1098 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240214COR Expiration Date: 5/14/24  
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 22HP41201 Expiration Date: 8/24/24  
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106  
Calibration Due Date: 8/19/2025

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 3/28/24 MNC 3/29/2024 (if applicable)  
Data Interpretation Date (Technician): 3/29/2024 supervised by CKG  
Data Interpretation Date (Analyst): 3/29/2024 supervised by CKG

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100695  
-----

Date: 03/28/2024  
Time: 09:15:34

VERSIONS  
DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 46.4°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.76 V PASSED  
(1.07 V - 2.51 V)  
Cooler Voltage = 1.79 V PASSED  
(1.07 V - 2.51 V)  
Bias Voltage = 79 V PASSED  
(48 V - 112 V)  
Chopper Freq = 566 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.275 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.001 V <= 0.010 V)  
PUMP OFF PASSED  
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

PASSED  
Xq = 0.113 0.70% (0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100695  
-----

Date: 03/28/2024  
Time: 9:23 AM

Temperatures (°C)  
Sample Cell: 48.8°C  
Breath Tube: 46.1°C

Current Barometer 29.6 in  
Volume (Ltr) 1.58

Settings  
Lamp: 1.76 V  
Bias: 79 V  
Cooler: 1.90 V  
Chopper: 565 Hz

Voltages (V)  
Flow: 1.04 V  
Detector: -0.014 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100695  
-----

Date: 11/07/2023  
Time: 08:48:24

OPERATOR NAME:  
CARLIE GLAISTER  
CERTIFICATE #: 10436

Ca = 0.1000  
CAL = 0.980197    0.800 <= CAL < 1.200  
b1 = 0.0006    0.0000 <= b1 < 0.0040  
b2 = 0.0057    0.0010 <= b2 < 0.0100  
b3 = 0.0004    0.0000 <= b3 < 0.0040  
Xq = 0.1136    0.0500 <= Xq < 0.2000  
a21 = 1.137430    1.050 <= a21 < 1.300  
a31 = 0.528219    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100695

Date: 03/28/2024

Time: 09:50:32

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CROUSE

OPERATOR'S #: 10747

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.61: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	09:51
BLANK TEST	0.000	09:51
INTERNAL STANDARD	VERIFIED	09:51
EXTERNAL STANDARD	0.078	09:52
BLANK TEST	0.000	09:52
SUBJECT SAMPLE (Vol=1.56L)	0.000	09:54
BLANK TEST	0.000	09:55
EXTERNAL STANDARD	0.079	09:55
BLANK TEST	0.000	09:56

MNC

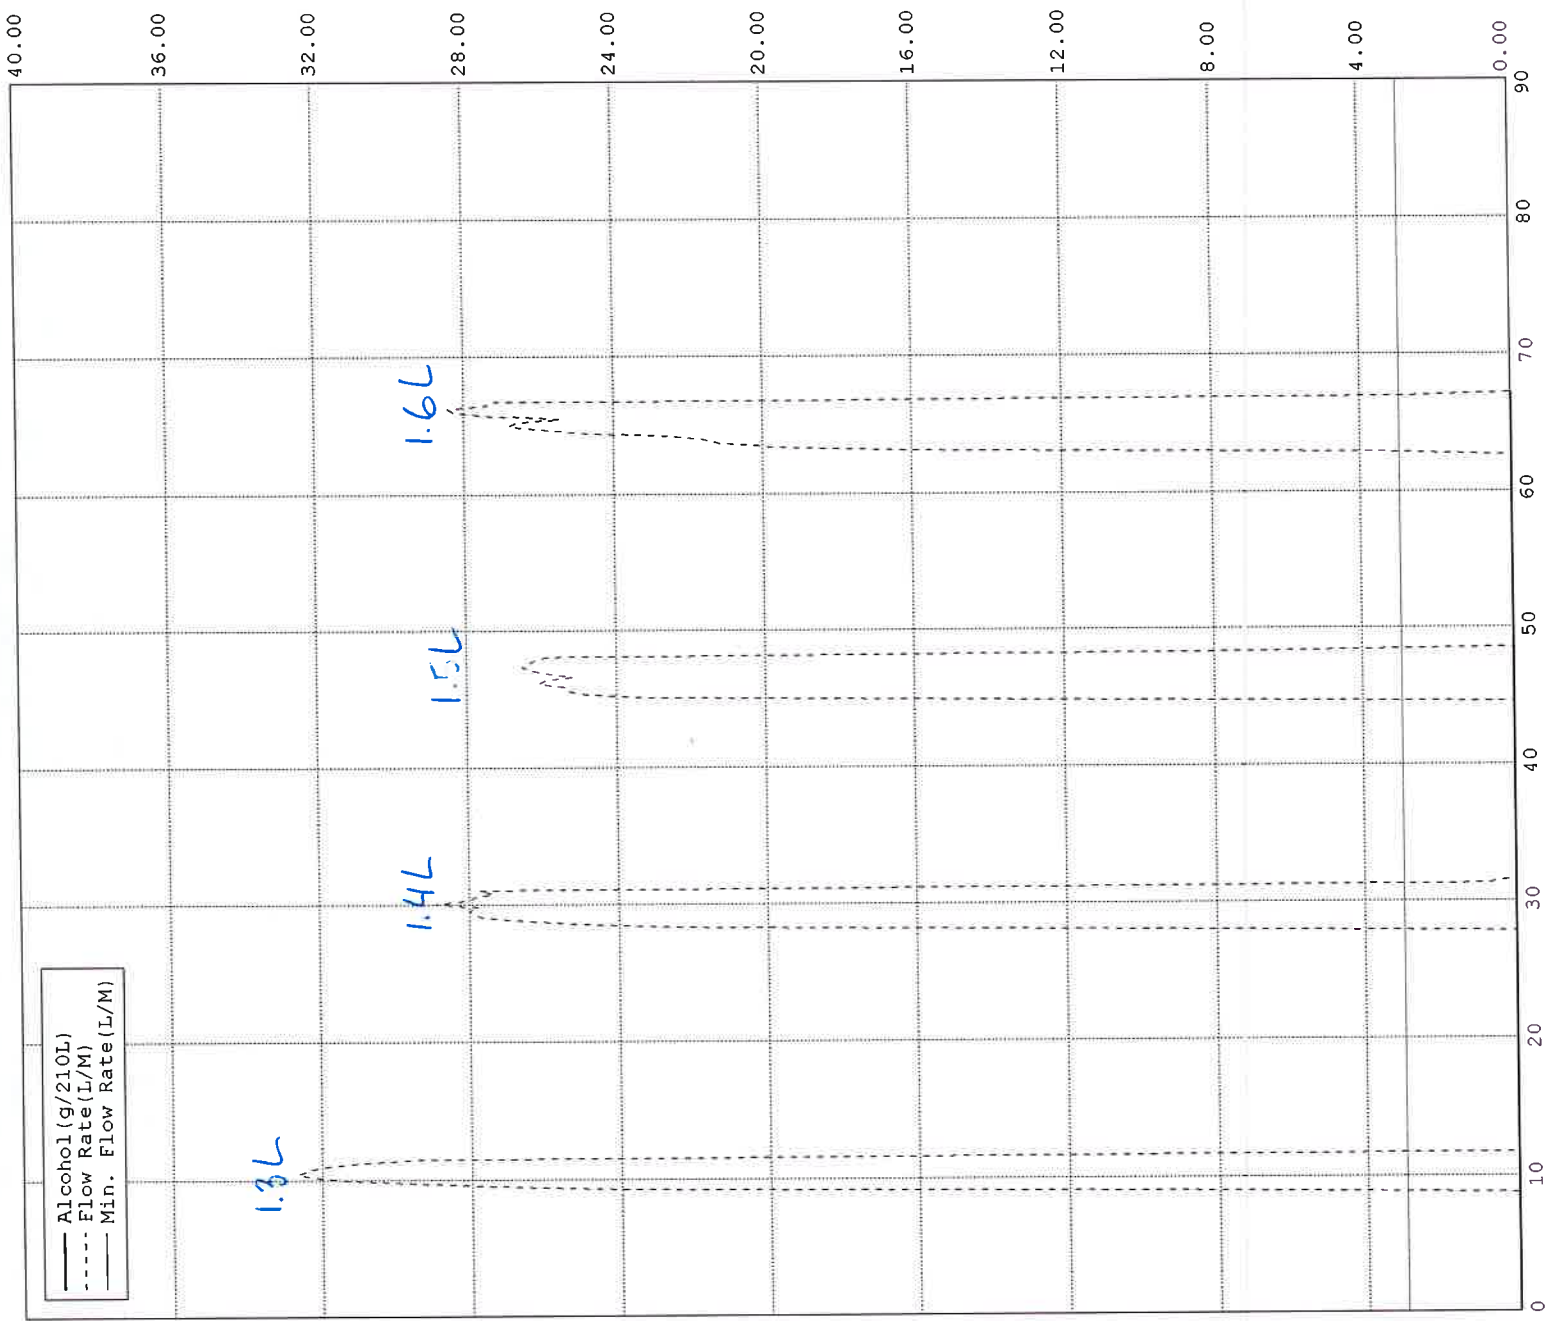

LINEARITY CHECK


Alaska Department of Public Safety  
 DATAMASTER dmt: 100695

Date: 03/28/2024  
 Time: 09:59:15

SUPERVISOR NAME:  
 MEGAN CROUSE  
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.040	0.0400	0.0000
0.079	0.0788	0.0004
0.099	0.0990	0.0000
0.148	0.1460	0.0000
0.297	0.2972	0.0004

SLOPE = 0.999509  
 R<sup>2</sup> = 0.999932

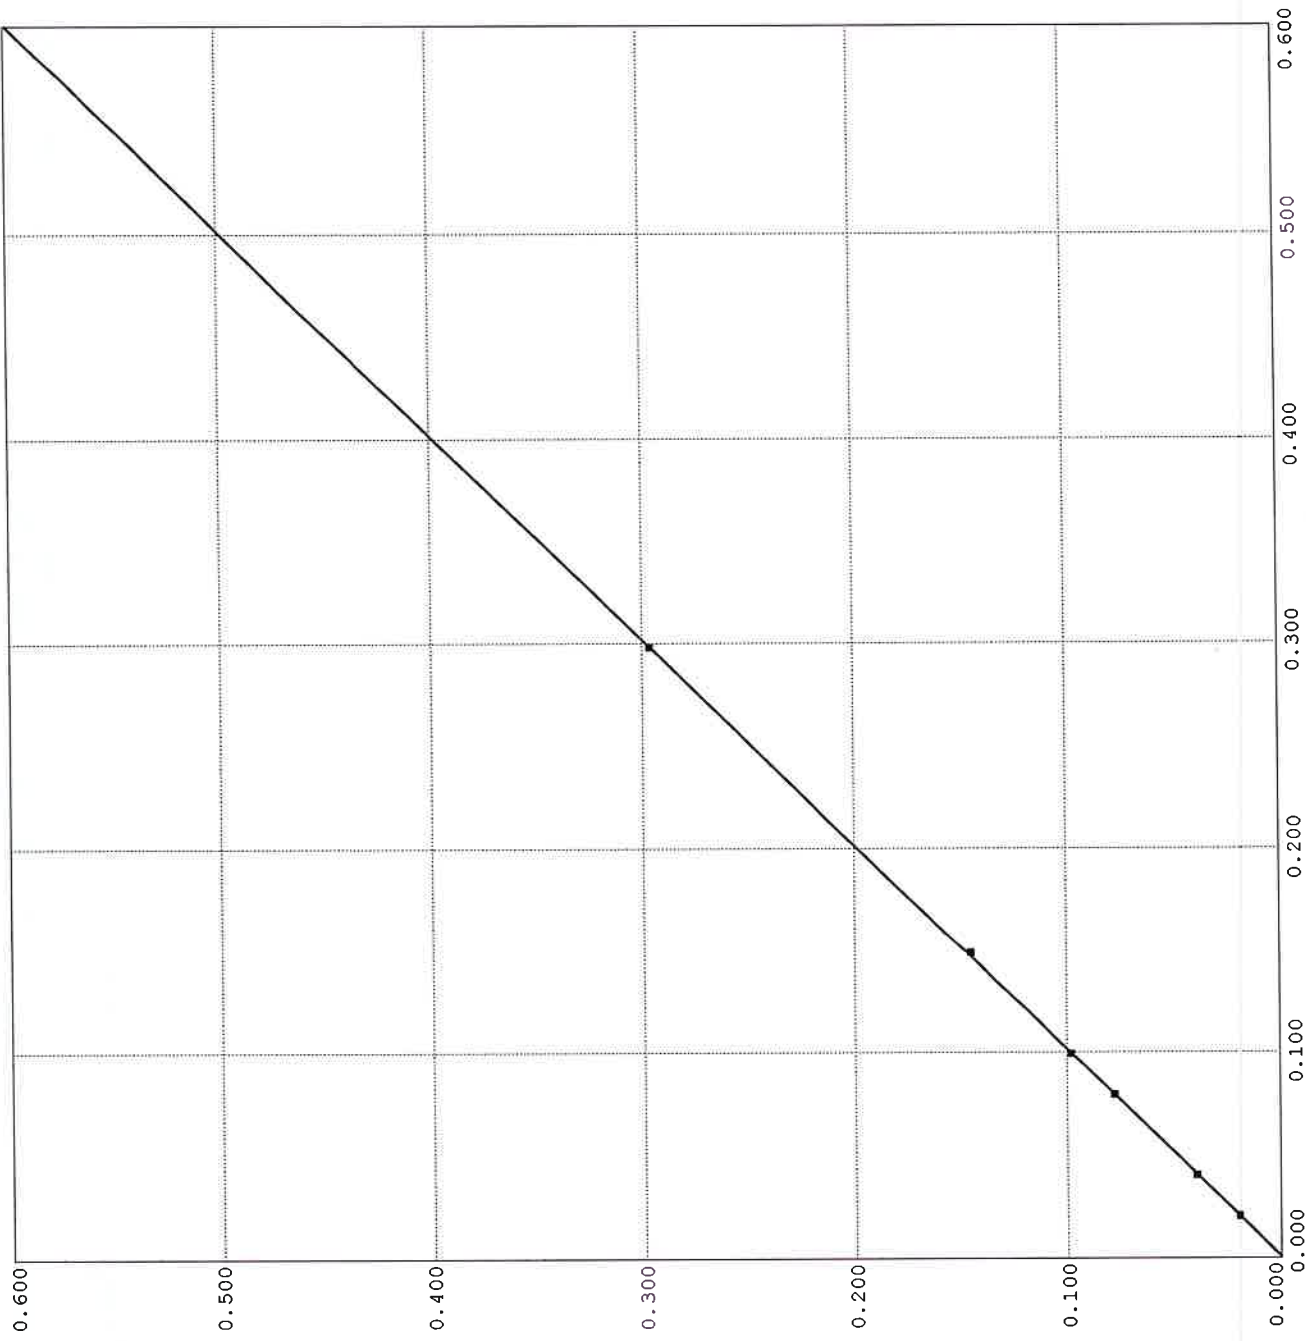

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100695






Date: 03/28/2024  
Time: 09:59:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.61: 0.020  
LOT #: AG217902  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 192 psi

BLANK TEST	0.000	10:00
INTERNAL STANDARD	VERIFIED	10:00
EXTERNAL STANDARD	0.020	10:01
BLANK TEST	0.000	10:01
EXTERNAL STANDARD	0.020	10:02
BLANK TEST	0.000	10:03
EXTERNAL STANDARD	0.020	10:03
BLANK TEST	0.000	10:04
EXTERNAL STANDARD	0.020	10:04
BLANK TEST	0.000	10:05
EXTERNAL STANDARD	0.020	10:05
BLANK TEST	0.000	10:06

Average = 0.0200  
Std Dev = 0.0000

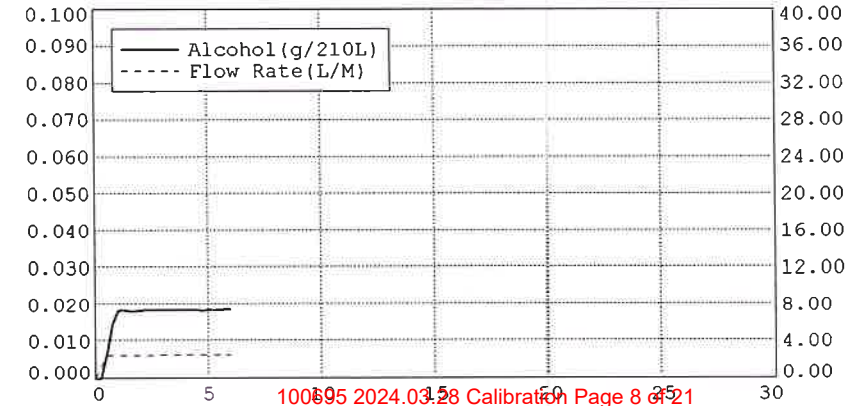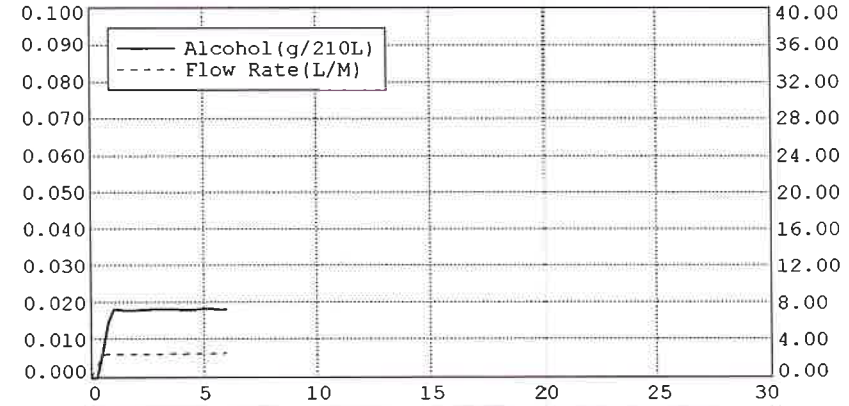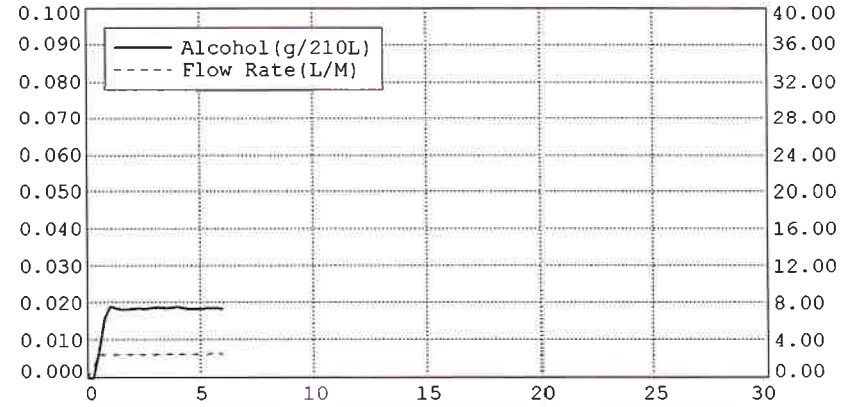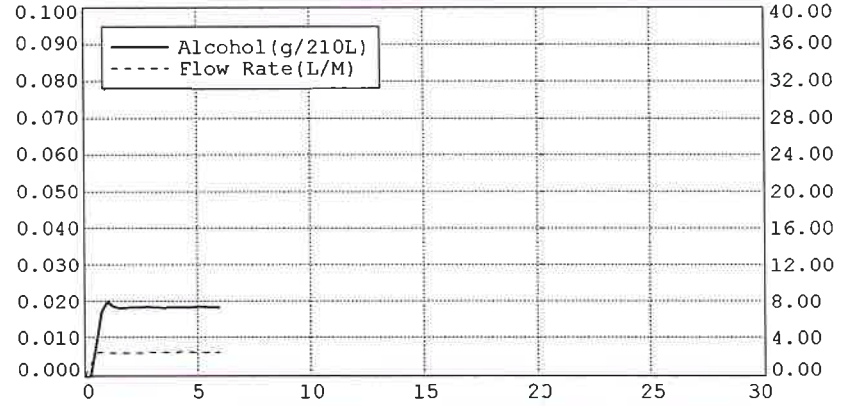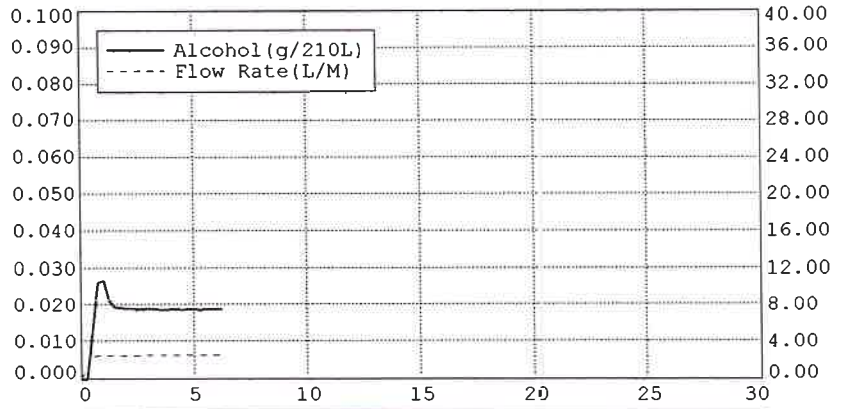



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100695






Date: 03/28/2024  
 Time: 10:08:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.61: 0.040  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 816 psi

BLANK TEST	0.000	10:09
INTERNAL STANDARD	VERIFIED	10:09
EXTERNAL STANDARD	0.040	10:09
BLANK TEST	0.000	10:10
EXTERNAL STANDARD	0.040	10:10
BLANK TEST	0.000	10:11
EXTERNAL STANDARD	0.040	10:11
BLANK TEST	0.000	10:12
EXTERNAL STANDARD	0.040	10:12
BLANK TEST	0.000	10:13
EXTERNAL STANDARD	0.040	10:13
BLANK TEST	0.000	10:14

Average = 0.0400  
 Std Dev = 0.0000

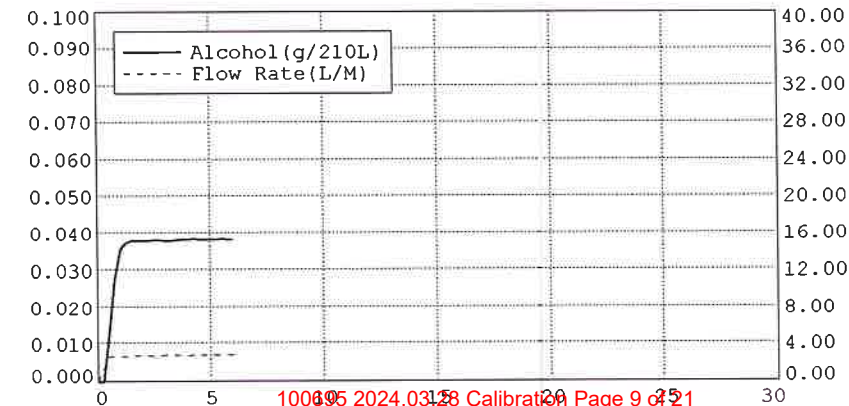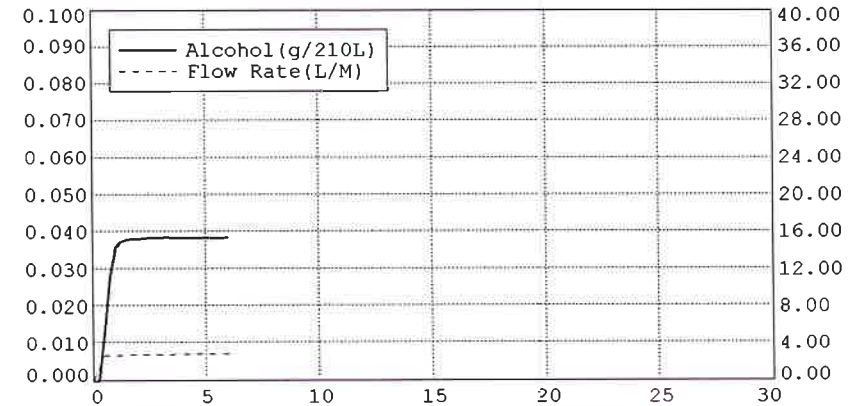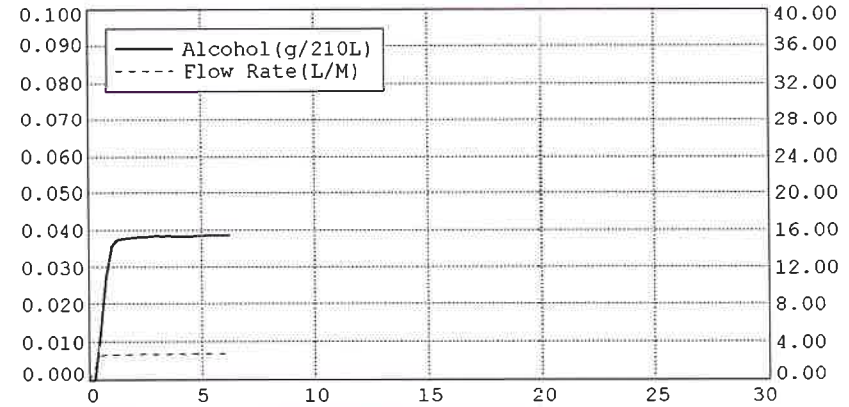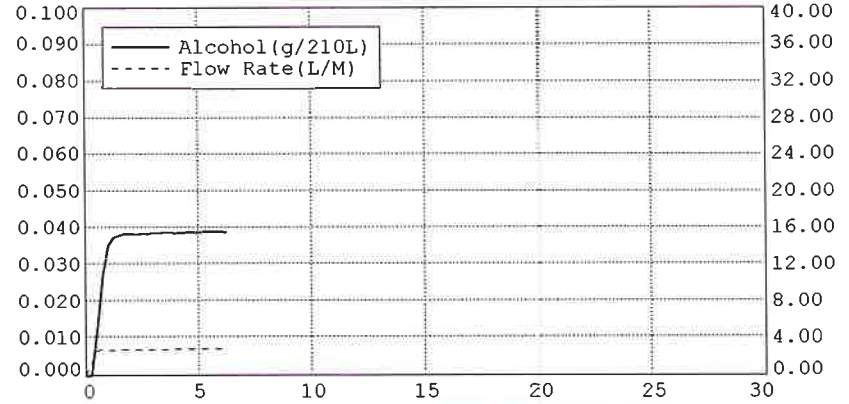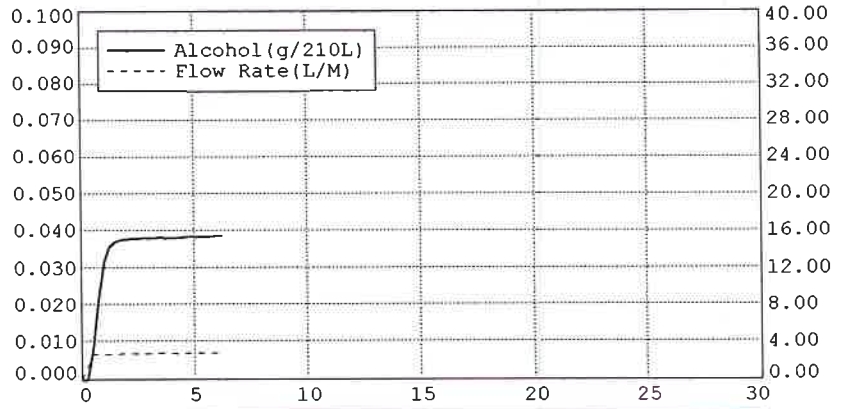

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
DATAMASTER dmt: 100695






Date: 03/28/2024  
Time: 10:16:10

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.61: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025  
TANK PRESSURE: 140 psi

BLANK TEST	0.000	10:17
INTERNAL STANDARD	VERIFIED	10:17
EXTERNAL STANDARD	0.079	10:17
BLANK TEST	0.000	10:18
EXTERNAL STANDARD	0.079	10:18
BLANK TEST	0.000	10:19
EXTERNAL STANDARD	0.079	10:19
BLANK TEST	0.000	10:20
EXTERNAL STANDARD	0.079	10:20
BLANK TEST	0.000	10:21
EXTERNAL STANDARD	0.078	10:22
BLANK TEST	0.000	10:22

Average = 0.0788  
Std Dev = 0.0004

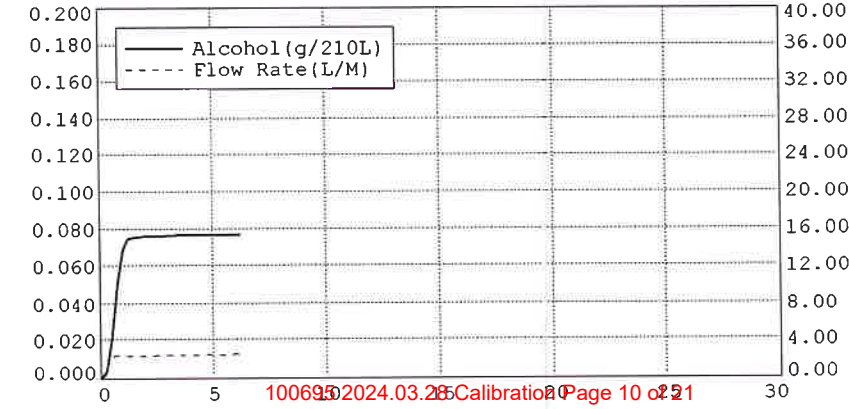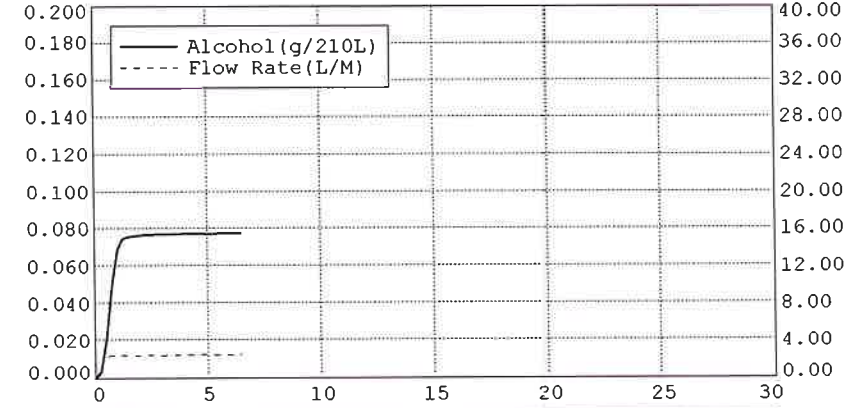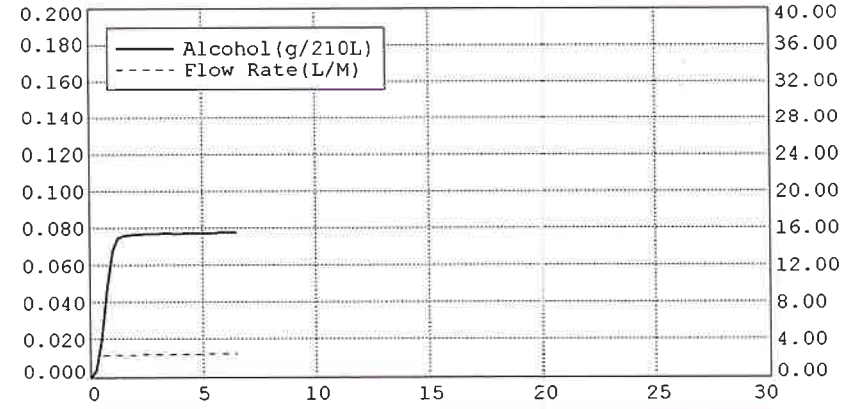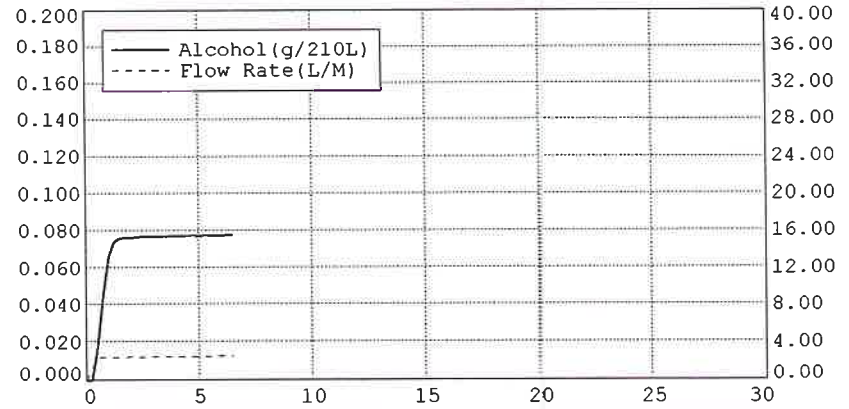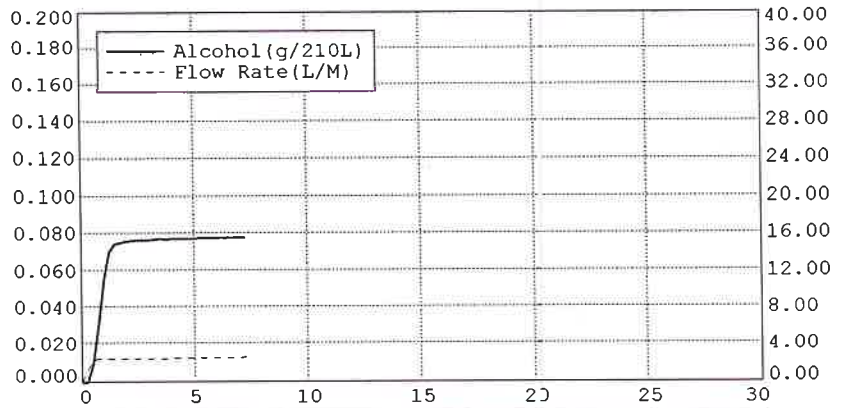

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
DATAMASTER dmt: 100695






Date: 03/28/2024  
Time: 10:24:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
TARGET AT 29.61: 0.099  
LOT #: AG211003  
EXPIRATION: 04/20/2024  
TANK PRESSURE: 397 psi

BLANK TEST	0.000	10:26
INTERNAL STANDARD	VERIFIED	10:26
EXTERNAL STANDARD	0.099	10:26
BLANK TEST	0.000	10:27
EXTERNAL STANDARD	0.099	10:27
BLANK TEST	0.000	10:28
EXTERNAL STANDARD	0.099	10:28
BLANK TEST	0.000	10:29
EXTERNAL STANDARD	0.099	10:29
BLANK TEST	0.000	10:30
EXTERNAL STANDARD	0.099	10:30
BLANK TEST	0.000	10:31

Average = 0.0990  
Std Dev = 0.0000

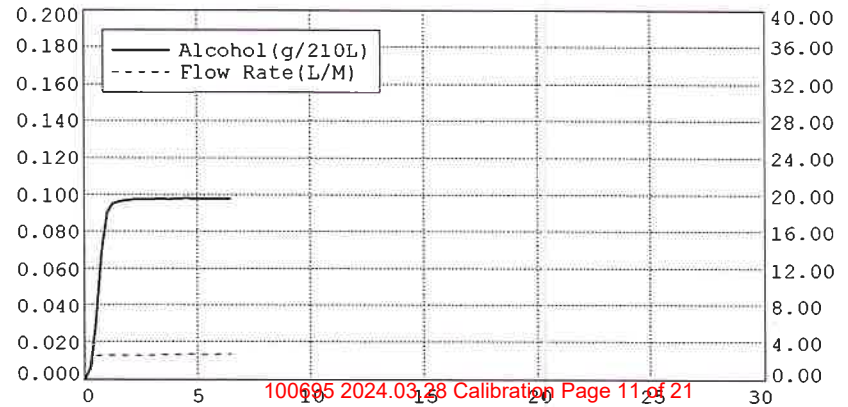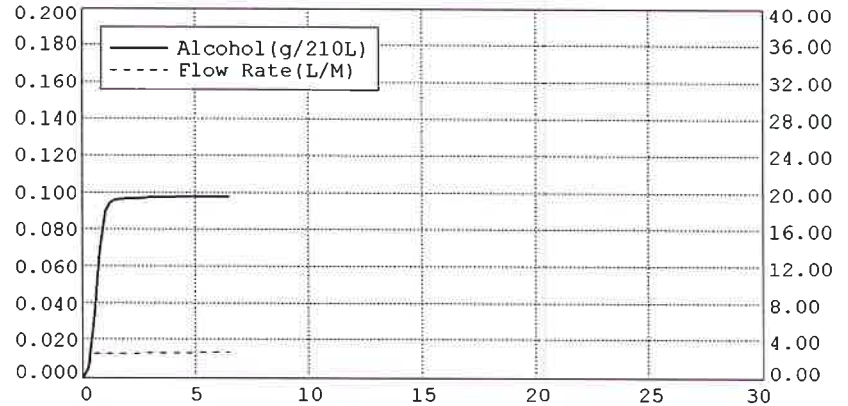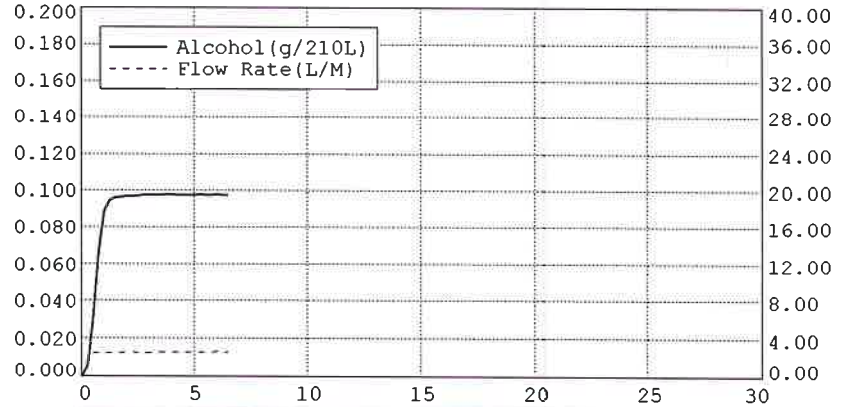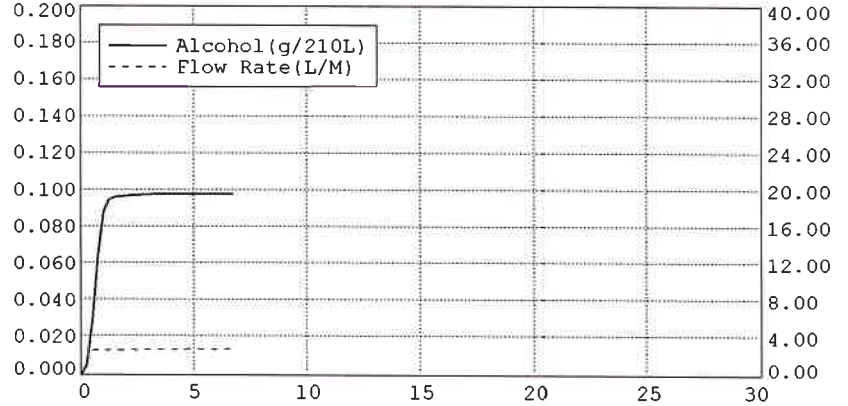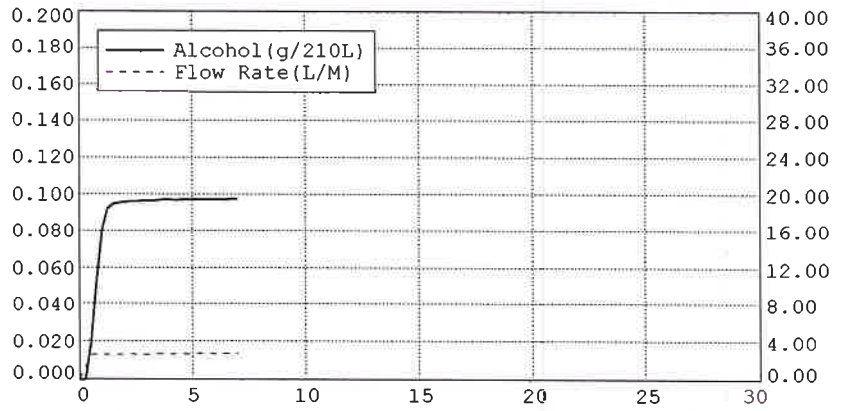

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100695






Date: 03/28/2024  
 Time: 10:38:42

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.61: 0.148  
 LOT #: AG332004  
 EXPIRATION: 11/16/2025  
 TANK PRESSURE: 611 psi

BLANK TEST	0.000	10:39
INTERNAL STANDARD	VERIFIED	10:39
EXTERNAL STANDARD	0.146	10:40
BLANK TEST	0.000	10:41
EXTERNAL STANDARD	0.146	10:41
BLANK TEST	0.000	10:42
EXTERNAL STANDARD	0.146	10:42
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.146	10:43
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.146	10:44
BLANK TEST	0.000	10:45

Average = 0.1460  
 Std Dev = 0.0000

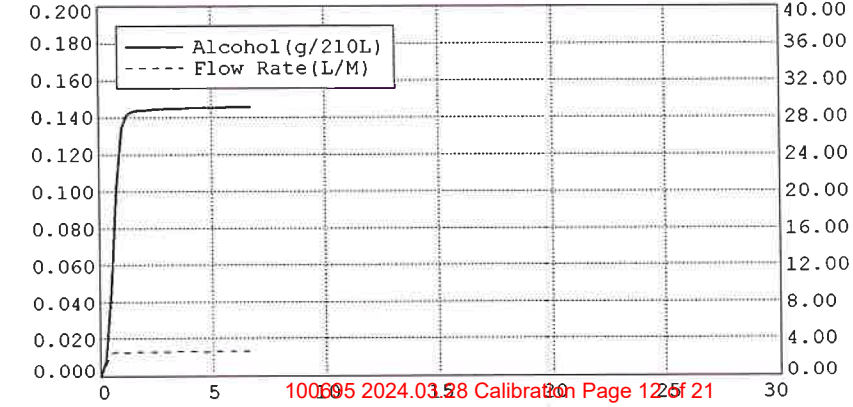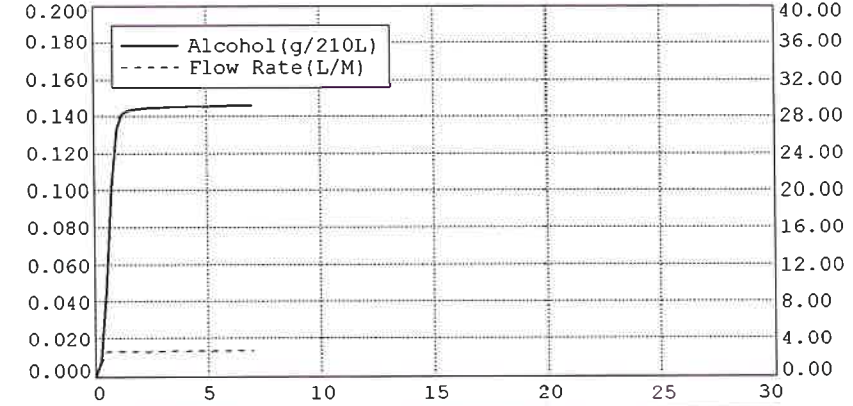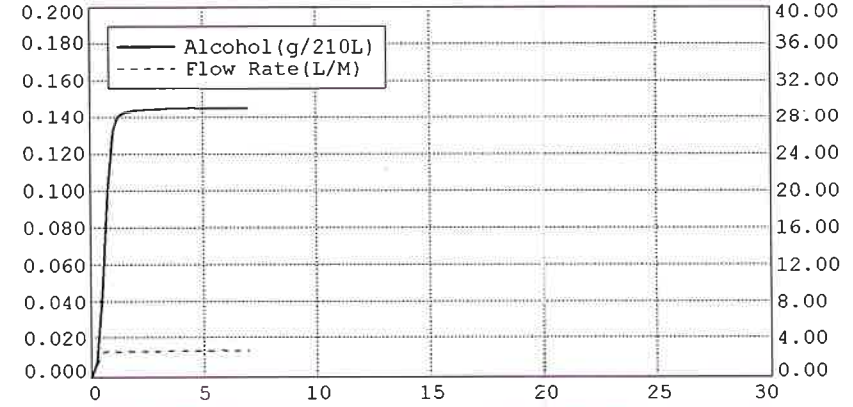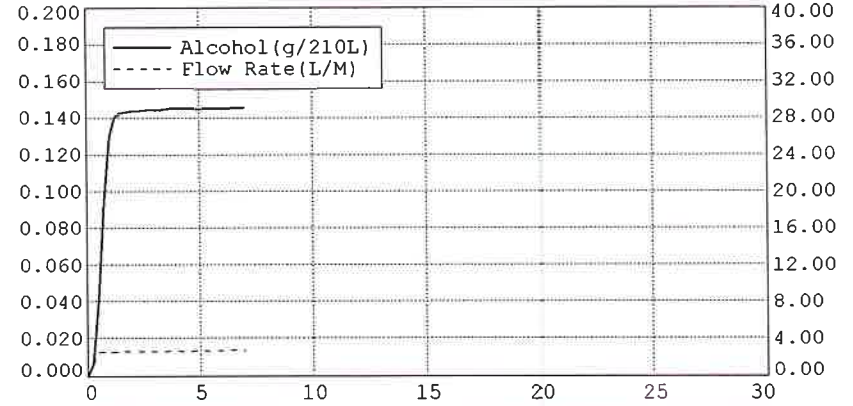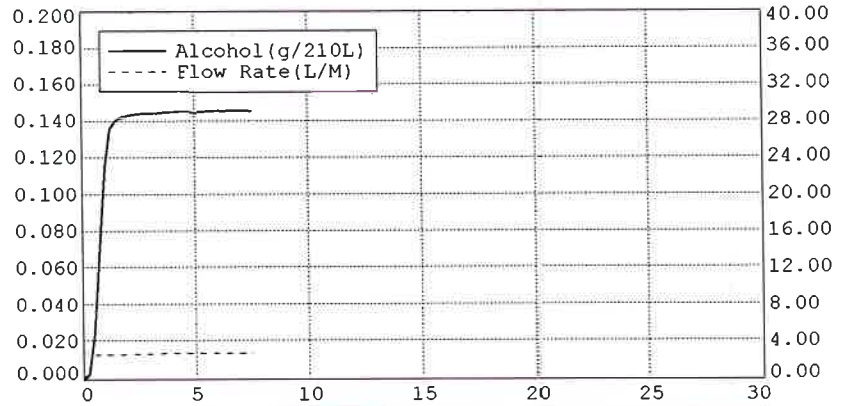

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100695






Date: 03/28/2024  
 Time: 10:53:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.61: 0.297  
 LOT #: AG327804  
 EXPIRATION: 10/05/2025  
 TANK PRESSURE: 266 psi

BLANK TEST	0.000	10:54
INTERNAL STANDARD	VERIFIED	10:54
EXTERNAL STANDARD	0.298	10:55
BLANK TEST	0.000	10:56
EXTERNAL STANDARD	0.297	10:56
BLANK TEST	0.000	10:57
EXTERNAL STANDARD	0.297	10:57
BLANK TEST	0.000	10:58
EXTERNAL STANDARD	0.297	10:58
BLANK TEST	0.000	10:59
EXTERNAL STANDARD	0.297	10:59
BLANK TEST	0.000	11:00

Average = 0.2972  
 Std Dev = 0.0004

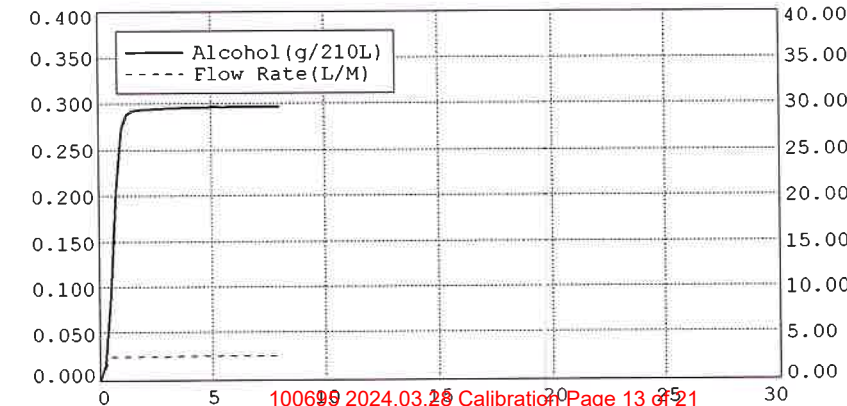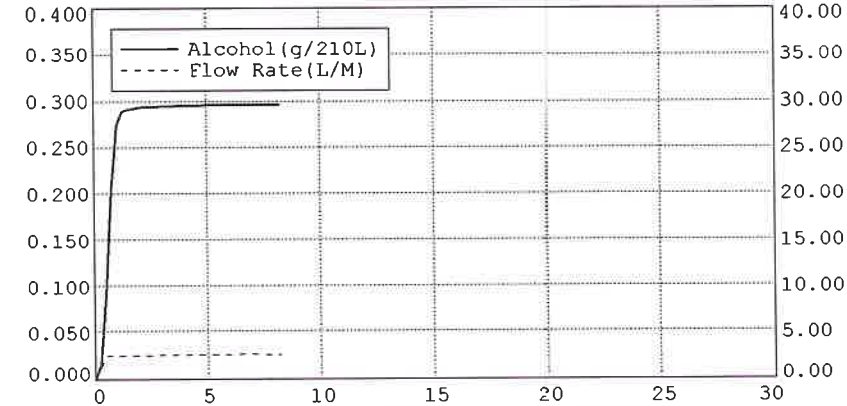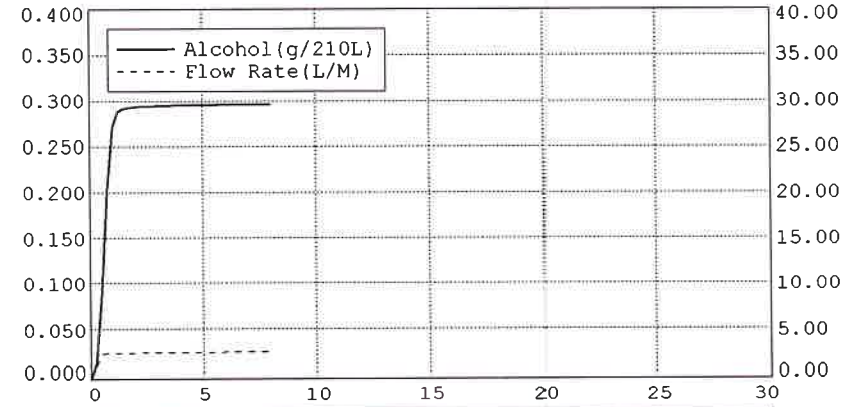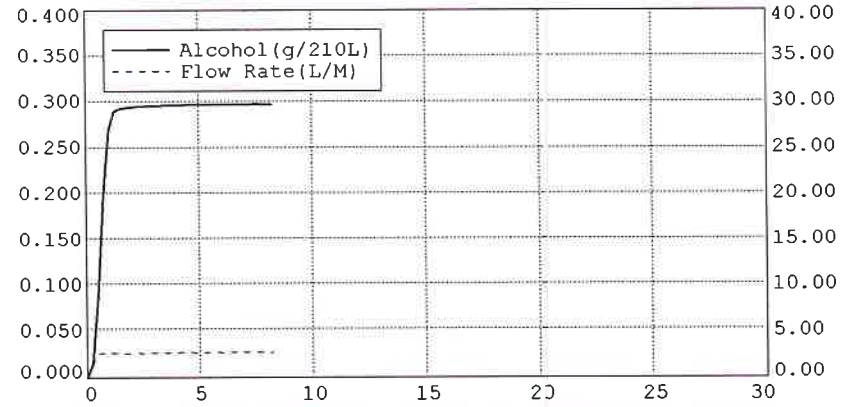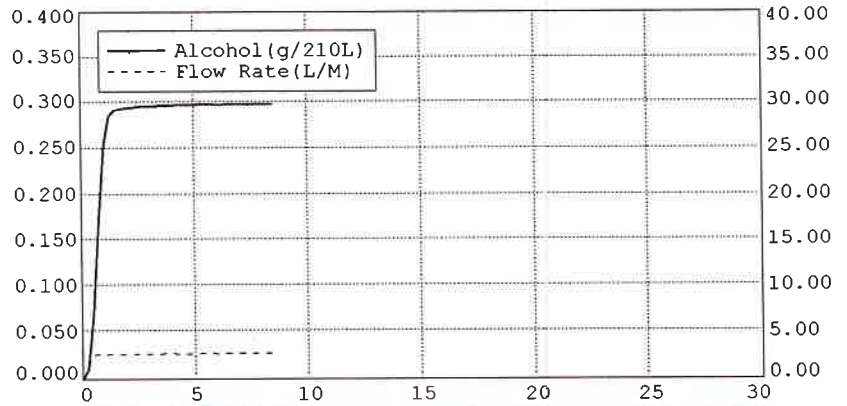

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100695

Date: 03/28/2024

Time: 11:04:24

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CROUSE

OPERATOR'S #: 10747

DEPT/AGENCY:

INCOMPLETE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.62: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 11:05  
0.000 11:05  
VERIFIED 11:06  
0.080 11:06  
0.000 11:07  
INCOMPLETE 11:09

MJC



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100695

Date: 03/28/2024  
Time: 11:25:53

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CROUSE  
OPERATOR'S #: 10747

DEPT/AGENCY:  
MAXIMUM ATTEMPTS EXCEEDED  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.62: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 11:26  
BLANK TEST 0.000 11:26  
INTERNAL STANDARD VERIFIED 11:27  
EXTERNAL STANDARD 0.079 11:27  
BLANK TEST 0.000 11:28  
SUBJECT SAMPLE XXX 11:28

Maximum Attempts Exceeded

Performed after invalid test,  
residual mouthwash in mouth.  
MNC 3/29/24 GMM-329124

MNC

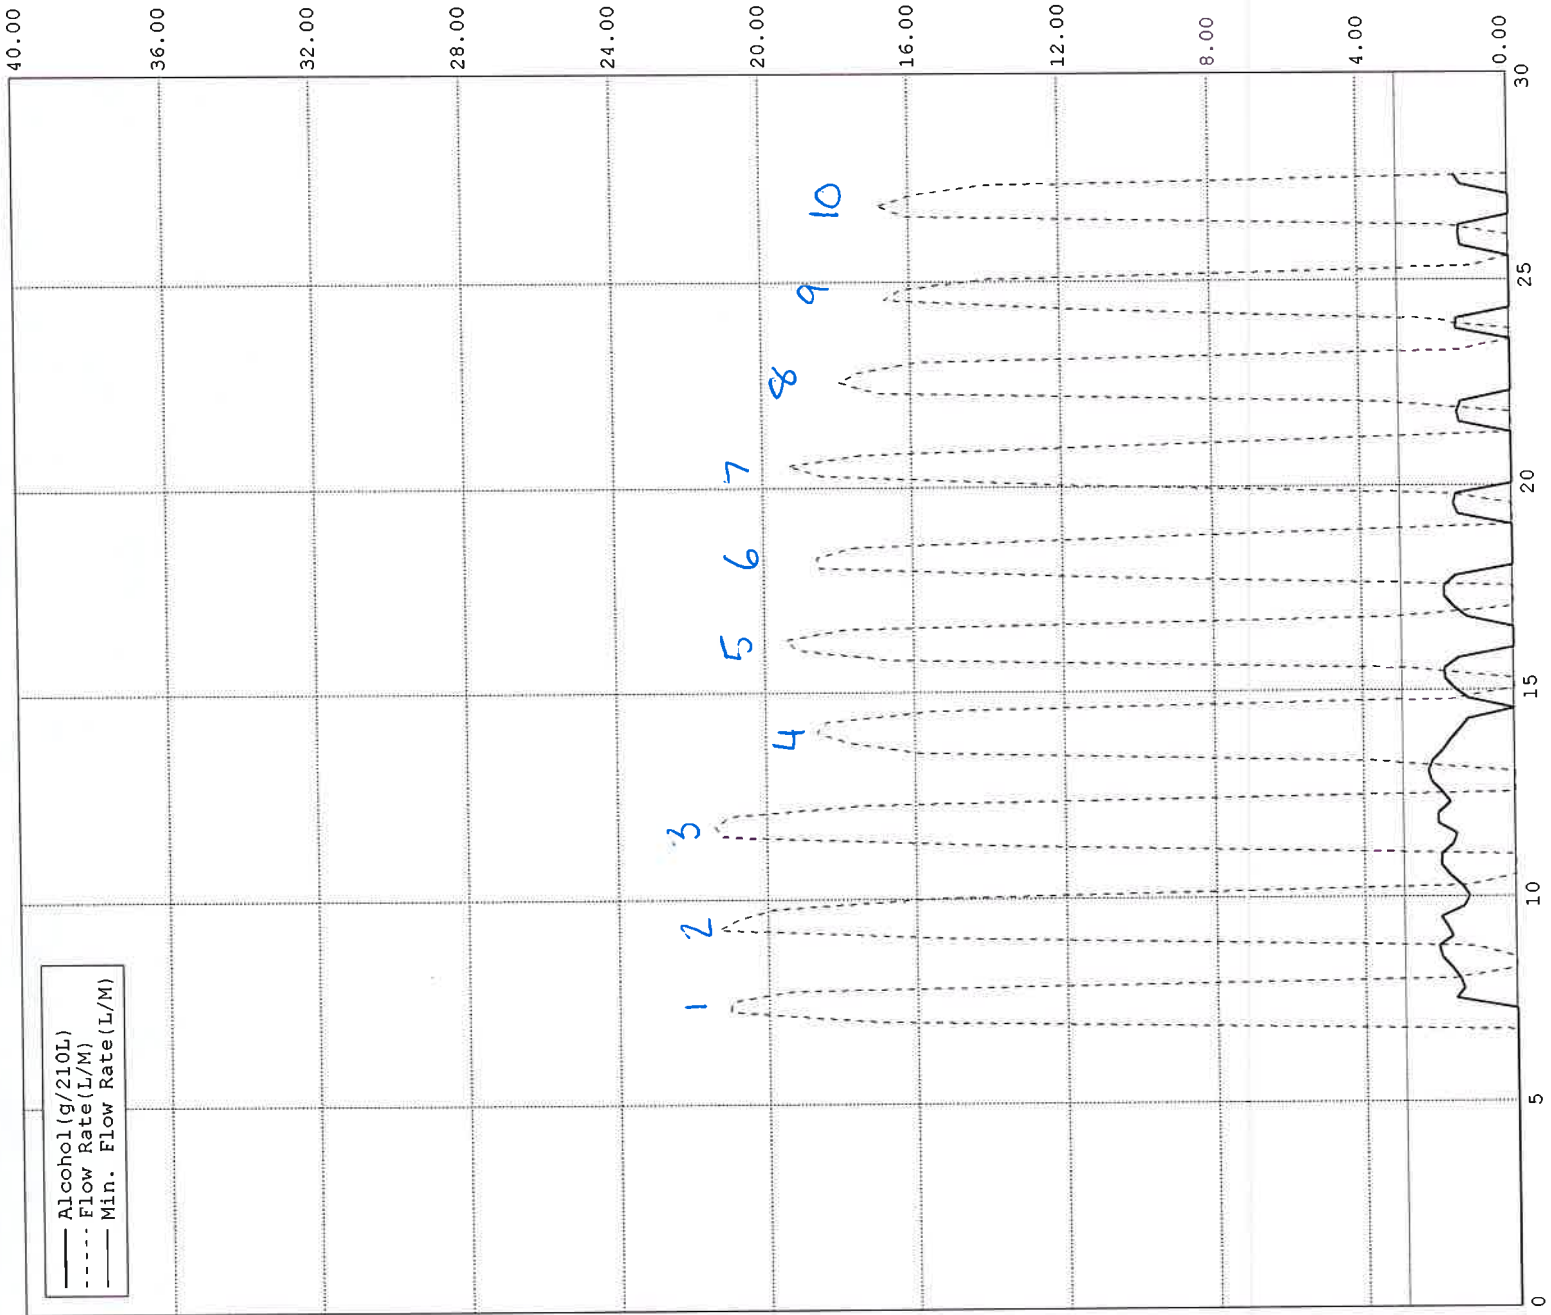

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100695

Date: 03/28/2024

Time: 11:13:59

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CROUSE

OPERATOR'S #: 10747

DEPT/AGENCY:

INVALID

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.62: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD


BLANK TEST

SUBJECT SAMPLE

PASSED 11:15  
0.000 11:15  
VERIFIED 11:15  
0.079 11:16  
0.000 11:17  
INVALID 11:17

MWC

Alcohol (g/210L)  
Flow Rate (L/M)  
Min. Flow Rate (L/M)

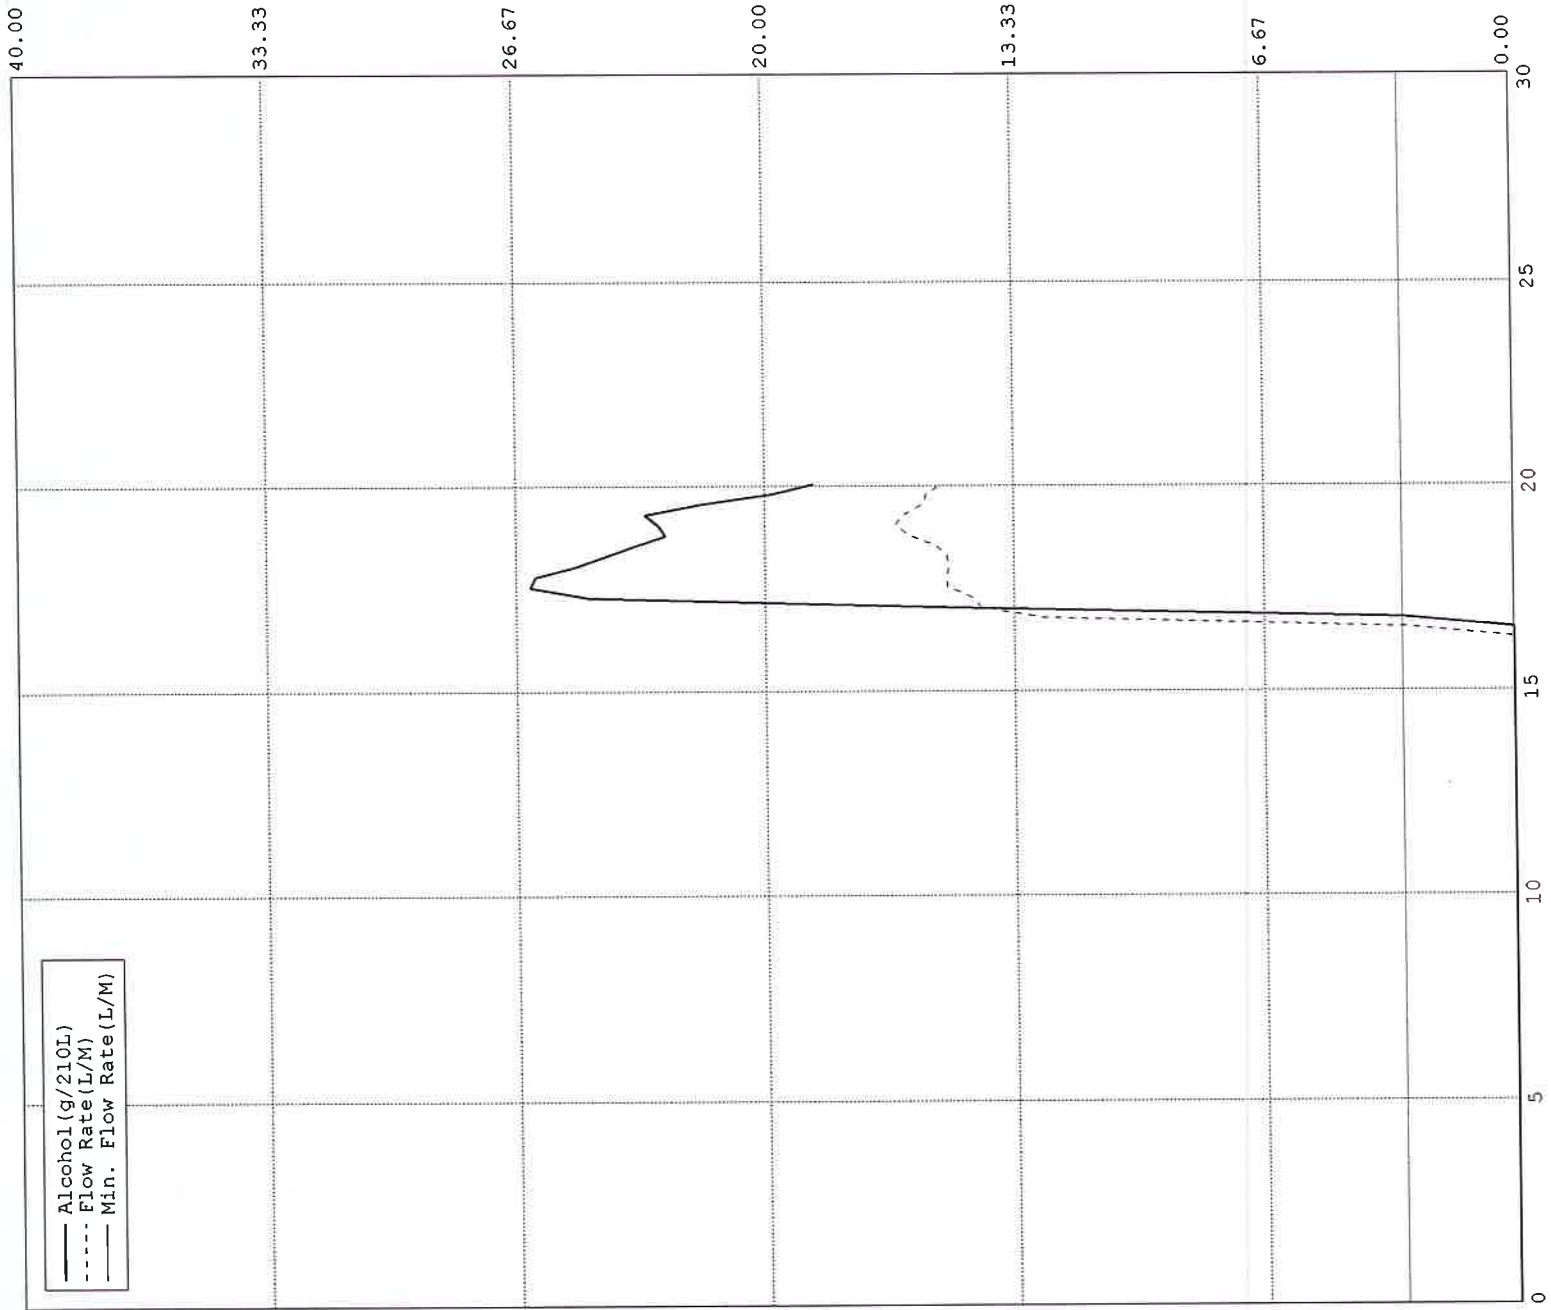



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100695

Date: 03/28/2024  
Time: 11:19:05

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CROUSE  
OPERATOR'S #: 10747


DEPT/AGENCY:  
RFI  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.61: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 11:20  
BLANK TEST 0.000 11:20  
INTERNAL STANDARD VERIFIED 11:20  
EXTERNAL STANDARD 0.079 11:20  
BLANK TEST 0.000 11:21

RFI DETECTED

MJC

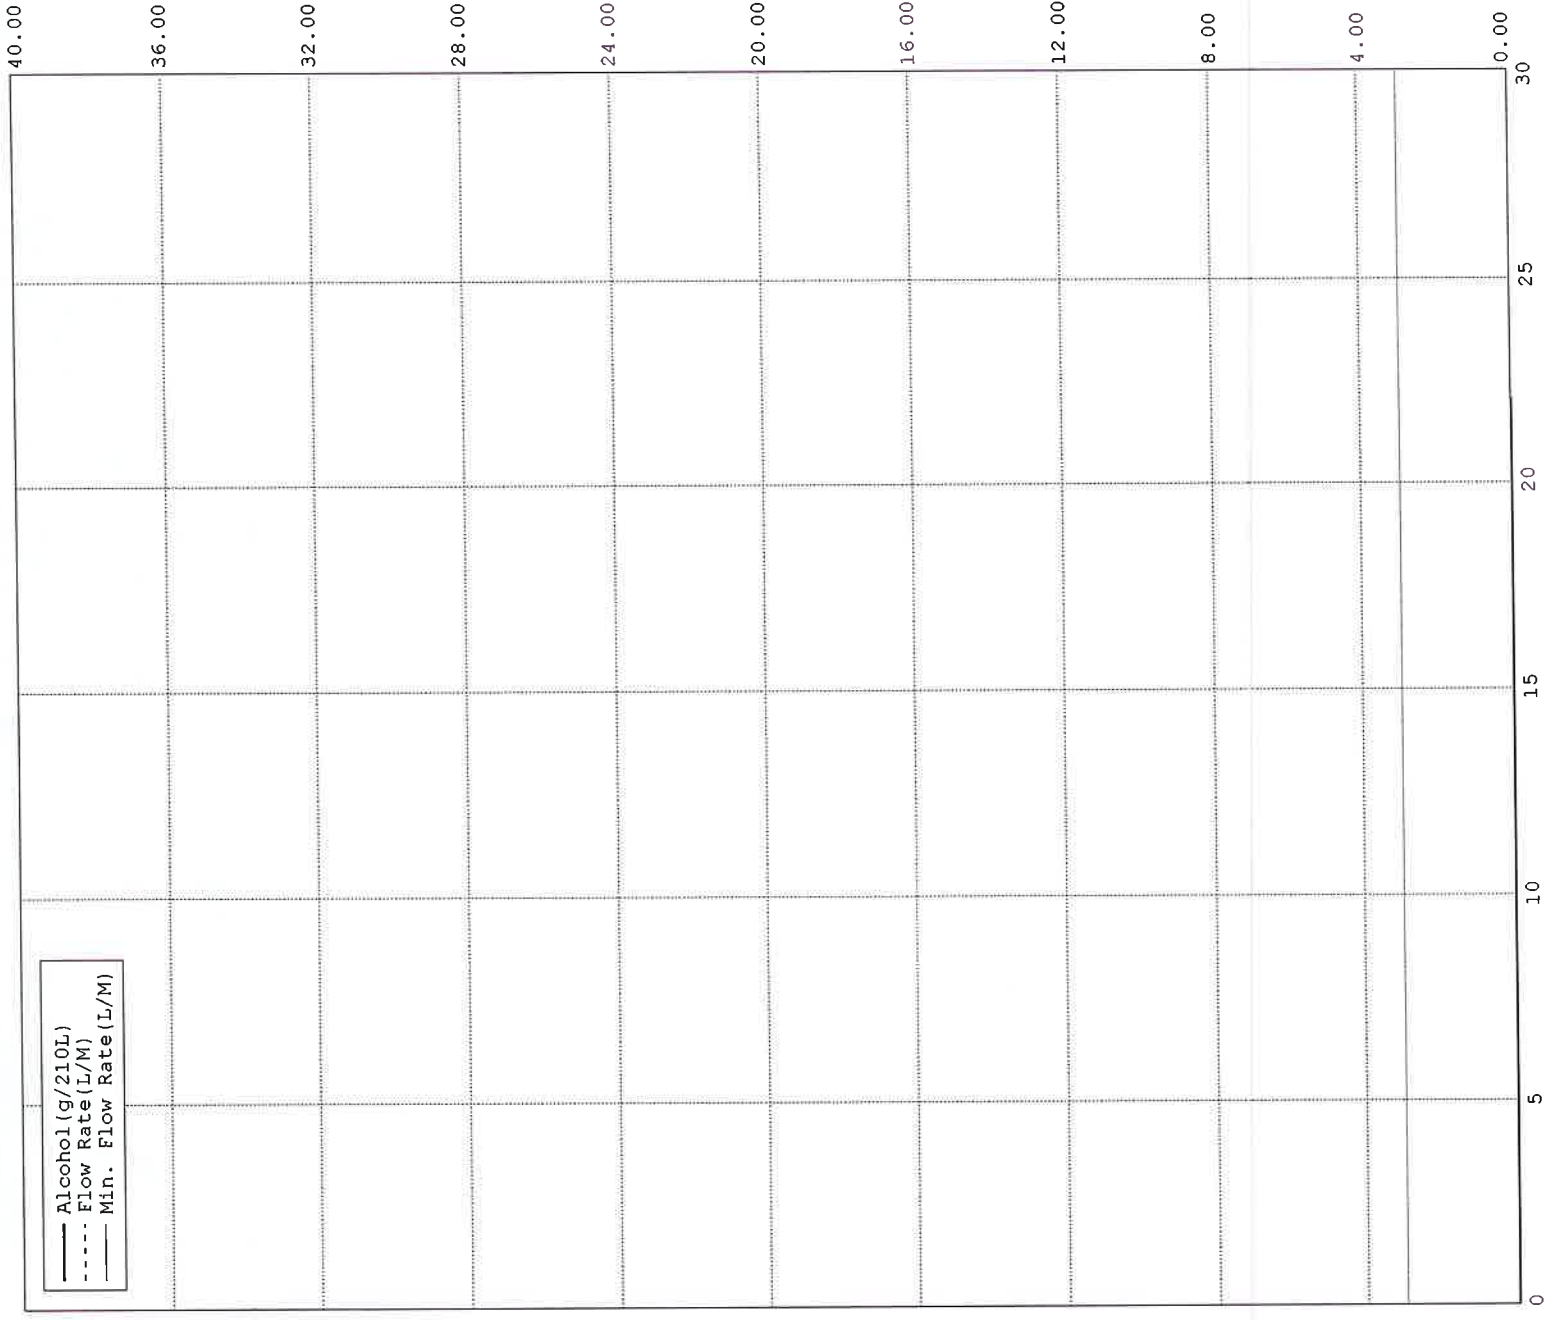

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100695

Date: 03/28/2024  
Time: 13:23:16

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CROUSE  
OPERATOR'S #: 10747

DEPT/AGENCY:  
INTERFERENCE - ACETONE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.62: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025


DIAGNOSTIC CHECK PASSED 13:24  
BLANK TEST 0.000 13:24  
INTERNAL STANDARD VERIFIED 13:24  
Xg = 0.113 (0.78%)  
EXTERNAL STANDARD 0.079 13:24  
X[1] = 0.0787 (-0.0021) (0.0017)  
BLANK TEST 0.000 13:25  
SUBJECT SAMPLE XXX 13:26  
X[1] = 0.1086 (-0.0193) (0.0007)

Interference Detected

Filter 2 Average: -0.0019 MNC 3/29/24  
Filter 3 Average: 0.0019

*Handwritten initials/signature*

MNC

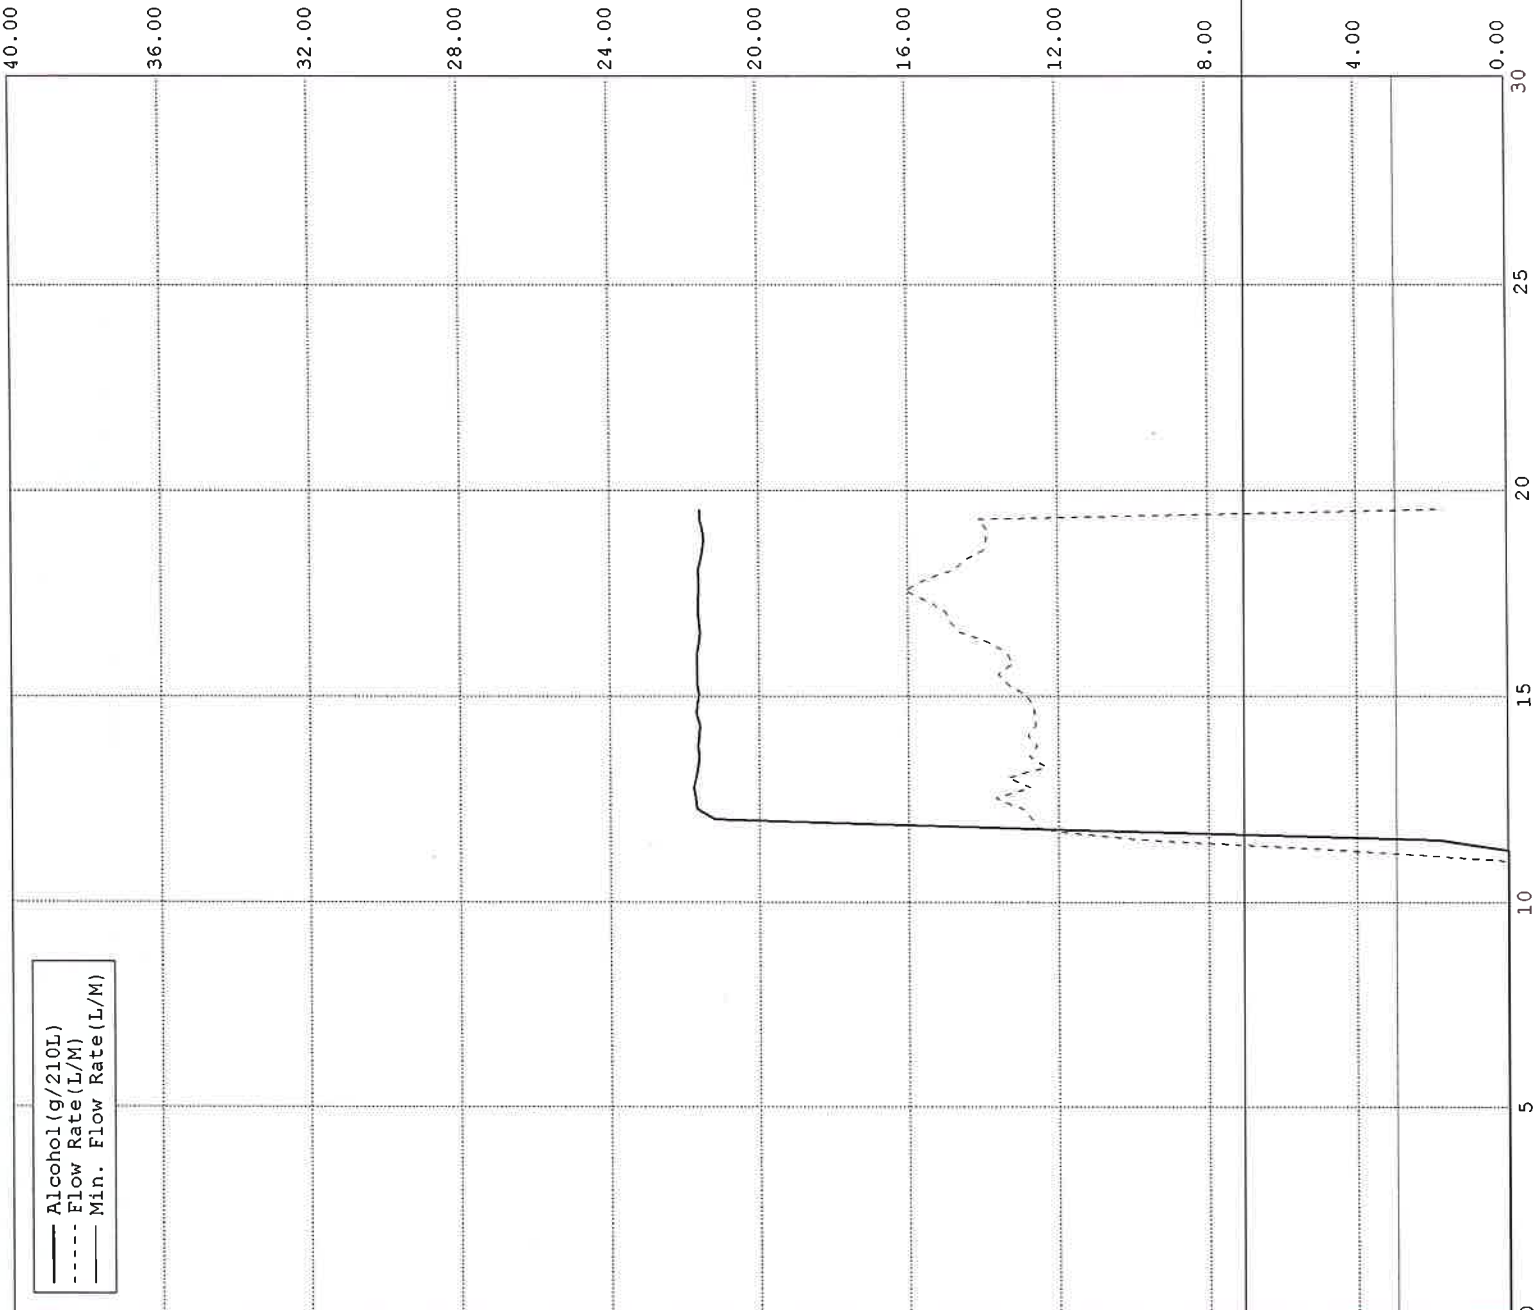

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100695

Date: 03/28/2024  
Time: 13:47:11

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CROUSE  
OPERATOR'S #: 10747

DEPT/AGENCY:  
INTERFERENCE - IPA  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.62: 0.079  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	13:48
BLANK TEST	0.000	13:48
INTERNAL STANDARD	VERIFIED	13:48
Xg = 0.113 (0.23%)		
EXTERNAL STANDARD	0.079	13:48
X[1] = 0.0793 (-0.0016) (0.0025)		
BLANK TEST	0.000	13:49
SUBJECT SAMPLE	XXX	13:50
X[1] = 0.1177 (-0.0216) (0.0010)		

Interference Detected

MNC

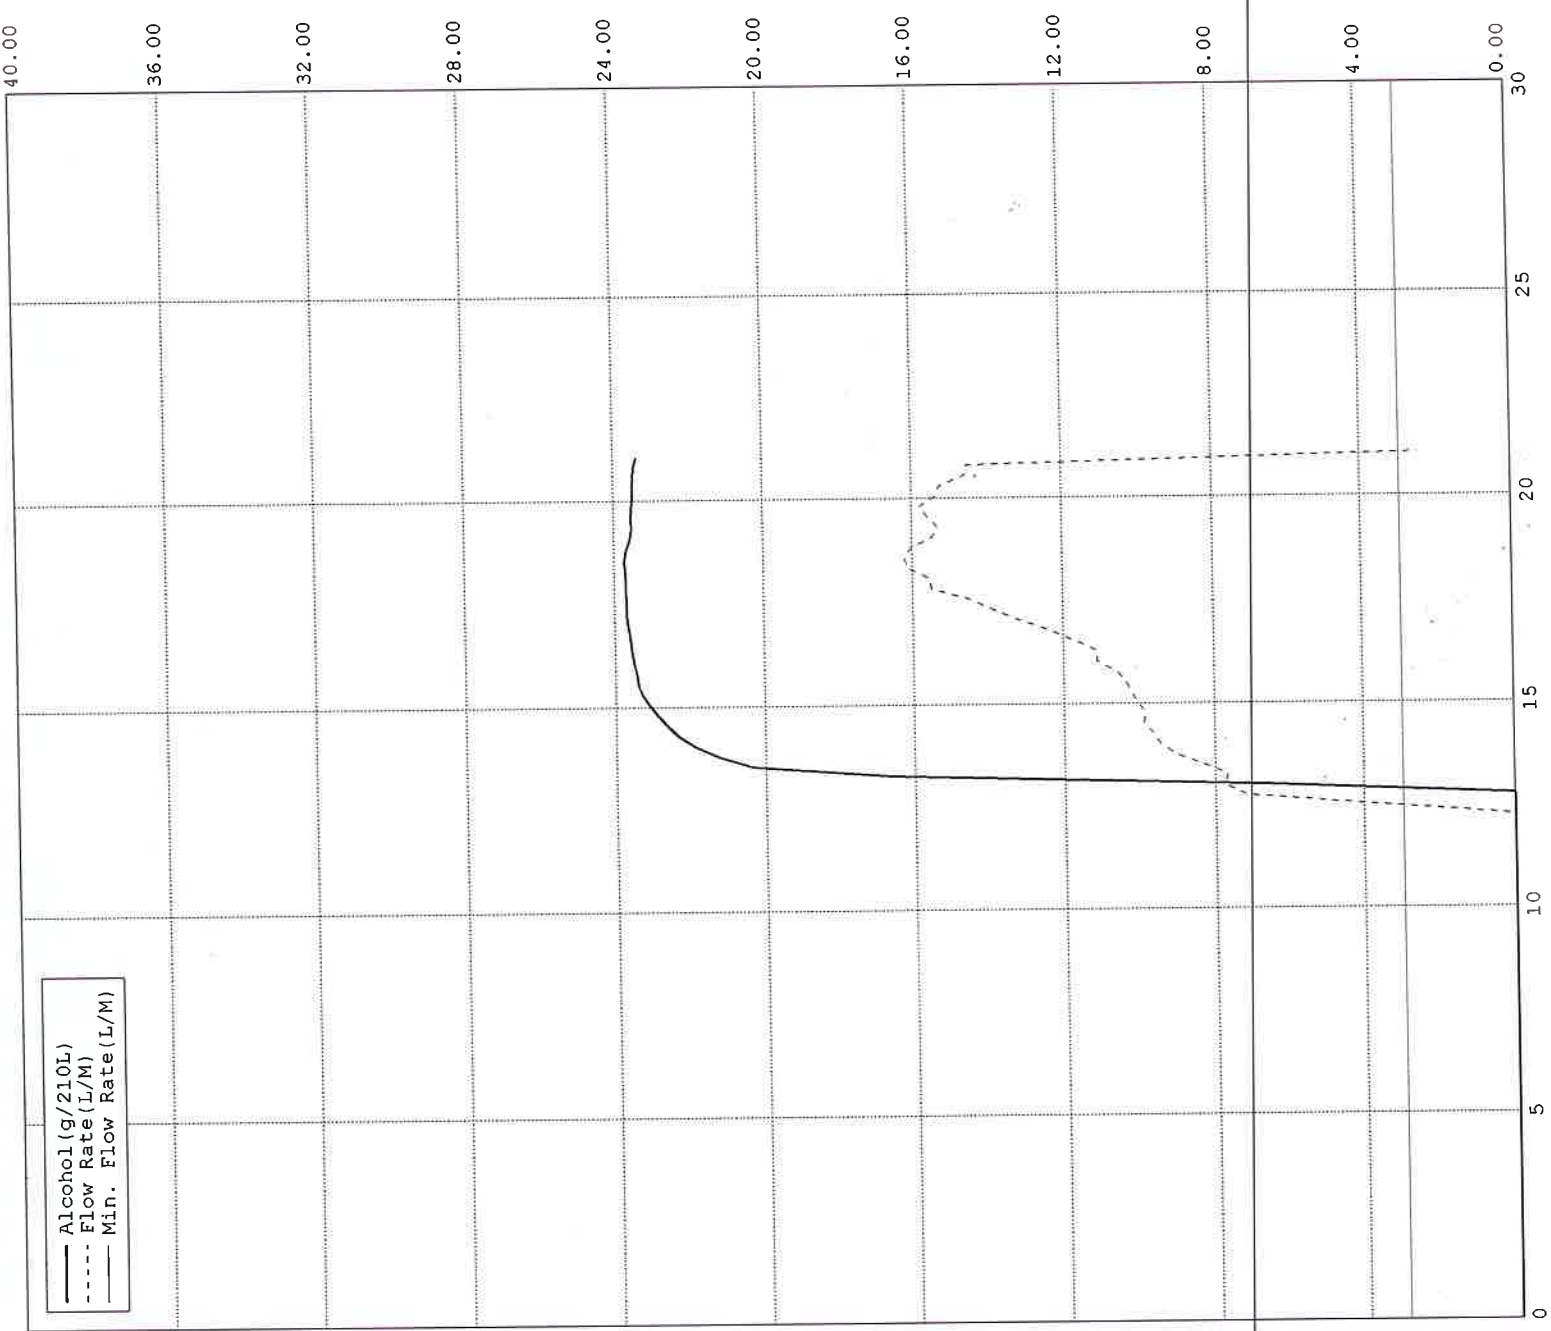

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100695

Date: 03/28/2024  
Time: 13:28:43

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CROUSE  
OPERATOR'S #: 10747

DEPT/AGENCY:  
INTERFERENCE - NEGATIVE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.63: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	13:29
BLANK TEST	0.000	13:30
INTERNAL STANDARD	VERIFIED	13:30
Xg = 0.113 (0.16%)		
EXTERNAL STANDARD	0.079	13:30
X[1] = 0.0789 (-0.0017) (0.0017)		
BLANK TEST	0.000	13:31
SUBJECT SAMPLE (Vol=2.05L)	0.093	13:31
X[1] = 0.0938 (-0.0010) (0.0000)		
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.078	13:32
X[1] = 0.0782 (-0.0020) (0.0015)		
BLANK TEST	0.000	13:33

MNC



SUBJECT TEST

Alaska Department of Public Safety  
DATA MASTER dmt: 100695

Date: 03/28/2024  
Time: 14:07:01

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
MEGAN CROUSE  
OPERATOR'S #: 10747

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.62: 0.079  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	14:08
BLANK TEST	0.000	14:08
INTERNAL STANDARD	VERIFIED	14:08
EXTERNAL STANDARD	0.079	14:08
BLANK TEST	0.000	14:09
SUBJECT SAMPLE (Vol=1.82L)	0.000	14:10
BLANK TEST	0.000	14:11
EXTERNAL STANDARD	0.080	14:11
BLANK TEST	0.000	14:12

MNC

