



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100392

Report Issue Date: 07/06/2023
Date Received: 2023-06-06
Condition of Item: Good

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

Start Date 06/06/2023 - As Found - **End Date 06/08/2023** As Found - Evaluation Analyst: Tatiana Malnoske
 As Found Conditions - Barometric Pressure (inHg): 29.73 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.3
 Relative Humidity (%): 33%

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.019	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.080	09523080A1	0.080	0.080	0.080	0.080	0.080	0.080	0.080
0.300	0.298	AG217903	0.301	0.301	0.302	0.301	0.301	0.301	0.301

Start Date 06/13/2023 - As Left - **End Date 06/13/2023**
 As Left Conditions - Barometric Pressure (inHg): 29.93 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.0 Relative Humidity (%): 34

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.021	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG217904	0.040	0.041	0.040	0.040	0.041	0.040	+/- 0.003
0.080	0.080	09523080A1	0.081	0.080	0.081	0.080	0.081	0.081	+/- 0.004
0.100	0.100	AG211003	0.101	0.101	0.101	0.101	0.100	0.101	+/- 0.004
0.150	0.150	AG134205	0.151	0.151	0.151	0.152	0.151	0.151	+/- 0.005
0.300	0.300	AG217903	0.304	0.303	0.304	0.304	0.304	0.304	+/- 0.011

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Colleen O'Bryant on 06/29/2023

colleen.obryant@alaska.gov

Technically and administratively reviewed by Brandi Barnett on 07/06/2023

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100392 Analyst: C. O. Bryant Start Date: 6/13/23

- Diagnostic Test (attached) Internal Standard value \leq 3.00%
 Adjust voltages, if needed

- Lamp (2.60 V Maximum) Chopper Frequency
 Bias Detector Voltage
 Cooler (2.00 V Maximum) (-0.100V to 0.100V)

- Set RFI Sensitivity
 Adjust internal barometer reading to match NIST-traceable barometer
 Adjust volume setting, if needed (1.50 L +/- 0.10 L)
 Print Technician Screen (attached)
 Print Calibration Factors (attached)
 Minimum Volume Test 1.5 L (1.3L to 1.7L)

Data Interpretation 2023.06.13
COB

As Left Conditions:

Barometric Pressure (in Hg): 29.93 Temperature (C): 22.0 Relative Humidity (%) 34

Linearity Test (attached)

0.020g/210L Mnf: Argas Lot: AG217902 Exp: 6/28/24
 0.040g/210L Mnf: Argas Lot: AG217904 Exp: 6/28/24
 0.080g/210L Mnf: ILMO Lot: 09523080A1 Exp: 5/5/25
 0.100g/210L Mnf: Argas Lot: AG211003 Exp: 4/20/24
 0.150g/210L Mnf: Argas Lot: AG134205 Exp: 10/8/23
 0.300g/210L Mnf: Argas Lot: AG217903 Exp: 6/28/24

Functional Tests (attached)

- Incomplete Invalid
 Maximum Attempts Exceeded Radio Frequency Interference (RFI)
 Interference (Volatiles)

Acetone Mnf: LifeLoc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24Simulator S/N: DR4176 Verification Performed? Isopropanol Mnf: LifeLoc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24Simulator S/N: DR4177 Verification Performed? Neg. Control Mnf: LifeLoc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23Simulator S/N: DR6267 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/9/23

- Verify stylus is calibrated Non-Drinking Subject Test
 Reset Options Upload
 Clear Memory Remove Tank Prior to Shutdown
 Verification of Calibration (VOC) Calibration End Date: 6/13/23

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 06/13/2023
Time: 07:31:45

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 46.8°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.68 V PASSED
(1.01 V - 2.35 V)
Cooler Voltage = 1.57 V PASSED
(0.97 V - 2.27 V)
Bias Voltage = 79 V PASSED
(48 V - 112 V)
Chopper Freq = 536 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 30.0 in

PUMP INFO

Flow Rate = 4.756 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.003 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.098 (1.27%) (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100392

Date: 06/13/2023
Time: 9:55 AM

Temperatures (°C)
Sample Cell: 48.9°C
Breath Tube: 45.9°C

Current Barometer 29.9 in
Volume (Ltr) 1.46

Settings
Lamp: 1.79 V
Bias: 80 V
Cooler: 1.60 V
Chopper: 535 Hz

Voltages (V)
Flow: 1.07 V
Detector: 0.075 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 03/15/2011
Time: 07:58:03

Ca = 0.1000
CAL = 0.990755 0.800 <= CAL < 1.200
b1 = 0.0000 0.0000 <= b1 < 0.0040
b2 = 0.0037 0.0010 <= b2 < 0.0100
b3 = 0.0002 0.0000 <= b3 < 0.0040
Xq = 0.0967 0.0500 <= Xq < 0.2000
a21 = 1.157321 1.050 <= a21 < 1.300
a31 = 0.392902 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100392

Date: 06/13/2023

Time: 09:56:25

SUBJECT NAME:

TEST TEST

LICENSE #: VOLUME TEST

OPERATOR NAME:

COLLEEN S OBRYANT

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 23-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080

TARGET AT 29.93: 0.080

LOT #: 09523080A1

EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	09:58
BLANK TEST	0.000	09:58
INTERNAL STANDARD	VERIFIED	09:58
EXTERNAL STANDARD	0.080	09:58
BLANK TEST	0.000	09:59
SUBJECT SAMPLE (Vol=1.53L)	0.000	10:01
BLANK TEST	0.000	10:02
EXTERNAL STANDARD	0.080	10:02
BLANK TEST	0.000	10:03

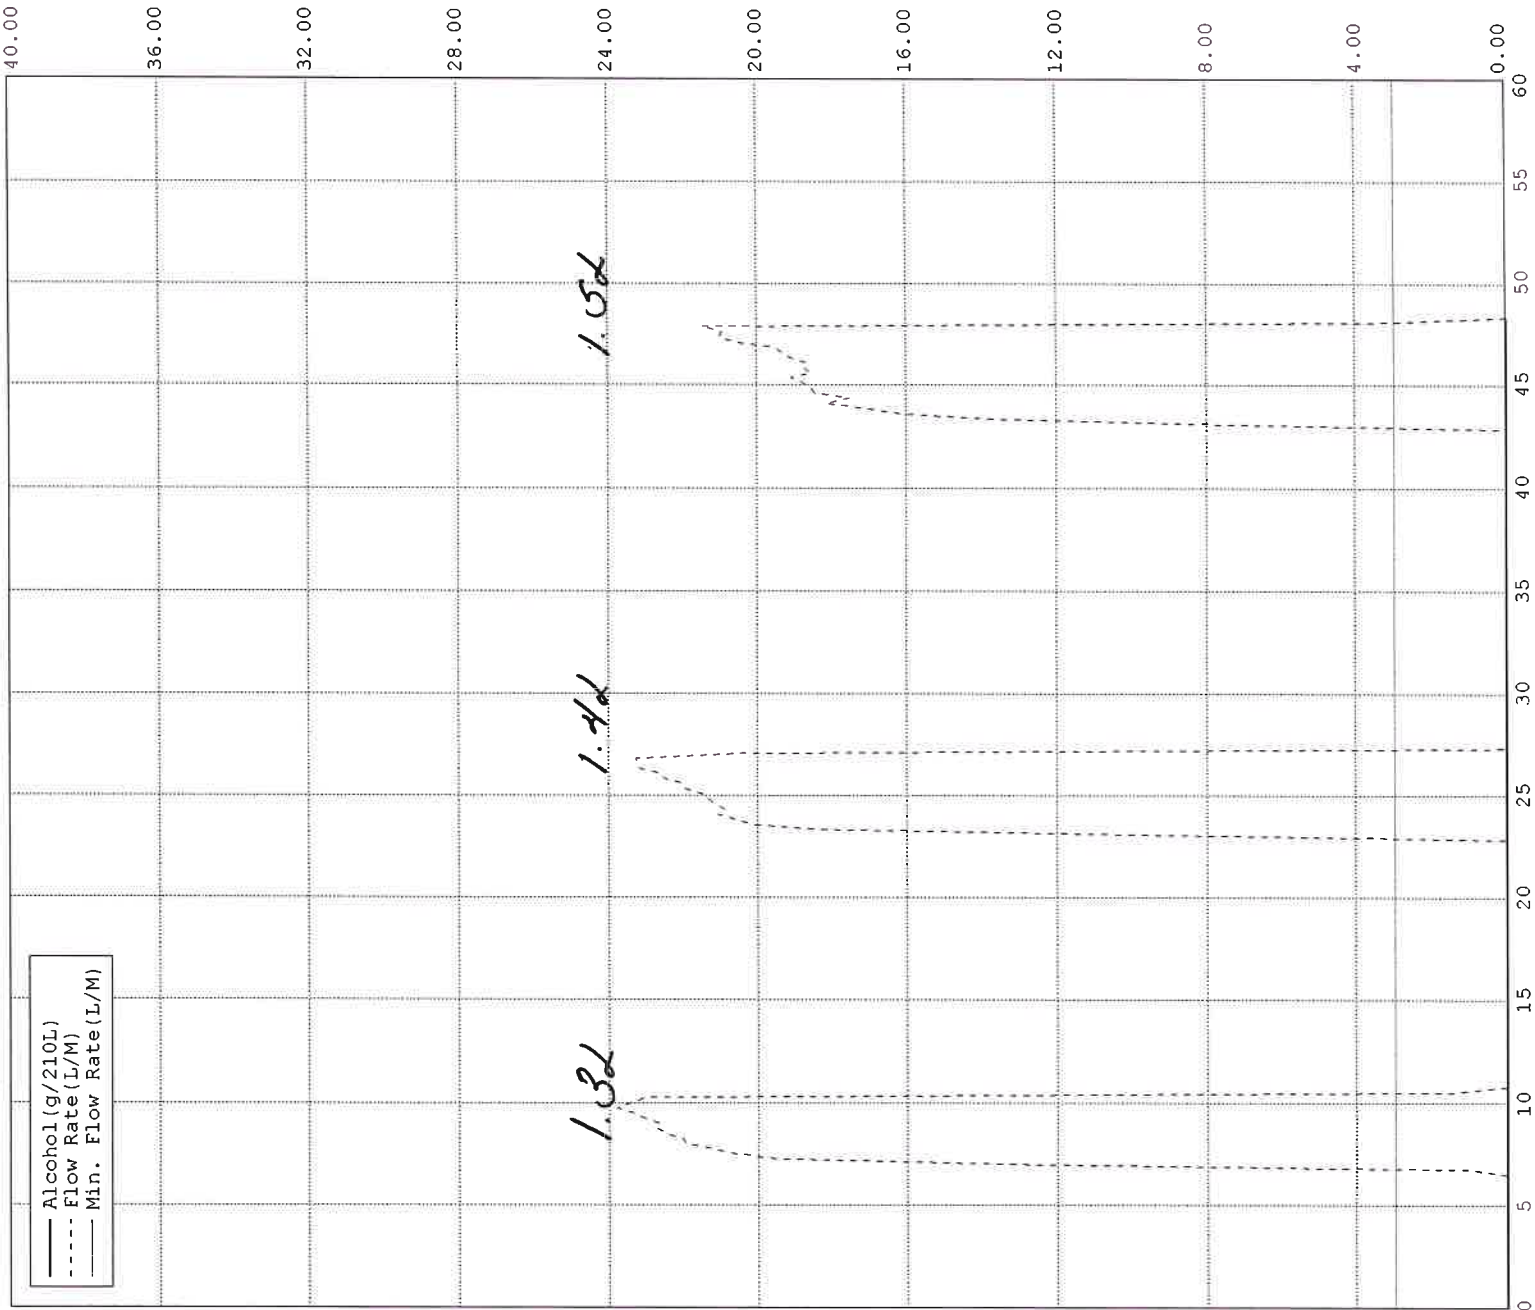

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100392

Date: 06/13/2023
 Time: 10:07:27

SUPERVISOR NAME:
 COLLEEN S O'BRYAN
 OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0004
0.040	0.0404	0.0005
0.080	0.0806	0.0005
0.100	0.1008	0.0004
0.150	0.1512	0.0004
0.300	0.3038	0.0004

SLOPE = 1.012861
 R² = 0.9999993

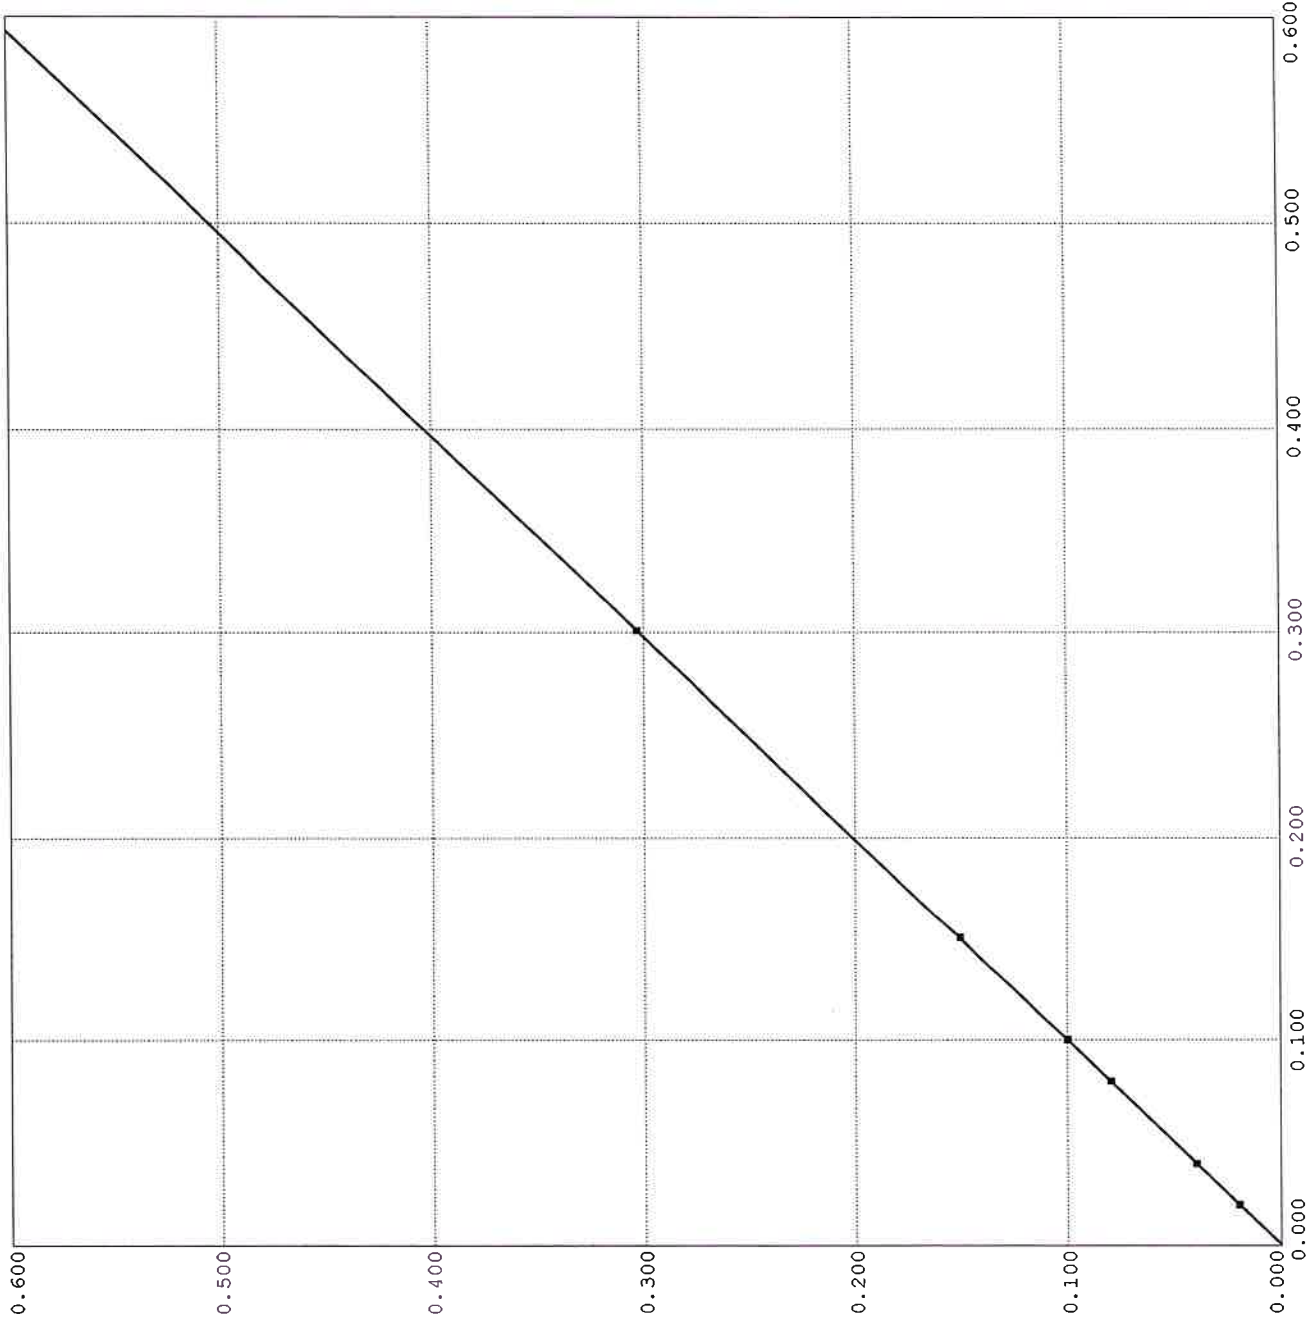

COG

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 06/13/2023
 Time: 10:07:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.93: 0.020
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 740 psi

BLANK TEST	0.000	10:08
INTERNAL STANDARD	VERIFIED	10:08
EXTERNAL STANDARD	0.021	10:08
BLANK TEST	0.000	10:09
EXTERNAL STANDARD	0.020	10:10
BLANK TEST	0.000	10:10
EXTERNAL STANDARD	0.020	10:11
BLANK TEST	0.000	10:12
EXTERNAL STANDARD	0.020	10:12
BLANK TEST	0.000	10:13
EXTERNAL STANDARD	0.020	10:13
BLANK TEST	0.000	10:14

Average = 0.0202
 Std Dev = 0.0004

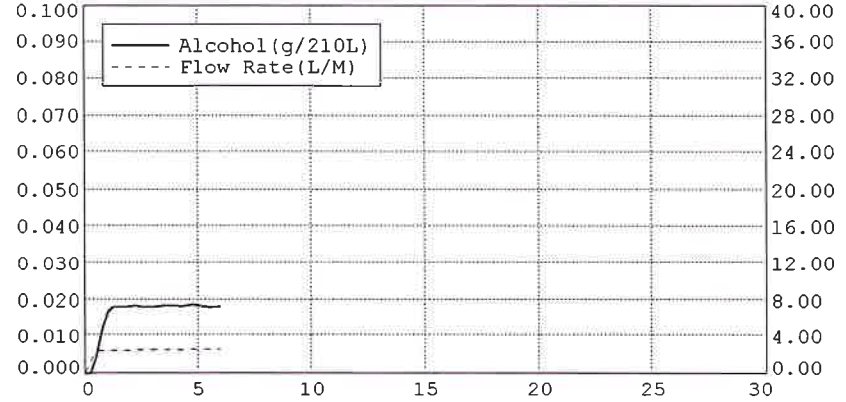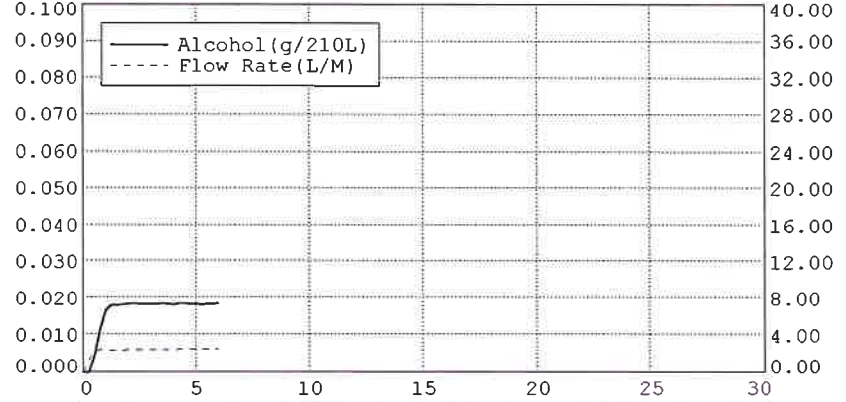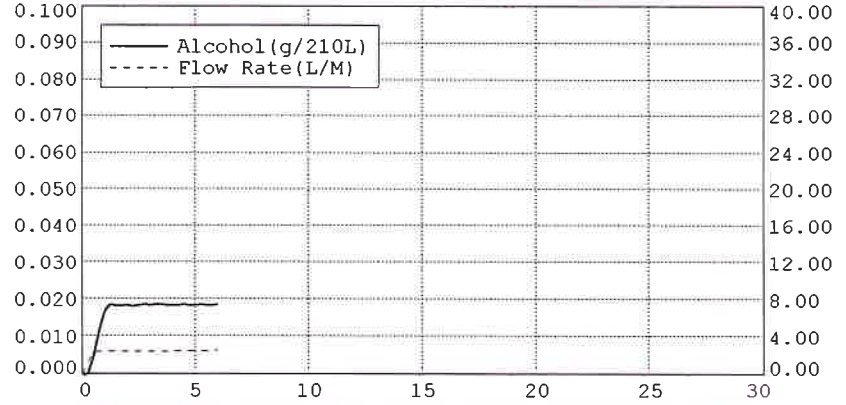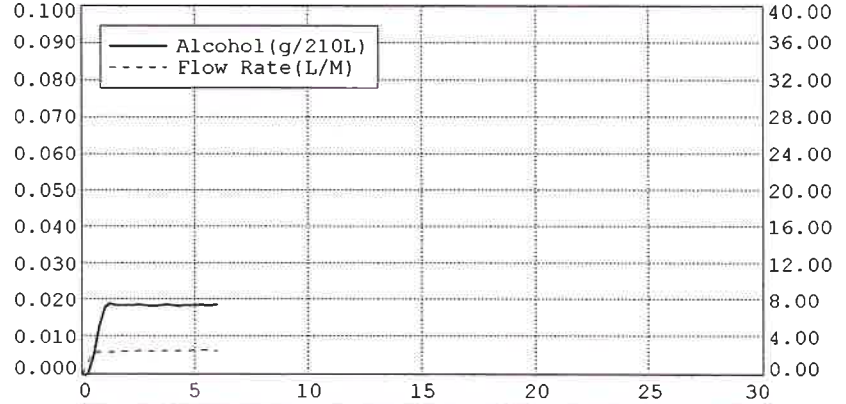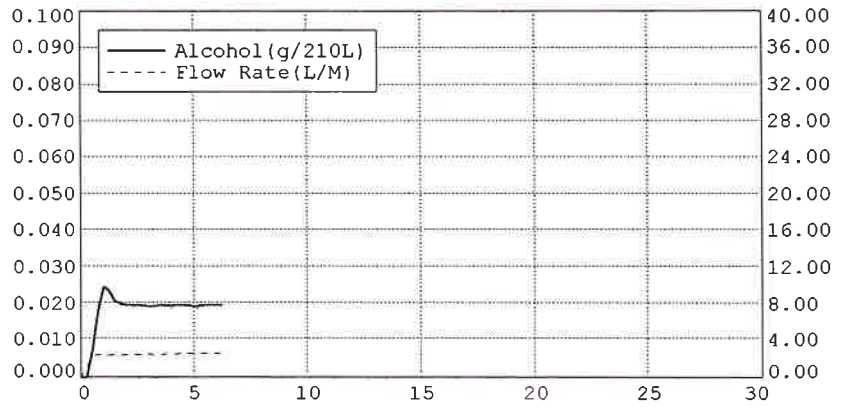

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 06/13/2023
 Time: 10:14:33

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.92: 0.040
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 927 psi

BLANK TEST	0.000	10:15
INTERNAL STANDARD	VERIFIED	10:15
EXTERNAL STANDARD	0.040	10:16
BLANK TEST	0.000	10:16
EXTERNAL STANDARD	0.041	10:17
BLANK TEST	0.000	10:18
EXTERNAL STANDARD	0.040	10:18
BLANK TEST	0.000	10:19
EXTERNAL STANDARD	0.040	10:19
BLANK TEST	0.000	10:20
EXTERNAL STANDARD	0.041	10:20
BLANK TEST	0.000	10:21

Average = 0.0404
 Std Dev = 0.0005

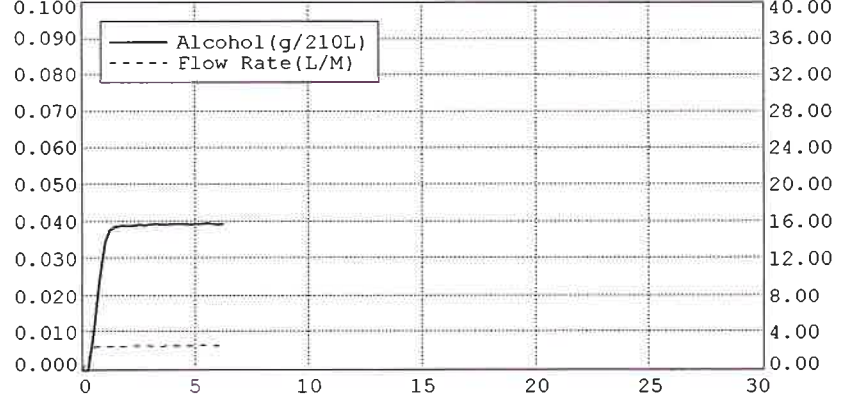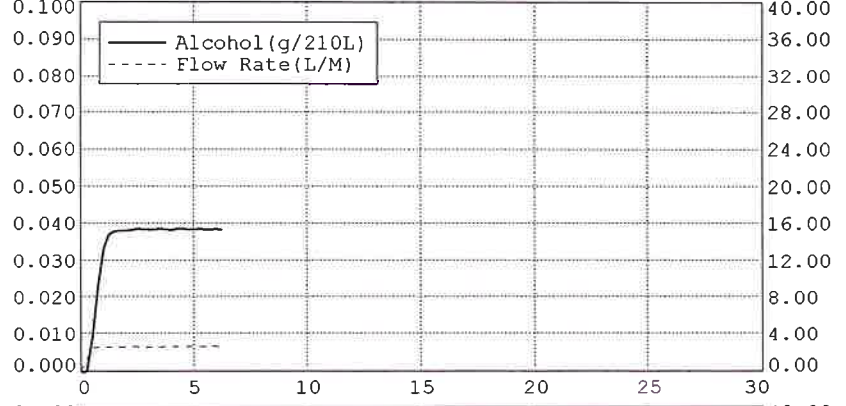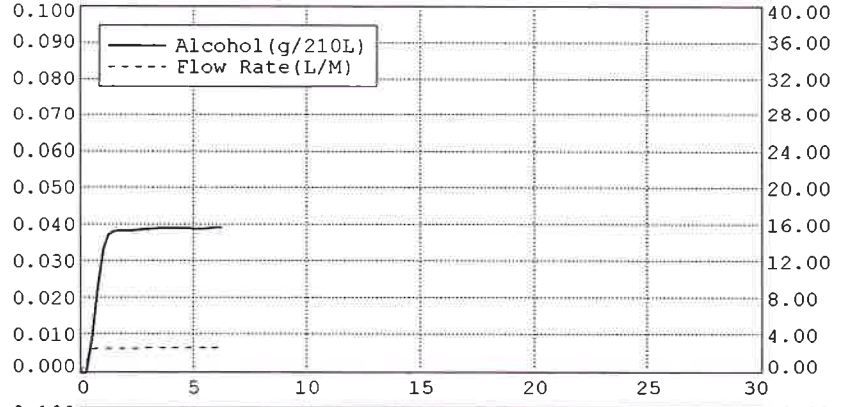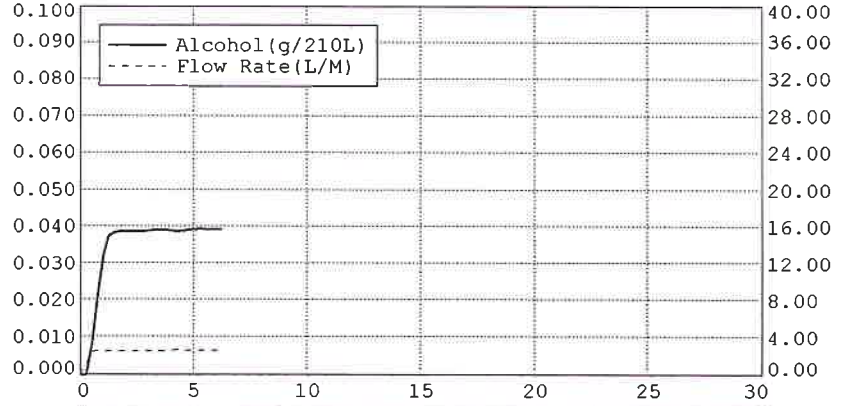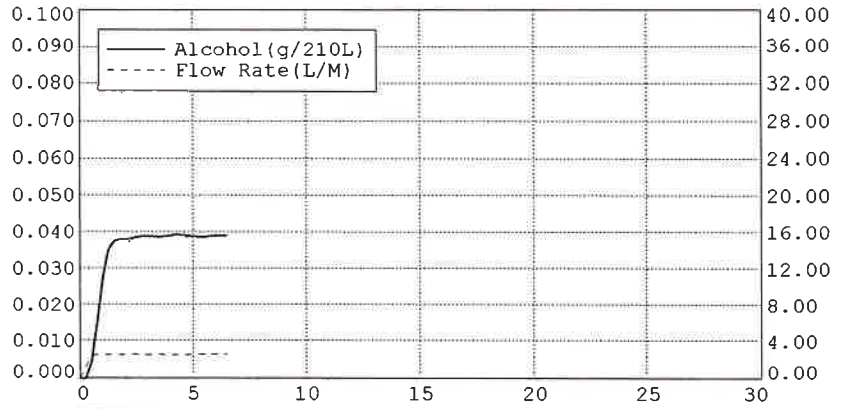

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 06/13/2023
 Time: 10:22:10

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.92: 0.080
 LOT #: 09523080A1
 EXPIRATION: 05/05/2025
 TANK PRESSURE: 944 psi

BLANK TEST	0.000	10:23
INTERNAL STANDARD	VERIFIED	10:23
EXTERNAL STANDARD	0.081	10:23
BLANK TEST	0.000	10:24
EXTERNAL STANDARD	0.080	10:24
BLANK TEST	0.000	10:25
EXTERNAL STANDARD	0.081	10:25
BLANK TEST	0.000	10:26
EXTERNAL STANDARD	0.080	10:27
BLANK TEST	0.000	10:27
EXTERNAL STANDARD	0.081	10:28
BLANK TEST	0.000	10:29

Average = 0.0806
 Std Dev = 0.0005

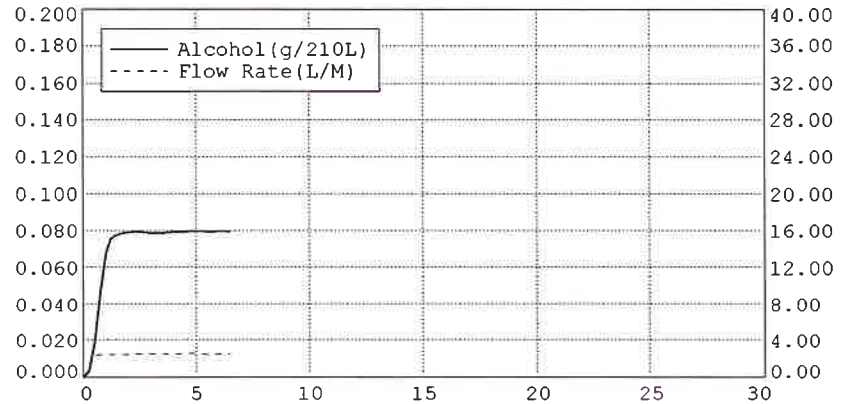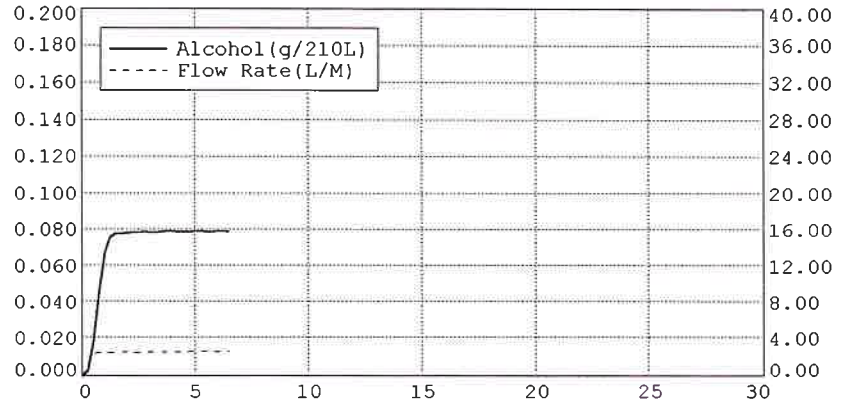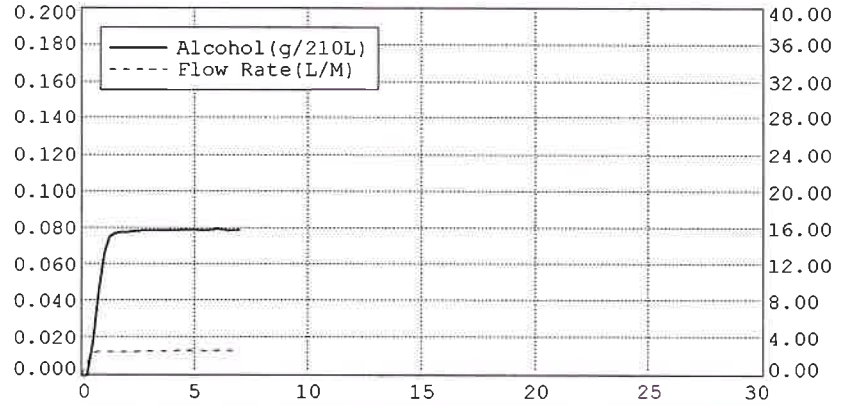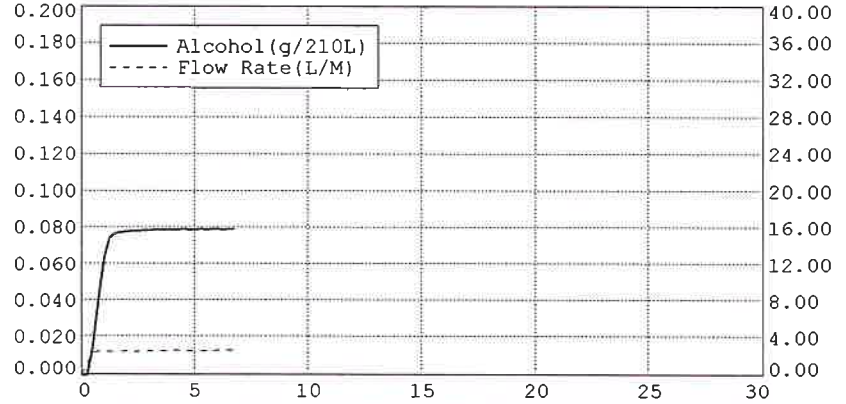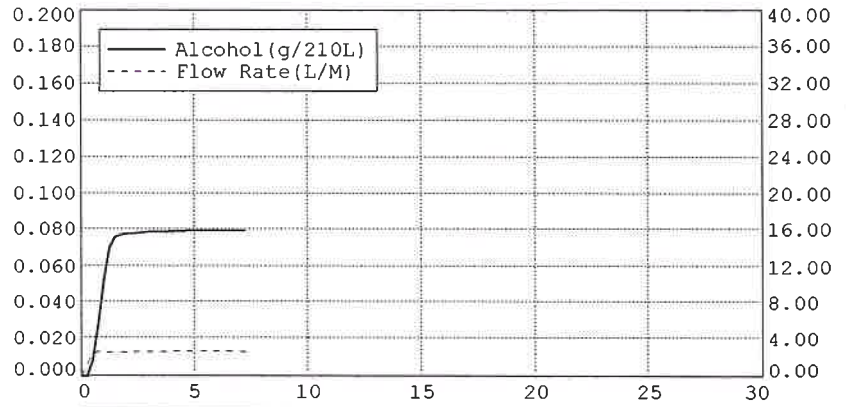

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 06/13/2023
 Time: 10:29:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.92: 0.100
 LOT #: AG211003
 EXPIRATION: 04/20/2024
 TANK PRESSURE: 682 psi

BLANK TEST	0.000	10:31
INTERNAL STANDARD	VERIFIED	10:31
EXTERNAL STANDARD	0.101	10:31
BLANK TEST	0.000	10:32
EXTERNAL STANDARD	0.101	10:32
BLANK TEST	0.000	10:33
EXTERNAL STANDARD	0.101	10:33
BLANK TEST	0.000	10:34
EXTERNAL STANDARD	0.101	10:34
BLANK TEST	0.000	10:35
EXTERNAL STANDARD	0.100	10:35
BLANK TEST	0.000	10:36

Average = 0.1008
 Std Dev = 0.0004

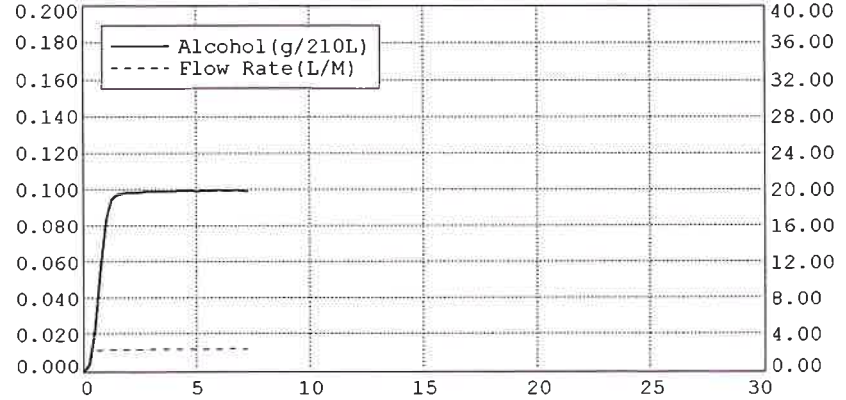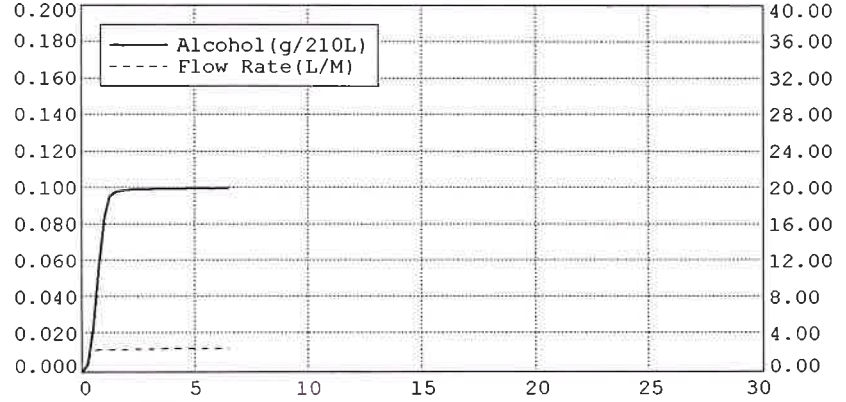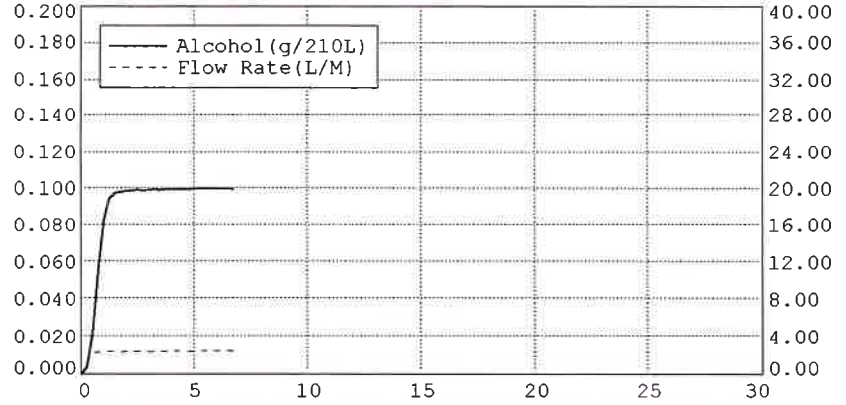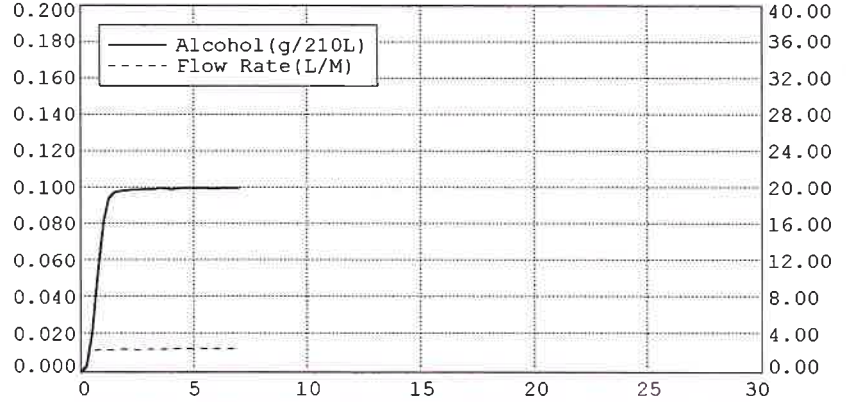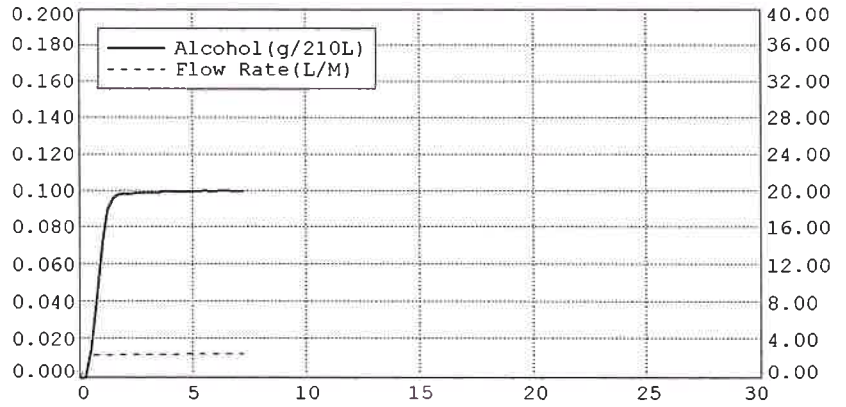

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 06/13/2023
 Time: 10:38:21

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.92: 0.150
 LOT #: AG134205
 EXPIRATION: 12/08/2023
 TANK PRESSURE: 816 psi

BLANK TEST	0.000	10:39
INTERNAL STANDARD	VERIFIED	10:39
EXTERNAL STANDARD	0.151	10:39
BLANK TEST	0.000	10:40
EXTERNAL STANDARD	0.151	10:41
BLANK TEST	0.000	10:41
EXTERNAL STANDARD	0.151	10:42
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.152	10:43
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.151	10:44
BLANK TEST	0.000	10:45

Average = 0.1512
 Std Dev = 0.0004

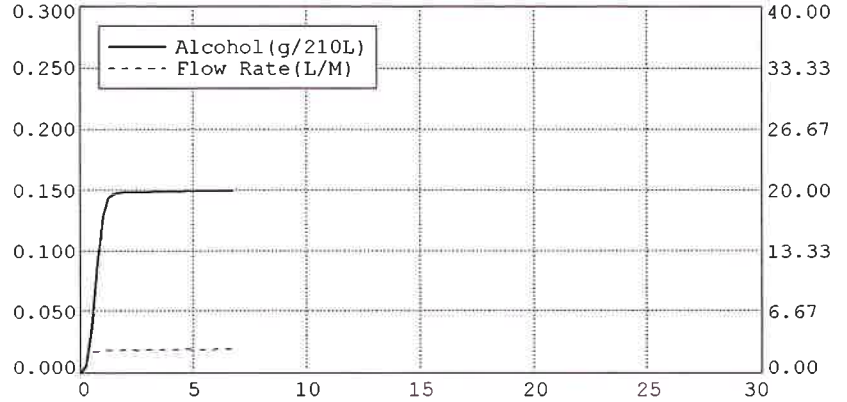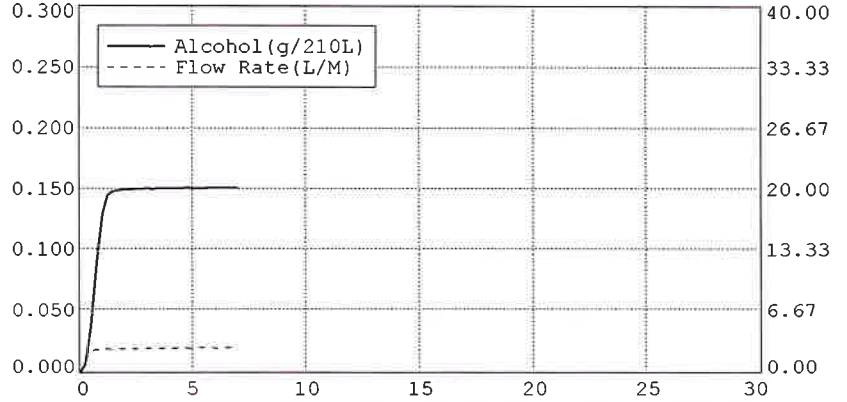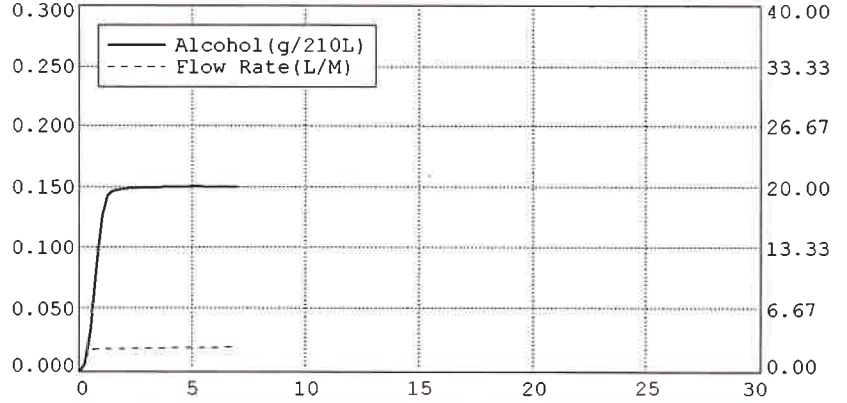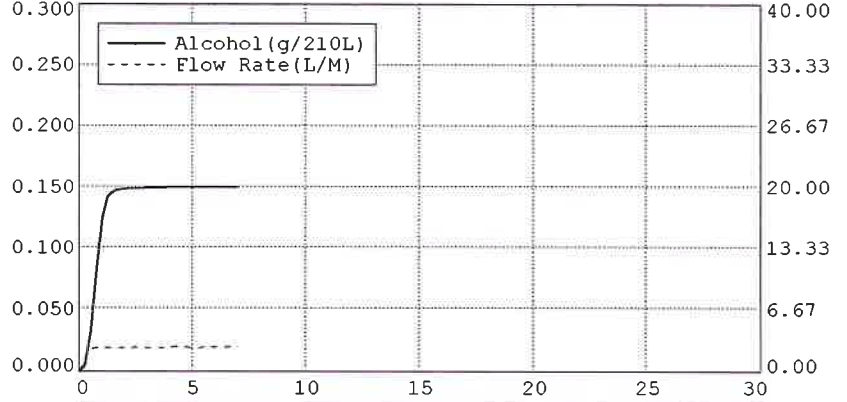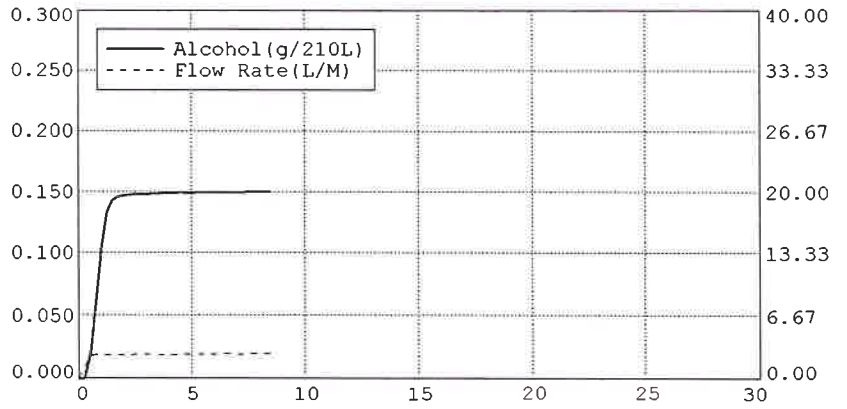

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 06/13/2023
 Time: 11:17:50

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.92: 0.300
 LOT #: AG217903
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 378 psi

BLANK TEST	0.000	11:19
INTERNAL STANDARD	VERIFIED	11:19
EXTERNAL STANDARD	0.304	11:19
BLANK TEST	0.000	11:20
EXTERNAL STANDARD	0.303	11:20
BLANK TEST	0.000	11:21
EXTERNAL STANDARD	0.304	11:21
BLANK TEST	0.000	11:22
EXTERNAL STANDARD	0.304	11:22
BLANK TEST	0.000	11:23
EXTERNAL STANDARD	0.304	11:24
BLANK TEST	0.000	11:24

Average = 0.3038
 Std Dev = 0.0004

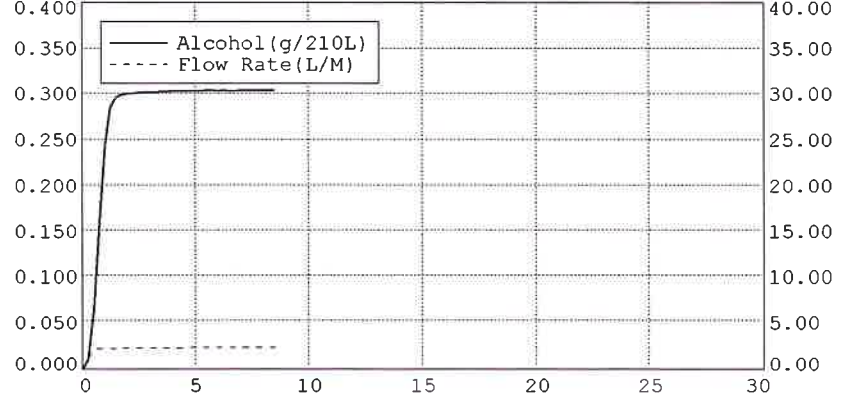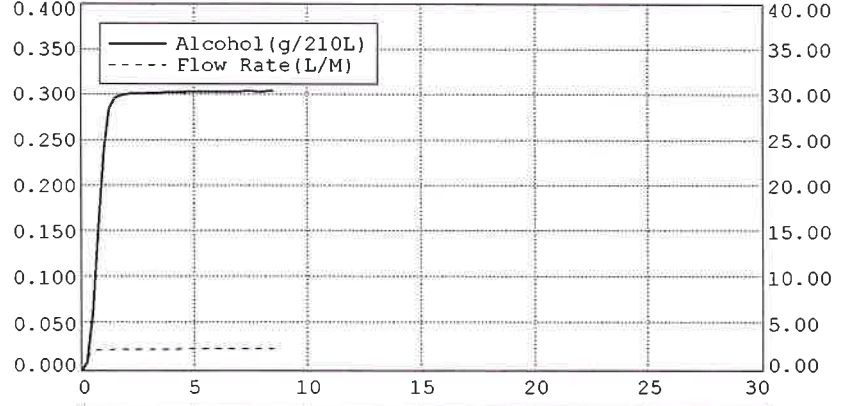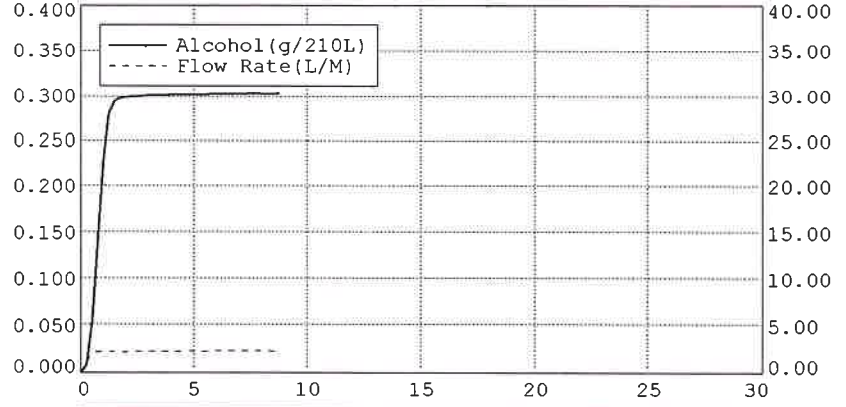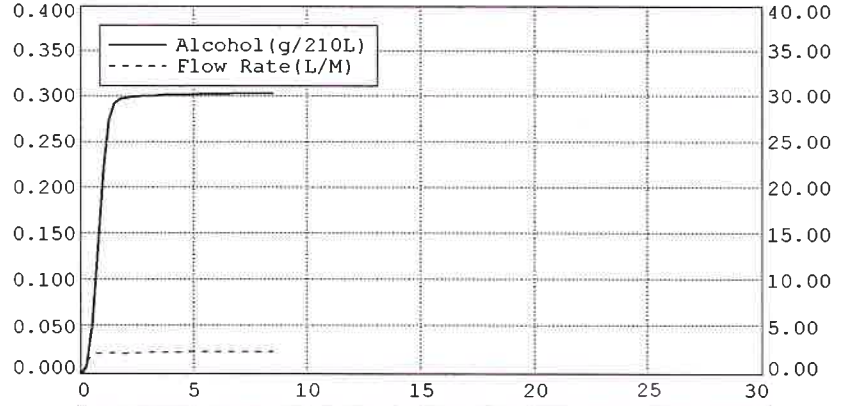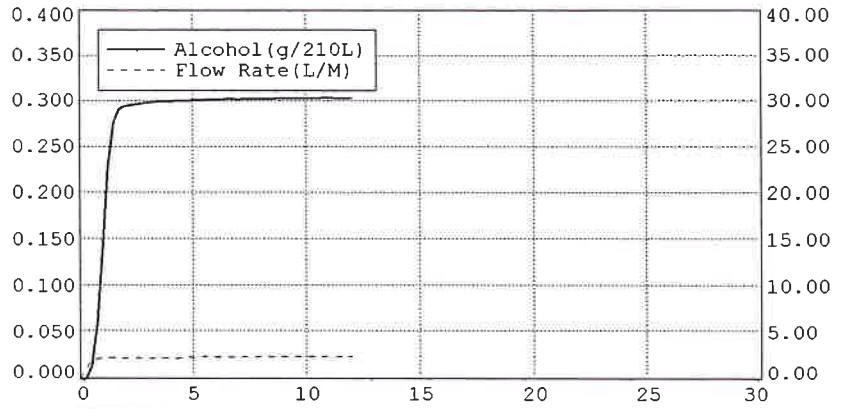

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 06/13/2023
Time: 11:36:18


SUBJECT NAME:
TEST TEST
LICENSE #: INCOMPLETE

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.92: 0.080
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK PASSED 11:38
BLANK TEST 0.000 11:38
INTERNAL STANDARD VERIFIED 11:38
EXTERNAL STANDARD 0.081 11:38
BLANK TEST 0.000 11:39
SUBJECT SAMPLE INCOMPLETE 11:41

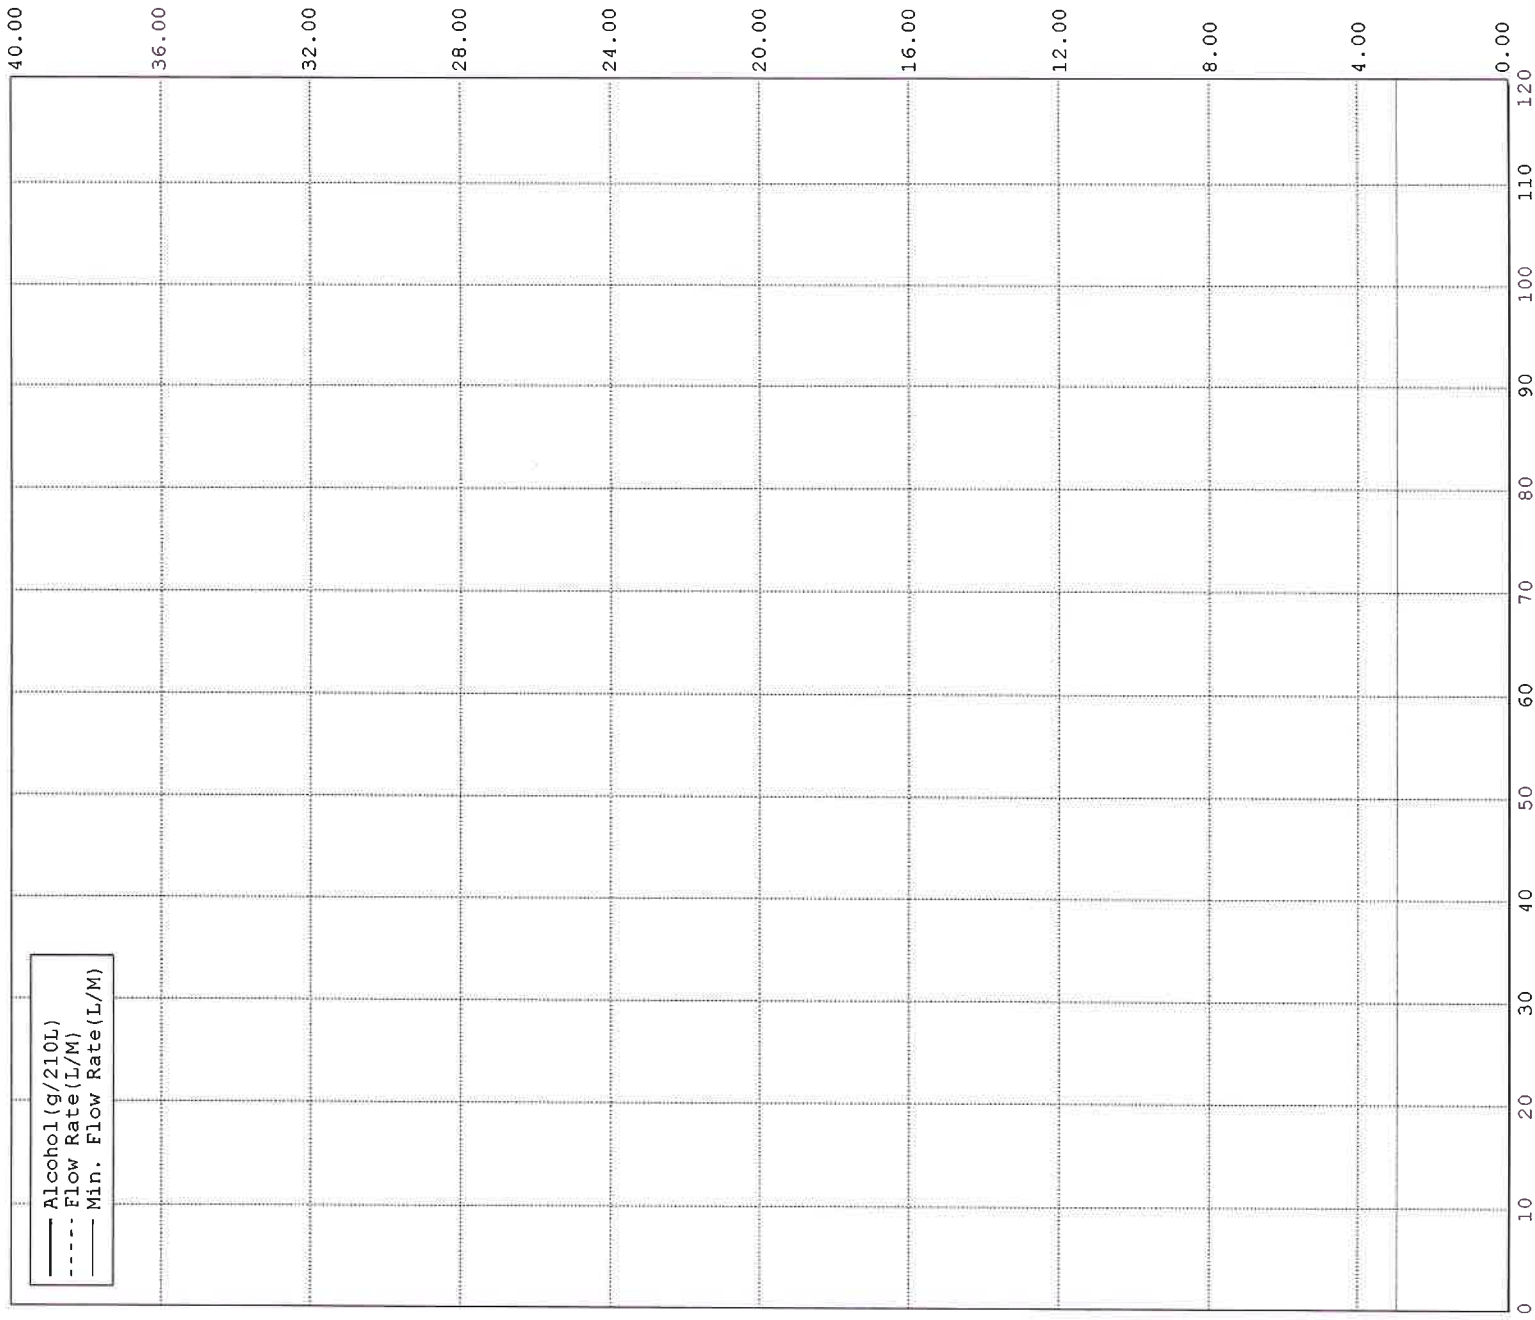

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 06/13/2023
Time: 12:14:40

SUBJECT NAME:
TEST TEST
LICENSE #: MAX ATTEMPTS

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1


CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.92: 0.080
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK PASSED 12:15
BLANK TEST 0.000 12:15
INTERNAL STANDARD VERIFIED 12:15
EXTERNAL STANDARD 0.081 12:16
BLANK TEST 0.000 12:17
SUBJECT SAMPLE XXX 12:17

Maximum Attempts Exceeded

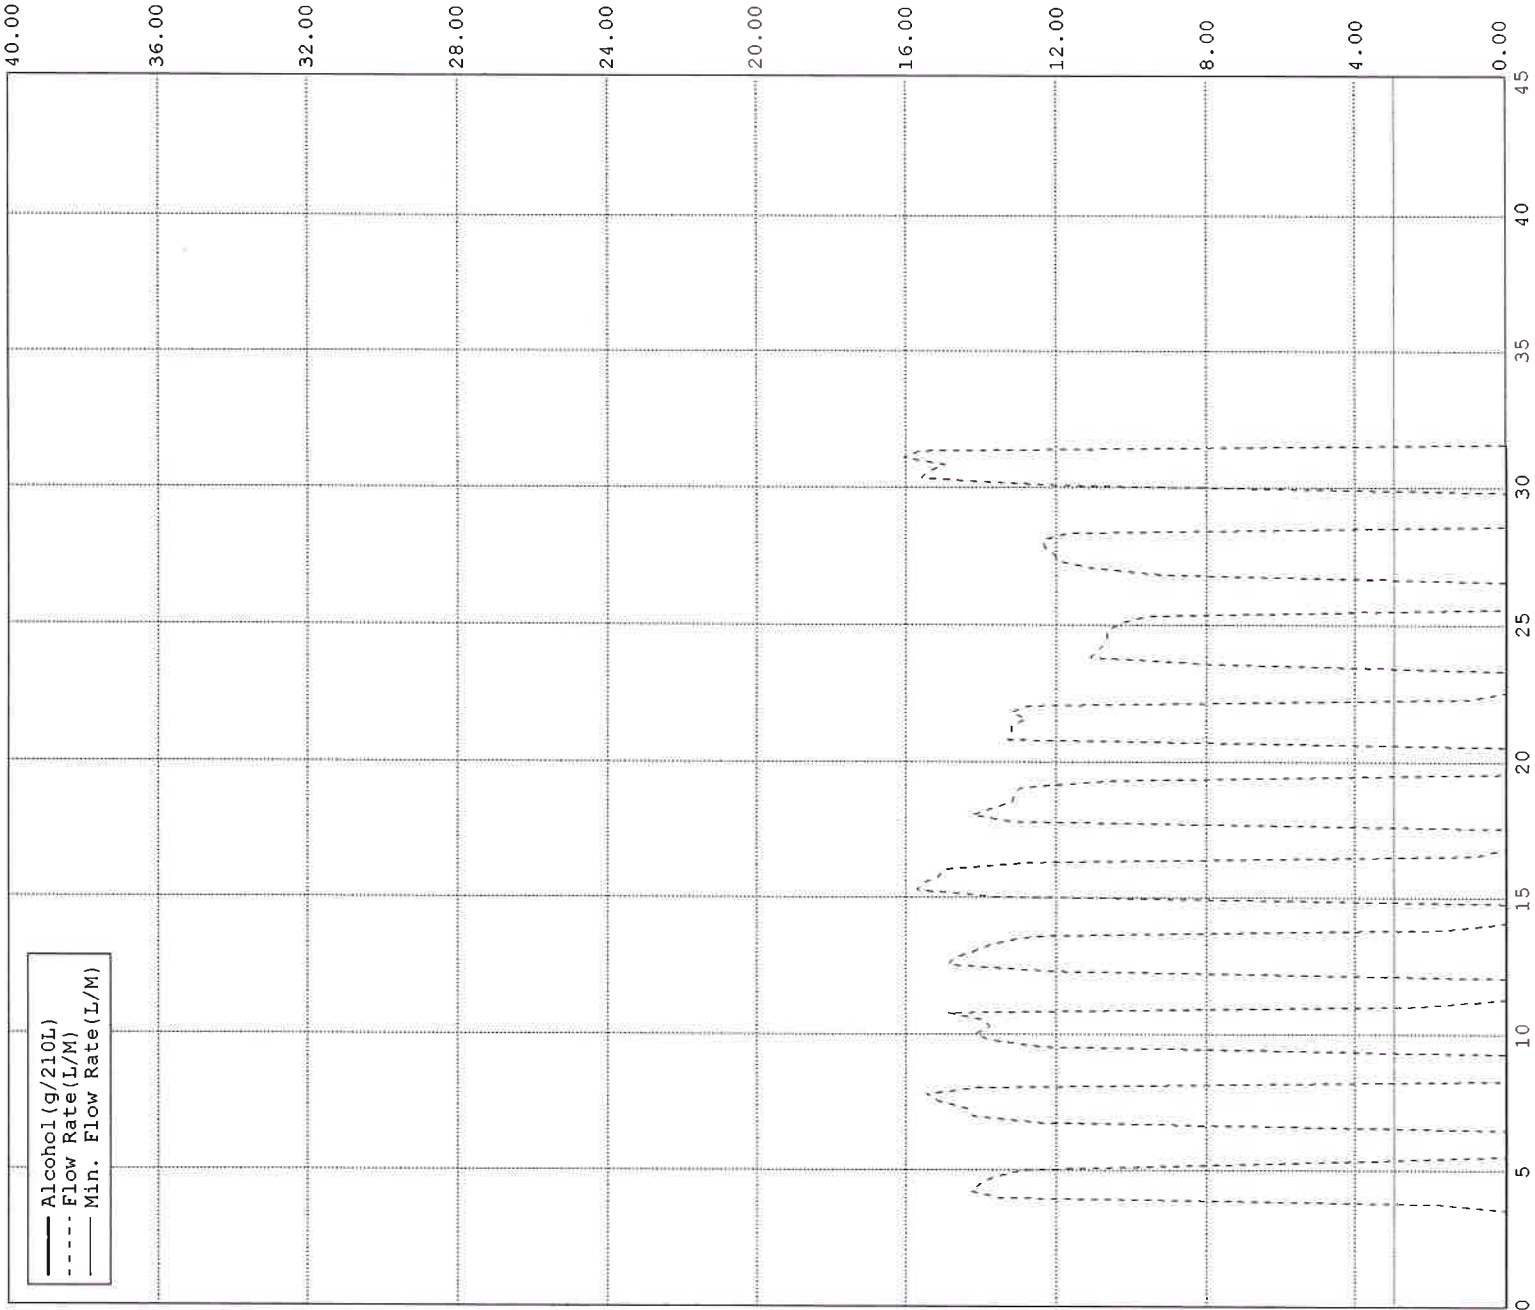



SUBJECT TEST

 Alaska Department of Public Safety
 DATAMASTER dmt: 100392

 Date: 06/13/2023
 Time: 12:26:07

SUBJECT NAME:
TEST TEST
LICENSE #: INVALID

OPERATOR NAME:
 COLLEEN S OBRYANT
 OPERATOR'S #: 6237

DEPT/AGENCY:
 AAA1

CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.92: 0.080
 LOT #: 09523080A1
 EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	12:27
BLANK TEST	0.000	12:27
INTERNAL STANDARD	VERIFIED	12:27
EXTERNAL STANDARD	0.081	12:27
BLANK TEST	0.000	12:28
SUBJECT SAMPLE	INVALID	12:28

COB

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100392

Date: 06/13/2023

Time: 12:21:00

SUBJECT NAME:

TEST TEST

LICENSE #: RFI

OPERATOR NAME:

COLLEEN S OBRVANT

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 23-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.92: 0.080

LOT #: 09523080A1

EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK

BLANK TEST


INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

RFI DETECTED

PASSED 12:21
0.000 12:22
VERIFIED 12:22
0.081 12:22
0.000 12:23

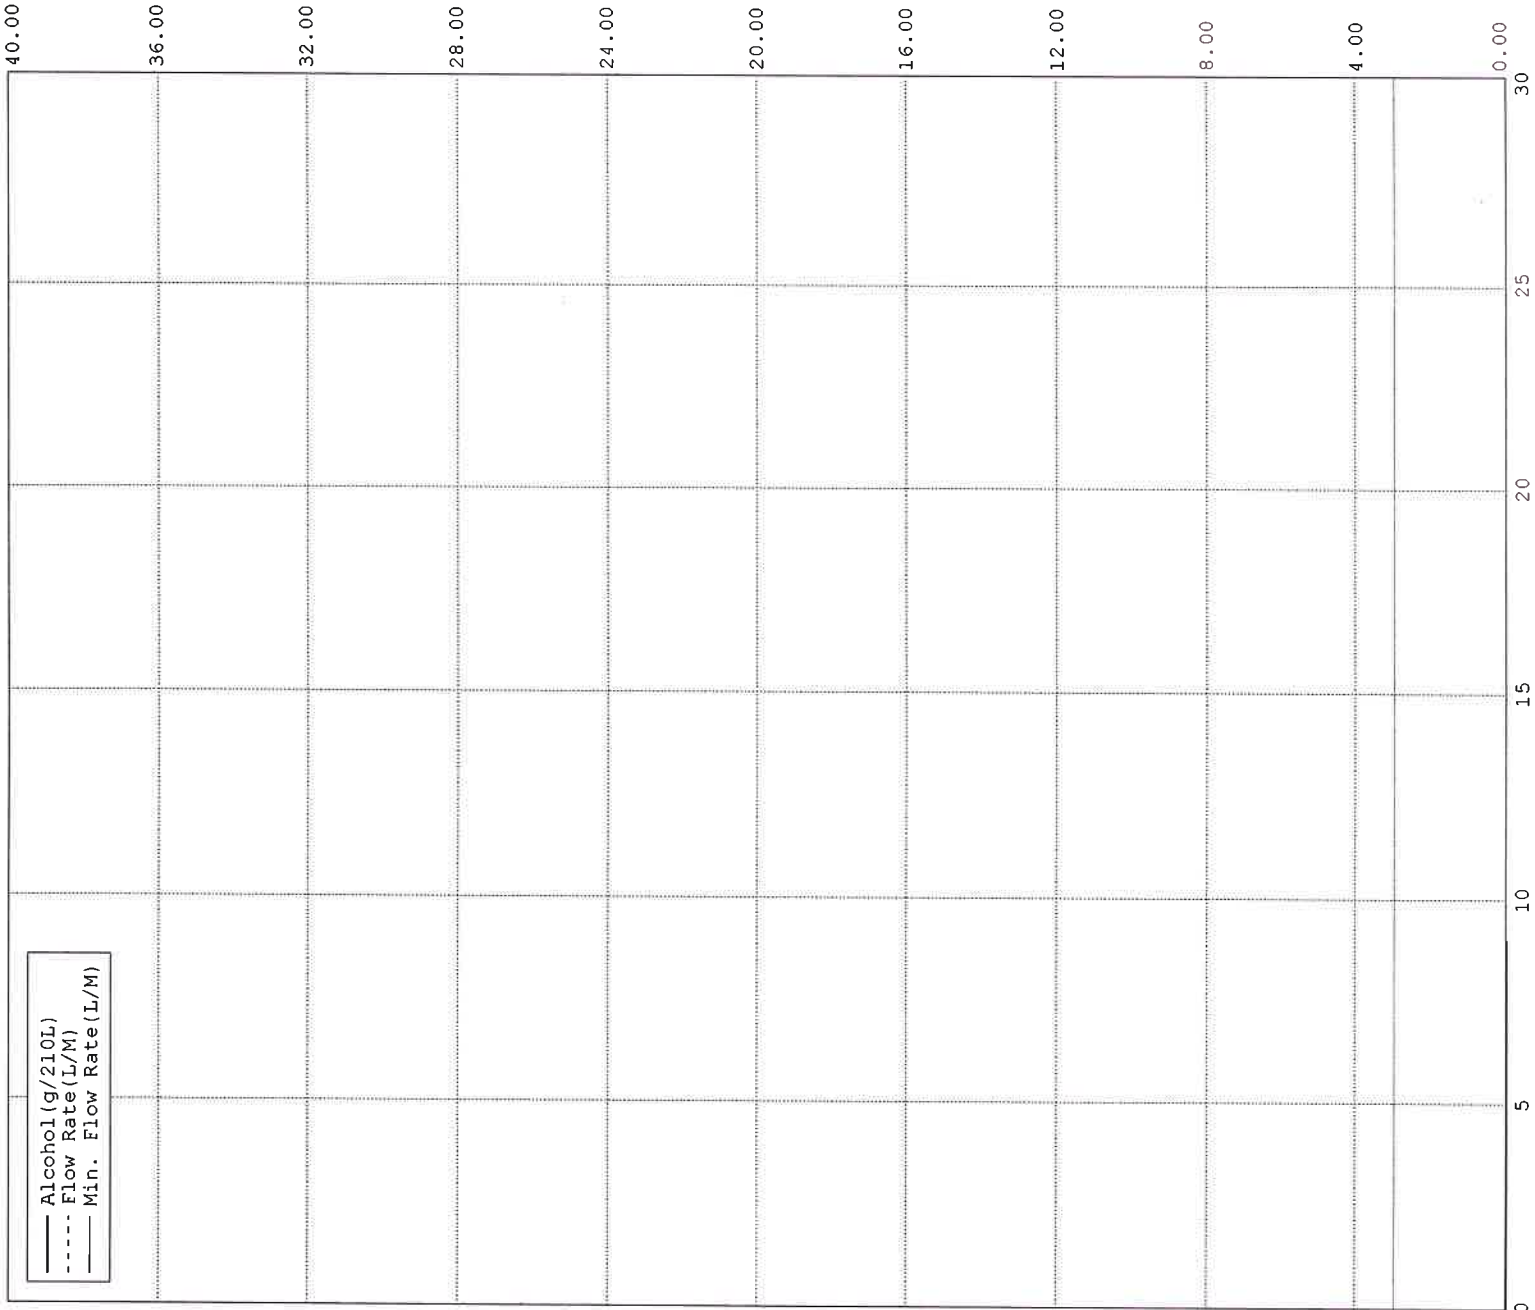

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 06/13/2023
Time: 14:00:02

SUBJECT NAME:
TEST TEST
LICENSE #: INT-ACETONE


OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.94: 0.080
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK PASSED 14:01
BLANK TEST 0.000 14:01
INTERNAL STANDARD VERIFIED 14:01
Xq = 0.099 (2.45%) 0.081 14:01
EXTERNAL STANDARD X[1] = 0.0806 (-0.0002) (0.0029)
BLANK TEST 0.000 14:02
SUBJECT SAMPLE XXX 14:03
X[1] = 0.1124 (-0.0206) (-0.0002)

Interference Detected

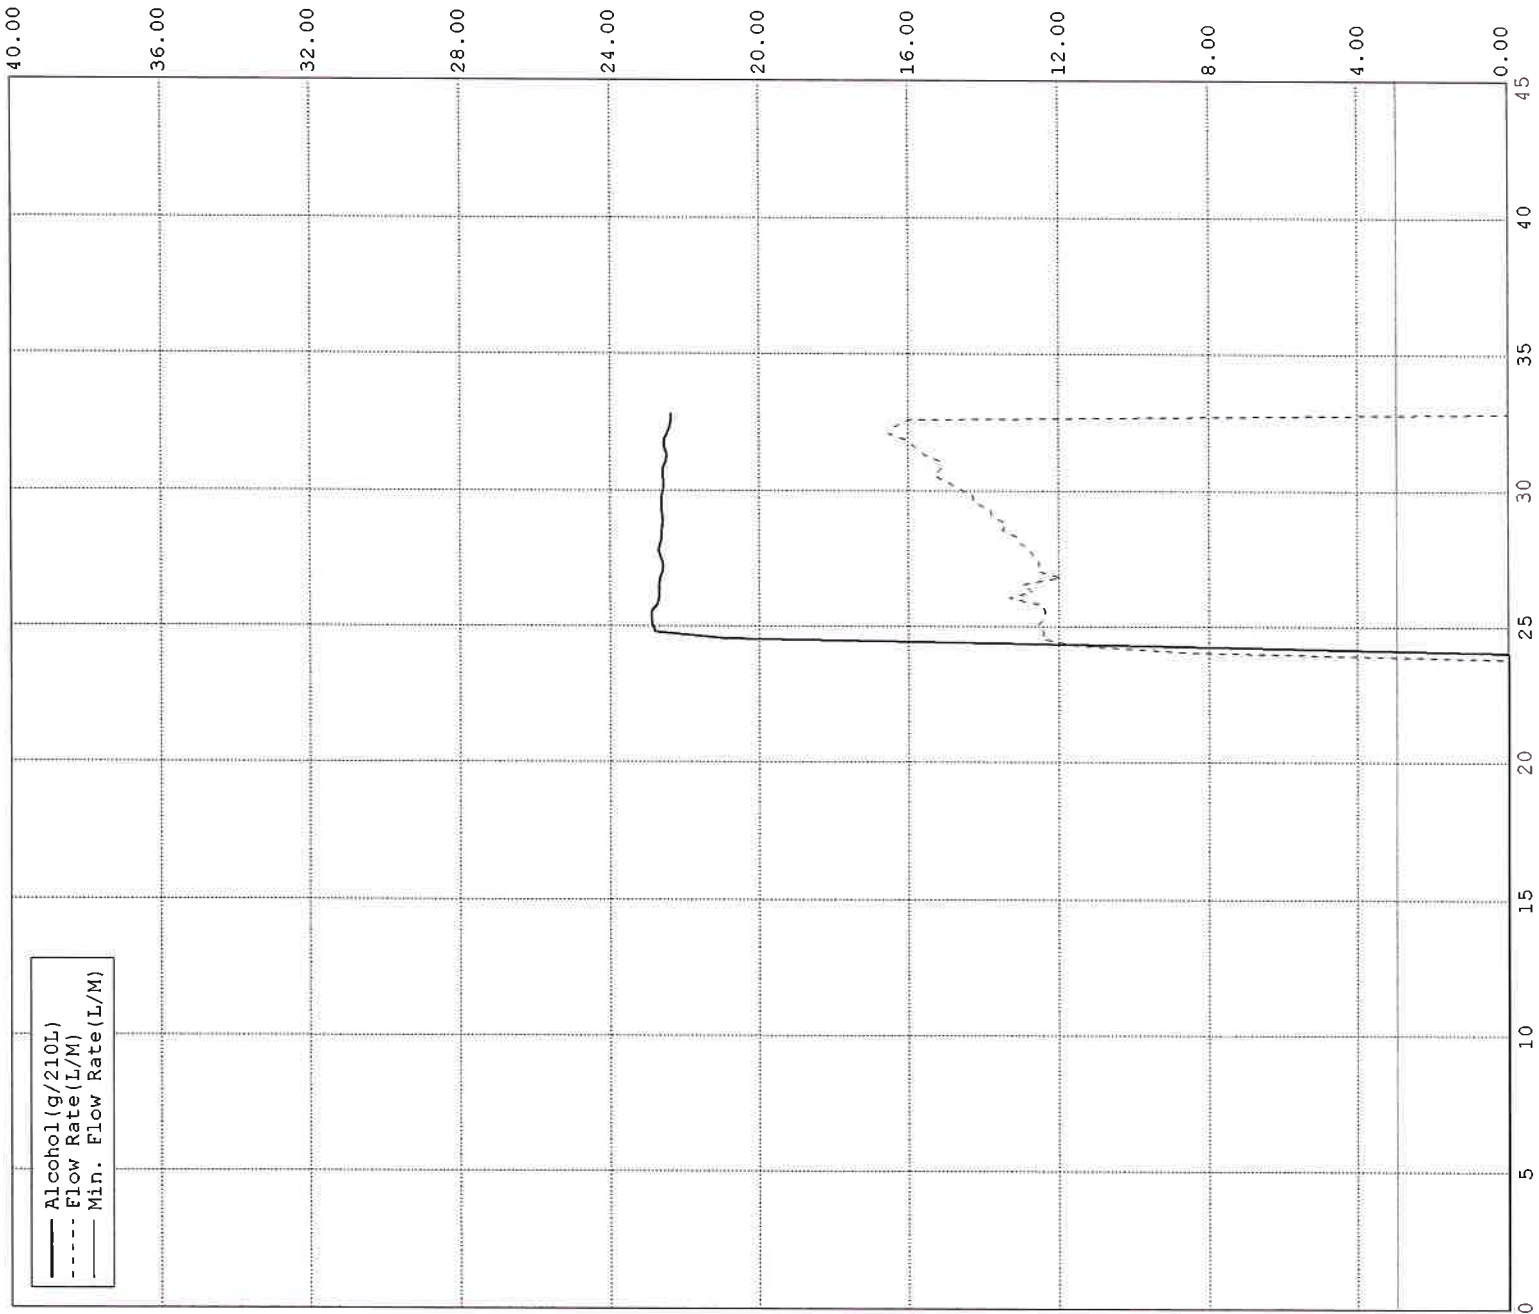

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 06/13/2023
Time: 14:21:15

SUBJECT NAME:
TEST TEST
LICENSE #: INT-IPA


OPERATOR NAME:
COLLEEN S O'BRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.92: 0.080
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK PASSED 14:22
BLANK TEST 0.000 14:22
INTERNAL STANDARD VERIFIED 14:22
Xq = 0.098 (1.72%) 0.080 14:22
X[1] = 0.0803 (0.0004) (0.0029) 0.000 14:23
BLANK TEST 0.000 14:23
SUBJECT SAMPLE XXX 14:24
X[1] = 0.1286 (-0.0298) (0.0027)

Interference Detected

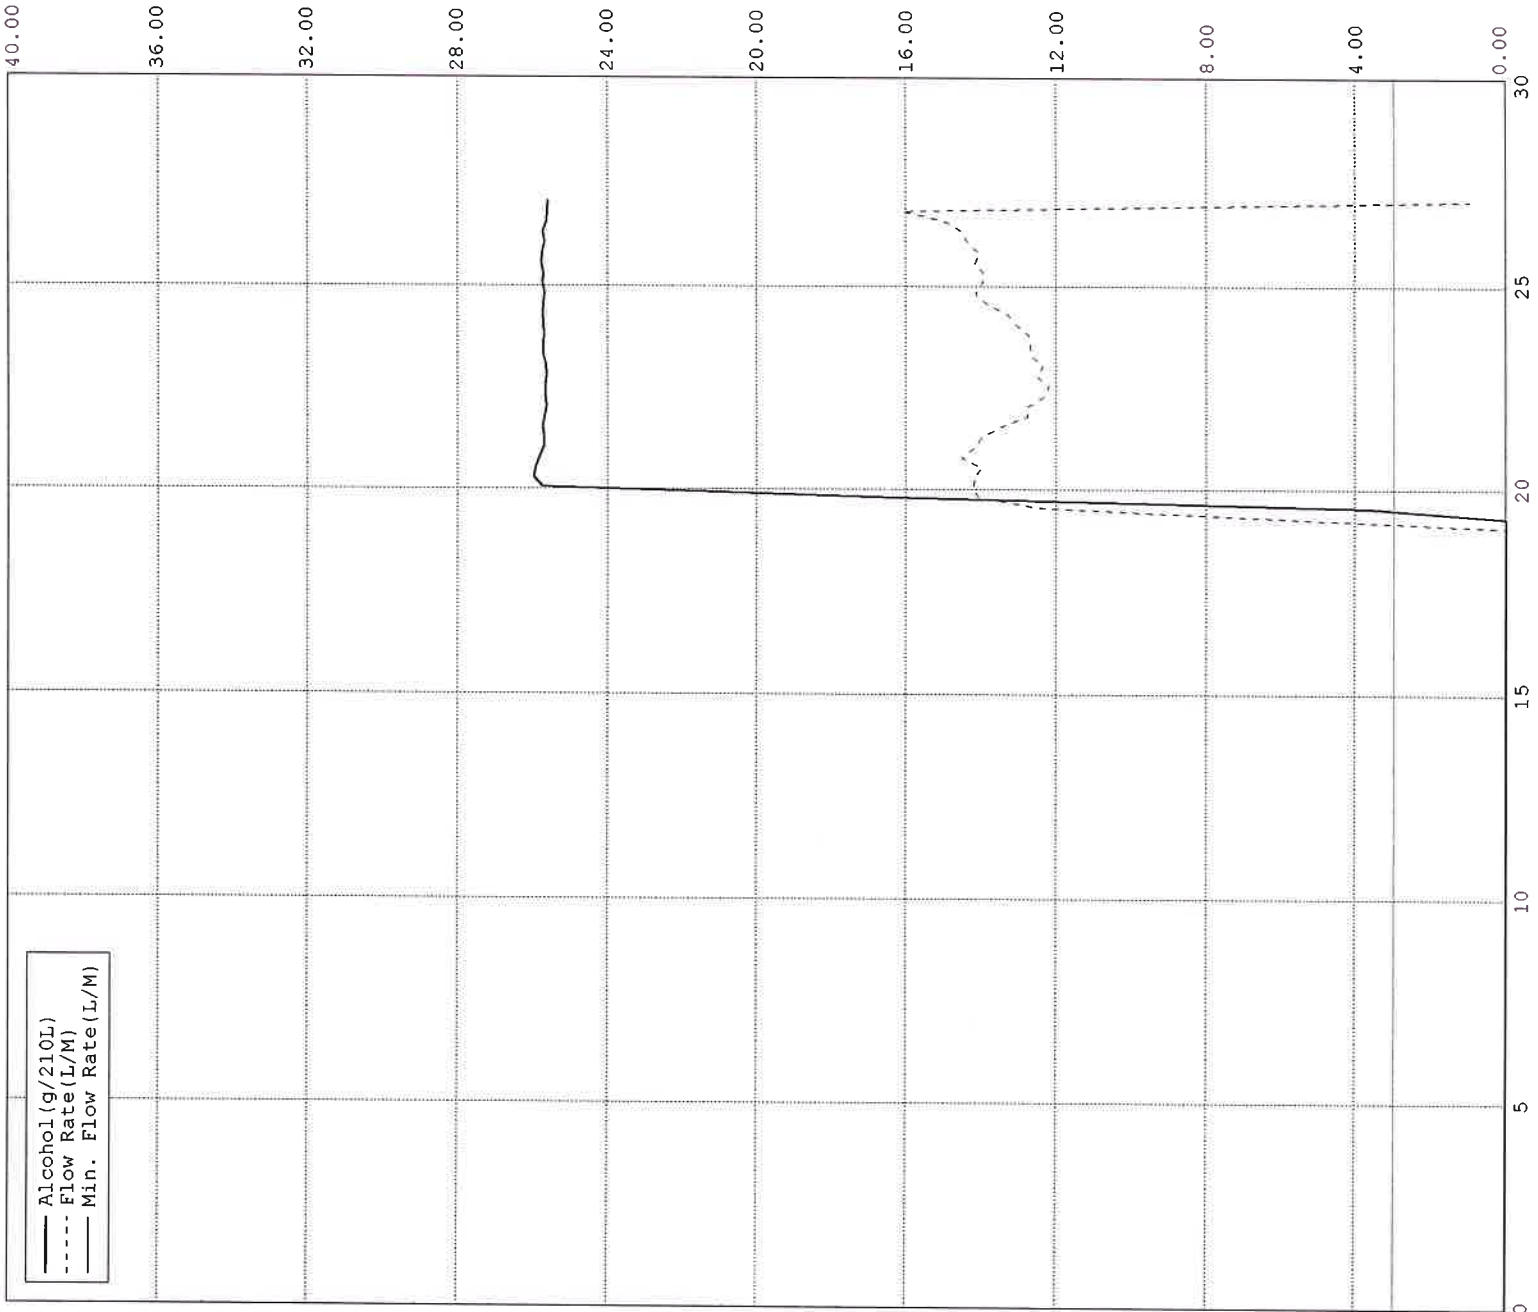

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 06/13/2023
Time: 14:28:22

SUBJECT NAME:
TEST TEST
LICENSE #: INT-NEGATIVE

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.92: 0.080
LOT #: 09523080A1
EXPIRATION: 05/05/2025


DIAGNOSTIC CHECK	PASSED	14:30
BLANK TEST	0.000	14:30
INTERNAL STANDARD	VERIFIED	14:30
Xq = 0.099 (2.08%)		
EXTERNAL STANDARD	0.080	14:30
X[1] = 0.0801 (-0.0001) (0.0020)		
BLANK TEST	0.000	14:31
SUBJECT SAMPLE (Vol=2.10L)	0.097	14:32
X[1] = 0.0979 (-0.0009) (0.0001)		
BLANK TEST	0.000	14:33
EXTERNAL STANDARD	0.080	14:33
X[1] = 0.0800 (0.0004) (0.0012)		
BLANK TEST	0.000	14:34

Filter 2 Avg = 0.0001
~~0.0000~~ ^{0.000}

Filter 3 Avg = 0.0003

COB

COB 6/13/23

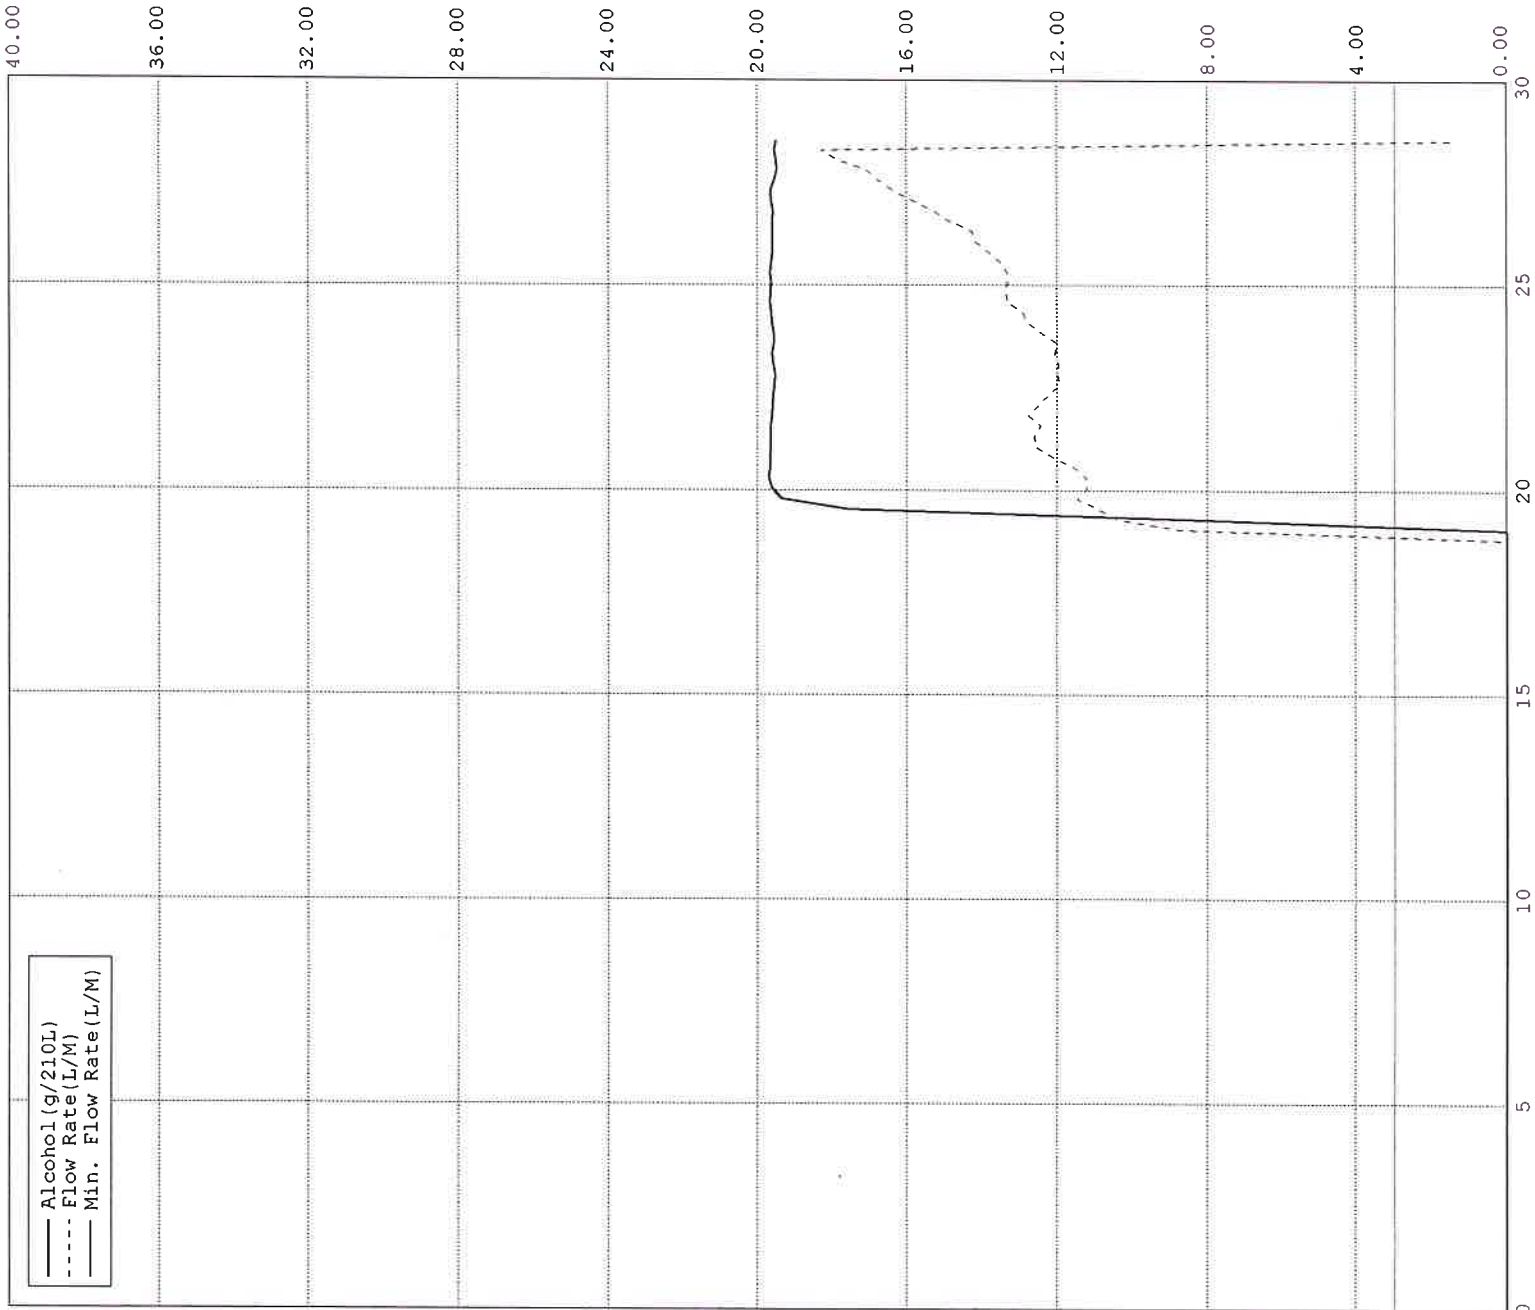

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 06/13/2023
Time: 14:55:00

SUBJECT NAME:
TEST TEST
LICENSE #: NON-DRINKING

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.92: 0.080
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 14:56
INTERNAL STANDARD VERIFIED 14:56
EXTERNAL STANDARD 0.081 14:56
BLANK TEST 0.000 14:57
SUBJECT SAMPLE (Vol=2.66L) 0.000 14:57
BLANK TEST 0.000 14:58
EXTERNAL STANDARD 0.081 14:58
BLANK TEST 0.000 14:59

