

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument
State of Alaska

Serial #: 100667

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 09/20/2014

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.12: 0.077
LOT #: 09214080A2
EXPIRATION: 05/01/2016

BLANK TEST	0.000	15:12
INTERNAL STANDARD	VERIFIED	15:12
EXTERNAL STANDARD	0.076	15:13
BLANK TEST	0.000	15:14
EXTERNAL STANDARD	0.076	15:14
BLANK TEST	0.000	15:15
EXTERNAL STANDARD	0.076	15:15
BLANK TEST	0.000	15:16
EXTERNAL STANDARD	0.077	15:16
BLANK TEST	0.000	15:17
EXTERNAL STANDARD	0.077	15:17
BLANK TEST	0.000	15:18

Average = 0.0764
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 2.00
PIC: 3.03
Modem: 2.3
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
Breath Tube = 46.2°C PASSED

PUMP INFO

Flow Rate = 5.411 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO

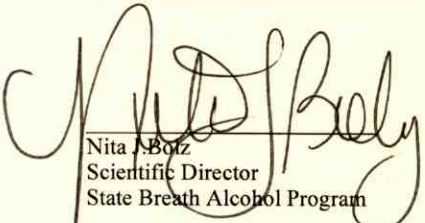
Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

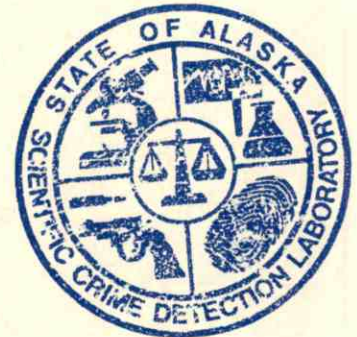

Nita J. Bolz
Scientific Director
State Breath Alcohol Program

10/16/2014

Subscribed and sworn before me this 16th day of Oct, 20 14



Nikki Roth, Notary Public
My Commission Expires With Office



003 10/16/14