



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100683

Report Issue Date: 06/13/2023
Date Received: 2023-03-06
Condition of Item: Good

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

Start Date 03/08/2023 - As Found - **End Date 03/08/2023** As Found - Evaluation Analyst: Tatiana Malnoske
 As Found Conditions - Barometric Pressure (inHg): 29.97 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.7
 Relative Humidity (%): 14%

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.021	0.020	
0.080	0.080	AG113402	0.079	0.079	0.079	0.079	0.080	0.079	
0.300	0.301	AG217903	0.298	0.298	0.298	0.298	0.298	0.298	

Start Date 04/11/2023 - As Left - **End Date 04/11/2023**
 As Left Conditions - Barometric Pressure (inHg): 29.65 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.8 Relative Humidity (%): 14

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.020	0.021	0.021	0.021	0.021	0.021	+/- 0.002
0.040	0.040	AG217904	0.040	0.039	0.040	0.040	0.039	0.040	+/- 0.003
0.080	0.079	AG113402	0.077	0.078	0.078	0.077	0.078	0.078	+/- 0.003
0.100	0.099	AG211003	0.098	0.099	0.099	0.099	0.099	0.099	+/- 0.003
0.150	0.149	AG134205	0.147	0.147	0.148	0.148	0.148	0.148	+/- 0.004
0.300	0.297	AG130502	0.293	0.293	0.293	0.293	0.293	0.293	+/- 0.008

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Colleen O'Bryant on 06/05/2023

colleen.obryant@alaska.gov

Technically and administratively reviewed by Brandi Barnett on 06/13/2023

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100683 Analyst: Tatiana Maliniche Start Date: 04/11/2023

- Diagnostic Test (attached)
- Adjust voltages, if needed
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
- Internal Standard value \leq 3.00%
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.6 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.65 Temperature (C): 22.8 Relative Humidity (%): 14%

Linearity Test (attached)

0.020g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG1217902</u>	Exp:	<u>06/28/2024</u>
0.040g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG1217904</u>	Exp:	<u>06/28/2024</u>
0.080g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG1113402</u>	Exp:	<u>05/14/2023</u>
0.100g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG1211003</u>	Exp:	<u>04/20/2024</u>
0.150g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG134205</u>	Exp:	<u>12/08/2023</u>
0.300g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG130502</u>	Exp:	<u>11/01/2023</u>

Functional Tests (attached)

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles)
- Acetone Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/09/2023
Simulator S/N: DK4161 Verification Performed?
- Isopropanol Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/09/2023
Simulator S/N: SD1088 Verification Performed?
- Neg. Control Mnf: Lifeloc Lot: 21KP41172 Level: 0.100 Exp: 11/09/2023
Simulator S/N: SD1177 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/09/2023

- Verify stylus is calibrated
- Non-Drinking Subject Test
- Reset Options
- Upload
- Clear Memory
- Remove Tank Prior to Shutdown
- Verification of Calibration (VOC)
- Calibration End Date: 04/11/2023

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 06:43:10

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.76 V PASSED
(1.17 V - 2.73 V)
Cooler Voltage = 1.79 V PASSED
(1.13 V - 2.65 V)
Bias Voltage = 79 V PASSED
(47 V - 111 V)
Chopper Freq = 530 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.144 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED

Xq = 0.103 2.00% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 6:59 AM

Temperatures (°C)

Sample Cell: 48.7°C
Breath Tube: 47.8°C

Current Barometer 29.6 in
Volume (Ltr) 1.50

Settings

Lamp: 1.76 V
Bias: 79 V
Cooler: 1.79 V
Chopper: 529 Hz

Voltages (V)

Flow: 1.02 V
Detector: -0.082 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 09/01/2022
Time: 11:28:48

OPERATOR NAME:
TATIANA MALNOSKE
CERTIFICATE #: 10437

Ca = 0.1000
CAL = 0.965272 0.800 <= CAL < 1.200
b1 = 0.0011 0.0000 <= b1 < 0.0040
b2 = 0.0076 0.0010 <= b2 < 0.0100
b3 = 0.0005 0.0000 <= b3 < 0.0040
Xq = 0.1052 0.0500 <= Xq < 0.2000
a21 = 1.200662 1.050 <= a21 < 1.300
a31 = 0.521225 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 07:01:12


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	07:02
BLANK TEST	0.000	07:02
INTERNAL STANDARD	VERIFIED	07:02
EXTERNAL STANDARD	0.077	07:02
BLANK TEST	0.000	07:03
SUBJECT SAMPLE (Vol=1.58L)	0.000	07:04
BLANK TEST	0.000	07:05
EXTERNAL STANDARD	0.078	07:05
BLANK TEST	0.000	07:06

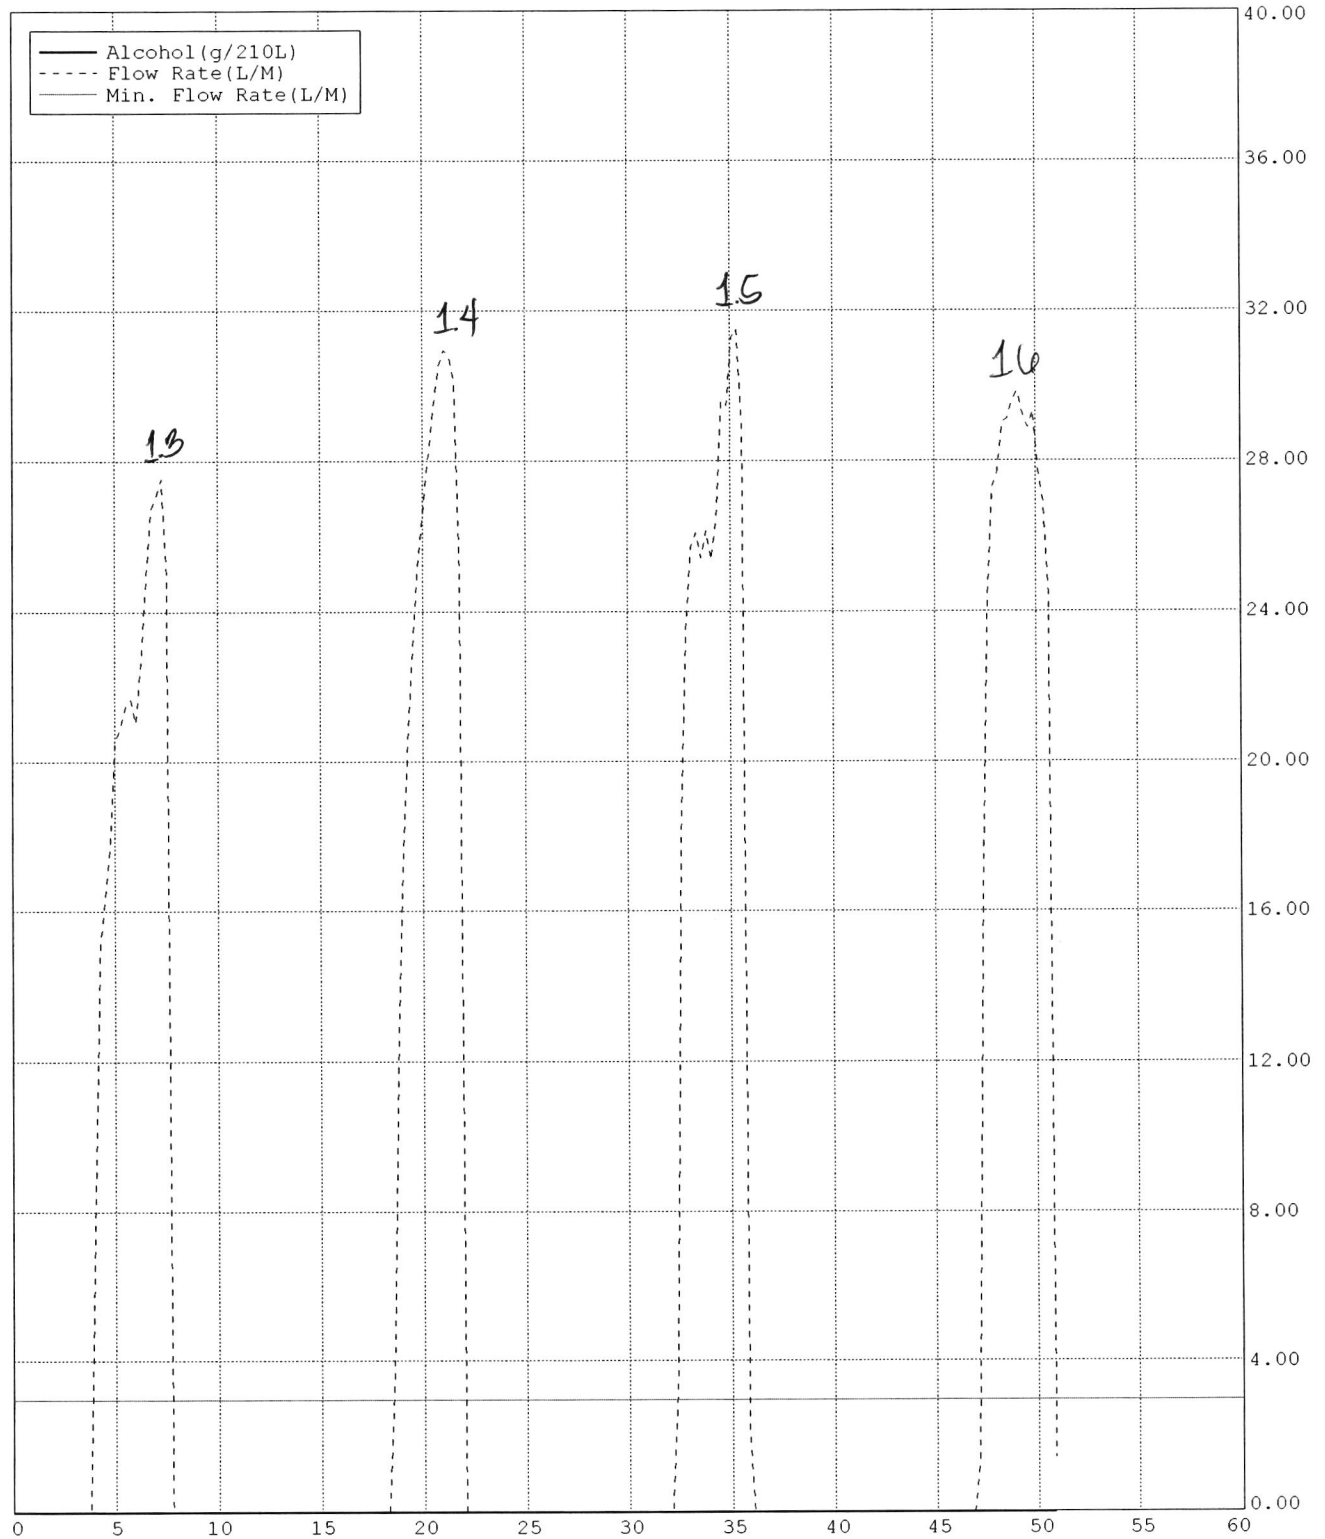

LINEARITY CHECK

Alaska Department of Public Safety
DATAMASTER dmt: 100683


Date: 04/11/2023
Time: 07:08:35

SUPERVISOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

TARGET	AVERAGE	STD. DEV.
0.020	0.0208	0.0004
0.040	0.0396	0.0005
0.079	0.0776	0.0005
0.099	0.0988	0.0004
0.149	0.1476	0.0005
0.297	0.2930	0.0000

SLOPE = 0.984654
R² = 0.999967

TMM

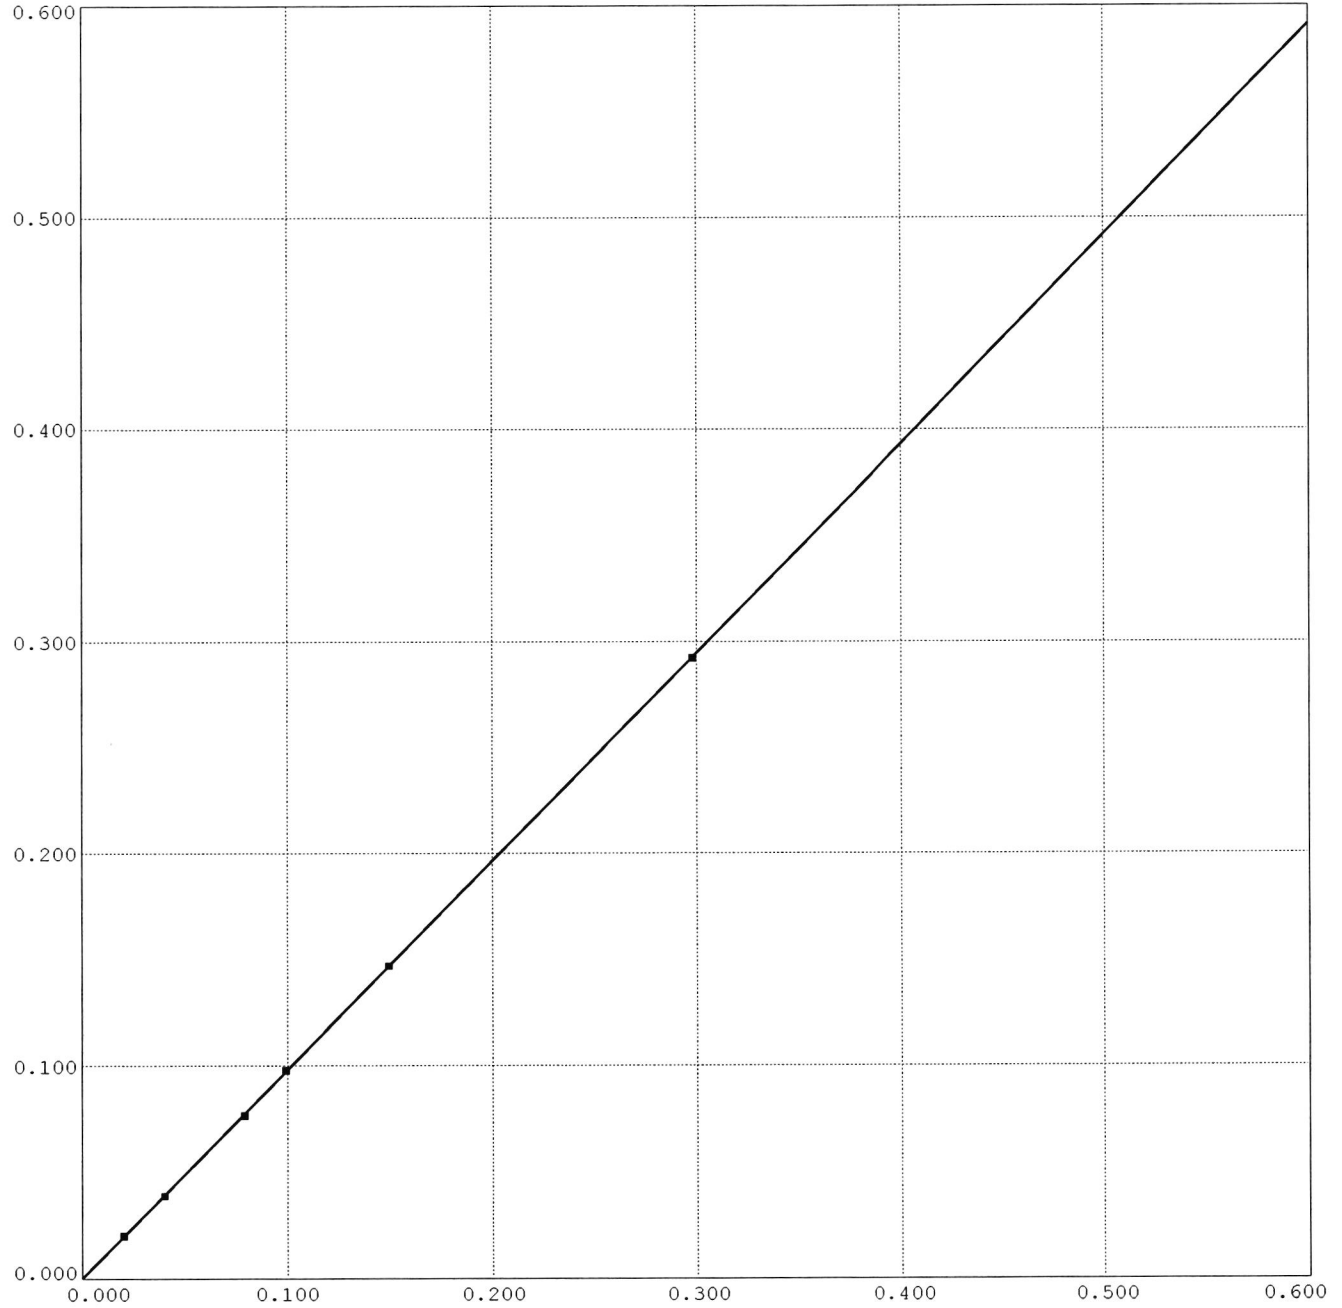

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100683






Date: 04/11/2023
Time: 07:08:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.65: 0.020
LOT #: AG217902
EXPIRATION: 06/28/2024
TANK PRESSURE: 866 psi

BLANK TEST	0.000	07:09
INTERNAL STANDARD	VERIFIED	07:10
EXTERNAL STANDARD	0.020	07:10
BLANK TEST	0.000	07:11
EXTERNAL STANDARD	0.021	07:11
BLANK TEST	0.000	07:12
EXTERNAL STANDARD	0.021	07:12
BLANK TEST	0.000	07:13
EXTERNAL STANDARD	0.021	07:13
BLANK TEST	0.000	07:14
EXTERNAL STANDARD	0.021	07:14
BLANK TEST	0.000	07:15

Average = 0.0208
Std Dev = 0.0004

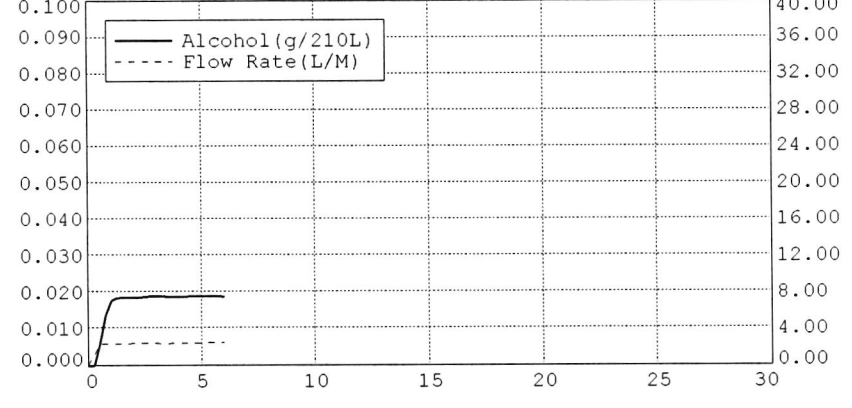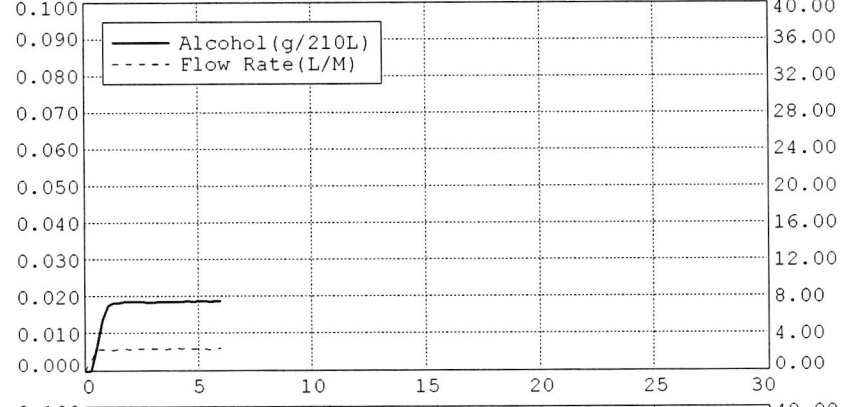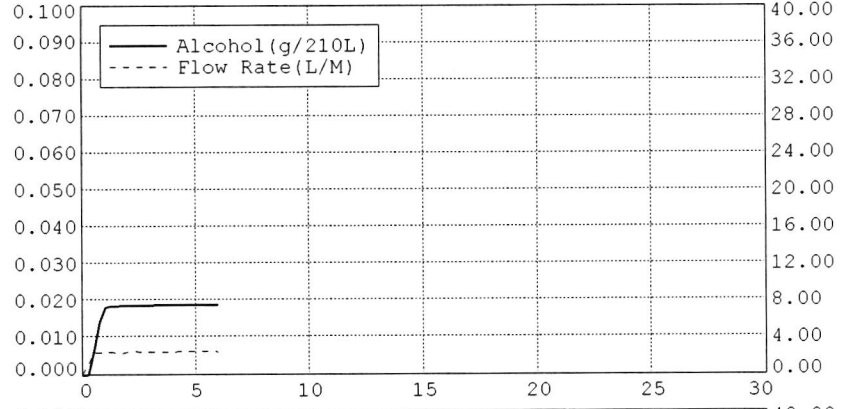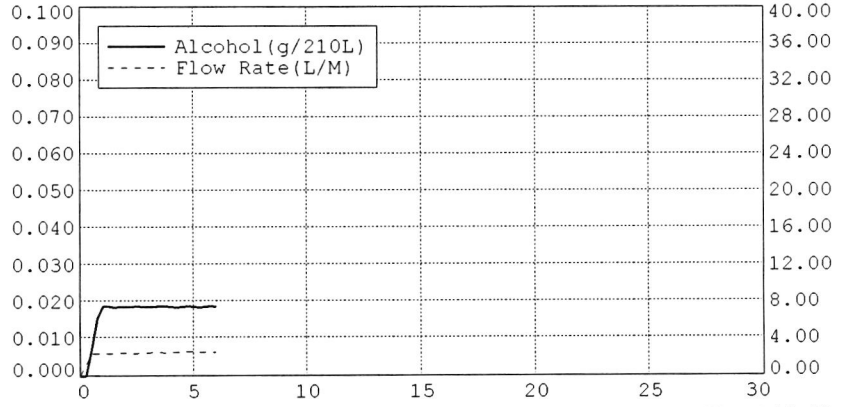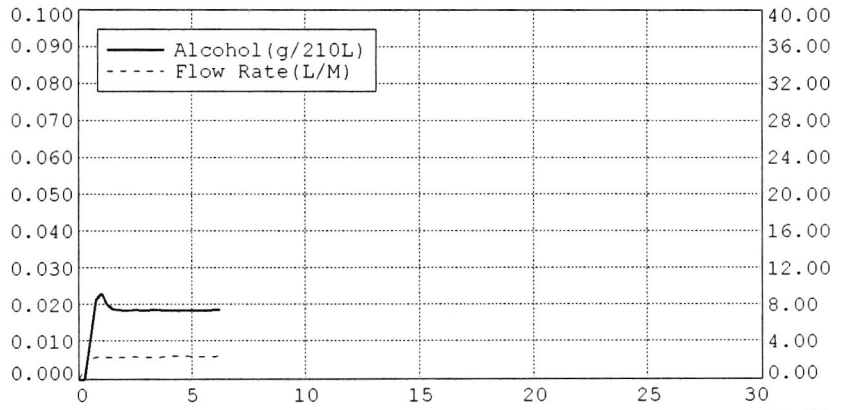

LINEARITY CHECK: Control Test 2

 Alaska Department of Public Safety
 DATAMASTER dmt: 100683






Date: 04/11/2023
 Time: 07:19:07

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.65: 0.040
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 986 psi

BLANK TEST	0.000	07:20
INTERNAL STANDARD	VERIFIED	07:20
EXTERNAL STANDARD	0.040	07:20
BLANK TEST	0.000	07:21
EXTERNAL STANDARD	0.039	07:21
BLANK TEST	0.000	07:22
EXTERNAL STANDARD	0.040	07:22
BLANK TEST	0.000	07:23
EXTERNAL STANDARD	0.040	07:23
BLANK TEST	0.000	07:24
EXTERNAL STANDARD	0.039	07:25
BLANK TEST	0.000	07:25

Average = 0.0396
 Std Dev = 0.0005

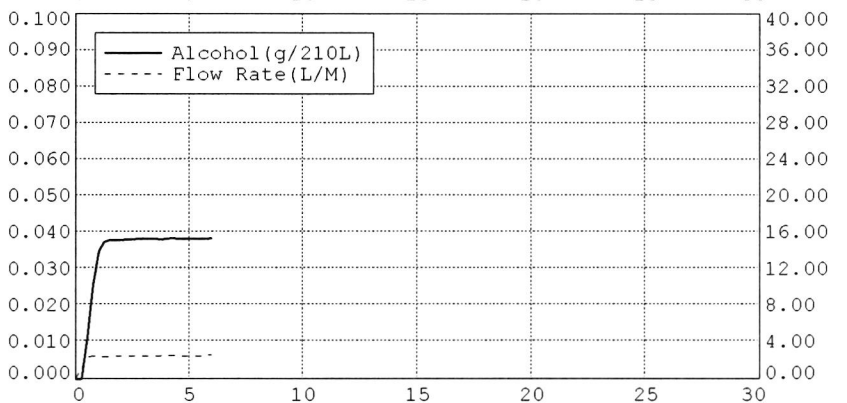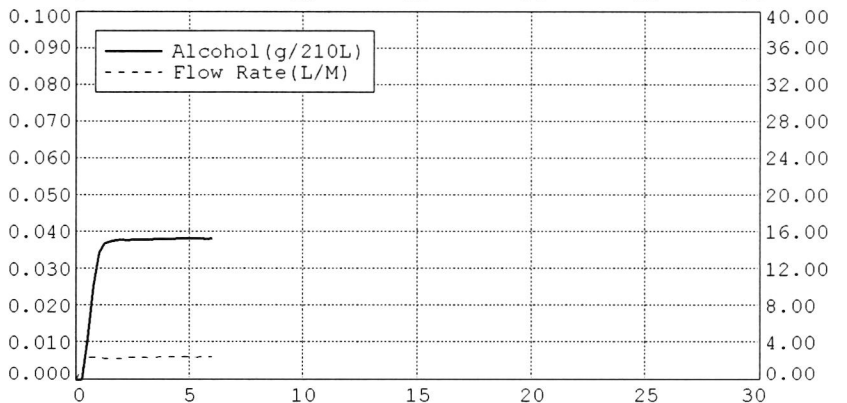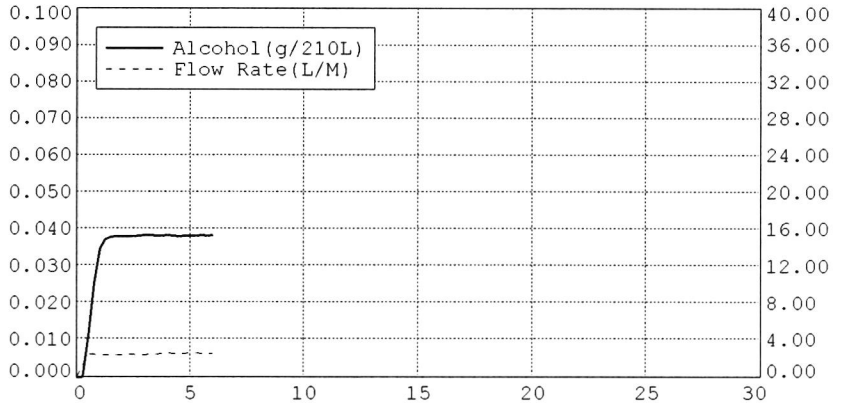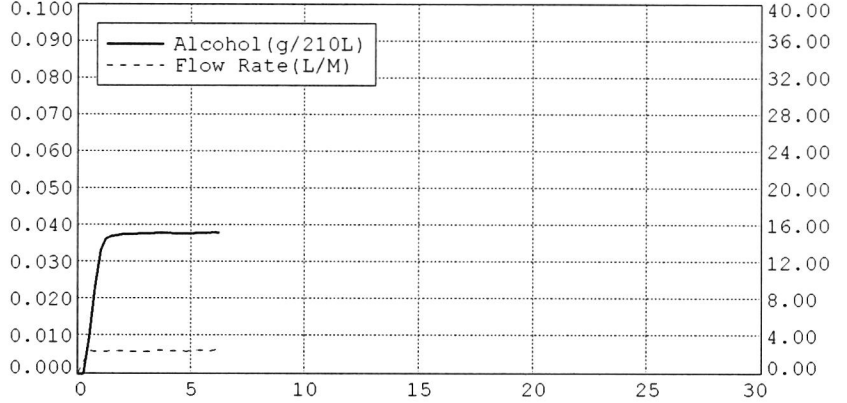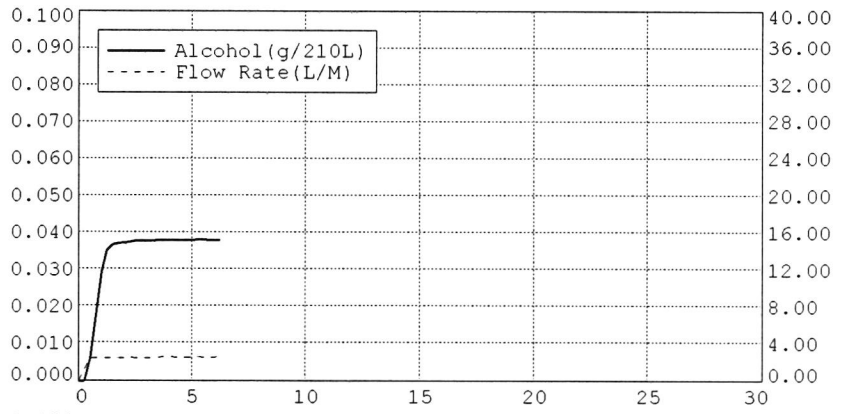

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100683






Date: 04/11/2023
 Time: 07:26:36

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.65: 0.079
 LOT #: AG113402
 EXPIRATION: 05/14/2023
 TANK PRESSURE: 288 psi

BLANK TEST	0.000	07:27
INTERNAL STANDARD	VERIFIED	07:27
EXTERNAL STANDARD	0.077	07:28
BLANK TEST	0.000	07:29
EXTERNAL STANDARD	0.078	07:29
BLANK TEST	0.000	07:30
EXTERNAL STANDARD	0.078	07:30
BLANK TEST	0.000	07:31
EXTERNAL STANDARD	0.077	07:31
BLANK TEST	0.000	07:32
EXTERNAL STANDARD	0.078	07:32
BLANK TEST	0.000	07:33

Average = 0.0776
 Std Dev = 0.0005

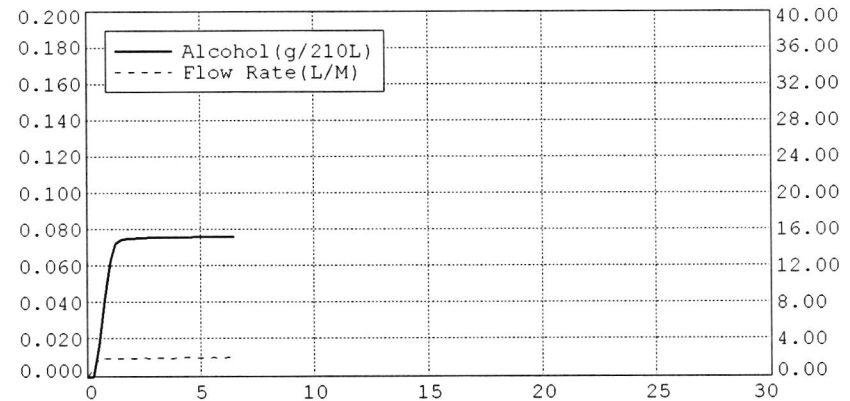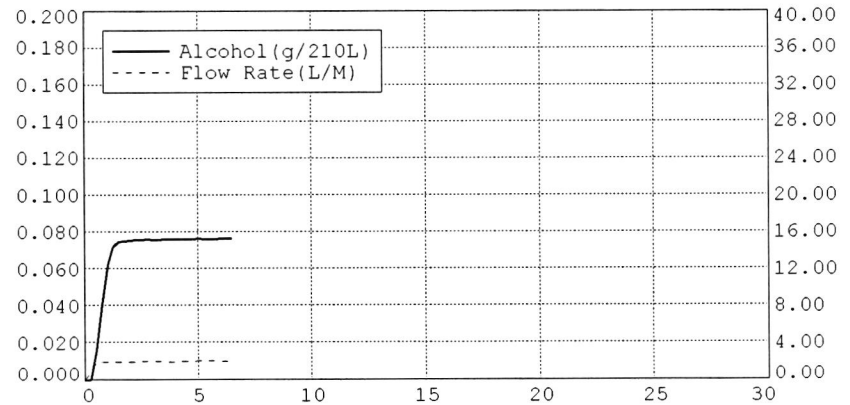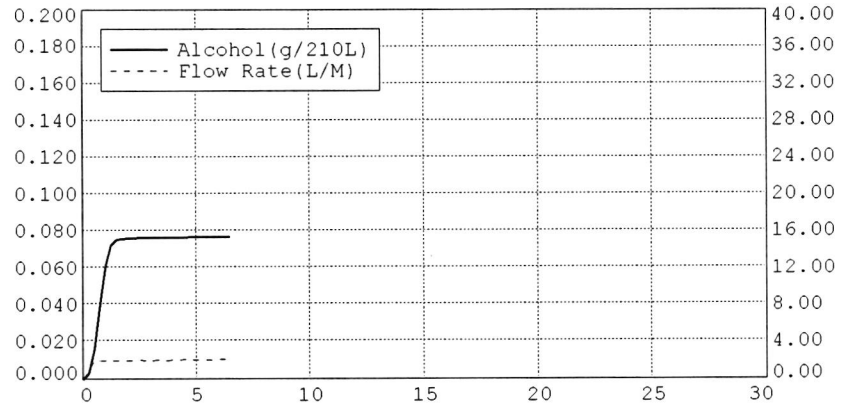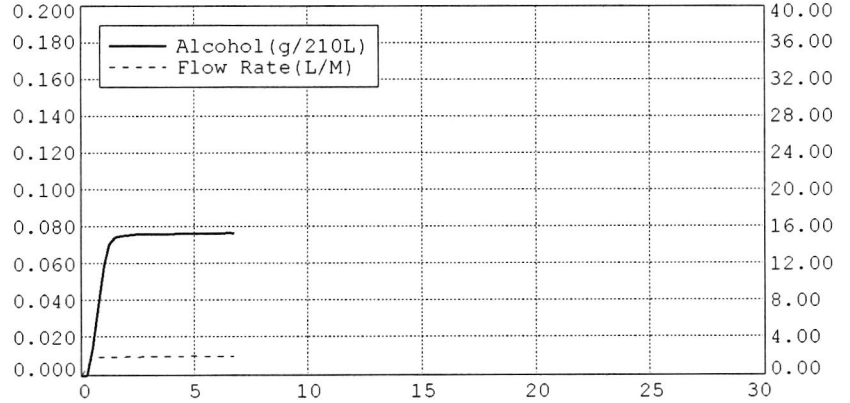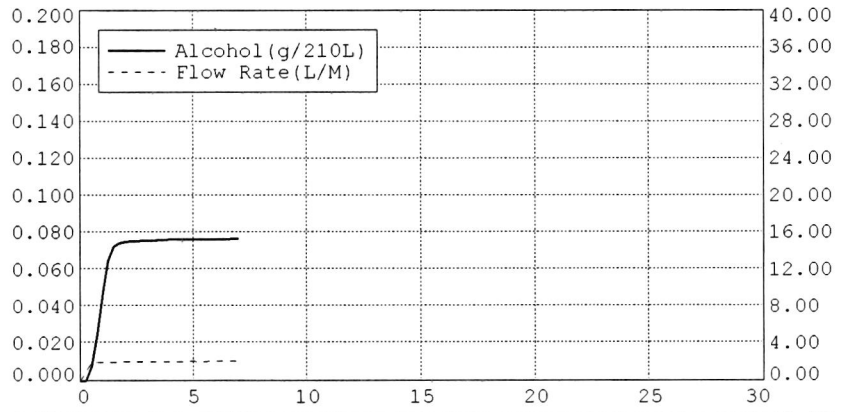

LINEARITY CHECK: Control Test 4






Alaska Department of Public Safety
 DATAMASTER dmt: 100683

Date: 04/11/2023
 Time: 07:34:05

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.100
 TARGET AT 29.65: 0.099
 LOT #: AGG211003 AG211003 TLM 04/12/23
 EXPIRATION: 04/20/2024
 TANK PRESSURE: 956 psi

BLANK TEST	0.000	07:35
INTERNAL STANDARD	VERIFIED	07:35
EXTERNAL STANDARD	0.098	07:35
BLANK TEST	0.000	07:36
EXTERNAL STANDARD	0.099	07:36
BLANK TEST	0.000	07:37
EXTERNAL STANDARD	0.099	07:37
BLANK TEST	0.000	07:38
EXTERNAL STANDARD	0.099	07:39
BLANK TEST	0.000	07:39
EXTERNAL STANDARD	0.099	07:40
BLANK TEST	0.000	07:41

Average = 0.0988
 Std Dev = 0.0004

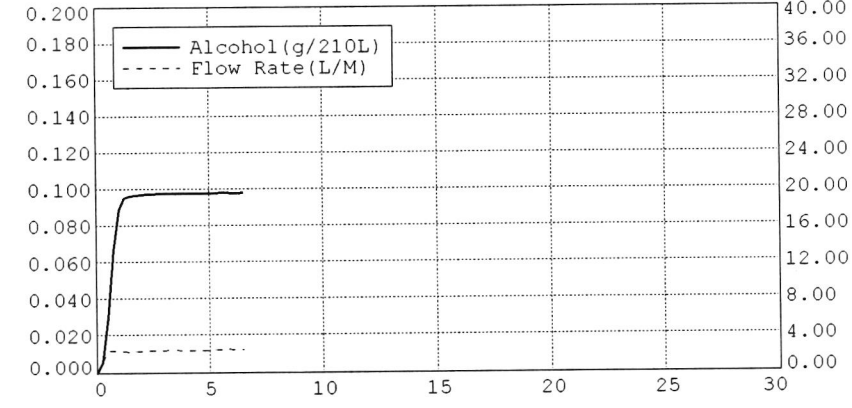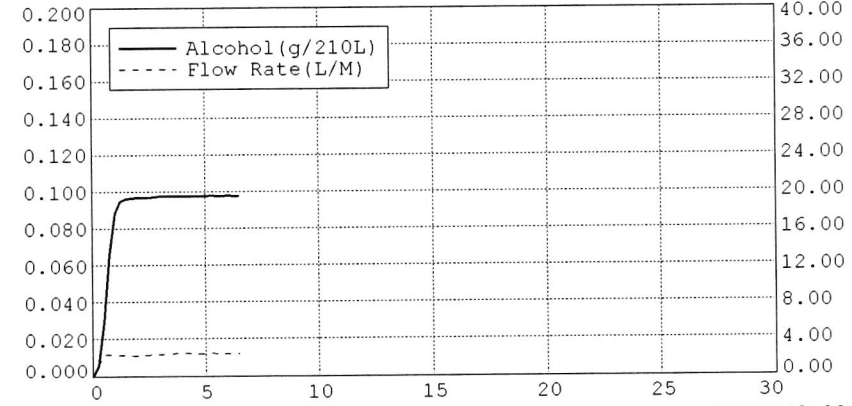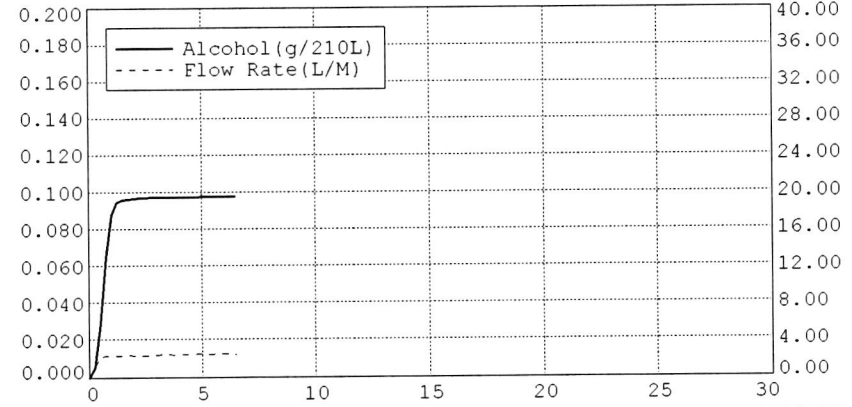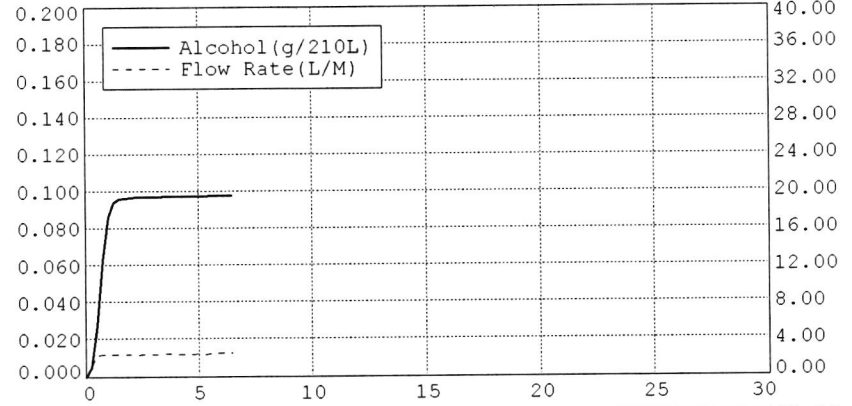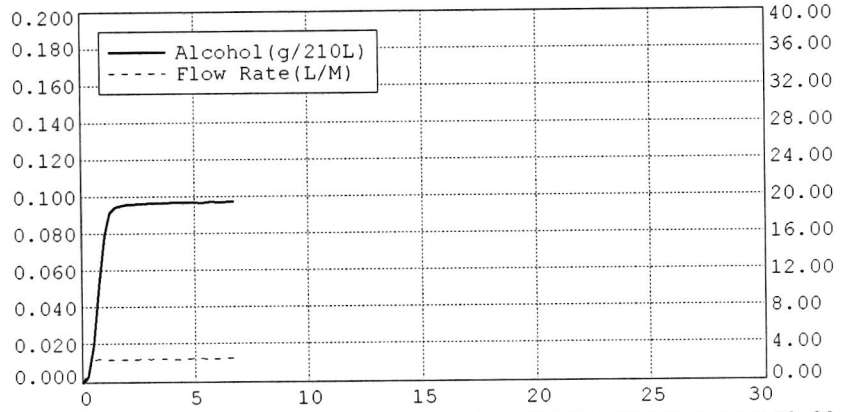

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100683






Date: 04/11/2023
 Time: 08:04:55

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.64: 0.149
 LOT #: AG134205
 EXPIRATION: 12/08/2023
 TANK PRESSURE: 958 psi

BLANK TEST	0.000	08:06
INTERNAL STANDARD	VERIFIED	08:06
EXTERNAL STANDARD	0.147	08:06
BLANK TEST	0.000	08:07
EXTERNAL STANDARD	0.147	08:07
BLANK TEST	0.000	08:08
EXTERNAL STANDARD	0.148	08:08
BLANK TEST	0.000	08:09
EXTERNAL STANDARD	0.148	08:10
BLANK TEST	0.000	08:10
EXTERNAL STANDARD	0.148	08:11
BLANK TEST	0.000	08:12

Average = 0.1476
 Std Dev = 0.0005

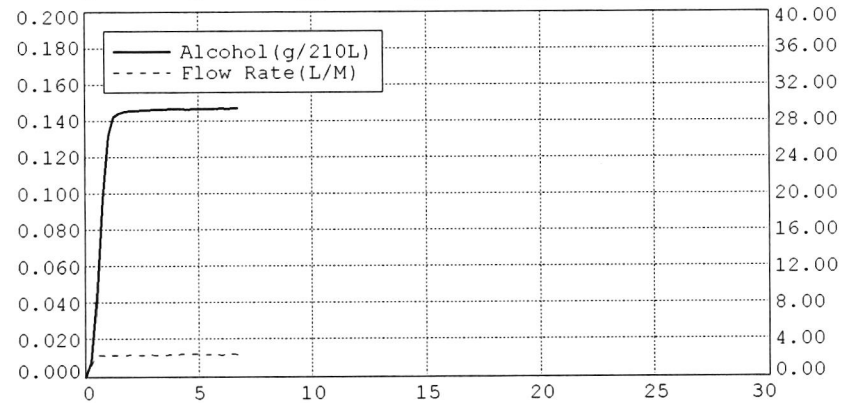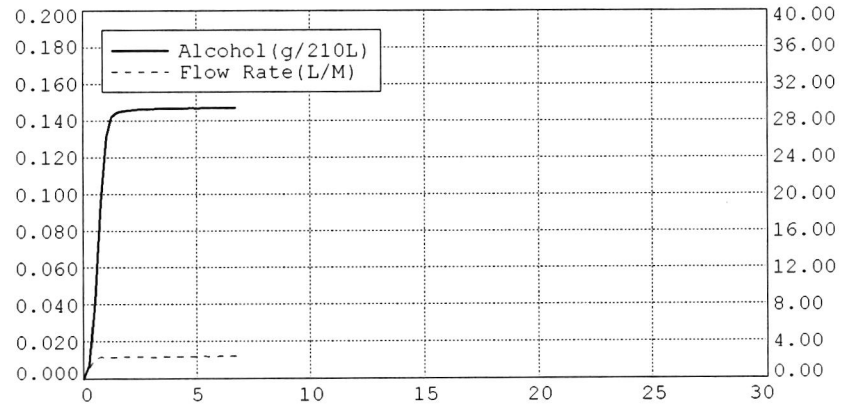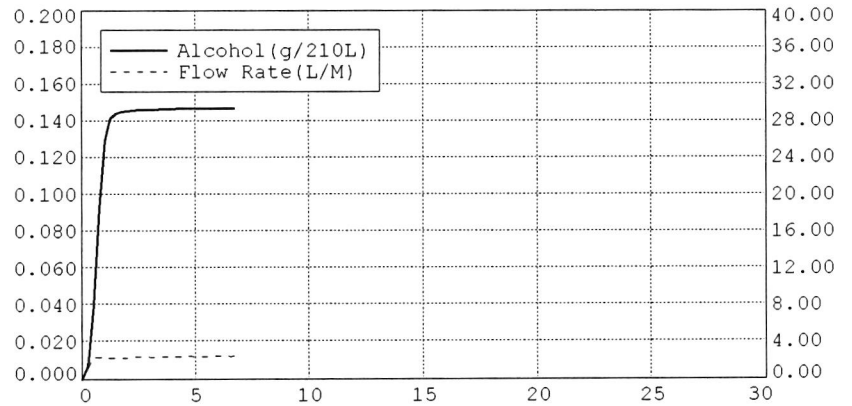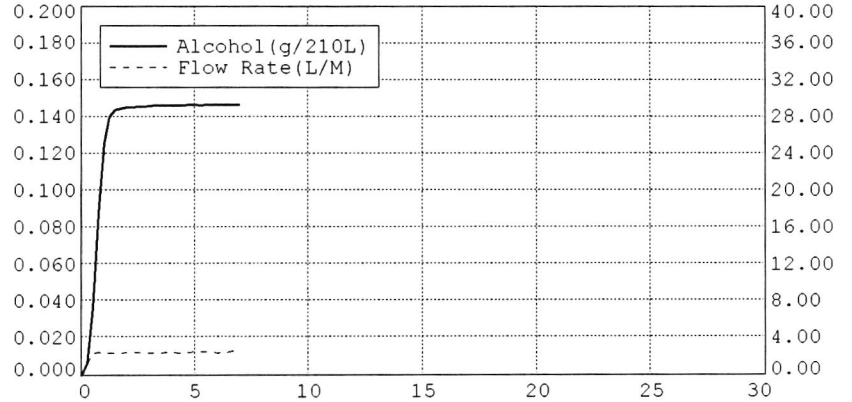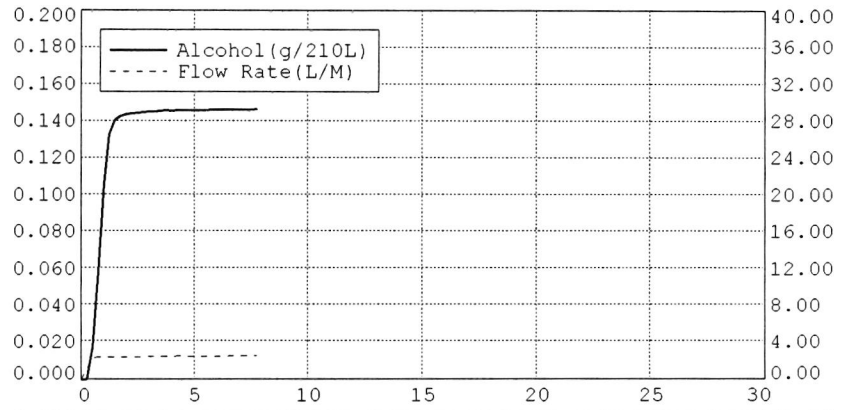

LINEARITY CHECK: Control Test 6

 Alaska Department of Public Safety
 DATAMASTER dmt: 100683






Date: 04/11/2023
 Time: 08:12:31

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.64: 0.297
 LOT #: AG130502
 EXPIRATION: 11/01/2023
 TANK PRESSURE: 121 psi

BLANK TEST	0.000	08:13
INTERNAL STANDARD	VERIFIED	08:13
EXTERNAL STANDARD	0.293	08:14
BLANK TEST	0.000	08:15
EXTERNAL STANDARD	0.293	08:15
BLANK TEST	0.000	08:16
EXTERNAL STANDARD	0.293	08:16
BLANK TEST	0.000	08:17
EXTERNAL STANDARD	0.293	08:17
BLANK TEST	0.000	08:18
EXTERNAL STANDARD	0.293	08:18
BLANK TEST	0.000	08:19

Average = 0.2930
 Std Dev = 0.0000

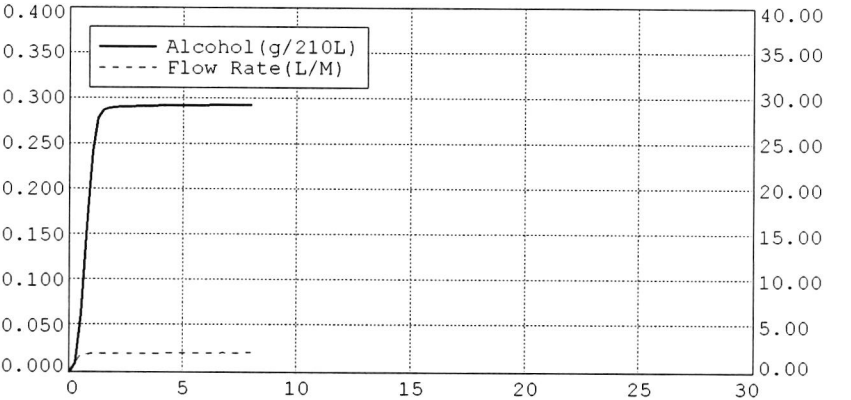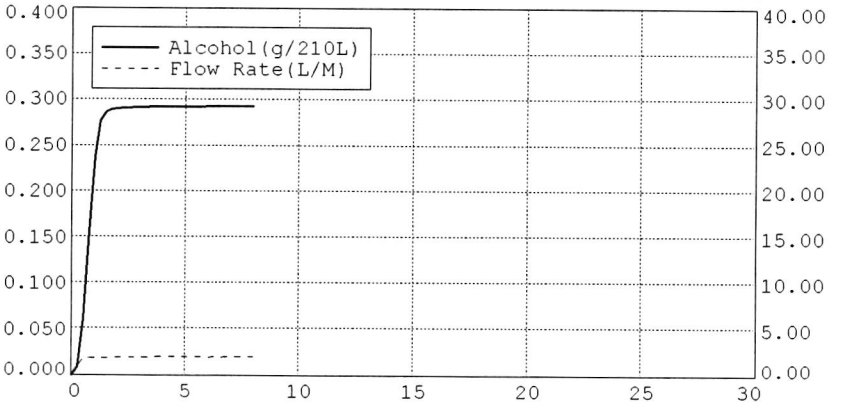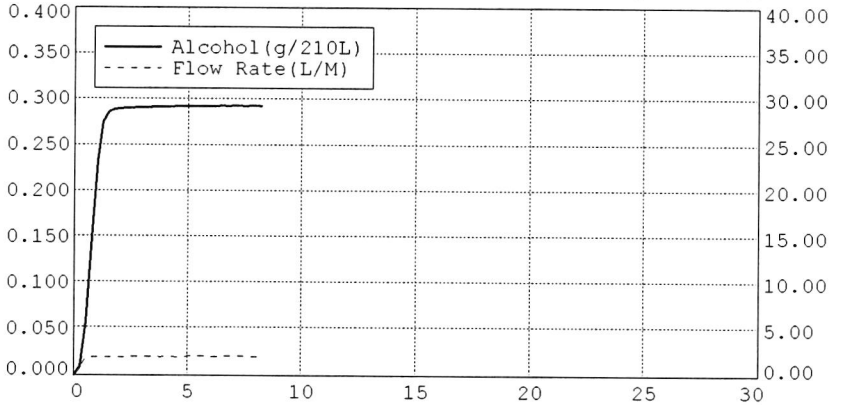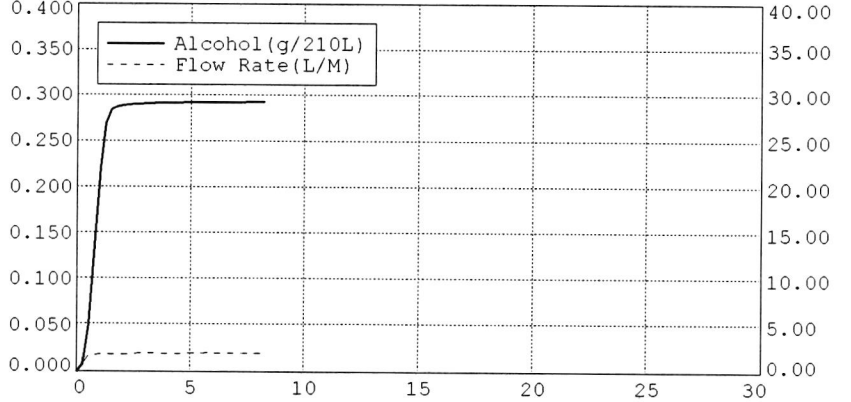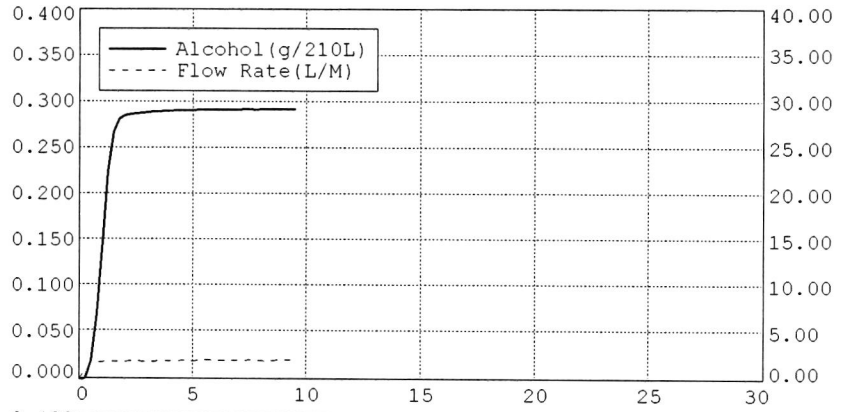

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 09:01:52


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.65: 0.079
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:02
BLANK TEST	0.000	09:02
INTERNAL STANDARD	VERIFIED	09:03
EXTERNAL STANDARD	0.078	09:03
BLANK TEST	0.000	09:04
SUBJECT SAMPLE	INCOMPLETE	09:06

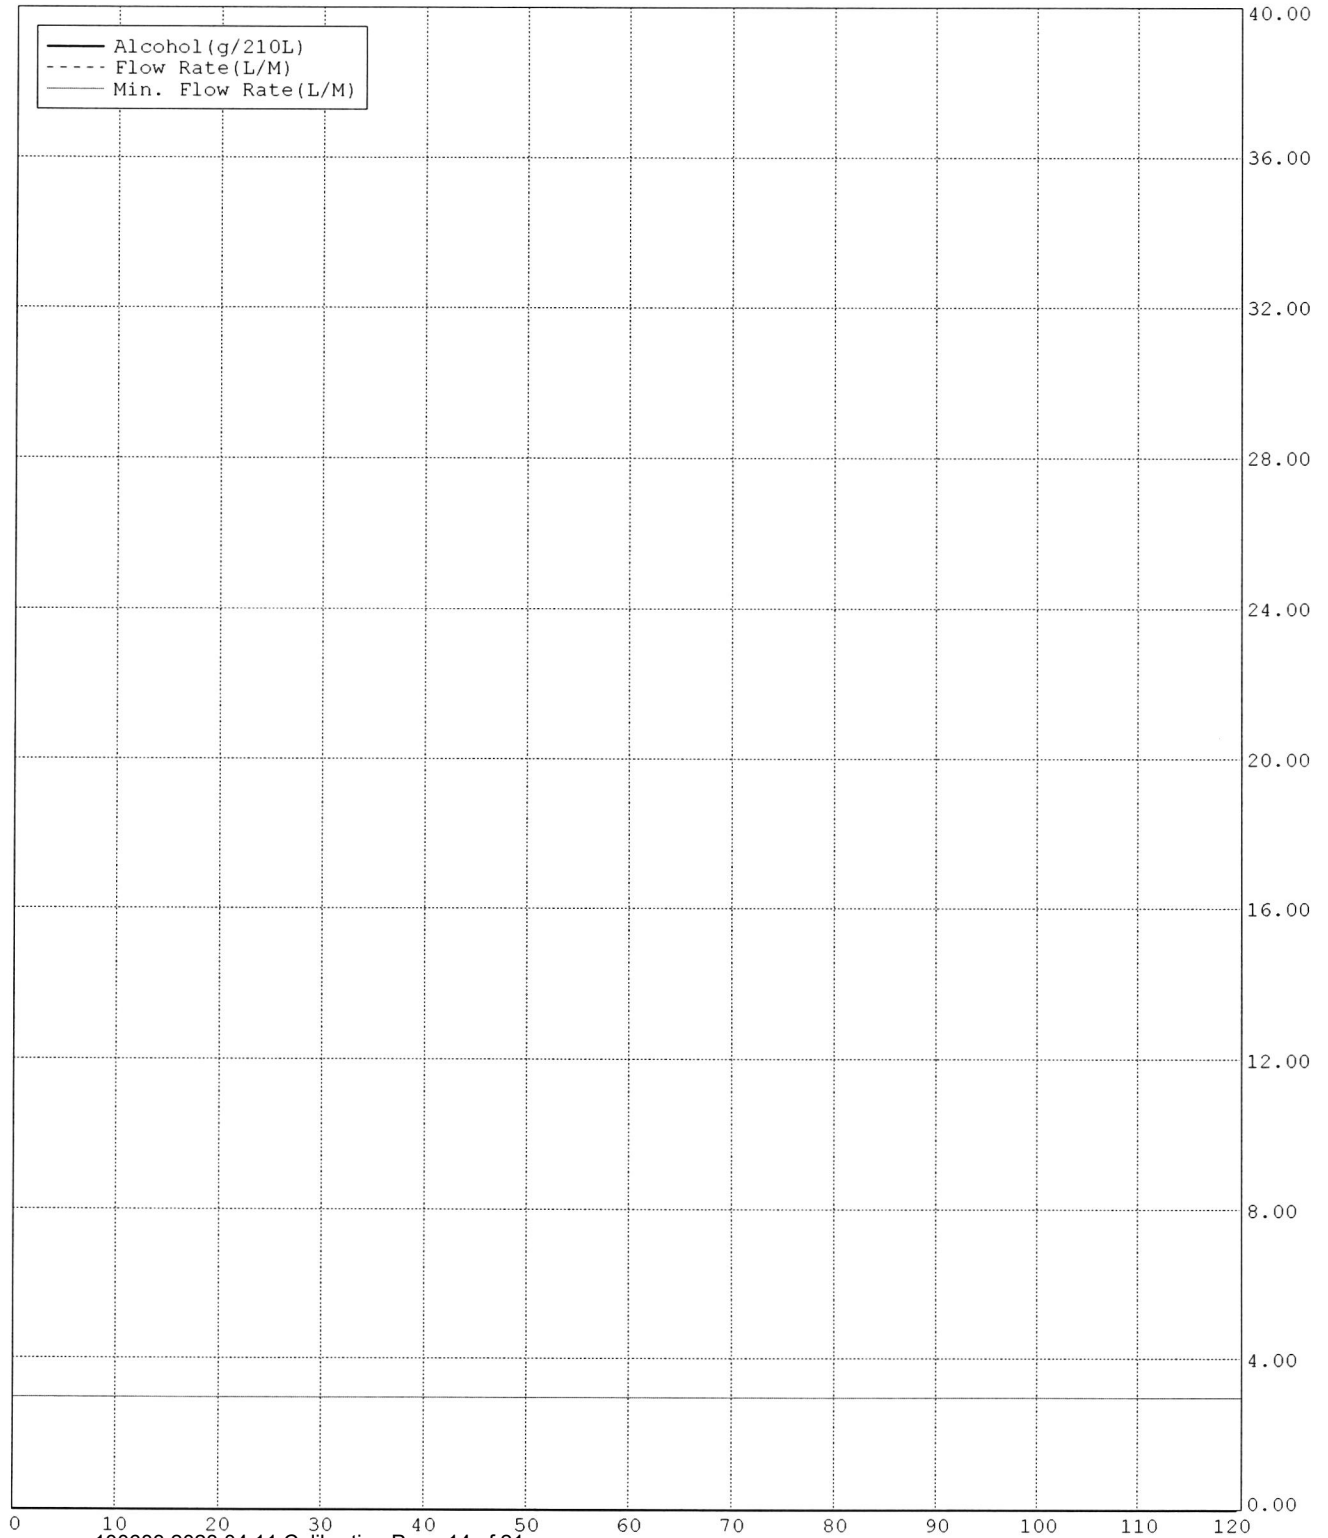

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 09:13:30

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:14
BLANK TEST	0.000	09:14
INTERNAL STANDARD	VERIFIED	09:14
EXTERNAL STANDARD	0.078	09:14
BLANK TEST	0.000	09:15
SUBJECT SAMPLE	XXX	09:16

Maximum Attempts Exceeded

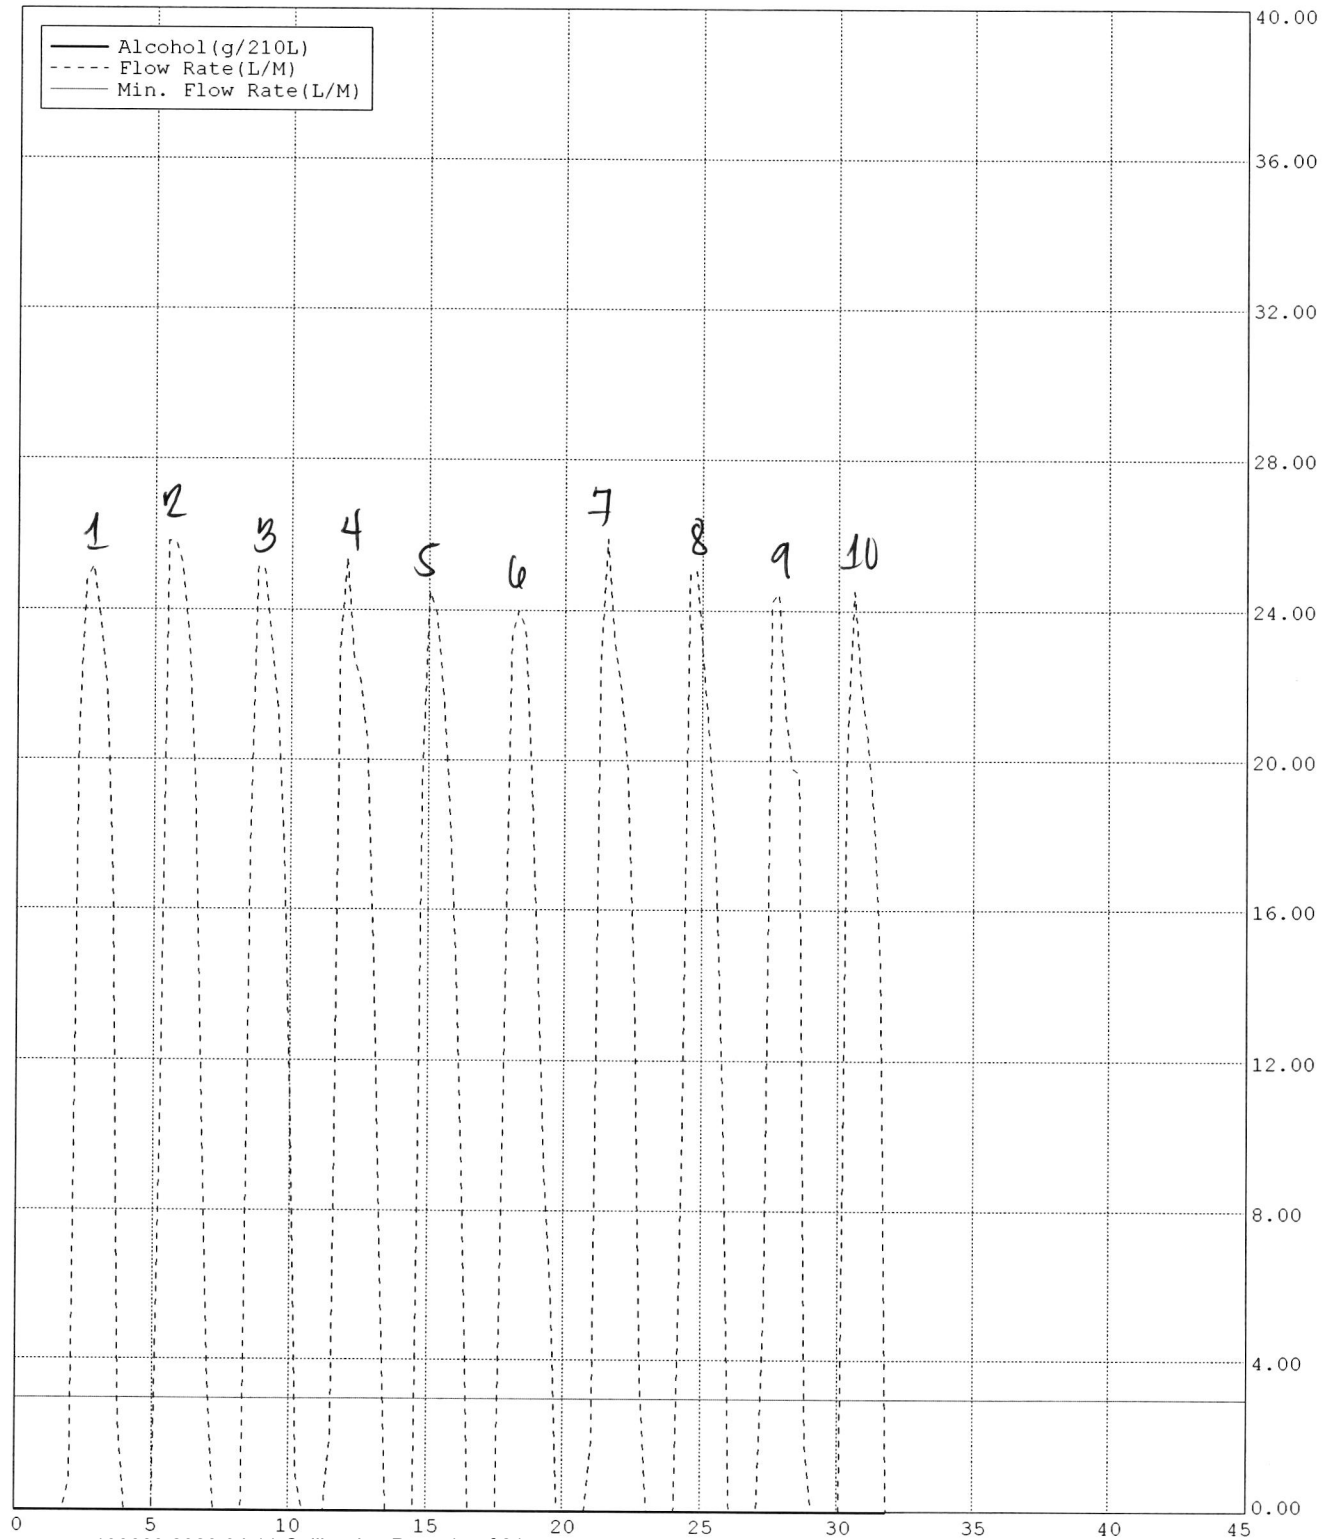

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 09:34:34


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.65: 0.079
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:35
BLANK TEST	0.000	09:35
INTERNAL STANDARD	VERIFIED	09:35
EXTERNAL STANDARD	0.076	09:36
BLANK TEST	0.000	09:36
SUBJECT SAMPLE	INVALID	09:37

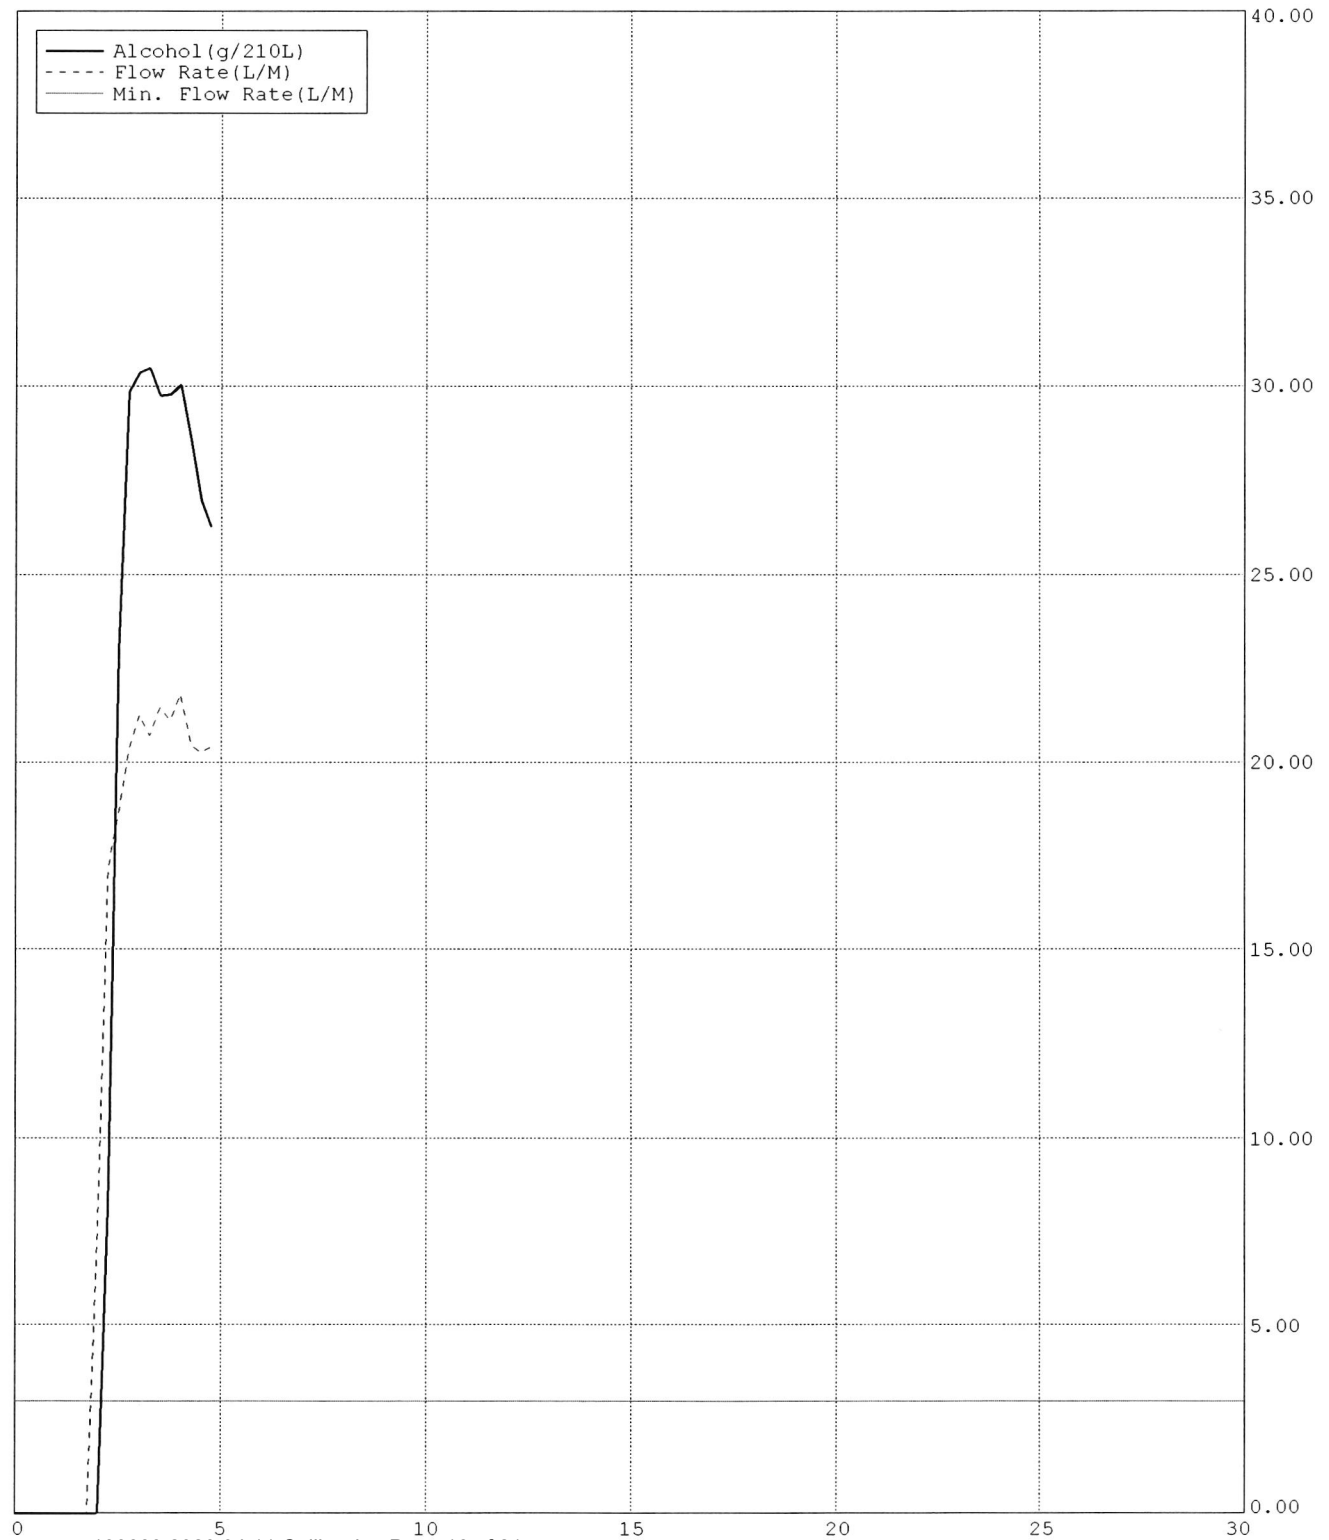

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 09:43:07

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
RADIO FREQUENCY INTERFERENCE (RFI)
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.65: 0.079
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:44
BLANK TEST	0.000	09:44
INTERNAL STANDARD	VERIFIED	09:44
EXTERNAL STANDARD	0.077	09:44
BLANK TEST	0.000	09:45

RFI DETECTED

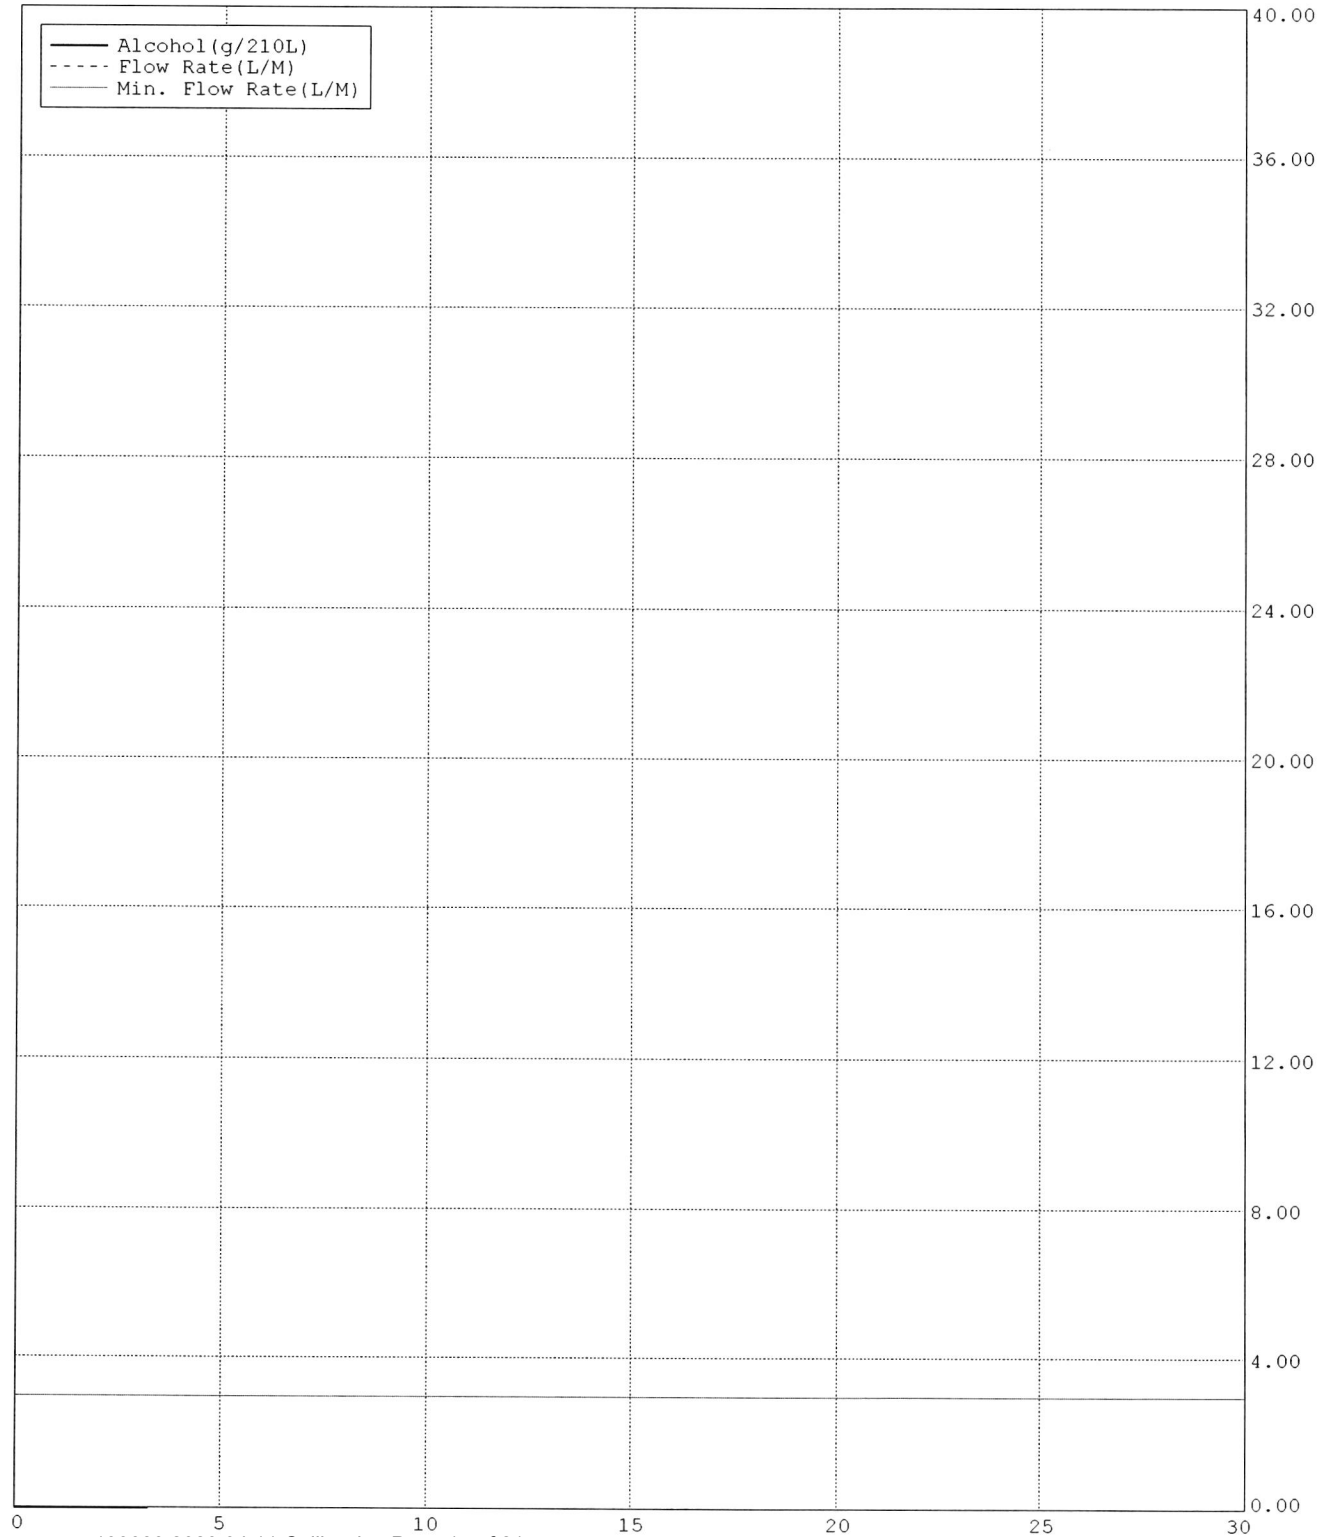

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 08:42:07

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INTERFERENCE DETECTED - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG113402
EXPIRATION: 05/14/2023


DIAGNOSTIC CHECK	PASSED	08:43
BLANK TEST	0.000	08:43
INTERNAL STANDARD	VERIFIED	08:43
Xq = 0.104 (0.92%)		
EXTERNAL STANDARD	0.077	08:43
X[1] = 0.0774 (-0.0026) (0.0042)		
BLANK TEST	0.000	08:44
SUBJECT SAMPLE	XXX	08:45
X[1] = 0.1040 (-0.0184) (0.0017)		

Interference Detected

Filter 2 Average μ : -0.0024

Filter 3 Average: 0.0032

04/11/23 TMM

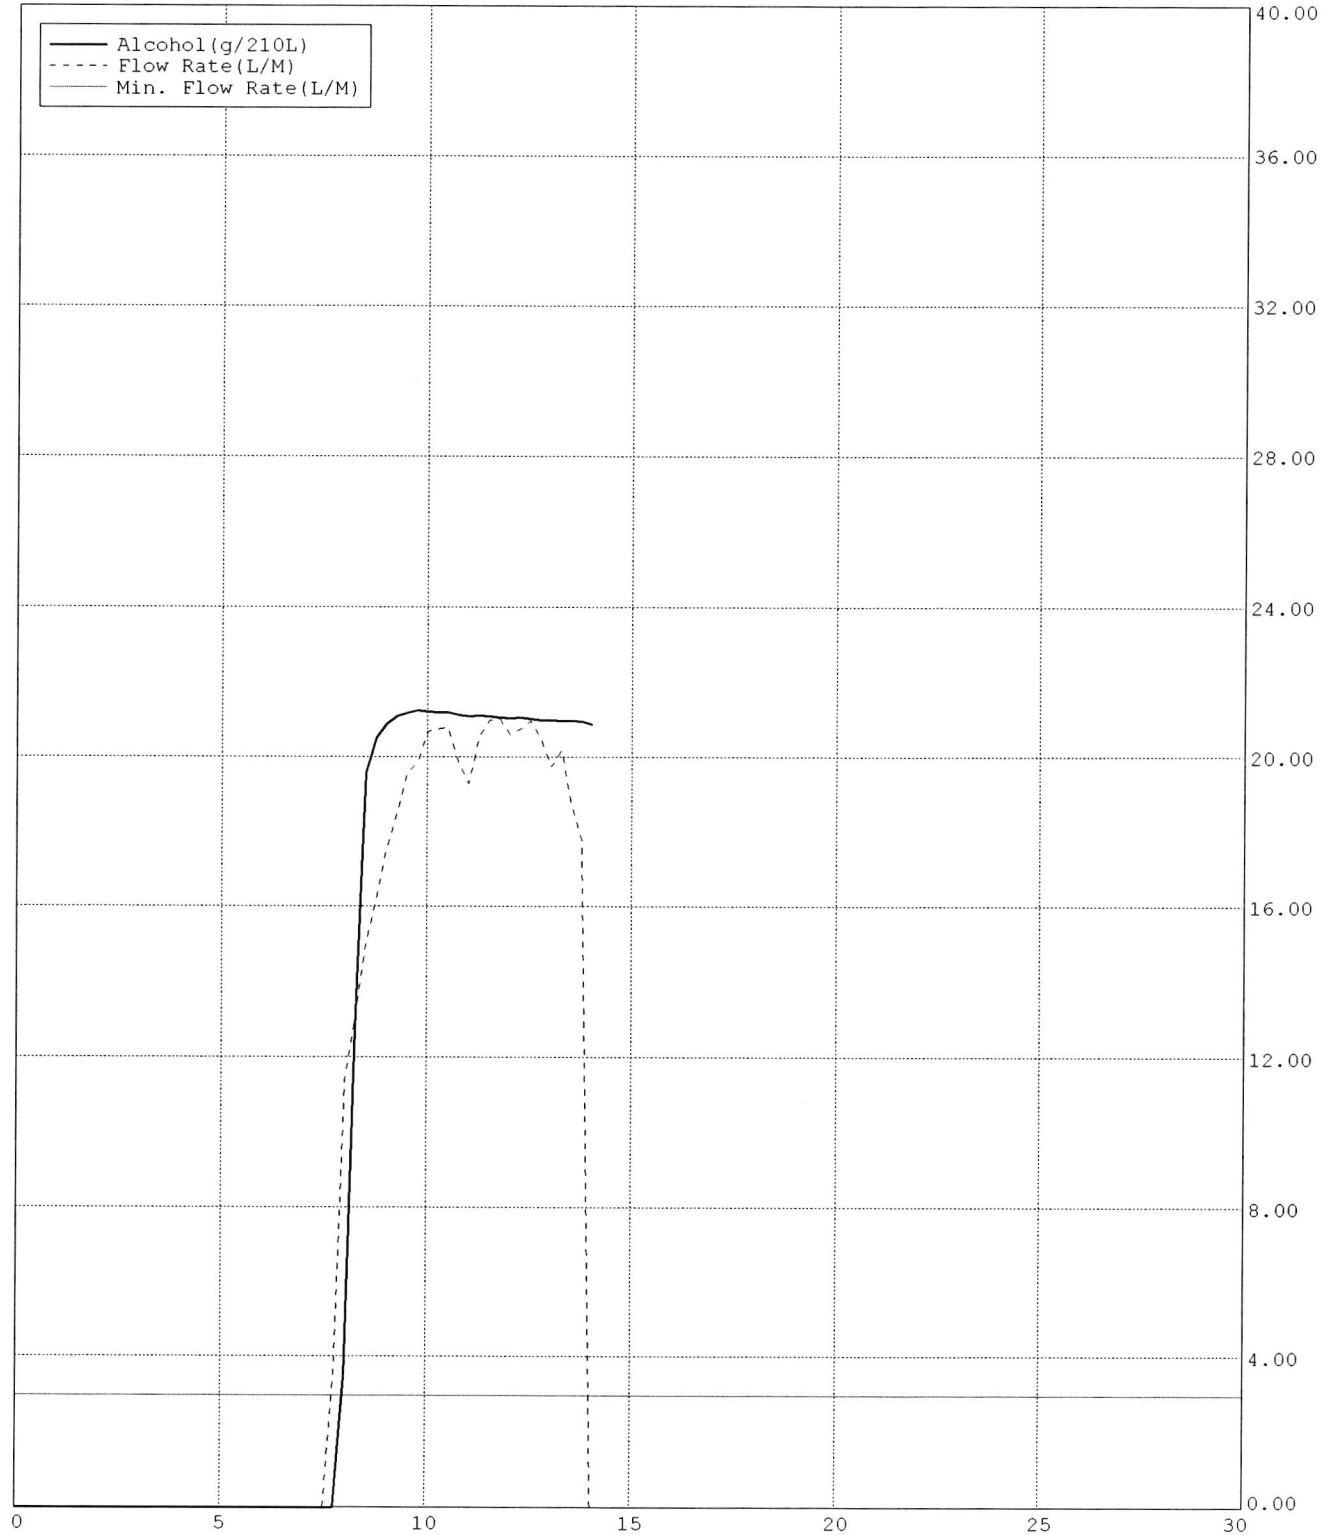

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 08:46:43

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INTERFERENCE DETECTED - ISOPROPANOL
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.65: 0.079
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	08:48
BLANK TEST	0.000	08:48
INTERNAL STANDARD	VERIFIED	08:48
Xq = 0.105 (0.42%)		
EXTERNAL STANDARD	0.078	08:48
X[1] = 0.0776 (-0.0021) (0.0025)		
BLANK TEST	0.000	08:49
SUBJECT SAMPLE	XXX	08:49
X[1] = 0.1143 (-0.0337) (0.0016)		

Interference Detected

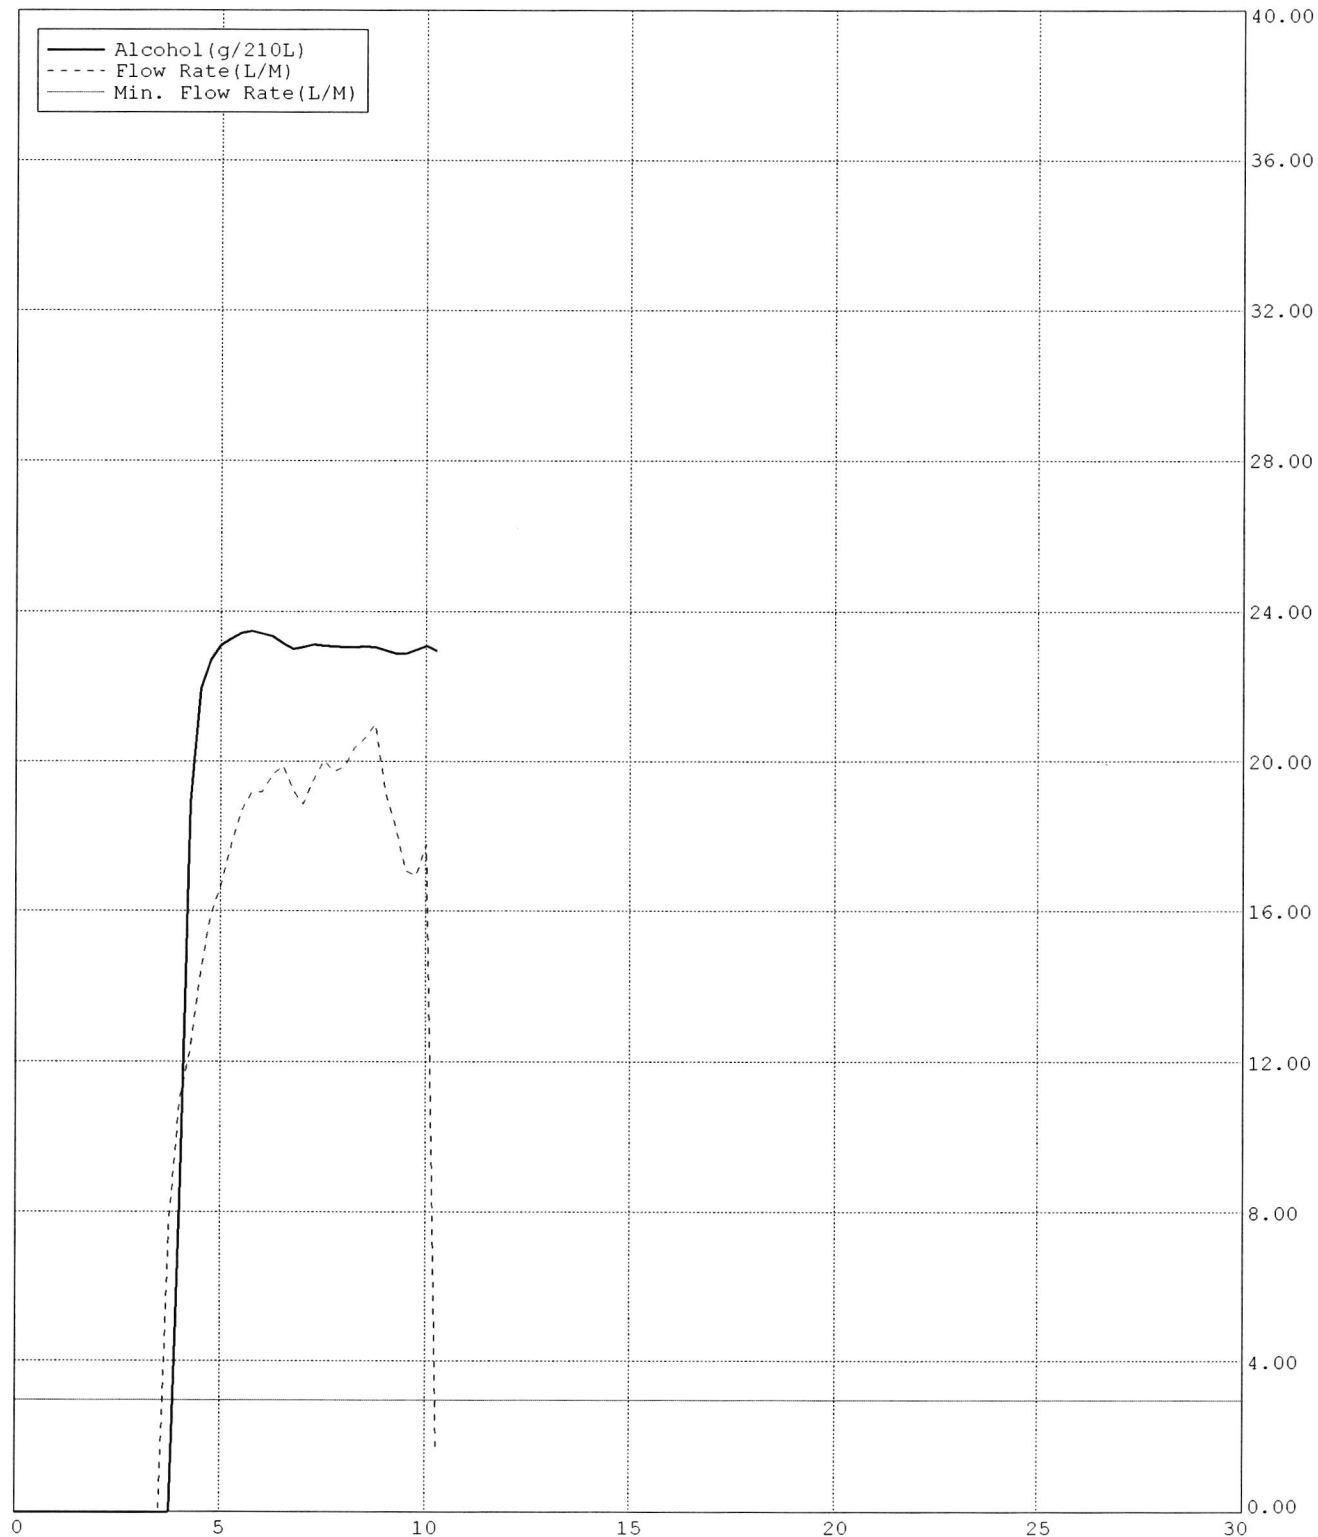

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 08:52:05


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INTERFERENCE DETECTED - NEGATIVE CONTROL
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.65: 0.079
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	08:53
BLANK TEST	0.000	08:53
INTERNAL STANDARD	VERIFIED	08:53
Xq = 0.105 (0.00%)		
EXTERNAL STANDARD	0.078	08:53
X[1] = 0.0780 (-0.0024) (0.0031)		
BLANK TEST	0.000	08:54
SUBJECT SAMPLE (Vol=1.91L)	0.090	08:55
X[1] = 0.0903 (-0.0015) (0.0016)		
BLANK TEST	0.000	08:56
EXTERNAL STANDARD	0.077	08:56
X[1] = 0.0768 (-0.0023) (0.0031)		
BLANK TEST	0.000	08:57

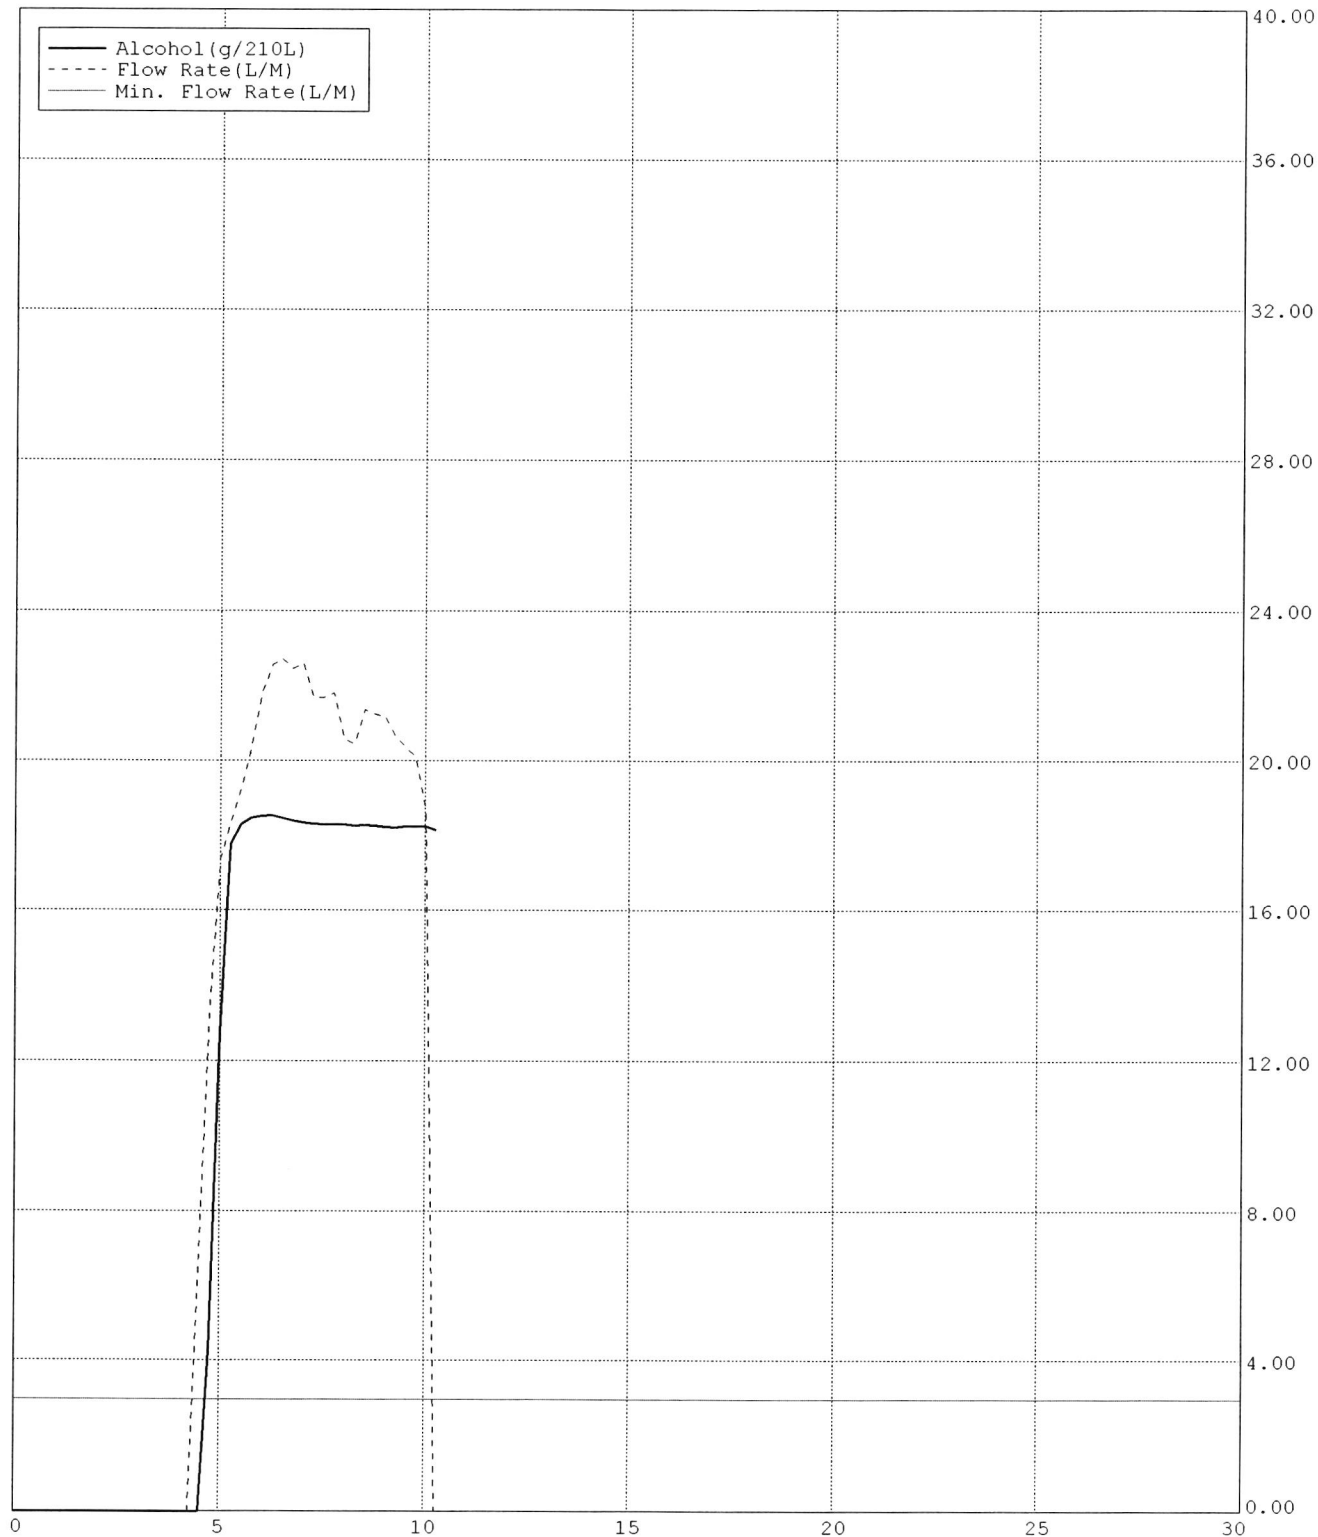

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100683

Date: 04/11/2023
Time: 10:09:37

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.66: 0.079
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:10
BLANK TEST	0.000	10:10
INTERNAL STANDARD	VERIFIED	10:10
EXTERNAL STANDARD	0.077	10:11
BLANK TEST	0.000	10:12
SUBJECT SAMPLE (Vol=1.68L)	0.000	10:12
BLANK TEST	0.000	10:13
EXTERNAL STANDARD	0.078	10:13
BLANK TEST	0.000	10:14

TMM

