

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100364

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 02/05/2021

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.01: 0.080
LOT #: AG923401
EXPIRATION: 08/22/2021
TANK PRESSURE: 920 psi

BLANK TEST	0.000	09:52
INTERNAL STANDARD	VERIFIED	09:52
EXTERNAL STANDARD	0.082	09:53
BLANK TEST	0.000	09:53
EXTERNAL STANDARD	0.082	09:54
BLANK TEST	0.000	09:55
EXTERNAL STANDARD	0.081	09:55
BLANK TEST	0.000	09:56
EXTERNAL STANDARD	0.082	09:56
BLANK TEST	0.000	09:57
EXTERNAL STANDARD	0.081	09:57
BLANK TEST	0.000	09:58

Average = 0.0816
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
Breath Tube = 39.9°C PASSED

PUMP INFO

Flow Rate = 4.576 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED


FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED

I, Brandi M. Barnett, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

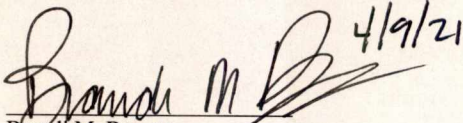 4/9/21



Brandi M. Barnett
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this

9 day of 4, 20 21

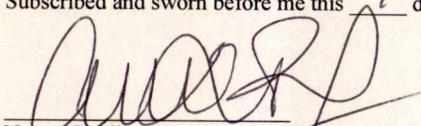
Notary Public

My Commission Expires With Office

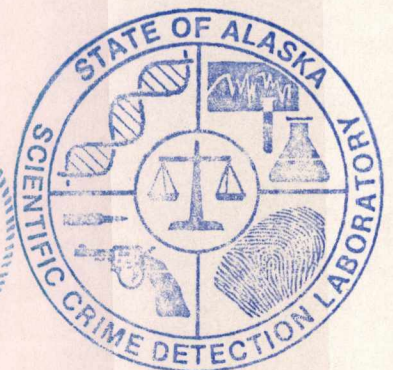

DM 02/05/21