

# Alaska Scientific Crime Detection Laboratory

## DataMaster Certification Form

Issued: 7/10/2015  
Effective: 7/10/2015

Version: DMCEF 2015 R.  
Status: Active

Instrument S/N 100367 Analyst Derech Walton Start Date 03/20/20

1. Diagnostic Test (attached)  Internal Standard value  $\leq 3.00\%$  Yes
1. Voltage Checks
- a. Adjust voltages, if needed 
    - i. Lamp (2.6V Maximum)
    - ii. Bias
    - iii. Cooler (2.0V Maximum)
    - iv. Chopper Frequency
    - v. Detector Voltage (-0.100V to 0.100V)
  - b. Set RFI
  - c. Adjust barometer reading to match NIST traceable barometer
  - d. Adjust volume setting, if needed (1.5L +/- 0.1L)
  - e. Print Technician Screen (attached)
2. Print Calibration Factors (attached)
3. Volume Test - Minimum 1.5 L (1.3L to 1.7L)
4. Linearity Test (attached)

- a. Levels Used
- i. 0.020g/210L Mnf Airgas Lot AG928203 Exp 10/09/21
  - ii. 0.040g/210L Mnf Airgas Lot AG915607 Exp 06/05/21
  - iii. 0.080g/210L Mnf Airgas Lot AG826101 Exp 09/18/20
  - iv. 0.100g/210L Mnf Airgas Lot AG924701 Exp 09/04/21
  - v. 0.200g/210L Mnf Cuth Lot 19200 Exp 08/06/21
    - 1. Simulator S/N DR4176 Date Calibrated 10/07/19
  - vi. 0.300g/210L Mnf Cuth Lot 19330 Exp 11/13/21
    - 1. Simulator S/N DR4178 Date Calibrated 10/04/19

5. Functional Tests (attached)
- a. Incomplete
  - b. Invalid
  - c. Interference  DJW 03/27/2020
  - d. Exceeded attempts

- i. Acetone - Mnf Cuth Lot 19301 Level 0.100 Exp 10/30/21
  - 1. Simulator S/N DR4162 Date Calibrated 10/07/19
- ii. Isopropanol - Mnf Cuth Lot 19301 Level 0.100 Exp 10/30/21
  - 1. Simulator S/N DR4163 Date Calibrated 10/04/19
- iii. Negative Control - Mnf Cuth Lot 19301 Level 0.100 Exp 10/30/21
  - 1. Simulator S/N SD1176 Date Calibrated 10/07/19

e. RFI

- 6. Verify stylus is calibrated
- 7. Reset Options
- 8. Clear Memory
- 9. Verification of Calibration
- 10. Non-Drinking Subject Test (attached)
- 11. Upload  DJW
- 13. Remove tank prior to shut down  03/27/2020

End Date 03/24/20

All printed copies are uncontrolled.

Would not upload initially. Replaced modem. Still did not upload. Replaced modem board and went back to old modem. Now uploads. DJW 03/24/20  
Page 1 of 1  
Approved by Forensic Alcohol Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100367  
-----

Date: 03/20/2020  
Time: 16:49:37

VERSIONS  
DMT: 3.02  
PIC: 3.06  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 44.4°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.59 V PASSED  
(0.92 V - 2.16 V)  
Cooler Voltage = 1.61 V PASSED  
(1.01 V - 2.35 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 527 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 30.3 in

PUMP INFO

Flow Rate = 4.680 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF PASSED  
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD ✓ PASSED  
Xq = 0.082 0.11% (0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100367  
-----

Date: 03/20/2020  
Time: 5:02 PM

Temperatures (°C)  
Sample Cell: 48.9°C  
Breath Tube: 44.7°C

Current Barometer 30.3 in  
Volume (Ltr) 1.54

Settings  
Lamp: 1.59 V  
Bias: 80 V  
Cooler: 1.56 V  
Chopper: 525 Hz

Voltages (V)  
Flow: 1.03 v  
Detector: -0.049 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100367  
-----

Date: 01/24/2020  
Time: 12:27:46

OPERATOR NAME:  
INTOX I METERS  
CERTIFICATE #: 1

Ca = 0.2000  
CAL = 0.990191    0.800 <= CAL < 1.200  
b1 = 0.0000    0.0000 <= b1 < 0.0040  
b2 = 0.0049    0.0010 <= b2 < 0.0100  
b3 = 0.0003    0.0000 <= b3 < 0.0040  
Xq = 0.0816    0.0500 <= Xq < 0.2000  
a21 = 1.171546    1.050 <= a21 < 1.300  
a31 = 0.414106    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 03/20/2020  
Time: 17:13:27

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
MINIMUM VOLUME  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 30.30: 0.081  
LOT #: AG826101  
EXPIRATION: 09/18/2020

DIAGNOSTIC CHECK	PASSED	17:14
BLANK TEST	0.000	17:14
INTERNAL STANDARD	VERIFIED	17:14
EXTERNAL STANDARD	0.081	17:15
BLANK TEST	0.000	17:16
SUBJECT SAMPLE (Vol=1.57L)	0.000	17:16
BLANK TEST	0.000	17:17
EXTERNAL STANDARD	0.082	17:18
BLANK TEST	0.000	17:19

*Handwritten signature*

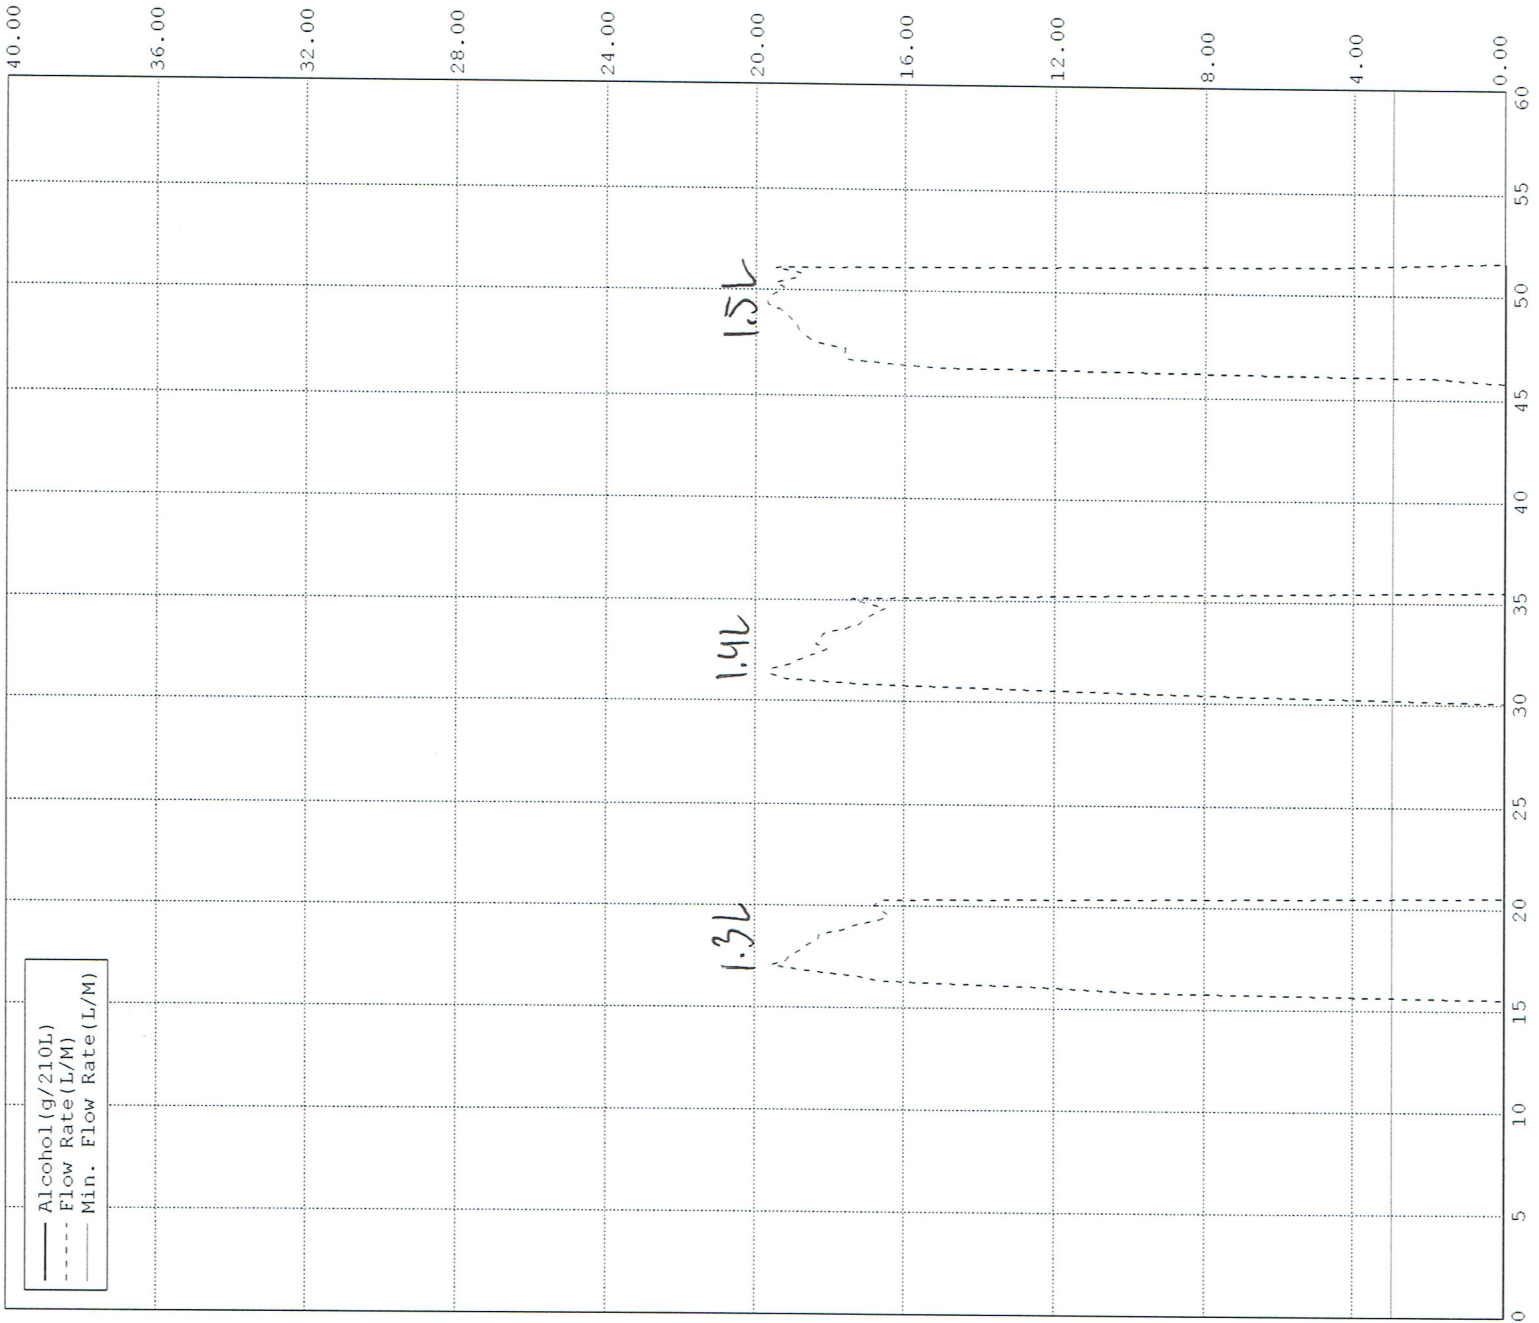

LINEARITY CHECK


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100367  
 -----

Date: 03/20/2020  
 Time: 17:28:05

SUPERVISOR NAME:  
 DEREK WALTON  
 OPERATOR'S #: 9508

TARGET	AVERAGE	STD. DEV.
0.020	0.0210	0.0000
0.040	0.0410	0.0000
0.081	0.0810	0.0000
0.101	0.1024	0.0005
0.200	0.2040	0.0007
0.300	0.3050	0.0000

SLOPE = 1.016981  
 R<sup>2</sup> = 0.999951

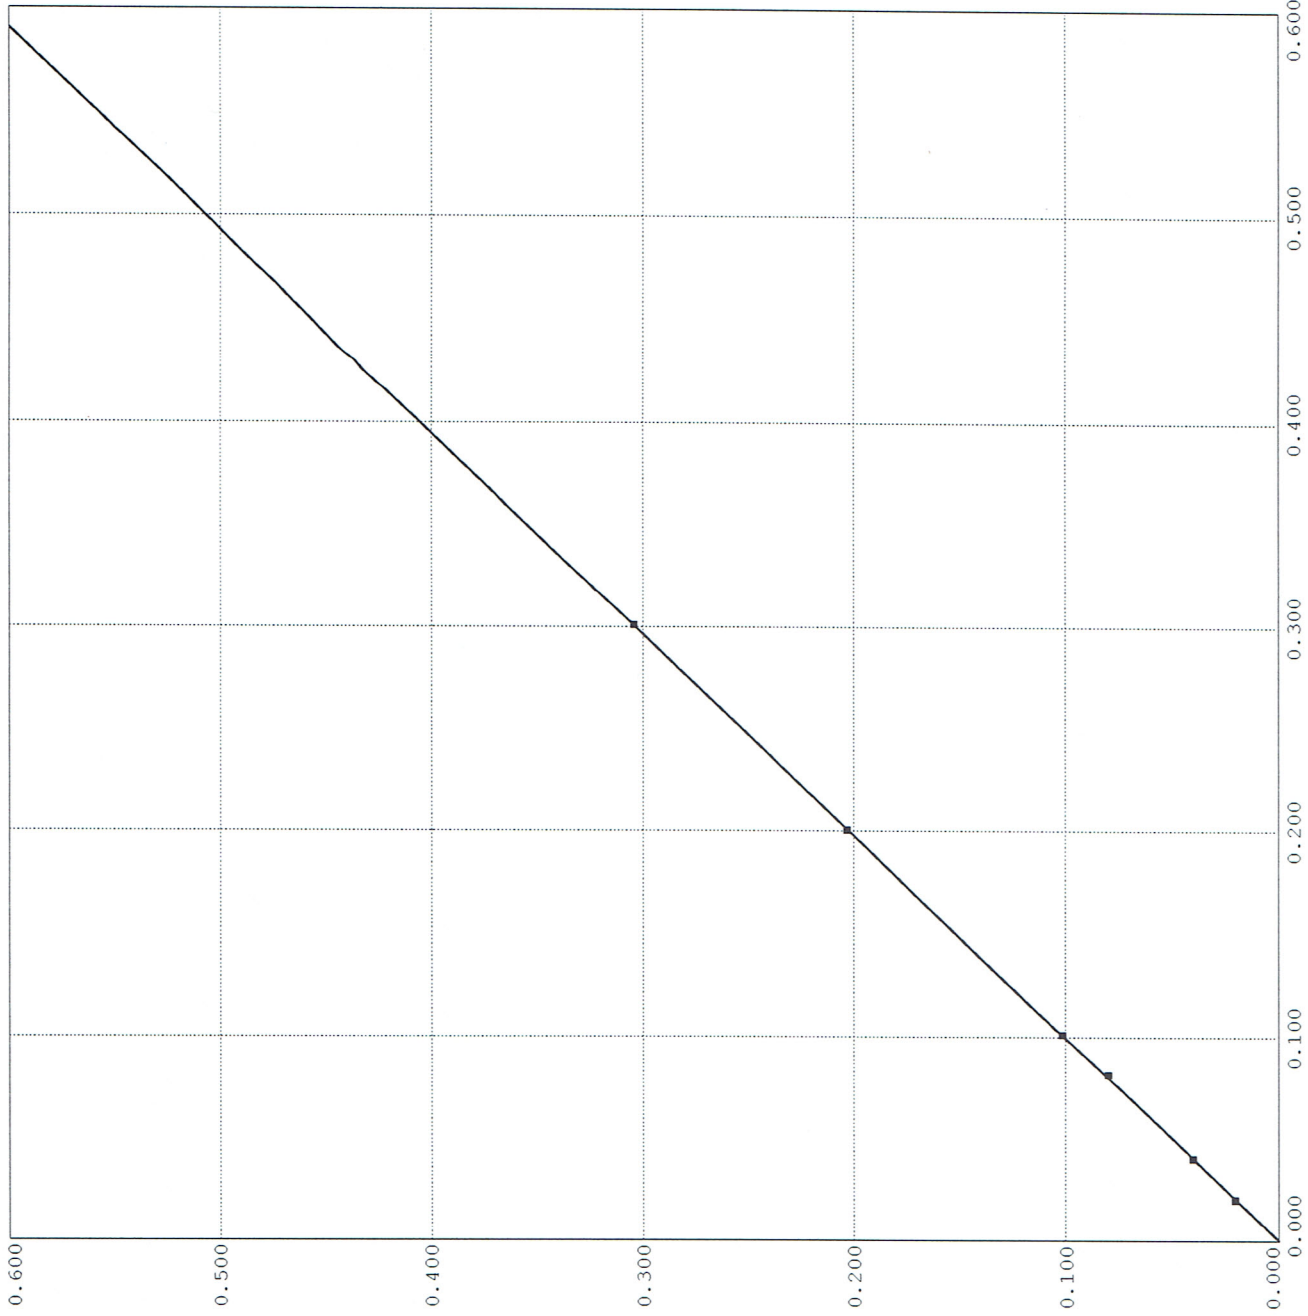

*DM*

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100367






Date: 03/20/2020  
 Time: 17:28:08

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 30.29: 0.020  
 LOT #: AG928203  
 EXPIRATION: 10/09/2021  
 TANK PRESSURE: 1118 psi

BLANK TEST	0.000	17:29
INTERNAL STANDARD	VERIFIED	17:29
EXTERNAL STANDARD	0.021	17:29
BLANK TEST	0.000	17:30
EXTERNAL STANDARD	0.021	17:30
BLANK TEST	0.000	17:31
EXTERNAL STANDARD	0.021	17:31
BLANK TEST	0.000	17:32
EXTERNAL STANDARD	0.021	17:33
BLANK TEST	0.000	17:33
EXTERNAL STANDARD	0.021	17:34
BLANK TEST	0.000	17:35

Average = 0.0210  
 Std Dev = 0.0000

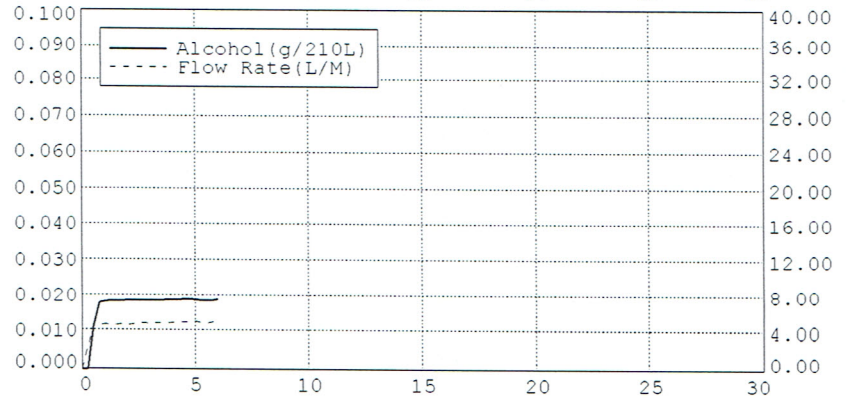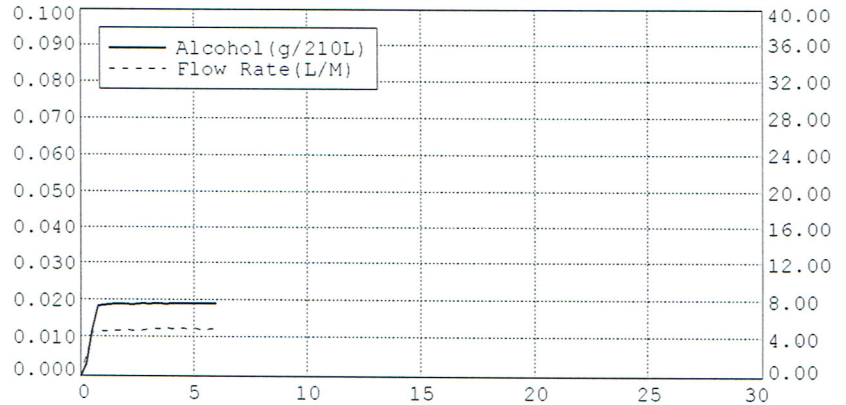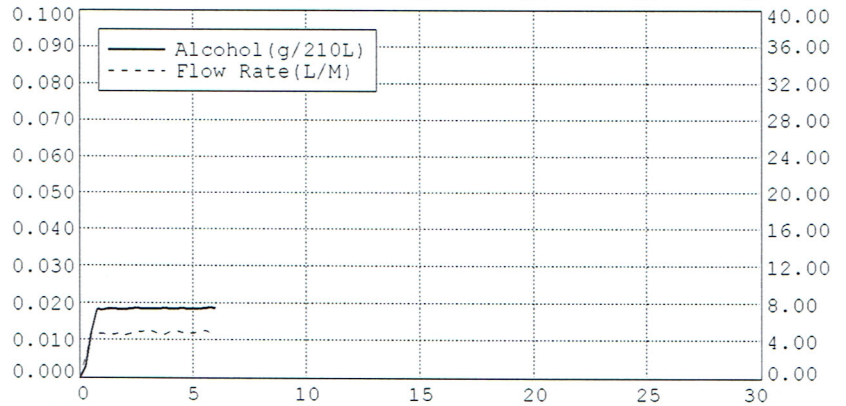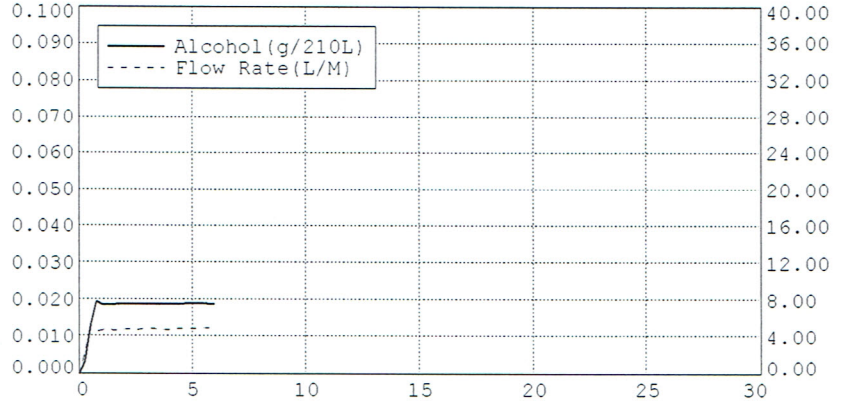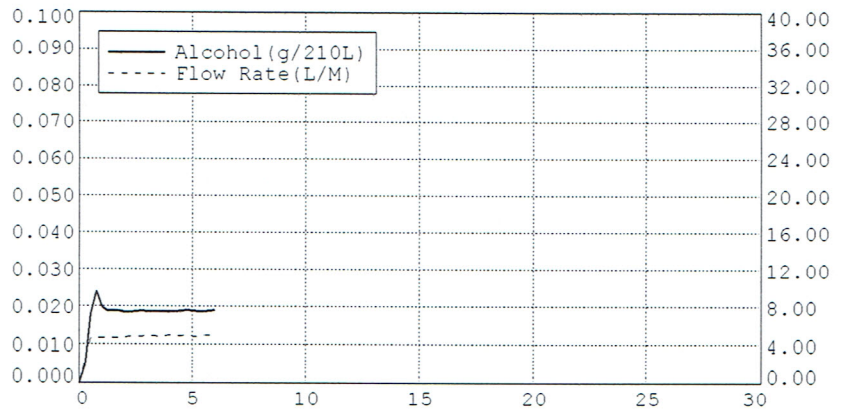

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100367






Date: 03/20/2020  
 Time: 17:37:26

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 30.29: 0.040  
 LOT #: AG915607  
 EXPIRATION: 06/05/2021  
 TANK PRESSURE: 940 psi

BLANK TEST	0.000	17:38
INTERNAL STANDARD	VERIFIED	17:38
EXTERNAL STANDARD	0.041	17:38
BLANK TEST	0.000	17:39
EXTERNAL STANDARD	0.041	17:40
BLANK TEST	0.000	17:41
EXTERNAL STANDARD	0.041	17:41
BLANK TEST	0.000	17:42
EXTERNAL STANDARD	0.041	17:42
BLANK TEST	0.000	17:43
EXTERNAL STANDARD	0.041	17:43
BLANK TEST	0.000	17:44

Average = 0.0410  
 Std Dev = 0.0000

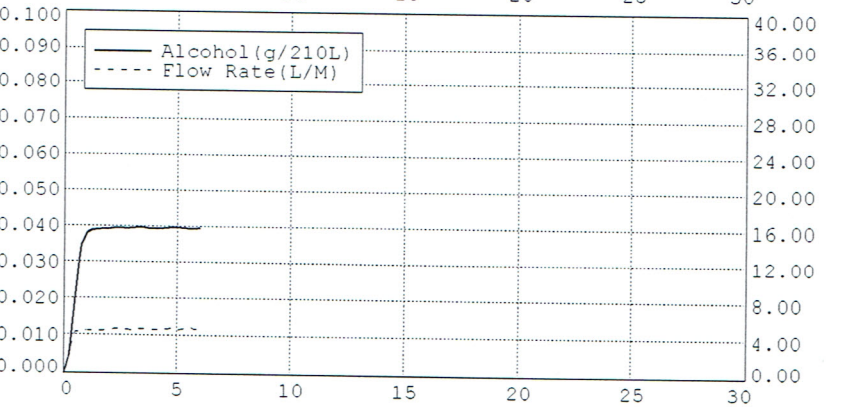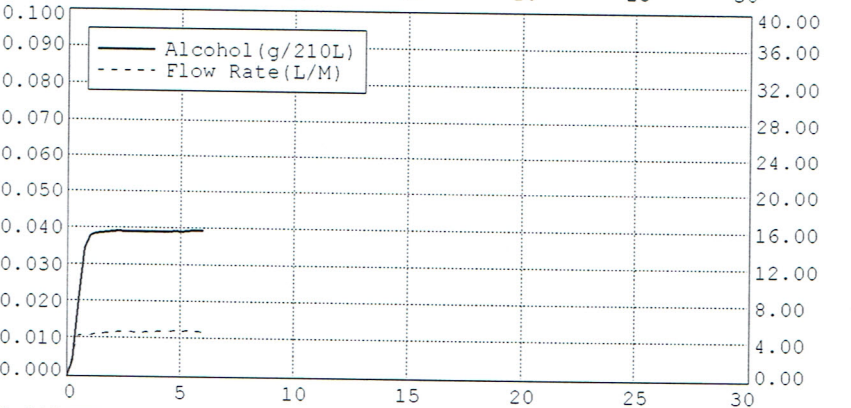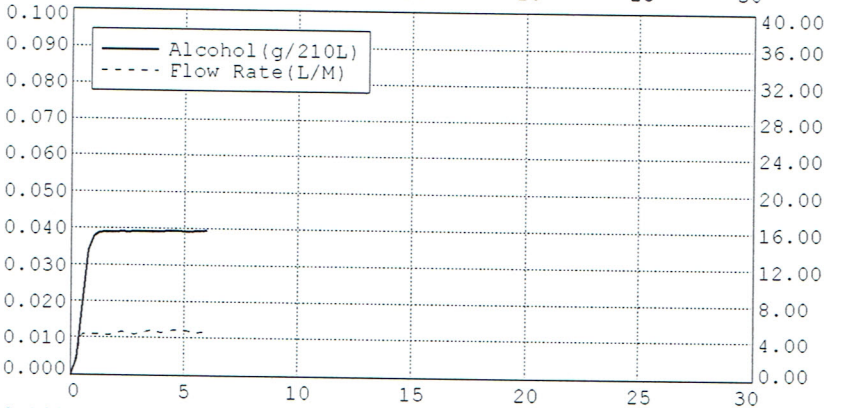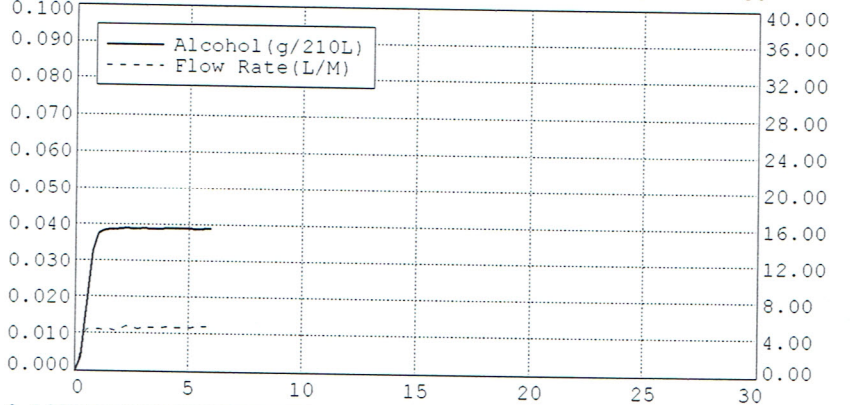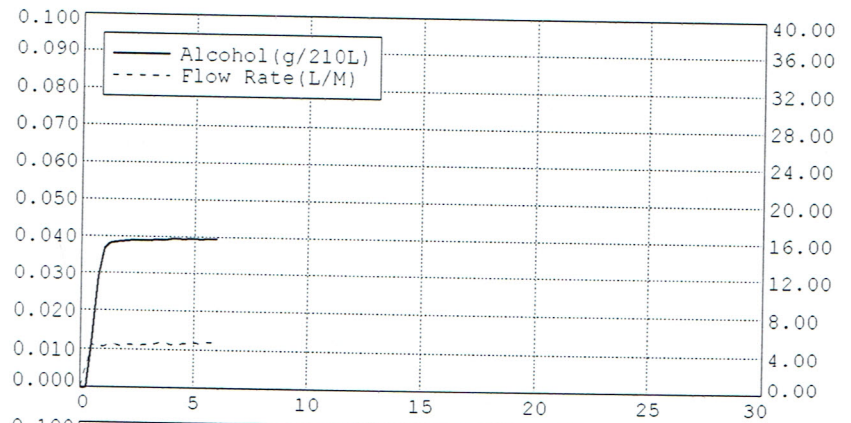



LINEARITY CHECK: Control Test 3

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100367  
 -----






Date: 03/20/2020  
 Time: 17:50:13

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 30.30: 0.081  
 LOT #: AG826101  
 EXPIRATION: 09/18/2020  
 TANK PRESSURE: 878 psi

BLANK TEST	0.000	17:51
INTERNAL STANDARD	VERIFIED	17:51
EXTERNAL STANDARD	0.081	17:51
BLANK TEST	0.000	17:52
EXTERNAL STANDARD	0.081	17:52
BLANK TEST	0.000	17:53
EXTERNAL STANDARD	0.081	17:53
BLANK TEST	0.000	17:54
EXTERNAL STANDARD	0.081	17:55
BLANK TEST	0.000	17:55
EXTERNAL STANDARD	0.081	17:56
BLANK TEST	0.000	17:57

Average = 0.0810  
 Std Dev = 0.0000

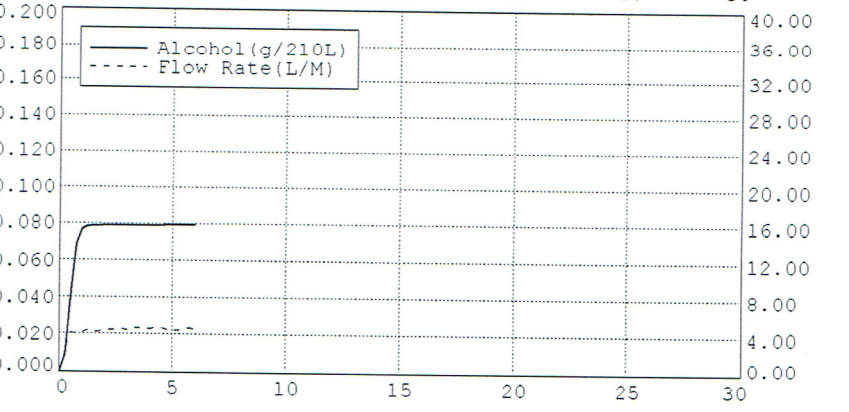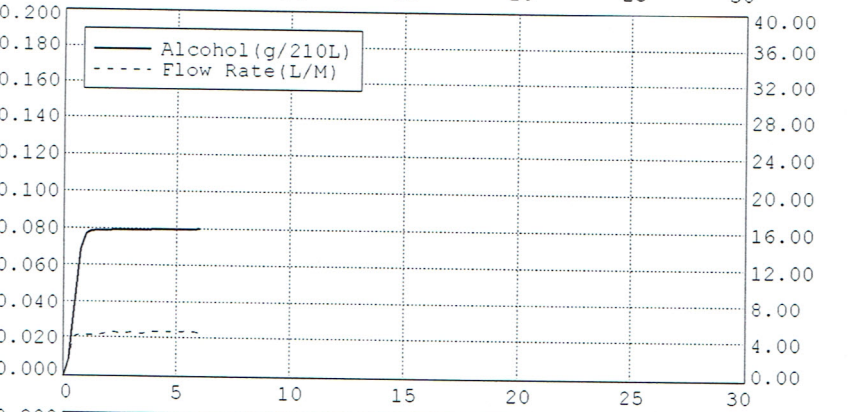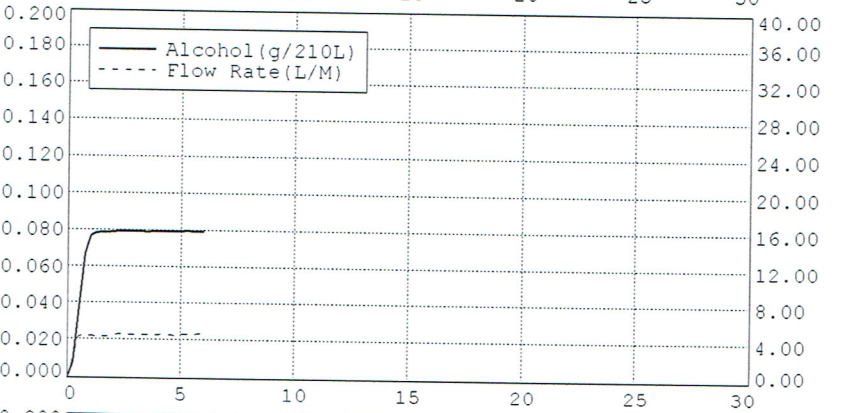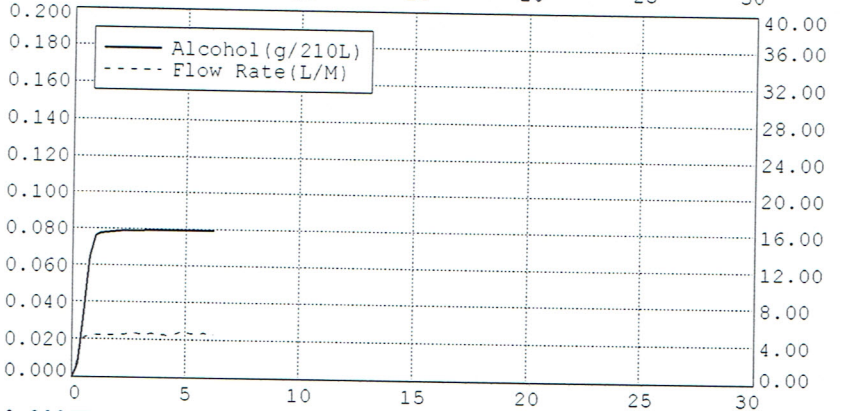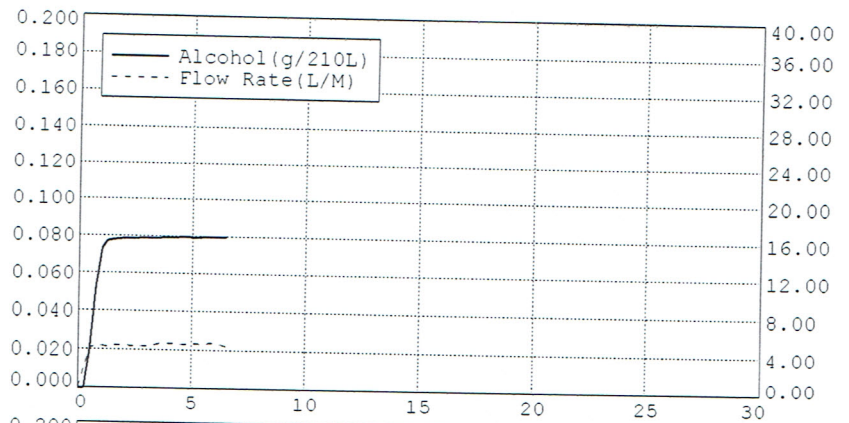

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100367






Date: 03/20/2020  
 Time: 17:57:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 30.31: 0.101  
 LOT #: AG924701  
 EXPIRATION: 09/04/2021  
 TANK PRESSURE: 723 psi

BLANK TEST	0.000	17:59
INTERNAL STANDARD	VERIFIED	17:59
EXTERNAL STANDARD	0.103	17:59
BLANK TEST	0.000	18:00
EXTERNAL STANDARD	0.102	18:00
BLANK TEST	0.000	18:01
EXTERNAL STANDARD	0.103	18:01
BLANK TEST	0.000	18:02
EXTERNAL STANDARD	0.102	18:02
BLANK TEST	0.000	18:03
EXTERNAL STANDARD	0.102	18:03
BLANK TEST	0.000	18:04

Average = 0.1024  
 Std Dev = 0.0005

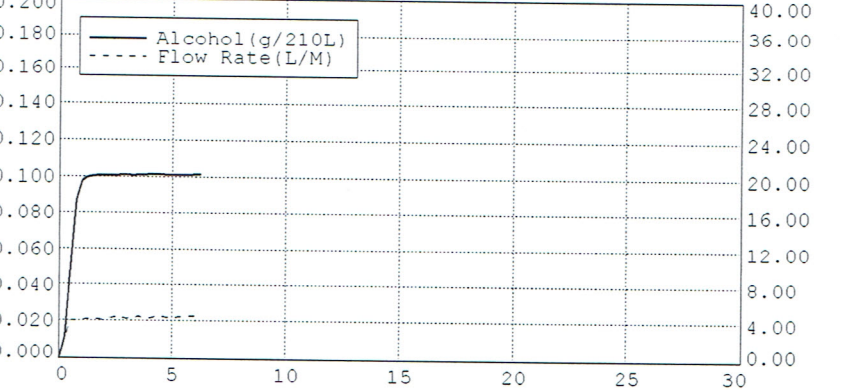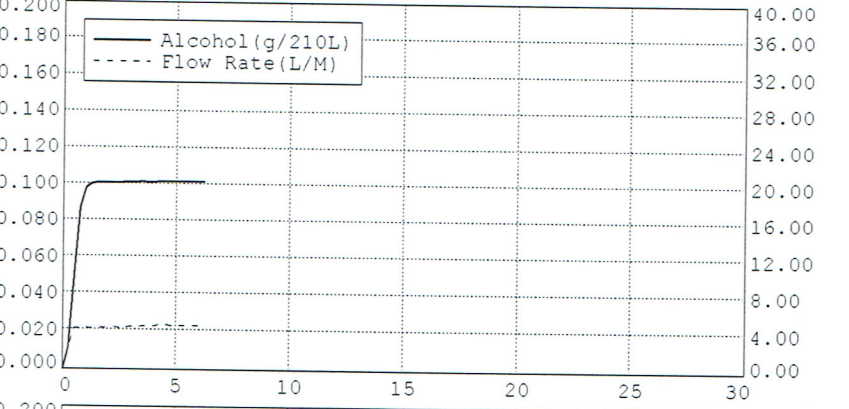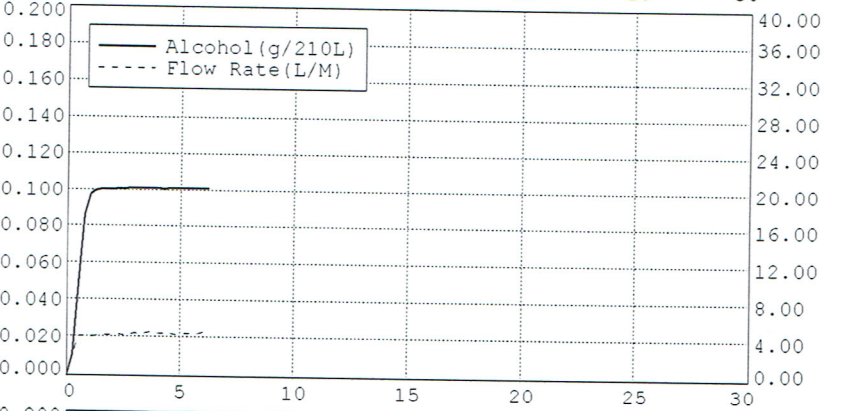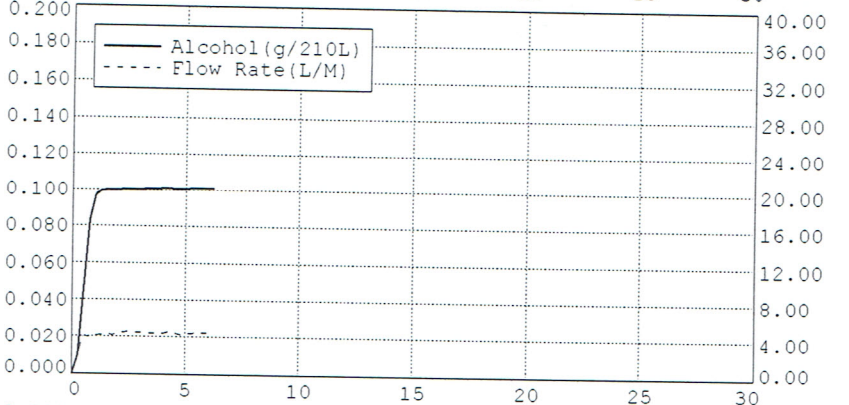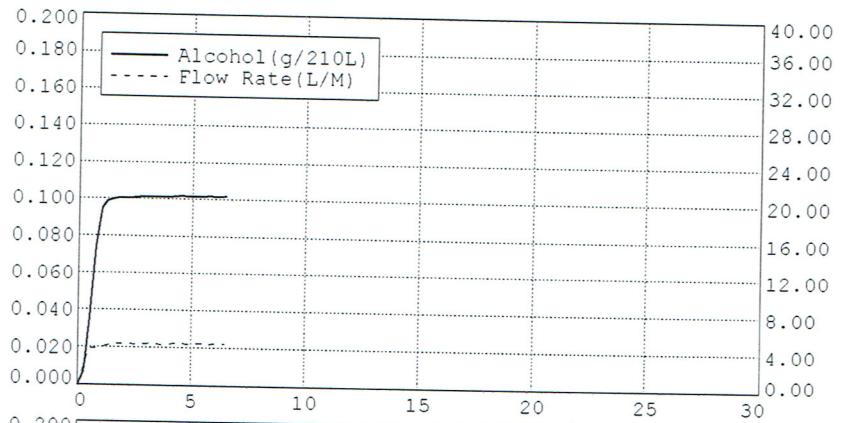

LINEARITY CHECK: Control Test 5






Alaska Department of Public Safety  
 DATAMASTER dmt: 100367

Date: 03/20/2020  
 Time: 18:11:01

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.200  
 LOT #: 19200  
 EXPIRATION: 08/06/2021

BLANK TEST	0.000	18:12
INTERNAL STANDARD	VERIFIED	18:12
EXTERNAL STANDARD	0.203	18:12
BLANK TEST	0.000	18:13
EXTERNAL STANDARD	0.204	18:13
BLANK TEST	0.000	18:14
EXTERNAL STANDARD	0.205	18:15
BLANK TEST	0.000	18:16
EXTERNAL STANDARD	0.204	18:16
BLANK TEST	0.000	18:17
EXTERNAL STANDARD	0.204	18:17
BLANK TEST	0.000	18:18

Average = 0.2040  
 Std Dev = 0.0007

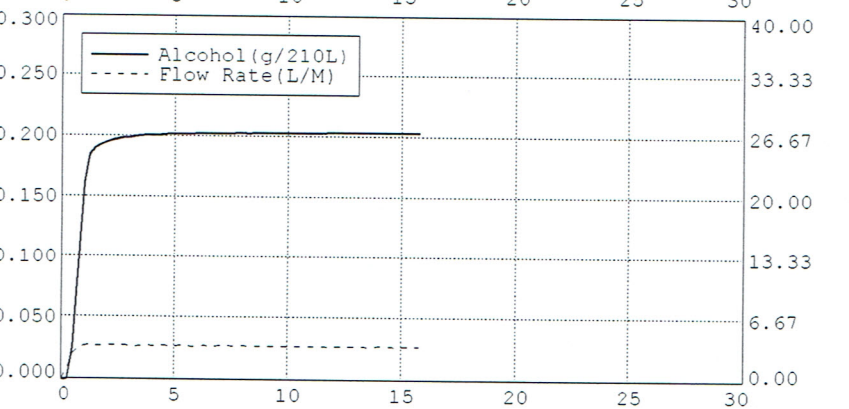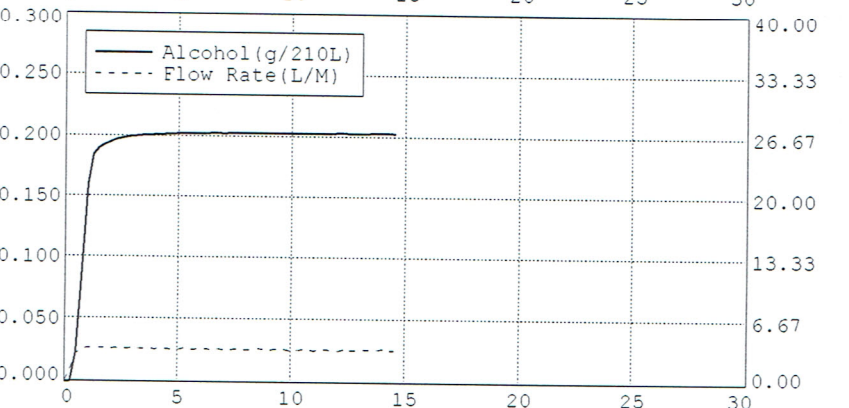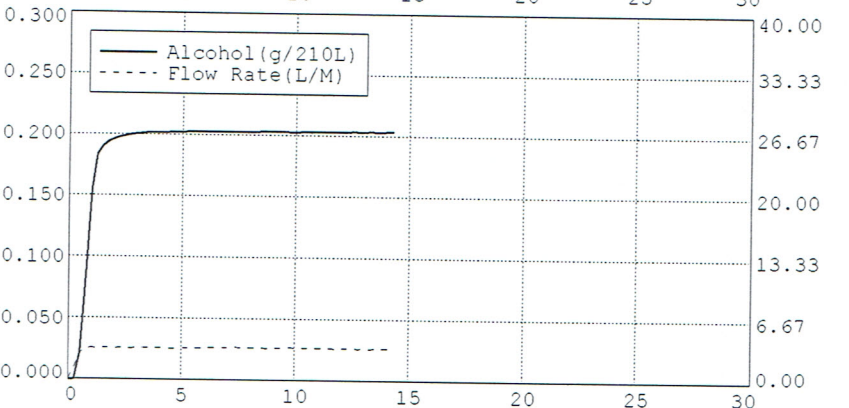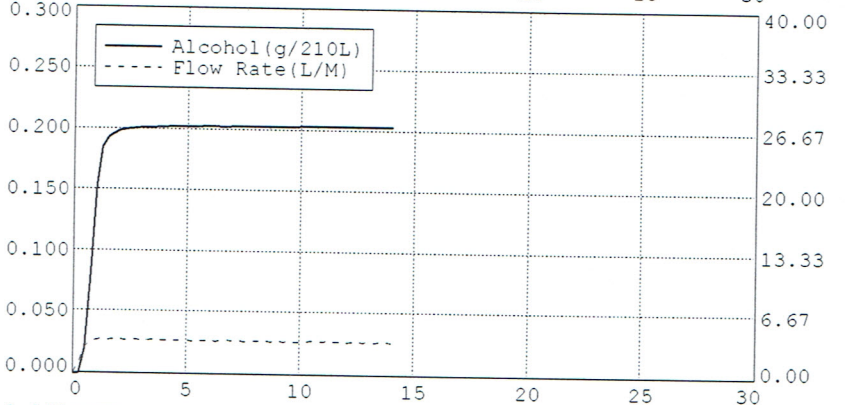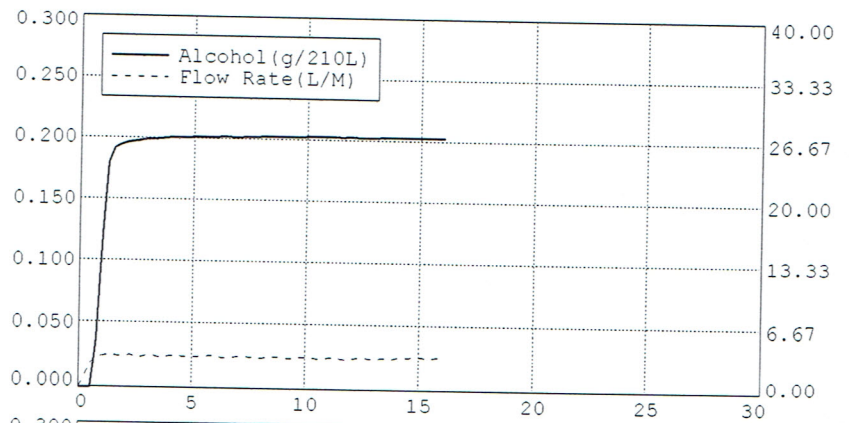

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100367






Date: 03/20/2020  
 Time: 18:21:20

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 LOT #: 19330  
 EXPIRATION: 11/13/2021

BLANK TEST	0.000	18:22
INTERNAL STANDARD	VERIFIED	18:22
EXTERNAL STANDARD	0.305	18:23
BLANK TEST	0.000	18:24
EXTERNAL STANDARD	0.305	18:24
BLANK TEST	0.000	18:25
EXTERNAL STANDARD	0.305	18:26
BLANK TEST	0.000	18:26
EXTERNAL STANDARD	0.305	18:27
BLANK TEST	0.000	18:28
EXTERNAL STANDARD	0.305	18:28
BLANK TEST	0.000	18:29

Average = 0.3050  
 Std Dev = 0.0000

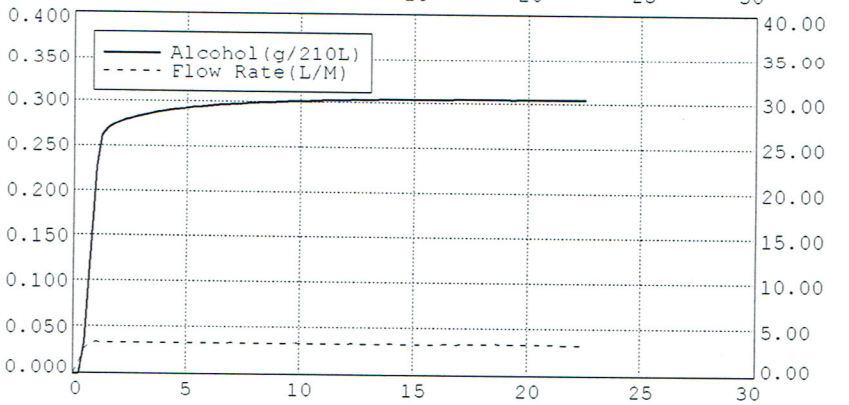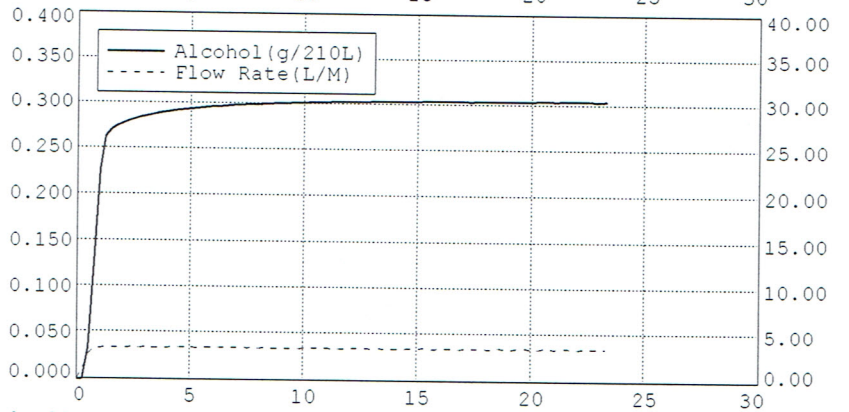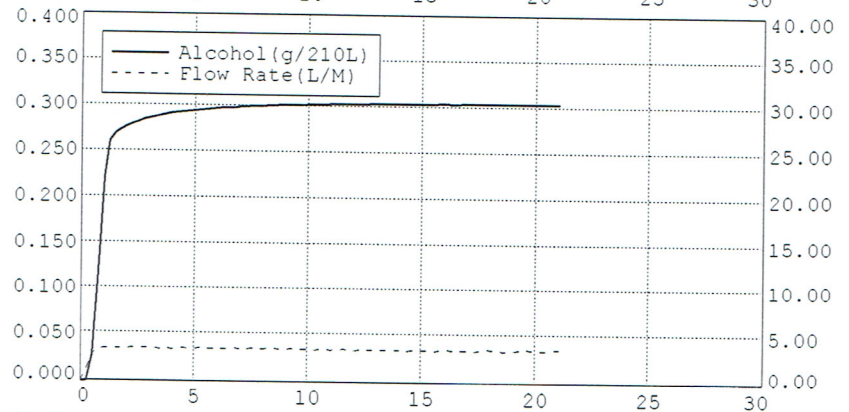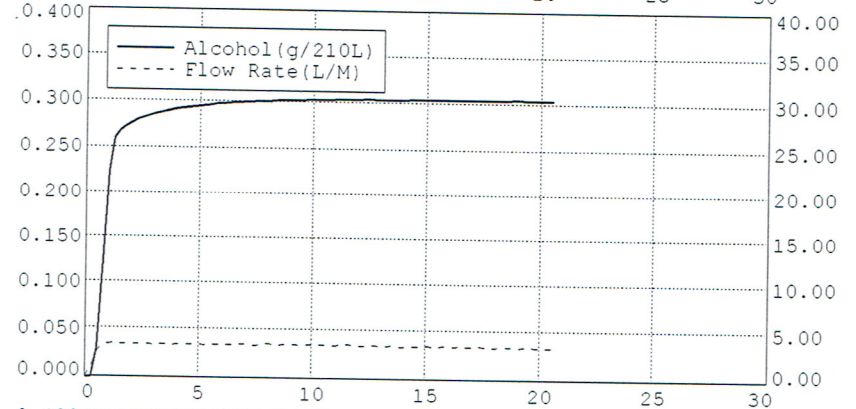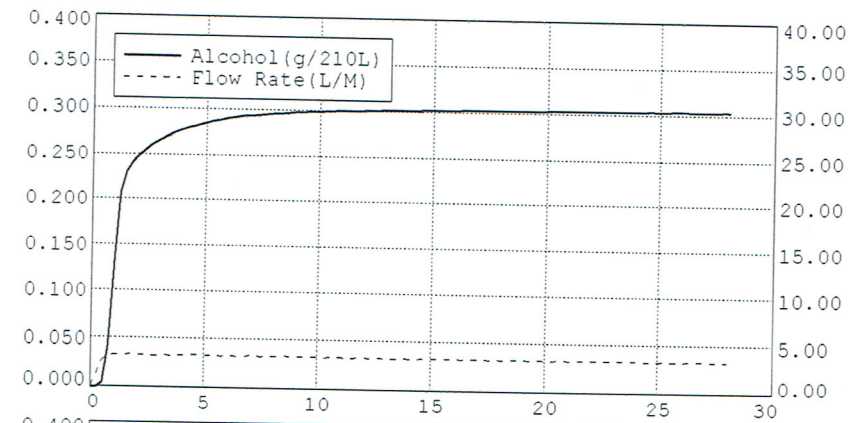

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100367  
-----

Date: 03/20/2020  
Time: 18:36:49


SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 30.30: 0.081  
LOT #: AG826101  
EXPIRATION: 09/18/2020

DIAGNOSTIC CHECK PASSED 18:39  
BLANK TEST 0.000 18:39  
INTERNAL STANDARD VERIFIED 18:39  
EXTERNAL STANDARD 0.081 18:40  
BLANK TEST 0.000 18:41  
SUBJECT SAMPLE INCOMPLETE 18:43

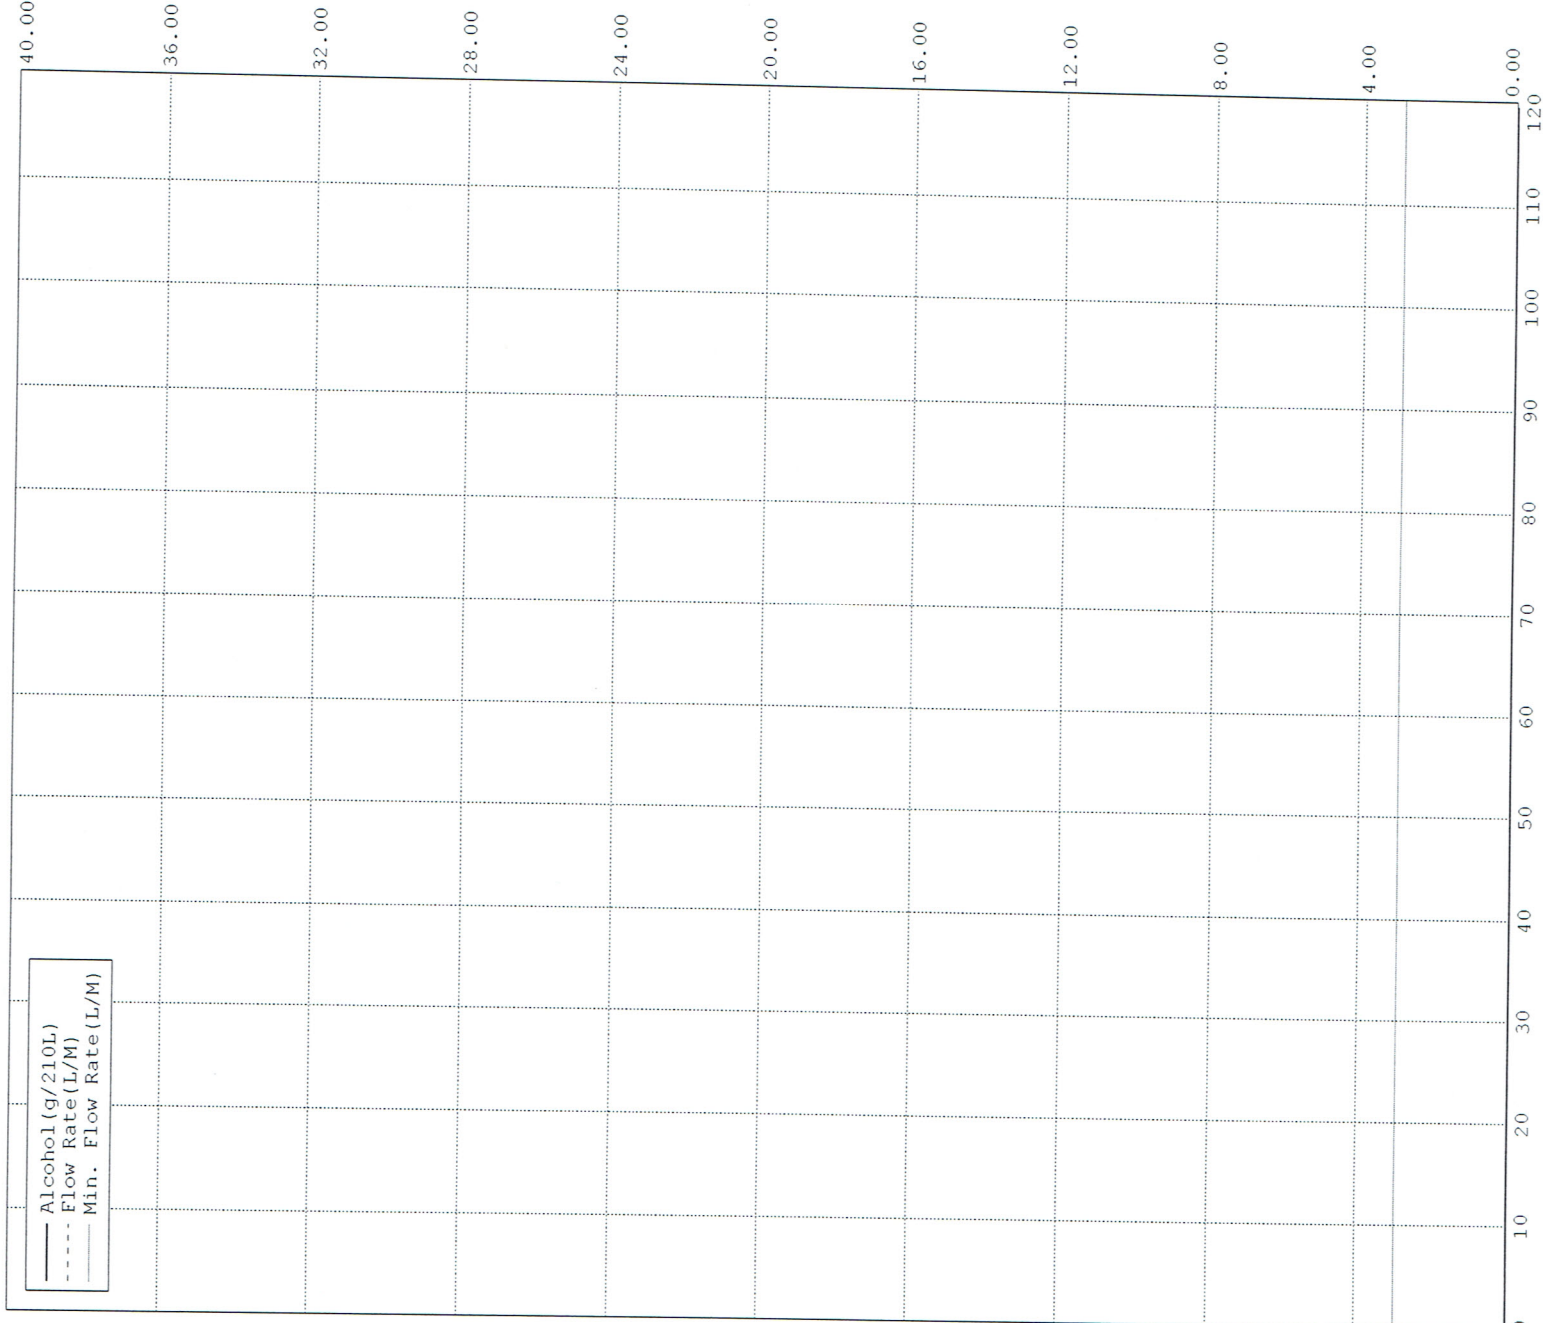

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 03/20/2020  
Time: 18:45:23

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
MAXIMUM ATTEMPTS  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 30.31: 0.081  
LOT #: AG826101  
EXPIRATION: 09/18/2020

DIAGNOSTIC CHECK PASSED 18:47  
BLANK TEST 0.000 18:47  
INTERNAL STANDARD VERIFIED 18:47  
EXTERNAL STANDARD 0.082 18:47  
BLANK TEST 0.000 18:48  
SUBJECT SAMPLE XXX 18:49

Maximum Attempts Exceeded

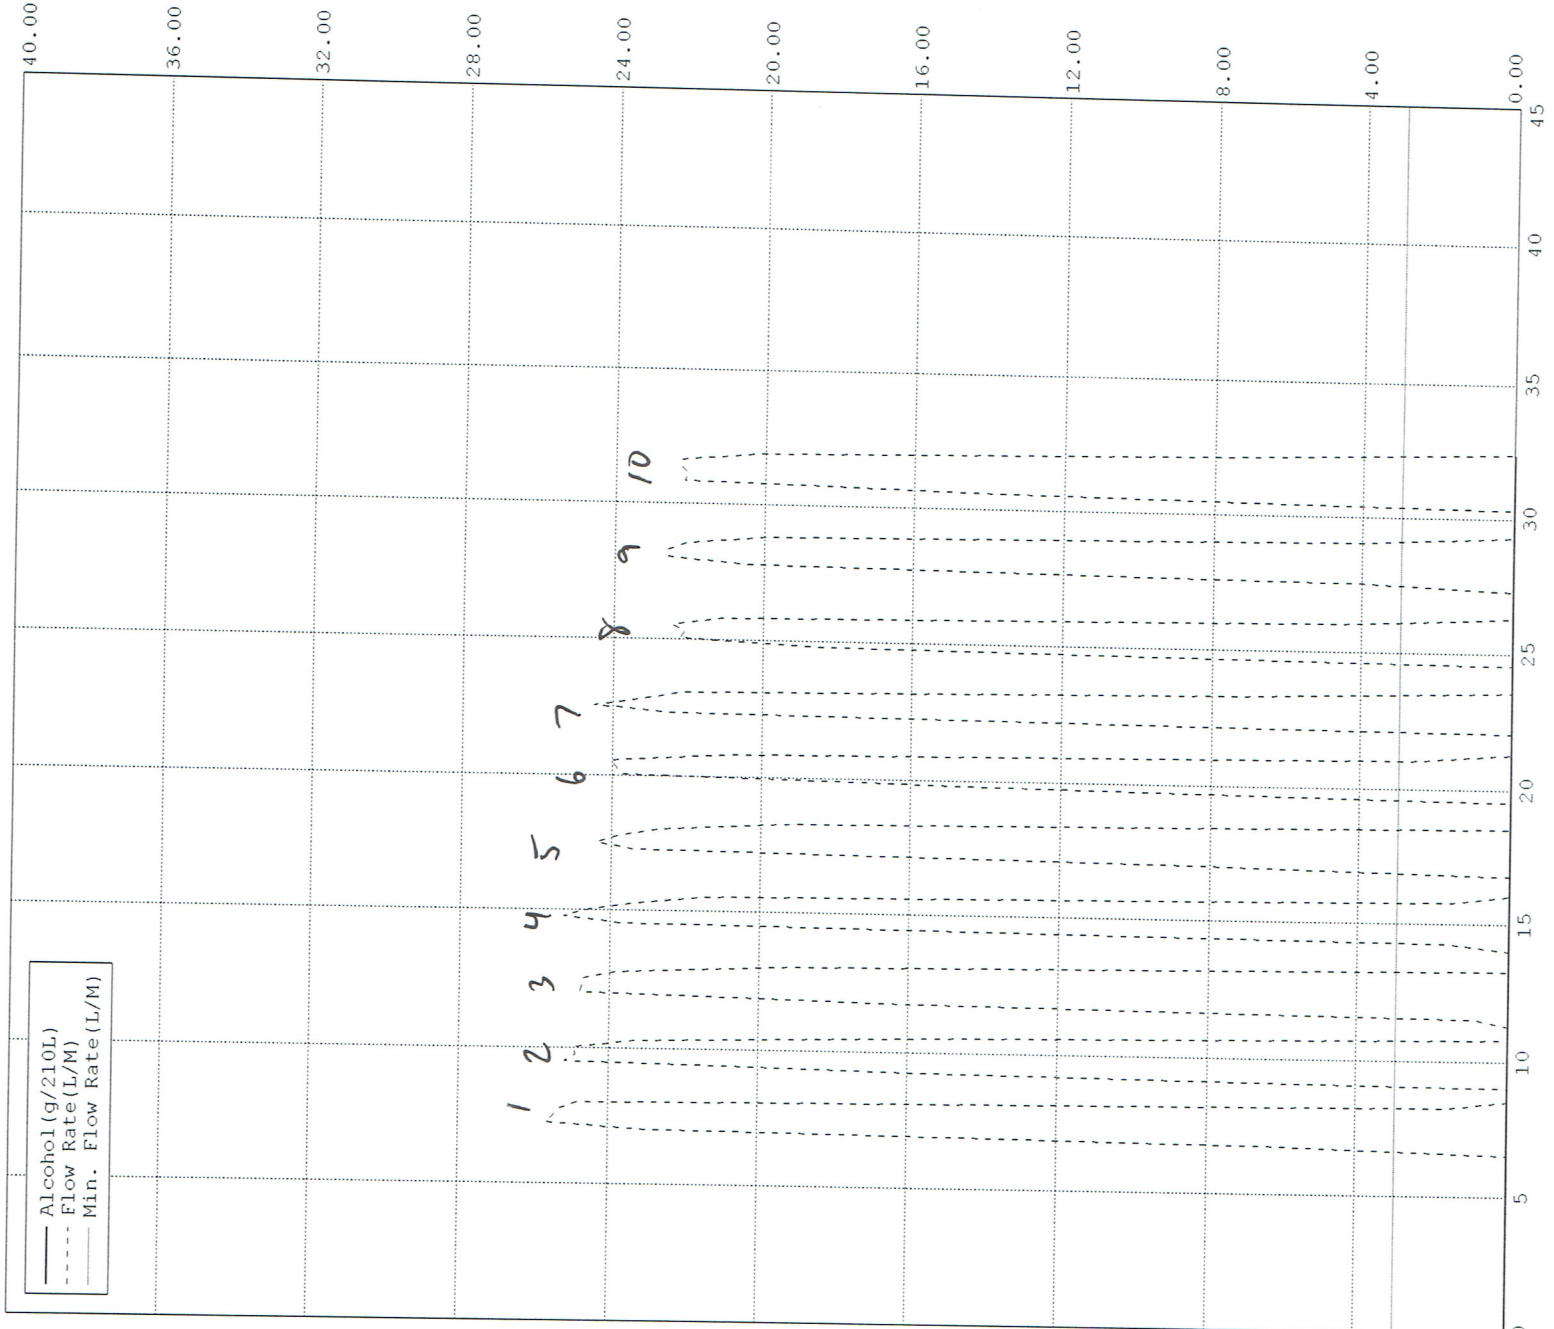

SUBJECT TEST

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100367  
 -----

Date: 03/20/2020  
 Time: 20:13:12  
 -----

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX


OPERATOR NAME:  
 DEREK WALTON  
 OPERATOR'S #: 9508

DEPT/AGENCY:  
 RADIO FREQUENCY  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 30.27: 0.081  
 LOT #: AG826101  
 EXPIRATION: 09/18/2020

DIAGNOSTIC CHECK PASSED 20:19  
 BLANK TEST 0.000 20:19  
 INTERNAL STANDARD VERIFIED 20:19  
 EXTERNAL STANDARD 0.082 20:19  
 BLANK TEST 0.000 20:20

RFI DETECTED

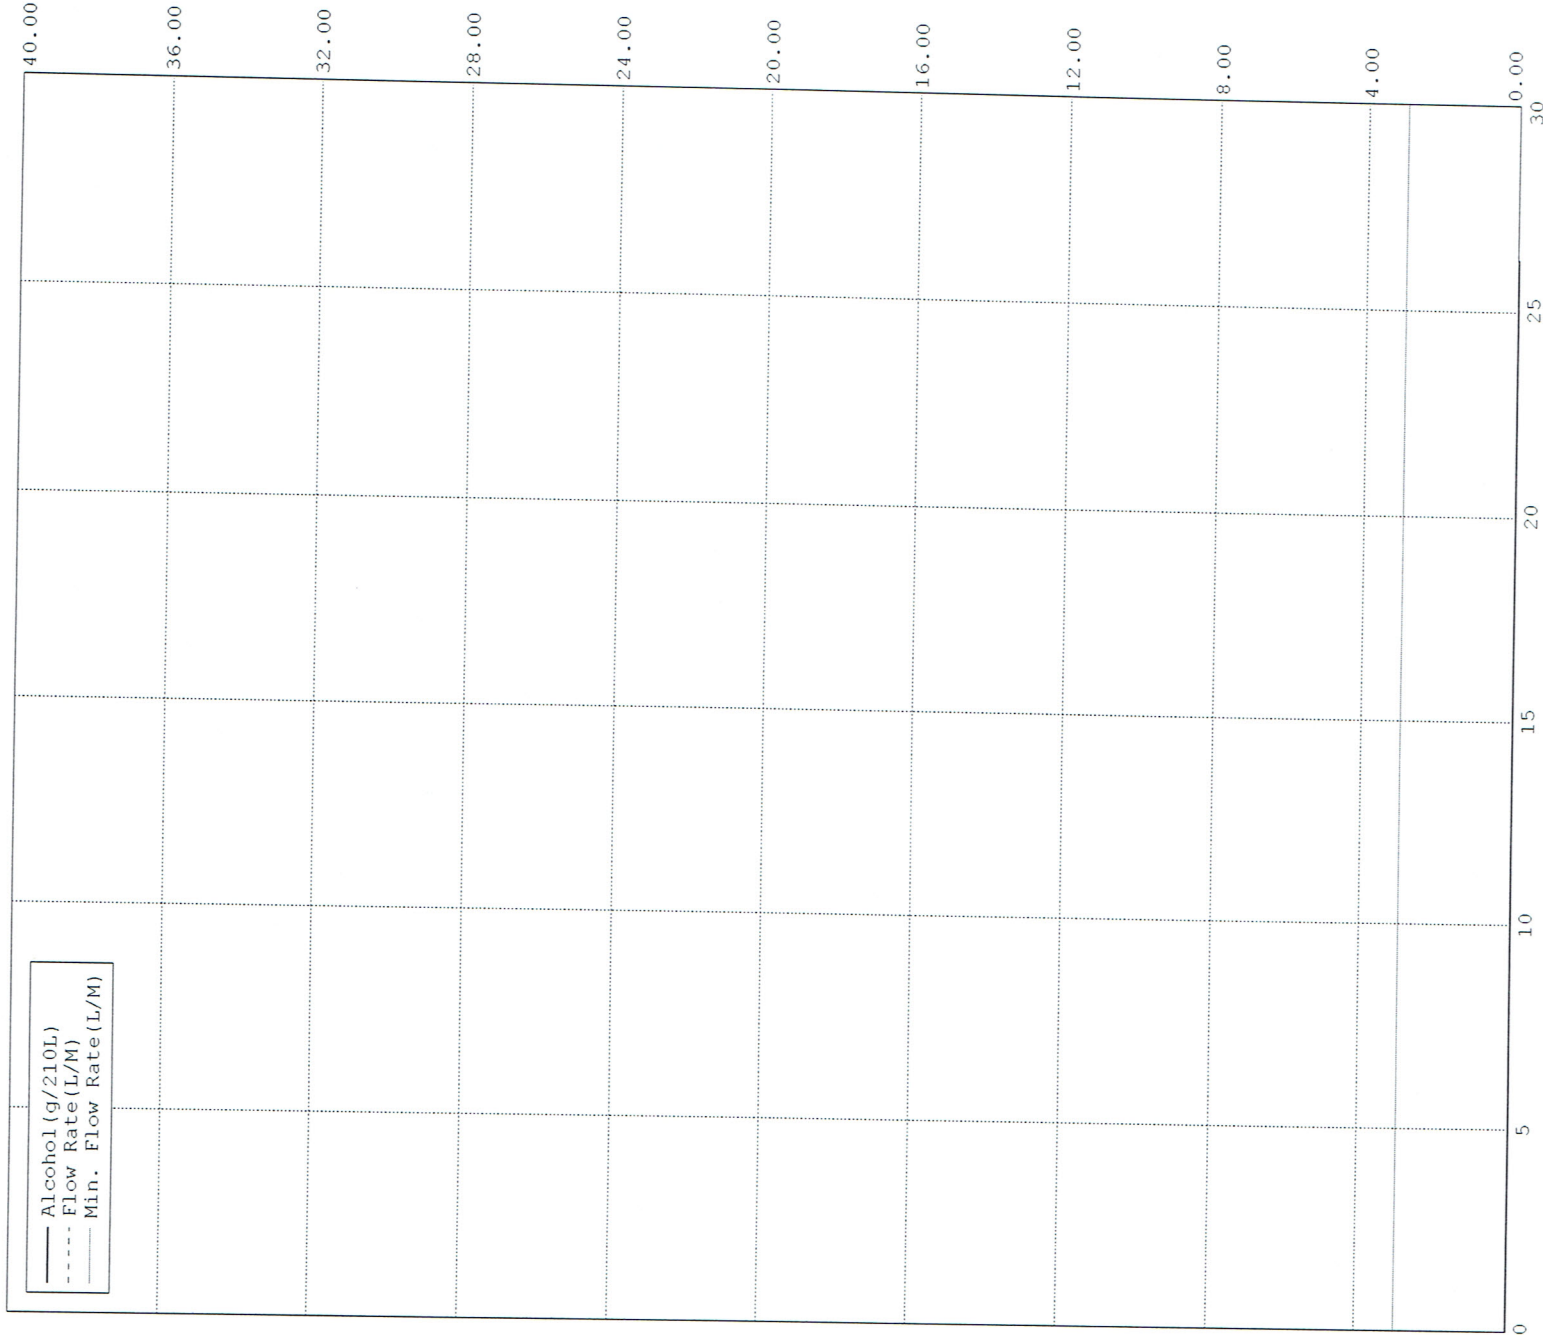

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 03/20/2020  
Time: 20:26:05

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
INVALID  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 30.27: 0.081  
LOT #: AG826101  
EXPIRATION: 09/18/2020

DIAGNOSTIC CHECK PASSED 20:27  
BLANK TEST 0.000 20:27  
INTERNAL STANDARD VERIFIED 20:28  
EXTERNAL STANDARD 0.081 20:28  
BLANK TEST 0.000 20:29  
SUBJECT SAMPLE INVALID 20:29

*DM*

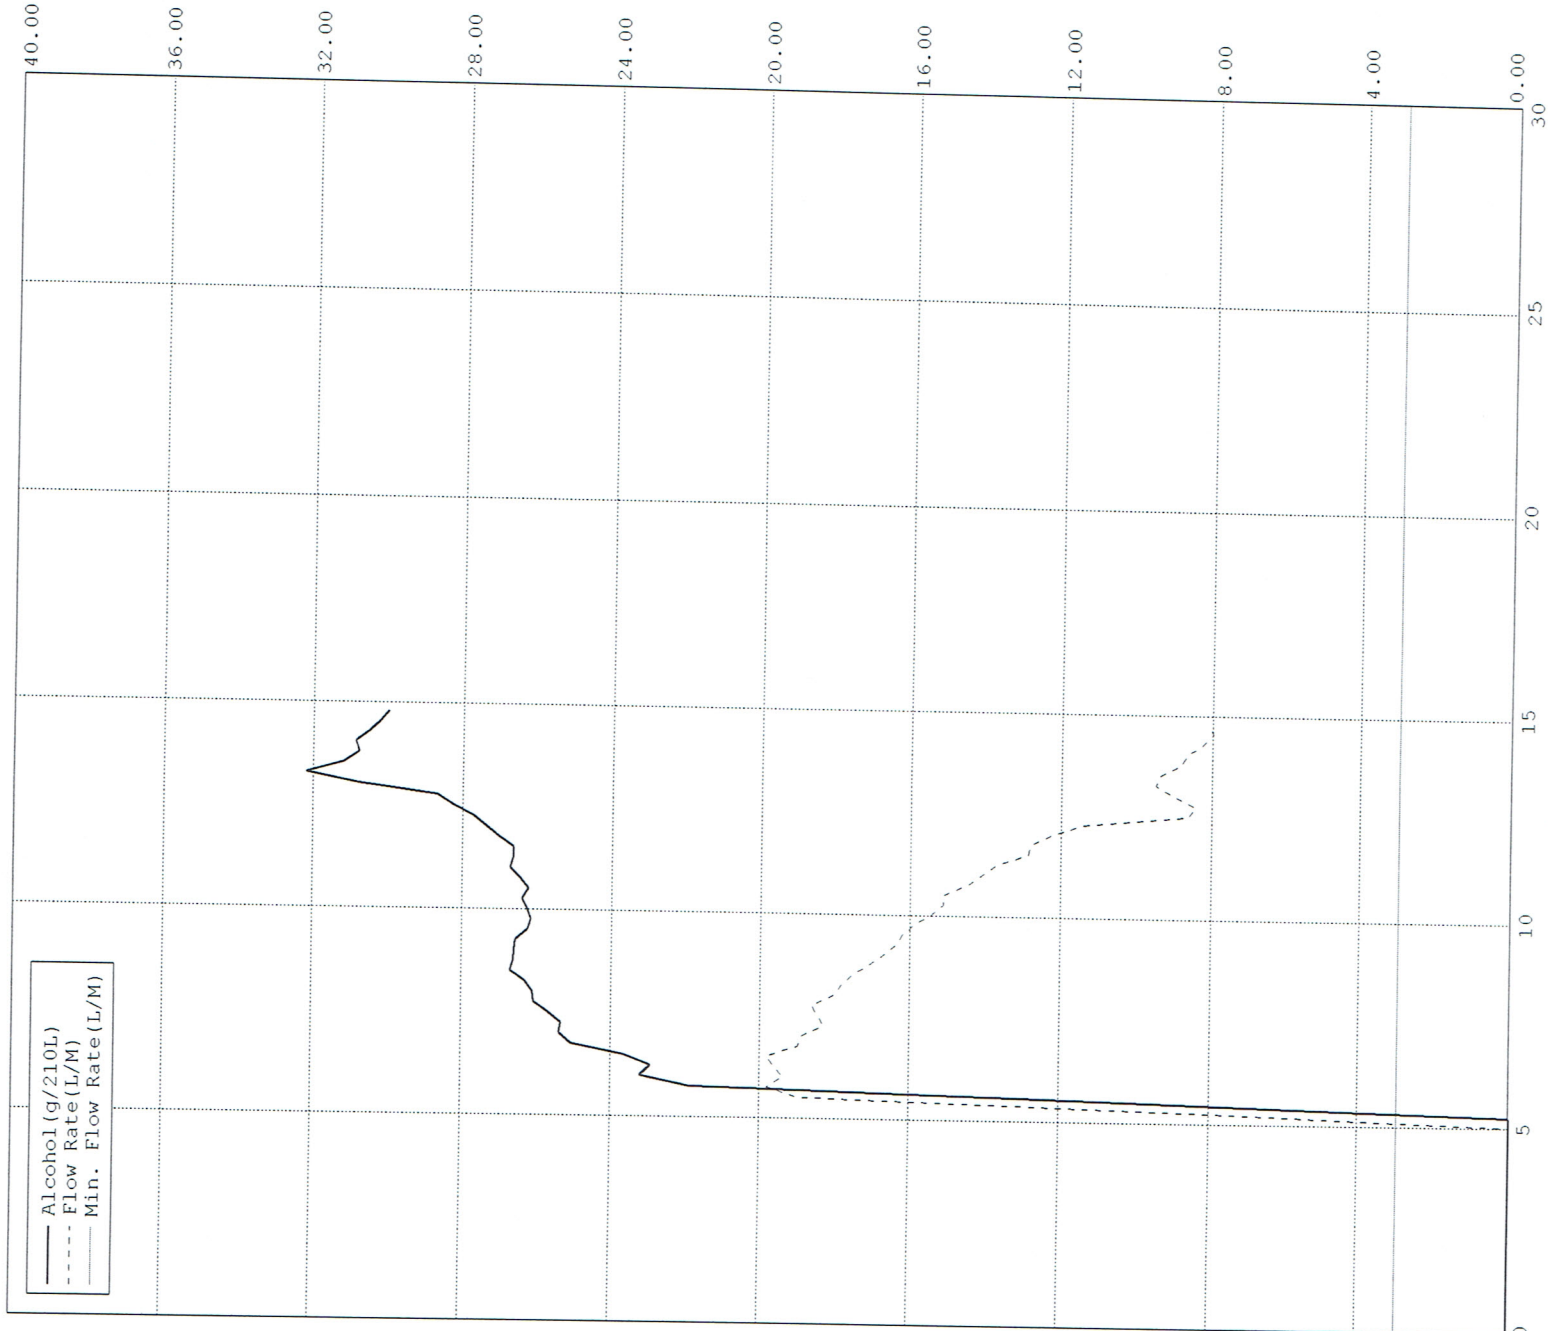



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 03/23/2020  
Time: 16:37:13

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508



DEPT/AGENCY:  
INTERFERENCE ACETONE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 30.25: 0.081  
LOT #: AG826101  
EXPIRATION: 09/18/2020

DIAGNOSTIC CHECK PASSED 16:42  
BLANK TEST 0.000 16:42  
INTERNAL STANDARD VERIFIED 16:42  
 $X_q = 0.083 (1.07\%)$   
EXTERNAL STANDARD 0.081 16:42  
 $X[1] = 0.0814 (-0.0016) (0.0007)$   
BLANK TEST 0.000 16:43  
SUBJECT SAMPLE XXX 16:44  
 $X[1] = 0.1130 (-0.0212) (-0.0006)$

Interference Detected

Filter 2 Average: -0.0017  
Filter 3 Average: 0.0004  
DJW 03/27/2020

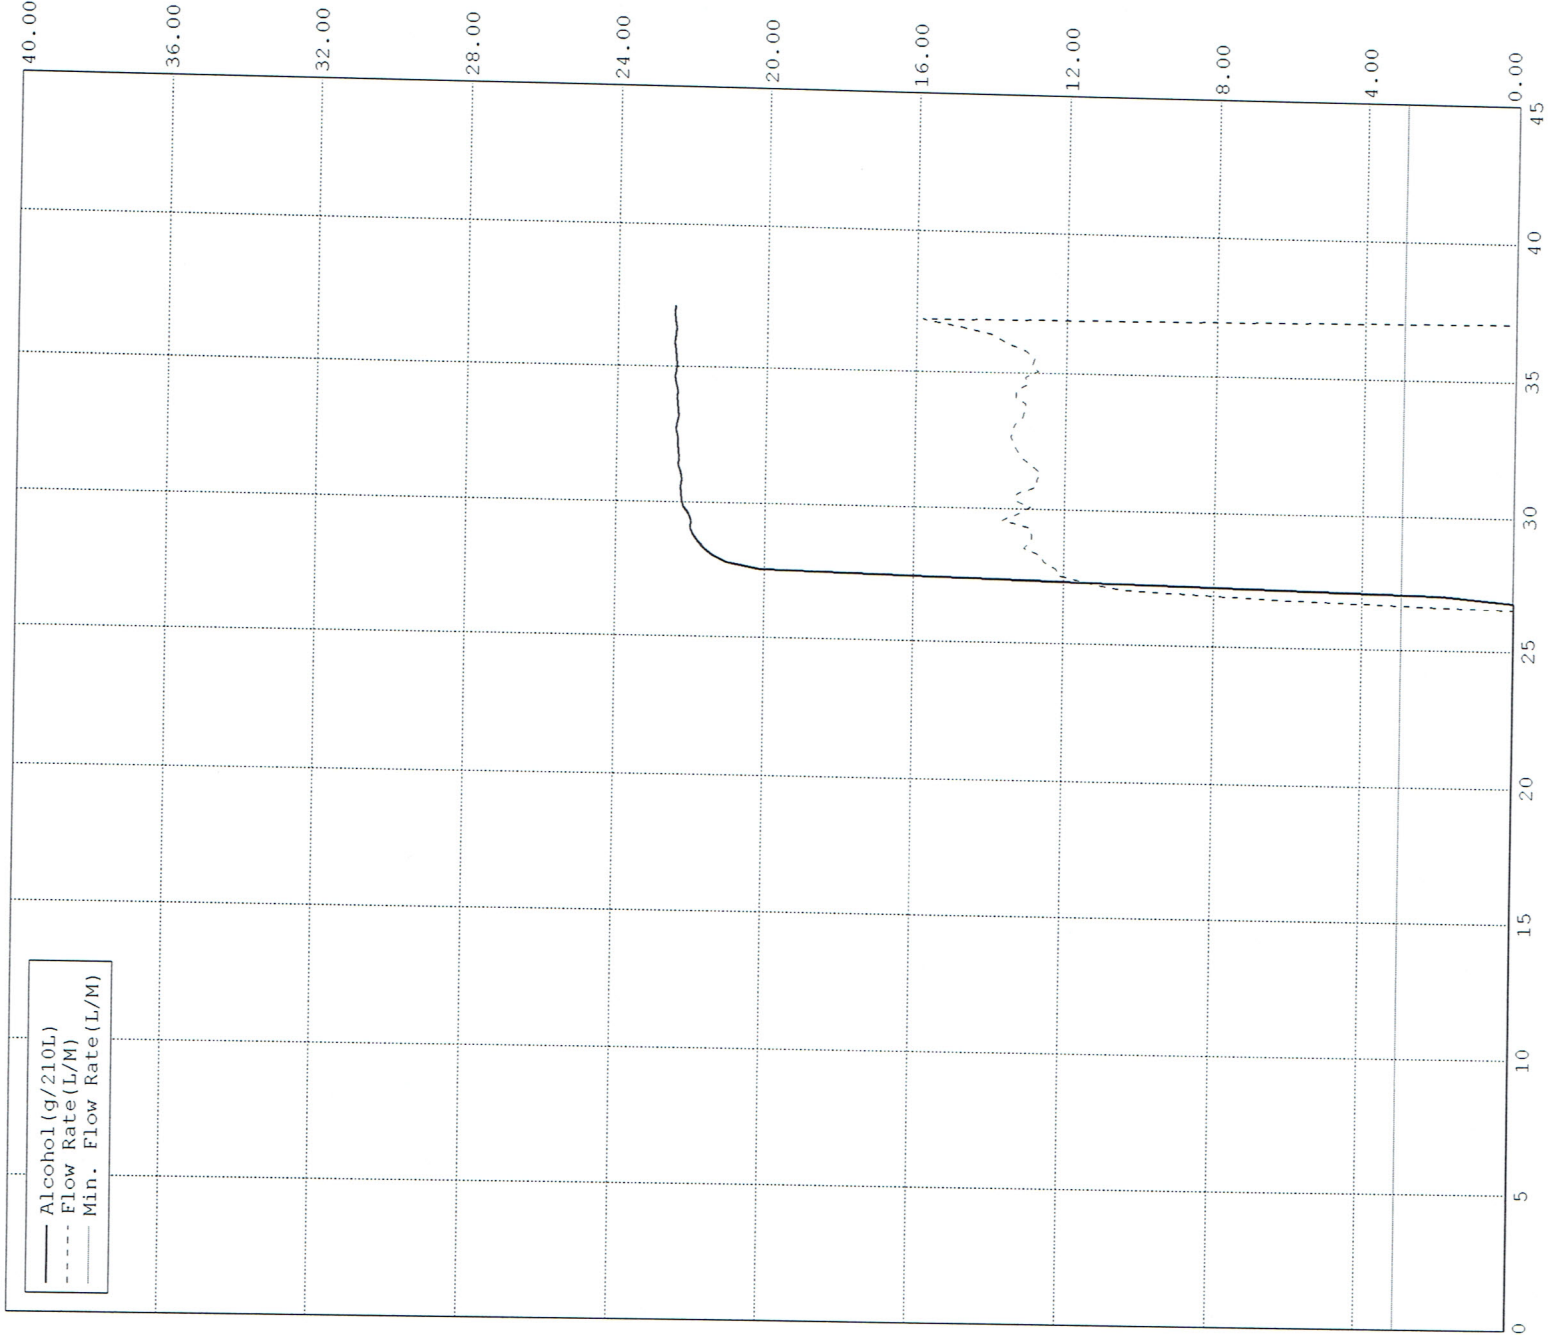

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100367

Date: 03/23/2020

Time: 16:13:36

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

DEREK WALTON

OPERATOR'S #: 9508

DEPT/AGENCY:

INTERFERENCE ISOPROPANOL

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 30.26: 0.081

LOT #: AG826101

EXPIRATION: 09/18/2020

DIAGNOSTIC CHECK

PASSED 16:14

BLANK TEST 0.000 16:14

INTERNAL STANDARD VERIFIED 16:15

Xq = 0.082 (0.32%)

EXTERNAL STANDARD 0.081 16:15


X[1] = 0.0813 (-0.0016) (-0.0003)

BLANK TEST 0.000 16:16

SUBJECT SAMPLE XXX 16:16

X[1] = 0.1130 (-0.0214) (-0.0016)

Interference Detected

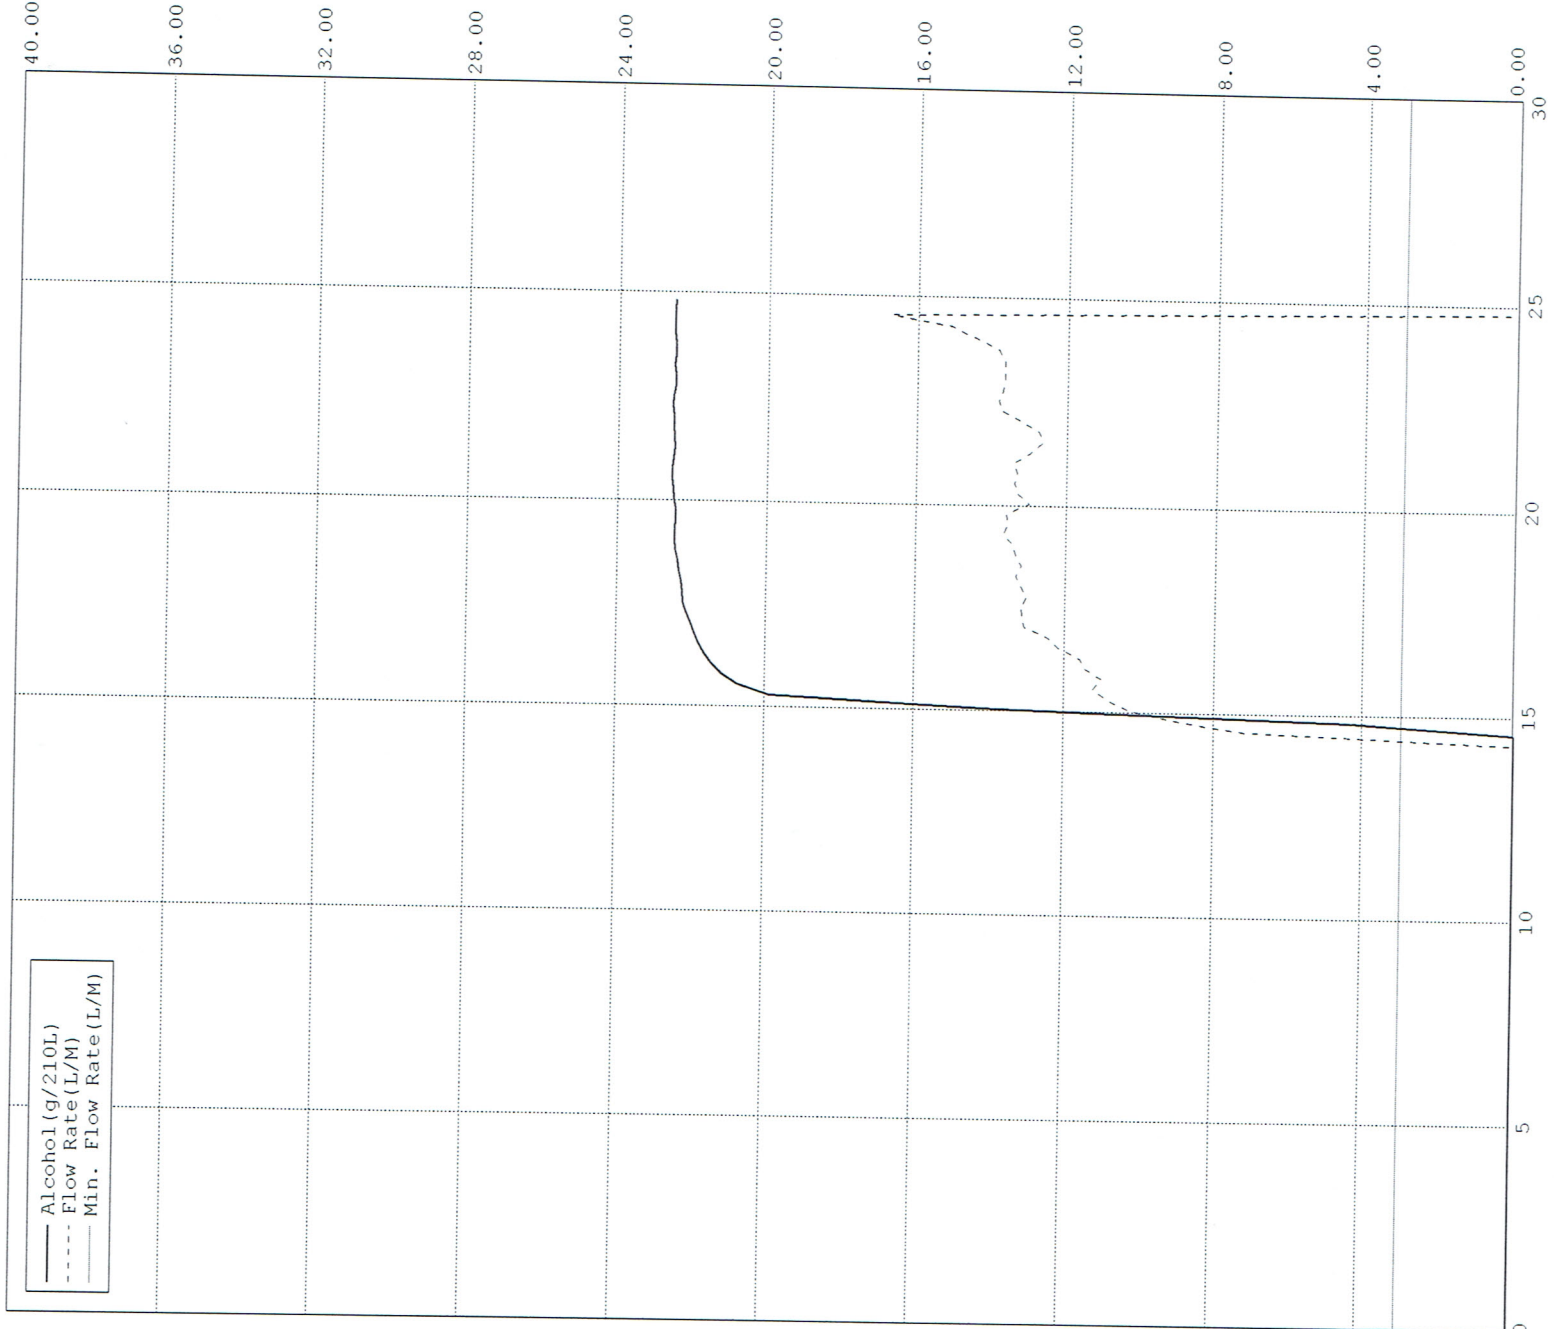

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100367  
-----

Date: 03/23/2020  
Time: 16:19:29

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
INTERFERENCE NEGATIVE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 30.27: 0.081  
LOT #: AG826101  
EXPIRATION: 09/18/2020

DIAGNOSTIC CHECK	PASSED	16:29
BLANK TEST	0.000	16:30
INTERNAL STANDARD	VERIFIED	16:30
$X_q = 0.082$ (0.21%)		
EXTERNAL STANDARD	0.081	16:30
$X[1] = 0.0814$ (-0.0018)	(0.0005)	
BLANK TEST	0.000	16:31
SUBJECT SAMPLE (Vol=2.19L)	0.096	16:32
$X[1] = 0.0960$ (-0.0004)	(-0.0013)	
BLANK TEST	0.000	16:33
EXTERNAL STANDARD	0.081	16:33
$X[1] = 0.0807$ (-0.0017)	(0.0005)	
BLANK TEST	0.000	16:34

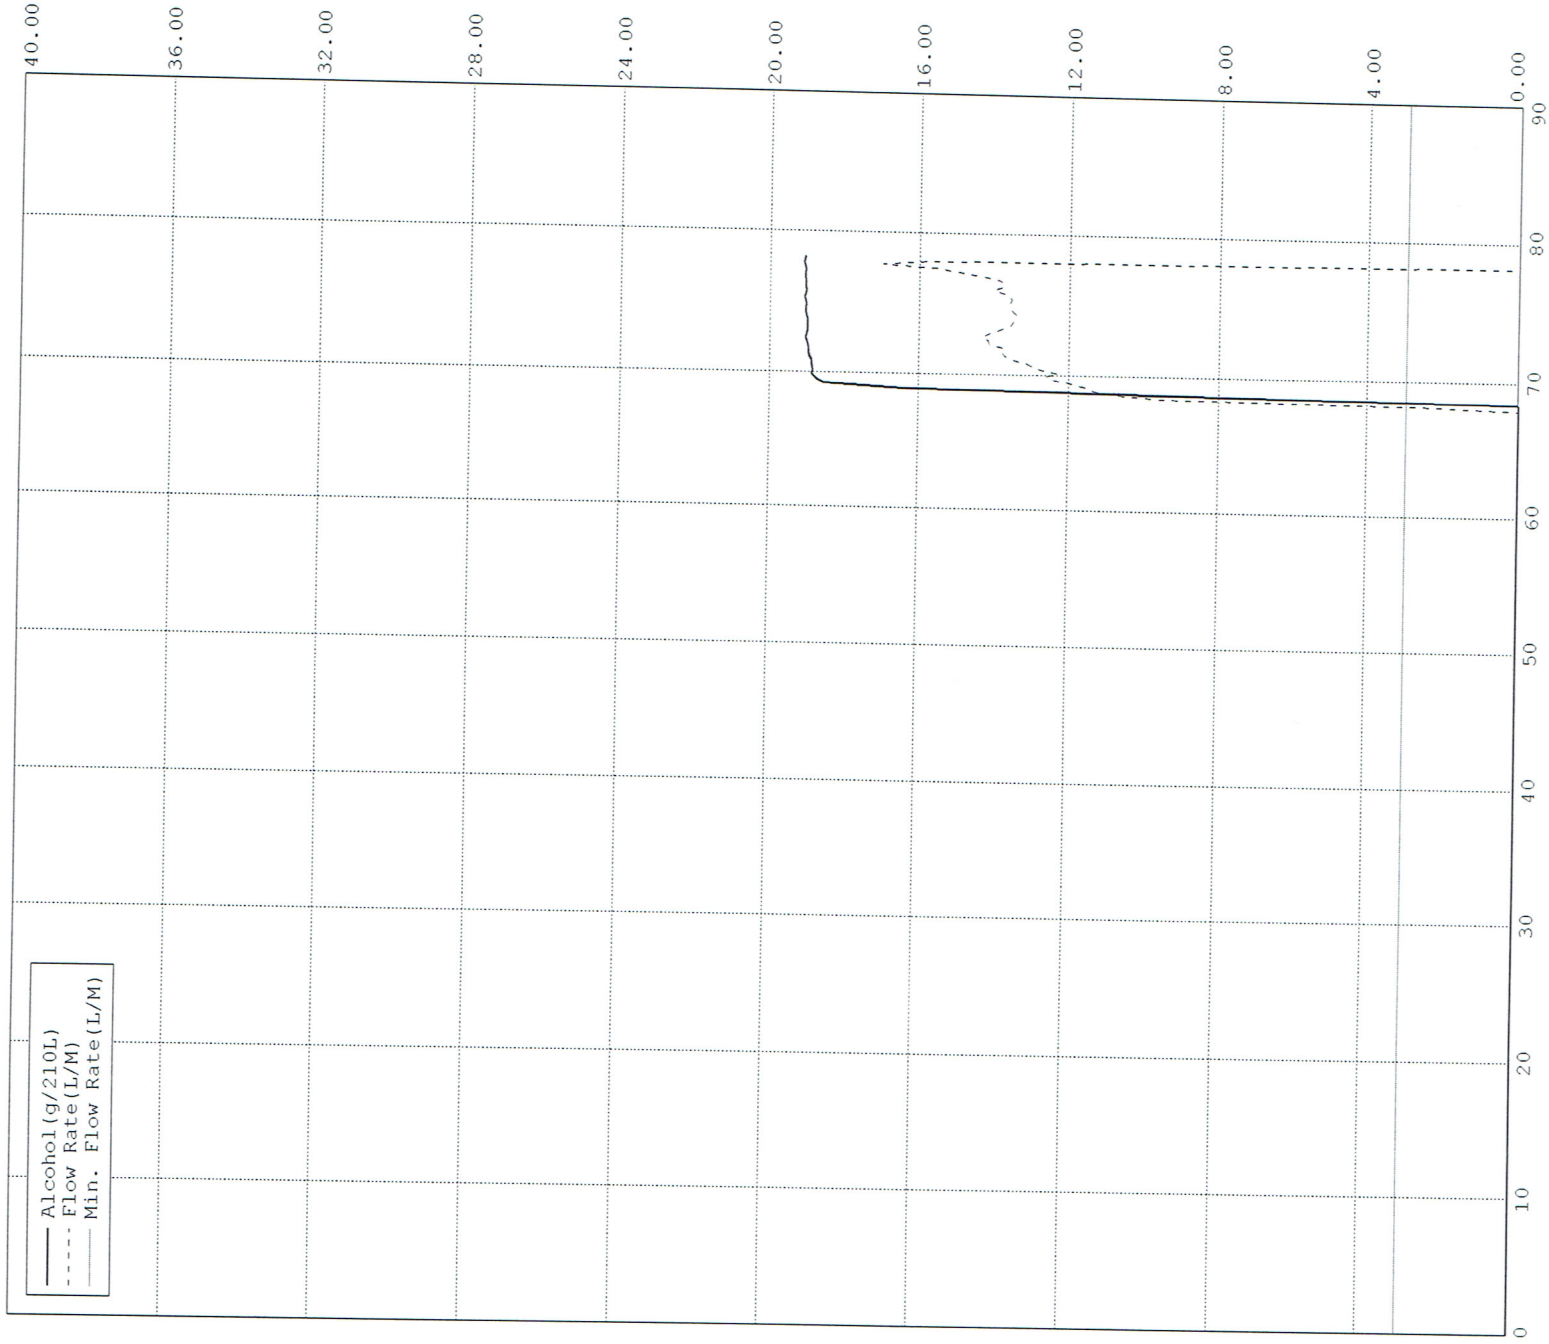

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100367

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 03/23/2020

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 30.24: 0.081  
LOT #: AG826101  
EXPIRATION: 09/18/2020  
TANK PRESSURE: 798 psi

BLANK TEST	0.000	16:54
INTERNAL STANDARD	VERIFIED	16:54
EXTERNAL STANDARD	0.081	16:55
BLANK TEST	0.000	16:55
EXTERNAL STANDARD	0.081	16:56
BLANK TEST	0.000	16:57
EXTERNAL STANDARD	0.081	16:57
BLANK TEST	0.000	16:58
EXTERNAL STANDARD	0.081	16:58
BLANK TEST	0.000	16:59
EXTERNAL STANDARD	0.081	16:59
BLANK TEST	0.000	17:00

Average = 0.0810  
Std Dev = 0.0000

## Diagnostic Check

### VERSIONS

DMT: 3.02  
PIC: 3.06  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.8°C PASSED  
Breath Tube = 45.7°C PASSED

### PUMP INFO

Flow Rate = 4.562 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

### FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

### INTERNAL STANDARD

PASSED

Before modem board

replacement. DM 03/24/20

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 03/23/2020  
Time: 17:01:41

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
DEREK WALTON  
OPERATOR'S #: 9508

DEPT/AGENCY:  
NON-DRINKING SUBJECT  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 30.23: 0.081  
LOT #: AG826101  
EXPIRATION: 09/18/2020

DIAGNOSTIC CHECK PASSED 17:03  
BLANK TEST 0.000 17:03  
INTERNAL STANDARD VERIFIED 17:03  
EXTERNAL STANDARD 0.082 17:03  
BLANK TEST 0.000 17:04  
SUBJECT SAMPLE (Vol=3.41L) 0.000 17:04  
BLANK TEST 0.000 17:05  
EXTERNAL STANDARD 0.081 17:05  
BLANK TEST 0.000 17:06

