

1- 907-868-7720

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100374

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 08/05/2013

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.84: 0.079  
LOT #: 02012080A1  
EXPIRATION: 03/01/2014

BLANK TEST	0.000	10:29
INTERNAL STANDARD	VERIFIED	10:29
EXTERNAL STANDARD	0.078	10:30
BLANK TEST	0.000	10:31
EXTERNAL STANDARD	0.077	10:31
BLANK TEST	0.000	10:32
EXTERNAL STANDARD	0.077	10:32
BLANK TEST	0.000	10:33
EXTERNAL STANDARD	0.077	10:33
BLANK TEST	0.000	10:34
EXTERNAL STANDARD	0.078	10:34
BLANK TEST	0.000	10:35

Average = 0.0774  
Std Dev = 0.0005

## Diagnostic Check

### VERSIONS

DMT: 2.00  
PIC: 3.02  
Modem: 2.3  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.6°C PASSED  
Breath Tube = 46.5°C PASSED

### PUMP INFO

Flow Rate = 5.340 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

### FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

### INTERNAL STANDARD

PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

*Nita J. Bolz*  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

8/13/2013

Subscribed and sworn before me this 13 day of Aug, 20 13

*Nikki Roth*  
Nikki Roth, Notary Public  
My Commission Expires With Office

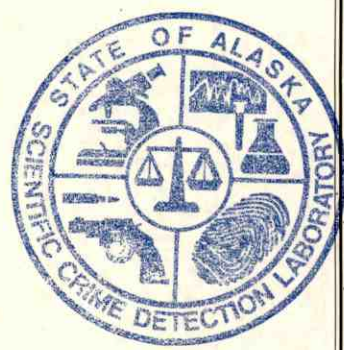

CB 8/9/13