



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100665

**Report Issue Date:** 01/12/2023  
**Date Received:** 2022-10-04  
**Condition of Item:** Needs Repair

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 12/14/2022** - As Found - **End Date 12/22/2022** As Found - Evaluation Analyst: Colleen O'Bryant  
 As Found Conditions - Barometric Pressure (inHg): 30.16 Barometer Used: Fisher S/N 221250180 Temperature (C): 21.6  
 Relative Humidity (%): 4

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.081	AG135004	0.080	0.079	0.079	0.079	0.079	0.079	0.079
0.300	0.302	AG130502	0.295	0.295	0.295	0.295	0.295	0.295	0.295

Regulator makes a loud clicking sound while pulling gas. The flow rate is visibly variable in wave form. Replace regulator.

**Start Date 01/05/2023** - As Left - **End Date 01/05/2023**

As Left Conditions - Barometric Pressure (inHg): 29.25 Barometer Used: Fisher S/N 221250180 Temperature (C): 21.1 Relative Humidity (%): 16

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG217902	0.019	0.019	0.019	0.019	0.019	0.019	+/- 0.002	
0.040	0.039	AG217904	0.039	0.038	0.038	0.038	0.038	0.038	+/- 0.003	
0.080	0.078	AG135004	0.076	0.076	0.076	0.076	0.076	0.076	+/- 0.003	
0.100	0.098	AG211003	0.096	0.096	0.096	0.096	0.096	0.096	+/- 0.003	
0.150	0.147	AG134205	0.145	0.144	0.145	0.145	0.144	0.145	+/- 0.004	
0.300	0.293	AG130502	0.286	0.285	0.286	0.286	0.286	0.286	+/- 0.008	

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Technically and administratively reviewed by Carlie Glaister on 01/12/2023

Results authorized by Colleen O'Bryant on 01/10/2023  
[colleen.obryant@alaska.gov](mailto:colleen.obryant@alaska.gov)

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100665 Analyst: C. O. Bryant Start Date: 1/5/23

- Diagnostic Test (attached)
- Adjust voltages, if needed
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Internal Standard value  $\leq$  3.00%
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.6 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.25 Temperature (C): 21.1 Relative Humidity (%): 16

Linearity Test (attached)

0.020g/210L Mnf:	<u>Aargas</u>	Lot:	<u>AG217902</u>	Exp:	<u>6/28/24</u>
0.040g/210L Mnf:	<u>Aargas</u>	Lot:	<u>AG217904</u>	Exp:	<u>6/28/24</u>
0.080g/210L Mnf:	<u>Aargas</u>	Lot:	<u>AB135004</u>	Exp:	<u>12/16/23</u>
0.100g/210L Mnf:	<u>Aargas</u>	Lot:	<u>AG11003</u>	Exp:	<u>4/20/24</u>
0.150g/210L Mnf:	<u>Aargas</u>	Lot:	<u>AG134205</u>	Exp:	<u>12/8/23</u>
0.300g/210L Mnf:	<u>Aargas</u>	Lot:	<u>AG130502</u>	Exp:	<u>11/1/23</u>

Functional Tests (attached)

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles)

Acetone Mnf: LifeLoc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: DR5298 Verification Performed?

Isopropanol Mnf: LifeLoc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: SD1198 Verification Performed?

Neg. Control Mnf: LifeLoc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: SD1202 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 2210958384 Calibration Due Date: 11/9/23

- Verify stylus is calibrated
- Non-Drinking Subject Test
- Reset Options
- Upload
- Clear Memory
- Remove Tank Prior to Shutdown
- Verification of Calibration (VOC)
- Calibration End Date: 1/5/23

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100665  
-----

Date: 01/05/2023  
Time: 04:56:03

VERSIONS  
DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 45.0°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.70 V PASSED  
(0.98 V - 2.30 V)  
Cooler Voltage = 1.67 V PASSED  
(1.03 V - 2.41 V)  
Bias Voltage = 79 V PASSED  
(47 V - 111 V)  
Chopper Freq = 540 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.2 in

PUMP INFO

Flow Rate = 4.996 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.001 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.128 0.28% (0.00% - 4.00%) PASSED

Technician Screen

-----  
DATAMASTER dmt: 100665  
-----

Date: 01/05/2023  
Time: 5:30 AM

Temperatures (°C)

Sample Cell: 49.2°C  
Breath Tube: 45.4°C

Current Barometer 29.3 in  
Volume (Ltr) 1.45

Settings

Lamp: 1.81 V  
Bias: 80 V  
Cooler: 1.67 V  
Chopper: 541 Hz

Voltages (V)

Flow: 1.07 V  
Detector: -0.070 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100665  
-----

Date: 04/17/2012  
Time: 04:30:06

Ca = 0.1000  
CAL = 0.968497    0.800 <= CAL < 1.200  
b1 = 0.0001    0.0000 <= b1 < 0.0040  
b2 = 0.0054    0.0010 <= b2 < 0.0100  
b3 = 0.0003    0.0000 <= b3 < 0.0040  
Xq = 0.1289    0.0500 <= Xq < 0.2000  
a21 = 1.229257    1.050 <= a21 < 1.300  
a31 = 0.541082    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100665

Date: 01/05/2023  
Time: 05:32:10

SUBJECT NAME:  
TEST TEST  
LICENSE #: VOLUME TEST

OPERATOR NAME:  
COLLEEN S OBRYANT  
OPERATOR'S #: 6237


DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.25: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	05:33
BLANK TEST	0.000	05:33
INTERNAL STANDARD	VERIFIED	05:33
EXTERNAL STANDARD	0.076	05:33
BLANK TEST	0.000	05:34
SUBJECT SAMPLE (Vol=1.63L)	0.000	05:36
BLANK TEST	0.000	05:36
EXTERNAL STANDARD	0.076	05:37
BLANK TEST	0.000	05:38

— Alcohol (g/210L)  
 - - - - Flow Rate (L/M)  
 — Min. Flow Rate (L/M)

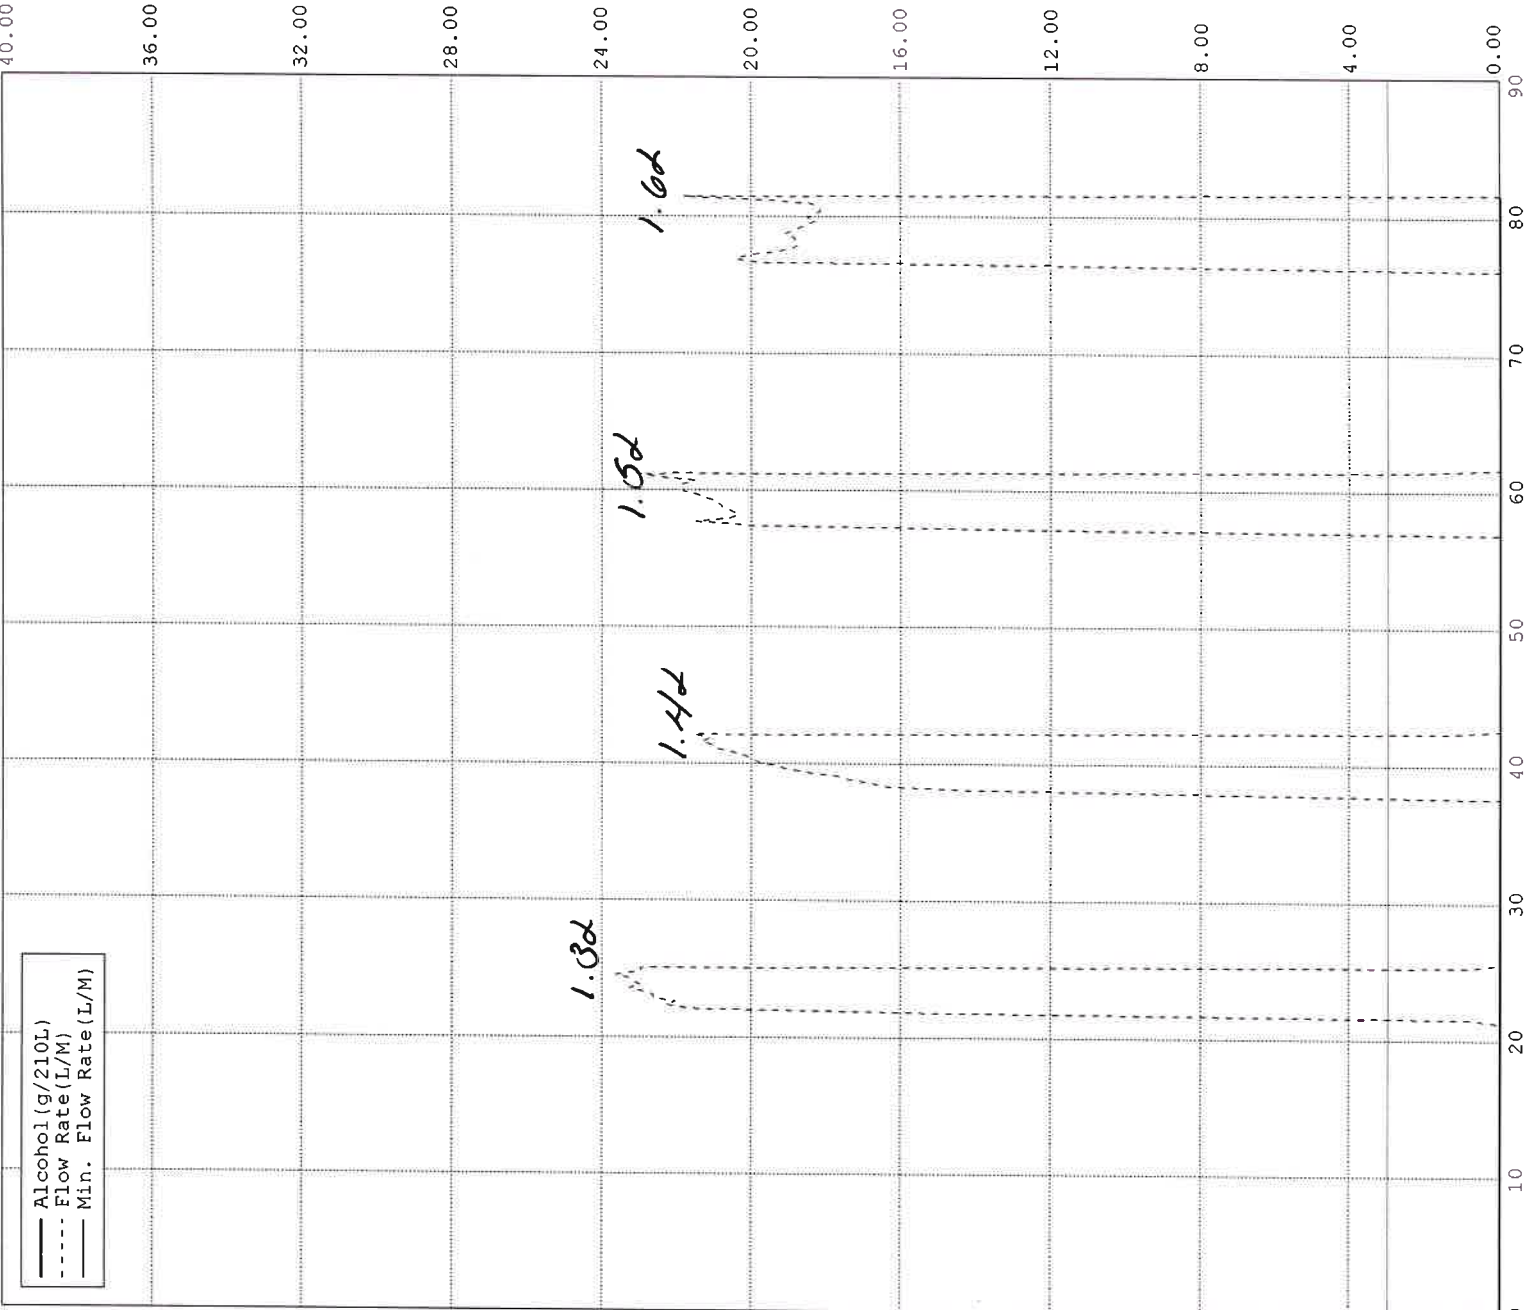

**LINEARITY CHECK**


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100665  
 -----

Date: 01/05/2023  
 Time: 05:40:44

SUPERVISOR NAME:  
 COLLEEN S OBRyant  
 OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0190	0.0000
0.039	0.0382	0.0004
0.078	0.0760	0.0000
0.098	0.0960	0.0000
0.147	0.1446	0.0005
0.293	0.2858	0.0004

SLOPE = 0.976936  
 R<sup>2</sup> = 0.999966

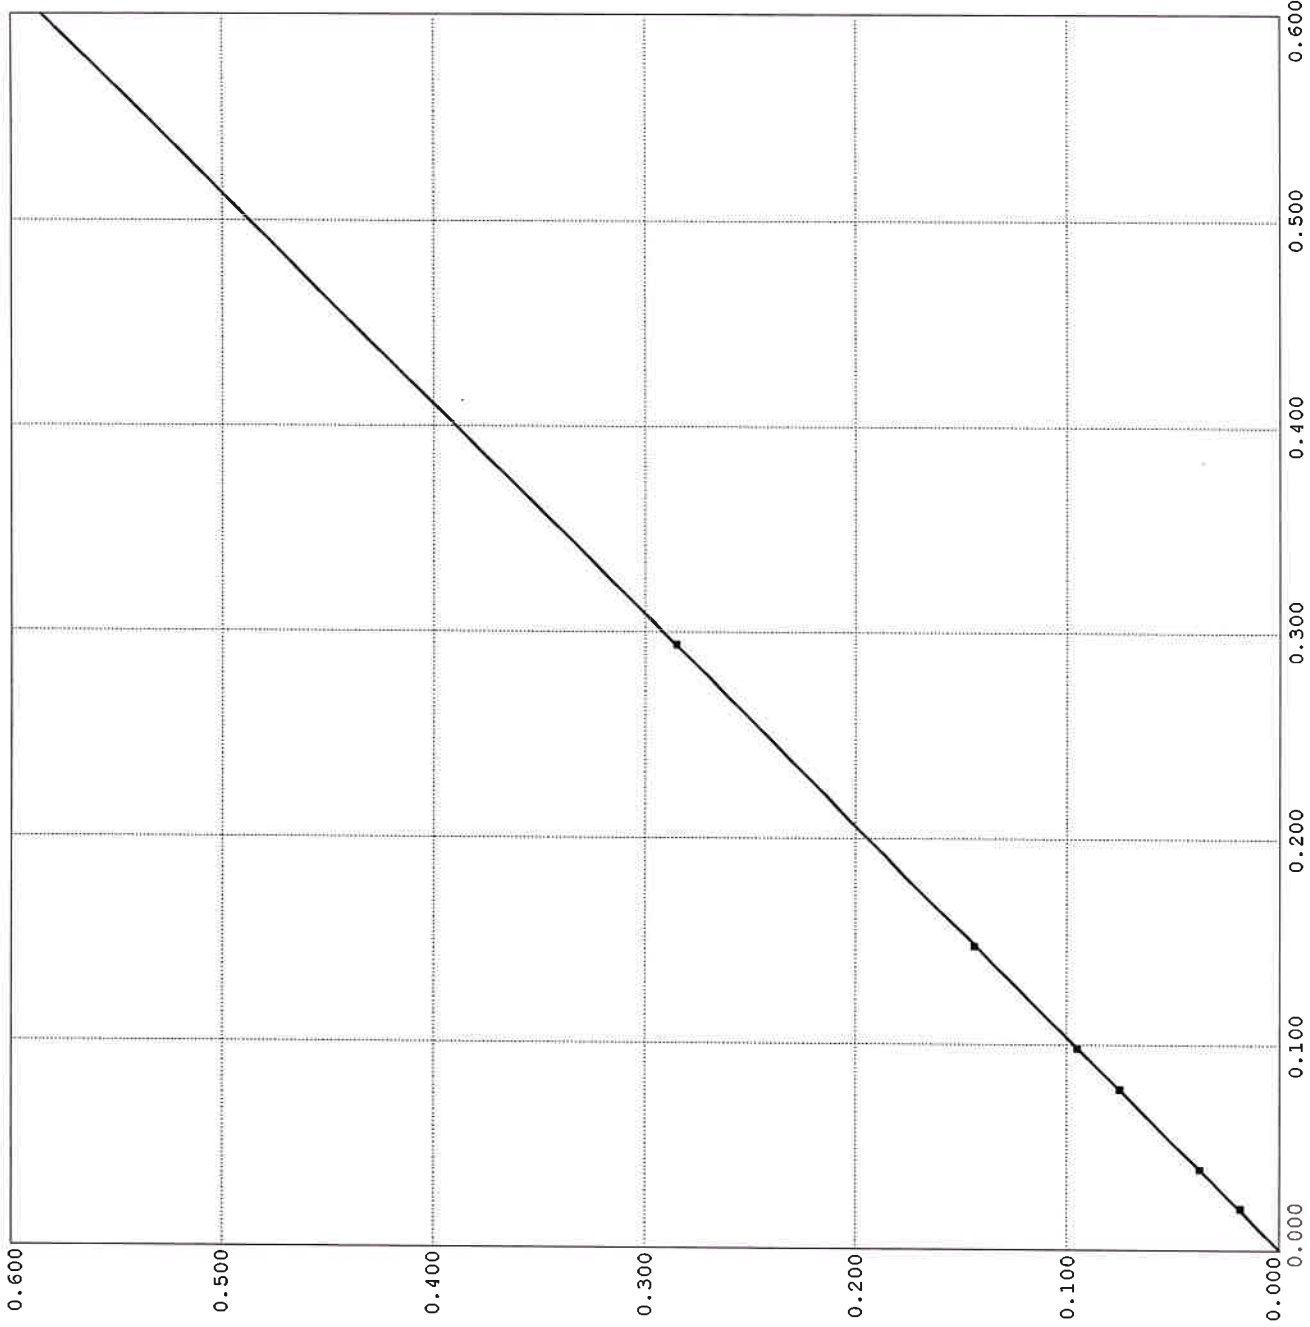

*CPB*

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100665






Date: 01/05/2023  
Time: 05:40:46

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.25: 0.020  
LOT #: AG217902  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 977 psi

BLANK TEST	0.000	05:41
INTERNAL STANDARD	VERIFIED	05:42
EXTERNAL STANDARD	0.019	05:42
BLANK TEST	0.000	05:43
EXTERNAL STANDARD	0.019	05:43
BLANK TEST	0.000	05:44
EXTERNAL STANDARD	0.019	05:44
BLANK TEST	0.000	05:45
EXTERNAL STANDARD	0.019	05:45
BLANK TEST	0.000	05:46
EXTERNAL STANDARD	0.019	05:46
BLANK TEST	0.000	05:47

Average = 0.0190  
Std Dev = 0.0000

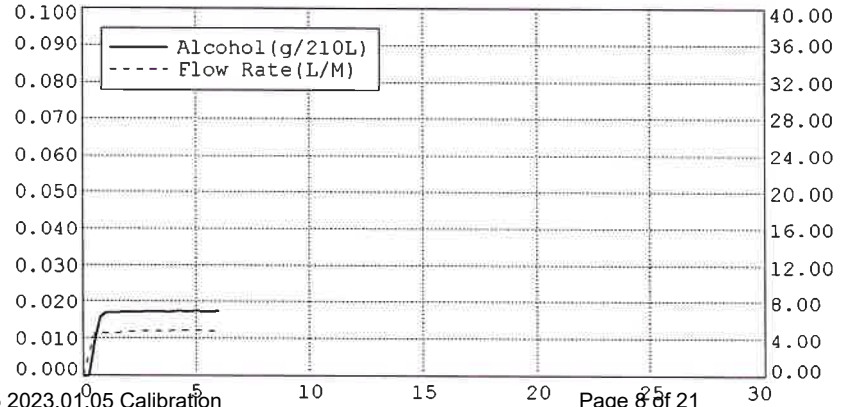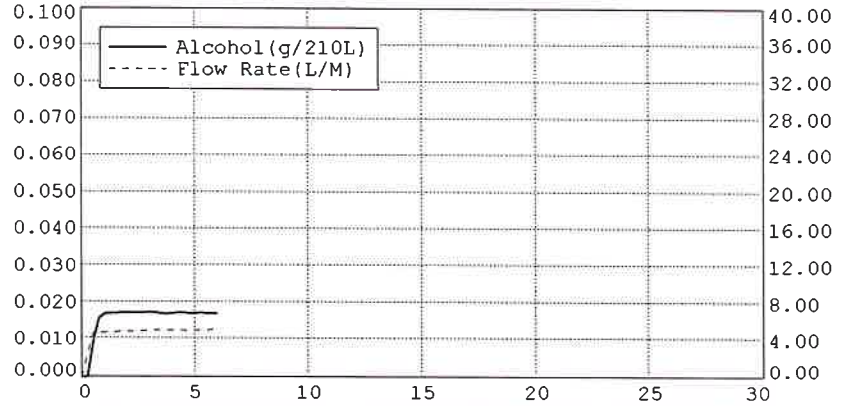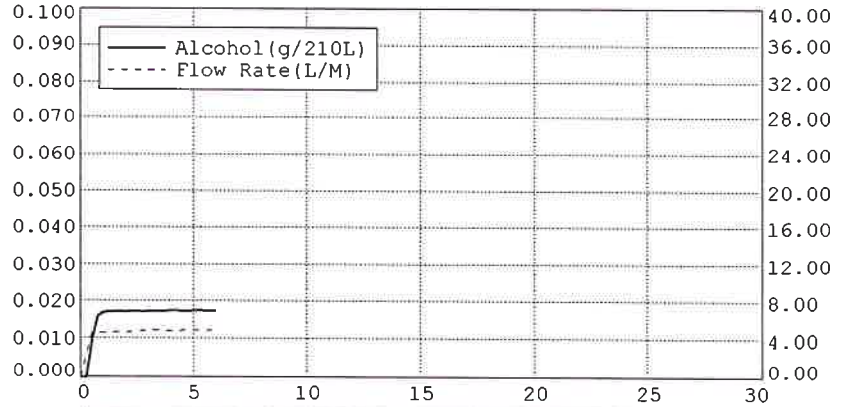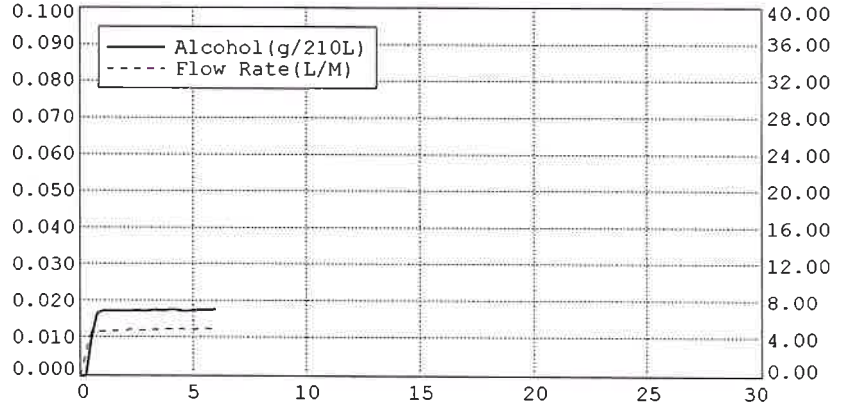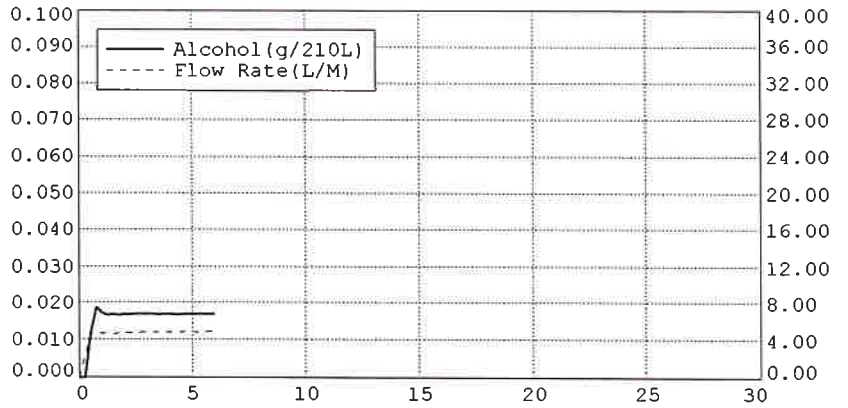



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100665






Date: 01/05/2023  
 Time: 05:48:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.25: 0.039  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 1051 psi

BLANK TEST	0.000	05:50
INTERNAL STANDARD	VERIFIED	05:50
EXTERNAL STANDARD	0.039	05:50
BLANK TEST	0.000	05:51
EXTERNAL STANDARD	0.038	05:51
BLANK TEST	0.000	05:52
EXTERNAL STANDARD	0.038	05:52
BLANK TEST	0.000	05:53
EXTERNAL STANDARD	0.038	05:53
BLANK TEST	0.000	05:54
EXTERNAL STANDARD	0.038	05:55
BLANK TEST	0.000	05:55

Average = 0.0382  
 Std Dev = 0.0004

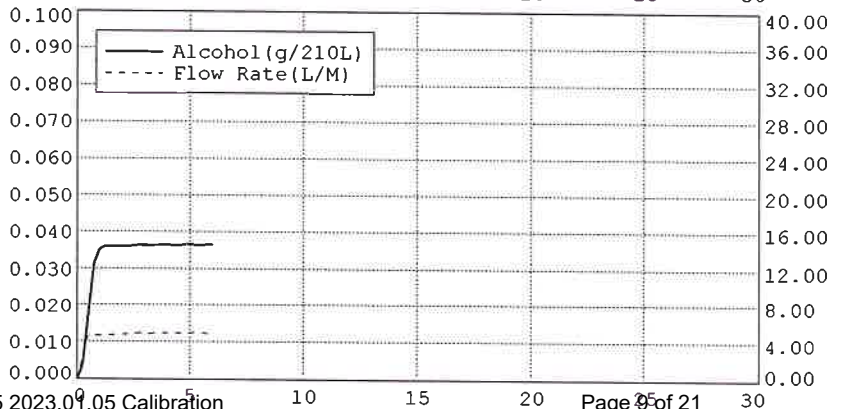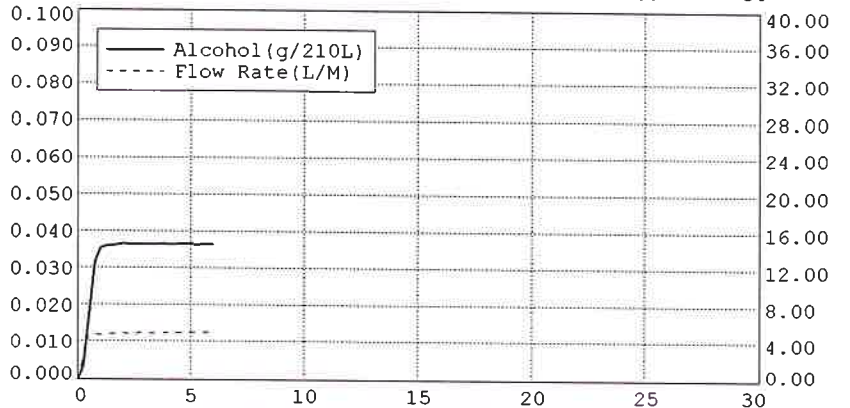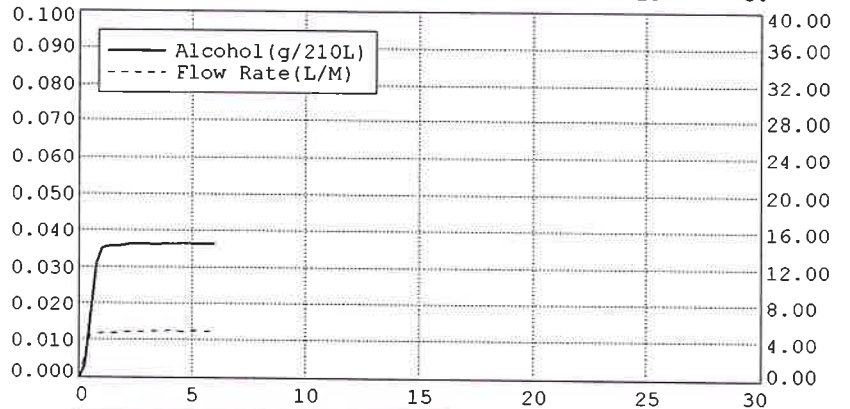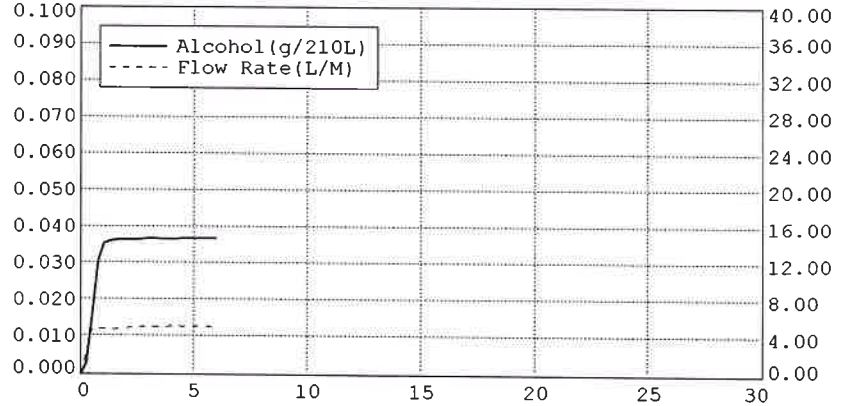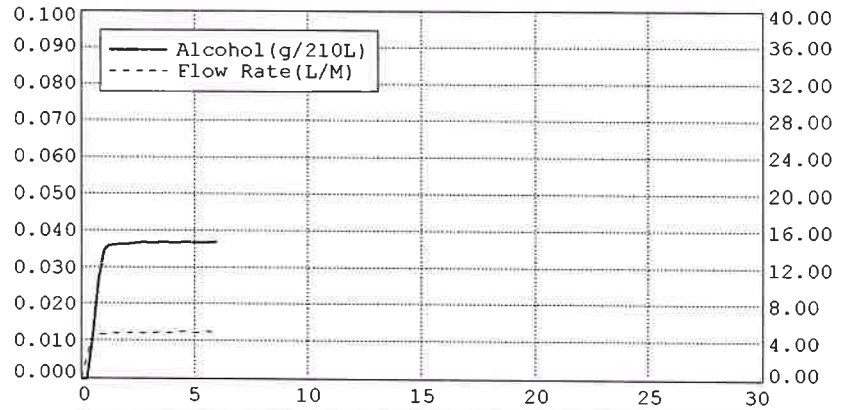

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
DATAMASTER dmt: 100665






Date: 01/05/2023  
Time: 05:56:15

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.25: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023  
TANK PRESSURE: 780 psi

BLANK TEST	0.000	05:57
INTERNAL STANDARD	VERIFIED	05:57
EXTERNAL STANDARD	0.076	05:57
BLANK TEST	0.000	05:58
EXTERNAL STANDARD	0.076	05:58
BLANK TEST	0.000	05:59
EXTERNAL STANDARD	0.076	05:59
BLANK TEST	0.000	06:00
EXTERNAL STANDARD	0.076	06:01
BLANK TEST	0.000	06:01
EXTERNAL STANDARD	0.076	06:02
BLANK TEST	0.000	06:03

Average = 0.0760  
Std Dev = 0.0000

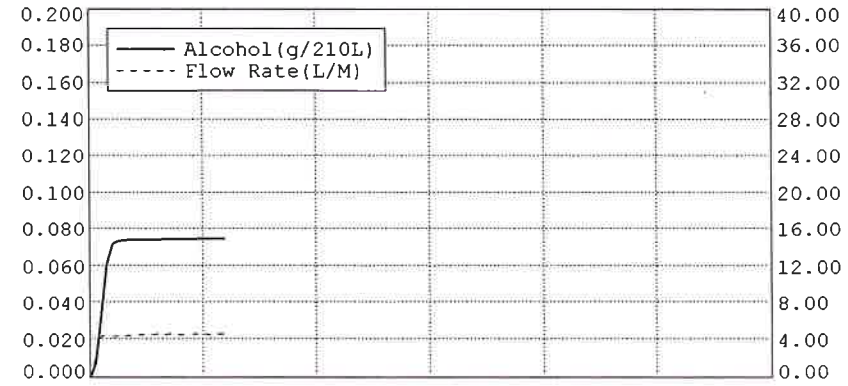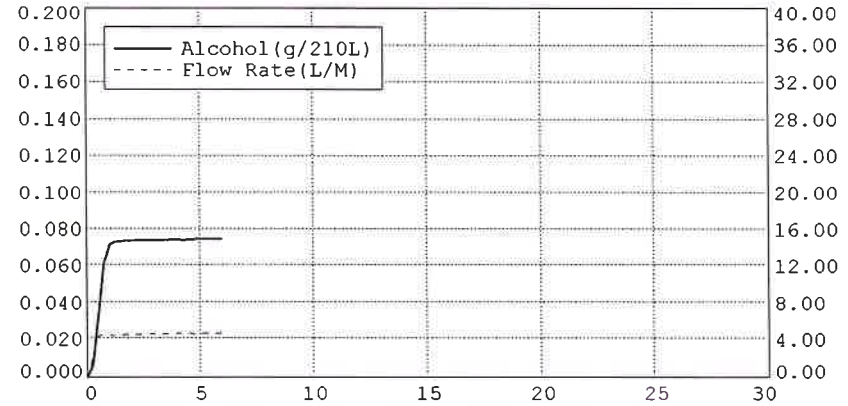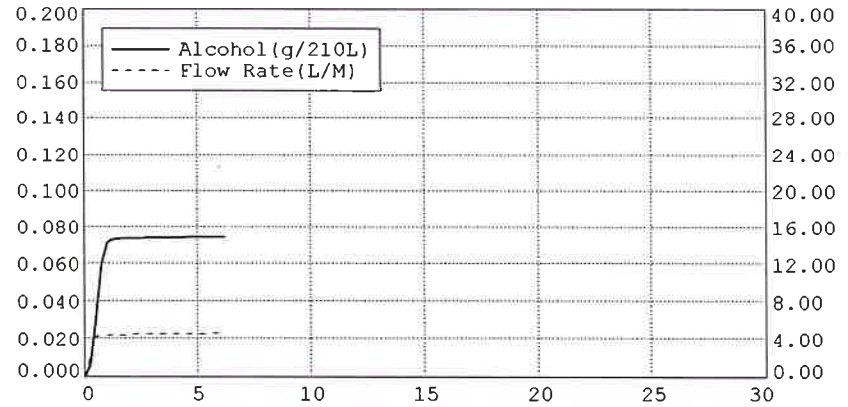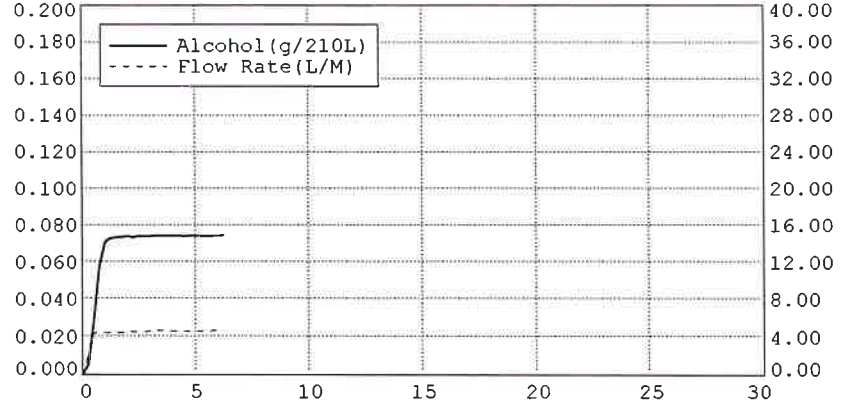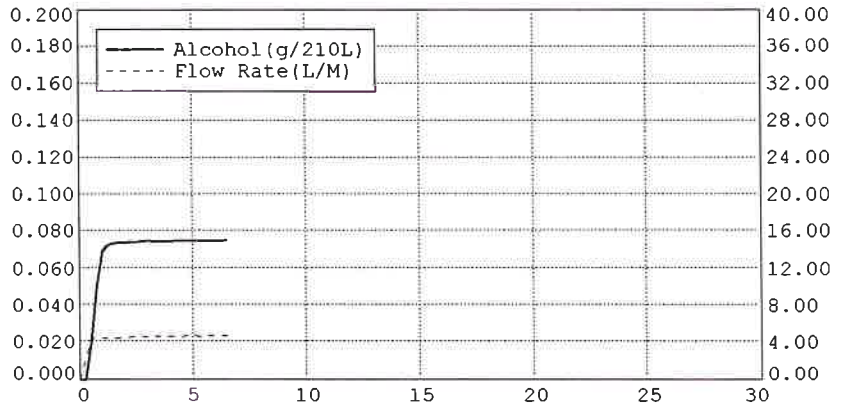

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100665






Date: 01/05/2023  
 Time: 06:05:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.25: 0.098  
 LOT #: AG211003  
 EXPIRATION: 04/20/2024  
 TANK PRESSURE: 915 psi

BLANK TEST	0.000	06:06
INTERNAL STANDARD	VERIFIED	06:06
EXTERNAL STANDARD	0.096	06:06
BLANK TEST	0.000	06:07
EXTERNAL STANDARD	0.096	06:07
BLANK TEST	0.000	06:08
EXTERNAL STANDARD	0.096	06:09
BLANK TEST	0.000	06:09
EXTERNAL STANDARD	0.096	06:10
BLANK TEST	0.000	06:11
EXTERNAL STANDARD	0.096	06:11
BLANK TEST	0.000	06:12

Average = 0.0960  
 Std Dev = 0.0000

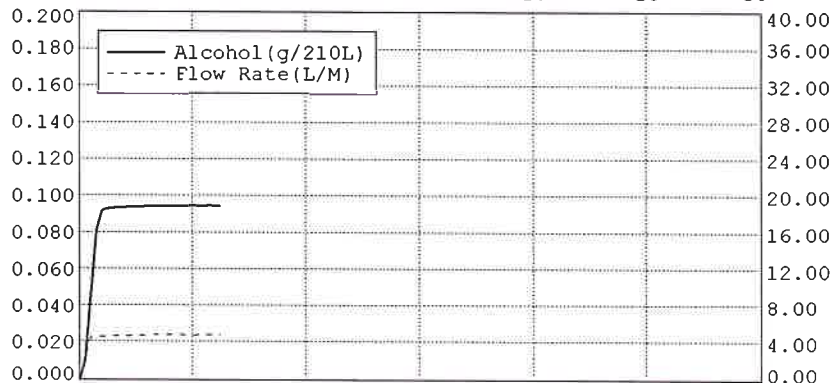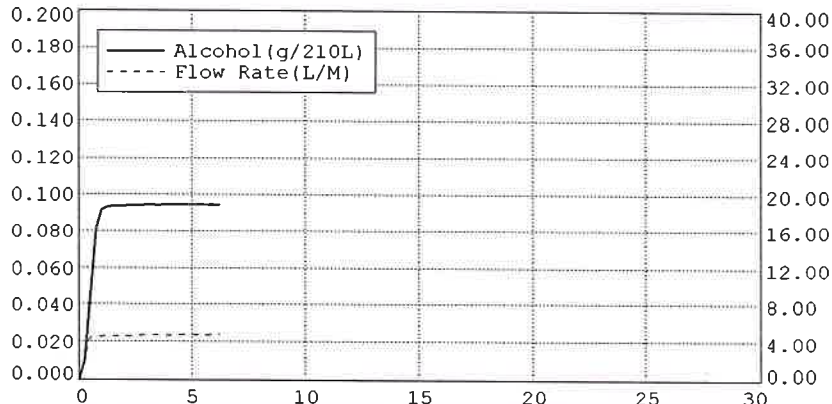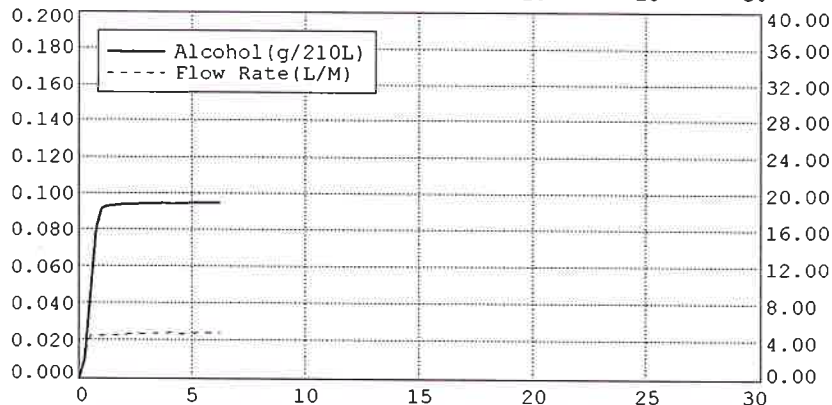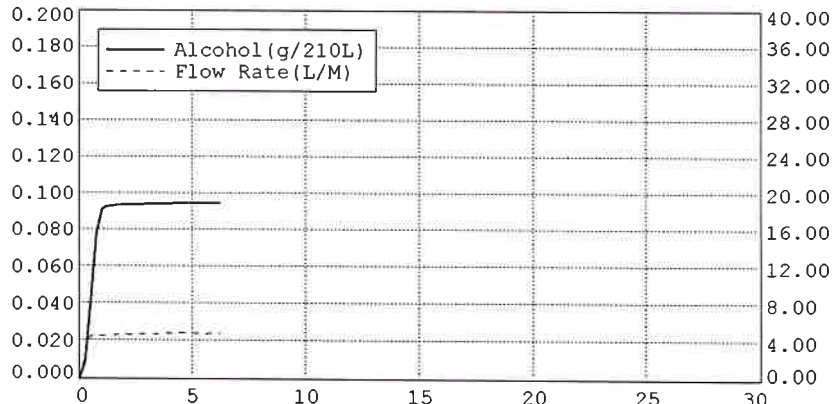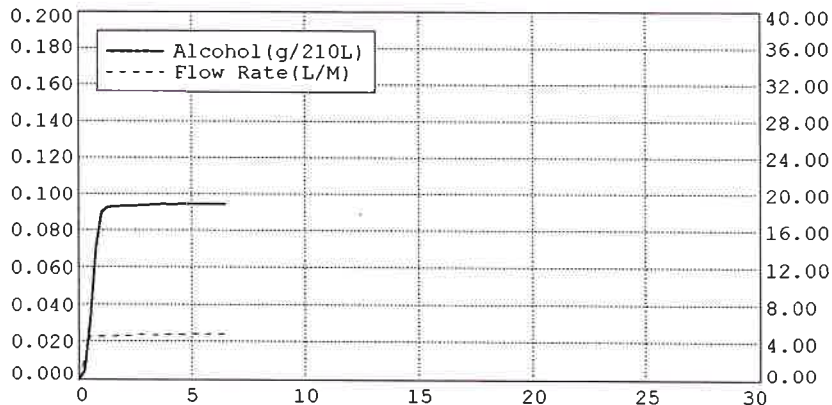

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100665






Date: 01/05/2023  
 Time: 06:12:34

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.25: 0.147  
 LOT #: AG134205  
 EXPIRATION: 12/08/2023  
 TANK PRESSURE: 945 psi

BLANK TEST	0.000	06:13
INTERNAL STANDARD	VERIFIED	06:13
EXTERNAL STANDARD	0.145	06:14
BLANK TEST	0.000	06:15
EXTERNAL STANDARD	0.144	06:15
BLANK TEST	0.000	06:16
EXTERNAL STANDARD	0.145	06:16
BLANK TEST	0.000	06:17
EXTERNAL STANDARD	0.145	06:17
BLANK TEST	0.000	06:18
EXTERNAL STANDARD	0.144	06:18
BLANK TEST	0.000	06:19

Average = 0.1446  
 Std Dev = 0.0005

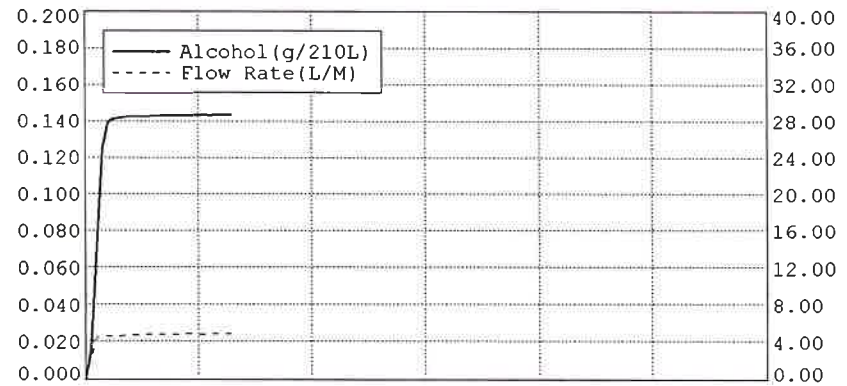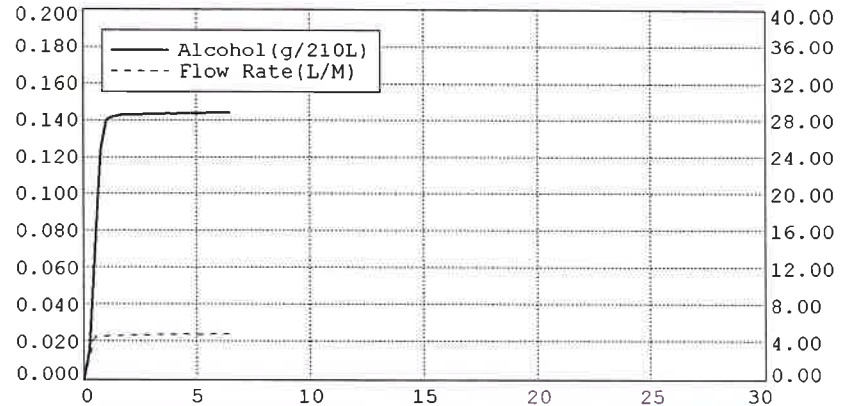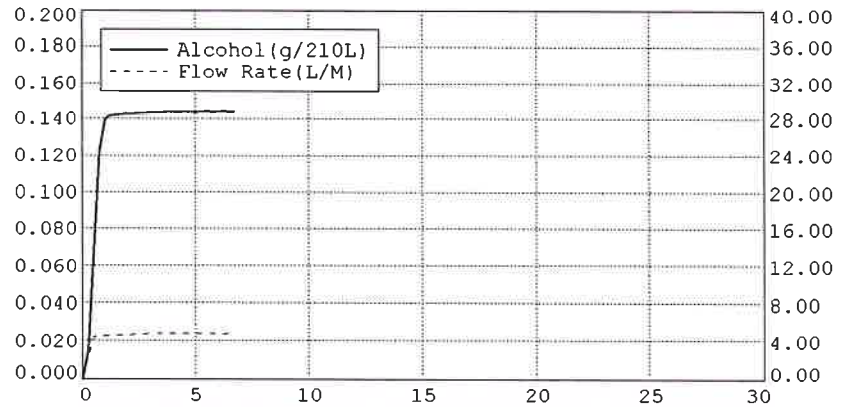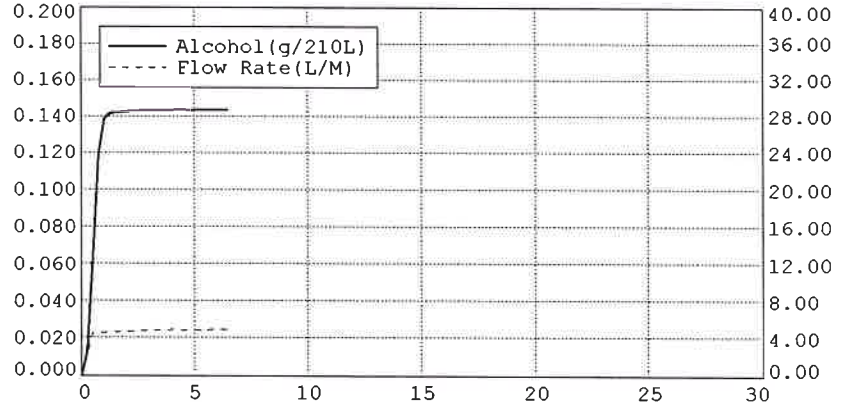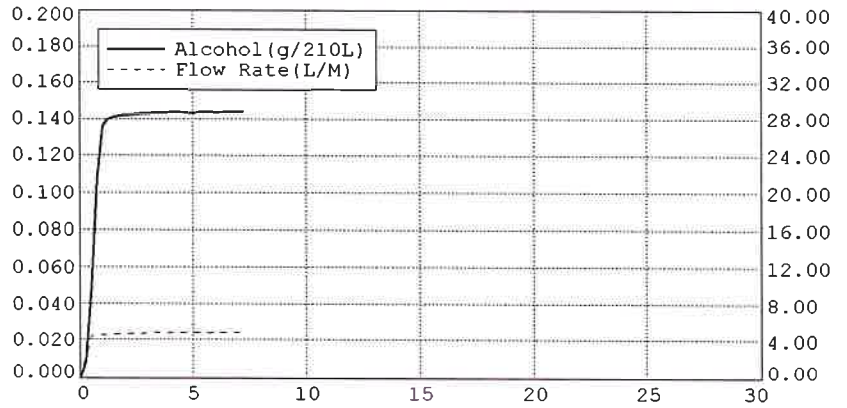

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100665






Date: 01/05/2023  
 Time: 06:21:57

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.25: 0.293  
 LOT #: AG130502  
 EXPIRATION: 11/01/2023  
 TANK PRESSURE: 225 psi

BLANK TEST	0.000	06:22
INTERNAL STANDARD	VERIFIED	06:23
EXTERNAL STANDARD	0.286	06:23
BLANK TEST	0.000	06:24
EXTERNAL STANDARD	0.285	06:24
BLANK TEST	0.000	06:25
EXTERNAL STANDARD	0.286	06:25
BLANK TEST	0.000	06:26
EXTERNAL STANDARD	0.286	06:26
BLANK TEST	0.000	06:27
EXTERNAL STANDARD	0.286	06:27
BLANK TEST	0.000	06:28

Average = 0.2858  
 Std Dev = 0.0004

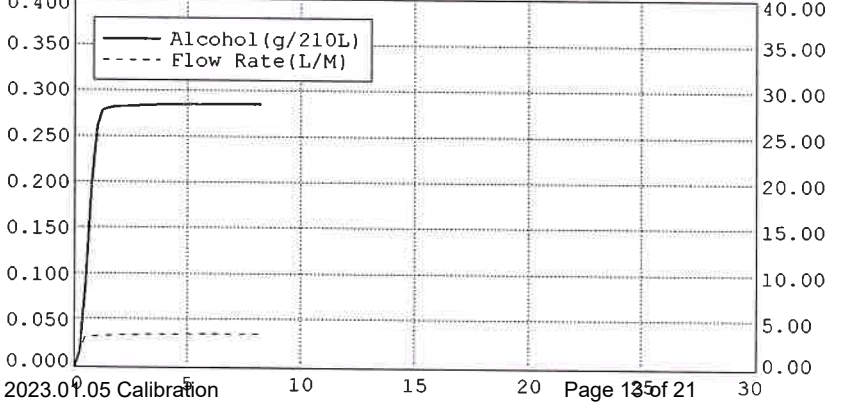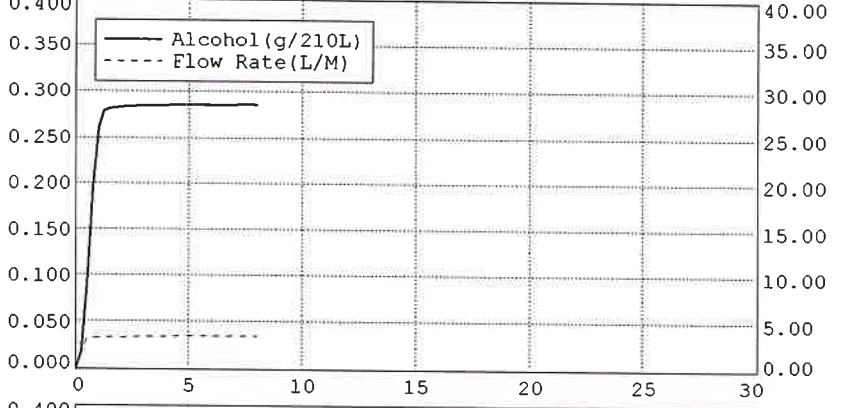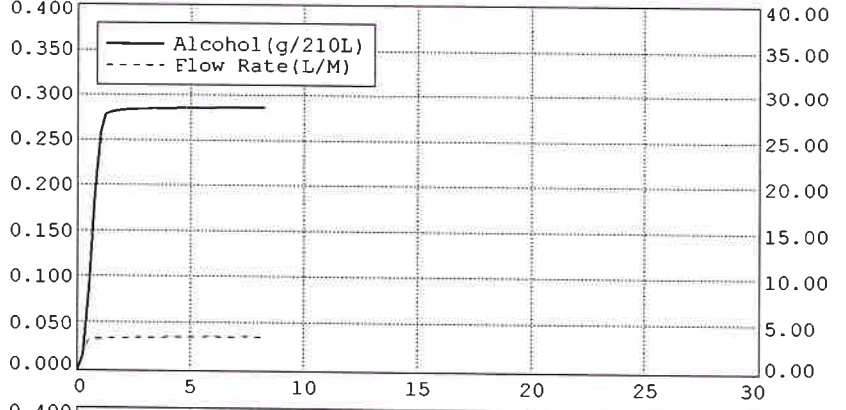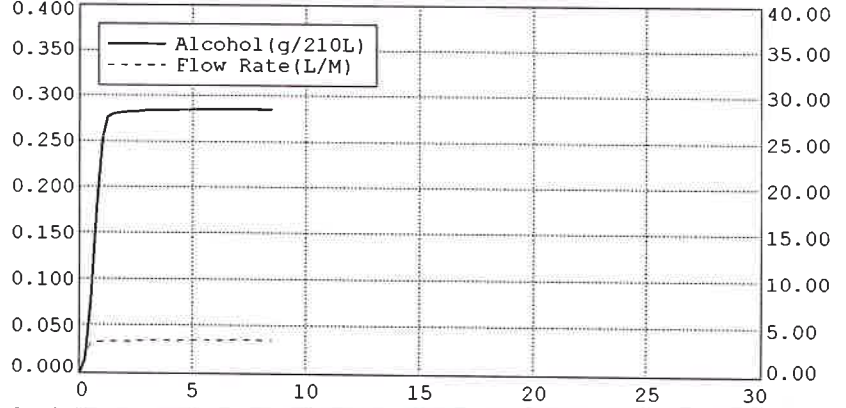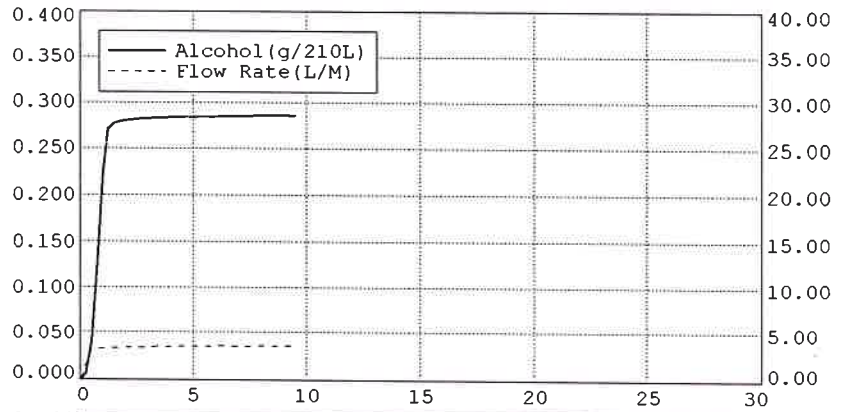

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100665

Date: 01/05/2023

Time: 07:01:22

SUBJECT NAME:

TEST TEST

LICENSE #: INCOMPLETE

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 23-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.25: 0.078

LOT #: AG135004

EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 07:08  
0.000 07:09  
VERIFIED 07:09  
0.076 07:09  
0.000 07:10  
INCOMPLETE 07:12

CAB

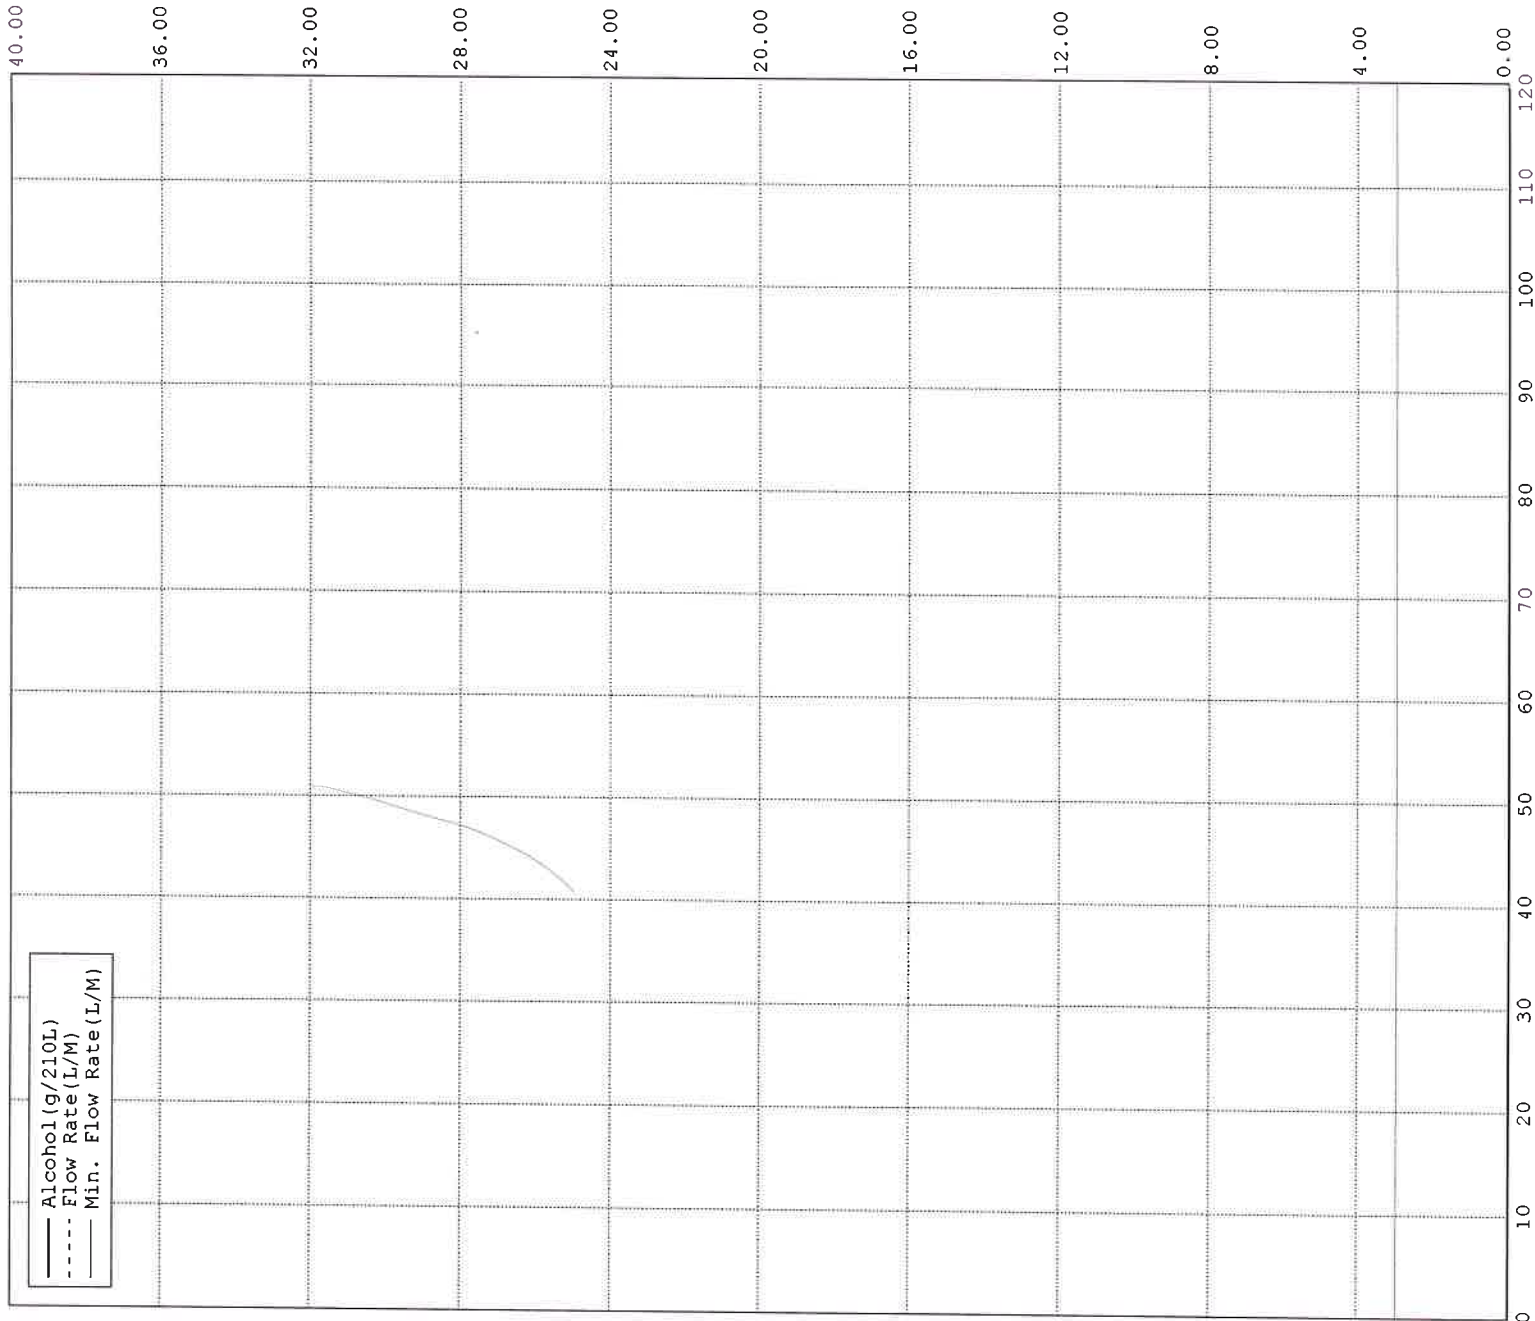

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100665

Date: 01/05/2023  
Time: 07:32:27


SUBJECT NAME:  
TEST TEST  
LICENSE #: INVALID

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.26: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	07:33
BLANK TEST	0.000	07:33
INTERNAL STANDARD	VERIFIED	07:33
EXTERNAL STANDARD	0.076	07:33
BLANK TEST	0.000	07:34
SUBJECT SAMPLE	INVALID	07:35

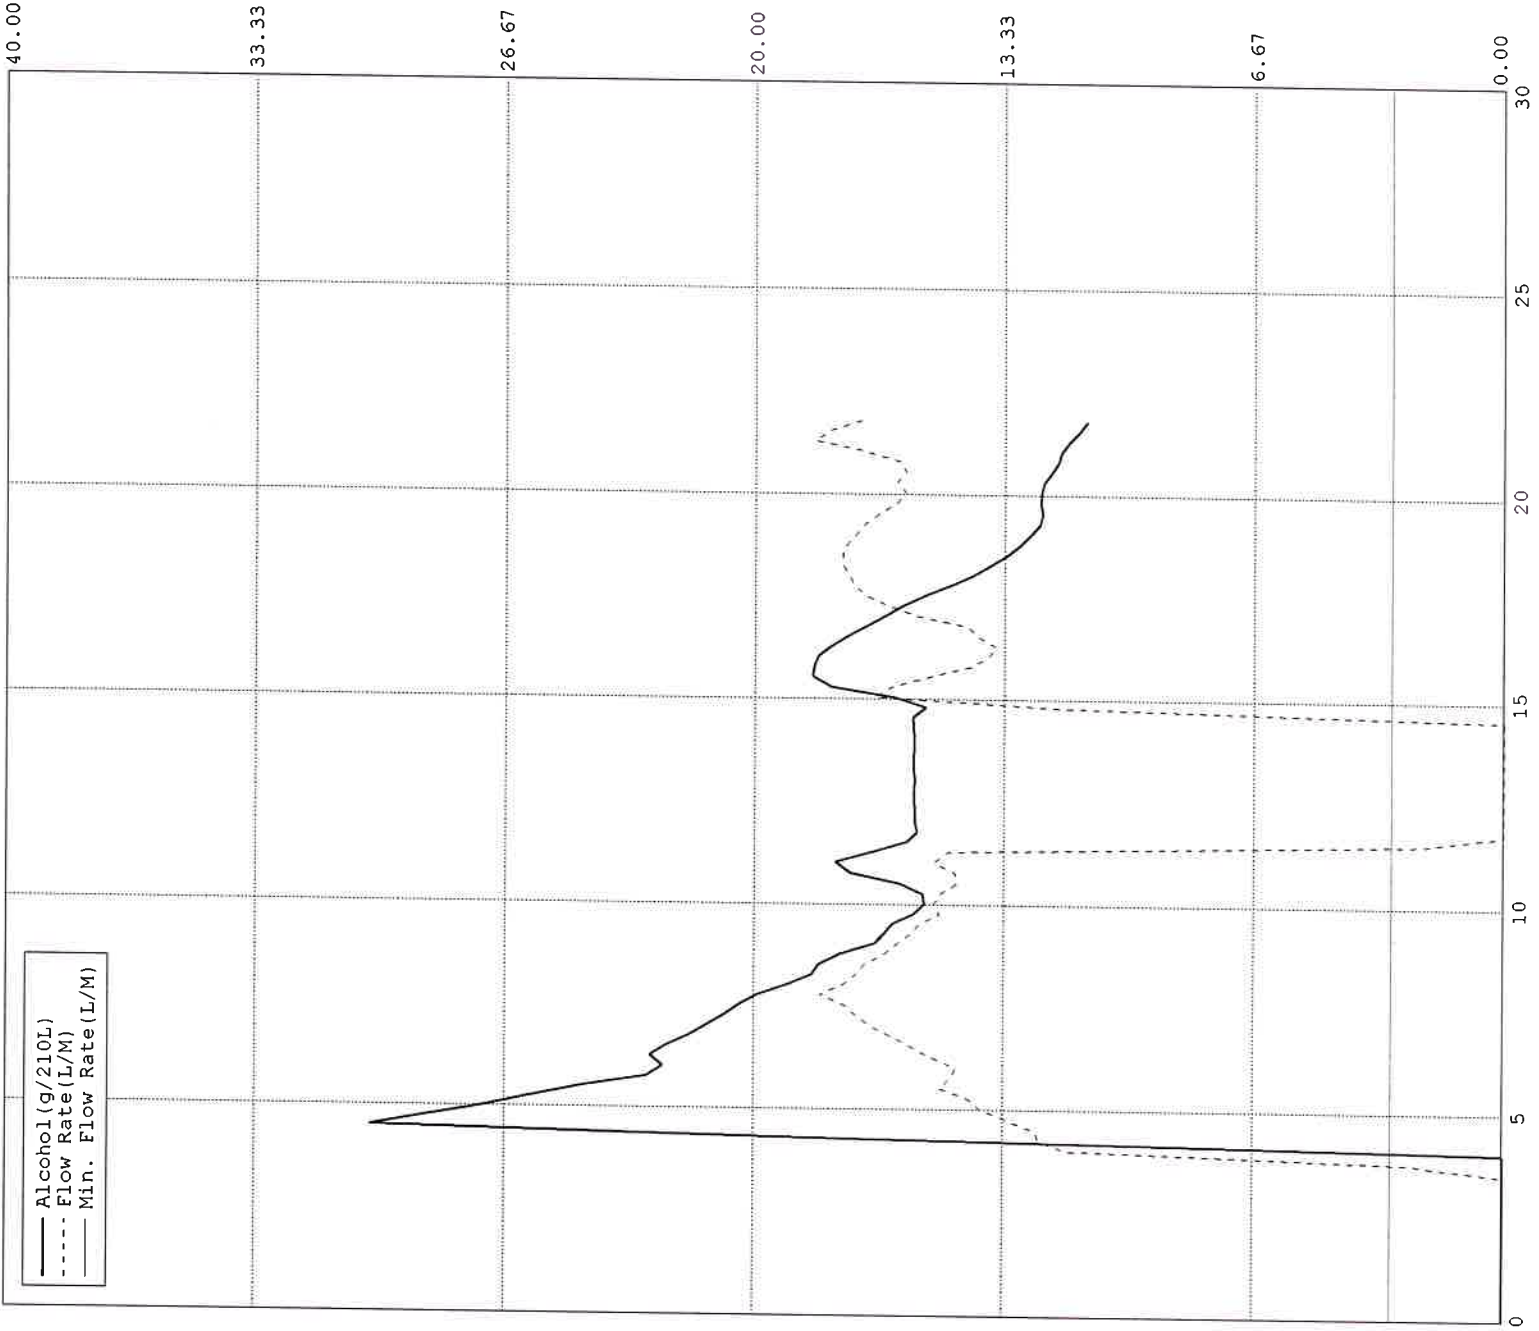

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100665

Date: 01/05/2023  
Time: 07:24:07

SUBJECT NAME:  
TEST TEST  
LICENSE #: MAX ATTEMPTS


OPERATOR NAME:  
COLLEEN S OBRYANT  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.25: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	07:25
BLANK TEST	0.000	07:25
INTERNAL STANDARD	VERIFIED	07:25
EXTERNAL STANDARD	0.076	07:25
BLANK TEST	0.000	07:26
SUBJECT SAMPLE	XXX	07:27

Maximum Attempts Exceeded

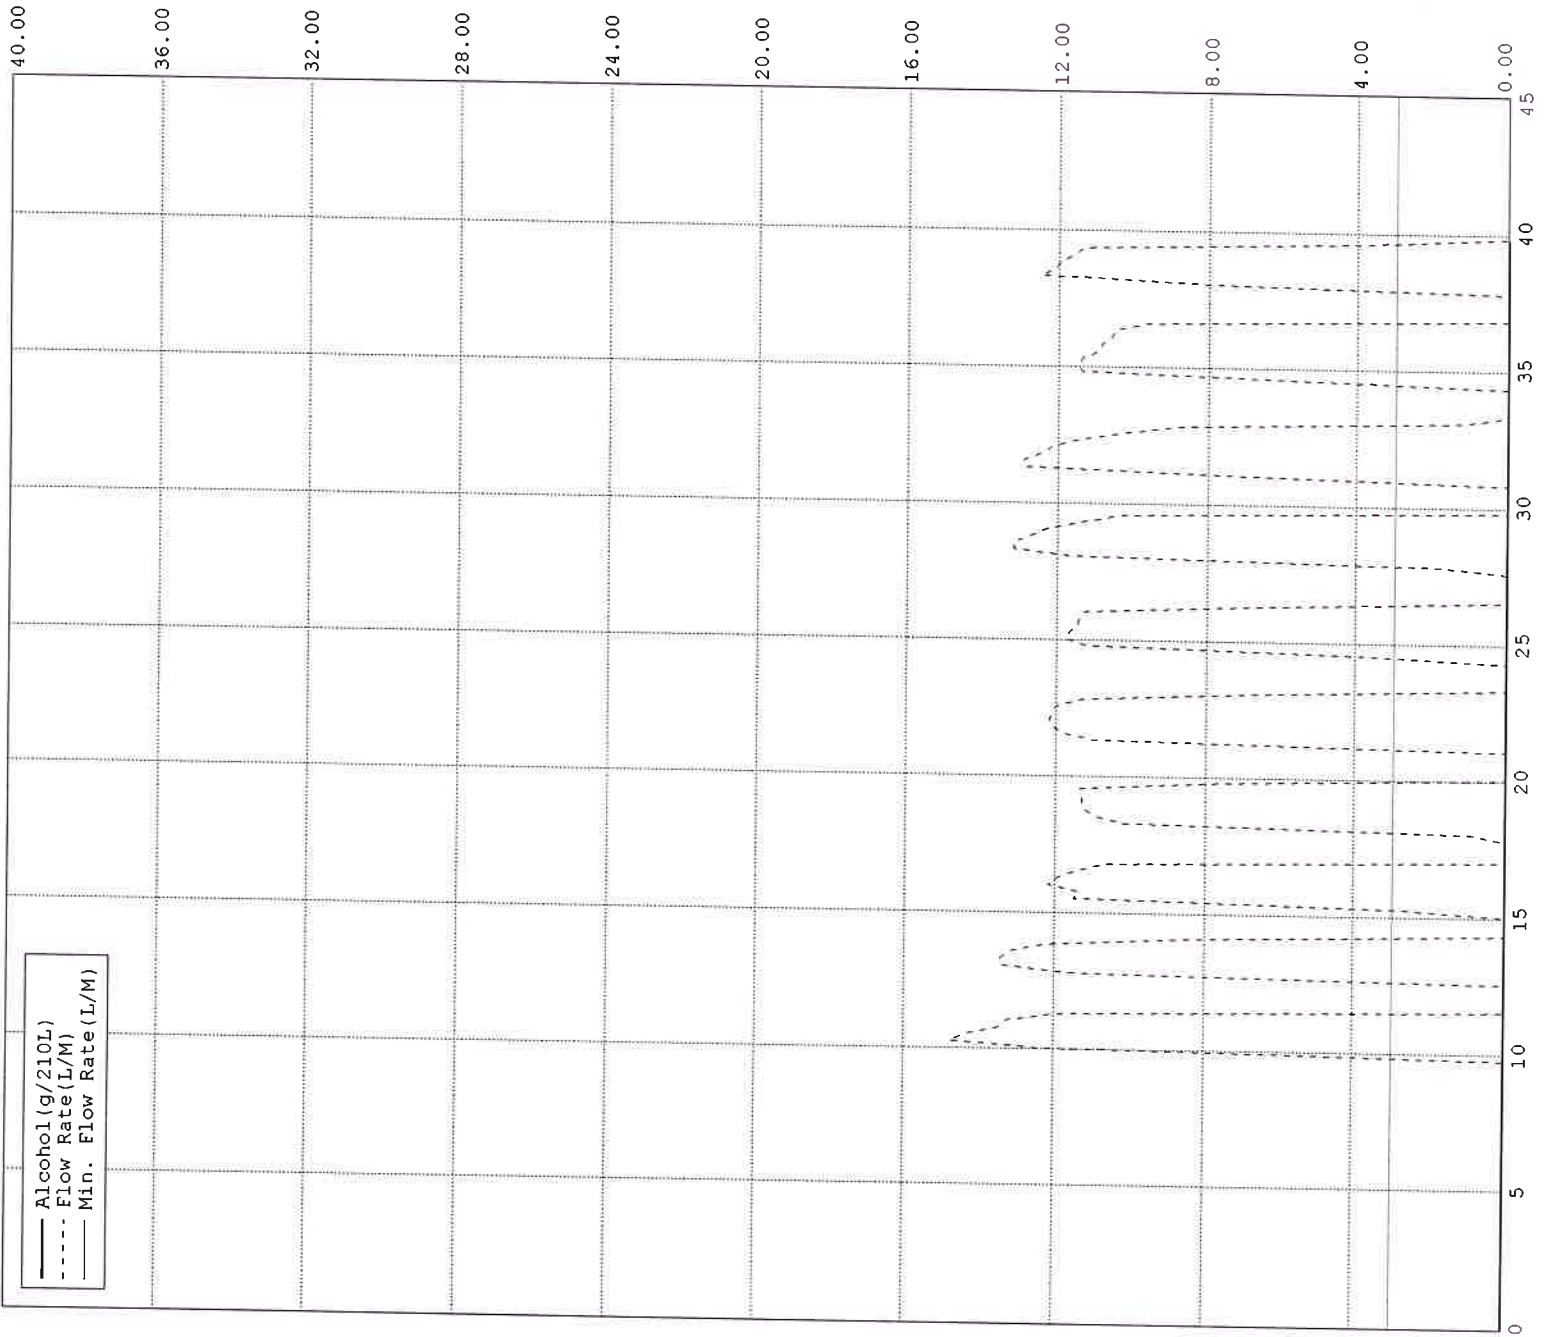



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100665

Date: 01/05/2023  
Time: 07:15:30

SUBJECT NAME:  
TEST TEST  
LICENSE #: RFI


OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAAI  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.25: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 07:19  
BLANK TEST 0.000 07:19  
INTERNAL STANDARD VERIFIED 07:20  
EXTERNAL STANDARD 0.076 07:20  
BLANK TEST 0.000 07:21

RFI DETECTED

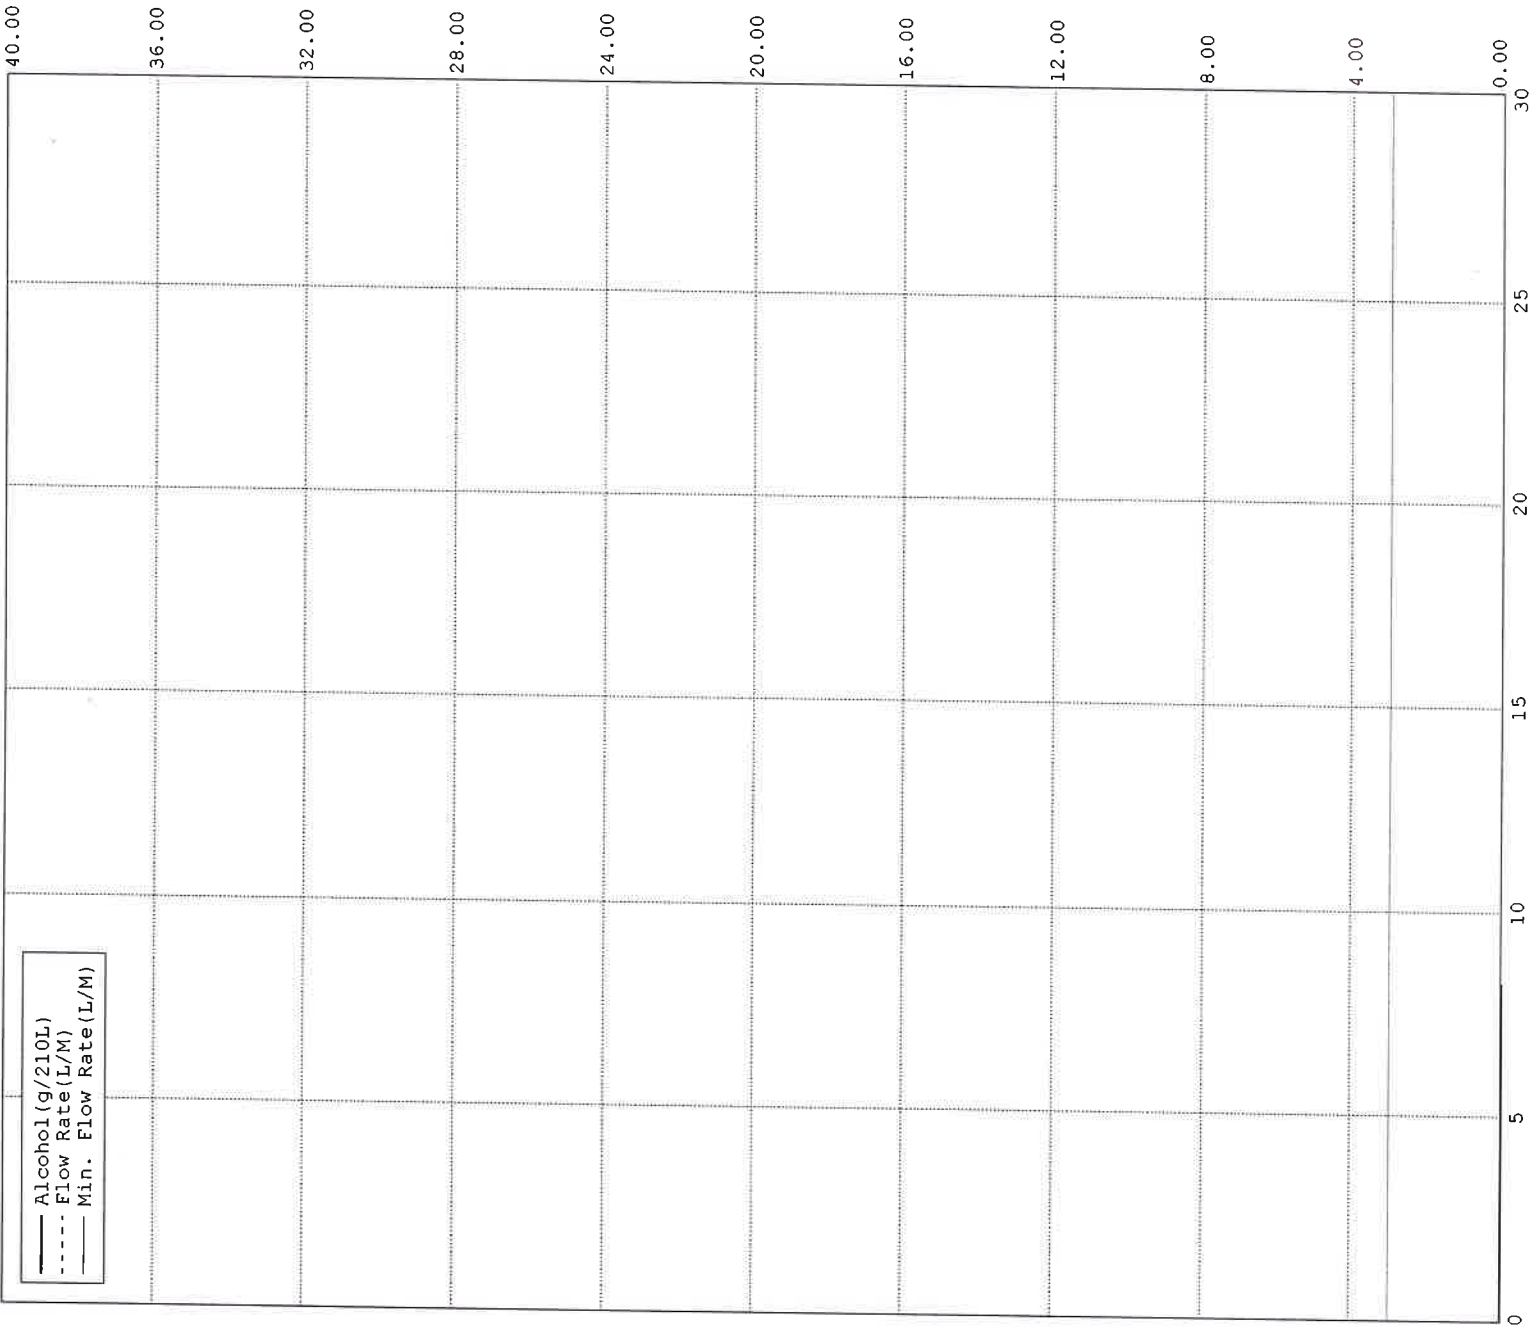

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100665

Date: 01/05/2023  
Time: 07:36:55

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-ACETONE

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237


DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.25: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 07:38  
BLANK TEST 0.000 07:38  
INTERNAL STANDARD VERIFIED 07:38  
Xg = 0.128 (0.48%)  
EXTERNAL STANDARD 0.076 07:39  
X[1] = 0.0760 (-0.0003) (0.0023)  
BLANK TEST 0.000 07:40  
SUBJECT SAMPLE XXX 07:40  
X[1] = 0.1049 (-0.0185) (0.0015)

Interference Detected

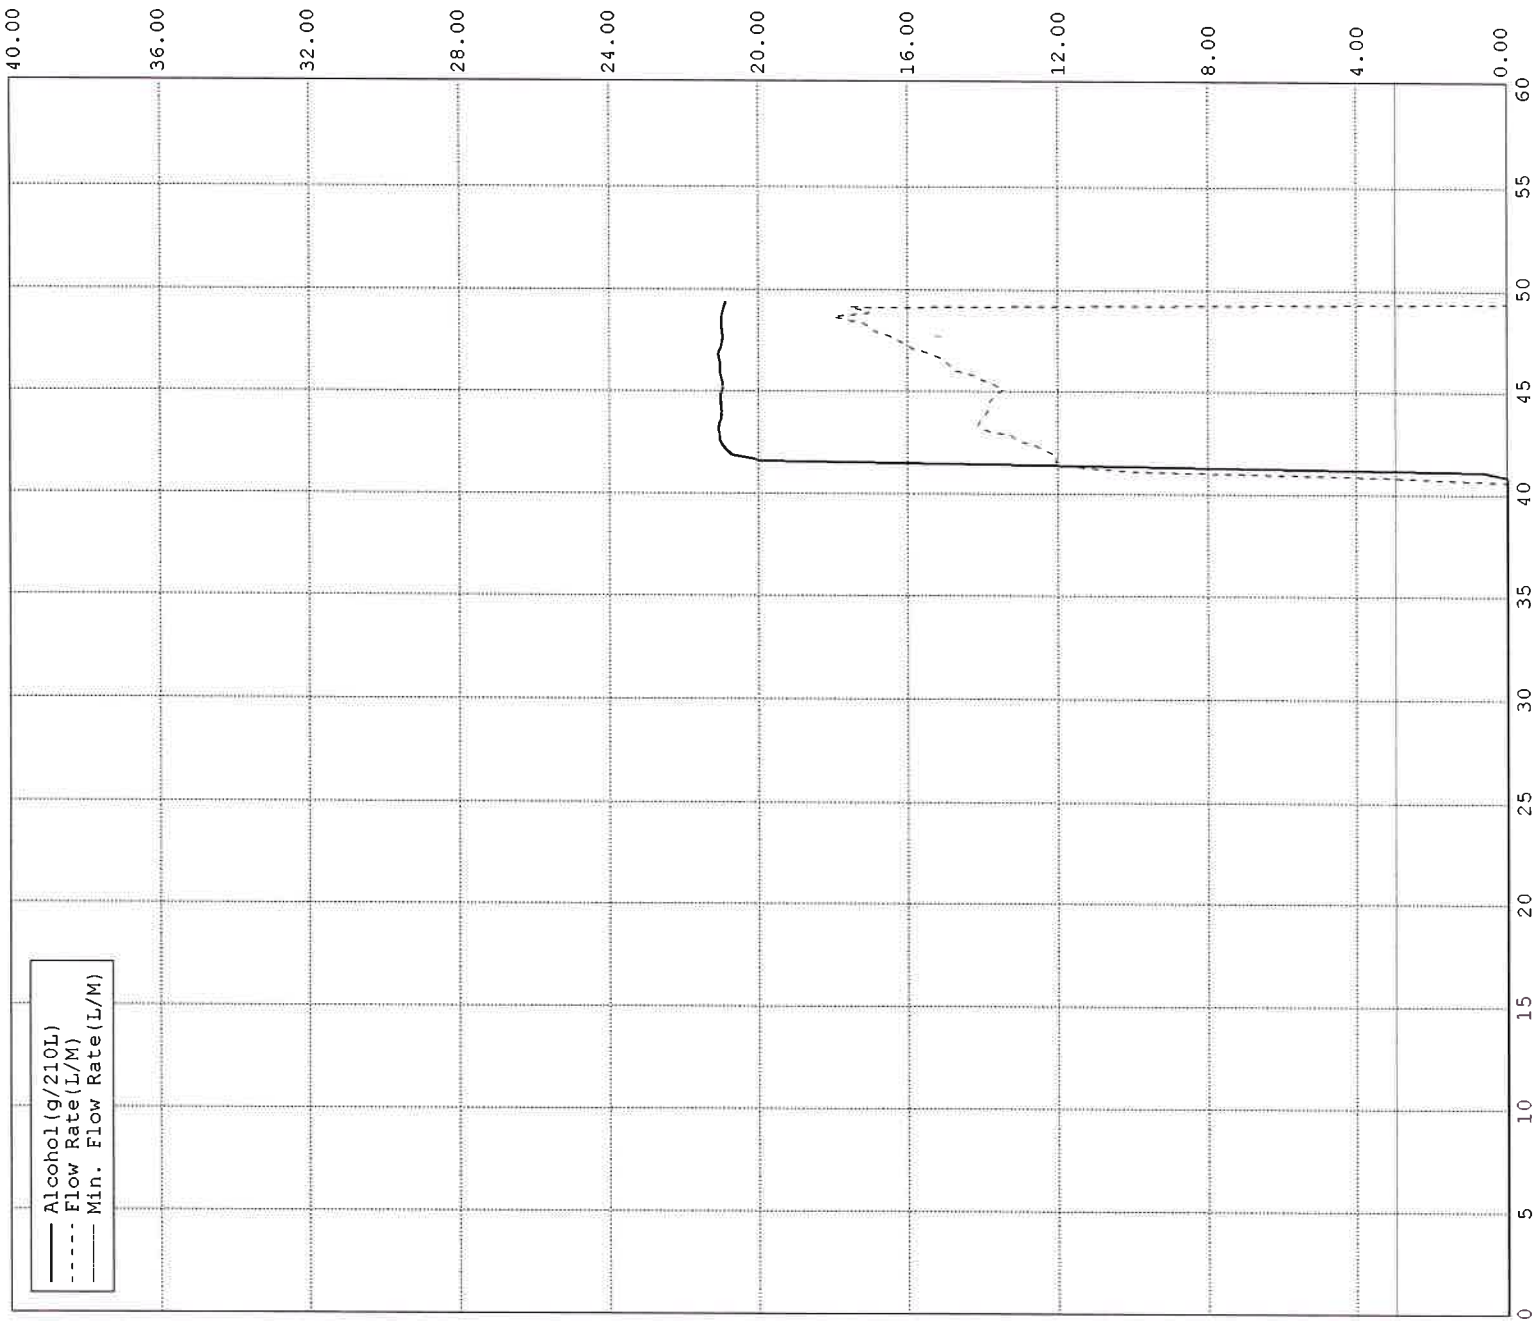

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100665

Date: 01/05/2023  
Time: 07:43:33

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-IPA


OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 23-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.25: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 07:44  
BLANK TEST 0.000 07:44  
INTERNAL STANDARD VERIFIED 07:45  
Xg = 0.128 (0.28%)  
EXTERNAL STANDARD 0.076 07:45  
X[1] = 0.0764 (-0.0001) (0.0030)  
BLANK TEST 0.000 07:46  
SUBJECT SAMPLE XXX 07:47  
X[1] = 0.1110 (-0.0260) (0.0016)

Interference Detected

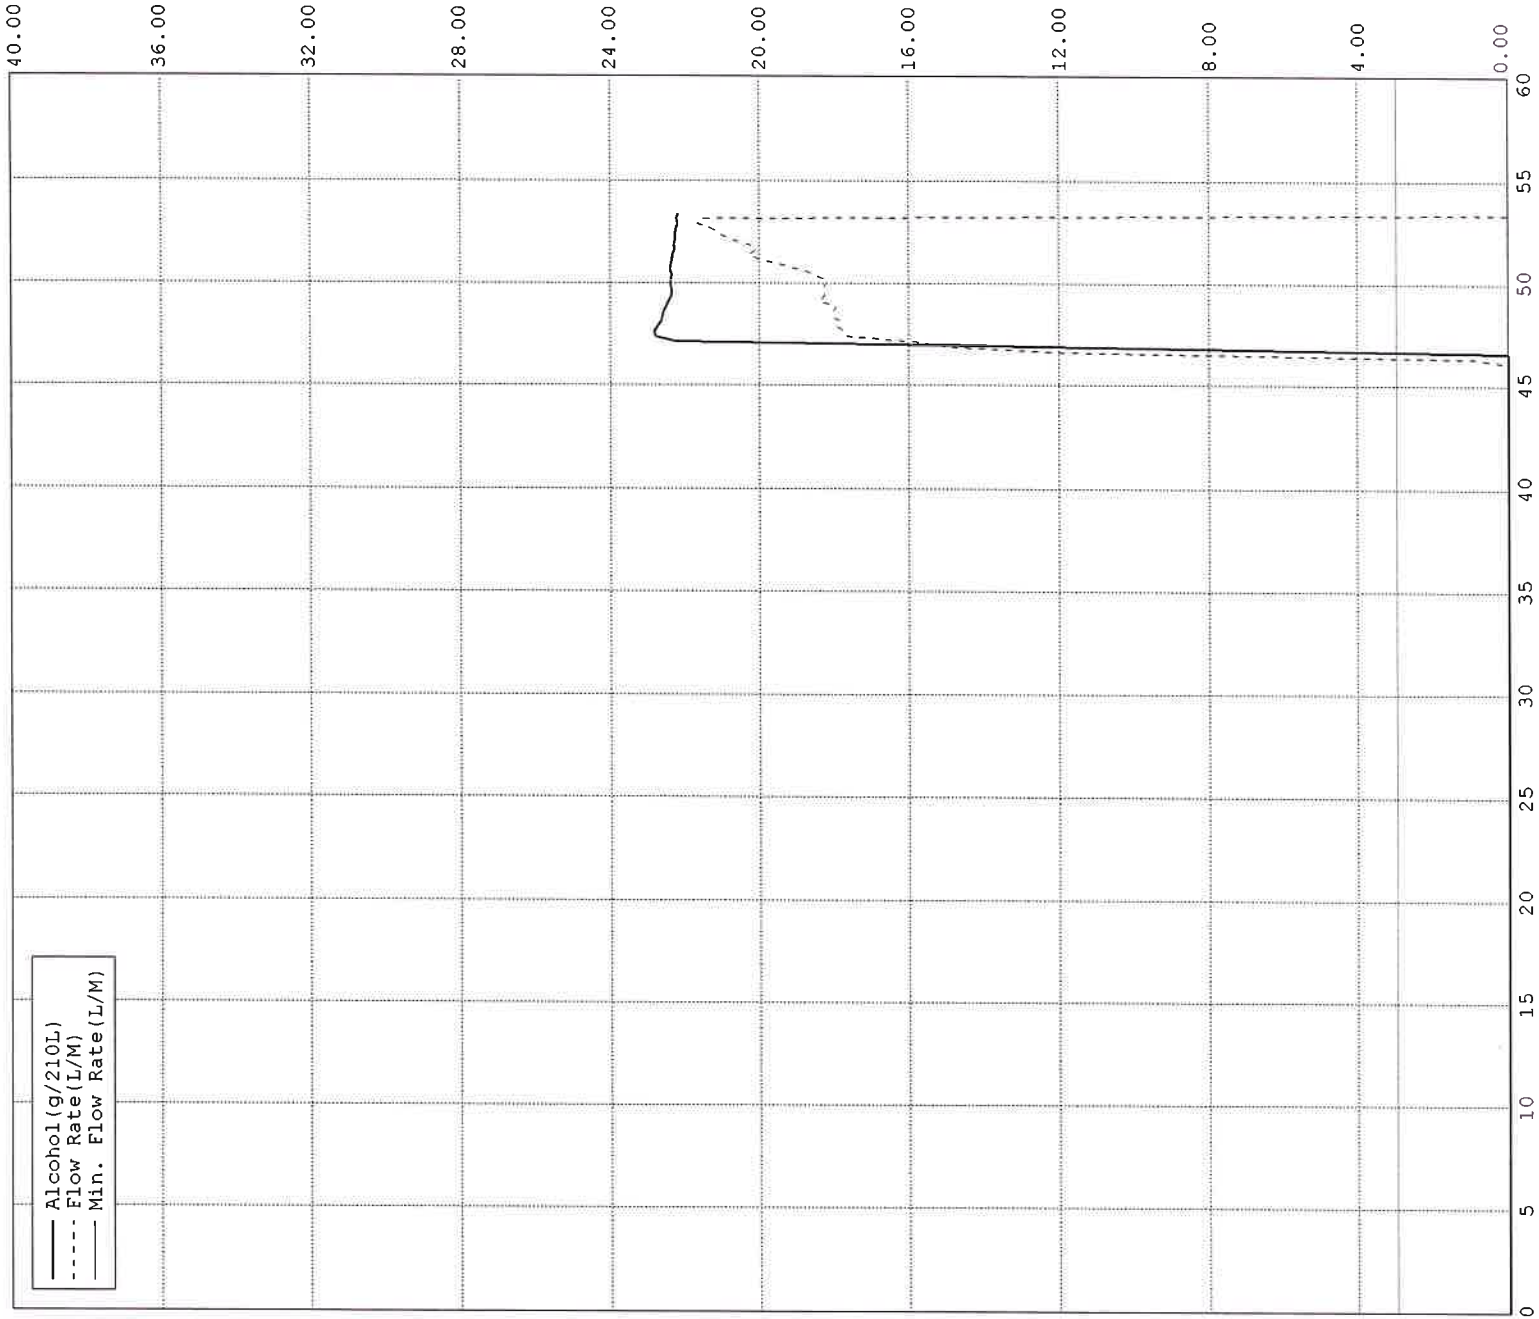

**SUBJECT TEST**

Alaska Department of Public Safety  
 DATAMASTER dmt: 100665

Date: 01/05/2023  
 Time: 07:49:41

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: INT-NEGATIVE


OPERATOR NAME:  
 COLLEEN S O'BRYAN  
 OPERATOR'S #: 6237

DEPT/AGENCY:  
 AAA1  
 CASE/REPORT: 23-1234  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.26: 0.078  
 LOT #: AG135004  
 EXPIRATION: 12/16/2023

TEST TYPE	RESULT	STATUS	TIME
DIAGNOSTIC CHECK	PASSED		07:50
BLANK TEST	0.000		07:50
INTERNAL STANDARD	VERIFIED		07:51
Xg = 0.129 (0.21%)	0.076		07:51
EXTERNAL STANDARD	X[1] = 0.0758 (-0.0003)	(0.0028)	
BLANK TEST	0.000		07:52
SUBJECT SAMPLE (Vol=2.02L)	0.093		07:53
X[1] = 0.0934 (-0.0012)	(0.0008)		
BLANK TEST	0.000		07:54
EXTERNAL STANDARD	0.076		07:54
X[1] = 0.0760 (-0.0001)	(0.0022)		
BLANK TEST	0.000		07:55

Filter 2 Average = -0.0002  
 Filter 3 Average = 0.0026

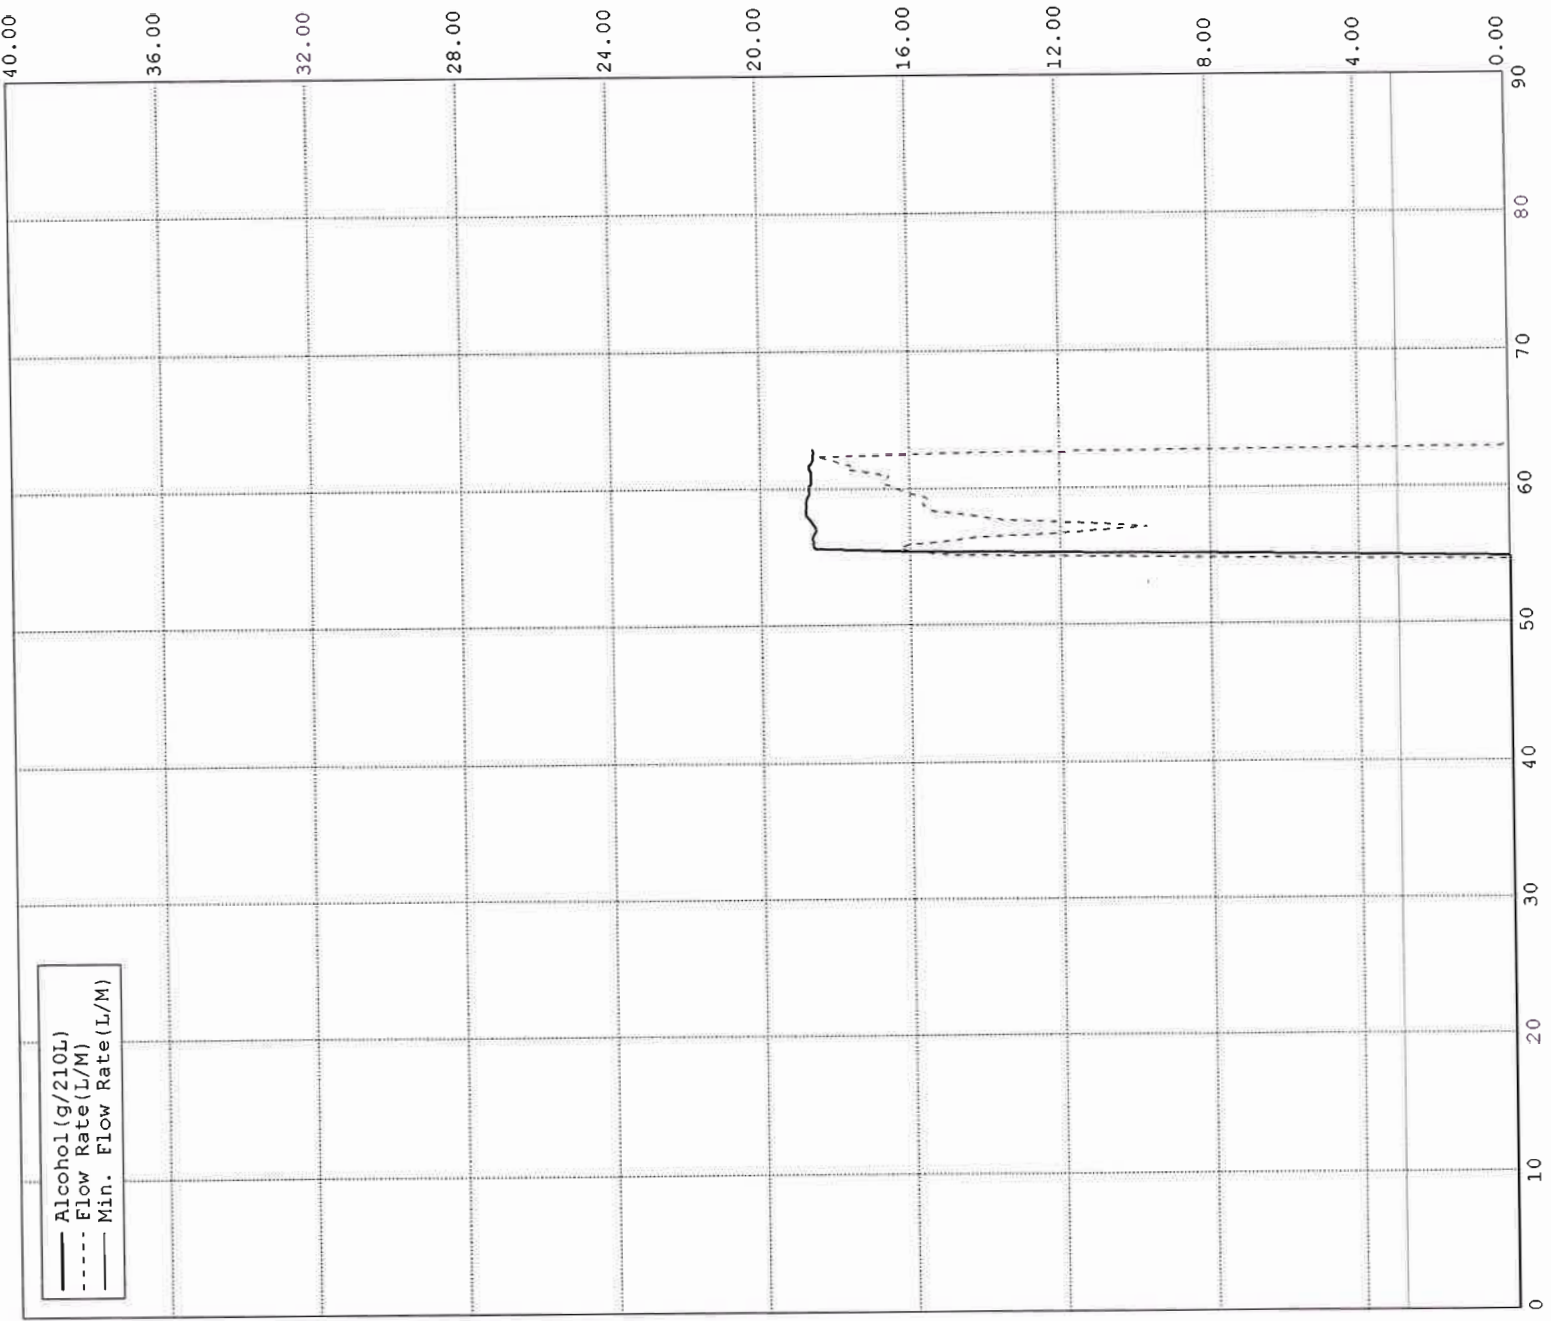

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100665

Date: 01/05/2023

Time: 08:07:52

SUBJECT NAME:

TEST TEST

LICENSE #: NON-DRINKING

OPERATOR NAME:

COLLEEN S OBRYANT

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 23-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.26: 0.078

LOT #: AG135004

EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	08:09
BLANK TEST	0.000	08:09
INTERNAL STANDARD	VERIFIED	08:09
EXTERNAL STANDARD	0.076	08:09
BLANK TEST	0.000	08:10
SUBJECT SAMPLE (Vol=1.63L)	0.000	08:11
BLANK TEST	0.000	08:12
EXTERNAL STANDARD	0.077	08:12
BLANK TEST	0.000	08:13

