




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100412

Report Issue Date: 10/06/2025
Date Received: 2025-08-13
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.019	0.020	0.021	0.020
0.080	0.079	AG335202	0.077	0.077	0.077	0.077	0.077	0.077
0.300	0.298	AG427706	0.294	0.293	0.293	0.292	0.294	0.293

As Found - Evaluation Analyst: Carlie Glaister

As Found Conditions - Barometric Pressure (inHg): 29.73 Barometer Used: VWR S/N 240680771 Temperature (C): 24.3 Relative Humidity (%): 35

As-Found Lab Activity Date Range: 08/13/2025 - 08/14/2025

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG408002	0.019	0.020	0.020	0.020	0.019	0.020	+/- 0.002
0.040	0.039	AG407908	0.038	0.039	0.038	0.038	0.038	0.038	+/- 0.003
0.080	0.078	AG335202	0.075	0.076	0.075	0.075	0.076	0.075	+/- 0.004
0.100	0.097	AG333401	0.096	0.097	0.097	0.098	0.097	0.097	+/- 0.004
0.150	0.146	AG515604	0.143	0.143	0.143	0.143	0.143	0.143	+/- 0.006
0.300	0.292	AG427706	0.288	0.287	0.287	0.287	0.289	0.288	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.14 Barometer Used: VWR S/N 240680771 Temperature (C): 22.3 Relative Humidity (%): 40

As-Left Lab Activity Date Range: 09/22/2025 - 09/23/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Kaija Swisher on 10/06/2025

kaija.swisher@alaska.gov

Technically and administratively reviewed by Derek Walton on 10/06/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100412 Analyst or Technician Name: Kaija Shisher

DataMaster DMT Calibration Start Date: 9/22/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 9/10/26
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5L liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.14 Temperature(C) 22.3 Relative Humidity(%) 40

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) - *Print with View Details*
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20250922KS Expiration Date: 12/22/25

Simulator S/N: DR4178 Thermometer Verification Performed? ☒

2. Isopropanol Reagent Lot Number: 20250922KS Expiration Date: 12/22/25

Simulator S/N: DR4177 Thermometer Verification Performed? ☒

3. Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 12/22/25

Simulator S/N: DR4163 Thermometer Verification Performed? ☒

3/19/27 KS 10/6/25
(solution)

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 3/14/27 250159297 KS 10/6/25

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 9/22/25

Data Interpretation Date (Technician): NX (if applicable)

Data Interpretation Date (Analyst): 9/23/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100412

Date: 09/22/2025
Time: 09:33:02

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C (44.0°C - 52.0°C)	PASSED
Breath Tube = 45.2°C (38.0°C - 50.0°C)	PASSED

SETTINGS

Lamp Voltage = 1.70 V (1.02 V - 2.38 V)	PASSED
Cooler Voltage = 1.66 V (1.03 V - 2.39 V)	PASSED
Bias Voltage = 80 V (48 V - 112 V)	PASSED
Chopper Freq = 516 Hz (475 Hz - 575 Hz)	PASSED
Barometer = 29.1 in	

PUMP INFO

Flow Rate = 4.704 L/M (3.500 L/M - 6.500 L/M)	PASSED
--	--------

DETECTOR INFO

PUMP ON (0.003 V <= 0.010 V)	PASSED
PUMP OFF (0.003 V <= 0.010 V)	PASSED

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
Xq = 0.088 2.02% (0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100412

Date: 09/22/2025

Time: 10:31 AM

Temperatures (°C)

Sample Cell: 48.8°C

Breath Tube: 46.3°C

Current Barometer 29.1 in

Volume (Ltr) 1.47

Settings

Lamp: 1.76 V

Bias: 80 V

Cooler: 1.61 V

Chopper: 521 Hz

Voltages (V)

Flow: 1.04 V

Detector: 0.018 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100412

Date: 05/19/2021
Time: 11:49:16

OPERATOR NAME:
CARLIE BAILEY
CERTIFICATE #: 10436

Ca	=	0.1000		
CAL	=	0.957572	0.800	<= CAL < 1.200
b1	=	0.0010	0.0000	<= b1 < 0.0040
b2	=	0.0054	0.0010	<= b2 < 0.0100
b3	=	0.0004	0.0000	<= b3 < 0.0040
Xq	=	0.0862	0.0500	<= Xq < 0.2000
a21	=	1.162237	1.050	<= a21 < 1.300
a31	=	0.556113	0.300	<= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100412

Date: 09/22/2025
Time: 10:57:33

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.14: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:58
BLANK TEST	0.000	10:58
INTERNAL STANDARD	VERIFIED	10:58
EXTERNAL STANDARD	0.075	10:59
BLANK TEST	0.000	11:00
SUBJECT SAMPLE (Vol=1.54L)	0.000	11:00
BLANK TEST	0.000	11:01
EXTERNAL STANDARD	0.076	11:02
BLANK TEST	0.000	11:02

KS

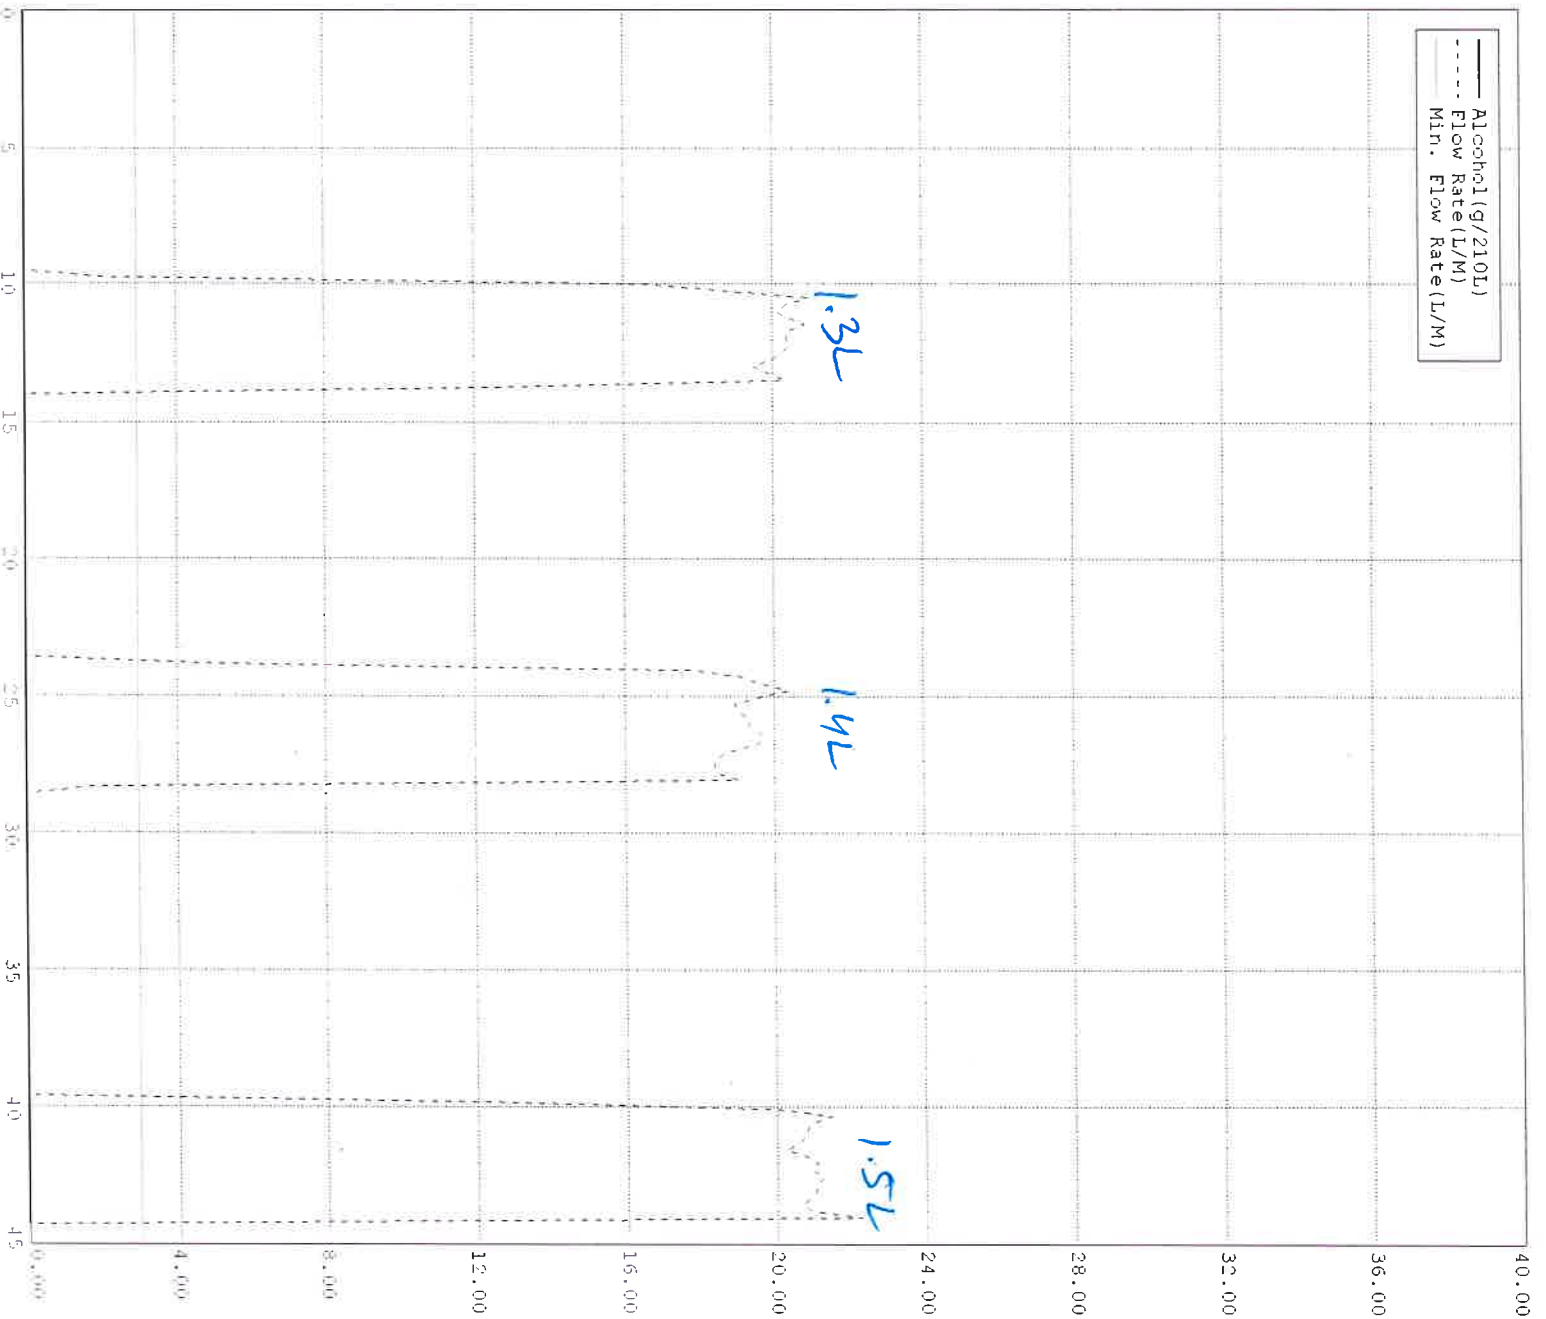


LINEARITY CHECK

Alaska Department of Public Safety
DATAMASTER dmt: 100412

Date: 09/22/2025
Time: 11:06:04

SUPERVISOR NAME:
KALUA SWISHER
OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.019	0.0196	0.0005
0.039	0.0382	0.0004
0.078	0.0754	0.0005
0.097	0.0970	0.0007
0.146	0.1430	0.0000
0.292	0.2876	0.0009
SLOPE	= 0.983549	
R ²	= 0.999883	

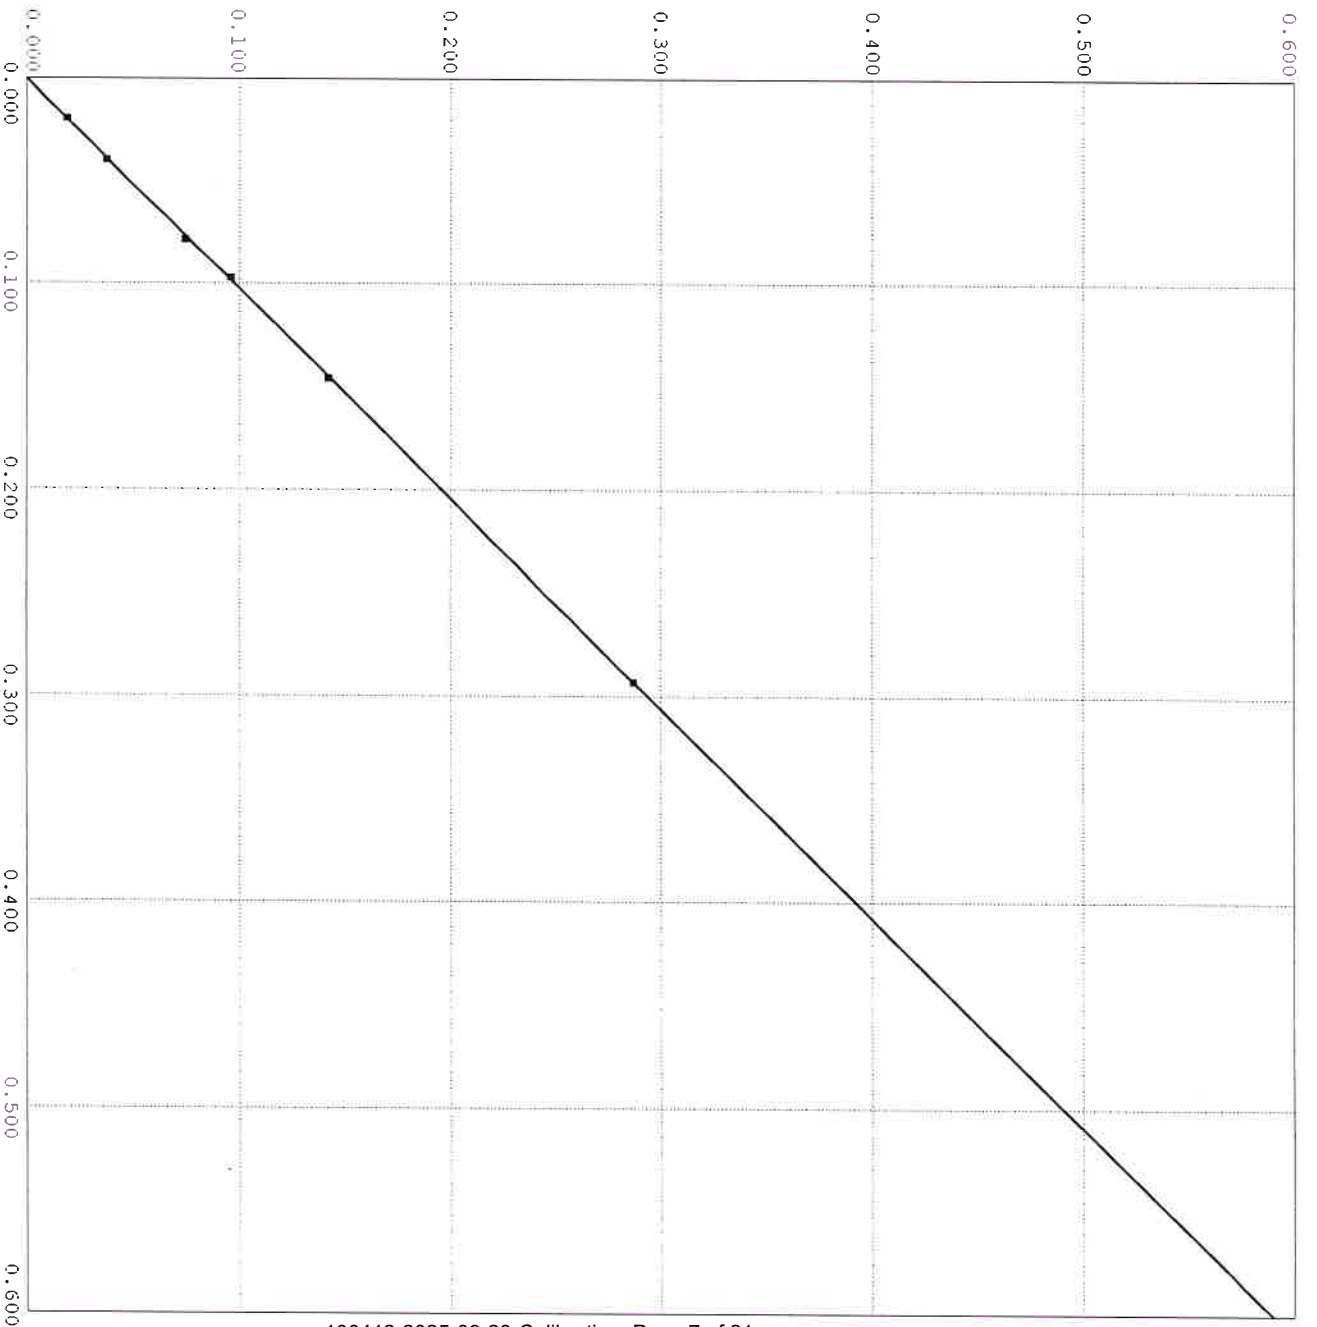

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100412






Date: 09/22/2025
Time: 11:06:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.14: 0.019
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 1028 psi

BLANK TEST	0.000	11:07
INTERNAL STANDARD	VERIFIED	11:07
EXTERNAL STANDARD	0.019	11:07
BLANK TEST	0.000	11:08
EXTERNAL STANDARD	0.020	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.020	11:09
BLANK TEST	0.000	11:10
EXTERNAL STANDARD	0.020	11:10
BLANK TEST	0.000	11:11
EXTERNAL STANDARD	0.019	11:12
BLANK TEST	0.000	11:12

Average = 0.0196
Std Dev = 0.0005

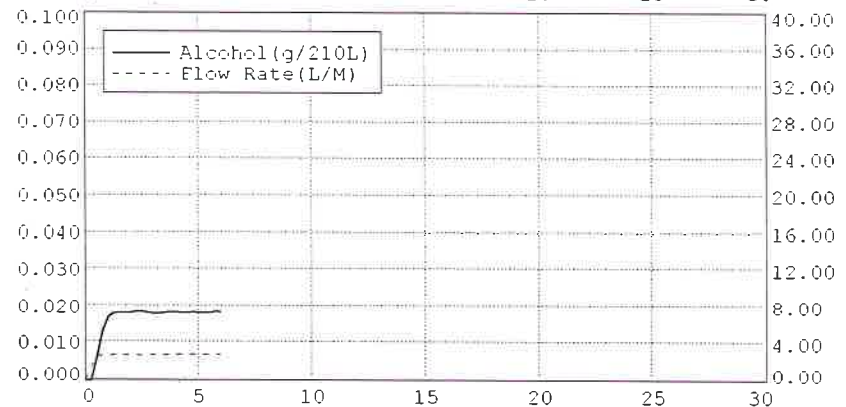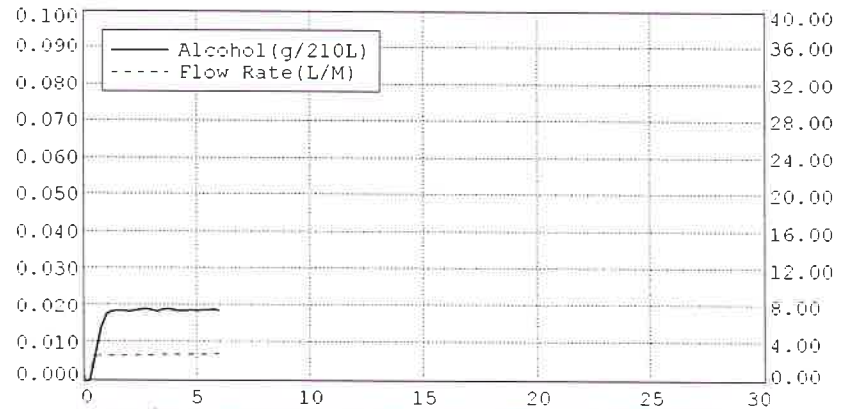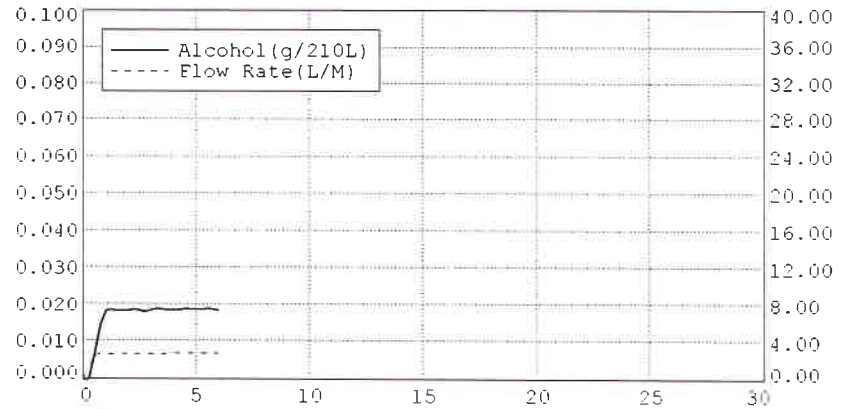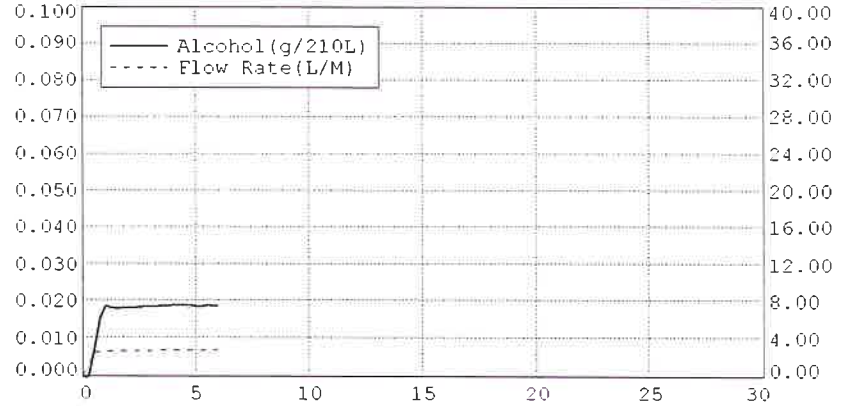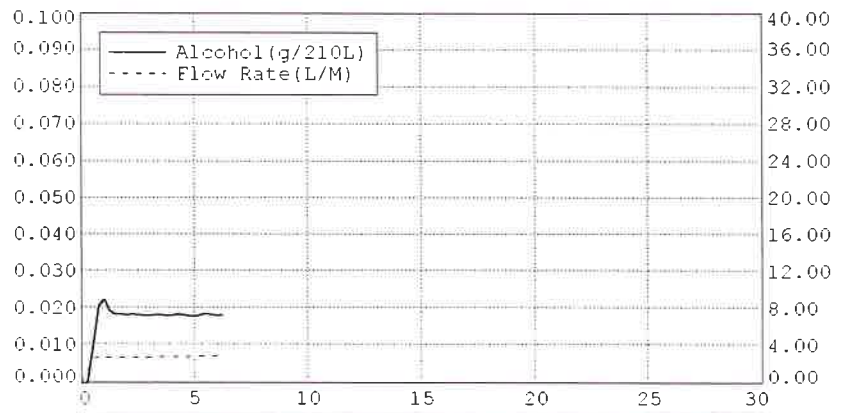

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100412






Date: 09/22/2025
Time: 11:14:28

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.14: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 674 psi

Test Type	Value	Time
BLANK TEST	0.000	11:15
INTERNAL STANDARD	VERIFIED	11:16
EXTERNAL STANDARD	0.038	11:16
BLANK TEST	0.000	11:17
EXTERNAL STANDARD	0.039	11:17
BLANK TEST	0.000	11:18
EXTERNAL STANDARD	0.038	11:18
BLANK TEST	0.000	11:19
EXTERNAL STANDARD	0.038	11:19
BLANK TEST	0.000	11:20
EXTERNAL STANDARD	0.038	11:20
BLANK TEST	0.000	11:21

Average = 0.0382
Std Dev = 0.0004

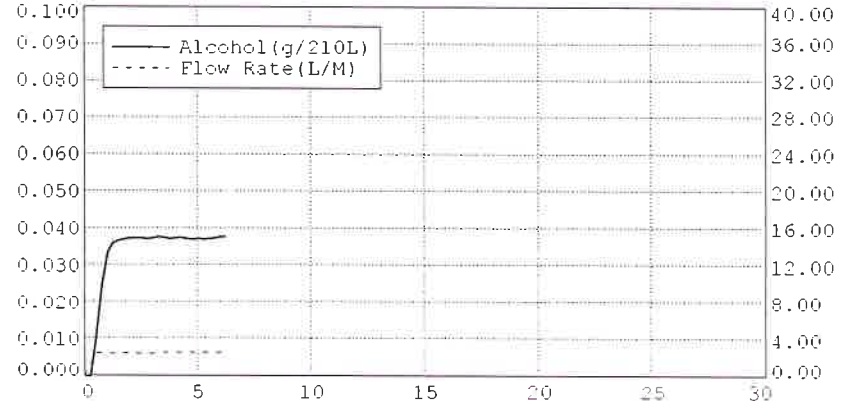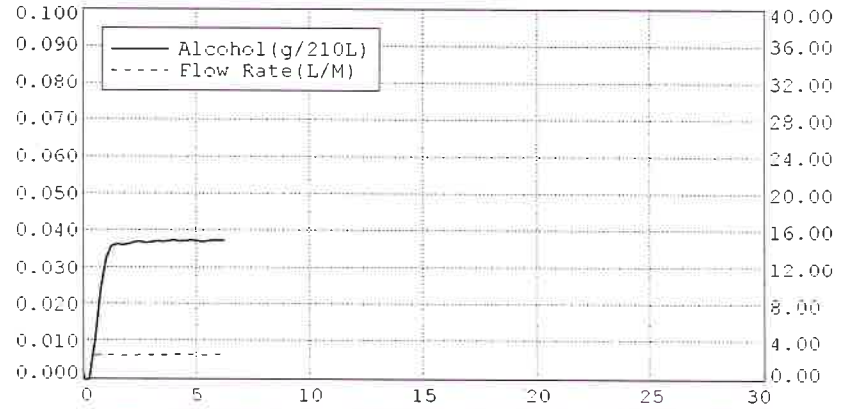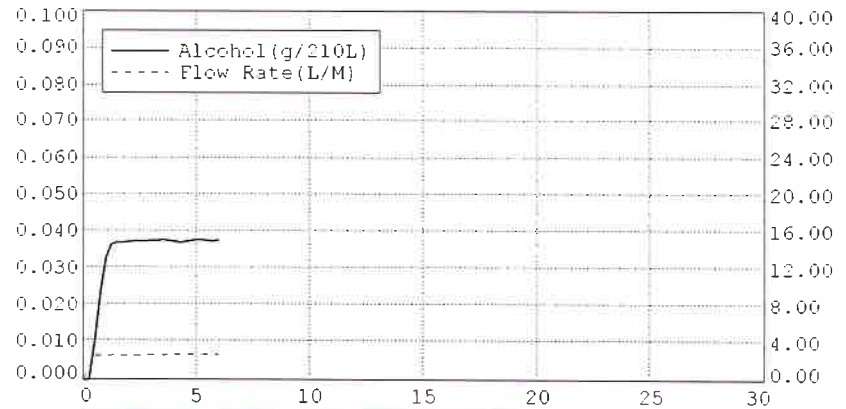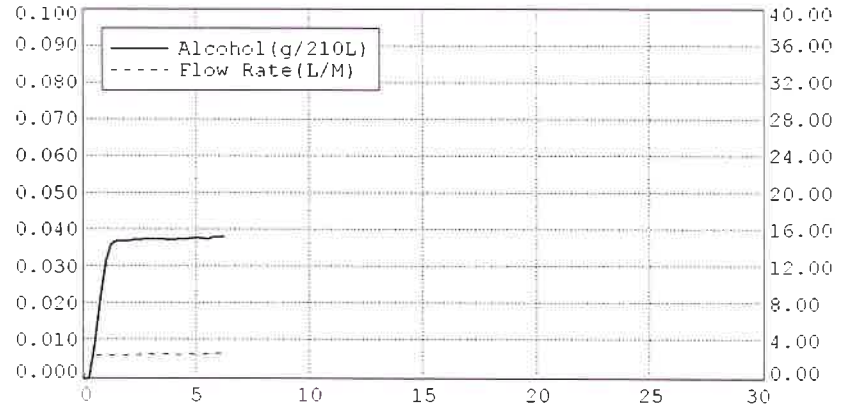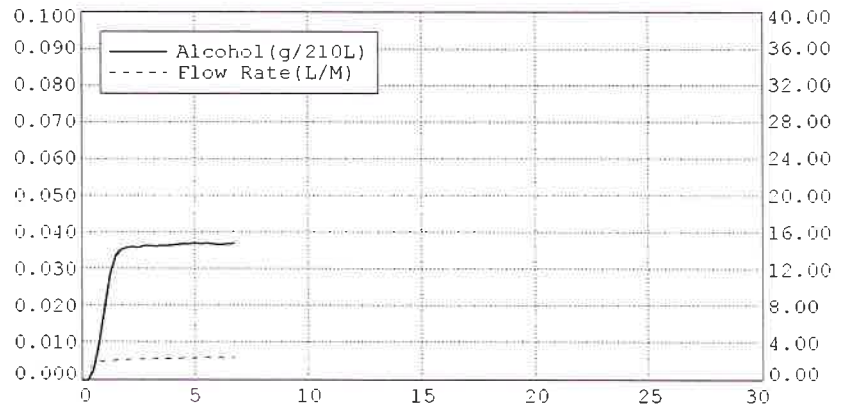

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100412






Date: 09/22/2025
Time: 11:23:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.14: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 182 psi

BLANK TEST	0.000	11:24
INTERNAL STANDARD	VERIFIED	11:25
EXTERNAL STANDARD	0.075	11:25
BLANK TEST	0.000	11:26
EXTERNAL STANDARD	0.076	11:26
BLANK TEST	0.000	11:27
EXTERNAL STANDARD	0.075	11:27
BLANK TEST	0.000	11:28
EXTERNAL STANDARD	0.075	11:28
BLANK TEST	0.000	11:29
EXTERNAL STANDARD	0.076	11:29
BLANK TEST	0.000	11:30

Average = 0.0754
Std Dev = 0.0005

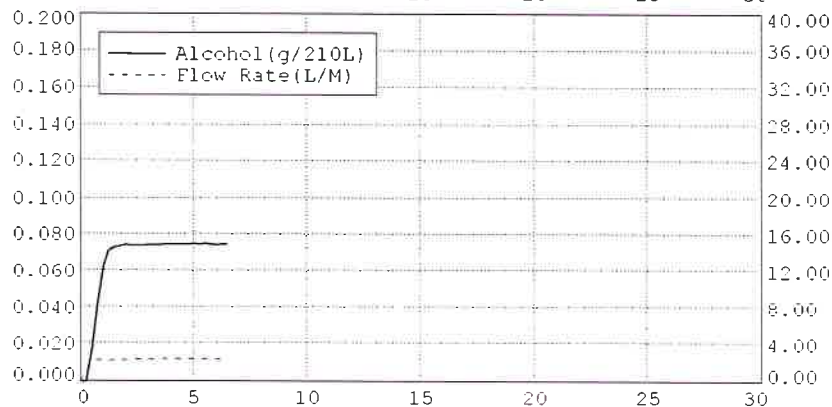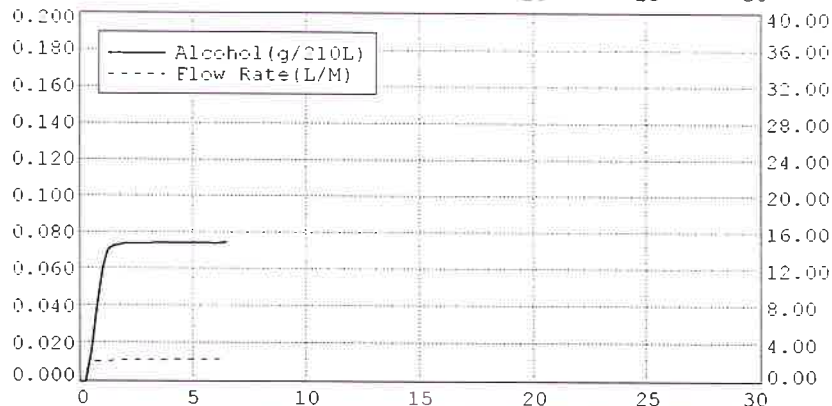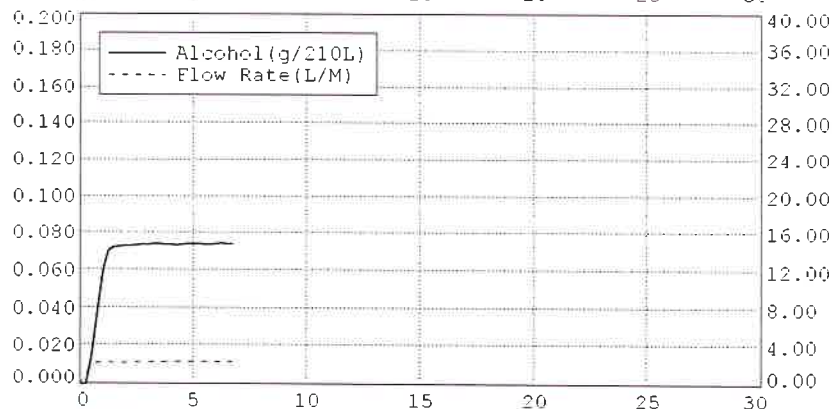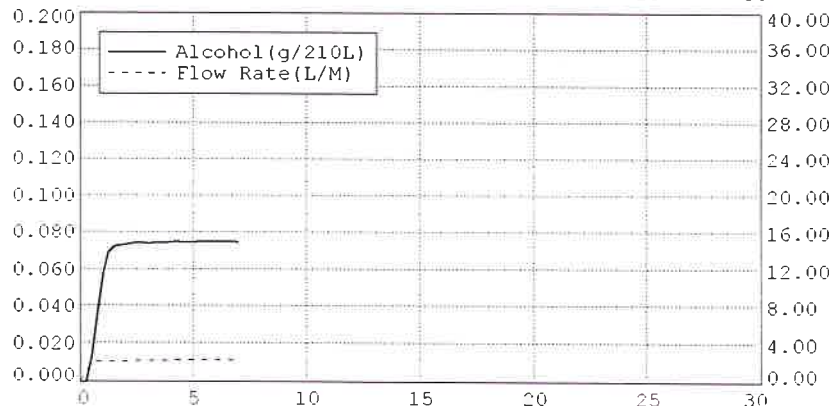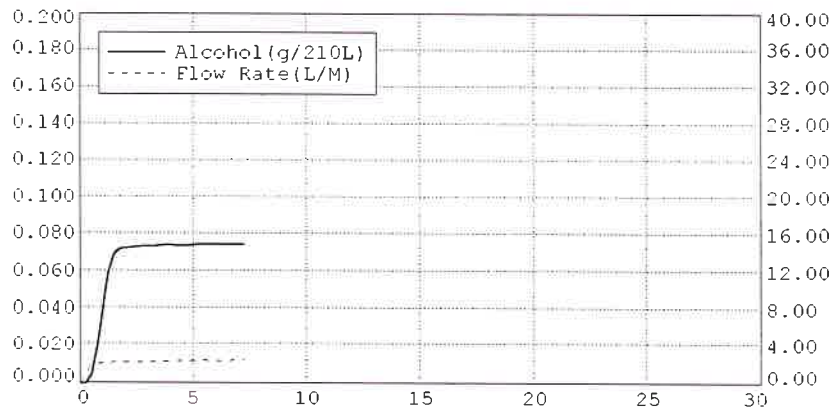

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100412






Date: 09/22/2025
Time: 11:32:04

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.14: 0.097
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 847 psi

BLANK TEST	0.000	11:33
INTERNAL STANDARD	VERIFIED	11:33
EXTERNAL STANDARD	0.096	11:33
BLANK TEST	0.000	11:34
EXTERNAL STANDARD	0.097	11:34
BLANK TEST	0.000	11:35
EXTERNAL STANDARD	0.097	11:36
BLANK TEST	0.000	11:36
EXTERNAL STANDARD	0.098	11:37
BLANK TEST	0.000	11:38
EXTERNAL STANDARD	0.097	11:38
BLANK TEST	0.000	11:39

Average = 0.0970
Std Dev = 0.0007

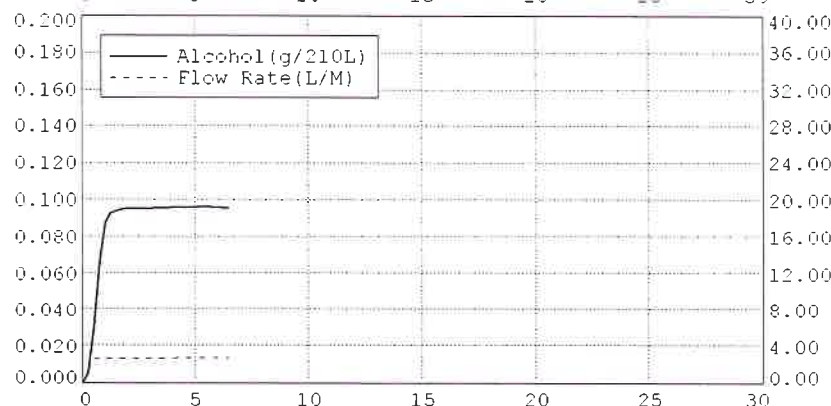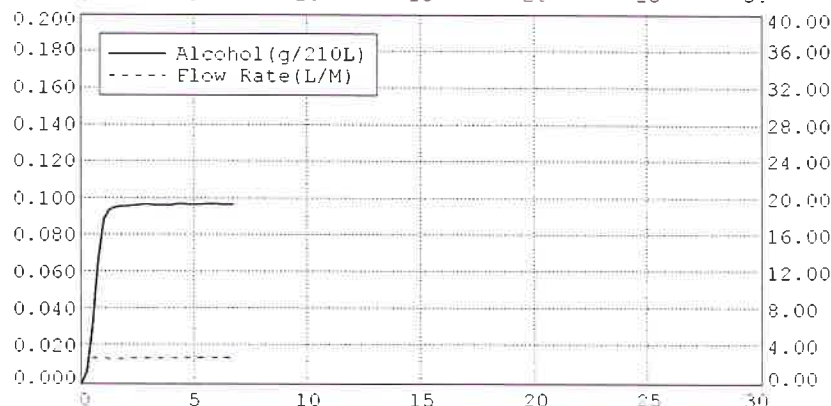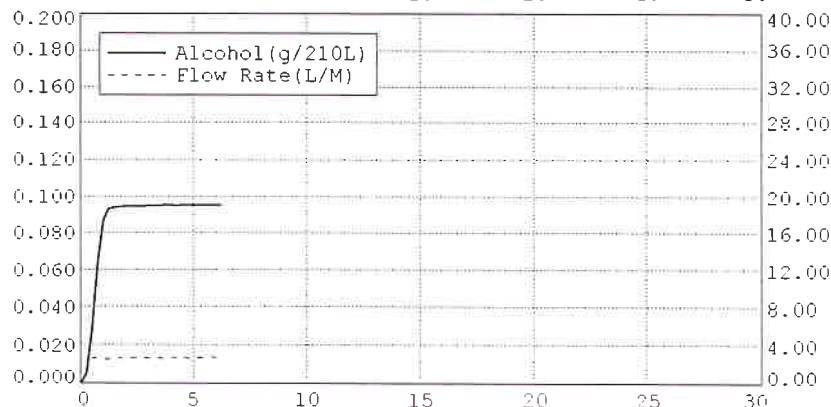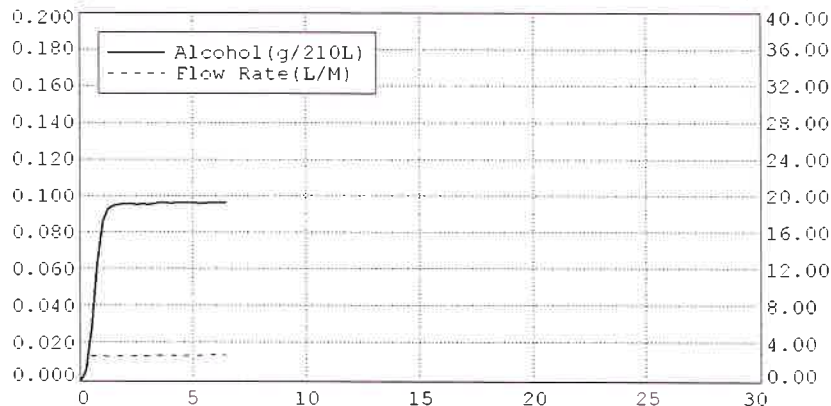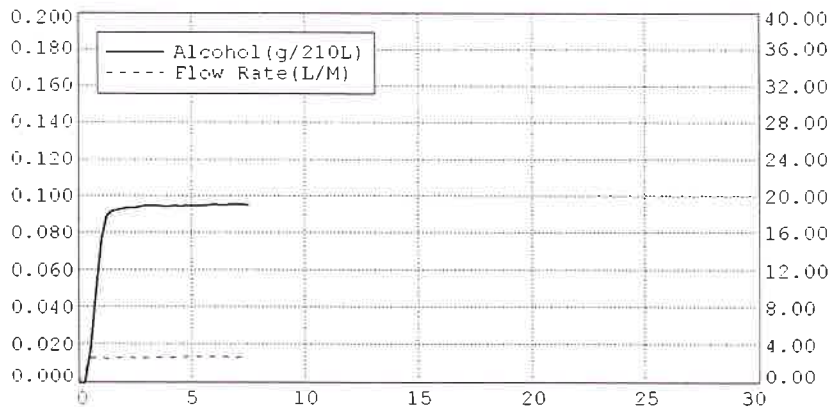

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100412






Date: 09/22/2025
Time: 11:42:15

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.14: 0.146
LOT #: AG515604
EXPIRATION: 06/05/2027
TANK PRESSURE: 773 psi

BLANK TEST	0.000	11:43
INTERNAL STANDARD	VERIFIED	11:43
EXTERNAL STANDARD	0.143	11:43
BLANK TEST	0.000	11:44
EXTERNAL STANDARD	0.143	11:45
BLANK TEST	0.000	11:45
EXTERNAL STANDARD	0.143	11:46
BLANK TEST	0.000	11:47
EXTERNAL STANDARD	0.143	11:47
BLANK TEST	0.000	11:48
EXTERNAL STANDARD	0.143	11:48
BLANK TEST	0.000	11:49

Average = 0.1430
Std Dev = 0.0000

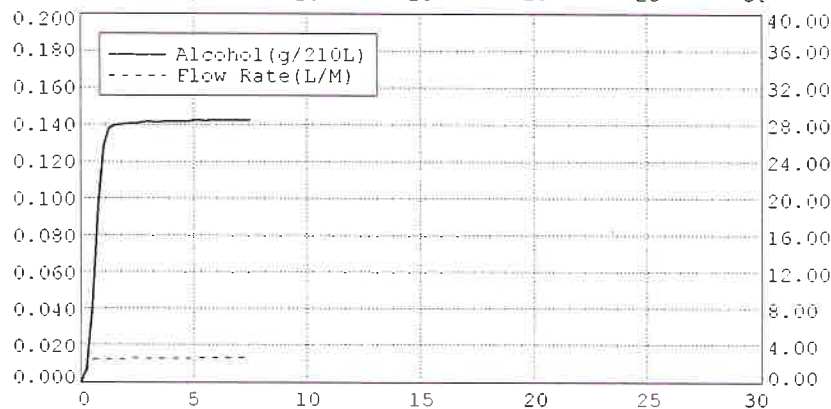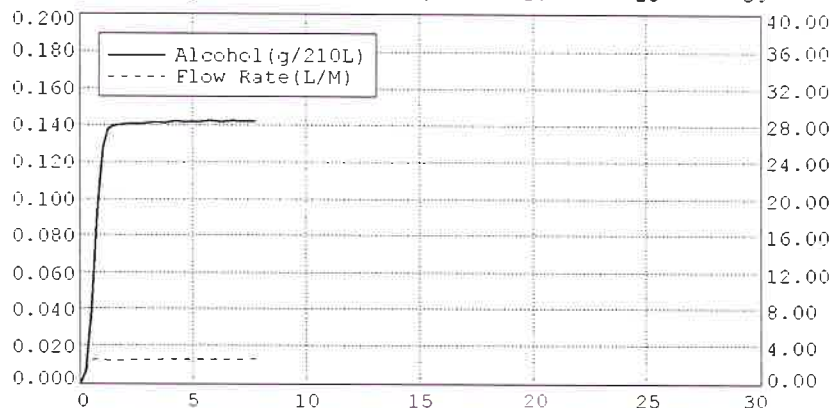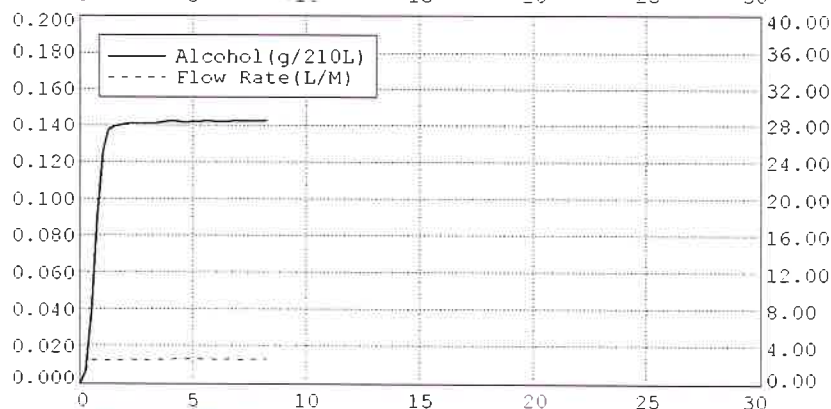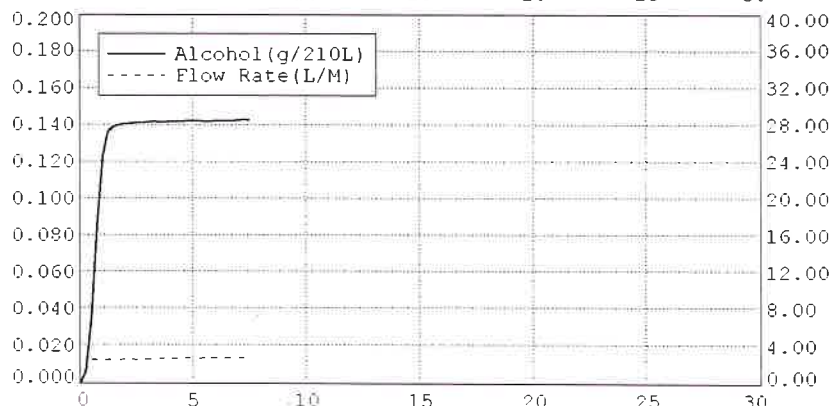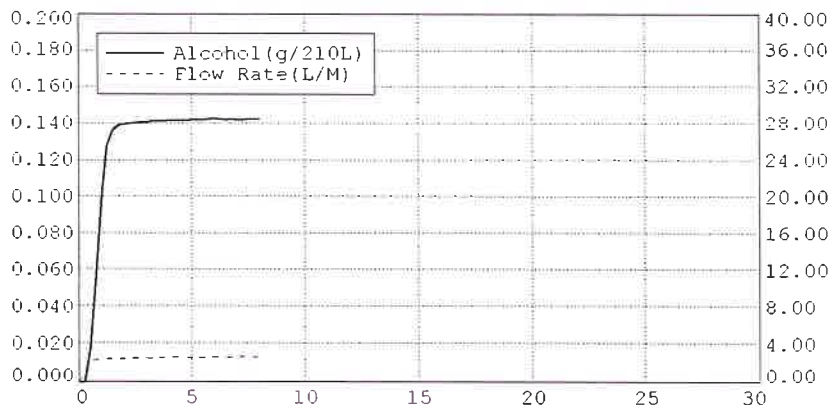

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100412






Date: 09/22/2025
Time: 11:51:33

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.15: 0.292
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 131 psi

BLANK TEST	0.000	11:52
INTERNAL STANDARD	VERIFIED	11:52
EXTERNAL STANDARD	0.288	11:53
BLANK TEST	0.000	11:54
EXTERNAL STANDARD	0.287	11:54
BLANK TEST	0.000	11:55
EXTERNAL STANDARD	0.287	11:55
BLANK TEST	0.000	11:56
EXTERNAL STANDARD	0.287	11:56
BLANK TEST	0.000	11:57
EXTERNAL STANDARD	0.289	11:57
BLANK TEST	0.000	11:58

Average = 0.2876
Std Dev = 0.0009

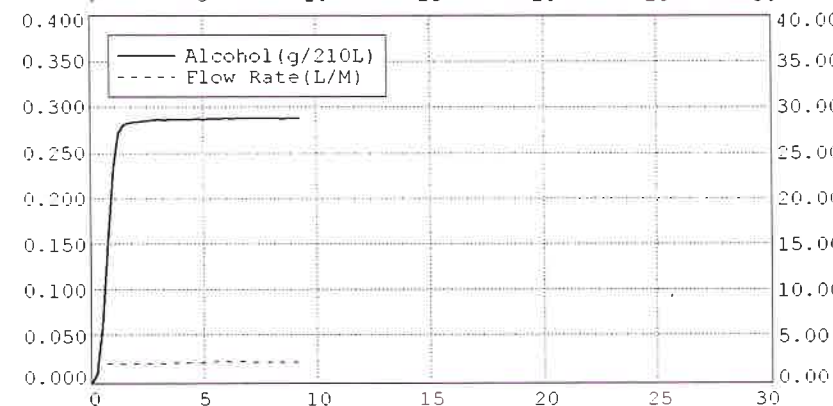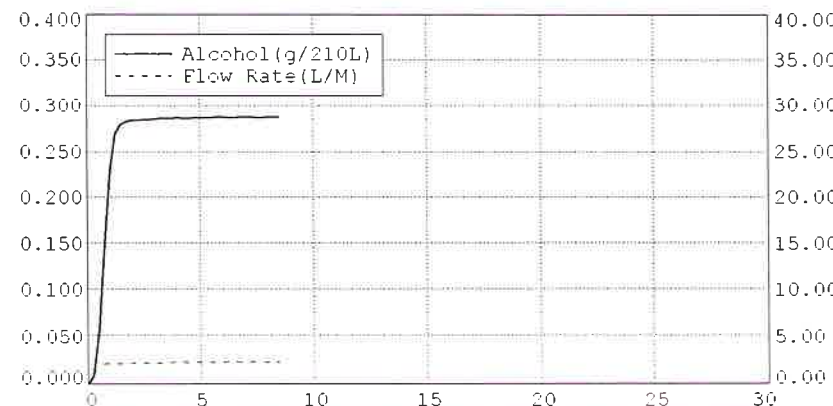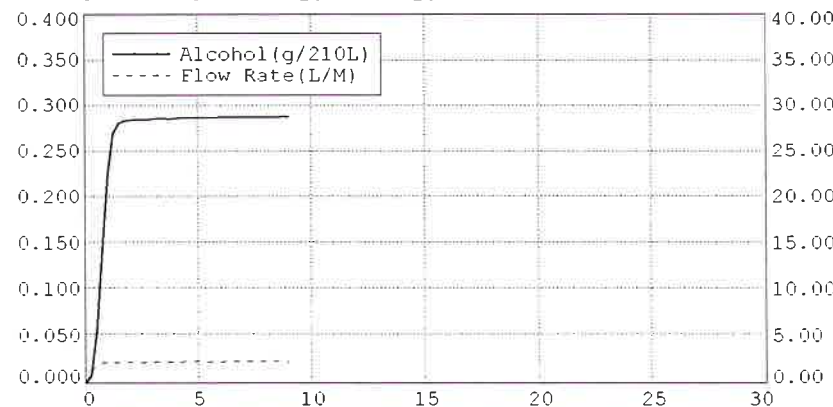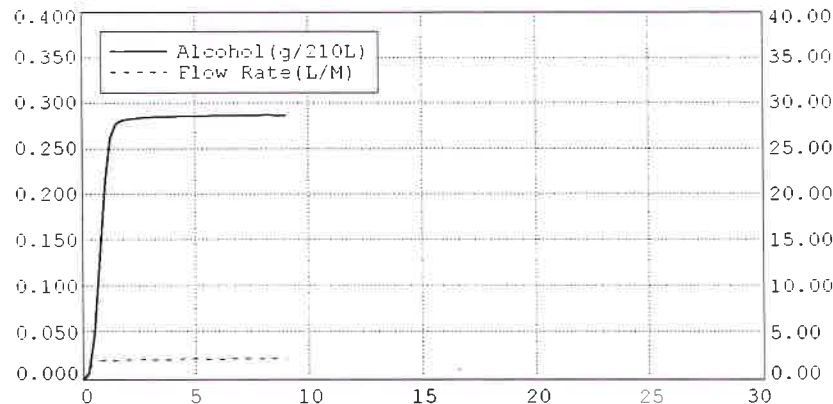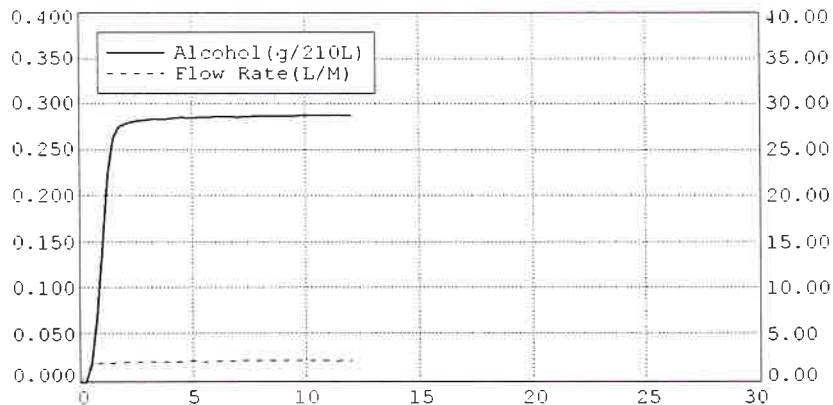

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100412

Date: 09/22/2025
Time: 12:12:21


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: XXX

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.15: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:13
BLANK TEST	0.000	12:13
INTERNAL STANDARD	VERIFIED	12:13
EXTERNAL STANDARD	0.077	12:13
BLANK TEST	0.000	12:14
SUBJECT SAMPLE	INCOMPLETE	12:16

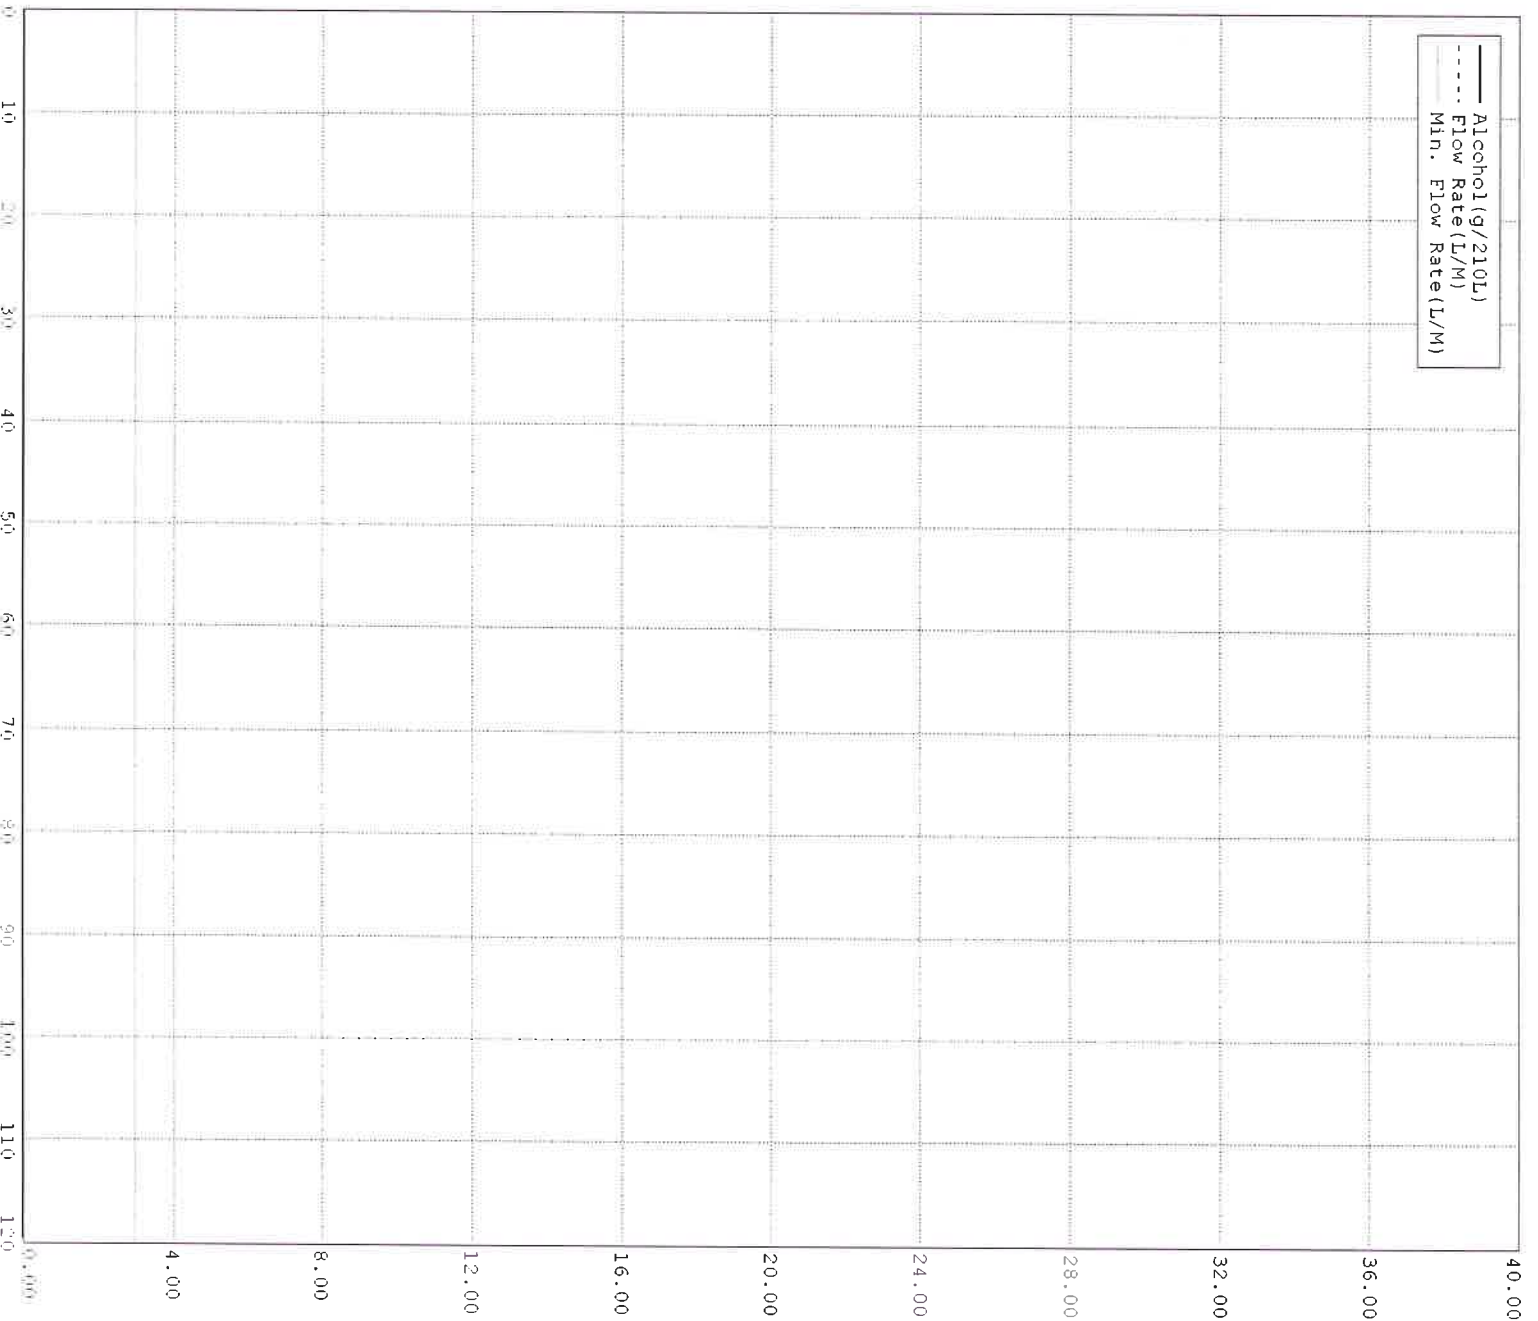

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100412

Date: 09/22/2025
Time: 12:21:21


SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: XXX

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.15: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:22
BLANK TEST	0.000	12:22
INTERNAL STANDARD	VERIFIED	12:22
EXTERNAL STANDARD	0.077	12:22
BLANK TEST	0.000	12:23
SUBJECT SAMPLE	INVALID	12:24

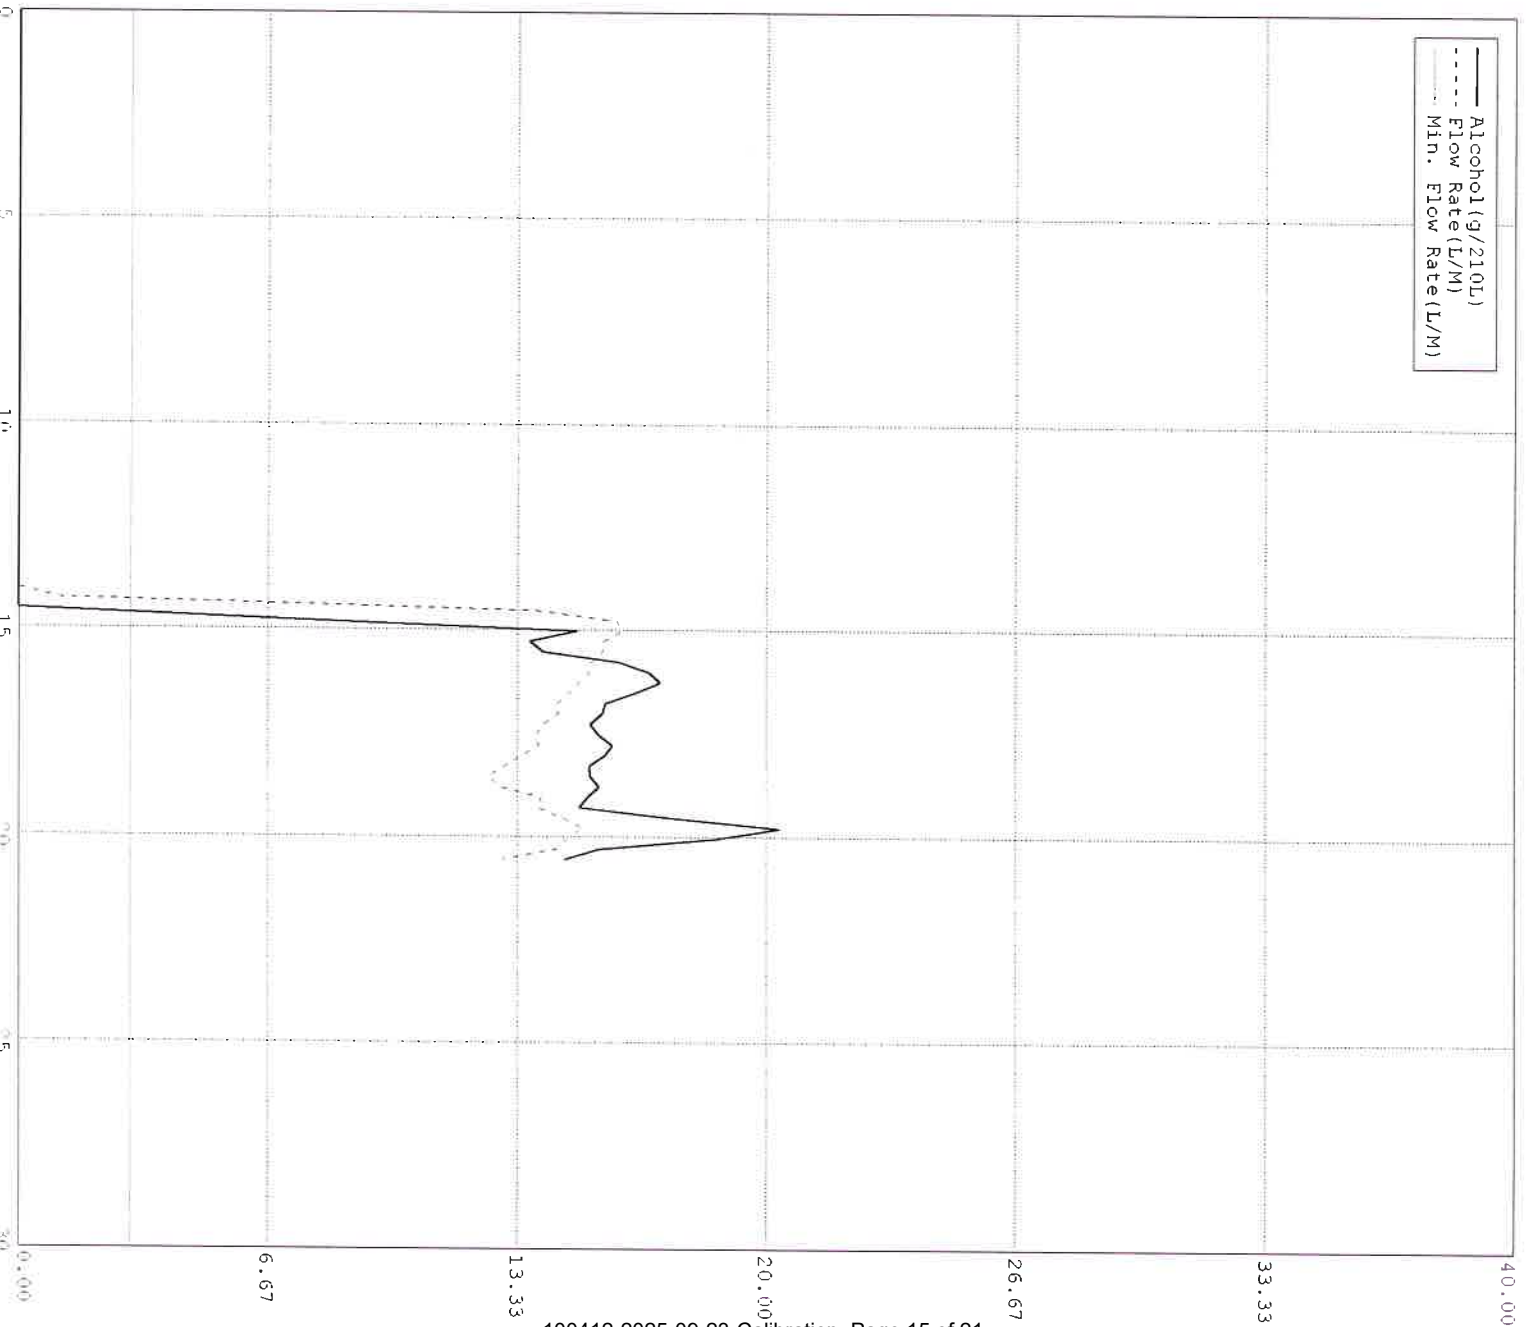

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100412

Date: 09/22/2025
Time: 13:02:24

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAJJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MAX ATTEMPTS
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.16: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:03
BLANK TEST	0.000	13:03
INTERNAL STANDARD	VERIFIED	13:04
EXTERNAL STANDARD	0.076	13:04
BLANK TEST	0.000	13:05
SUBJECT SAMPLE	XXX	13:05

Maximum Attempts Exceeded

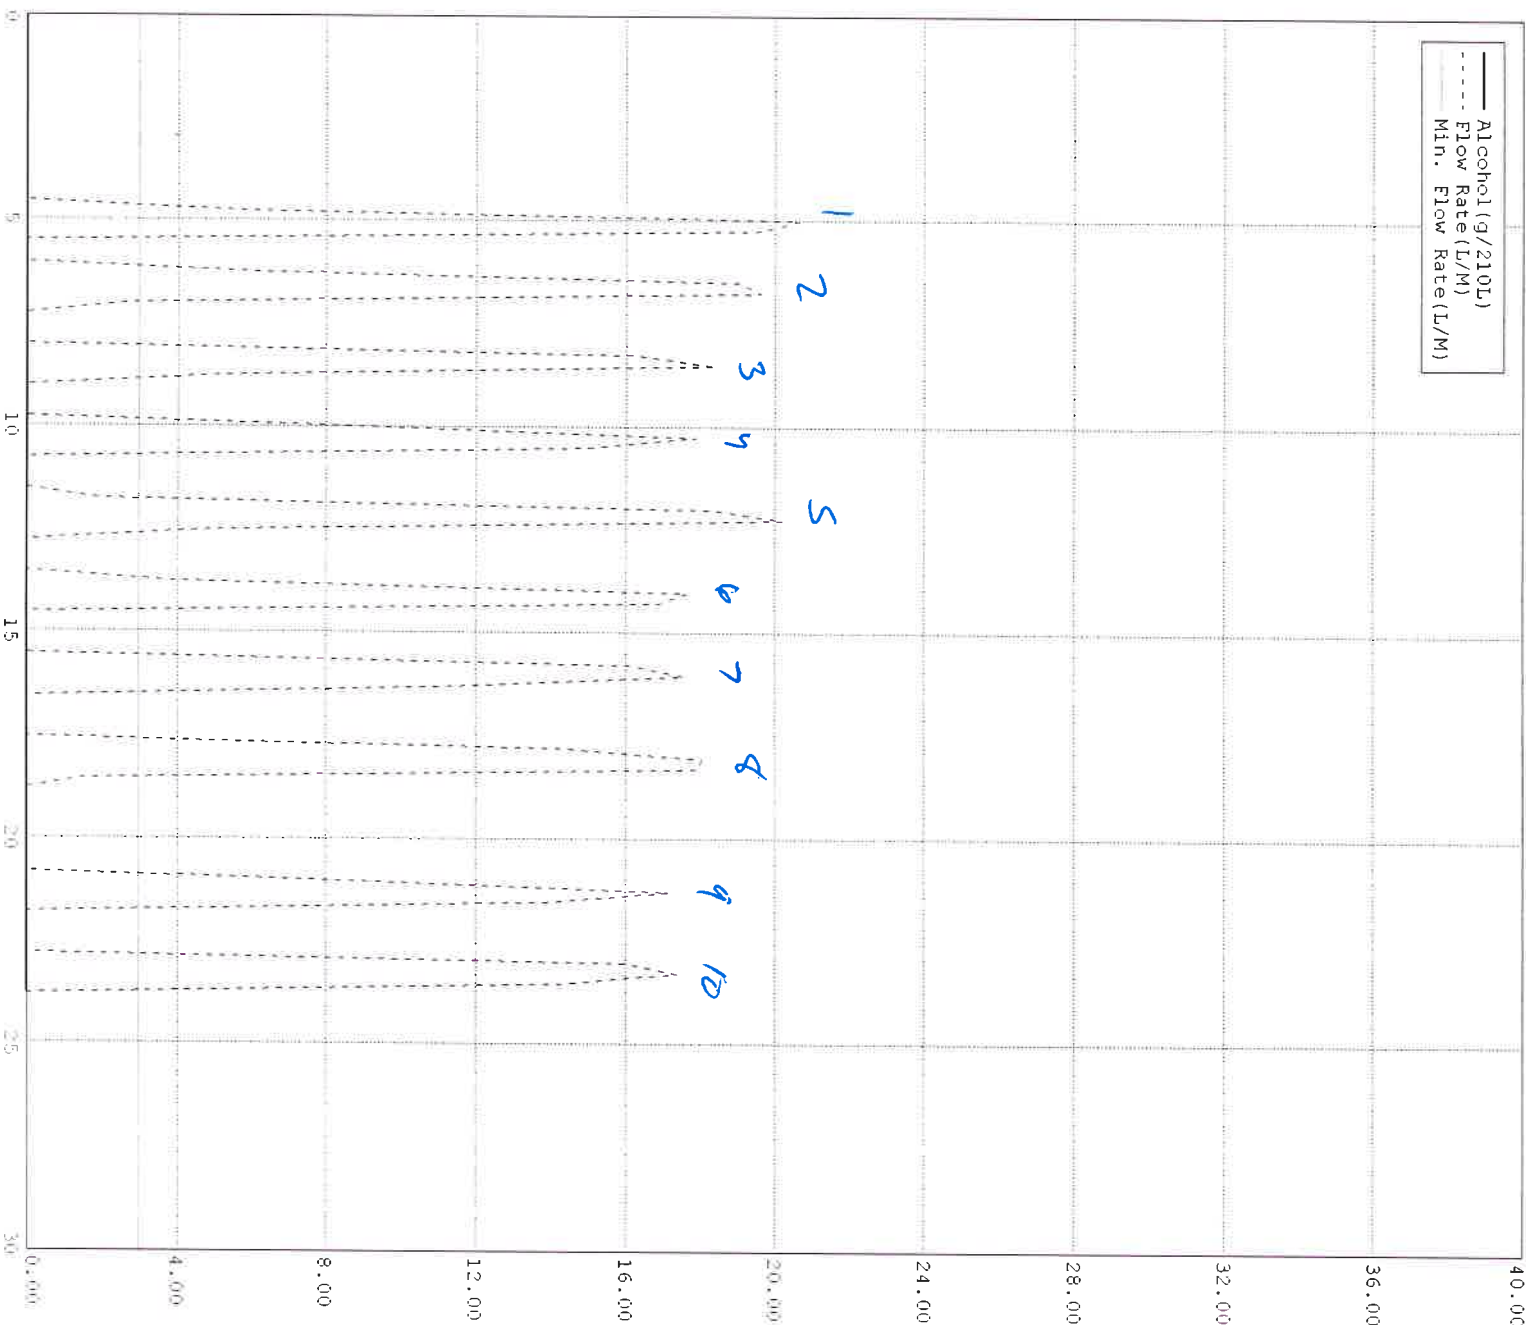

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100412

Date: 09/22/2025
Time: 13:12:32

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.16: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:13
BLANK TEST	0.000	13:13
INTERNAL STANDARD	VERIFIED	13:13
EXTERNAL STANDARD	0.076	13:14
BLANK TEST	0.000	13:14

RFI DETECTED

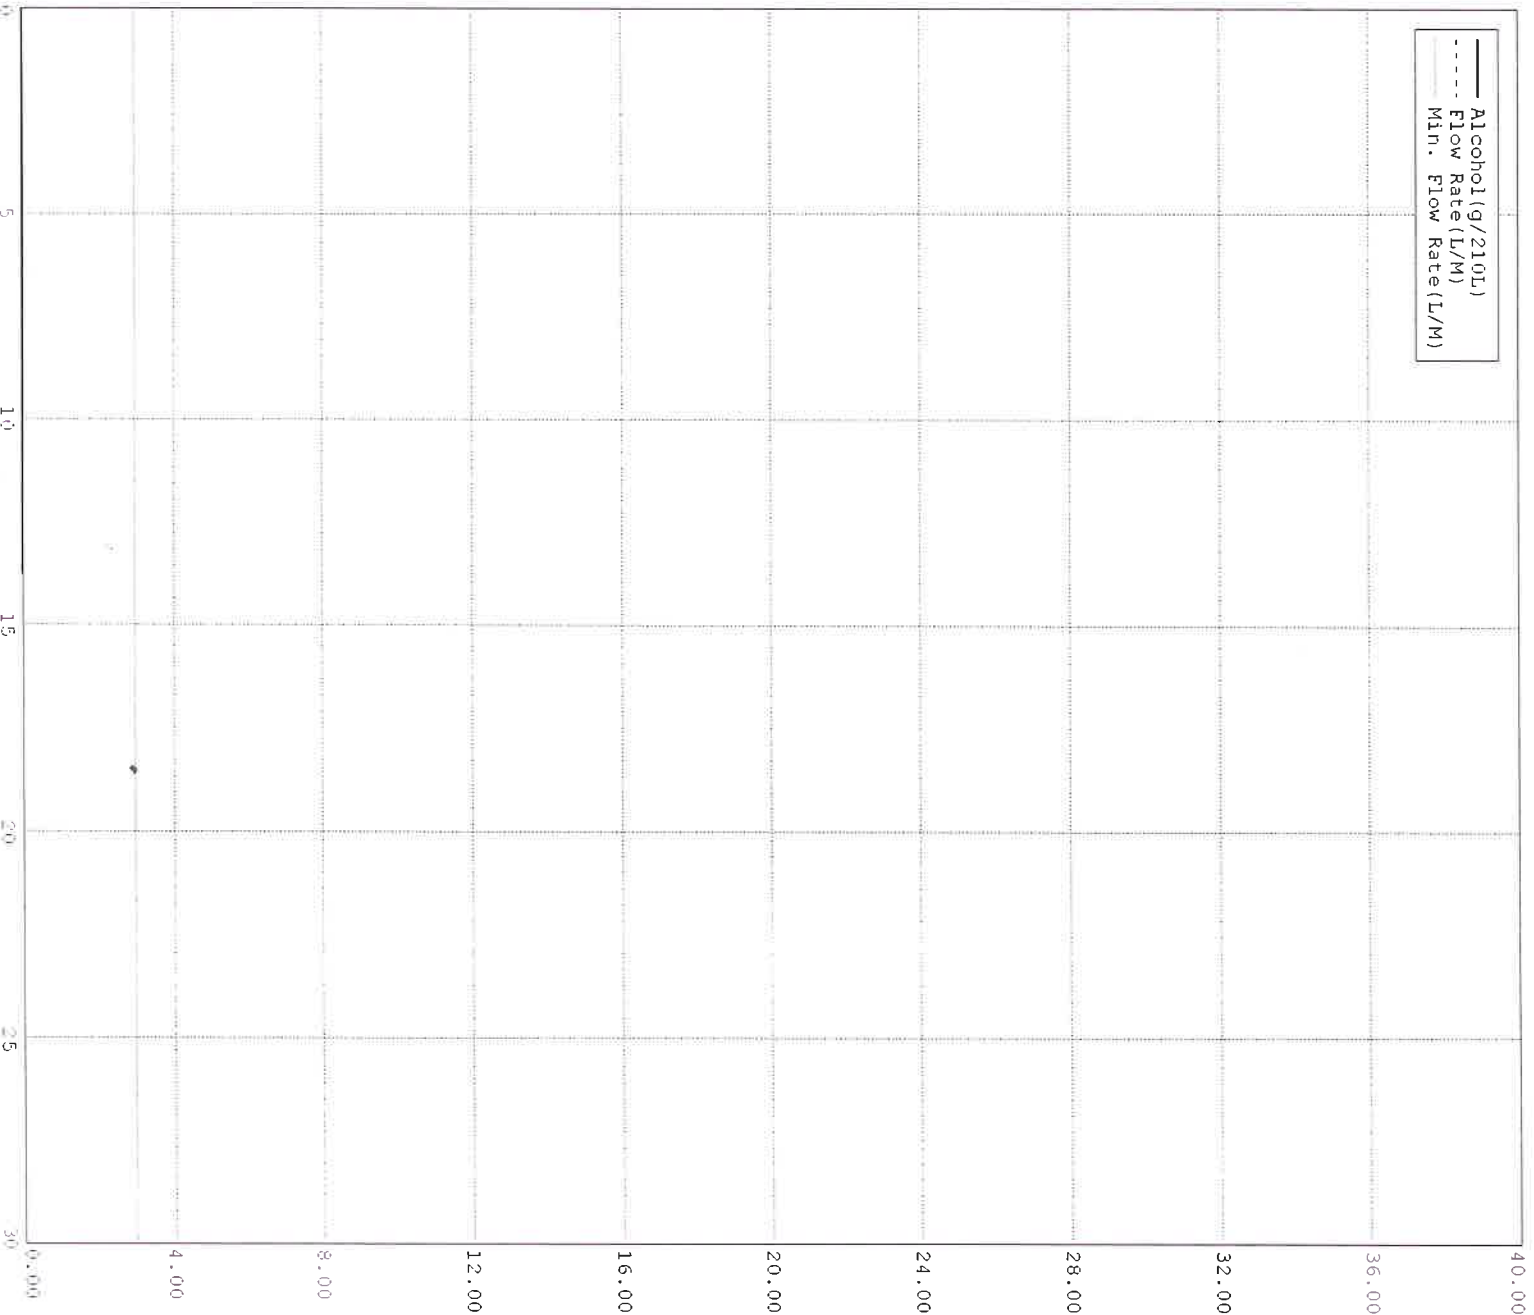

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100412

Date: 09/22/2025
Time: 13:31:56

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:33
BLANK TEST	0.000	13:33
INTERNAL STANDARD	VERIFIED	13:33
Xg = 0.089 (3.03%)		
EXTERNAL STANDARD	0.076	13:34
X[1] = 0.0755 (-0.0025)	(0.0029)	
BLANK TEST	0.000	13:35
SUBJECT SAMPLE	XXX	13:35
X[1] = 0.1102 (-0.0159)	(0.0031)	

Interference Detected

Filter 2ave: -0.0006
Filter 3ave: 0.0026

KS 9/23/25

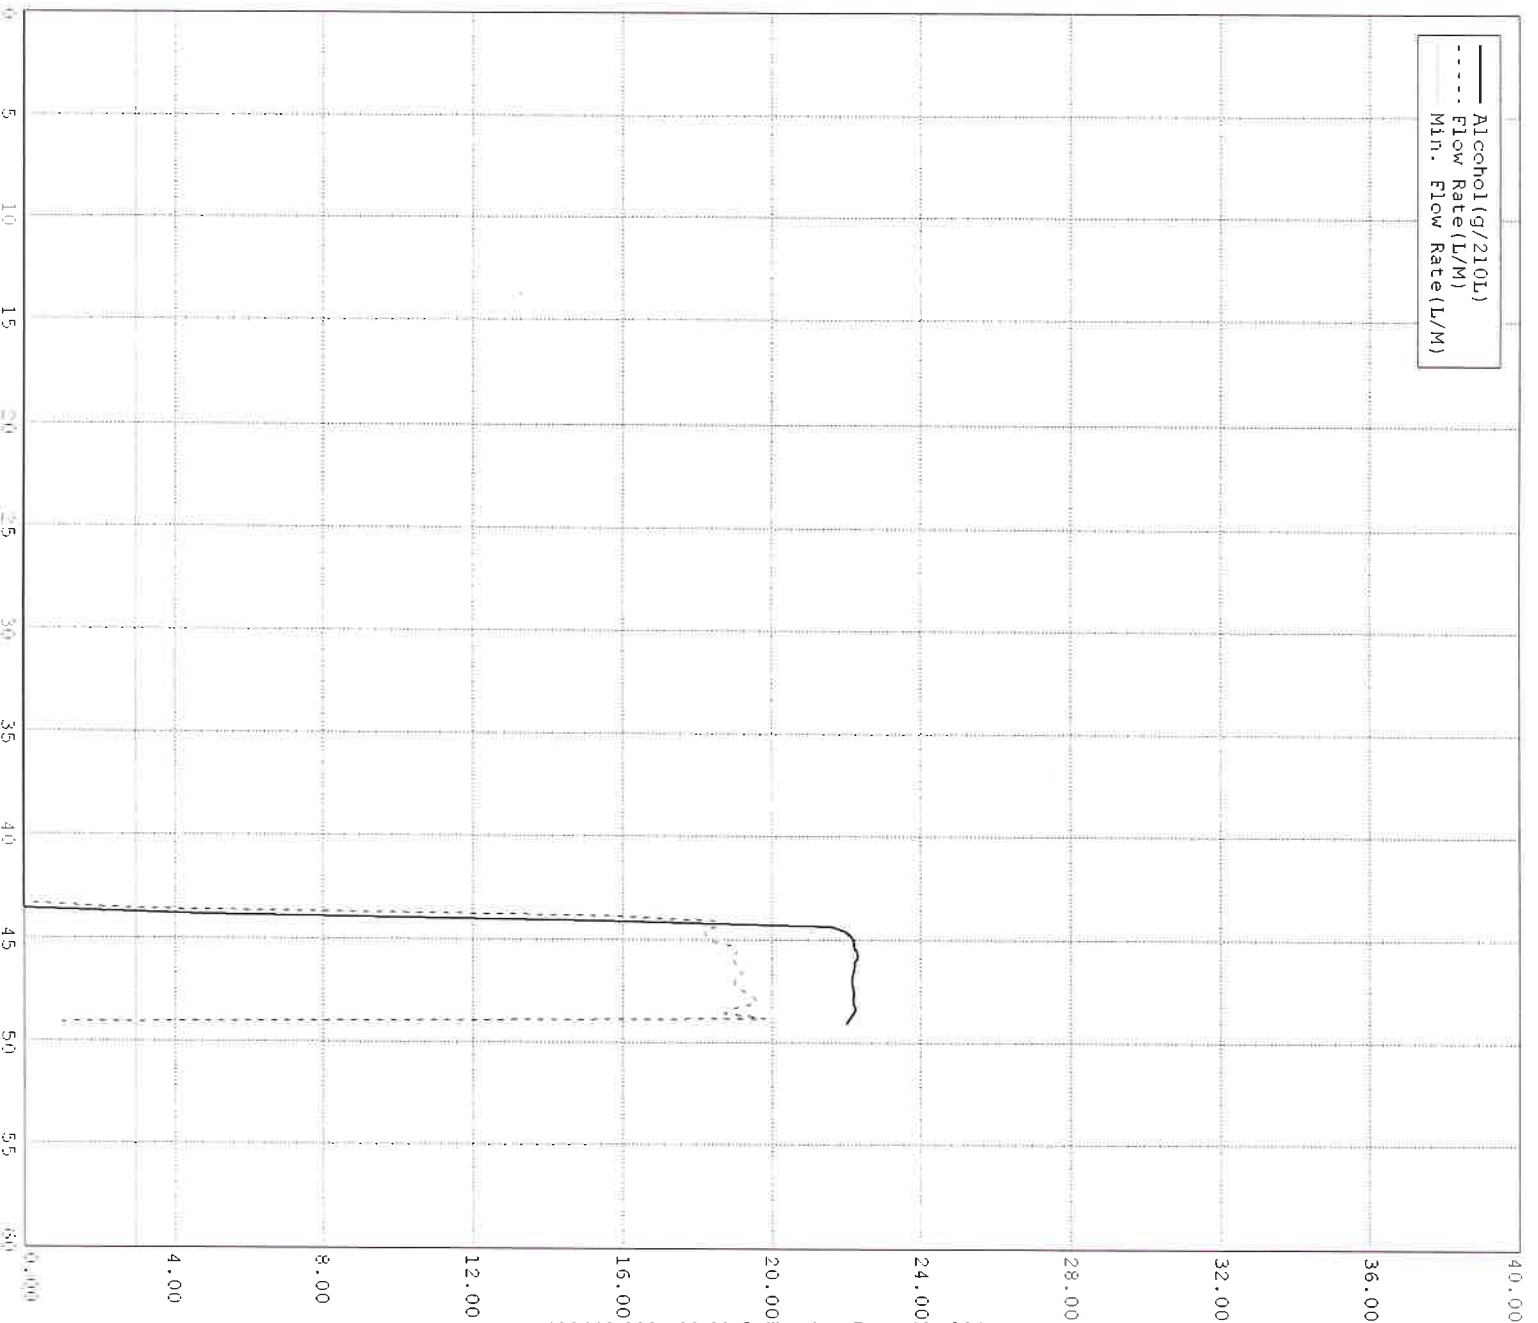

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100412

Date: 09/22/2025
Time: 13:25:30

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:26
BLANK TEST	0.000	13:26
INTERNAL STANDARD	VERIFIED	13:27
Xq = 0.088 (2.02%)		
EXTERNAL STANDARD	0.076	13:27
X[1] = 0.0760 (-0.0002)	(0.0024)	
BLANK TEST	0.000	13:28
SUBJECT SAMPLE	XXX	13:28
X[1] = 0.1176 (-0.0299)	(0.0008)	

Interference Detected

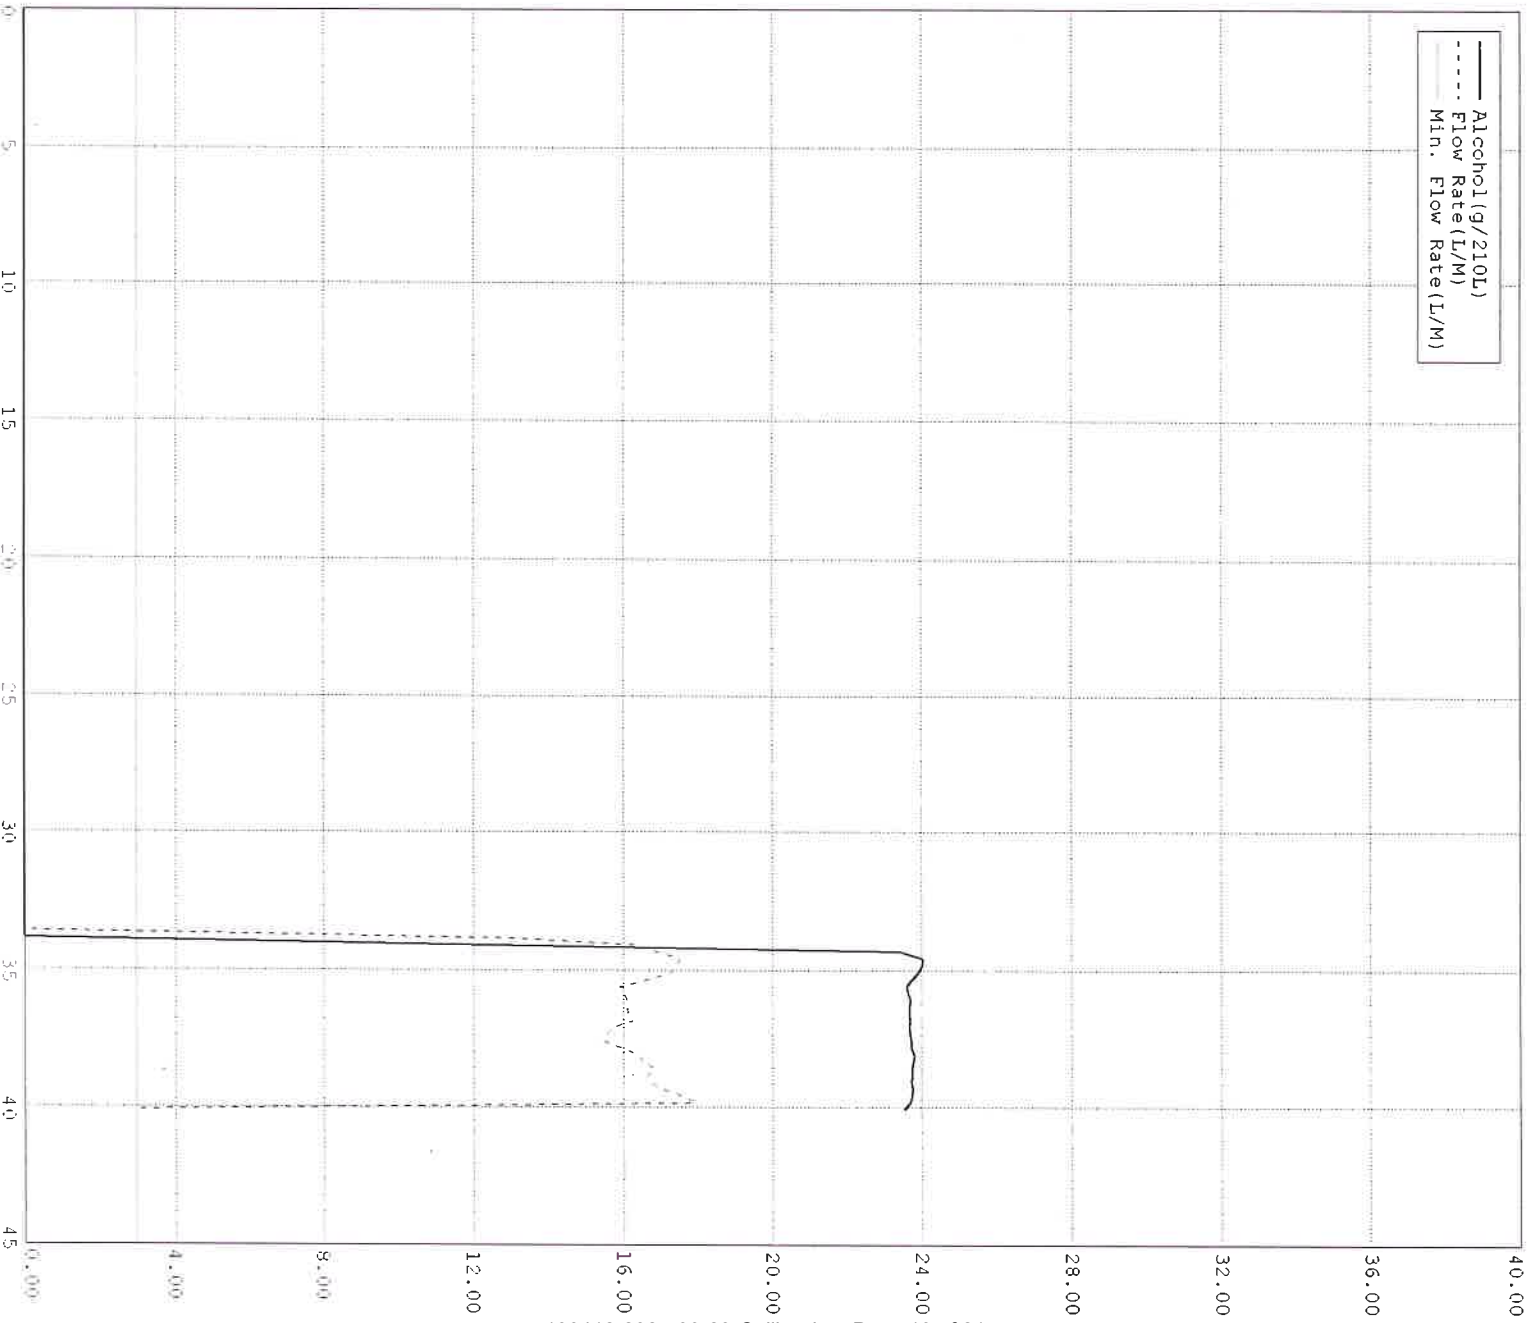

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100412

Date: 09/22/2025
 Time: 13:38:24


SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

DEPT/AGENCY:
 NEGATIVE
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.17: 0.078
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:39
BLANK TEST	0.000	13:39
INTERNAL STANDARD	VERIFIED	13:39
Xq = 0.088 (2.43%)		
EXTERNAL STANDARD	0.076	13:39
X[1] = 0.0764 (0.0007)	(0.0030)	
BLANK TEST	0.000	13:40
SUBJECT SAMPLE (Vol=1.59L)	0.093	13:41
X[1] = 0.0937 (-0.0007)	(0.0006)	
BLANK TEST	0.000	13:42
EXTERNAL STANDARD	0.076	13:42
X[1] = 0.0757 (-0.0005)	(0.0022)	
BLANK TEST	0.000	13:43

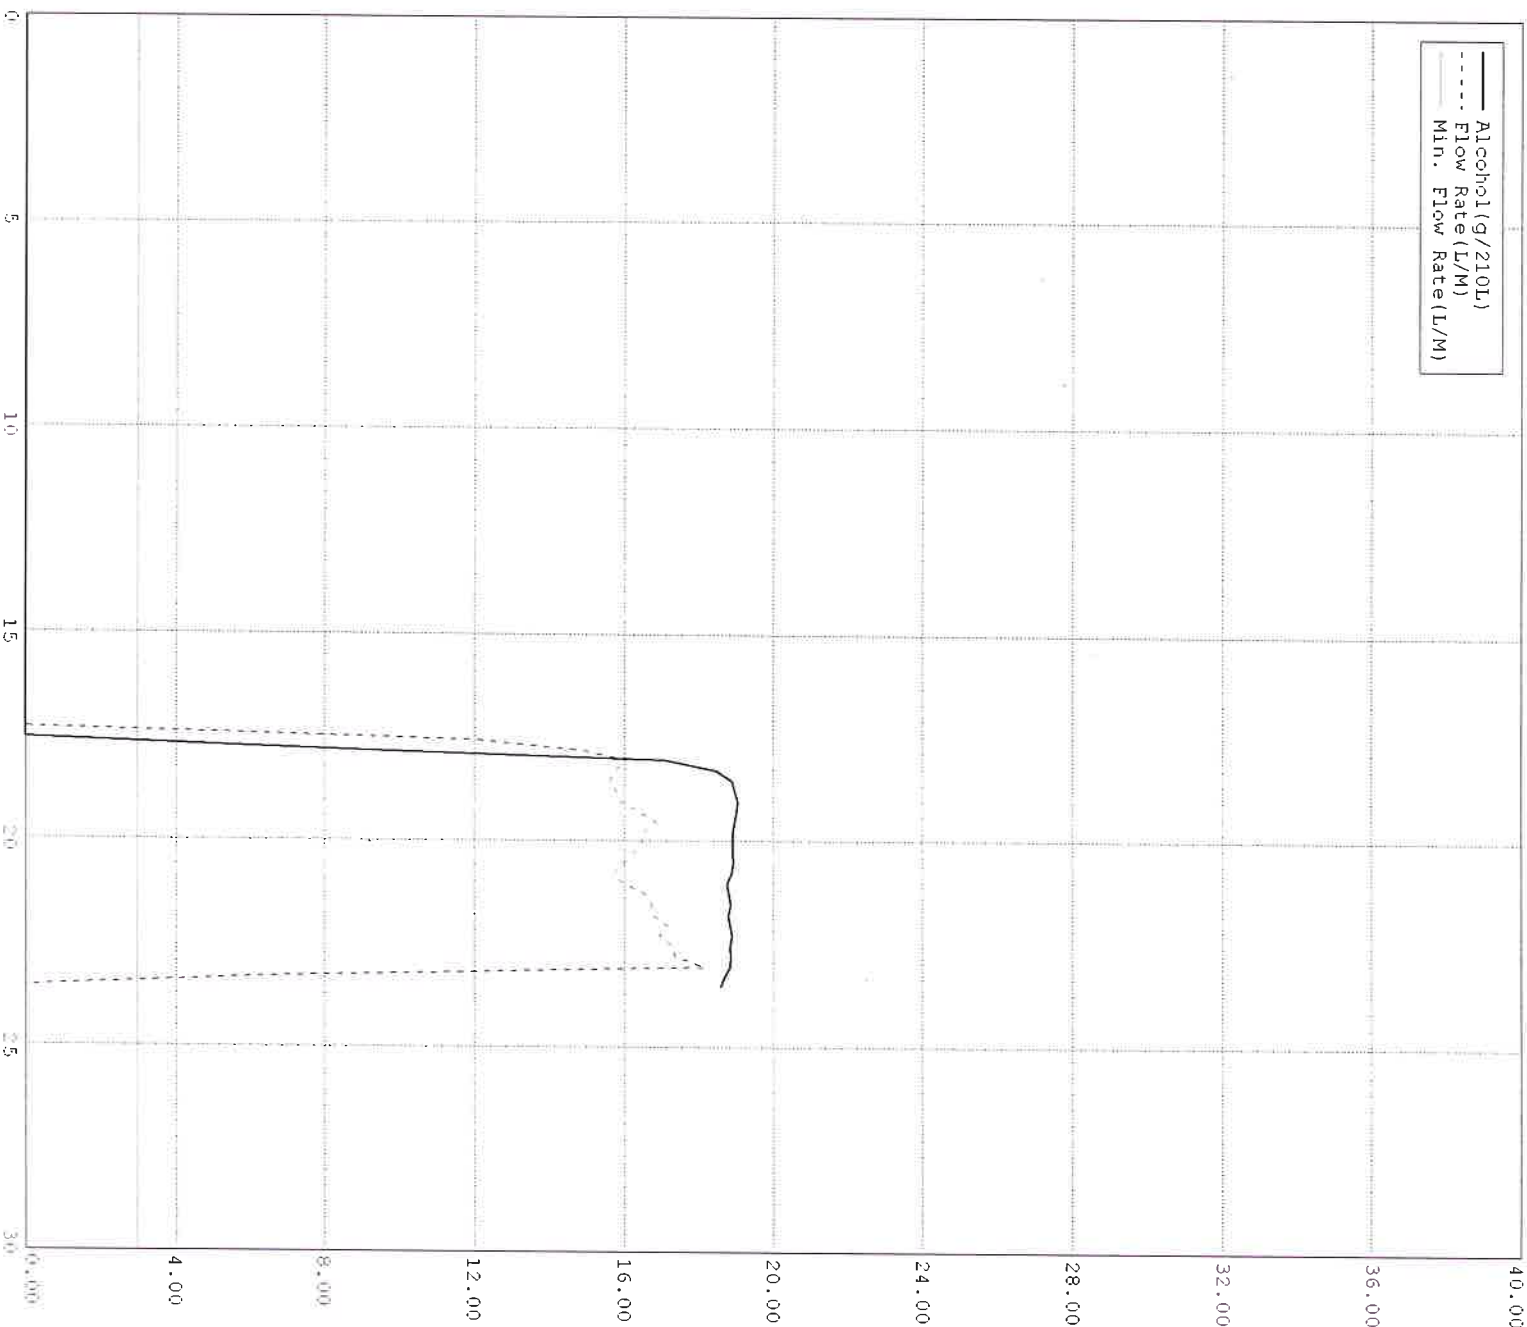

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100412

Date: 09/22/2025
Time: 14:30:52

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON-DRINKING TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:32
BLANK TEST	0.000	14:32
INTERNAL STANDARD	VERIFIED	14:32
EXTERNAL STANDARD	0.075	14:32
BLANK TEST	0.000	14:33
SUBJECT SAMPLE (Vol=1.89L)	0.000	14:34
BLANK TEST	0.000	14:35
EXTERNAL STANDARD	0.076	14:35
BLANK TEST	0.000	14:36

