



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100342

**Report Issue Date:** 07/18/2024  
**Date Received:** 2024-05-28  
**Condition of Item:** No apparent damage

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.019	0.019	0.020	0.020	0.019	0.019	
0.080	0.079	AG335202	0.079	0.078	0.078	0.079	0.079	0.079	
0.300	0.297	AG327804	0.298	0.297	0.298	0.298	0.298	0.298	

As Found - Evaluation Analyst: Kaija Swisher  
 As Found Conditions - Barometric Pressure (inHg): 29.61 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.5 Relative Humidity (%): 34  
 As-Found Lab Activity Date Range: 05/28/2024 - 06/17/2024

Replaced O-Ring. Supervised casework with Derek Walton.

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG408002	0.021	0.021	0.020	0.019	0.020	0.020	+/- 0.002	
0.040	0.039	AG407908	0.040	0.040	0.039	0.040	0.040	0.040	+/- 0.003	
0.080	0.078	AG335202	0.080	0.080	0.079	0.080	0.080	0.080	+/- 0.004	
0.100	0.098	AG333401	0.100	0.100	0.099	0.100	0.100	0.100	+/- 0.004	
0.150	0.147	AG332004	0.147	0.147	0.147	0.147	0.147	0.147	+/- 0.005	
0.300	0.294	AG327804	0.298	0.298	0.299	0.298	0.298	0.298	+/- 0.011	

As Left Conditions - Barometric Pressure (inHg): 29.35 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.2 Relative Humidity (%): 51  
 As-Left Lab Activity Date Range: 07/15/2024 - 07/16/2024

Supervised casework with Kaija Swisher.

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Derek Walton on 07/16/2024

[derek.walton@alaska.gov](mailto:derek.walton@alaska.gov)

Technically and administratively reviewed by Colleen O'Bryant on 07/18/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100342 Analyst or Technician Name: Kaija Swisher

DataMaster DMT Calibration Start Date: 7/15/24

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

Supervised casework with

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 230307229  
Calibration Due Date: May 2, 2025
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Dereen Walton DMV  
7/15/24

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.35 Temperature(C) 20.2 Relative Humidity(%) 51

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20240501KS Expiration Date: 8/1/24  
Simulator S/N: SD1088 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240501MNC Expiration Date: 8/1/24  
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 22MP41201 Expiration Date: 8/1/24  
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 9/19/2025

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 7/15/24

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): 7/15/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100342  
-----

Date: 07/15/2024  
Time: 09:49:19

VERSIONS  
DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 47.0°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.65 V PASSED  
(0.99 V - 2.31 V)  
Cooler Voltage = 1.66 V PASSED  
(0.97 V - 2.25 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 533 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.238 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED  
Xq = 0.085 0.31% (0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100342  
-----

Date: 07/15/2024  
Time: 9:55 AM

Temperatures (°C)

Sample Cell: 48.9°C  
Breath Tube: 46.2°C

Current Barometer 29.4 in  
Volume (Ltr) 1.58

Settings

Lamp: 1.65 V  
Bias: 80 V  
Cooler: 1.66 V  
Chopper: 533 Hz

Voltages (V)

Flow: 1.02 V  
Detector: -0.024 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100342  
-----

Date: 06/19/2024  
Time: 10:31:28

OPERATOR NAME:  
KAIJA SWISHER  
CERTIFICATE #: 10746

Ca = 0.1000  
CAL = 0.985943    0.800 <= CAL < 1.200  
b1 = 0.0008    0.0000 <= b1 < 0.0040  
b2 = 0.0045    0.0010 <= b2 < 0.0100  
b3 = 0.0010    0.0000 <= b3 < 0.0040  
Xq = 0.0855    0.0500 <= Xq < 0.2000  
a21 = 1.186599    1.050 <= a21 < 1.300  
a31 = 0.494774    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100342

Date: 07/15/2024  
Time: 09:56:43

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746


DEPT/AGENCY:  
MINIMUM VOLUME TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.36: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	09:57
BLANK TEST	0.000	09:57
INTERNAL STANDARD	VERIFIED	09:57
EXTERNAL STANDARD	0.079	09:58
BLANK TEST	0.000	09:59
SUBJECT SAMPLE (Vol=1.57L)	0.000	09:59
BLANK TEST	0.000	10:00
EXTERNAL STANDARD	0.080	10:01
BLANK TEST	0.000	10:01

KS

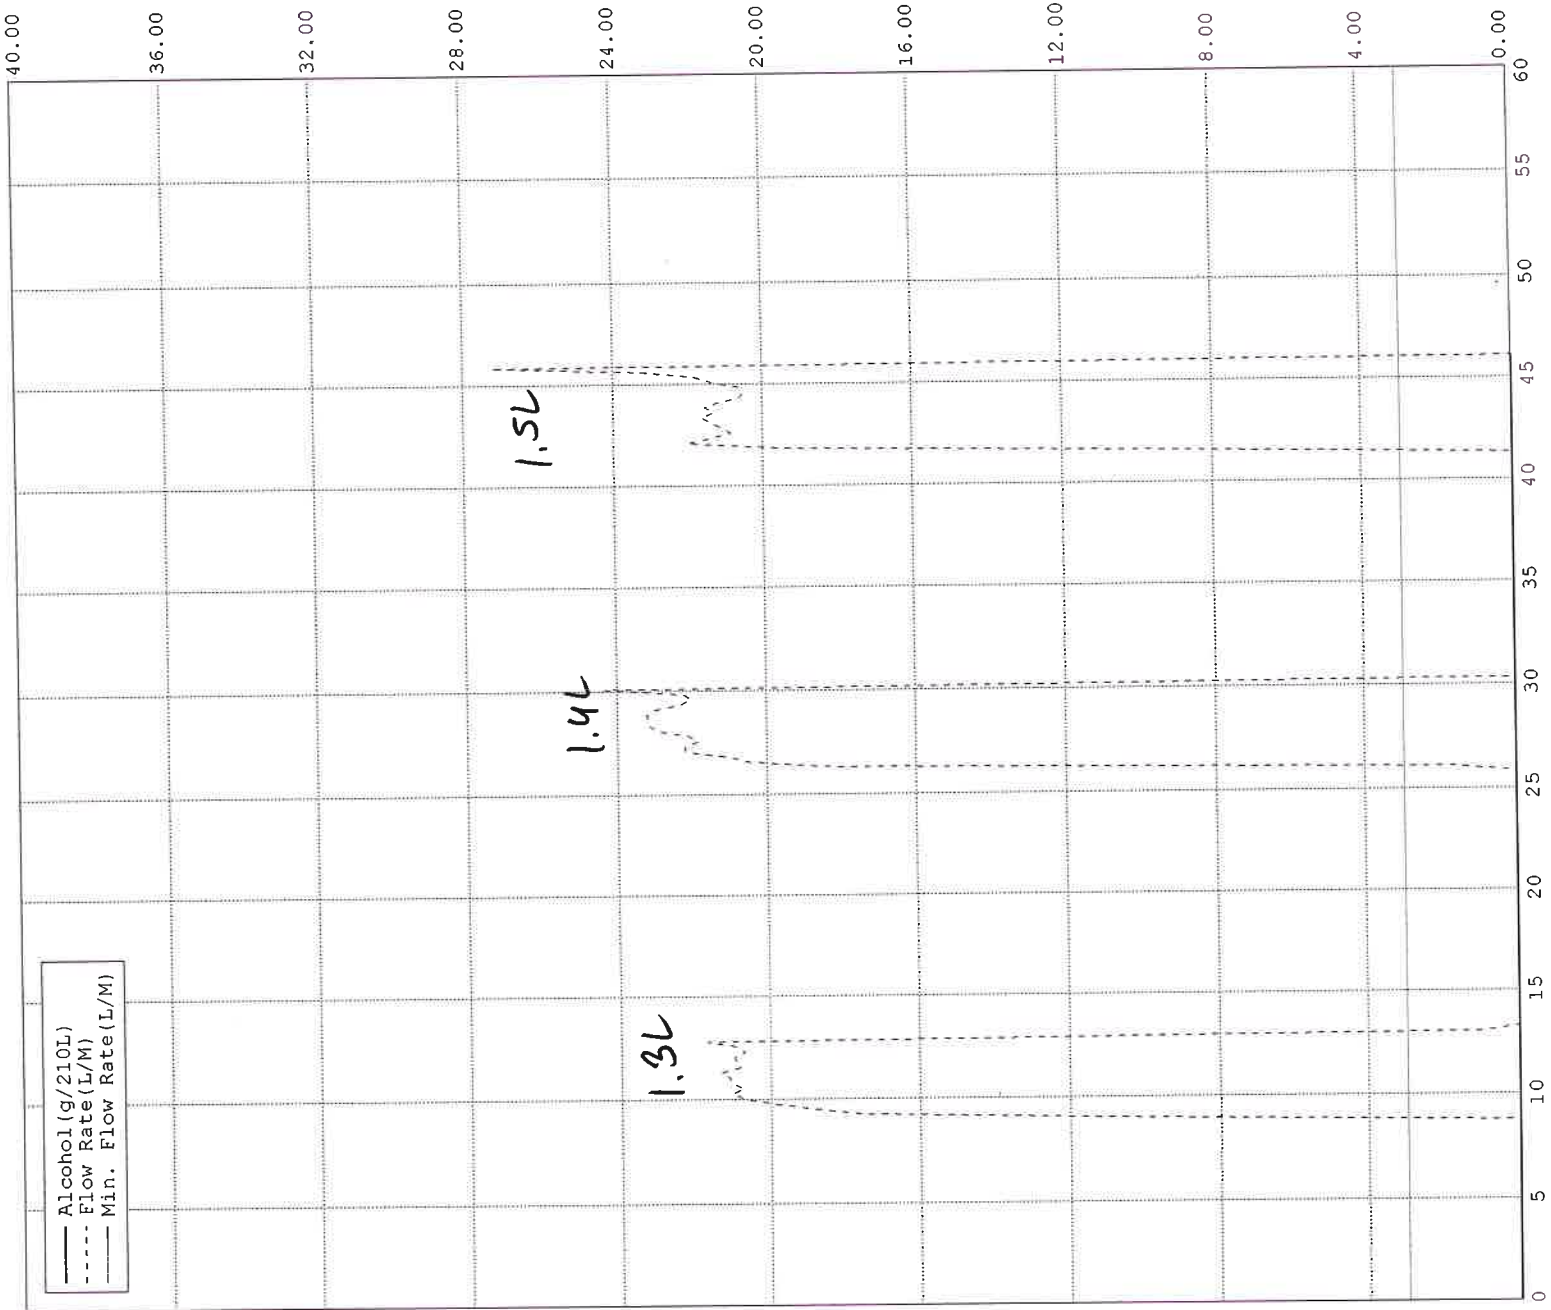

LINEARITY CHECK


Alaska Department of Public Safety  
 DATAMASTER dmt: 100342

Date: 07/15/2024  
 Time: 10:04:27

SUPERVISOR NAME:  
 KAIJA SWISHER  
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0008
0.039	0.0398	0.0004
0.078	0.0798	0.0004
0.098	0.0998	0.0004
0.147	0.1470	0.0000
0.294	0.2982	0.0004

SLOPE = 1.012029  
 SLOPE<sup>2</sup> = 0.9999907

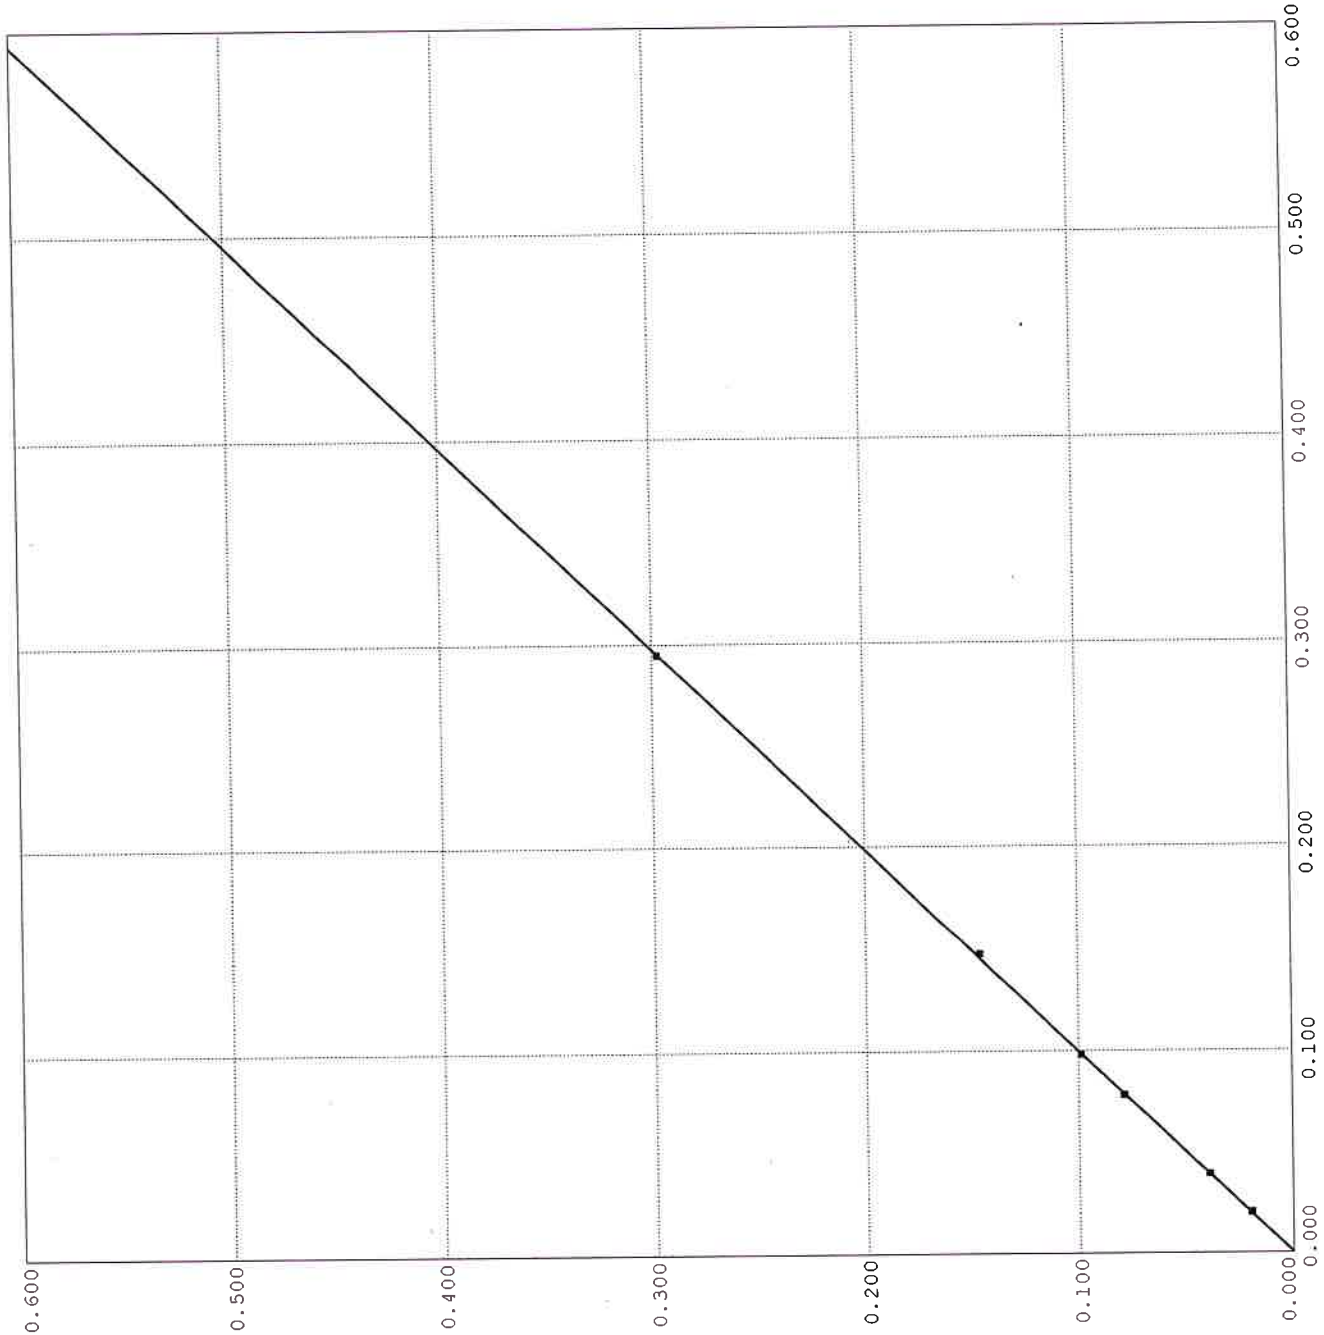

KS

LINEARITY CHECK: Control Test 1






Alaska Department of Public Safety  
 DATAMASTER dmt: 100342

Date: 07/15/2024  
 Time: 10:04:29

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.020  
 TARGET AT 29.36: 0.020  
 LOT #: AG408002  
 EXPIRATION: 03/20/2026  
 TANK PRESSURE: 1064 psi

BLANK TEST	0.000	10:05
INTERNAL STANDARD	VERIFIED	10:06
EXTERNAL STANDARD	0.021	10:06
BLANK TEST	0.000	10:07
EXTERNAL STANDARD	0.021	10:07
BLANK TEST	0.000	10:08
EXTERNAL STANDARD	0.020	10:08
BLANK TEST	0.000	10:09
EXTERNAL STANDARD	0.019	10:09
BLANK TEST	0.000	10:10
EXTERNAL STANDARD	0.020	10:10
BLANK TEST	0.000	10:11

Average = 0.0202  
 Std Dev = 0.0008

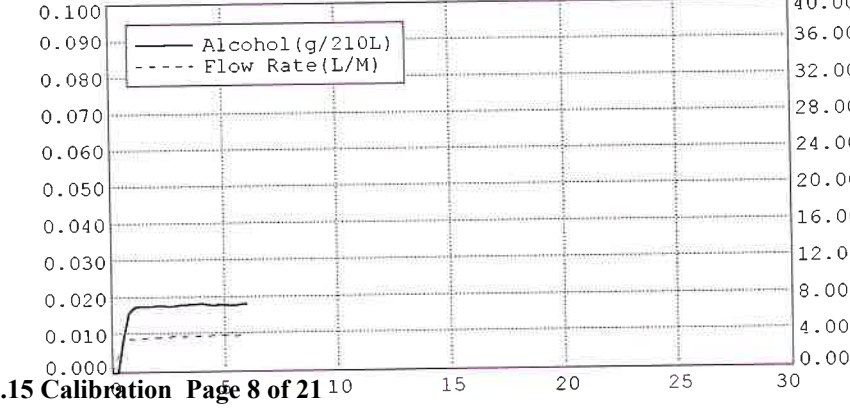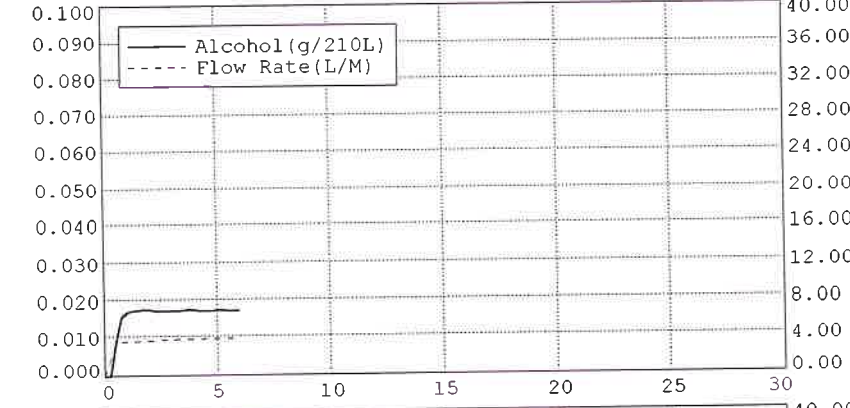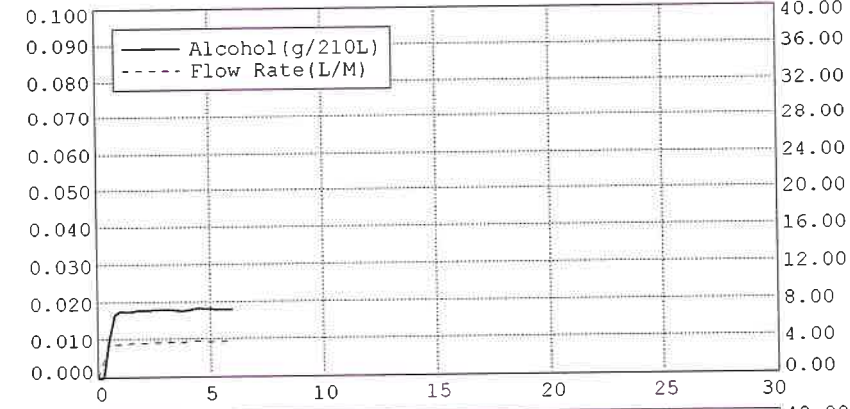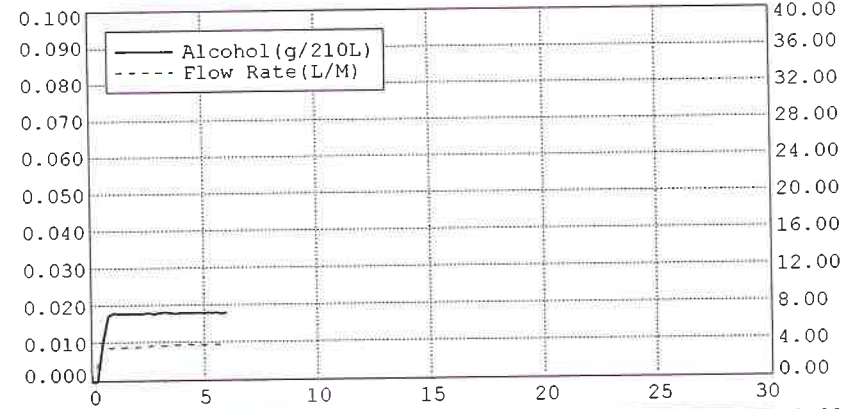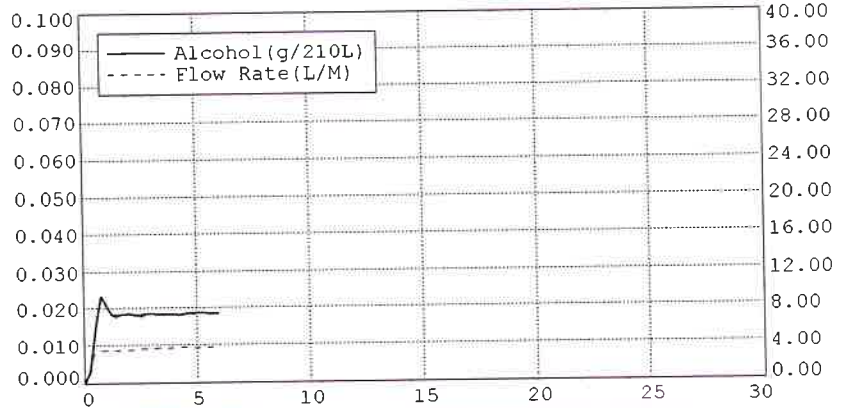



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
DATAMASTER dmt: 100342






Date: 07/15/2024  
Time: 10:12:07

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
TARGET AT 29.36: 0.039  
LOT #: AG407908  
EXPIRATION: 03/19/2026  
TANK PRESSURE: 1168 psi

BLANK TEST	0.000	10:13
INTERNAL STANDARD	VERIFIED	10:13
EXTERNAL STANDARD	0.040	10:13
BLANK TEST	0.000	10:14
EXTERNAL STANDARD	0.040	10:14
BLANK TEST	0.000	10:15
EXTERNAL STANDARD	0.039	10:16
BLANK TEST	0.000	10:16
EXTERNAL STANDARD	0.040	10:17
BLANK TEST	0.000	10:18
EXTERNAL STANDARD	0.040	10:18
BLANK TEST	0.000	10:19

Average = 0.0398  
Std Dev = 0.0004

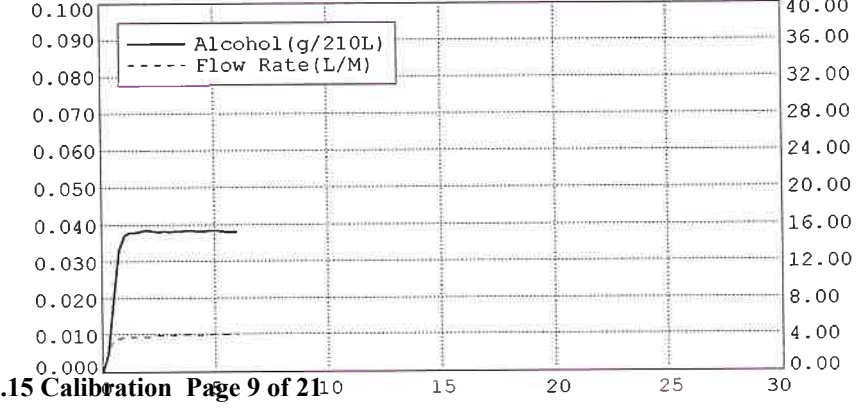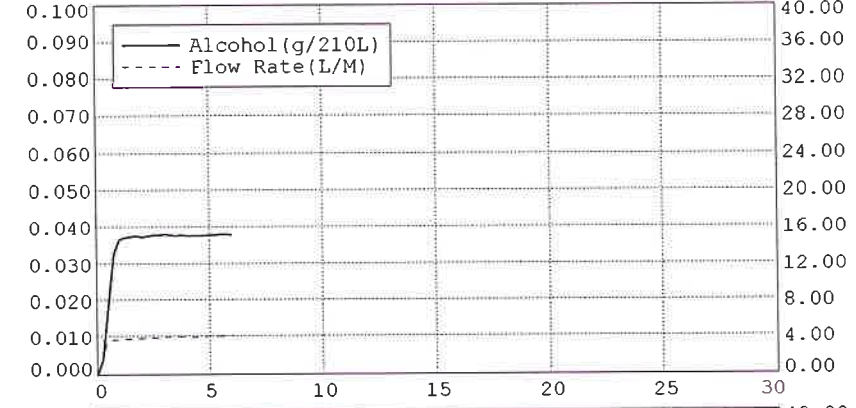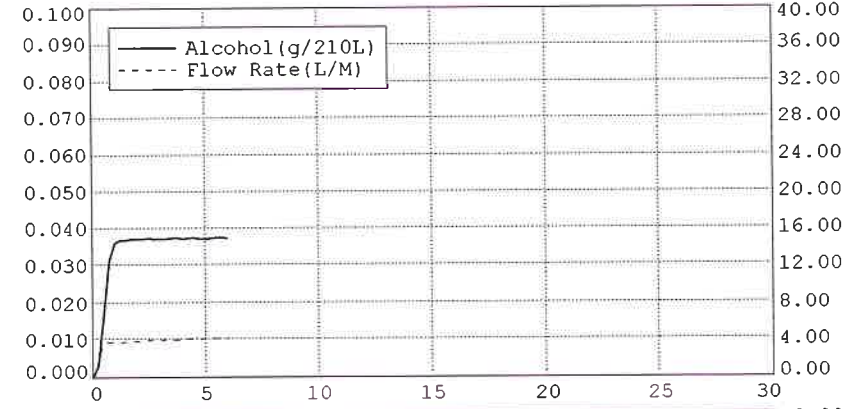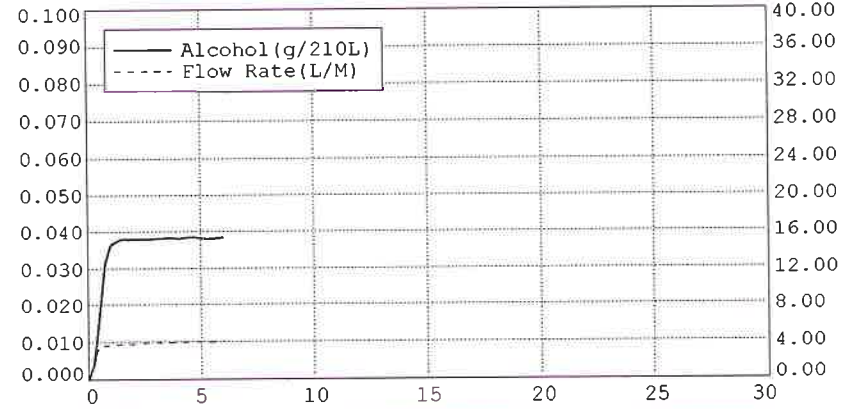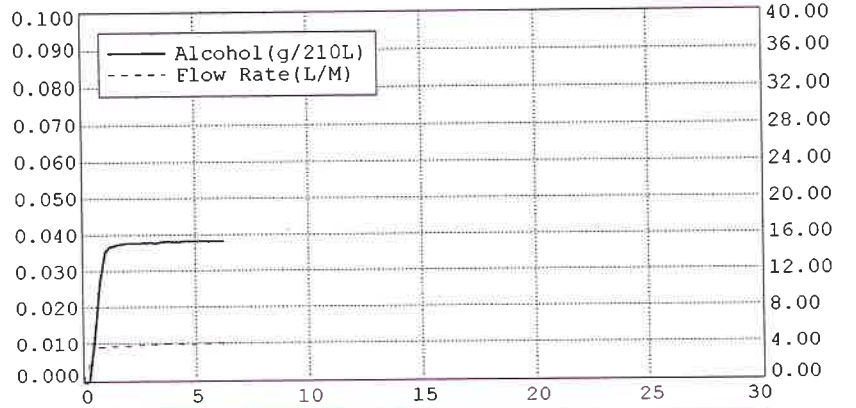

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100342






Date: 07/15/2024  
 Time: 10:19:46

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.36: 0.078  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025  
 TANK PRESSURE: 1078 psi

BLANK TEST	0.000	10:21
INTERNAL STANDARD	VERIFIED	10:21
EXTERNAL STANDARD	0.080	10:21
BLANK TEST	0.000	10:22
EXTERNAL STANDARD	0.080	10:22
BLANK TEST	0.000	10:23
EXTERNAL STANDARD	0.079	10:23
BLANK TEST	0.000	10:24
EXTERNAL STANDARD	0.080	10:24
BLANK TEST	0.000	10:25
EXTERNAL STANDARD	0.080	10:25
BLANK TEST	0.000	10:26

Average = 0.0798  
 Std Dev = 0.0004

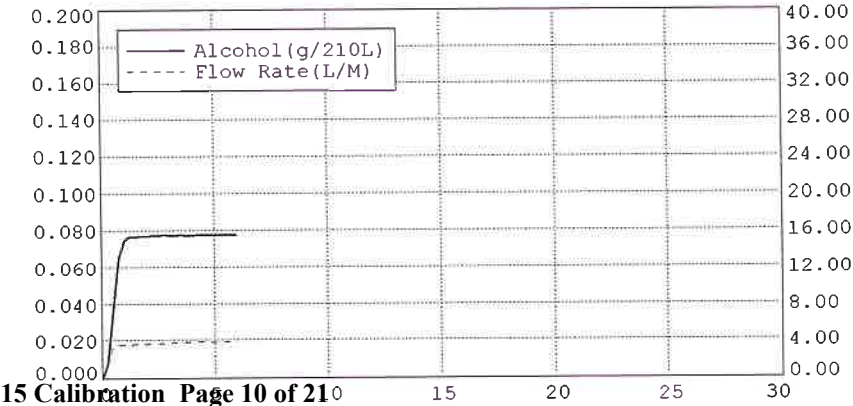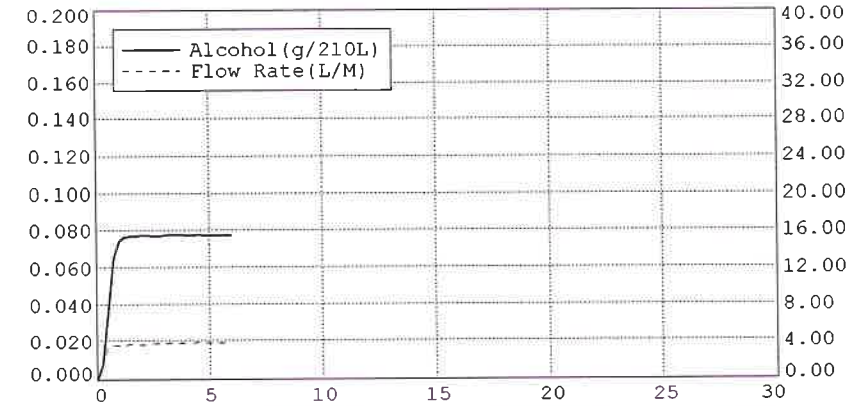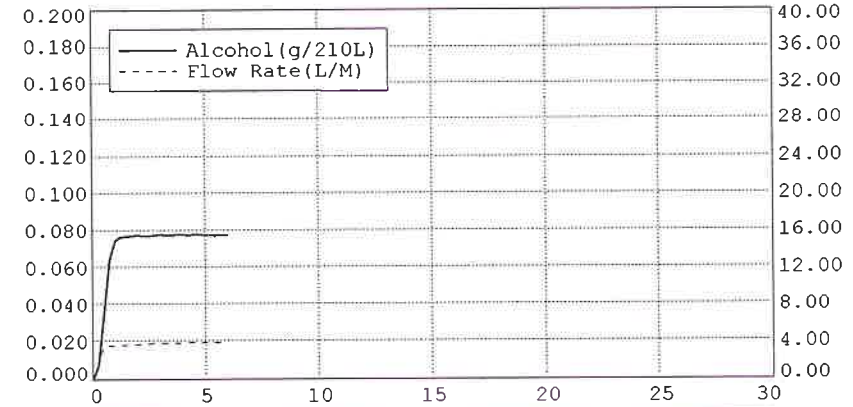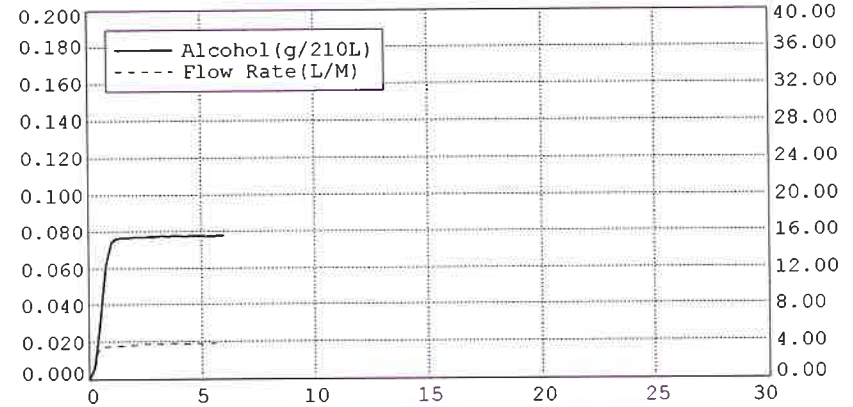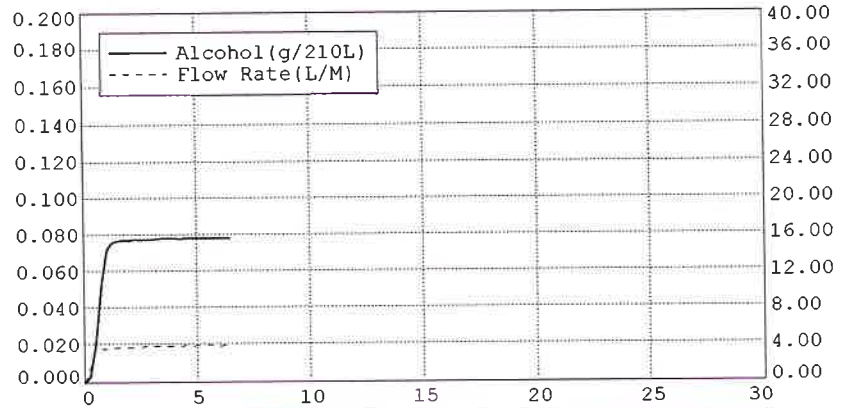

LINEARITY CHECK: Control Test 4






Alaska Department of Public Safety  
DATAMASTER dmt: 100342

Date: 07/15/2024  
Time: 10:30:21

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.100  
TARGET AT 29.36: 0.098  
LOT #: AG333401  
EXPIRATION: 11/30/2025  
TANK PRESSURE: 876 psi

BLANK TEST	0.000	10:31
INTERNAL STANDARD	VERIFIED	10:31
EXTERNAL STANDARD	0.100	10:32
BLANK TEST	0.000	10:33
EXTERNAL STANDARD	0.100	10:33
BLANK TEST	0.000	10:34
EXTERNAL STANDARD	0.099	10:34
BLANK TEST	0.000	10:35
EXTERNAL STANDARD	0.100	10:35
BLANK TEST	0.000	10:36
EXTERNAL STANDARD	0.100	10:36
BLANK TEST	0.000	10:37

Average = 0.0998  
Std Dev = 0.0004

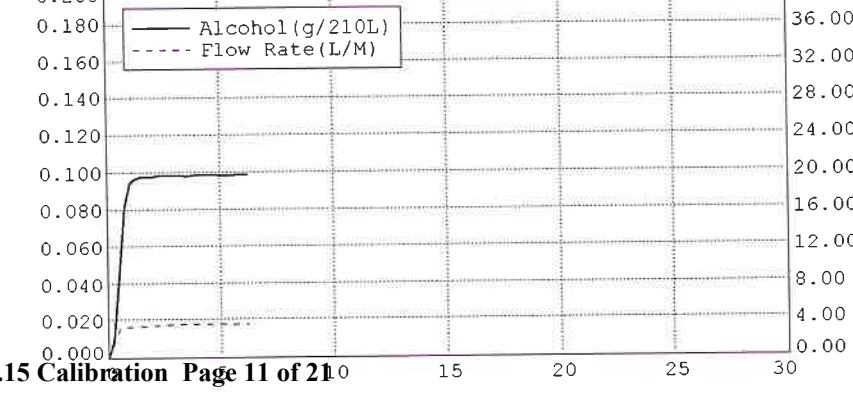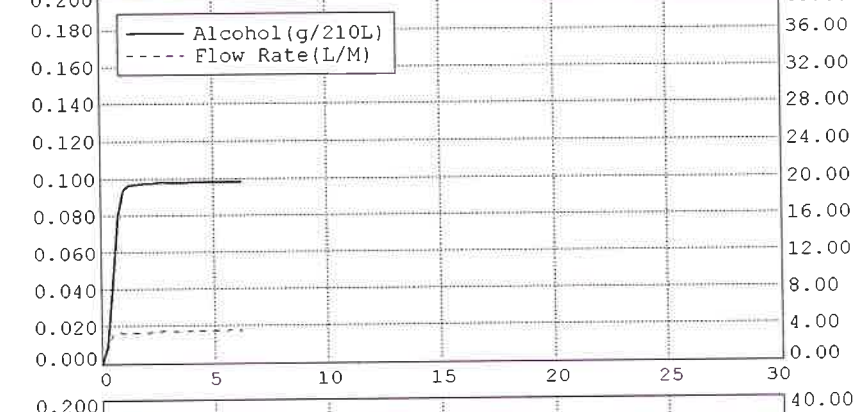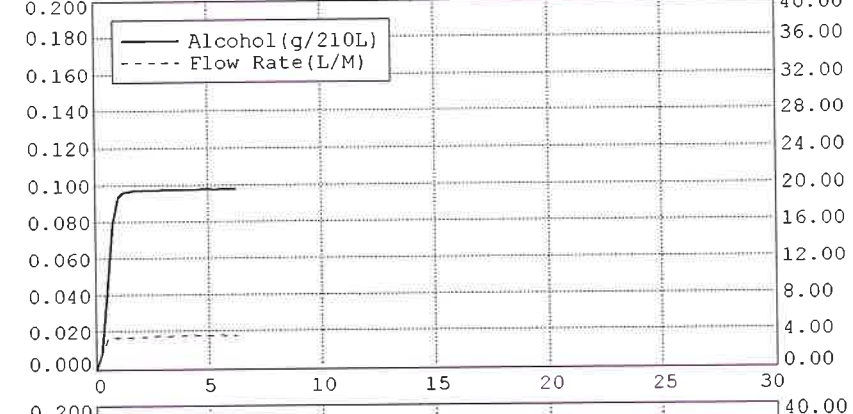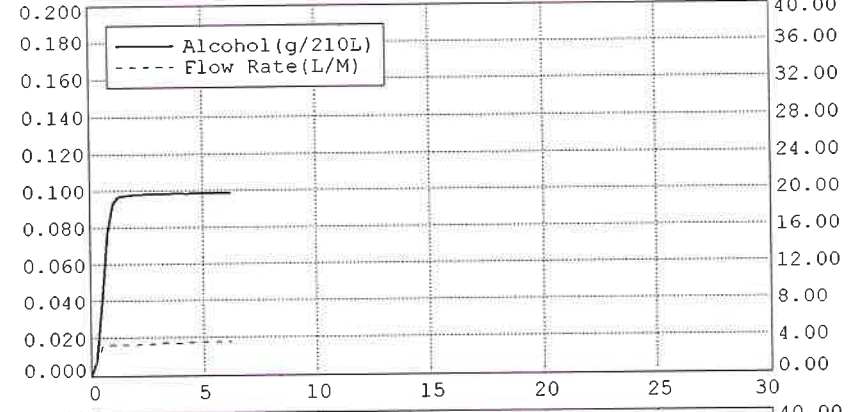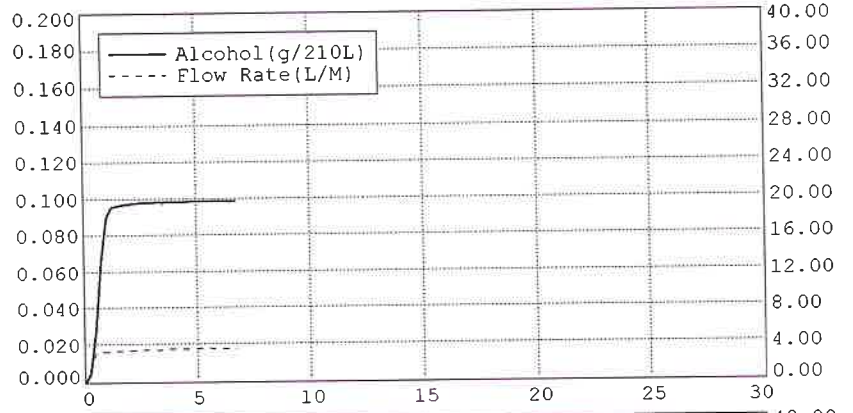

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
DATAMASTER dmt: 100342






Date: 07/15/2024  
Time: 10:38:59

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
TARGET AT 29.36: 0.147  
LOT #: AG332004  
EXPIRATION: 11/16/2025  
TANK PRESSURE: 525 psi

BLANK TEST	0.000	10:40
INTERNAL STANDARD	VERIFIED	10:40
EXTERNAL STANDARD	0.147	10:40
BLANK TEST	0.000	10:41
EXTERNAL STANDARD	0.147	10:41
BLANK TEST	0.000	10:42
EXTERNAL STANDARD	0.147	10:42
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.147	10:44
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.147	10:45
BLANK TEST	0.000	10:46

Average = 0.1470  
Std Dev = 0.0000

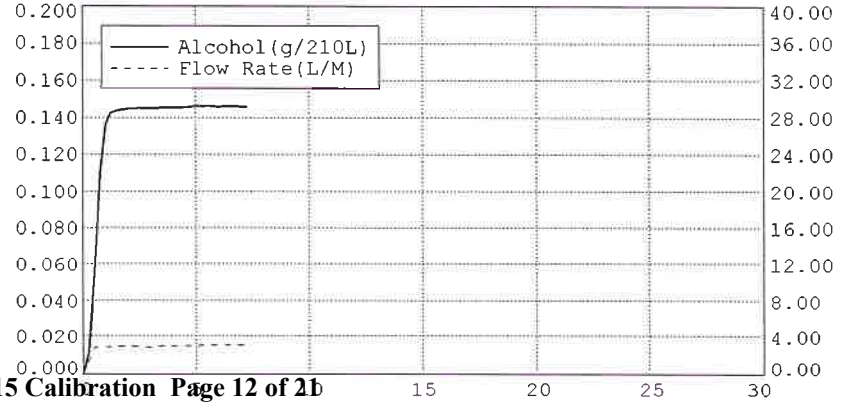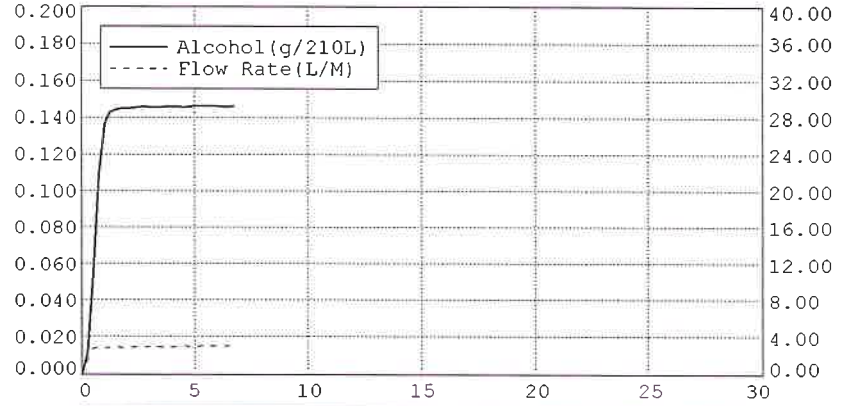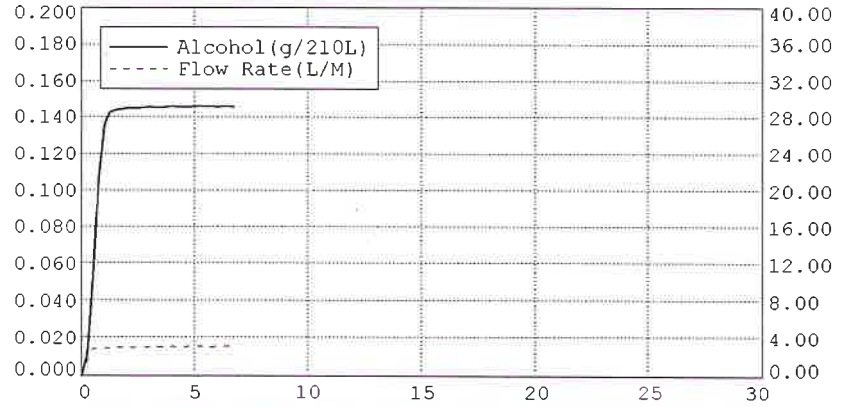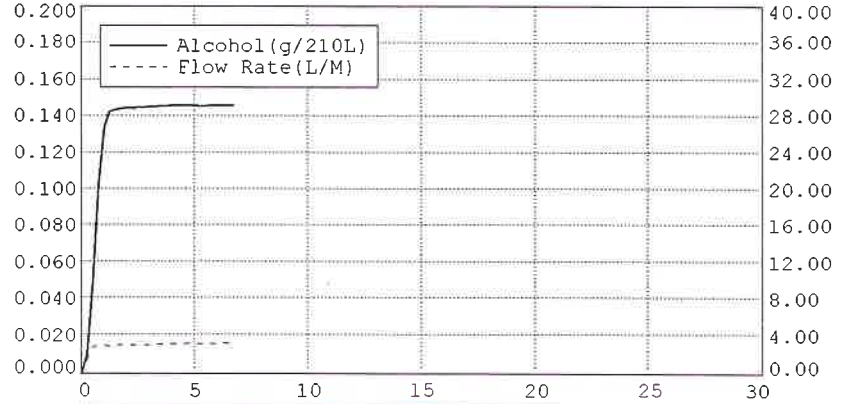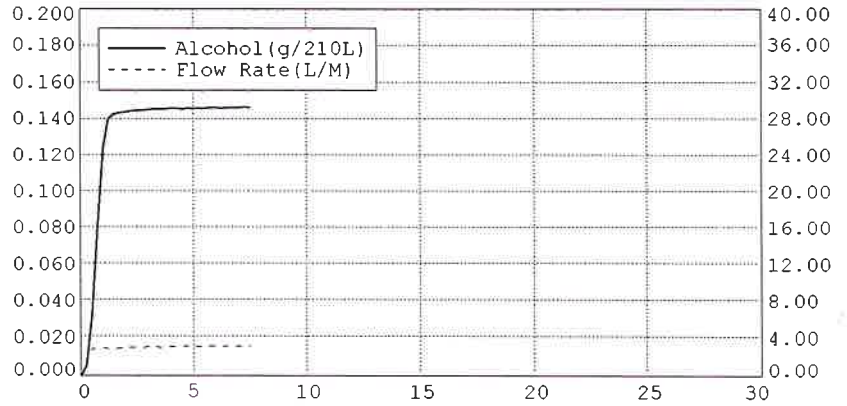

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
DATAMASTER dmt: 100342






Date: 07/15/2024  
Time: 10:48:10

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
TARGET AT 29.36: 0.294  
LOT #: AG327804  
EXPIRATION: 10/05/2025  
TANK PRESSURE: 432 psi

BLANK TEST	0.000	10:49
INTERNAL STANDARD	VERIFIED	10:49
EXTERNAL STANDARD	0.298	10:49
BLANK TEST	0.000	10:50
EXTERNAL STANDARD	0.298	10:51
BLANK TEST	0.000	10:51
EXTERNAL STANDARD	0.299	10:52
BLANK TEST	0.000	10:53
EXTERNAL STANDARD	0.298	10:53
BLANK TEST	0.000	10:54
EXTERNAL STANDARD	0.298	10:54
BLANK TEST	0.000	10:55

Average = 0.2982  
Std Dev = 0.0004

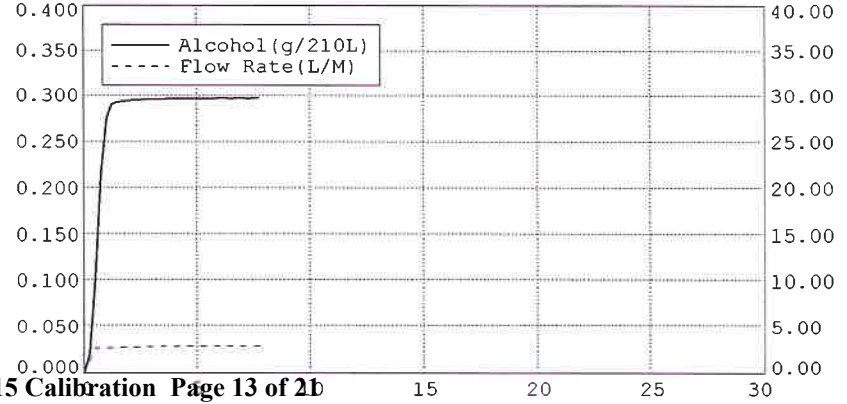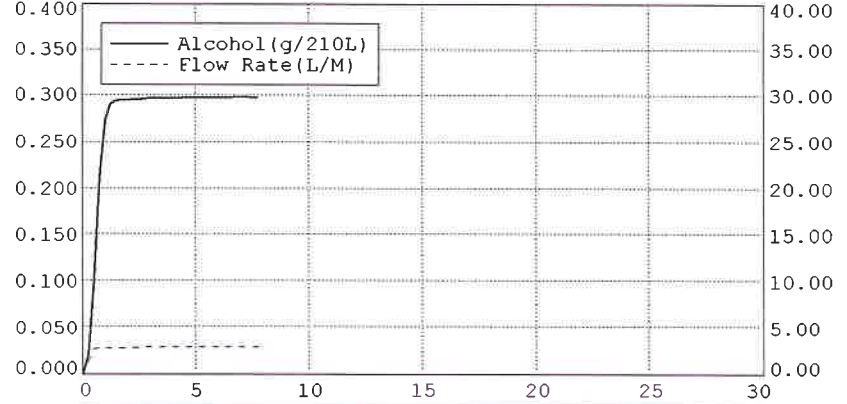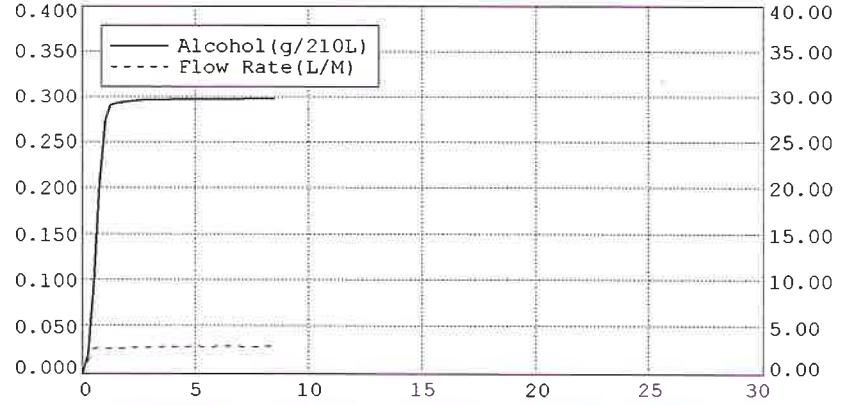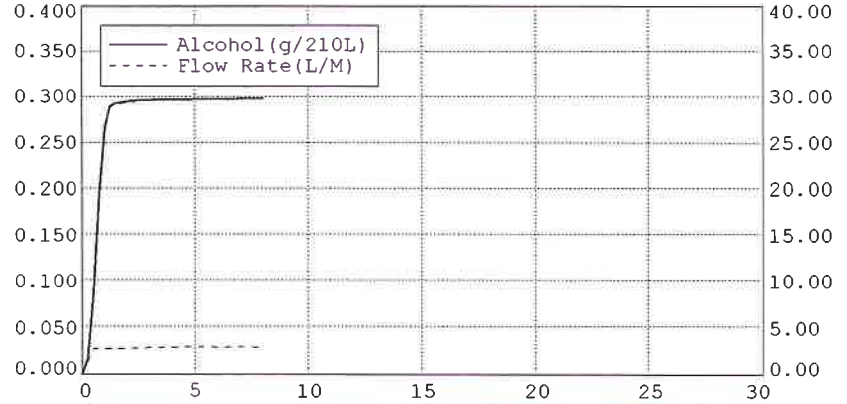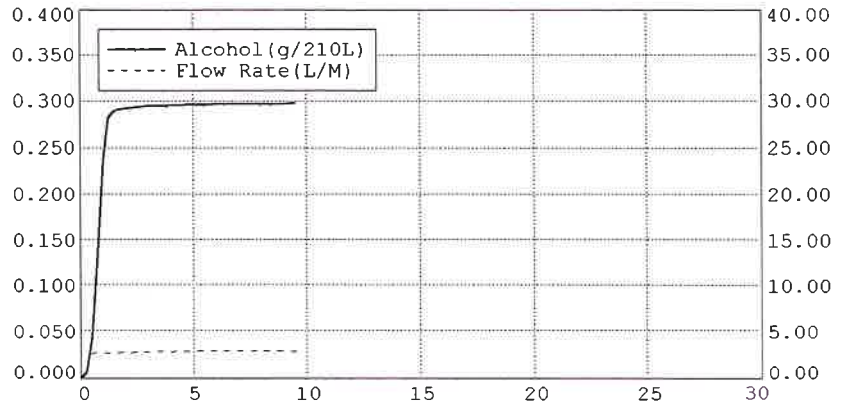

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100342

Date: 07/15/2024  
Time: 11:03:46

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.36: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:04  
BLANK TEST 0.000 11:04  
INTERNAL STANDARD VERIFIED 11:05  
EXTERNAL STANDARD 0.080 11:05  
BLANK TEST 0.000 11:06  
SUBJECT SAMPLE INCOMPLETE 11:08

KS

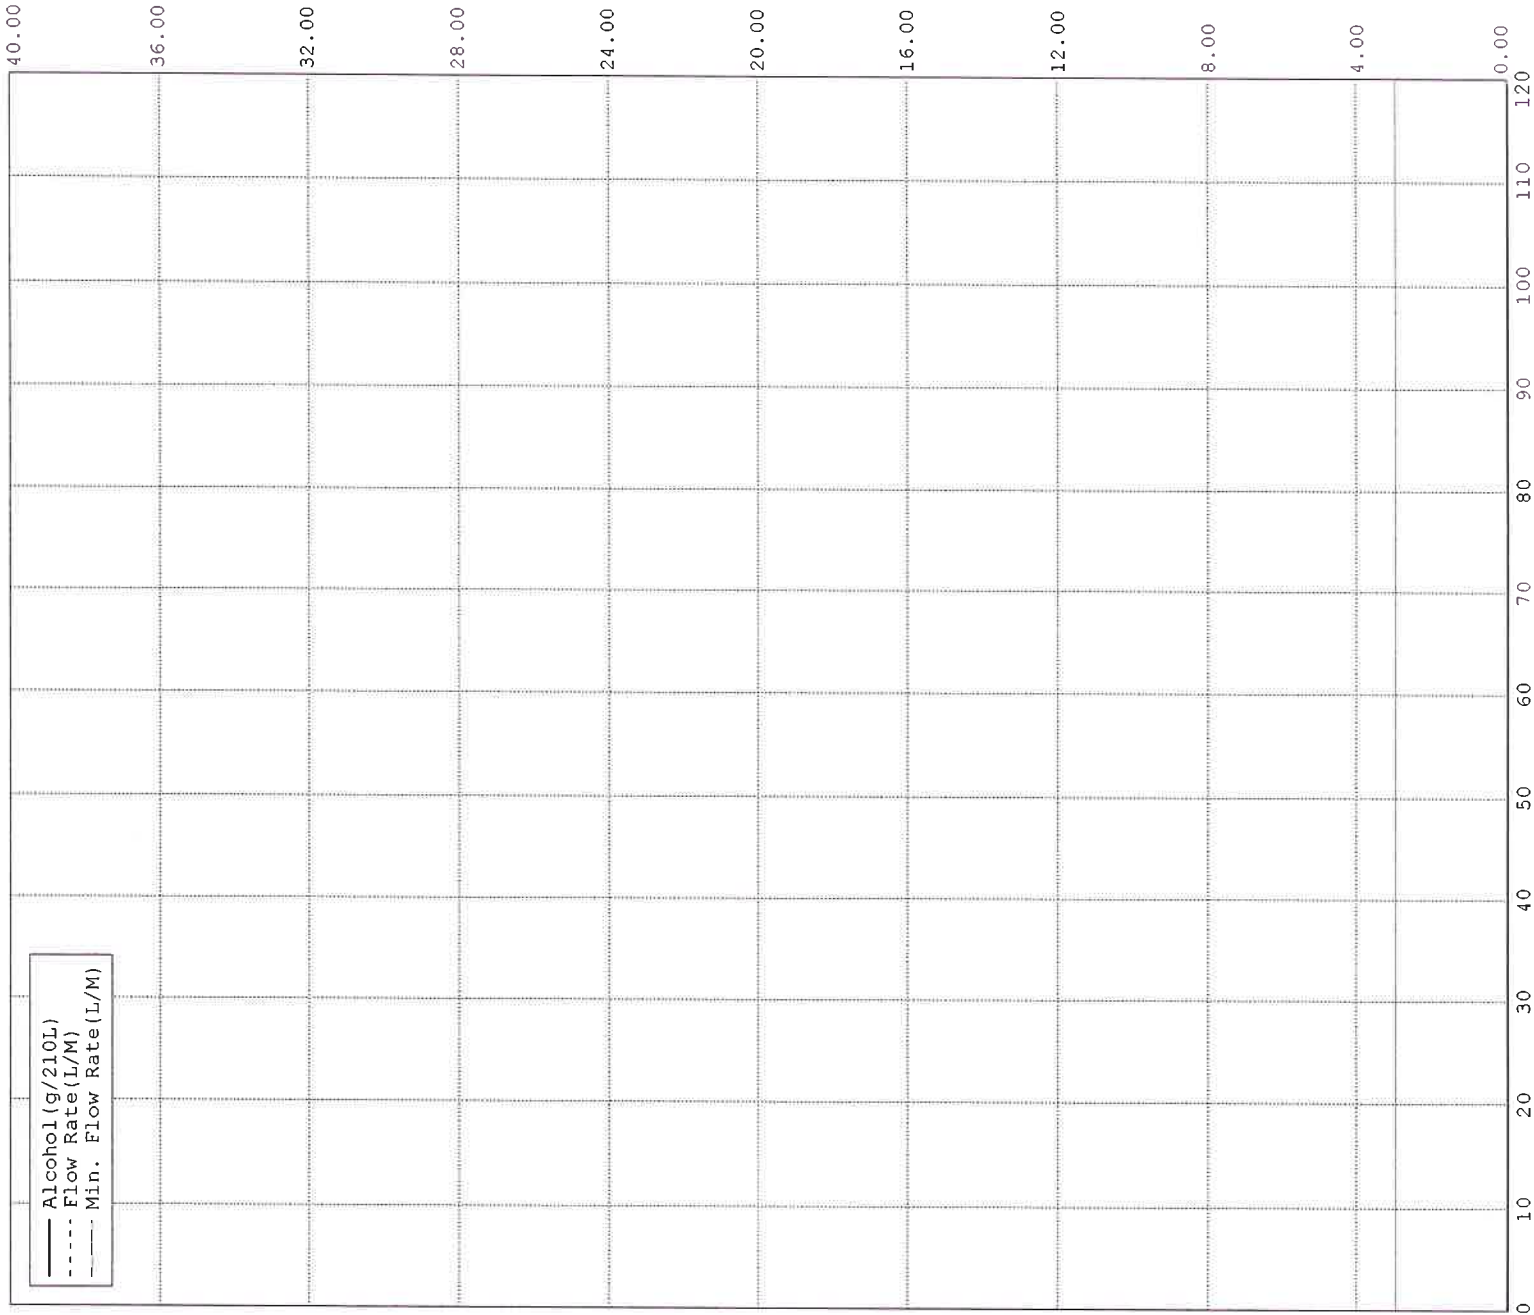

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100342

Date: 07/15/2024

Time: 11:19:44

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

MAXIMUM ATTEMPTS EXCEEDED

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.36: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:20

BLANK TEST 0.000 11:20


INTERNAL STANDARD VERIFIED 11:20

EXTERNAL STANDARD 0.080 11:21

BLANK TEST 0.000 11:22

SUBJECT SAMPLE XXX 11:22

Maximum Attempts Exceeded

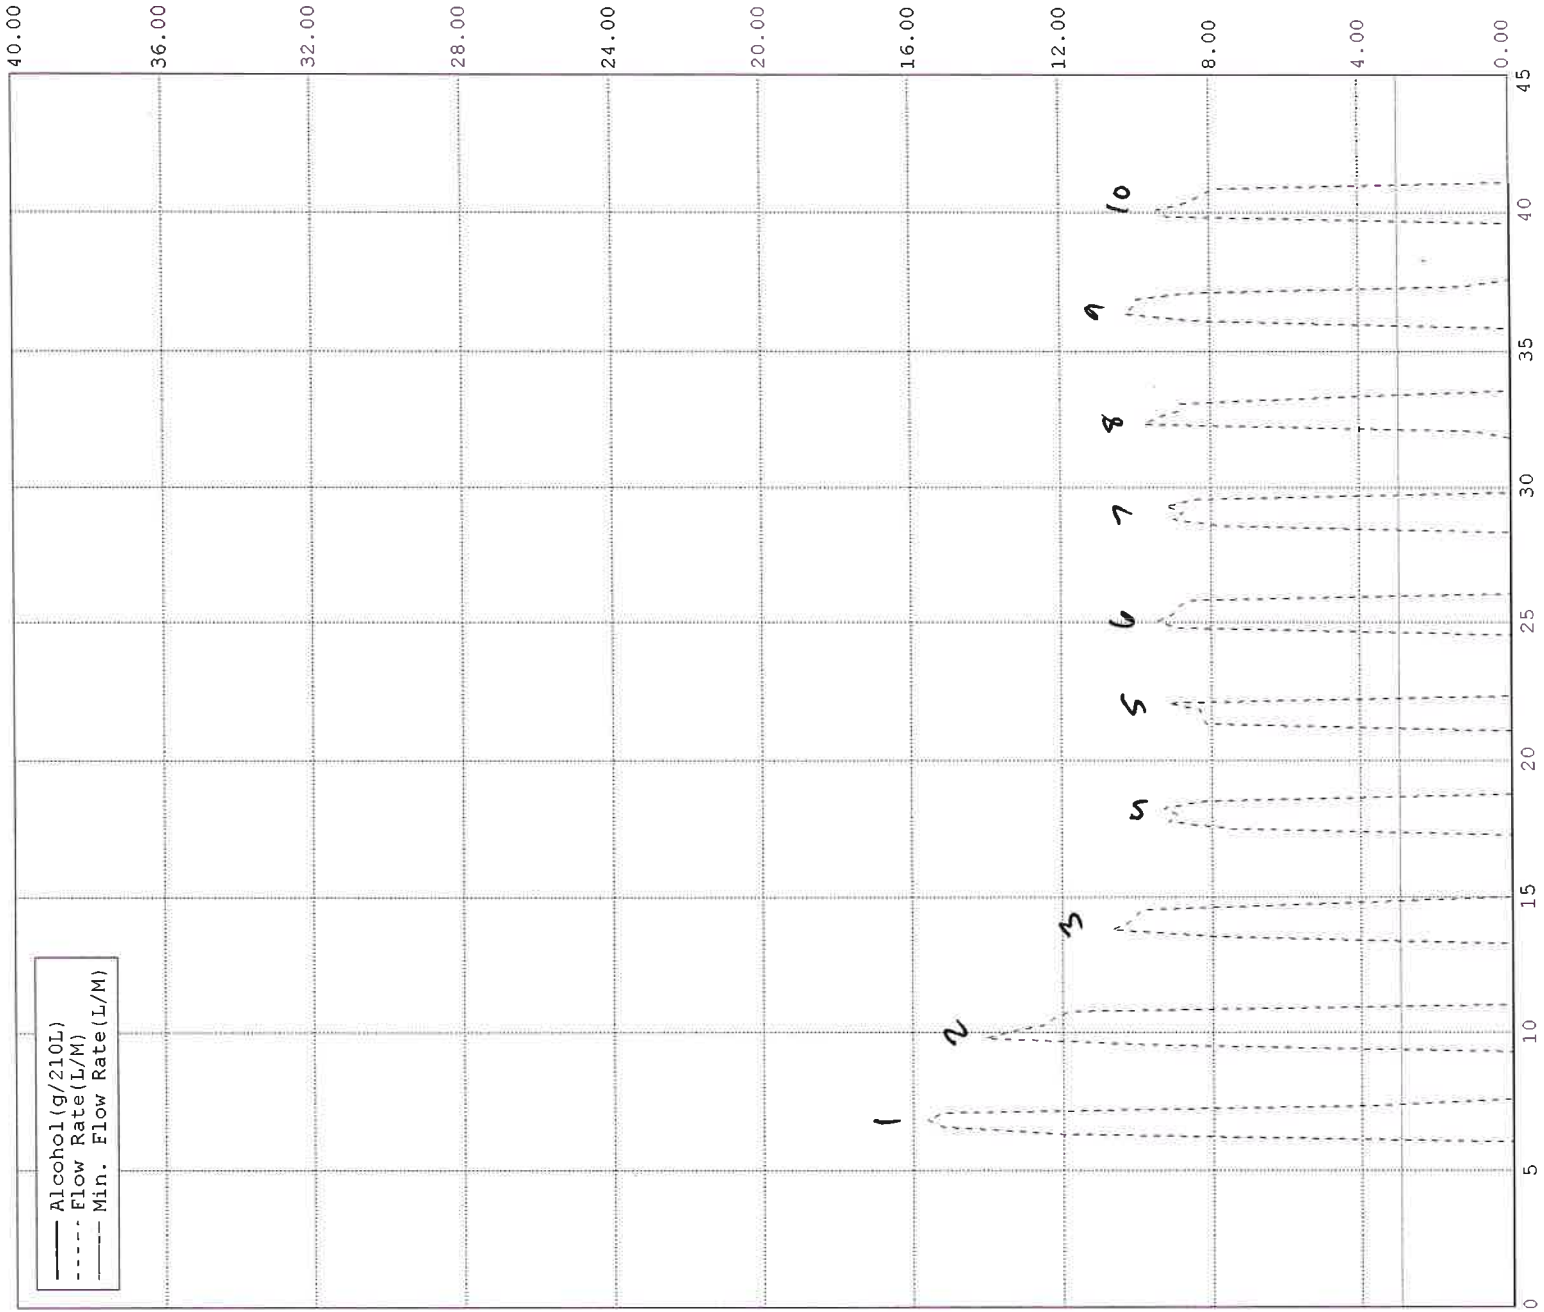

KS

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100342

Date: 07/15/2024

Time: 11:25:02

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

INVALID

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.35: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:26

BLANK TEST 0.000 11:26


INTERNAL STANDARD VERIFIED 11:26

EXTERNAL STANDARD 0.079 11:26

BLANK TEST 0.000 11:27

SUBJECT SAMPLE INVALID 11:28

VS

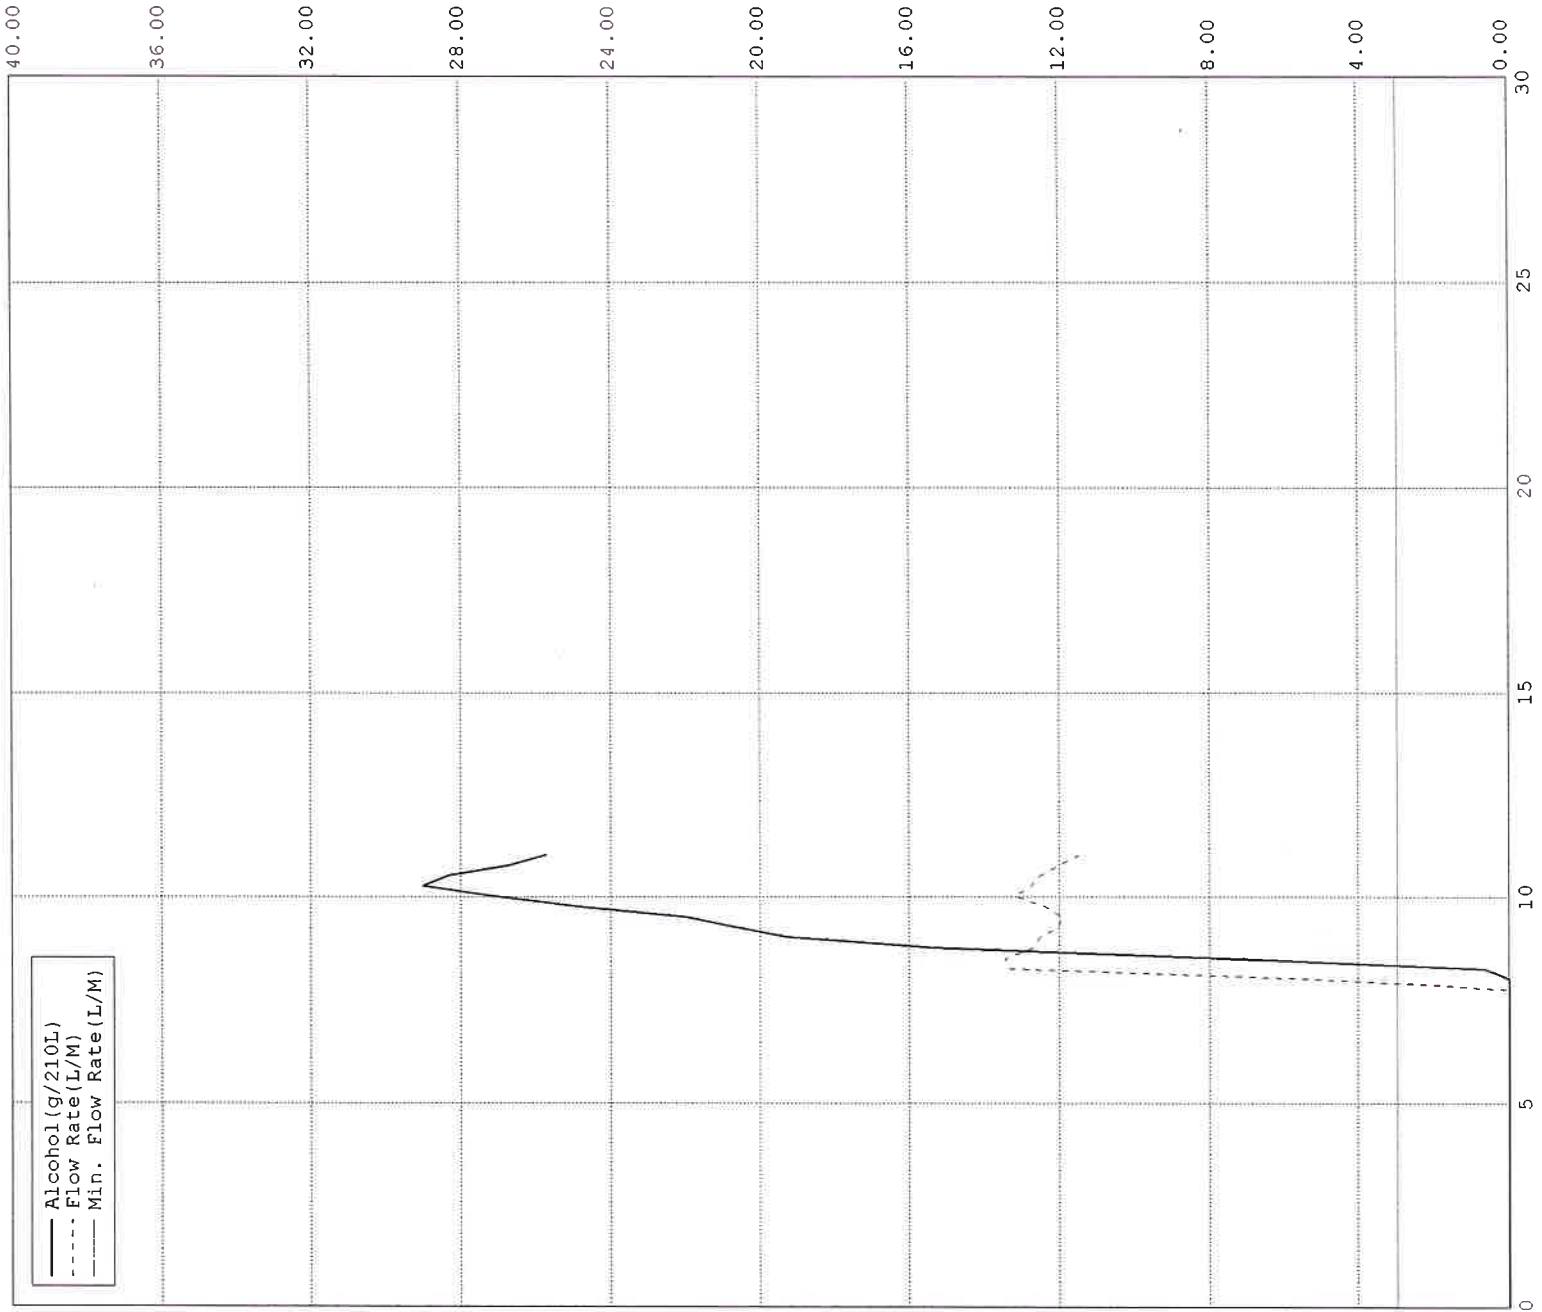



SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100342

Date: 07/15/2024

Time: 11:30:05

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

RFI

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.35: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

PASSED 11:31  
0.000 11:31  
VERIFIED 11:31  
0.079 11:31  
0.000 11:32

RFI DETECTED

KS

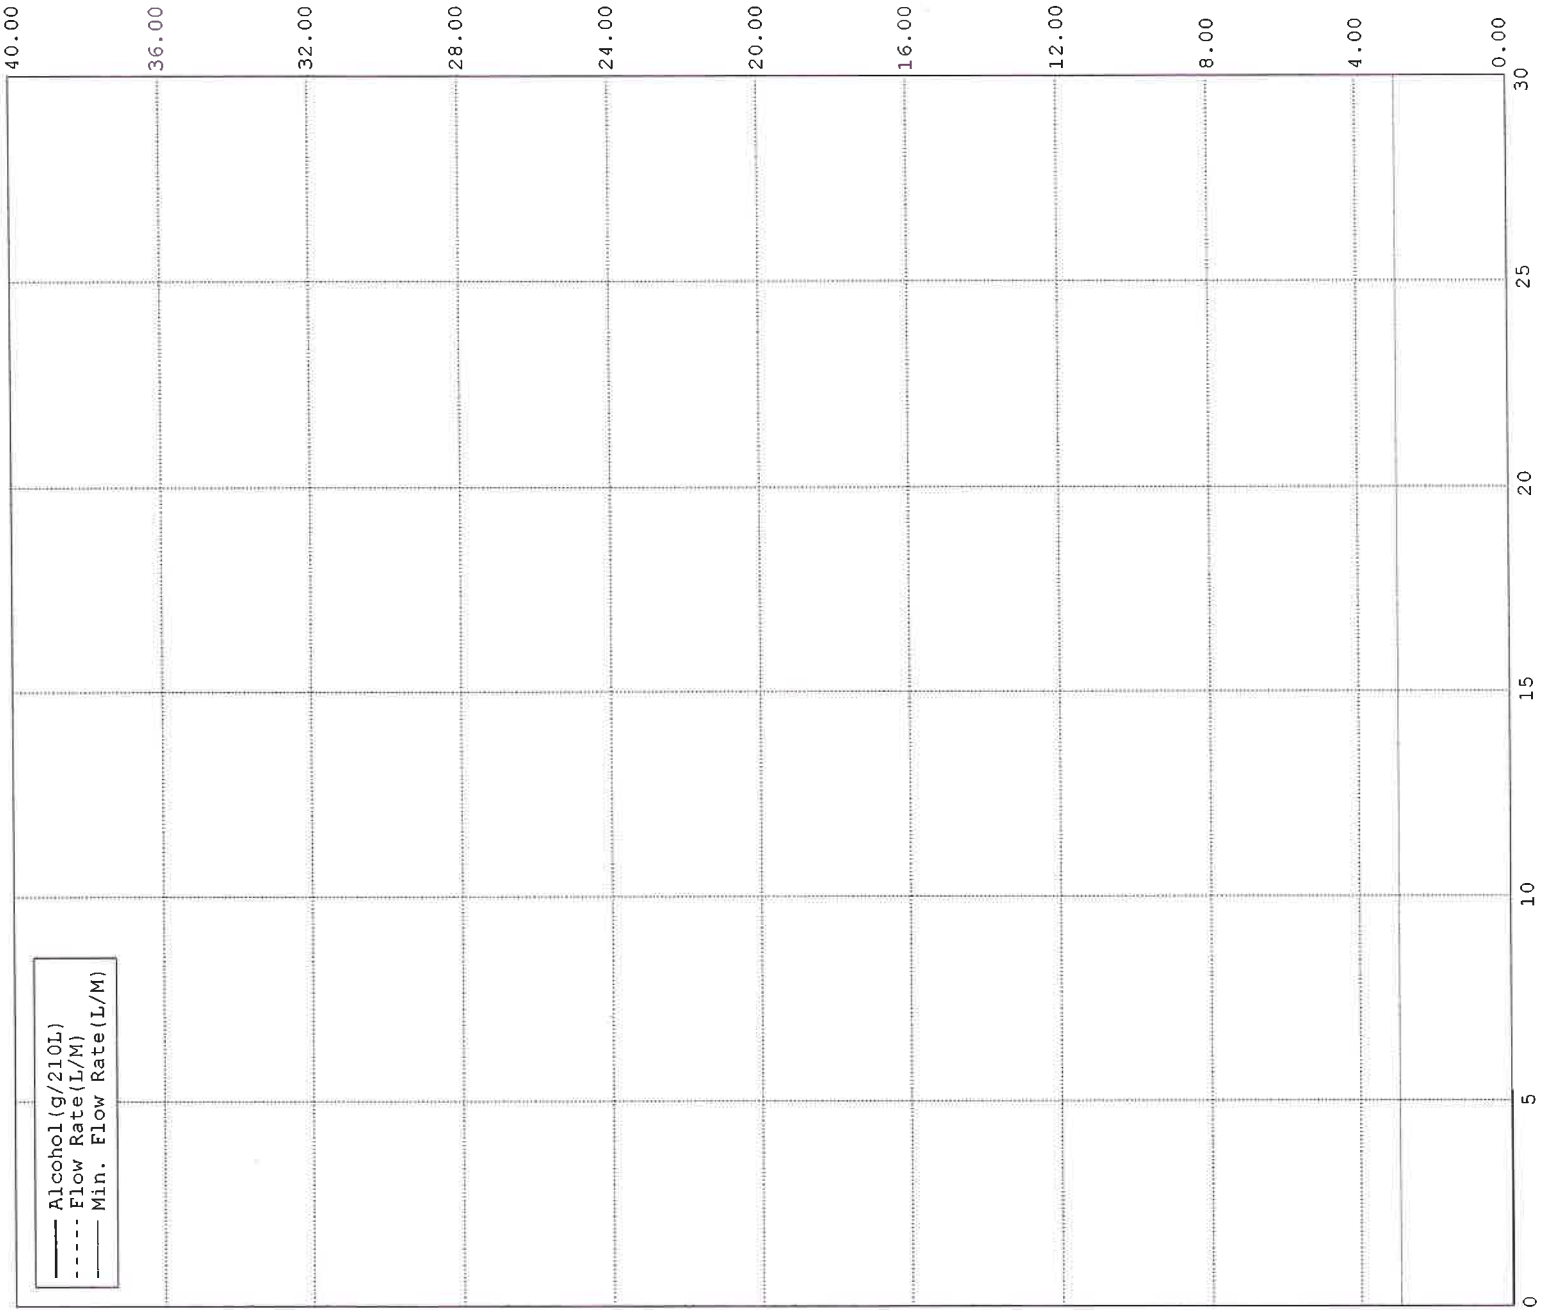

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100342

Date: 07/15/2024  
Time: 12:09:19

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAJJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
ACETONE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 12:10  
BLANK TEST 0.000 12:10  
INTERNAL STANDARD VERIFIED 12:10  
Xq = 0.086 (0.31%)  
EXTERNAL STANDARD 0.079 12:10  
X[l] = 0.0793 (-0.0003) (0.0027)  
BLANK TEST 0.000 12:11  
SUBJECT SAMPLE XXX 12:12  
X[i] = 0.1039 (-0.0135) (0.0023)

Interference Detected


Filter 2ave: 0.0001

Filter 3ave: 0.0020

KS 7/15/24

*Jm 07/15/24*

KS

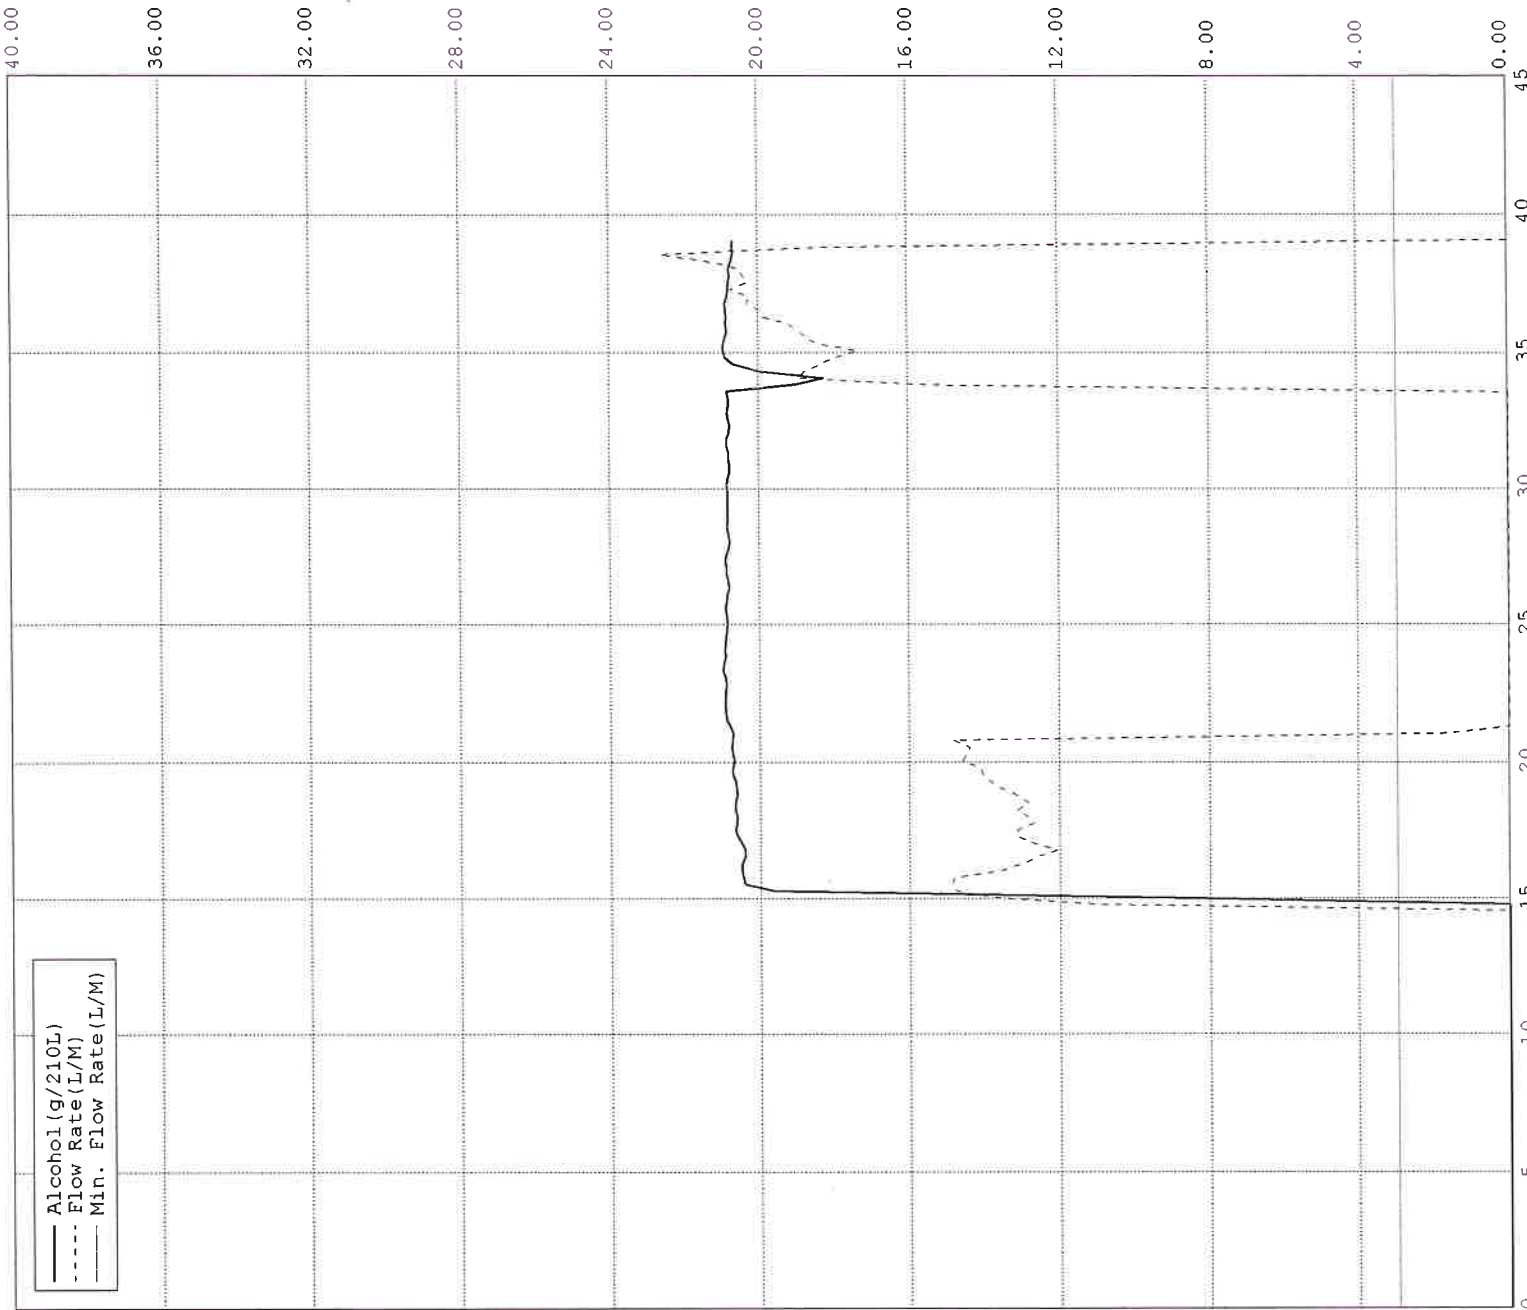

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100342

Date: 07/15/2024  
Time: 12:14:17

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
IPA

CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.35: 0.078  
LOF #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:15
BLANK TEST	0.000	12:15
INTERNAL STANDARD	VERIFIED	12:15
Xg = 0.086 (0.31%)		
EXTERNAL STANDARD	0.079	12:15
X[1] = 0.0792 (0.0003) (0.0014)		
BLANK TEST	0.000	12:16
SUBJECT SAMPLE	XXX	12:17
X[1] = 0.1063 (-0.0270) (0.0007)		

Interference Detected



KS

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100342

Date: 07/15/2024

Time: 12:19:01

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

NEGATIVE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.34: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	TIME
BLANK TEST	0.000	12:20
INTERNAL STANDARD	VERIFIED	12:20
Xq = 0.086 (0.31%)		
EXTERNAL STANDARD	0.079	12:20
X[1] = 0.0793 (0.0004) (0.0022)		
BLANK TEST	0.000	12:21
SUBJECT SAMPLE (Vol=1.66L)	0.087	12:22
X[1] = 0.0877 (-0.0015) (0.0016)		
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.079	12:23
X[1] = 0.0793 (-0.0002) (0.0015)		
BLANK TEST	0.000	12:24

VS

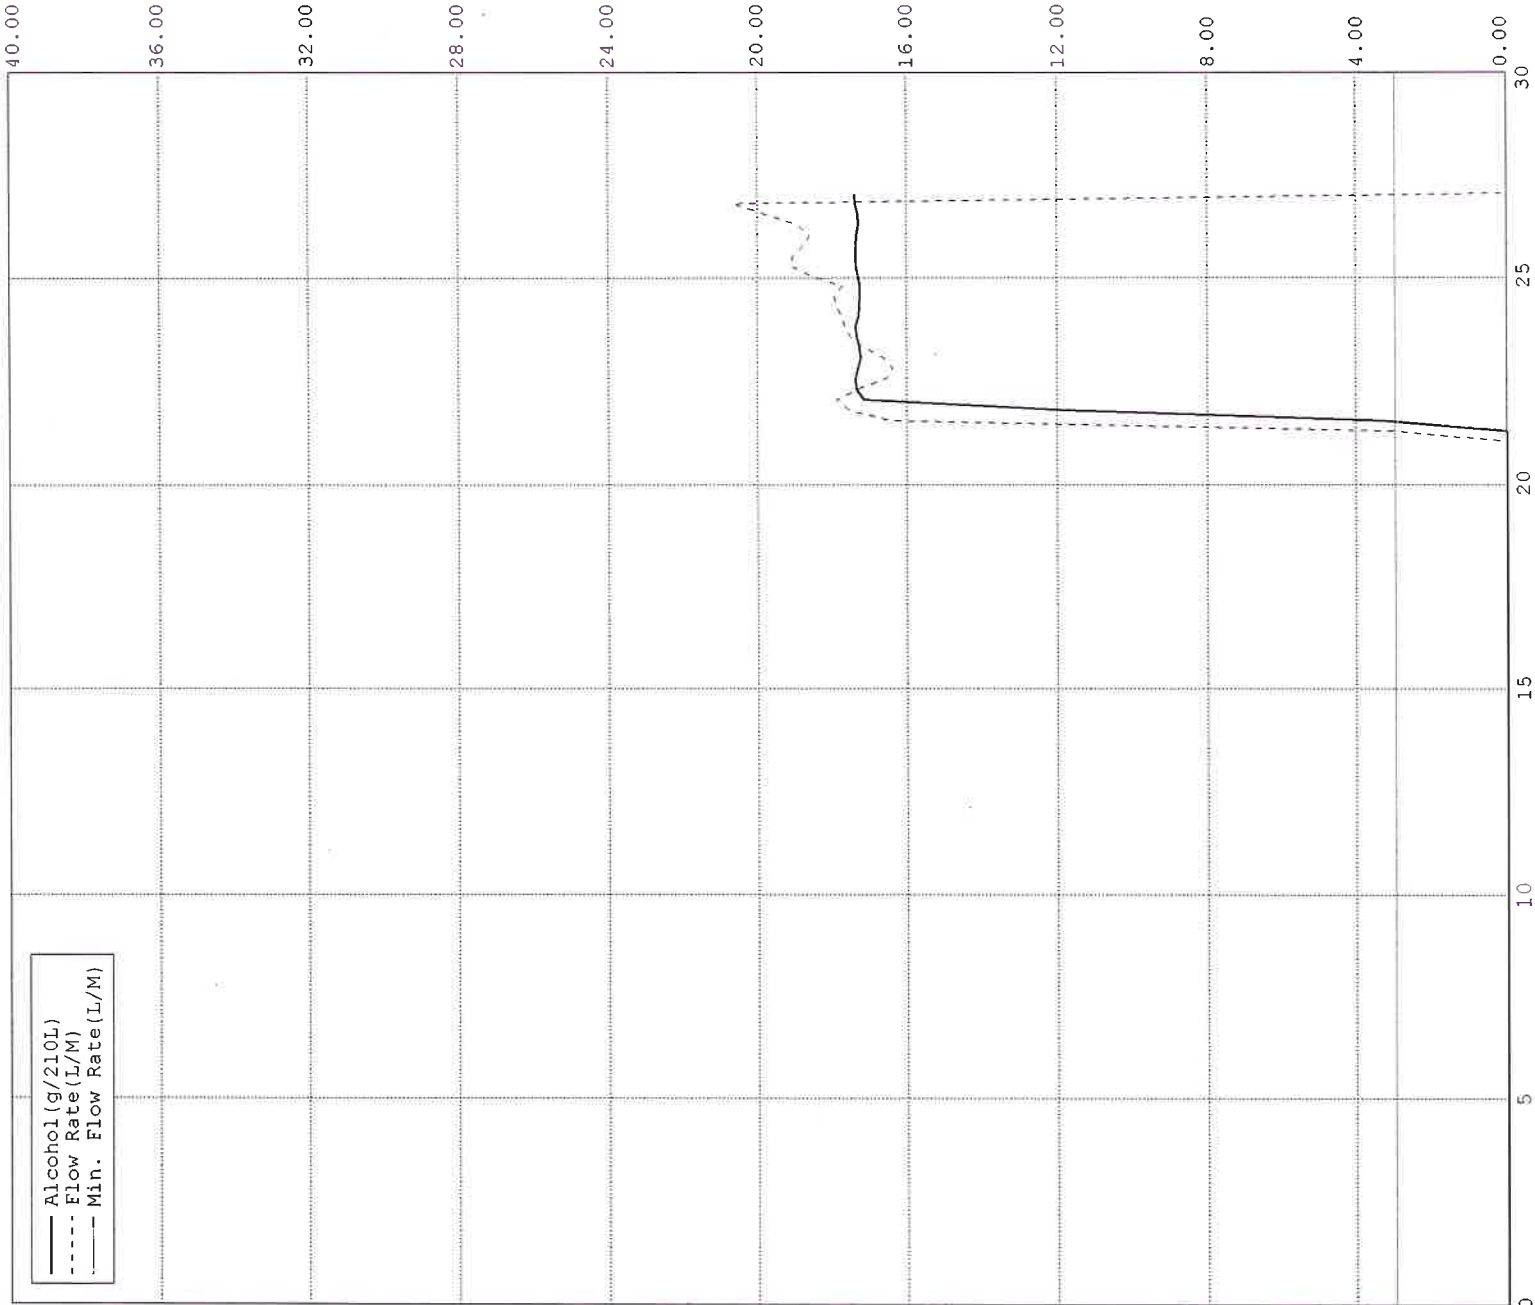

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100342

Date: 07/15/2024

Time: 12:38:17

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

NON-DRINKING SUBJECT TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.35: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:39
BLANK TEST	0.000	12:39
INTERNAL STANDARD	VERIFIED	12:39
EXTERNAL STANDARD	0.080	12:39
BLANK TEST	0.000	12:40
SUBJECT SAMPLE (Vol=1.75L)	0.000	12:41
BLANK TEST	0.000	12:41
EXTERNAL STANDARD	0.080	12:42
BLANK TEST	0.000	12:43

✓

