

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100413

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 01/10/2013

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.00: 0.080
LOT #: 22612080A1
EXPIRATION: 09/01/2014

BLANK TEST	0.000	13:31
INTERNAL STANDARD	VERIFIED	13:31
EXTERNAL STANDARD	0.079	13:31
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.079	13:32
BLANK TEST	0.000	13:33
EXTERNAL STANDARD	0.078	13:33
BLANK TEST	0.000	13:34
EXTERNAL STANDARD	0.079	13:35
BLANK TEST	0.000	13:36
EXTERNAL STANDARD	0.079	13:36
BLANK TEST	0.000	13:37

Average = 0.0788
Std Dev = 0.0004

Diagnostic Check

VERSIONS

DMT: 2.00
PIC: 3.02
Modem: 2.3
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.6°C PASSED
Breath Tube = 44.1°C PASSED

PUMP INFO

Flow Rate = 4.918 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

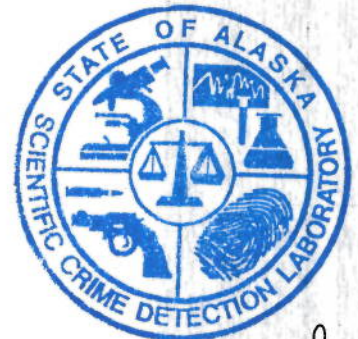


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

1/23/2013

Subscribed and sworn before me this 23 day of Jan, 20 13



Nikki Roth, Notary Public
My Commission Expires With Office



BMB
1/15/13