



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100368

Report Issue Date: 07/10/2024
Date Received: 2023-10-23
Condition of Item: Good

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG217902	0.019	0.019	0.019	0.019	0.019	0.019
0.080	0.078	AG310901	0.074	0.074	0.074	0.074	0.074	0.074
0.300	0.293	AG217903	0.281	0.280	0.280	0.279	0.280	0.280

As Found - Evaluation Analyst: Carlie Glaister
 As Found Conditions - Barometric Pressure (inHg): 29.13 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.7 Relative Humidity (%): 24
 As-Found Lab Activity Date Range: 11/06/2023 - 11/06/2023

Replaced o-ring. As found passed, recommending adjustment due to 0.080 & 0.300 standards reading close to 5%.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG217904	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.079	AG310901	0.078	0.077	0.077	0.078	0.078	0.078	+/- 0.004
0.100	0.099	AG333401	0.099	0.099	0.099	0.099	0.099	0.099	+/- 0.004
0.150	0.149	AG332004	0.147	0.146	0.146	0.147	0.146	0.146	+/- 0.005
0.300	0.298	AG327804	0.297	0.297	0.296	0.297	0.297	0.297	+/- 0.011

As Left Conditions - Barometric Pressure (inHg): 29.75 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.3 Relative Humidity (%): 41
 As-Left Lab Activity Date Range: 06/07/2024 - 06/14/2024

Supervised casework with Megan Carlock.

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Derek Walton on 06/21/2024

derek.walton@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 07/10/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100368 Analyst or Technician Name: Megan Cartack

DataMaster DMT Calibration Start Date: 6/7/24

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

*Supervised casework
with Derek Watson*

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: 05/02/2025
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

06/14/24 JMW

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.75 Temperature(C) 20.3 Relative Humidity(%) 41
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20240501KS Expiration Date: 08/01/2024
Simulator S/N: SD1088 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20240501MNC Expiration Date: 08/01/2024
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 22HP41201 Expiration Date: 08/24/2024
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 09/19/2025

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 6/7/24
Data Interpretation Date (Technician): N/A (if applicable)
Data Interpretation Date (Analyst): 6/7/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100368

Date: 06/07/2024
Time: 10:28:40

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 42.9°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.65 V PASSED
(0.97 V - 2.27 V)
Cooler Voltage = 1.71 V PASSED
(1.03 V - 2.39 V)
Bias Voltage = 79 V PASSED
(47 V - 111 V)
Chopper Freq = 539 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 30.0 in

PUMP INFO

Flow Rate = 4.729 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 v <= 0.010 v)
PUMP OFF PASSED
(0.002 v <= 0.010 v)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.076 0.23% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100368

Date: 06/07/2024
Time: 10:40 AM

Temperatures (°C)

Sample Cell: 48.9°C
Breath Tube: 40.6°C

Current Barometer 29.7 in
Volume (Ltr) 1.55

Settings

Lamp: 1.70 V
Bias: 79 V
Cooler: 1.71 V
Chopper: 548 Hz

Voltages (V)

Flow: 1.07 V
Detector: -0.021 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100368

Date: 04/29/2024
Time: 13:57:18

OPERATOR NAME:
COLLEEN S OBRYANT
CERTIFICATE #: 6237

Ca = 0.1000
CAL = 0.930620 0.800 <= CAL < 1.200
b1 = 0.0004 0.0000 <= b1 < 0.0040
b2 = 0.0060 0.0010 <= b2 < 0.0100
b3 = 0.0004 0.0000 <= b3 < 0.0040
Xq = 0.0759 0.0500 <= Xq < 0.2000
a21 = 1.183378 1.050 <= a21 < 1.300
a31 = 0.431992 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100368

Date: 06/07/2024
 Time: 10:44:58

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX


OPERATOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

DEPT/AGENCY:
 MINIMUM VOLUME TEST
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.72: 0.079
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	10:45
BLANK TEST	0.000	10:46
INTERNAL STANDARD	VERIFIED	10:46
EXTERNAL STANDARD	0.078	10:46
BLANK TEST	0.000	10:47
SUBJECT SAMPLE (Vol=1.61L)	0.000	10:48
BLANK TEST	0.000	10:49
EXTERNAL STANDARD	0.078	10:49
BLANK TEST	0.000	10:50

MNC

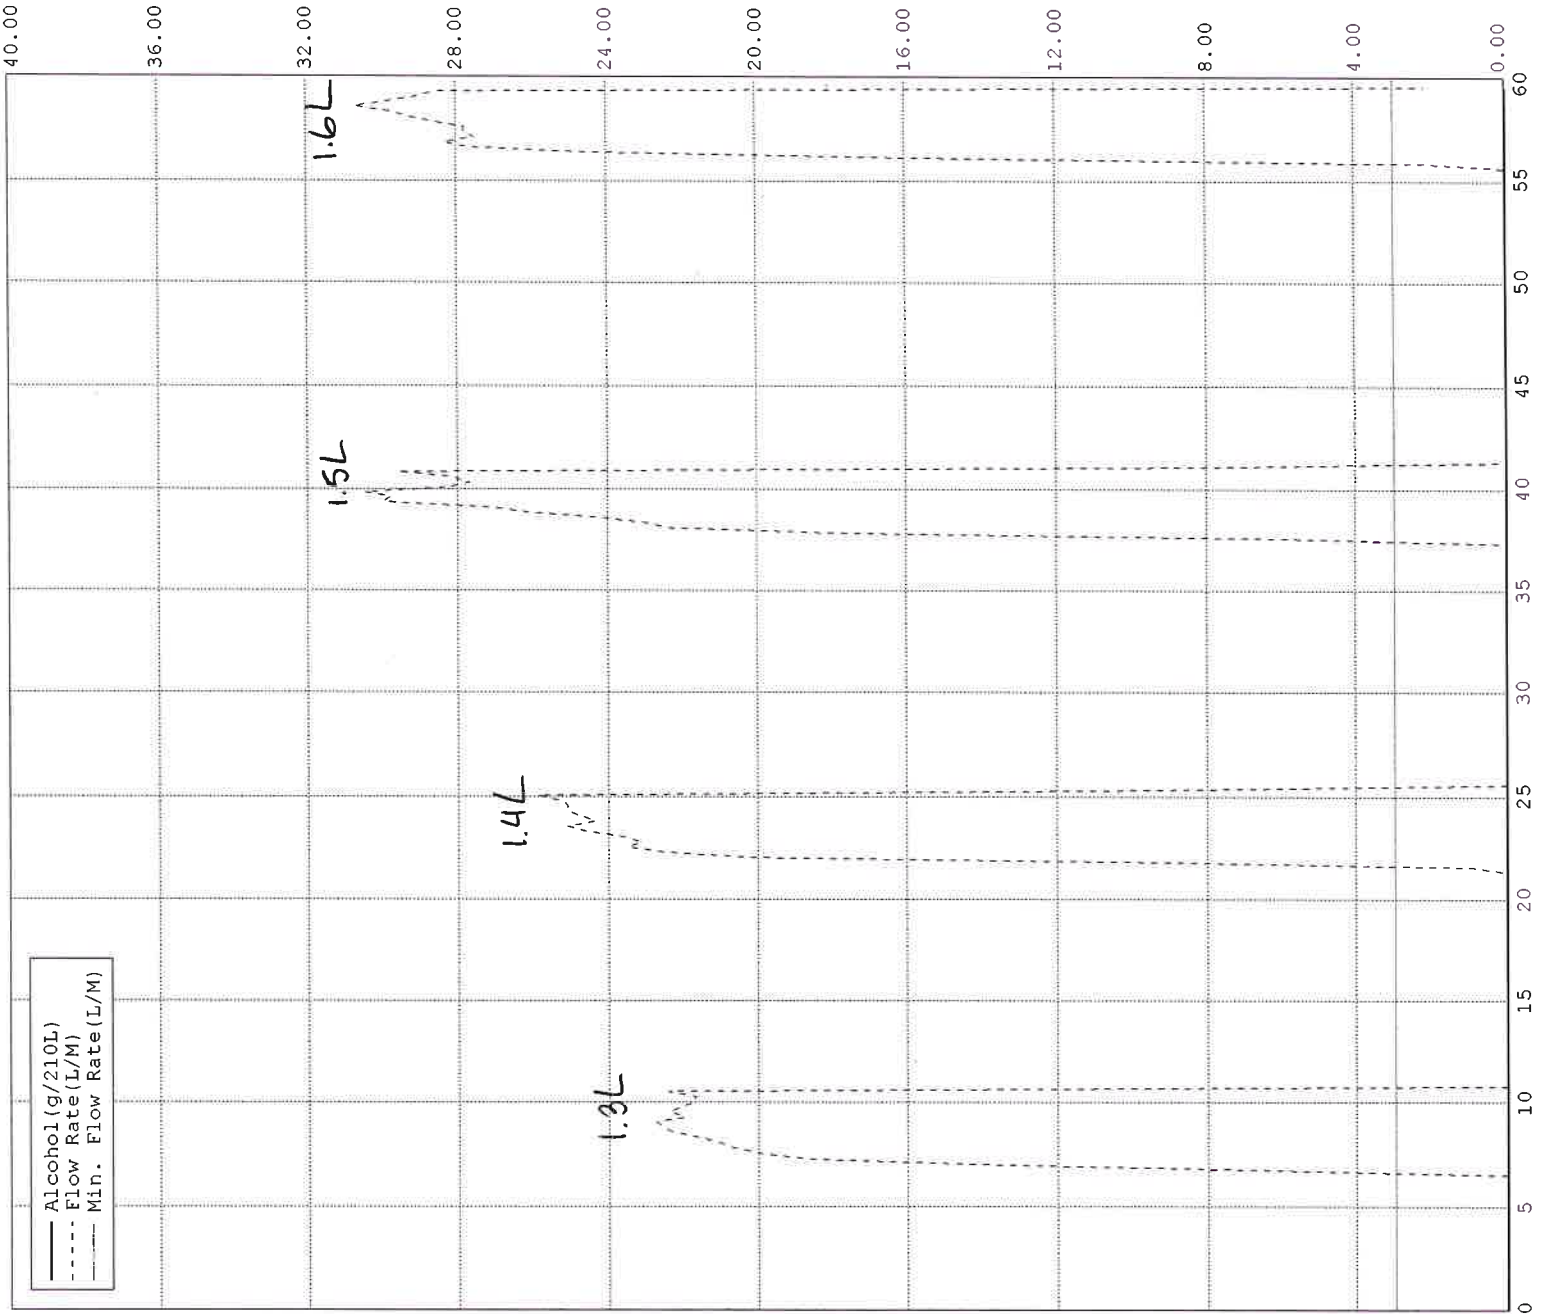

LINEARITY CHECK


Alaska Department of Public Safety
 DATAMASTER dmt: 100368

Date: 06/07/2024
 Time: 10:53:41

SUPERVISOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.040	0.0400	0.0000
0.079	0.0776	0.0005
0.099	0.0990	0.0000
0.149	0.1464	0.0005
0.298	0.2968	0.0004

SLOPE = 0.994848
 SLOPE² = 0.999914

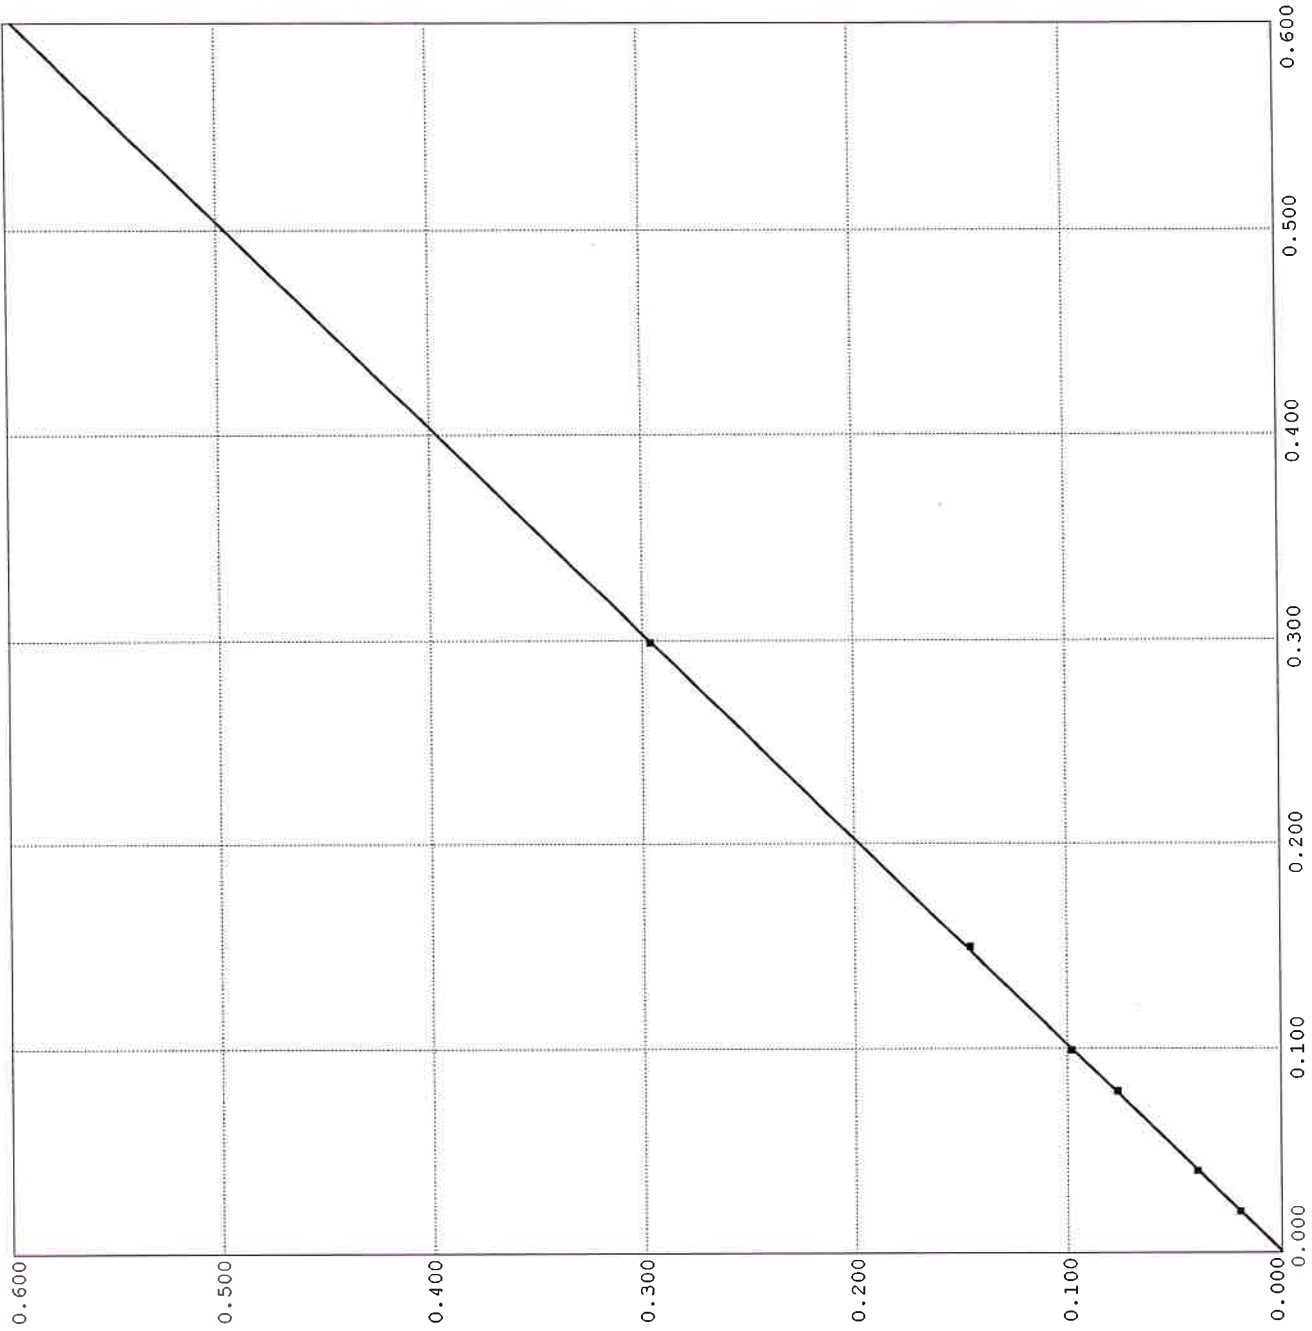

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100368






Date: 06/07/2024
 Time: 10:57:04

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.71: 0.020
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 410 psi

BLANK TEST	0.000	10:58
INTERNAL STANDARD	VERIFIED	10:58
EXTERNAL STANDARD	0.020	10:58
BLANK TEST	0.000	10:59
EXTERNAL STANDARD	0.020	10:59
BLANK TEST	0.000	11:00
EXTERNAL STANDARD	0.020	11:00
BLANK TEST	0.000	11:01
EXTERNAL STANDARD	0.020	11:01
BLANK TEST	0.000	11:02
EXTERNAL STANDARD	0.020	11:02
BLANK TEST	0.000	11:03

Average = 0.0200
 Std Dev = 0.0000

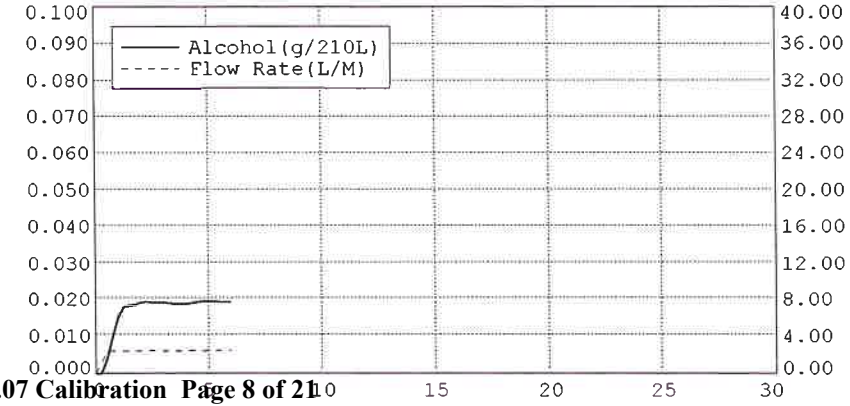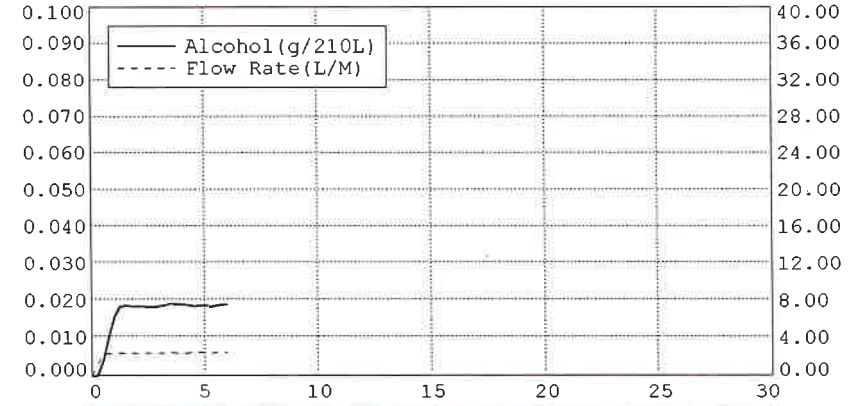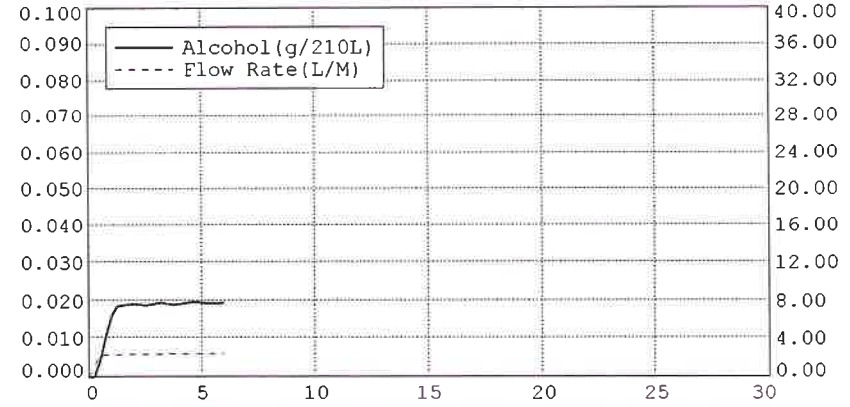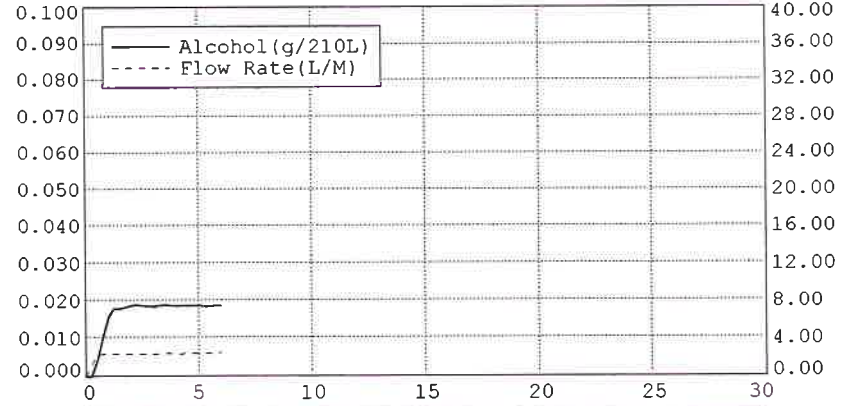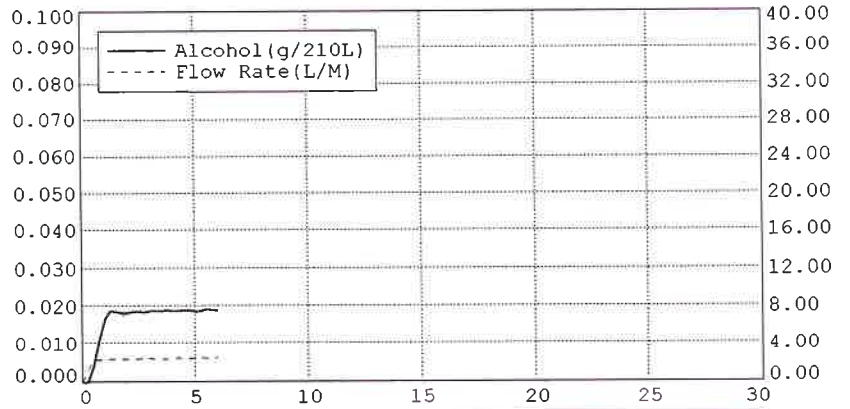

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100368






Date: 06/07/2024
Time: 11:06:07

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.72: 0.040
LOT #: AG217904
EXPIRATION: 06/28/2024
TANK PRESSURE: 627 psi

BLANK TEST	0.000	11:07
INTERNAL STANDARD	VERIFIED	11:07
EXTERNAL STANDARD	0.040	11:07
BLANK TEST	0.000	11:08
EXTERNAL STANDARD	0.040	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.040	11:10
BLANK TEST	0.000	11:10
EXTERNAL STANDARD	0.040	11:11
BLANK TEST	0.000	11:12
EXTERNAL STANDARD	0.040	11:12
BLANK TEST	0.000	11:13

Average = 0.0400
Std Dev = 0.0000

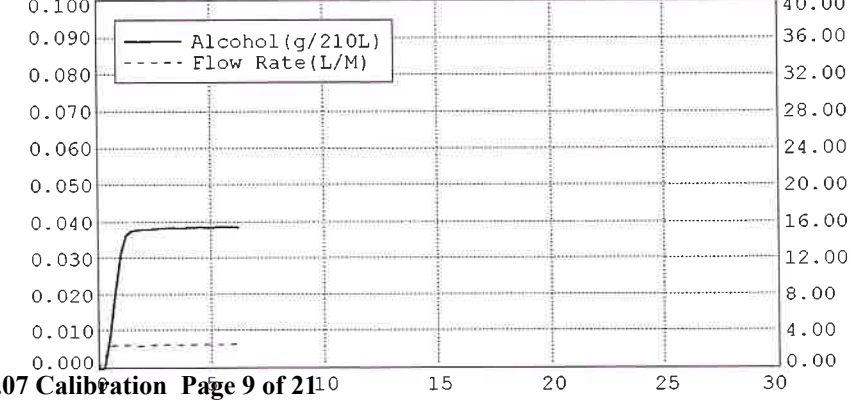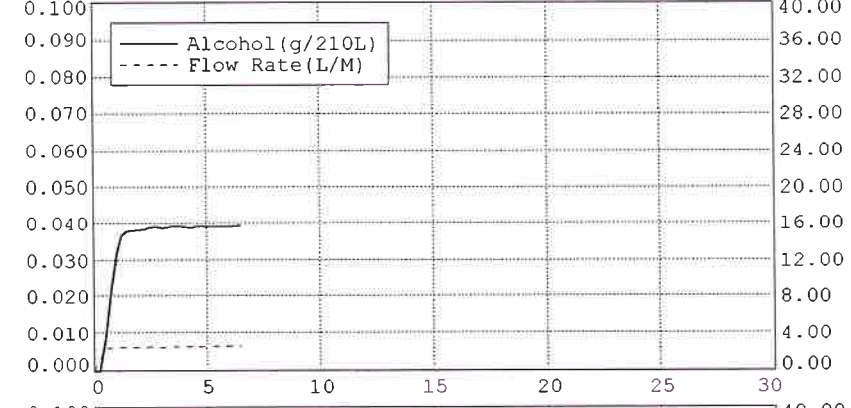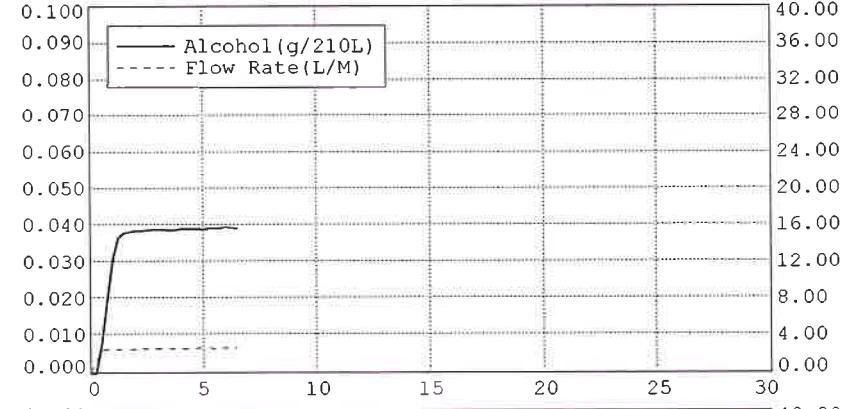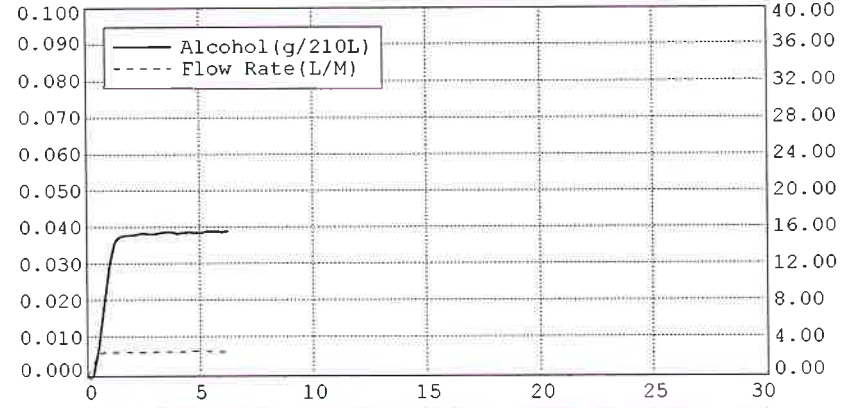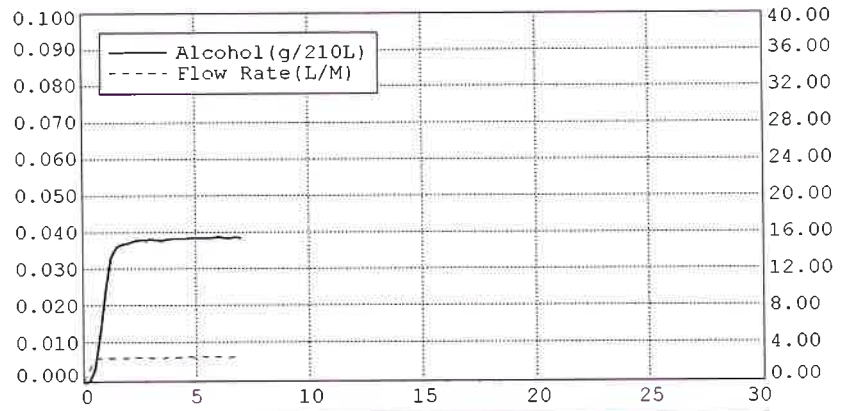

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100368






Date: 06/07/2024
 Time: 11:13:55

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.71: 0.079
 LOT #: AG310901
 EXPIRATION: 04/19/2025
 TANK PRESSURE: 127 psi

BLANK TEST	0.000	11:15
INTERNAL STANDARD	VERIFIED	11:15
EXTERNAL STANDARD	0.078	11:15
BLANK TEST	0.000	11:16
EXTERNAL STANDARD	0.077	11:16
BLANK TEST	0.000	11:17
EXTERNAL STANDARD	0.077	11:17
BLANK TEST	0.000	11:18
EXTERNAL STANDARD	0.078	11:18
BLANK TEST	0.000	11:19
EXTERNAL STANDARD	0.078	11:20
BLANK TEST	0.000	11:21

Average = 0.0776
 Std Dev = 0.0005

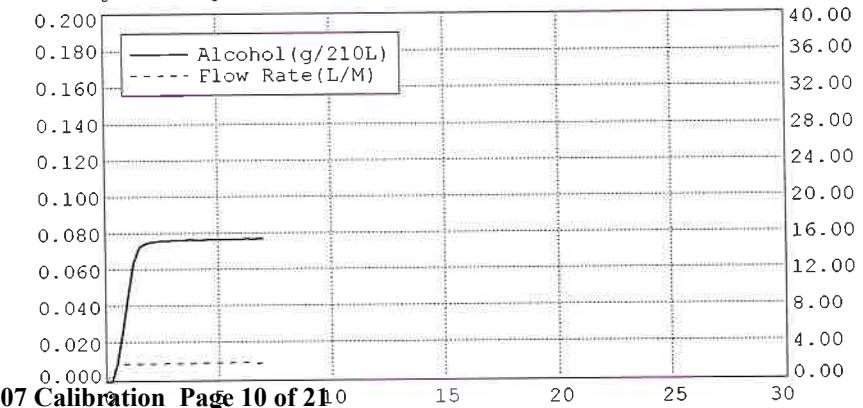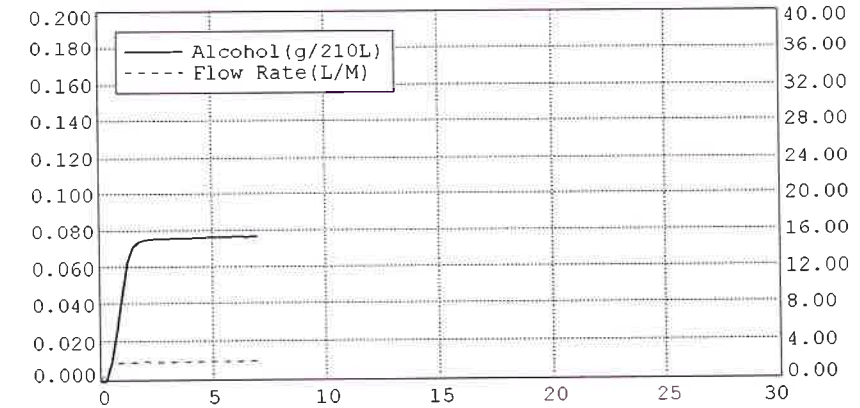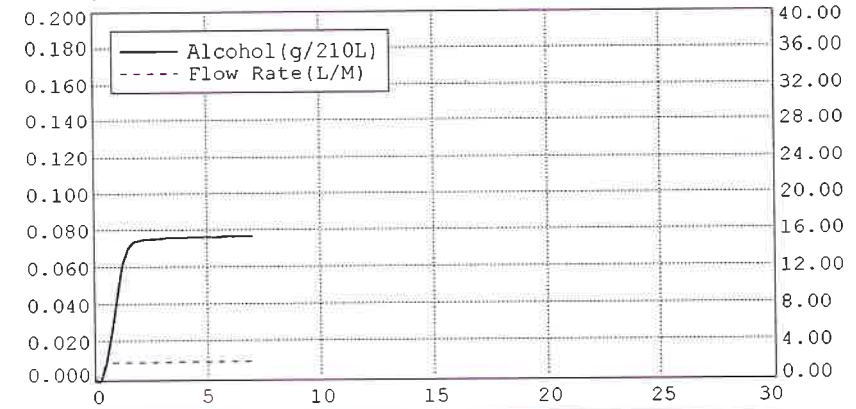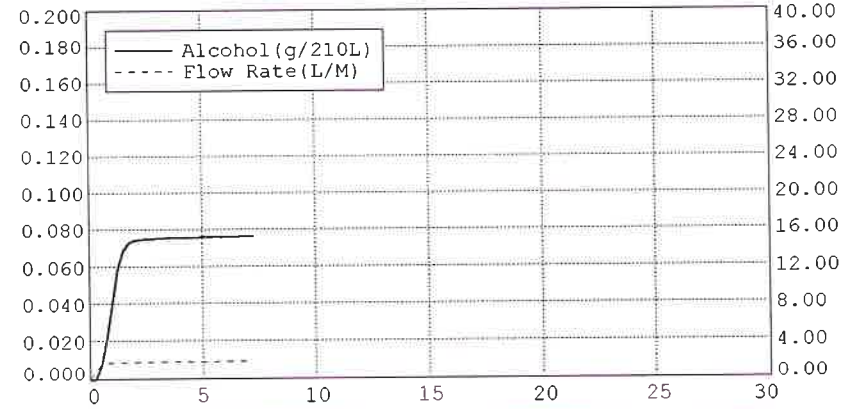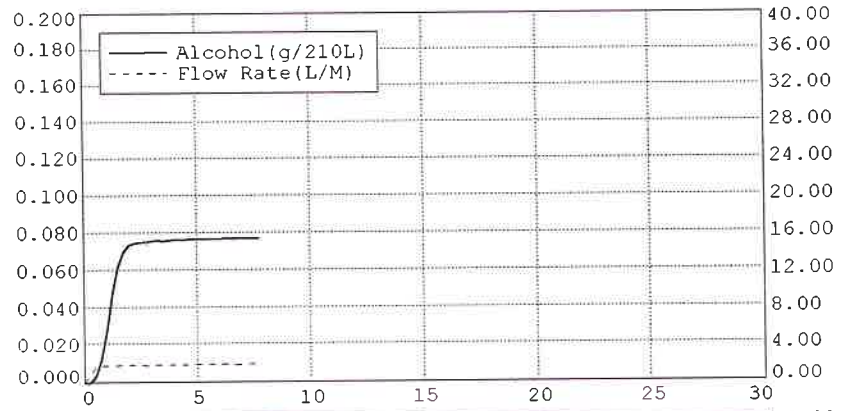

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100368






Date: 06/07/2024
 Time: 11:21:41

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.72: 0.099
 LOT #: AG333401
 EXPIRATION: 11/30/2025
 TANK PRESSURE: 937 psi

BLANK TEST	0.000	11:23
INTERNAL STANDARD	VERIFIED	11:23
EXTERNAL STANDARD	0.099	11:23
BLANK TEST	0.000	11:24
EXTERNAL STANDARD	0.099	11:24
BLANK TEST	0.000	11:25
EXTERNAL STANDARD	0.099	11:25
BLANK TEST	0.000	11:26
EXTERNAL STANDARD	0.099	11:26
BLANK TEST	0.000	11:27
EXTERNAL STANDARD	0.099	11:27
BLANK TEST	0.000	11:28

Average = 0.0990
 Std Dev = 0.0000

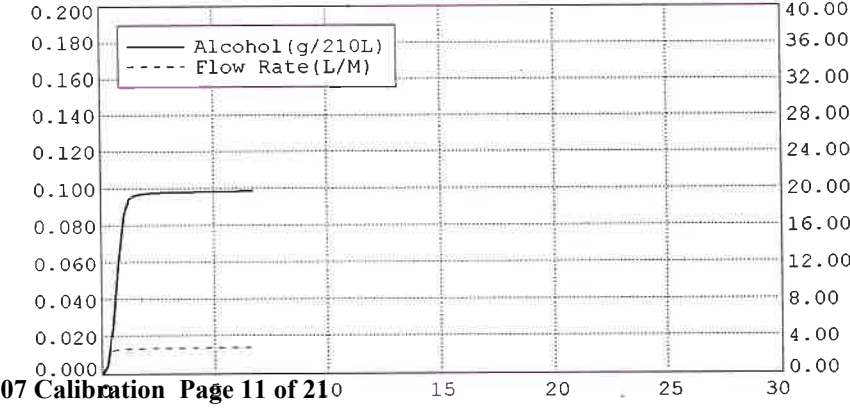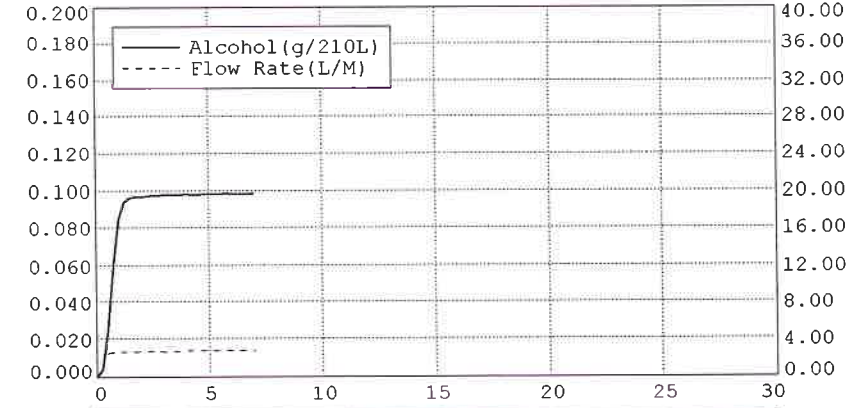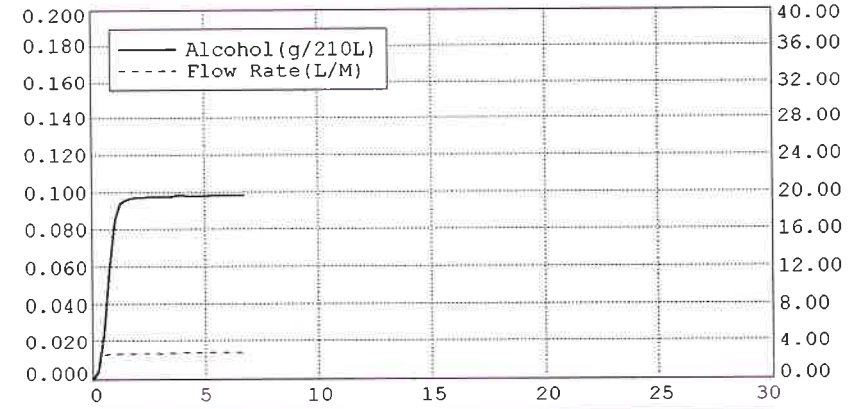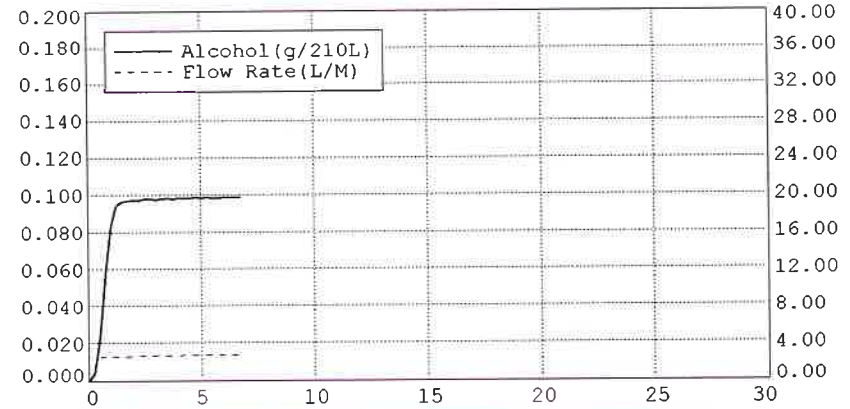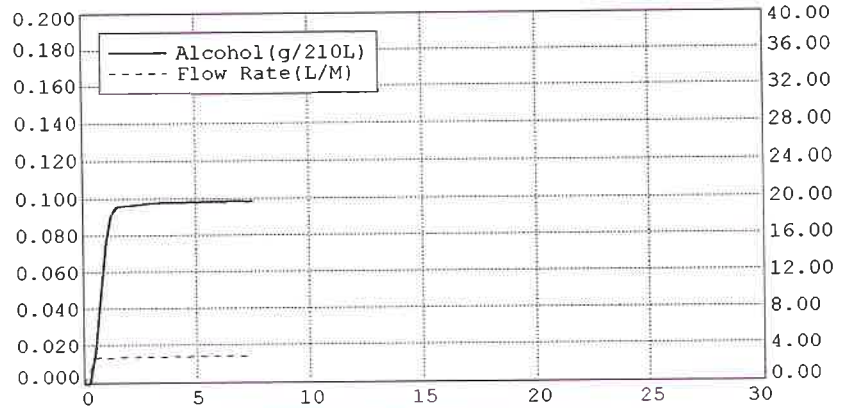

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100368






Date: 06/07/2024
Time: 11:30:25

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.72: 0.149
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 599 psi

BLANK TEST	0.000	11:31
INTERNAL STANDARD	VERIFIED	11:32
EXTERNAL STANDARD	0.147	11:32
BLANK TEST	0.000	11:33
EXTERNAL STANDARD	0.146	11:33
BLANK TEST	0.000	11:34
EXTERNAL STANDARD	0.146	11:34
BLANK TEST	0.000	11:35
EXTERNAL STANDARD	0.147	11:35
BLANK TEST	0.000	11:36
EXTERNAL STANDARD	0.146	11:36
BLANK TEST	0.000	11:37

Average = 0.1464
Std Dev = 0.0005

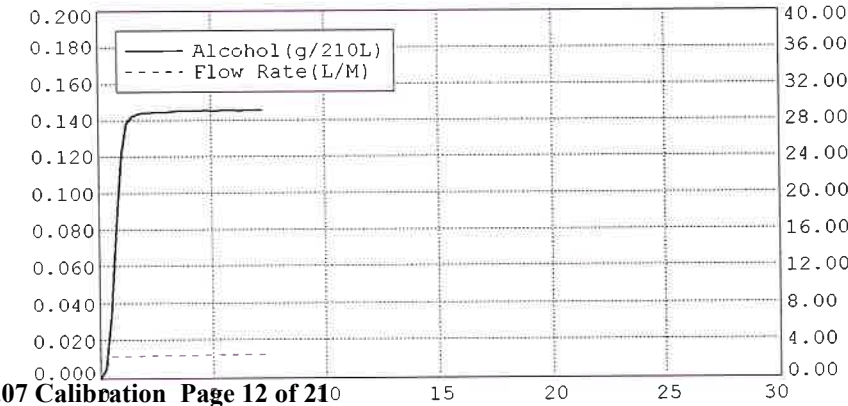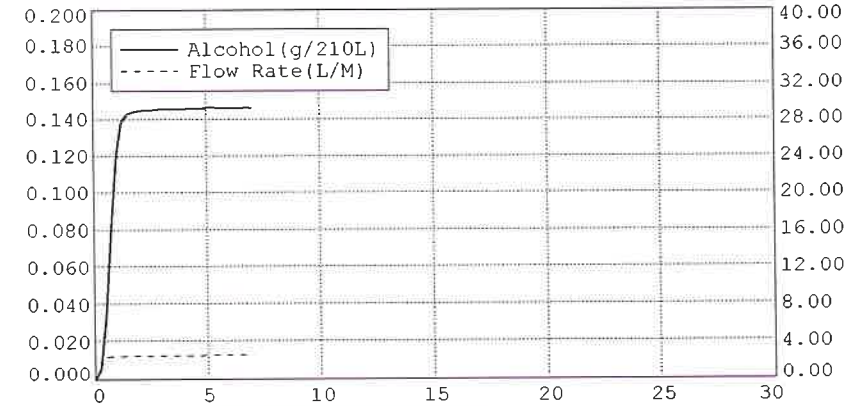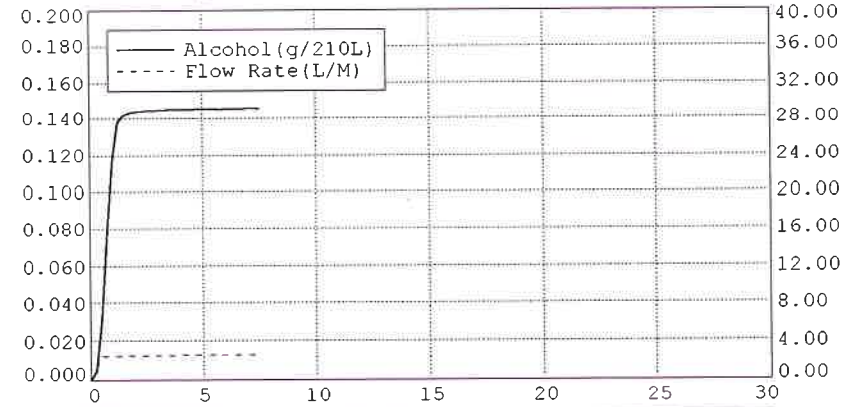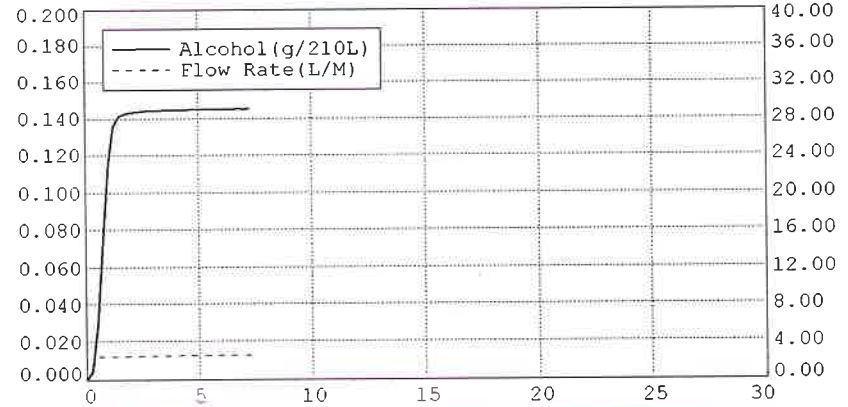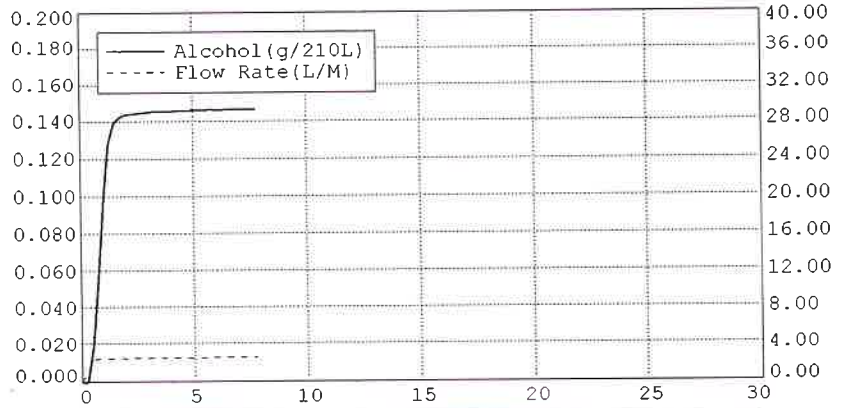

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100368






Date: 06/07/2024
 Time: 11:39:15

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.71: 0.298
 LOT #: AG327804
 EXPIRATION: 10/05/2025
 TANK PRESSURE: 224 psi

BLANK TEST	0.000	11:40
INTERNAL STANDARD	VERIFIED	11:40
EXTERNAL STANDARD	0.297	11:40
BLANK TEST	0.000	11:41
EXTERNAL STANDARD	0.297	11:41
BLANK TEST	0.000	11:42
EXTERNAL STANDARD	0.296	11:43
BLANK TEST	0.000	11:44
EXTERNAL STANDARD	0.297	11:44
BLANK TEST	0.000	11:45
EXTERNAL STANDARD	0.297	11:45
BLANK TEST	0.000	11:46

Average = 0.2968
 Std Dev = 0.0004

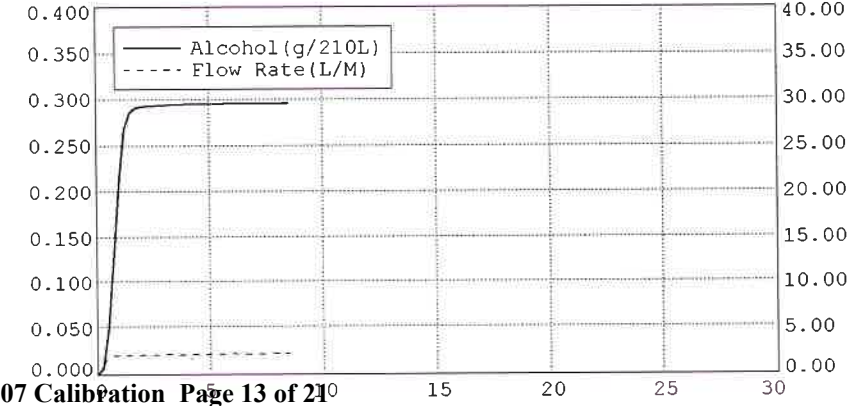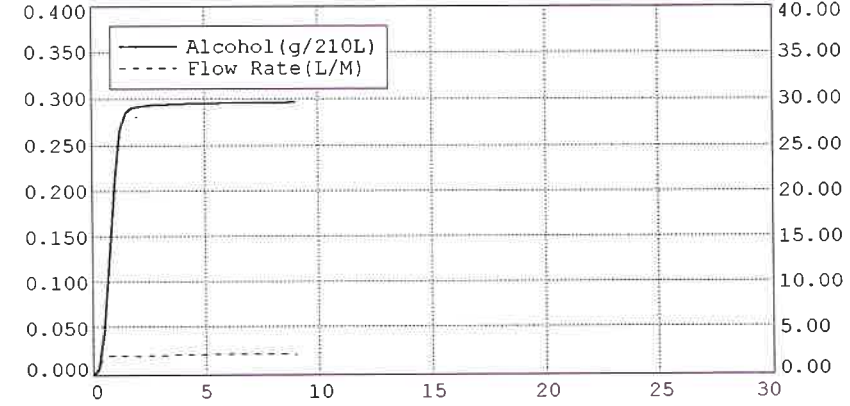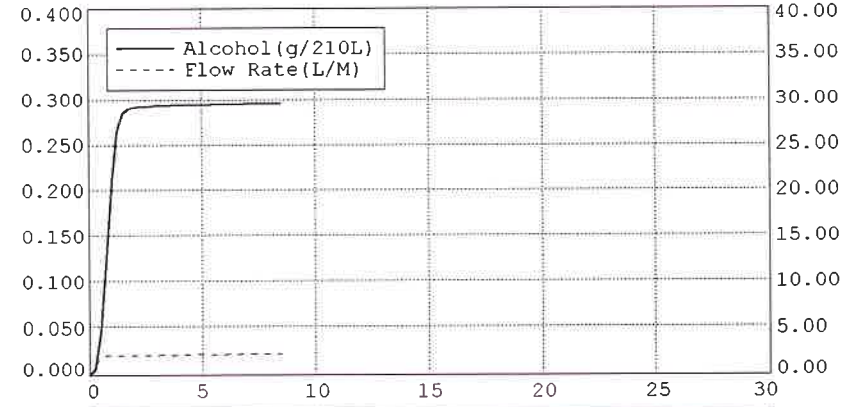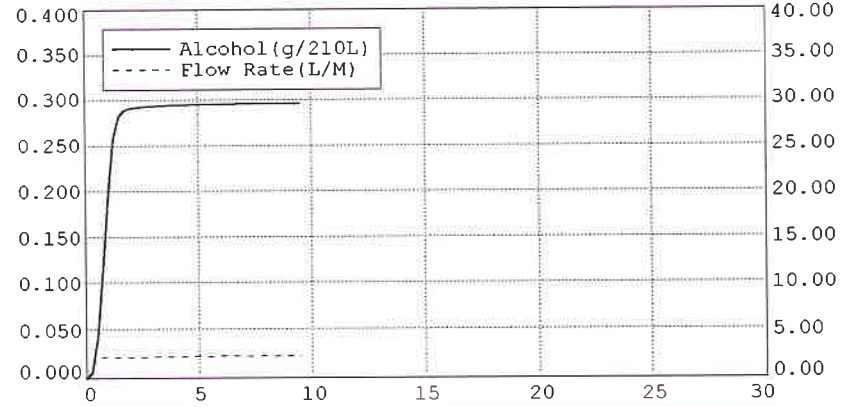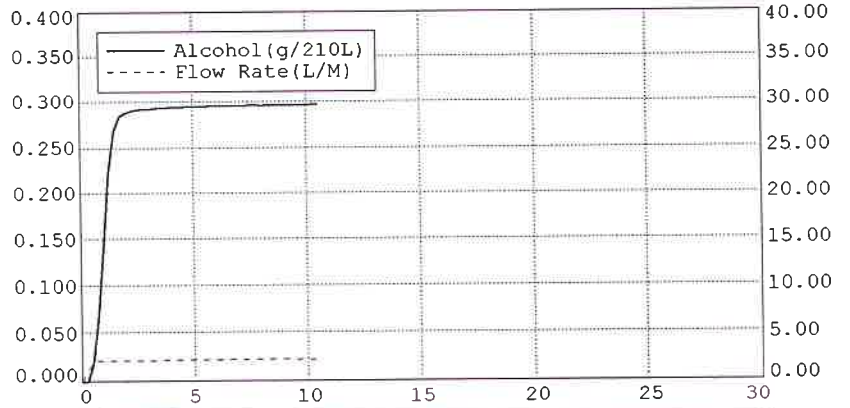

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100368

Date: 06/07/2024
Time: 11:50:13

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.71: 0.079
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 11:51
BLANK TEST 0.000 11:51
INTERNAL STANDARD VERIFIED 11:51
EXTERNAL STANDARD 0.079 11:51
BLANK TEST 0.000 11:52
SUBJECT SAMPLE INCOMPLETE 11:54

MNC

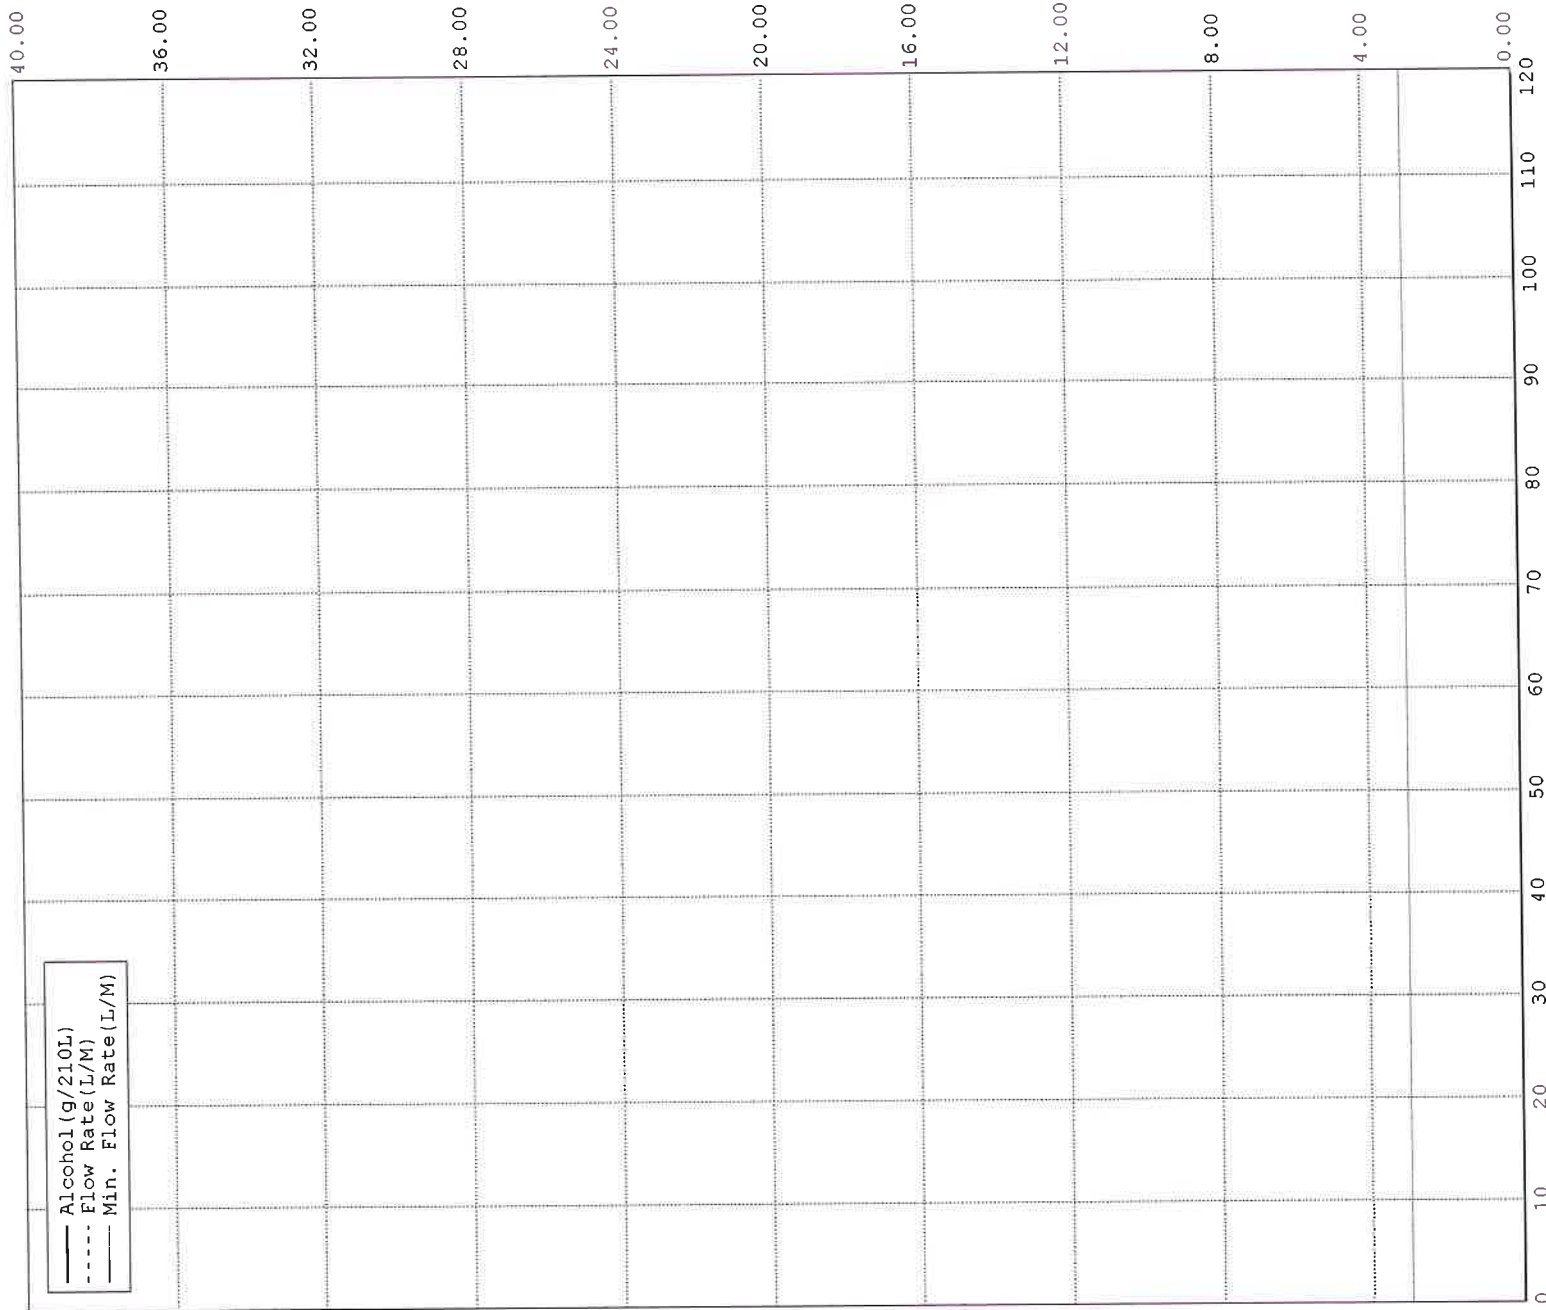

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100368

Date: 06/07/2024
Time: 11:56:57

SUBJECT NAME:
TEST TEST
LICENSE #: XXX
OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.72: 0.079
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 11:58
BLANK TEST 0.000 11:58
INTERNAL STANDARD VERIFIED 11:58
EXTERNAL STANDARD 0.079 11:58
BLANK TEST 0.000 11:59
SUBJECT SAMPLE XXX 12:00

Maximum Attempts Exceeded

MNC

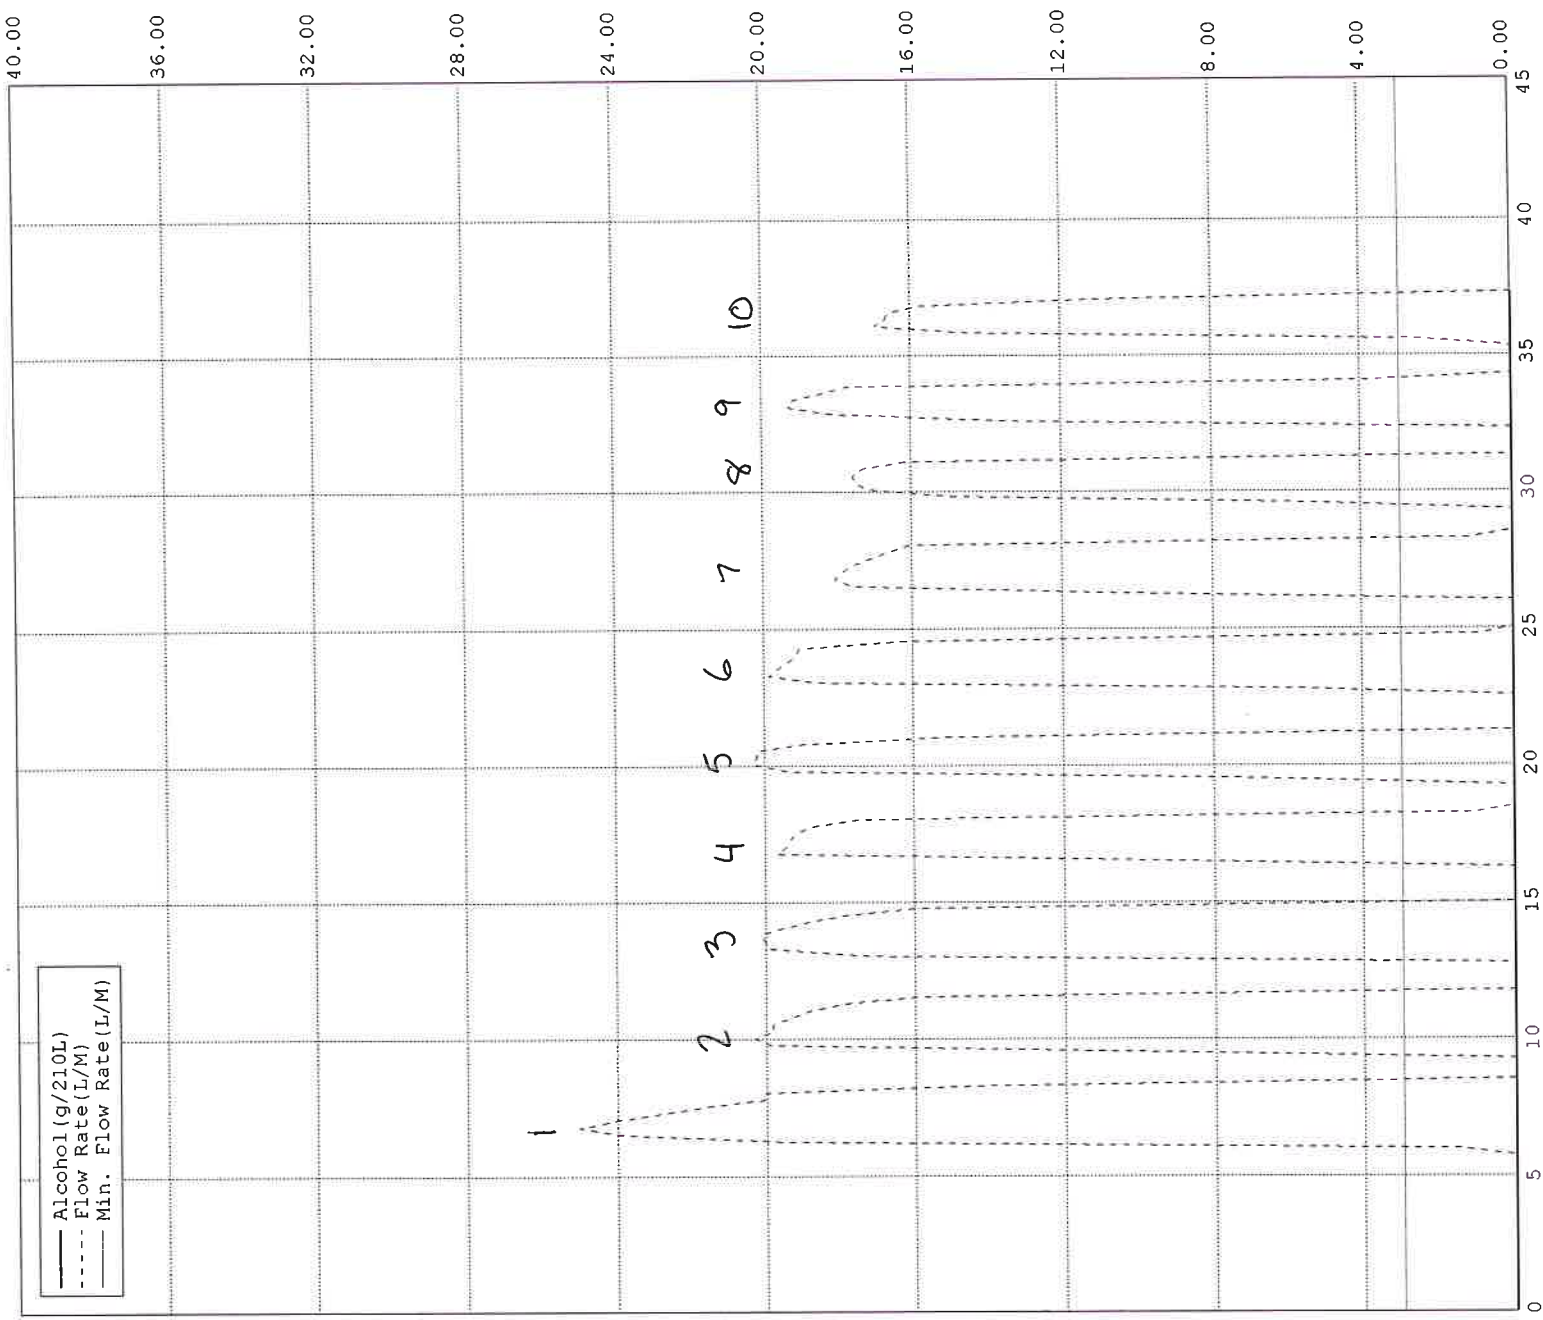

40.00

36.00

32.00

28.00

24.00

20.00

16.00


12.00

8.00

4.00

0.00

— Alcohol (g/210L)
 - - - - Flow Rate (L/M)
 - - - - Min. Flow Rate (L/M)

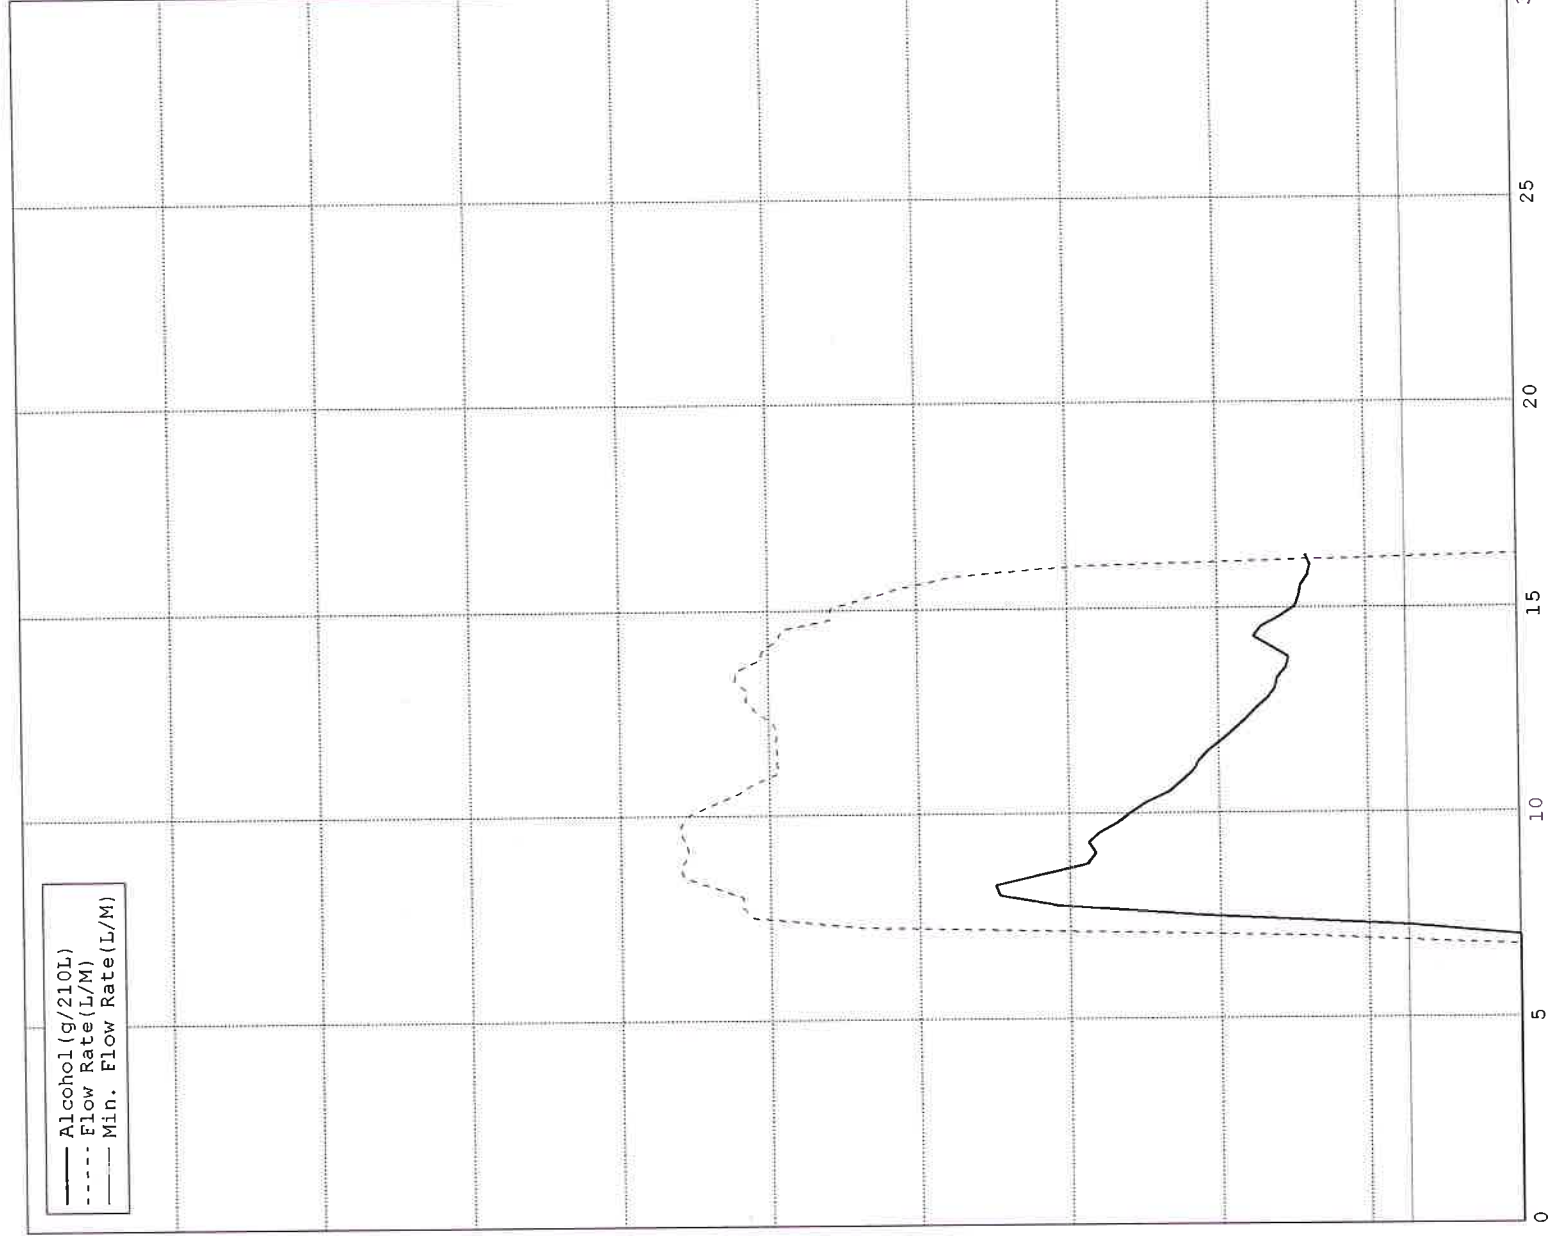

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100368

Date: 06/07/2024

Time: 12:13:33

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INVALID

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.71: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

PASSED 12:14

BLANK TEST 12:14

INTERNAL STANDARD 12:14

VERIFIED 12:14

EXTERNAL STANDARD 12:15

BLANK TEST 12:15

SUBJECT SAMPLE 12:16

INVALID 12:16

MNC

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100368

Date: 06/07/2024
 Time: 12:04:31

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

DEPT/AGENCY:

RFI
 CASE/REPORT: XXX
 TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.71: 0.079
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 12:05
 BLANK TEST 0.000 12:05
 INTERNAL STANDARD VERIFIED 12:05
 EXTERNAL STANDARD 0.078 12:05
 BLANK TEST 0.000 12:06

RFI DETECTED

MNC

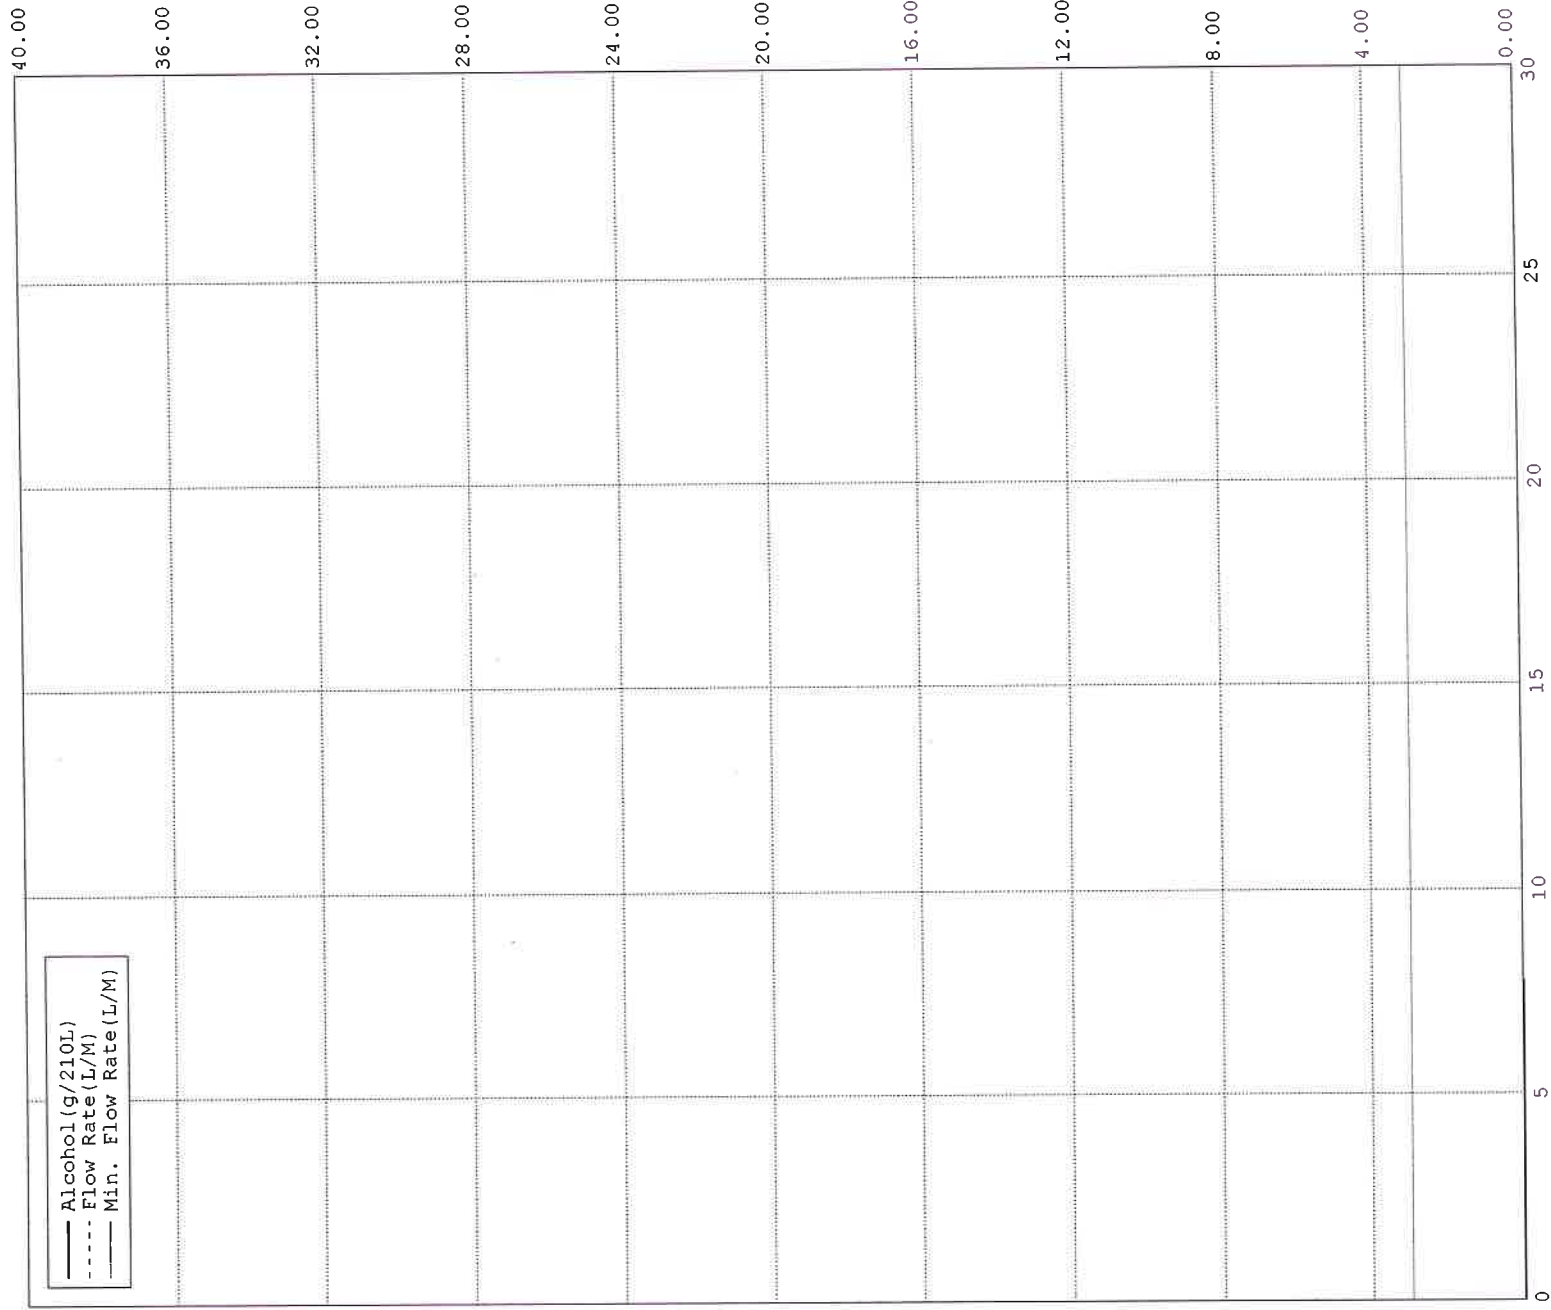

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100368

Date: 06/07/2024
Time: 12:31:45

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.70: 0.079
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 12:32
BLANK TEST 0.000 12:32
INTERNAL STANDARD VERIFIED 12:32
Xq = 0.076 (0.34%)
INTERNAL STANDARD 0.077 12:33
X[1] = 0.0769 (-0.0016) (0.0017)
BLANK TEST 0.000 12:34
SUBJECT SAMPLE XXX 12:34
X[1] = 0.1036 (-0.0177) (-0.0001)


Interference Detected

Filter 2 Average: -0.0012

Filter 3 Average: 0.0016

NWC 6/7/24

NWC
dmt
06/14/24

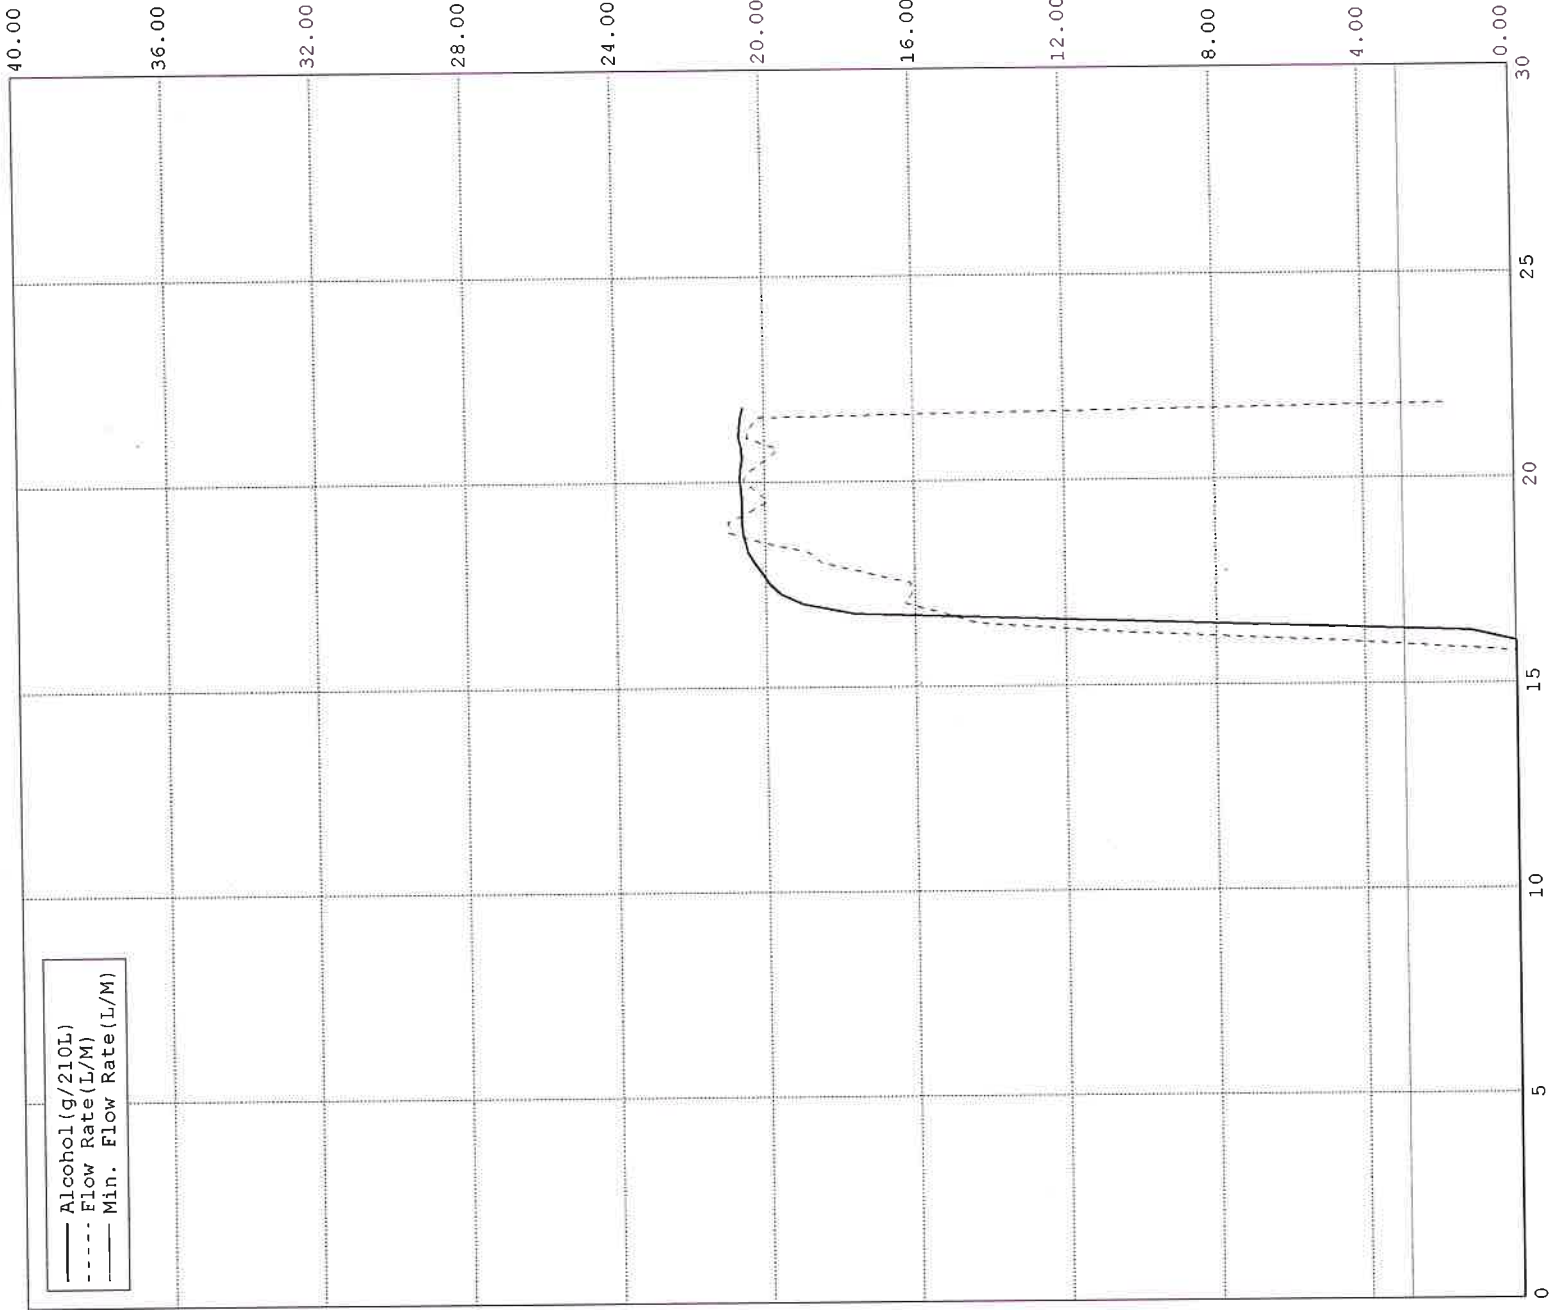

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100368

Date: 06/07/2024
Time: 12:36:27

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.69: 0.079
LOT #: AG310901
EXPIRATION: 04/19/2025

TEST TYPE	RESULT	TIME
DIAGNOSTIC CHECK	PASSED	12:37
BLANK TEST	0.000	12:37
INTERNAL STANDARD	VERIFIED	12:37
Xq = 0.077 (1.49%)		
EXTERNAL STANDARD	0.078	12:37
X[1] = 0.0780 (-0.0007) (0.0019)		
BLANK TEST	0.000	12:38
SUBJECT SAMPLE	XXX	12:39
X[1] = 0.1125 (-0.0266) (0.0008)		

Interference Detected

MNC



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100368

Date: 06/07/2024

Time: 12:21:04

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INTERFERENCE - NEGATIVE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.71: 0.079

LOT #: AG310901

EXPIRATION: 04/19/2025

TEST TYPE	RESULT	TIME
DIAGNOSTIC CHECK	PASSED	12:22
BLANK TEST	0.000	12:22
INTERNAL STANDARD	VERIFIED	12:22
Xq = 0.076 (0.23%)		
EXTERNAL STANDARD	0.078	12:22
X[1] = 0.0779 (-0.0009)	(0.0020)	
BLANK TEST	0.000	12:23
SUBJECT SAMPLE (Vol=1.56L)	0.091	12:23
X[1] = 0.0918 (-0.0002)	(-0.0004)	
BLANK TEST	0.000	12:24
EXTERNAL STANDARD	0.077	12:25
X[1] = 0.0772 (-0.0017)	(0.0009)	
BLANK TEST	0.000	12:25

MNC

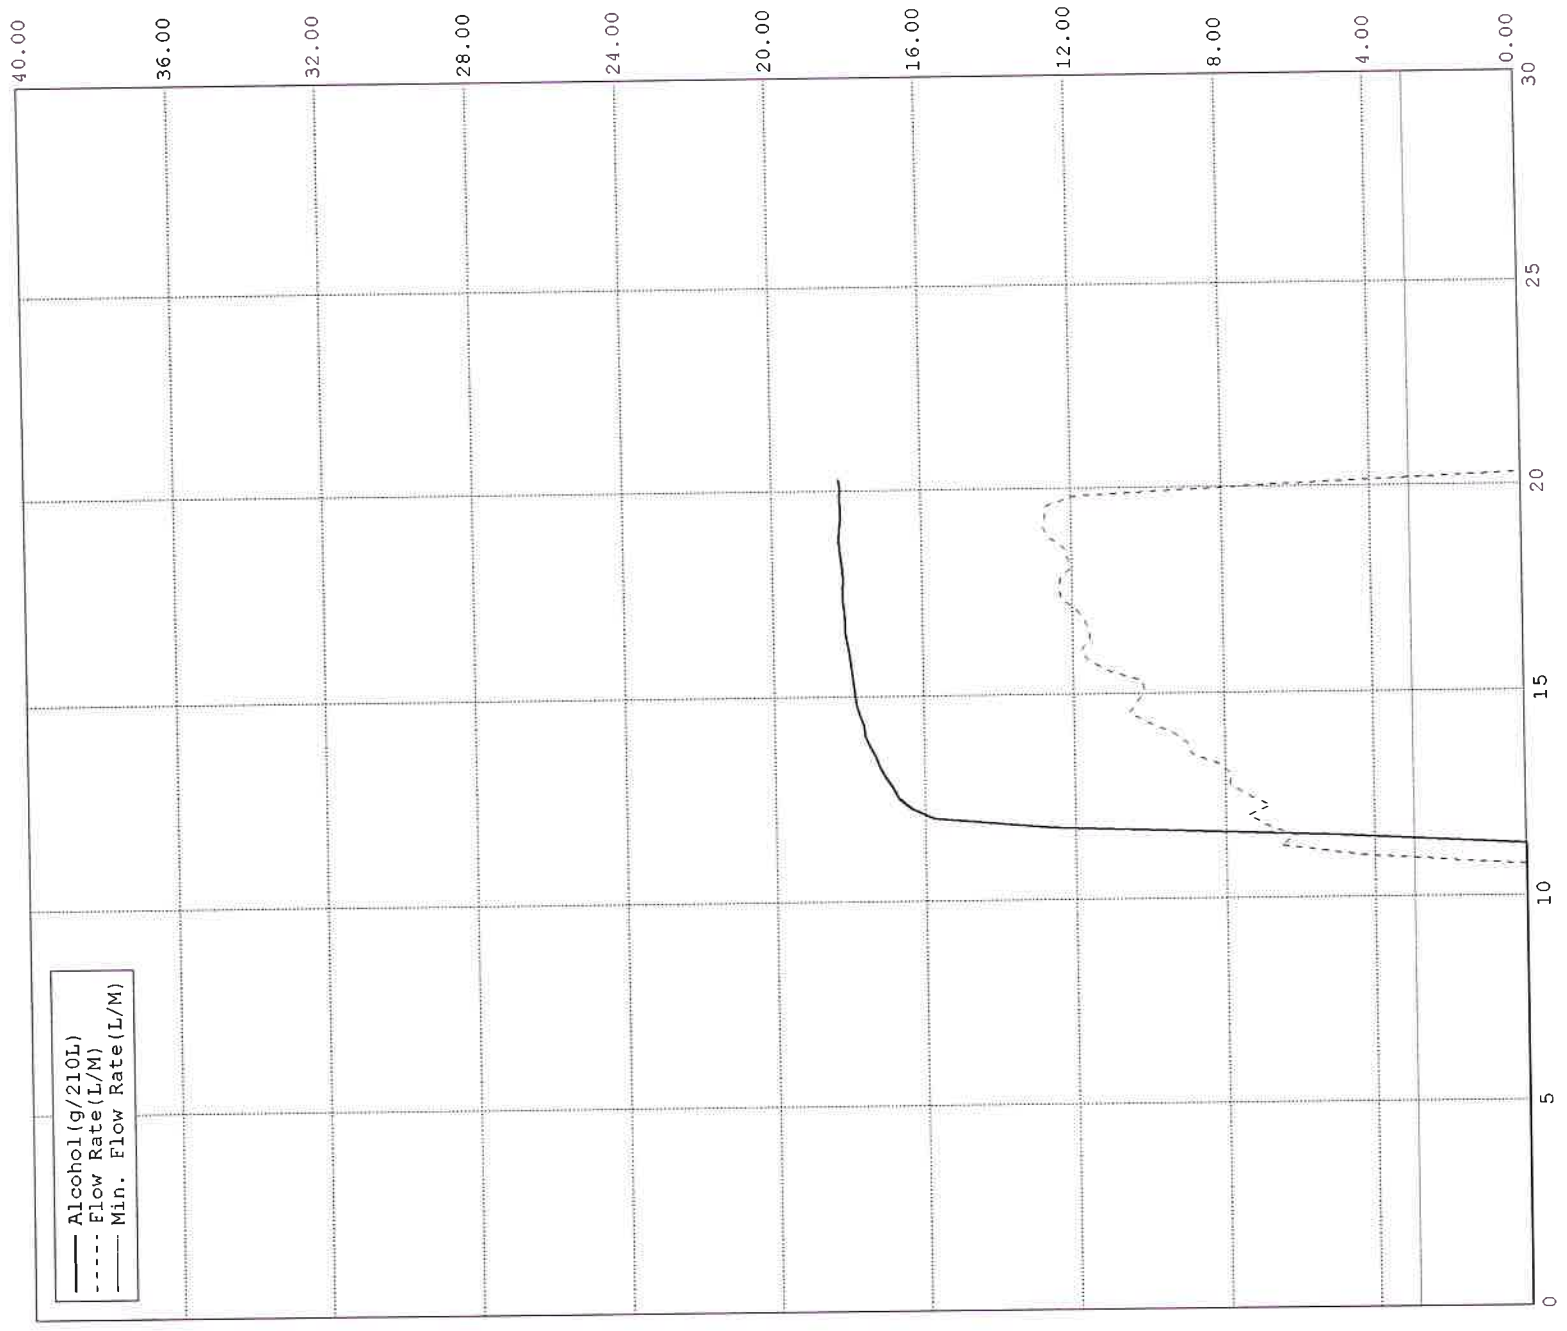

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100368

Date: 06/07/2024
Time: 12:54:14

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.70: 0.079
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	12:55
BLANK TEST	0.000	12:55
INTERNAL STANDARD	VERIFIED	12:55
EXTERNAL STANDARD	0.078	12:55
BLANK TEST	0.000	12:56
SUBJECT SAMPLE (Vol=2.70L)	0.000	12:56
BLANK TEST	0.000	12:57
EXTERNAL STANDARD	0.078	12:58
BLANK TEST	0.000	12:58

MNC

