

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100346

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 06/04/2020

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.33: 0.078
LOT #: AG826101
EXPIRATION: 09/18/2020
TANK PRESSURE: 1087 psi

BLANK TEST	0.000	14:15
INTERNAL STANDARD	VERIFIED	14:15
EXTERNAL STANDARD	0.077	14:15
BLANK TEST	0.000	14:16
EXTERNAL STANDARD	0.077	14:16
BLANK TEST	0.000	14:17
EXTERNAL STANDARD	0.077	14:18
BLANK TEST	0.000	14:18
EXTERNAL STANDARD	0.077	14:19
BLANK TEST	0.000	14:19
EXTERNAL STANDARD	0.077	14:20
BLANK TEST	0.000	14:21

Average = 0.0770
Std Dev = 0.0000

Diagnostic Check

VERSIONS

DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C	PASSED
Breath Tube = 44.4°C	PASSED

PUMP INFO

Flow Rate = 4.202 L/M	PASSED
-----------------------	--------

DETECTOR INFO

PUMP ON	PASSED
PUMP OFF	PASSED


FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
-------------------	--------


I, Brandi M. Barnett, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.



 7/7/20

Brandi M. Barnett
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 7th day of July, 20 20



Notary Public
My Commission Expires With Office

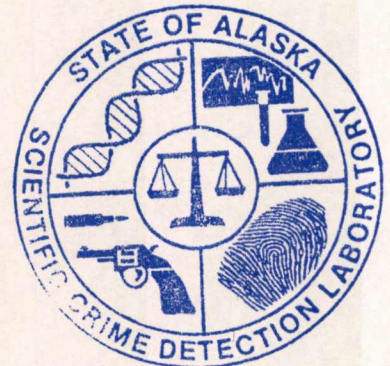

DM 06/05/20