




State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100392

Report Issue Date: 03/10/2026
Date Received: 2025-12-16
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG515609	0.020	0.020	0.020	0.019	0.020	0.020
0.080	0.078	AG436502	0.078	0.079	0.078	0.078	0.079	0.078
0.300	0.293	AG427706	0.294	0.294	0.294	0.294	0.294	0.294

As Found - Evaluation Analyst: Kaija Swisher
 As Found Conditions - Barometric Pressure (inHg): 29.22 Barometer Used: VWR S/N 240680771 Temperature (C): 20.1 Relative Humidity (%): 0
 As-Found Lab Activity Date Range: 12/16/2025 - 12/16/2025

VOC internal standard greater than 3%. Adjustment needed.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.021	0.021	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG407908	0.041	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.080	AG436502	0.079	0.079	0.080	0.080	0.080	0.080	+/- 0.004
0.100	0.100	AG516101	0.098	0.098	0.099	0.099	0.099	0.099	+/- 0.004
0.150	0.150	AG515604	0.148	0.148	0.148	0.148	0.148	0.148	+/- 0.006
0.300	0.299	AG427706	0.299	0.299	0.299	0.300	0.299	0.299	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.87 Barometer Used: VWR S/N 240680771 Temperature (C): 19.9 Relative Humidity (%): 9
 As-Left Lab Activity Date Range: 02/18/2026 - 02/19/2026

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Colleen O'Bryant on 03/10/2026

colleen.obryant@alaska.gov

Technically and administratively reviewed by Derek Walton on 03/10/2026

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100392 Analyst or Technician Name: C.O. Bryant

DataMaster DMT Calibration Start Date: 2/18/26

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 10 Sep 2026
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.87 Temperature(C) 19.9 Relative Humidity(%) 9

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
 - Invalid
 - Interference (Volatiles) - *Print with View Details*
 - Maximum Attempts Exceeded
 - Radio Frequency Interference (RFI)
- 5/18/26 COB 2026.03.10
- Acetone Reagent Lot Number: 20260218COB Expiration Date: 3/19/27
Simulator S/N: SD1088 Thermometer Verification Performed? 5/18/26 COB 2026.03.10
 - Isopropanol Reagent Lot Number: 20260218COB Expiration Date: 3/19/27
Simulator S/N: SD1199 Thermometer Verification Performed?
 - Negative (Ethanol Only) Lot Number: 2026041280 Expiration Date: 3/19/27
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 14 Mar 2027

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 2/19/26

Data Interpretation Date (Technician): _____ (if applicable)

Data Interpretation Date (Analyst): 2/19/26

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 02/18/2026
Time: 12:23:16

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 45.7°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.74 V PASSED
(1.06 V - 2.46 V)
Cooler Voltage = 1.65 V PASSED
(0.94 V - 2.20 V)
Bias Voltage = 79 V PASSED
(48 V - 112 V)
Chopper Freq = 532 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.9 in

PUMP INFO

Flow Rate = 4.828 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.100 0.09% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100392

Date: 02/18/2026
Time: 12:38 PM

Temperatures (°C)

Sample Cell: 49.1°C
Breath Tube: 47.1°C

Current Barometer 29.9 in
Volume (Ltr) 1.56

Settings

Lamp: 1.74 V
Bias: 79 V
Cooler: 1.65 V
Chopper: 532 Hz

Voltages (V)

Flow: 1.07 V
Detector: 0.045 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 01/08/2026
Time: 15:22:03

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca = 0.1000
CAL = 0.982362 0.800 <= CAL < 1.200
b1 = 0.0001 0.0000 <= b1 < 0.0040
b2 = 0.0057 0.0010 <= b2 < 0.0100
b3 = 0.0001 0.0000 <= b3 < 0.0040
Xq = 0.1000 0.0500 <= Xq < 0.2000
a21 = 1.149226 1.050 <= a21 < 1.300
a31 = 0.389914 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 02/18/2026
Time: 12:40:16


SUBJECT NAME:
TEST TEST
LICENSE #: MIN VOLUME

OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.91: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	12:41
BLANK TEST	0.000	12:41
INTERNAL STANDARD	VERIFIED	12:41
EXTERNAL STANDARD	0.080	12:41
BLANK TEST	0.000	12:42
SUBJECT SAMPLE (Vol=1.56L)	0.000	12:43
BLANK TEST	0.000	12:44
EXTERNAL STANDARD	0.080	12:44
BLANK TEST	0.000	12:45

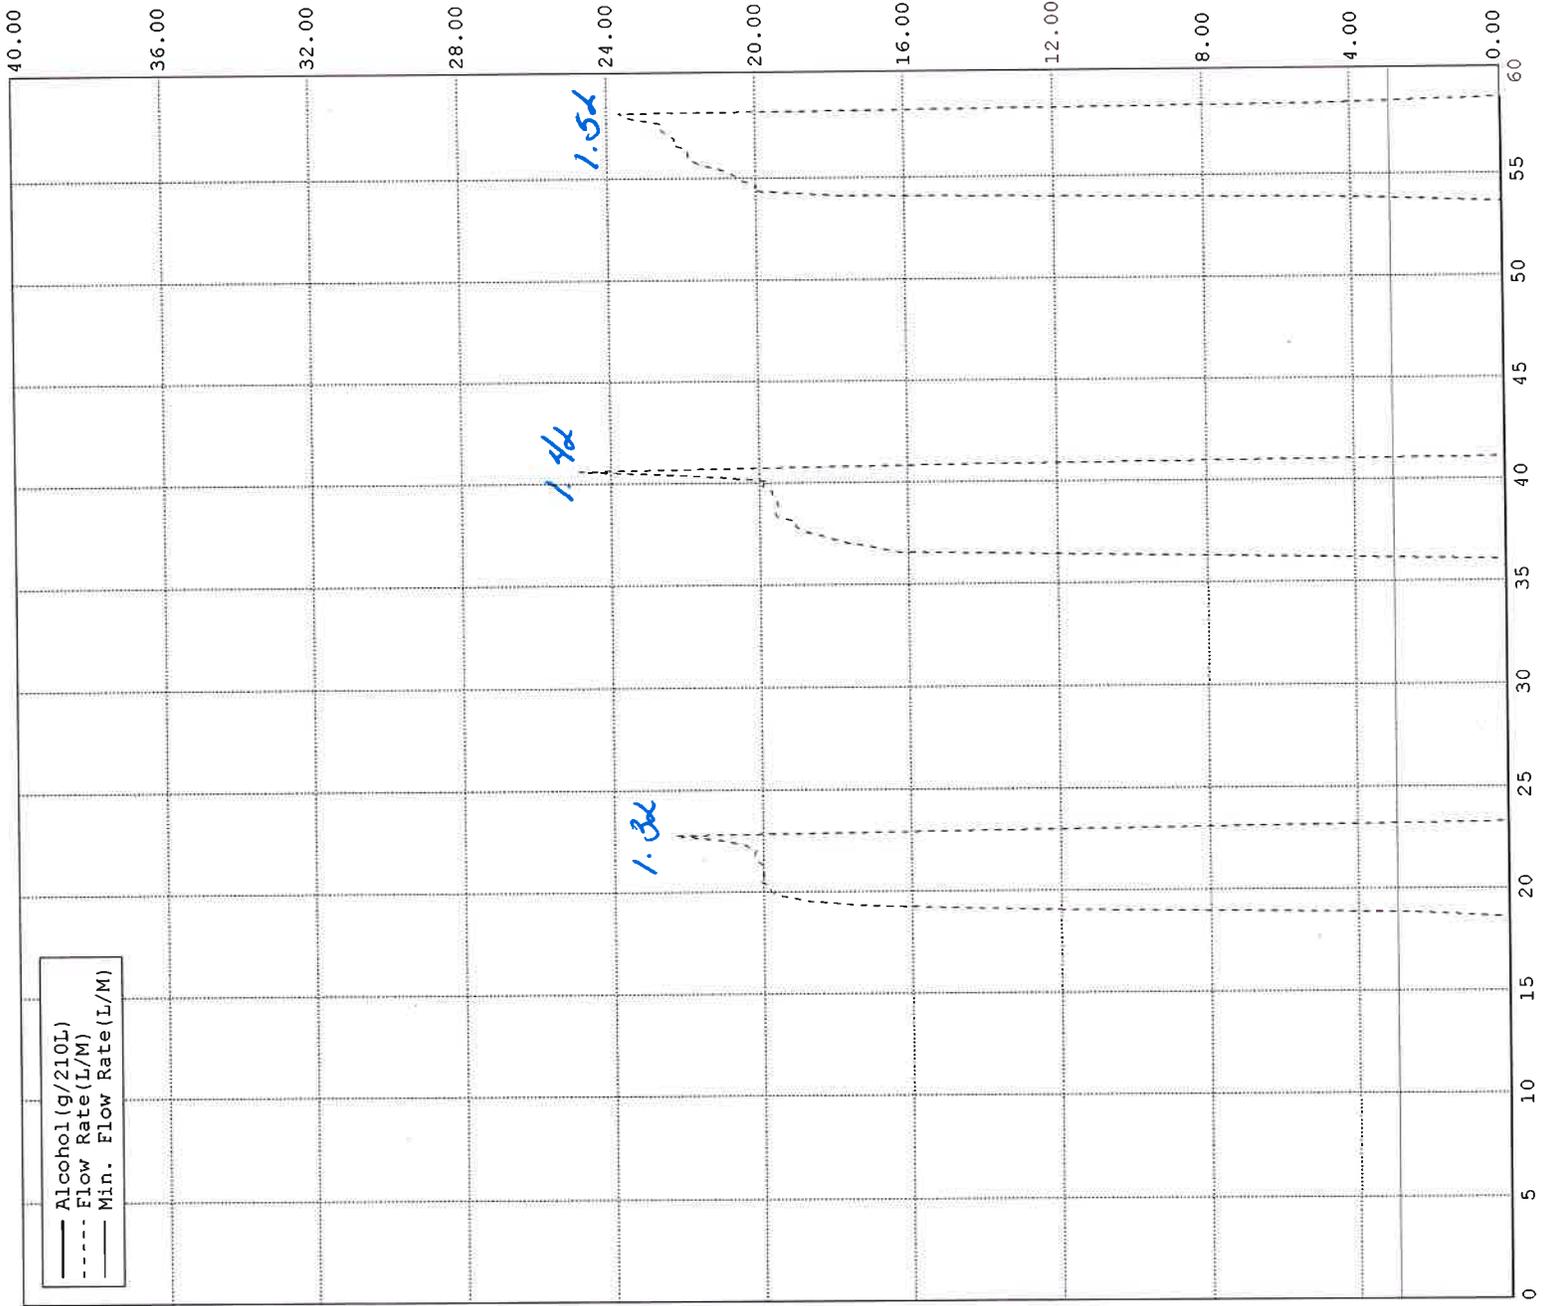

LINEARITY CHECK

Alaska Department of Public Safety

DATAMASTER dmt: 100392

Date: 02/19/2026

Time: 07:07:09

SUPERVISOR NAME:


COLLEEN S OBRyant

OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0204	0.0005
0.040	0.0402	0.0004
0.080	0.0796	0.0005
0.100	0.0986	0.0005
0.150	0.1480	0.0000
0.299	0.2992	0.0004

SLOPE = 0.998990
 R² = 0.999906

CS

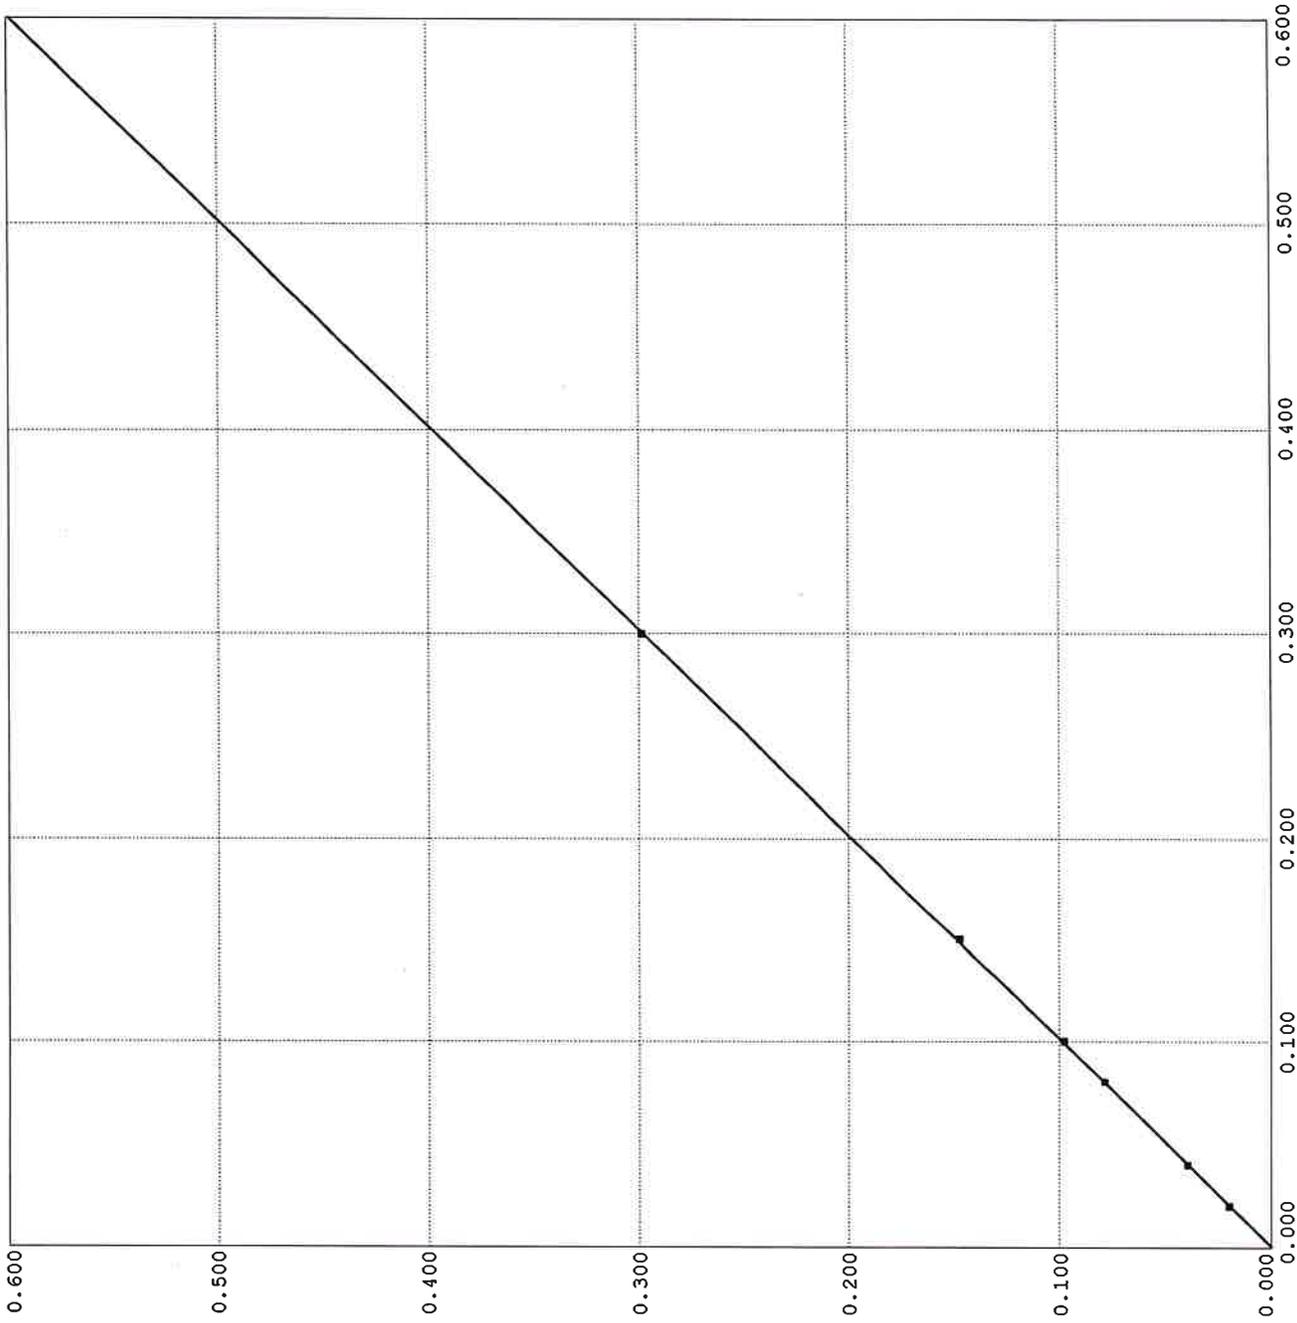

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 02/19/2026
 Time: 07:07:11

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.86: 0.020
 LOT #: ~~AG403002~~ AG408002 0080/5/26
 EXPIRATION: 03/20/2026
 TANK PRESSURE: 634 psi

BLANK TEST	0.000	07:16
INTERNAL STANDARD	VERIFIED	07:16
EXTERNAL STANDARD	0.020	07:16
BLANK TEST	0.000	07:17
EXTERNAL STANDARD	0.021	07:17
BLANK TEST	0.000	07:18
EXTERNAL STANDARD	0.021	07:18
BLANK TEST	0.000	07:19
EXTERNAL STANDARD	0.020	07:19
BLANK TEST	0.000	07:20
EXTERNAL STANDARD	0.020	07:20
BLANK TEST	0.000	07:21

Average = 0.0204
 Std Dev = 0.0005

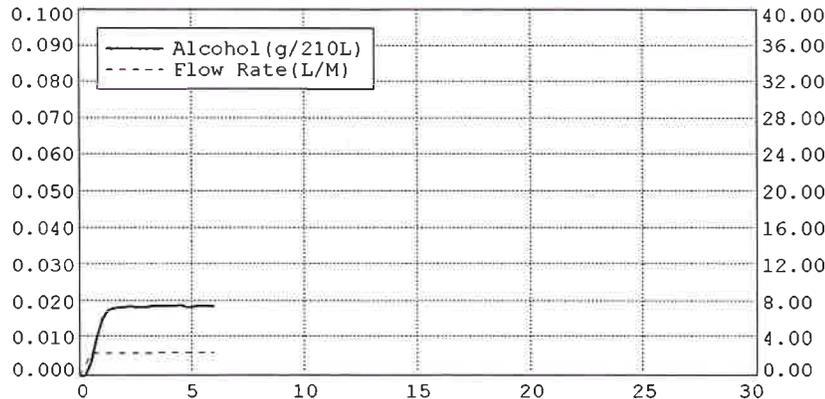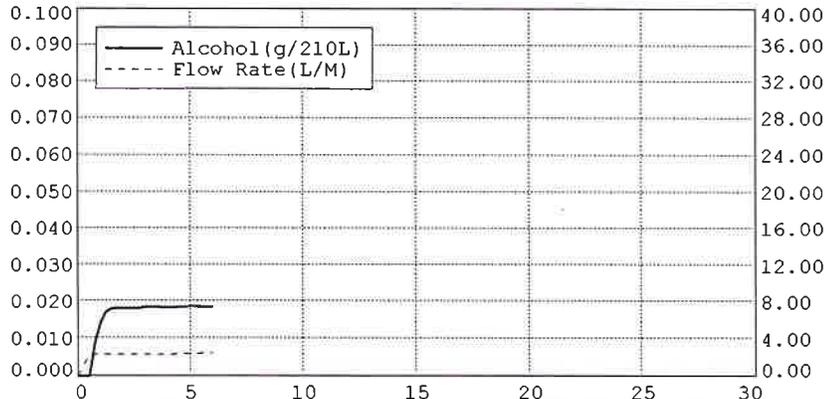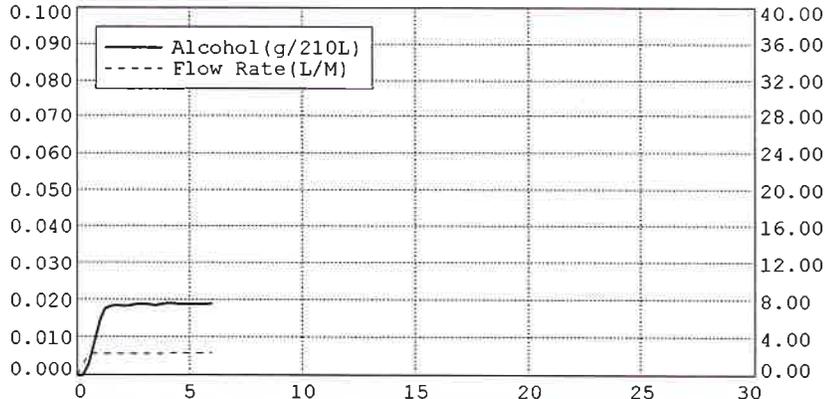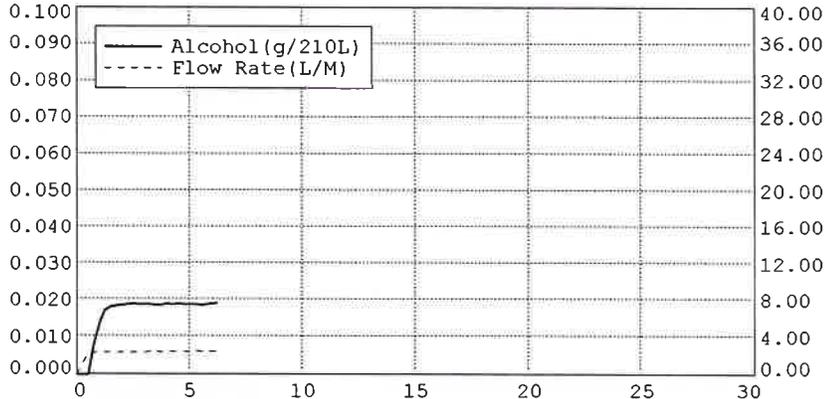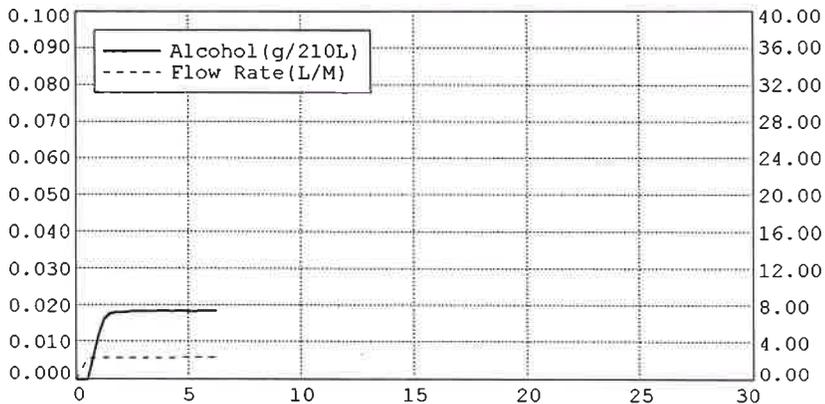

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 02/19/2026
 Time: 07:23:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.86: 0.040
 LOT #: AG407908
 EXPIRATION: 03/19/2026
 TANK PRESSURE: 642 psi

BLANK TEST	0.000	07:24
INTERNAL STANDARD	VERIFIED	07:24
EXTERNAL STANDARD	0.041	07:25
BLANK TEST	0.000	07:26
EXTERNAL STANDARD	0.040	07:26
BLANK TEST	0.000	07:27
EXTERNAL STANDARD	0.040	07:27
BLANK TEST	0.000	07:28
EXTERNAL STANDARD	0.040	07:28
BLANK TEST	0.000	07:29
EXTERNAL STANDARD	0.040	07:29
BLANK TEST	0.000	07:30

Average = 0.0402
 Std Dev = 0.0004

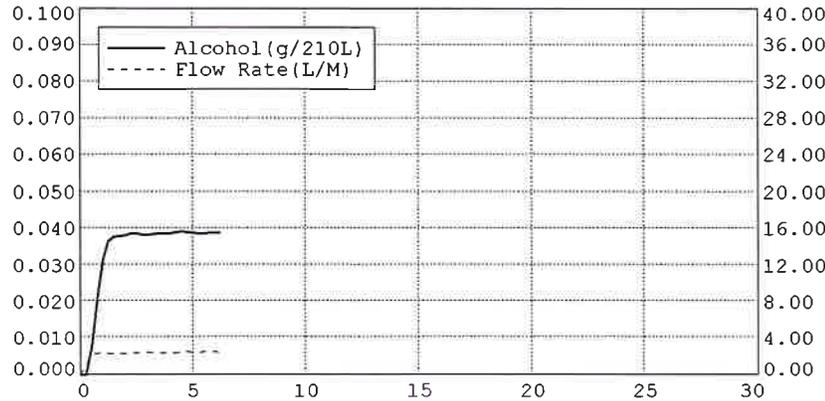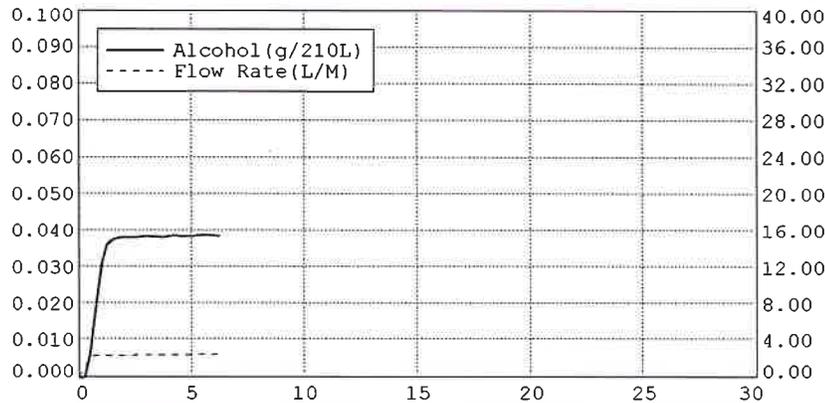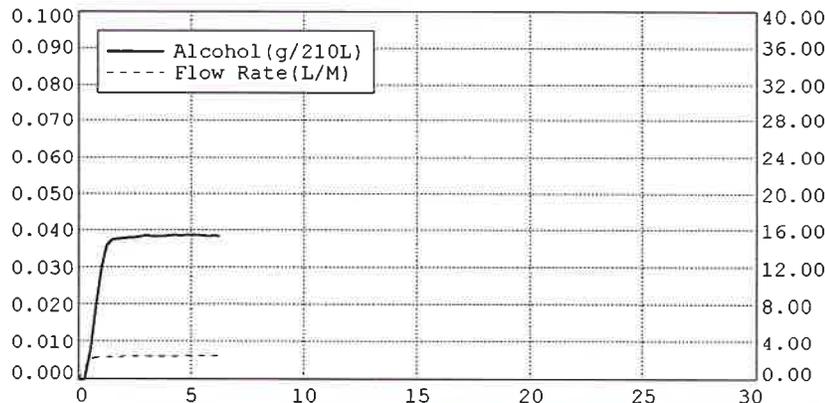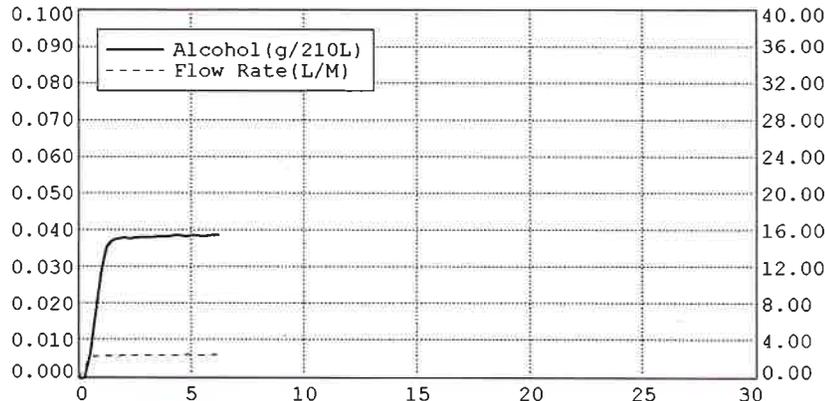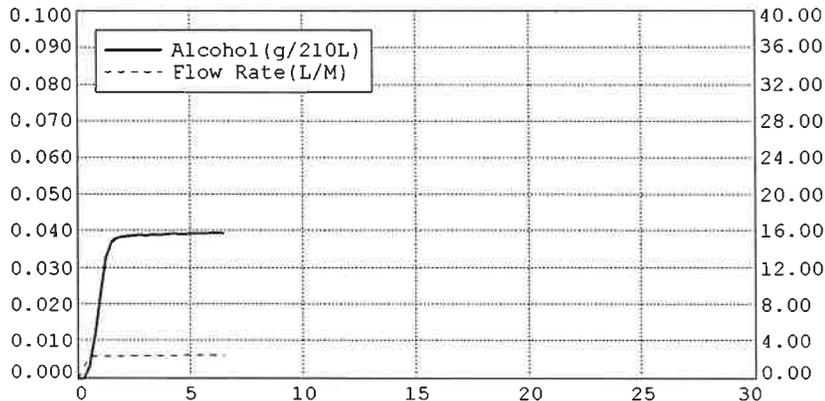

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 02/19/2026
 Time: 07:46:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.86: 0.080
 LOT #: AG436502
 EXPIRATION: 12/30/2026
 TANK PRESSURE: 931 psi

BLANK TEST	0.000	07:47
INTERNAL STANDARD	VERIFIED	07:47
EXTERNAL STANDARD	0.079	07:47
BLANK TEST	0.000	07:48
EXTERNAL STANDARD	0.079	07:49
BLANK TEST	0.000	07:50
EXTERNAL STANDARD	0.080	07:50
BLANK TEST	0.000	07:51
EXTERNAL STANDARD	0.080	07:51
BLANK TEST	0.000	07:52
EXTERNAL STANDARD	0.080	07:52
BLANK TEST	0.000	07:53

Average = 0.0796
 Std Dev = 0.0005

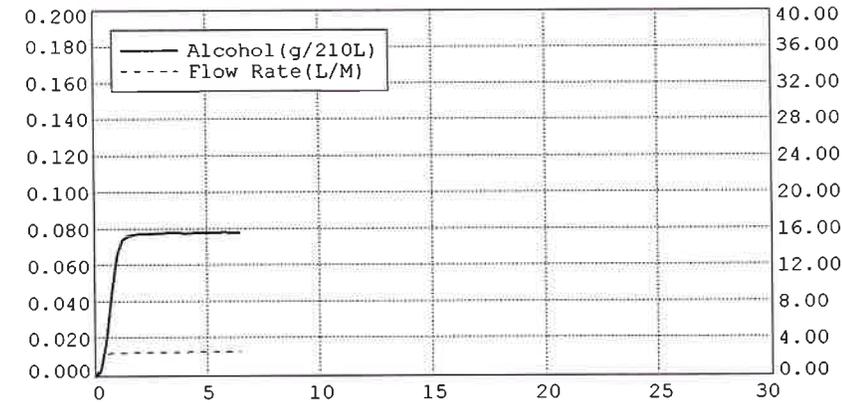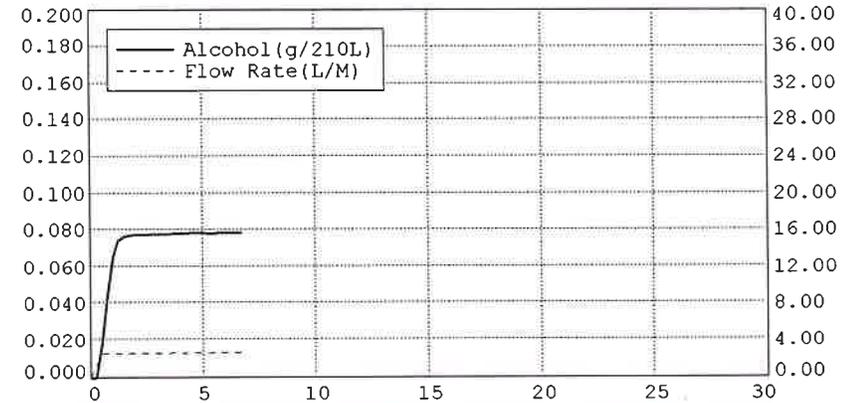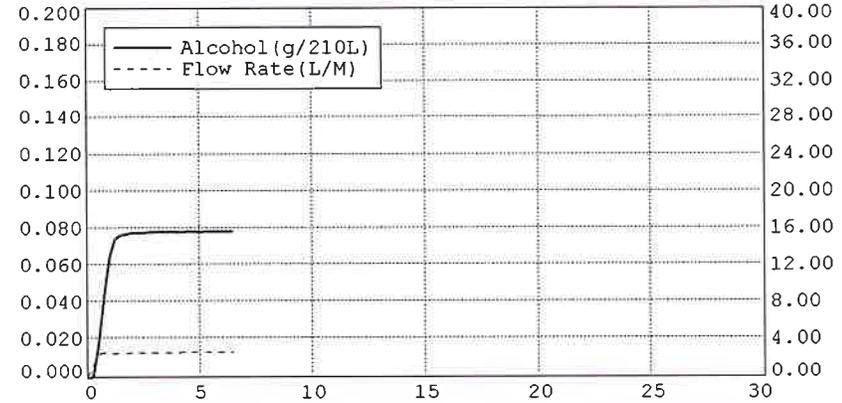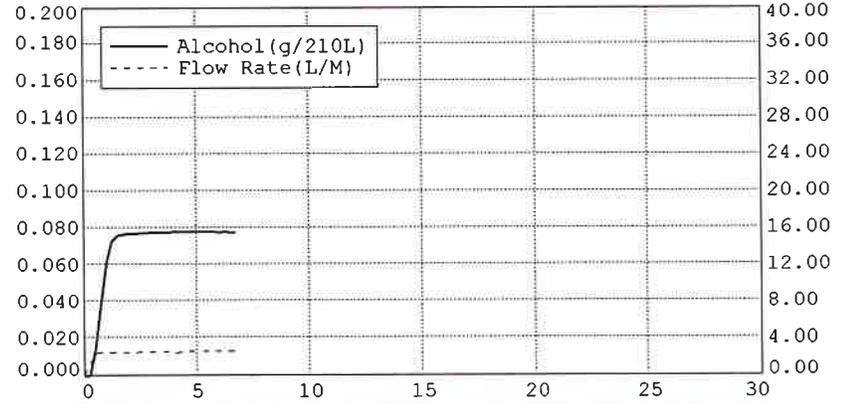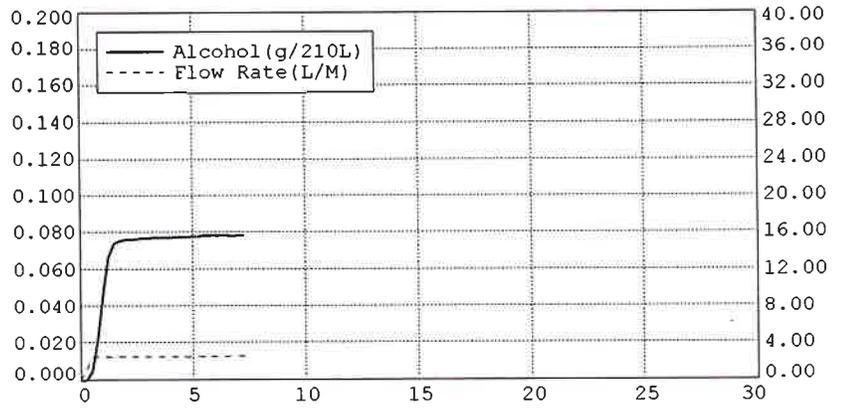

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 02/19/2026
 Time: 07:56:35

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.86: 0.100
 LOT #: AG516101
 EXPIRATION: 06/10/2027
 TANK PRESSURE: 1029 psi

BLANK TEST	0.000	07:57
INTERNAL STANDARD	VERIFIED	07:57
EXTERNAL STANDARD	0.098	07:58
BLANK TEST	0.000	07:58
EXTERNAL STANDARD	0.098	07:59
BLANK TEST	0.000	08:00
EXTERNAL STANDARD	0.099	08:00
BLANK TEST	0.000	08:01
EXTERNAL STANDARD	0.099	08:01
BLANK TEST	0.000	08:02
EXTERNAL STANDARD	0.099	08:02
BLANK TEST	0.000	08:03

Average = 0.0986
 Std Dev = 0.0005

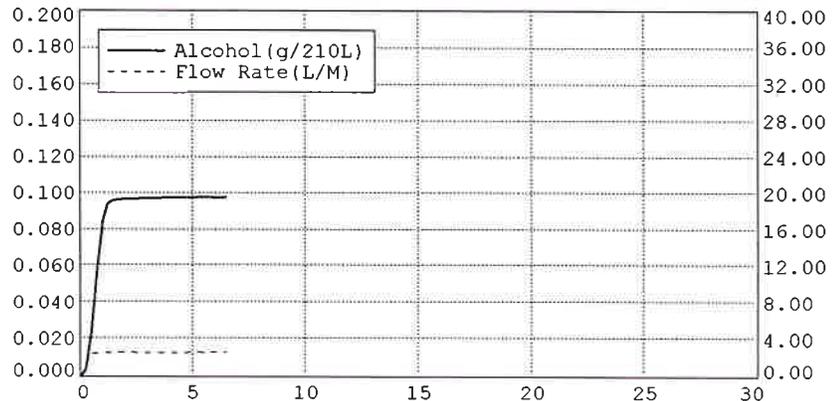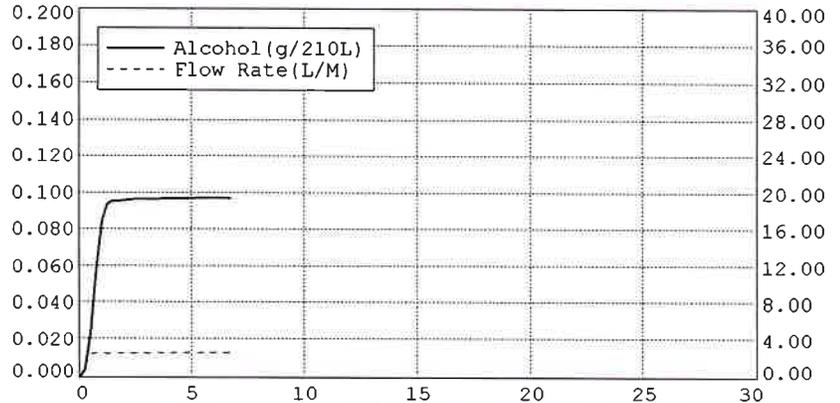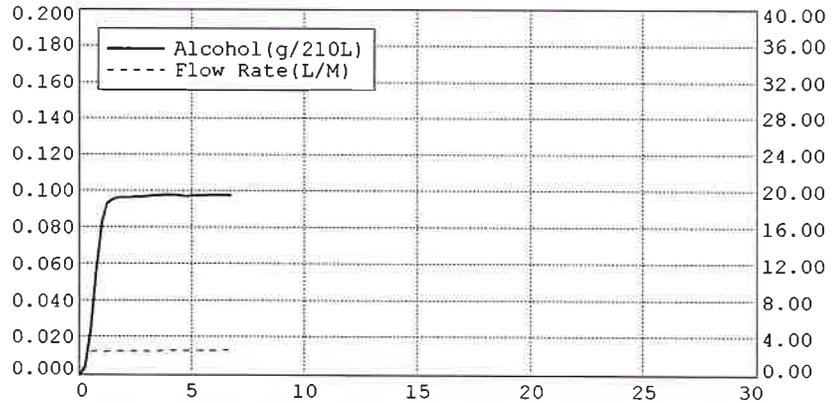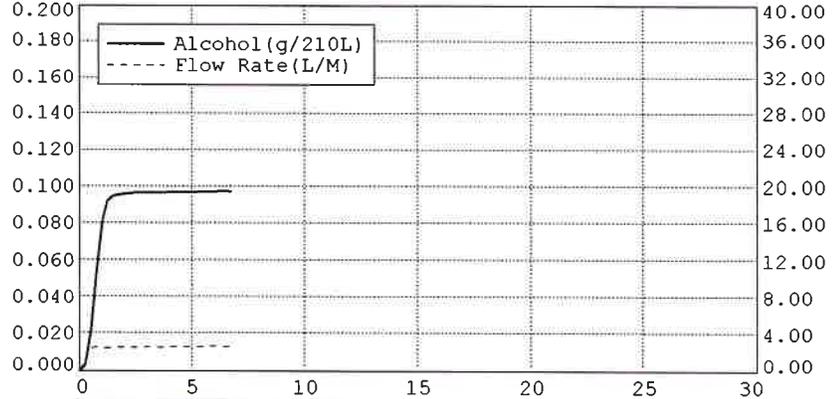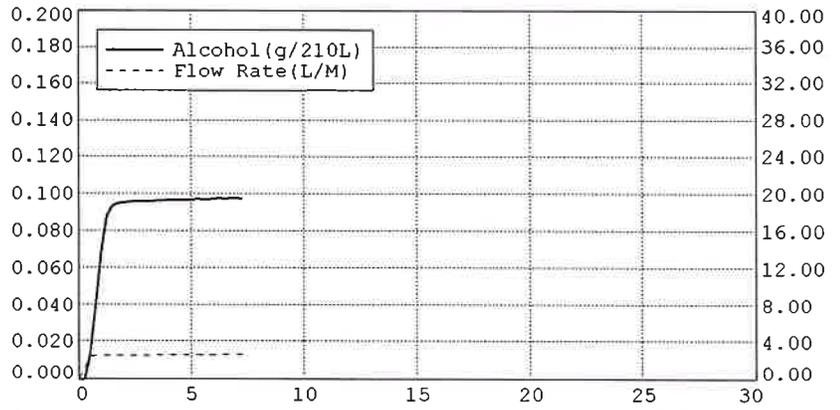

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 02/19/2026
 Time: 08:43:14

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.86: 0.150
 LOT #: AG515604
 EXPIRATION: 06/05/2027
 TANK PRESSURE: 636 psi

BLANK TEST	0.000	08:50
INTERNAL STANDARD	VERIFIED	08:50
EXTERNAL STANDARD	0.148	08:51
BLANK TEST	0.000	08:52
EXTERNAL STANDARD	0.148	08:52
BLANK TEST	0.000	08:53
EXTERNAL STANDARD	0.148	08:53
BLANK TEST	0.000	08:54
EXTERNAL STANDARD	0.148	08:54
BLANK TEST	0.000	08:55
EXTERNAL STANDARD	0.148	08:55
BLANK TEST	0.000	08:56

Average = 0.1480
 Std Dev = 0.0000

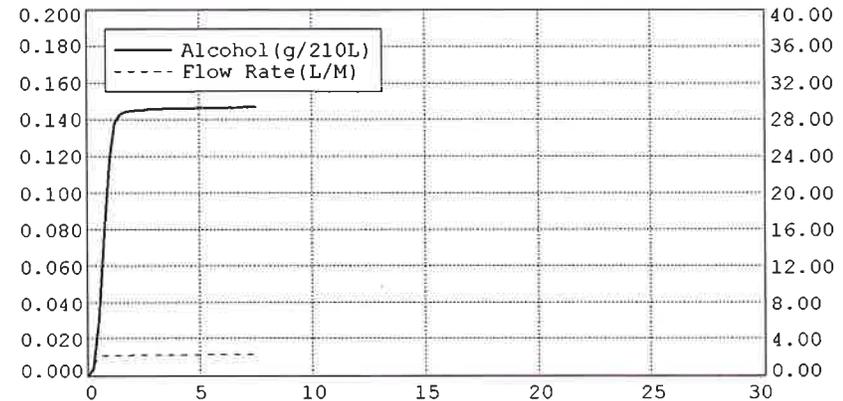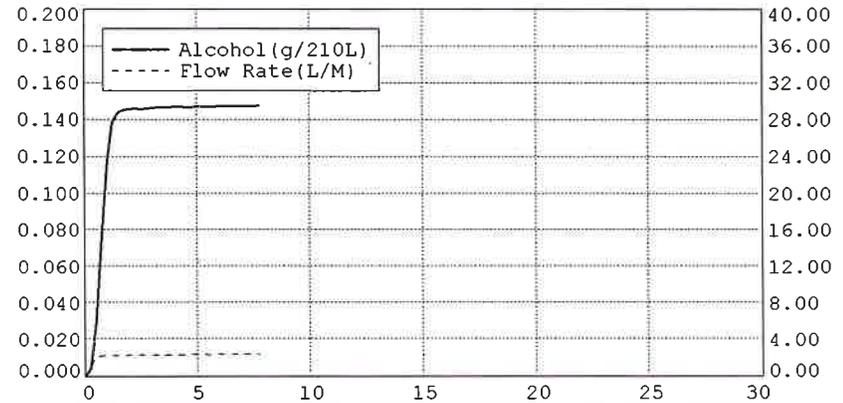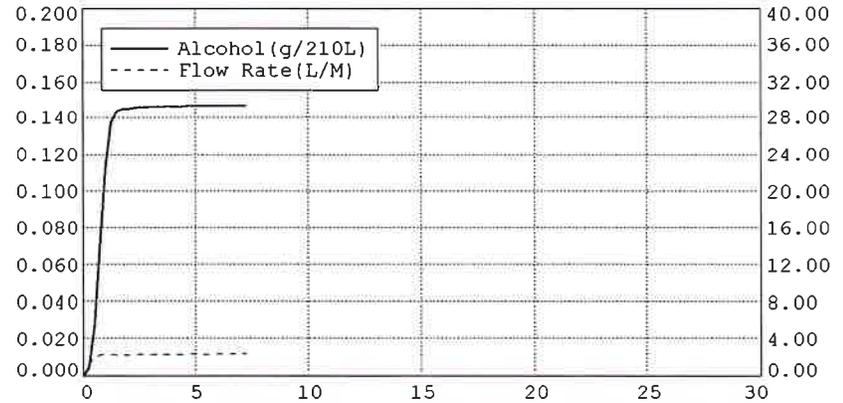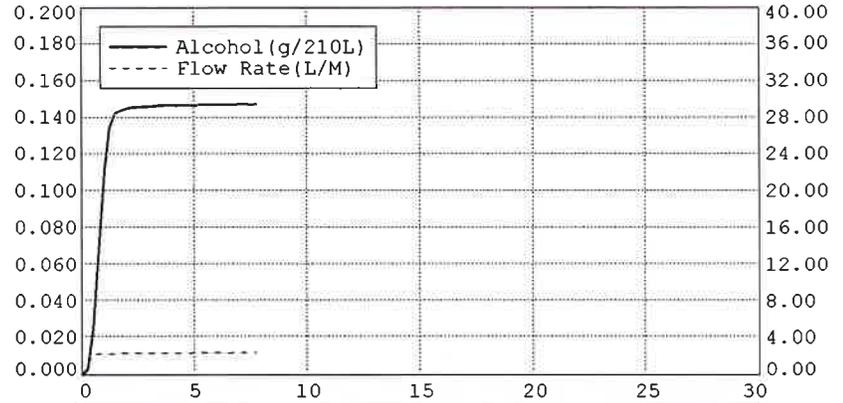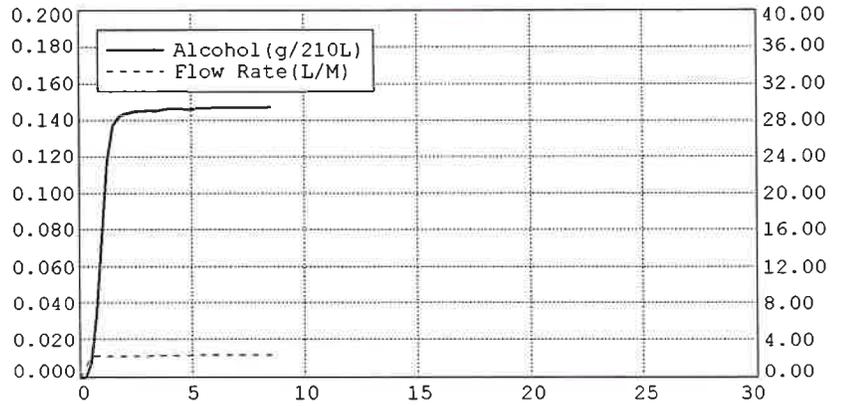

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100392






Date: 02/19/2026
 Time: 08:57:14

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.86: 0.299
 LOT #: AG427706
 EXPIRATION: 10/03/2026
 TANK PRESSURE: 177 psi

BLANK TEST	0.000	08:58
INTERNAL STANDARD	VERIFIED	08:58
EXTERNAL STANDARD	0.299	08:58
BLANK TEST	0.000	08:59
EXTERNAL STANDARD	0.299	08:59
BLANK TEST	0.000	09:00
EXTERNAL STANDARD	0.299	09:01
BLANK TEST	0.000	09:02
EXTERNAL STANDARD	0.300	09:02
BLANK TEST	0.000	09:03
EXTERNAL STANDARD	0.299	09:03
BLANK TEST	0.000	09:04

Average = 0.2992
 Std Dev = 0.0004

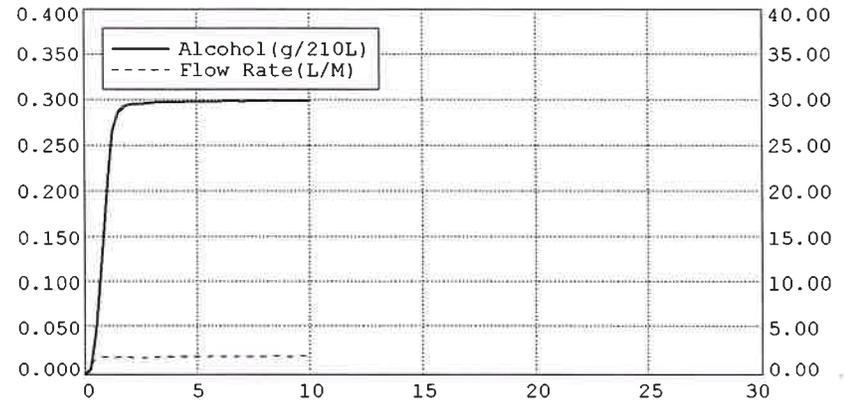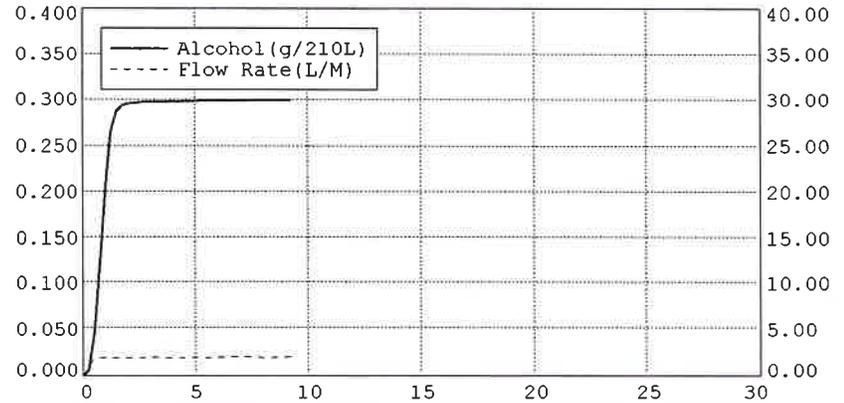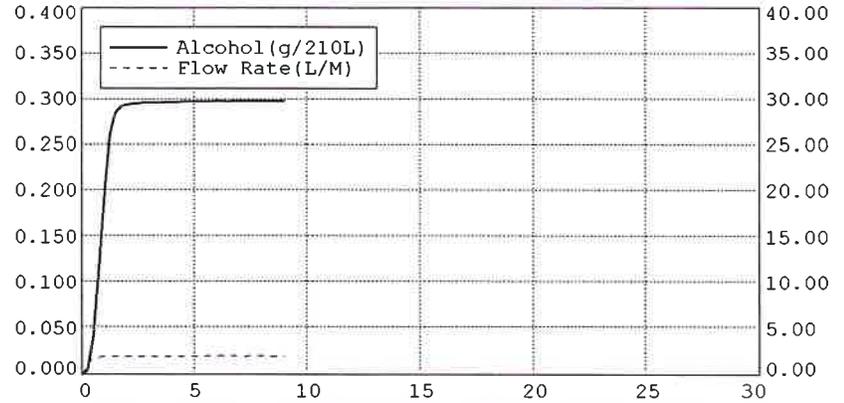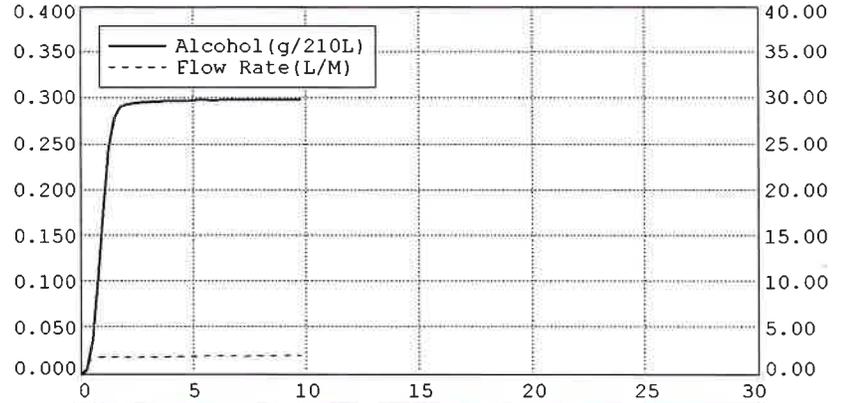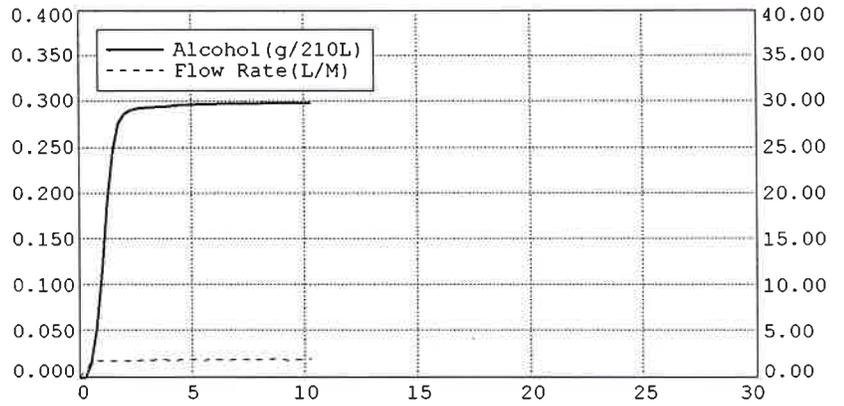

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 02/19/2026
Time: 11:15:23


SUBJECT NAME:
TEST TEST
LICENSE #: MAX ATTEMPTS

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.84: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 11:18
BLANK TEST 0.000 11:18
INTERNAL STANDARD VERIFIED 11:18
EXTERNAL STANDARD 0.079 11:18
BLANK TEST 0.000 11:19
SUBJECT SAMPLE INCOMPLETE 11:21

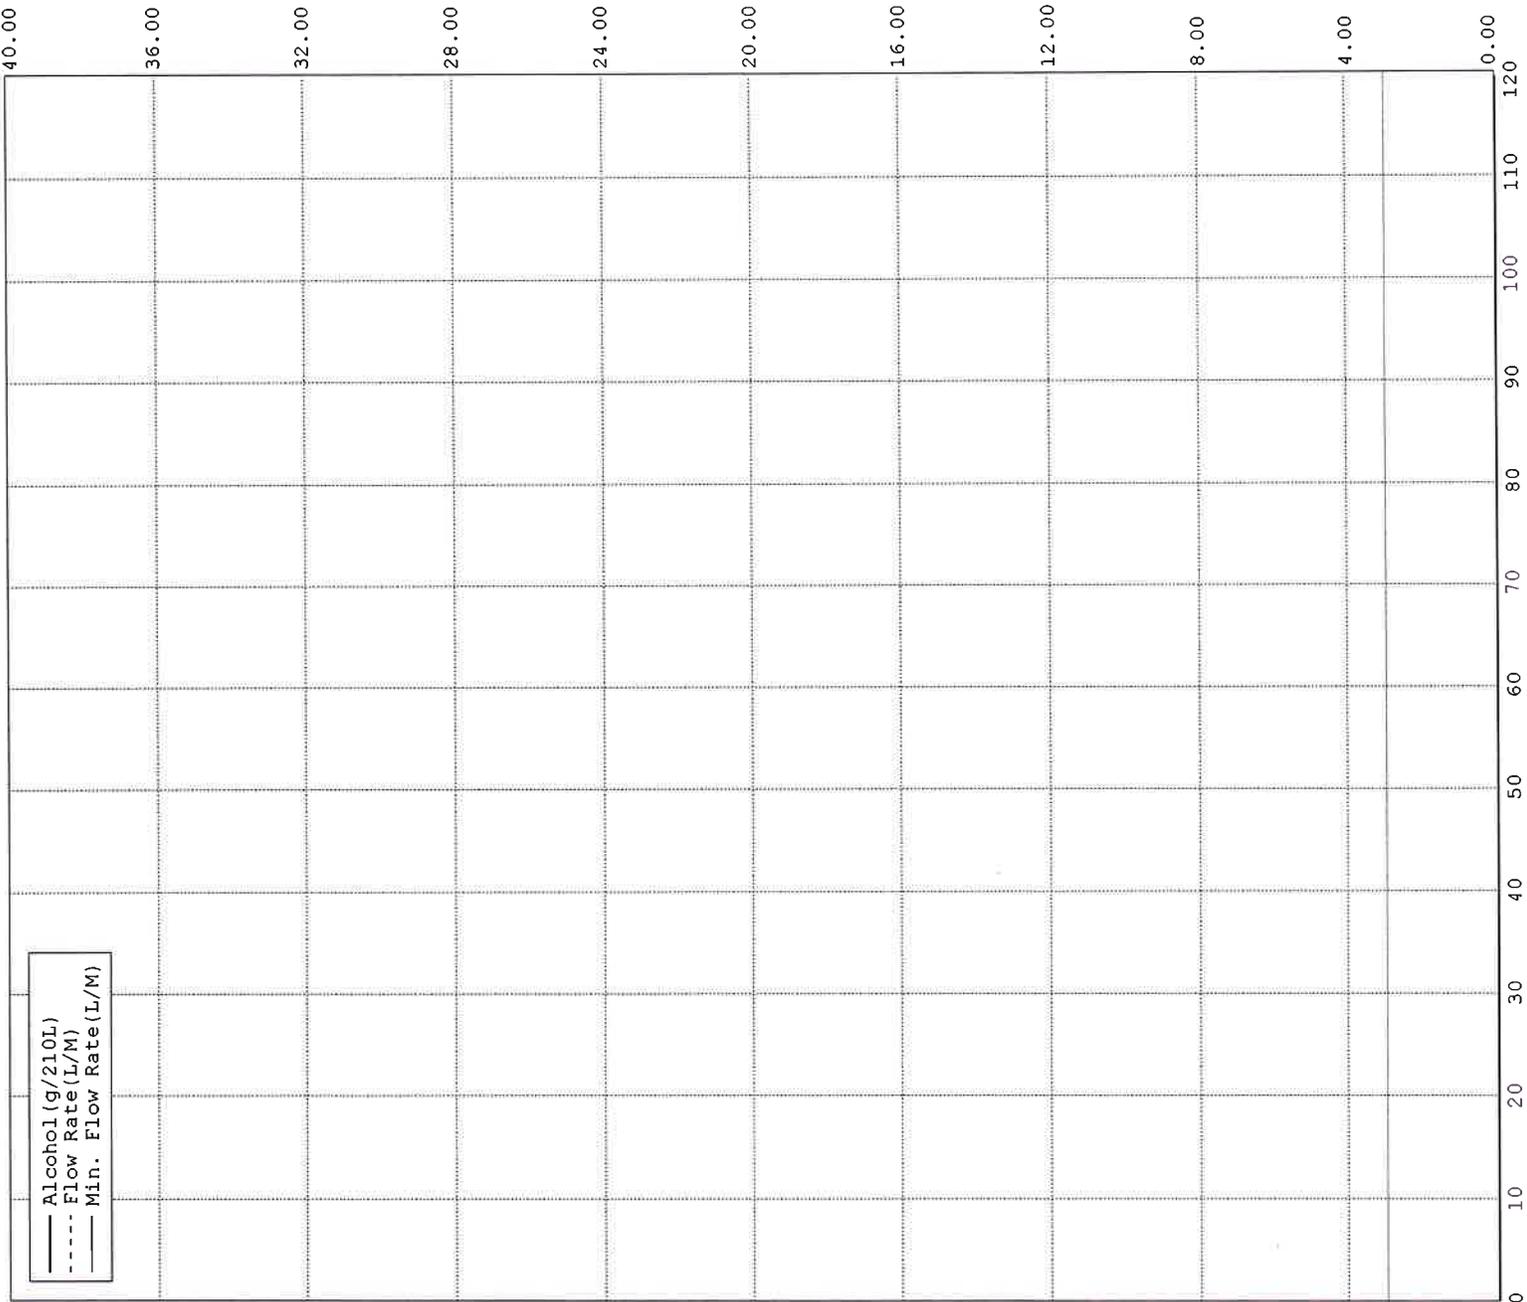

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100392

Date: 02/19/2026
Time: 11:29:40

SUBJECT NAME:
TEST TEST
LICENSE #: MAX ATTEMPTS


OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 11:31
BLANK TEST 0.000 11:31
INTERNAL STANDARD VERIFIED 11:31
EXTERNAL STANDARD 0.080 11:32
BLANK TEST 0.000 11:32
SUBJECT SAMPLE XXX 11:33

Maximum Attempts Exceeded

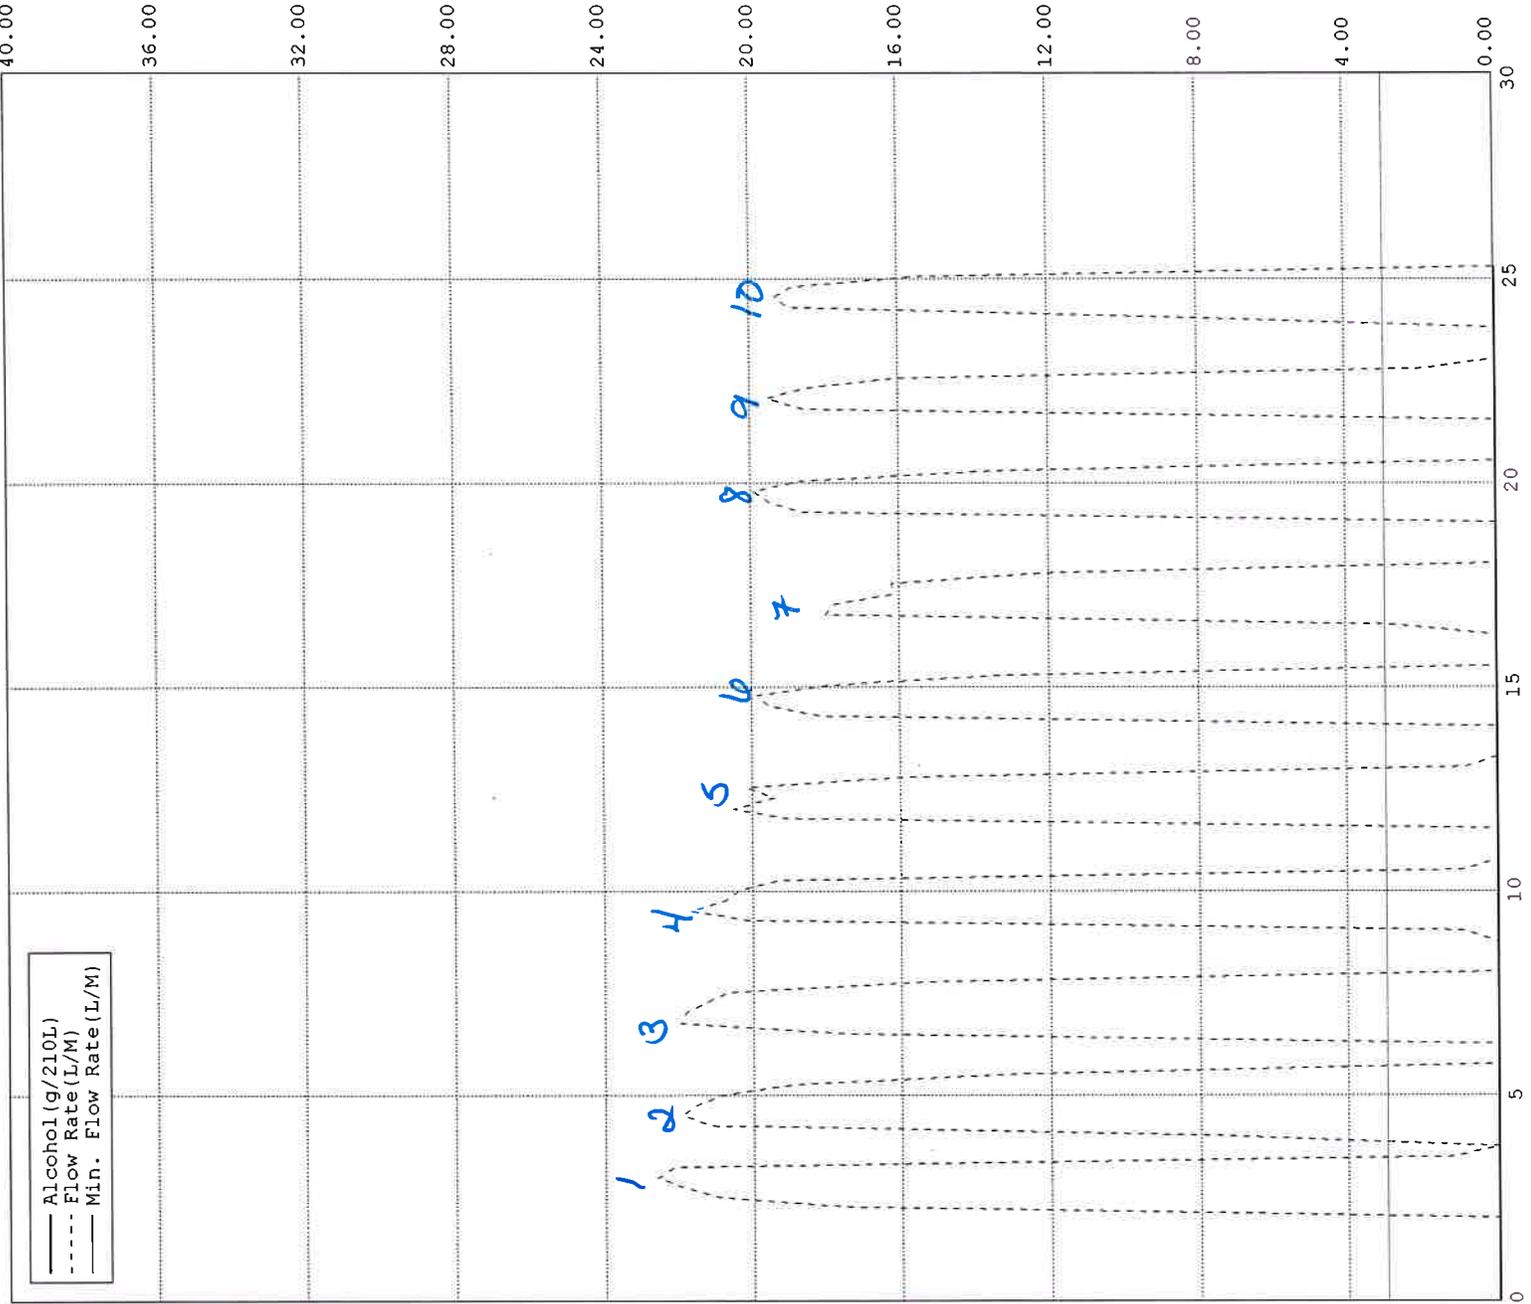

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100392

Date: 02/19/2026

Time: 11:07:44

SUBJECT NAME:

TEST TEST

LICENSE #: INVALID

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 26-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.84: 0.080

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 11:10

0.000 11:10


VERIFIED 11:10

0.080 11:10

0.000 11:11

INVALID 11:12

NCB

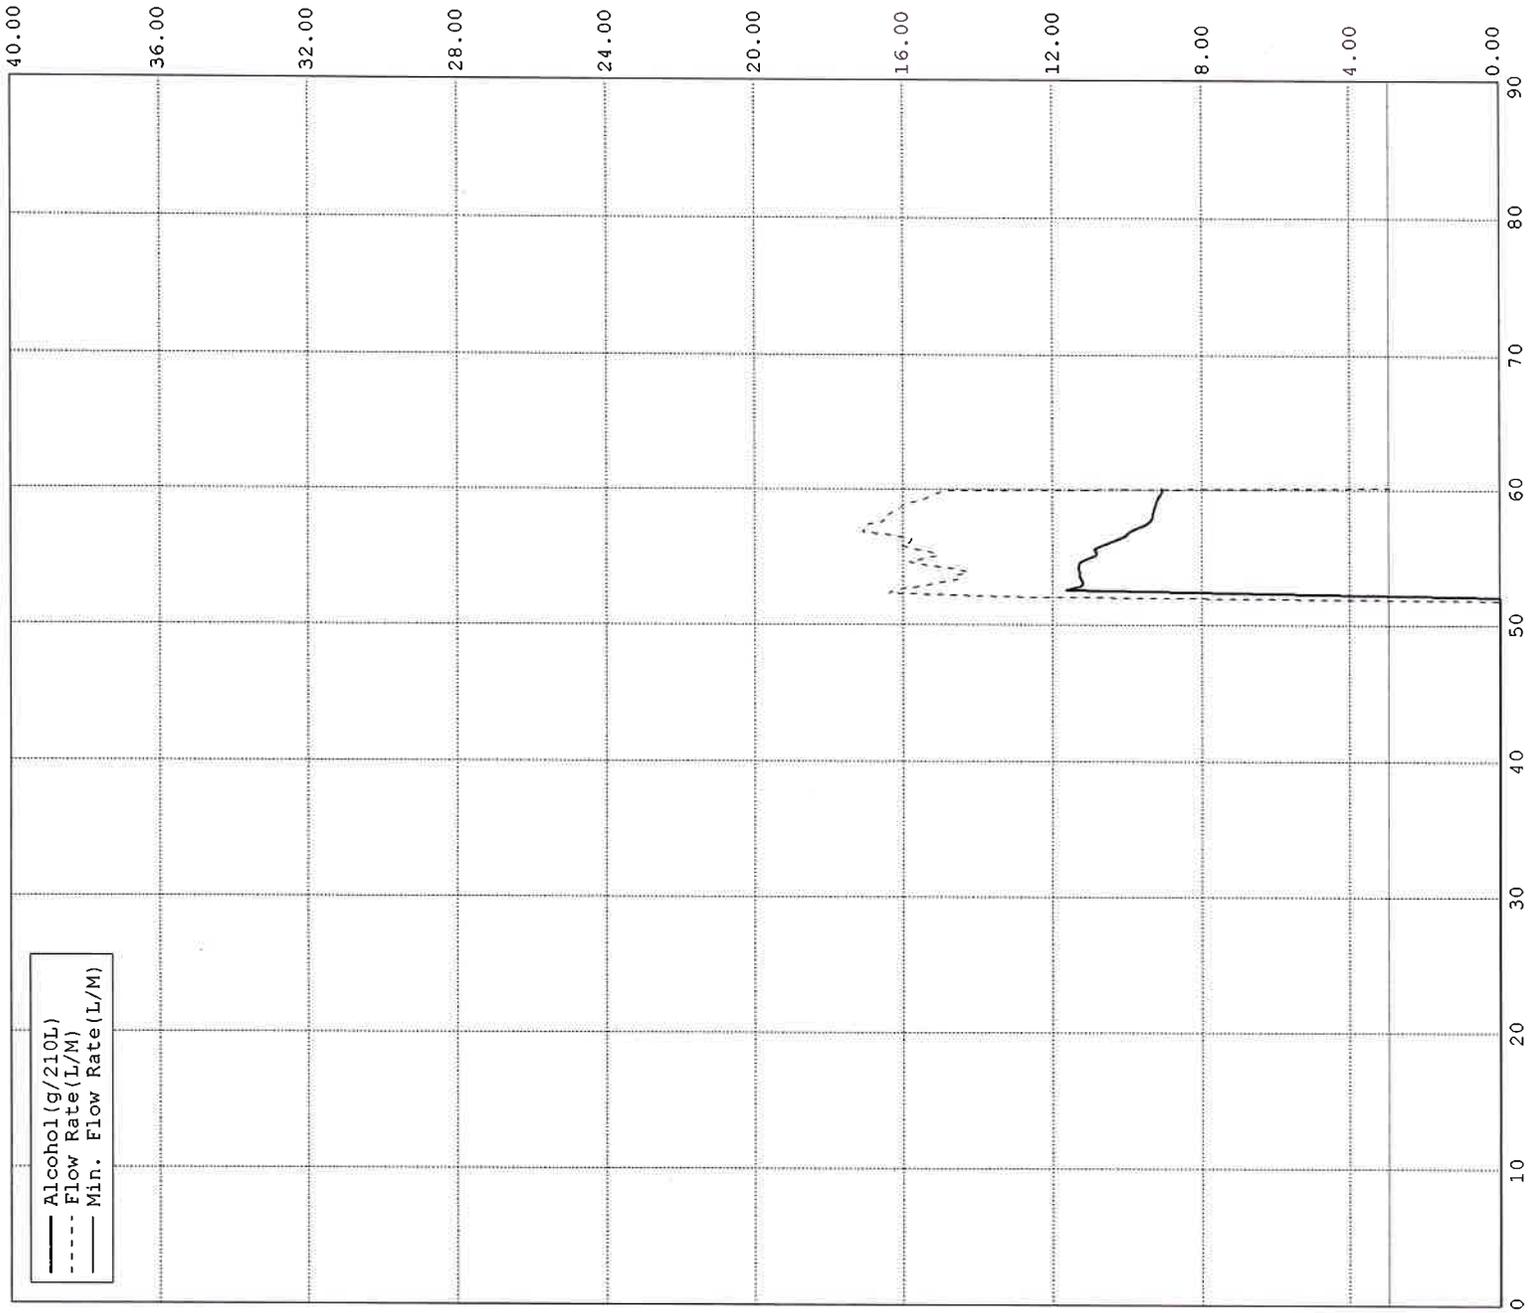

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 02/19/2026
Time: 11:01:24

SUBJECT NAME:
TEST TEST
LICENSE #: RFI


OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.84: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 11:02
BLANK TEST 0.000 11:03
INTERNAL STANDARD VERIFIED 11:03
EXTERNAL STANDARD 0.079 11:03
BLANK TEST 0.000 11:04

RFI DETECTED

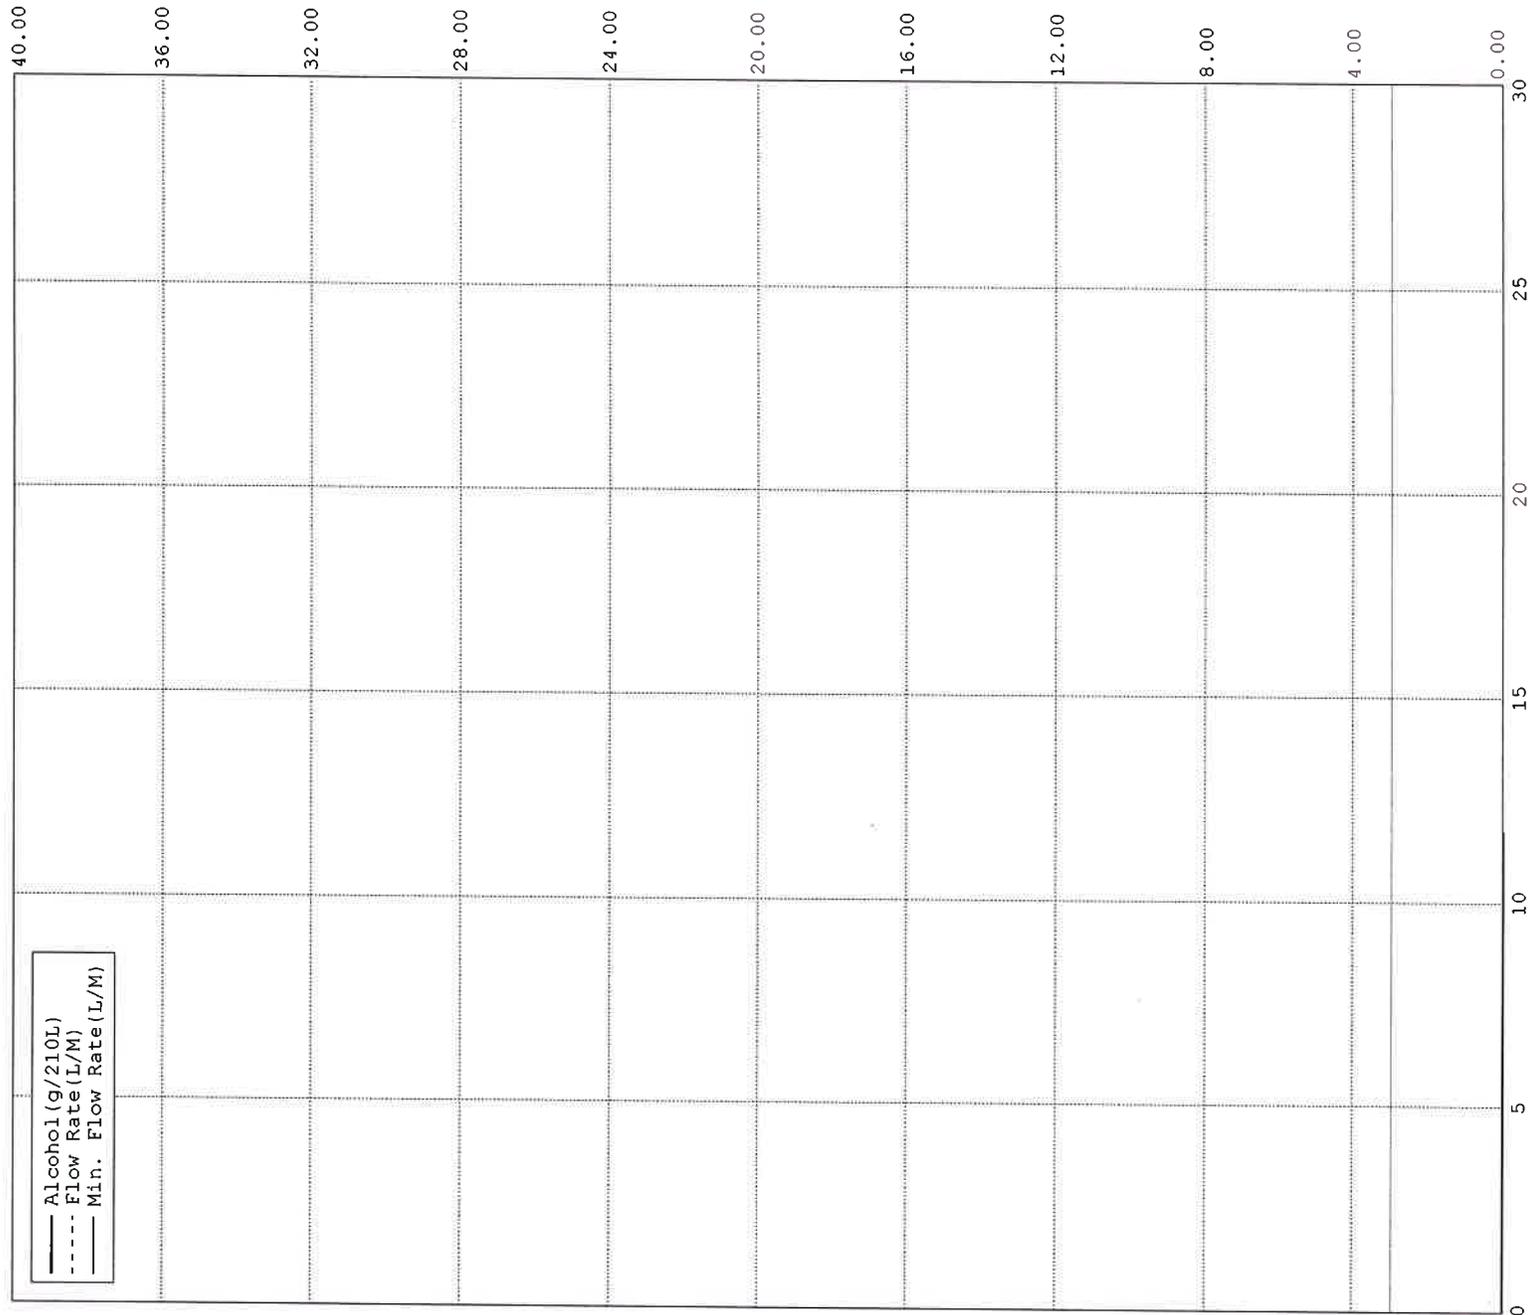

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100392

Date: 02/19/2026
 Time: 09:15:11

SUBJECT NAME:
 TEST TEST
 LICENSE #: INT-ACETONE

OPERATOR NAME:
 COLLEEN S OBRyant
 OPERATOR'S #: 6237

DEPT/AGENCY:
 AAA1
 CASE/REPORT: 26-1234
 TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.86: 0.080
 LOT #: AG436502
 EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	09:16
BLANK TEST	0.000	09:16
INTERNAL STANDARD	VERIFIED	09:16
Xq = 0.100 (0.53%)	0.080	09:16
EXTERNAL STANDARD	(0.0039)	
X[1] = 0.0797 (-0.0019)	0.000	09:17
BLANK TEST	XXX	09:18
SUBJECT SAMPLE	X[1] = 0.1086 (-0.0190) (0.0003)	

Interference Detected

Filter 2 Avg = -0.0013
Filter 3 Avg = 0.0009

CSB

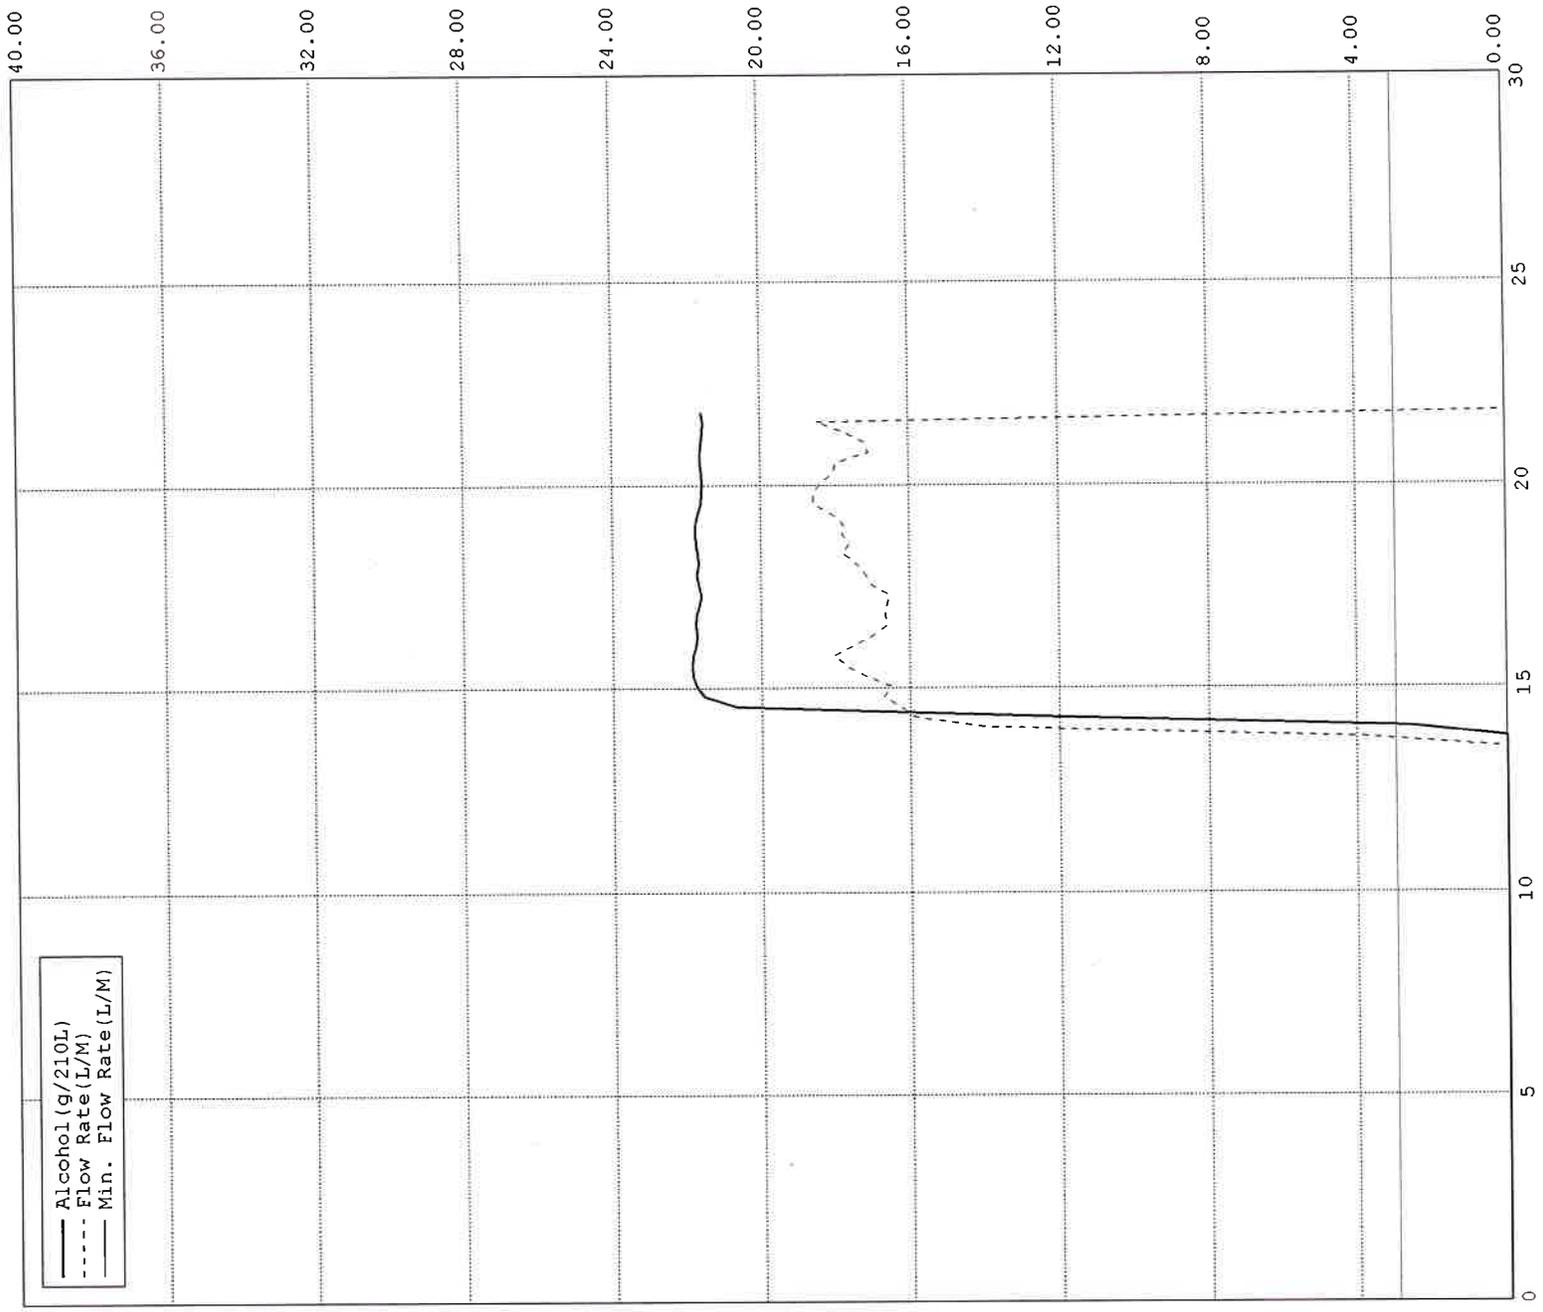

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100392

Date: 02/19/2026
Time: 09:24:38

SUBJECT NAME:
TEST TEST
LICENSE #: INT-IPA


OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.86: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 09:26
BLANK TEST 0.000 09:26
INTERNAL STANDARD VERIFIED 09:26
Xq = 0.100 (0.35%) 0.080 09:27
EXTERNAL STANDARD X[1] = 0.0801 (-0.0013) (0.0029)
BLANK TEST 0.000 09:28
SUBJECT SAMPLE XXX 09:28
X[1] = 0.1185 (-0.0219) (0.0016)

Interference Detected

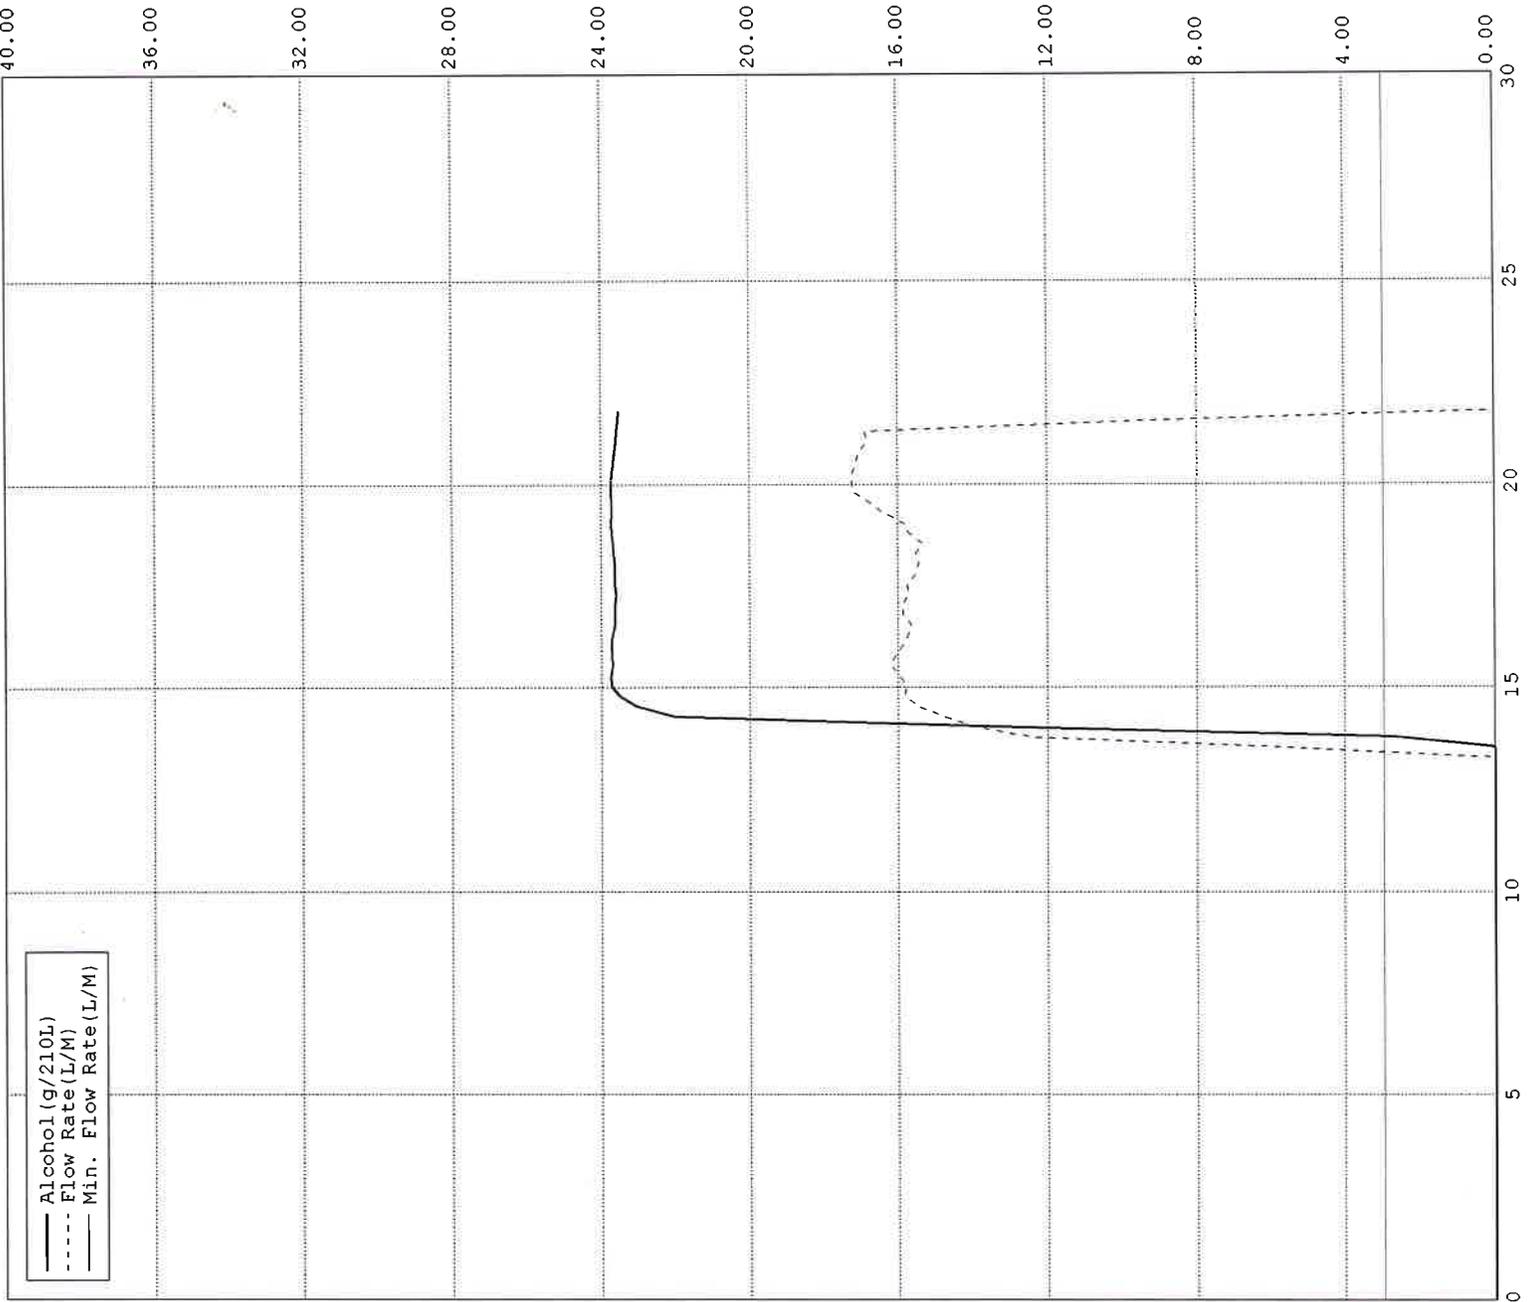

SUBJECT TEST

 Alaska Department of Public Safety
 DATAMASTER dmt: 100392

Date: 02/19/2026
 Time: 09:33:02

SUBJECT NAME:
 TEST TEST
 LICENSE #: INT-NEGATIVE


OPERATOR NAME:
 COLLEEN S OBRyant
 OPERATOR'S #: 6237

DEPT/AGENCY:
 AAA1
 CASE/REPORT: 26-1234
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.86: 0.080
 LOT #: AG436502
 EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	09:34
BLANK TEST	0.000	09:34
INTERNAL STANDARD	VERIFIED	09:34
EXTERNAL STANDARD	0.080	09:35
Xq = 0.100 (0.53%)		
X[1] = 0.0800 (-0.0008)	(0.0031)	
BLANK TEST	0.000	09:36
SUBJECT SAMPLE (Vol=2.15L)	0.094	09:36
X[1] = 0.0944 (0.0003)	(0.0013)	
BLANK TEST	0.000	09:37
EXTERNAL STANDARD	0.080	09:37
X[1] = 0.0799 (-0.0012)	(0.0015)	
BLANK TEST	0.000	09:38

CA

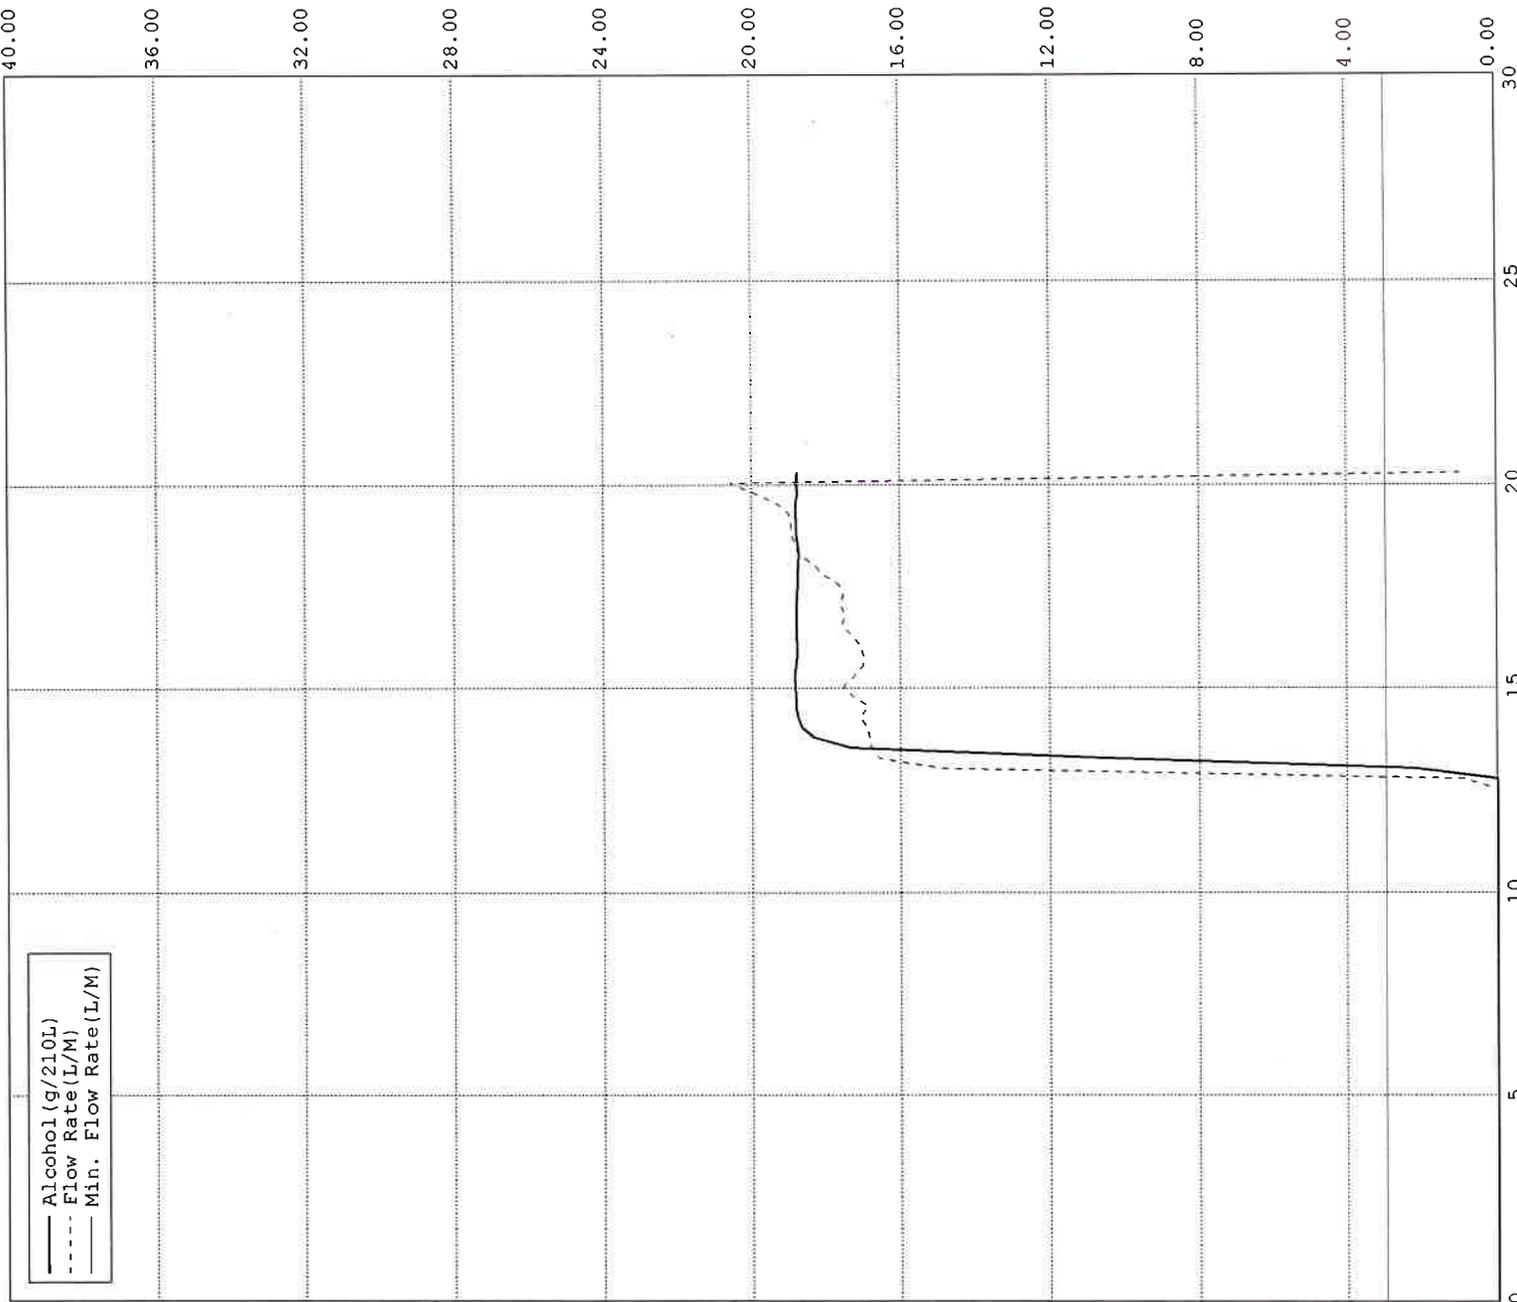

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100392

Date: 02/19/2026

Time: 11:48:04

SUBJECT NAME:

TEST TEST

LICENSE #: NDS1

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 26-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.83: 0.080

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	TIME
BLANK TEST	0.000	11:49
INTERNAL STANDARD	VERIFIED	11:49
EXTERNAL STANDARD	0.081	11:49
BLANK TEST	0.000	11:50
SUBJECT SAMPLE (Vol=1.99L)	0.000	11:51
BLANK TEST	0.000	11:51
EXTERNAL STANDARD	0.080	11:52
BLANK TEST	0.000	11:53

