



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100387

Report Issue Date: 12/21/2023
Date Received: 2023-10-23
Condition of Item: Good

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

Start Date 11/06/2023 - As Found - **End Date 11/06/2023** As Found - Evaluation Analyst: Carlie Glaister
 As Found Conditions - Barometric Pressure (inHg): 29.13 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.9
 Relative Humidity (%): 22

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.019	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.078	AG310901	0.079	0.079	0.079	0.079	0.079	0.079	0.079
0.300	0.292	AG217903	0.298	0.297	0.297	0.298	0.297	0.297	0.297

Cleared memory & reset options before eval. Recommend adjustment due to internal standard being near 3%.

Start Date 11/30/2023 - As Left - **End Date 12/04/2023**

As Left Conditions - Barometric Pressure (inHg): 28.83 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.4 Relative Humidity (%): 19

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.190	AG217902	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002	
0.040	0.039	AG217904	0.039	0.039	0.039	0.039	0.040	0.039	+/- 0.003	
0.080	0.077	AG310901	0.078	0.078	0.078	0.078	0.078	0.078	+/- 0.004	
0.100	0.096	AG211003	0.098	0.098	0.098	0.097	0.098	0.098	+/- 0.004	
0.150	0.145	AG134205	0.147	0.147	0.147	0.147	0.147	0.147	+/- 0.005	
0.300	0.289	AG217903	0.294	0.294	0.295	0.295	0.295	0.295	+/- 0.011	

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Carlie Glaister on 12/04/2023

carlie.glaister@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 12/21/2023

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100387 Analyst: Carlie Glaister Start Date: 11/30/23

- Diagnostic Test (attached)
- Internal Standard value \leq 3.00%
- Adjust voltages, if needed
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.5 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.83 Temperature (C): 22.4 Relative Humidity (%) 19

Linearity Test (attached)

0.020g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217902</u>	Exp: <u>6/28/24</u>
0.040g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217904</u>	Exp: <u>6/28/24</u>
0.080g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-310901</u>	Exp: <u>4/19/25</u>
0.100g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-211003</u>	Exp: <u>4/20/24</u>
0.150g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-134205</u>	Exp: <u>12/8/23</u>
0.300g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217903</u>	Exp: <u>6/28/24</u>

Functional Tests (attached)

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles)

Acetone Mnf: Lifoloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR24176 Verification Performed?

Isopropanol Mnf: Lifoloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR24177 Verification Performed?

Neg. Control Mnf: Lifoloc Lot: 22HP41201 Level: 0.100 Exp: 9/24/24

Simulator S/N: DR26267 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 230631104 Calibration Due Date: 9/19/2025

- Verify stylus is calibrated
- Non-Drinking Subject Test
- Reset Options
- Upload
- Clear Memory
- Remove Tank Prior to Shutdown
- Verification of Calibration (VOC)
- Calibration End Date: 12/1/23

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100387

Date: 11/30/2023
Time: 09:25:43

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 46.3°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.83 V PASSED
(1.10 V - 2.56 V)
Cooler Voltage = 1.76 V PASSED
(1.06 V - 2.46 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Freq = 543 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 28.8 in

PUMP INFO

Flow Rate = 4.515 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.092 1.22% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100387

Date: 11/30/2023
Time: 11:47 AM

Temperatures (°C)

Sample Cell: 48.9°C
Breath Tube: 46.6°C

Current Barometer 28.8 in
Volume (Ltr) 1.49

Settings

Lamp: 1.83 V
Bias: 80 V
Cooler: 1.66 V
Chopper: 543 Hz

Voltages (V)

Flow: 1.05 V
Detector: 0.051 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100387

Date: 11/07/2023
Time: 09:05:01

OPERATOR NAME:
CARLIE GLAISTER
CERTIFICATE #: 10436

Ca = 0.1000
CAL = 0.989575 0.800 <= CAL < 1.200
b1 = 0.0011 0.0000 <= b1 < 0.0040
b2 = 0.0059 0.0010 <= b2 < 0.0100
b3 = 0.0008 0.0000 <= b3 < 0.0040
Xq = 0.0932 0.0500 <= Xq < 0.2000
a21 = 1.172262 1.050 <= a21 < 1.300
a31 = 0.477361 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100387

Date: 11/30/2023
Time: 11:49:41

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.84: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	11:50
BLANK TEST	0.000	11:50
INTERNAL STANDARD	VERIFIED	11:50
EXTERNAL STANDARD	0.078	11:51
BLANK TEST	0.000	11:52
SUBJECT SAMPLE (Vol=1.60L)	0.000	11:53
BLANK TEST	0.000	11:54
EXTERNAL STANDARD	0.078	11:54
BLANK TEST	0.000	11:55

* 1.4L - syringe slipped out of breath hose, 1.4L was repeated. 066-11/30/23

CYG

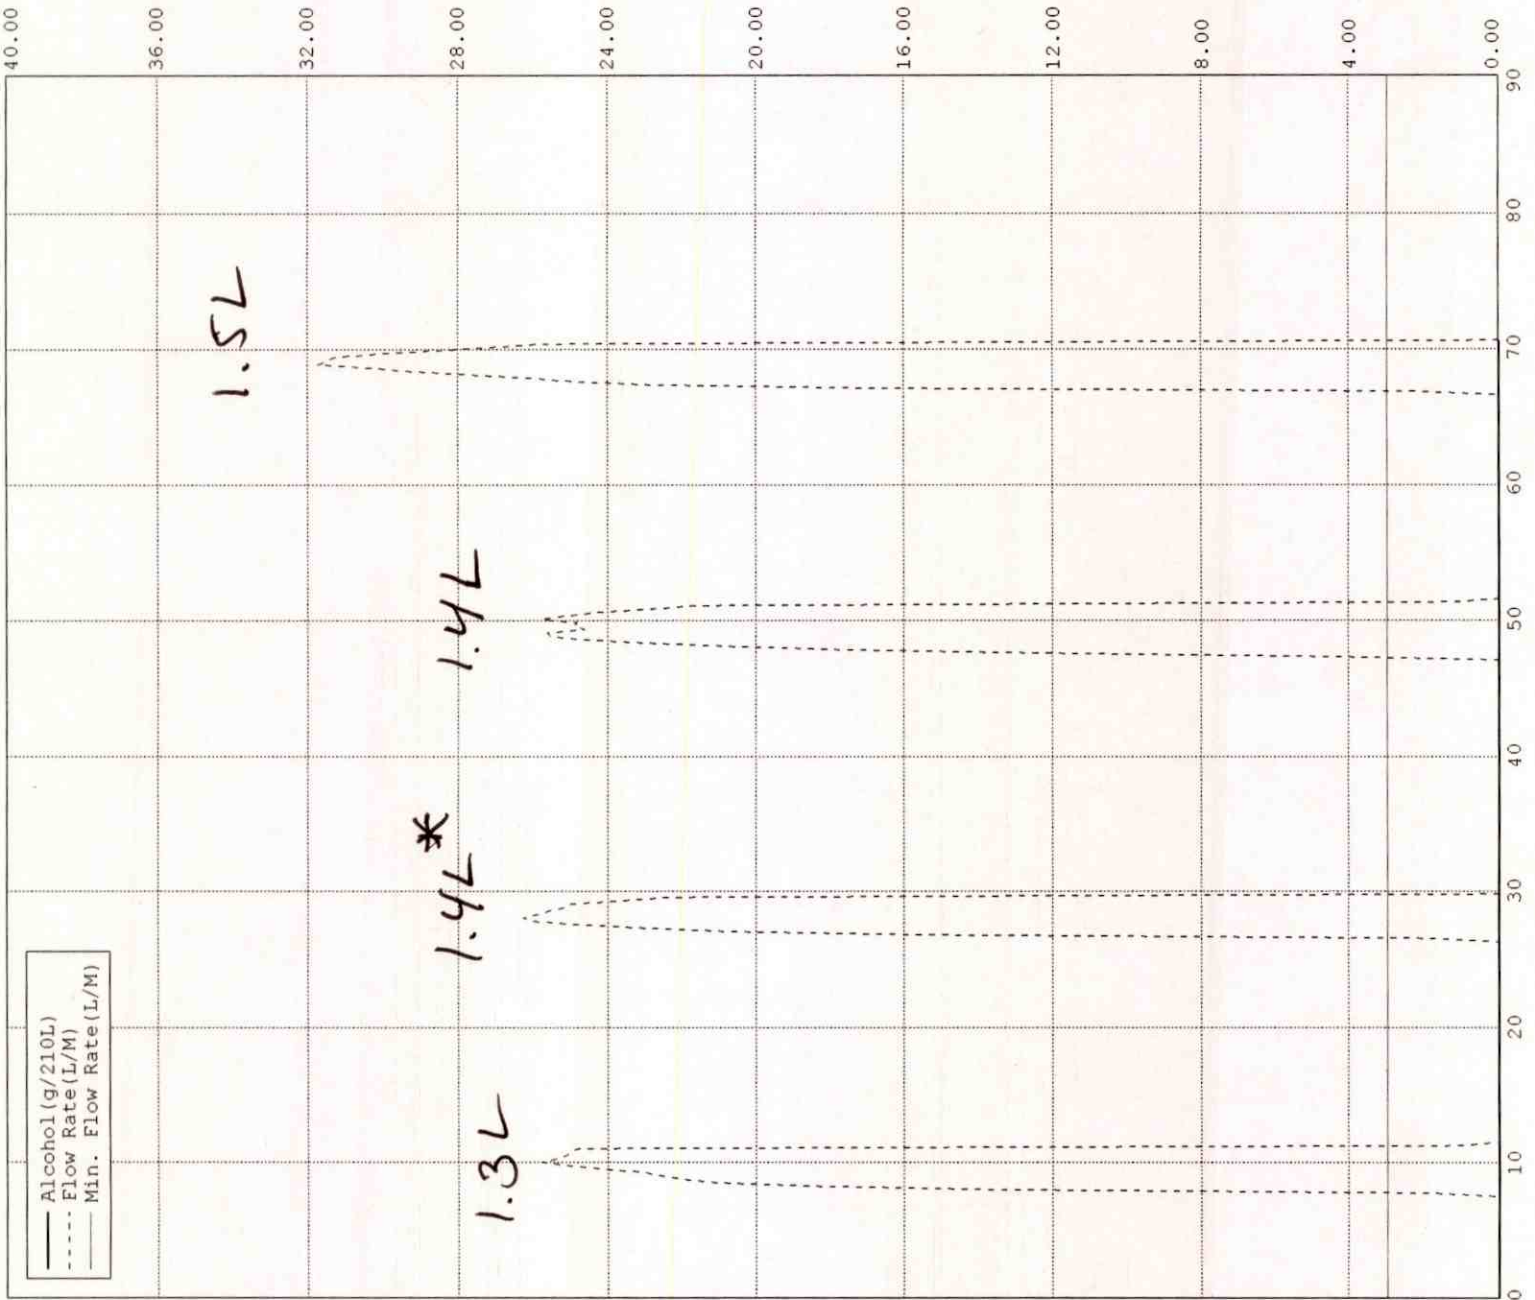

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100387

Date: 11/30/2023
 Time: 12:17:17

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.019	0.0200	0.0000
0.039	0.0392	0.0004
0.077	0.0780	0.0000
0.096	0.0978	0.0004
0.145	0.1470	0.0000
0.289	0.2946	0.0005

SLOPE = 1.018787
 R² = 0.999973

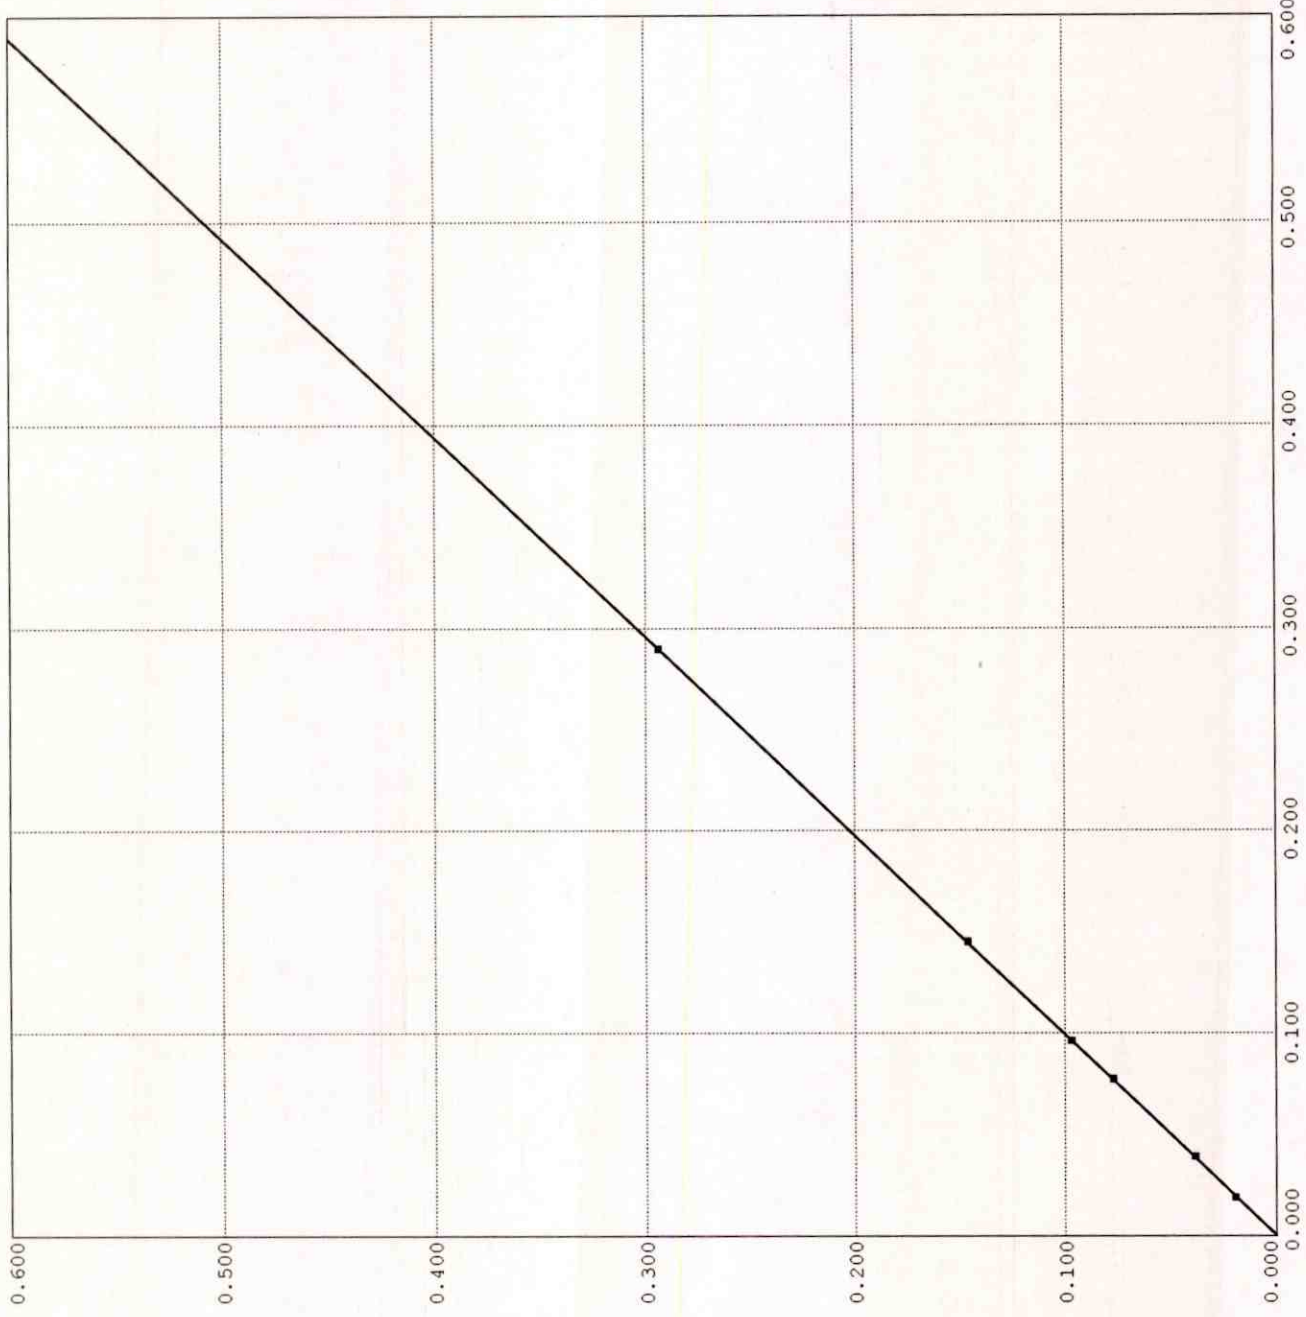

OK

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100387






Date: 11/30/2023
 Time: 12:17:19

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 28.85: 0.019
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 503 psi

BLANK TEST	0.000	12:18
INTERNAL STANDARD	VERIFIED	12:18
EXTERNAL STANDARD	0.020	12:18
BLANK TEST	0.000	12:19
EXTERNAL STANDARD	0.020	12:20
BLANK TEST	0.000	12:20
EXTERNAL STANDARD	0.020	12:21
BLANK TEST	0.000	12:22
EXTERNAL STANDARD	0.020	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.020	12:23
BLANK TEST	0.000	12:24

Average = 0.0200
 Std Dev = 0.0000

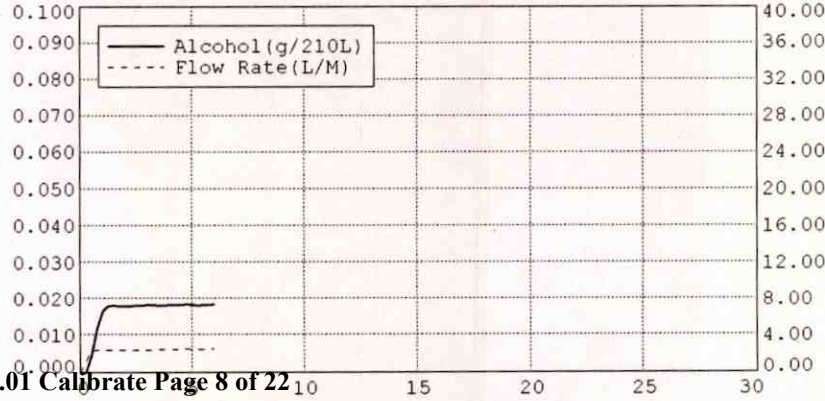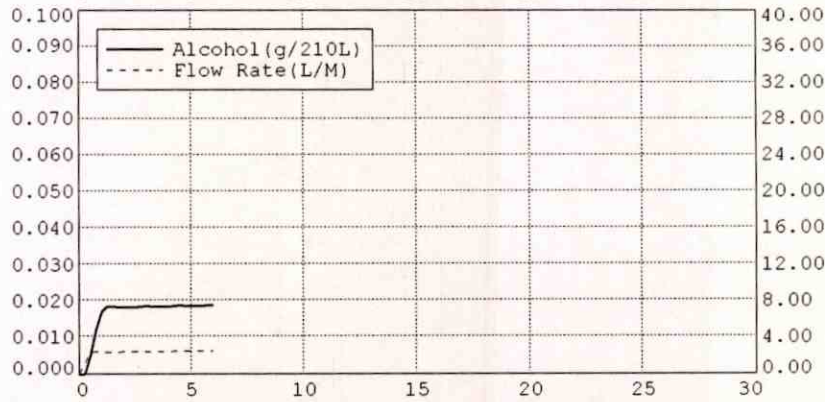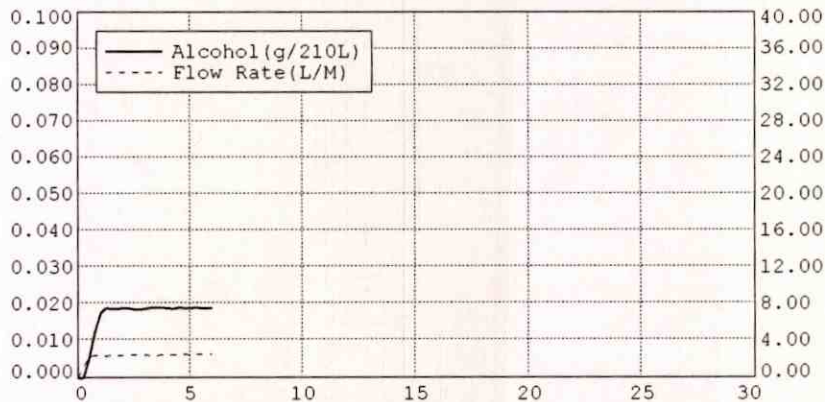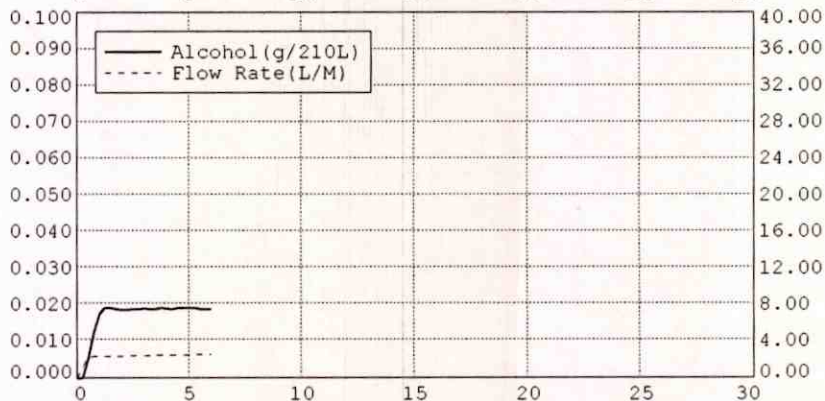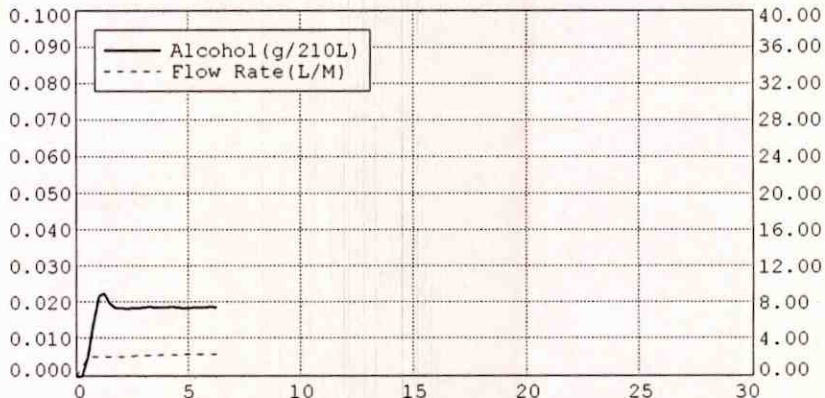

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100387






Date: 11/30/2023
 Time: 12:32:57

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 28.85: 0.039
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 922 psi

BLANK TEST	0.000	12:34
INTERNAL STANDARD	VERIFIED	12:34
EXTERNAL STANDARD	0.039	12:34
BLANK TEST	0.000	12:35
EXTERNAL STANDARD	0.039	12:35
BLANK TEST	0.000	12:36
EXTERNAL STANDARD	0.039	12:36
BLANK TEST	0.000	12:37
EXTERNAL STANDARD	0.039	12:37
BLANK TEST	0.000	12:38
EXTERNAL STANDARD	0.040	12:38
BLANK TEST	0.000	12:39

Average = 0.0392
 Std Dev = 0.0004

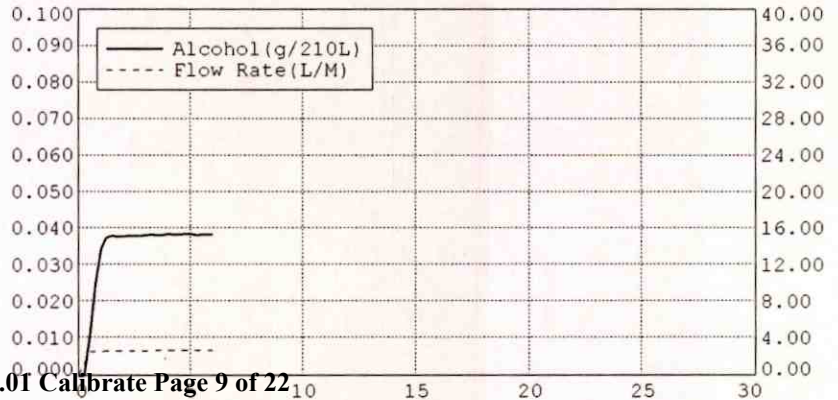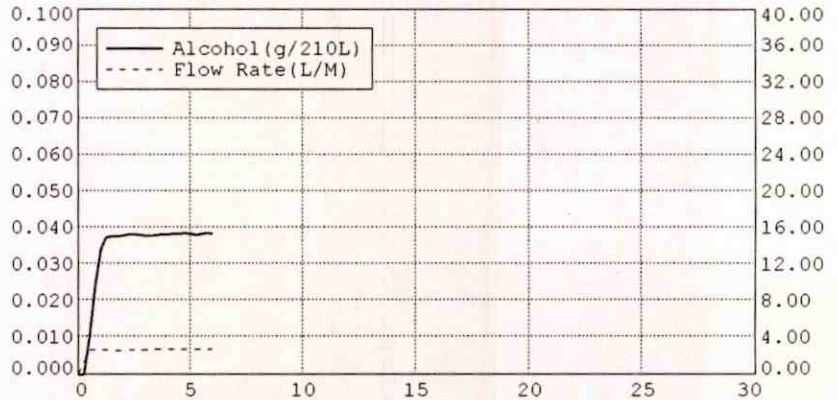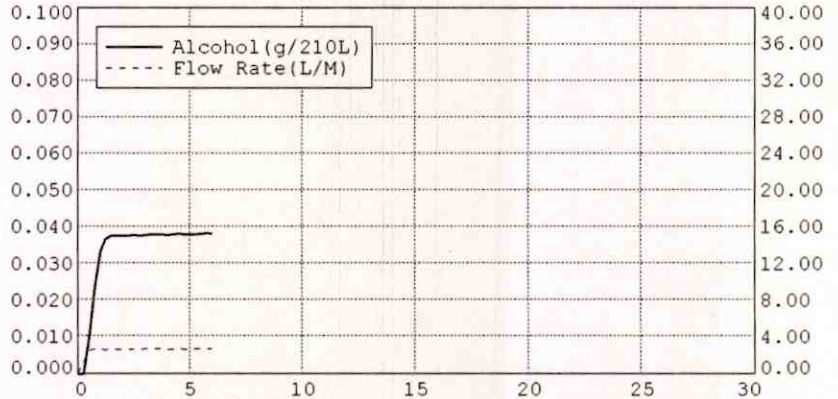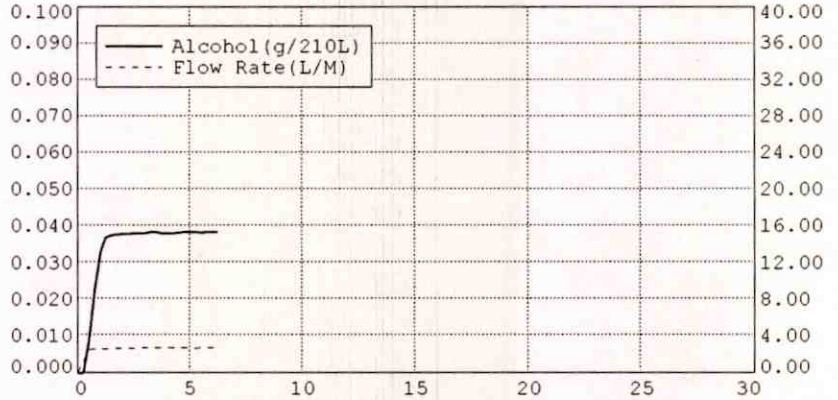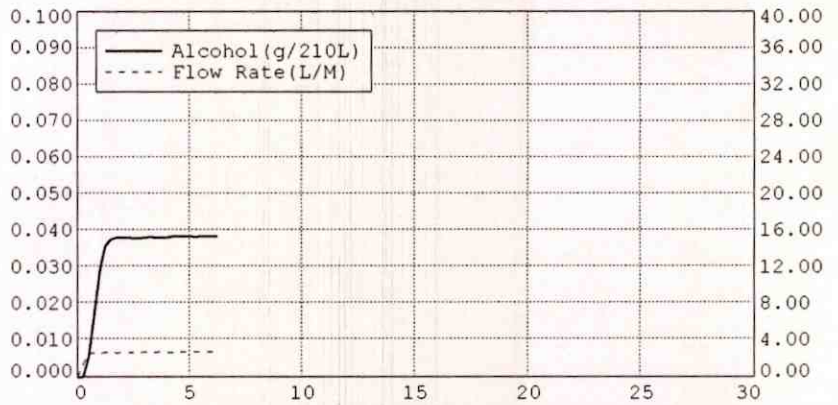

LINEARITY CHECK: Control Test 3

 Alaska Department of Public Safety
 DATAMASTER dmt: 100387






Date: 11/30/2023
 Time: 14:29:14

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 28.84: 0.077
 LOT #: AG310901
 EXPIRATION: 04/19/2025
 TANK PRESSURE: 1090 psi

BLANK TEST	0.000	14:30
INTERNAL STANDARD	VERIFIED	14:30
EXTERNAL STANDARD	0.078	14:30
BLANK TEST	0.000	14:31
EXTERNAL STANDARD	0.078	14:31
BLANK TEST	0.000	14:32
EXTERNAL STANDARD	0.078	14:33
BLANK TEST	0.000	14:33
EXTERNAL STANDARD	0.078	14:34
BLANK TEST	0.000	14:35
EXTERNAL STANDARD	0.078	14:35
BLANK TEST	0.000	14:36

Average = 0.0780
 Std Dev = 0.0000

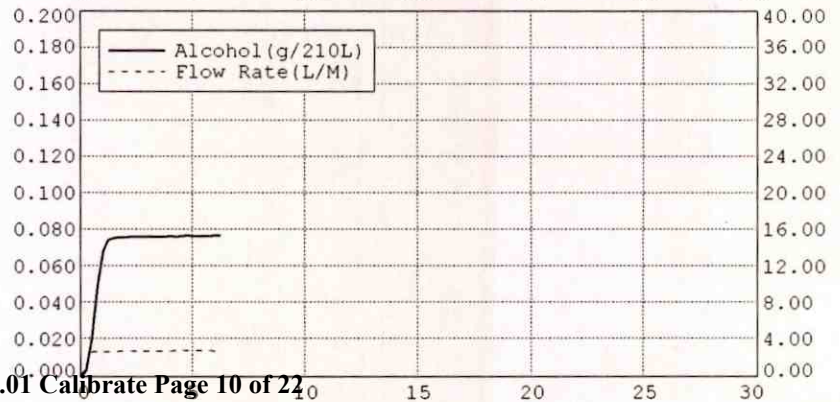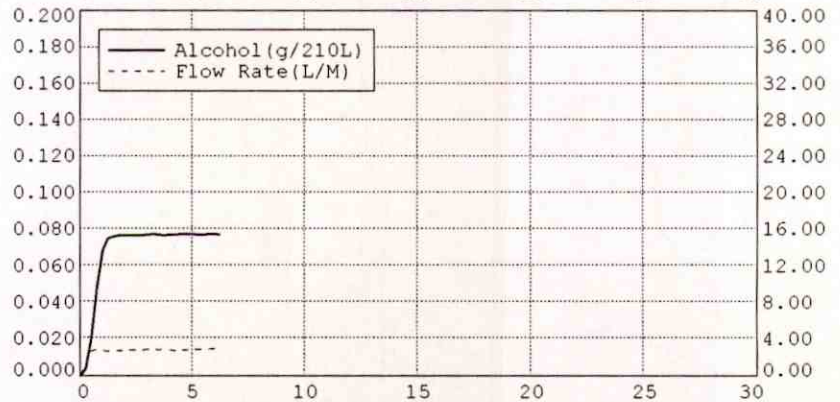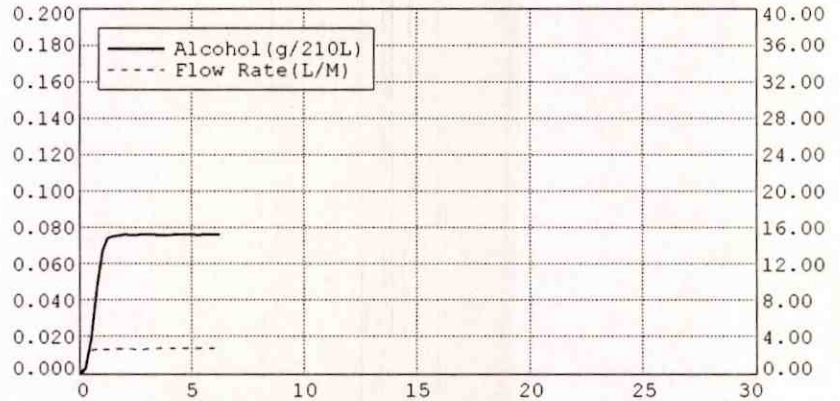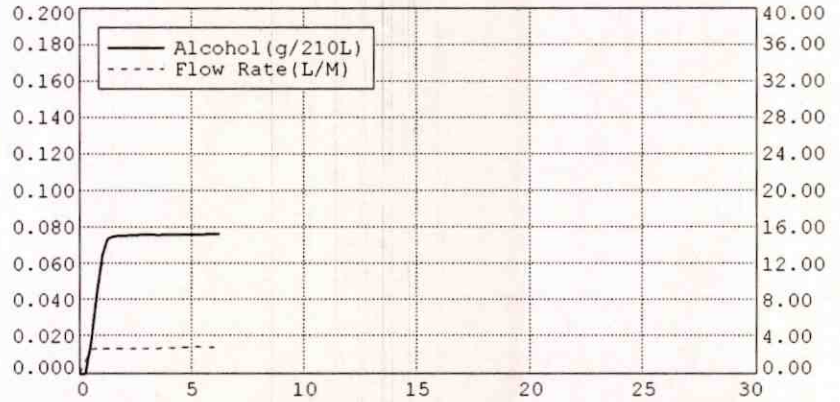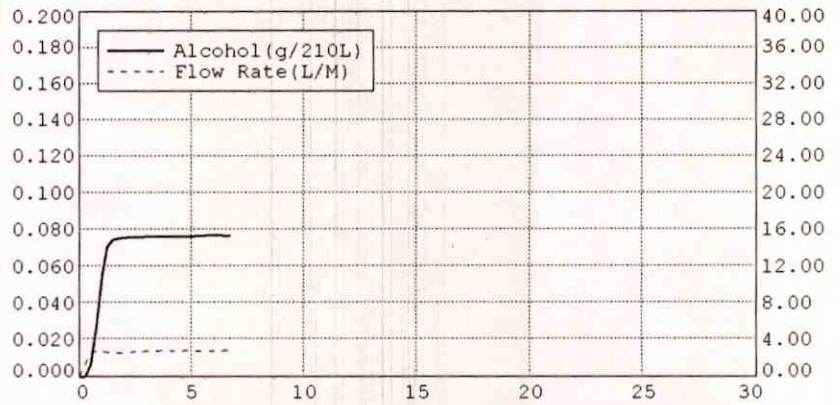

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100387






Date: 11/30/2023
 Time: 14:44:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 28.85: 0.096
 LOT #: AG211003
 EXPIRATION: 04/20/2024
 TANK PRESSURE: 459 psi

BLANK TEST	0.000	14:46
INTERNAL STANDARD	VERIFIED	14:46
EXTERNAL STANDARD	0.098	14:46
BLANK TEST	0.000	14:47
EXTERNAL STANDARD	0.098	14:47
BLANK TEST	0.000	14:48
EXTERNAL STANDARD	0.098	14:48
BLANK TEST	0.000	14:49
EXTERNAL STANDARD	0.097	14:49
BLANK TEST	0.000	14:50
EXTERNAL STANDARD	0.098	14:50
BLANK TEST	0.000	14:51

Average = 0.0978
 Std Dev = 0.0004

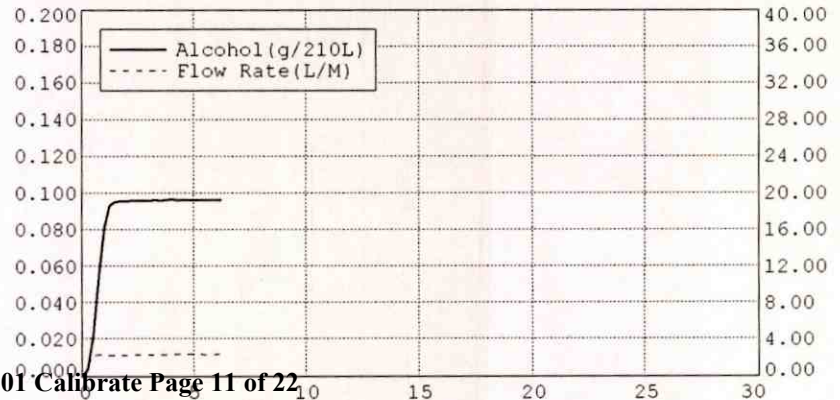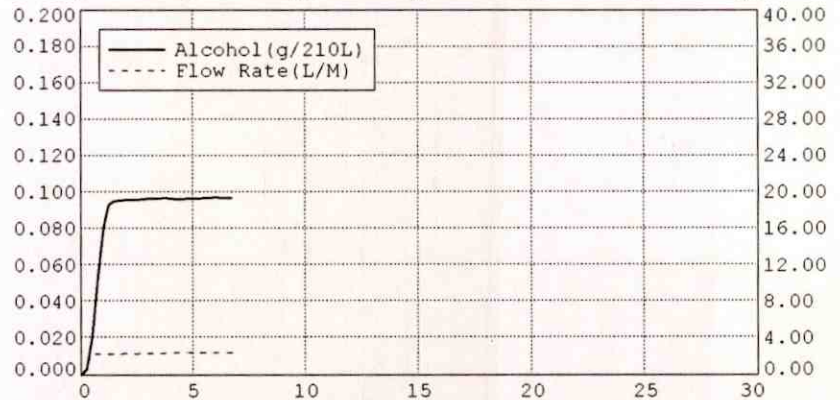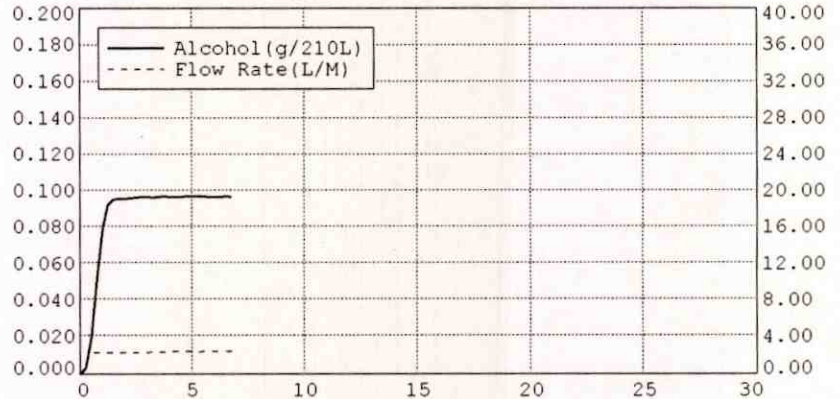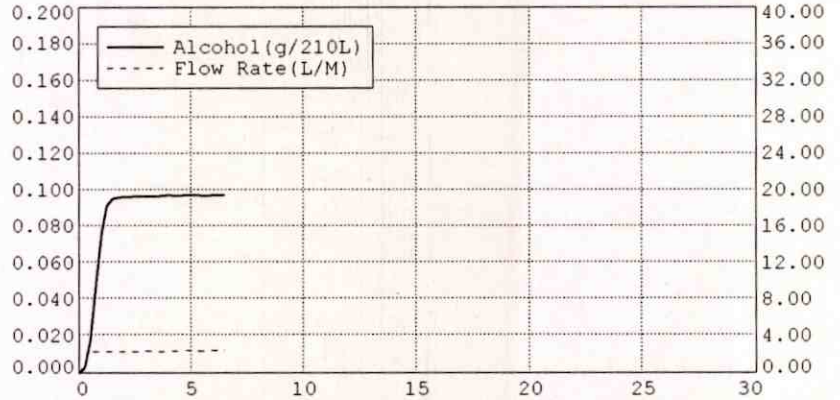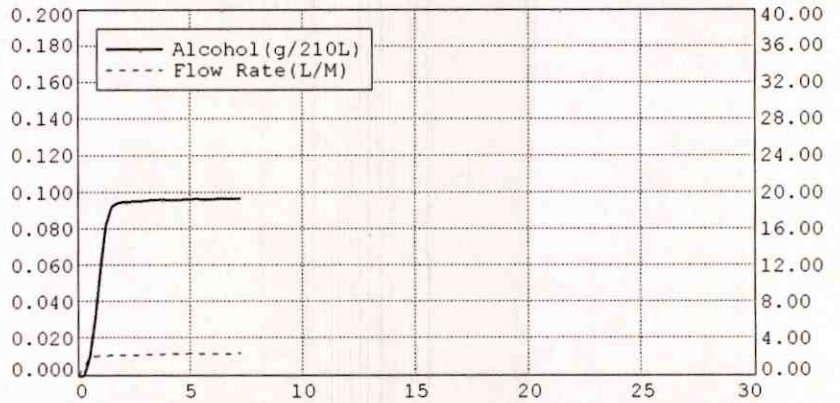

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100387






Date: 11/30/2023
 Time: 14:52:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 28.85: 0.145
 LOT #: AG134205
 EXPIRATION: 12/08/2023
 TANK PRESSURE: 474 psi

BLANK TEST	0.000	14:54
INTERNAL STANDARD	VERIFIED	14:54
EXTERNAL STANDARD	0.147	14:54
BLANK TEST	0.000	14:55
EXTERNAL STANDARD	0.147	14:55
BLANK TEST	0.000	14:56
EXTERNAL STANDARD	0.147	14:57
BLANK TEST	0.000	14:57
EXTERNAL STANDARD	0.147	14:58
BLANK TEST	0.000	14:59
EXTERNAL STANDARD	0.147	14:59
BLANK TEST	0.000	15:00

Average = 0.1470
 Std Dev = 0.0000

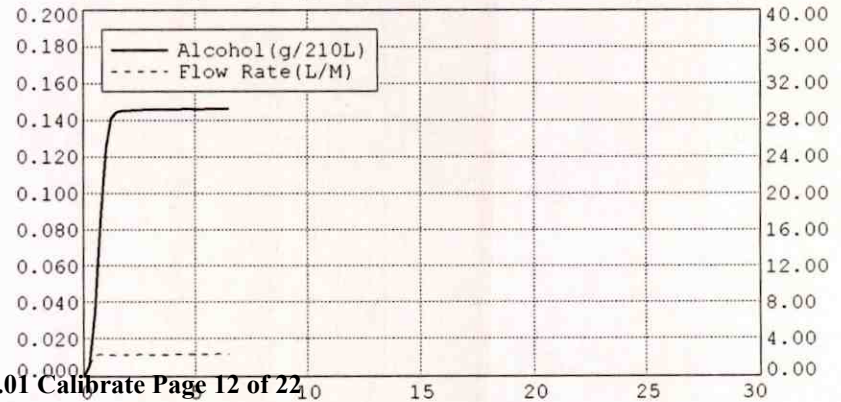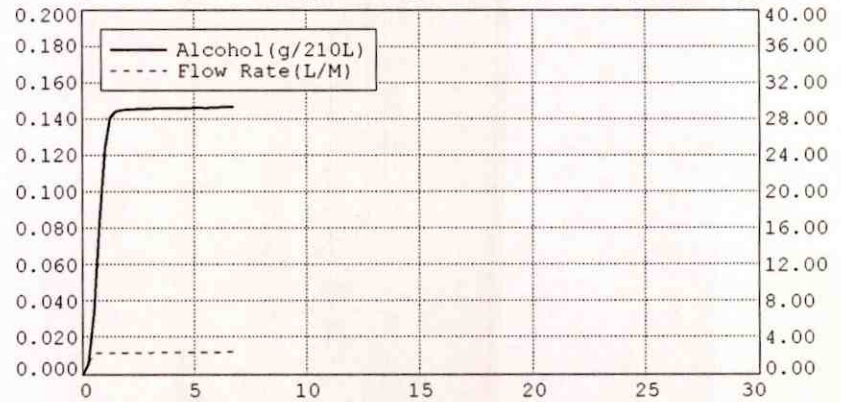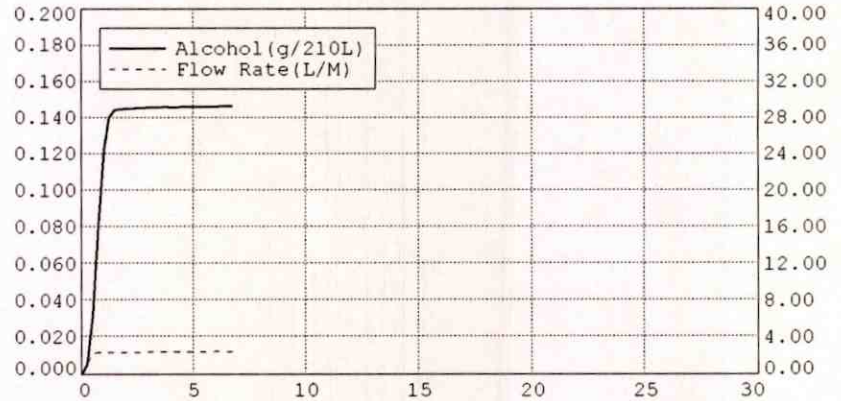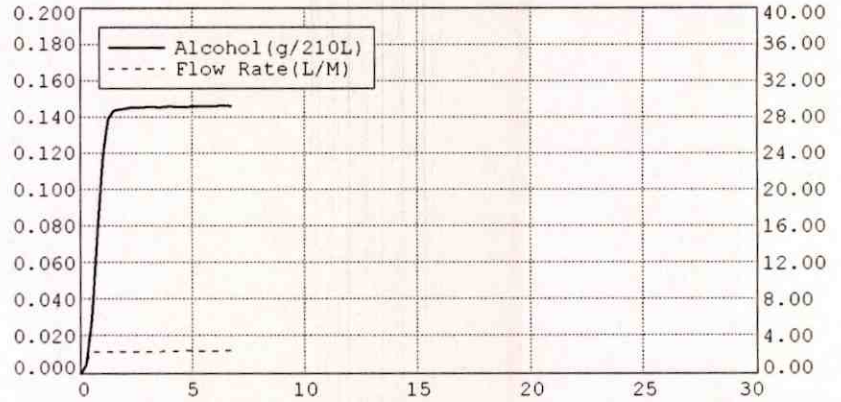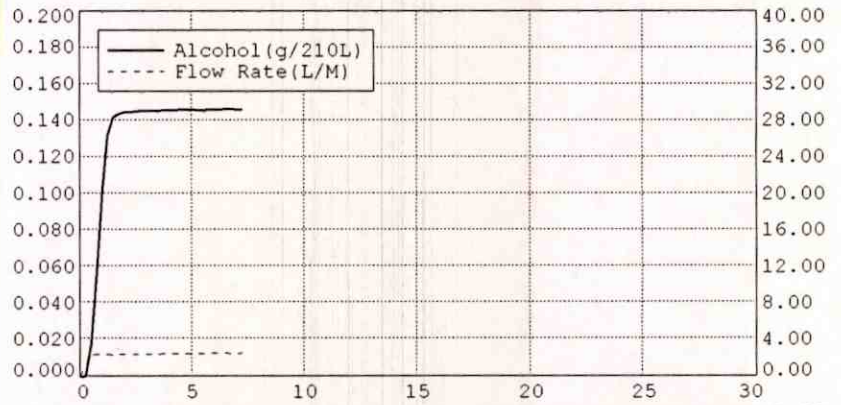

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100387






Date: 11/30/2023
 Time: 15:07:31


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 28.86: 0.289
 LOT #: AG217903
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 130 psi

BLANK TEST	0.000	15:08
INTERNAL STANDARD	VERIFIED	15:09
EXTERNAL STANDARD	0.294	15:09
BLANK TEST	0.000	15:10
EXTERNAL STANDARD	0.294	15:10
BLANK TEST	0.000	15:11
EXTERNAL STANDARD	0.295	15:11
BLANK TEST	0.000	15:12
EXTERNAL STANDARD	0.295	15:12
BLANK TEST	0.000	15:13
EXTERNAL STANDARD	0.295	15:13
BLANK TEST	0.000	15:14

Average = 0.2946
 Std Dev = 0.0005

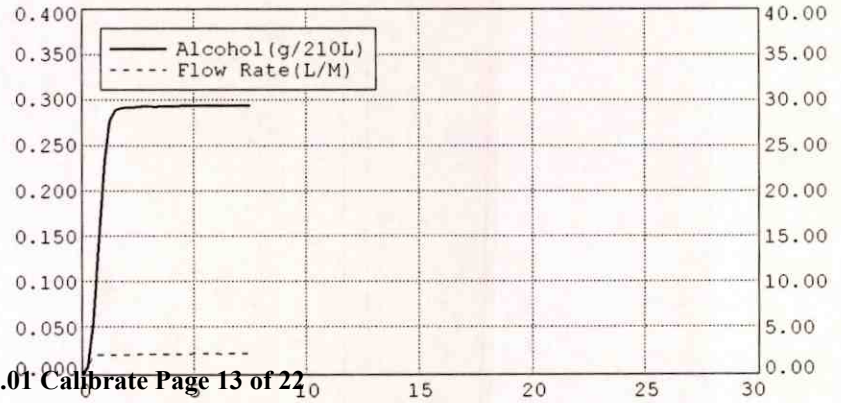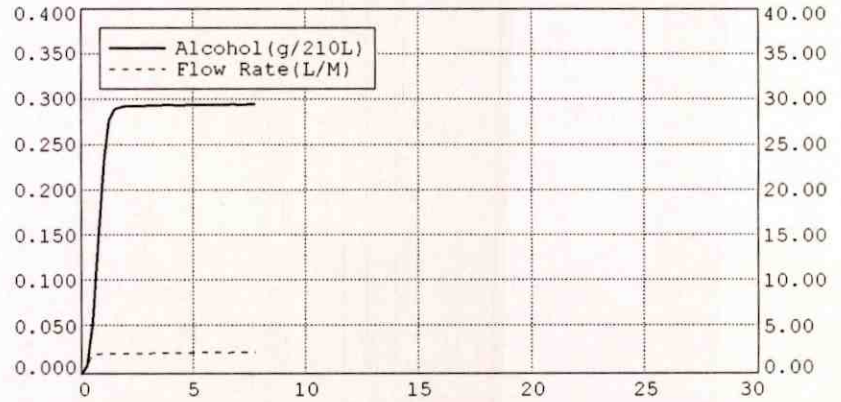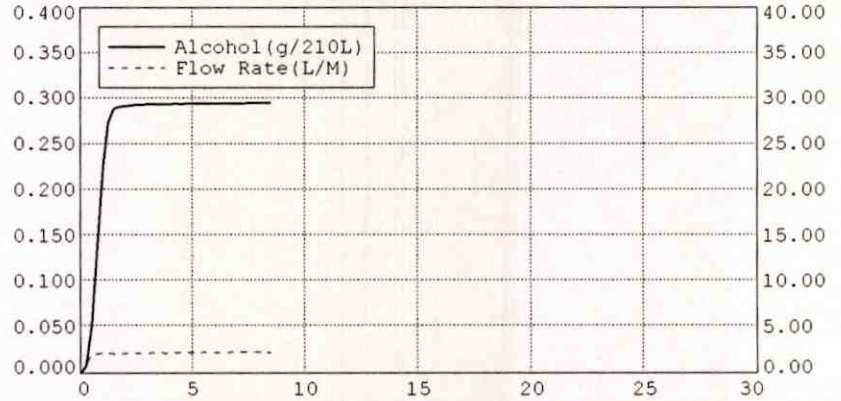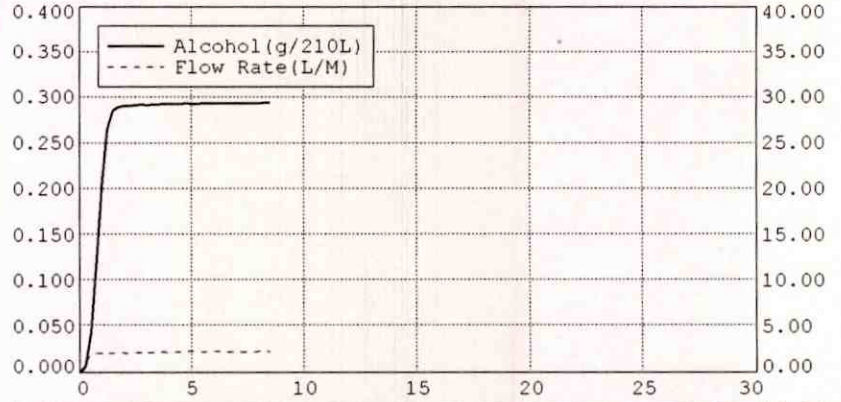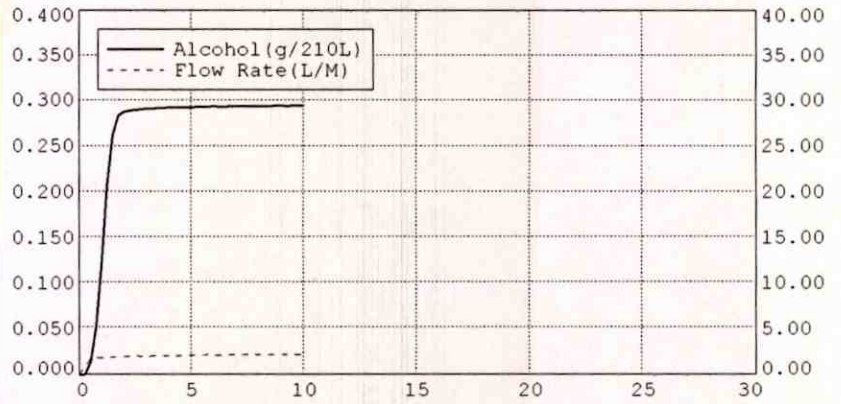

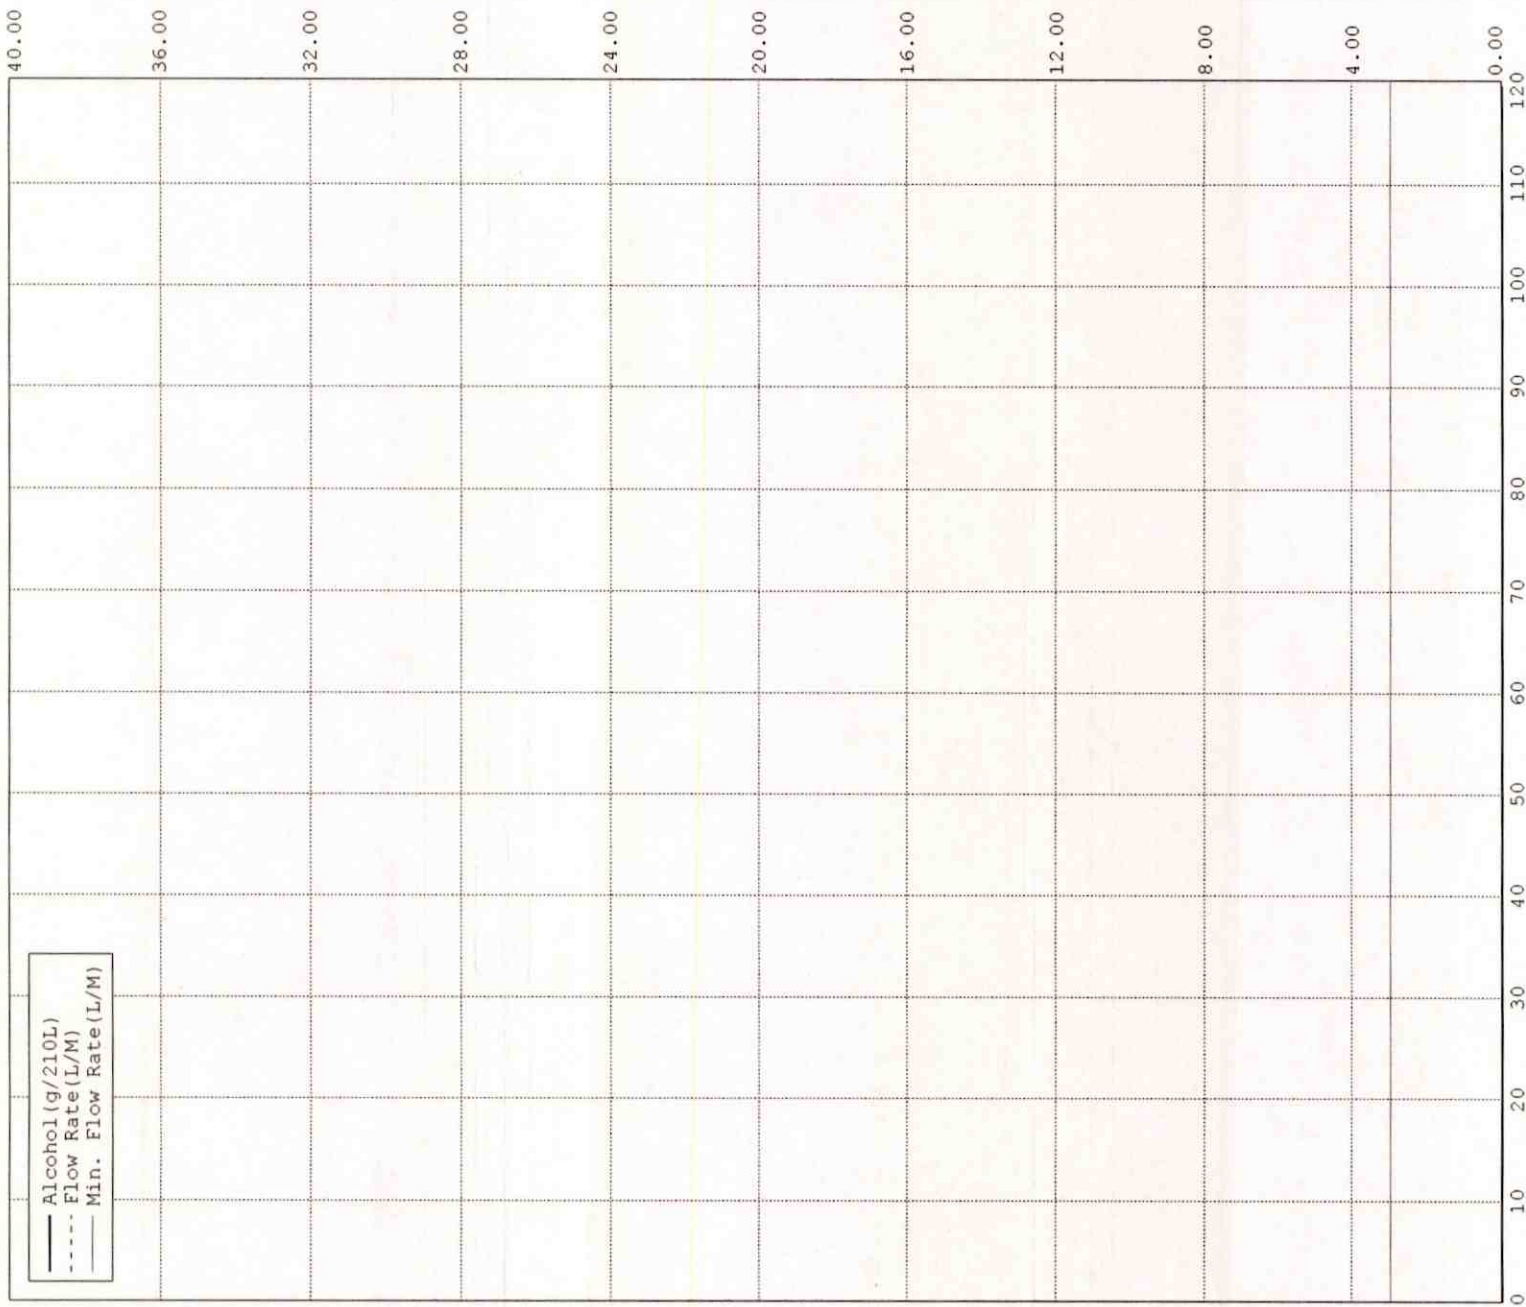

SUBJECT TEST

 Alaska Department of Public Safety
 DATAMASTER dmt: 100387

 Date: 11/30/2023
 Time: 15:24:59

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX

OPERATOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

DEPT/AGENCY:
 INCOMPLETE
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 28.87: 0.077
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK
 BLANK TEST PASSED 15:27
 0.000 15:27
 INTERNAL STANDARD VERIFIED 15:27
 0.079 15:27
 EXTERNAL STANDARD 0.000 15:28
 BLANK TEST INCOMPLETE 15:30
 SUBJECT SAMPLE

OKG

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100387

Date: 12/01/2023
Time: 08:57:40

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.96: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 08:58
BLANK TEST 0.000 08:58
INTERNAL STANDARD VERIFIED 08:59
EXTERNAL STANDARD 0.078 08:59
BLANK TEST 0.000 09:00
SUBJECT SAMPLE XXX 09:00

Maximum Attempts Exceeded

OKG

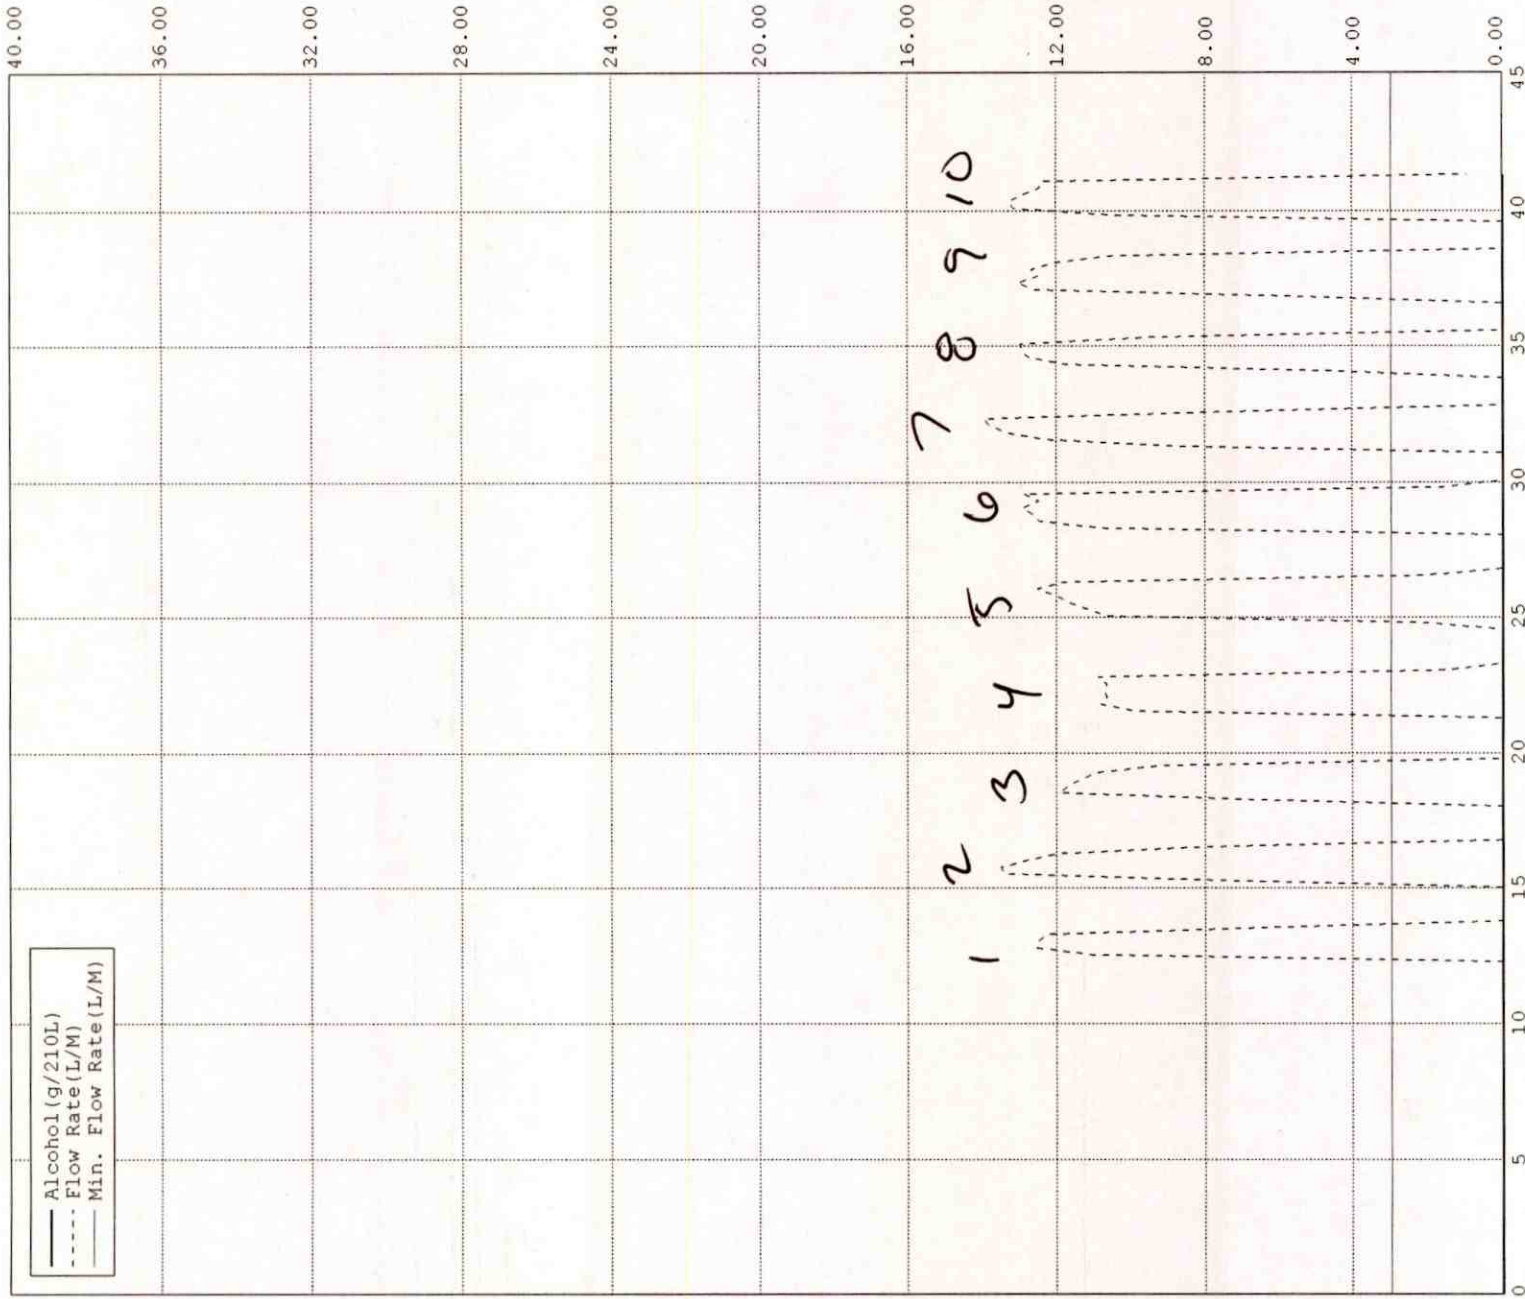

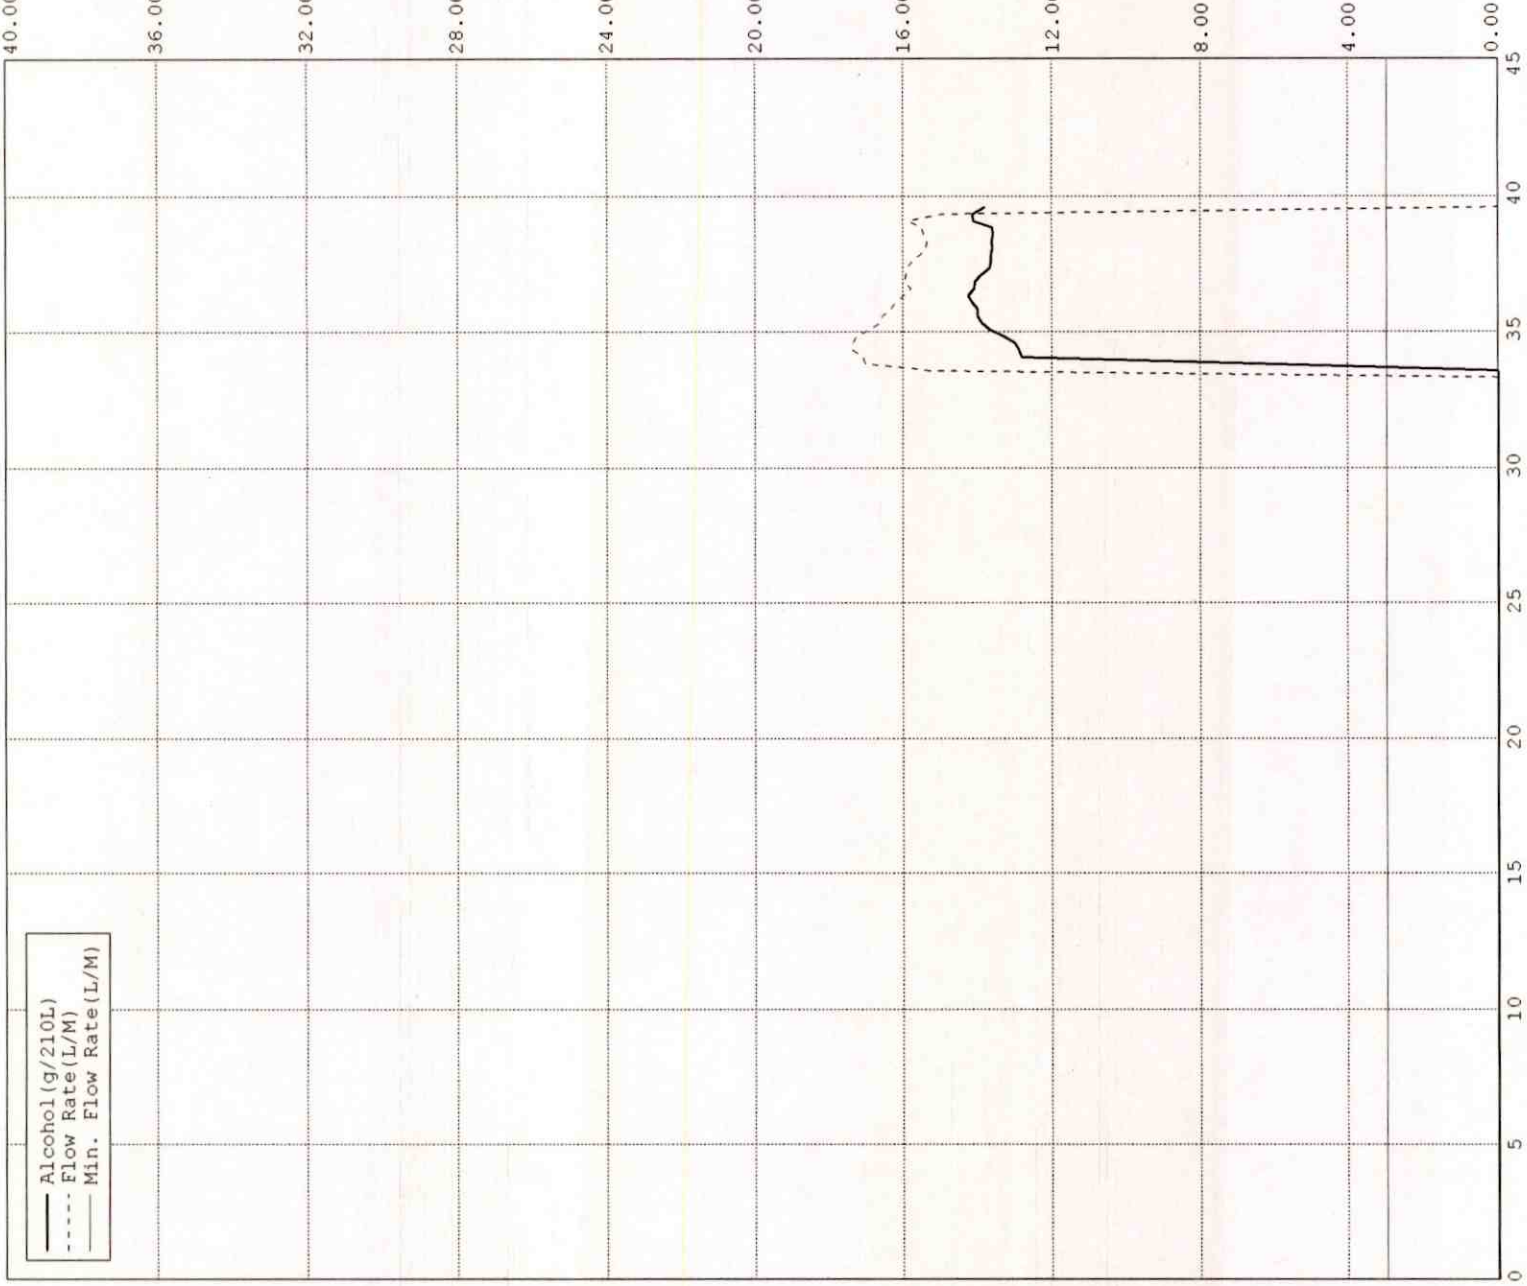

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100387

Date: 12/01/2023
 Time: 09:10:15

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX

OPERATOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

DEPT/AGENCY:
 INVALID

CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 28.96: 0.077
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	09:15
BLANK TEST	0.000	09:15
INTERNAL STANDARD	VERIFIED	09:15
EXTERNAL STANDARD	0.079	09:15
BLANK TEST	0.000	09:16
SUBJECT SAMPLE (Vol=1.62L)	0.069	09:17
BLANK TEST	0.000	09:18
EXTERNAL STANDARD	0.078	09:18
BLANK TEST	0.000	09:19

1st Invalid attempt
 accepted. I had switched
 w/ water after much
 wash & did not blow
 long enough. CMB 12/1/23

CMB

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100387

Date: 12/01/2023
Time: 09:21:36

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CHARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INVALID
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.96: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 09:23
BLANK TEST 0.000 09:23
INTERNAL STANDARD VERIFIED 09:23
EXTERNAL STANDARD 0.079 09:23
BLANK TEST 0.000 09:24
SUBJECT SAMPLE INVALID 09:24

CMG

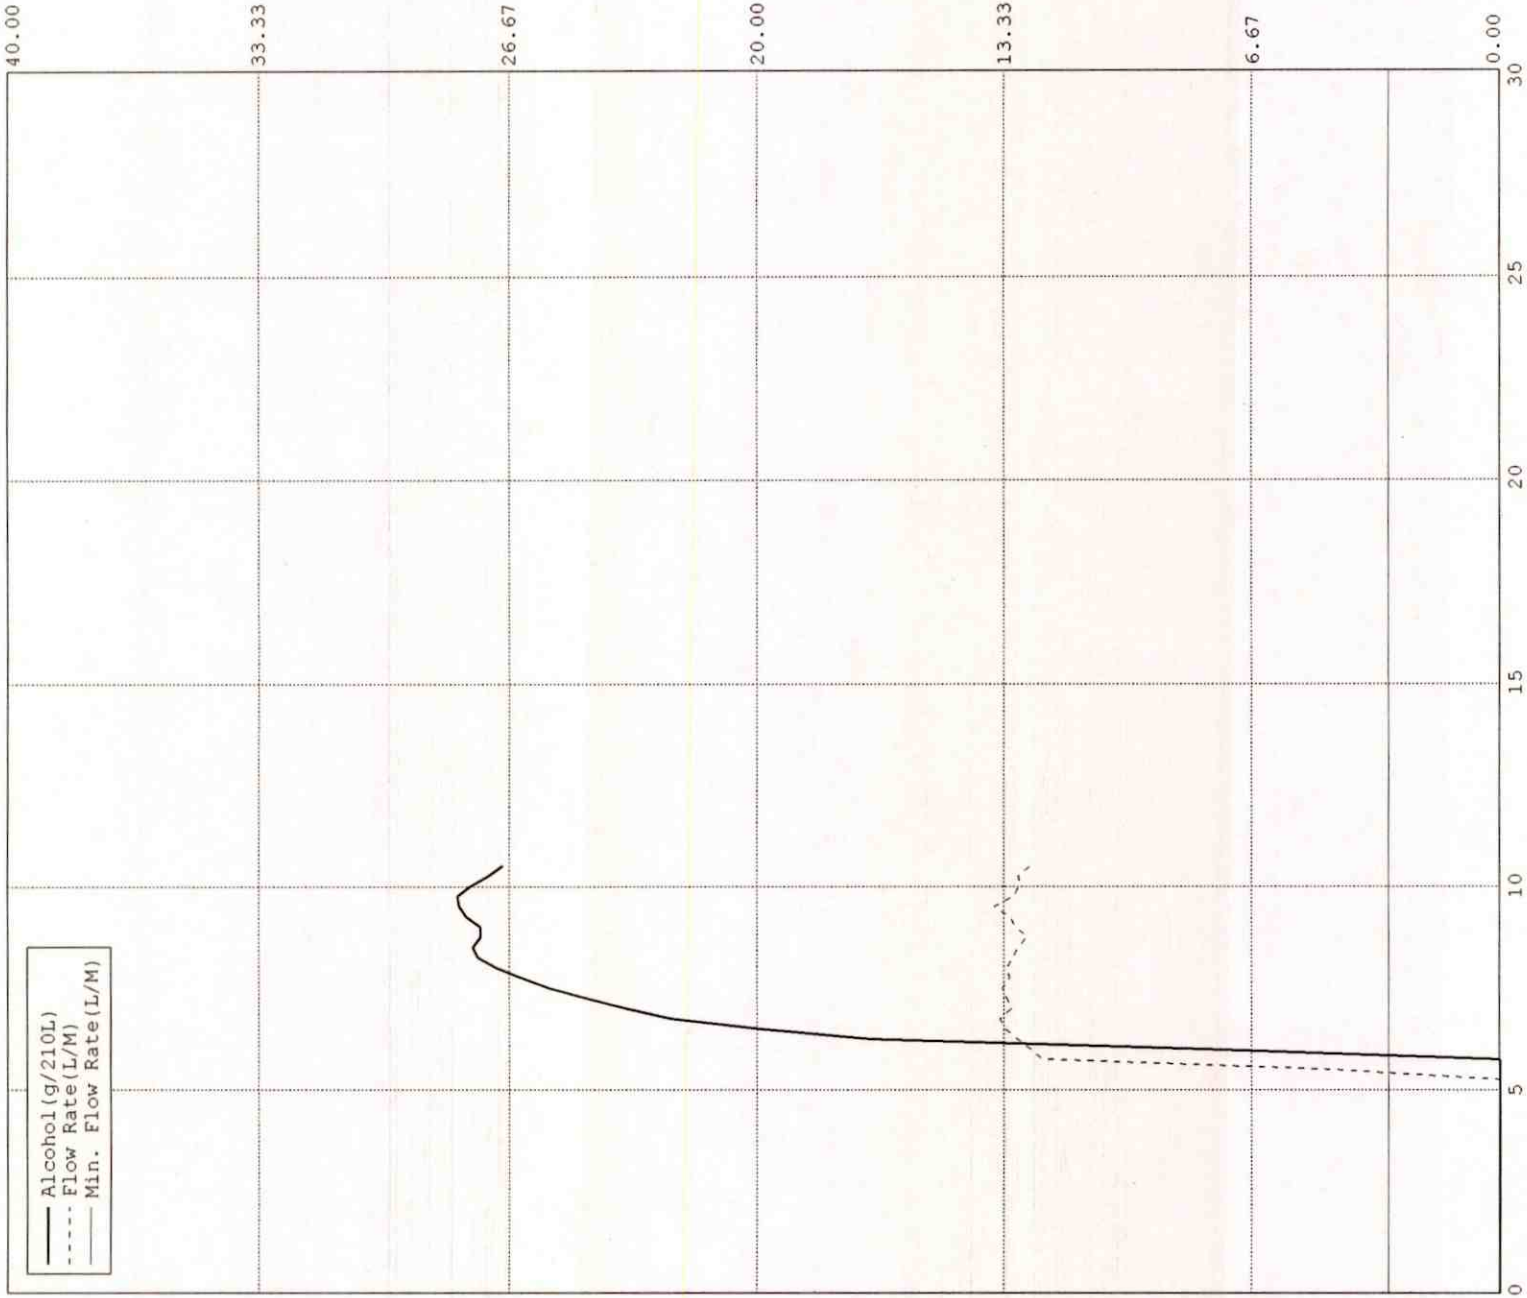

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100387

Date: 12/01/2023
Time: 09:27:33

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
RFI
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 28.96: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 09:29
BLANK TEST 0.000 09:29
INTERNAL STANDARD VERIFIED 09:29
EXTERNAL STANDARD 0.079 09:29
BLANK TEST 0.000 09:30

RFI DETECTED

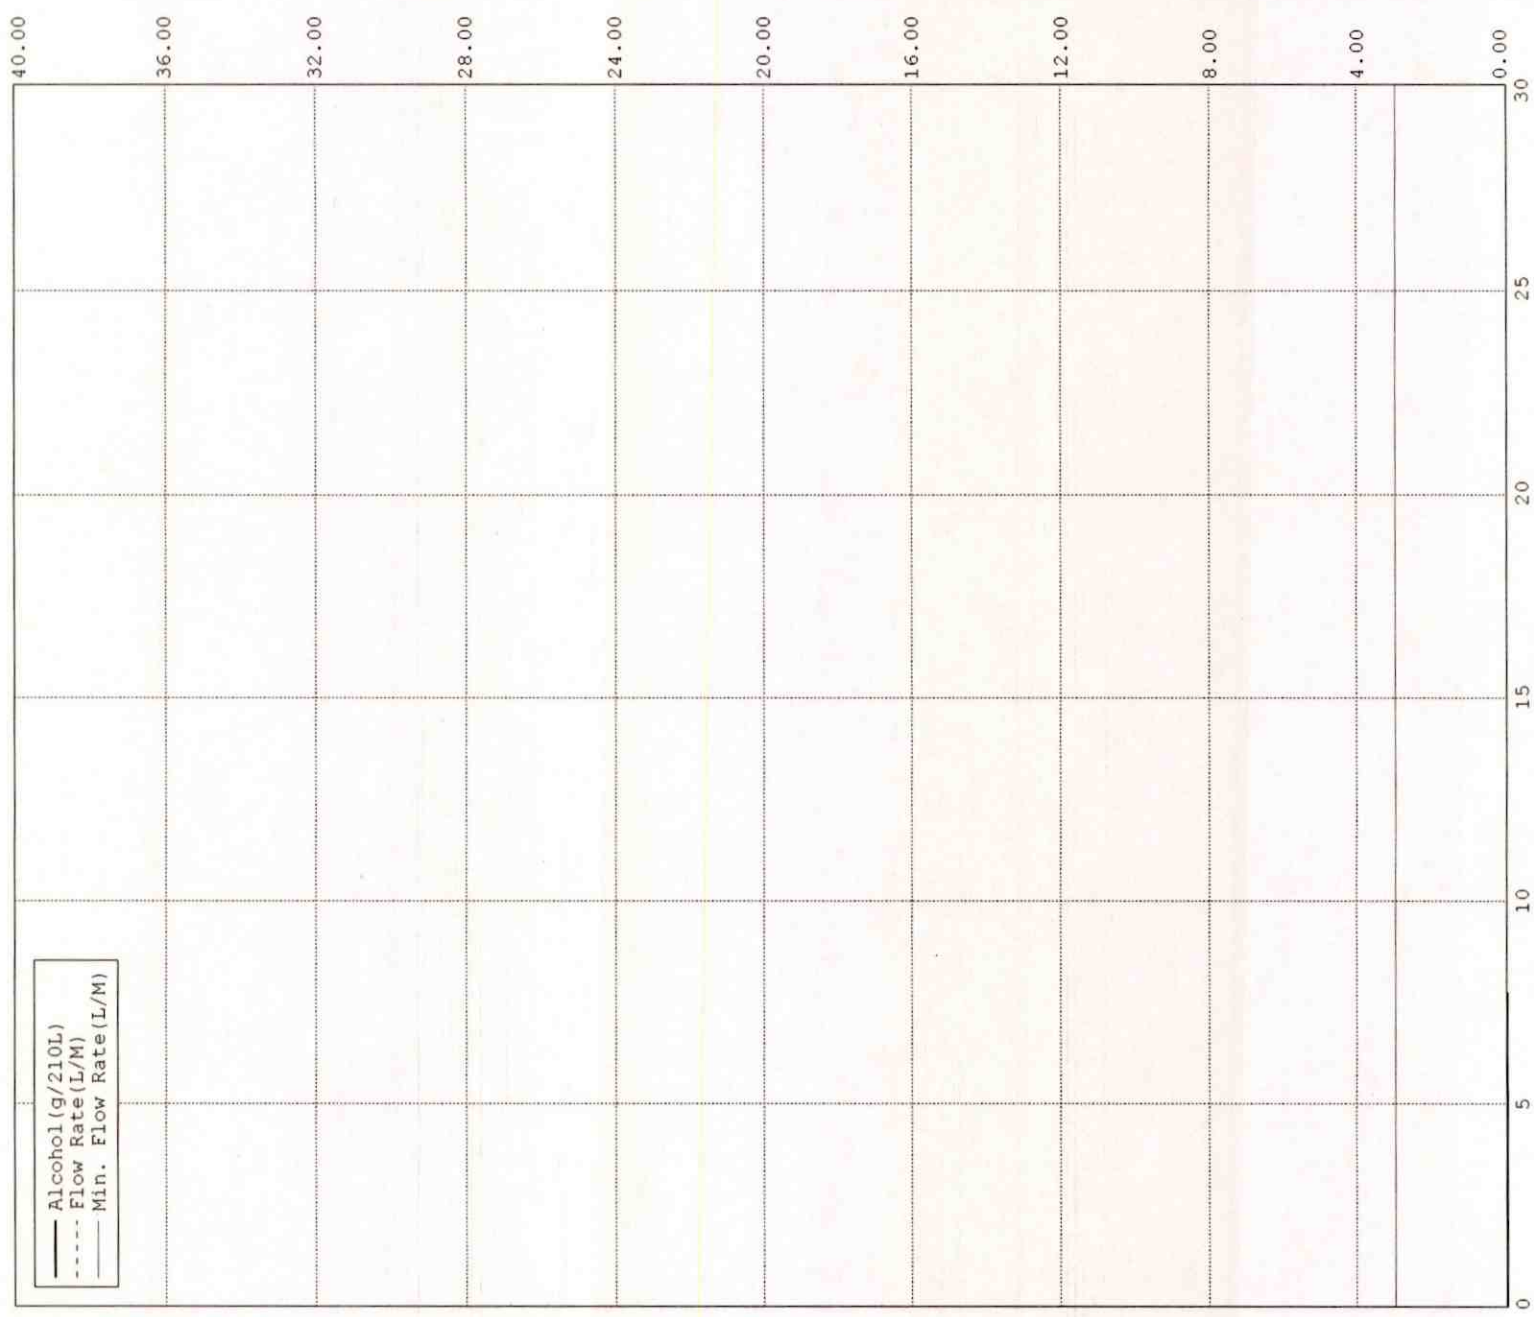

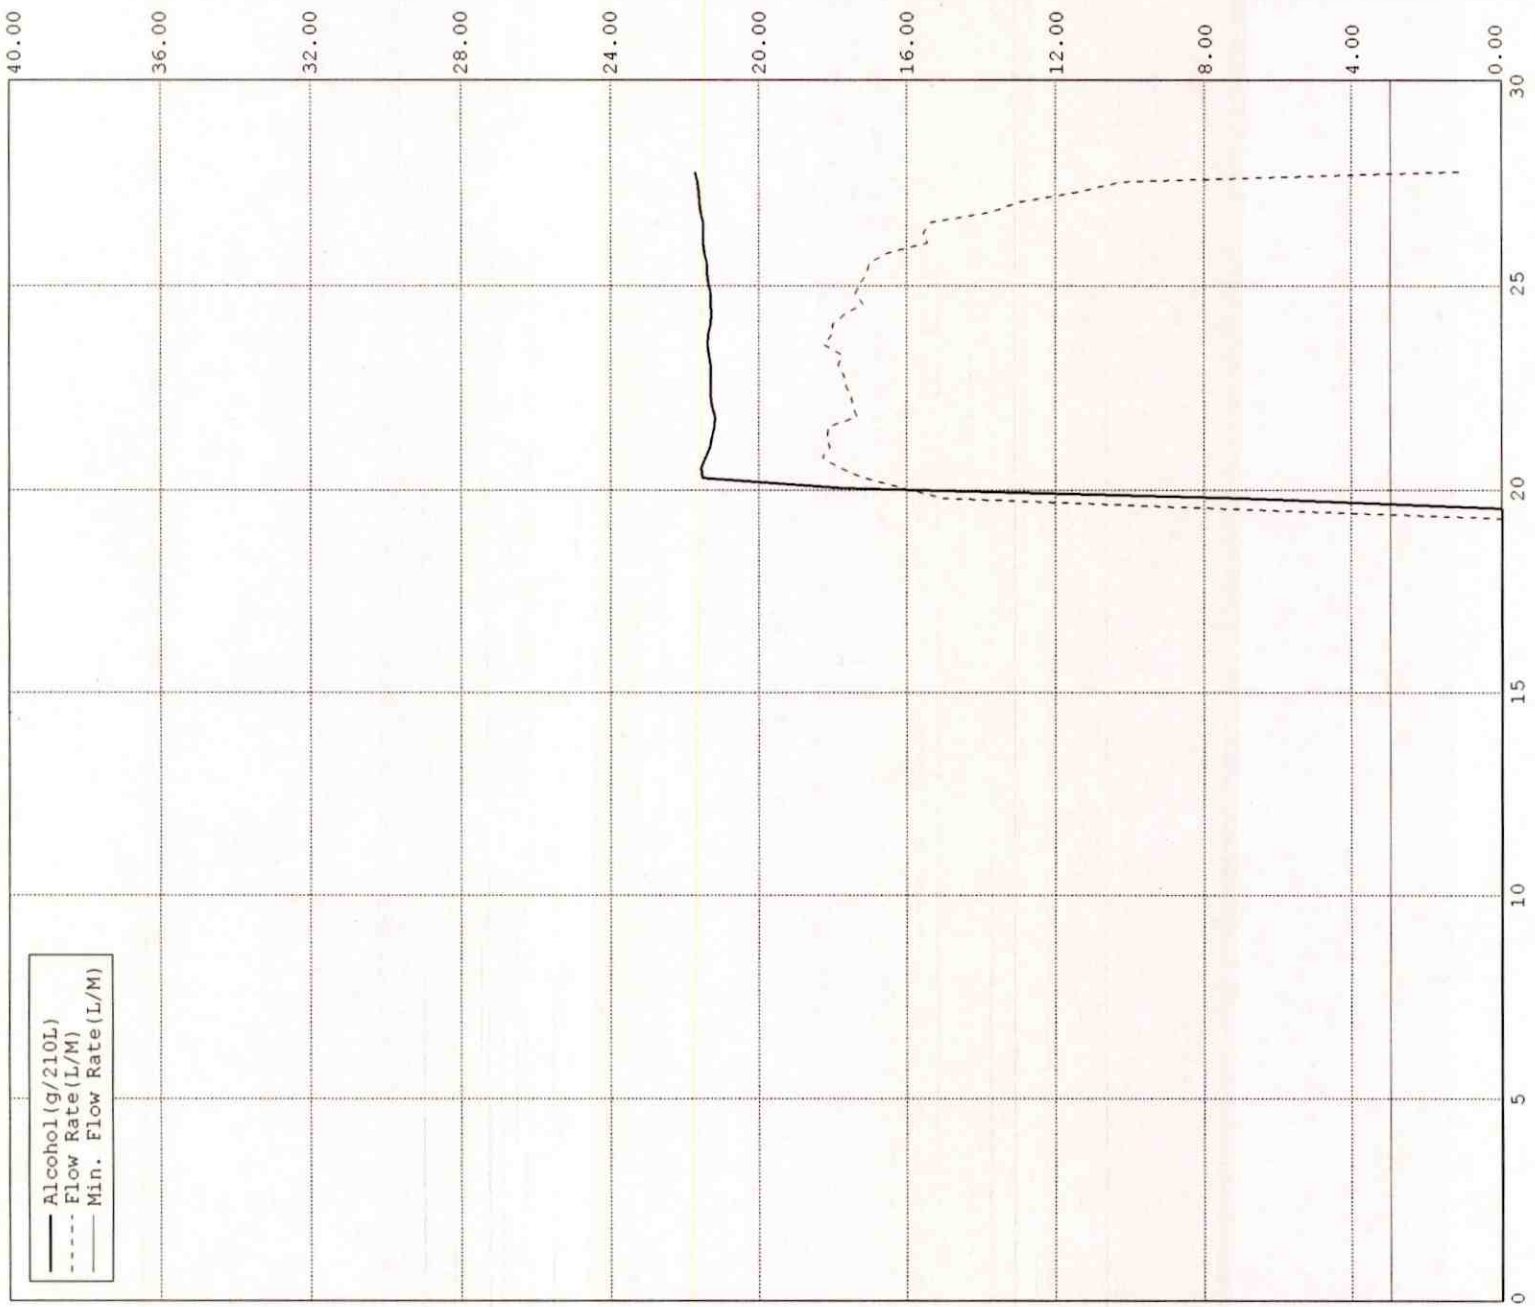

SUBJECT TEST

 Alaska Department of Public Safety
 DATAMASTER dmt: 100387

 Date: 12/01/2023
 Time: 10:41:59

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX

OPERATOR NAME:
 CHARLIE GLAISTER
 OPERATOR'S #: 10436

DEPT/AGENCY:
 INTERFERENCE ACETONE
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 28.97: 0.077
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 10:43
 BLANK TEST 0.000 10:43
 INTERNAL STANDARD VERIFIED 10:43
 Xq = 0.092 (1.22%)
 EXTERNAL STANDARD 0.079 10:43
 X[1] = 0.0786 (-0.0002) (0.0023)
 BLANK TEST 0.000 10:44
 SUBJECT SAMPLE XXX 10:45
 X[1] = 0.1101 (-0.0176) (0.0022)

Interference Detected

Filter 2 Average: -0.0000
 Filter 3 Average: 0.0010
 OW- 12/1/23
 CLK

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100387

Date: 12/01/2023
Time: 10:32:56

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE IPA
CASE/REPORT: XXXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.97: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	10:35
BLANK TEST	0.000	10:35
INTERNAL STANDARD	VERIFIED	10:35
Xq = 0.093 (0.75%)		
EXTERNAL STANDARD	0.079	10:35
X[1] = 0.0786 (-0.0007) (0.0015)		
BLANK TEST	0.000	10:36
SUBJECT SAMPLE	XXX	10:36
X[1] = 0.1164 (-0.0326) (0.0016)		

Interference Detected

CVW

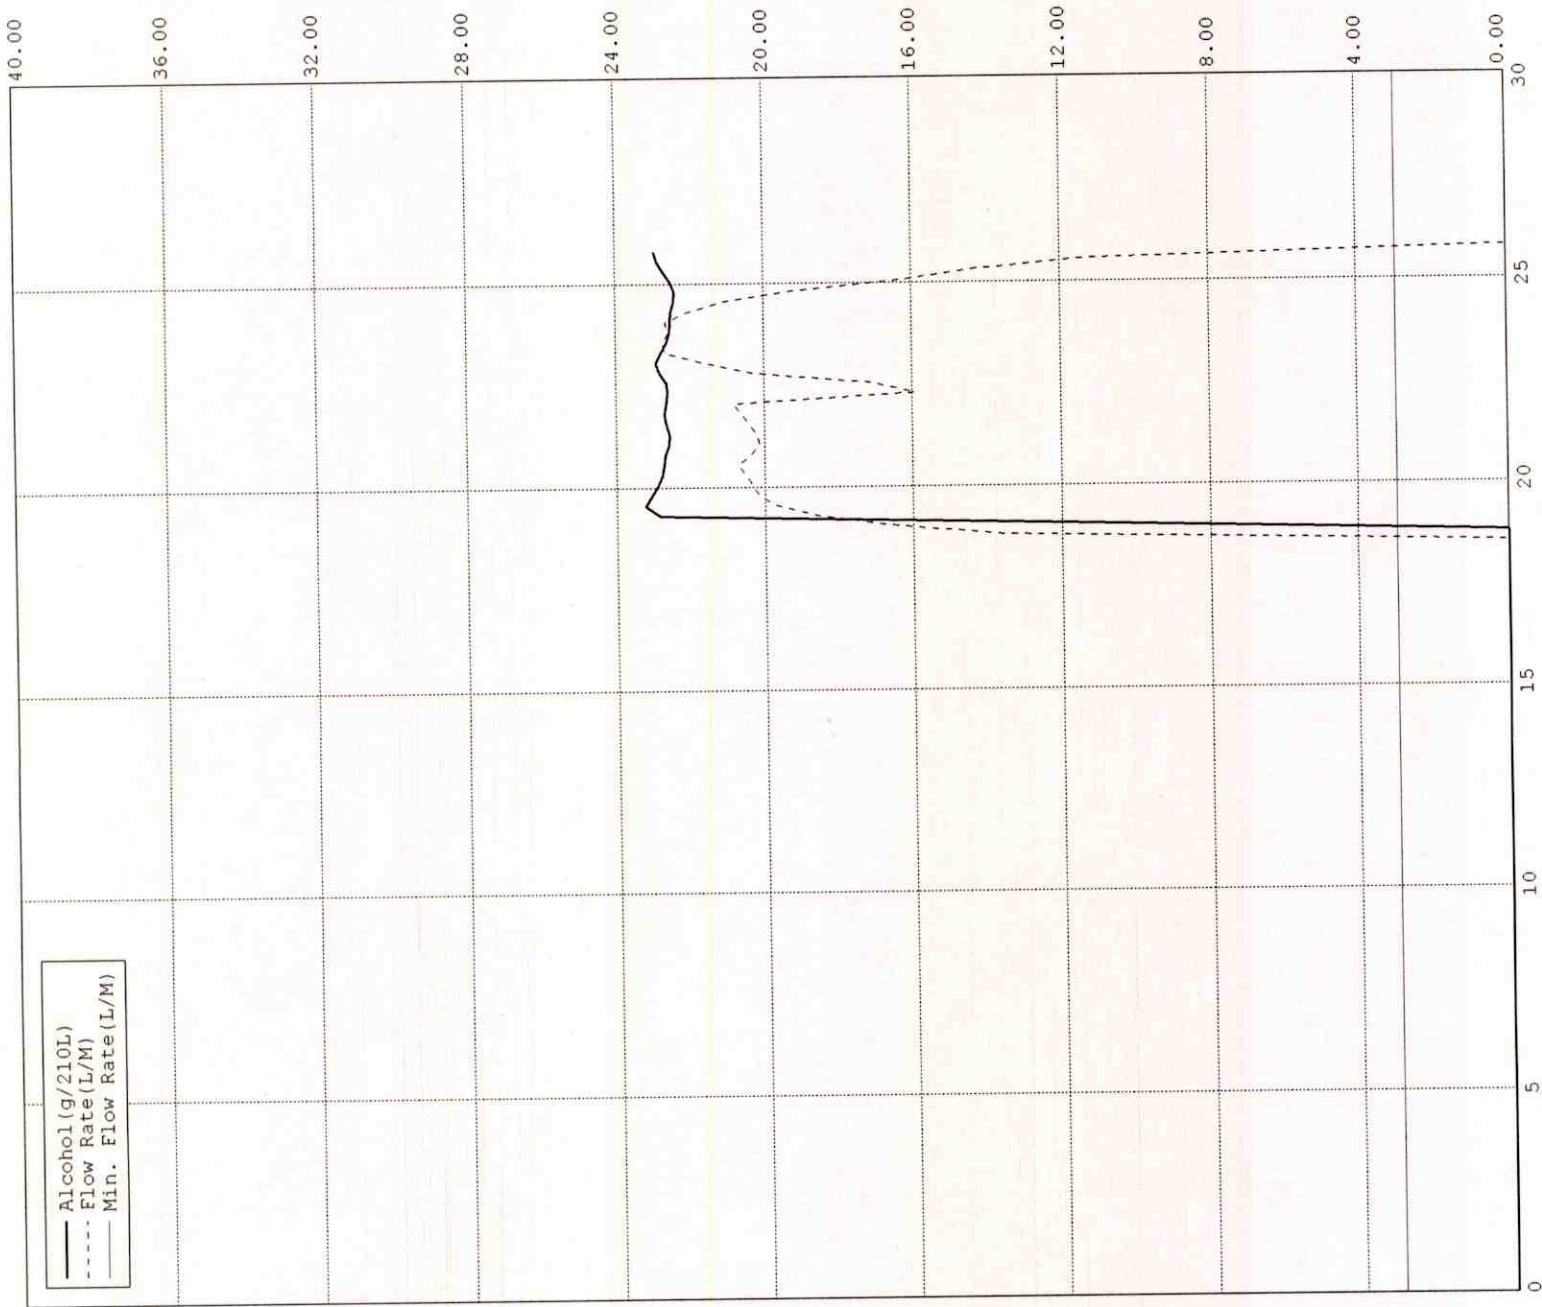

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100387

Date: 12/01/2023
 Time: 10:21:01

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX

OPERATOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436


DEPT/AGENCY:
 INTERFERENCE NEGATIVE
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 28.97: 0.077
 LOT #: AG310901
 EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	10:22
BLANK TEST	0.000	10:22
INTERNAL STANDARD	VERIFIED	10:22
Xq = 0.092 (0.84%)		
EXTERNAL STANDARD	0.079	10:22
X[1] = 0.0786 (-0.0010)	(0.0019)	
BLANK TEST	0.000	10:23
SUBJECT SAMPLE (Vol=2.12L)	0.090	10:24
X[1] = 0.0905 (-0.0014)	(0.0004)	
BLANK TEST	0.000	10:25
EXTERNAL STANDARD	0.078	10:25
X[1] = 0.0783 (-0.0006)	(0.0005)	
BLANK TEST	0.000	10:26

OKG

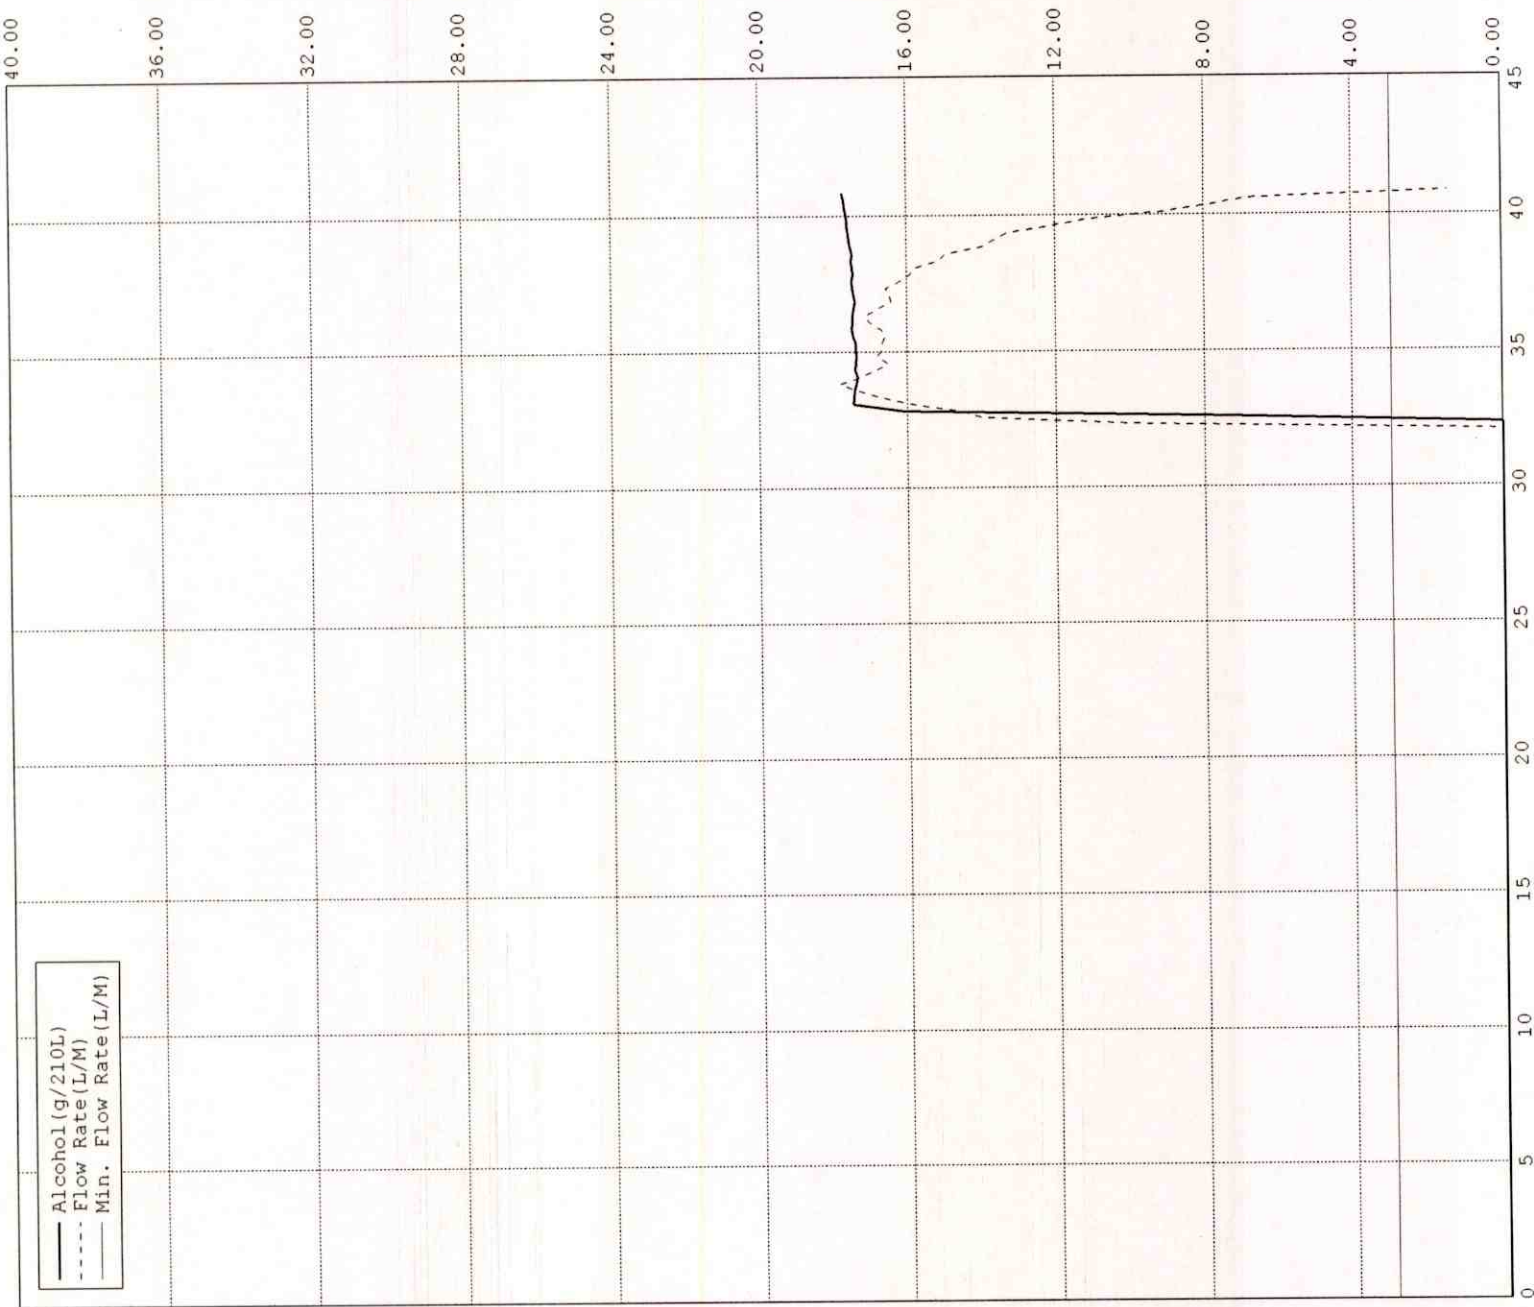

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100387

Date: 12/01/2023
Time: 11:05:31

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 28.97: 0.077
LOT #: AG310901
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	11:06
BLANK TEST	0.000	11:06
INTERNAL STANDARD	VERIFIED	11:06
EXTERNAL STANDARD	0.079	11:07
BLANK TEST	0.000	11:08
SUBJECT SAMPLE (Vol=1.81L)	0.000	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.079	11:09
BLANK TEST	0.000	11:10

OK

