

State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100357

**Report Issue Date:** 12/03/2024  
**Date Received:** 2024-08-01  
**Condition of Item:** No apparent damage

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.019	0.020	0.019	0.020
0.080	0.079	AG335202	0.079	0.078	0.078	0.078	0.078	0.078
0.300	0.295	AG427706	0.302	0.302	0.301	0.300	0.299	0.301

As Found - Evaluation Analyst: Megan Carlock  
 As Found Conditions - Barometric Pressure (inHg): 29.47 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.1 Relative Humidity (%): 17  
 As-Found Lab Activity Date Range: 10/28/2024 - 10/29/2024

O-ring changed. One tube was not securely attached, it was placed back onto the correct fitting.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG408002	0.019	0.020	0.019	0.019	0.019	0.019	+/- 0.002
0.040	0.039	AG407908	0.039	0.038	0.038	0.038	0.038	0.038	+/- 0.003
0.080	0.077	AG335202	0.077	0.076	0.076	0.077	0.076	0.076	+/- 0.004
0.100	0.096	AG333401	0.098	0.097	0.097	0.098	0.097	0.097	+/- 0.004
0.150	0.145	AG332004	0.145	0.144	0.145	0.143	0.143	0.144	+/- 0.006
0.300	0.289	AG427706	0.296	0.295	0.294	0.294	0.293	0.294	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 28.86 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.8 Relative Humidity (%): 19  
 As-Left Lab Activity Date Range: 11/07/2024 - 11/07/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Kaija Swisher on 12/03/2024

[kaija.swisher@alaska.gov](mailto:kaija.swisher@alaska.gov)

Technically and administratively reviewed by Colleen O'Bryant on 12/03/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100357 Analyst or Technician Name: Laya Swisher

DataMaster DMT Calibration Start Date: 11/7/24

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 236307229  
Calibration Due Date: 5/2/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 28.86 Temperature(C) 21.8 Relative Humidity(%) 19  
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20241107KS Expiration Date: 2/7/25  
Simulator S/N: DR4161 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20241107KS Expiration Date: 2/7/25  
Simulator S/N: DR5298 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 231P41233 Expiration Date: 2/7/25  
Simulator S/N: DR4163 Thermometer Verification Performed?

The second exp date is  
09/20/2025  
KS 12/2/24

Calibrated External Thermometer S/N: 236631106  
Calibration Due Date: 9/19/25

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 11/7/24  
Data Interpretation Date (Technician): NK (if applicable)  
Data Interpretation Date (Analyst): 11/7/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100357  
-----

Date: 11/07/2024  
Time: 09:22:05

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C            PASSED  
(44.0°C - 52.0°C)  
Breath Tube        = 47.1°C        PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage    = 1.81 V            PASSED  
(1.09 V - 2.53 V)  
Cooler Voltage = 1.94 V            PASSED  
(1.13 V - 2.65 V)  
Bias Voltage    = 80 V                PASSED  
(48 V - 112 V)  
Chopper Freq   = 526 Hz            PASSED  
(475 Hz - 575 Hz)  
Barometer       = 28.9 in

PUMP INFO

Flow Rate = 4.601 L/M            PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON                            PASSED  
(0.001 V <= 0.010 V)  
PUMP OFF                           PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1                            PASSED  
Filter 2                            PASSED  
Filter 3                            PASSED

INTERNAL STANDARD

Xq = 0.086 0.40% (0.00% - 4.00%)            PASSED

Technician Screen

-----  
DATAMASTER dmt: 100357  
-----

Date: 11/07/2024  
Time: 9:43 AM

Temperatures (°C)

Sample Cell: 48.7°C  
Breath Tube: 46.8°C

Current Barometer 28.9 in  
Volume (Ltr) 1.49

Settings

Lamp: 1.81 V  
Bias: 80 V  
Cooler: 1.94 V  
Chopper: 524 Hz

Voltages (V)

Flow: 1.05 V  
Detector: -0.030 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100357  
-----

Date: 07/26/2021  
Time: 14:51:58

OPERATOR NAME:  
BRANDI BARNETT  
CERTIFICATE #: 7038

Ca = 0.1000  
CAL = 0.972666    0.800 <= CAL < 1.200  
b1 = 0.0000    0.0000 <= b1 < 0.0040  
b2 = 0.0042    0.0010 <= b2 < 0.0100  
b3 = 0.0003    0.0000 <= b3 < 0.0040  
Xq = 0.0861    0.0500 <= Xq < 0.2000  
a21 = 1.170709    1.050 <= a21 < 1.300  
a31 = 0.526742    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100357

Date: 11/07/2024  
Time: 09:58:09

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
MINIMUM VOLUME TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.85: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

TEST TYPE	RESULT	TIME
DIAGNOSTIC CHECK	PASSED	09:59
BLANK TEST	0.000	09:59
INTERNAL STANDARD	VERIFIED	09:59
EXTERNAL STANDARD	0.076	09:59
BLANK TEST	0.000	10:00
SUBJECT SAMPLE (Vol=1.53L)	0.000	10:01
BLANK TEST	0.000	10:02
EXTERNAL STANDARD	0.077	10:02
BLANK TEST	0.000	10:03

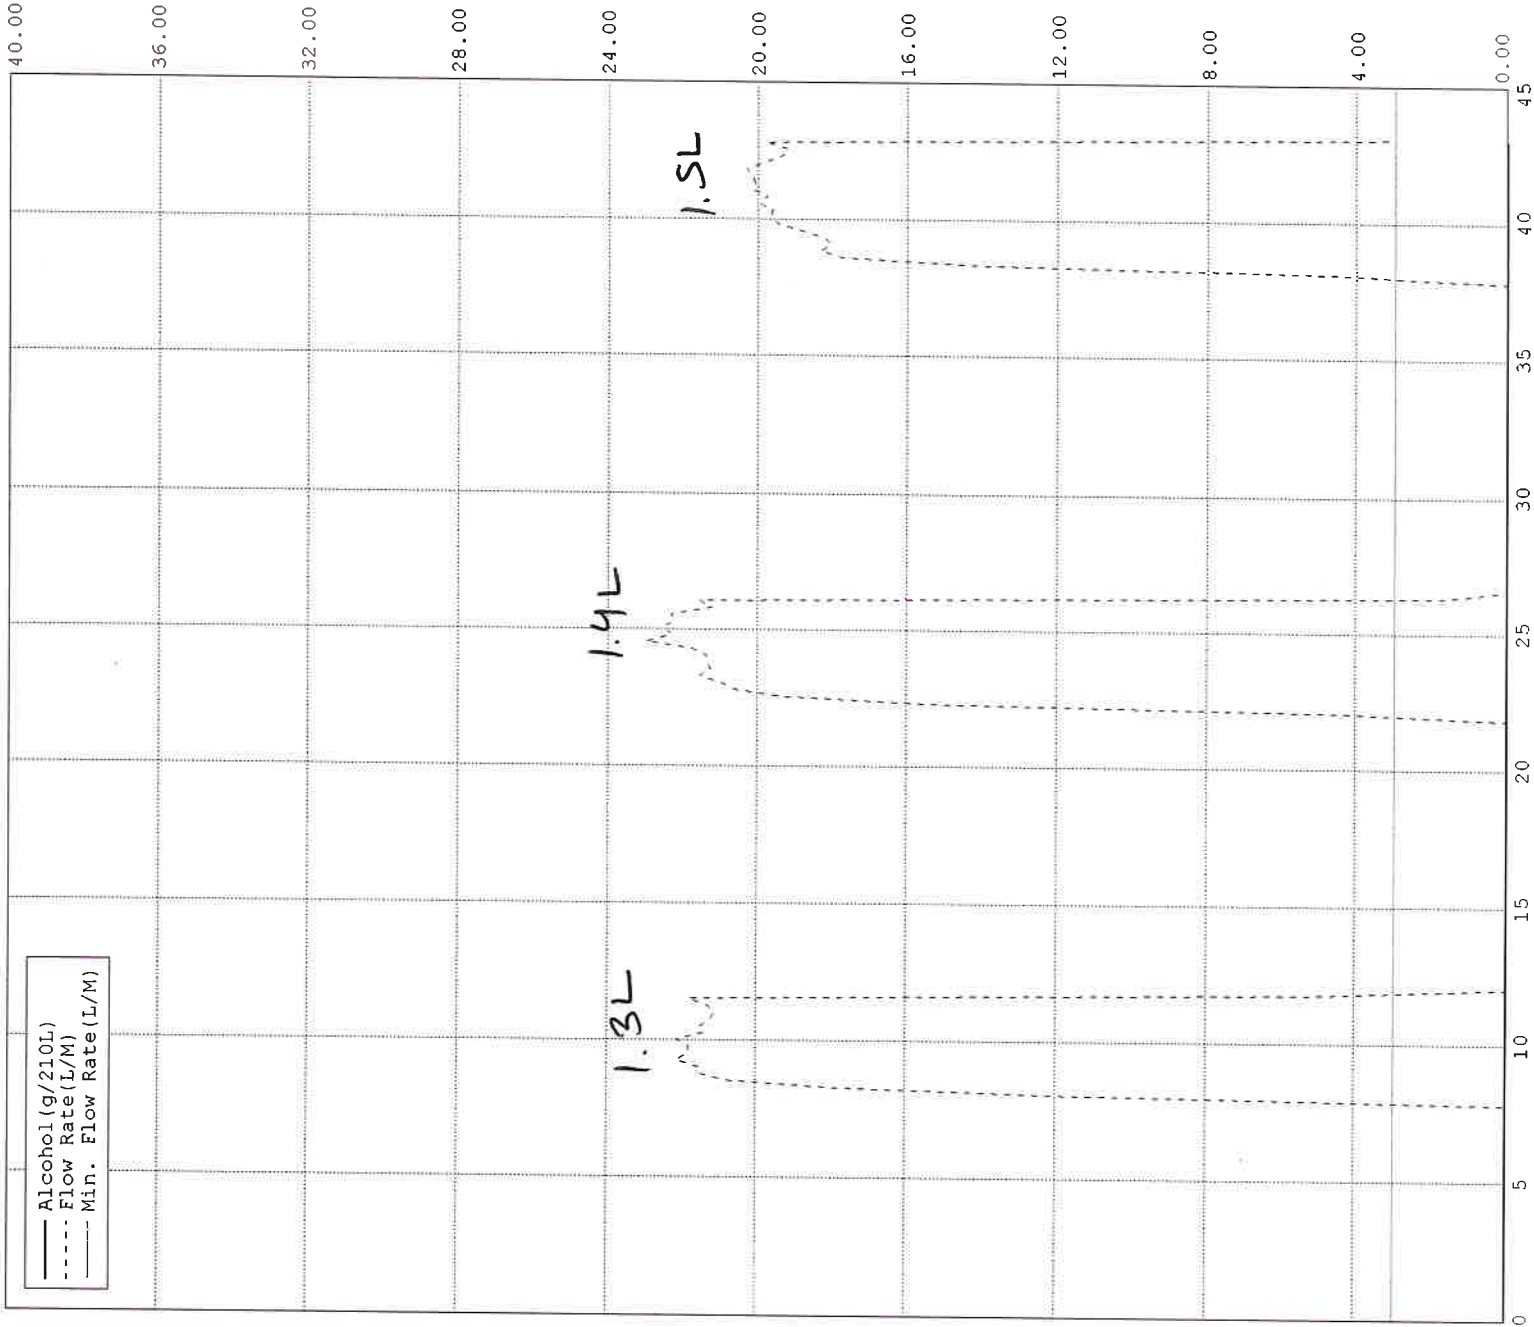

KS

LINEARITY CHECK


Alaska Department of Public Safety  
 DATAMASTER dmt: 100357

Date: 11/07/2024  
 Time: 10:16:29

SUPERVISOR NAME:  
 KAIJA SWISHER  
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.019	0.0192	0.0004
0.039	0.0382	0.0004
0.077	0.0764	0.0005
0.096	0.0974	0.0005
0.145	0.1440	0.0010
0.289	0.2944	0.0011

SLOPE = 1.020192  
 R<sup>2</sup> = 0.999797

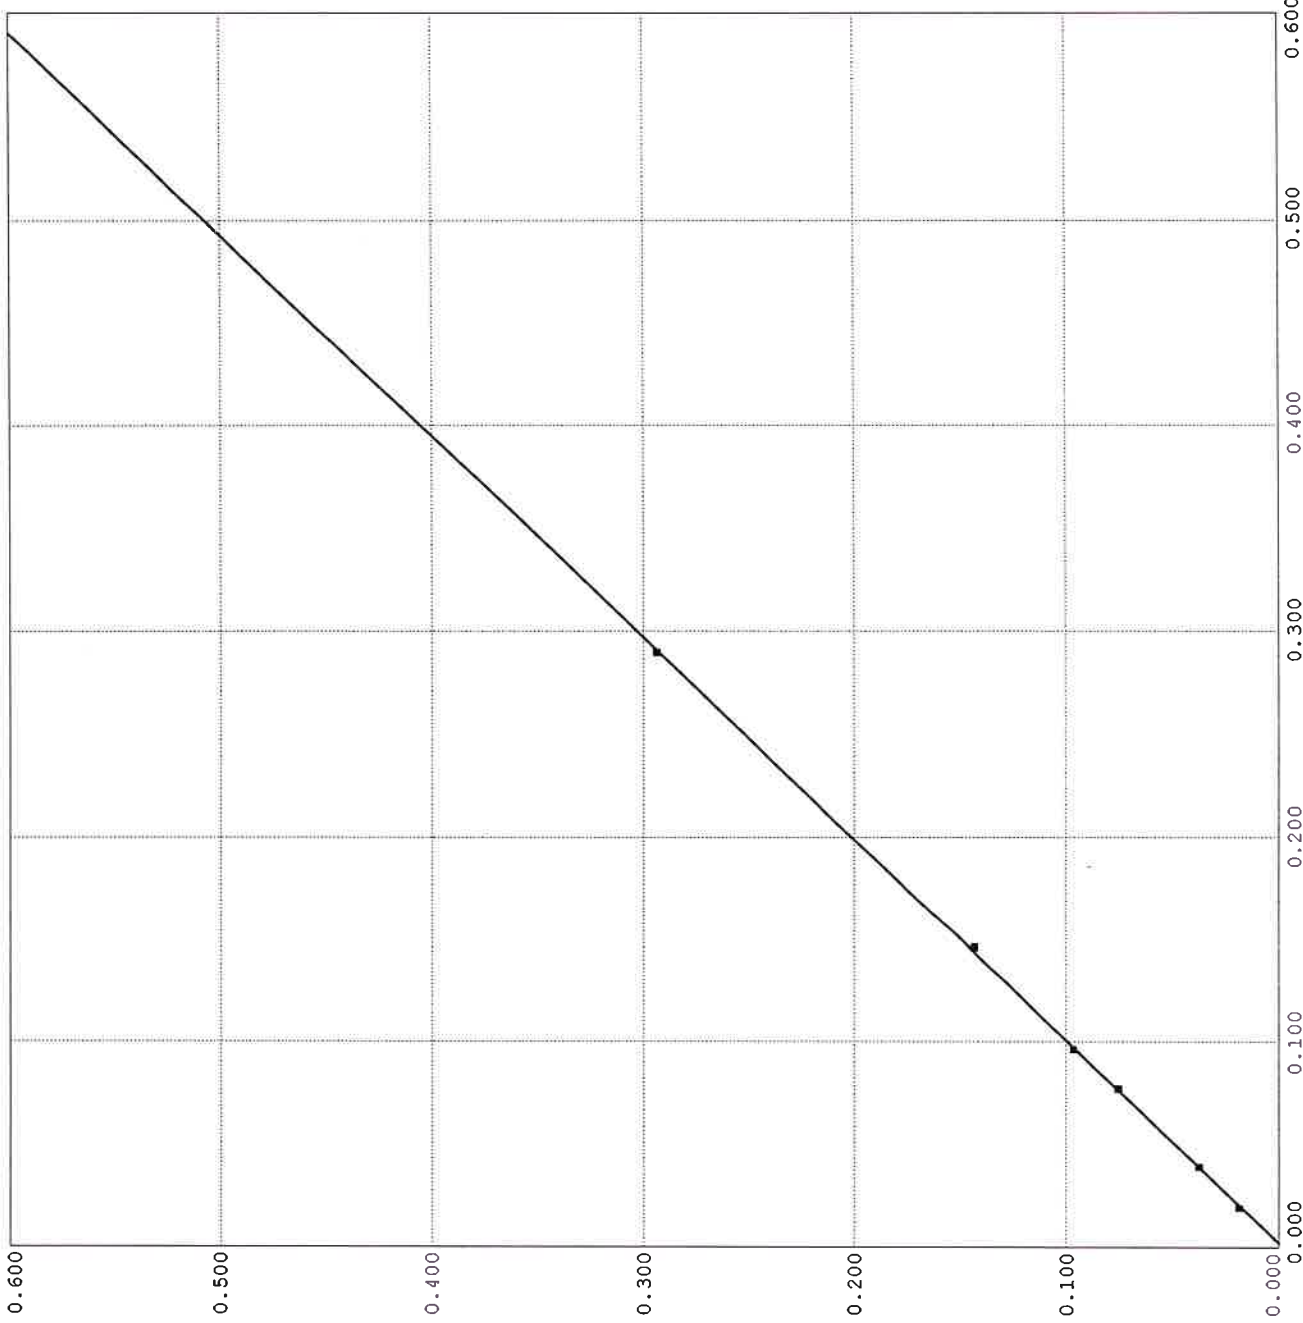

KS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100357






Date: 11/07/2024  
Time: 10:17:42

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 28.85: 0.019  
LOT #: AG408002  
EXPIRATION: 03/20/2026  
TANK PRESSURE: 756 psi

BLANK TEST	0.000	10:18
INTERNAL STANDARD	VERIFIED	10:19
EXTERNAL STANDARD	0.019	10:19
BLANK TEST	0.000	10:20
EXTERNAL STANDARD	0.020	10:20
BLANK TEST	0.000	10:21
EXTERNAL STANDARD	0.019	10:21
BLANK TEST	0.000	10:22
EXTERNAL STANDARD	0.019	10:22
BLANK TEST	0.000	10:23
EXTERNAL STANDARD	0.019	10:23
BLANK TEST	0.000	10:24

Average = 0.0192  
Std Dev = 0.0004

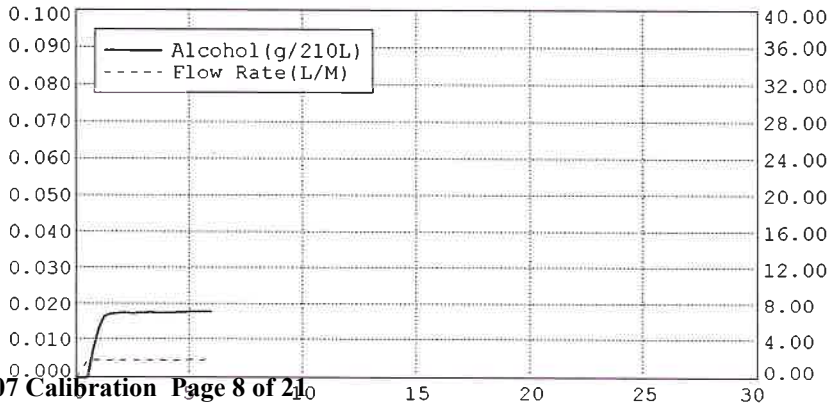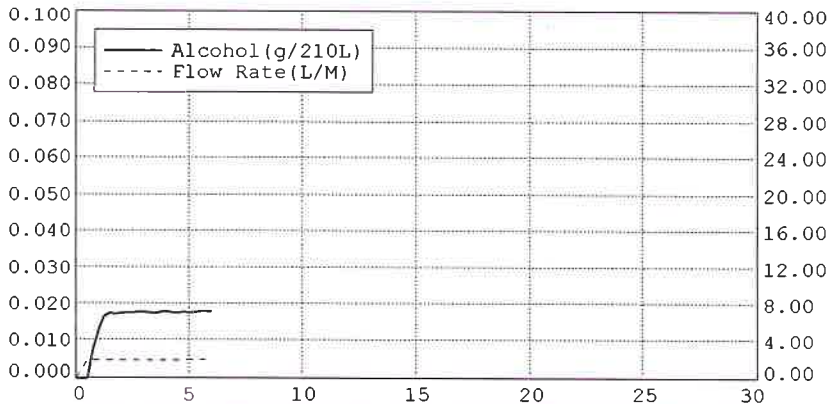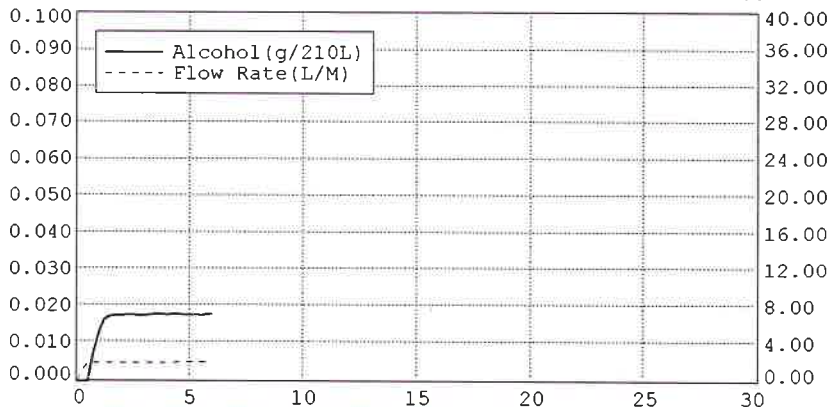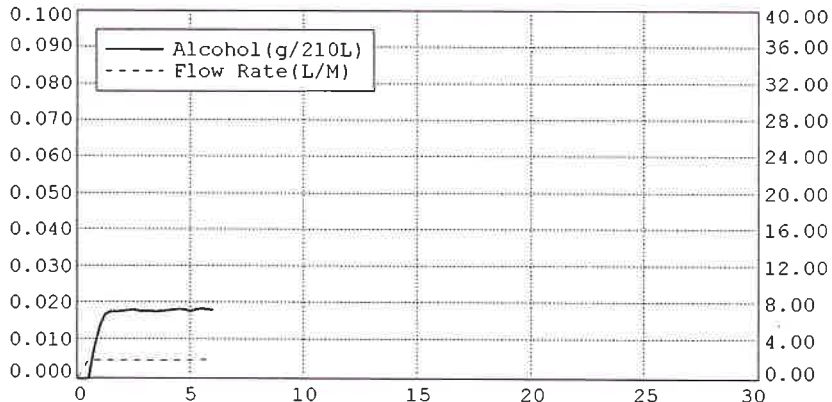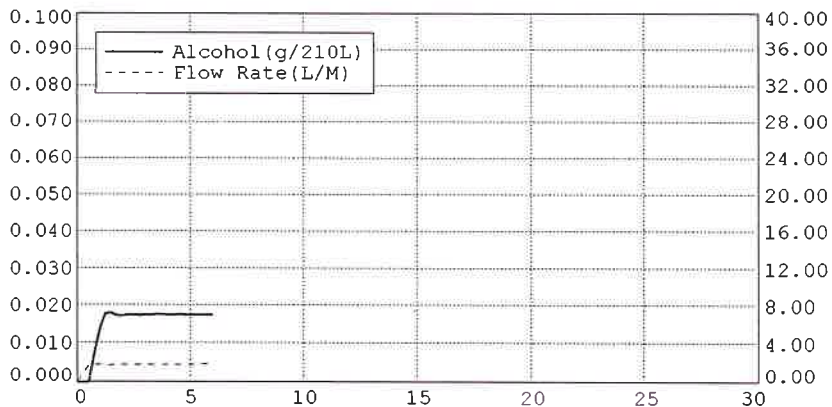



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
DATAMASTER dmt: 100357






Date: 11/07/2024  
Time: 10:25:15

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
TARGET AT 28.85: 0.039  
LOT #: AG407908  
EXPIRATION: 03/19/2026  
TANK PRESSURE: 1029 psi

BLANK TEST	0.000	10:26
INTERNAL STANDARD	VERIFIED	10:26
EXTERNAL STANDARD	0.039	10:26
BLANK TEST	0.000	10:27
EXTERNAL STANDARD	0.038	10:27
BLANK TEST	0.000	10:28
EXTERNAL STANDARD	0.038	10:29
BLANK TEST	0.000	10:30
EXTERNAL STANDARD	0.038	10:30
BLANK TEST	0.000	10:31
EXTERNAL STANDARD	0.038	10:31
BLANK TEST	0.000	10:32

Average = 0.0382  
Std Dev = 0.0004

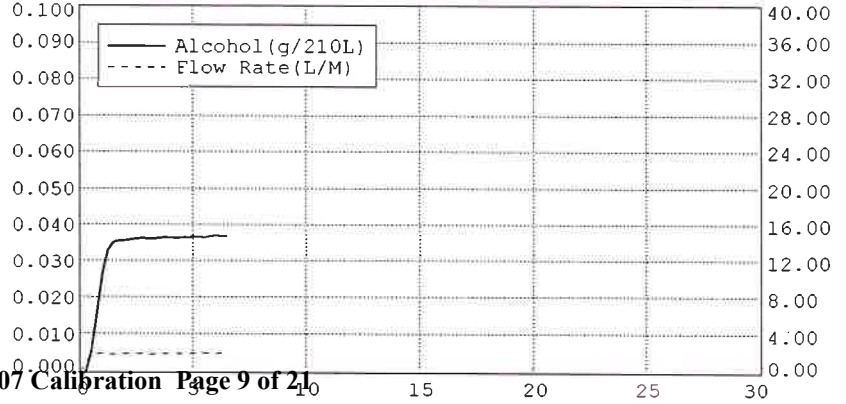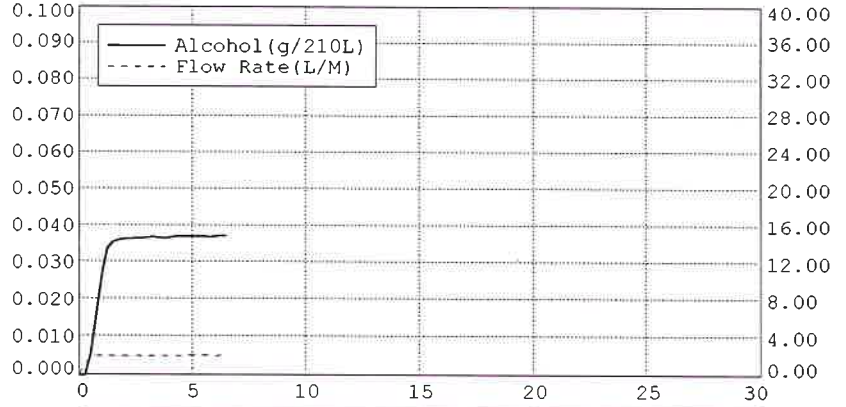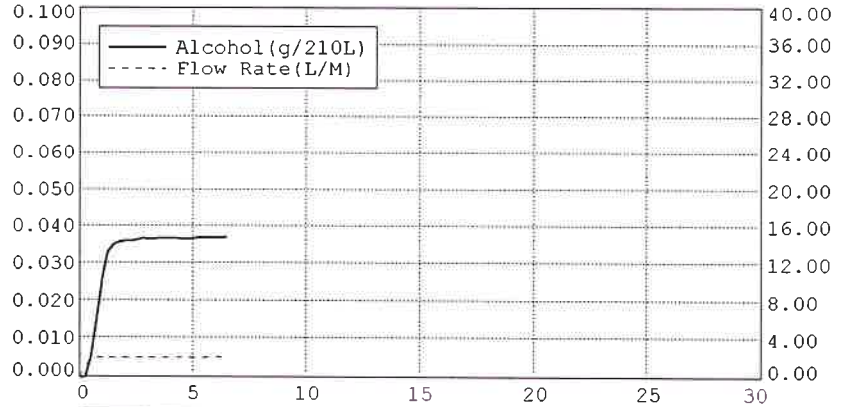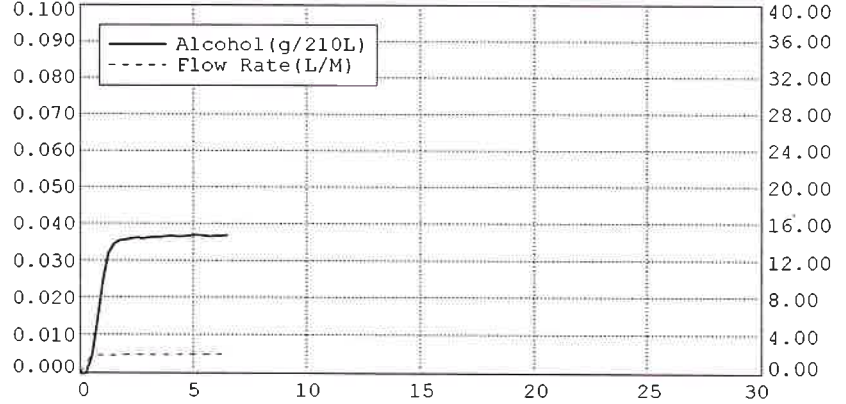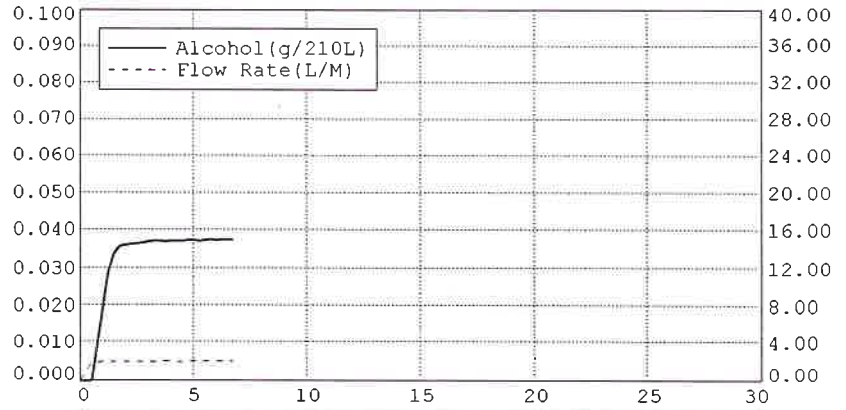

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100357






Date: 11/07/2024  
 Time: 10:33:10

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 28.85: 0.077  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025  
 TANK PRESSURE: 545 psi

BLANK TEST	0.000	10:34
INTERNAL STANDARD	VERIFIED	10:34
EXTERNAL STANDARD	0.077	10:34
BLANK TEST	0.000	10:35
EXTERNAL STANDARD	0.076	10:35
BLANK TEST	0.000	10:36
EXTERNAL STANDARD	0.076	10:37
BLANK TEST	0.000	10:37
EXTERNAL STANDARD	0.077	10:38
BLANK TEST	0.000	10:39
EXTERNAL STANDARD	0.076	10:39
BLANK TEST	0.000	10:40

Average = 0.0764  
 Std Dev = 0.0005

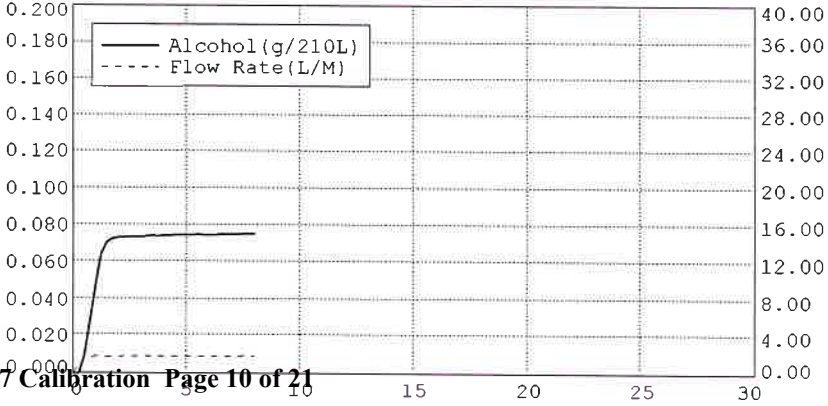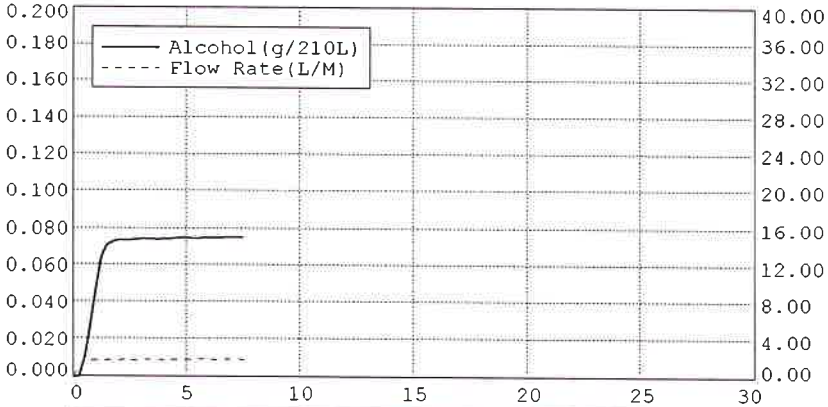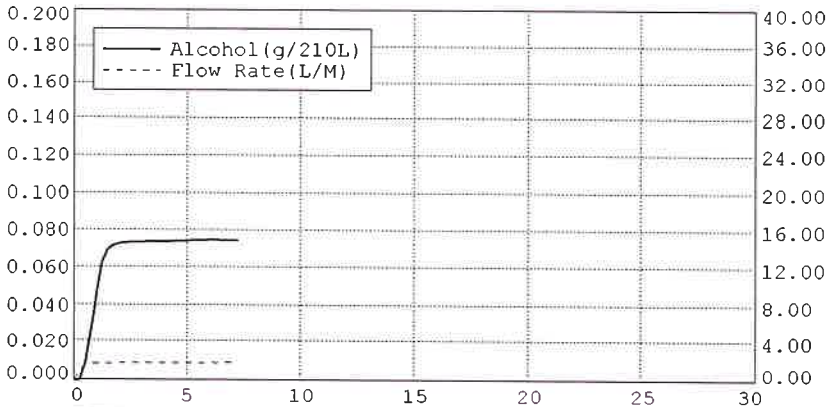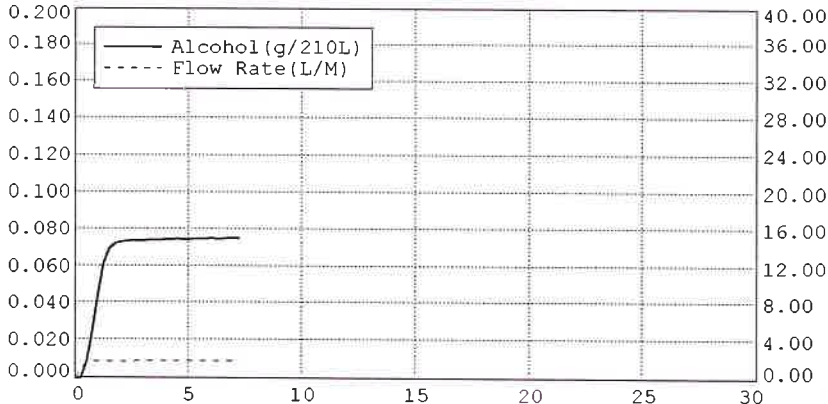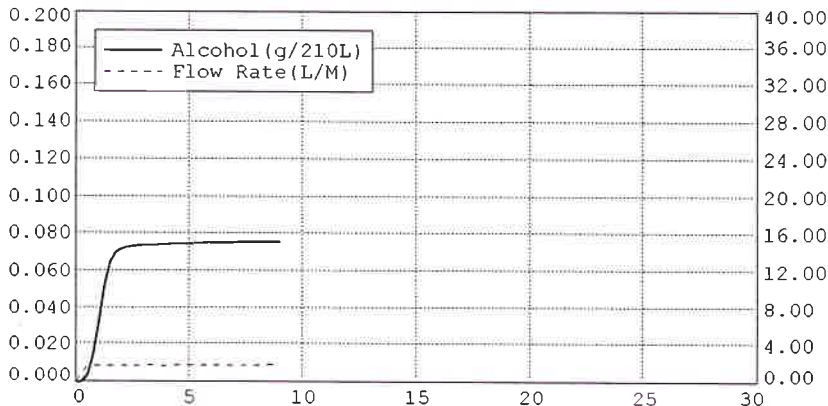

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
DATAMASTER dmt: 100357






Date: 11/07/2024  
Time: 10:41:42

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
TARGET AT 28.85: 0.096  
LOT #: AG333401  
EXPIRATION: 11/30/2025  
TANK PRESSURE: 727 psi

BLANK TEST	0.000	10:42
INTERNAL STANDARD	VERIFIED	10:43
EXTERNAL STANDARD	0.098	10:43
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.097	10:44
BLANK TEST	0.000	10:45
EXTERNAL STANDARD	0.097	10:45
BLANK TEST	0.000	10:46
EXTERNAL STANDARD	0.098	10:46
BLANK TEST	0.000	10:47
EXTERNAL STANDARD	0.097	10:48
BLANK TEST	0.000	10:48

Average = 0.0974  
Std Dev = 0.0005

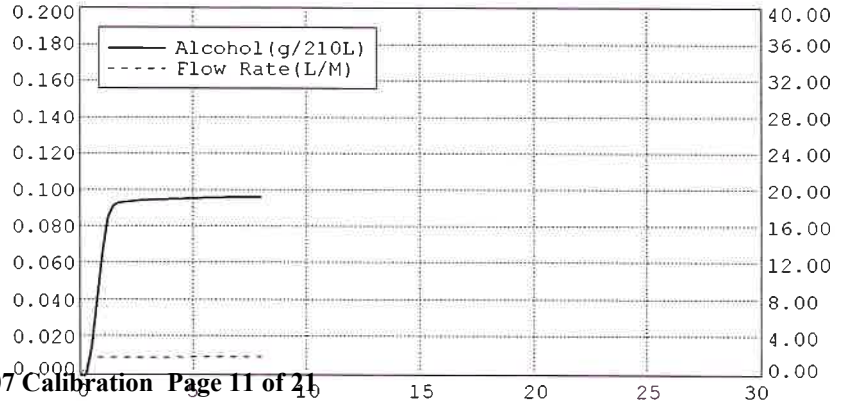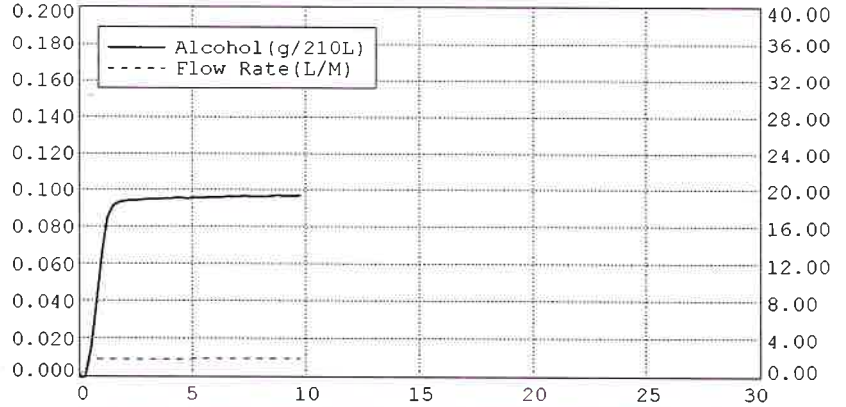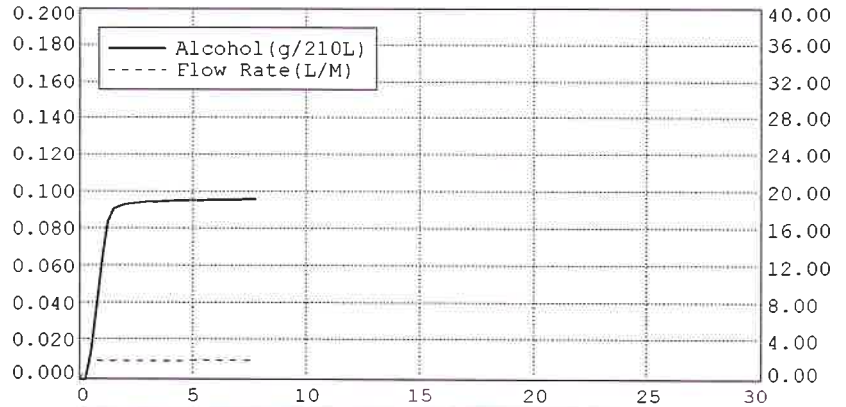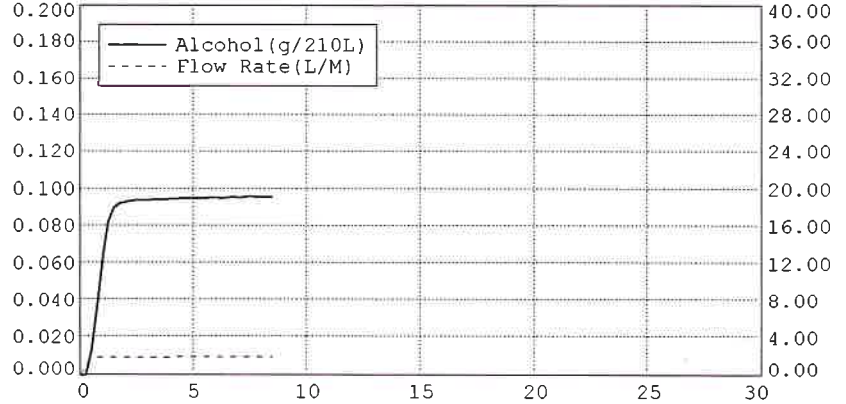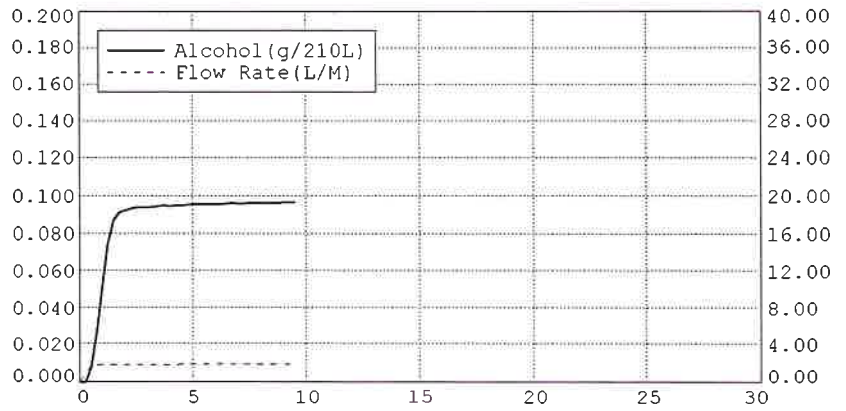

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100357






Date: 11/07/2024  
 Time: 10:49:50

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 28.85: 0.145  
 LOT #: AG332004  
 EXPIRATION: 11/16/2025  
 TANK PRESSURE: 348 psi

BLANK TEST	0.000	10:51
INTERNAL STANDARD	VERIFIED	10:51
EXTERNAL STANDARD	0.145	10:51
BLANK TEST	0.000	10:52
EXTERNAL STANDARD	0.144	10:52
BLANK TEST	0.000	10:53
EXTERNAL STANDARD	0.145	10:54
BLANK TEST	0.000	10:55
EXTERNAL STANDARD	0.143	10:55
BLANK TEST	0.000	10:56
EXTERNAL STANDARD	0.143	10:56
BLANK TEST	0.000	10:57

Average = 0.1440  
 Std Dev = 0.0010

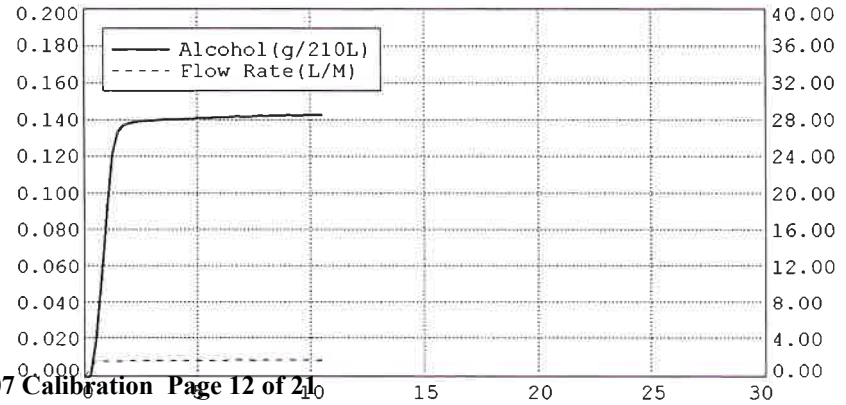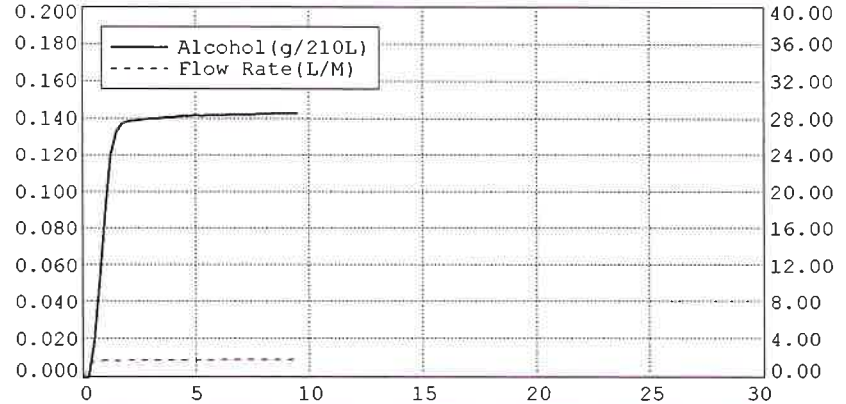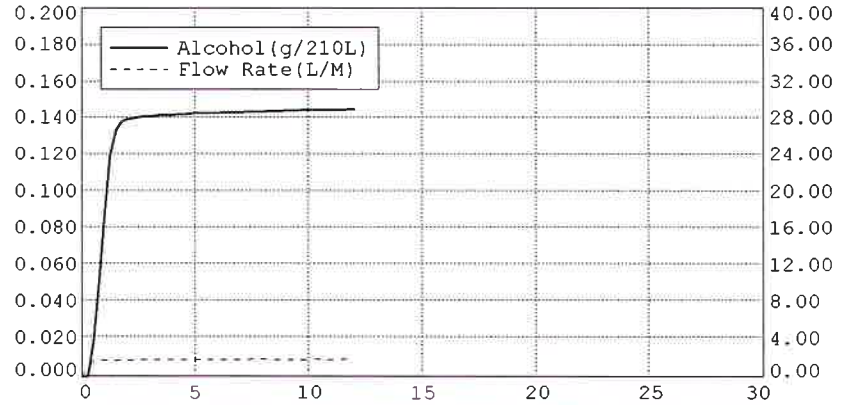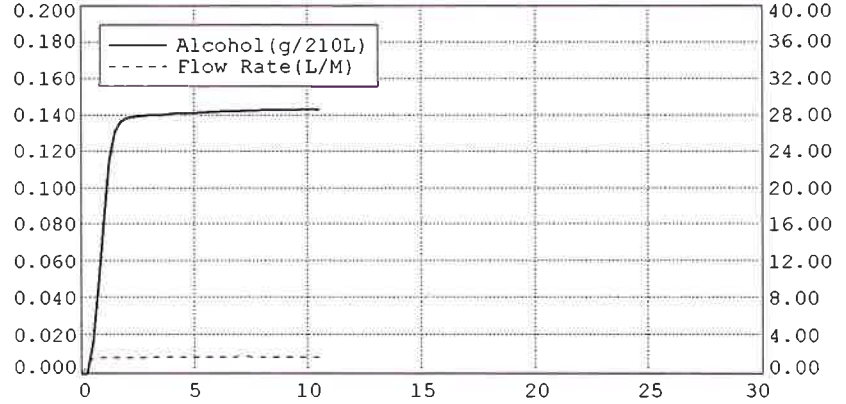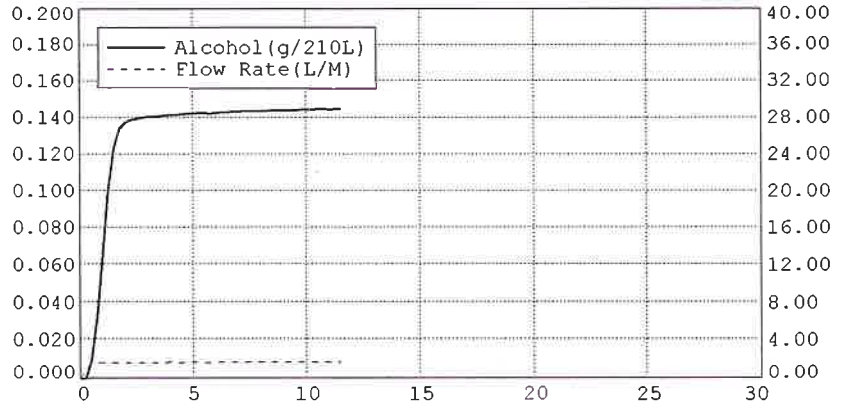

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100357






Date: 11/07/2024  
 Time: 10:58:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 28.85: 0.289  
 LOT #: AG427706  
 EXPIRATION: 10/03/2026  
 TANK PRESSURE: 368 psi

BLANK TEST	0.000	11:00
INTERNAL STANDARD	VERIFIED	11:00
EXTERNAL STANDARD	0.296	11:00
BLANK TEST	0.000	11:01
EXTERNAL STANDARD	0.295	11:02
BLANK TEST	0.000	11:03
EXTERNAL STANDARD	0.294	11:03
BLANK TEST	0.000	11:05
EXTERNAL STANDARD	0.294	11:05
BLANK TEST	0.000	11:06
EXTERNAL STANDARD	0.293	11:07
BLANK TEST	0.000	11:08

Average = 0.2944  
 Std Dev = 0.0011

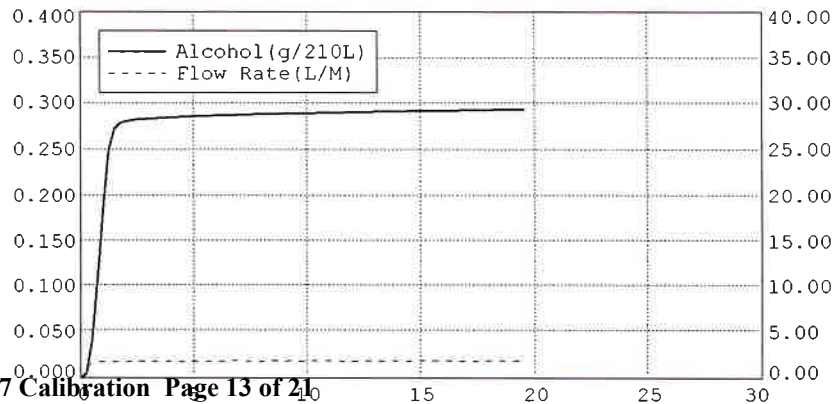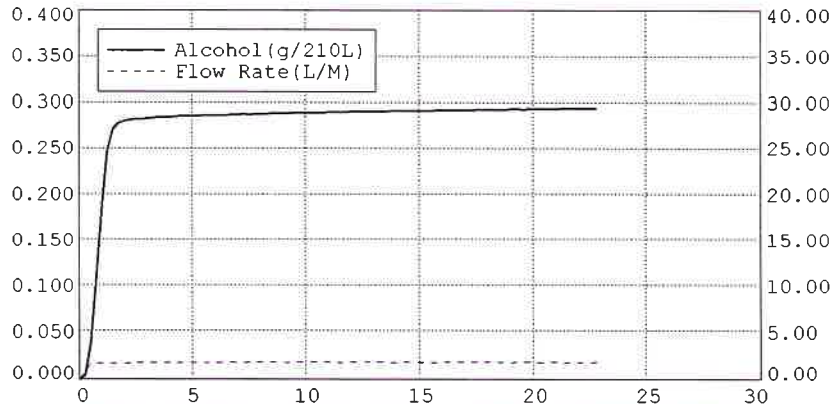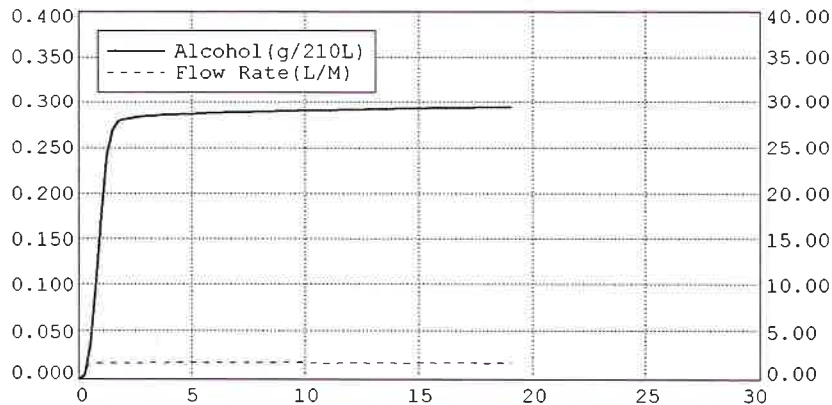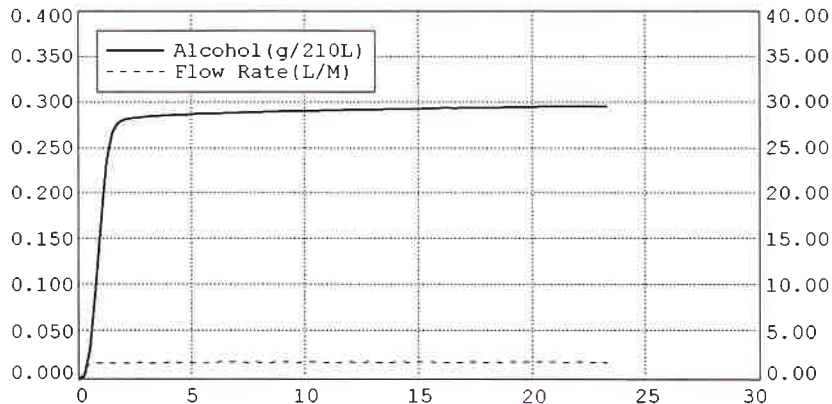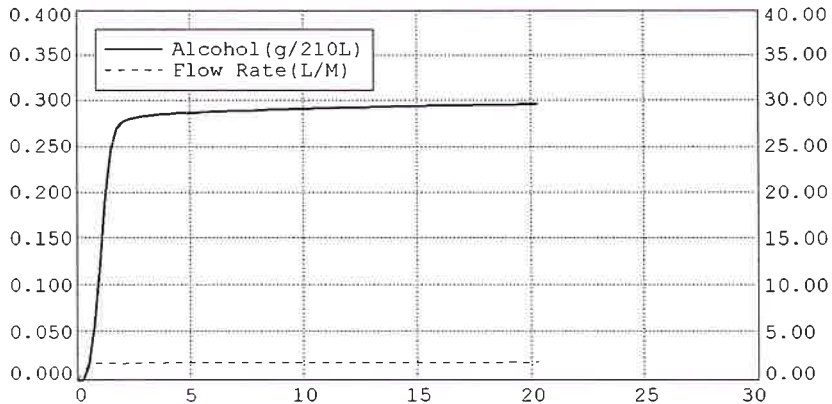

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100357

Date: 11/07/2024  
Time: 11:19:21

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746


DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.85: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:20  
BLANK TEST 0.000 11:20  
INTERNAL STANDARD VERIFIED 11:20  
EXTERNAL STANDARD 0.077 11:20  
BLANK TEST 0.000 11:21  
SUBJECT SAMPLE INCOMPLETE 11:23

KS

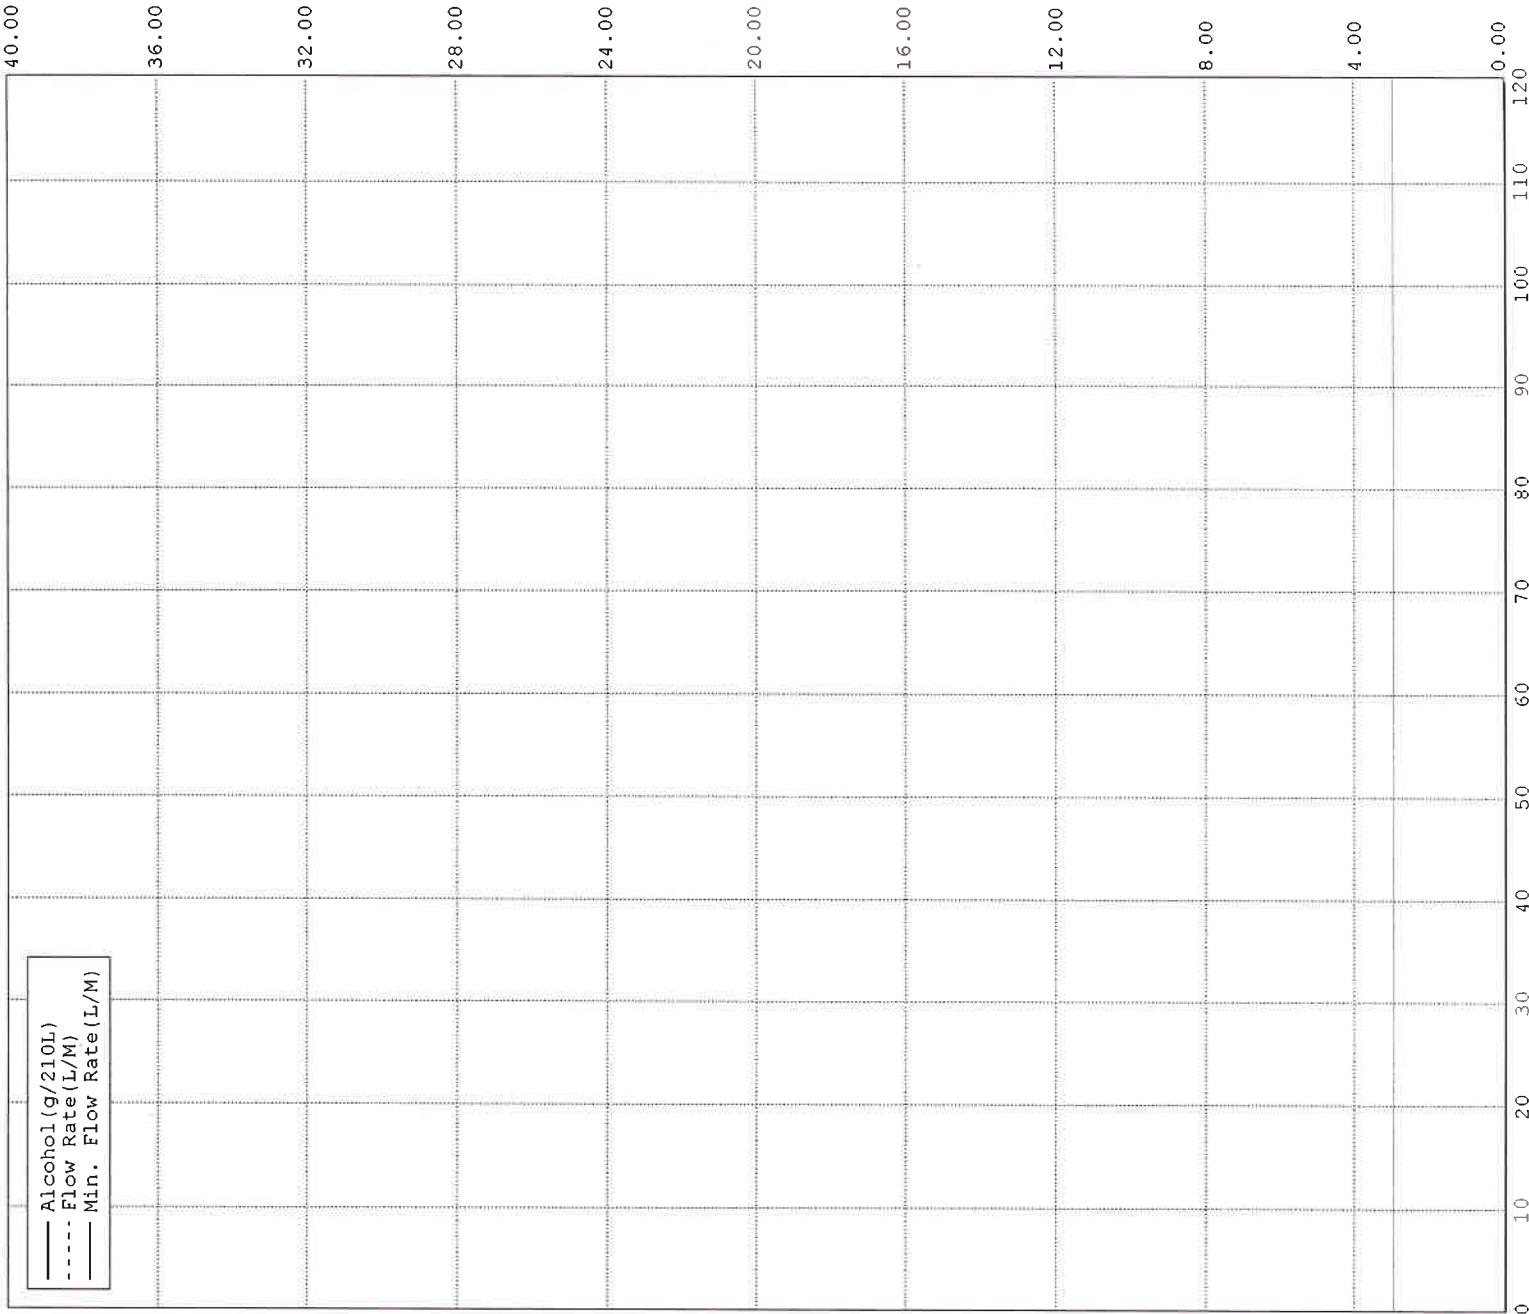

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100357

Date: 11/07/2024

Time: 11:25:22

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

KAIJA SWISHER

OPERATOR'S #: 10746

DEPT/AGENCY:

MAX ATTEMPTS

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 28.85: 0.077

LOT #: AG335202

EXPIRATION: 12/18/2025

PASSED 11:26

BLANK TEST 0.000 11:27

INTERNAL STANDARD VERIFIED 11:27


EXTERNAL STANDARD 0.077 11:27

BLANK TEST 0.000 11:28

SUBJECT SAMPLE XXX 11:28

Maximum Attempts Exceeded

KS

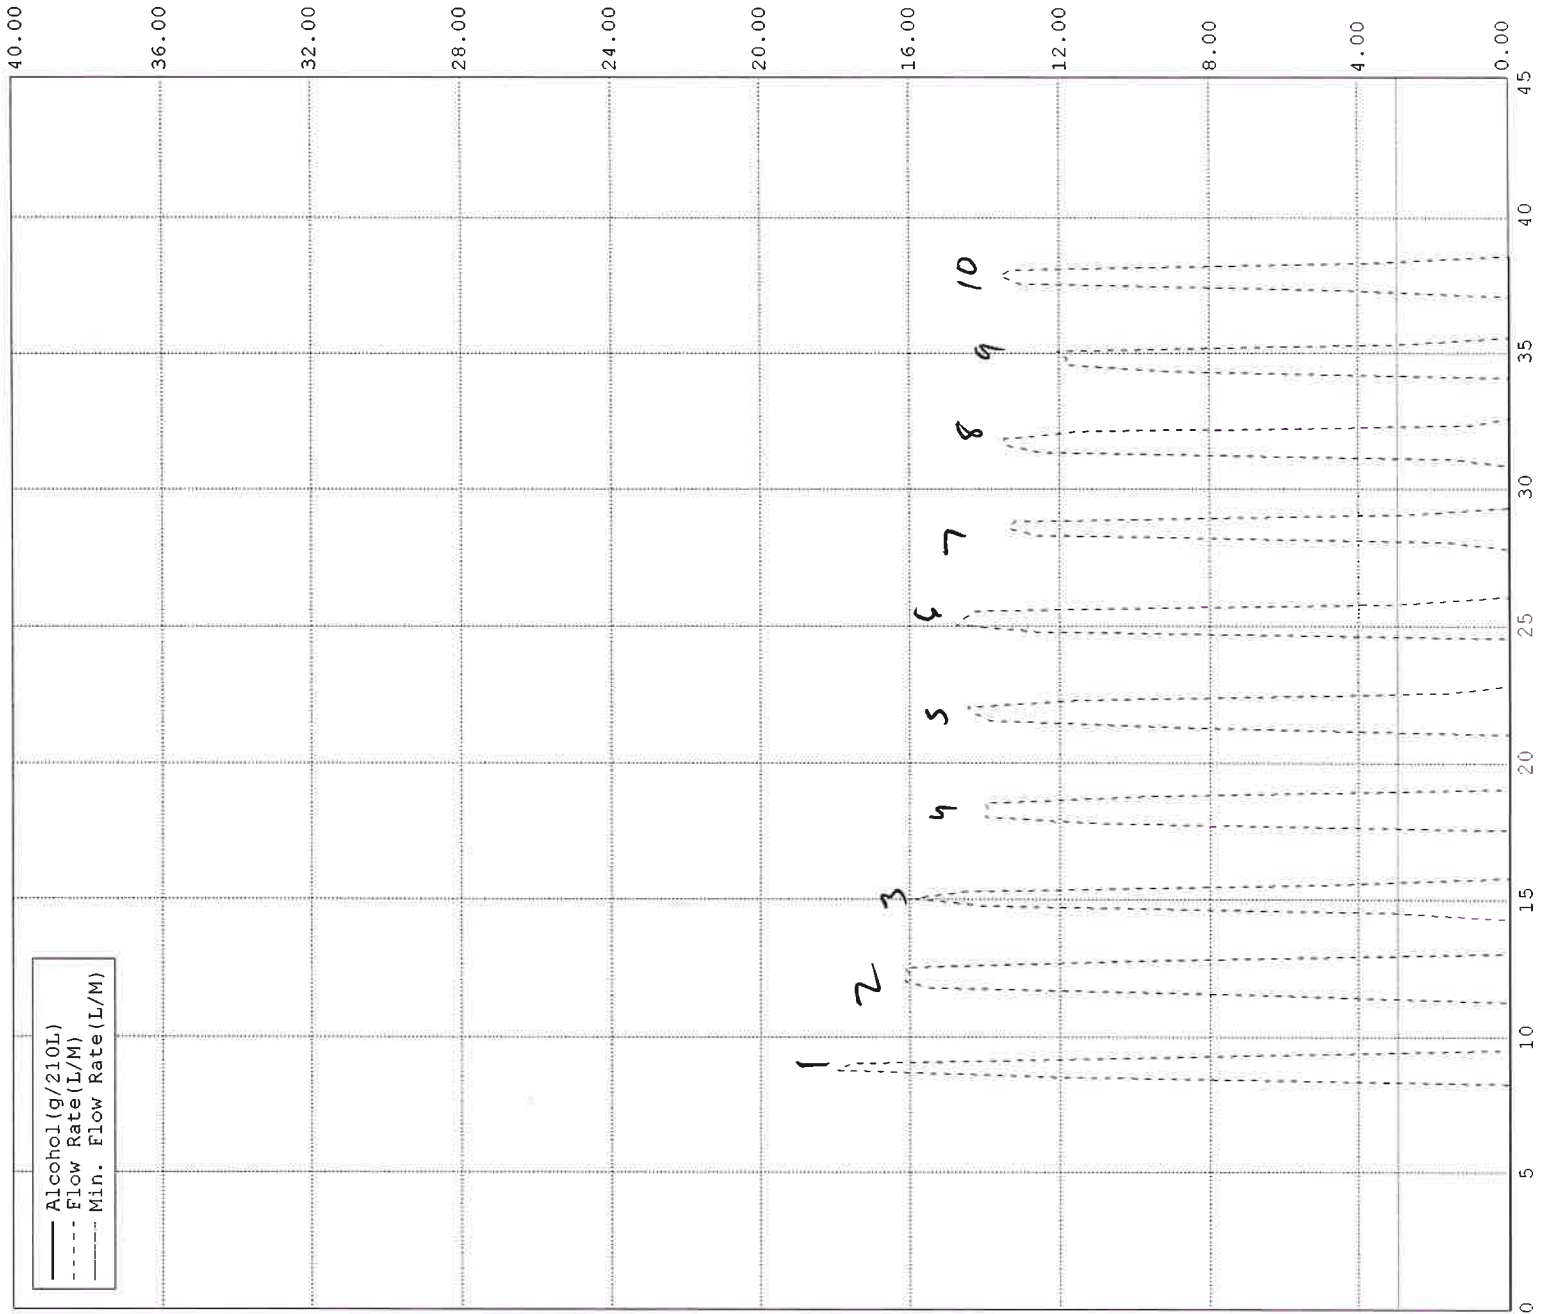

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100357

Date: 11/07/2024  
Time: 11:39:30

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAJJA SWISHER  
OPERATOR'S #: 10746


DEPT/AGENCY:  
INVALID  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.84: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK  
BLANK TEST PASSED 11:41  
INTERNAL STANDARD VERIFIED 11:42  
EXTERNAL STANDARD 0.077 11:42  
BLANK TEST 0.000 11:43  
SUBJECT SAMPLE INVALID 11:44

KS

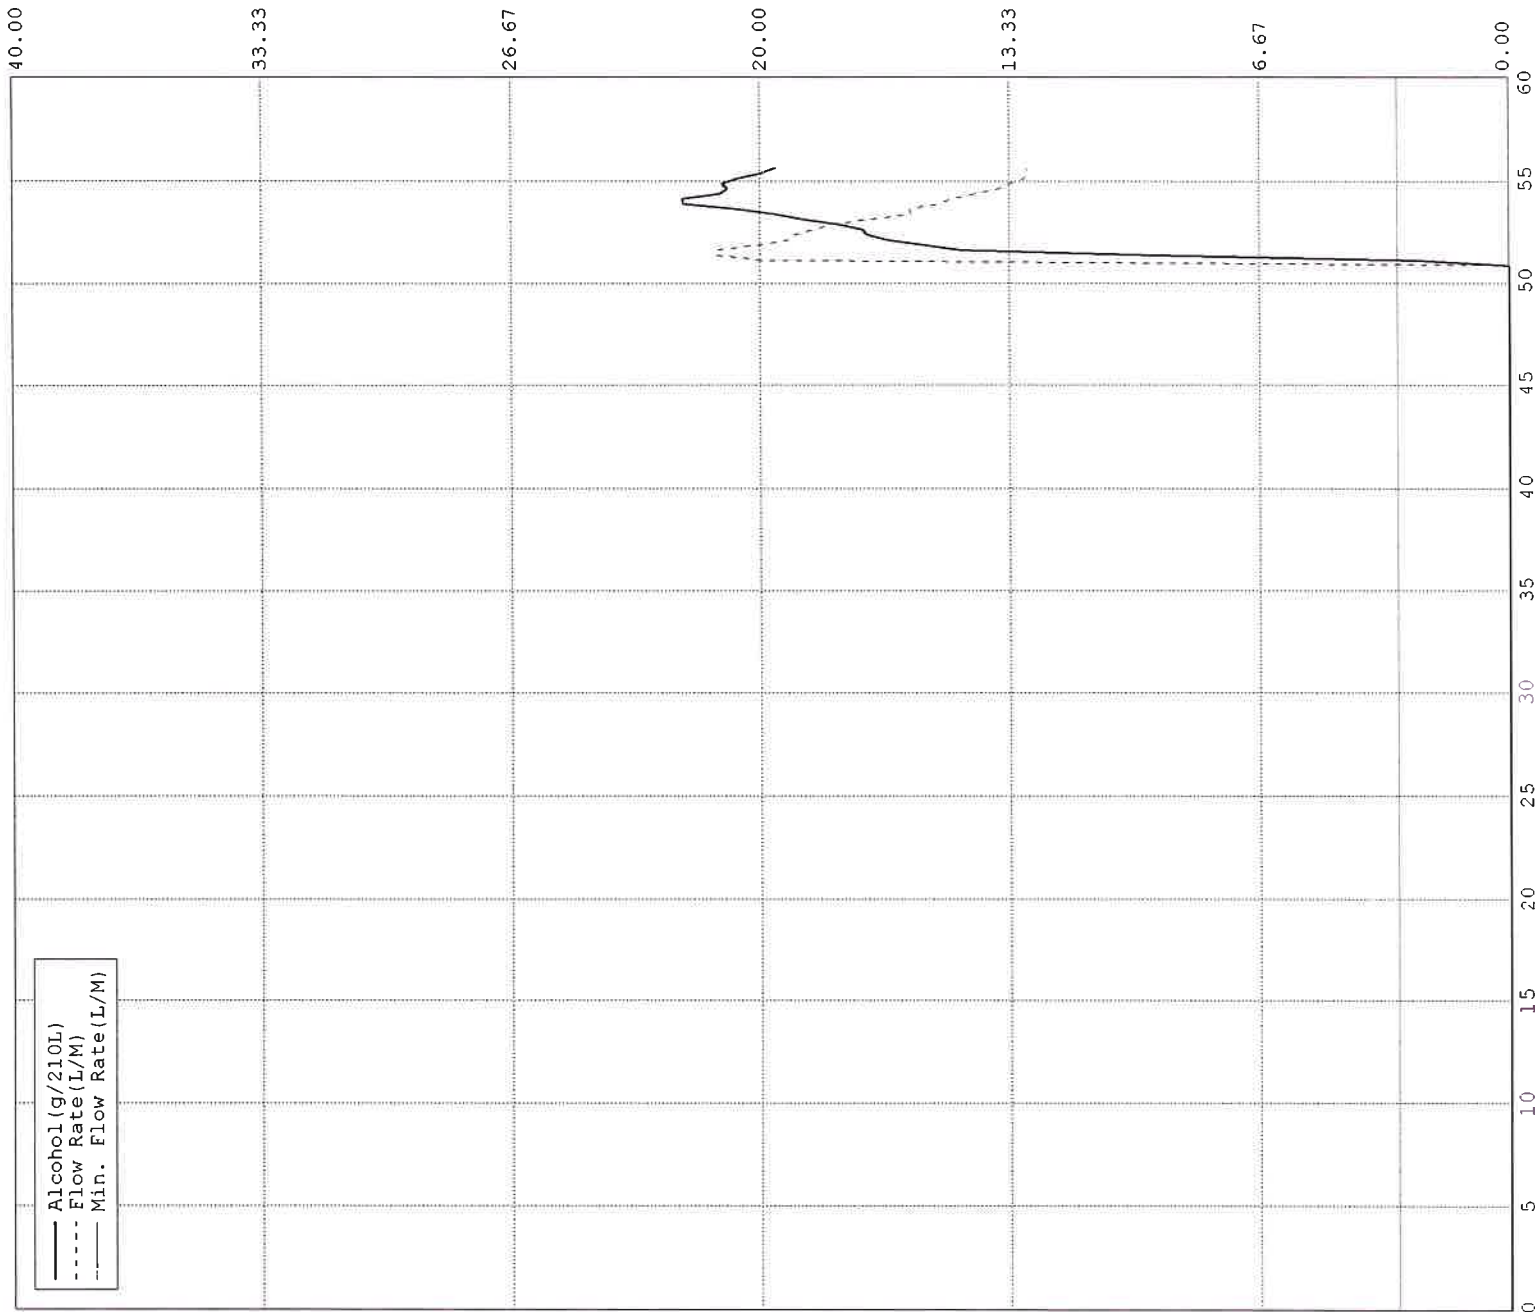



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100357

Date: 11/07/2024  
Time: 11:46:28

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
RFI

CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.83: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:48  
BLANK TEST 0.000 11:49  
INTERNAL STANDARD VERIFIED 11:49  
EXTERNAL STANDARD 0.077 11:49  
BLANK TEST 0.000 11:50

RFI DETECTED

KS

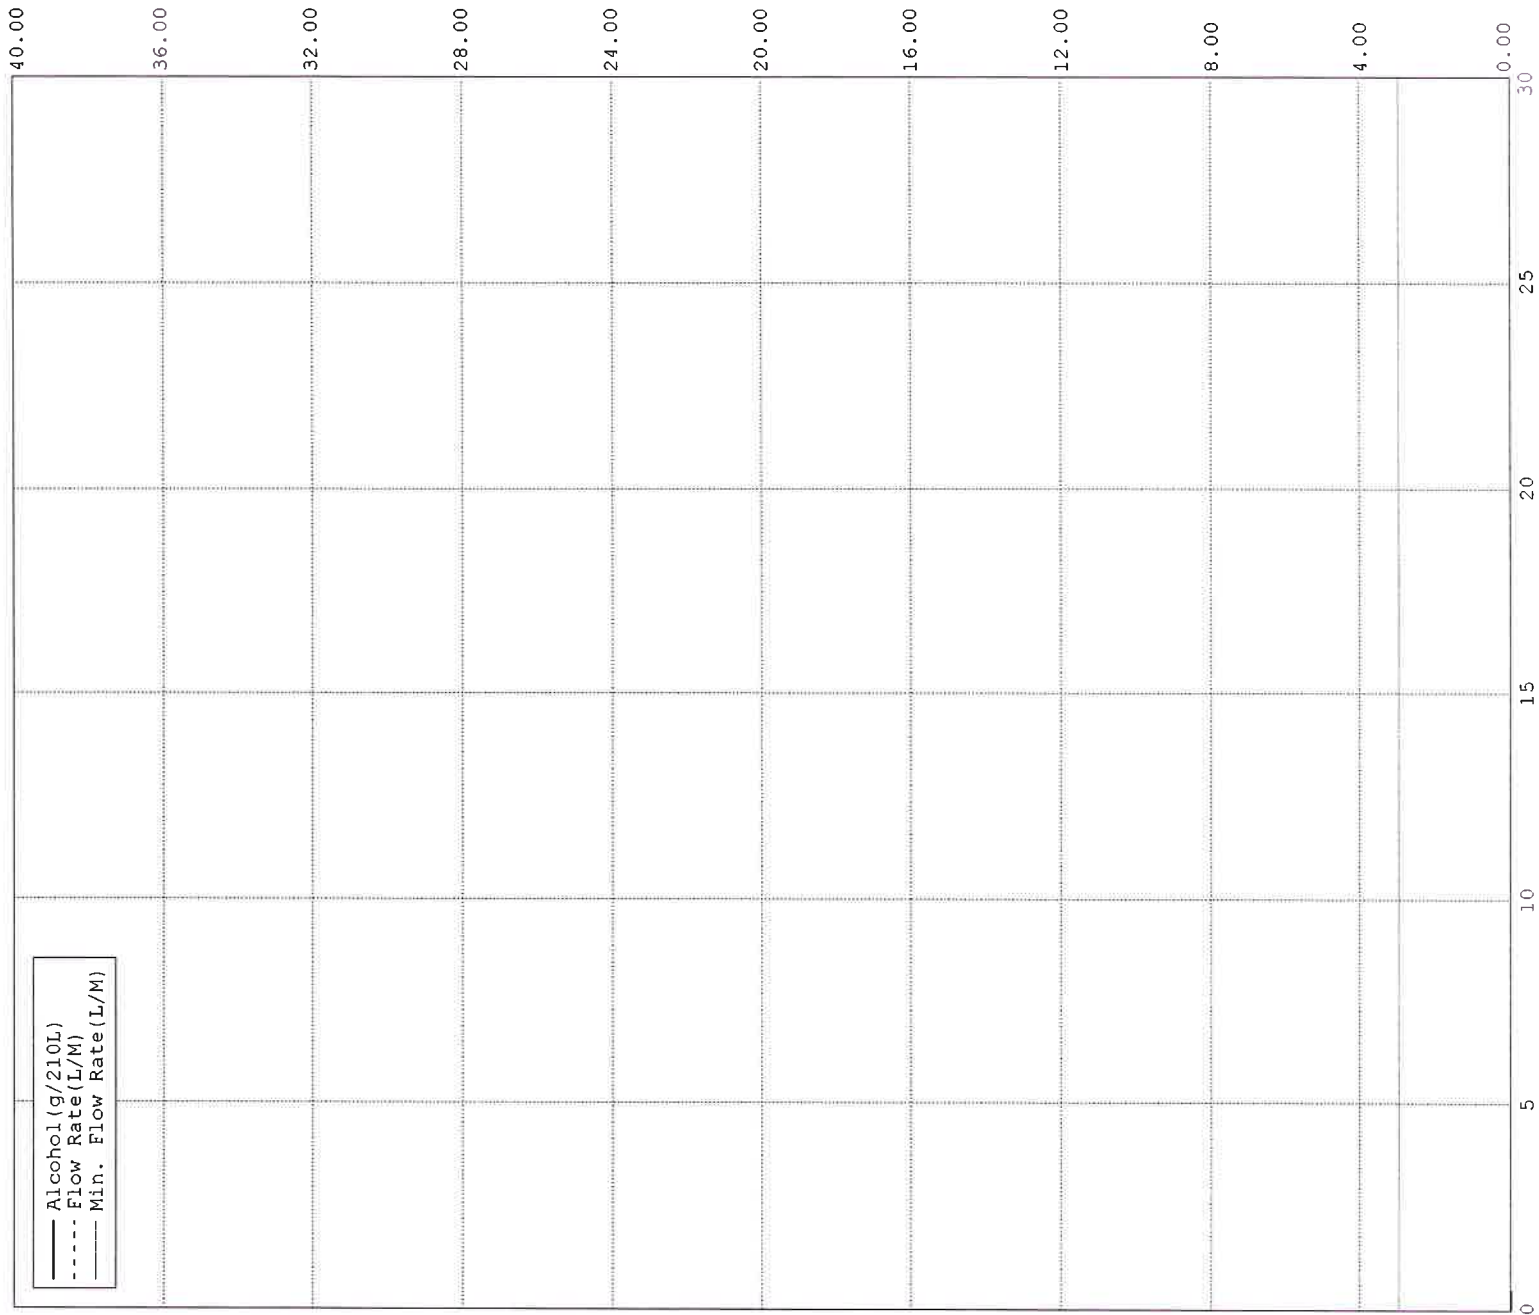

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100357

Date: 11/07/2024  
Time: 12:44:06

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
INTERFERENCE - ACETONE  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 28.82: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:45
BLANK TEST	0.000	12:45
INTERNAL STANDARD	VERIFIED	12:45
$x_g = 0.087$ (0.71%)	0.077	12:45
EXTERNAL STANDARD	$x[1] = 0.0022$ (0.0022)	
BLANK TEST	0.000	12:46
SUBJECT SAMPLE	XXX	12:47
$x[1] = 0.1216$ (-0.0192) (0.0038)		

Interference Detected

Filter 2 average is -0.0009  
Filter 3 average is 0.0022  
KS 11/7/24

KS

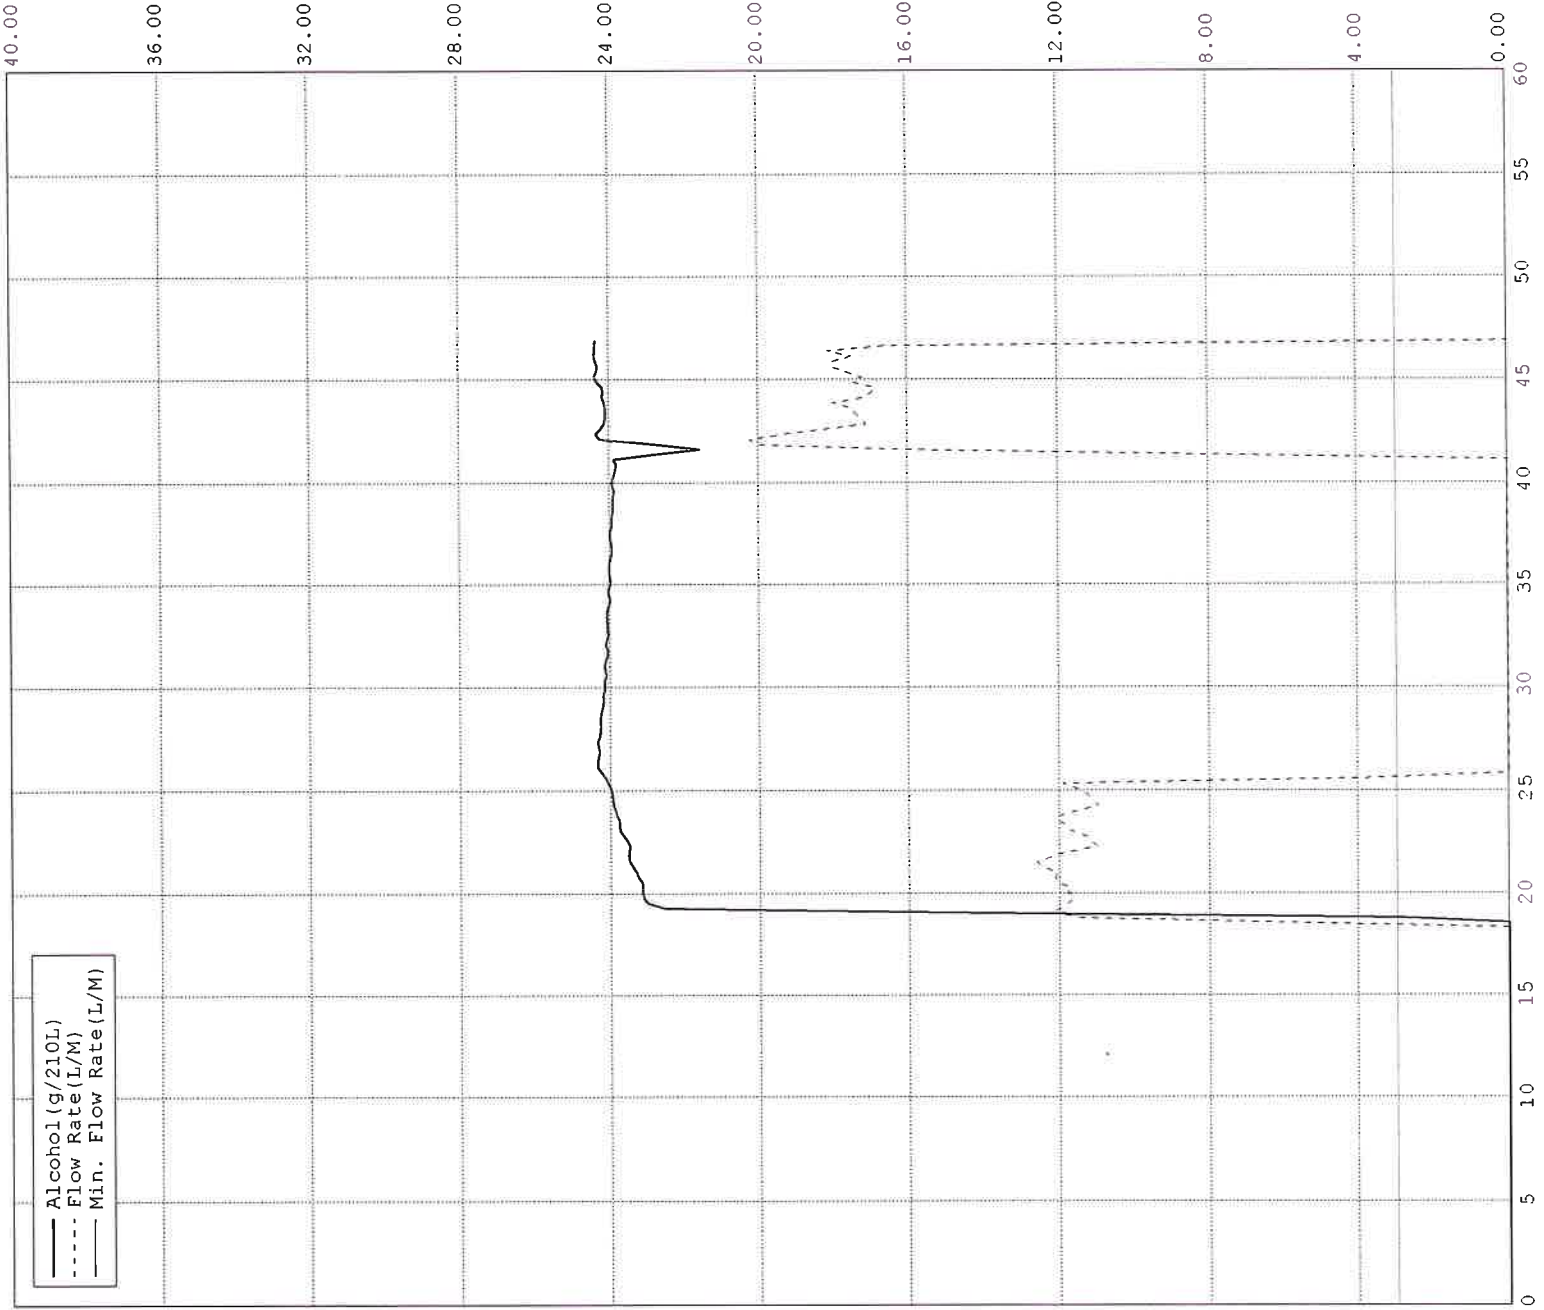

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100357

Date: 11/07/2024  
Time: 12:49:55

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KALJA SWISHER  
OPERATOR'S #: 10746


DEPT/AGENCY:  
INTERFERENCE - IPA  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.81: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 12:50  
BLANK TEST 0.000 12:51  
INTERNAL STANDARD VERIFIED 12:51  
Xg = 0.087 (0.71%)  
EXTERNAL STANDARD 0.077 12:51  
X[1] = 0.0771 (-0.0008) (0.0022)  
BLANK TEST 0.000 12:52  
SUBJECT SAMPLE XXX 12:52  
X[1] = 0.1255 (-0.0301) (0.0011)

Interference Detected

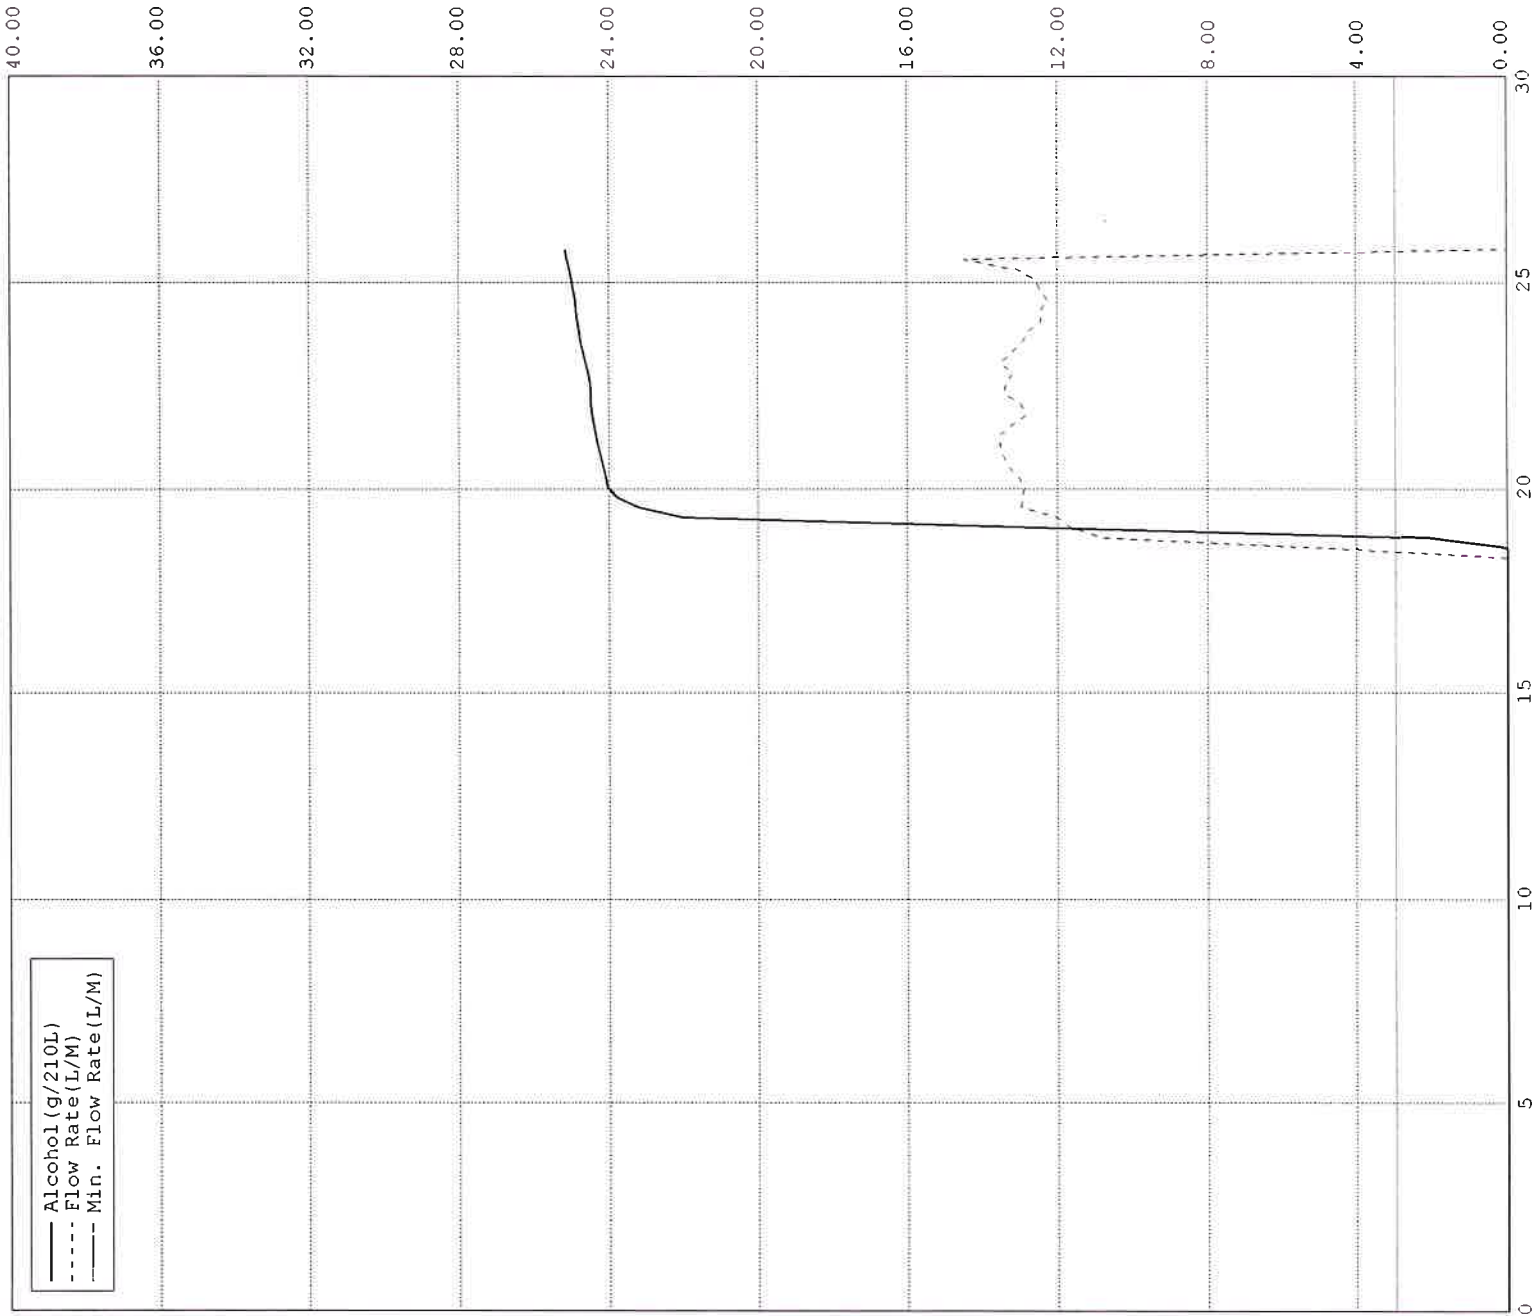

CS

SUBJECT TEST

Alaska Department of Public Safety  
 DATAMASTER dmt: 100357

Date: 11/07/2024  
 Time: 12:55:38

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXX

OPERATOR NAME:  
 KAIJA SWISHER  
 OPERATOR'S #: 10746


DEPT/AGENCY:  
 INTERFERENCE - NEGATIVE  
 CASE/REPORT: XXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 28.82: 0.077  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:56
BLANK TEST	0.000	12:56
INTERNAL STANDARD	VERIFIED	12:56
Xq = 0.087 (1.01%)		
EXTERNAL STANDARD	0.077	12:57
X[1] = 0.0768 (-0.0009) (0.0024)		
BLANK TEST	0.000	12:58
SUBJECT SAMPLE (Vol=1.53L)	0.100	12:58
X[1] = 0.1002 (-0.0013) (0.0014)		
BLANK TEST	0.000	12:59
EXTERNAL STANDARD	0.076	12:59
X[1] = 0.0763 (-0.0006) (0.0021)		
BLANK TEST	0.000	13:00

KS

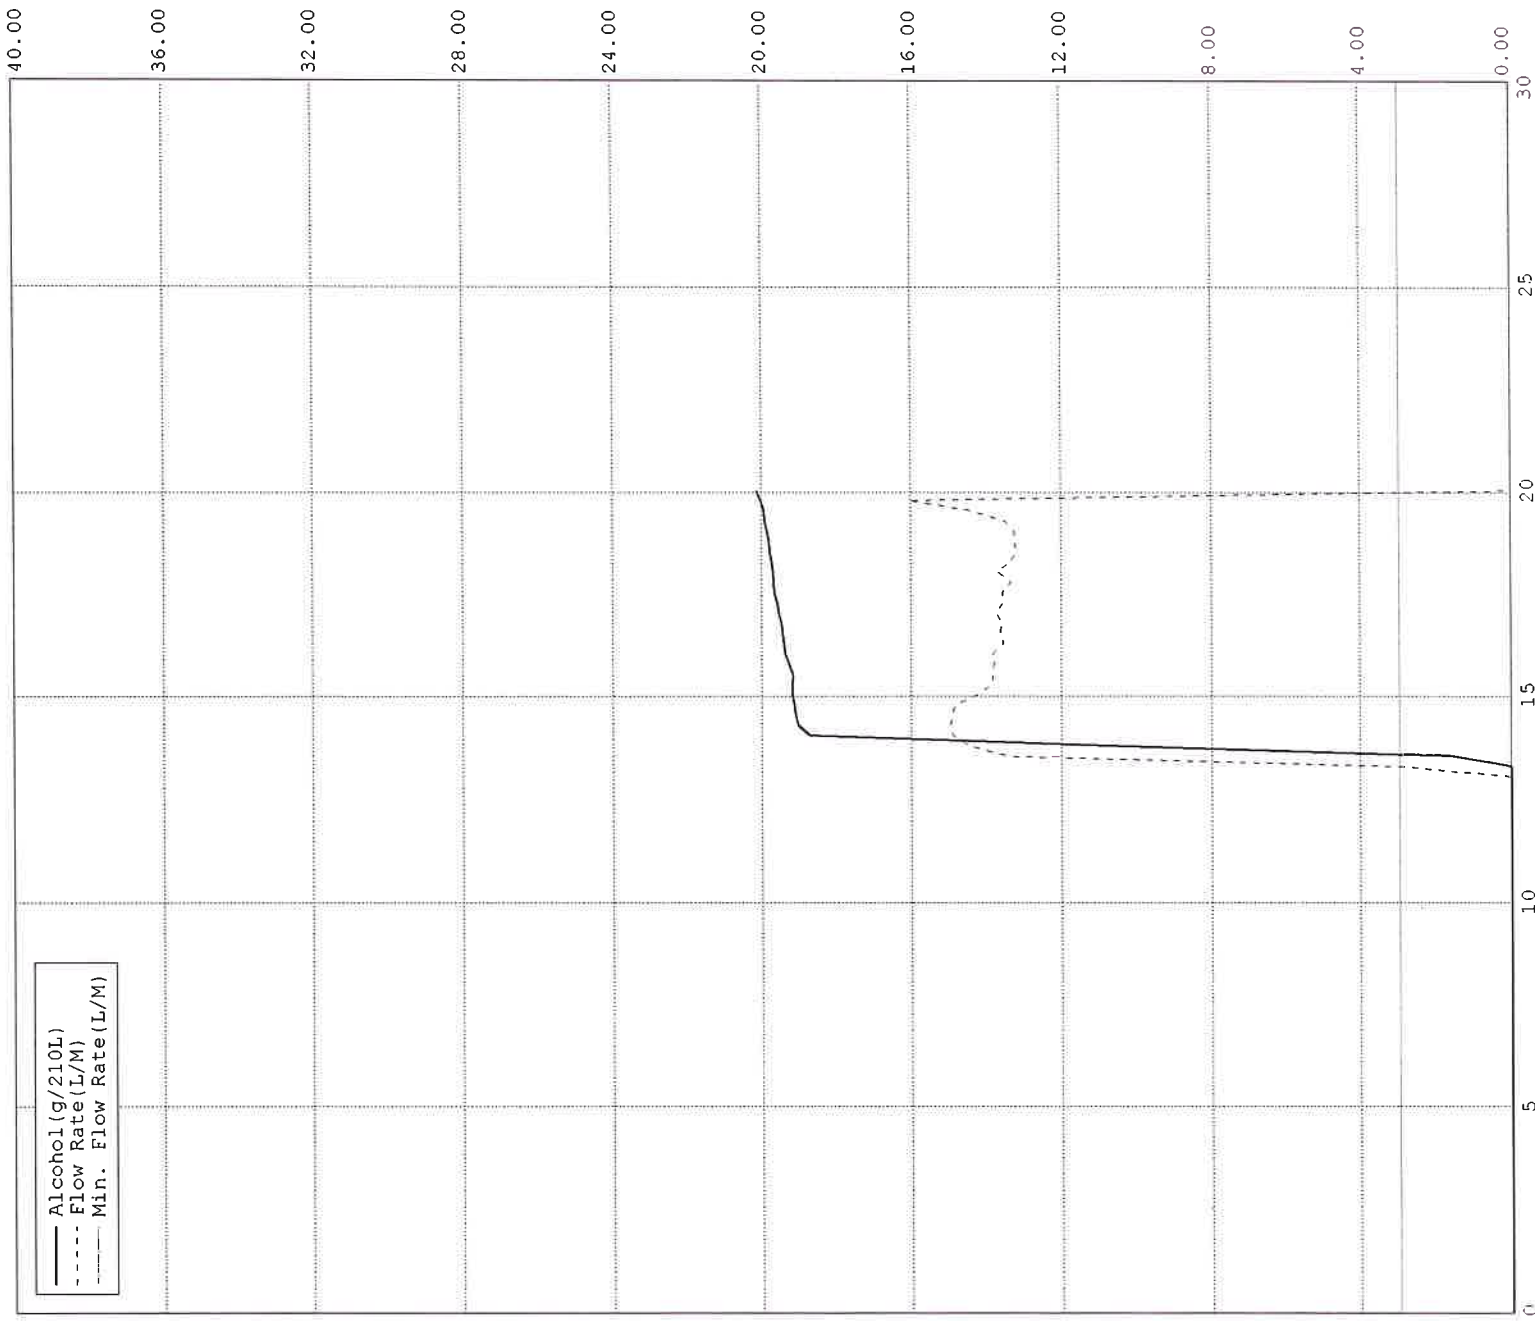

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100357

Date: 11/07/2024  
Time: 13:59:14

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 28.81: 0.077  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:00
BLANK TEST	0.000	14:00
INTERNAL STANDARD	VERIFIED	14:01
EXTERNAL STANDARD	0.077	14:01
BLANK TEST	0.000	14:02
SUBJECT SAMPLE (Vol=2.44L)	0.000	14:02
BLANK TEST	0.000	14:03
EXTERNAL STANDARD	0.077	14:03
BLANK TEST	0.000	14:04

KS

