

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100376

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 10/27/2021

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 28.98: 0.077

LOT #: ~~AG10102~~ ~~AG0618102~~ OKC 11/8/2021 ✗

EXPIRATION: 06/29/2022

TANK PRESSURE: 1162 psi

BLANK TEST	0.000	01:44
INTERNAL STANDARD	VERIFIED	01:44
EXTERNAL STANDARD	0.076	01:45
BLANK TEST	0.000	01:46
EXTERNAL STANDARD	0.076	01:46
BLANK TEST	0.000	01:47
EXTERNAL STANDARD	0.077	01:47
BLANK TEST	0.000	01:48
EXTERNAL STANDARD	0.077	01:48
BLANK TEST	0.000	01:49
EXTERNAL STANDARD	0.077	01:49
BLANK TEST	0.000	01:50

Average = 0.0766

Std Dev = 0.0005

## Diagnostic Check

### VERSIONS

DMT: 3.02

PIC: 3.02

Modem: 2.6

Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.9°C PASSED

Breath Tube = 46.7°C PASSED

### PUMP INFO

Flow Rate = 3.881 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED

PUMP OFF PASSED

### FILTER INFO

Filter 1 PASSED

Filter 2 PASSED

Filter 3 PASSED

INTERNAL STANDARD PASSED

\* Incorrect lot #.

See 100376 2021.11.08 Change In Status  
OKC-11/9/21

I, Brandi M. Barnett, after being first duly sworn, depose and state as follows:

(1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.

(2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.

(3) I am the Scientific Director of the State Breath Alcohol Program.

(4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.


(5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.

(6) The referenced instrument is certified for evidentiary use in the State of Alaska.



 12/3/21

Brandi M. Barnett  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 03 day of 12, 20 21



Notary Public  
My Commission Expires With Office

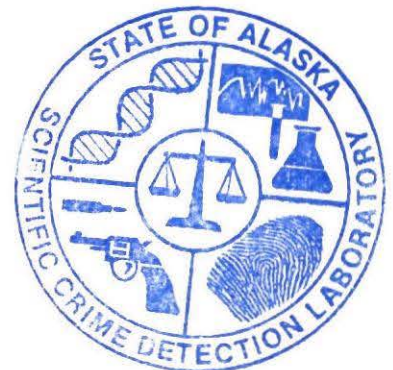

OKC  
11/8/21