

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100378

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 05/19/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.93: 0.080
LOT #: 09214080A3
EXPIRATION: 05/01/2016
TANK PRESSURE: 599 psi

BLANK TEST	0.000	10:02
INTERNAL STANDARD	VERIFIED	10:03
EXTERNAL STANDARD	0.081	10:03
BLANK TEST	0.000	10:04
EXTERNAL STANDARD	0.080	10:04
BLANK TEST	0.000	10:05
EXTERNAL STANDARD	0.080	10:05
BLANK TEST	0.000	10:06
EXTERNAL STANDARD	0.081	10:06
BLANK TEST	0.000	10:07
EXTERNAL STANDARD	0.080	10:07
BLANK TEST	0.000	10:08

Average = 0.0804
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 3.00
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
Breath Tube = 48.1°C PASSED

PUMP INFO

Flow Rate = 4.411 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO

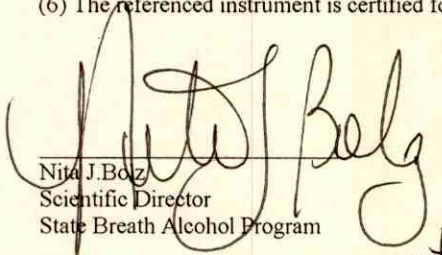
Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

7/20/2015

Subscribed and sworn before me this 20th day of July, 2015


Nikki Roth, Notary Public
My Commission Expires With Office



7/15/15
003