	State of Alaska Scientific Crime Detection Laboratory	
	DataMaster Acceptance Form -- DMAF2011R0	
	Issuing Authority -- Nita Bolz, Scientific Director	
Approval date: 03/01/11	Effective date: 03/01/11	Archive date: Active


DataMaster DMT Acceptance Form

Instrument # 100405

Date: 5/31/11

Analyst: Colleen O'Bryant

1. Check in instrument in to JusticeTrax Breath Alcohol Database:
2. Visual Inspection
3. Update software
4. Print calibration factors (attached)
5. NPAS calibration paperwork (attached)
6. Barcode Instrument
7. State of Alaska Property ID# PGS 5/31/11 12-FD347

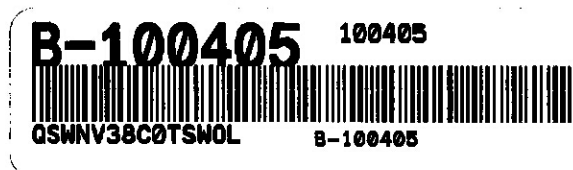

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100405

Date: 05/03/2011
Time: 11:47:16

Ca = 0.1000
CAL = 0.983919 0.800 <= CAL < 1.200
b1 = 0.0003 0.0000 <= b1 < 0.0040
b2 = 0.0028 0.0010 <= b2 < 0.0100
b3 = 0.0000 0.0000 <= b3 < 0.0040
Xq = 0.0855 0.0500 <= Xq < 0.2000
a21 = 1.121109 1.050 <= a21 < 1.300
a31 = 0.488526 0.300 <= a31 < 0.800

COB 2/3



Certificate of Calibration

100405

Instrument Serial Number

10180

Standard Reference Number

The above instrument has been calibrated and is hereby certified for use in determining alcohol breath concentration when used in accordance with the operating guidelines by a properly trained operator.

5-3-11

Date

A handwritten signature in black ink, appearing to be "C. Bryant", written over a horizontal line.

Technician

COB 5/3

Final page for report

\

\\ANCSCLSAN01\JTRAX\CASEDOCS\B-100405\B-100405 ECF-20140

7/9/2014