



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100371

**Report Issue Date:** 06/13/2023  
**Date Received:** 2023-01-25  
**Condition of Item:** Good

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 01/25/2023 - As Found - End Date 01/25/2023 As Found - Evaluation Analyst:** Colleen O'Bryant  
 As Found Conditions - Barometric Pressure (inHg): 29.37 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.1  
 Relative Humidity (%): 22

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.018	0.019	0.019	0.019	0.019	0.019	0.019
0.080	0.079	AG135004	0.075	0.075	0.076	0.076	0.076	0.076	0.076
0.300	0.295	AG217903	0.288	0.287	0.288	0.289	0.289	0.289	0.288

**Start Date 04/11/2023 - As Left - End Date 04/11/2023**  
 As Left Conditions - Barometric Pressure (inHg): 29.65 Barometer Used: Fisher S/N 221250180 Temperature (C): 23.1 Relative  
 Humidity (%): 14

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG217902	0.019	0.019	0.020	0.020	0.019	0.019	+/- 0.002	
0.040	0.040	AG217904	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003	
0.080	0.079	AG113402	0.077	0.077	0.076	0.077	0.077	0.077	+/- 0.003	
0.100	0.099	AG211003	0.097	0.097	0.097	0.097	0.097	0.097	+/- 0.003	
0.150	0.149	AG134205	0.146	0.146	0.146	0.146	0.146	0.146	+/- 0.004	
0.300	0.297	AG217903	0.292	0.292	0.292	0.293	0.293	0.292	+/- 0.008	

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Colleen O'Bryant on 06/05/2023

[colleen.obryant@alaska.gov](mailto:colleen.obryant@alaska.gov)

Technically and administratively reviewed by Brandi Barnett on 06/13/2023

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100371 Analyst: Tatiana Malinck Start Date: 04/11/2023

- Diagnostic Test (attached)
- Adjust voltages, if needed
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
- Internal Standard value  $\leq$  3.00%
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.6 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.65 Temperature (C): 23.1 Relative Humidity (%): 14%

Linearity Test (attached)

0.020g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG217902</u>	Exp:	<u>06/28/2024</u>
0.040g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG217904</u>	Exp:	<u>06/28/2024</u>
0.080g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG113402</u>	Exp:	<u>05/14/2023</u>
0.100g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG211003</u>	Exp:	<u>04/20/2024</u>
0.150g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG134205</u>	Exp:	<u>12/08/2023</u>
0.300g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG217903</u>	Exp:	<u>06/28/2024</u>

Functional Tests (attached)

- Incomplete
- Maximum Attempts Exceeded
- Interference (Volatiles)
- Invalid
- Radio Frequency Interference (RFI)

Acetone Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11/09/2023

Simulator S/N: DR41U1 Verification Performed?

Isopropanol Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11/09/2023

Simulator S/N: SD1088 Verification Performed?

Neg. Control Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11/09/2023

Simulator S/N: SD1177 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/09/2023

- Verify stylus is calibrated
  - Reset Options
  - Clear Memory
  - Verification of Calibration (VOC)
  - Non-Drinking Subject Test
  - Upload
  - Remove Tank Prior to Shutdown
- Calibration End Date: 04/11/2023

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100371  
-----

Date: 04/11/2023  
Time: 07:49:31

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C                    PASSED  
(44.0°C - 52.0°C)  
Breath Tube       = 48.1°C                   PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage     = 1.83 V                   PASSED  
(1.00 V - 2.34 V)  
Cooler Voltage   = 1.79 V                   PASSED  
(1.04 V - 2.44 V)  
Bias Voltage     = 78 V                     PASSED  
(47 V - 111 V)  
Chopper Freq    = 535 Hz                     PASSED  
(475 Hz - 575 Hz)  
Barometer        = 29.6 in

PUMP INFO

Flow Rate = 4.322 L/M                    PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON                                   PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF                                  PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1                                   PASSED  
Filter 2                                   PASSED  
Filter 3                                   PASSED

INTERNAL STANDARD                       PASSED  
Xq = 0.082 1.62% (0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100371  
-----

Date: 04/11/2023  
Time: 7:55 AM

Temperatures (°C)  
Sample Cell: 48.9°C  
Breath Tube: 47.8°C

Current Barometer 29.6 in  
Volume (Ltr) 1.57

Settings  
Lamp: 1.91 V  
Bias: 78 V  
Cooler: 1.74 V  
Chopper: 534 Hz

Voltages (V)  
Flow: 1.05 V  
Detector: 0.083 V



CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100371  
-----

Date: 09/20/2018  
Time: 15:09:09

OPERATOR NAME:  
DEREK WALTON  
CERTIFICATE #: 9508

Ca = 0.1000  
CAL = 0.963456    0.800 <= CAL < 1.200  
b1 = 0.0001    0.0000 <= b1 < 0.0040  
b2 = 0.0050    0.0010 <= b2 < 0.0100  
b3 = 0.0003    0.0000 <= b3 < 0.0040  
Xq = 0.0804    0.0500 <= Xq < 0.2000  
a21 = 1.174632    1.050 <= a21 < 1.300  
a31 = 0.497645    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100371

Date: 04/11/2023  
Time: 07:56:24

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
MINIMUM VOLUME TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.64: 0.079  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	07:57
BLANK TEST	0.000	07:57
INTERNAL STANDARD	VERIFIED	07:57
EXTERNAL STANDARD	0.077	07:57
BLANK TEST	0.000	07:58
SUBJECT SAMPLE (Vol=1.58L)	0.000	07:59
BLANK TEST	0.000	08:00
EXTERNAL STANDARD	0.076	08:01
BLANK TEST	0.000	08:01

TLM

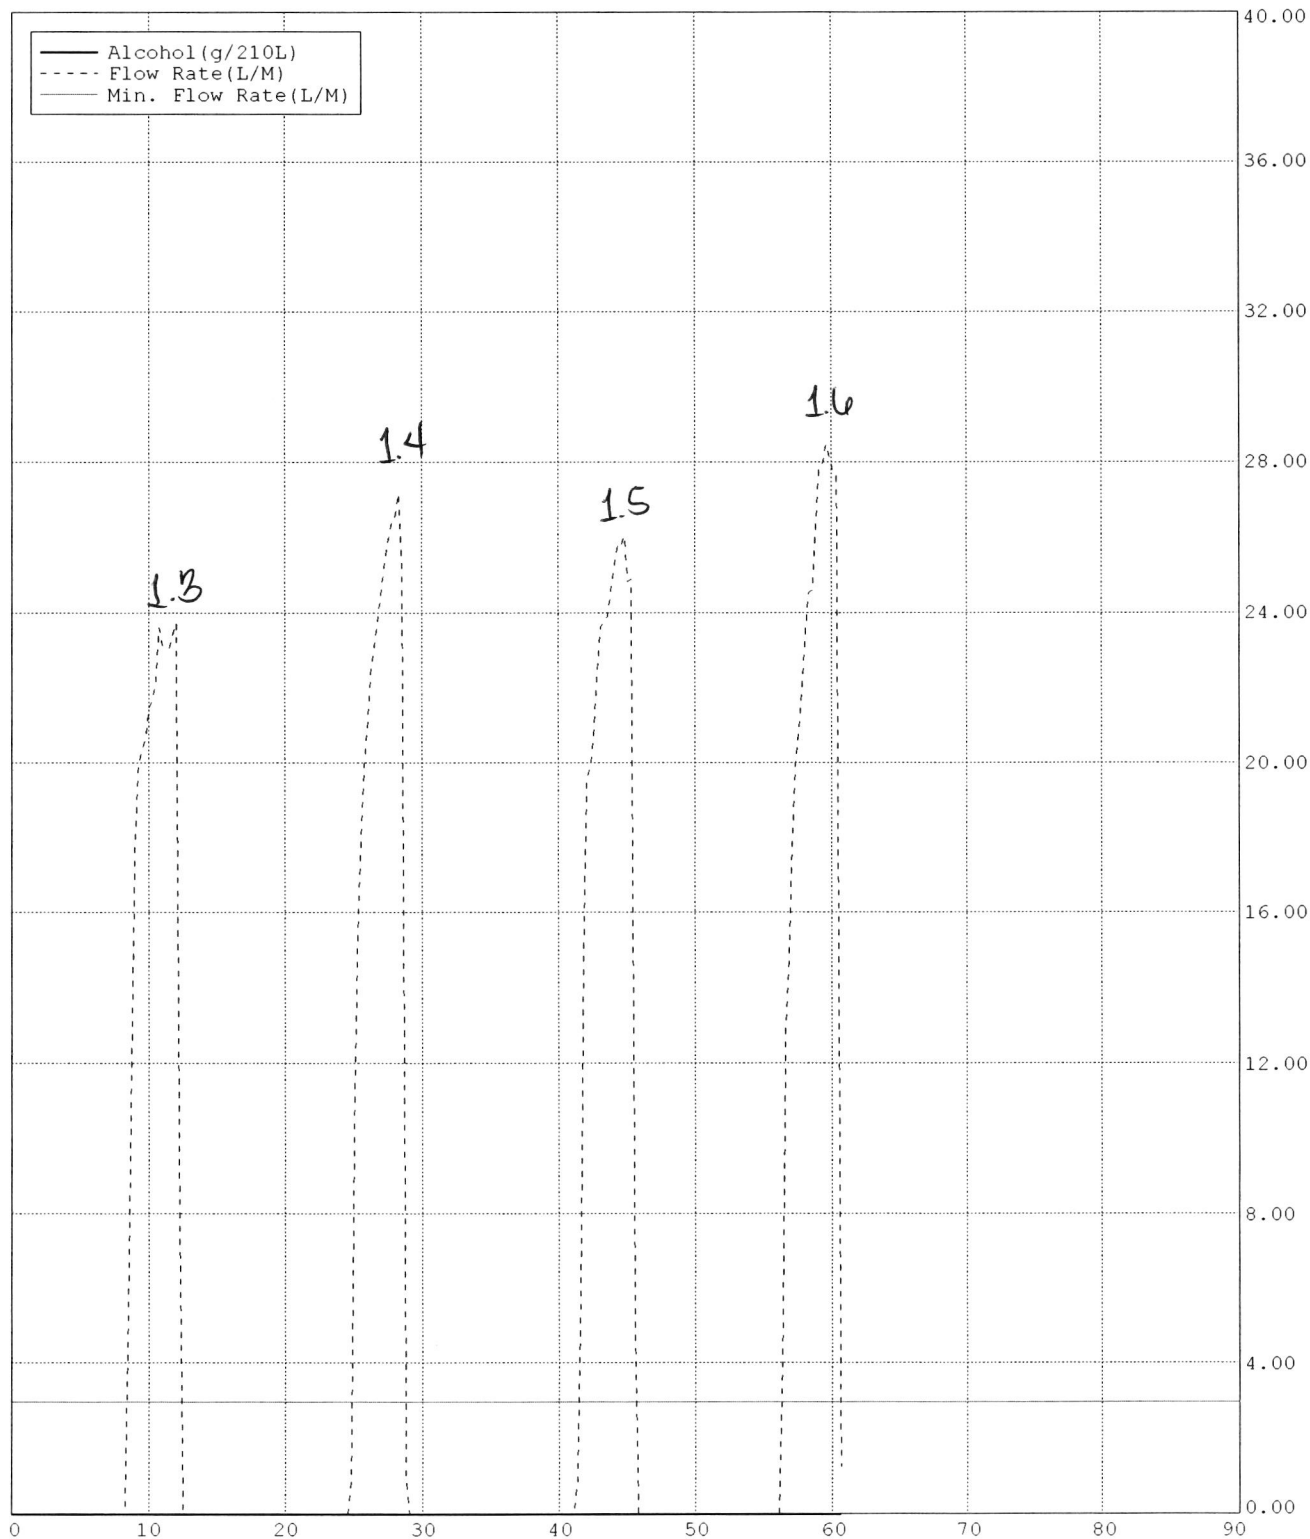

LINEARITY CHECK

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100371  
-----


Date: 04/11/2023  
Time: 08:10:08

SUPERVISOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

TARGET	AVERAGE	STD. DEV.
0.020	0.0194	0.0005
0.040	0.0390	0.0000
0.079	0.0768	0.0004
0.099	0.0970	0.0000
0.149	0.1460	0.0000
0.297	0.2924	0.0005

SLOPE = 0.985946  
R<sup>2</sup> = 0.999991

TM

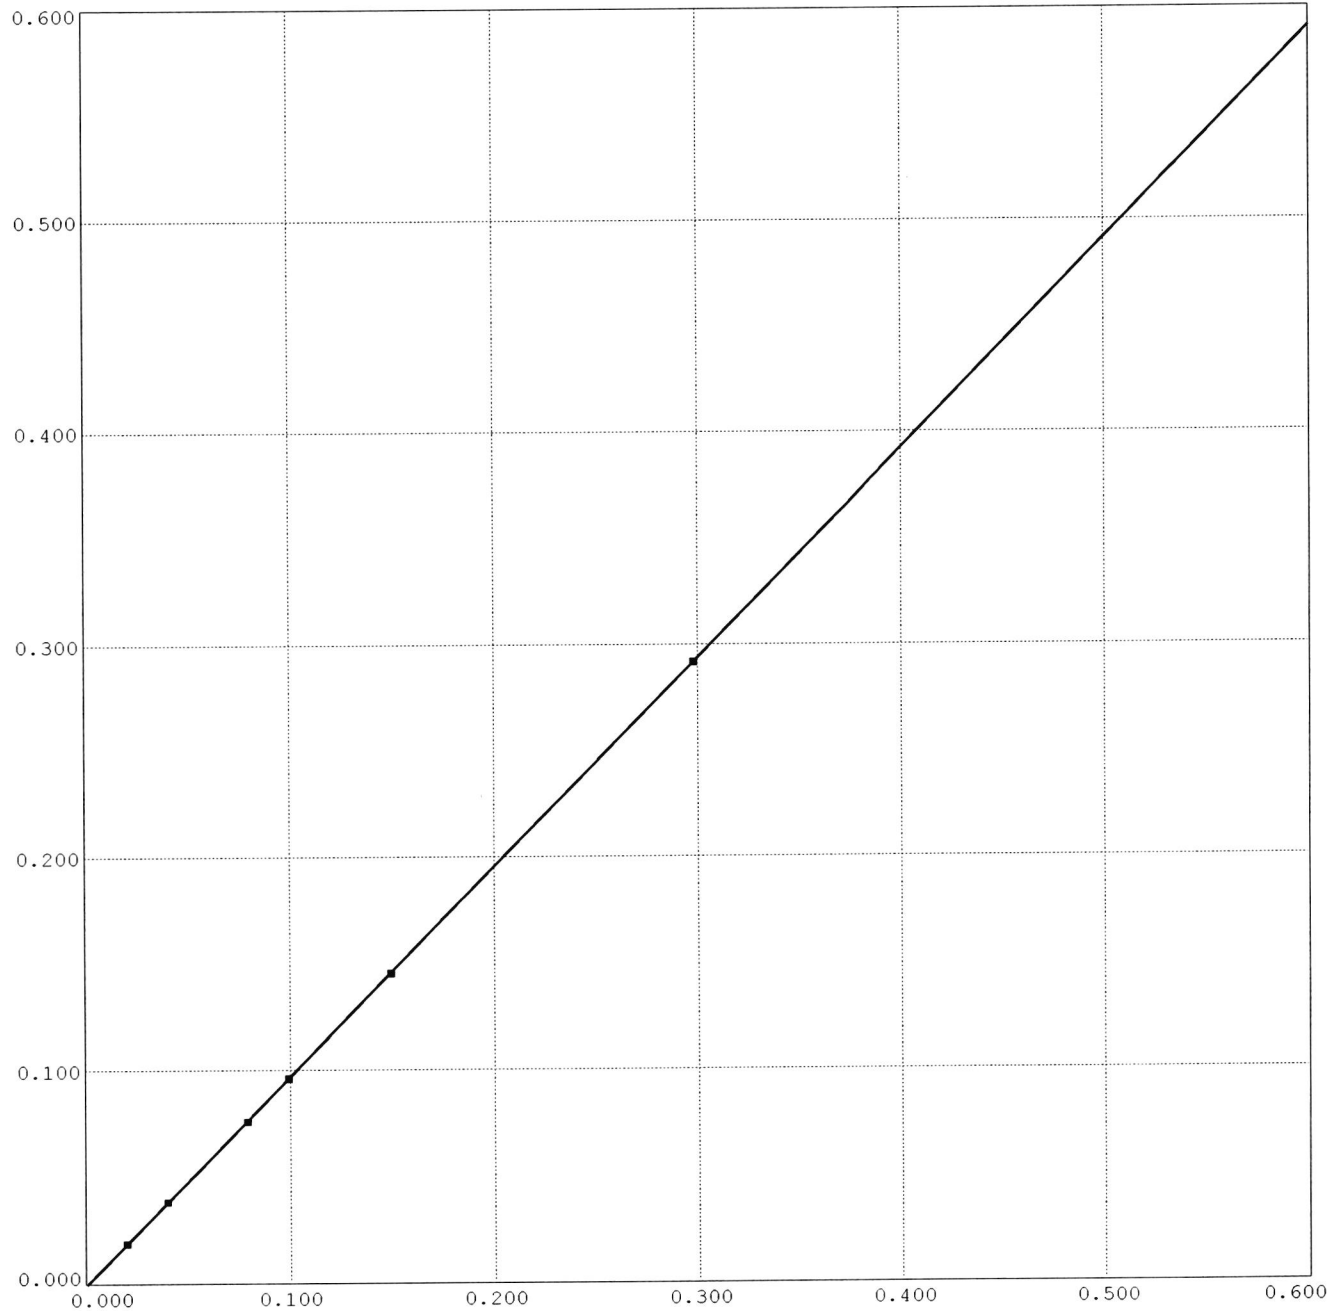

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100371






Date: 04/11/2023  
 Time: 08:10:10

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.65: 0.020  
 LOT #: AG217902  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 922 psi

BLANK TEST	0.000	08:11
INTERNAL STANDARD	VERIFIED	08:11
EXTERNAL STANDARD	0.019	08:11
BLANK TEST	0.000	08:12
EXTERNAL STANDARD	0.019	08:12
BLANK TEST	0.000	08:13
EXTERNAL STANDARD	0.020	08:13
BLANK TEST	0.000	08:14
EXTERNAL STANDARD	0.020	08:15
BLANK TEST	0.000	08:15
EXTERNAL STANDARD	0.019	08:16
BLANK TEST	0.000	08:17

Average = 0.0194  
 Std Dev = 0.0005

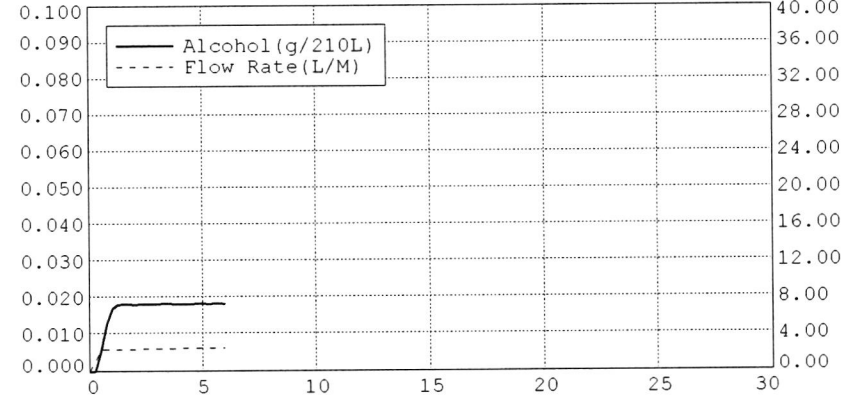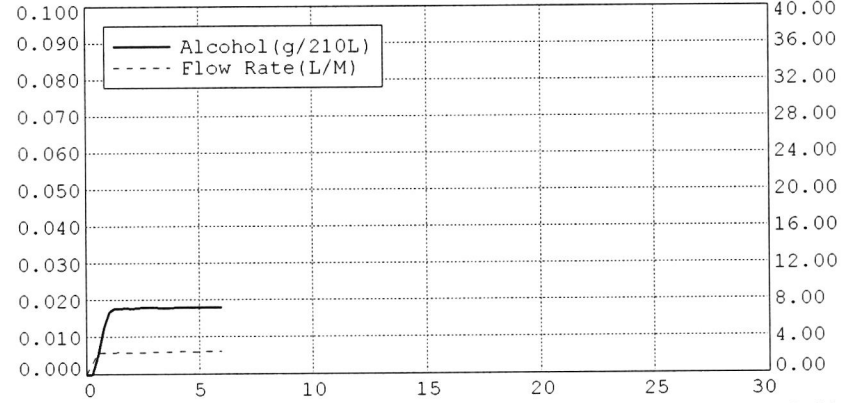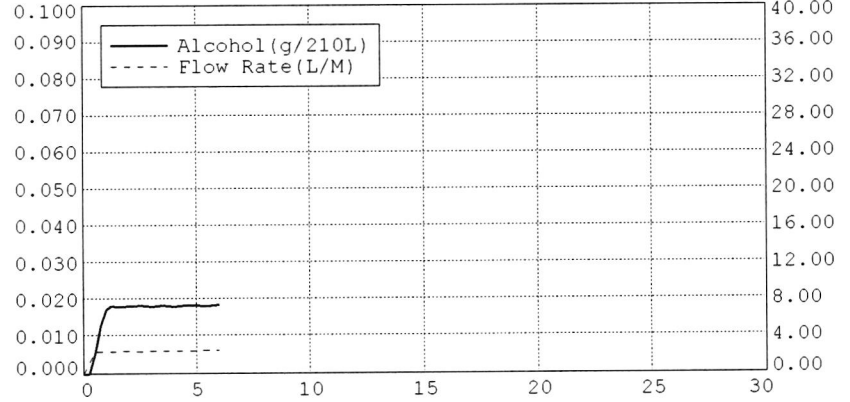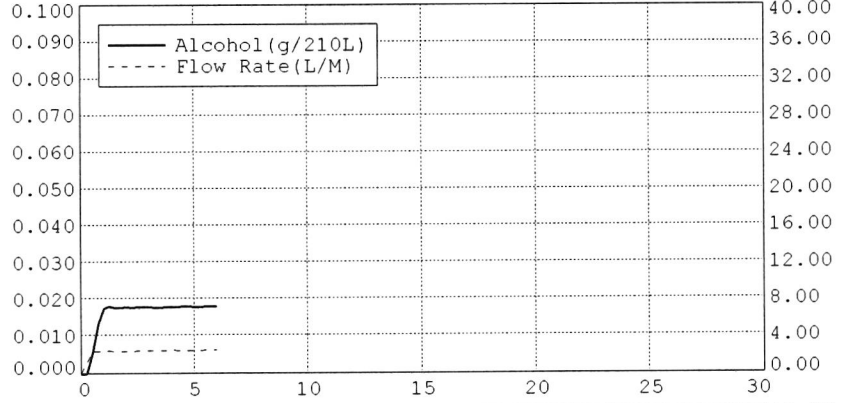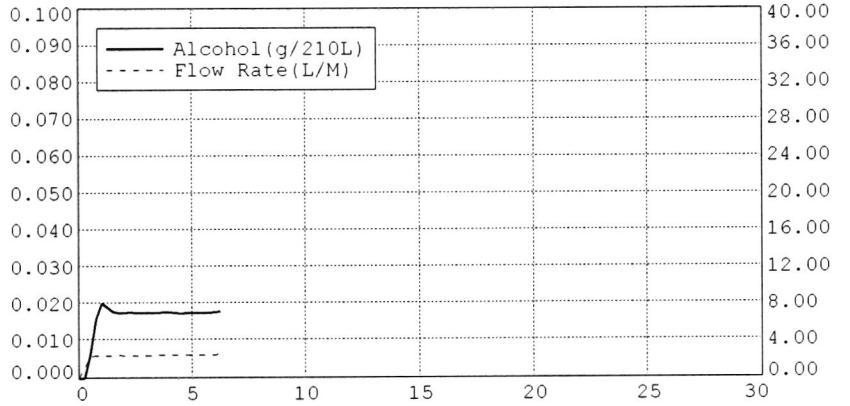

LINEARITY CHECK: Control Test 2






Alaska Department of Public Safety  
DATAMASTER dmt: 100371

Date: 04/11/2023  
Time: 08:17:27

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.040  
TARGET AT 29.65: 0.040  
LOT #: AG217904  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 1003 psi

BLANK TEST	0.000	08:18
INTERNAL STANDARD	VERIFIED	08:18
EXTERNAL STANDARD	0.039	08:19
BLANK TEST	0.000	08:19
EXTERNAL STANDARD	0.039	08:20
BLANK TEST	0.000	08:21
EXTERNAL STANDARD	0.039	08:21
BLANK TEST	0.000	08:22
EXTERNAL STANDARD	0.039	08:22
BLANK TEST	0.000	08:23
EXTERNAL STANDARD	0.039	08:23
BLANK TEST	0.000	08:24

Average = 0.0390  
Std Dev = 0.0000

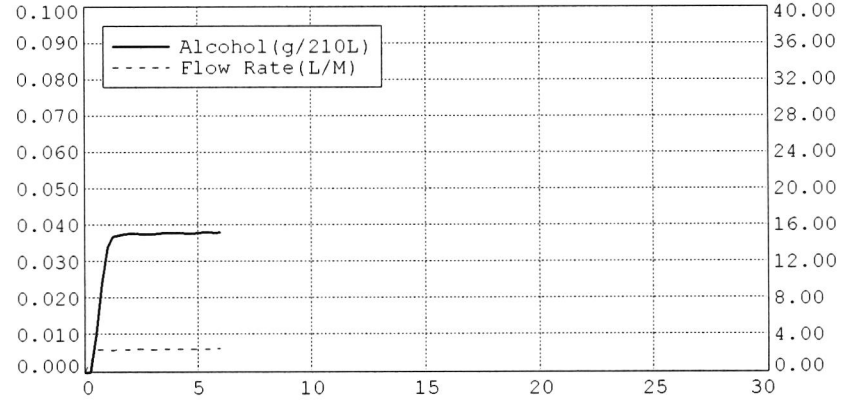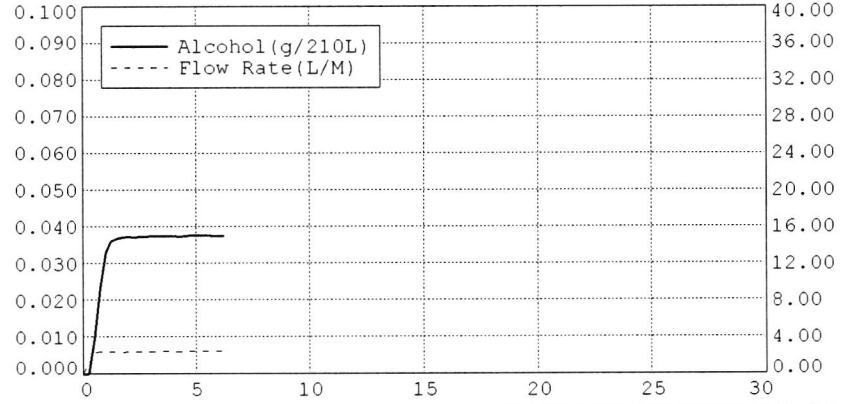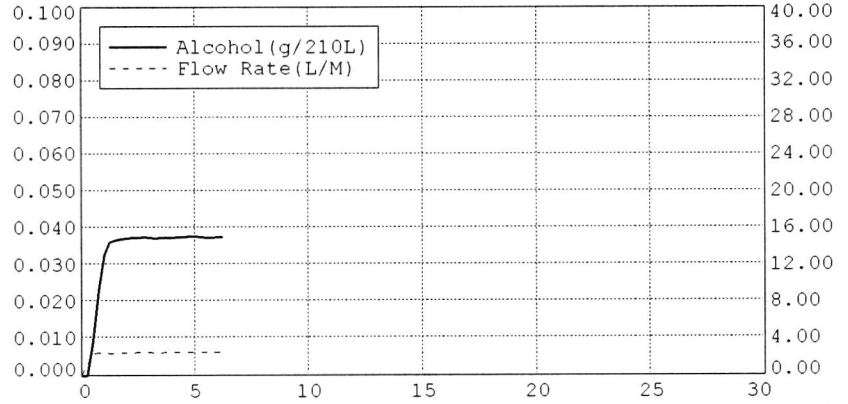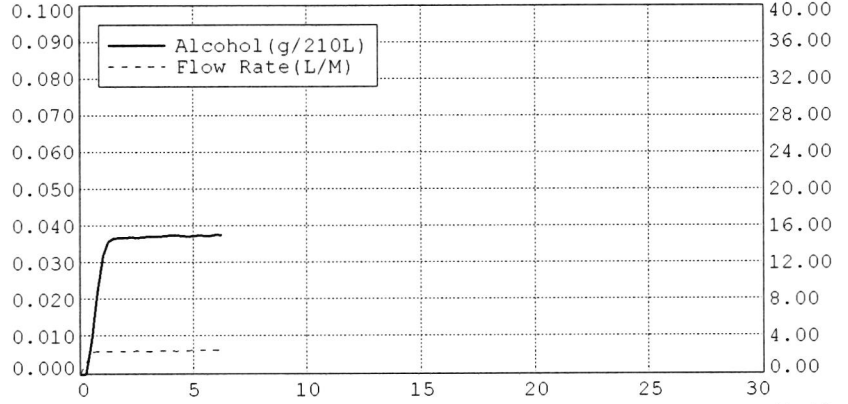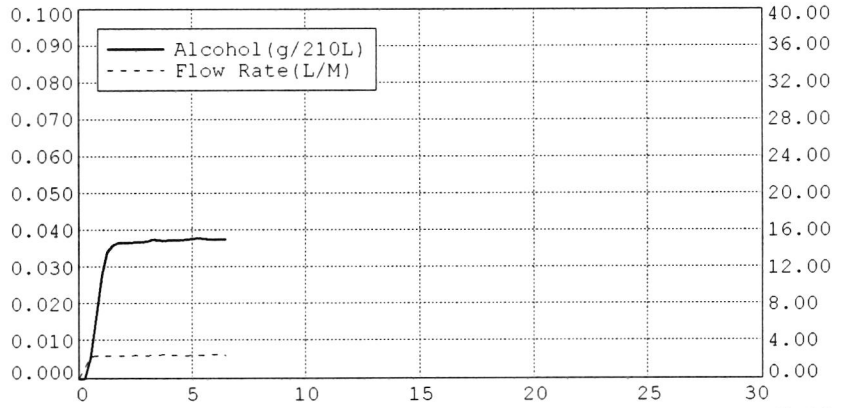

LINEARITY CHECK: Control Test 3






Alaska Department of Public Safety  
 DATAMASTER dmt: 100371

Date: 04/11/2023  
 Time: 08:24:58

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.65: 0.079  
 LOT #: AG113402  
 EXPIRATION: 05/14/2023  
 TANK PRESSURE: 657 psi

BLANK TEST	0.000	08:26
INTERNAL STANDARD	VERIFIED	08:26
EXTERNAL STANDARD	0.077	08:26
BLANK TEST	0.000	08:27
EXTERNAL STANDARD	0.077	08:27
BLANK TEST	0.000	08:28
EXTERNAL STANDARD	0.076	08:28
BLANK TEST	0.000	08:29
EXTERNAL STANDARD	0.077	08:29
BLANK TEST	0.000	08:30
EXTERNAL STANDARD	0.077	08:30
BLANK TEST	0.000	08:31

Average = 0.0768  
 Std Dev = 0.0004

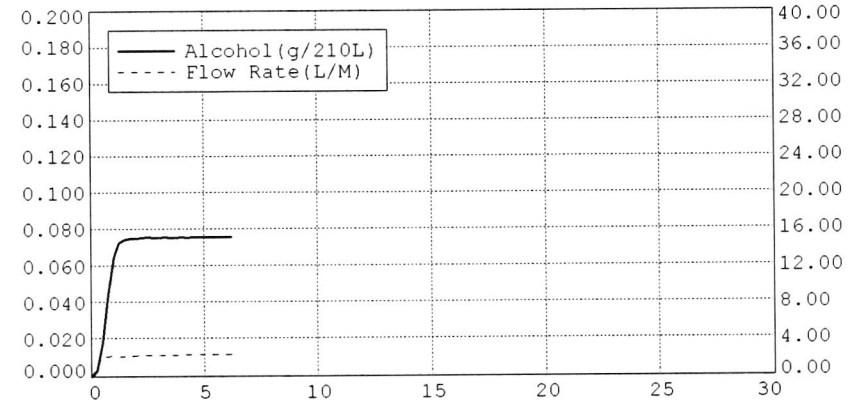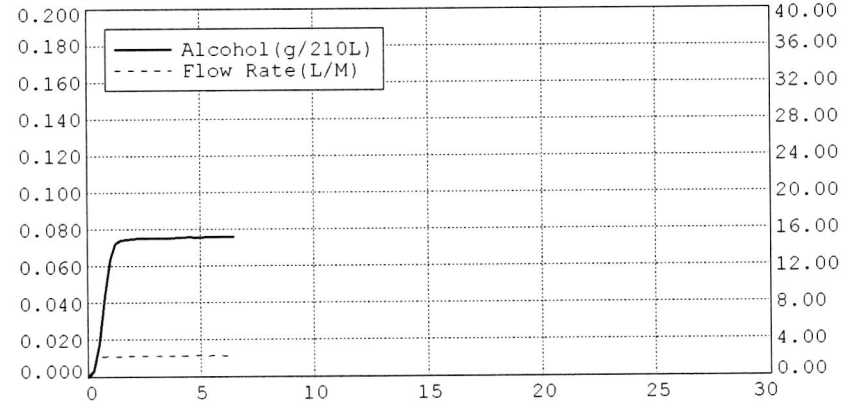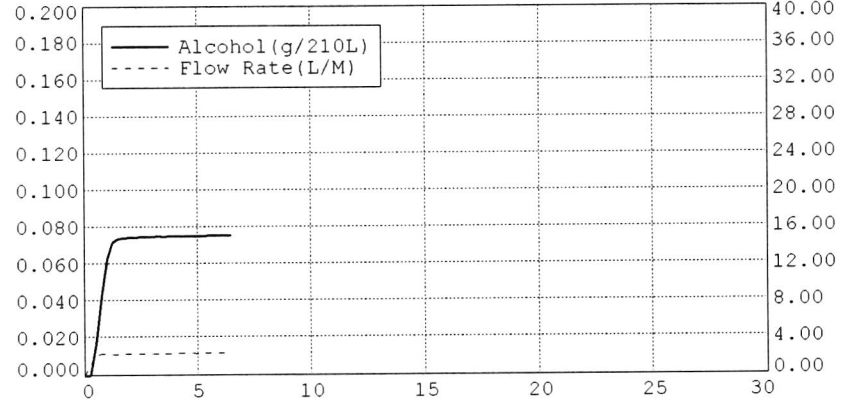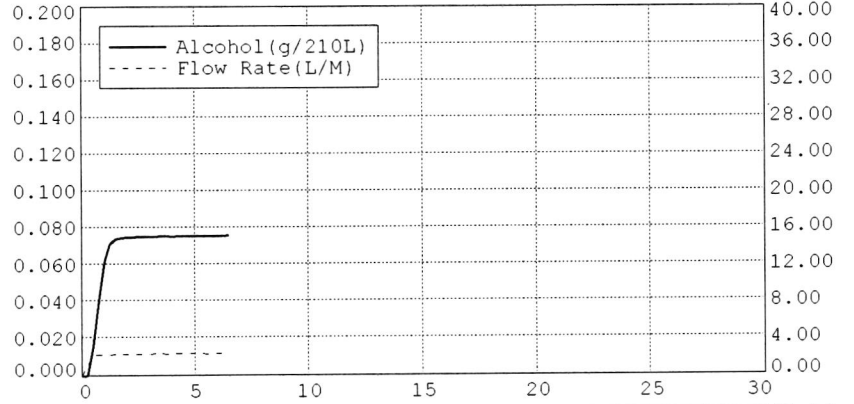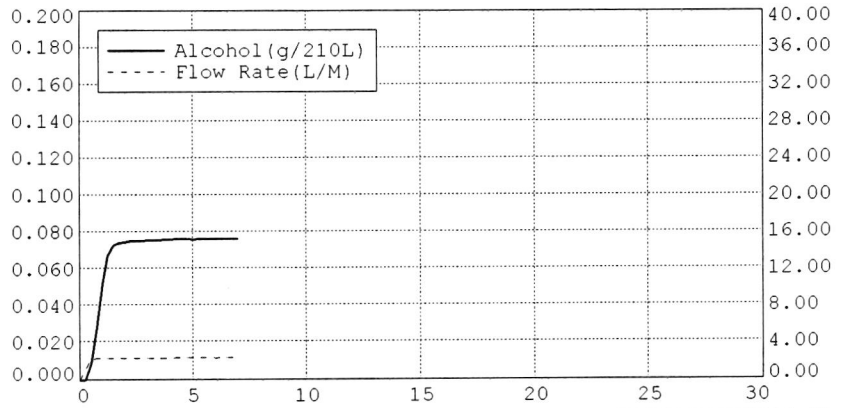



LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
DATAMASTER dmt: 100371






Date: 04/11/2023  
Time: 08:32:48

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
TARGET AT 29.65: 0.099  
LOT #: AG211003  
EXPIRATION: 04/20/2024  
TANK PRESSURE: 978 psi

BLANK TEST	0.000	08:34
INTERNAL STANDARD	VERIFIED	08:34
EXTERNAL STANDARD	0.097	08:34
BLANK TEST	0.000	08:35
EXTERNAL STANDARD	0.097	08:35
BLANK TEST	0.000	08:36
EXTERNAL STANDARD	0.097	08:36
BLANK TEST	0.000	08:37
EXTERNAL STANDARD	0.097	08:37
BLANK TEST	0.000	08:38
EXTERNAL STANDARD	0.097	08:38
BLANK TEST	0.000	08:39

Average = 0.0970  
Std Dev = 0.0000

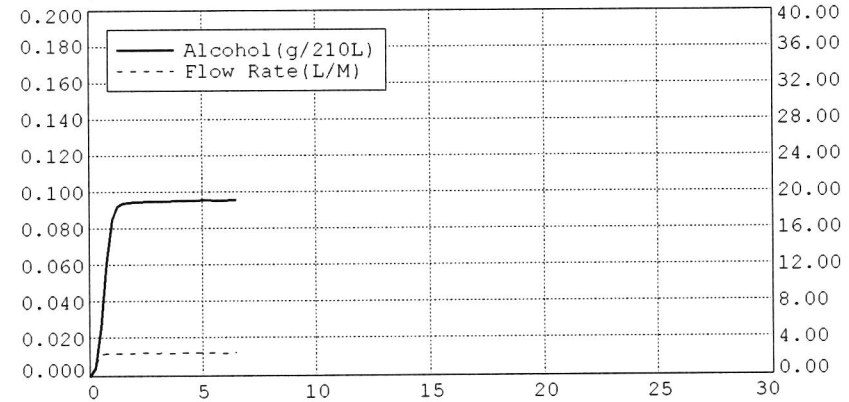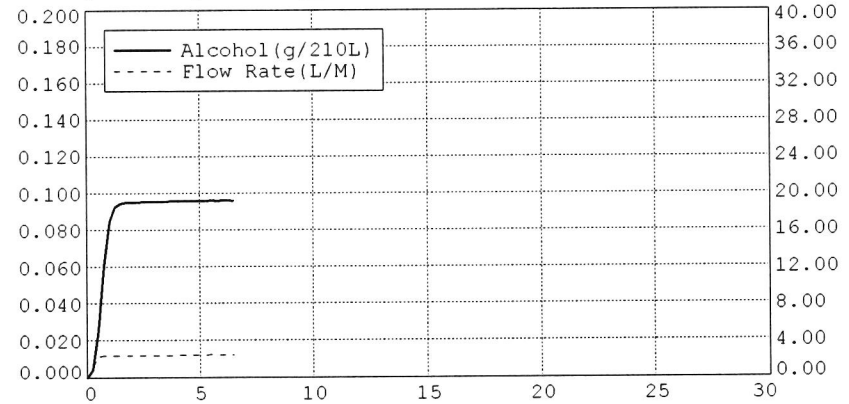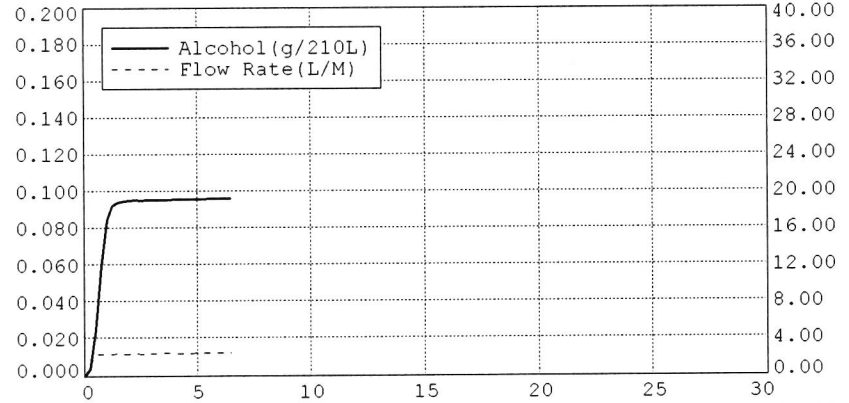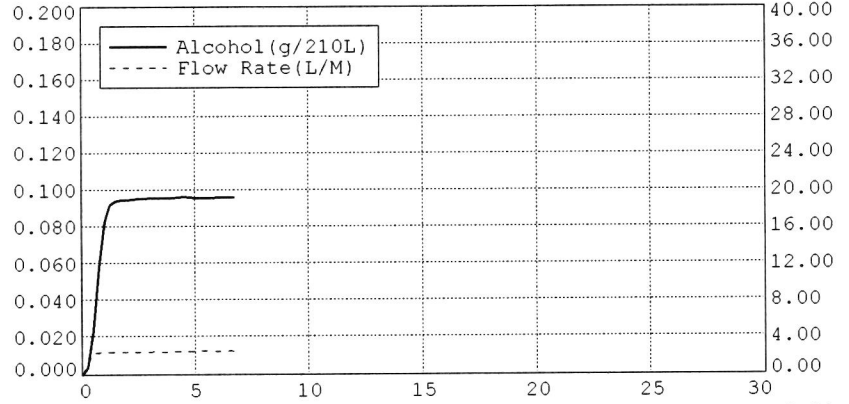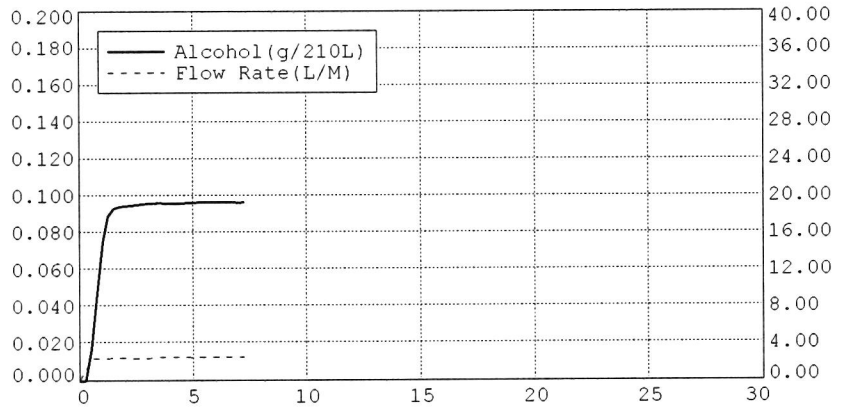

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100371






Date: 04/11/2023  
 Time: 08:40:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.65: 0.149  
 LOT #: AG134205  
 EXPIRATION: 12/08/2023  
 TANK PRESSURE: 975 psi

BLANK TEST	0.000	08:41
INTERNAL STANDARD	VERIFIED	08:41
EXTERNAL STANDARD	0.146	08:41
BLANK TEST	0.000	08:42
EXTERNAL STANDARD	0.146	08:42
BLANK TEST	0.000	08:43
EXTERNAL STANDARD	0.146	08:43
BLANK TEST	0.000	08:44
EXTERNAL STANDARD	0.146	08:45
BLANK TEST	0.000	08:45
EXTERNAL STANDARD	0.146	08:46
BLANK TEST	0.000	08:47

Average = 0.1460  
 Std Dev = 0.0000

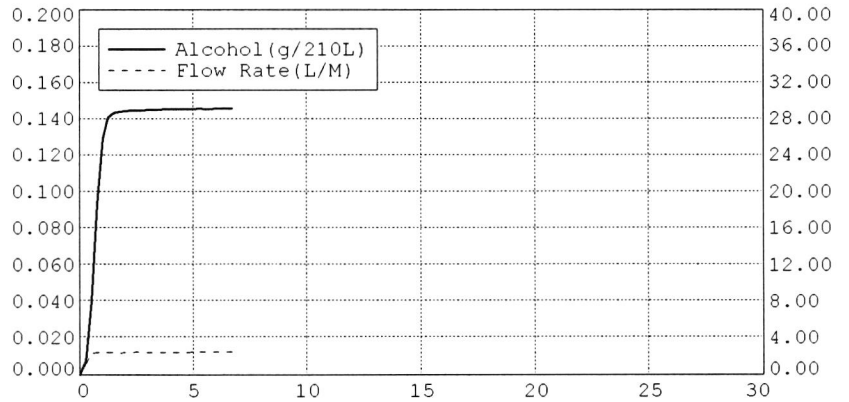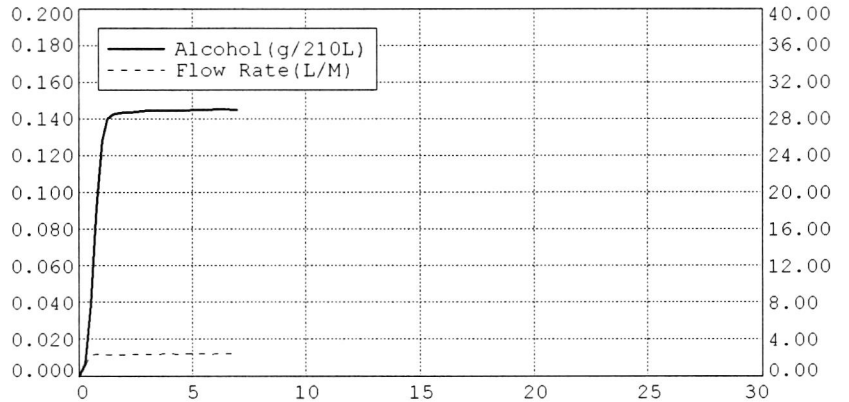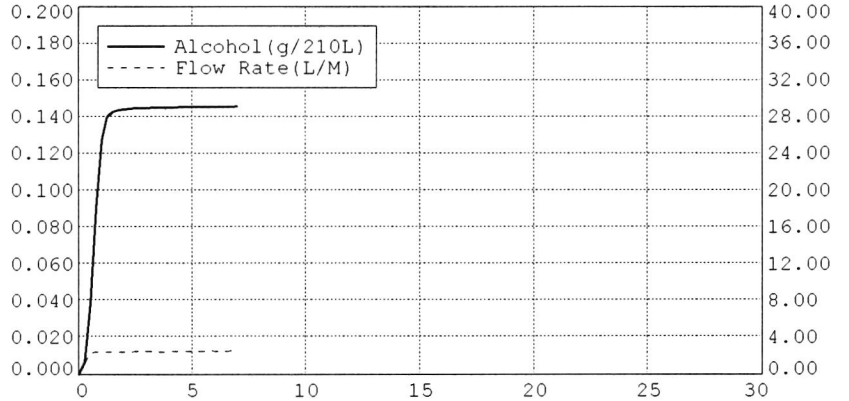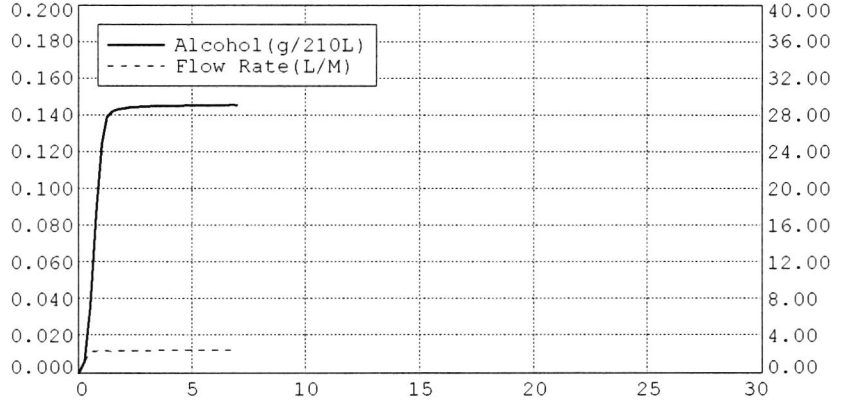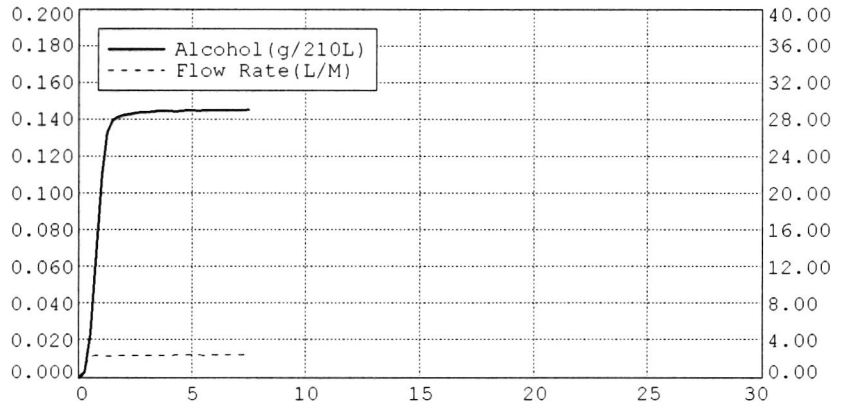

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100371






Date: 04/11/2023  
 Time: 09:08:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.64: 0.297  
 LOT #: AG217903  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 292 psi

BLANK TEST	0.000	09:10
INTERNAL STANDARD	VERIFIED	09:10
EXTERNAL STANDARD	0.292	09:10
BLANK TEST	0.000	09:11
EXTERNAL STANDARD	0.292	09:11
BLANK TEST	0.000	09:12
EXTERNAL STANDARD	0.292	09:12
BLANK TEST	0.000	09:13
EXTERNAL STANDARD	0.293	09:13
BLANK TEST	0.000	09:14
EXTERNAL STANDARD	0.293	09:15
BLANK TEST	0.000	09:15

Average = 0.2924  
 Std Dev = 0.0005

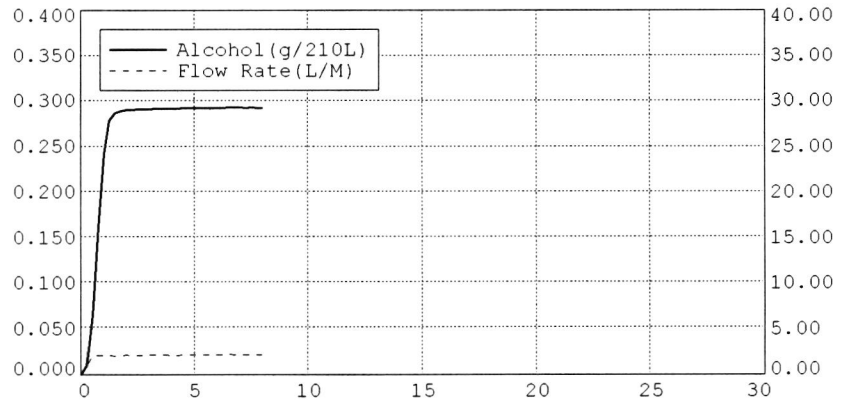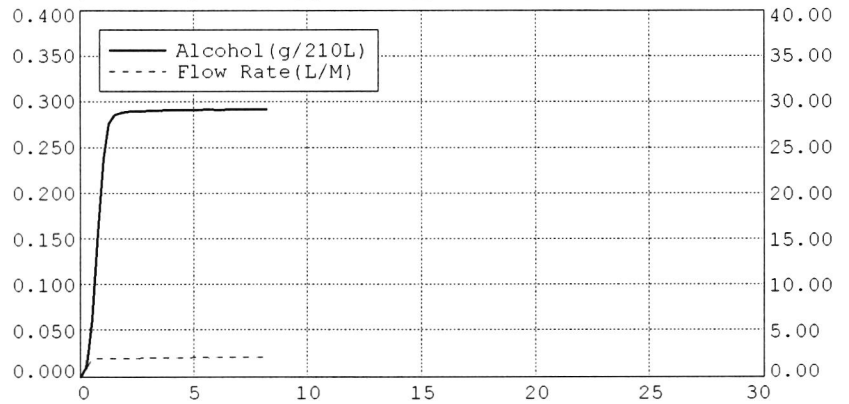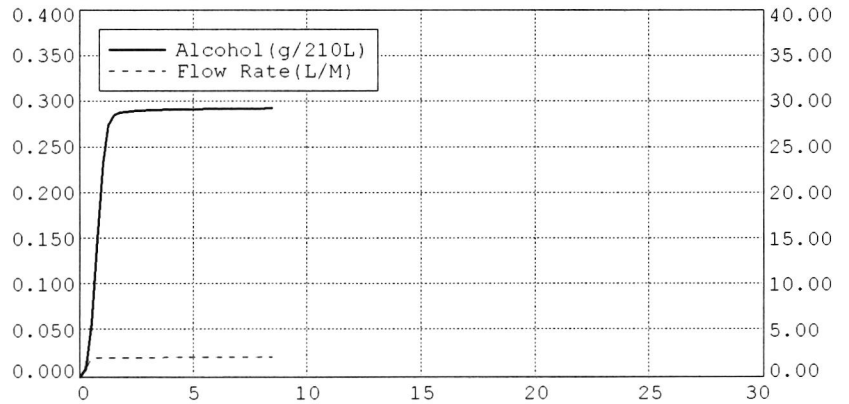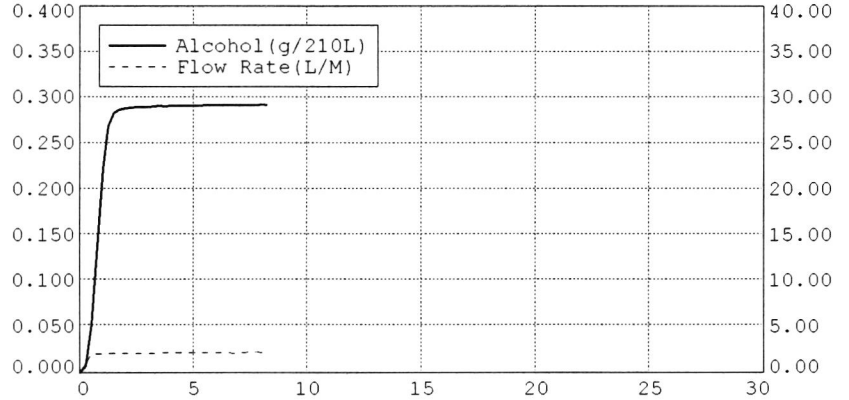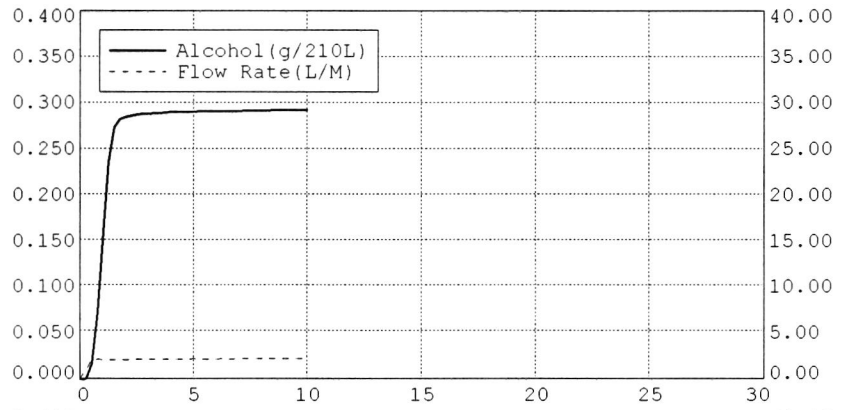

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100371  
-----

Date: 04/11/2023  
Time: 10:03:05

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.64: 0.079  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:04
BLANK TEST	0.000	10:04
INTERNAL STANDARD	VERIFIED	10:04
EXTERNAL STANDARD	0.077	10:04
BLANK TEST	0.000	10:05
SUBJECT SAMPLE	INCOMPLETE	10:07

TMA

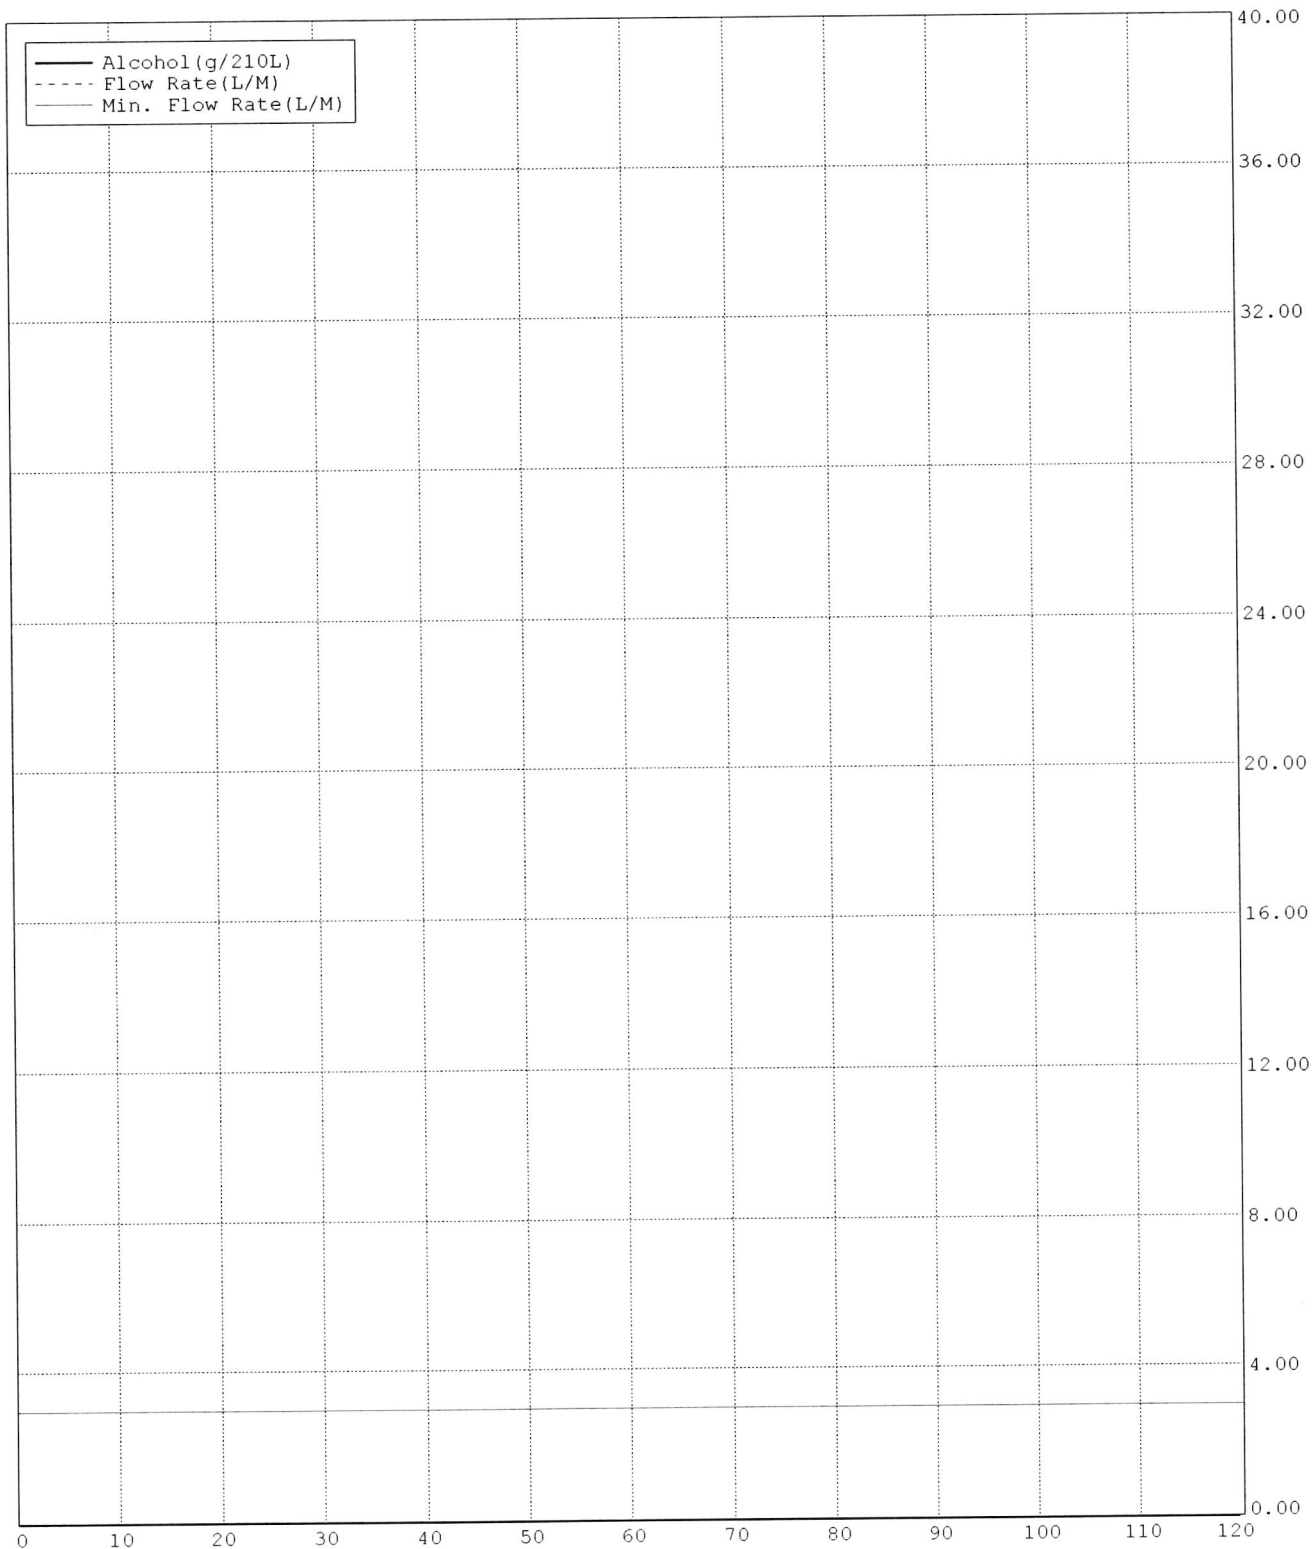

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100371  
-----

Date: 04/11/2023  
Time: 10:18:07

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437


DEPT/AGENCY:  
MAXIMUM ATTEMPTS EXCEEDED  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.64: 0.079  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:19
BLANK TEST	0.000	10:19
INTERNAL STANDARD	VERIFIED	10:19
EXTERNAL STANDARD	0.077	10:19
BLANK TEST	0.000	10:20
SUBJECT SAMPLE	XXX	10:21

Maximum Attempts Exceeded

TLM

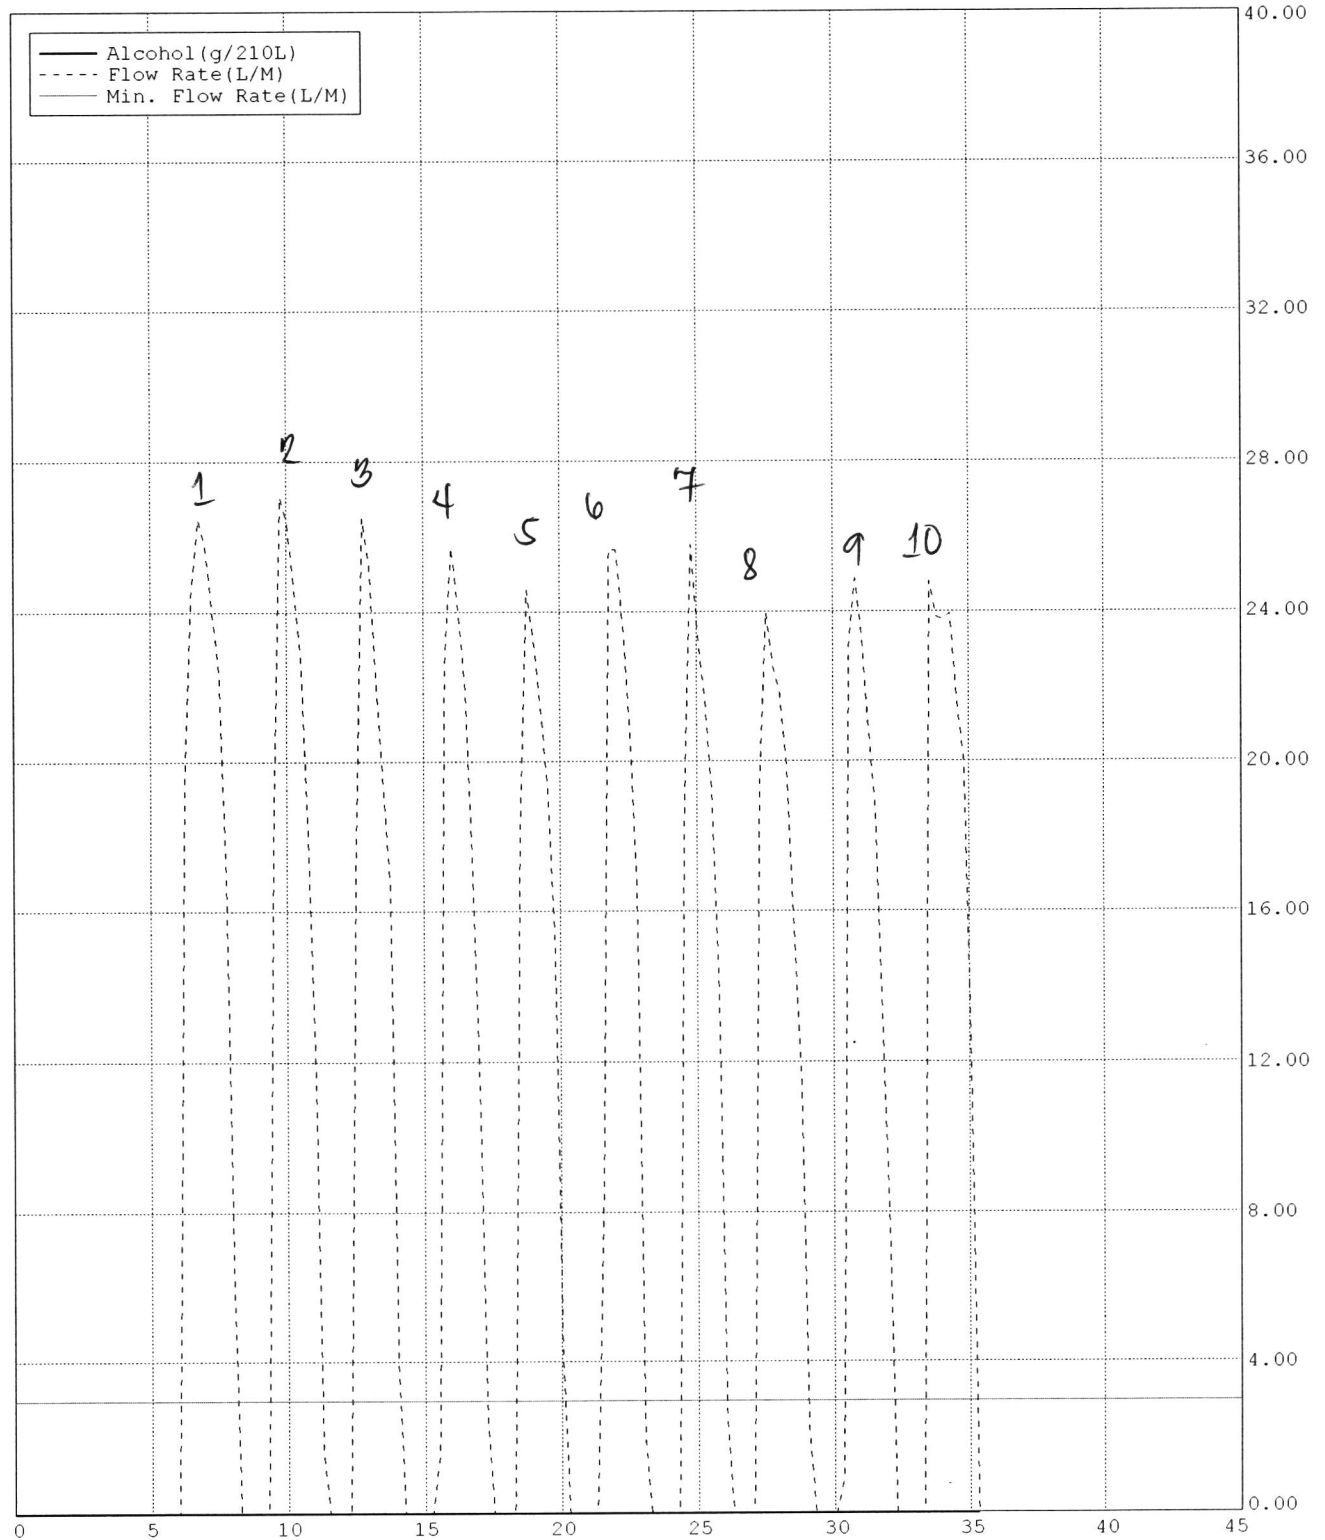

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100371

Date: 04/11/2023  
Time: 10:24:32

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
INVALID  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.65: 0.079  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:25
BLANK TEST	0.000	10:26
INTERNAL STANDARD	VERIFIED	10:26
EXTERNAL STANDARD	0.077	10:26
BLANK TEST	0.000	10:27
SUBJECT SAMPLE	INVALID	10:27

*tm*

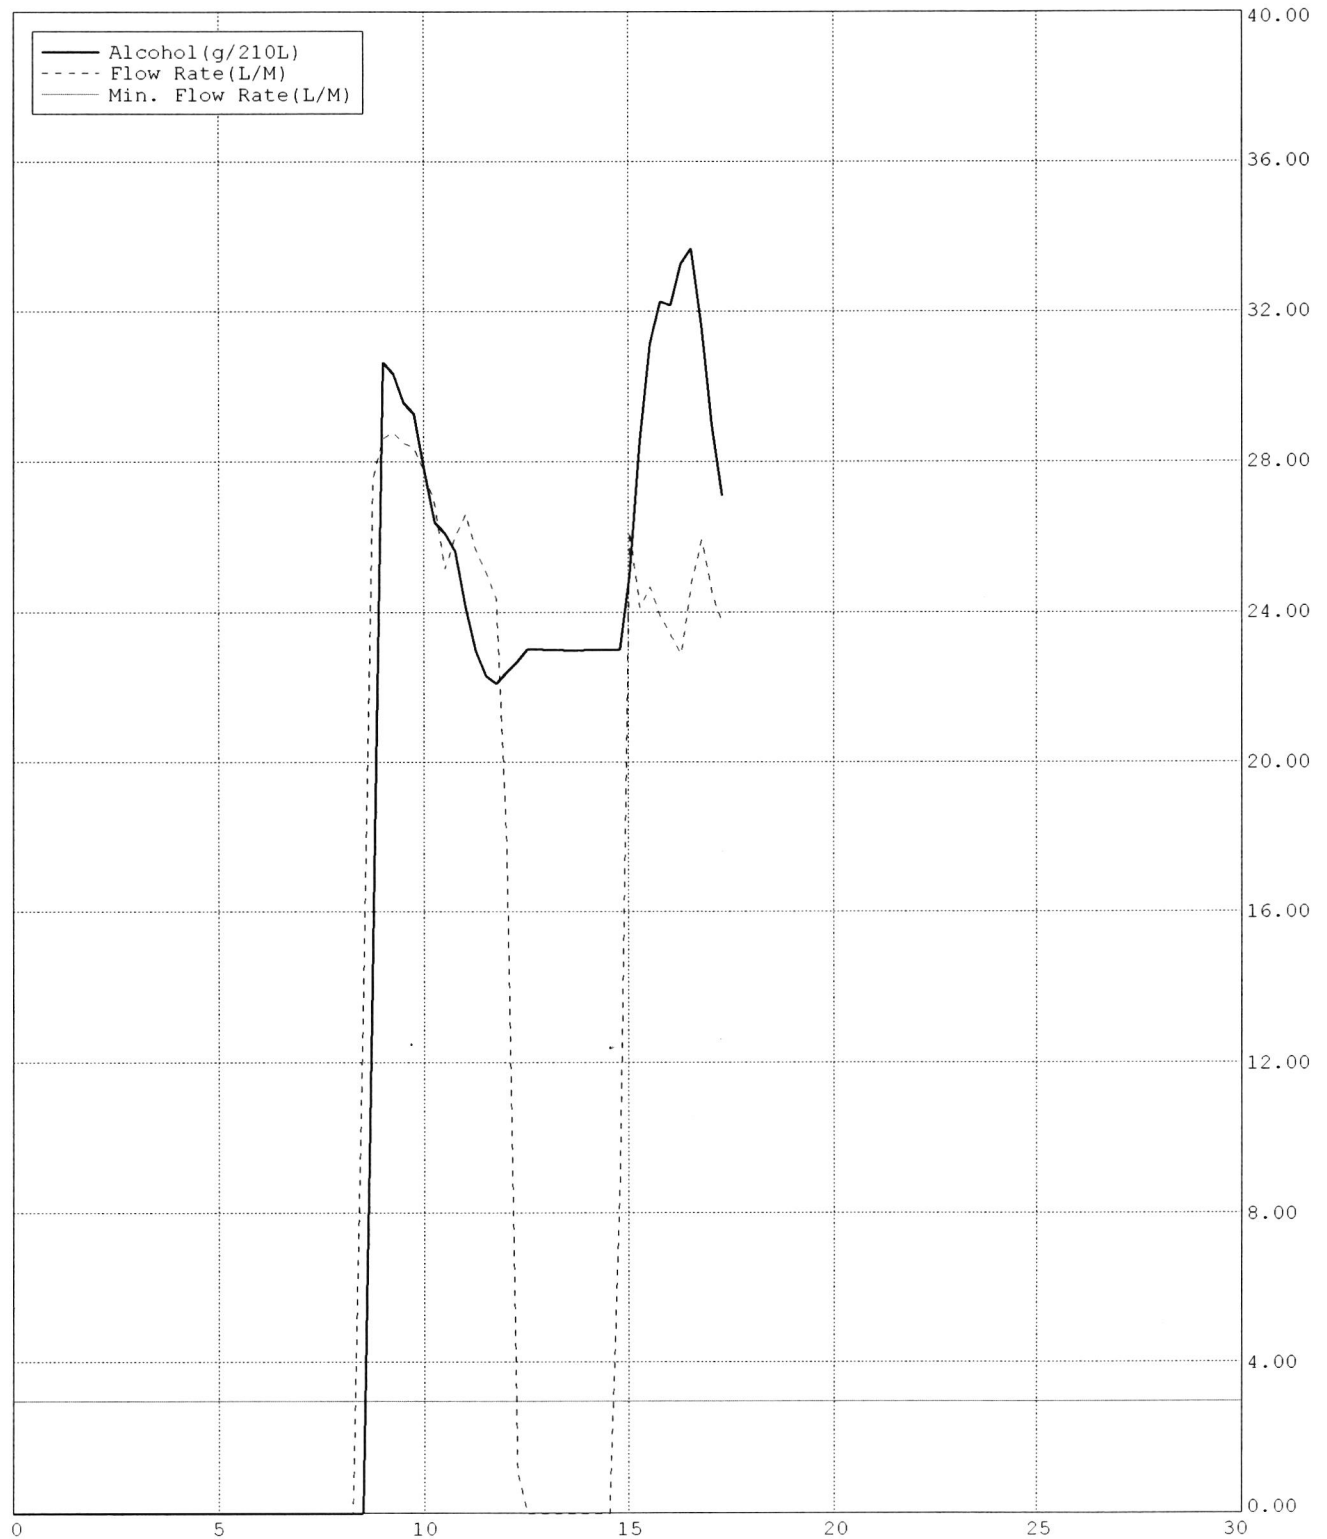



SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100371  
-----

Date: 04/11/2023  
Time: 10:49:50

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437


DEPT/AGENCY:  
RADIO FREQUENCY INTERFERENCE (RFI)  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.65: 0.079  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:51
BLANK TEST	0.000	10:51
INTERNAL STANDARD	VERIFIED	10:51
EXTERNAL STANDARD	0.077	10:51
BLANK TEST	0.000	10:52

RFI DETECTED

TMM

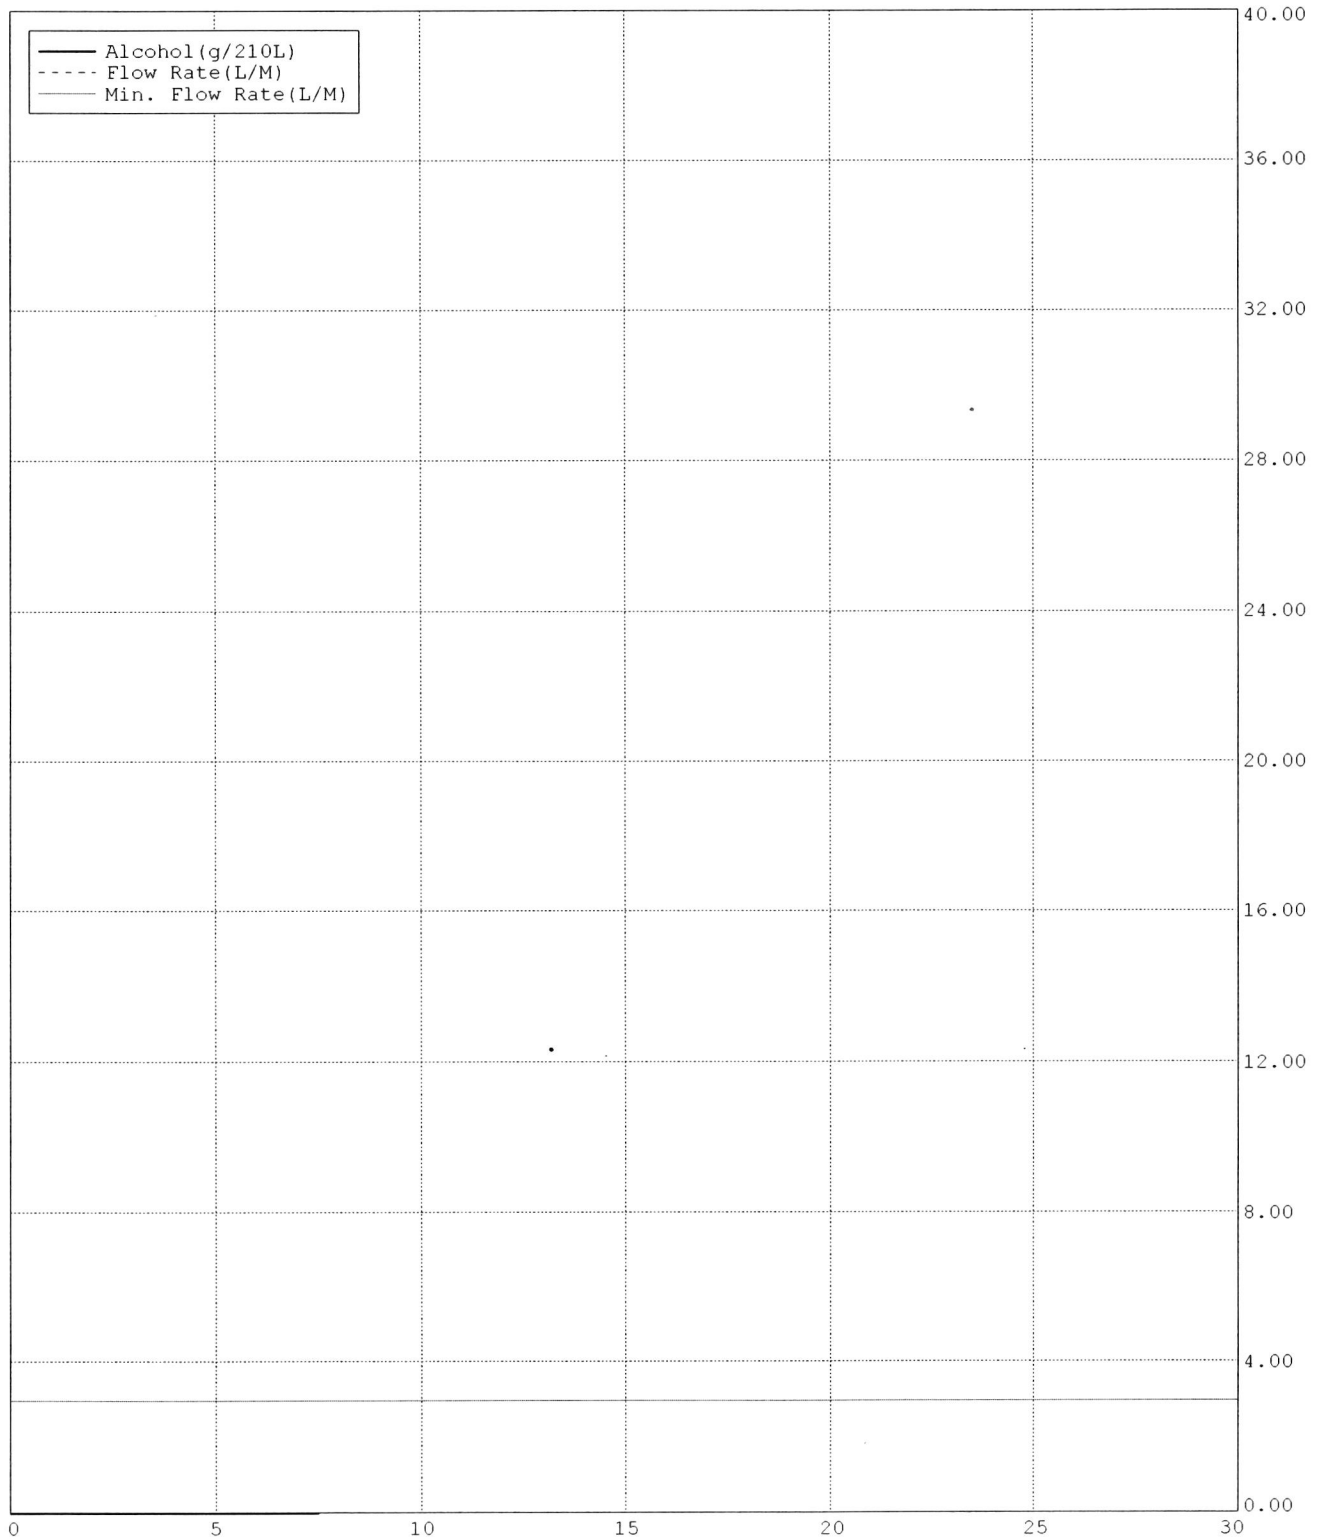

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100371

Date: 04/11/2023  
Time: 09:31:21

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
INTERFERENCE DETECTED - ACETONE  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.65: 0.079  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:32
BLANK TEST	0.000	09:32
INTERNAL STANDARD	VERIFIED	09:32
Xq = 0.082 (1.73%)		
EXTERNAL STANDARD	0.078	09:32
X[1] = 0.0776 (-0.0009) (0.0036)		
BLANK TEST	0.000	09:33
SUBJECT SAMPLE	XXX	09:34
X[1] = 0.1054 (-0.0147) (0.0029)		

Interference Detected

Filter 2 Average: -0.0011  
Filter 3 Average: 0.0029

TMM

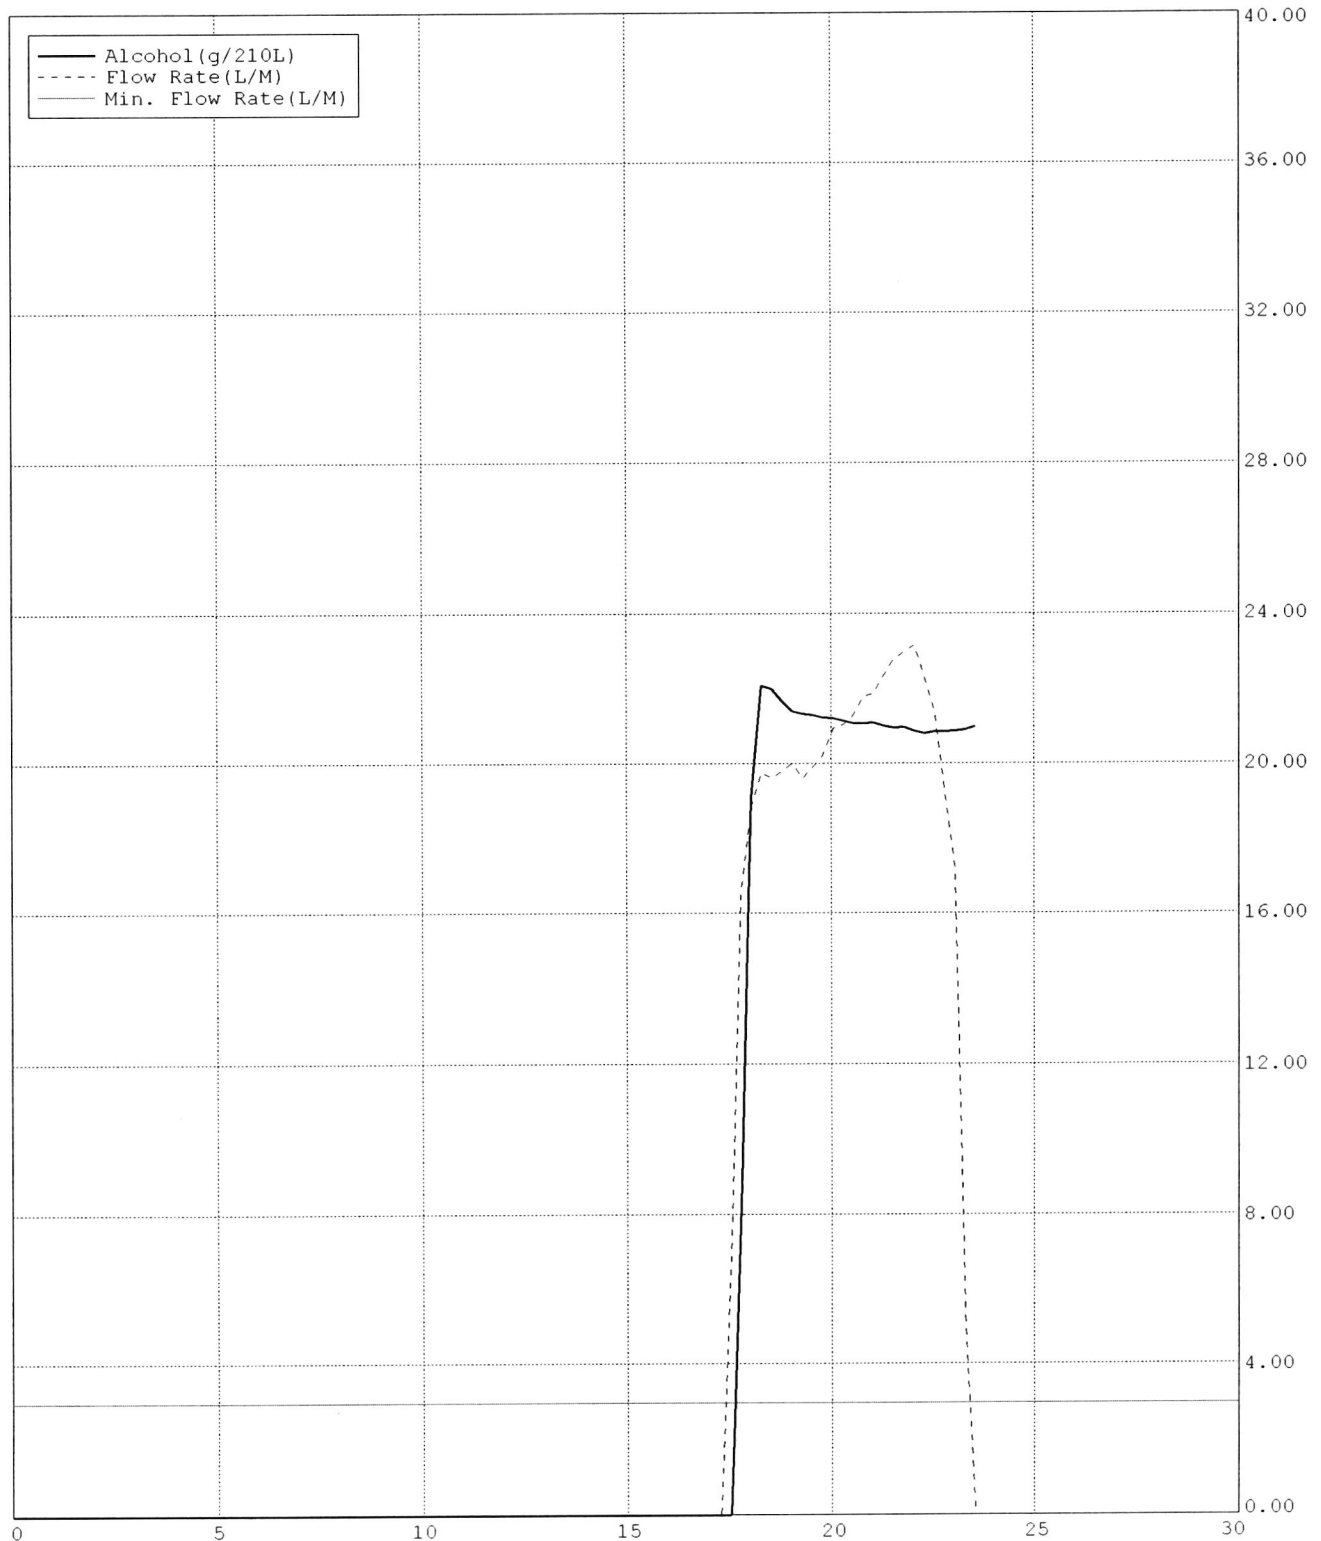

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100371

Date: 04/11/2023  
Time: 09:37:39

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437


DEPT/AGENCY:  
INTERFERENCE DETECTED - ISOPROPANOL  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.65: 0.079  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:38
BLANK TEST	0.000	09:38
INTERNAL STANDARD	VERIFIED	09:38
Xq = 0.082 (1.73%)		
EXTERNAL STANDARD	0.077	09:39
X[1] = 0.0771 (-0.0014) (0.0029)		
BLANK TEST	0.000	09:40
SUBJECT SAMPLE	XXX	09:40
X[1] = 0.1130 (-0.0273) (0.0023)		

Interference Detected

TML

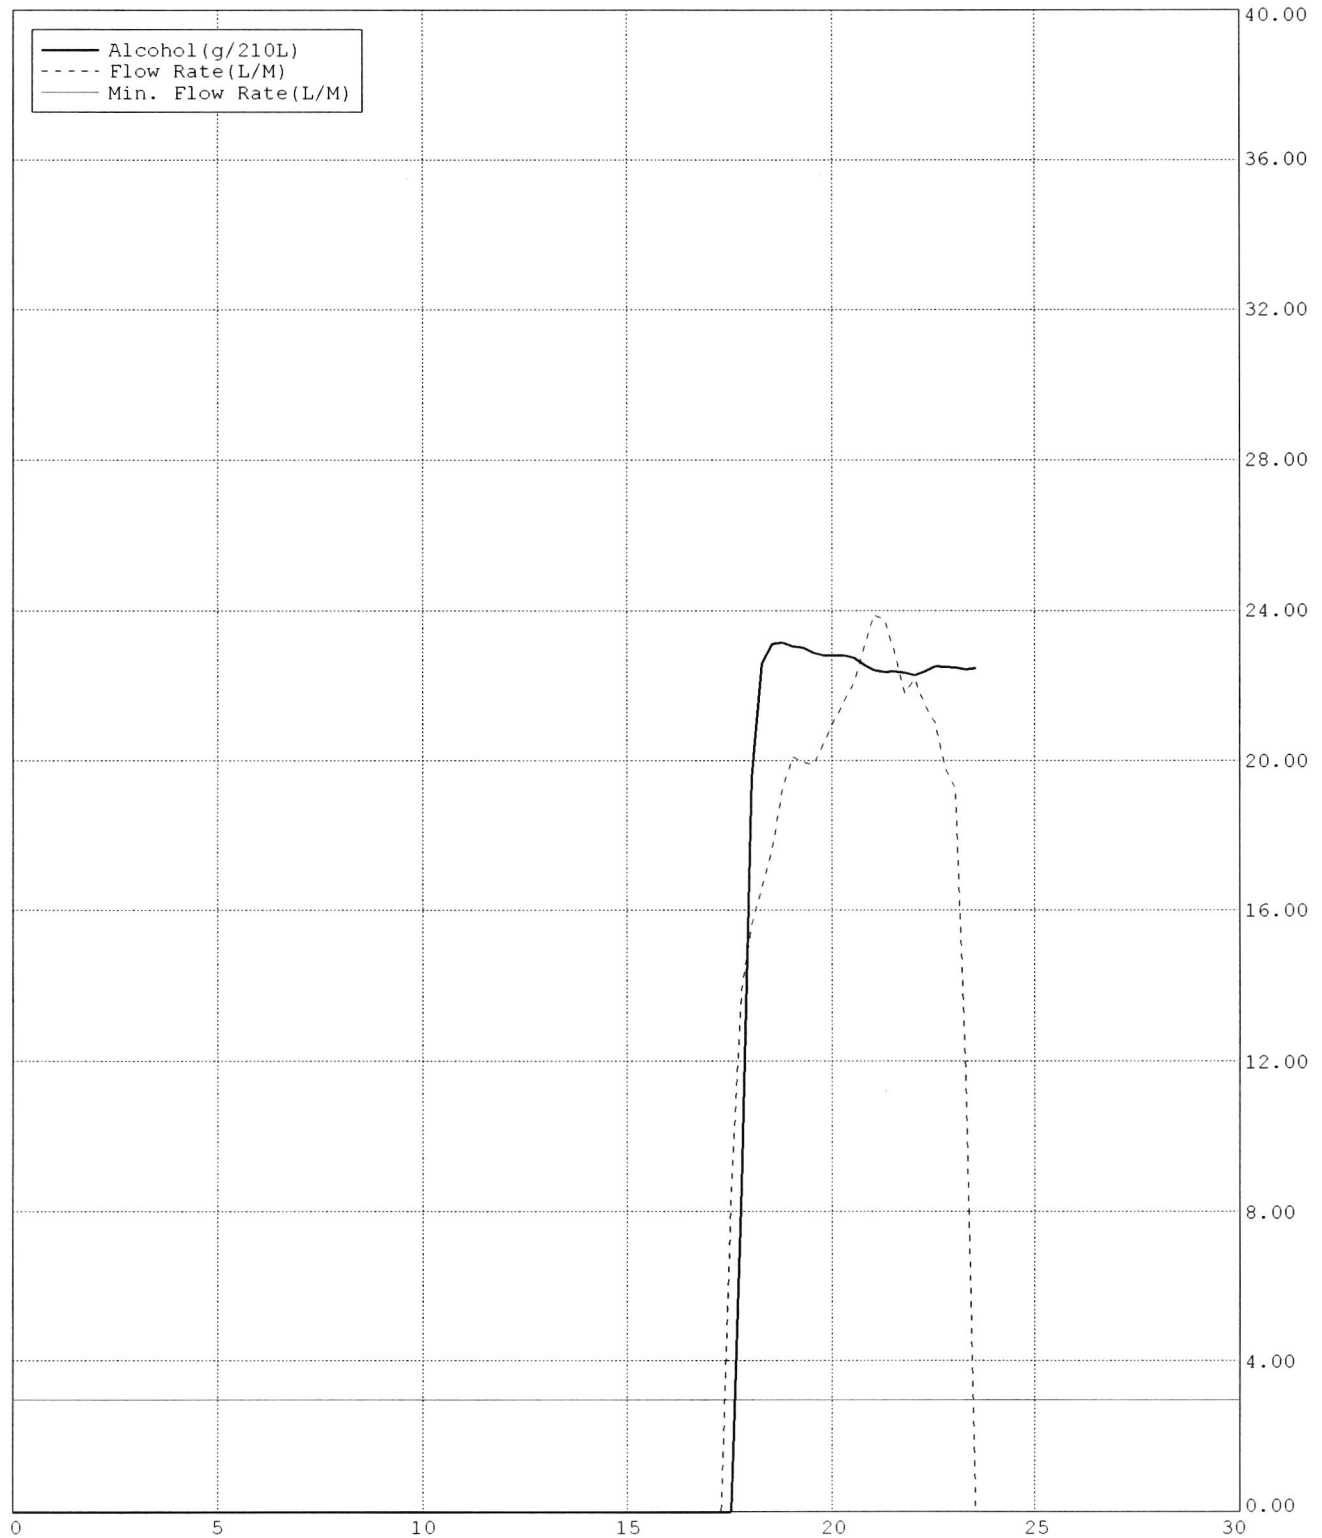

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100371

Date: 04/11/2023  
Time: 09:42:33

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
INTERFERENCE DETECTED - NEGATIVE CONTROL  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.64: 0.079  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:43
BLANK TEST	0.000	09:43
INTERNAL STANDARD	VERIFIED	09:43
Xq = 0.081 (0.97%)		
EXTERNAL STANDARD	0.077	09:43
X[1] = 0.0770 (-0.0015) (0.0027)		
BLANK TEST	0.000	09:44
SUBJECT SAMPLE (Vol=1.82L)	0.090	09:45
X[1] = 0.0907 (-0.0012) (0.0019)		
BLANK TEST	0.000	09:46
EXTERNAL STANDARD	0.077	09:46
X[1] = 0.0770 (-0.0006) (0.0023)		
BLANK TEST	0.000	09:47

*TJM*

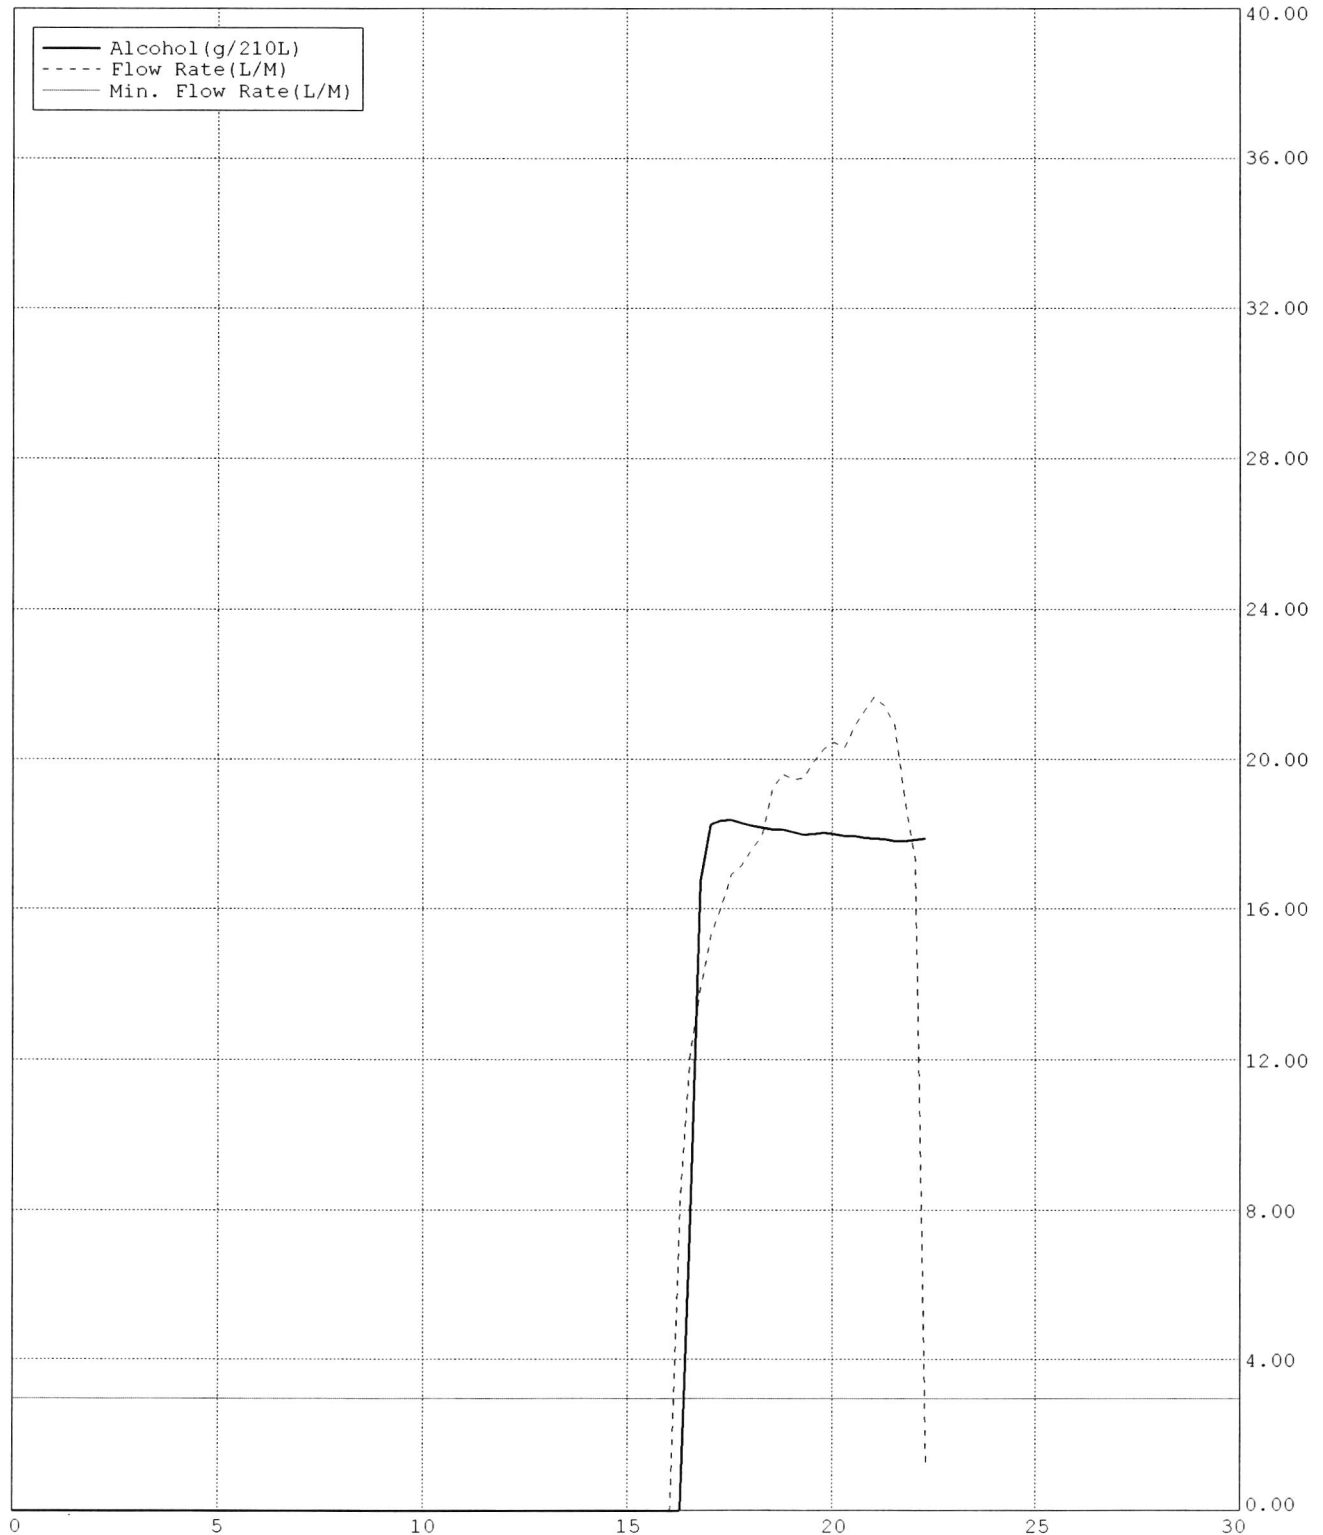

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100371  
-----

Date: 04/11/2023  
Time: 11:21:42

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
TATIANA MALNOSKE  
OPERATOR'S #: 10437

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.67: 0.079  
LOT #: AG113402  
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	11:22
BLANK TEST	0.000	11:22
INTERNAL STANDARD	VERIFIED	11:22
EXTERNAL STANDARD	0.078	11:23
BLANK TEST	0.000	11:24
SUBJECT SAMPLE (Vol=1.82L)	0.000	11:24
BLANK TEST	0.000	11:25
EXTERNAL STANDARD	0.077	11:25
BLANK TEST	0.000	11:26

*Tm*

