



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100367

**Report Issue Date:** 03/28/2024  
**Date Received:** 2023-12-20  
**Condition of Item:** Good

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 12/20/2023** - As Found - **End Date 12/21/2023** As Found - Evaluation Analyst: Colleen O'Bryant  
 As Found Conditions - Barometric Pressure (inHg): 29.01 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.0  
 Relative Humidity (%): 16

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.019	AG217902	0.020	0.020	0.019	0.020	0.020	0.020	0.020
0.080	0.078	09523080A1	0.078	0.078	0.078	0.078	0.078	0.078	0.078
0.300	0.291	AG327804	0.294	0.294	0.293	0.293	0.293	0.293	0.293

Internal standard errors in the field were at ~4.5%. One internal standard error during linearity.

**Start Date 02/23/2024** - As Left - **End Date 02/26/2024**

As Left Conditions - Barometric Pressure (inHg): 29.22 Barometer Used: Fisher S/N 230307229 Temperature (C): 23.6 Relative Humidity (%): 19

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.021	0.020	0.020	0.020	0.021	0.020	+/- 0.002
0.040	0.039	AG217904	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.078	09523080A1	0.080	0.079	0.079	0.079	0.079	0.079	+/- 0.004
0.100	0.098	AG211003	0.100	0.099	0.099	0.100	0.100	0.100	+/- 0.004
0.150	0.146	AG332004	0.147	0.147	0.147	0.147	0.147	0.147	+/- 0.005
0.300	0.293	AG327804	0.297	0.296	0.297	0.297	0.297	0.297	+/- 0.011

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Carlie Glaister on 03/28/2024

[carlie.glaister@alaska.gov](mailto:carlie.glaister@alaska.gov)

Technically and administratively reviewed by Colleen O'Bryant on 03/28/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100367 Analyst or Technician Name: Carlisle Glaister

DataMaster DMT Calibration Start Date: 2/23/24

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 230307229  
Calibration Due Date: 5/2/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.22 Temperature(C) 23.4 Relative Humidity(%) 19

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20240214COB Expiration Date: 5/14/24  
Simulator S/N: 501088 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: ~~DE 20240214COB~~ Expiration Date: 5/14/24  
Simulator S/N: DR4161 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 22HP41201 Expiration Date: 8/24/24  
Simulator S/N: 501177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 9/19/25

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 2/23/24

Data Interpretation Date (Technician): \_\_\_\_\_ (if applicable)

Data Interpretation Date (Analyst): 2/26/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100367  
-----

Date: 02/23/2024  
Time: 08:46:57

VERSIONS  
DMT: 3.02  
PIC: 3.06  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 48.1°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.59 V PASSED  
(0.95 V - 2.23 V)  
Cooler Voltage = 1.56 V PASSED  
(0.93 V - 2.17 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 529 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.655 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

PASSED  
Xq = 0.084 0.51% (0.00% - 4.00%)

Technician Screen

-----  
DATAMASTER dmt: 100367  
-----

Date: 02/23/2024  
Time: 9:06 AM

Temperatures (°C)

Sample Cell: 48.7°C  
Breath Tube: 47.7°C

Current Barometer 29.2 in  
Volume (Ltr) 1.51

Settings

Lamp: 1.59 V  
Bias: 80 V  
Cooler: 1.56 V  
Chopper: 529 Hz

Voltages (V)

Flow: 1.02 V  
Detector: 0.074 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100367  
-----

Date: 01/11/2024  
Time: 11:10:43

OPERATOR NAME:  
CARLIE GLAISTER  
CERTIFICATE #: 10436

Ca = 0.1000  
CAL = 0.978876    0.800 <= CAL < 1.200  
b1 = 0.0006    0.0000 <= b1 < 0.0040  
b2 = 0.0059    0.0010 <= b2 < 0.0100  
b3 = 0.0010    0.0000 <= b3 < 0.0040  
Xq = 0.0846    0.0500 <= Xq < 0.2000  
a21 = 1.181261    1.050 <= a21 < 1.300  
a31 = 0.415672    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 02/23/2024  
Time: 09:29:50

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
MINIMUM VOLUME TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.17: 0.078  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	09:30
BLANK TEST	0.000	09:30
INTERNAL STANDARD	VERIFIED	09:31
EXTERNAL STANDARD	0.079	09:31
BLANK TEST	0.000	09:32
SUBJECT SAMPLE (Vol=1.50L)	0.000	09:33
BLANK TEST	0.000	09:33
EXTERNAL STANDARD	0.080	09:34
BLANK TEST	0.000	09:35

CMG

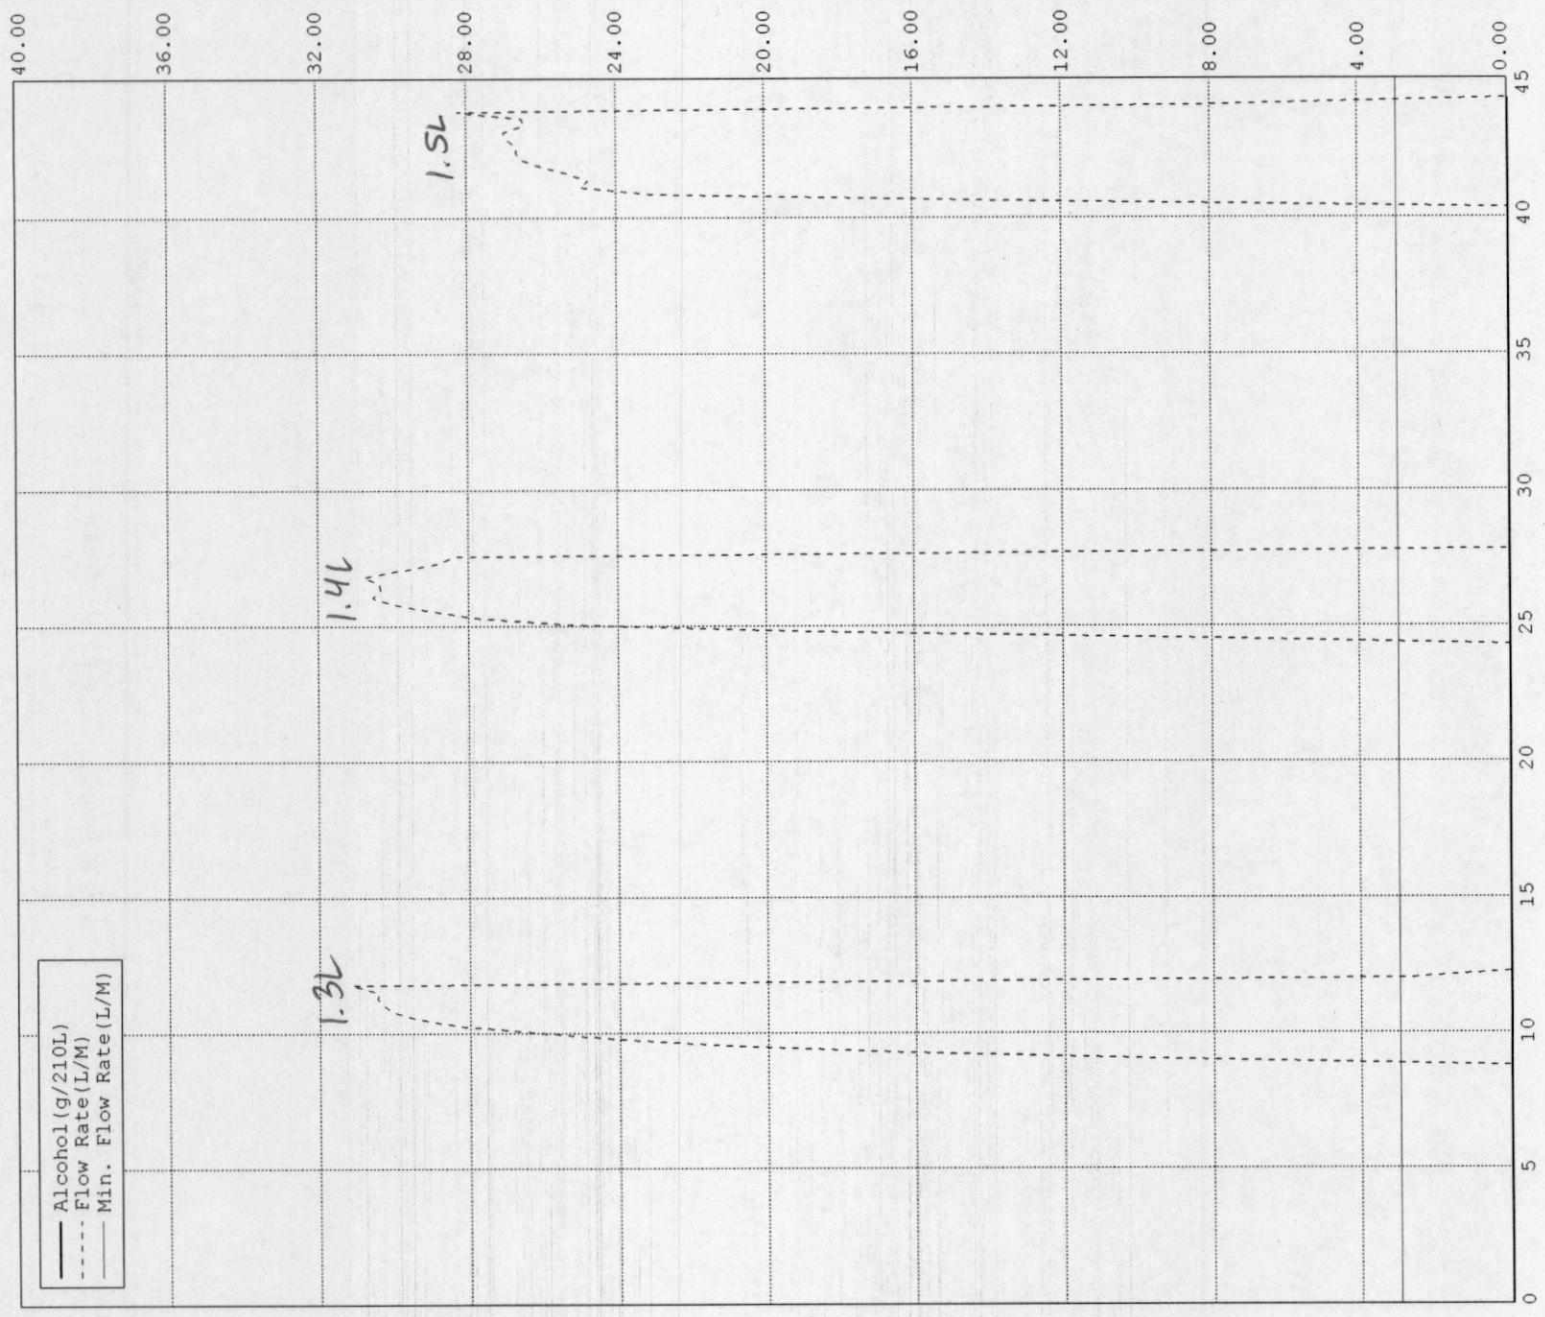

LINEARITY CHECK


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100367  
 -----

Date: 02/23/2024  
 Time: 09:41:26

SUPERVISOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0204	0.0005
0.039	0.0400	0.0000
0.078	0.0792	0.0004
0.098	0.0996	0.0005
0.146	0.1470	0.0000
0.293	0.2968	0.0004

SLOPE = 1.011125  
 R<sup>2</sup> = 0.999980

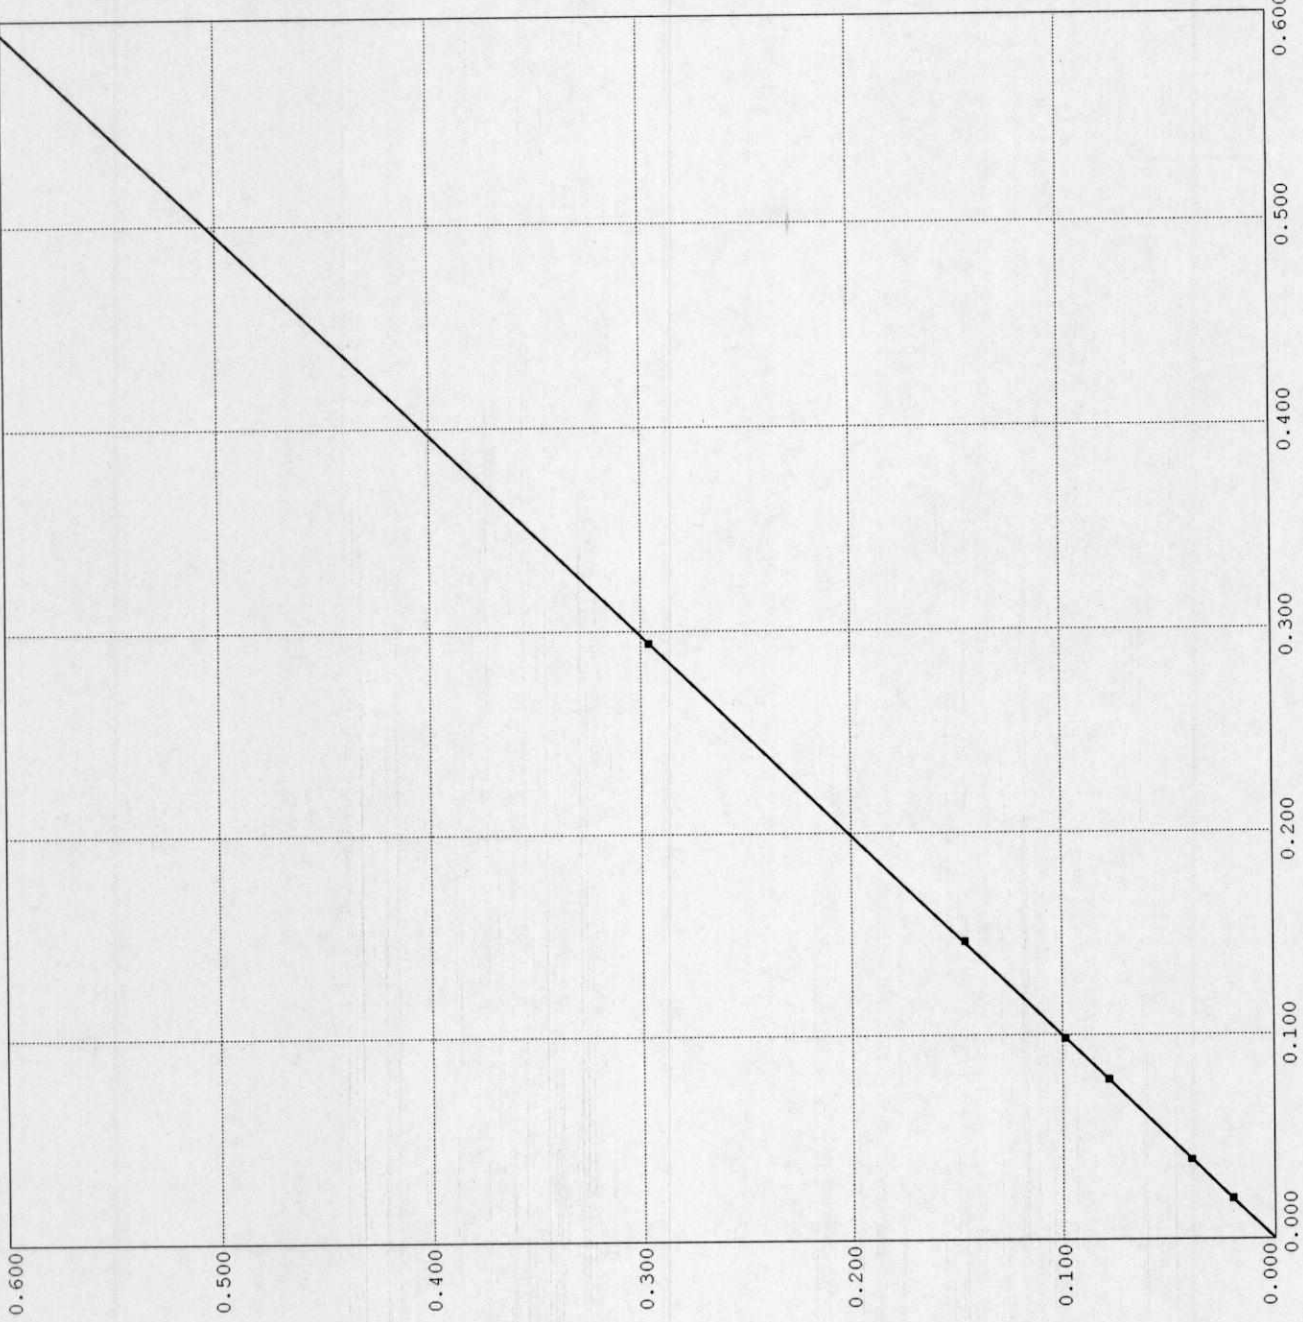

OKG

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100367






Date: 02/23/2024  
 Time: 09:41:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.18: 0.020  
 LOT #: AG217902  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 766 psi

BLANK TEST	0.000	09:43
INTERNAL STANDARD	VERIFIED	09:43
EXTERNAL STANDARD	0.021	09:43
BLANK TEST	0.000	09:44
EXTERNAL STANDARD	0.020	09:45
BLANK TEST	0.000	09:45
EXTERNAL STANDARD	0.020	09:46
BLANK TEST	0.000	09:47
EXTERNAL STANDARD	0.020	09:47
BLANK TEST	0.000	09:48
EXTERNAL STANDARD	0.021	09:48
BLANK TEST	0.000	09:49

Average = 0.0204  
 Std Dev = 0.0005

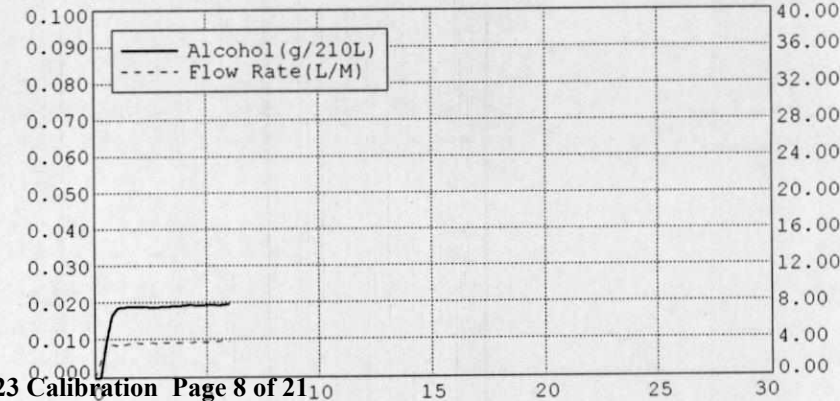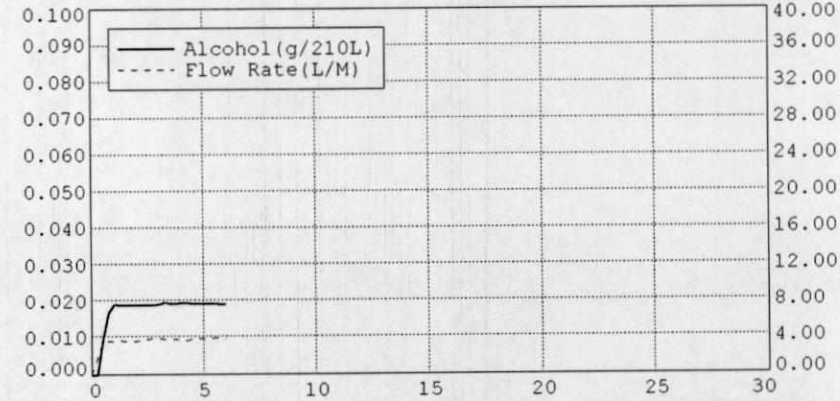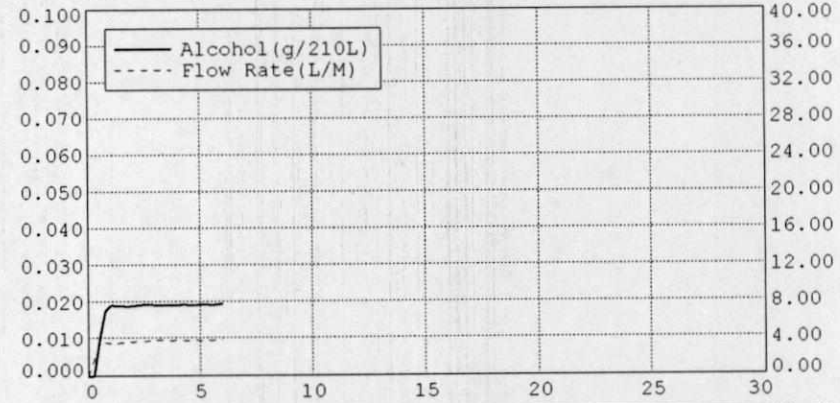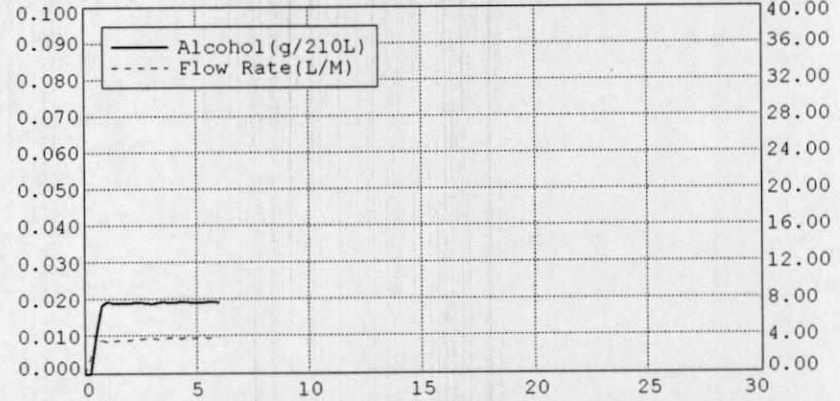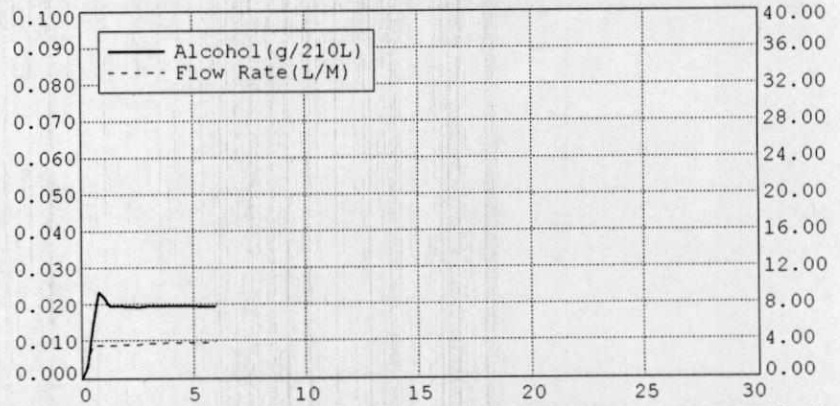



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100367






Date: 02/23/2024  
 Time: 09:56:12

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.17: 0.039  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 902 psi

BLANK TEST	0.000	09:57
INTERNAL STANDARD	VERIFIED	09:57
EXTERNAL STANDARD	0.040	09:57
BLANK TEST	0.000	09:58
EXTERNAL STANDARD	0.040	09:59
BLANK TEST	0.000	09:59
EXTERNAL STANDARD	0.040	10:00
BLANK TEST	0.000	10:01
EXTERNAL STANDARD	0.040	10:01
BLANK TEST	0.000	10:02
EXTERNAL STANDARD	0.040	10:02
BLANK TEST	0.000	10:03

Average = 0.0400  
 Std Dev = 0.0000

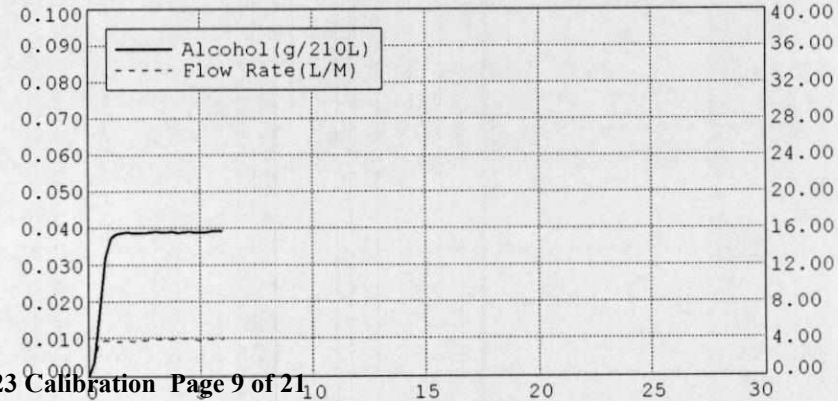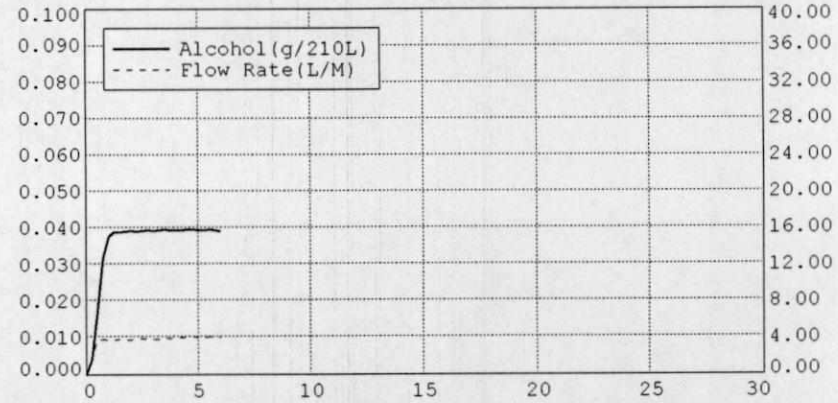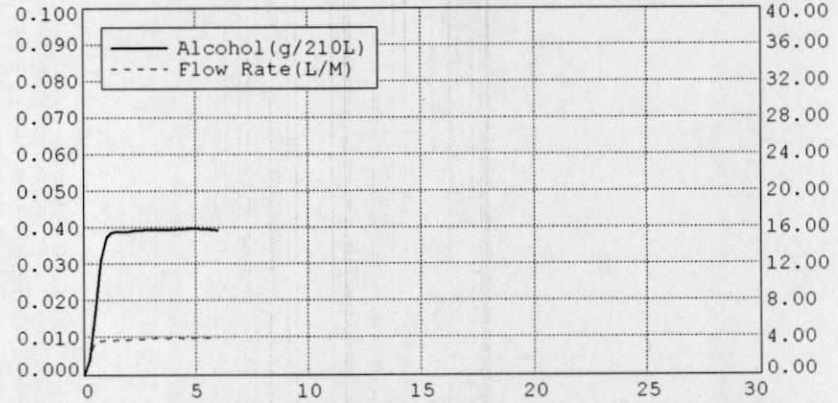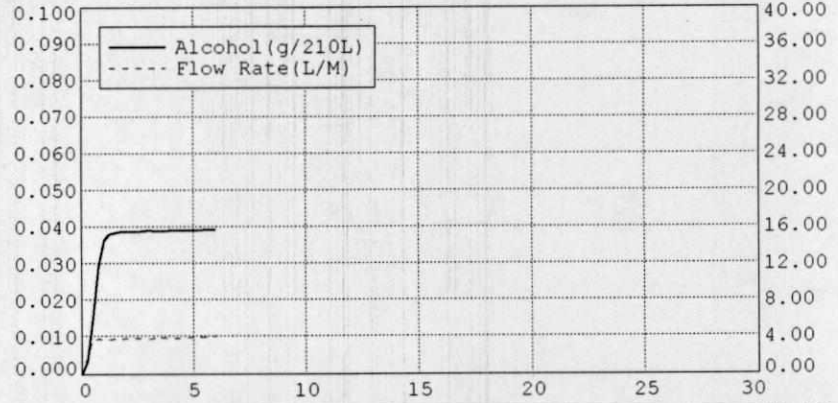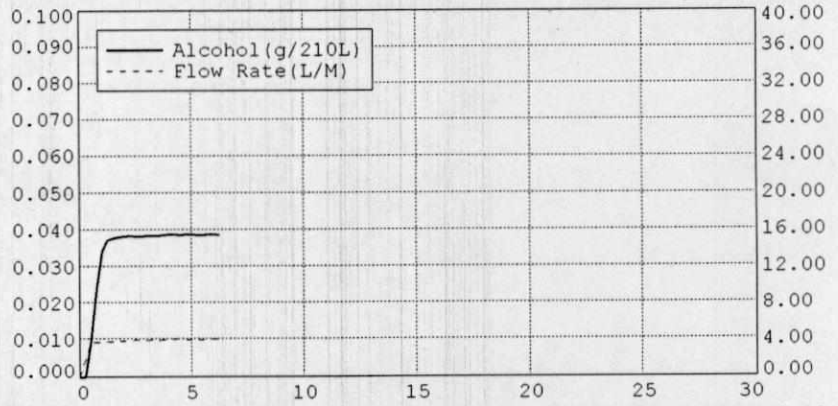

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100367






Date: 02/23/2024  
 Time: 10:03:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.17: 0.078  
 LOT #: 09523080A1  
 EXPIRATION: 05/05/2025  
 TANK PRESSURE: 419 psi

BLANK TEST	0.000	10:05
INTERNAL STANDARD	VERIFIED	10:05
EXTERNAL STANDARD	0.080	10:05
BLANK TEST	0.000	10:06
EXTERNAL STANDARD	0.079	10:06
BLANK TEST	0.000	10:07
EXTERNAL STANDARD	0.079	10:07
BLANK TEST	0.000	10:08
EXTERNAL STANDARD	0.079	10:09
BLANK TEST	0.000	10:09
EXTERNAL STANDARD	0.079	10:10
BLANK TEST	0.000	10:11

Average = 0.0792  
 Std Dev = 0.0004

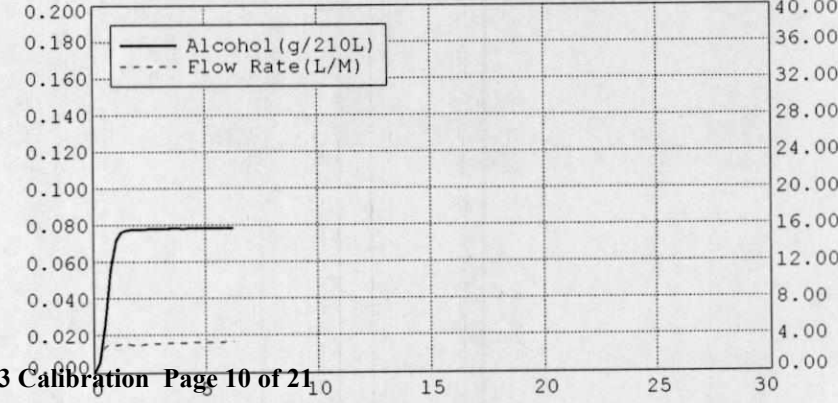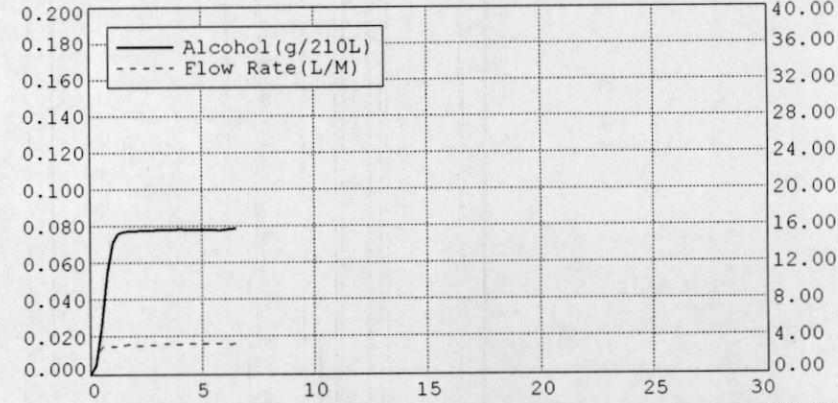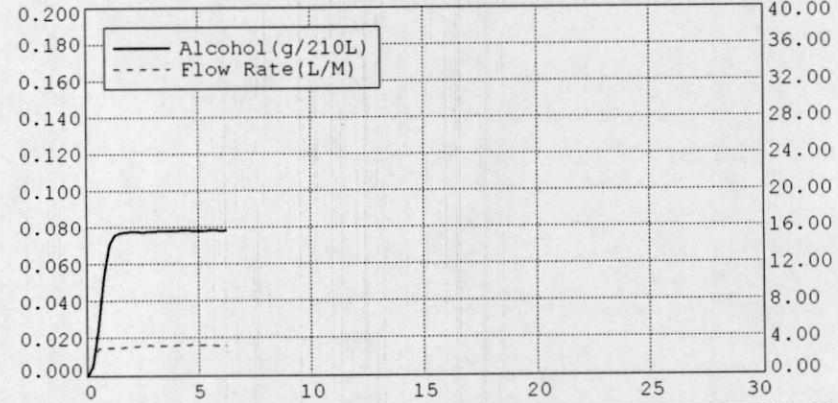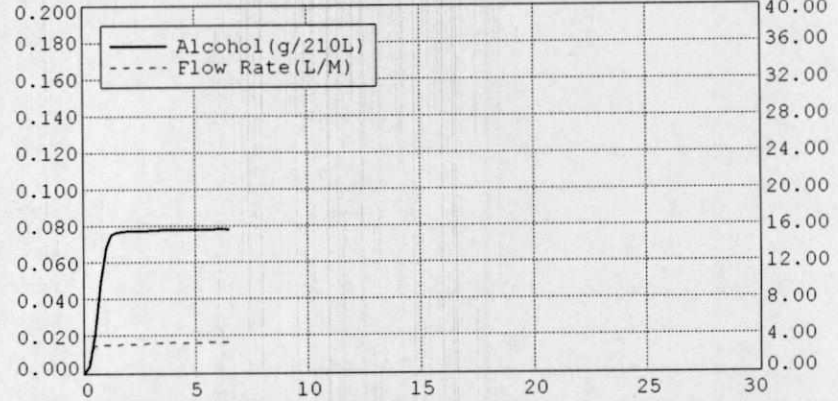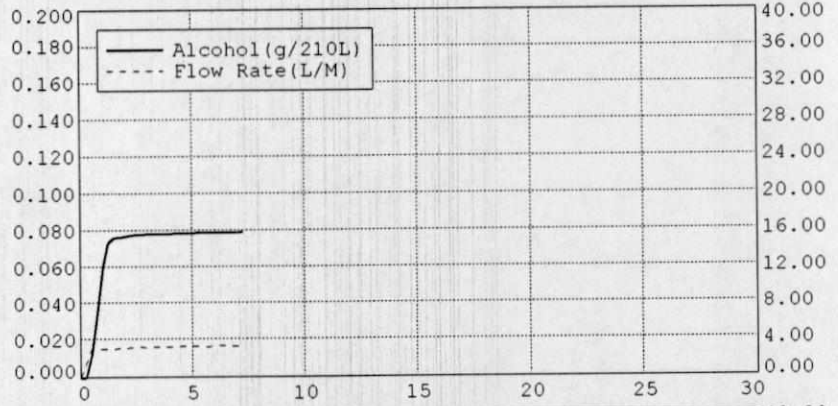

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100367






Date: 02/23/2024  
 Time: 10:13:27

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.17: 0.098  
 LOT #: AG211003  
 EXPIRATION: 04/20/2024  
 TANK PRESSURE: 954 psi

BLANK TEST	0.000	10:14
INTERNAL STANDARD	VERIFIED	10:15
EXTERNAL STANDARD	0.100	10:15
BLANK TEST	0.000	10:16
EXTERNAL STANDARD	0.099	10:16
BLANK TEST	0.000	10:17
EXTERNAL STANDARD	0.099	10:17
BLANK TEST	0.000	10:18
EXTERNAL STANDARD	0.100	10:18
BLANK TEST	0.000	10:19
EXTERNAL STANDARD	0.100	10:19
BLANK TEST	0.000	10:20

Average = 0.0996  
 Std Dev = 0.0005

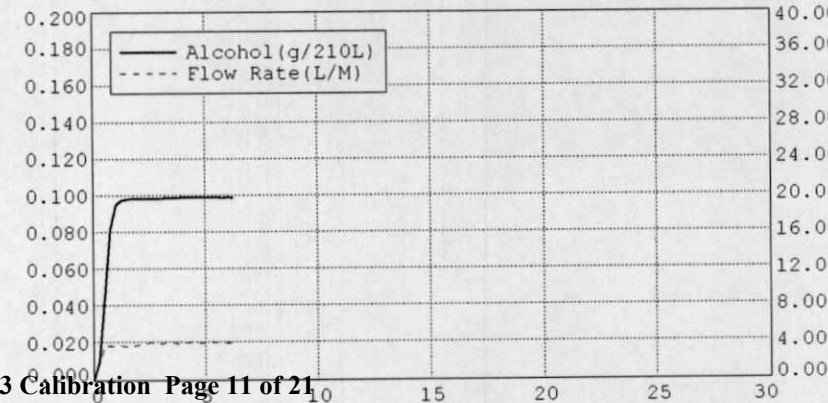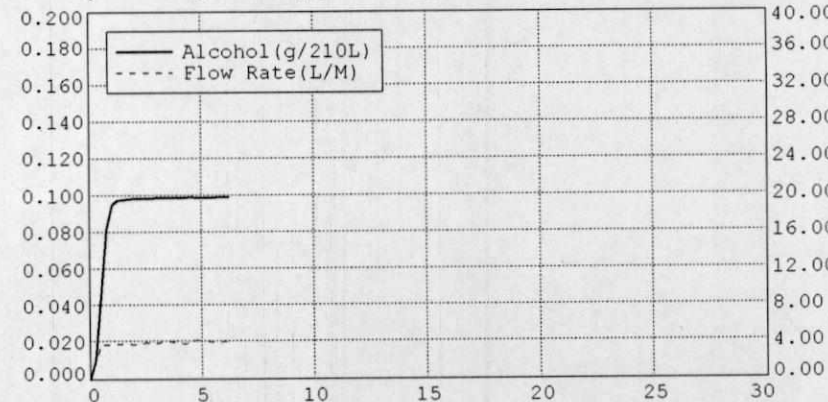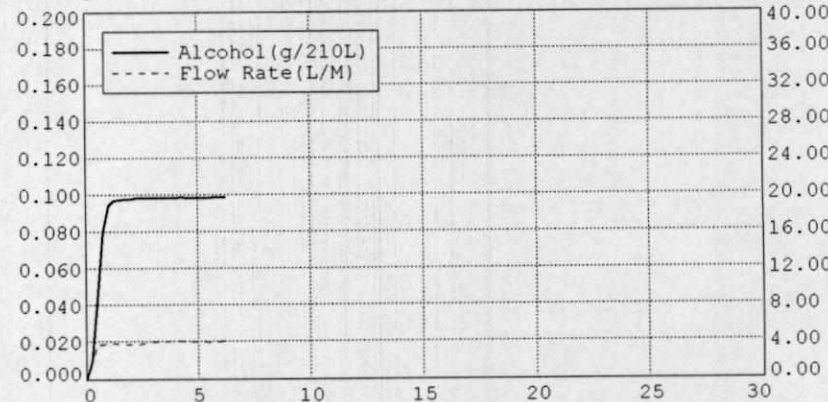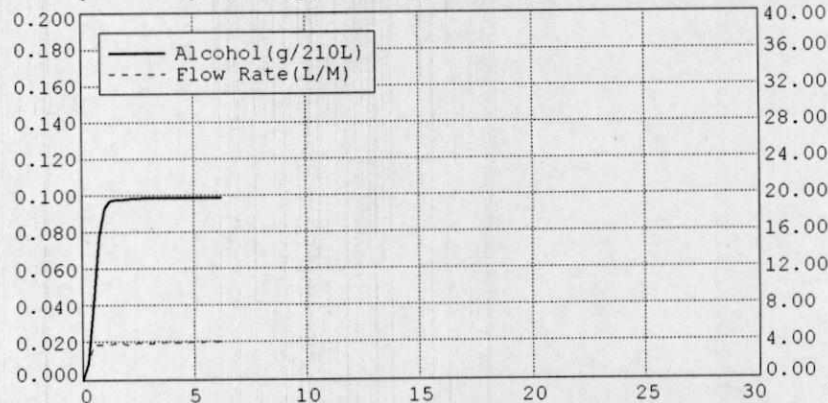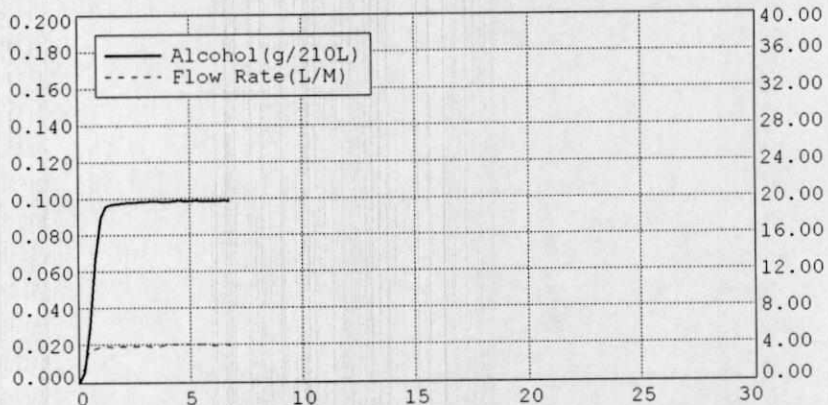

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100367






Date: 02/23/2024  
 Time: 10:21:19

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.17: 0.146  
 LOT #: AG332004  
 EXPIRATION: 11/16/2025  
 TANK PRESSURE: 700 psi

BLANK TEST	0.000	10:22
INTERNAL STANDARD	VERIFIED	10:23
EXTERNAL STANDARD	0.147	10:23
BLANK TEST	0.000	10:24
EXTERNAL STANDARD	0.147	10:24
BLANK TEST	0.000	10:25
EXTERNAL STANDARD	0.147	10:25
BLANK TEST	0.000	10:26
EXTERNAL STANDARD	0.147	10:26
BLANK TEST	0.000	10:27
EXTERNAL STANDARD	0.147	10:27
BLANK TEST	0.000	10:28

Average = 0.1470  
 Std Dev = 0.0000

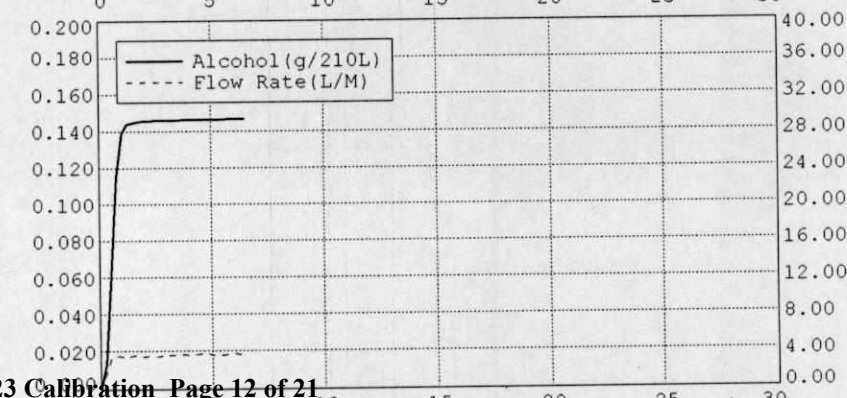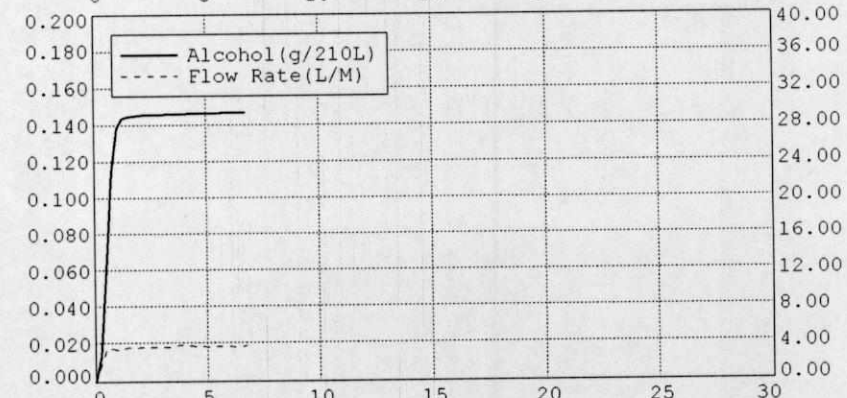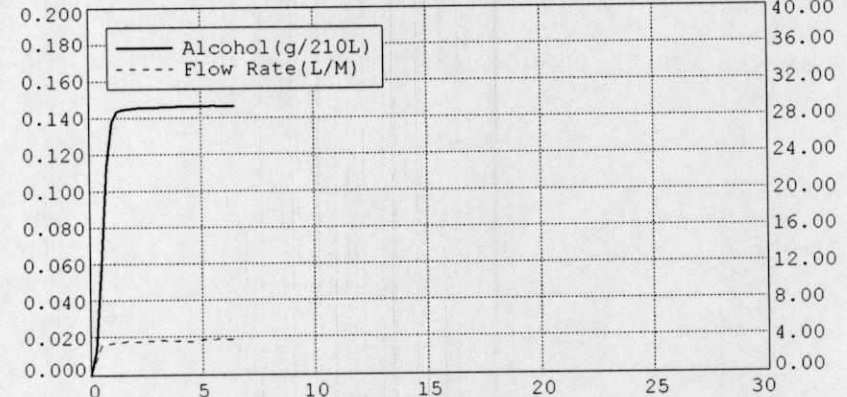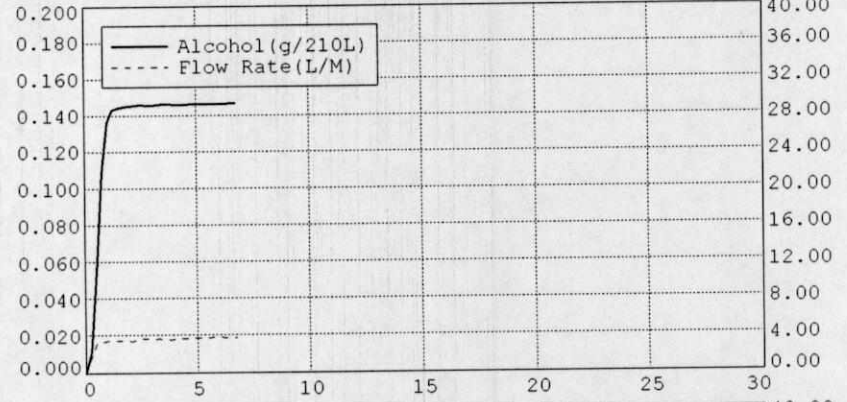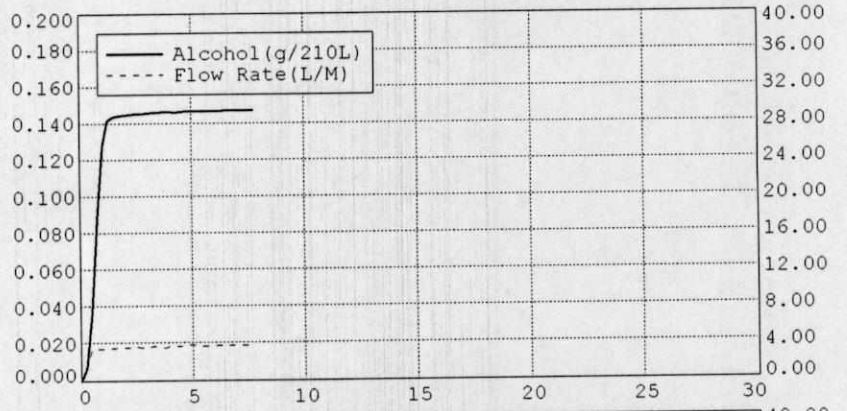

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100367






Date: 02/23/2024  
 Time: 10:29:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.17: 0.293  
 LOT #: AG327804  
 EXPIRATION: 10/05/2025  
 TANK PRESSURE: 515 psi

BLANK TEST	0.000	10:31
INTERNAL STANDARD	VERIFIED	10:31
EXTERNAL STANDARD	0.297	10:31
BLANK TEST	0.000	10:32
EXTERNAL STANDARD	0.296	10:33
BLANK TEST	0.000	10:33
EXTERNAL STANDARD	0.297	10:34
BLANK TEST	0.000	10:35
EXTERNAL STANDARD	0.297	10:35
BLANK TEST	0.000	10:36
EXTERNAL STANDARD	0.297	10:36
BLANK TEST	0.000	10:37

Average = 0.2968  
 Std Dev = 0.0004

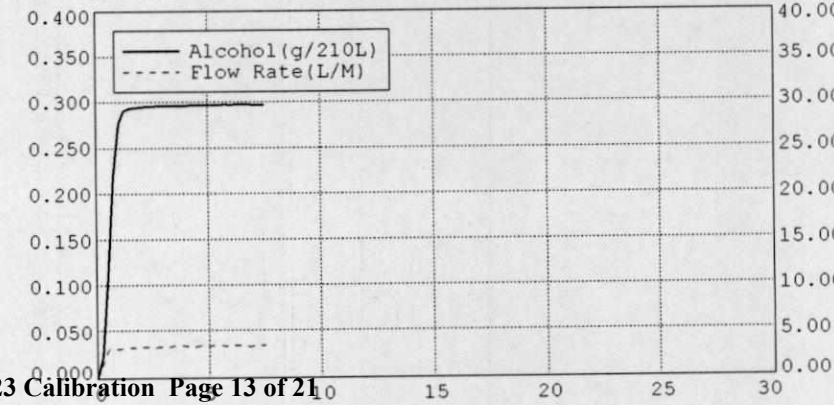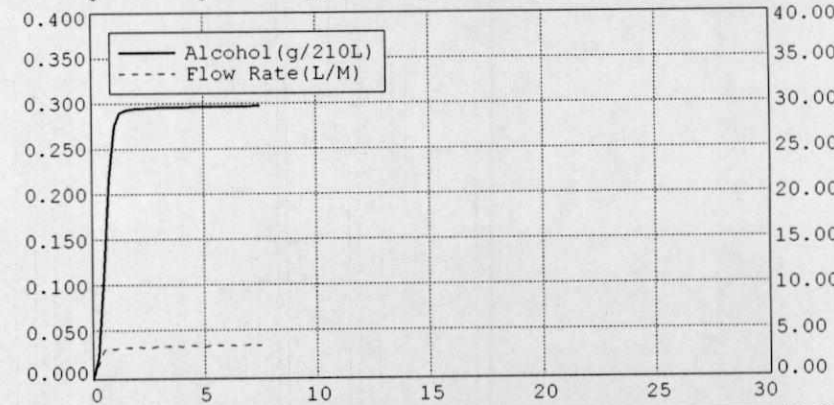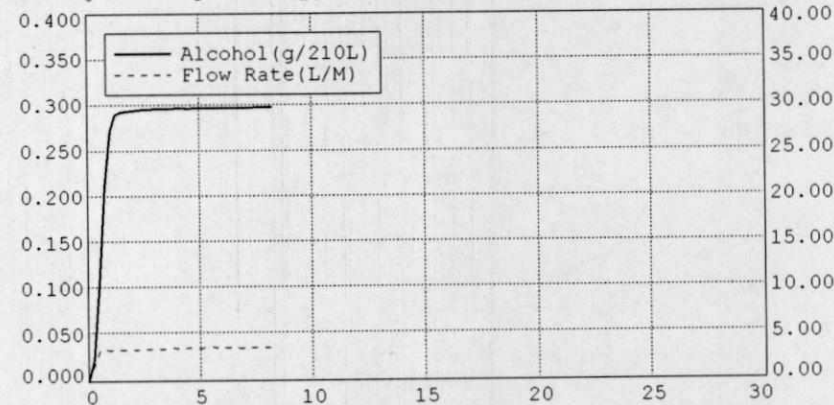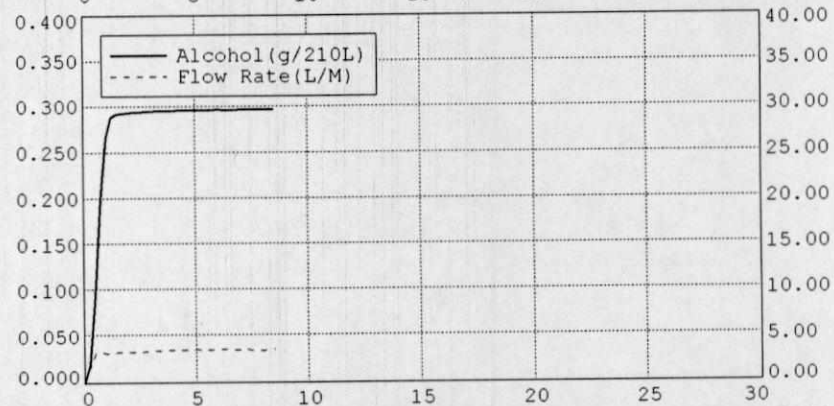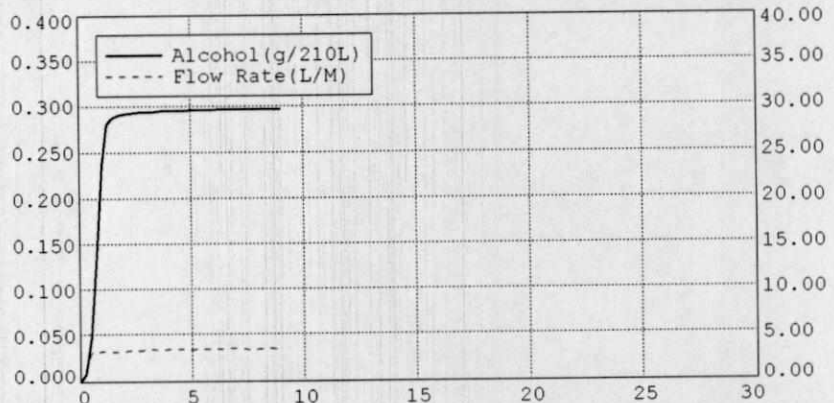

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 02/23/2024  
Time: 10:45:48

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INCOMPLETE TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.18: 0.078  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK PASSED 10:46  
BLANK TEST 0.000 10:47  
INTERNAL STANDARD VERIFIED 10:47  
EXTERNAL STANDARD 0.080 10:47  
BLANK TEST 0.000 10:48  
SUBJECT SAMPLE INCOMPLETE 10:50



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 02/23/2024  
Time: 10:52:10

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
MAXIMUM ATTEMPTS EXCEEDED  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.18: 0.078  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK PASSED 10:53  
BLANK TEST 0.000 10:53  
INTERNAL STANDARD VERIFIED 10:53  
EXTERNAL STANDARD 0.080 10:53  
BLANK TEST 0.000 10:54  
SUBJECT SAMPLE XXX 10:55

Maximum Attempts Exceeded

CVG

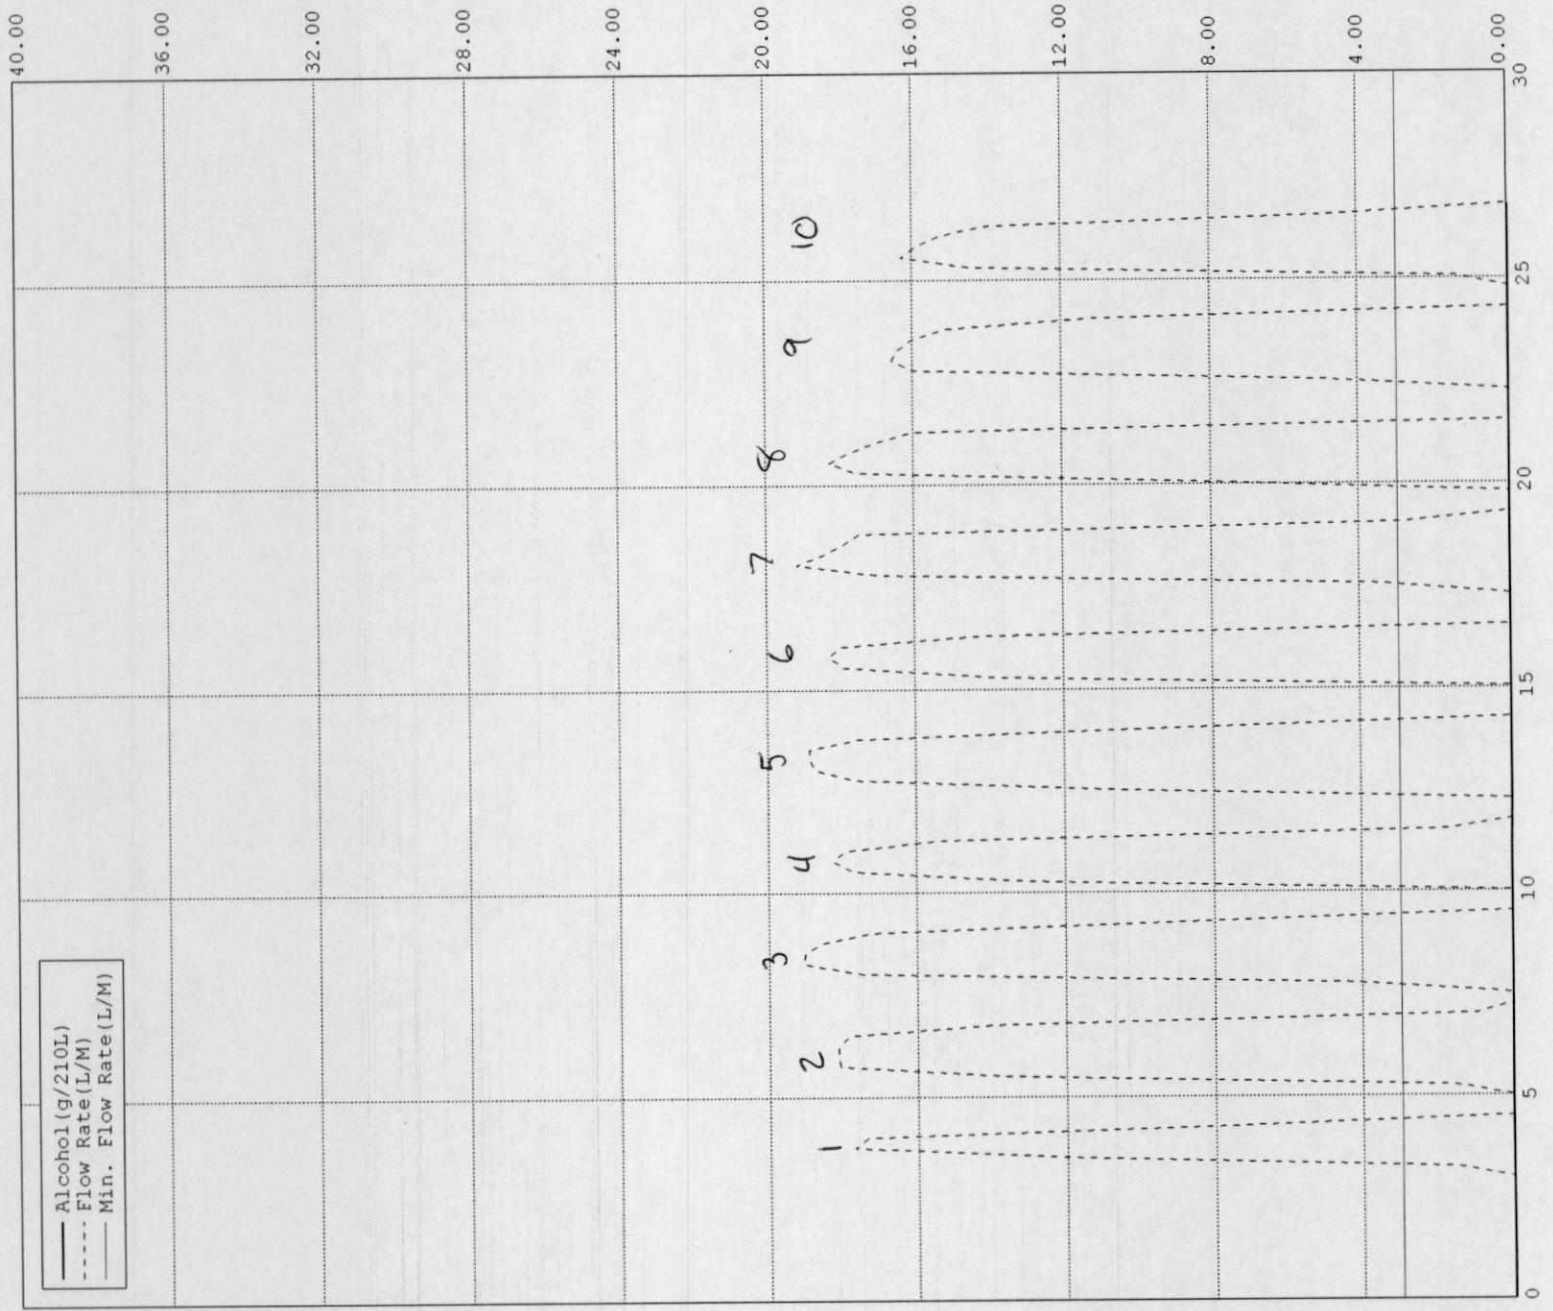

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 02/23/2024  
Time: 10:57:07

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
INVALID

CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.19: 0.078  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	10:58
BLANK TEST	0.000	10:58
INTERNAL STANDARD	VERIFIED	10:58
EXTERNAL STANDARD	0.080	10:59
BLANK TEST	0.000	11:00
SUBJECT SAMPLE	INVALID	11:00

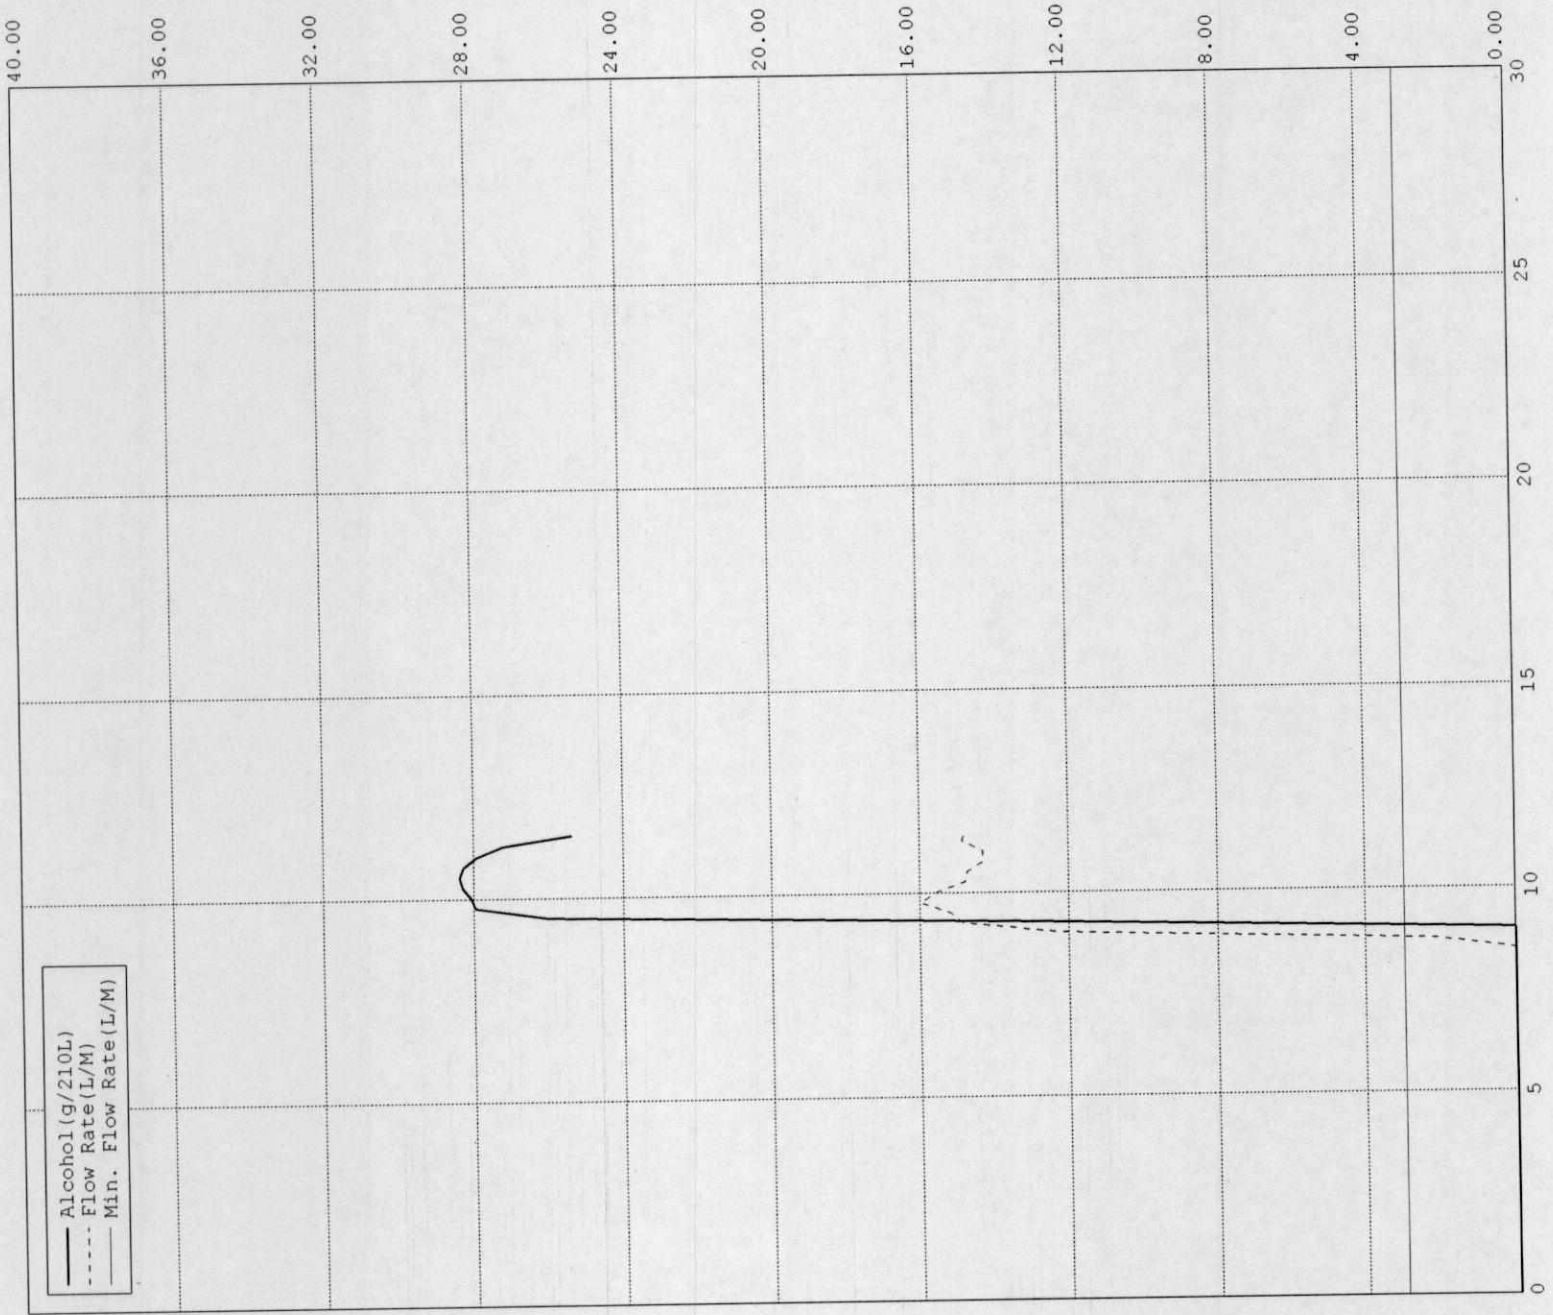



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 02/23/2024  
Time: 11:03:00

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
RFI

CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.20: 0.078  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK PASSED 11:04  
BLANK TEST 0.000 11:04  
INTERNAL STANDARD VERIFIED 11:04  
EXTERNAL STANDARD 0.079 11:04  
BLANK TEST 0.000 11:05

RFI DETECTED



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 02/23/2024  
Time: 12:18:13

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE ACETONE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.21: 0.078  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK PASSED 12:19  
BLANK TEST 0.000 12:19  
INTERNAL STANDARD VERIFIED 12:19  
Xq = 0.084 (0.31%)  
EXTERNAL STANDARD 0.079 12:19  
X[1] = 0.0792 (-0.0015) (0.0009)  
BLANK TEST 0.000 12:20  
SUBJECT SAMPLE XXX 12:21  
X[1] = 0.1070 (-0.0182) (-0.0002)

Interference Detected

~~-0.0004~~ -0.0008 corrected on 3/28/2024 CKG


Filter 2 Average: ~~0.0023~~

~~0.0006~~ 0.0010 corrected on 3/28/2024 CKG

Filter 3 Average: ~~0.0014~~

DMG 2/26/24

OK6

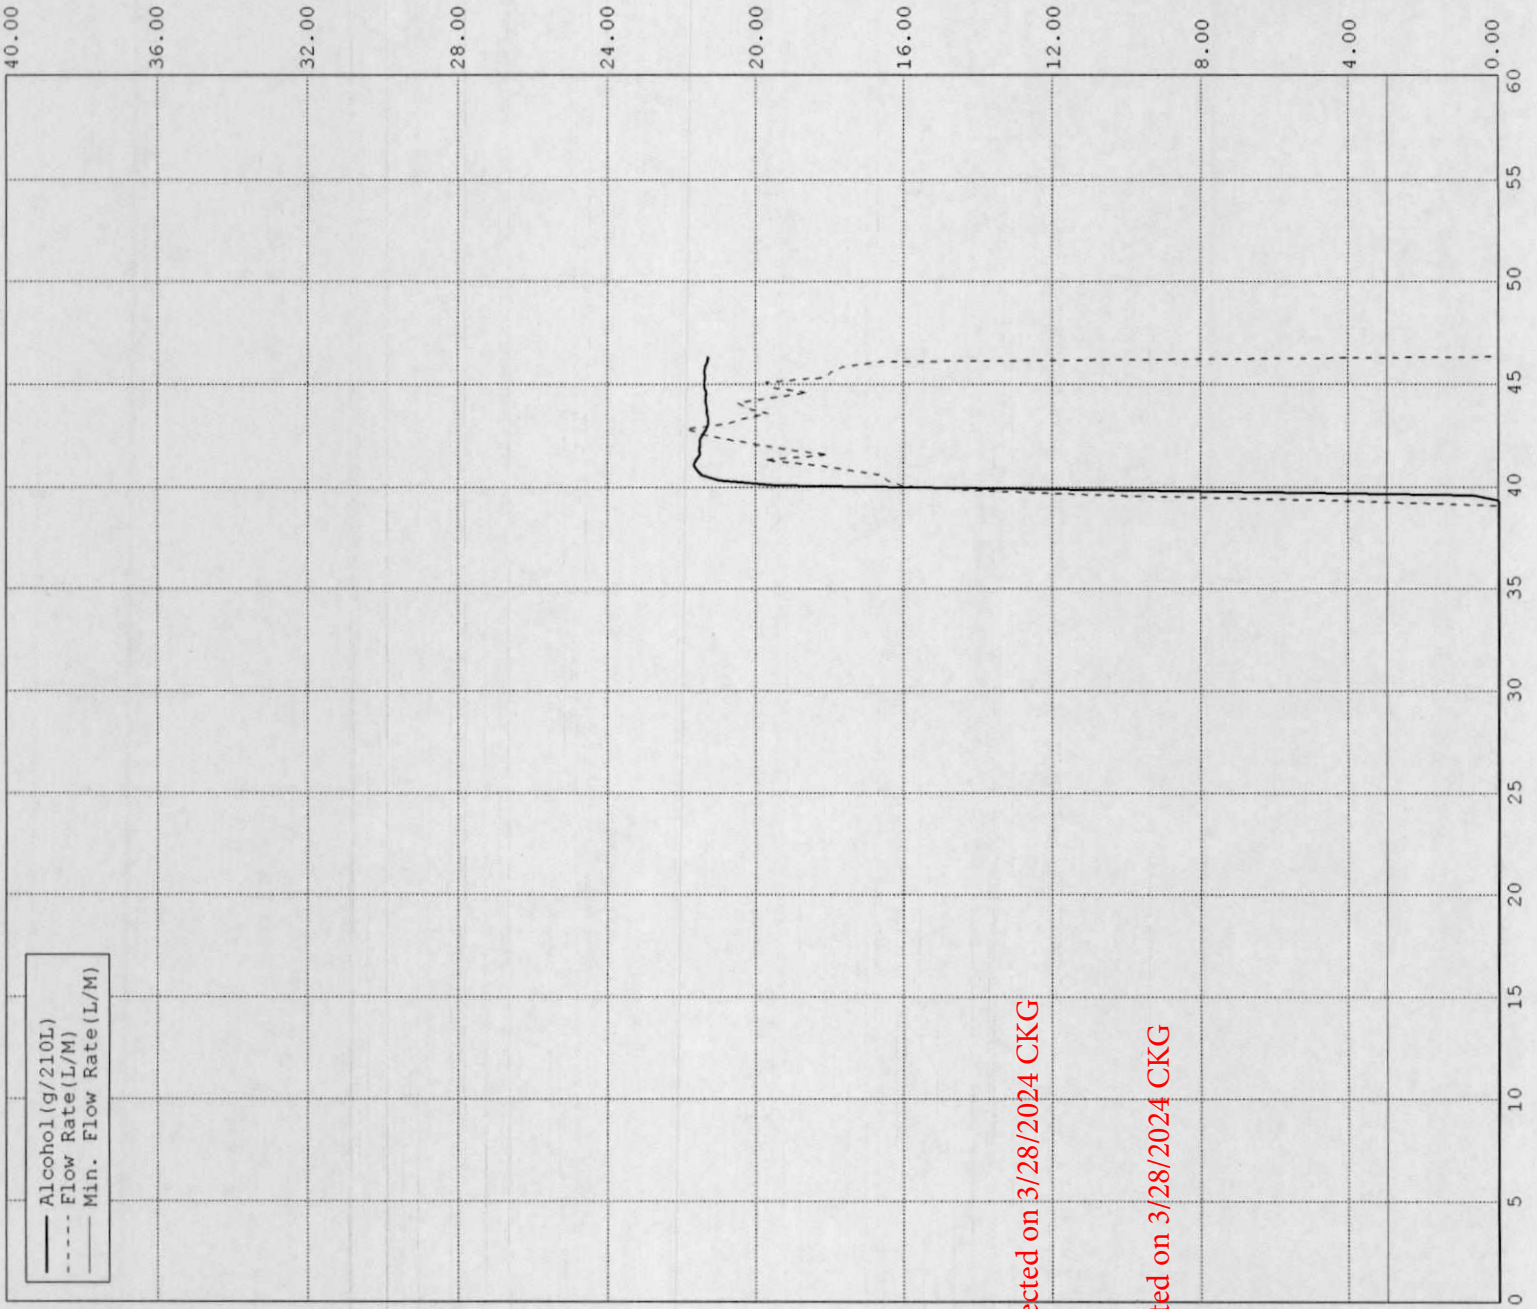

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 02/23/2024  
Time: 12:10:39

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE IPA  
CASE/REPORT: XXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.20: 0.078  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	12:11
BLANK TEST	0.000	12:11
INTERNAL STANDARD	VERIFIED	12:11
Xq = 0.085 (0.10%)		
EXTERNAL STANDARD	0.080	12:12
X[1] = 0.0795 (-0.0004) (0.0015)		
BLANK TEST	0.000	12:13
SUBJECT SAMPLE	XXX	12:13
X[1] = 0.1207 (-0.0255) (0.0017)		

Interference Detected

086

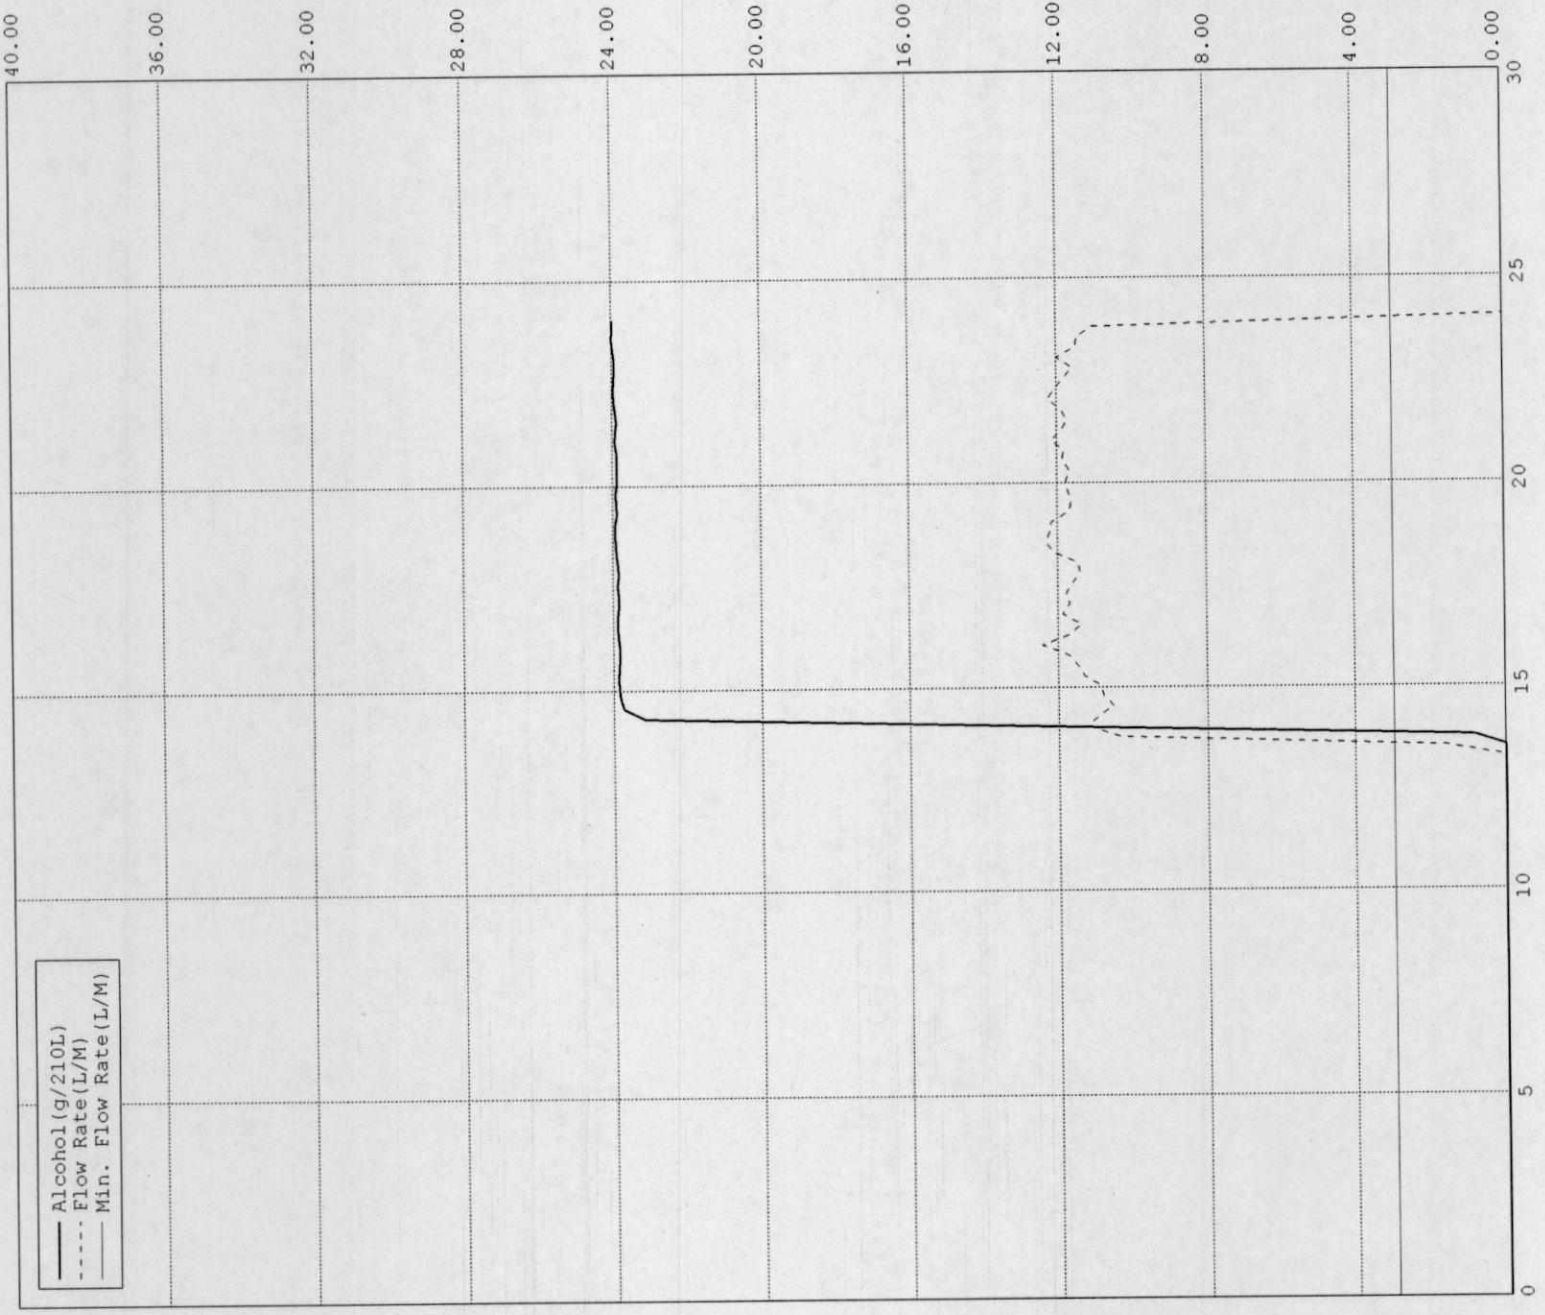

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 02/23/2024  
Time: 12:25:14

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE NEGATIVE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.21: 0.078  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	12:27
BLANK TEST	0.000	12:27
INTERNAL STANDARD	VERIFIED	12:27
Xq = 0.085 (0.21%)	0.080	12:27
X[1] = 0.0796 (-0.0010)	(0.0012)	12:28
BLANK TEST	0.000	12:28
SUBJECT SAMPLE (Vol=1.66L)	0.097	12:29
X[1] = 0.0974 (0.0008)	(-0.0005)	12:30
BLANK TEST	0.000	12:31
EXTERNAL STANDARD	0.079	12:31
X[1] = 0.0791 (-0.0004)	(0.0005)	12:32
BLANK TEST	0.000	12:32

DLG

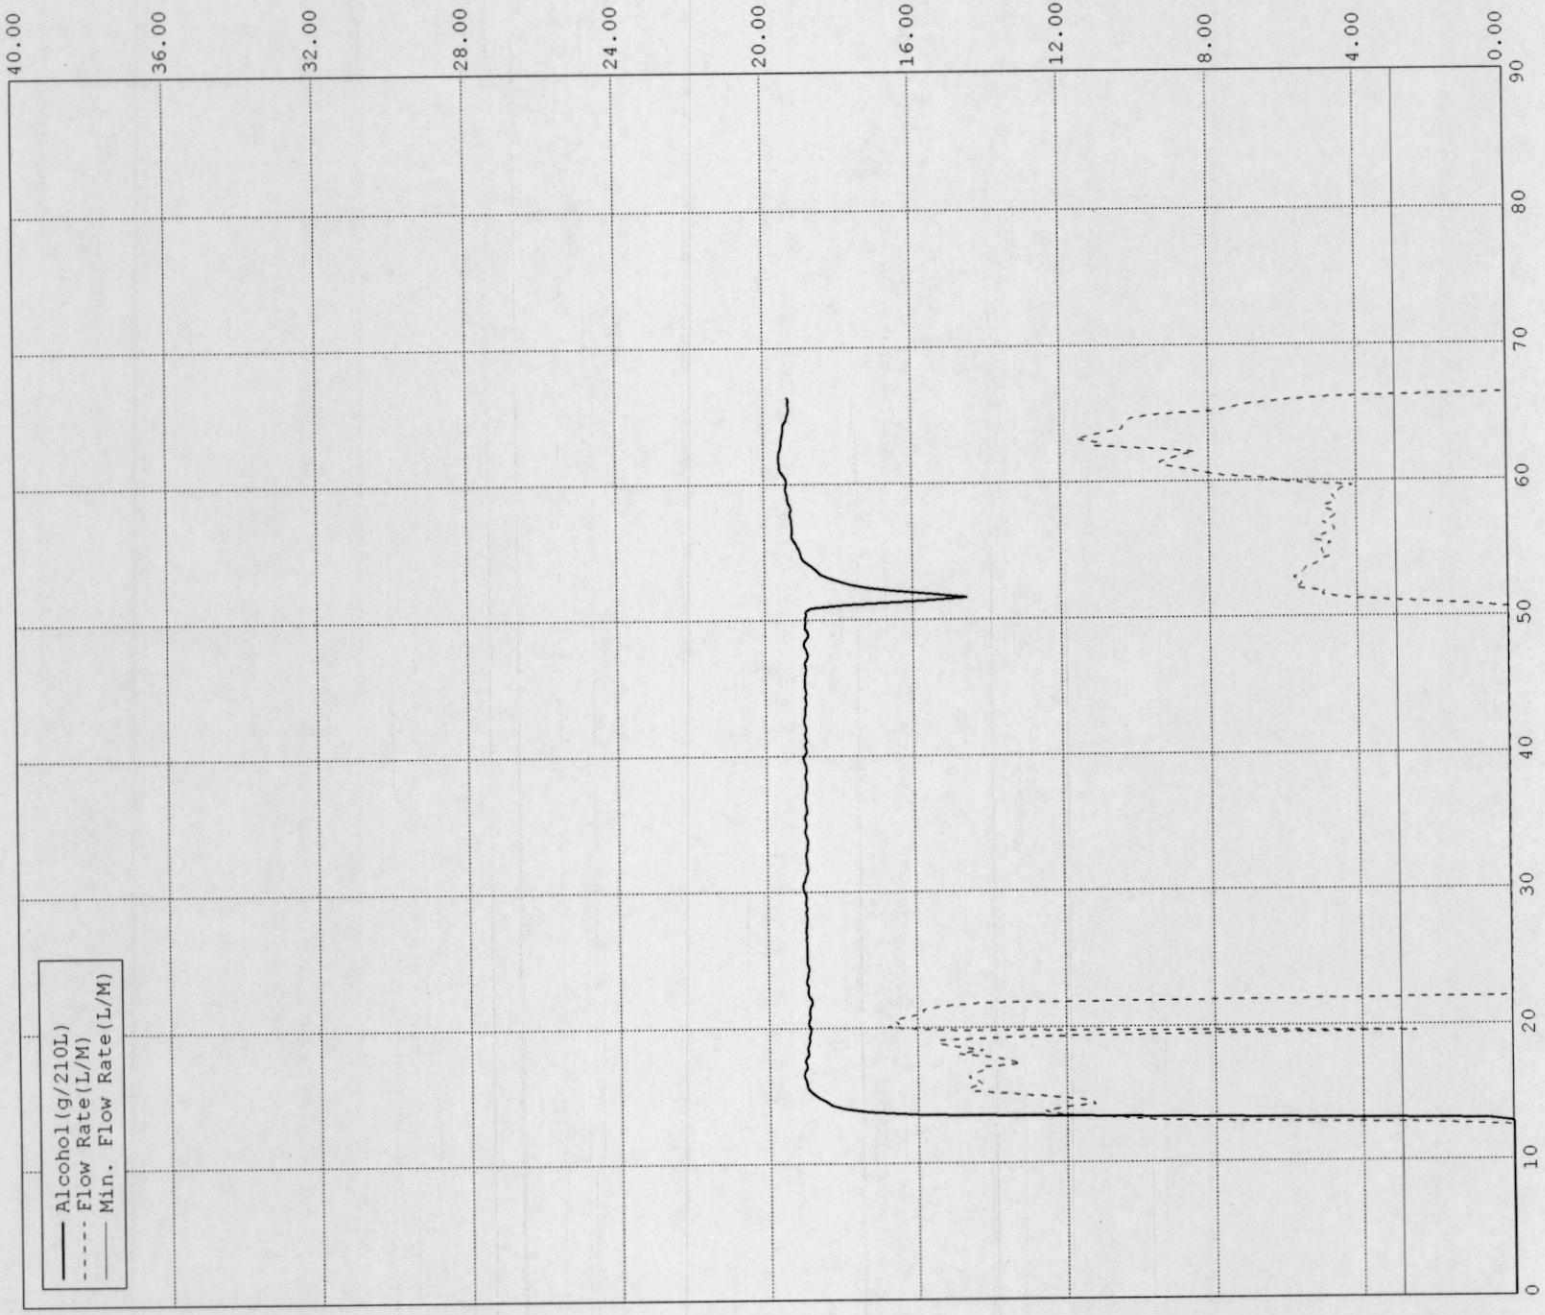

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100367

Date: 02/23/2024  
Time: 12:56:49

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
NON-DRINKING SUBJECT TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.19: 0.078  
LOT #: 09523080A1  
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	12:58
BLANK TEST	0.000	12:58
INTERNAL STANDARD	VERIFIED	12:58
EXTERNAL STANDARD	0.079	12:58
BLANK TEST	0.000	12:59
SUBJECT SAMPLE (Vol=2.01L)	0.000	13:00
BLANK TEST	0.000	13:01
EXTERNAL STANDARD	0.080	13:01
BLANK TEST	0.000	13:02

