

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster dmt Breath Test Instrument*  
 State of Alaska

Serial #: 100422

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Date: 07/24/2013

**External Standard Test Values**

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.75: 0.079  
 LOT #: 22612080A1  
 EXPIRATION: 09/01/2014

BLANK TEST	0.000	10:13
INTERNAL STANDARD	VERIFIED	10:13
EXTERNAL STANDARD	0.080	10:13
BLANK TEST	0.000	10:14
EXTERNAL STANDARD	0.080	10:15
BLANK TEST	0.000	10:15
EXTERNAL STANDARD	0.080	10:16
BLANK TEST	0.000	10:17
EXTERNAL STANDARD	0.081	10:17
BLANK TEST	0.000	10:18
EXTERNAL STANDARD	0.080	10:18
BLANK TEST	0.000	10:19

Average = 0.0802  
 Std Dev = 0.0004

**Diagnostic Check**

VERSIONS  
 DMT: 2.00  
 PIC: 3.03  
 Modem: 2.3  
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C	PASSED
Breath Tube = 47.9°C	PASSED

PUMP INFO

Flow Rate = 4.626 L/M	PASSED
-----------------------	--------

DETECTOR INFO

PUMP ON	PASSED
PUMP OFF	PASSED

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
-------------------	--------



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

*Nita J. Bolz* 8/2/2013  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 2nd day of Aug. 2013

*Nikki Roth*  
 Nikki Roth, Notary Public  
 My Commission Expires With Office

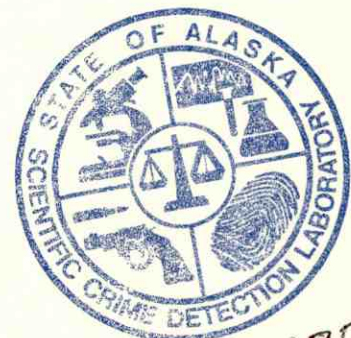

CRF  
 7/24/13