

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100403

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 01/03/2014

External Standard Test Values	Diagnostic Check																																																		
<p>EXTERNAL STANDARD INFORMATION</p> <p>NOMINAL: 0.080 TARGET AT 27.56: 0.073 LOT #: 11313080A1 EXPIRATION: 06/01/2015</p> <table style="width: 100%; border-collapse: collapse;"> <tr><td>BLANK TEST</td><td style="text-align: right;">0.000</td><td style="text-align: right;">12:02</td></tr> <tr><td>INTERNAL STANDARD</td><td style="text-align: right;">VERIFIED</td><td style="text-align: right;">12:02</td></tr> <tr><td>EXTERNAL STANDARD</td><td style="text-align: right;">0.076</td><td style="text-align: right;">12:02</td></tr> <tr><td>BLANK TEST</td><td style="text-align: right;">0.000</td><td style="text-align: right;">12:03</td></tr> <tr><td>EXTERNAL STANDARD</td><td style="text-align: right;">0.075</td><td style="text-align: right;">12:03</td></tr> <tr><td>BLANK TEST</td><td style="text-align: right;">0.000</td><td style="text-align: right;">12:04</td></tr> <tr><td>EXTERNAL STANDARD</td><td style="text-align: right;">0.075</td><td style="text-align: right;">12:04</td></tr> <tr><td>BLANK TEST</td><td style="text-align: right;">0.000</td><td style="text-align: right;">12:05</td></tr> <tr><td>EXTERNAL STANDARD</td><td style="text-align: right;">0.076</td><td style="text-align: right;">12:05</td></tr> <tr><td>BLANK TEST</td><td style="text-align: right;">0.000</td><td style="text-align: right;">12:06</td></tr> <tr><td>EXTERNAL STANDARD</td><td style="text-align: right;">0.076</td><td style="text-align: right;">12:06</td></tr> <tr><td>BLANK TEST</td><td style="text-align: right;">0.000</td><td style="text-align: right;">12:07</td></tr> </table> <p>Average = 0.0756 Std Dev = 0.0005</p>	BLANK TEST	0.000	12:02	INTERNAL STANDARD	VERIFIED	12:02	EXTERNAL STANDARD	0.076	12:02	BLANK TEST	0.000	12:03	EXTERNAL STANDARD	0.075	12:03	BLANK TEST	0.000	12:04	EXTERNAL STANDARD	0.075	12:04	BLANK TEST	0.000	12:05	EXTERNAL STANDARD	0.076	12:05	BLANK TEST	0.000	12:06	EXTERNAL STANDARD	0.076	12:06	BLANK TEST	0.000	12:07	<p>VERSIONS</p> <p>DMT: 2.00 PIC: 3.02 Modem: 2.3 Questions: 2.2</p> <p>TEMPERATURES</p> <table style="width: 100%; border-collapse: collapse;"> <tr><td>Sample Chamber = 48.9°C</td><td style="text-align: right;">PASSED</td></tr> <tr><td>Breath Tube = 46.5°C</td><td style="text-align: right;">PASSED</td></tr> </table> <p>PUMP INFO</p> <p>Flow Rate = 4.759 L/M PASSED</p> <p>DETECTOR INFO</p> <table style="width: 100%; border-collapse: collapse;"> <tr><td>PUMP ON</td><td style="text-align: right;">PASSED</td></tr> <tr><td>PUMP OFF</td><td style="text-align: right;">PASSED</td></tr> </table> <p>FILTER INFO</p> <table style="width: 100%; border-collapse: collapse;"> <tr><td>Filter 1</td><td style="text-align: right;">PASSED</td></tr> <tr><td>Filter 2</td><td style="text-align: right;">PASSED</td></tr> <tr><td>Filter 3</td><td style="text-align: right;">PASSED</td></tr> </table> <p>INTERNAL STANDARD PASSED</p>	Sample Chamber = 48.9°C	PASSED	Breath Tube = 46.5°C	PASSED	PUMP ON	PASSED	PUMP OFF	PASSED	Filter 1	PASSED	Filter 2	PASSED	Filter 3	PASSED
BLANK TEST	0.000	12:02																																																	
INTERNAL STANDARD	VERIFIED	12:02																																																	
EXTERNAL STANDARD	0.076	12:02																																																	
BLANK TEST	0.000	12:03																																																	
EXTERNAL STANDARD	0.075	12:03																																																	
BLANK TEST	0.000	12:04																																																	
EXTERNAL STANDARD	0.075	12:04																																																	
BLANK TEST	0.000	12:05																																																	
EXTERNAL STANDARD	0.076	12:05																																																	
BLANK TEST	0.000	12:06																																																	
EXTERNAL STANDARD	0.076	12:06																																																	
BLANK TEST	0.000	12:07																																																	
Sample Chamber = 48.9°C	PASSED																																																		
Breath Tube = 46.5°C	PASSED																																																		
PUMP ON	PASSED																																																		
PUMP OFF	PASSED																																																		
Filter 1	PASSED																																																		
Filter 2	PASSED																																																		
Filter 3	PASSED																																																		

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz


1/31/2014

Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 31 day of Jan, 2014

Nikki Roth

Nikki Roth, Notary Public
 My Commission Expires With Office

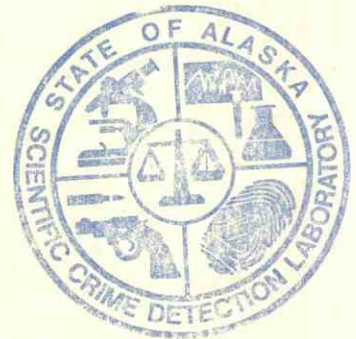

003/18/14