

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100682 Analyst: C. O. Bryant Start Date: 1/5/23

Diagnostic Test (attached) Internal Standard value \leq 3.00%

Adjust voltages, if needed

- Lamp (2.60 V Maximum)
- Bias
- Cooler (2.00 V Maximum)

- Chopper Frequency
- Detector Voltage
(-0.100V to 0.100V)

Set RFI Sensitivity

Adjust internal barometer reading to match NIST-traceable barometer

Adjust volume setting, if needed (1.50 L +/- 0.10 L)

Print Technician Screen (attached)

Print Calibration Factors (attached)

Minimum Volume Test 1.4 L (1.3L to 1.7L)

This Calibration was rejected due to the SD card creating a corrupt ticket db file during 100682 2022.12.13 Repair and then again during 100682 2023.01.05 Calibration. Recommend replacing SD Card. COB 2023.01.17

As Left Conditions:

Barometric Pressure (in Hg): 29.25 Temperature (C): 21.2 Relative Humidity (%) 16

Linearity Test (attached)

0.020g/210L Mnf: <u>Aargas</u>	Lot: <u>AG217902</u>	Exp: <u>6/28/24</u>
0.040g/210L Mnf: <u>Aargas</u>	Lot: <u>AG217904</u>	Exp: <u>6/28/24</u>
0.080g/210L Mnf: <u>Aargas</u>	Lot: <u>AG217902</u>	Exp: <u>5/14/23</u>
0.100g/210L Mnf: <u>Aargas</u>	Lot: <u>AG211003</u>	Exp: <u>4/20/24</u>
0.150g/210L Mnf: <u>Aargas</u>	Lot: <u>AG134205</u>	Exp: <u>12/8/23</u>
0.300g/210L Mnf: <u>Aargas</u>	Lot: <u>AG130502</u>	Exp: <u>11/1/23</u>

Functional Tests (attached)

Incomplete Invalid
 Maximum Attempts Exceeded Radio Frequency Interference (RFI)

Interference (Volatiles)

Acetone Mnf: LifeLoc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: DR5298 Verification Performed?

Isopropanol Mnf: LifeLoc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: SD1198 Verification Performed?

Neg. Control Mnf: LifeLoc Lot: 21KP41172 Level: 0.100 Exp: 11/9/23

Simulator S/N: SD1202 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 2010958384 Calibration Due Date: 11/9/23

Verify stylus is calibrated

Reset Options

Clear Memory

Verification of Calibration (VOC)

Non-Drinking Subject Test * See next page.

Upload

Remove Tank Prior to Shutdown

Calibration End Date: 1/5/23

2023.01.05 - 100682

***On 2023.01.05 upon completion of a non-drinking subject test during a calibration procedure, the ticket db file on the SD card in the instrument, became corrupt. The non-drinking subject test was complete, yet the screen never cleared and the report didn't print. I restarted the instrument and "Unable to load ticket db" pop up appeared. I restarted the instrument and "instrument restarted due to fatal error" pop up appeared. I removed the SD card from the instrument and inserted it into a card reader on the laboratory computer. I scanned the card and deleted the corrupt "ticket db" file. I removed the card, reinserted it and scanned it and made the system recommended repairs. I replaced the SD card into the instrument and restarted it. I was then able to reprint the non-drinking subject test results from the report menu. Instrument is calibrated and ready for use.**

C. O'Bryant 2023.01.05

Calibration Rejected

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 06:56:05

VERSIONS

DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 47.5°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 2.11 V PASSED
(1.36 V - 3.18 V)
Cooler Voltage = 1.69 V PASSED
(1.04 V - 2.44 V)
Bias Voltage = 79 V PASSED
(47 V - 111 V)
Chopper Freq = 534 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.3 in

PUMP INFO

Flow Rate = 4.549 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.093 0.76% (0.00% - 4.00%) PASSED

Calibration Rejected

Technician Screen

DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 7:33 AM

Temperatures (°C)

Sample Cell: 48.7°C
Breath Tube: 47.6°C

Current Barometer 29.3 in
Volume (Ltr) 1.60

Settings

Lamp: 2.14 V
Bias: 80 V
Cooler: 1.79 V
Chopper: 536 Hz

Voltages (V)

Flow: 1.05 V
Detector: 0.097 V

Calibration Rejected

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 04/01/2019
Time: 09:15:52

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca	=	0.1000			
CAL	=	0.962605	0.800	<=	CAL < 1.200
b1	=	0.0010	0.0000	<=	b1 < 0.0040
b2	=	0.0048	0.0010	<=	b2 < 0.0100
b3	=	0.0002	0.0000	<=	b3 < 0.0040
Xq	=	0.0924	0.0500	<=	Xq < 0.2000
a21	=	1.117691	1.050	<=	a21 < 1.300
a31	=	0.445338	0.300	<=	a31 < 0.800

Calibration Rejected

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 07:34:51


SUBJECT NAME:
TEST TEST
LICENSE #: NON=DRINKING

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.26: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK PASSED 07:36
BLANK TEST 0.000 07:36
INTERNAL STANDARD VERIFIED 07:36
EXTERNAL STANDARD 0.076 07:37
BLANK TEST 0.000 07:37
SUBJECT SAMPLE (Vol=1.50L) 0.000 07:38
BLANK TEST 0.000 07:39
EXTERNAL STANDARD 0.077 07:39
BLANK TEST 0.000 07:40

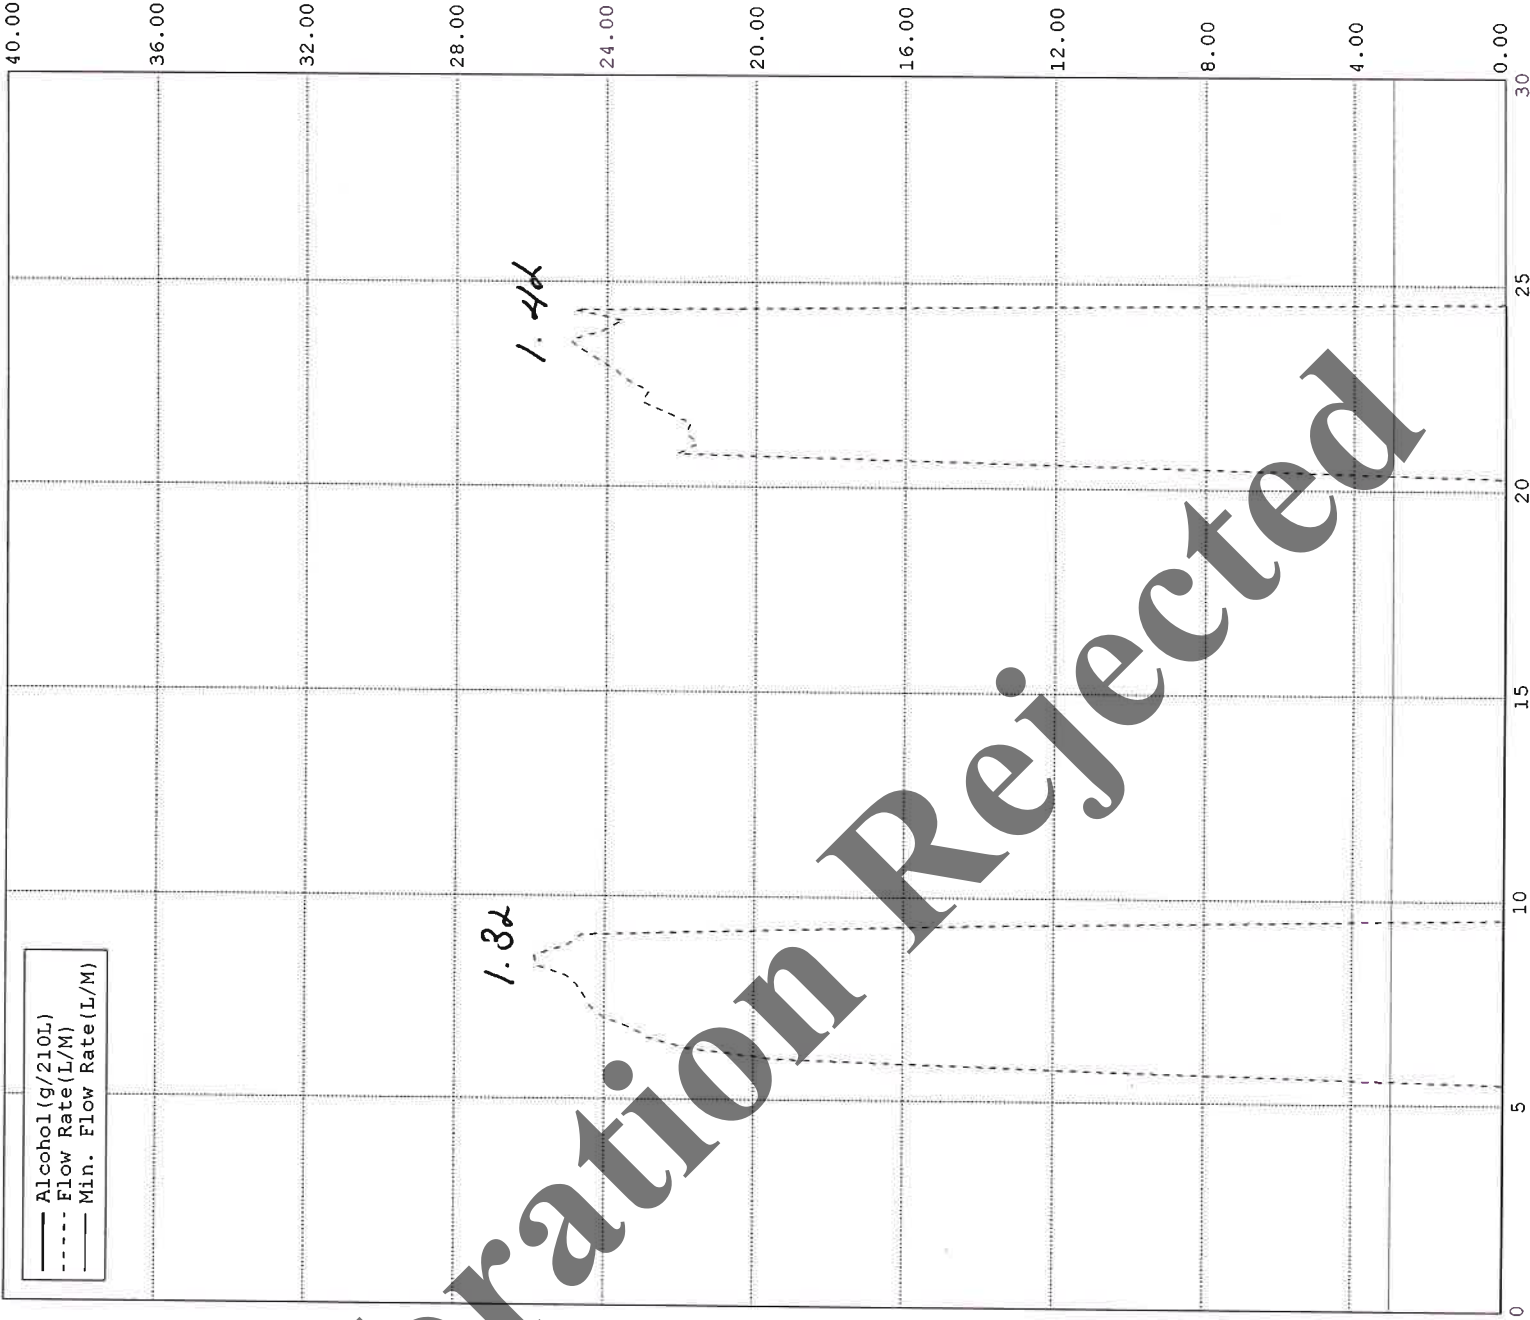

Calibration Rejected

LINEARITY CHECK


Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 07:42:17

SUPERVISOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0192	0.0004
0.039	0.0390	0.0000
0.078	0.0770	0.0000
0.098	0.0970	0.0000
0.147	0.1450	0.0000
0.293	0.2878	0.0004

SLOPE = 0.981995
R² = 0.999977

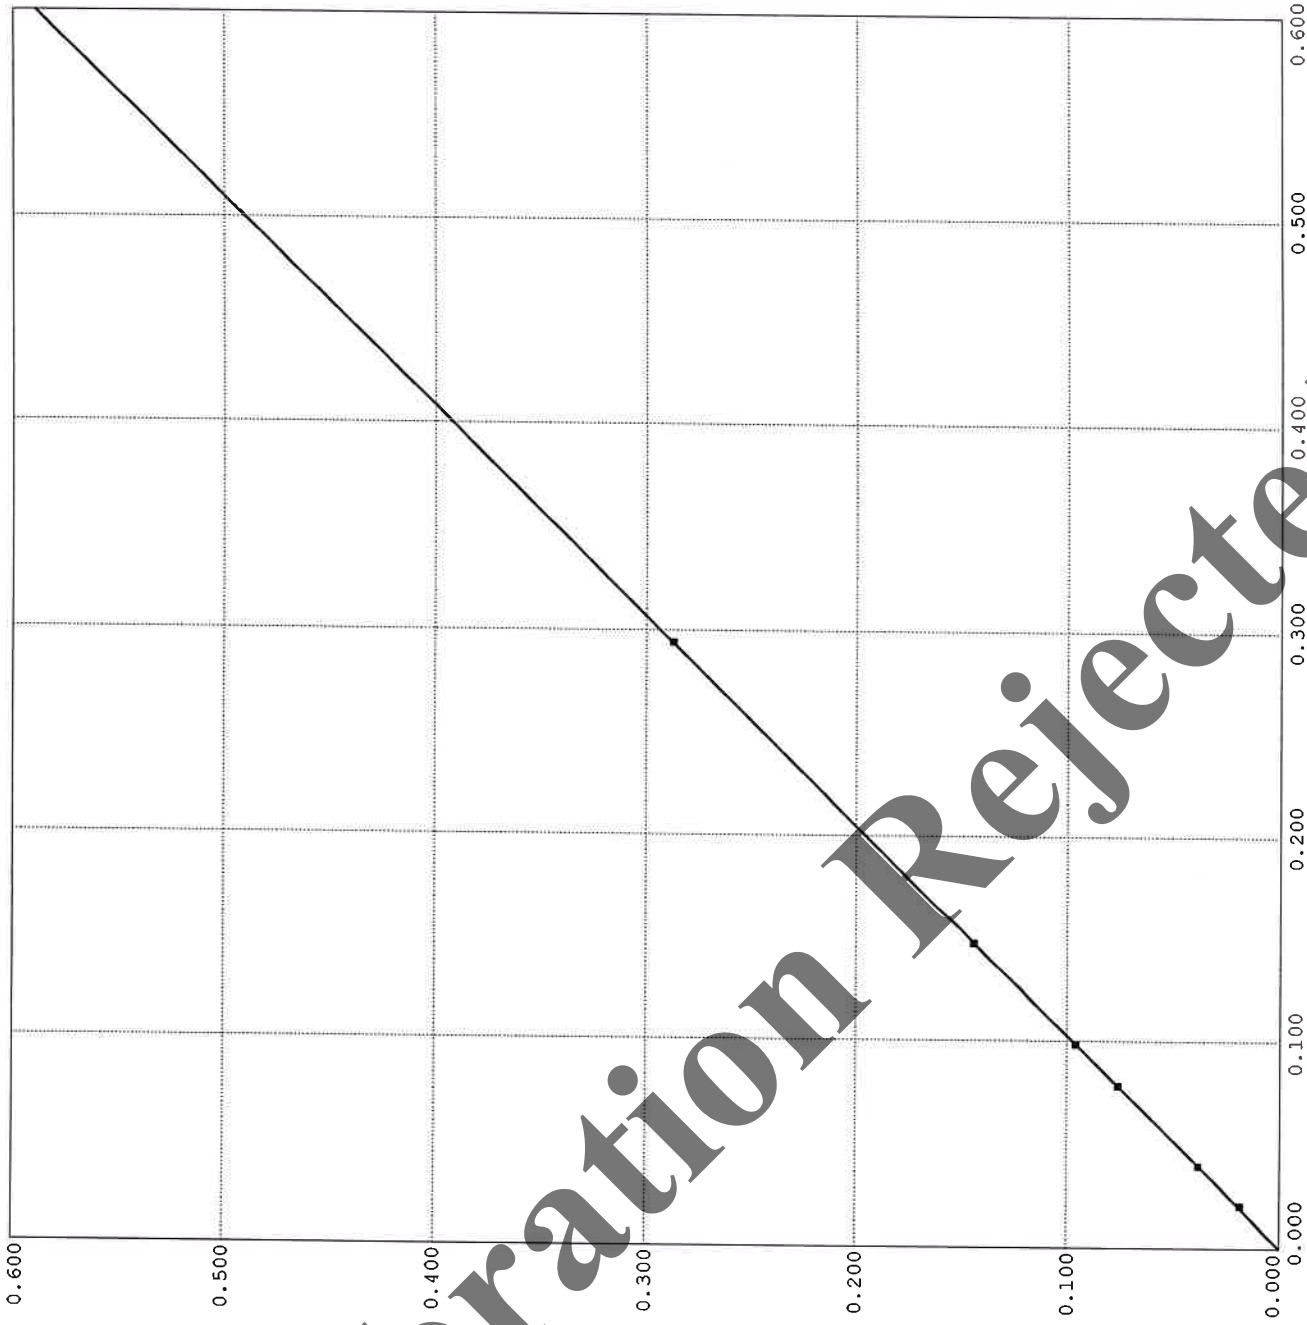

COB

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100682






Date: 01/05/2023
Time: 07:42:19

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.25: 0.020
LOT #: AG217902
EXPIRATION: 06/28/2024
TANK PRESSURE: 955 psi

BLANK TEST	0.000	07:50
INTERNAL STANDARD	VERIFIED	07:50
EXTERNAL STANDARD	0.020	07:50
BLANK TEST	0.000	07:51
EXTERNAL STANDARD	0.019	07:51
BLANK TEST	0.000	07:52
EXTERNAL STANDARD	0.019	07:52
BLANK TEST	0.000	07:53
EXTERNAL STANDARD	0.019	07:53
BLANK TEST	0.000	07:54
EXTERNAL STANDARD	0.019	07:54
BLANK TEST	0.000	07:55

Average = 0.0192
Std Dev = 0.0004

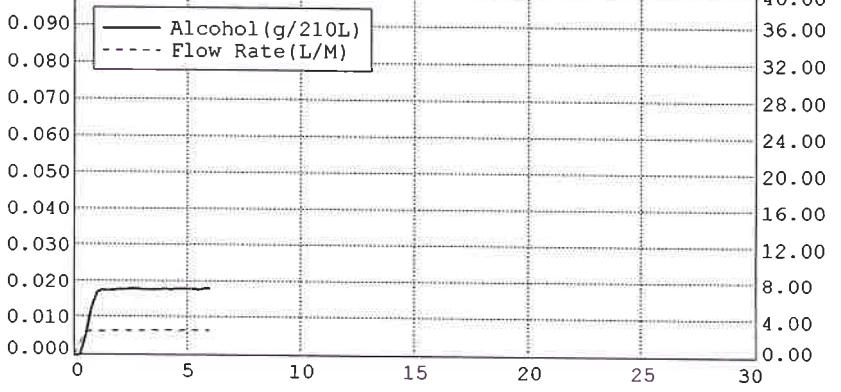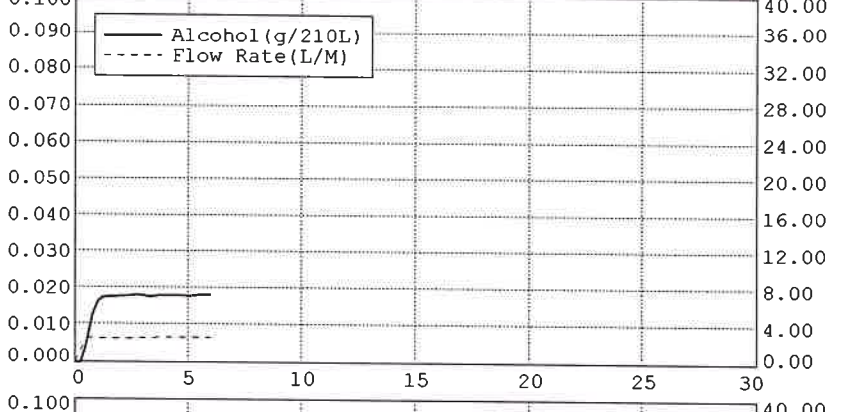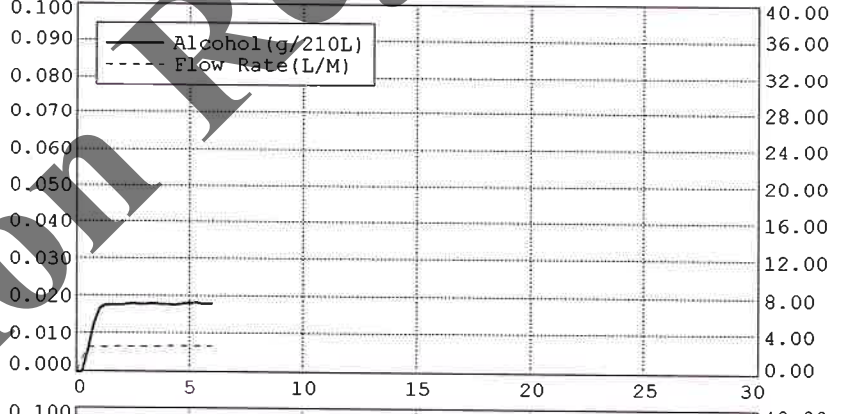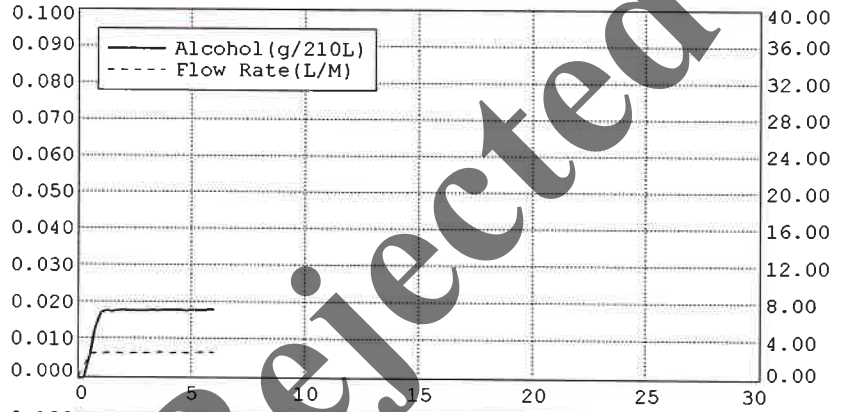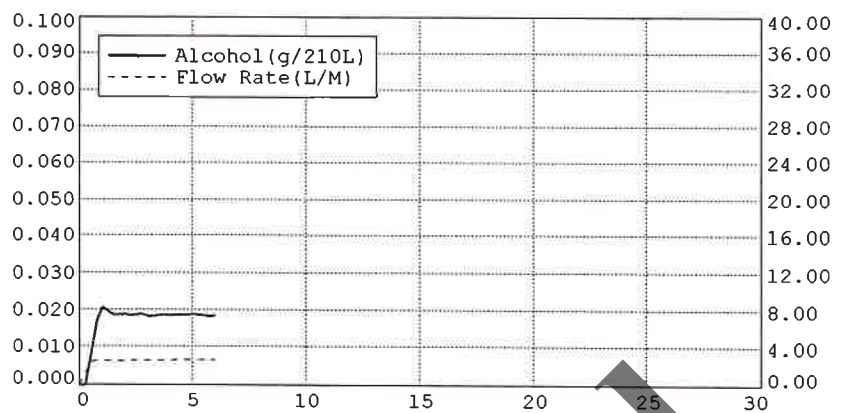

Calibration Rejected

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100682






Date: 01/05/2023
Time: 07:56:41

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.25: 0.039
LOT #: AG217904
EXPIRATION: 06/28/2024
TANK PRESSURE: 1025 psi

BLANK TEST	0.000	07:58
INTERNAL STANDARD	VERIFIED	07:58
EXTERNAL STANDARD	0.039	07:58
BLANK TEST	0.000	07:59
EXTERNAL STANDARD	0.039	07:59
BLANK TEST	0.000	08:00
EXTERNAL STANDARD	0.039	08:00
BLANK TEST	0.000	08:01
EXTERNAL STANDARD	0.039	08:01
BLANK TEST	0.000	08:02
EXTERNAL STANDARD	0.039	08:02
BLANK TEST	0.000	08:03

Average = 0.0390
Std Dev = 0.0000

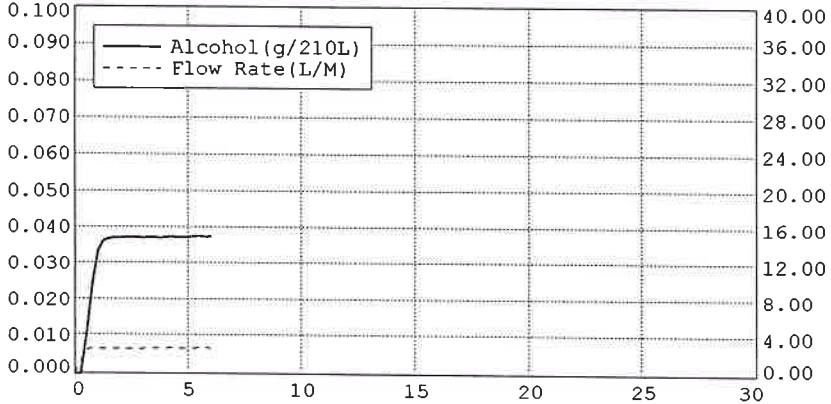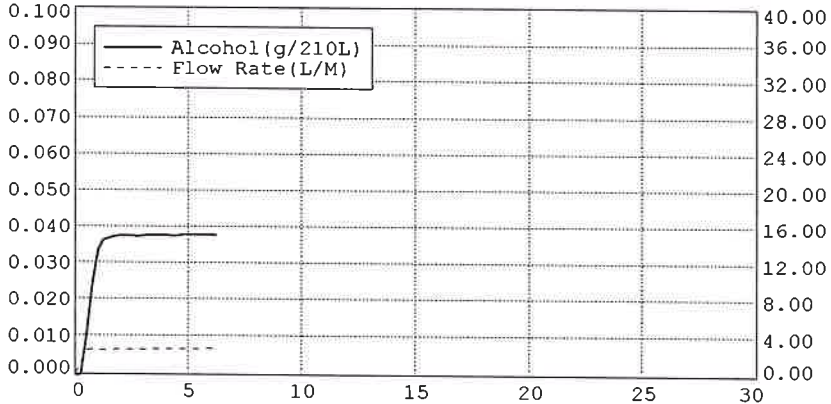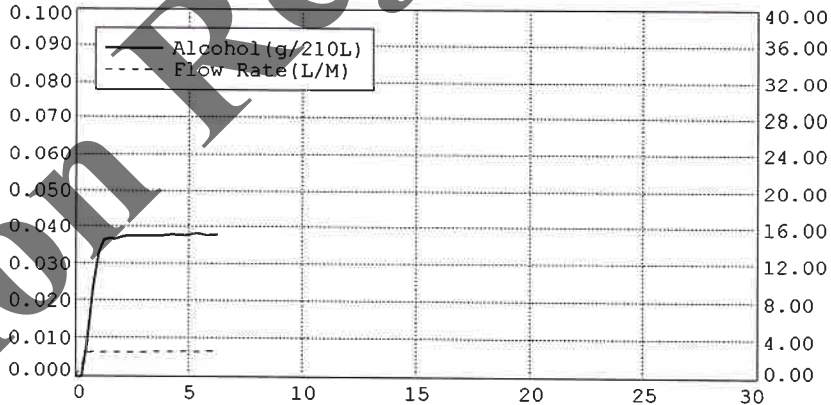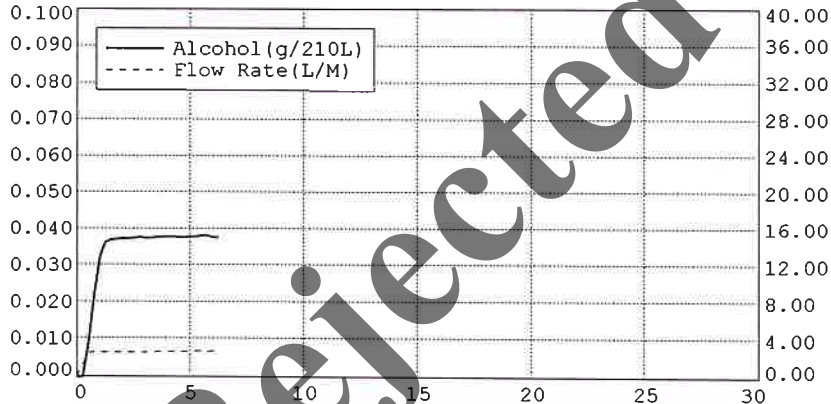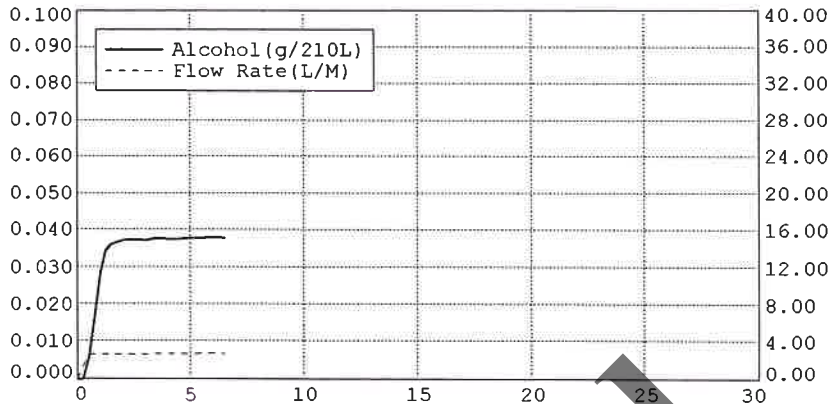

Calibration Rejected

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100682






Date: 01/05/2023
 Time: 08:05:50

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.25: 0.078
 LOT #: AG113402
 EXPIRATION: 05/14/2023
 TANK PRESSURE: 877 psi

BLANK TEST	0.000	08:06
INTERNAL STANDARD	VERIFIED	08:07
EXTERNAL STANDARD	0.077	08:07
BLANK TEST	0.000	08:08
EXTERNAL STANDARD	0.077	08:08
BLANK TEST	0.000	08:09
EXTERNAL STANDARD	0.077	08:09
BLANK TEST	0.000	08:10
EXTERNAL STANDARD	0.077	08:10
BLANK TEST	0.000	08:11
EXTERNAL STANDARD	0.077	08:11
BLANK TEST	0.000	08:12

Average = 0.0770
 Std Dev = 0.0000

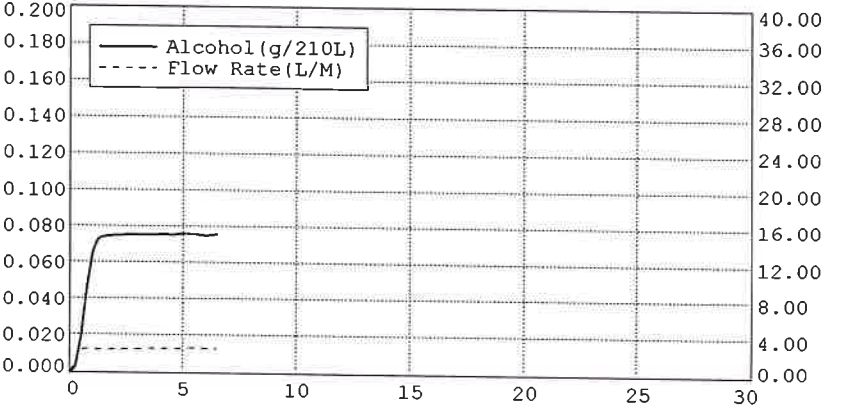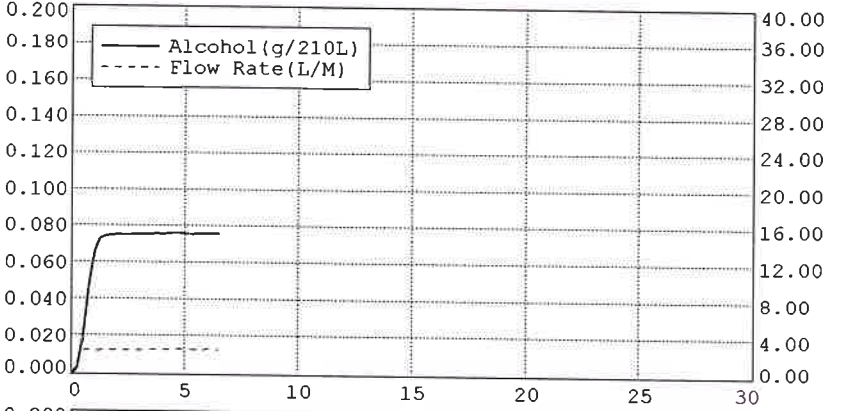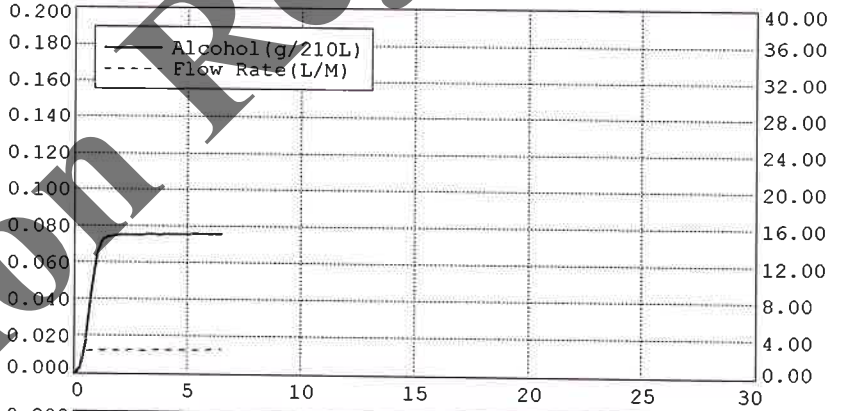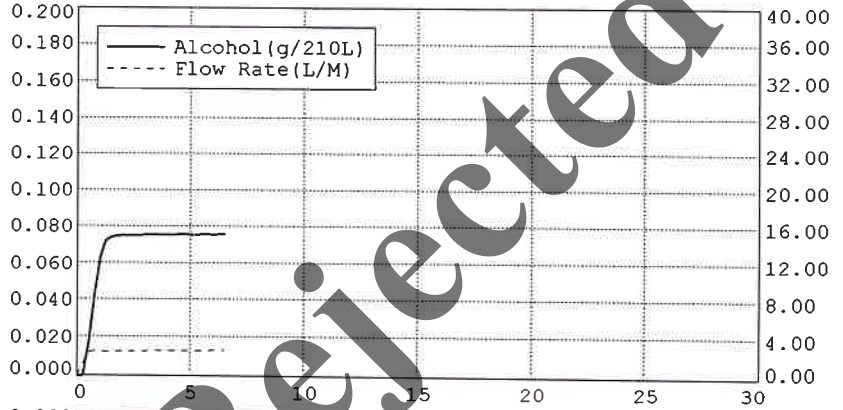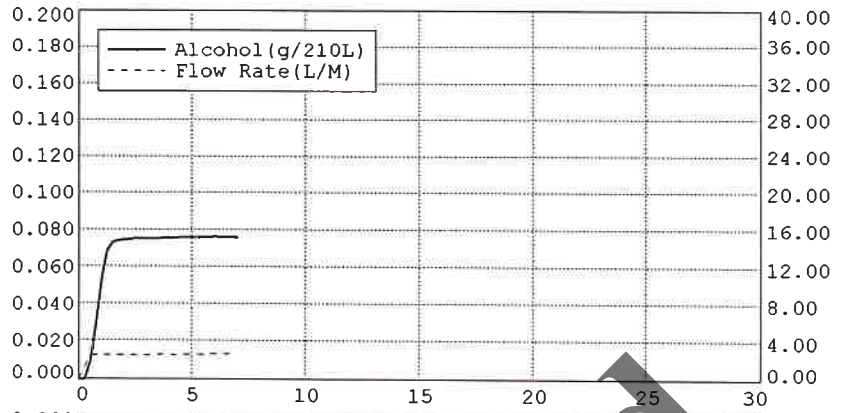

Calibration Rejected

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100682






Date: 01/05/2023
Time: 08:13:05

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.25: 0.098
LOT #: AG211003
EXPIRATION: 04/20/2024
TANK PRESSURE: 887 psi

BLANK TEST	0.000	08:14
INTERNAL STANDARD	VERIFIED	08:14
EXTERNAL STANDARD	0.097	08:14
BLANK TEST	0.000	08:15
EXTERNAL STANDARD	0.097	08:15
BLANK TEST	0.000	08:16
EXTERNAL STANDARD	0.097	08:16
BLANK TEST	0.000	08:17
EXTERNAL STANDARD	0.097	08:17
BLANK TEST	0.000	08:18
EXTERNAL STANDARD	0.097	08:19
BLANK TEST	0.000	08:19

Average = 0.0970
Std Dev = 0.0000

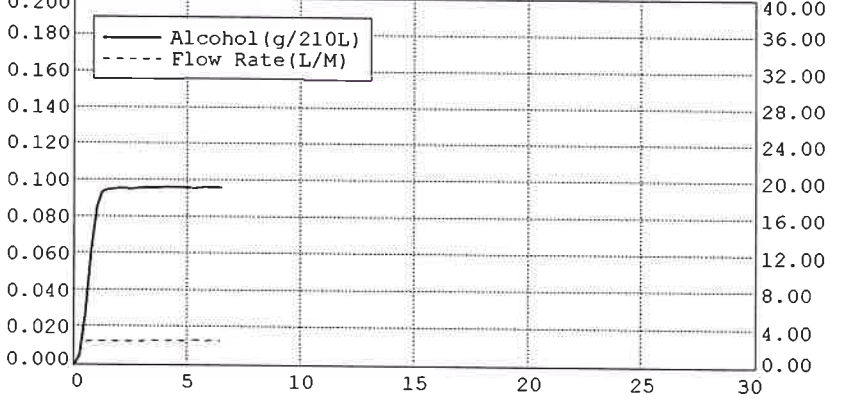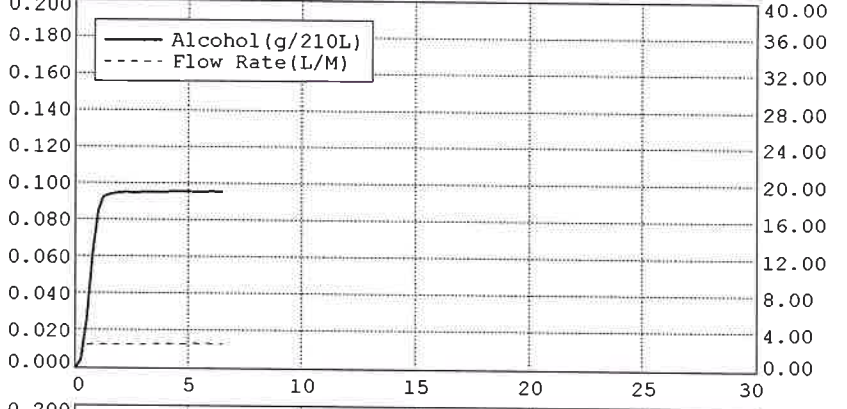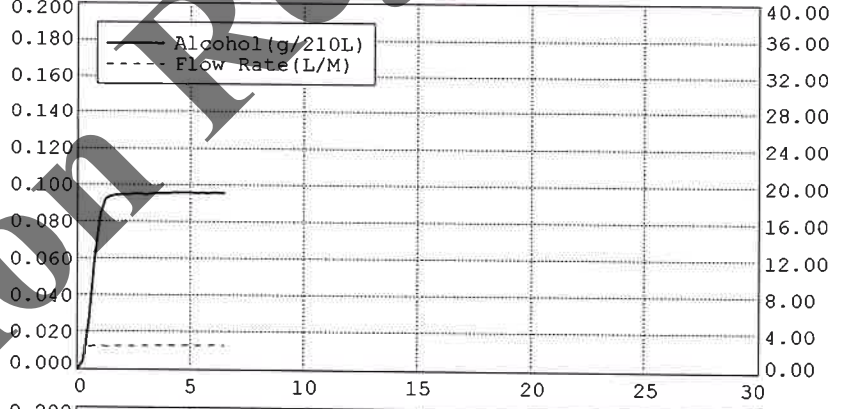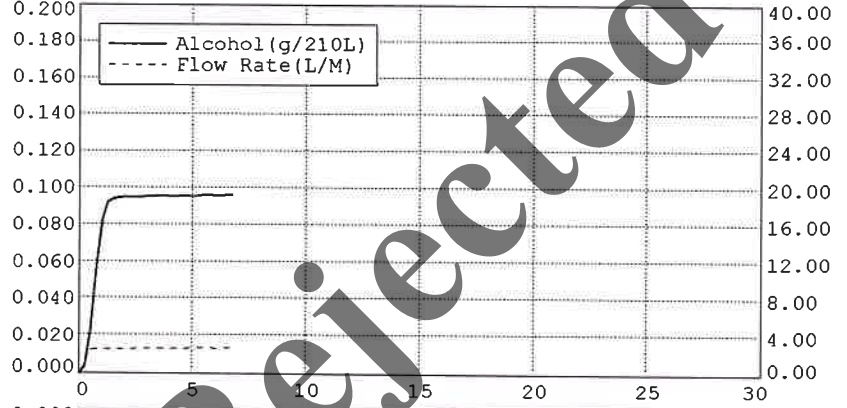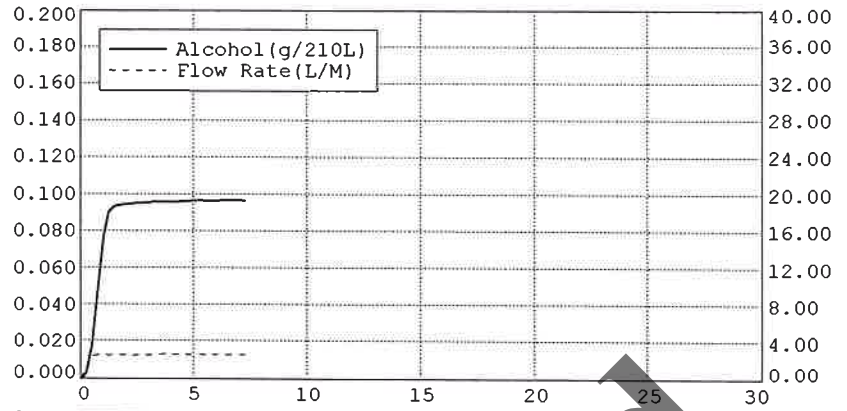

Calibration Rejected

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100682






Date: 01/05/2023
Time: 08:22:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.26: 0.147
LOT #: AG134205
EXPIRATION: 12/08/2023
TANK PRESSURE: 931 psi

BLANK TEST	0.000	08:23
INTERNAL STANDARD	VERIFIED	08:23
EXTERNAL STANDARD	0.145	08:23
BLANK TEST	0.000	08:24
EXTERNAL STANDARD	0.145	08:25
BLANK TEST	0.000	08:25
EXTERNAL STANDARD	0.145	08:26
BLANK TEST	0.000	08:27
EXTERNAL STANDARD	0.145	08:27
BLANK TEST	0.000	08:28
EXTERNAL STANDARD	0.145	08:28
BLANK TEST	0.000	08:29

Average = 0.1450
Std Dev = 0.0000

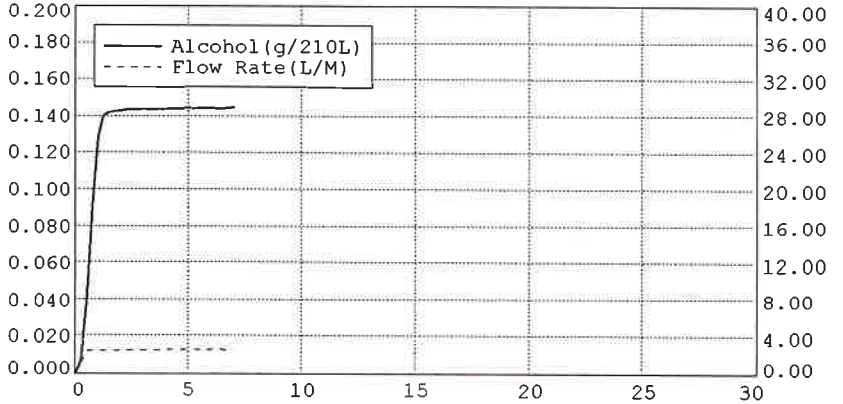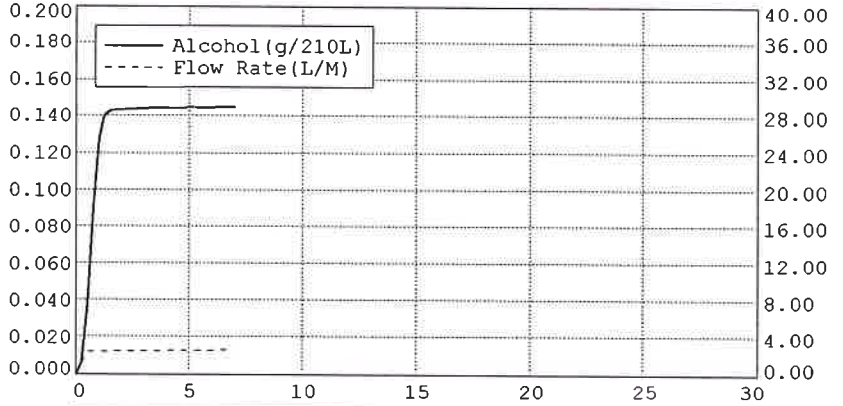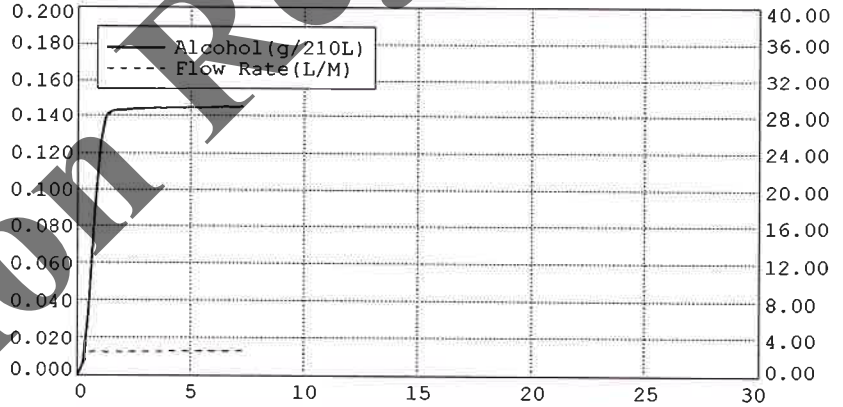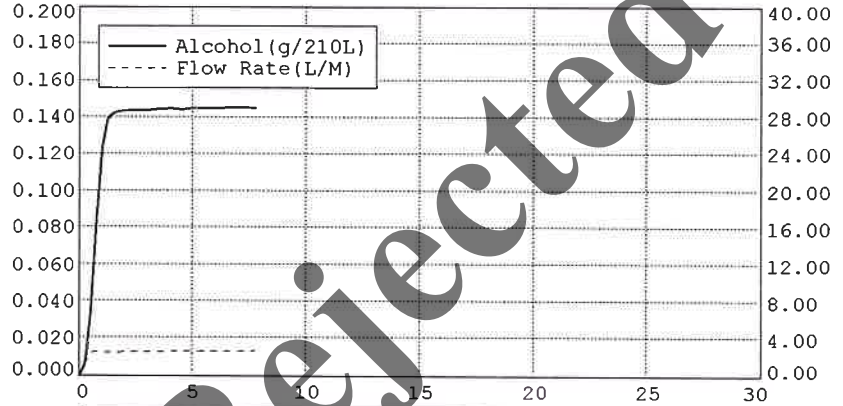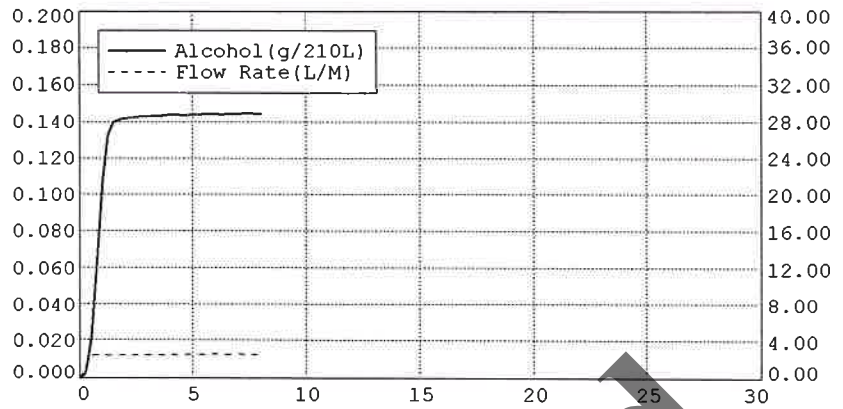

Calibration Rejected

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100682






Date: 01/05/2023
Time: 08:33:55

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.27: 0.293
LOT #: AG130502
EXPIRATION: 11/01/2023
TANK PRESSURE: 192 psi

BLANK TEST	0.000	08:35
INTERNAL STANDARD	VERIFIED	08:35
EXTERNAL STANDARD	0.288	08:35
BLANK TEST	0.000	08:36
EXTERNAL STANDARD	0.287	08:36
BLANK TEST	0.000	08:37
EXTERNAL STANDARD	0.288	08:37
BLANK TEST	0.000	08:38
EXTERNAL STANDARD	0.288	08:38
BLANK TEST	0.000	08:39
EXTERNAL STANDARD	0.288	08:40
BLANK TEST	0.000	08:41

Average = 0.2878
Std Dev = 0.0004

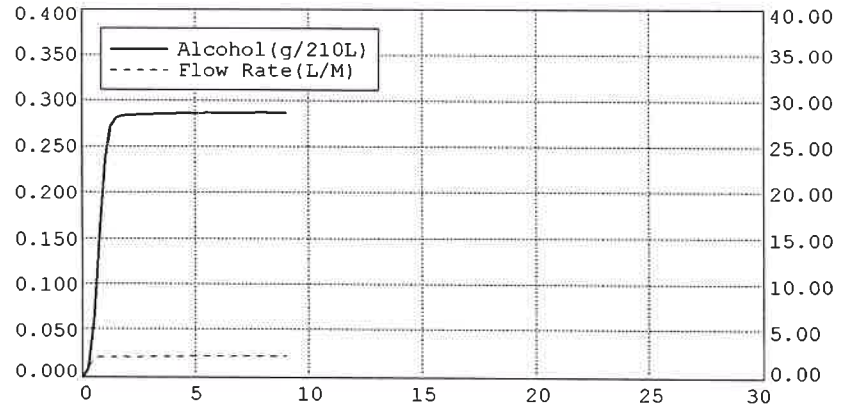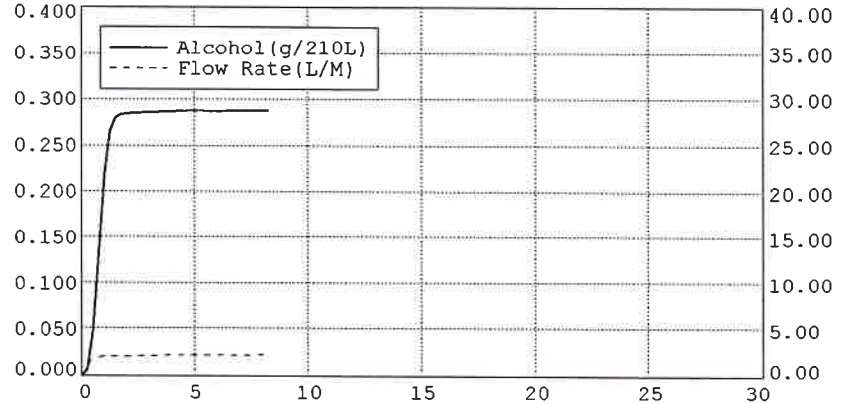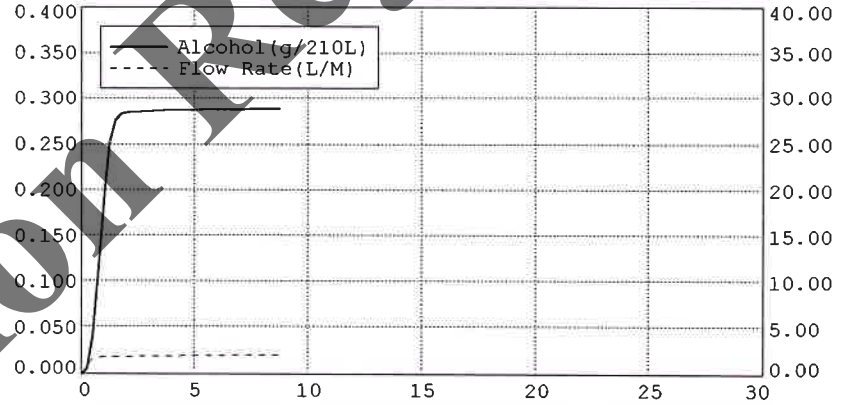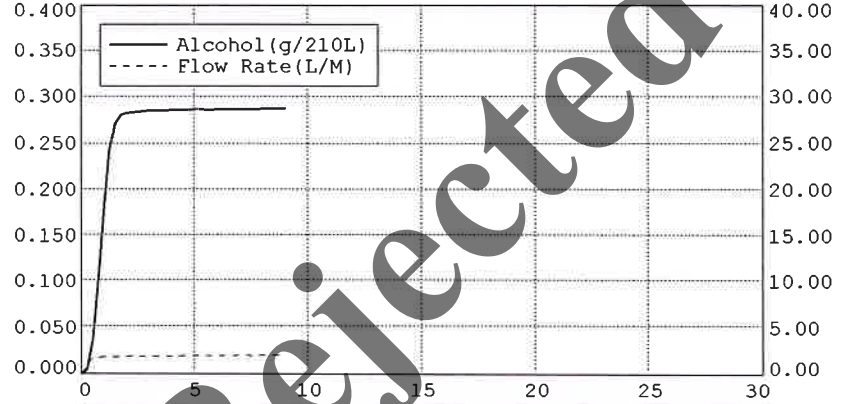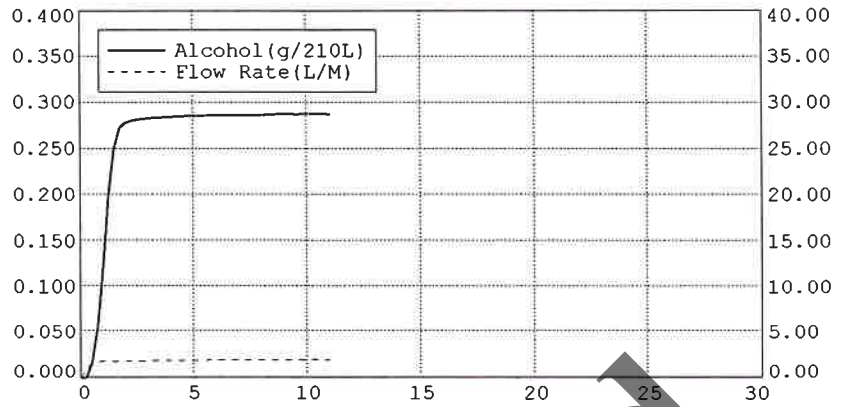

Calibration Rejected

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 09:01:32


SUBJECT NAME:
TEST TEST
LICENSE #: INCOMPLETE

OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK PASSED 09:08
BLANK TEST 0.000 09:08
INTERNAL STANDARD VERIFIED 09:09
EXTERNAL STANDARD 0.078 09:09
BLANK TEST 0.000 09:10
SUBJECT SAMPLE INCOMPLETE 09:12

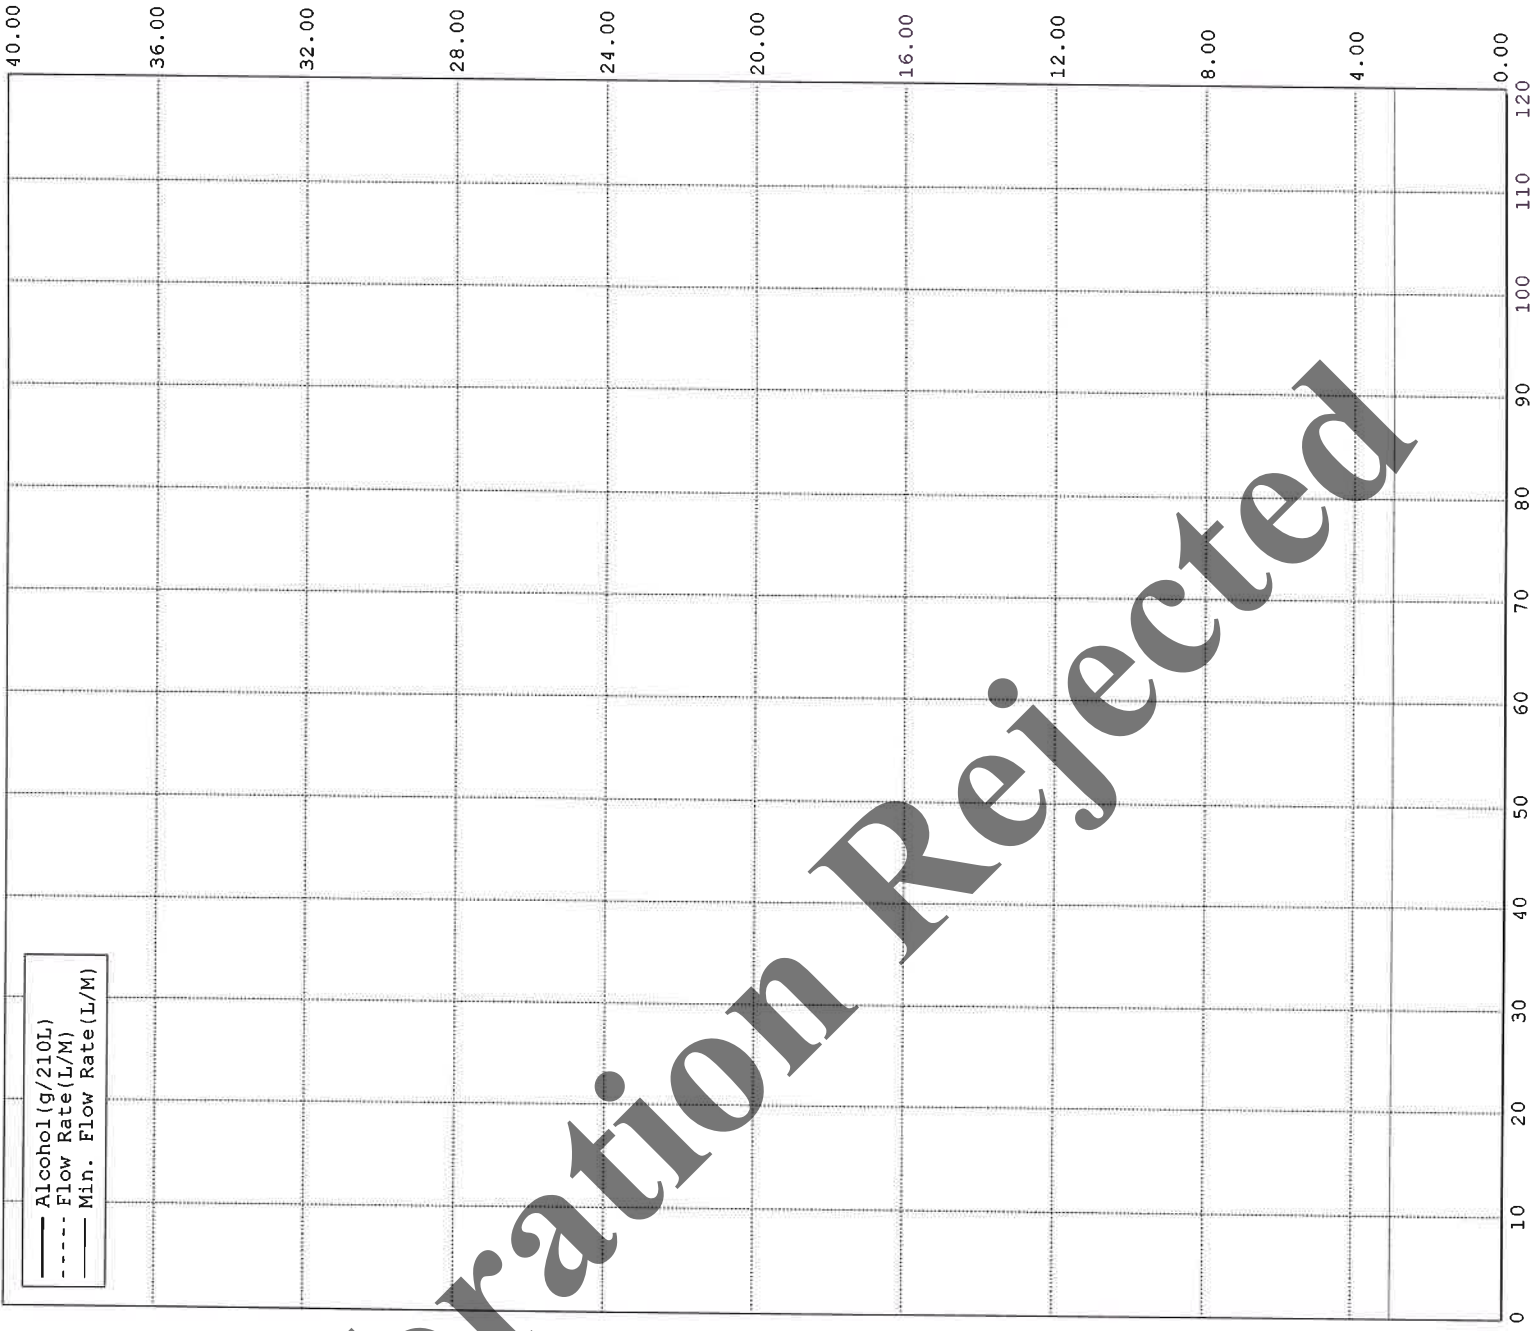

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 09:31:54

SUBJECT NAME:
TEST TEST
LICENSE #: INVALID

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1


CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.28: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:33
BLANK TEST	0.000	09:33
INTERNAL STANDARD	VERIFIED	09:33
EXTERNAL STANDARD	0.077	09:33
BLANK TEST	0.000	09:34
SUBJECT SAMPLE	INVALID	09:35

Calibration Rejected

Alcohol (g/210L)
Flow Rate (L/M)
Min. Flow Rate (L/M)

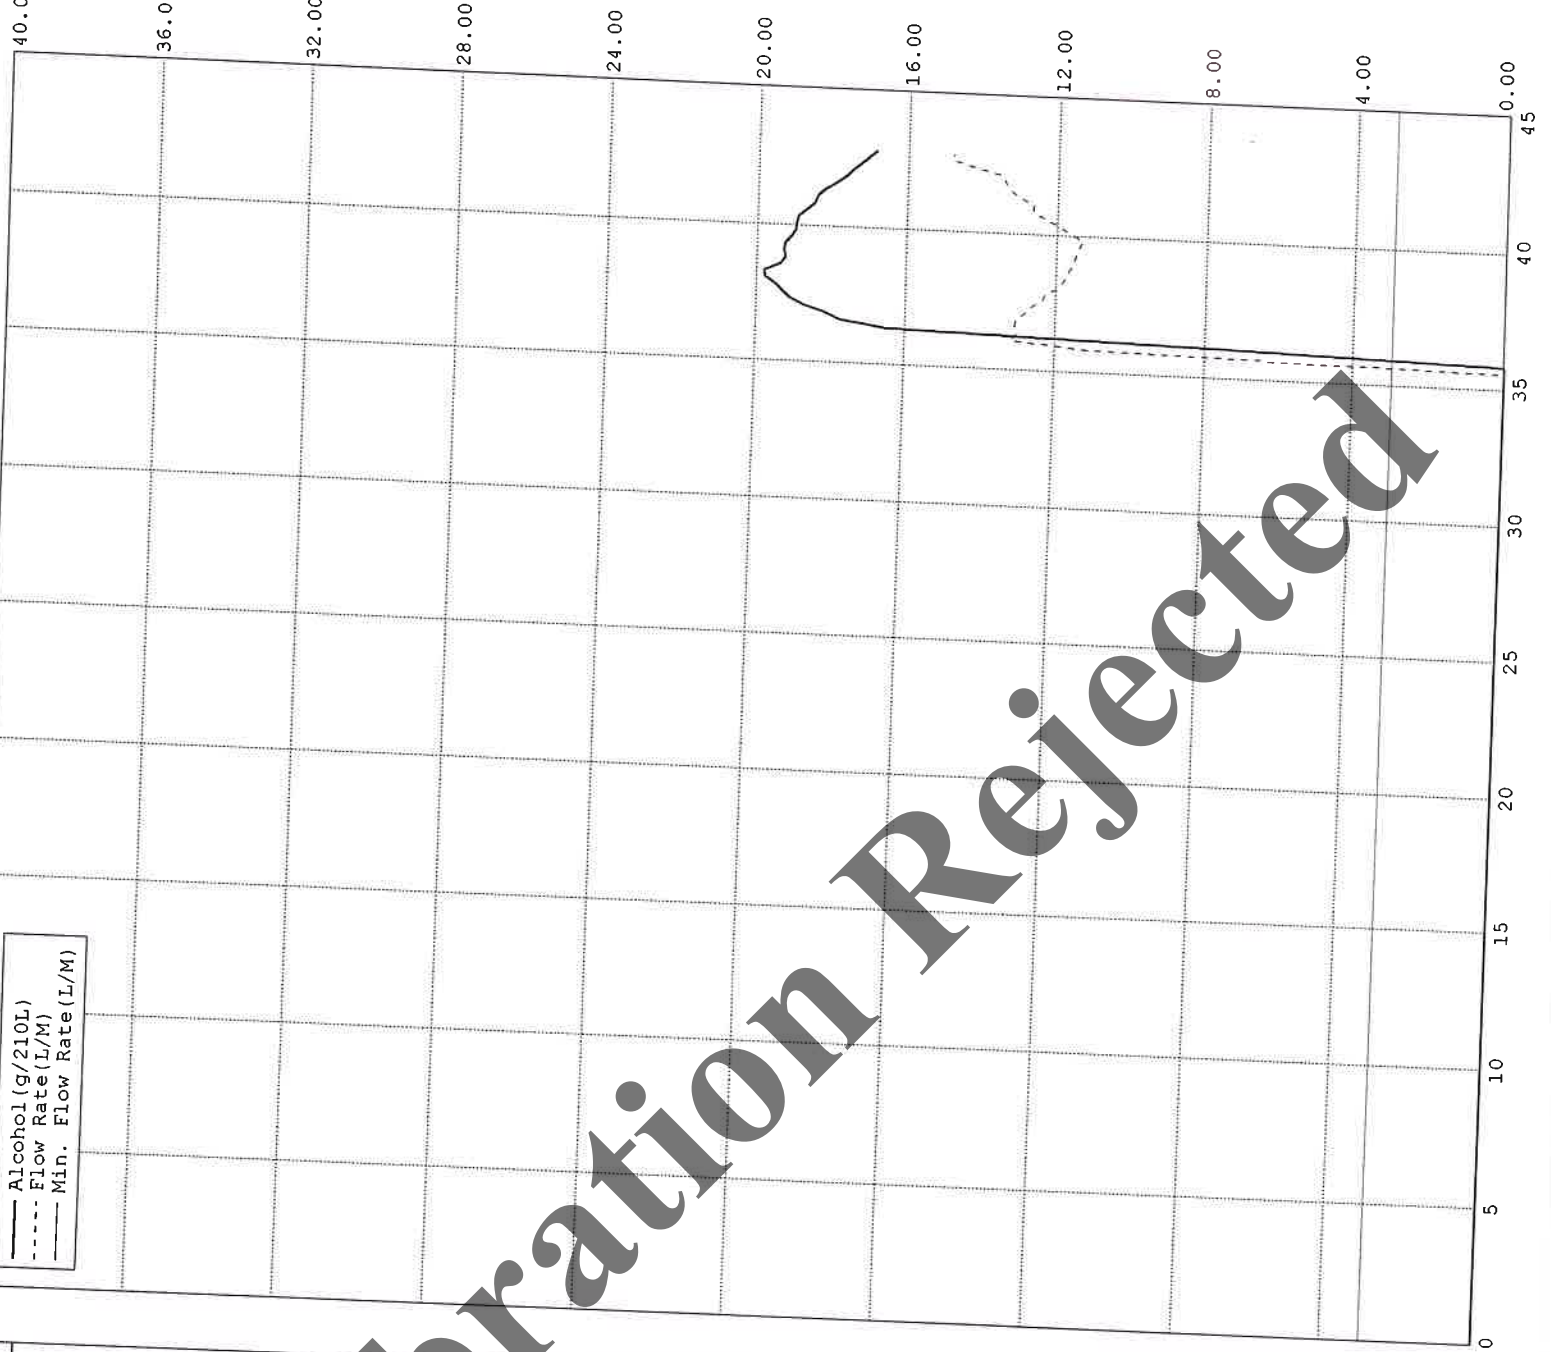

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 09:25:09

SUBJECT NAME:
TEST TEST
LICENSE #: MAX ATTEMPTS

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1

CASE/REPORT: 23-1234
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:26
BLANK TEST	0.000	09:26
INTERNAL STANDARD	VERIFIED	09:26
EXTERNAL STANDARD	0.078	09:26
BLANK TEST	0.000	09:27
SUBJECT SAMPLE	XXX	09:28

Maximum Attempts Exceeded

CS

Calibration Rejected

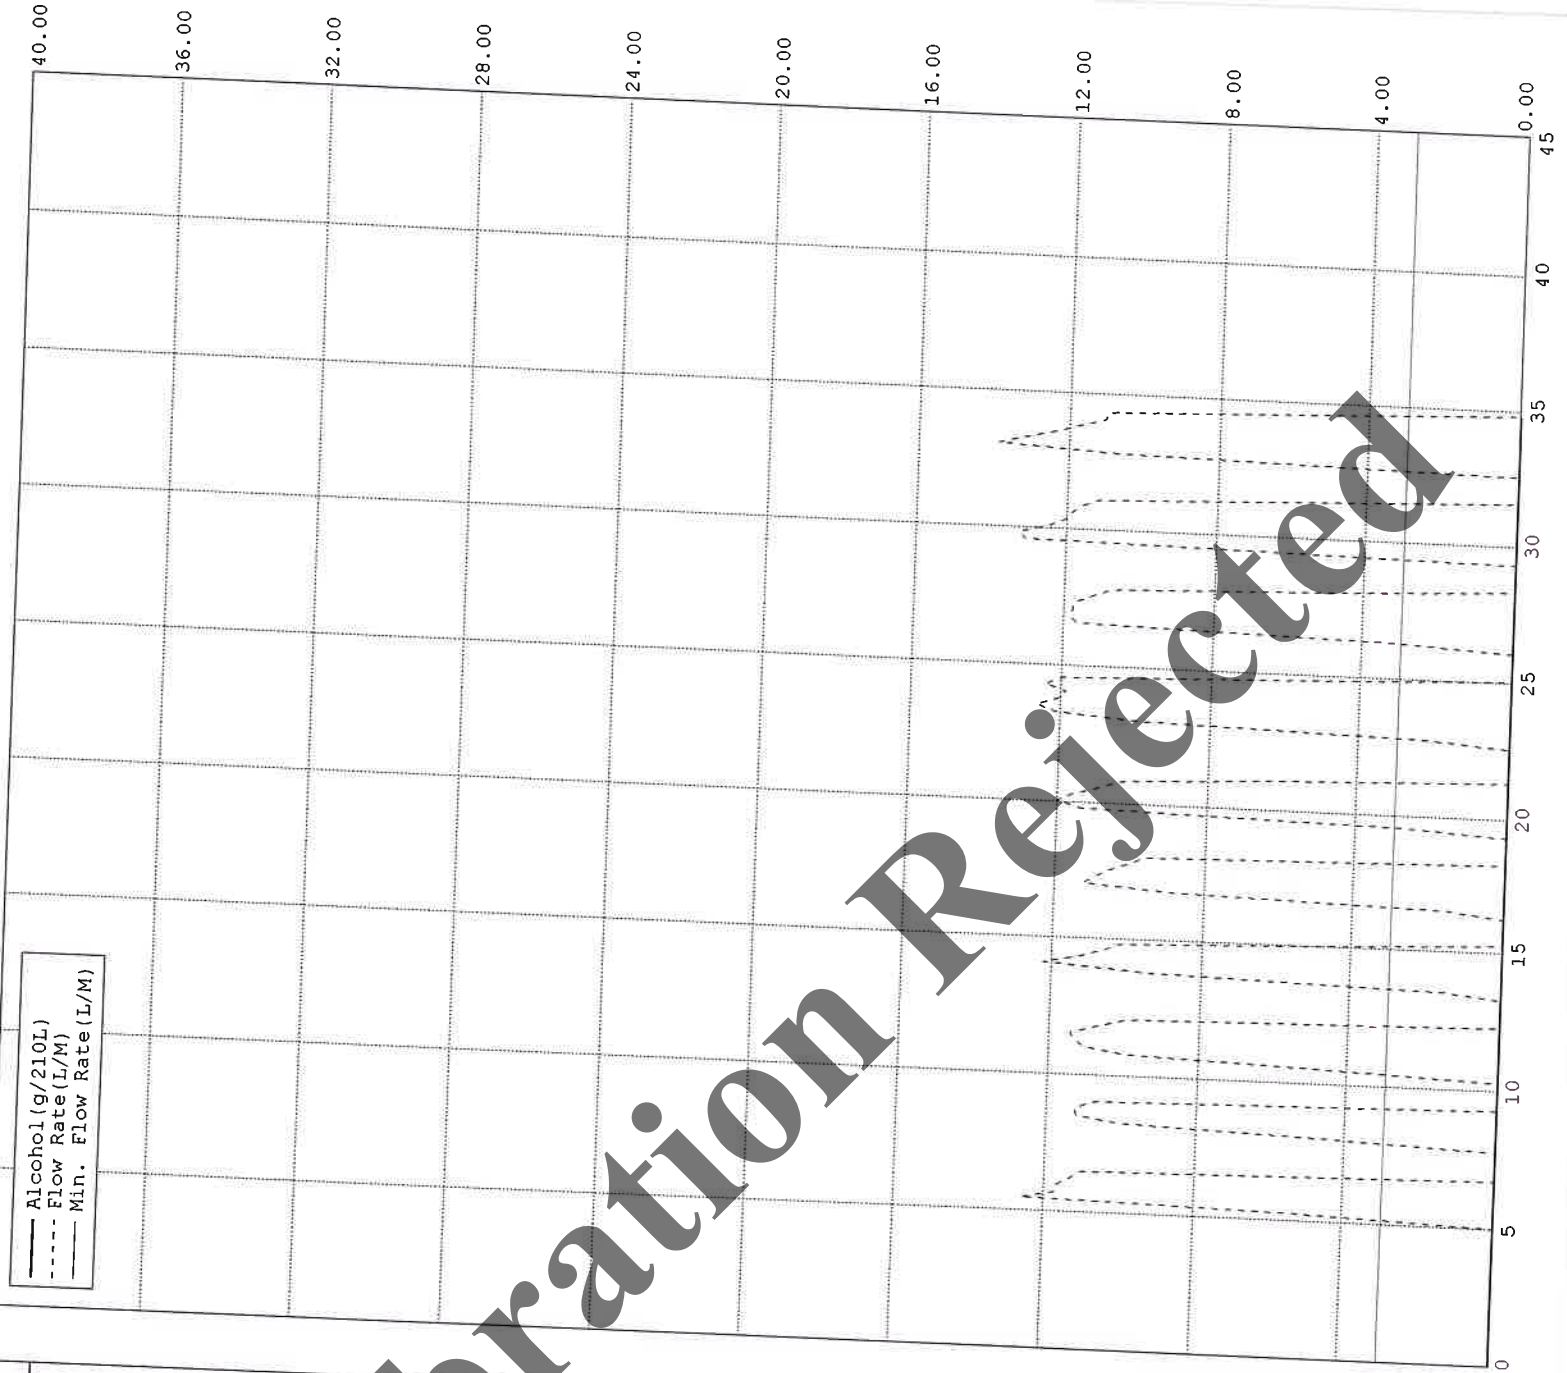

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 09:15:46

SUBJECT NAME:
TEST TEST
LICENSE #: RFI

OPERATOR NAME:
COLLEEN S OBYRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1

CASE/REPORT: 23-1234
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK PASSED 09:19
BLANK TEST 0.000 09:19
INTERNAL STANDARD VERIFIED 09:19
EXTERNAL STANDARD 0.077 09:20
BLANK TEST 0.000 09:21

RFI DETECTED

CRB

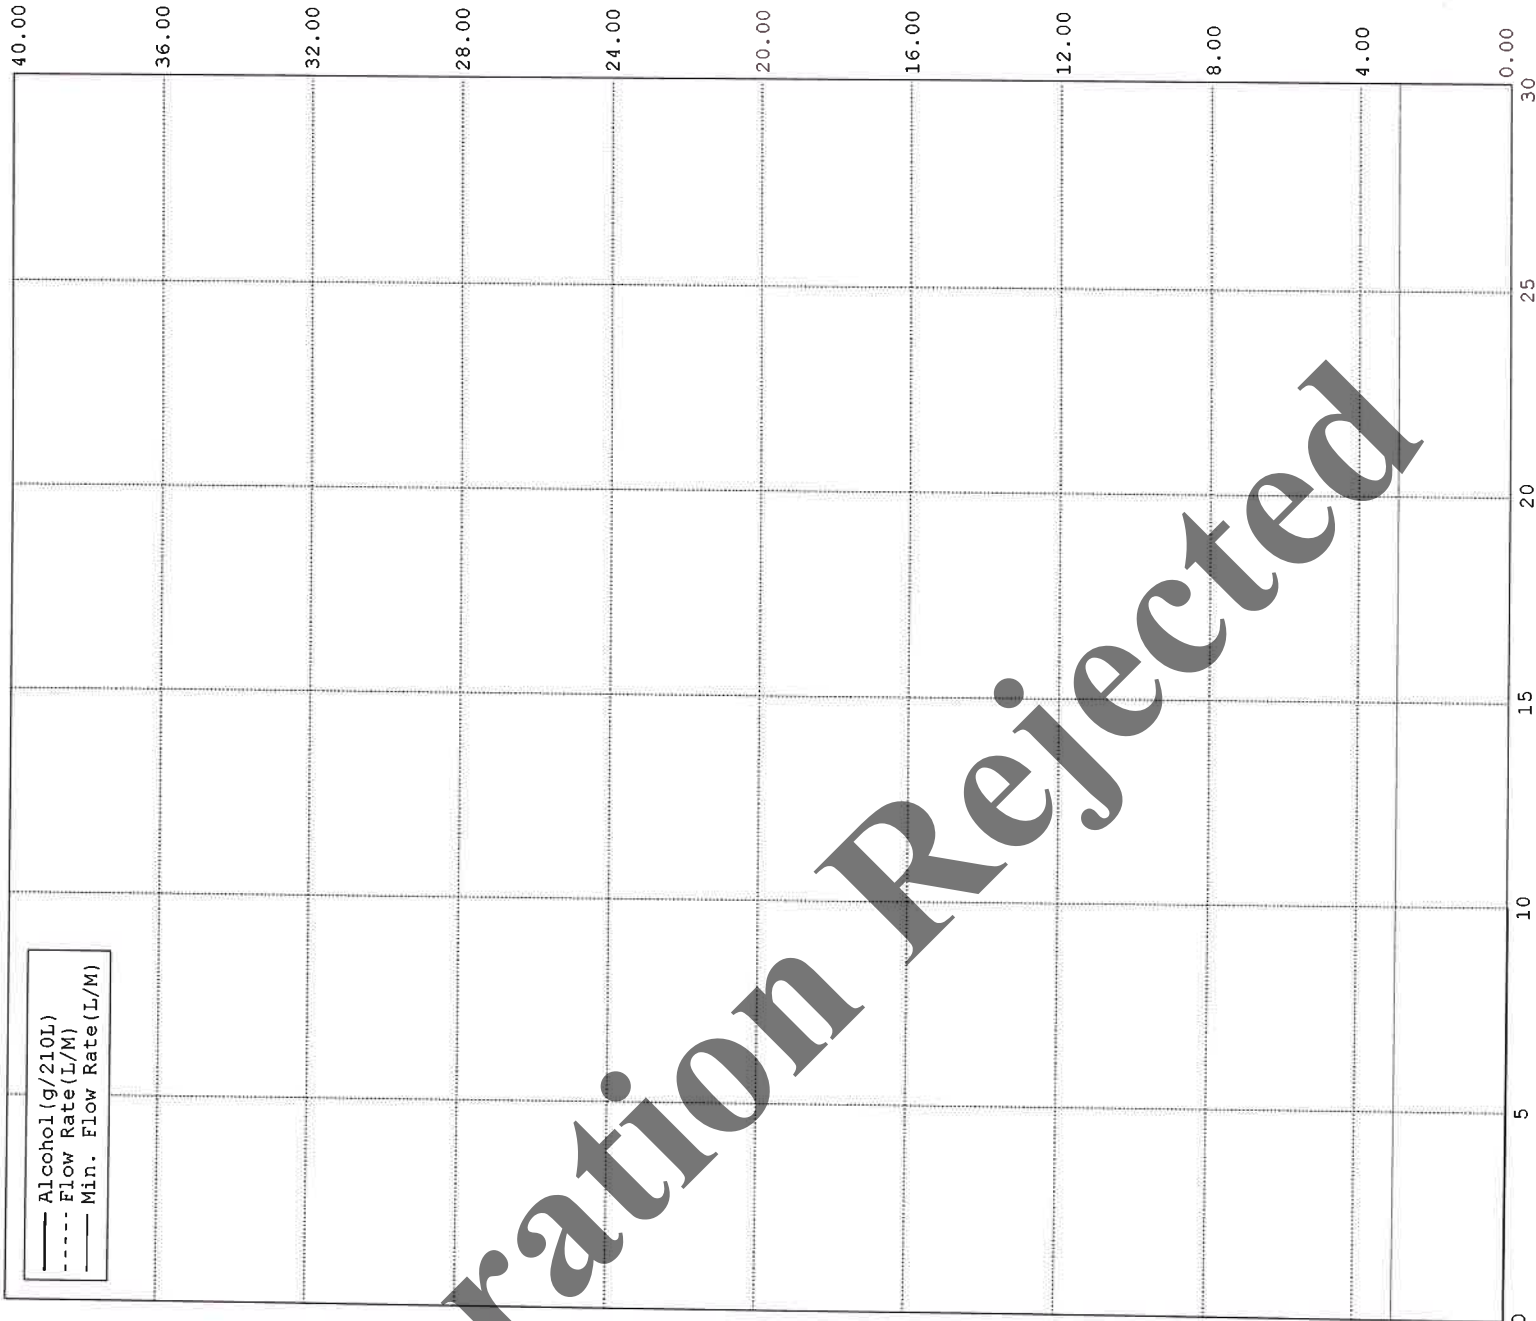

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 09:41:46

SUBJECT NAME:
TEST TEST
LICENSE #: INT-ACETONE
OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1

CASE/REPORT: 23-1234
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.28: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:42
BLANK TEST	0.000	09:42
INTERNAL STANDARD	VERIFIED	09:43
Xq = 0.093 (0.768)		
EXTERNAL STANDARD	0.077	09:43
X[1] = 0.0765 (-0.0011) (0.0036)		
BLANK TEST	0.000	09:44
SUBJECT SAMPLE	xxx	09:44
X[1] = 0.1085 (-0.0156) (0.0021)		

Interference Detected

003

Alcohol (g/210L)
Flow Rate (L/M)
Min. Flow Rate (L/M)

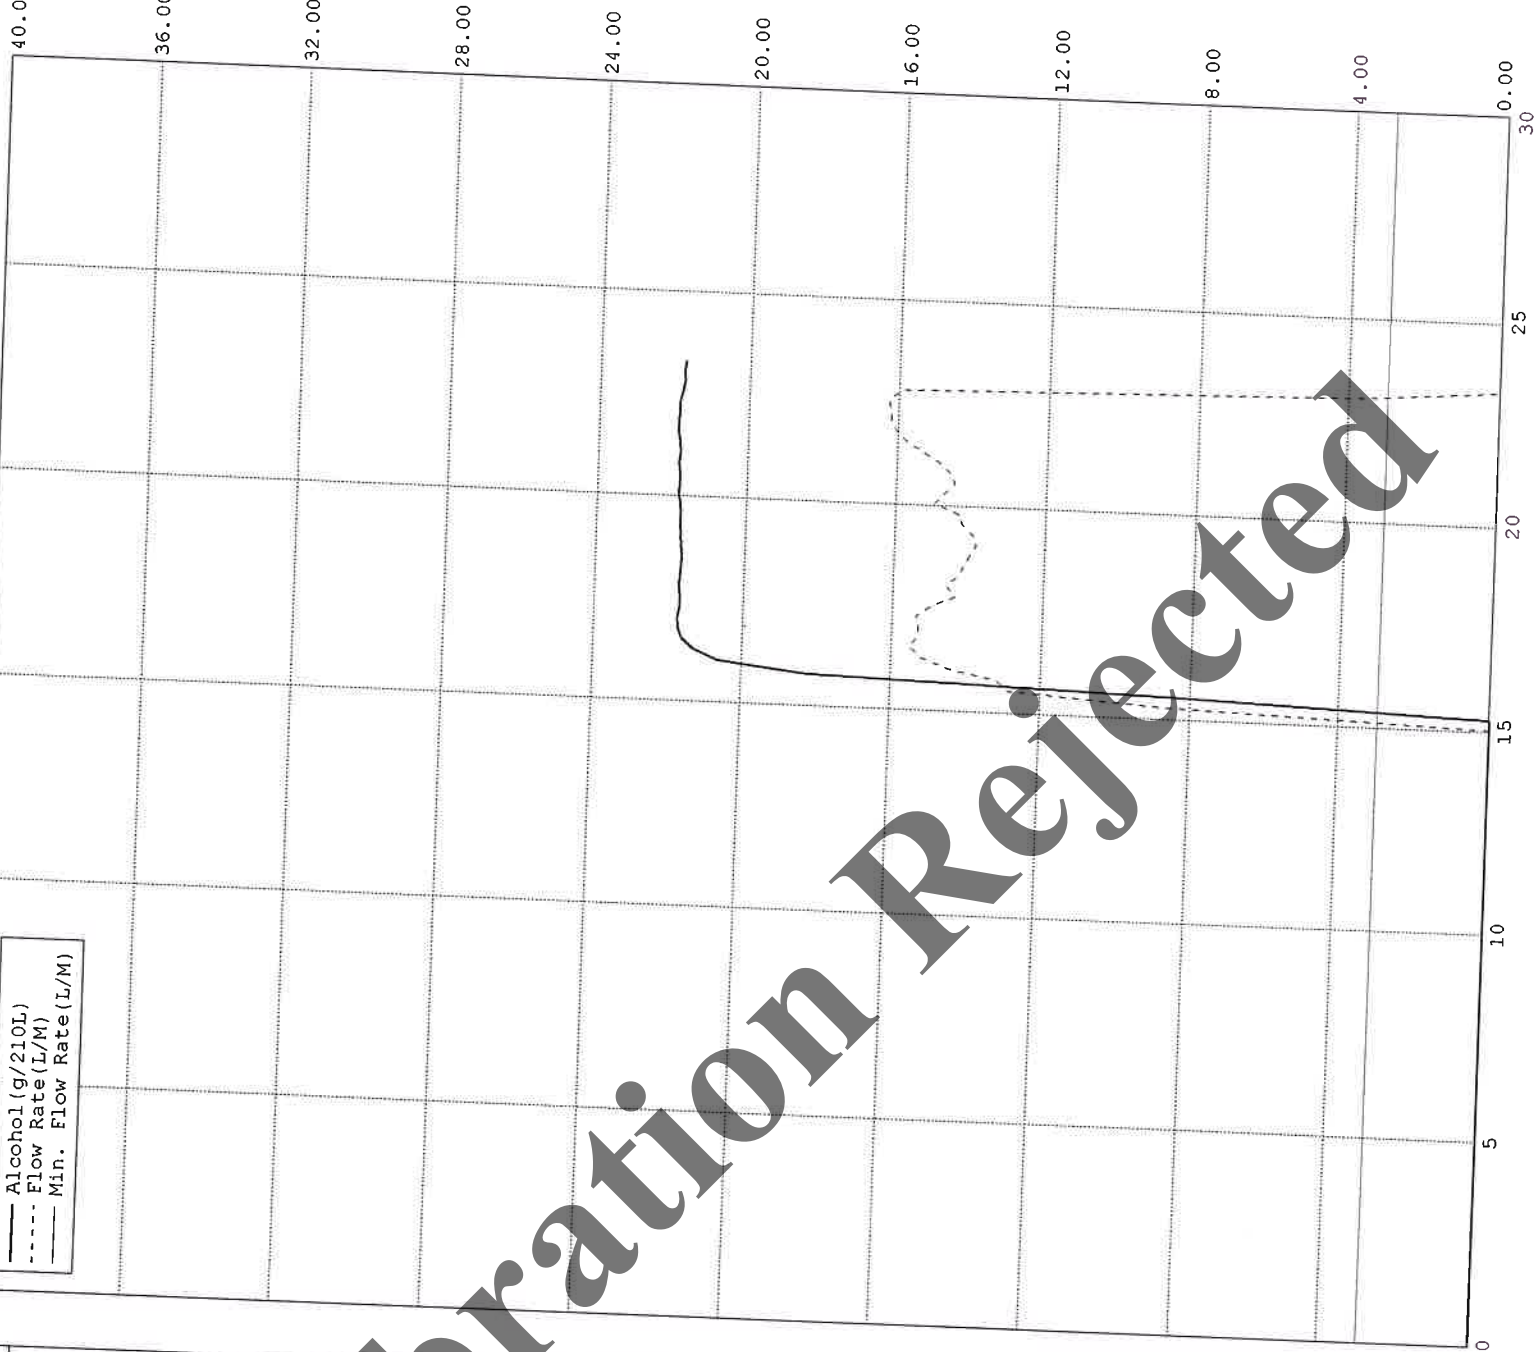

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 09:47:24

SUBJECT NAME:
TEST TEST
LICENSE #: INT-IPA

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:48
BLANK TEST	0.000	09:48
INTERNAL STANDARD	VERIFIED	09:48
Xq = 0.093 (0.85%)	0.077	09:49
EXTERNAL STANDARD	X[1] = 0.0770 (-0.0006)	(0.0033)
BLANK TEST	0.000	09:50
SUBJECT SAMPLE	XXX	09:50
X[1] = 0.1130 (-0.0178)	(0.0017)	

Interference Detected



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 09:53:39

SUBJECT NAME:
TEST TEST
LICENSE #: INT-NEGATIVE
OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.28: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023


DIAGNOSTIC CHECK	PASSED	09:54
INTERNAL STANDARD	0.000	09:54
INTERNAL STANDARD	VERIFIED	09:54
Xq = 0.094 (1.51%)		
EXTERNAL STANDARD	0.077	09:55
X[1] = 0.0769 (-0.0007)	(0.0027)	
BLANK TEST	0.000	09:56
SUBJECT SAMPLE (Vol=1.94L)	0.093	09:56
X[1] = 0.0937 (-0.0001)	(0.0010)	
BLANK TEST	0.000	09:57
EXTERNAL STANDARD	0.076	09:58
X[1] = 0.0763 (-0.0013)	(0.0023)	
BLANK TEST	0.000	09:58

Filter 2 Average = -0.0009
Filter 3 Average = 0.0030

CO3

Calibration Rejected

Alcohol (g/210L)
Flow Rate (L/M)
Min. Flow Rate (L/M)

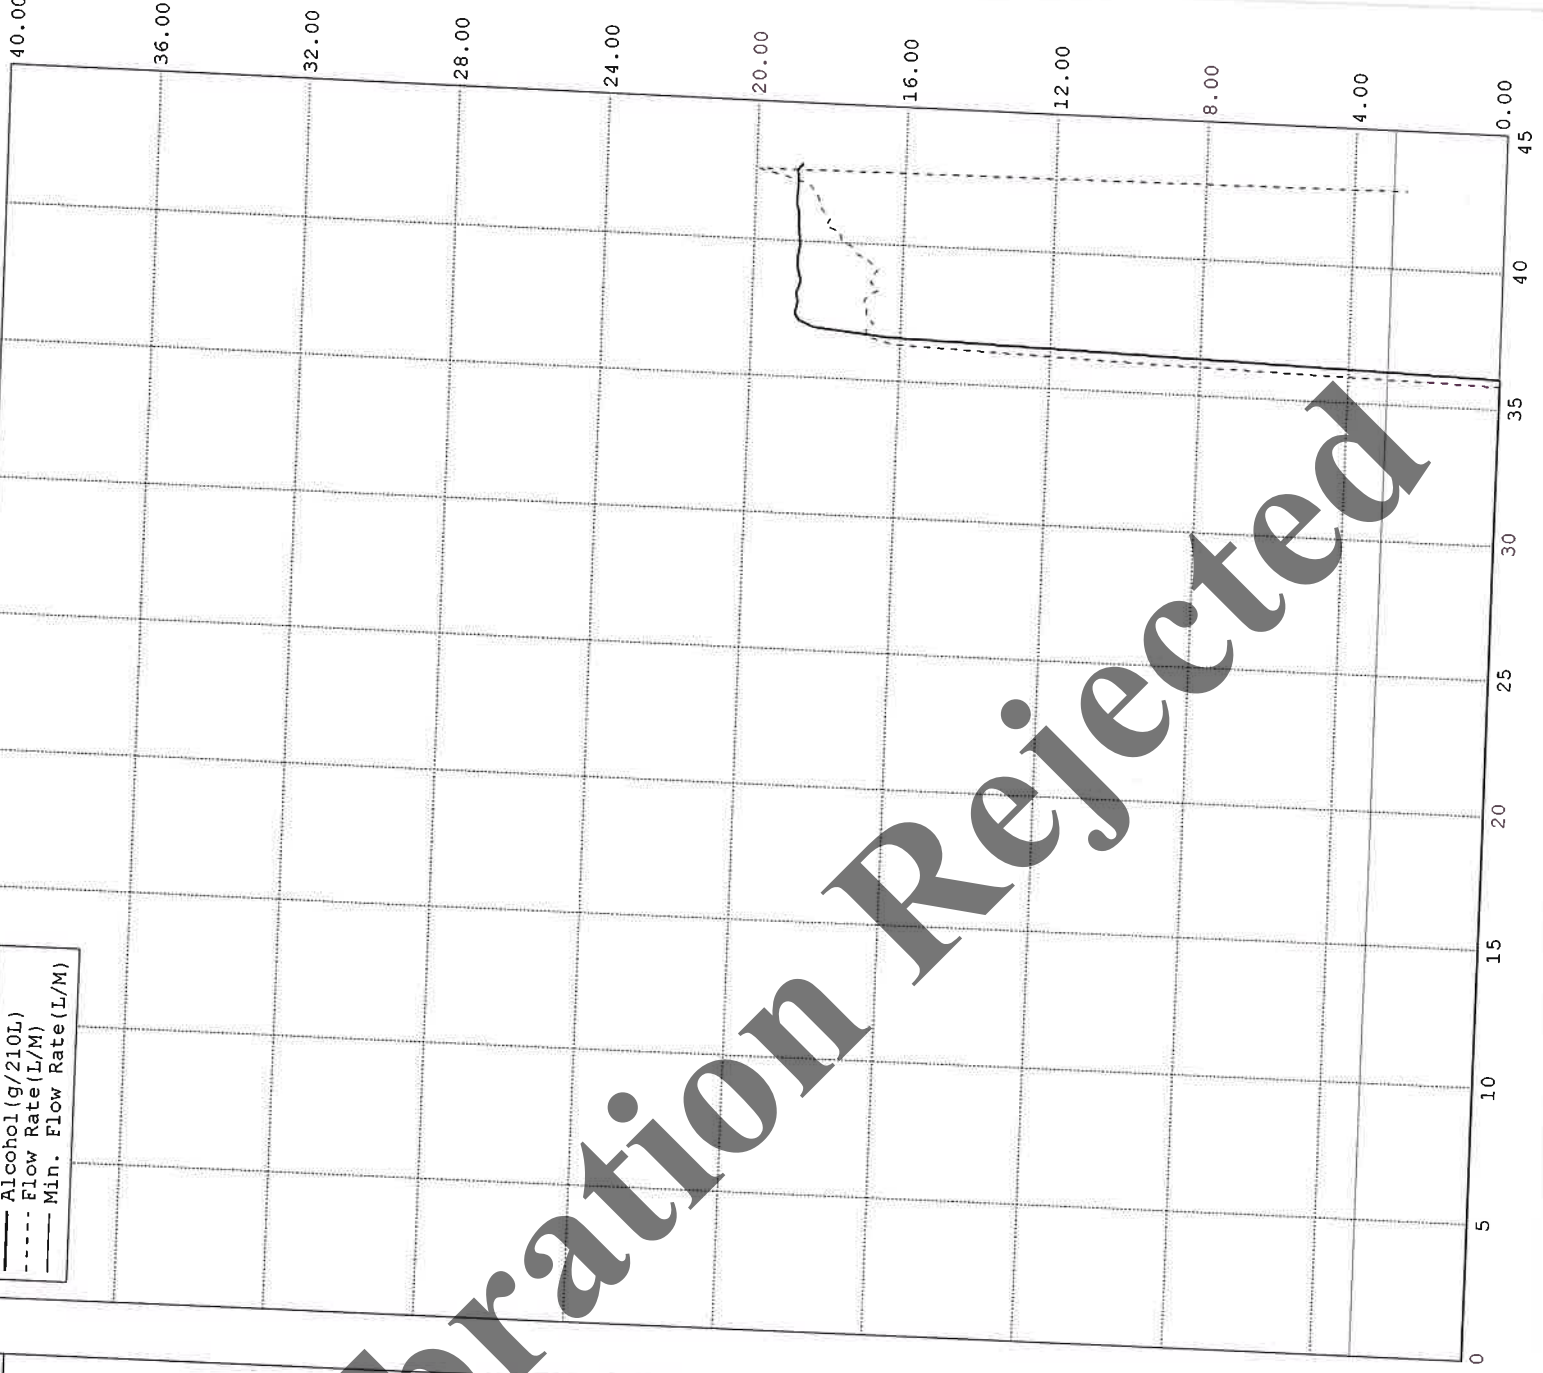

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 10:11:30

SUBJECT NAME:
TEST TEST
LICENSE #: NON-DRINKING

OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:12
BLANK TEST	0.000	10:12
INTERNAL STANDARD	VERIFIED	10:12
EXTERNAL STANDARD	0.077	10:12
BLANK TEST	0.000	10:13
SUBJECT SAMPLE (Vol=1.59L)	0.000	10:14
BLANK TEST	0.000	10:15
EXTERNAL STANDARD	0.077	10:15
BLANK TEST	0.000	10:16

Calibration Rejected

Alcohol (g/210L)
Flow Rate (L/M)
Min. Flow Rate (L/M)



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100682

Date: 01/05/2023
Time: 10:11:30

SUBJECT NAME:
TEST TEST
LICENSE #: NON-DRINKING

OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1

CASE/REPORT: 23-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:12
BLANK TEST	0.000	10:12
INTERNAL STANDARD	VERIFIED	10:12
EXTERNAL STANDARD	0.077	10:12
BLANK TEST	0.000	10:13
SUBJECT SAMPLE (Vol=1.59L)	0.000	10:14
BLANK TEST	0.000	10:15
EXTERNAL STANDARD	0.077	10:15
BLANK TEST	0.000	10:16

Calibration Rejected

Alcohol (g/210L)
Flow Rate (L/M)
Min. Flow Rate (L/M)

