

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument
State of Alaska

Serial #: 100381

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 03/24/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.80: 0.080
LOT #: 11313080A1
EXPIRATION: 06/01/2015
TANK PRESSURE: 792 psi

BLANK TEST	0.000	03:27
INTERNAL STANDARD	VERIFIED	03:27
EXTERNAL STANDARD	0.078	03:27
BLANK TEST	0.000	03:28
EXTERNAL STANDARD	0.078	03:28
BLANK TEST	0.000	03:29
EXTERNAL STANDARD	0.078	03:29
BLANK TEST	0.000	03:30
EXTERNAL STANDARD	0.079	03:31
BLANK TEST	0.000	03:32
EXTERNAL STANDARD	0.080	03:32
BLANK TEST	0.000	03:33

Average = 0.0786
Std Dev = 0.0009

Diagnostic Check

VERSIONS

DMT: 3.00
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
Breath Tube = 40.9°C PASSED

PUMP INFO

Flow Rate = 4.623 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO


Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED


INTERNAL STANDARD



PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

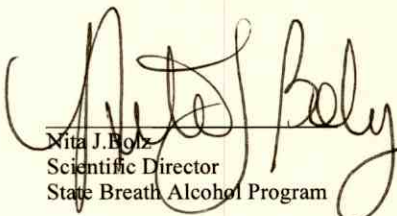
Nita J. Bolz
Scientific Director
State Breath Alcohol Program
5/4/2015
Subscribed and sworn before me this 4th day of May, 2015


Nikki Roth, Notary Public
My Commission Expires With Office

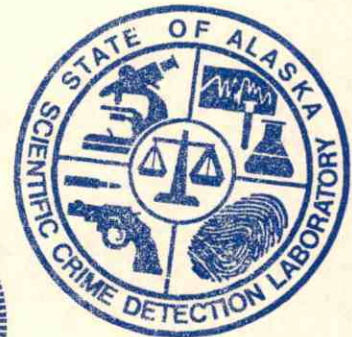

CRF
4/14/15