



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100360

**Report Issue Date:** 02/28/2024  
**Date Received:** 2023-12-20  
**Condition of Item:** Good

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 12/20/2023** - As Found - **End Date 12/21/2023** As Found - Evaluation Analyst: Colleen O'Bryant  
 As Found Conditions - Barometric Pressure (inHg): 28.99 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.5  
 Relative Humidity (%): 17

As-Found Data					
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)		Mean (g/210L)
0.020					
0.080					
0.300					

Unable to perform as-found due to blank errors on required VOC. Second attempt resulted in internal standard failure. (7.8%)

**Start Date 02/13/2024** - As Left - **End Date 02/15/2024**

As Left Conditions - Barometric Pressure (inHg): 29.78 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.02 Relative Humidity (%): 14

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.021	0.020	0.020	0.020	0.021	0.020	+/- 0.002
0.040	0.040	AG217904	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.080	AG310901	0.079	0.078	0.078	0.078	0.079	0.078	+/- 0.004
0.100	0.100	AG333401	0.100	0.099	0.100	0.100	0.100	0.100	+/- 0.004
0.150	0.149	AG332004	0.147	0.146	0.146	0.146	0.146	0.146	+/- 0.005
0.300	0.299	AG327804	0.296	0.297	0.296	0.297	0.297	0.297	+/- 0.011

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Colleen O'Bryant on 02/27/2024

[colleen.obryant@alaska.gov](mailto:colleen.obryant@alaska.gov)

Technically and administratively reviewed by Carlie Glaister on 02/28/2024

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100360 Analyst or Technician Name: C. O. Bryant

DataMaster DMT Calibration Start Date: 2/13/24

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 221250180  
Calibration Due Date: 2/14/24
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.78 Temperature(C) 22.2 Relative Humidity(%) 14  
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

- Acetone Reagent Lot Number: 20240214008 Expiration Date: 5/14/24  
Simulator S/N: SD1088 Thermometer Verification Performed?
- Isopropanol Reagent Lot Number: 20240214008 Expiration Date: 5/14/24  
Simulator S/N: DP4161 Thermometer Verification Performed?
- Negative (Ethanol Only) Lot Number: 22HP41201 Expiration Date: 5/14/24  
Simulator S/N: SD1177 Thermometer Verification Performed?  2024.08.24

Calibrated External Thermometer S/N: 230631106  
Calibration Due Date: 9/19/25

COB 2024.02.27

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 2/14/24  
Data Interpretation Date (Technician): N/A (if applicable)  
Data Interpretation Date (Analyst): 2/15/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100360  
-----

Date: 02/13/2024  
Time: 16:42:58

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 47.7°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.96 V PASSED  
(1.17 V - 2.73 V)  
Cooler Voltage = 1.66 V PASSED  
(1.00 V - 2.32 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 533 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.7 in

PUMP INFO

Flow Rate = 4.723 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF PASSED  
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.120 0.90% (0.00% - 4.00%) PASSED

Technician Screen

-----  
DATAMASTER dmt: 100360  
-----

Date: 02/14/2024  
Time: 10:56 AM

Temperatures (°C)

Sample Cell: 48.8°C  
Breath Tube: 47.1°C

Current Barometer 29.8 in  
Volume (Ltr) 1.59

Settings

Lamp: 1.93 V  
Bias: 80 V  
Cooler: 1.66 V  
Chopper: 532 Hz

Voltages (V)

Flow: 1.06 V  
Detector: -0.034 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100360  
-----

Date: 01/11/2024  
Time: 12:40:30

OPERATOR NAME:  
CARLIE GLAISTER  
CERTIFICATE #: 10436

Ca = 0.1000  
CAL = 0.977991    0.800 <= CAL < 1.200  
b1 = 0.0007    0.0000 <= b1 < 0.0040  
b2 = 0.0070    0.0010 <= b2 < 0.0100  
b3 = 0.0003    0.0000 <= b3 < 0.0040  
Xq = 0.1185    0.0500 <= Xq < 0.2000  
a21 = 1.221879    1.050 <= a21 < 1.300  
a31 = 0.504197    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100360

Date: 02/14/2024  
Time: 10:59:00

SUBJECT NAME:  
TEST TEST  
LICENSE #: VOLUME TEST

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237


DEPT/AGENCY:  
AAA1  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.79: 0.080  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	11:00
BLANK TEST	0.000	11:00
INTERNAL STANDARD	VERIFIED	11:00
EXTERNAL STANDARD	0.078	11:00
BLANK TEST	0.000	11:01
SUBJECT SAMPLE (Vol=1.61L)	0.000	11:03
BLANK TEST	0.000	11:04
EXTERNAL STANDARD	0.078	11:04
BLANK TEST	0.000	11:05

*COB*

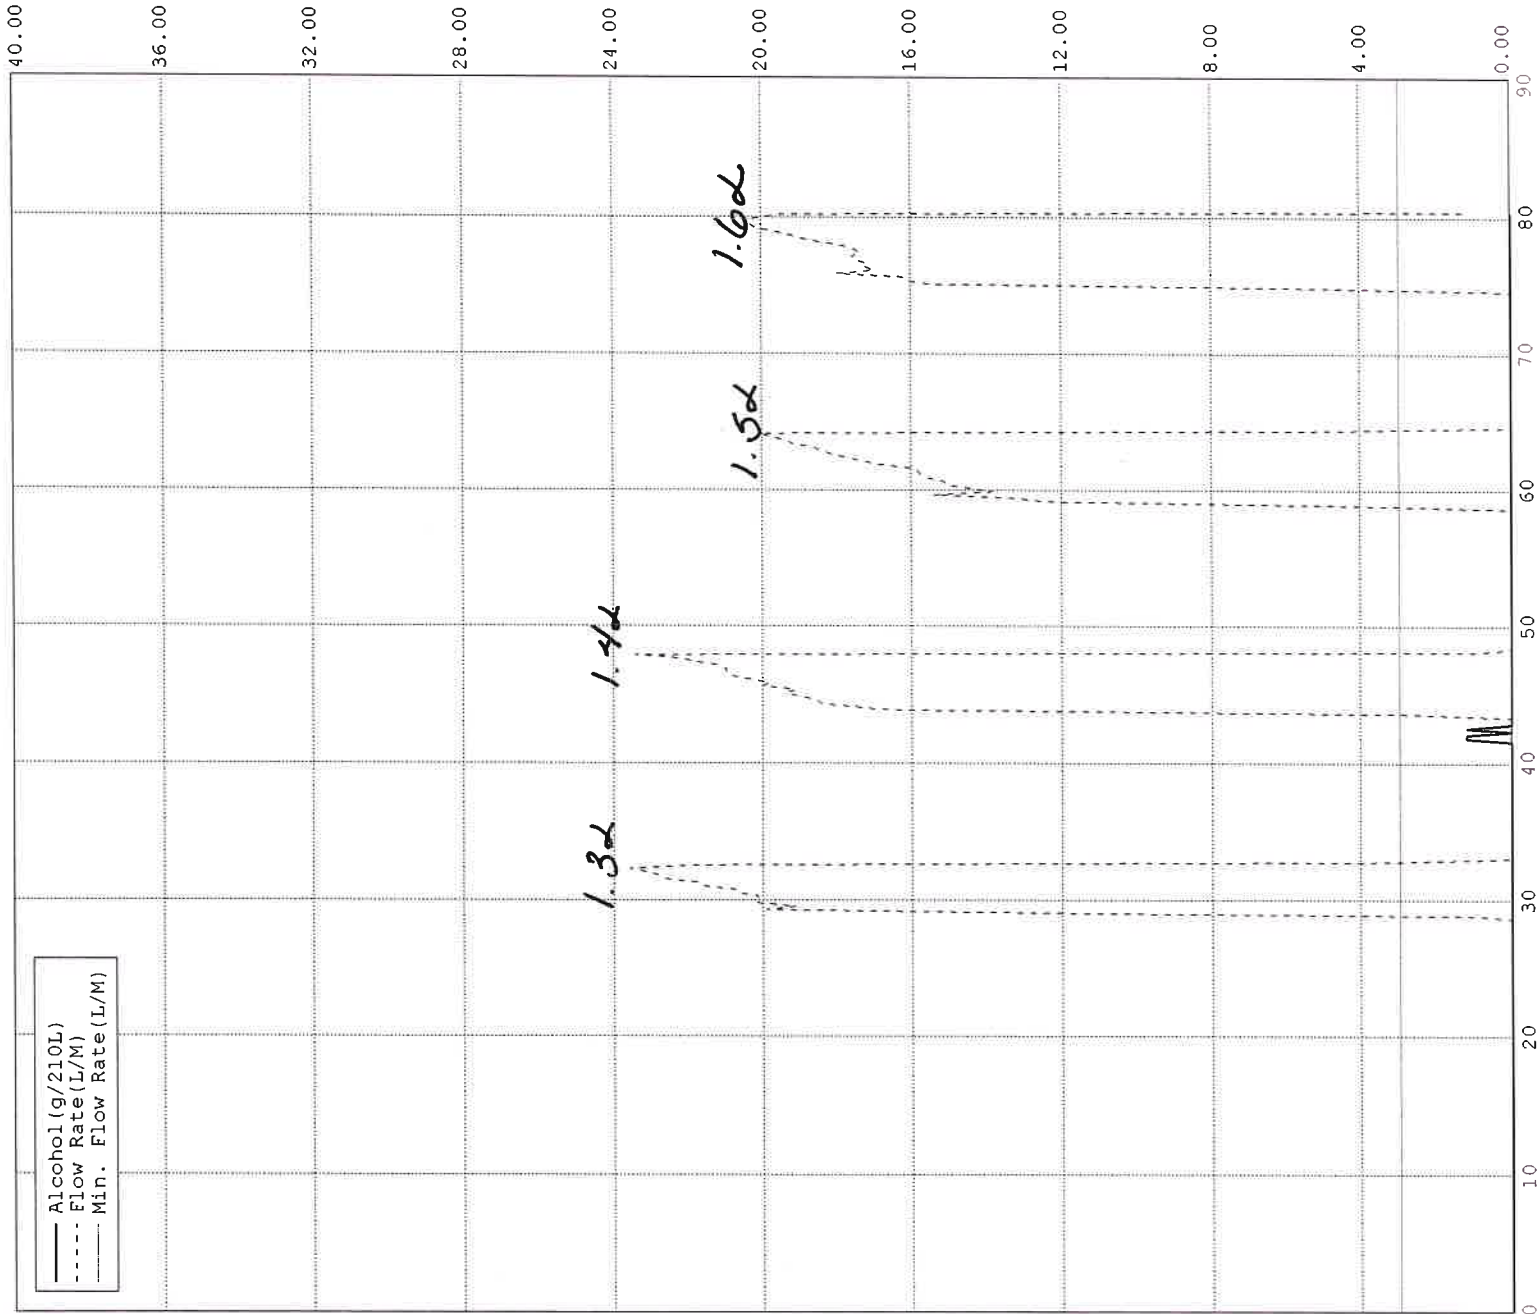

LINEARITY CHECK

Alaska Department of Public Safety  
 DATAMASTER dmt: 100360

Date: 02/14/2024  
 Time: 11:15:29


SUPERVISOR NAME:  
 COLLEEN S O'BRYAN  
 OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0204	0.0005
0.040	0.0400	0.0000
0.080	0.0784	0.0005
0.100	0.0998	0.0004
0.149	0.1462	0.0004
0.299	0.2966	0.0005

SLOPE = 0.989865  
 R<sup>2</sup> = 0.999923

100360 2024.02.15 Calibration

*CAS*

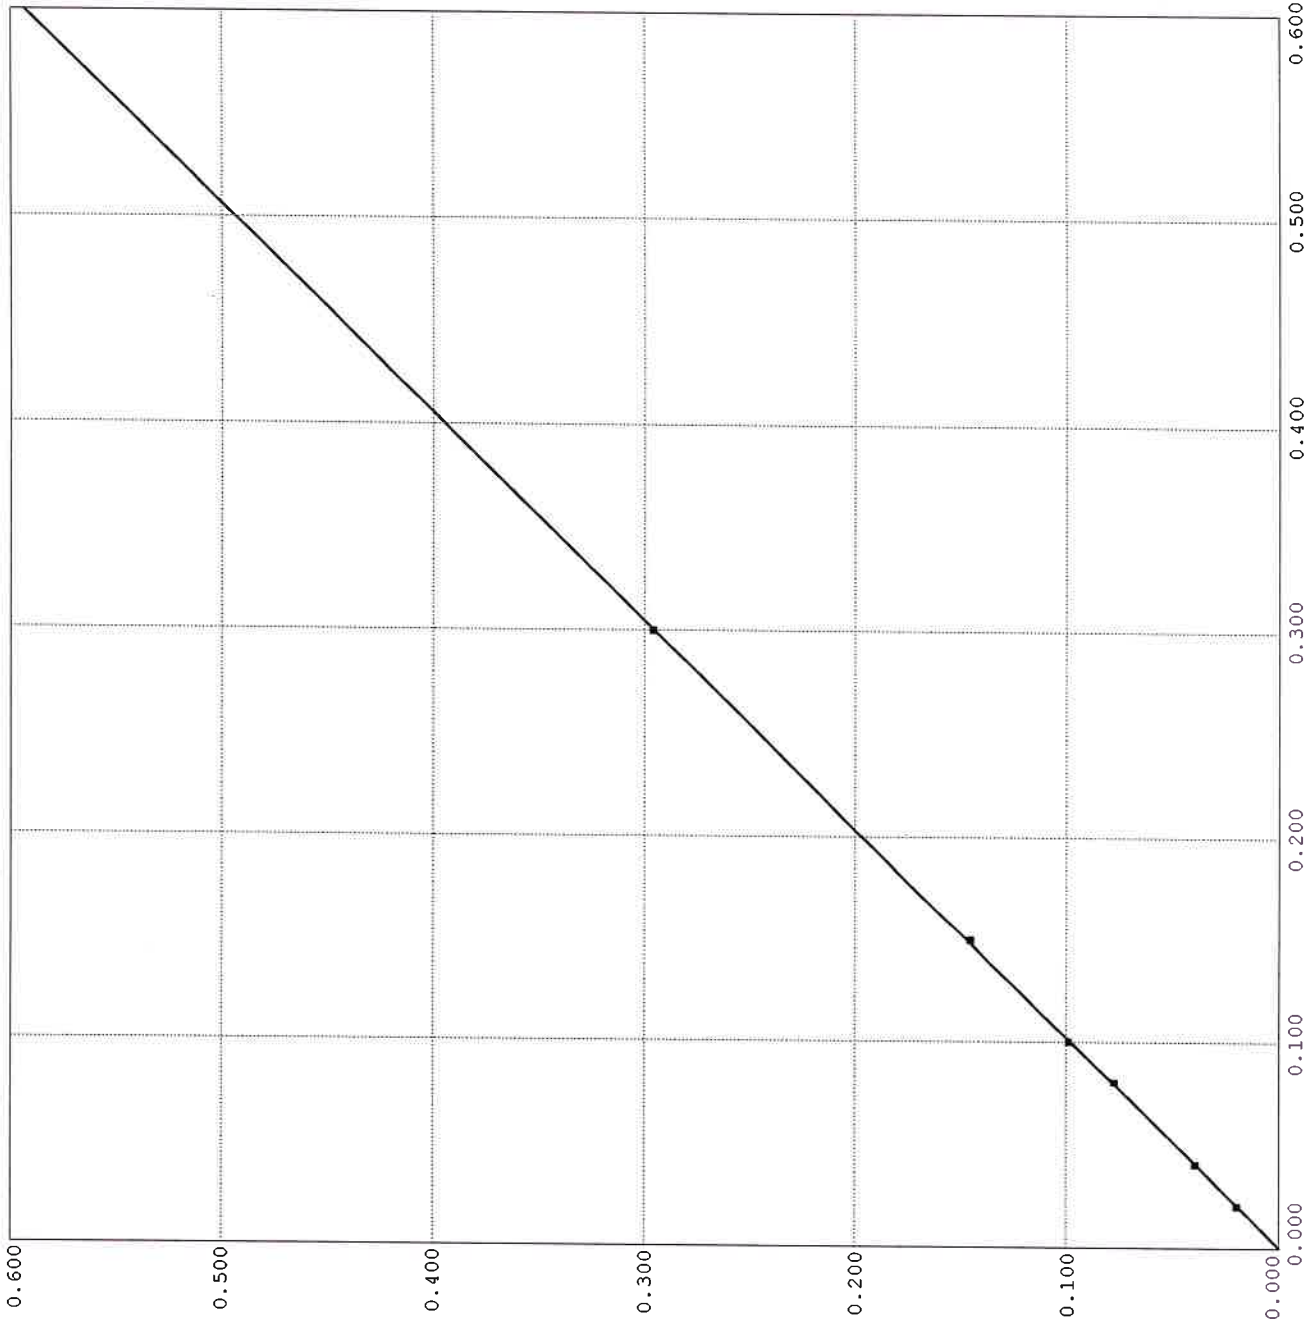

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100360






Date: 02/14/2024  
 Time: 11:15:31

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.79: 0.020  
 LOT #: AG217902  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 374 psi

BLANK TEST	0.000	11:20
INTERNAL STANDARD	VERIFIED	11:21
EXTERNAL STANDARD	0.021	11:21
BLANK TEST	0.000	11:22
EXTERNAL STANDARD	0.020	11:22
BLANK TEST	0.000	11:23
EXTERNAL STANDARD	0.020	11:23
BLANK TEST	0.000	11:24
EXTERNAL STANDARD	0.020	11:24
BLANK TEST	0.000	11:25
EXTERNAL STANDARD	0.021	11:25
BLANK TEST	0.000	11:26

Average = 0.0204  
 Std Dev = 0.0005

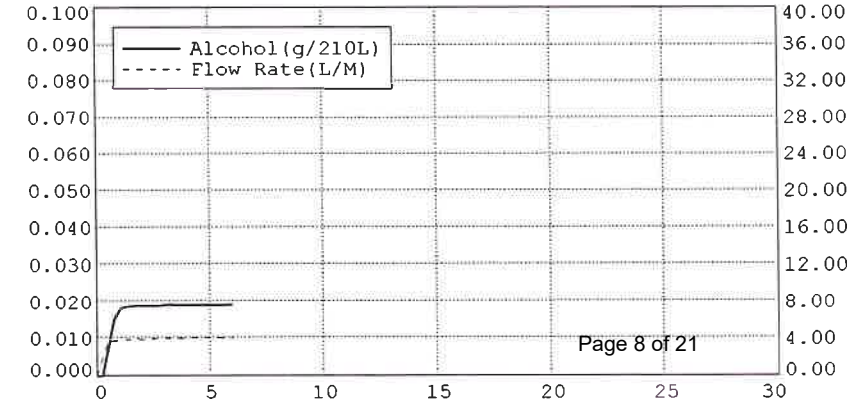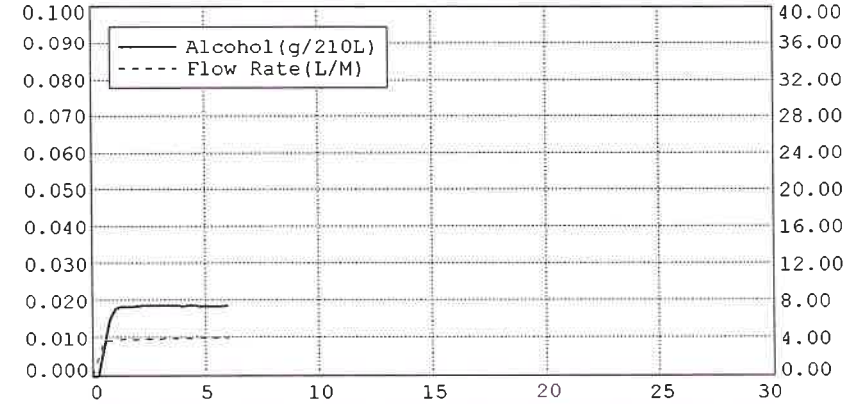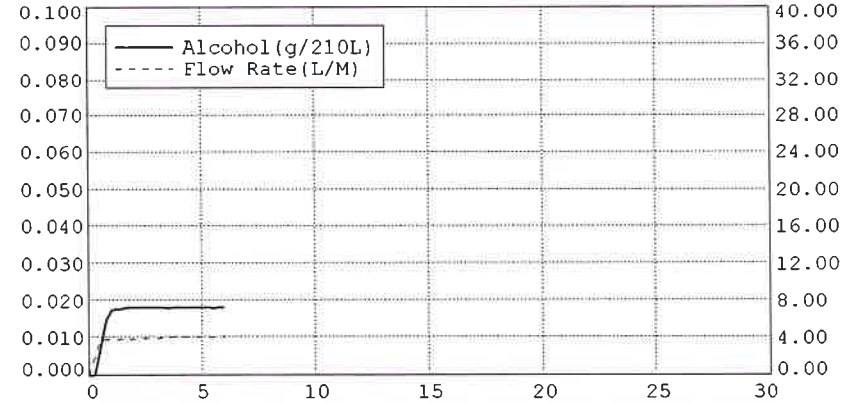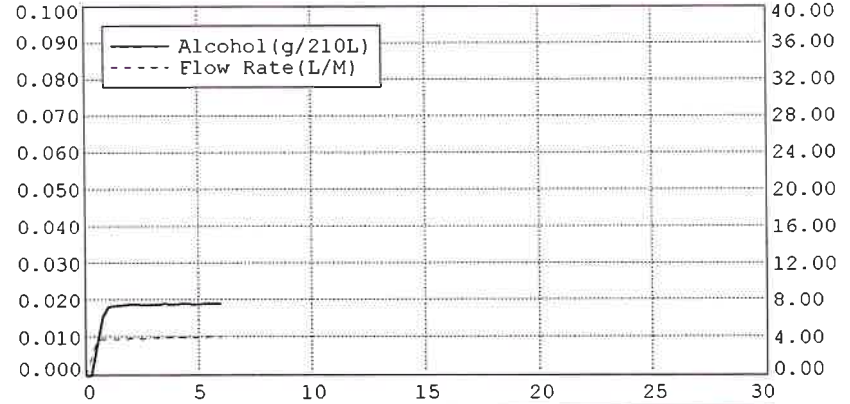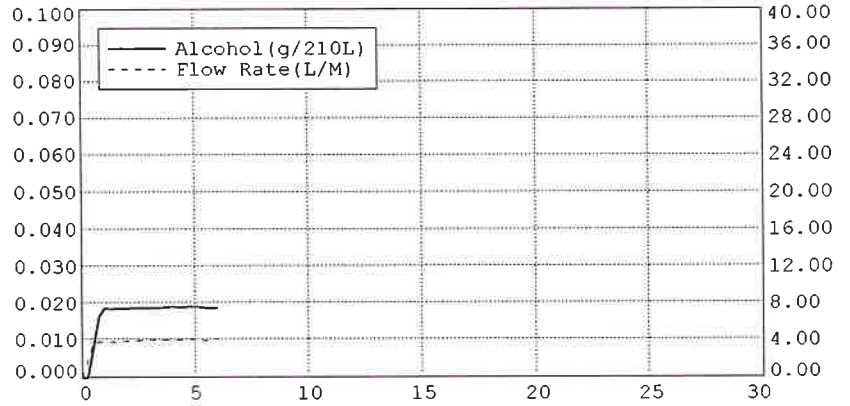



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
DATAMASTER dmt: 100360






Date: 02/14/2024  
Time: 11:29:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
TARGET AT 29.79: 0.040  
LOT #: AG217904  
EXPIRATION: 06/28/2024  
TANK PRESSURE: 0 psi

BLANK TEST	0.000	11:31
INTERNAL STANDARD	VERIFIED	11:31
EXTERNAL STANDARD	0.040	11:31
BLANK TEST	0.000	11:32
EXTERNAL STANDARD	0.040	11:32
BLANK TEST	0.000	11:33
EXTERNAL STANDARD	0.040	11:33
BLANK TEST	0.000	11:34
EXTERNAL STANDARD	0.040	11:34
BLANK TEST	0.000	11:35
EXTERNAL STANDARD	0.040	11:35
BLANK TEST	0.000	11:36

Average = 0.0400  
Std Dev = 0.0000

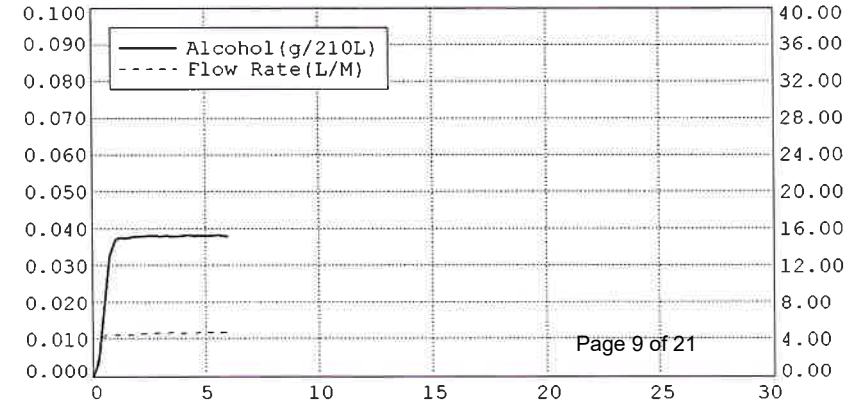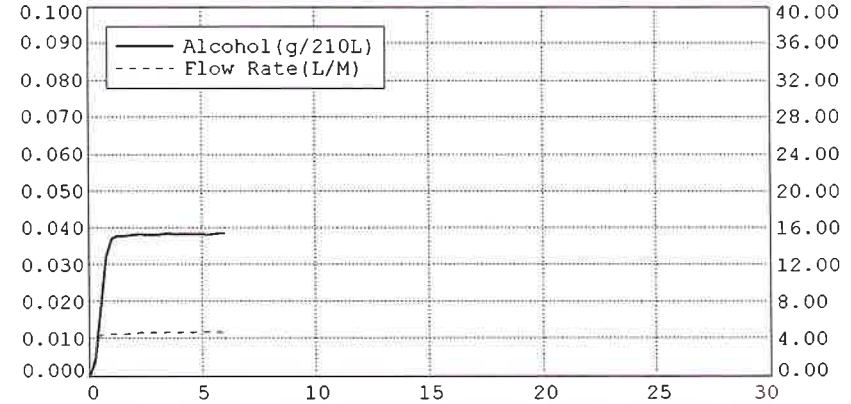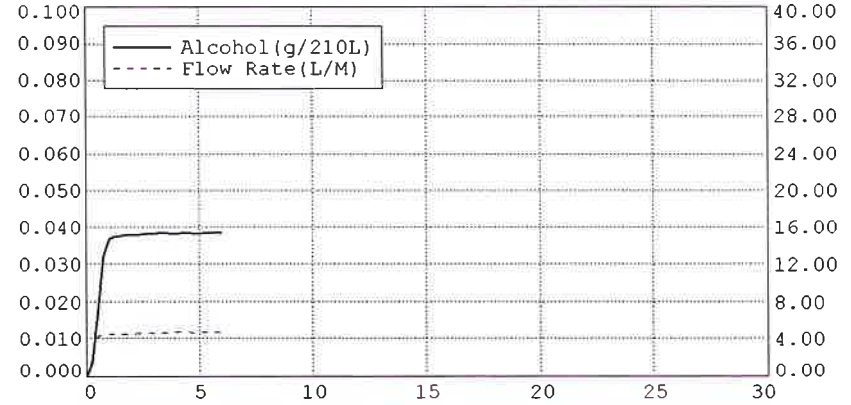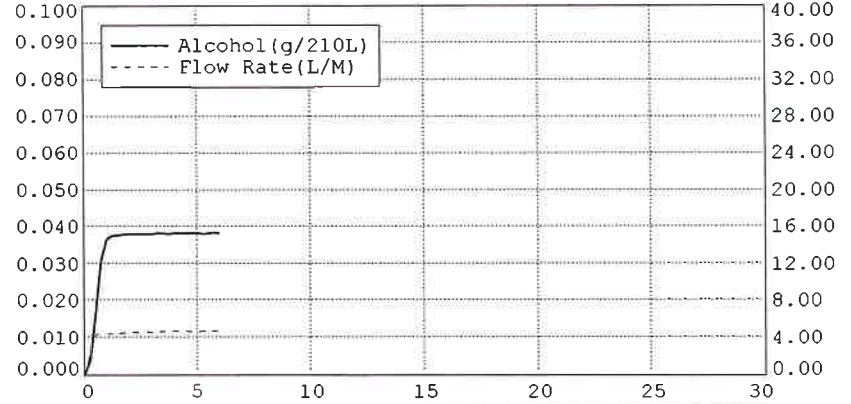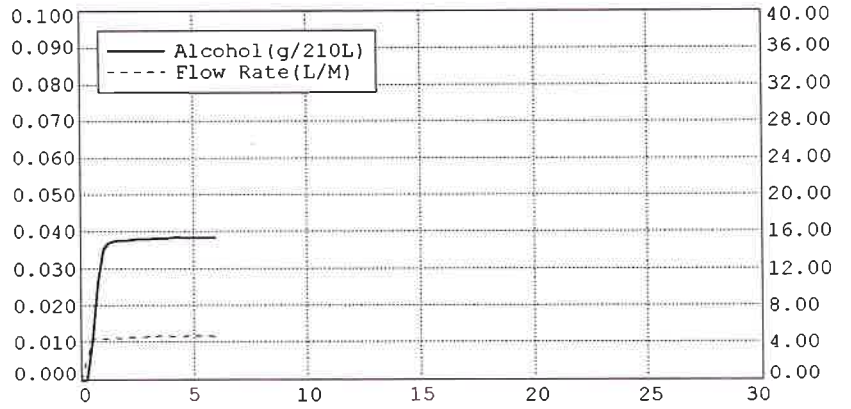

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
DATAMASTER dmt: 100360






Date: 02/14/2024  
Time: 11:38:22

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.79: 0.080  
LOT #: AG310901  
EXPIRATION: 04/19/2025  
TANK PRESSURE: 0 psi

BLANK TEST	0.000	11:39
INTERNAL STANDARD	VERIFIED	11:39
EXTERNAL STANDARD	0.079	11:39
BLANK TEST	0.000	11:40
EXTERNAL STANDARD	0.078	11:40
BLANK TEST	0.000	11:41
EXTERNAL STANDARD	0.078	11:41
BLANK TEST	0.000	11:42
EXTERNAL STANDARD	0.078	11:43
BLANK TEST	0.000	11:43
EXTERNAL STANDARD	0.079	11:44
BLANK TEST	0.000	11:45

Average = 0.0784  
Std Dev = 0.0005

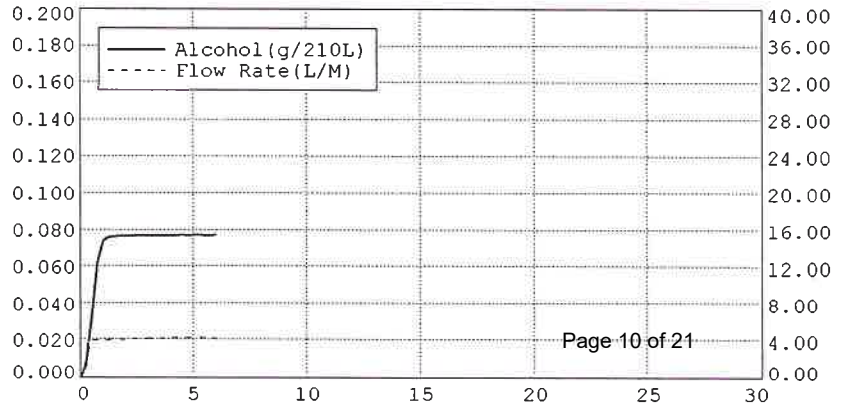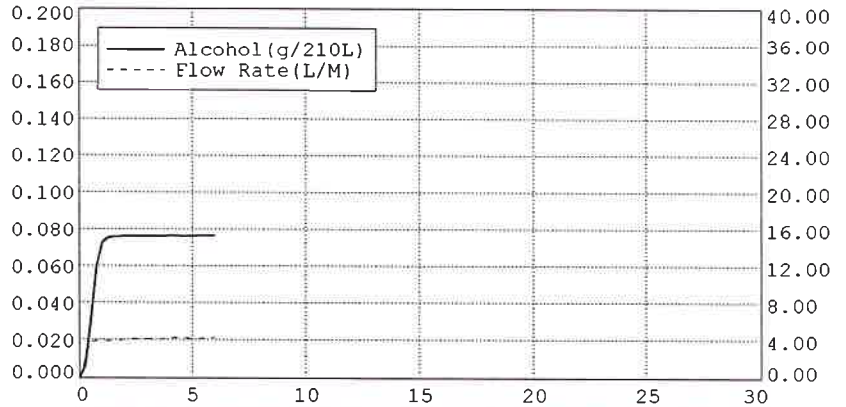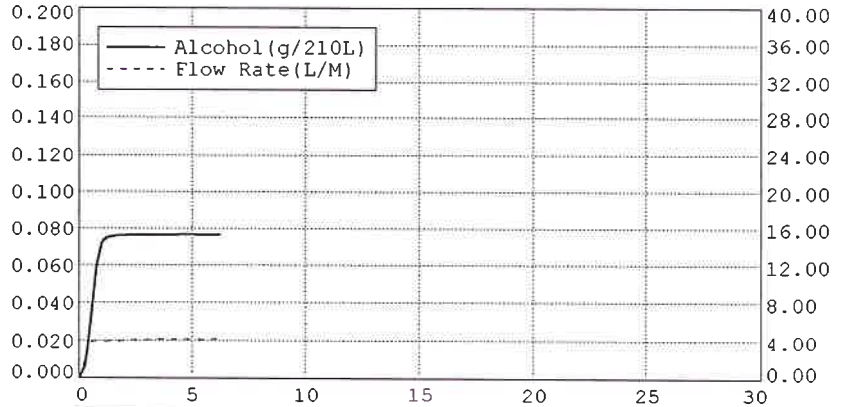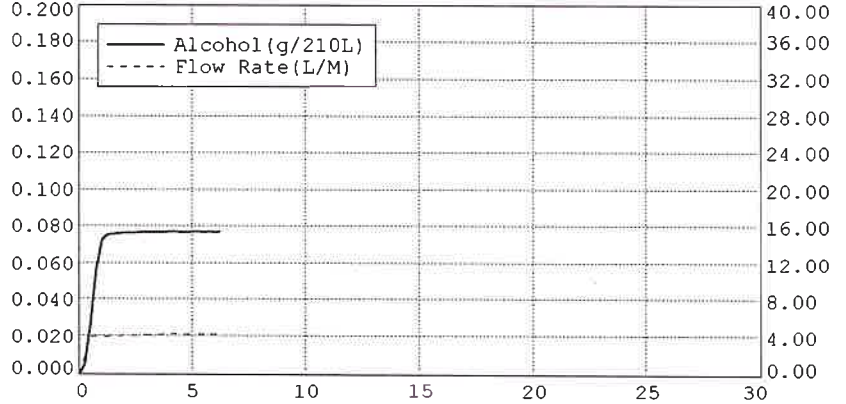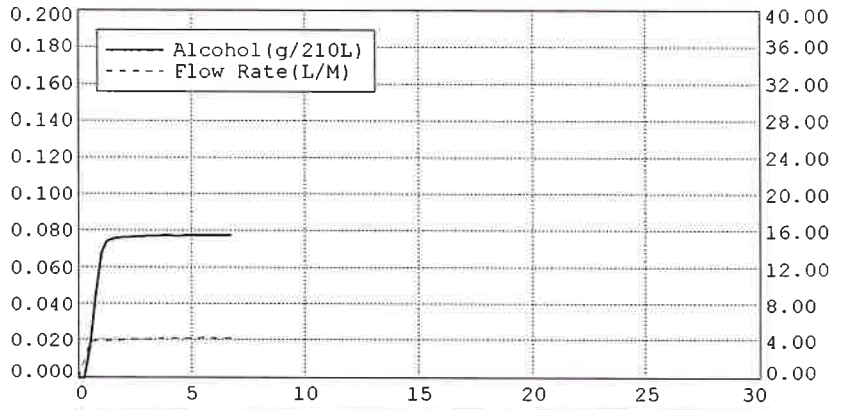

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100360






Date: 02/14/2024  
 Time: 11:46:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.78: 0.100  
 LOT #: AG333401  
 EXPIRATION: 11/30/2025  
 TANK PRESSURE: 1144 psi

BLANK TEST	0.000	11:51
INTERNAL STANDARD	VERIFIED	11:51
EXTERNAL STANDARD	0.100	11:51
BLANK TEST	0.000	11:52
EXTERNAL STANDARD	0.099	11:53
BLANK TEST	0.000	11:53
EXTERNAL STANDARD	0.100	11:54
BLANK TEST	0.000	11:55
EXTERNAL STANDARD	0.100	11:55
BLANK TEST	0.000	11:56
EXTERNAL STANDARD	0.100	11:56
BLANK TEST	0.000	11:57

Average = 0.0998  
 Std Dev = 0.0004

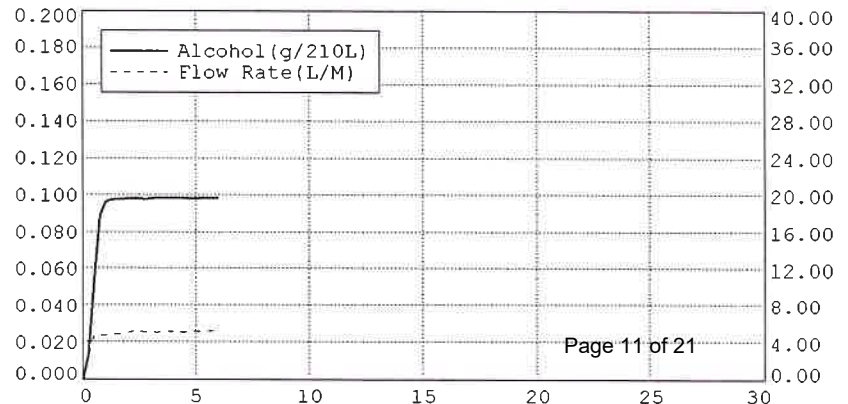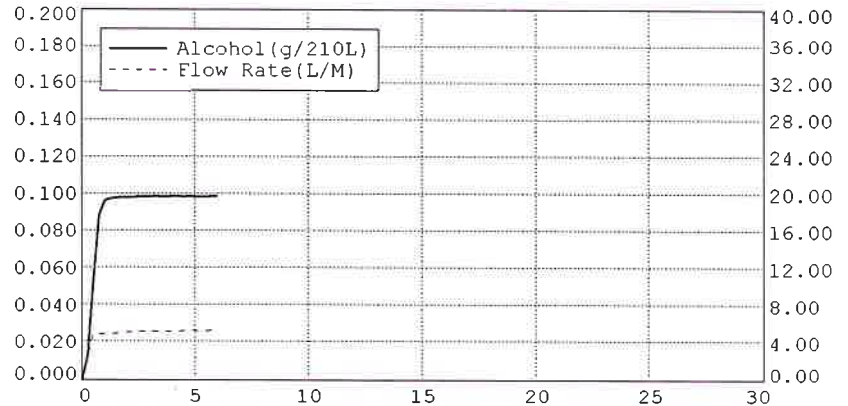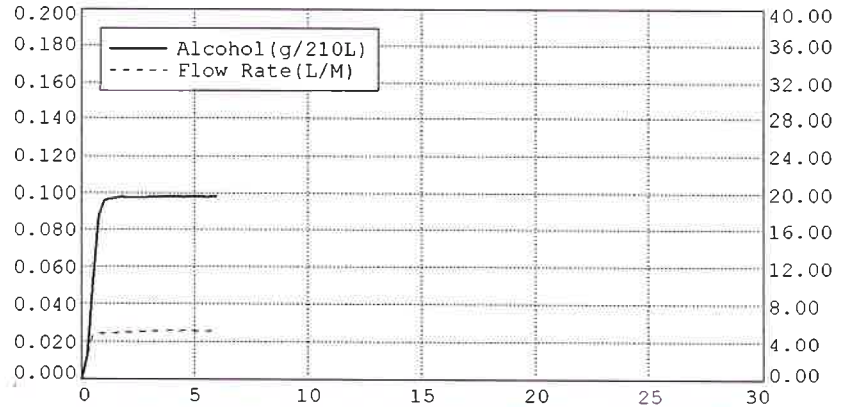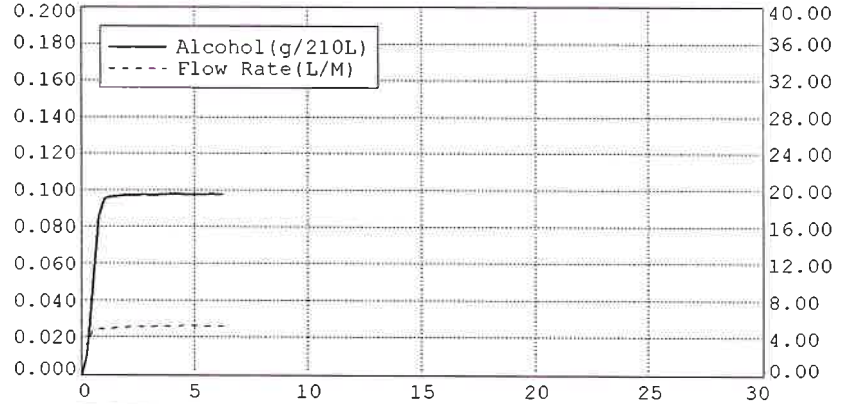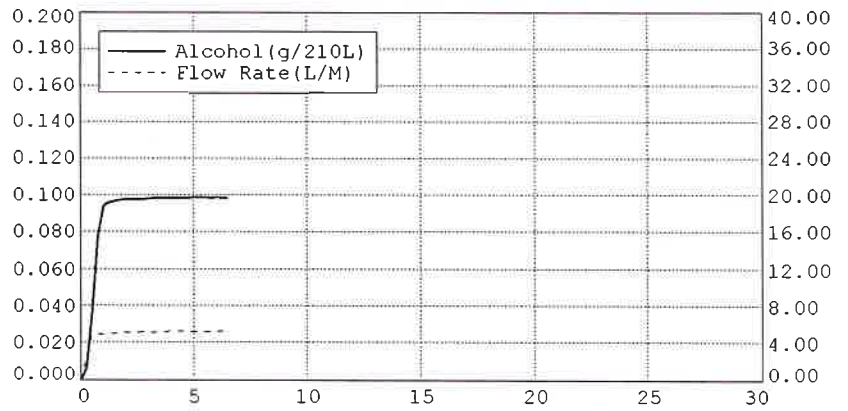

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
DATAMASTER dmt: 100360






Date: 02/14/2024  
Time: 11:59:39

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
TARGET AT 29.78: 0.149  
LOT #: AG332004  
EXPIRATION: 11/16/2025  
TANK PRESSURE: 758 psi

BLANK TEST	0.000	12:00
INTERNAL STANDARD	VERIFIED	12:00
EXTERNAL STANDARD	0.147	12:01
BLANK TEST	0.000	12:02
EXTERNAL STANDARD	0.146	12:02
BLANK TEST	0.000	12:03
EXTERNAL STANDARD	0.146	12:03
BLANK TEST	0.000	12:04
EXTERNAL STANDARD	0.146	12:04
BLANK TEST	0.000	12:05
EXTERNAL STANDARD	0.146	12:05
BLANK TEST	0.000	12:06

Average = 0.1462  
Std Dev = 0.0004

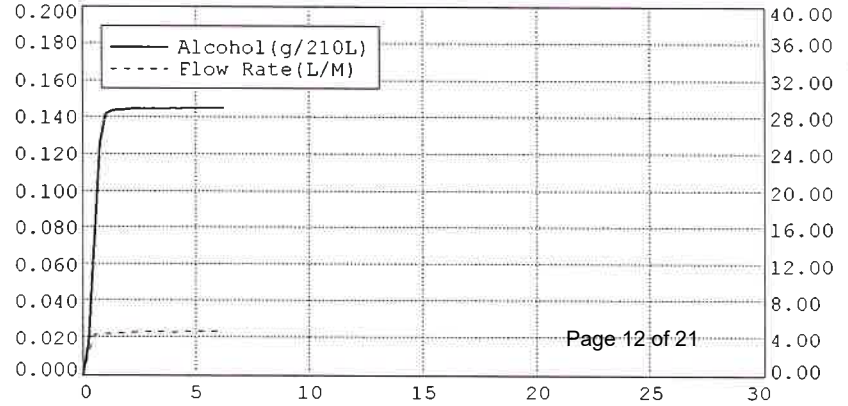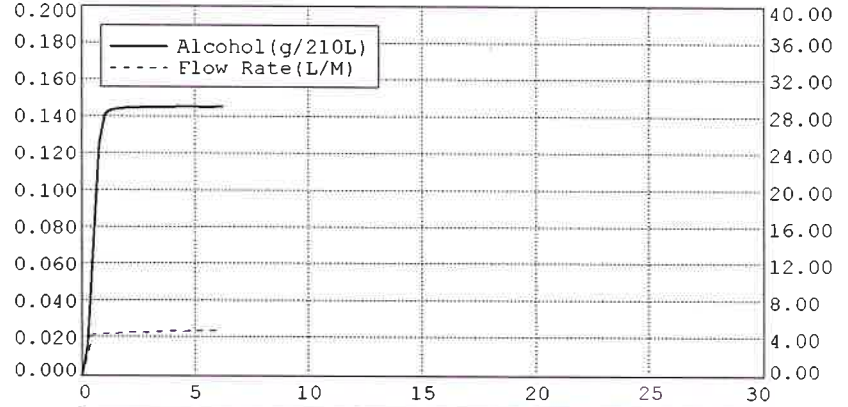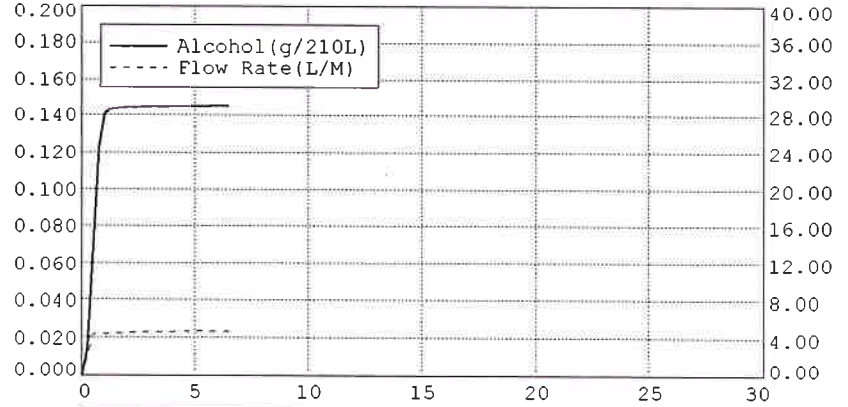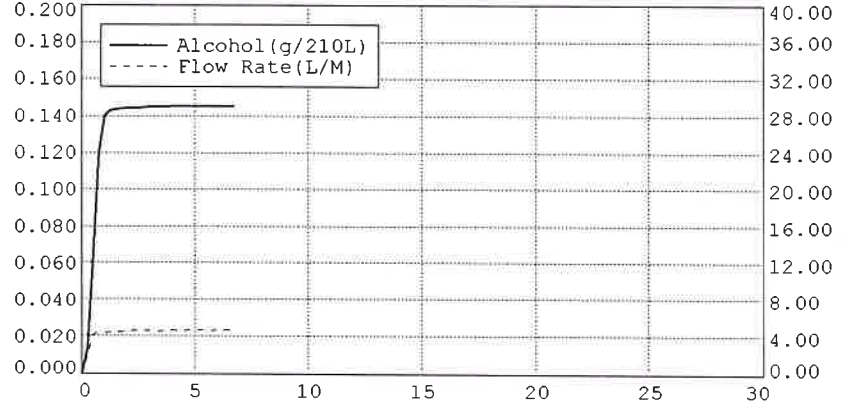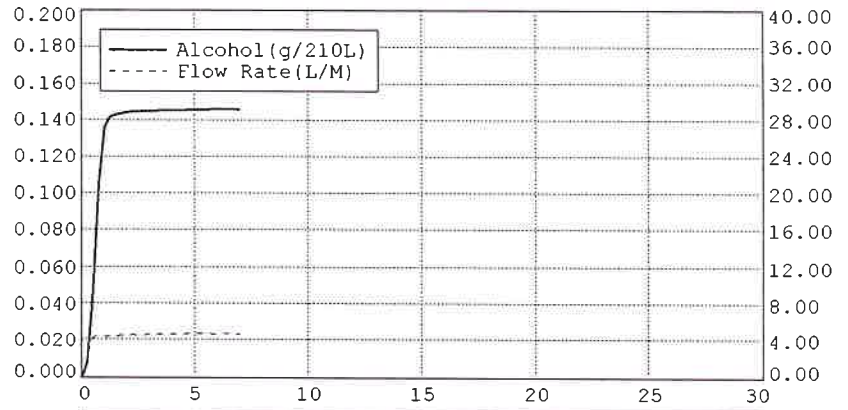

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100360






Date: 02/14/2024  
 Time: 12:07:07

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.78: 0.299  
 LOT #: AG327804  
 EXPIRATION: 10/05/2025  
 TANK PRESSURE: 336 psi

BLANK TEST	0.000	12:08
INTERNAL STANDARD	VERIFIED	12:08
EXTERNAL STANDARD	0.296	12:08
BLANK TEST	0.000	12:09
EXTERNAL STANDARD	0.297	12:09
BLANK TEST	0.000	12:10
EXTERNAL STANDARD	0.296	12:10
BLANK TEST	0.000	12:11
EXTERNAL STANDARD	0.297	12:12
BLANK TEST	0.000	12:12
EXTERNAL STANDARD	0.297	12:13
BLANK TEST	0.000	12:14

Average = 0.2966  
 Std Dev = 0.0005

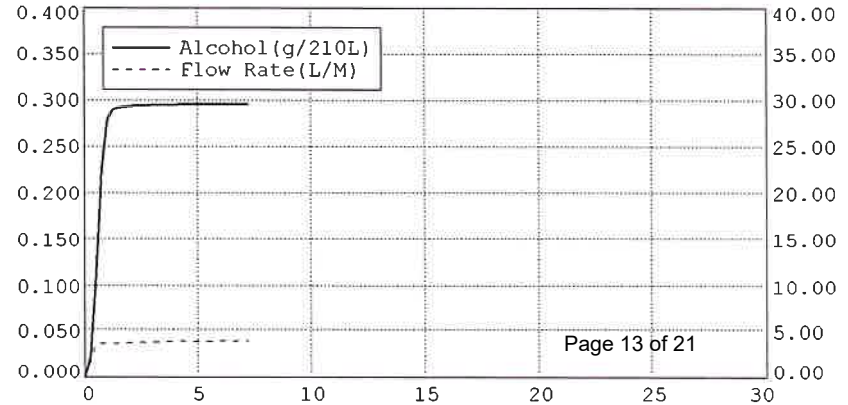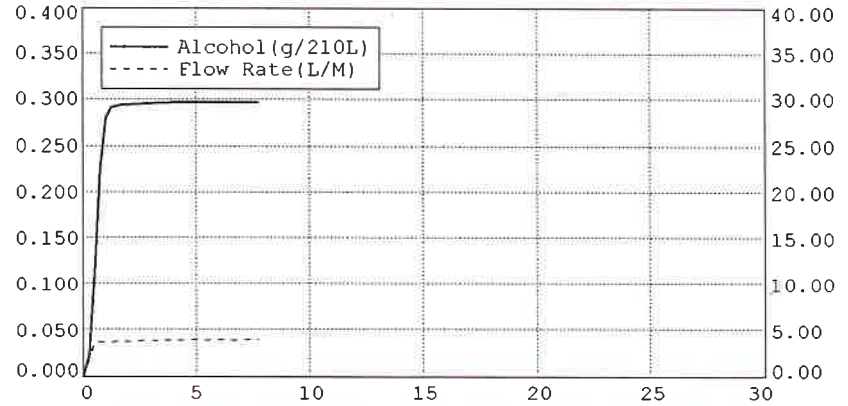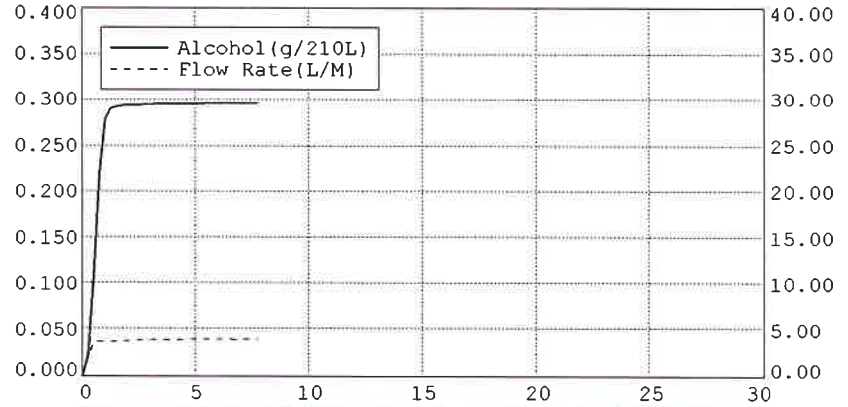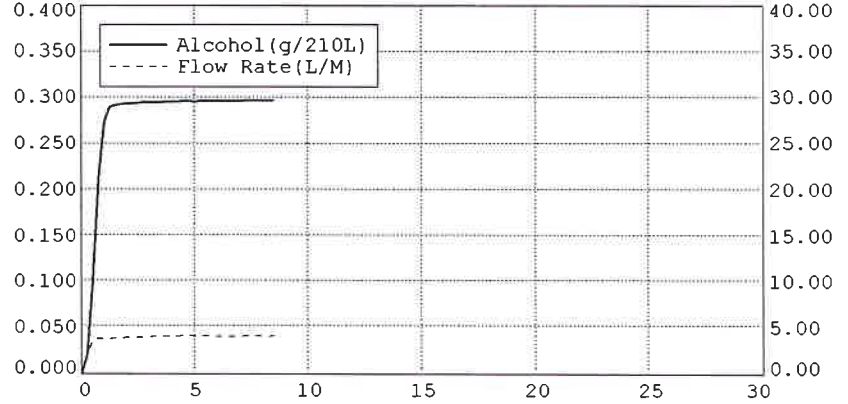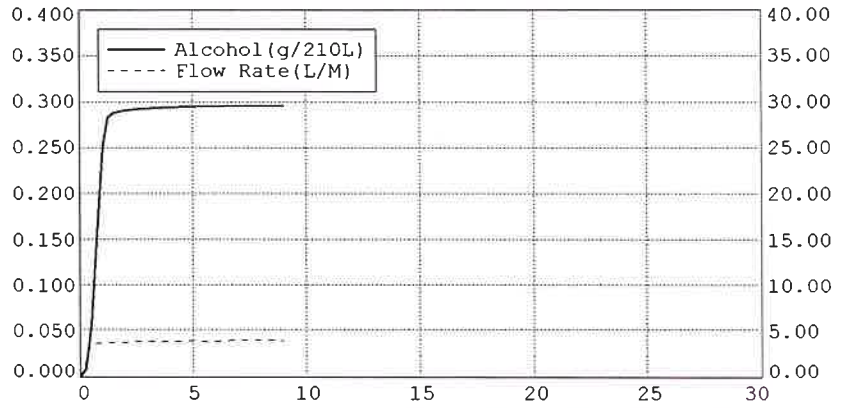

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100360

Date: 02/14/2024

Time: 13:41:51

SUBJECT NAME:

TEST TEST

LICENSE #: INCOMPLETE

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 24-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.74: 0.080

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

BLANK TEST


INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 13:42  
0.000 13:43  
VERIFIED 13:43  
0.079 13:43  
0.000 13:44  
INCOMPLETE 13:46

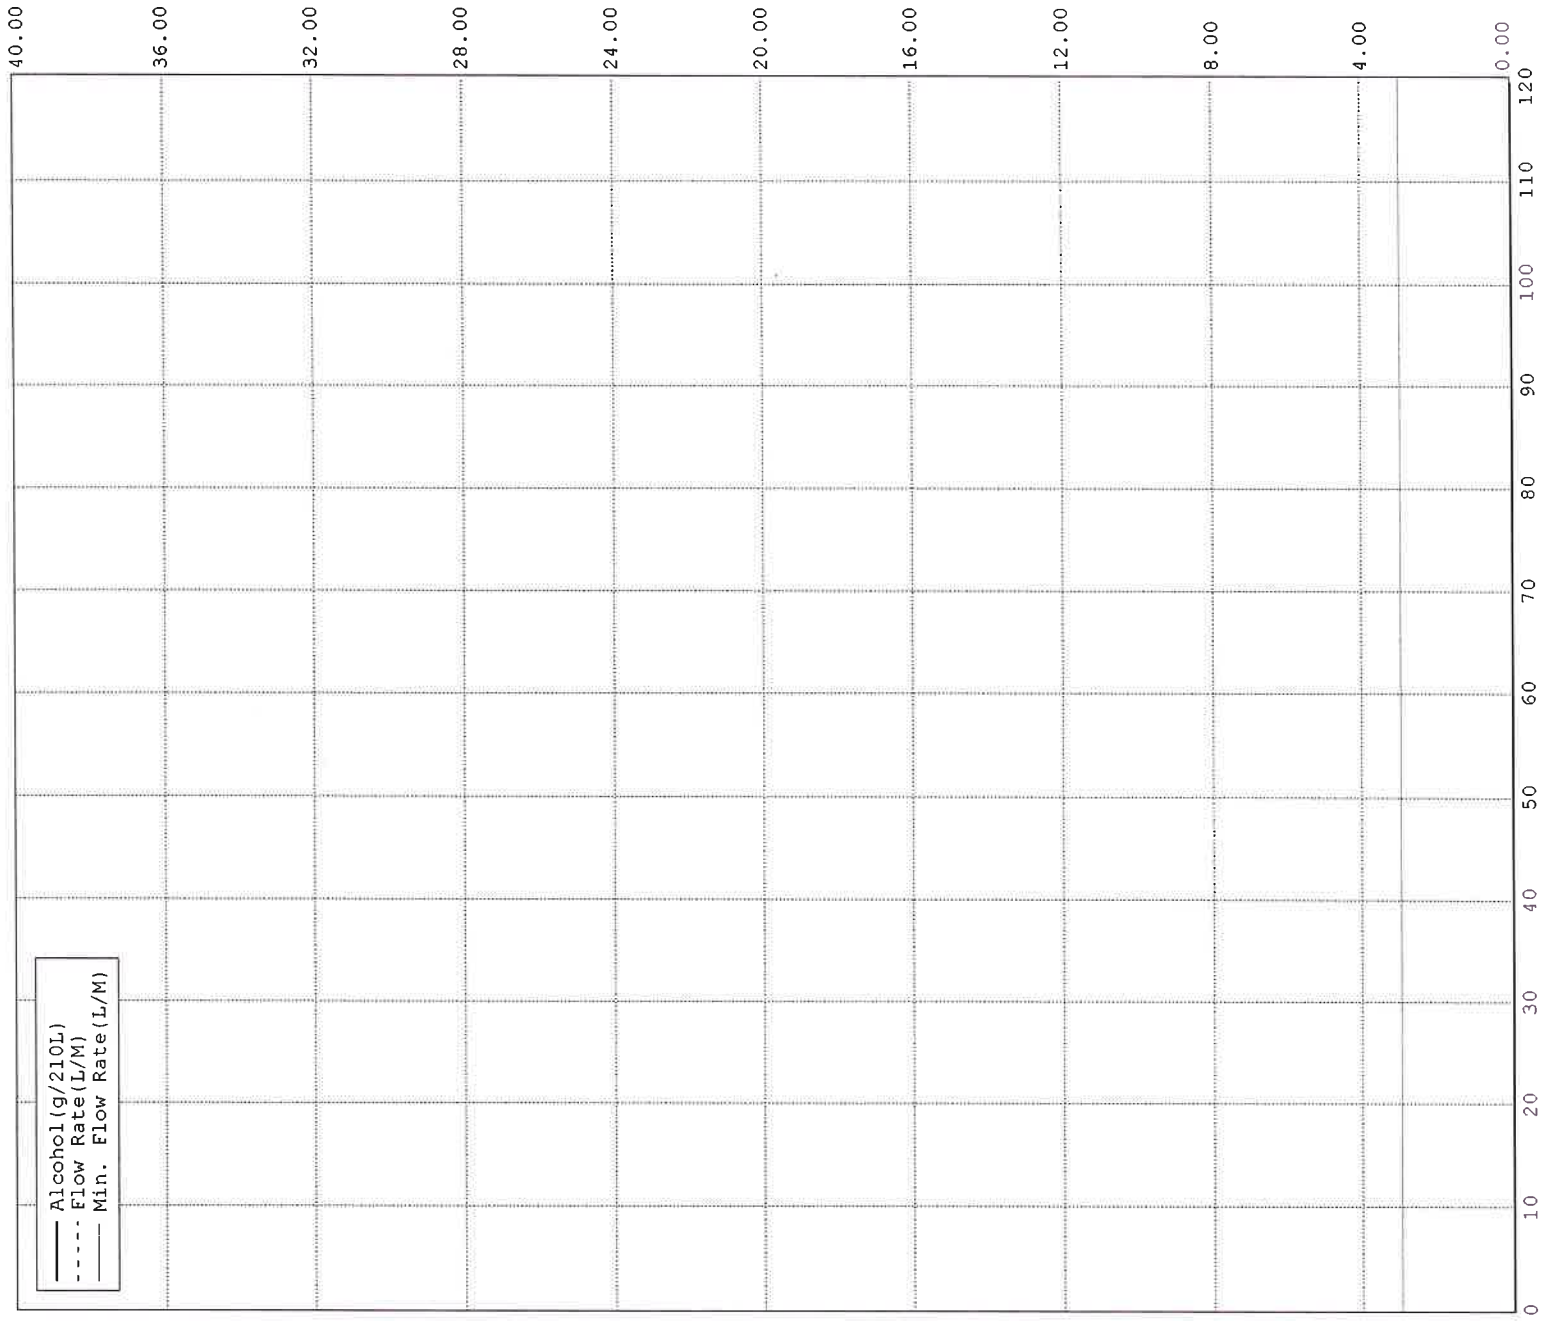

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100360

Date: 02/14/2024

Time: 14:08:51

SUBJECT NAME:

TEST TEST

LICENSE #: MAX ATTEMPTS

OPERATOR NAME:

COLLEEN S OBRYANT

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 24-12345

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.74: 0.080

LOT #: AG310901

EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK

PASSED 14:09

BLANK TEST

0.000 14:09

INTERNAL STANDARD

VERIFIED 14:10

0.078 14:10

EXTERNAL STANDARD


0.000 14:11

BLANK TEST

XXX 14:12

SUBJECT SAMPLE

Maximum Attempts Exceeded

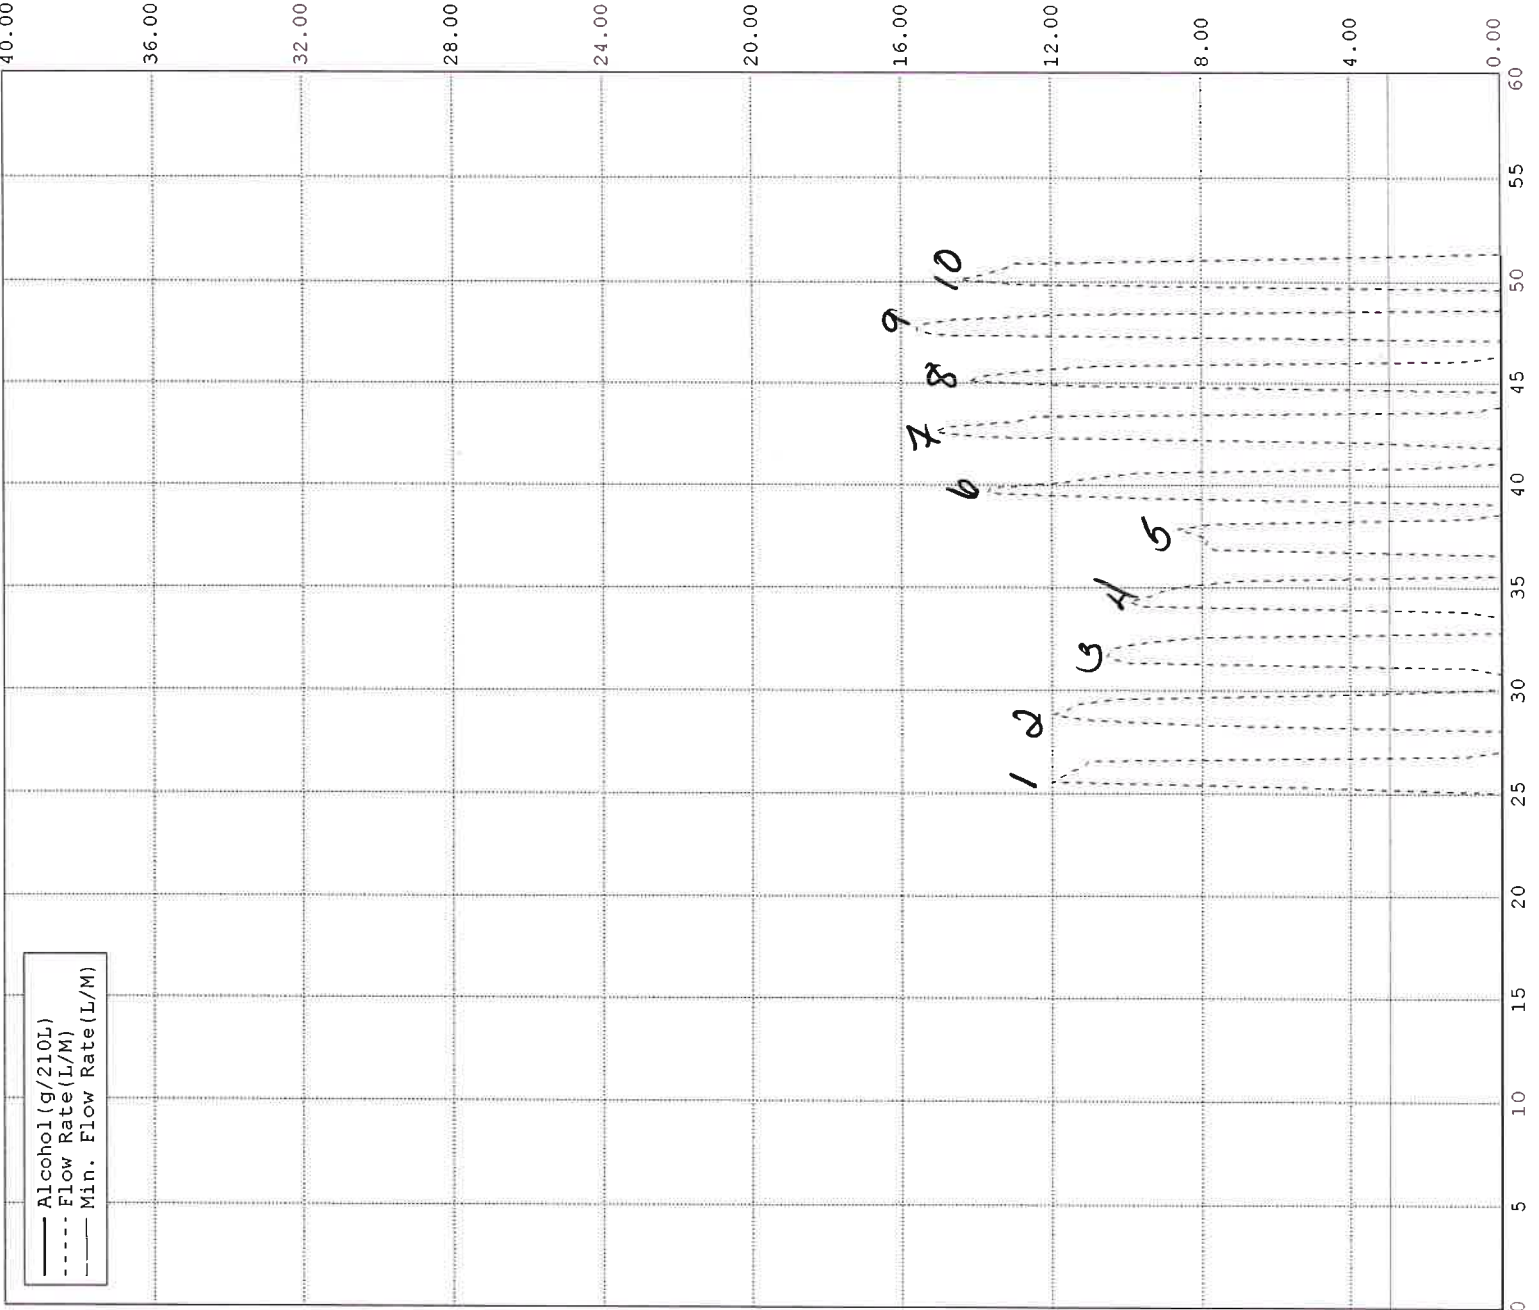

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100360

Date: 02/14/2024  
Time: 14:16:57

SUBJECT NAME:  
TEST TEST  
LICENSE #: INVALID


OPERATOR NAME:  
COLLEEN S OBRYANT  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 24-12345  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.74: 0.080  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:22
BLANK TEST	0.000	14:22
INTERNAL STANDARD	VERIFIED	14:22
EXTERNAL STANDARD	0.079	14:22
BLANK TEST	0.000	14:23
SUBJECT SAMPLE	INVALID	14:24

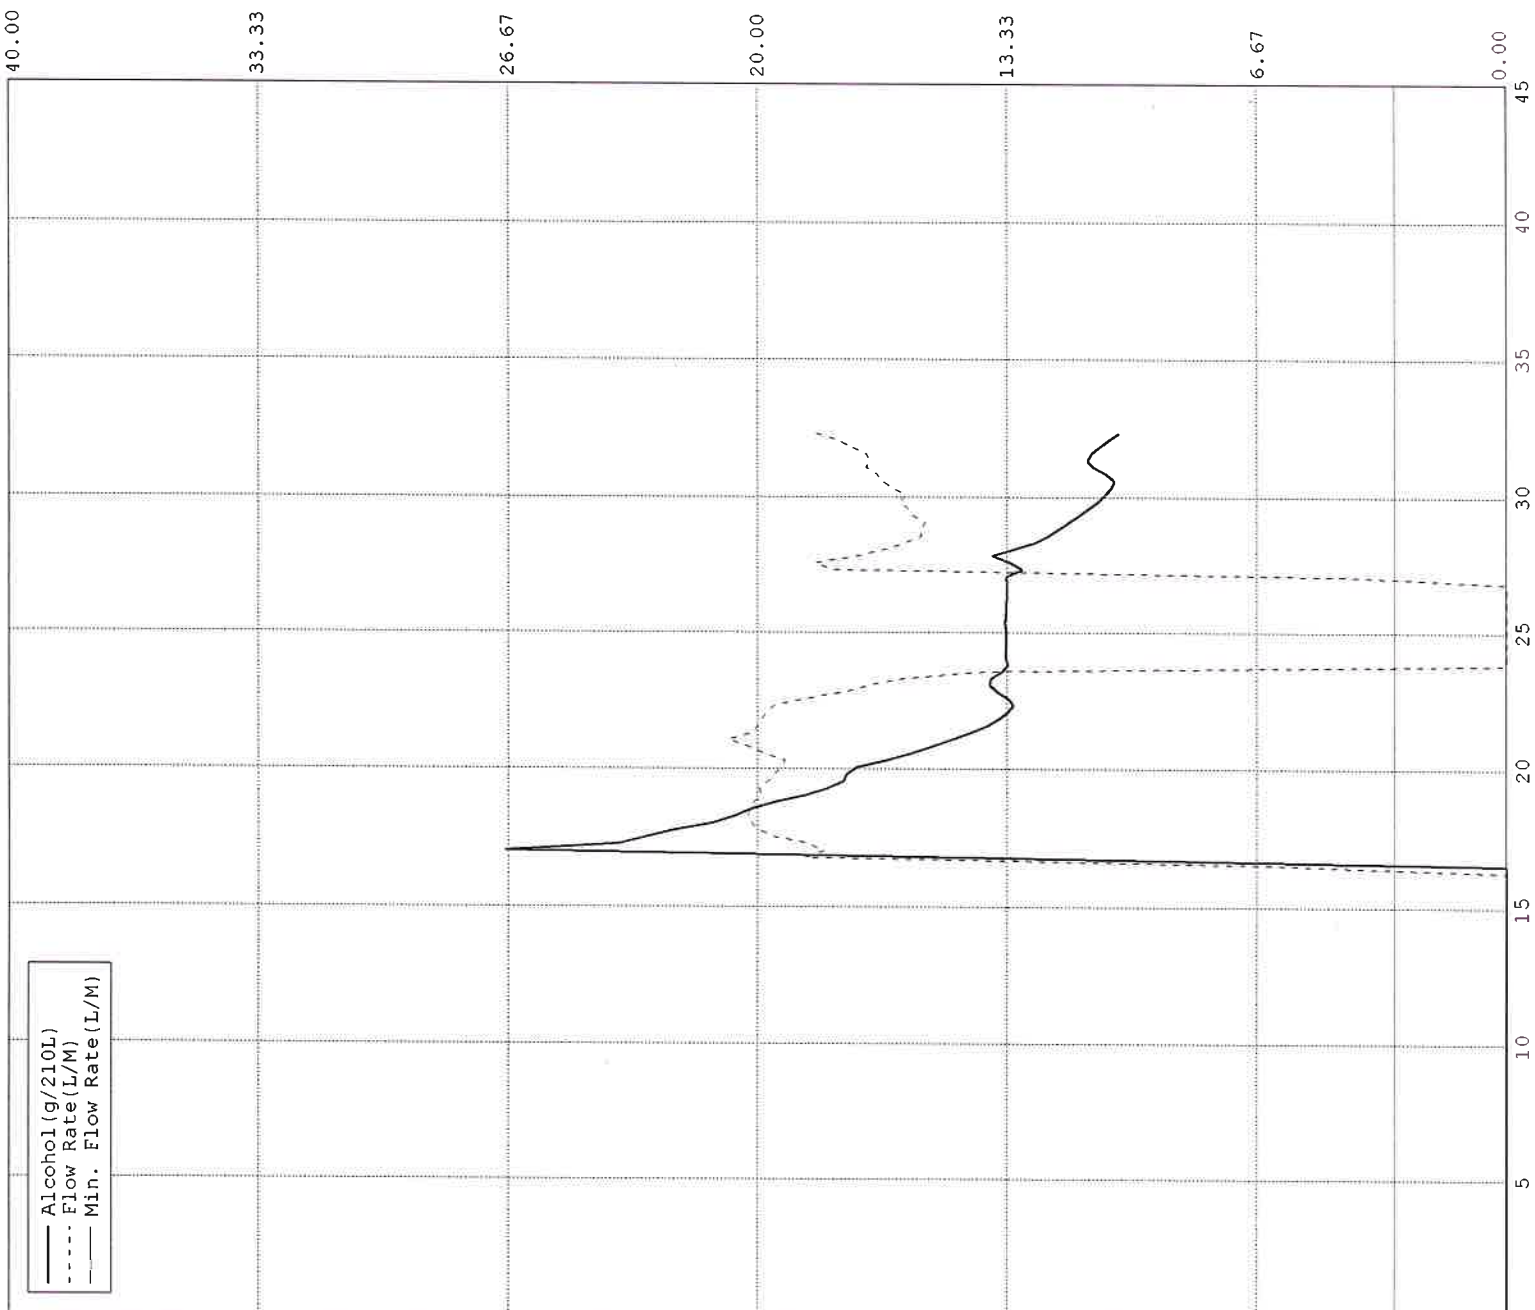



SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100360

Date: 02/14/2024  
Time: 14:26:18

SUBJECT NAME:  
TEST TEST  
LICENSE #: RFI

OPERATOR NAME:  
COLLEEN S OBRYANT  
OPERATOR'S #: 6237


DEPT/AGENCY:  
AAA1  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.74: 0.080  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 14:27  
BLANK TEST 0.000 14:27  
INTERNAL STANDARD VERIFIED 14:27  
EXTERNAL STANDARD 0.078 14:28  
BLANK TEST 0.000 14:28

RFI DETECTED

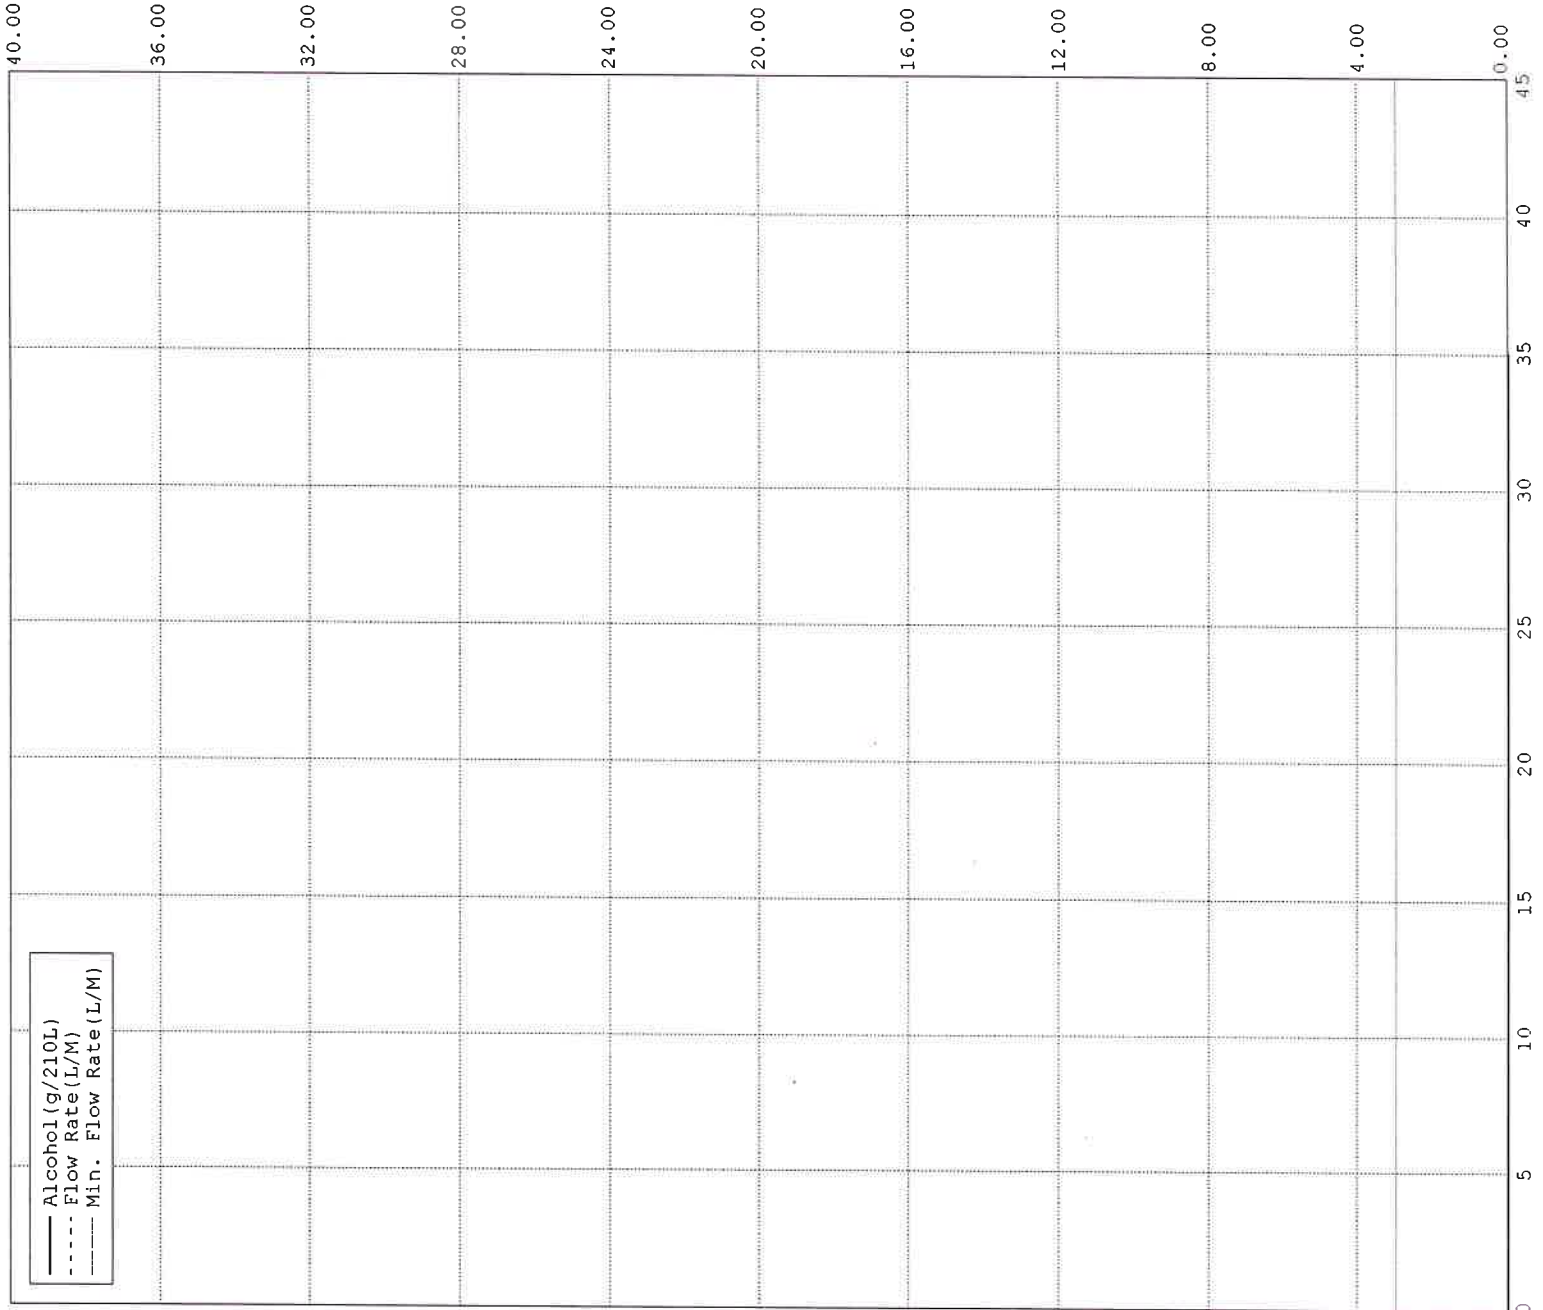

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100360

Date: 02/14/2024  
Time: 14:56:00

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-ACETONE

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAAA  
CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.72: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	14:57
BLANK TEST	0.000	14:57
INTERNAL STANDARD	VERIFIED	14:57
Xq = 0.120 (1.12%)		
EXTERNAL STANDARD	0.078	14:57
X[1] = 0.0785 (-0.0017) (0.0026)		
BLANK TEST	0.000	14:58
SUBJECT SAMPLE	XXX	14:59
X[1] = 0.1086 (-0.0190) (0.0009)		


Interference Detected

*Filter 2 Avg = -0.0018*

*Filter 3 Avg = 0.0020*

*OS*

*02/15/24*

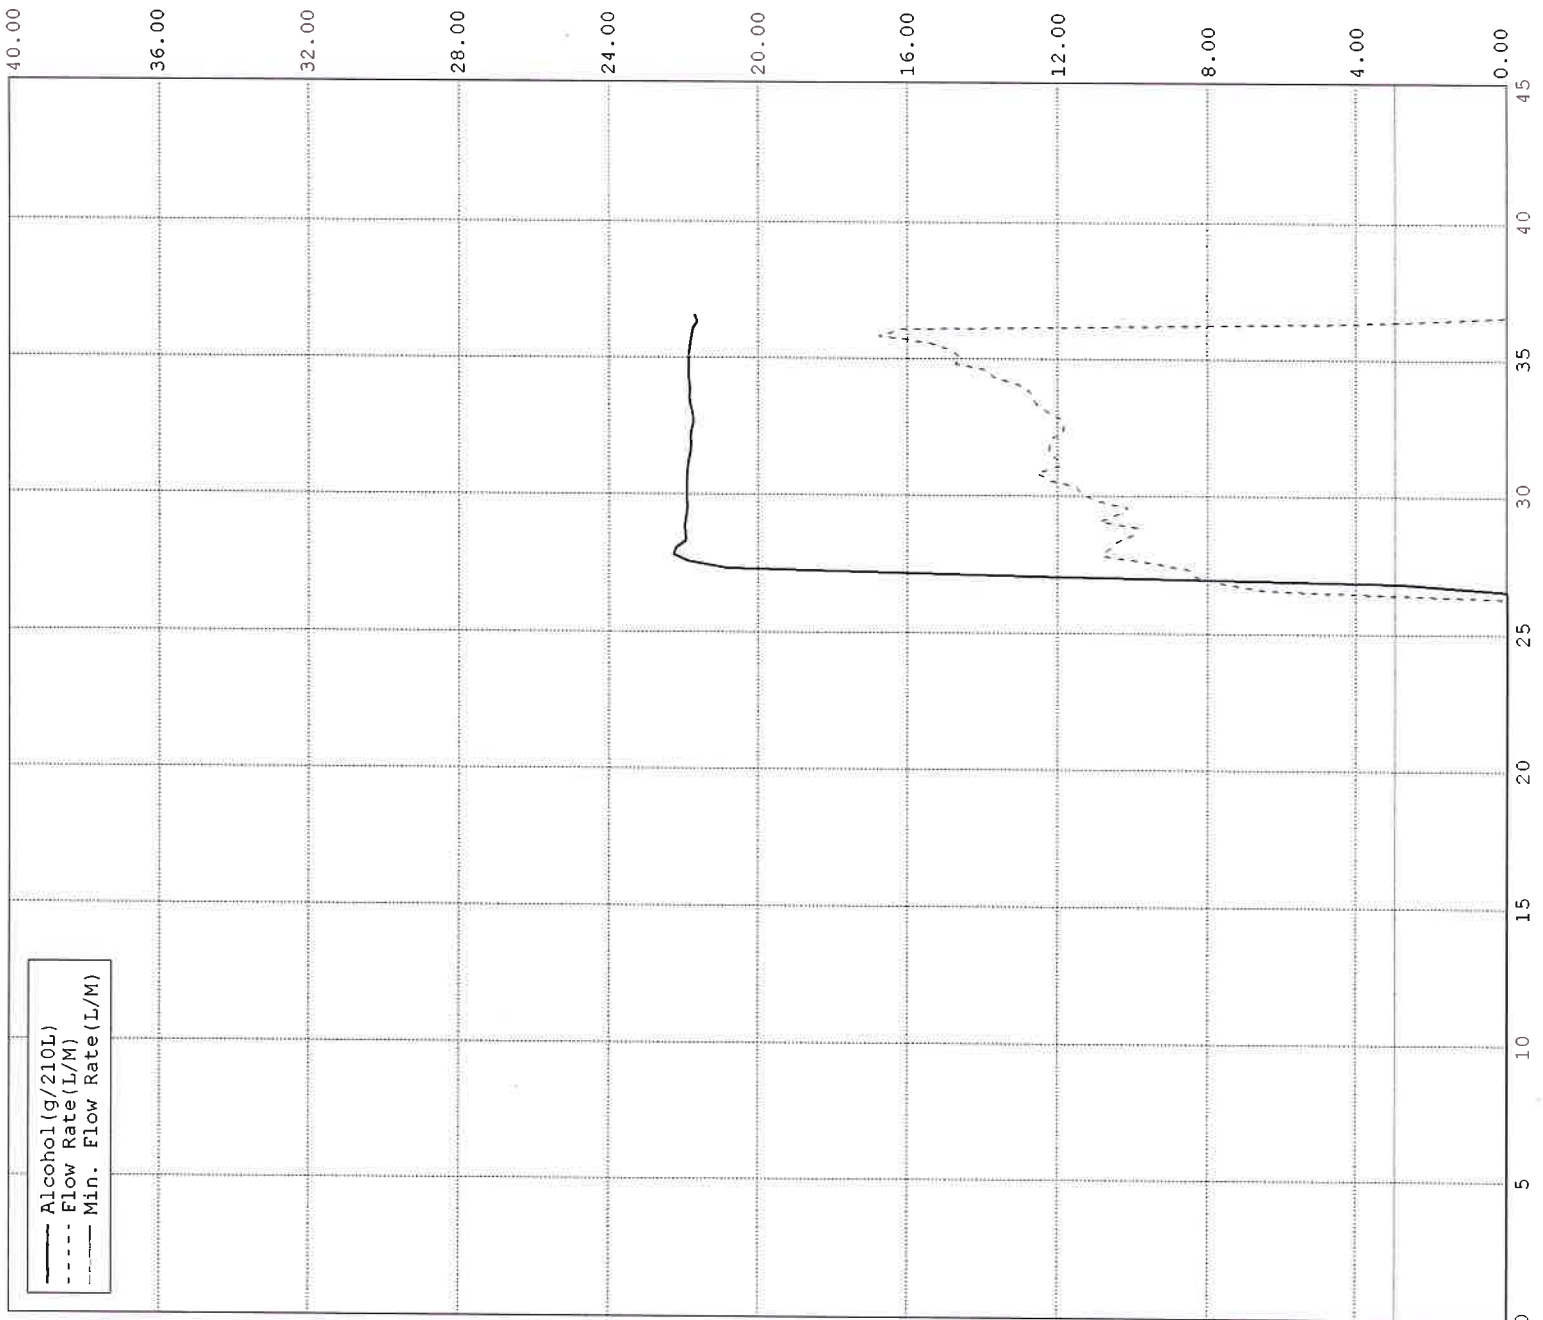

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100360

Date: 02/14/2024  
Time: 15:04:46

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-IPA

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1


CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.72: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK PASSED 15:06  
BLANK TEST 0.000 15:06  
INTERNAL STANDARD VERIFIED 15:06  
Xg = 0.120 (1.05%)  
EXTERNAL STANDARD 0.079 15:06  
X[1] = 0.0787 (-0.0018) (0.0023)  
BLANK TEST 0.000 15:07  
SUBJECT SAMPLE XXX 15:08  
X[1] = 0.1181 (-0.0314) (-0.0001)

Interference Detected

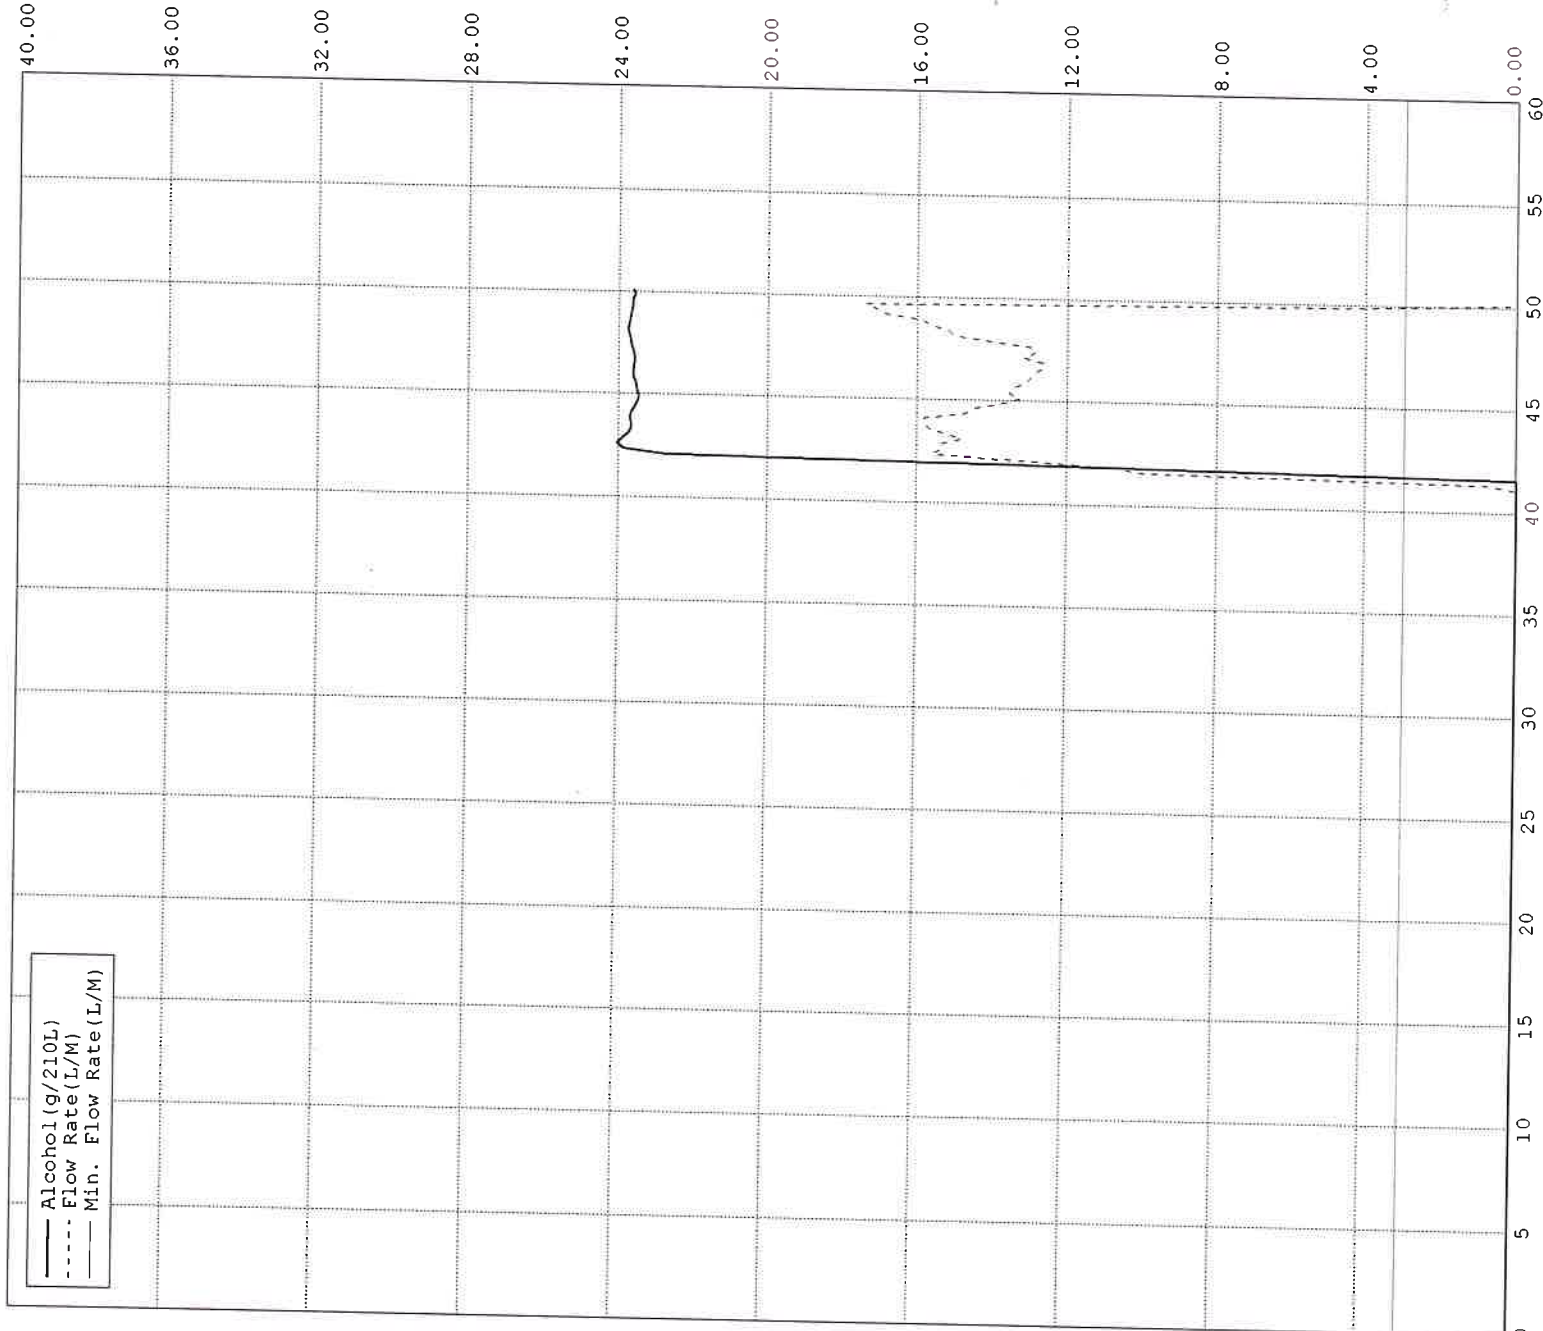

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100360

Date: 02/14/2024  
Time: 15:16:03

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-NEG

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237


DEPT/AGENCY:  
AAA1

CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.73: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	15:17
BLANK TEST	0.000	15:17
INTERNAL STANDARD	VERIFIED	15:17
Xg = 0.120 (1.05%)	0.079	15:17
EXTERNAL STANDARD	X[1] = 0.0788 (-0.0018) (0.0022)	
BLANK TEST	0.000	15:18
SUBJECT SAMPLE (Vol=1.96L)	0.094	15:19
X[1] = 0.0942 (-0.0009) (0.0011)	0.000	15:20
BLANK TEST	0.078	15:20
EXTERNAL STANDARD	X[1] = 0.0784 (-0.0020) (0.0009)	
BLANK TEST	0.000	15:21

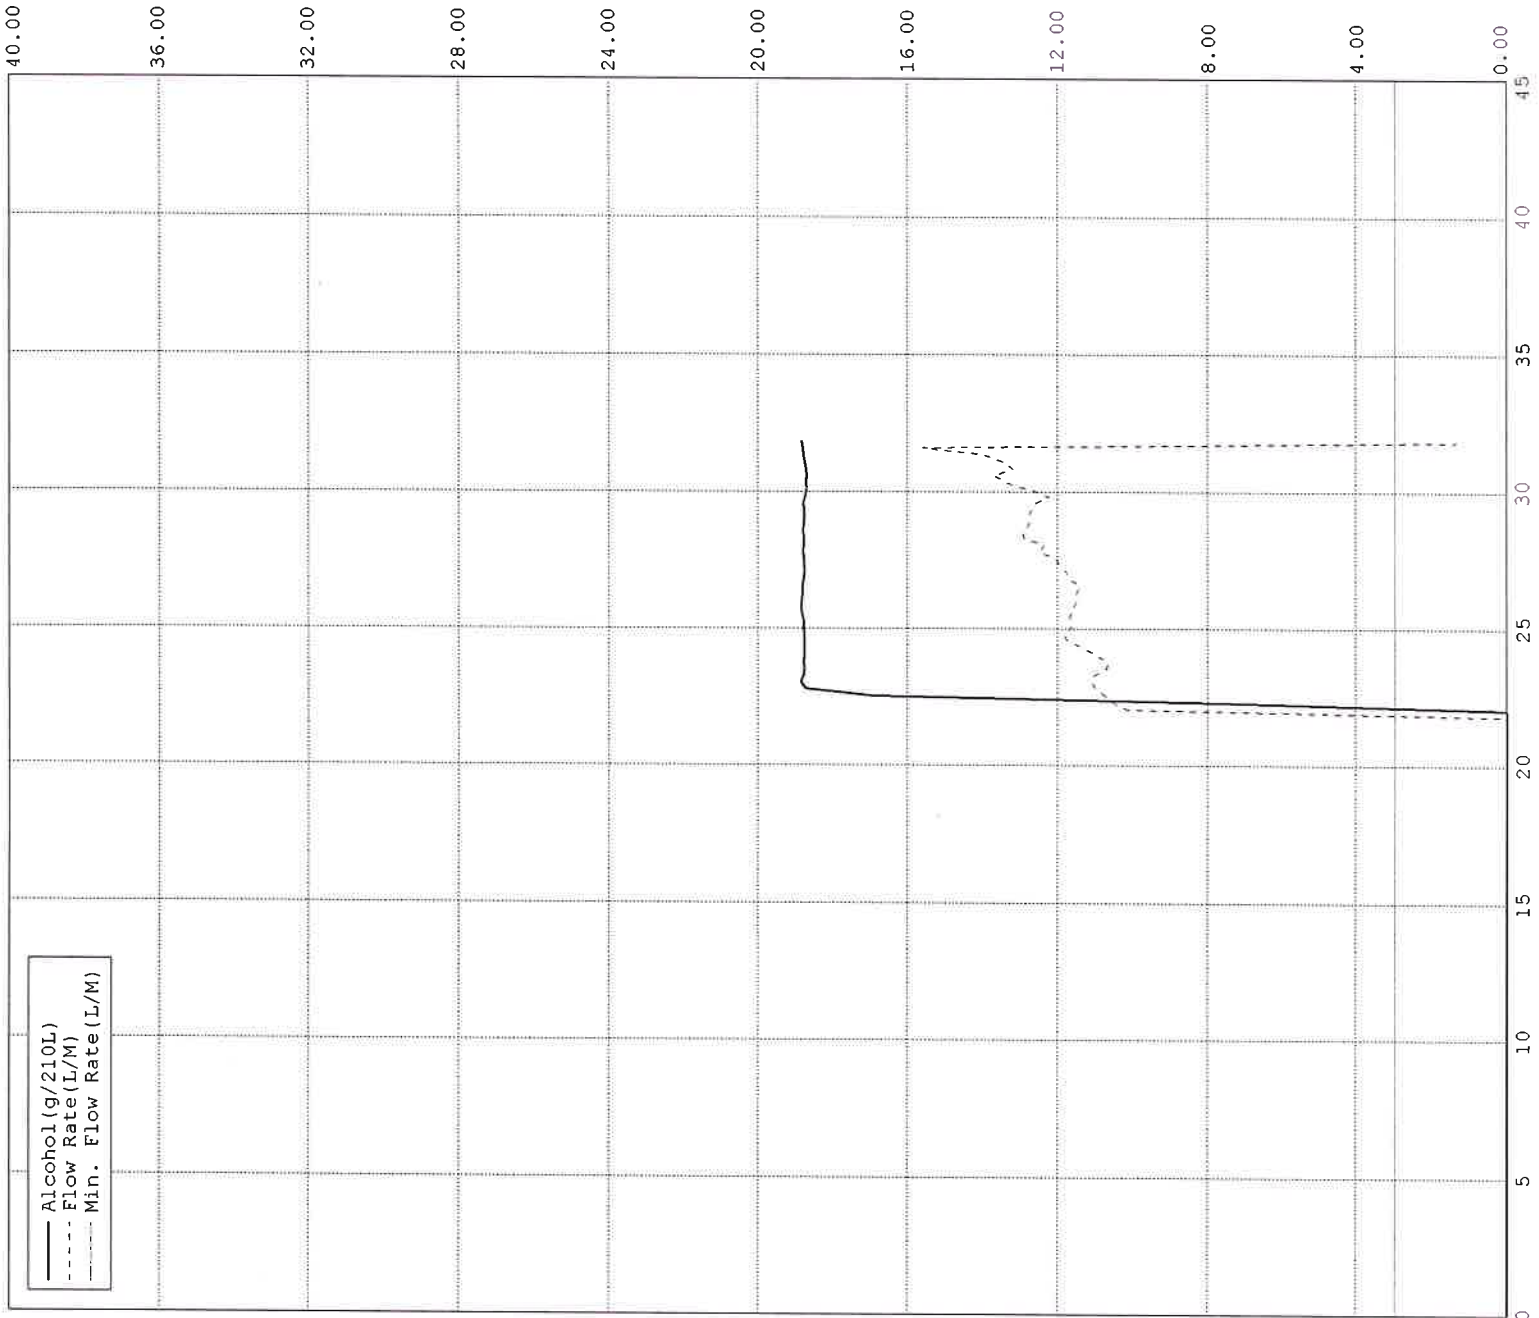

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100360

Date: 02/14/2024  
Time: 15:37:54

SUBJECT NAME:  
TEST TEST  
LICENSE #: NONDRINKING

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1

CASE/REPORT: 24-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.72: 0.079  
LOT #: AG310901  
EXPIRATION: 04/19/2025

DIAGNOSTIC CHECK	PASSED	15:38
BLANK TEST	0.000	15:39
INTERNAL STANDARD	VERIFIED	15:39
EXTERNAL STANDARD	0.079	15:39
BLANK TEST	0.000	15:40
SUBJECT SAMPLE (Vol=2.29L)	0.000	15:41
BLANK TEST	0.000	15:42
EXTERNAL STANDARD	0.079	15:42
BLANK TEST	0.000	15:43

