

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100364

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 08/16/2015

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.08: 0.080
LOT #: 09214080A2
EXPIRATION: 05/01/2016
TANK PRESSURE: 1108 psi

BLANK TEST	0.000	00:14
INTERNAL STANDARD	VERIFIED	00:15
EXTERNAL STANDARD	0.078	00:15
BLANK TEST	0.000	00:16
EXTERNAL STANDARD	0.079	00:16
BLANK TEST	0.000	00:17
EXTERNAL STANDARD	0.079	00:17
BLANK TEST	0.000	00:18
EXTERNAL STANDARD	0.079	00:18
BLANK TEST	0.000	00:19
EXTERNAL STANDARD	0.078	00:19
BLANK TEST	0.000	00:20

Average = 0.0786
Std Dev = 0.0005

Diagnostic Check

VERSIONS
DMT: 3.01
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
Breath Tube = 47.2°C PASSED

PUMP INFO

Flow Rate = 4.950 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO

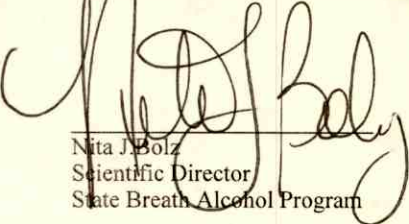
Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

9/10/2015

Subscribed and sworn before me this 10th day of Sept, 2015


Nikki Roth, Notary Public
My Commission Expires With Office



BMB
9/10/15