




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100681

Report Issue Date: 12/15/2025
Date Received: 2025-11-17
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.019	0.020
0.080	0.078	AG335202	0.077	0.077	0.077	0.077	0.078	0.077
0.300	0.294	AG427706	0.289	0.290	0.290	0.290	0.291	0.290

As Found - Evaluation Analyst: Kaija Swisher

As Found Conditions - Barometric Pressure (inHg): 29.38 Barometer Used: VWR S/N 240680771 Temperature (C): 20.8 Relative Humidity (%): 16

As-Found Lab Activity Date Range: 11/17/2025 - 11/18/2025

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.019	0.020	0.020	0.019	0.020	+/- 0.002
0.040	0.039	AG407908	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.078	AG436502	0.077	0.077	0.077	0.077	0.077	0.077	+/- 0.004
0.100	0.098	AG515610	0.097	0.097	0.097	0.097	0.096	0.097	+/- 0.004
0.150	0.147	AG515604	0.144	0.145	0.144	0.145	0.144	0.144	+/- 0.006
0.300	0.293	AG427706	0.292	0.292	0.292	0.291	0.292	0.292	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.26 Barometer Used: VWR S/N 240680771 Temperature (C): 21.6 Relative Humidity (%): 3

As-Left Lab Activity Date Range: 12/08/2025 - 12/08/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Carlie Glaister on 12/08/2025

carlie.glaister@alaska.gov

Technically and administratively reviewed by Kaija Swisher on 12/15/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100681 Analyst or Technician Name: Carlie Glaister

DataMaster DMT Calibration Start Date: 12/8/25

Diagnostic Test

☒ Perform Diagnostic Test (View Details)

☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

☒ Adjust Voltages (if needed)

- Lamp (2.60 V Maximum)
- Bias
- Cooler (2.00 V Maximum)
- Chopper Frequency
- Detector Voltage (-0.100V to 0.100V)

☒ Set RFI Sensitivity

☒ Adjust internal barometer reading to match NIST-traceable barometer

Barometer/Thermometer/Hygrometer S/N: 240680771

Calibration Due Date: 9/10/26

☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed

☒ Print Technician Screen

☒ Print "Cal Factors"

Minimum Volume Test

☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.26 Temperature(C) 21.6 Relative Humidity(%) 3

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

☒ Incomplete

☒ Maximum Attempts Exceeded

☒ Invalid

☒ Radio Frequency Interference (RFI)

☒ Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20250922KS Expiration Date: 12/22/25

Simulator S/N: DR4178 Thermometer Verification Performed? ☒

2. Isopropanol Reagent Lot Number: 20250922KS Expiration Date: 12/22/25

Simulator S/N: DR4177 Thermometer Verification Performed? ☒

3. Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 3/19/27 → sin.

Simulator S/N: DR4163 Thermometer Verification Performed? ☒ 12/22/25 → prep.

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 3/14/27

Administrative

☒ Verify Stylus Calibration

☒ Reset Options

☒ Clear Memory

☒ Verification of Calibration (VOC)

☒ Perform Non-Drinking Subject Test

☒ Upload Instrument

☒ Remove Dry Gas Tank Before Shutdown

☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 12/8/25

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): AKG

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

 Alaska Department of Public Safety
 DATAMASTER dmt: 100681

Date: 12/08/2025
 Time: 10:20:33

VERSIONS

DMT: 3.02
 PIC: 3.03
 Modem: 2.6
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 44.9°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.67 V	PASSED
(1.02 V - 2.38 V)	
Cooler Voltage = 1.58 V	PASSED
(0.92 V - 2.14 V)	
Bias Voltage = 78 V	PASSED
(47 V - 109 V)	
Chopper Freq = 524 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.2 in	

PUMP INFO

Flow Rate = 4.324 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.002 V <= 0.010 V)	
PUMP OFF	PASSED
(0.002 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

Xq = 0.108 1.07%	PASSED
(0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100681

Date: 12/08/2025

Time: 10:28 AM

Temperatures (°C)

Sample Cell: 48.7°C

Breath Tube: 44.4°C

Current Barometer 29.3 in

Volume (Ltr) 1.59

Settings

Lamp: 1.72 V

Bias: 78 V

Cooler: 1.63 V

Chopper: 524 Hz

Voltages (V)

Flow: 1.07 V

Detector: -0.004 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100681

Date: 10/29/2021
Time: 13:14:55

OPERATOR NAME:
CARLIE GLAISTER
CERTIFICATE #: 10436

Ca	=	0.1000		
CAL	=	0.984251	0.800	<= CAL < 1.200
b1	=	0.0004	0.0000	<= b1 < 0.0040
b2	=	0.0051	0.0010	<= b2 < 0.0100
b3	=	0.0001	0.0000	<= b3 < 0.0040
Xq	=	0.1066	0.0500	<= Xq < 0.2000
a21	=	1.158479	1.050	<= a21 < 1.300
a31	=	0.492122	0.300	<= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
 DATA MASTER dmt: 100681

Date: 12/08/2025
 Time: 10:29:08

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX


OPERATOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

DEPT/AGENCY:
 MINIMUM VOLUME TEST
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.27: 0.078
 LOT #: AG436502
 EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	10:30
BLANK TEST	0.000	10:31
INTERNAL STANDARD	VERIFIED	10:31
EXTERNAL STANDARD	0.077	10:31
BLANK TEST	0.000	10:32
SUBJECT SAMPLE (Vol=1.56L)	0.000	10:33
BLANK TEST	0.000	10:34
EXTERNAL STANDARD	0.077	10:34
BLANK TEST	0.000	10:35

CKB

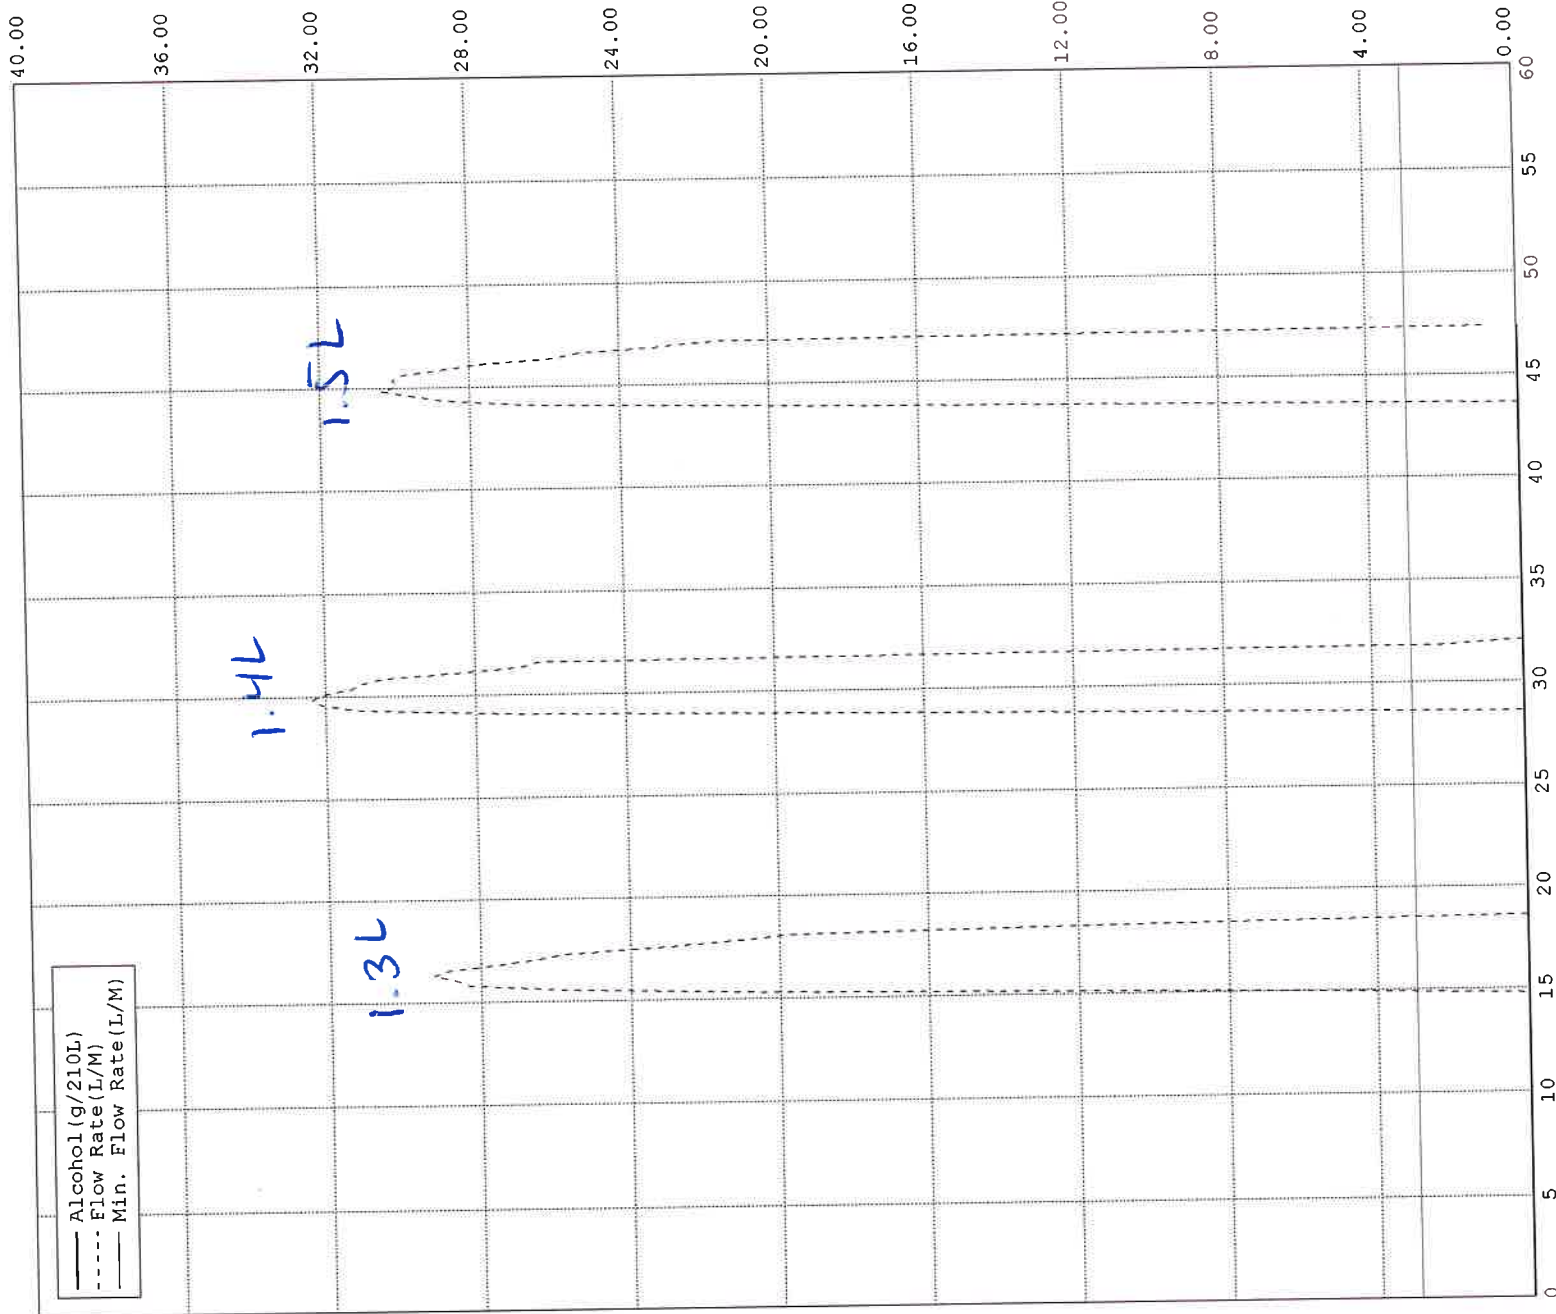

LINEARITY CHECK


Alaska Department of Public Safety
 DATAMASTER dmt: 100681

Date: 12/08/2025
 Time: 10:39:56

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0196	0.0005
0.039	0.0390	0.0000
0.078	0.0770	0.0000
0.098	0.0968	0.0004
0.147	0.1444	0.0005
0.293	0.2918	0.0004

SLOPE = 0.995575
 R^2 = 0.999938

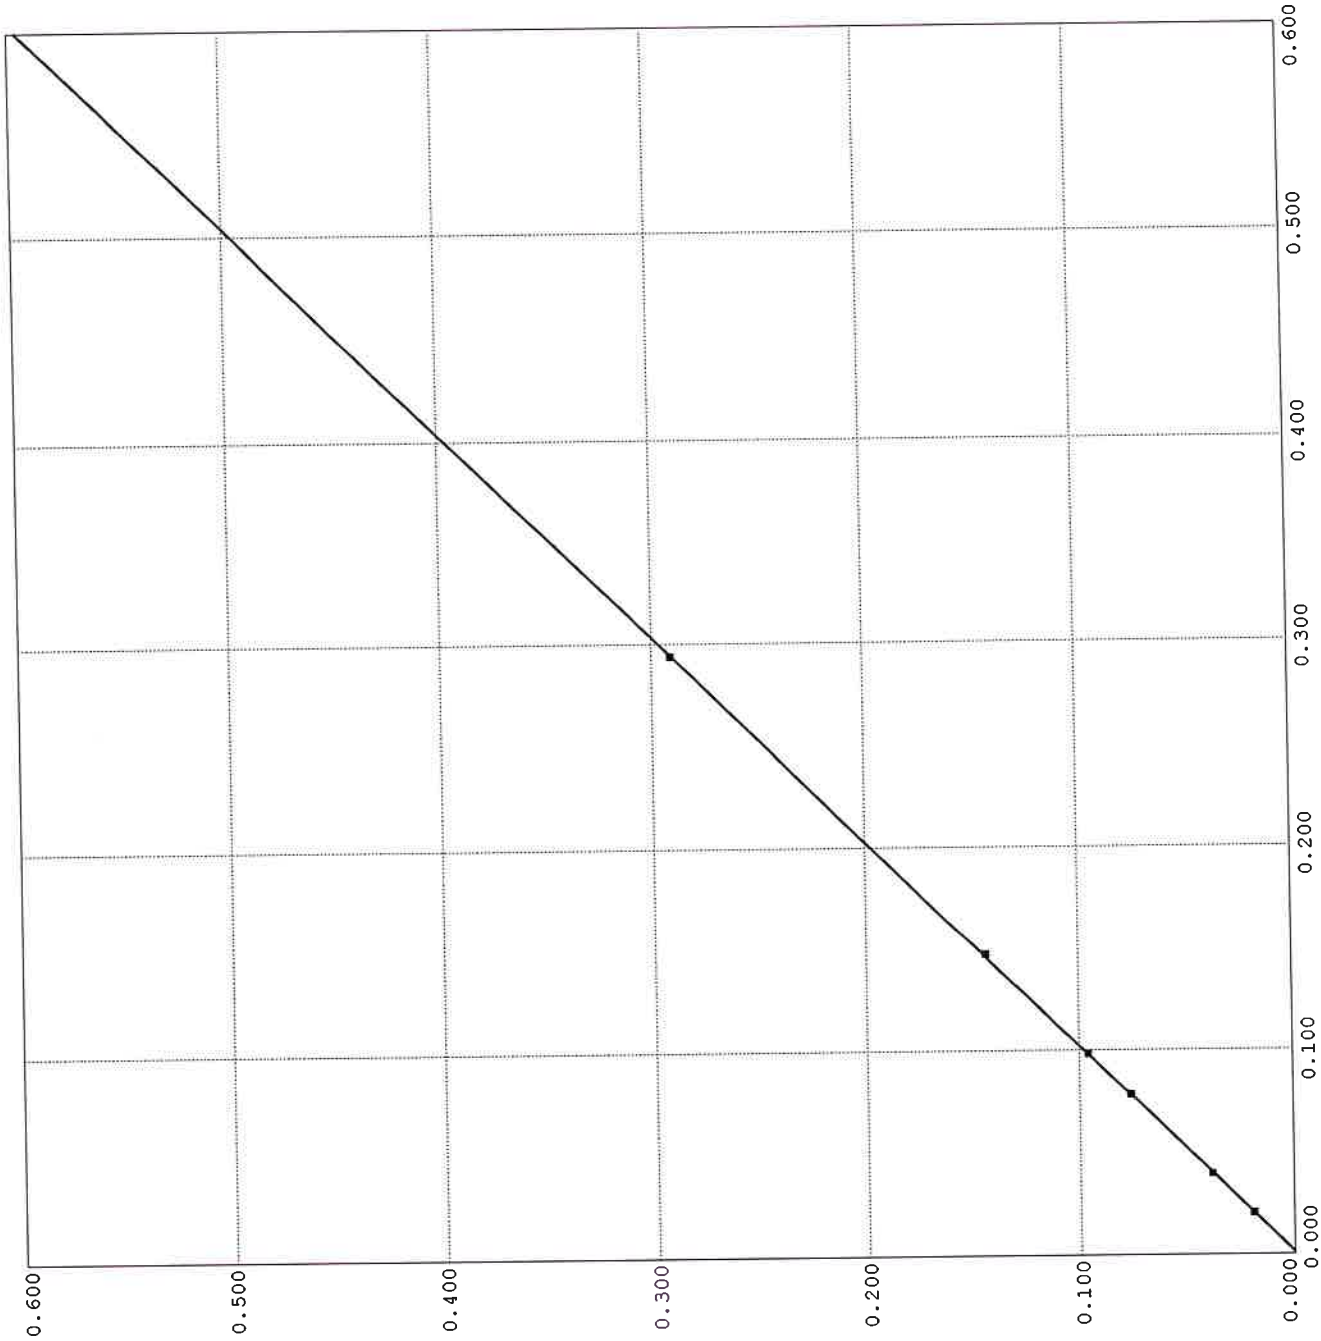

OK

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100681






Date: 12/08/2025
Time: 10:39:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.27: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 224 psi

BLANK TEST	0.000	10:41
INTERNAL STANDARD	VERIFIED	10:41
EXTERNAL STANDARD	0.020	10:41
BLANK TEST	0.000	10:42
EXTERNAL STANDARD	0.019	10:42
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.020	10:43
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.020	10:45
BLANK TEST	0.000	10:45
EXTERNAL STANDARD	0.019	10:46
BLANK TEST	0.000	10:47

Average = 0.0196
Std Dev = 0.0005

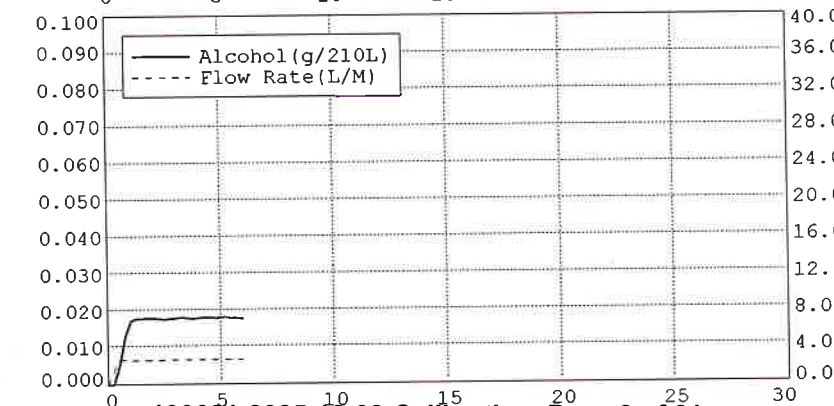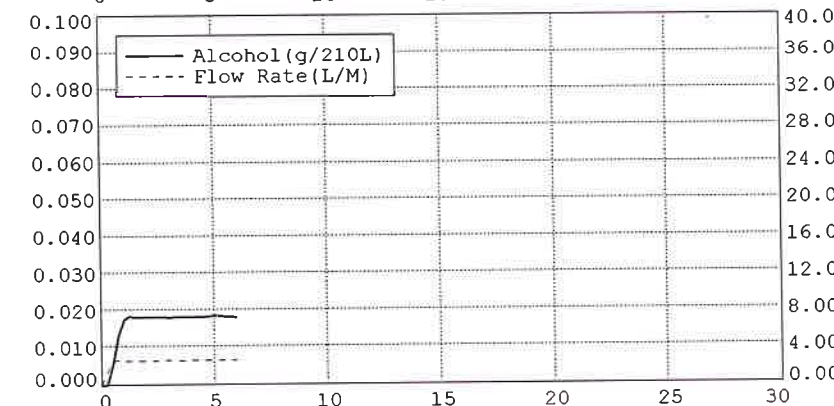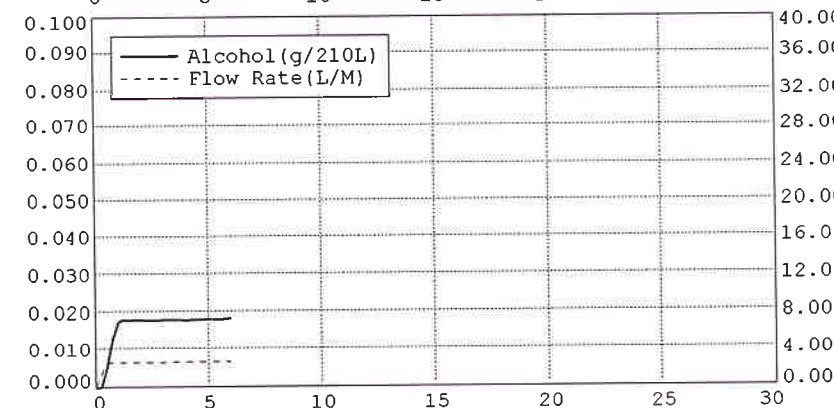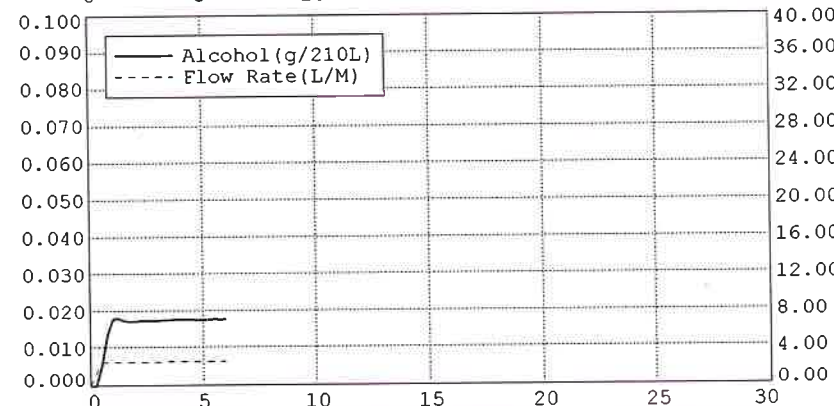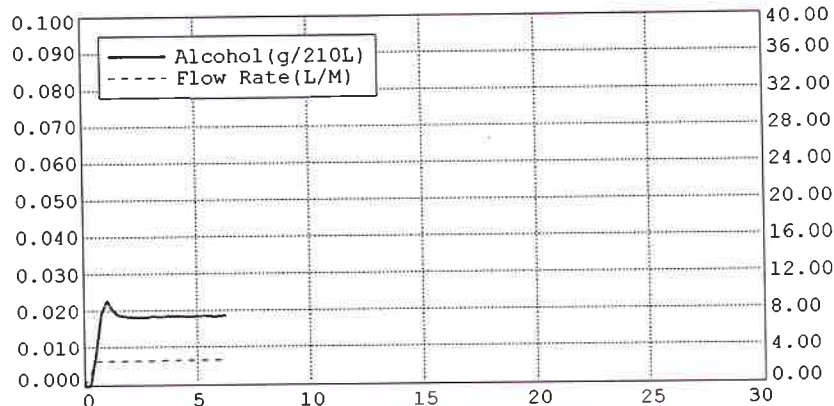

LINEARITY CHECK: Control Test 2






Alaska Department of Public Safety
DATAMASTER dmt: 100681

Date: 12/08/2025
Time: 10:48:29

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.040
TARGET AT 29.27: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 538 psi

BLANK TEST	0.000	10:49
INTERNAL STANDARD	VERIFIED	10:49
EXTERNAL STANDARD	0.039	10:50
BLANK TEST	0.000	10:51
EXTERNAL STANDARD	0.039	10:51
BLANK TEST	0.000	10:52
EXTERNAL STANDARD	0.039	10:52
BLANK TEST	0.000	10:53
EXTERNAL STANDARD	0.039	10:53
BLANK TEST	0.000	10:54
EXTERNAL STANDARD	0.039	10:54
BLANK TEST	0.000	10:55

Average = 0.0390
Std Dev = 0.0000

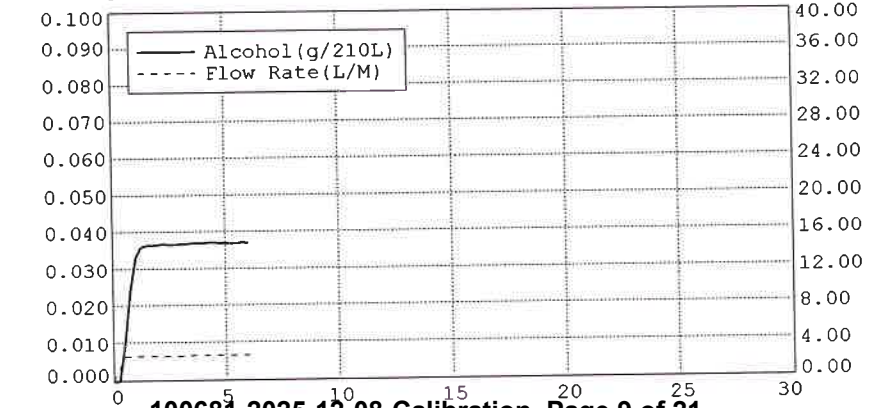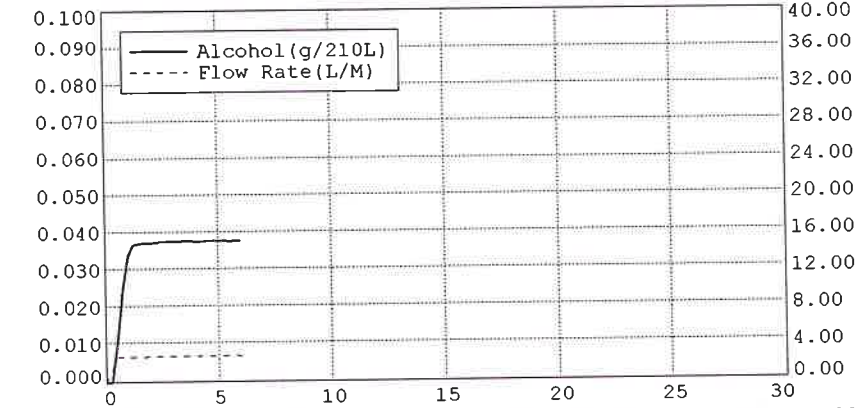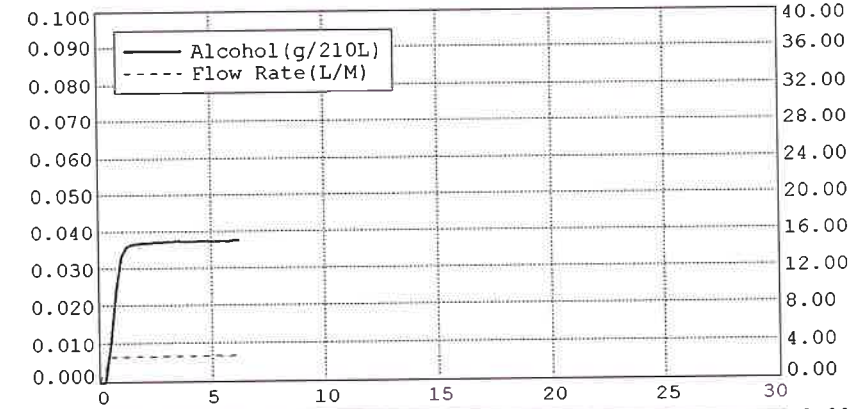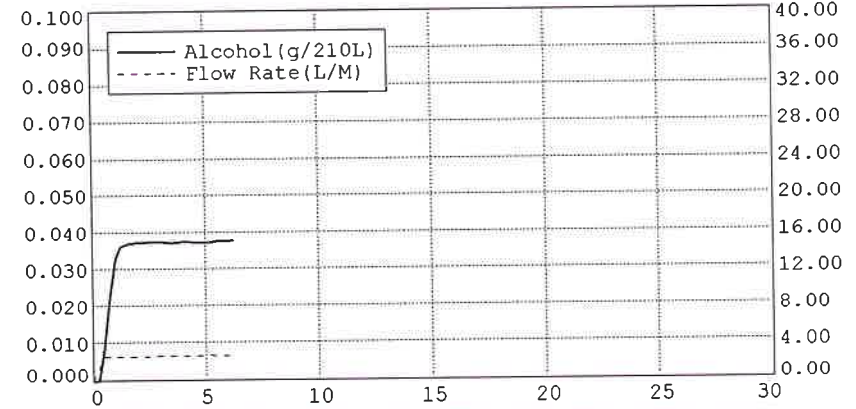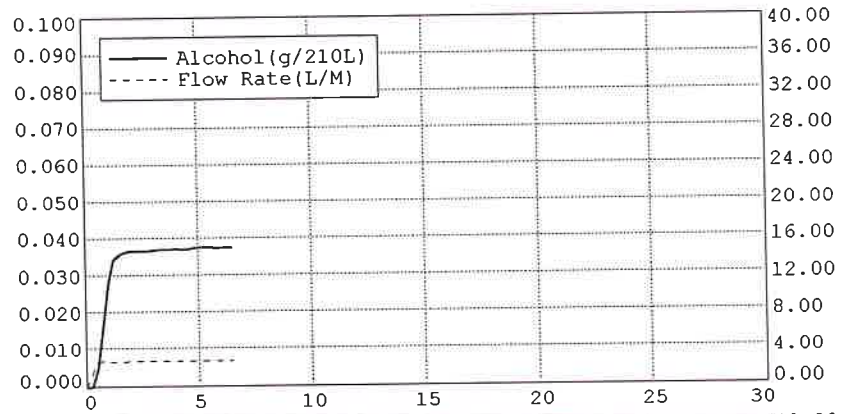

LINEARITY CHECK: Control Test 3






Alaska Department of Public Safety
DATAMASTER dmt: 100681

Date: 12/08/2025
Time: 10:56:28

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG436502
EXPIRATION: 12/30/2026
TANK PRESSURE: 1159 psi

BLANK TEST	0.000	10:57
INTERNAL STANDARD	VERIFIED	10:57
EXTERNAL STANDARD	0.077	10:58
BLANK TEST	0.000	10:58
EXTERNAL STANDARD	0.077	10:59
BLANK TEST	0.000	11:00
EXTERNAL STANDARD	0.077	11:00
BLANK TEST	0.000	11:01
EXTERNAL STANDARD	0.077	11:01
BLANK TEST	0.000	11:02
EXTERNAL STANDARD	0.077	11:02
BLANK TEST	0.000	11:03

Average = 0.0770
Std Dev = 0.0000

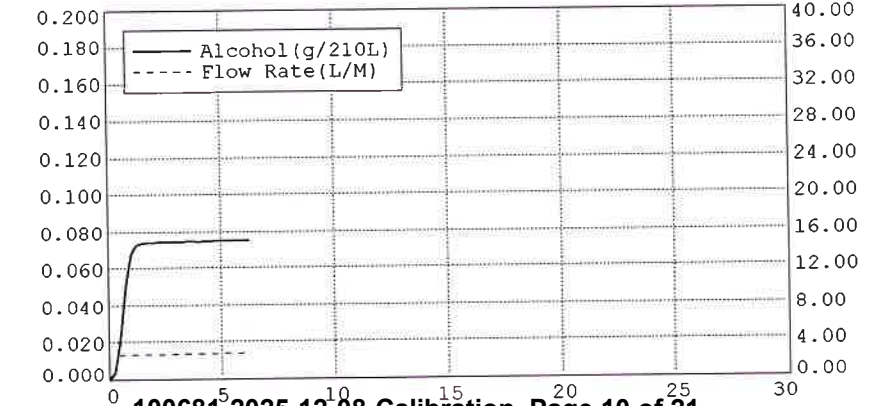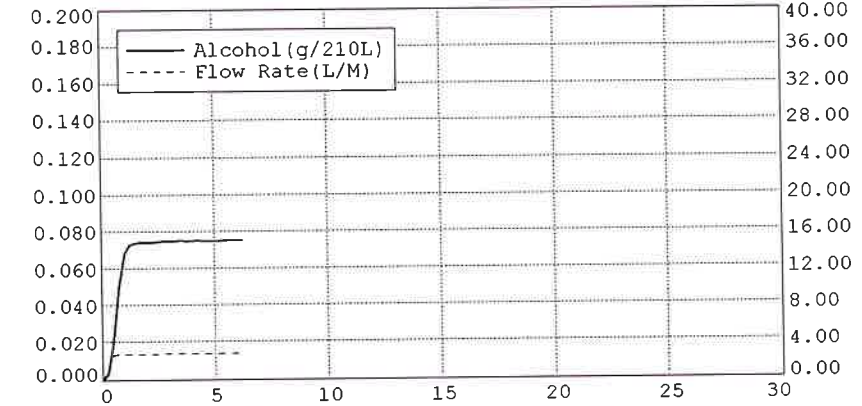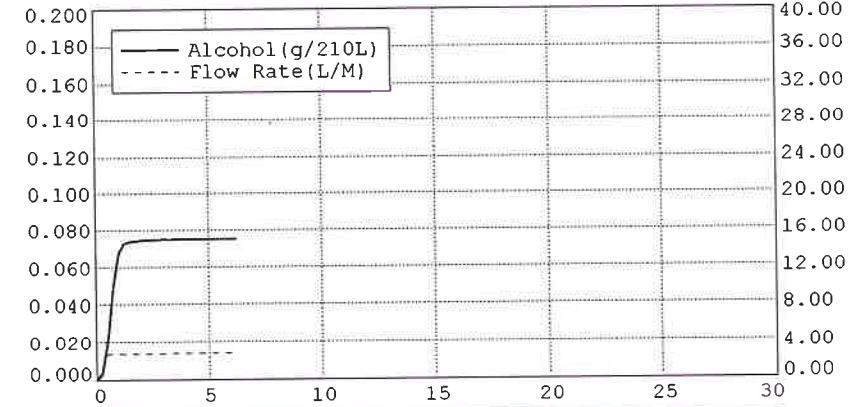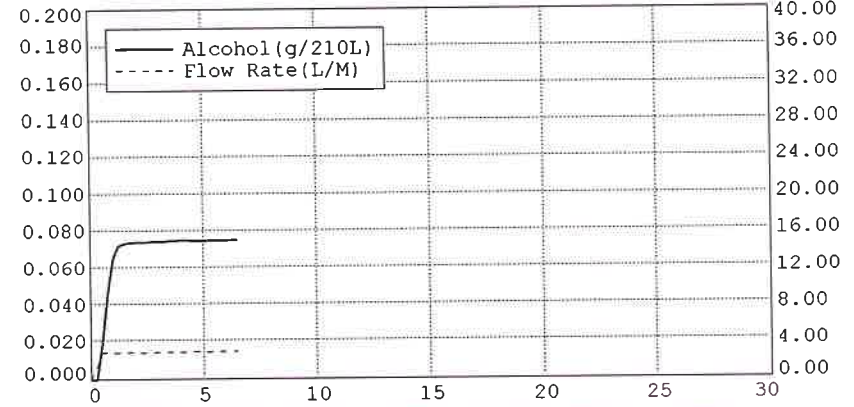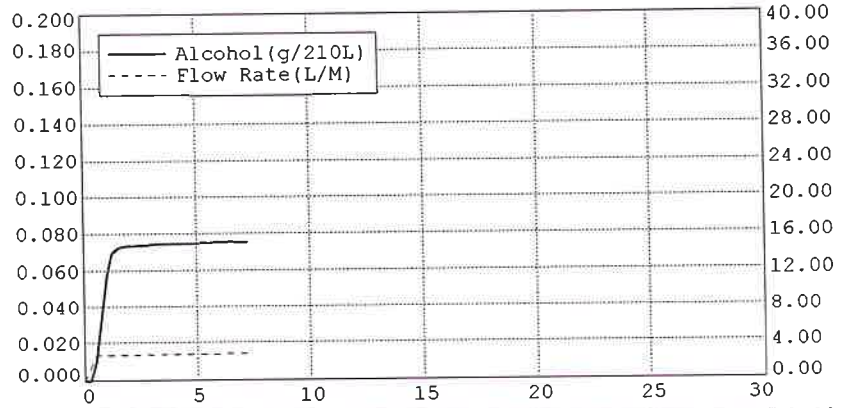

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100681






Date: 12/08/2025
Time: 11:05:19

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.27: 0.098
LOT #: AG515610
EXPIRATION: 06/05/2027
TANK PRESSURE: 1168 psi

BLANK TEST	0.000	11:06
INTERNAL STANDARD	VERIFIED	11:06
EXTERNAL STANDARD	0.097	11:06
BLANK TEST	0.000	11:07
EXTERNAL STANDARD	0.097	11:08
BLANK TEST	0.000	11:08
EXTERNAL STANDARD	0.097	11:09
BLANK TEST	0.000	11:10
EXTERNAL STANDARD	0.097	11:10
BLANK TEST	0.000	11:11
EXTERNAL STANDARD	0.096	11:11
BLANK TEST	0.000	11:12

Average = 0.0968
Std Dev = 0.0004

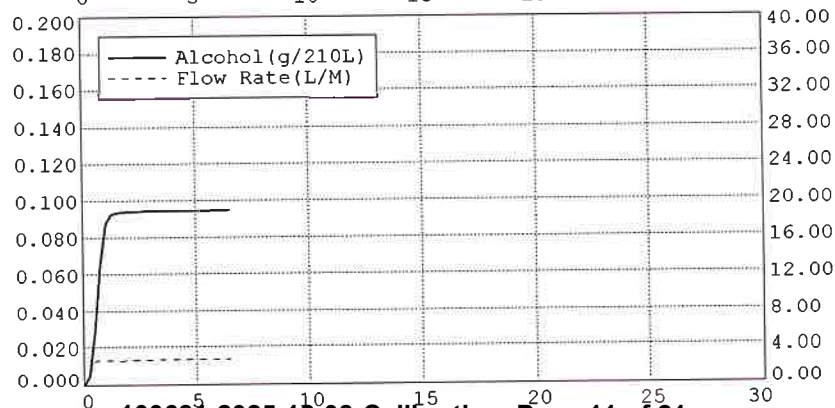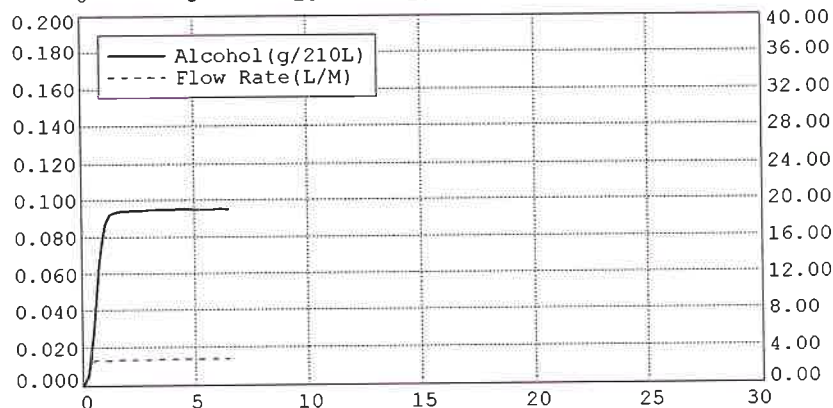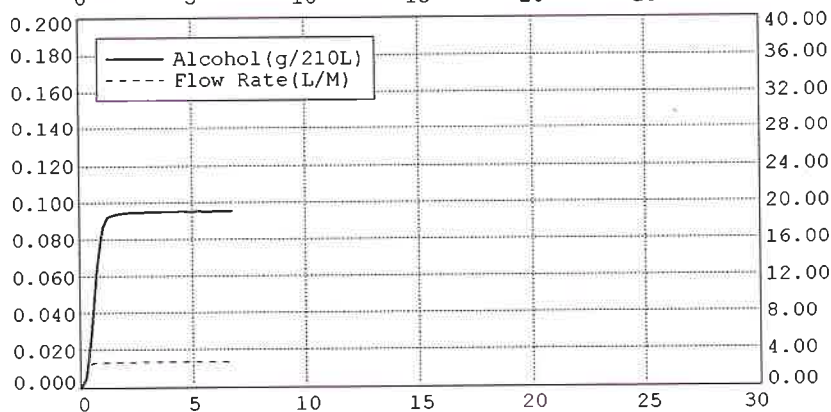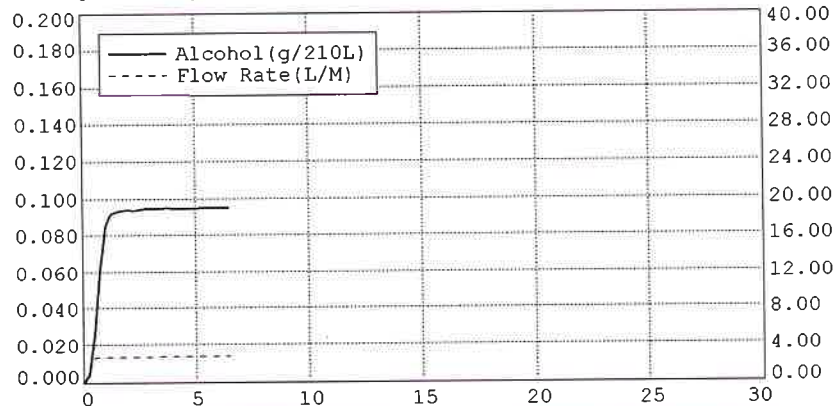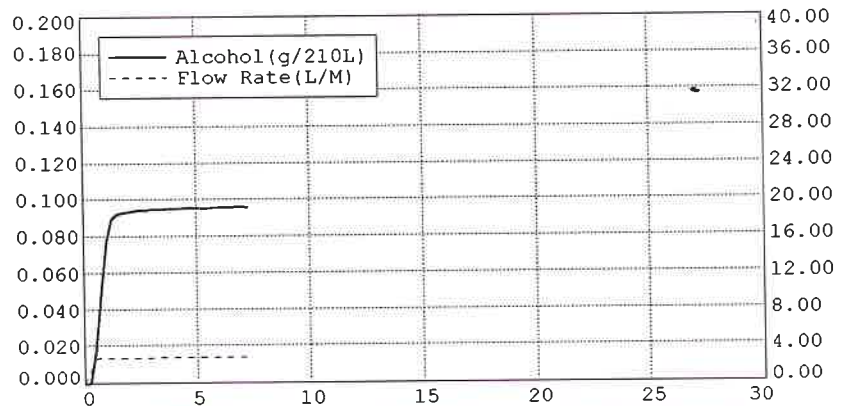

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100681






Date: 12/08/2025
Time: 11:12:50

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.27: 0.147
LOT #: AG515604
EXPIRATION: 06/05/2027
TANK PRESSURE: 663 psi

BLANK TEST	0.000	11:14
INTERNAL STANDARD	VERIFIED	11:14
EXTERNAL STANDARD	0.144	11:14
BLANK TEST	0.000	11:15
EXTERNAL STANDARD	0.145	11:15
BLANK TEST	0.000	11:16
EXTERNAL STANDARD	0.144	11:16
BLANK TEST	0.000	11:17
EXTERNAL STANDARD	0.145	11:17
BLANK TEST	0.000	11:18
EXTERNAL STANDARD	0.144	11:18
BLANK TEST	0.000	11:19

Average = 0.1444
Std Dev = 0.0005

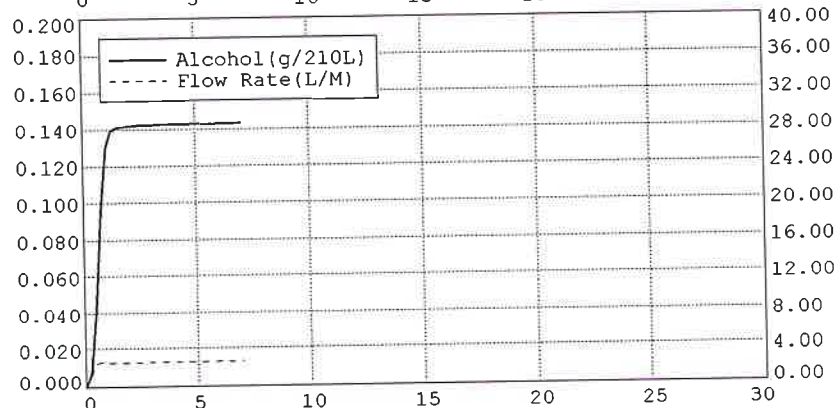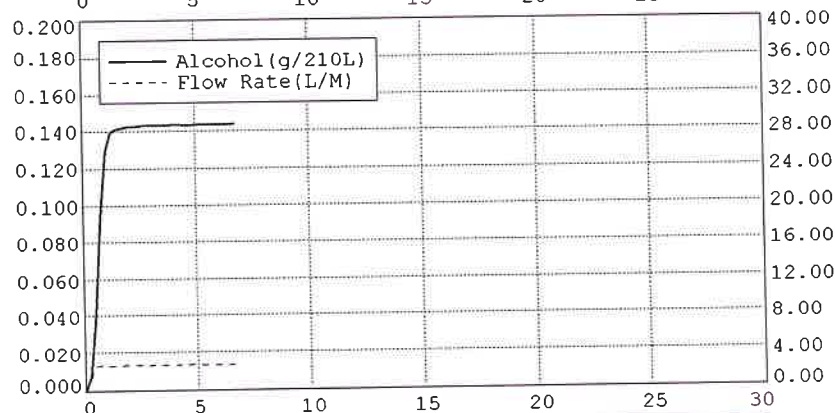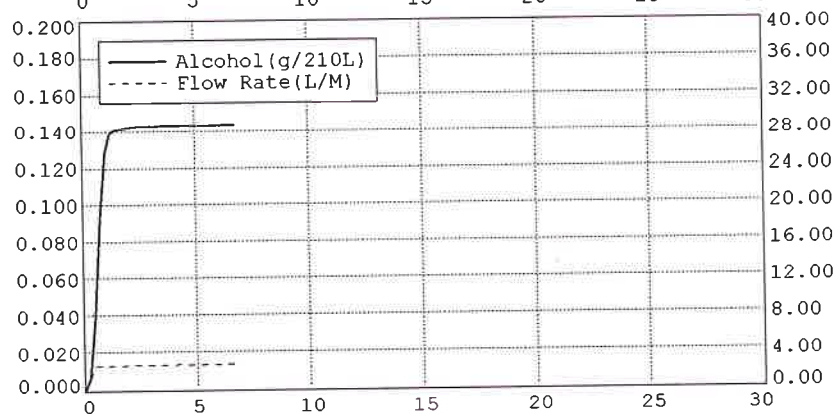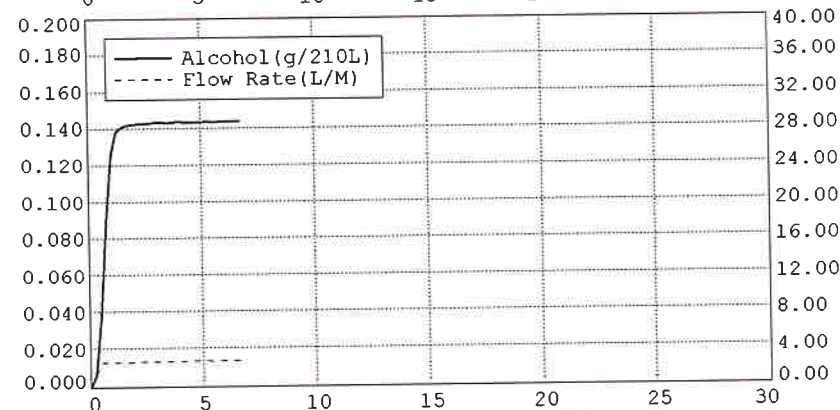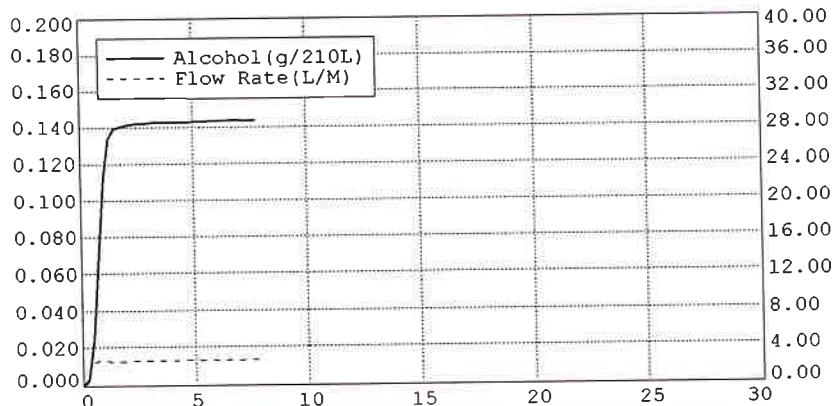

LINEARITY CHECK: Control Test 6






Alaska Department of Public Safety
DATAMASTER dmt: 100681

Date: 12/08/2025
Time: 11:24:45

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.300
TARGET AT 29.27: 0.293
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 387 psi

BLANK TEST	0.000	11:26
INTERNAL STANDARD	VERIFIED	11:26
EXTERNAL STANDARD	0.292	11:26
BLANK TEST	0.000	11:27
EXTERNAL STANDARD	0.292	11:27
BLANK TEST	0.000	11:28
EXTERNAL STANDARD	0.292	11:28
BLANK TEST	0.000	11:29
EXTERNAL STANDARD	0.291	11:30
BLANK TEST	0.000	11:30
EXTERNAL STANDARD	0.292	11:31
BLANK TEST	0.000	11:32

Average = 0.2918
Std Dev = 0.0004

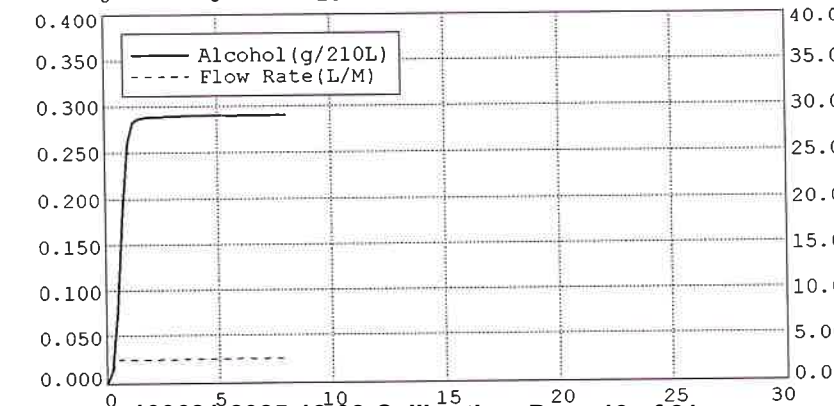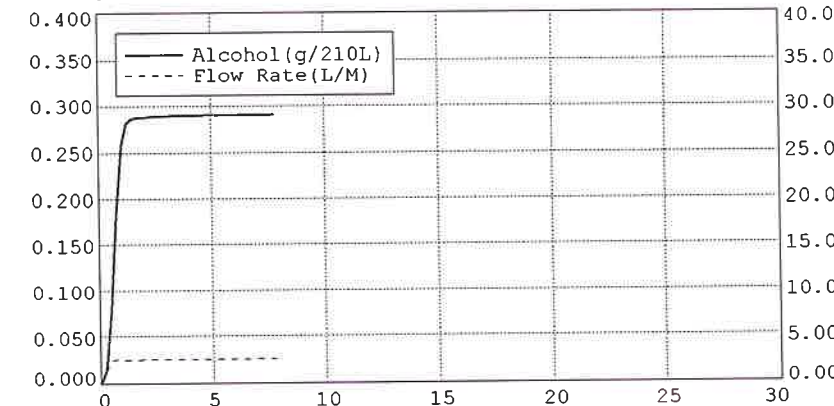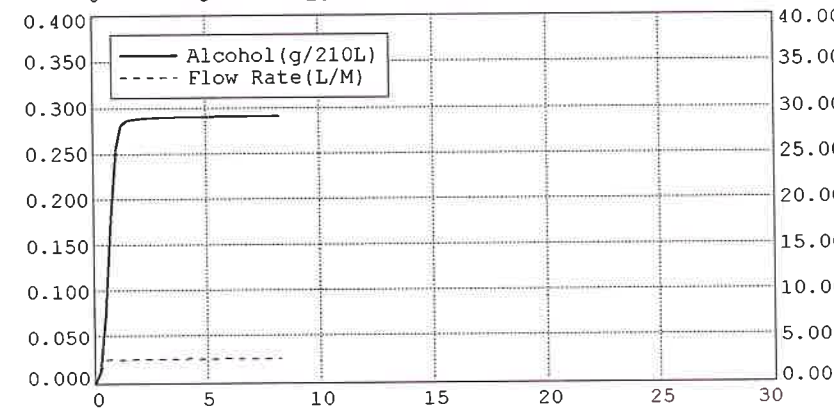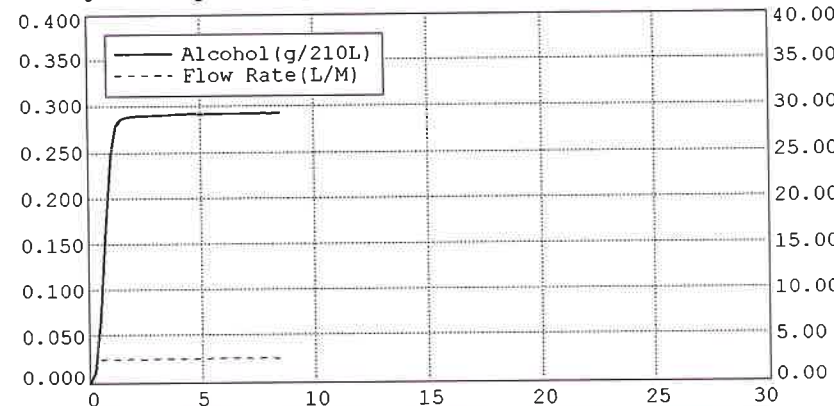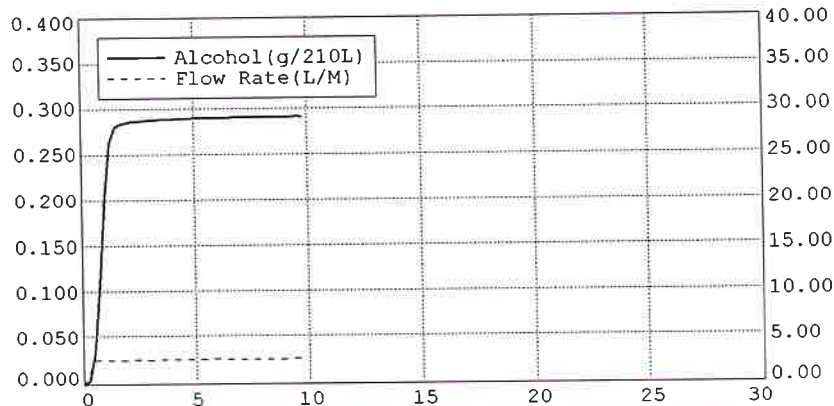

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100681

Date: 12/08/2025

Time: 11:38:44

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INCOMPLETE

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.27: 0.078

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 11:43
0.000 11:43
VERIFIED 11:43
0.078 11:43
0.000 11:44
INCOMPLETE 11:46

OK

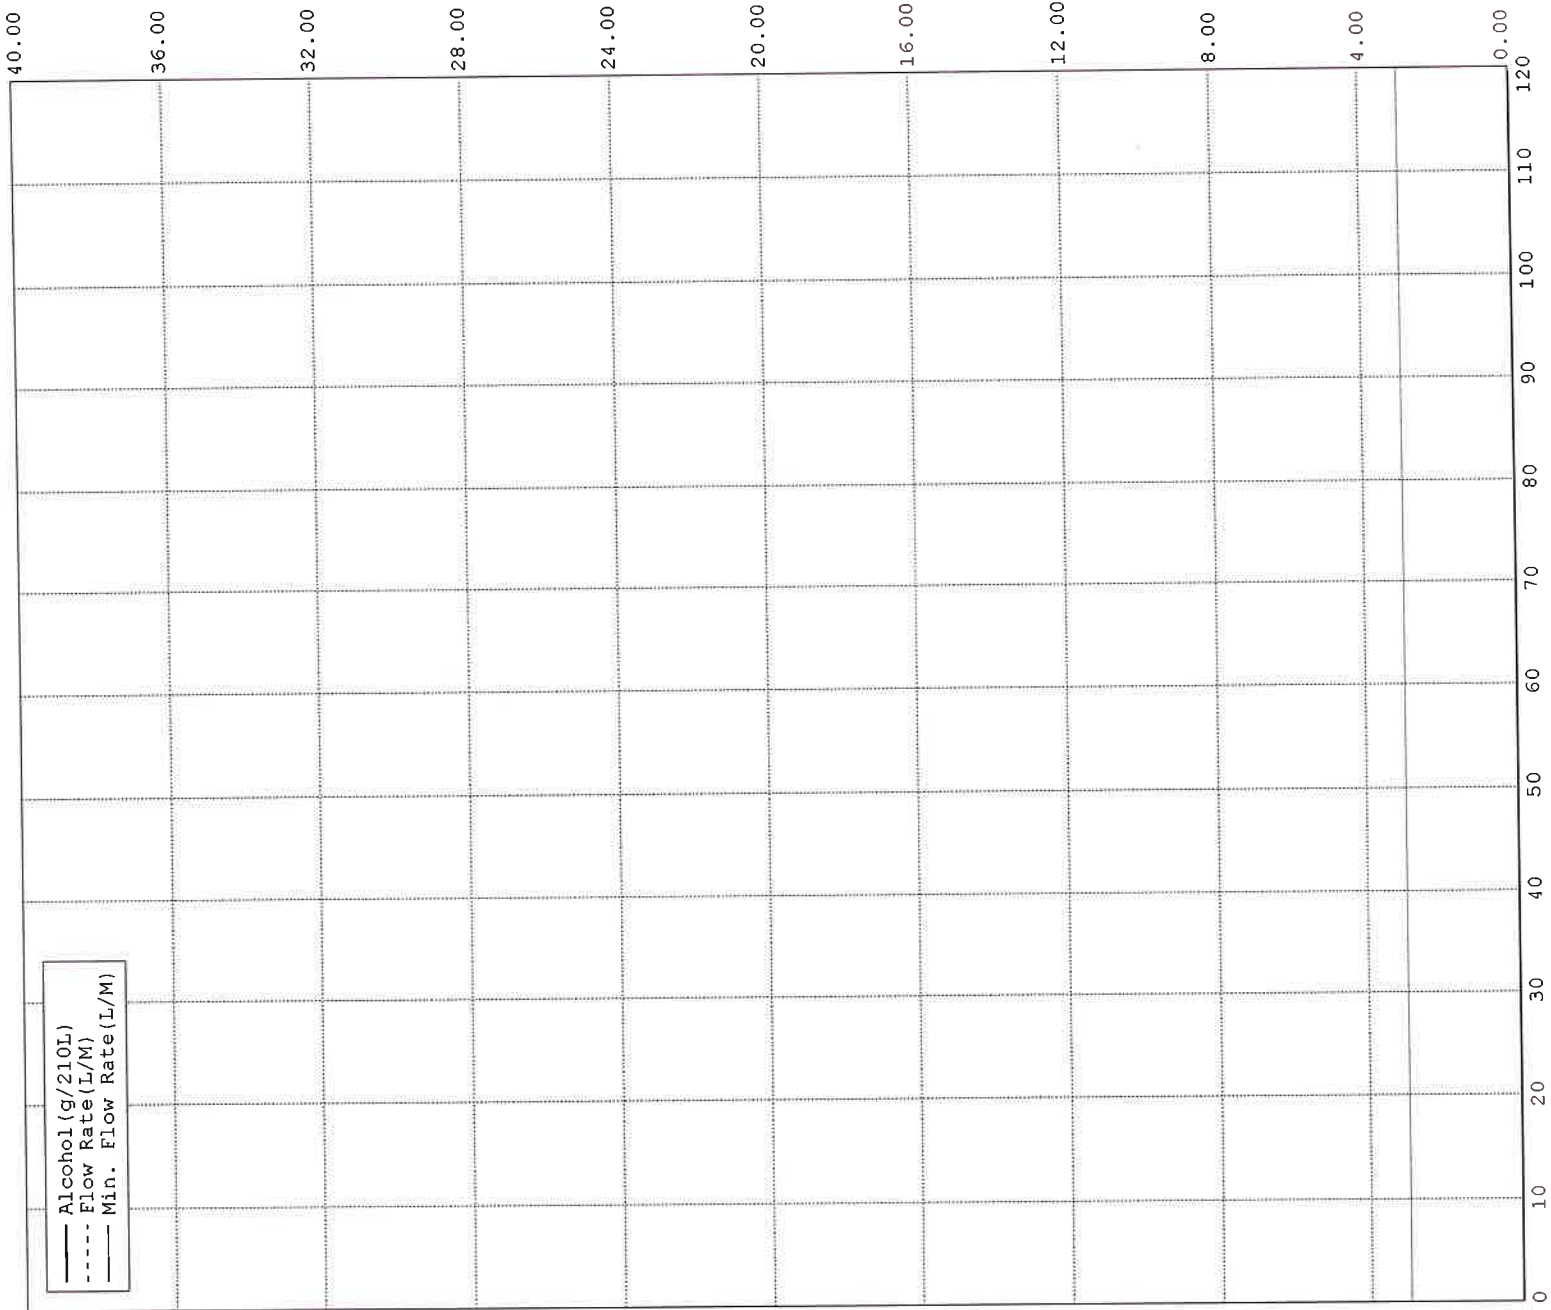

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 12/08/2025
Time: 11:52:57

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
MAX ATTEMPTS EXCEEDED
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	11:56
BLANK TEST	0.000	11:56
INTERNAL STANDARD	VERIFIED	11:56
EXTERNAL STANDARD	0.078	11:56
BLANK TEST	0.000	11:57
SUBJECT SAMPLE	XXX	11:58

Maximum Attempts Exceeded

Handwritten signature/initials

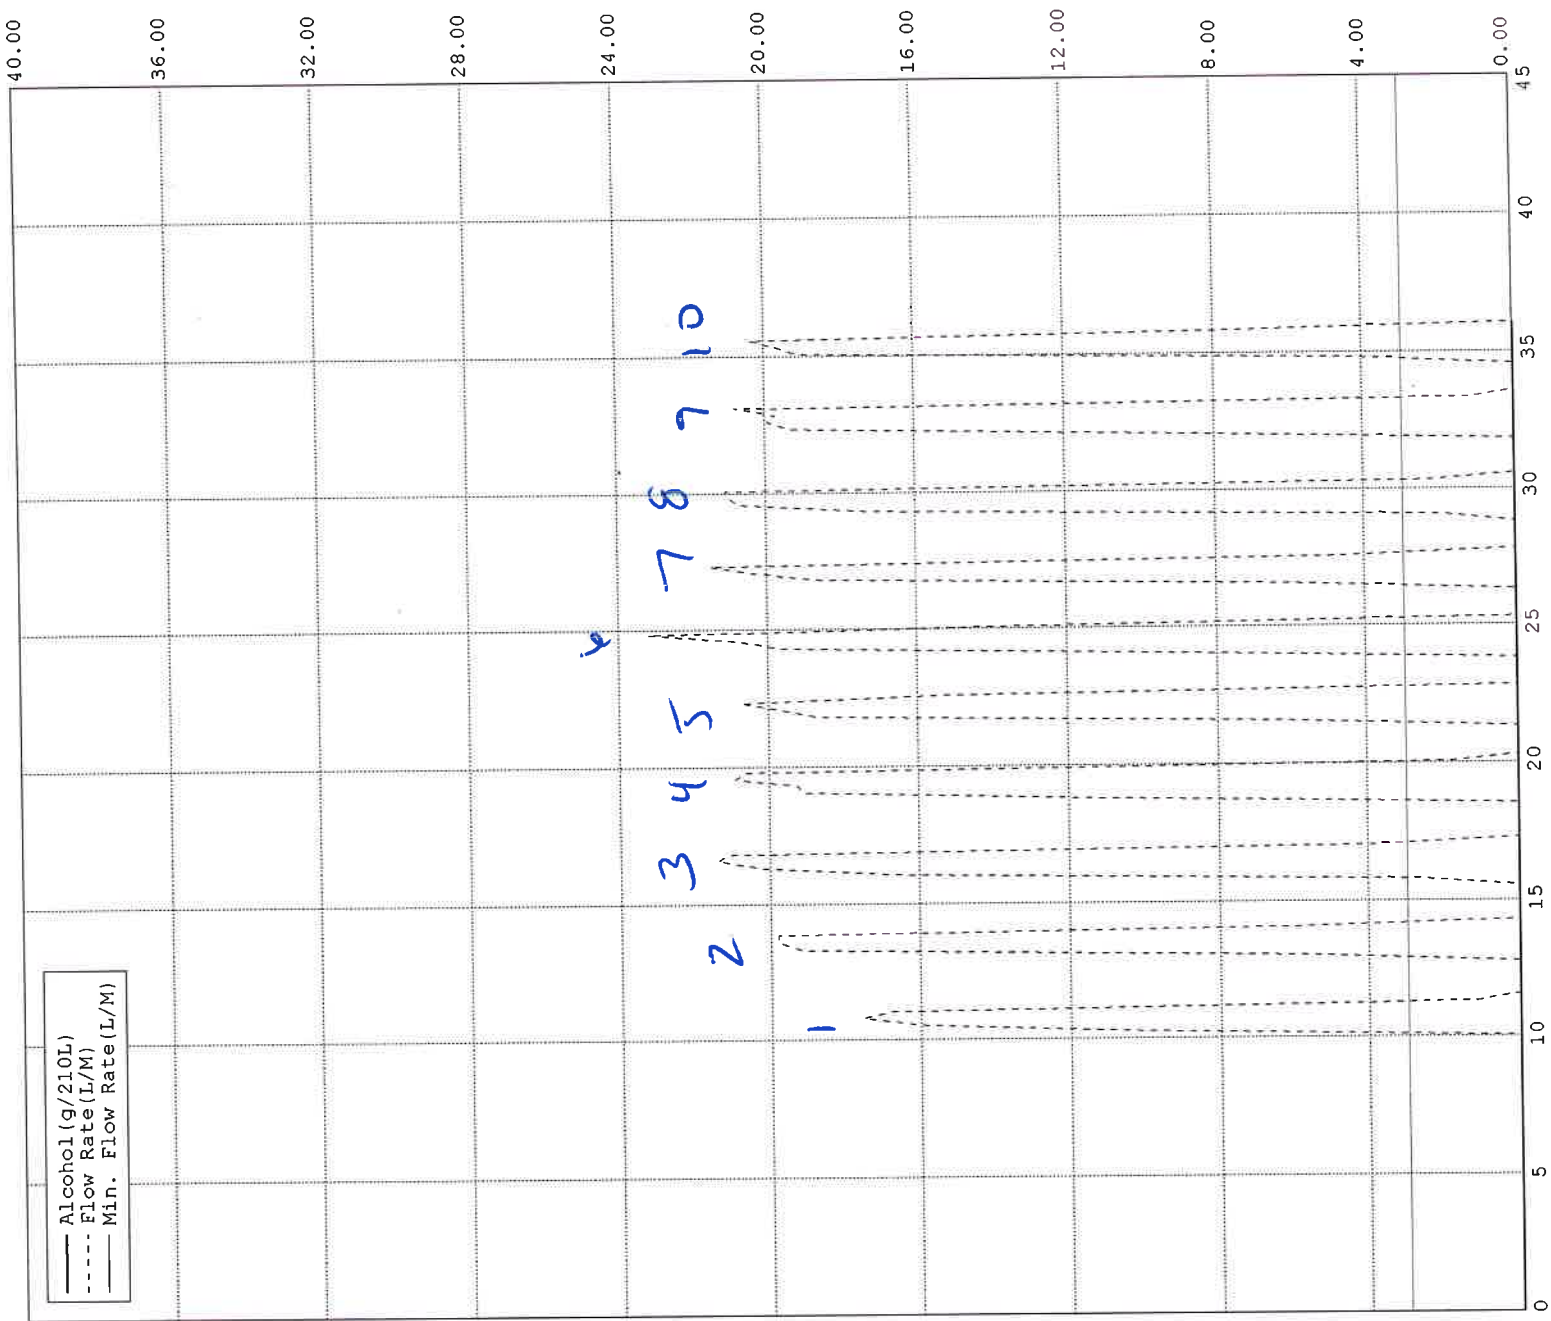

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 12/08/2025

Time: 14:10:04

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INVALID

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.27: 0.078

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 14:11

0.000 14:11


VERIFIED 14:11

0.077 14:11

0.000 14:12

INVALID 14:13

Handwritten signature

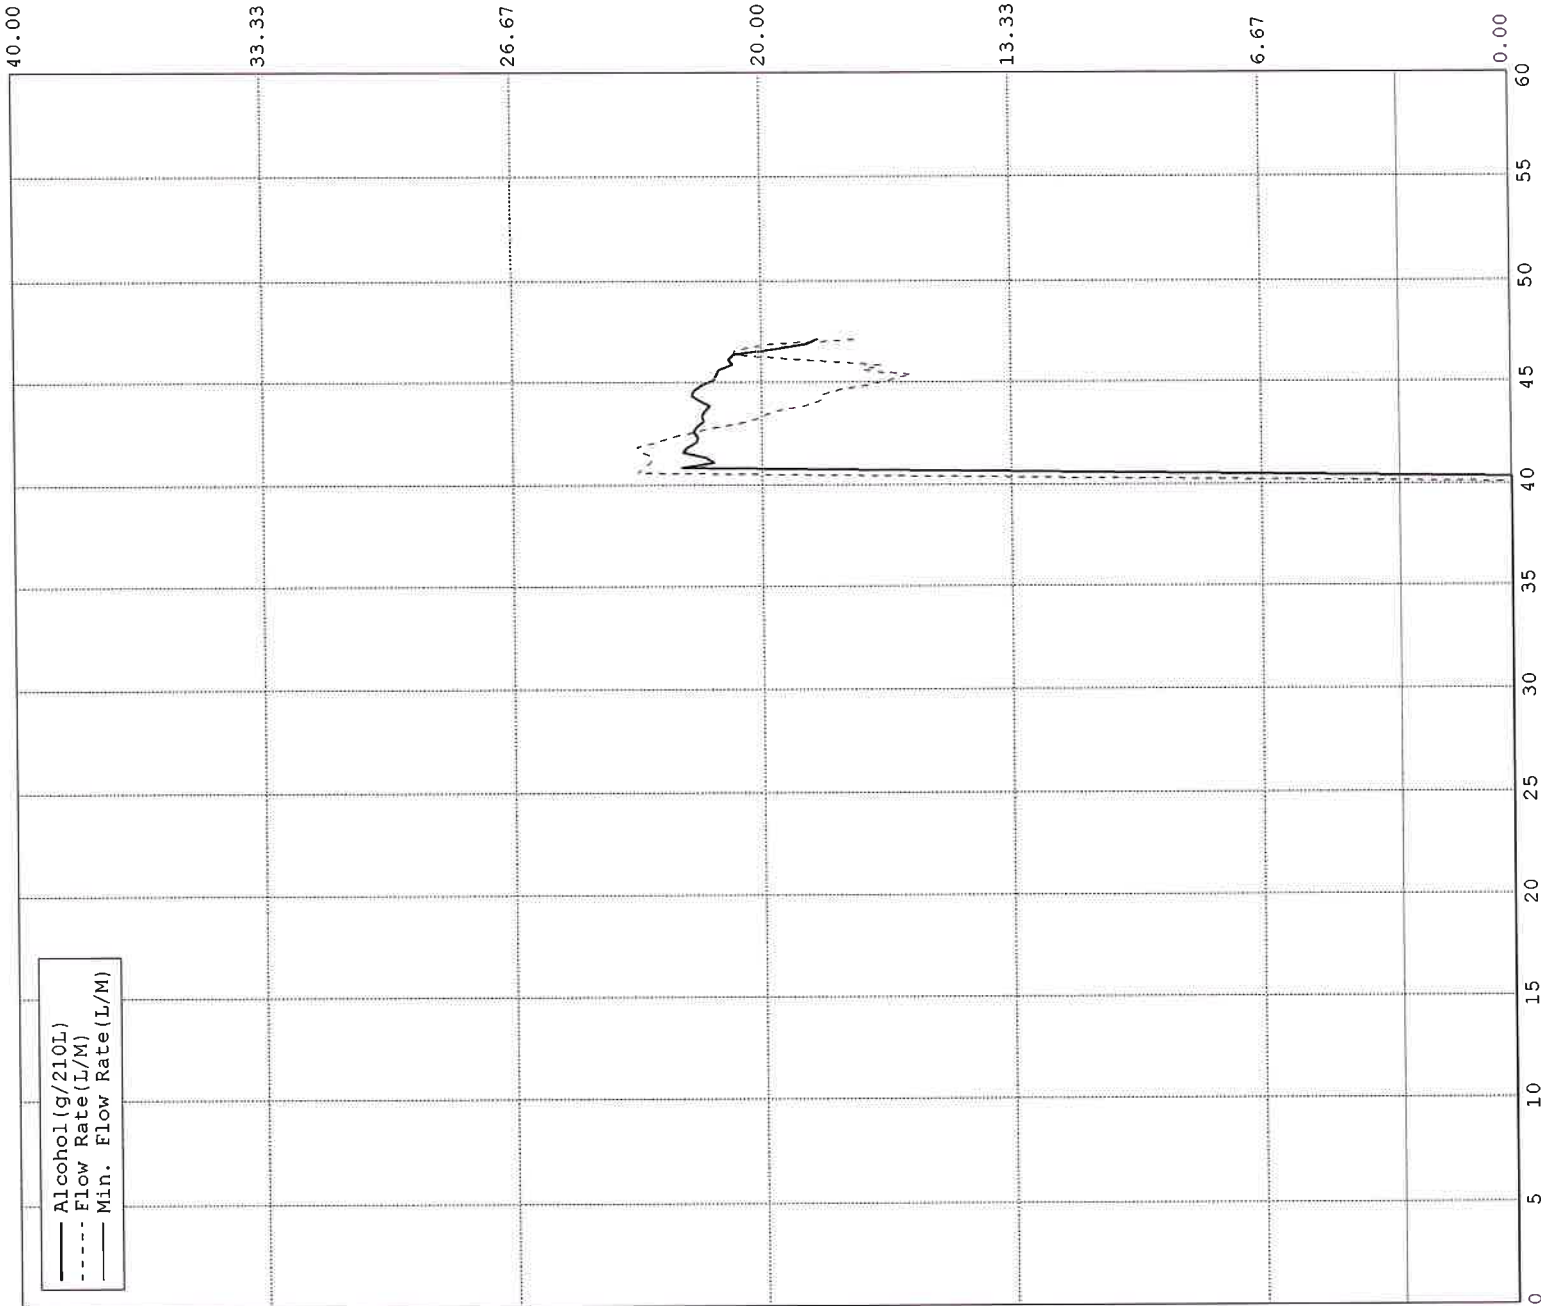

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 12/08/2025
Time: 14:16:00

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

RFI

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.27: 0.078

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK

BLANK TEST


INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

PASSED 14:17
0.000 14:17
VERIFIED 14:17
0.077 14:17
0.000 14:18

RFI DETECTED

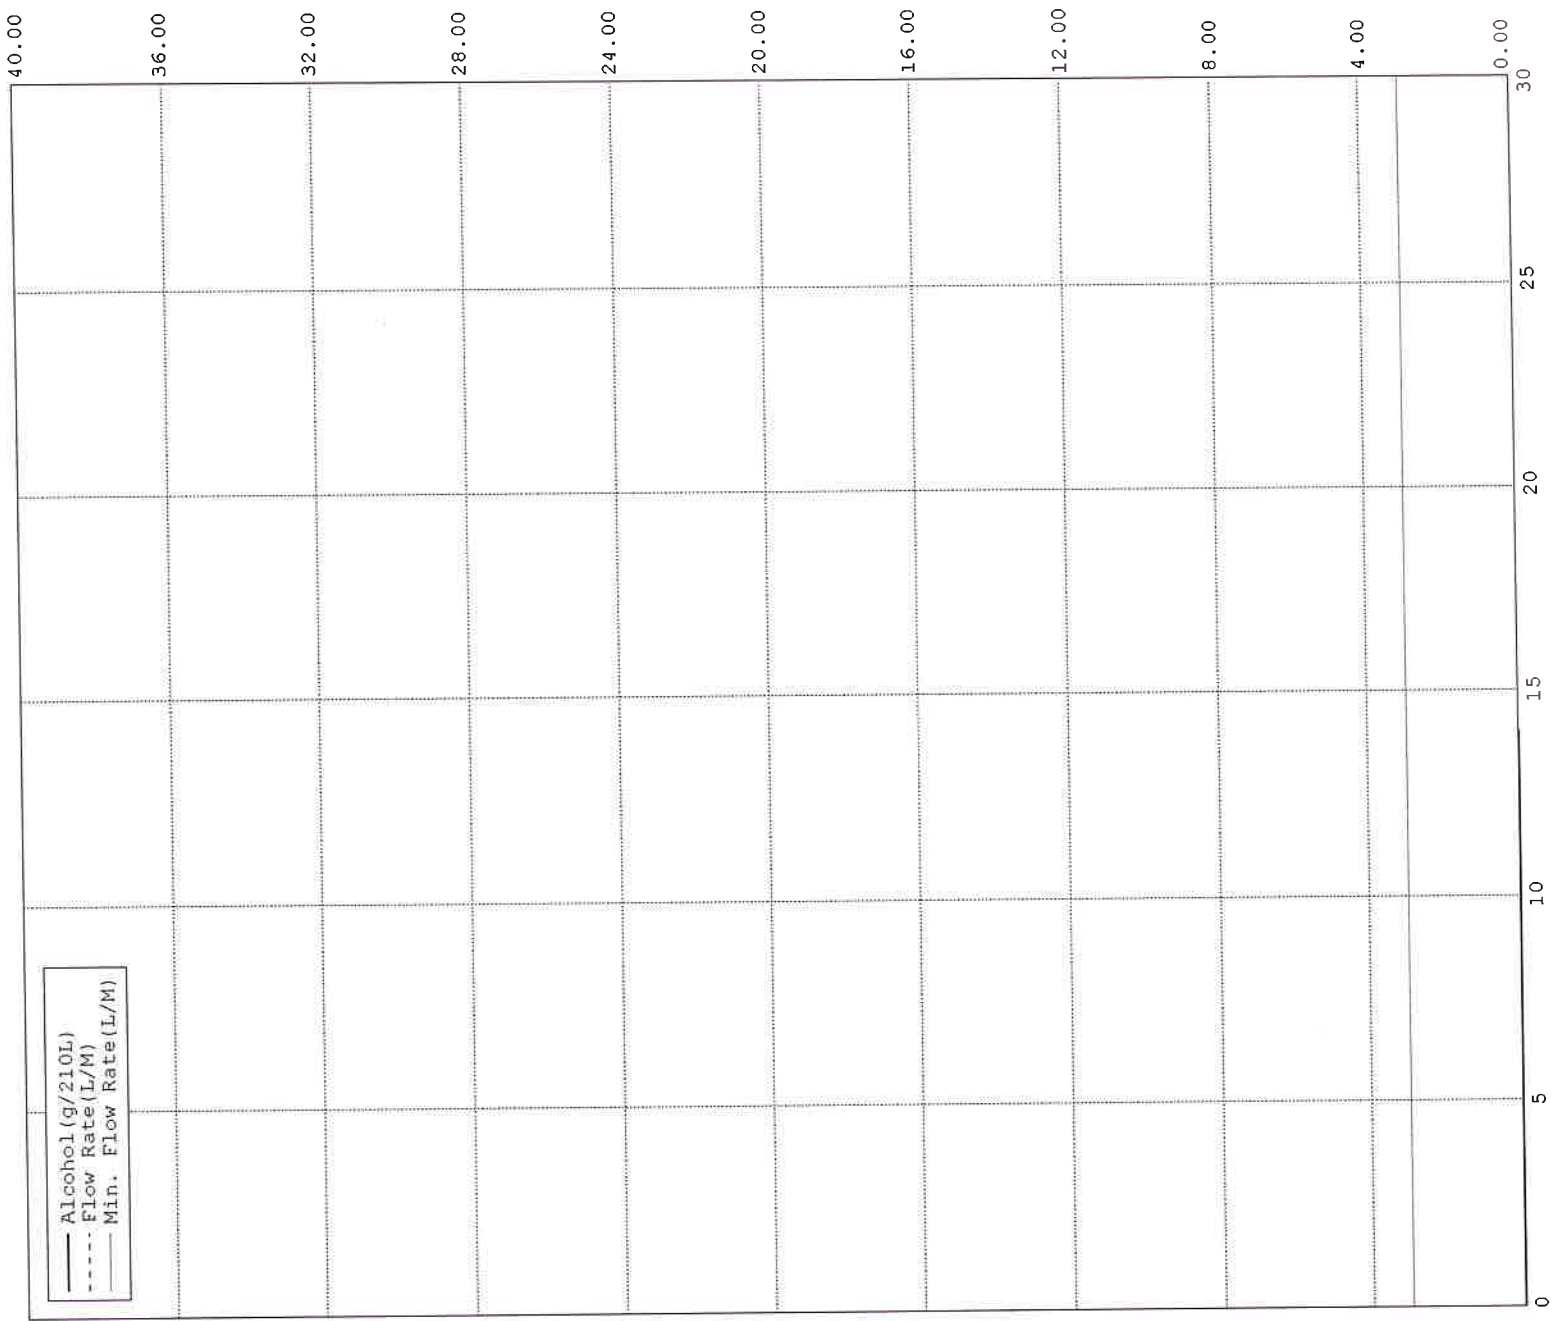

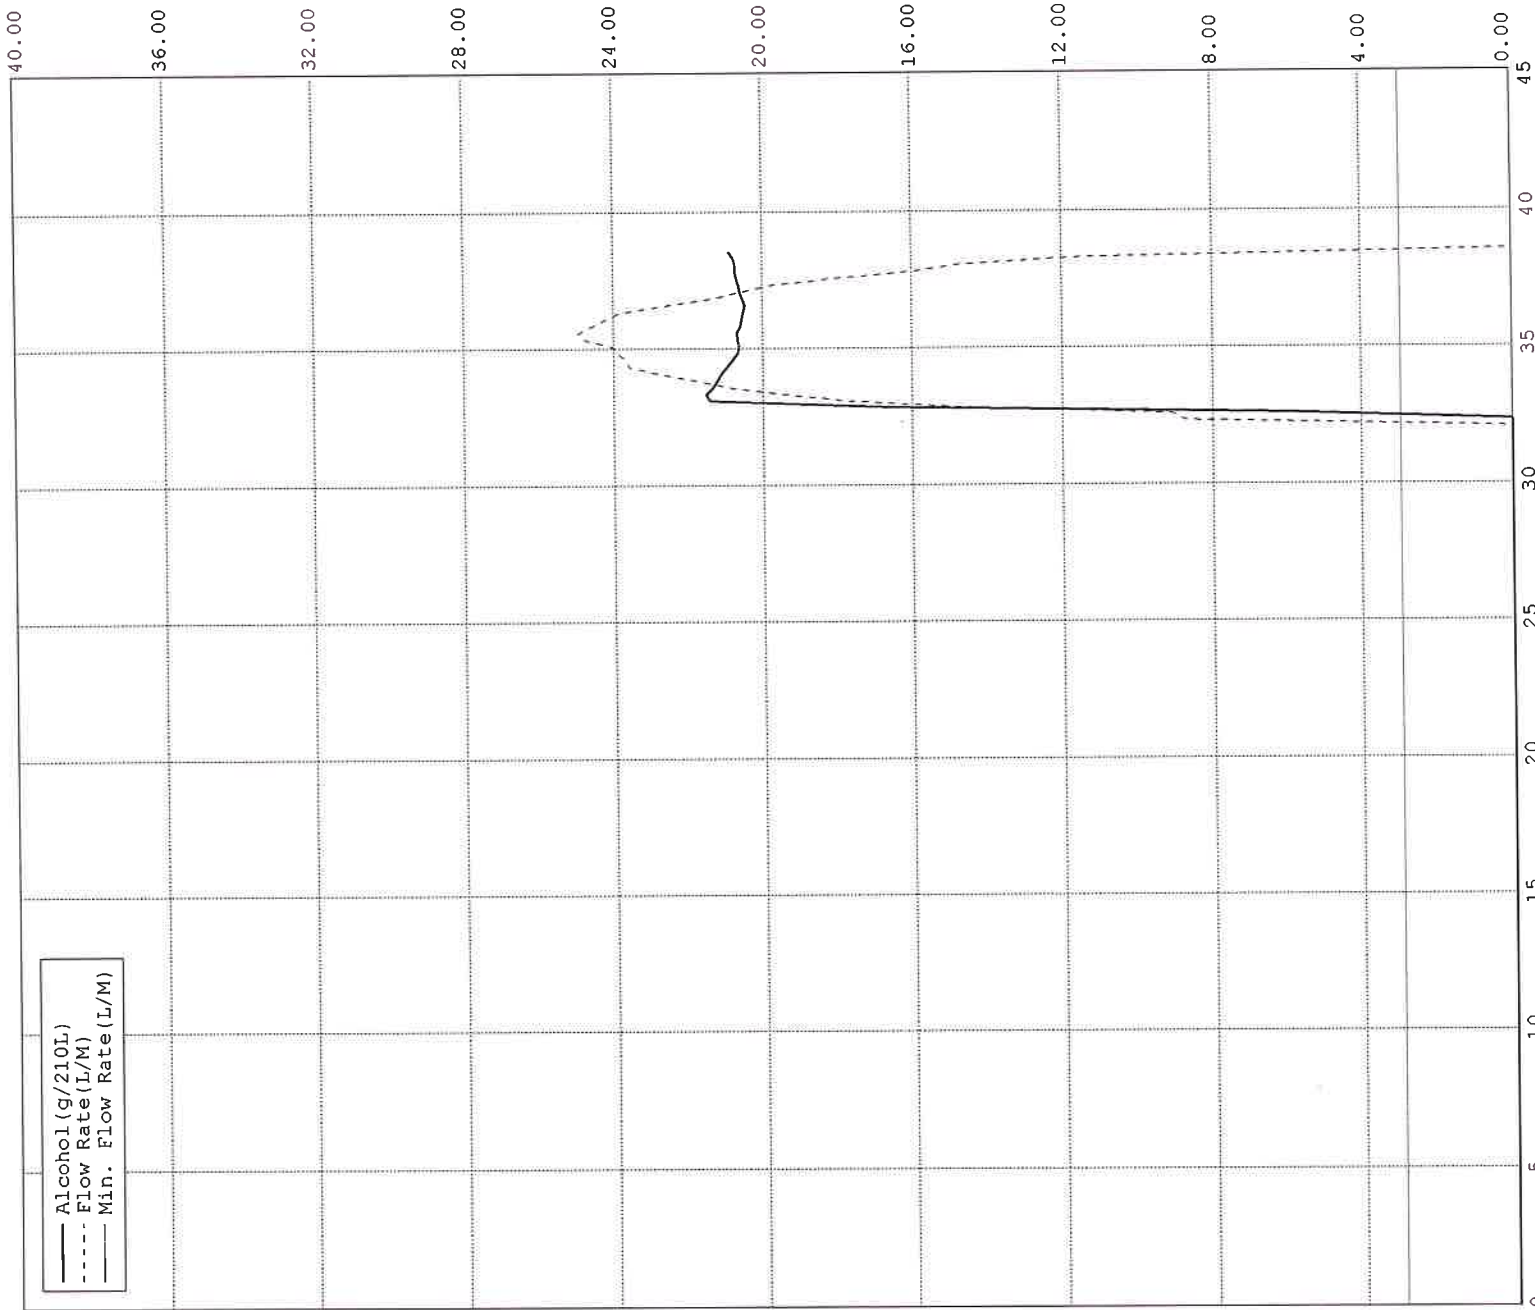

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 12/08/2025

Time: 12:07:57

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INTERFERENCE - ACETONE

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.28: 0.078

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 12:09

BLANK TEST 0.000 12:09

INTERNAL STANDARD VERIFIED 12:09

Xg = 0.107 (0.74%)

EXTERNAL STANDARD 0.077 12:09

X[1] = 0.0771 (-0.0014) (0.0029)

BLANK TEST 0.000 12:10

SUBJECT SAMPLE XXX 12:11

X[1] = 0.1056 (-0.0186) (0.0017)

Interference Detected

Filter 2 Avg: -0.0017

Filter 3 Avg: 0.0026

UV-1212125

CVL

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 12/08/2025

Time: 12:14:37

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INTERFERENCE - IPA

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.27: 0.078

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 12:15

BLANK TEST 0.000 12:15

INTERNAL STANDARD VERIFIED 12:15

$X_q = 0.108$ (1.07%)

EXTERNAL STANDARD 0.077 12:16

$X[1] = 0.0772$ (-0.0016) (0.0021)


BLANK TEST 0.000 12:17


SUBJECT SAMPLE XXX 12:17

$X[1] = 0.1166$ (-0.0259) (0.0013)

Interference Detected

OK

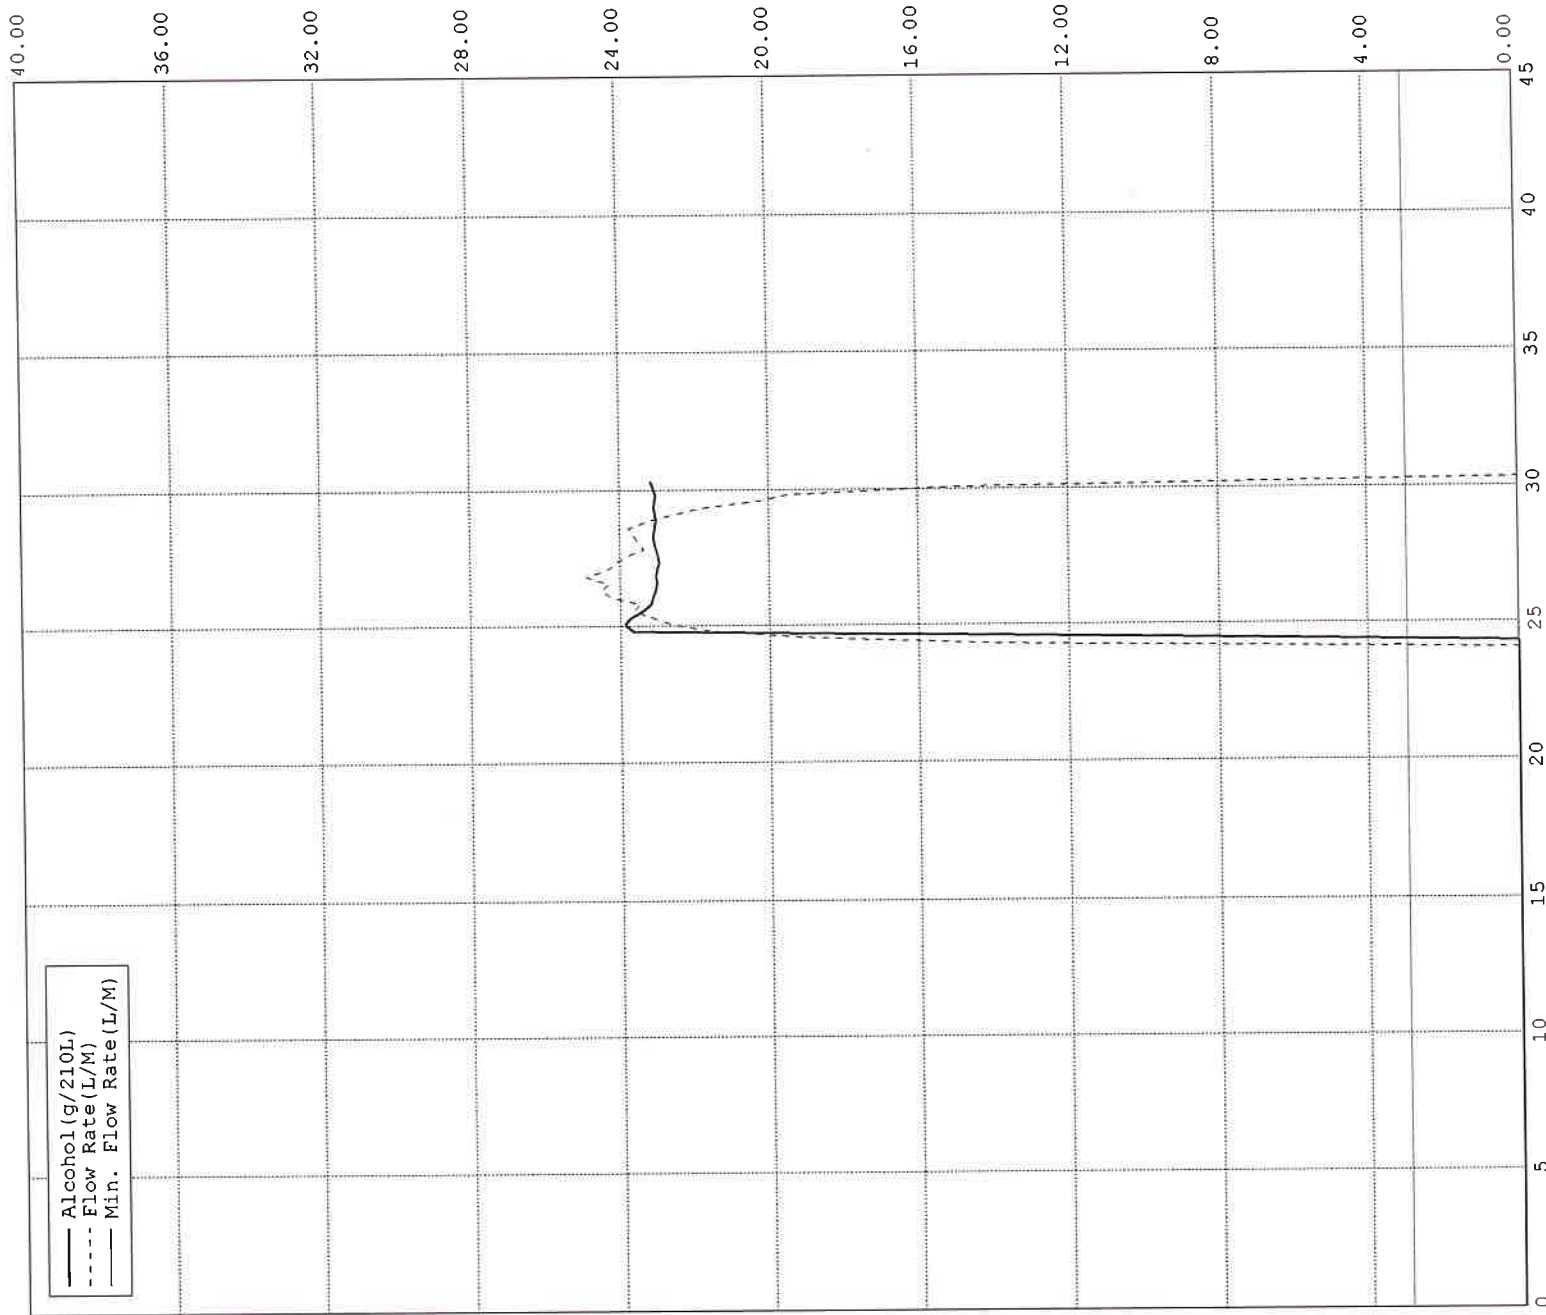

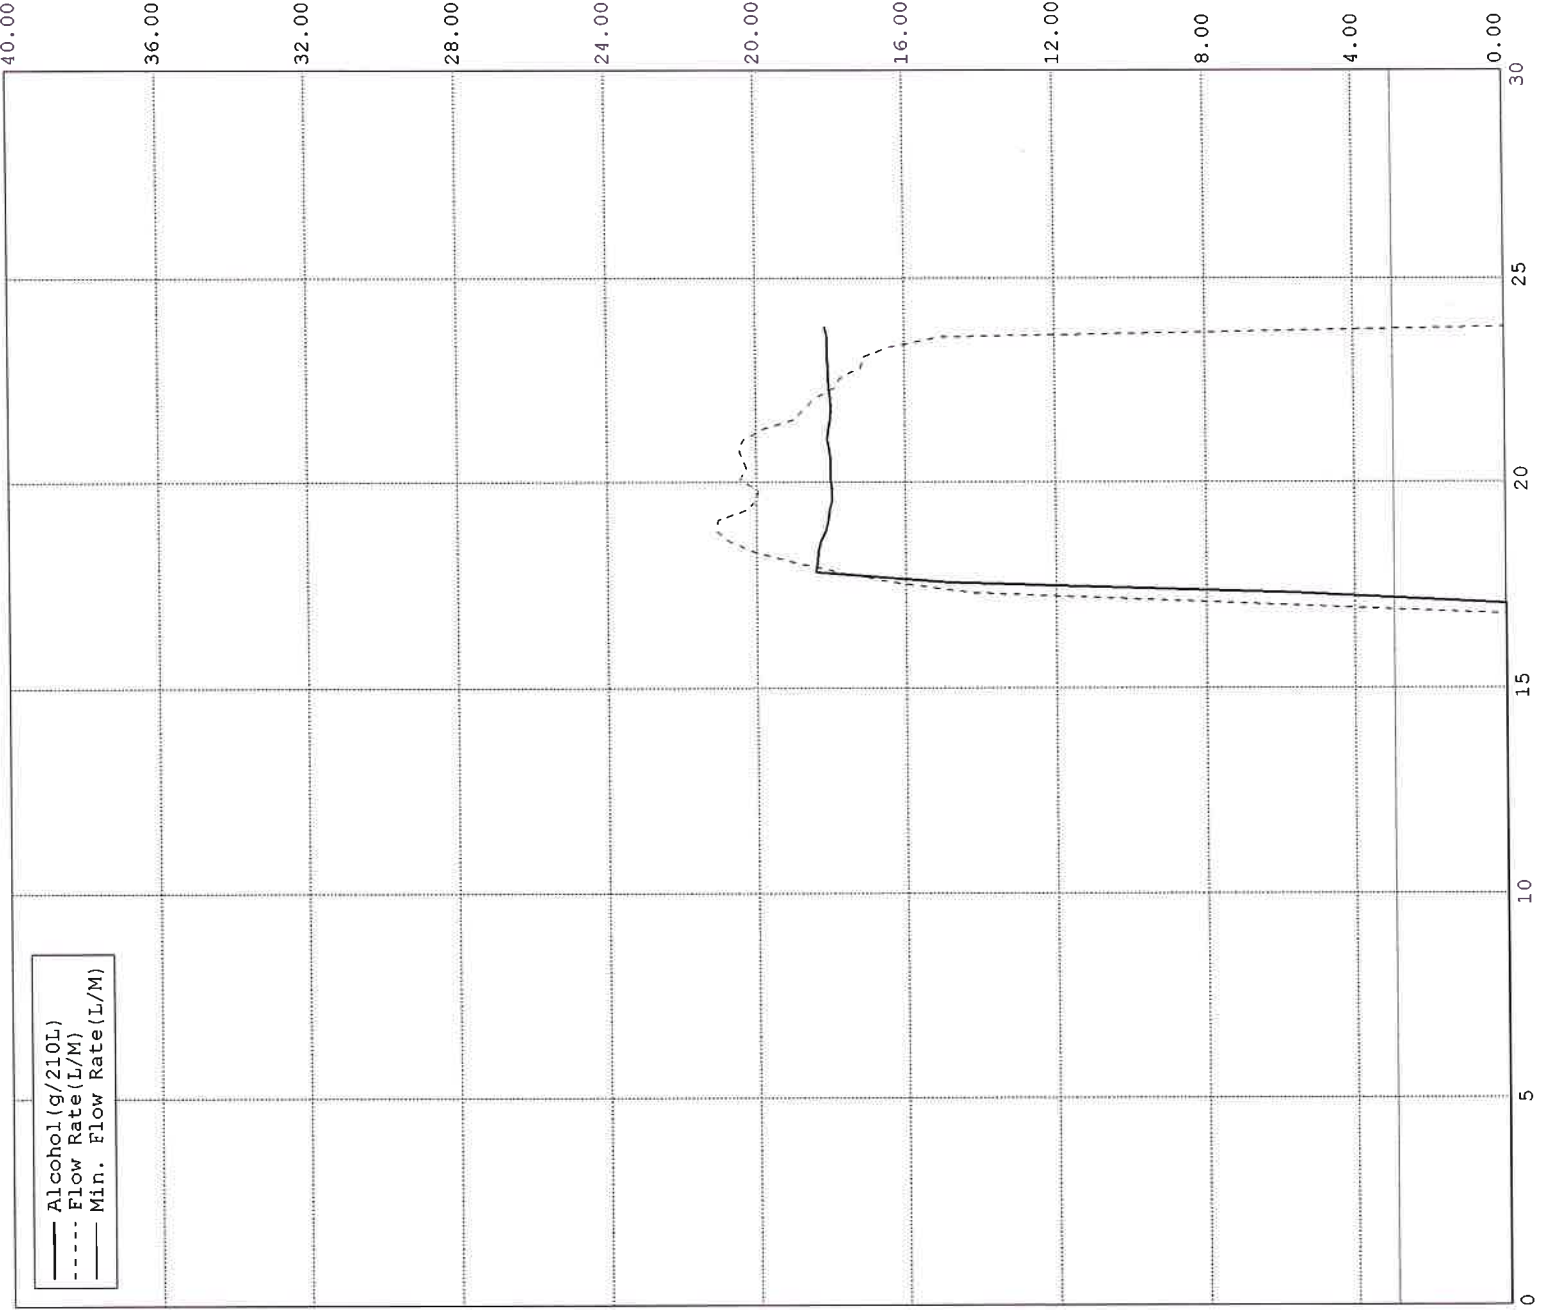

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100681

Date: 12/08/2025
Time: 12:21:16

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	12:22
BLANK TEST	0.000	12:22
INTERNAL STANDARD	VERIFIED	12:22
$X_g = 0.107$ (0.58%)		
EXTERNAL STANDARD	0.077	12:22
$X[1] = 0.0771$ (-0.0022)	(0.0024)	
BLANK TEST	0.000	12:23
SUBJECT SAMPLE (Vol=2.07L)	0.091	12:24
$X[1] = 0.0918$ (-0.0005)	(0.0001)	
BLANK TEST	0.000	12:25
EXTERNAL STANDARD	0.077	12:25
$X[1] = 0.0768$ (-0.0015)	(0.0028)	
BLANK TEST	0.000	12:26

Handwritten signature

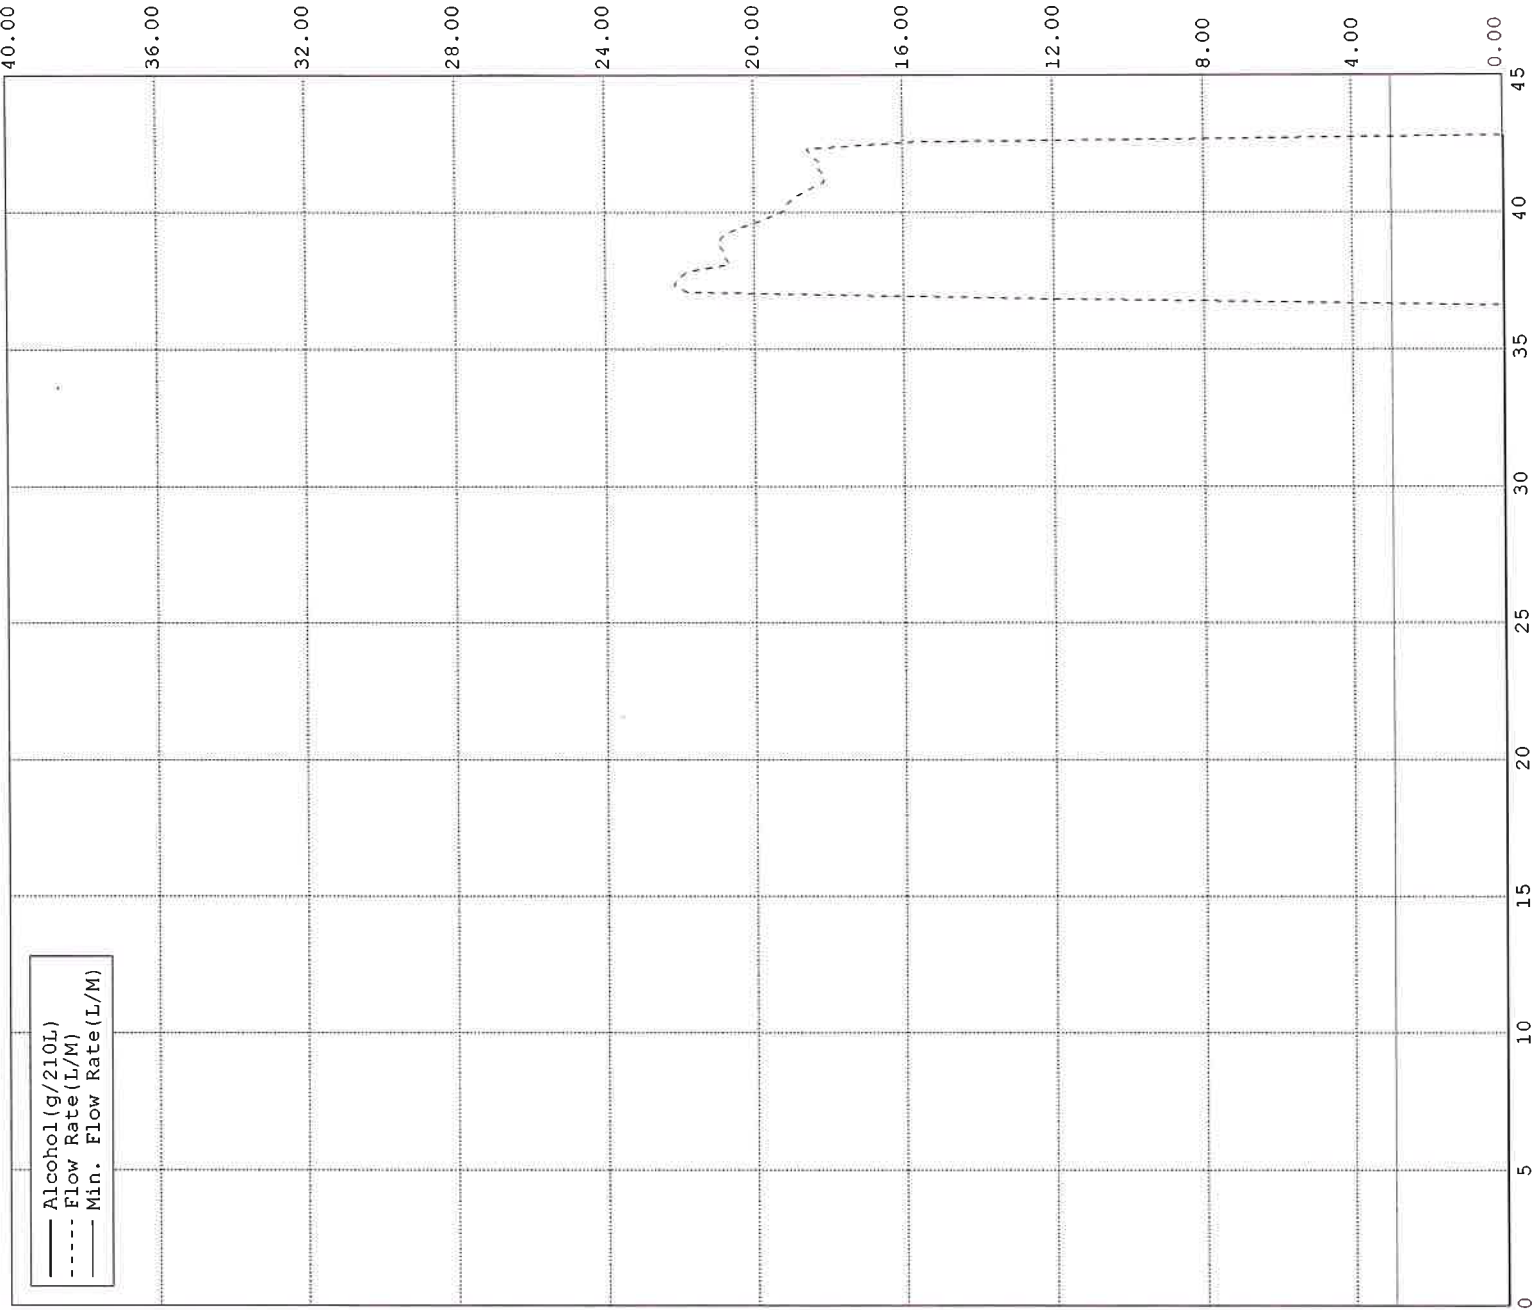

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100681

Date: 12/08/2025
Time: 14:45:20

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	14:46
BLANK TEST	0.000	14:46
INTERNAL STANDARD	VERIFIED	14:46
EXTERNAL STANDARD	0.077	14:46
BLANK TEST	0.000	14:47
SUBJECT SAMPLE (Vol=1.94L)	0.000	14:48
BLANK TEST	0.000	14:49
EXTERNAL STANDARD	0.077	14:49
BLANK TEST	0.000	14:50

CVG