




State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100681

Report Issue Date: 03/20/2026
Date Received: 2026-01-14
Condition of Item: Damaged

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data				
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)	Mean (g/210L)
0.020				
0.080				
0.300				

As Found - Evaluation Analyst: Colleen O'Bryant
 As Found Conditions - Barometric Pressure (inHg): 29.86 Barometer Used: VWR S/N 240680771 Temperature (C): 17.8 Relative Humidity (%): 14
 As-Found Lab Activity Date Range: 01/14/2026 - 01/14/2026

Screen wouldn't turn on. Frayed solenoid wires are causing the instrument to restart the instrument each time the lid is open. Solenoid needs to be replaced due to damaged wire. No linearity performed due to restarting issue.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.021	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG407908	0.039	0.039	0.039	0.040	0.039	0.039	+/- 0.003
0.080	0.079	AG436502	0.078	0.078	0.078	0.078	0.078	0.078	+/- 0.004
0.100	0.099	AG516101	0.097	0.097	0.097	0.097	0.097	0.097	+/- 0.004
0.150	0.149	AG515604	0.146	0.146	0.146	0.146	0.146	0.146	+/- 0.006
0.300	0.297	AG516110	0.292	0.291	0.291	0.291	0.291	0.291	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.64 Barometer Used: VWR S/N 240680771 Temperature (C): 22.0 Relative Humidity (%): 1
 As-Left Lab Activity Date Range: 03/09/2026 - 03/09/2026

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Carlie Glaister on 03/09/2026

carlie.glaister@alaska.gov

Technically and administratively reviewed by Kaija Swisher on 03/20/2026

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100681

Analyst or Technician Name: Carlie Glauster

DataMaster DMT Calibration Start Date: 3/9/26

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 9/10/2026
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.64 Temperature(C) 22.0 Relative Humidity(%) 1
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20260218COB Expiration Date: 5/18/26/3/19/27
Simulator S/N: SD1088 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20260218COB Expiration Date: 5/18/26/3/19/27
Simulator S/N: SD1199 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 250941280 Expiration Date: 3/19/27 (5/18/26 prep)
Simulator S/N: SD1177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 250159297
Calibration Due Date: 3/14/27

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 3/9/26
Data Interpretation Date (Technician): NA (if applicable)
Data Interpretation Date (Analyst): ckg 3/9/2026 ckg

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100681

Date: 03/09/2026
Time: 11:10:25

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 44.0°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.70 V PASSED
(1.02 V - 2.38 V)
Cooler Voltage = 1.60 V PASSED
(0.92 V - 2.14 V)
Bias Voltage = 77 V PASSED
(47 V - 109 V)
Chopper Freq = 512 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.6 in

PUMP INFO

Flow Rate = 4.372 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.009 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.108 1.07% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100681

Date: 03/09/2026
Time: 11:17 AM

Temperatures (°C)

Sample Cell: 48.9°C
Breath Tube: 44.6°C

Current Barometer 29.6 in
Volume (Ltr) 1.54

Settings

Lamp: 1.72 V
Bias: 77 V
Cooler: 1.65 V
Chopper: 513 Hz

Voltages (V)

Flow: 1.07 V
Detector: -0.002 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100681

Date: 10/29/2021
Time: 13:14:55

OPERATOR NAME:
CARLIE GLAISTER
CERTIFICATE #: 10436

Ca = 0.1000
CAL = 0.984251 0.800 <= CAL < 1.200
b1 = 0.0004 0.0000 <= b1 < 0.0040
b2 = 0.0051 0.0010 <= b2 < 0.0100
b3 = 0.0001 0.0000 <= b3 < 0.0040
Xq = 0.1066 0.0500 <= Xq < 0.2000
a21 = 1.158479 1.050 <= a21 < 1.300
a31 = 0.492122 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 03/09/2026

Time: 11:21:33

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080

TARGET AT 29.64: 0.079

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	11:22
BLANK TEST	0.000	11:22
INTERNAL STANDARD	VERIFIED	11:22
EXTERNAL STANDARD	0.078	11:23
BLANK TEST	0.000	11:23
SUBJECT SAMPLE (Vol=1.59L)	0.000	11:24
BLANK TEST	0.000	11:25
EXTERNAL STANDARD	0.078	11:25
BLANK TEST	0.000	11:26

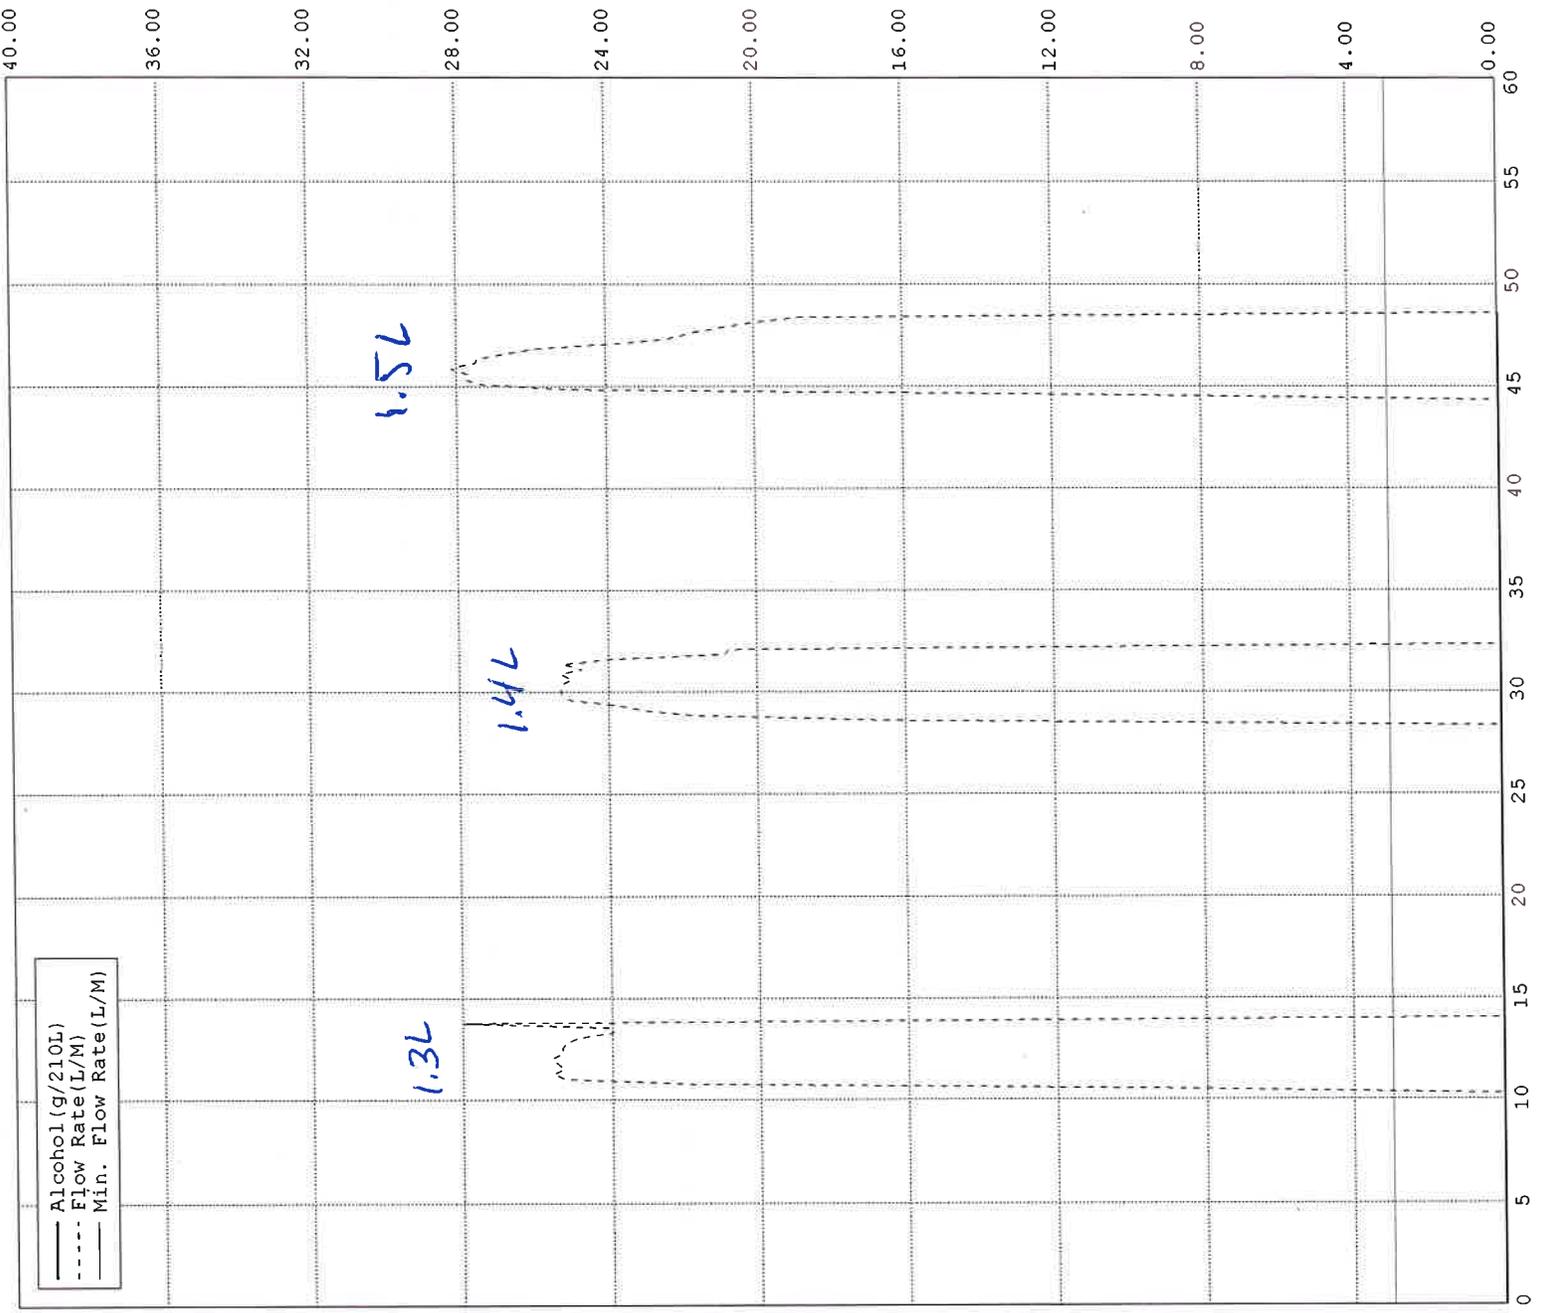

LINEARITY CHECK

 Alaska Department of Public Safety
 DATAMASTER dmt: 100681


Date: 03/09/2026
 Time: 11:32:01

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0004
0.040	0.0392	0.0004
0.079	0.0780	0.0000
0.099	0.0970	0.0000
0.149	0.1460	0.0000
0.297	0.2912	0.0004

SLOPE = 0.978980
 R² = 0.999992

OK

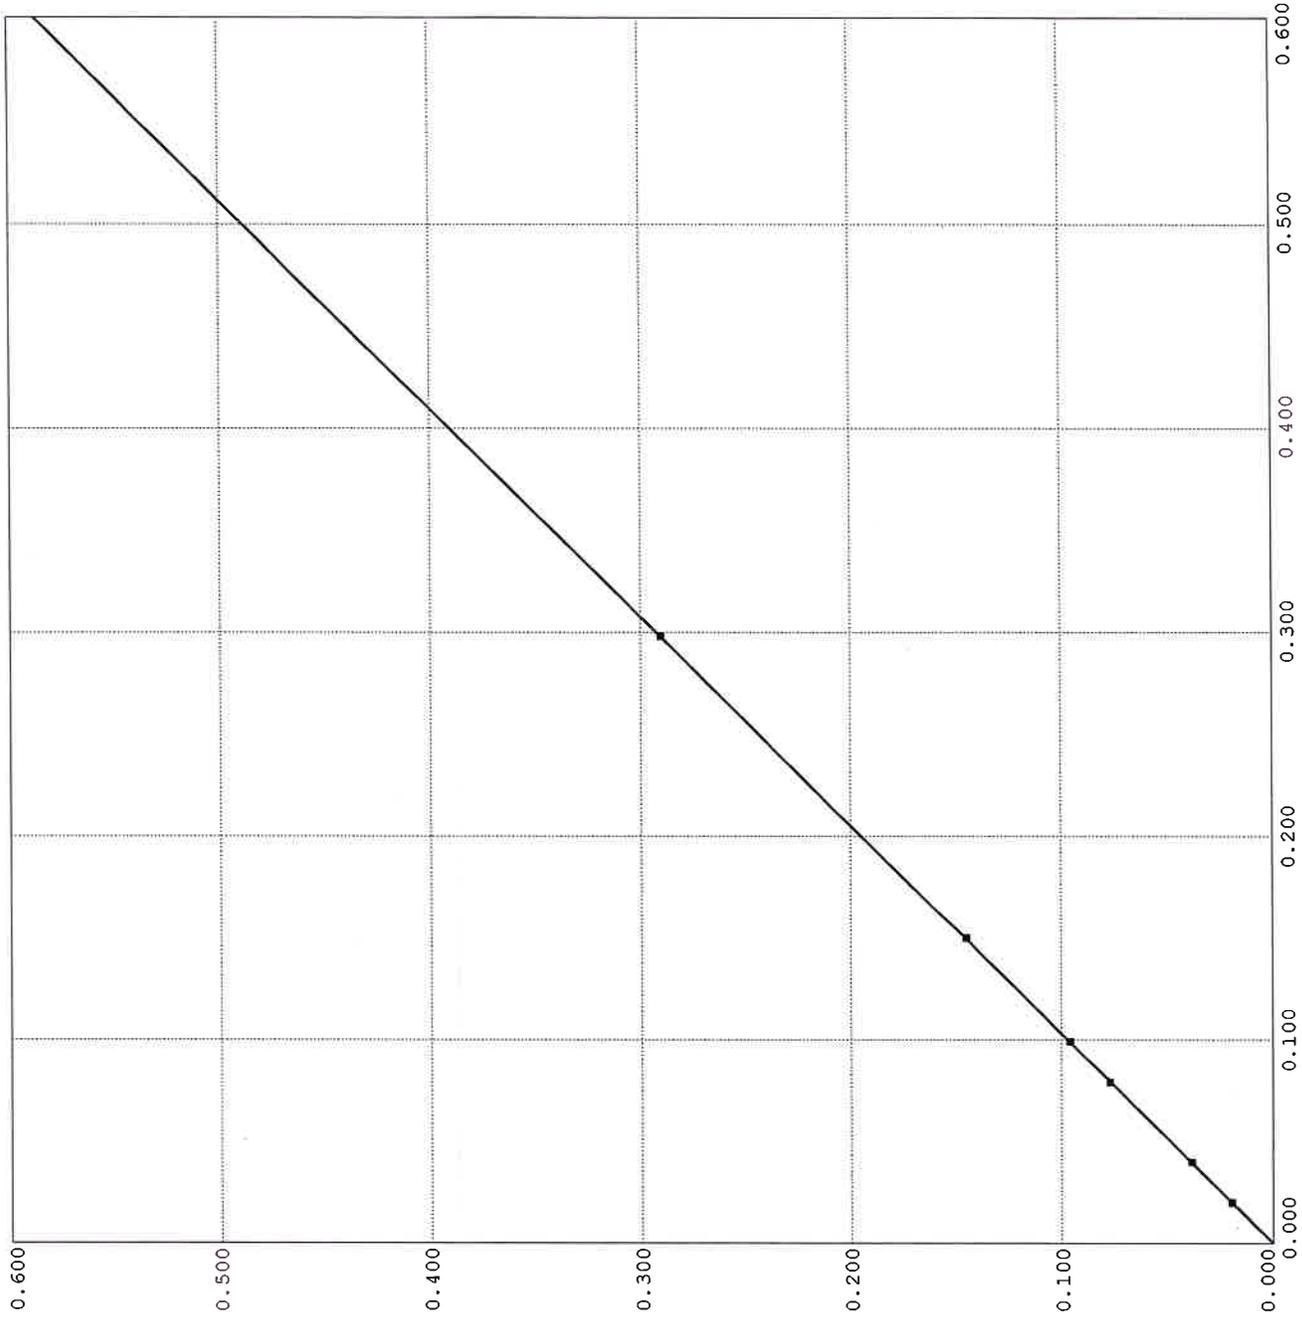

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100681






Date: 03/09/2026
Time: 11:32:03

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.63: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 578 psi

BLANK TEST	0.000	11:33
INTERNAL STANDARD	VERIFIED	11:33
EXTERNAL STANDARD	0.021	11:34
BLANK TEST	0.000	11:35
EXTERNAL STANDARD	0.020	11:35
BLANK TEST	0.000	11:36
EXTERNAL STANDARD	0.020	11:36
BLANK TEST	0.000	11:37
EXTERNAL STANDARD	0.020	11:37
BLANK TEST	0.000	11:38
EXTERNAL STANDARD	0.020	11:38
BLANK TEST	0.000	11:39

Average = 0.0202
Std Dev = 0.0004

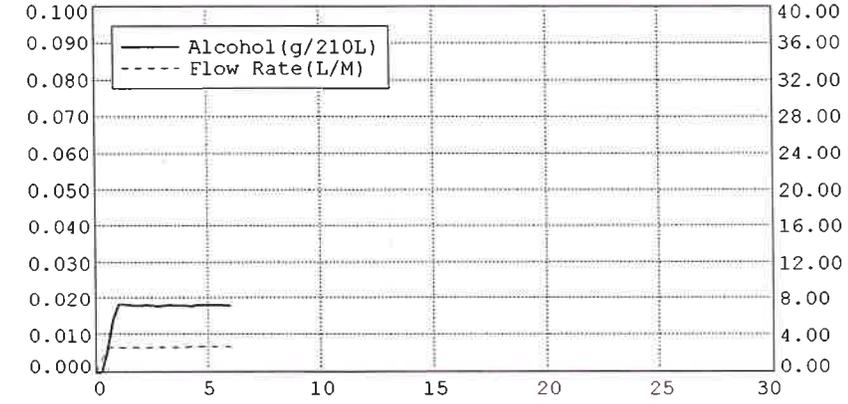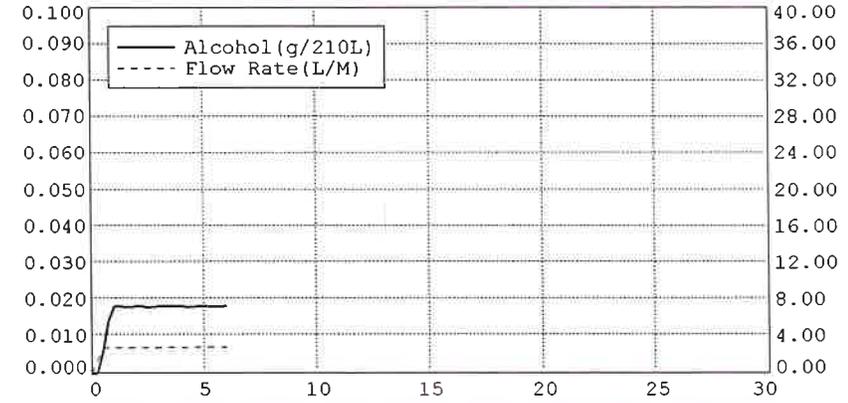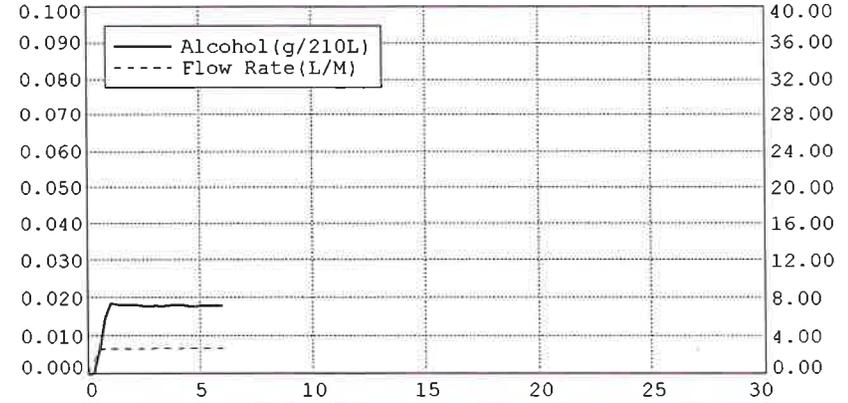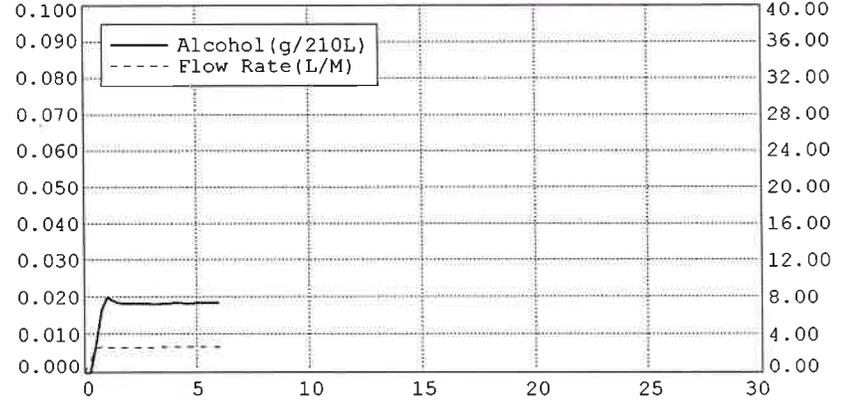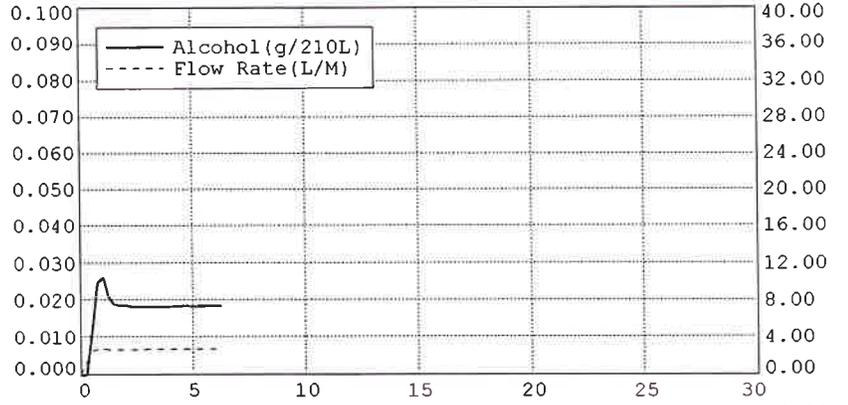

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100681






Date: 03/09/2026
Time: 11:39:54

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.63: 0.040
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 860 psi

BLANK TEST	0.000	11:41
INTERNAL STANDARD	VERIFIED	11:41
EXTERNAL STANDARD	0.039	11:41
BLANK TEST	0.000	11:42
EXTERNAL STANDARD	0.039	11:42
BLANK TEST	0.000	11:43
EXTERNAL STANDARD	0.039	11:43
BLANK TEST	0.000	11:44
EXTERNAL STANDARD	0.040	11:44
BLANK TEST	0.000	11:45
EXTERNAL STANDARD	0.039	11:45
BLANK TEST	0.000	11:46

Average = 0.0392
Std Dev = 0.0004

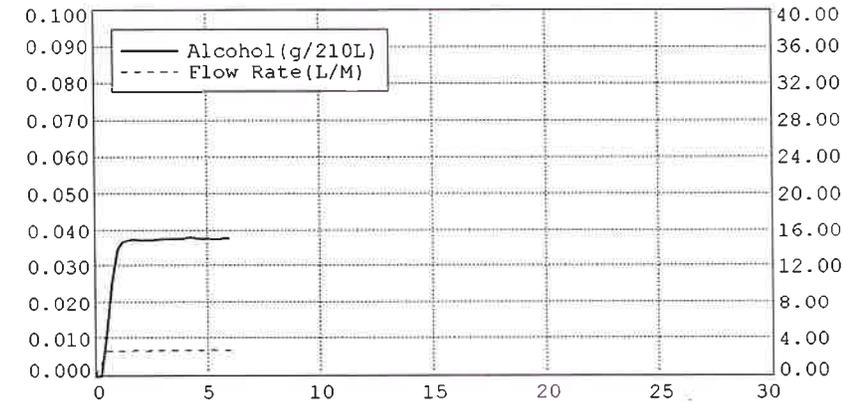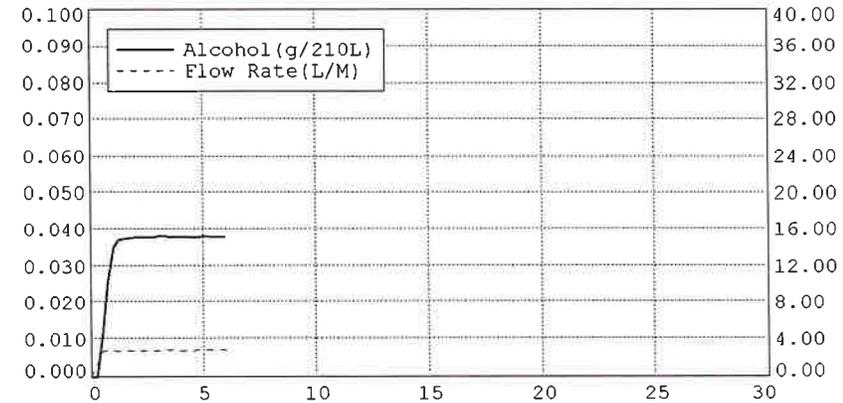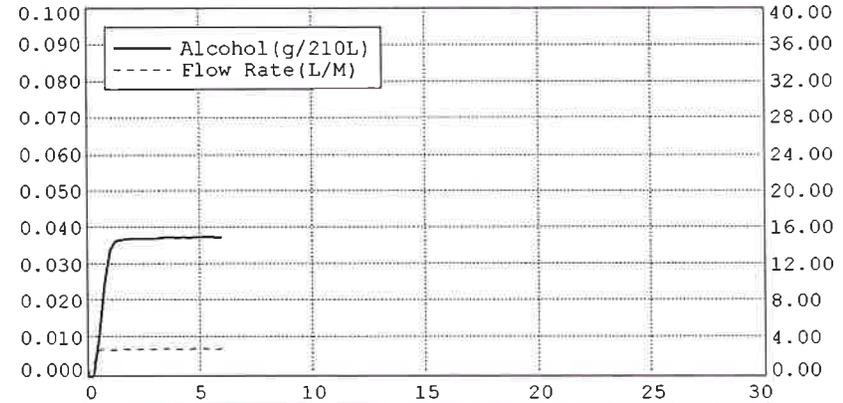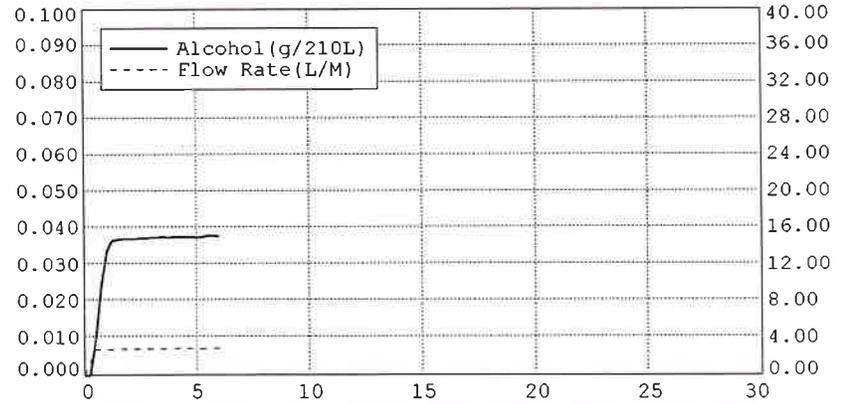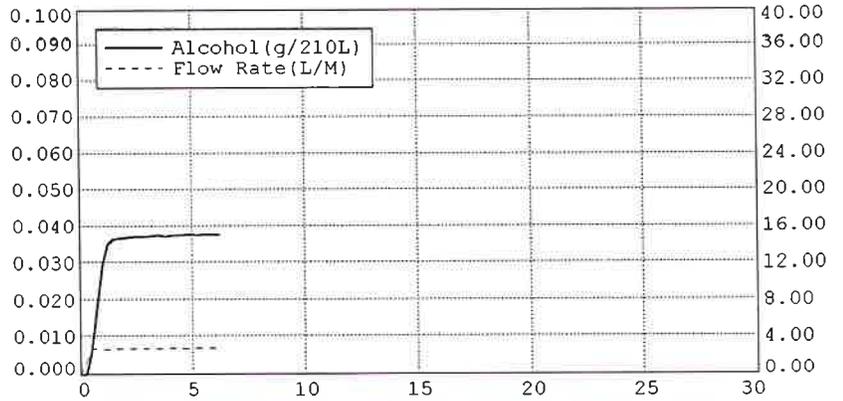

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100681






Date: 03/09/2026
 Time: 11:50:27

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.63: 0.079
 LOT #: AG436502
 EXPIRATION: 12/30/2026
 TANK PRESSURE: 976 psi

BLANK TEST	0.000	11:51
INTERNAL STANDARD	VERIFIED	11:51
EXTERNAL STANDARD	0.078	11:52
BLANK TEST	0.000	11:53
EXTERNAL STANDARD	0.078	11:53
BLANK TEST	0.000	11:54
EXTERNAL STANDARD	0.078	11:54
BLANK TEST	0.000	11:55
EXTERNAL STANDARD	0.078	11:55
BLANK TEST	0.000	11:56
EXTERNAL STANDARD	0.078	11:56
BLANK TEST	0.000	11:57

Average = 0.0780
 Std Dev = 0.0000

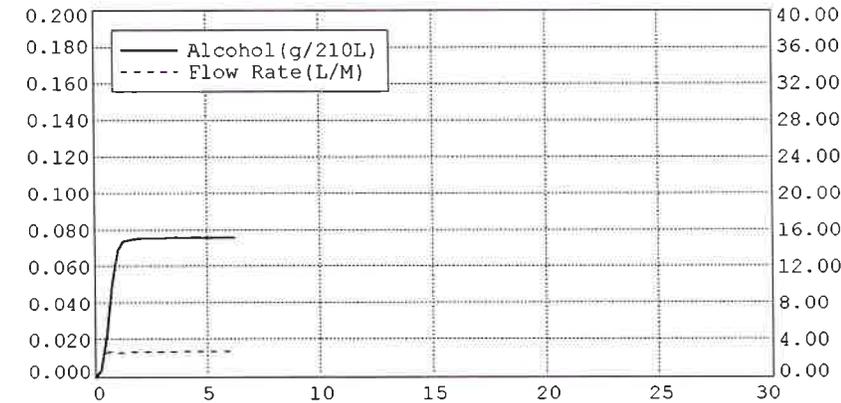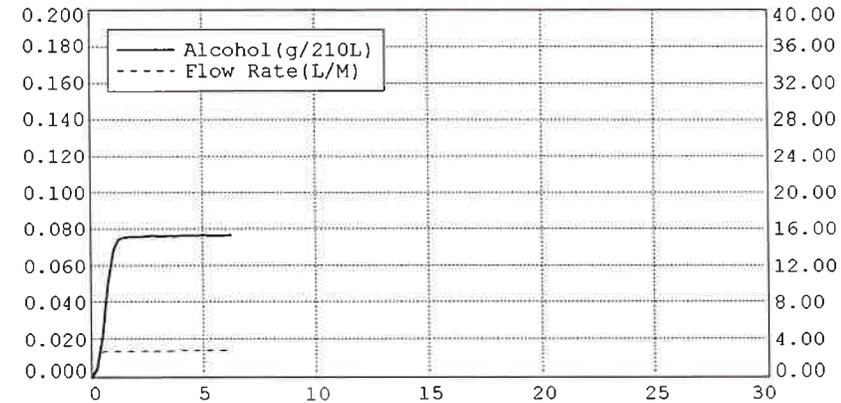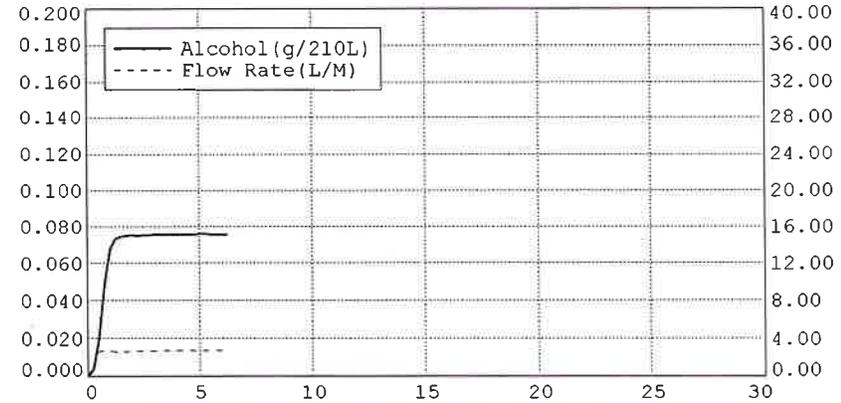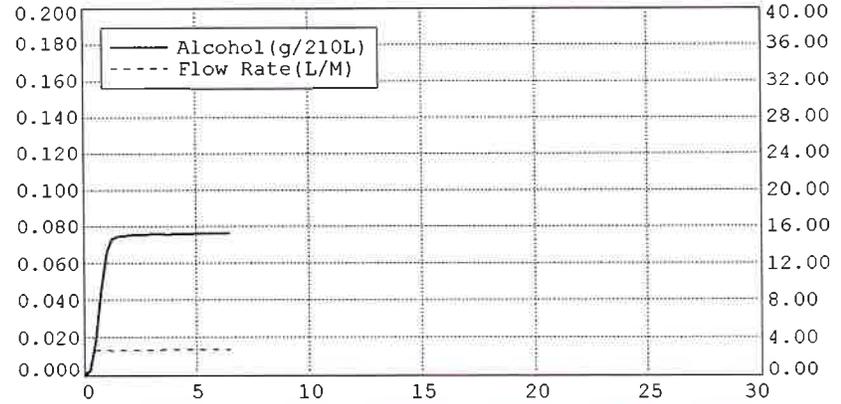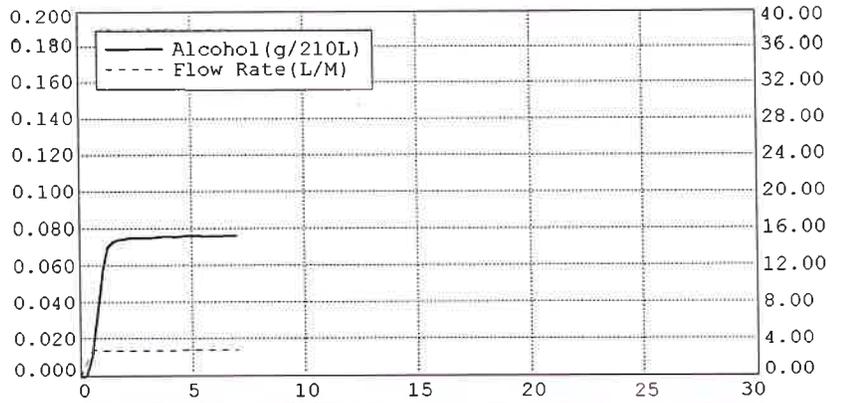

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100681






Date: 03/09/2026
 Time: 12:00:32

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.64: 0.099
 LOT #: AG516101
 EXPIRATION: 06/10/2027
 TANK PRESSURE: 958 psi

BLANK TEST	0.000	12:01
INTERNAL STANDARD	VERIFIED	12:01
EXTERNAL STANDARD	0.097	12:02
BLANK TEST	0.000	12:03
EXTERNAL STANDARD	0.097	12:03
BLANK TEST	0.000	12:04
EXTERNAL STANDARD	0.097	12:04
BLANK TEST	0.000	12:05
EXTERNAL STANDARD	0.097	12:05
BLANK TEST	0.000	12:06
EXTERNAL STANDARD	0.097	12:06
BLANK TEST	0.000	12:07

Average = 0.0970
 Std Dev = 0.0000

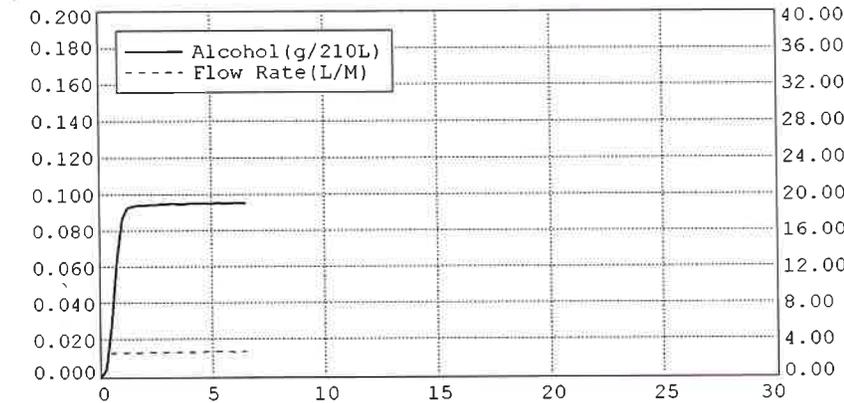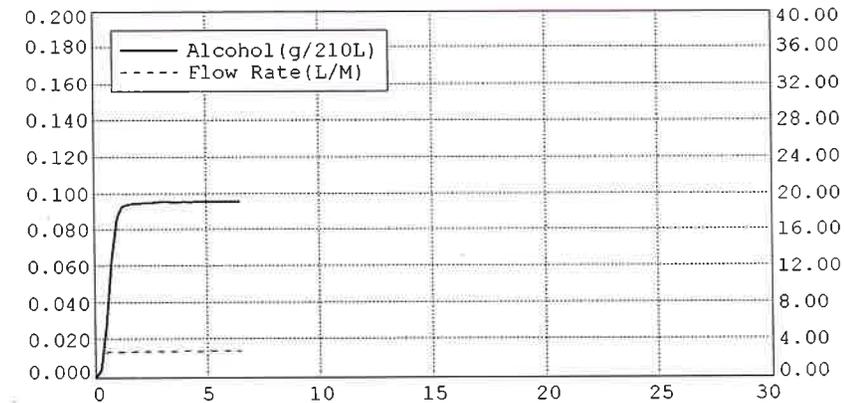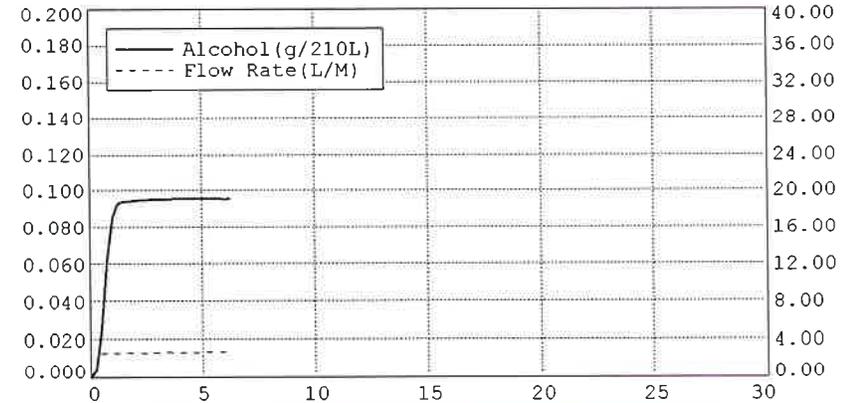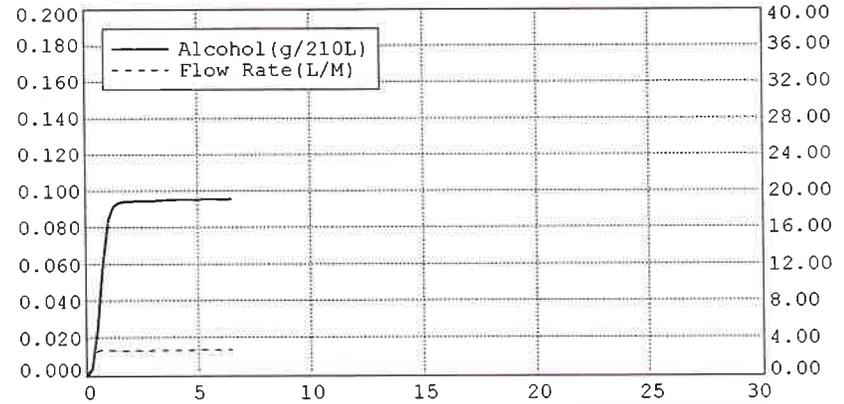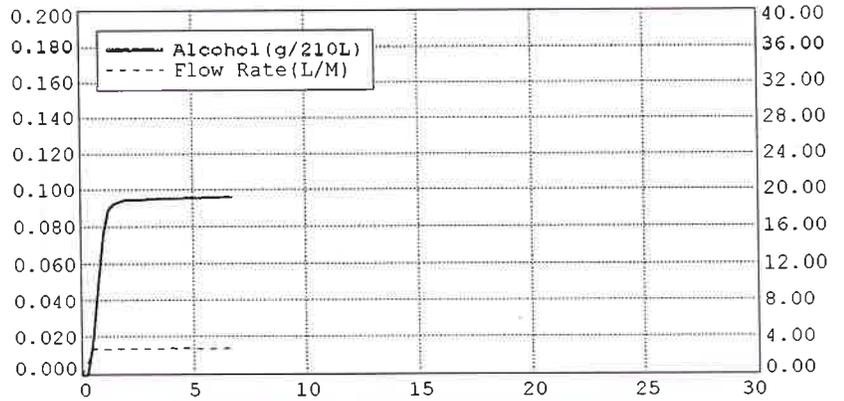

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100681






Date: 03/09/2026
 Time: 12:09:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.62: 0.149
 LOT #: AG515604
 EXPIRATION: 06/05/2027
 TANK PRESSURE: 680 psi

BLANK TEST	0.000	12:10
INTERNAL STANDARD	VERIFIED	12:10
EXTERNAL STANDARD	0.146	12:10
BLANK TEST	0.000	12:11
EXTERNAL STANDARD	0.146	12:12
BLANK TEST	0.000	12:13
EXTERNAL STANDARD	0.146	12:13
BLANK TEST	0.000	12:14
EXTERNAL STANDARD	0.146	12:14
BLANK TEST	0.000	12:15
EXTERNAL STANDARD	0.146	12:15
BLANK TEST	0.000	12:16

Average = 0.1460
 Std Dev = 0.0000

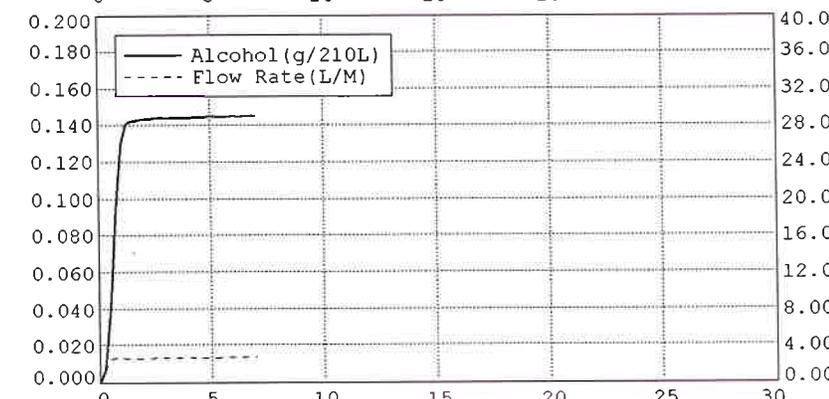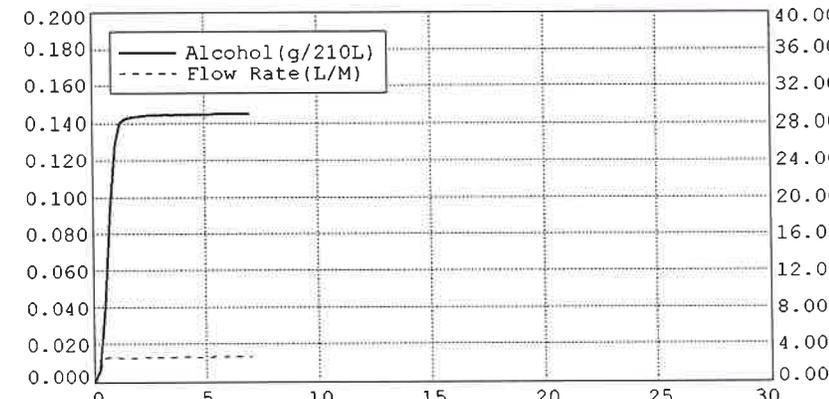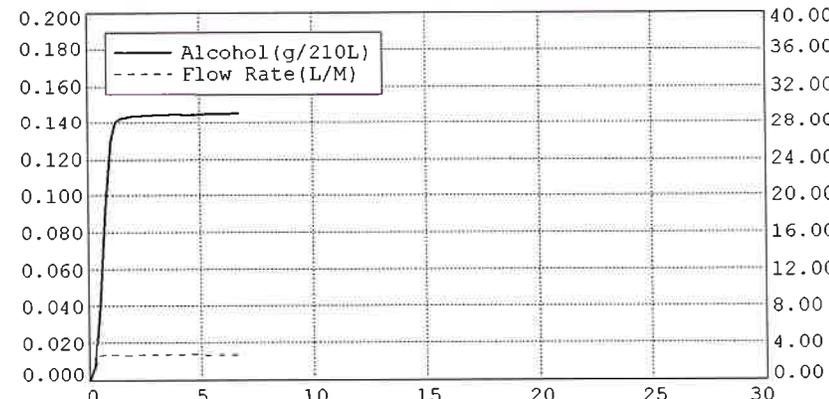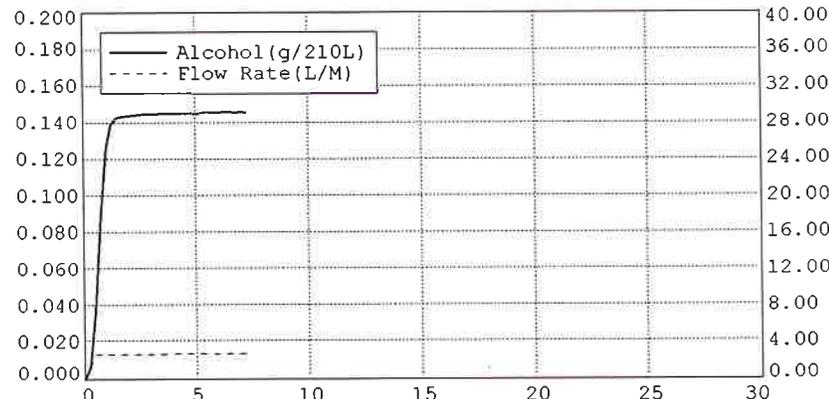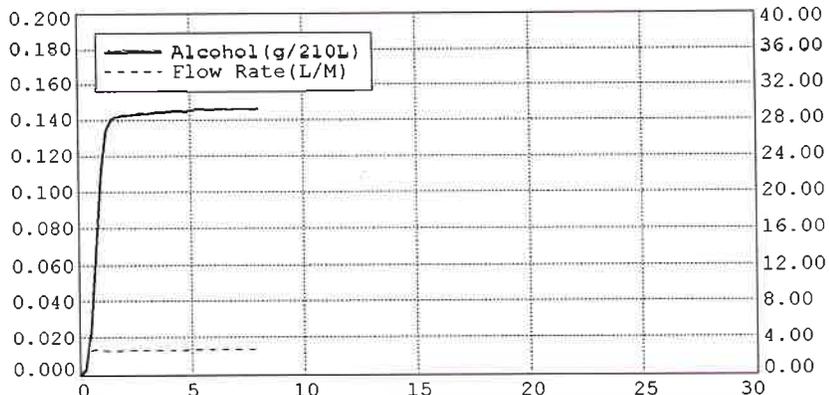

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100681






Date: 03/09/2026
 Time: 12:25:00

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.63: 0.297
 LOT #: AG516110
 EXPIRATION: 06/10/2027
 TANK PRESSURE: 467 psi

BLANK TEST	0.000	12:26
INTERNAL STANDARD	VERIFIED	12:26
EXTERNAL STANDARD	0.292	12:26
BLANK TEST	0.000	12:27
EXTERNAL STANDARD	0.291	12:27
BLANK TEST	0.000	12:28
EXTERNAL STANDARD	0.291	12:28
BLANK TEST	0.000	12:29
EXTERNAL STANDARD	0.291	12:29
BLANK TEST	0.000	12:30
EXTERNAL STANDARD	0.291	12:31
BLANK TEST	0.000	12:32

Average = 0.2912
 Std Dev = 0.0004

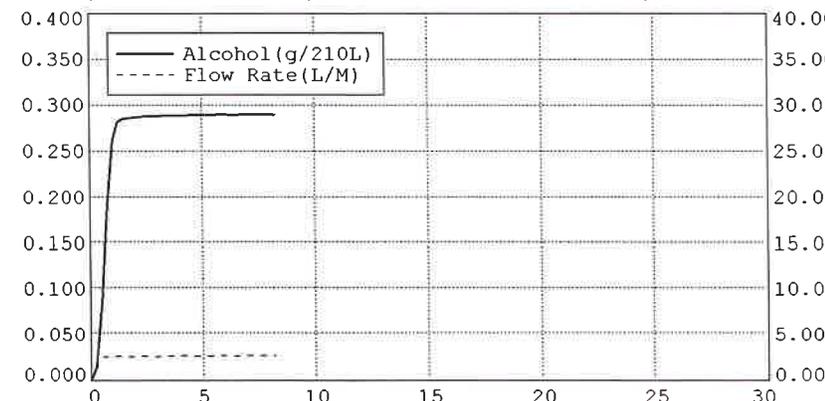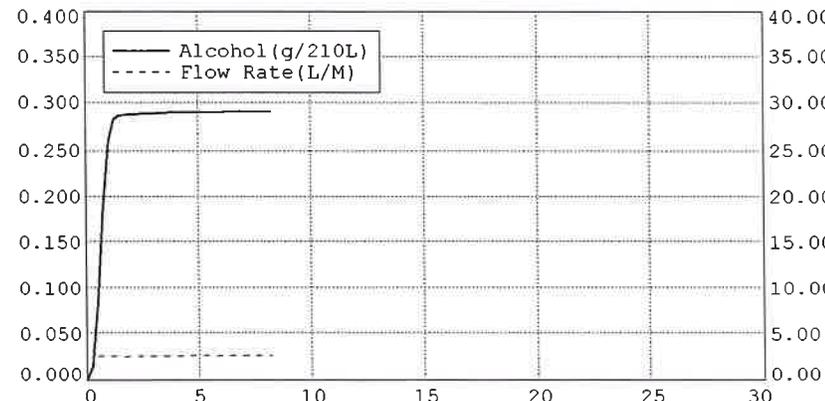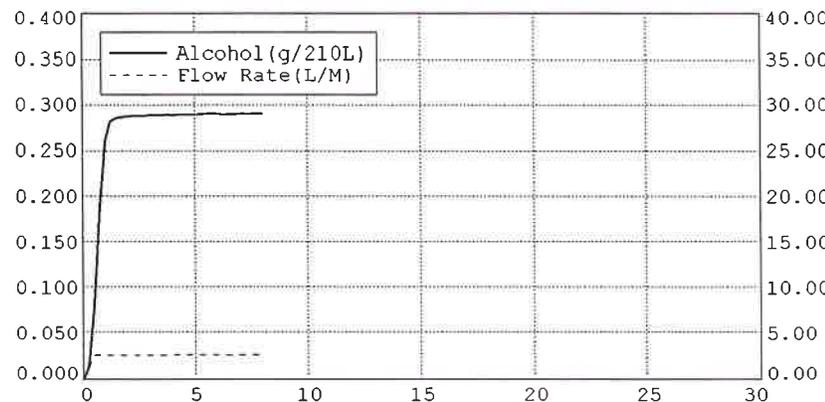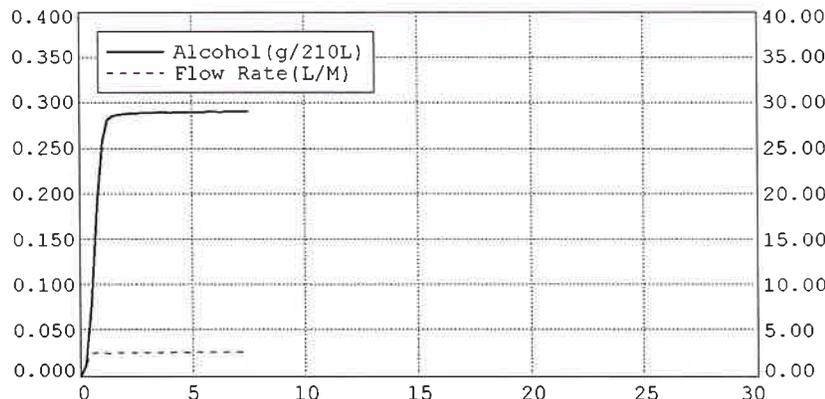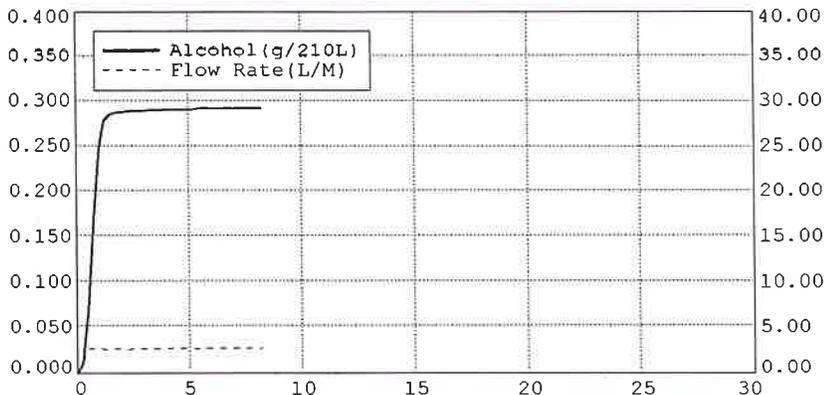

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 03/09/2026

Time: 12:36:36

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INCOMPLETE

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080

TARGET AT 29.63: 0.079

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	12:38
BLANK TEST	0.000	12:38
INTERNAL STANDARD	VERIFIED	12:38
EXTERNAL STANDARD	0.079	12:39
BLANK TEST	0.000	12:40
SUBJECT SAMPLE	INCOMPLETE	12:42

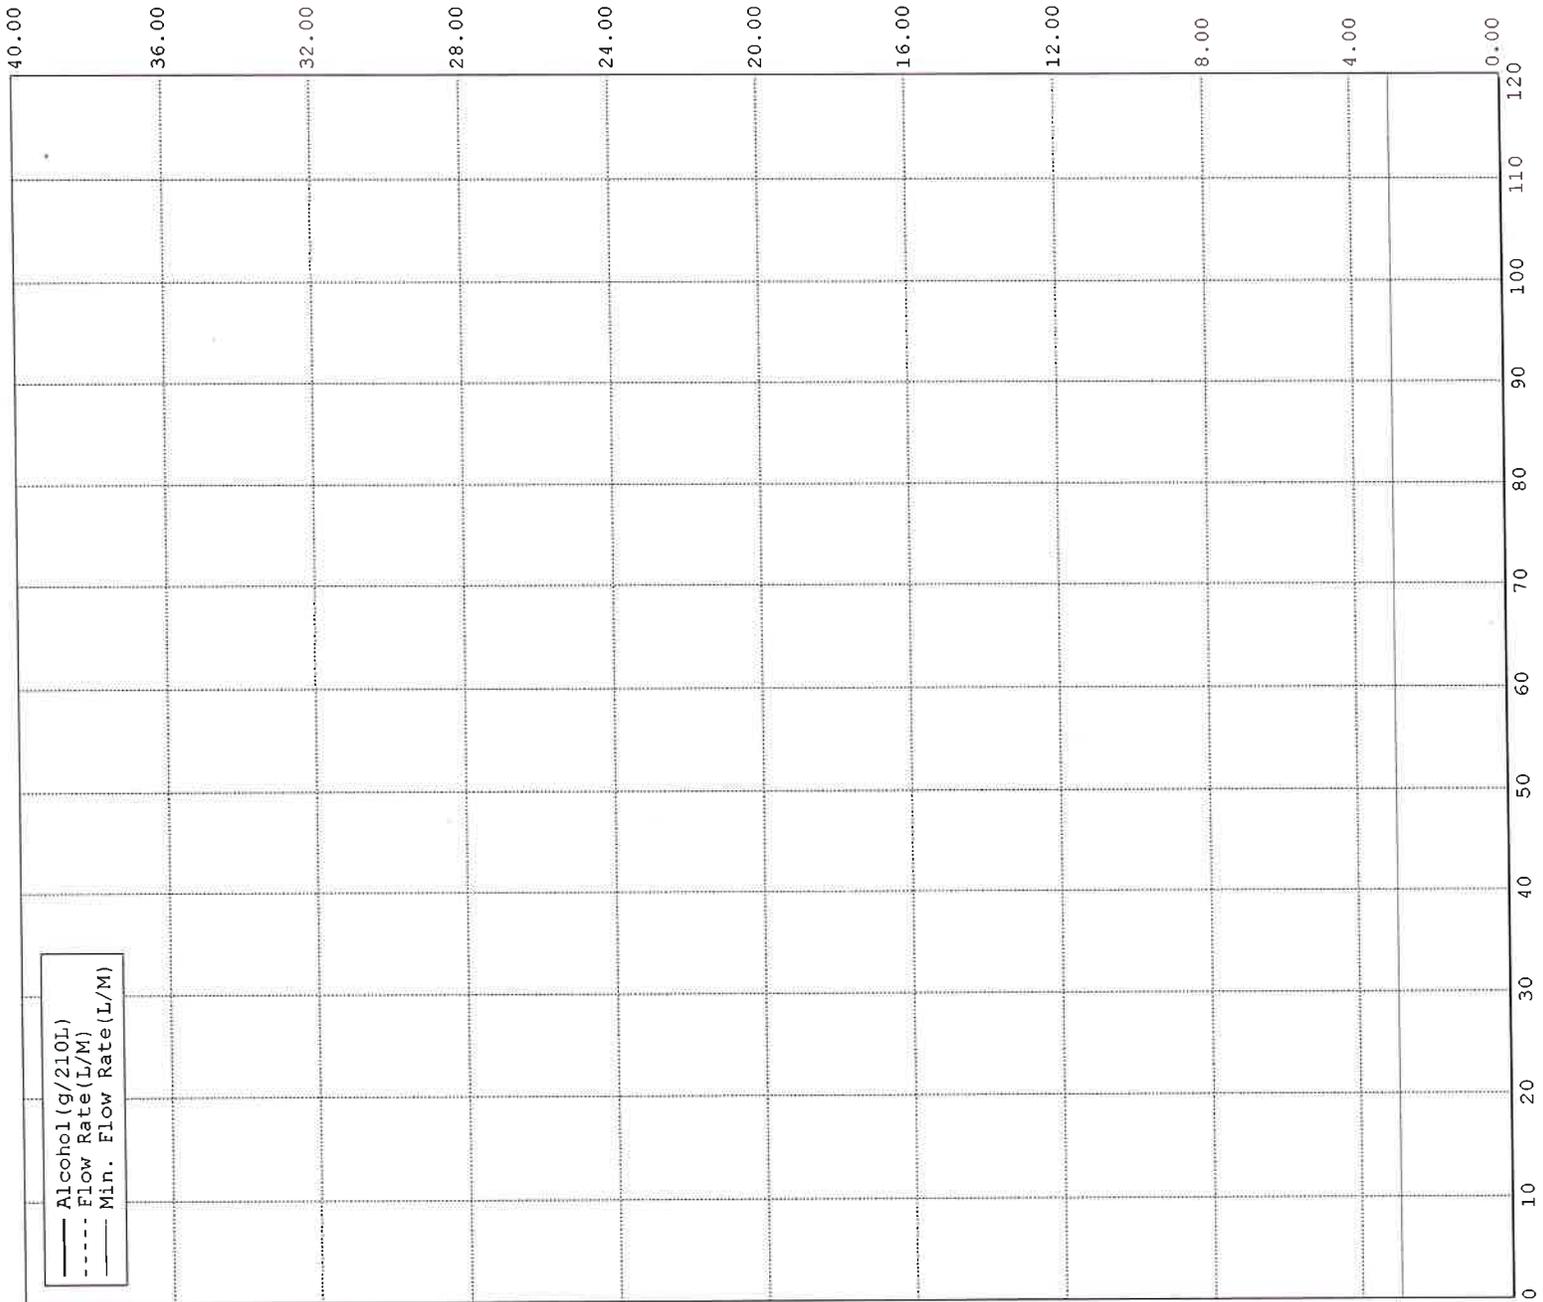

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 03/09/2026
Time: 12:44:01

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 12:45
BLANK TEST 0.000 12:45
INTERNAL STANDARD VERIFIED 12:45
EXTERNAL STANDARD 0.079 12:45
BLANK TEST 0.000 12:46
SUBJECT SAMPLE XXX 12:47

Maximum Attempts Exceeded

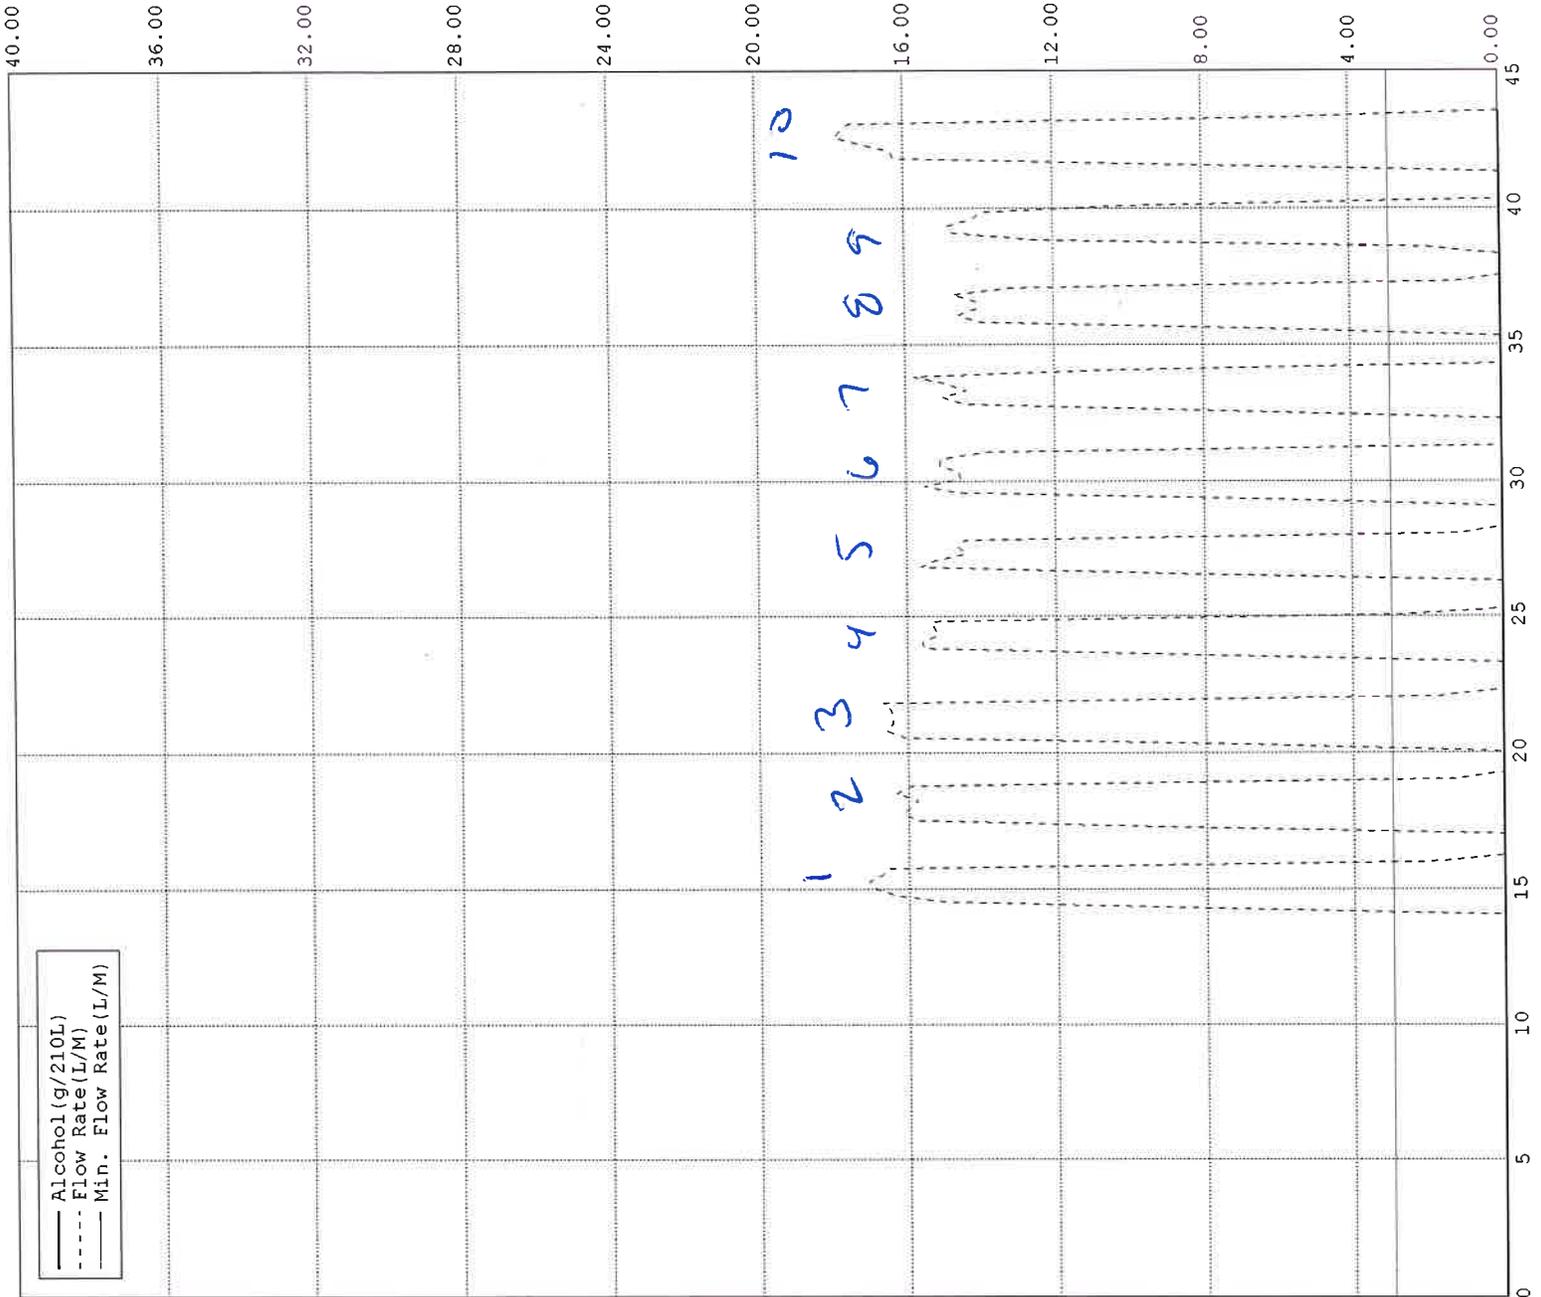

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100681

Date: 03/09/2026
Time: 12:53:42

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INVALID
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	12:54
BLANK TEST	0.000	12:54
INTERNAL STANDARD	VERIFIED	12:55
EXTERNAL STANDARD	0.078	12:55
BLANK TEST	0.000	12:56
SUBJECT SAMPLE	INVALID	12:56

*unable to see end of
detector response.
Performed a second invalid
test. CMG-319124*

CMG

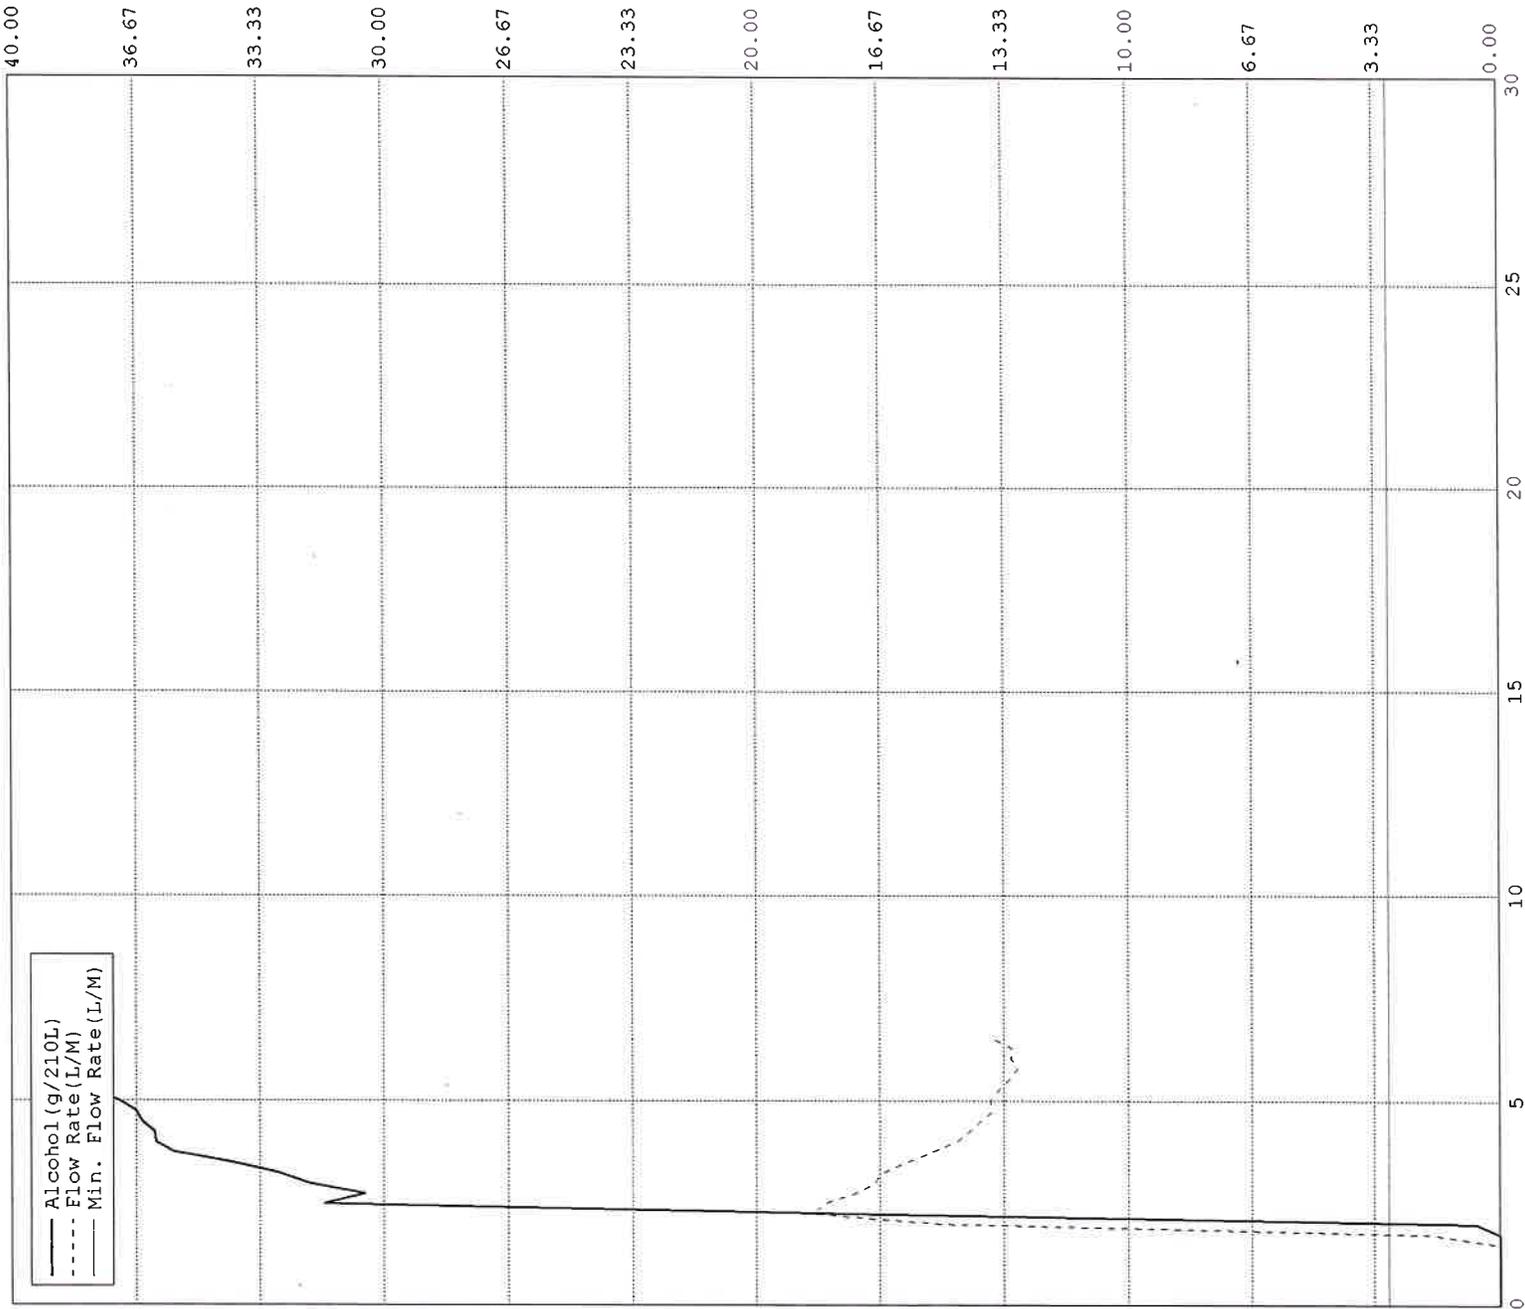

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 03/09/2026
Time: 12:58:41

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INVALID

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.62: 0.079

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK

PASSED 12:59


BLANK TEST 0.000 13:00

INTERNAL STANDARD VERIFIED 13:00

EXTERNAL STANDARD 0.078 13:00

BLANK TEST 0.000 13:01

SUBJECT SAMPLE INVALID 13:01

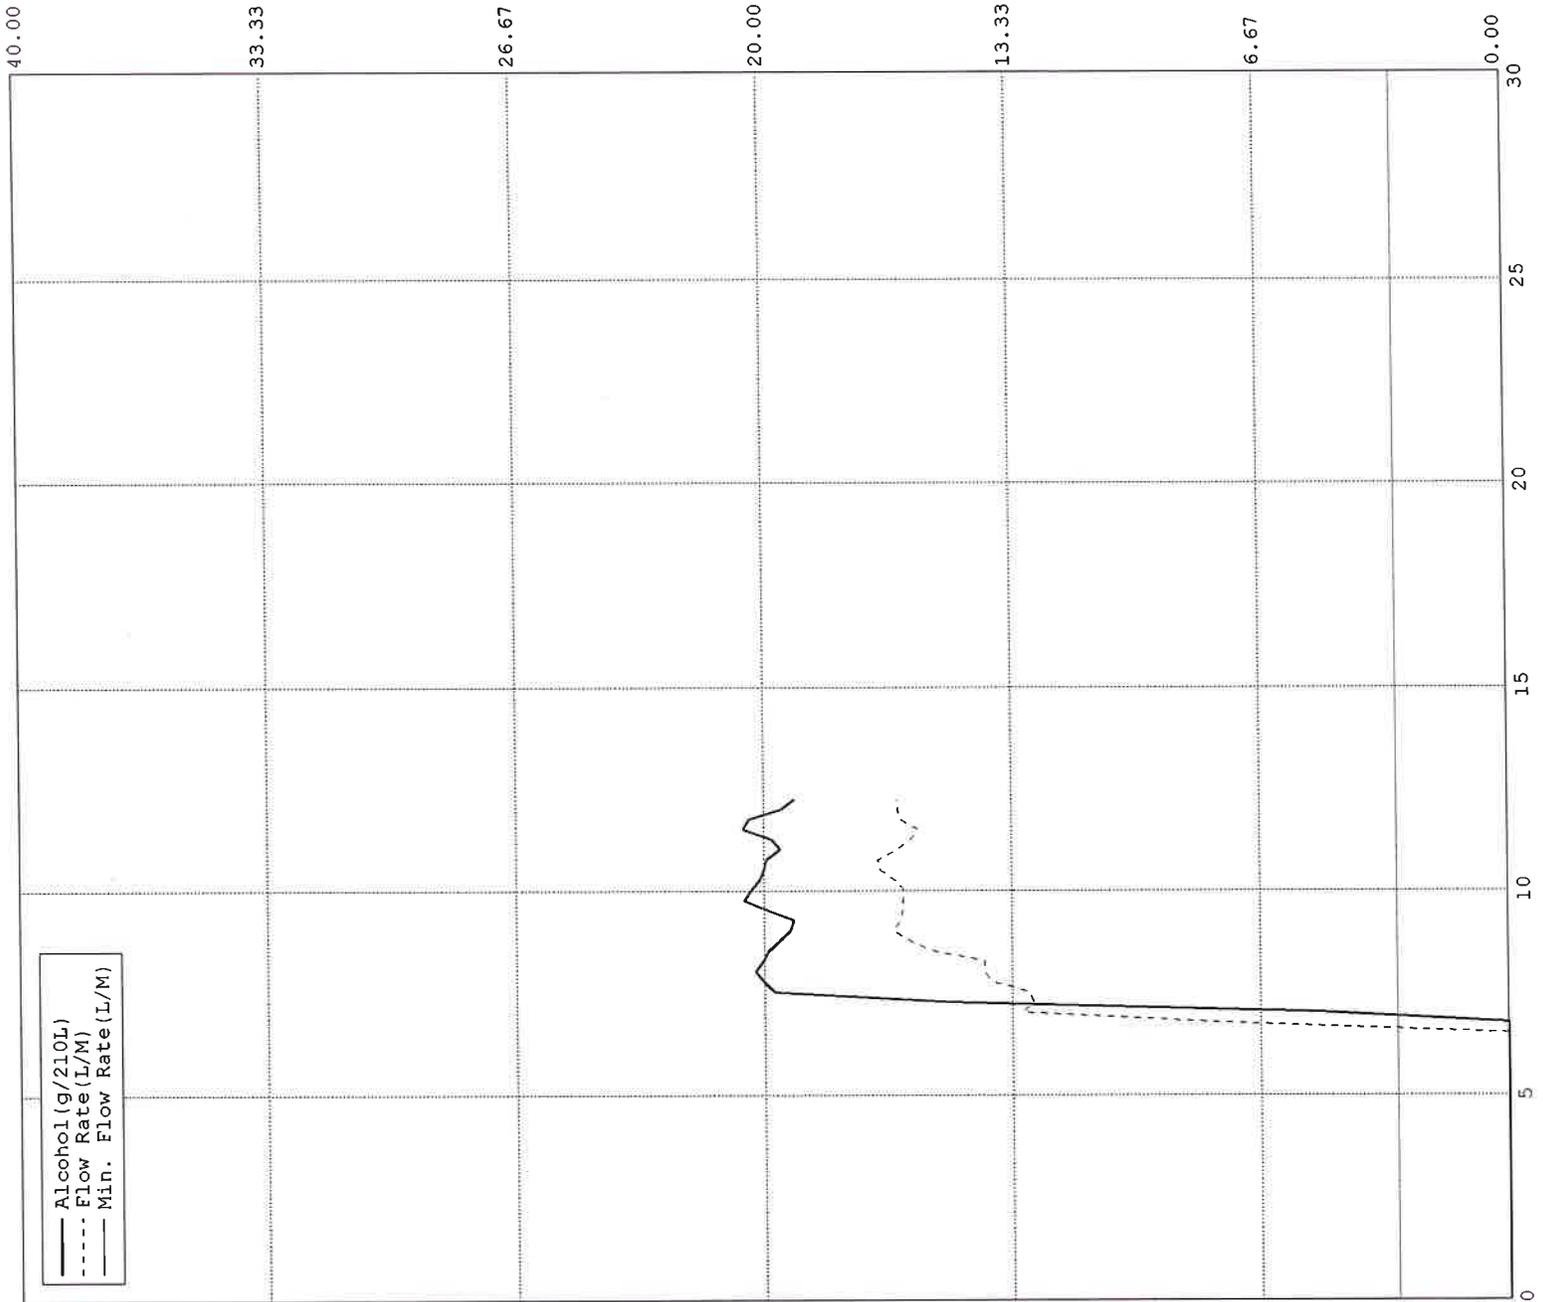

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 03/09/2026
Time: 13:04:08

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

RFI

CASE/REPORT: XXXX


TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 13:05
BLANK TEST 0.000 13:05
INTERNAL STANDARD VERIFIED 13:05
EXTERNAL STANDARD 0.078 13:05
BLANK TEST 0.000 13:06

RFI DETECTED

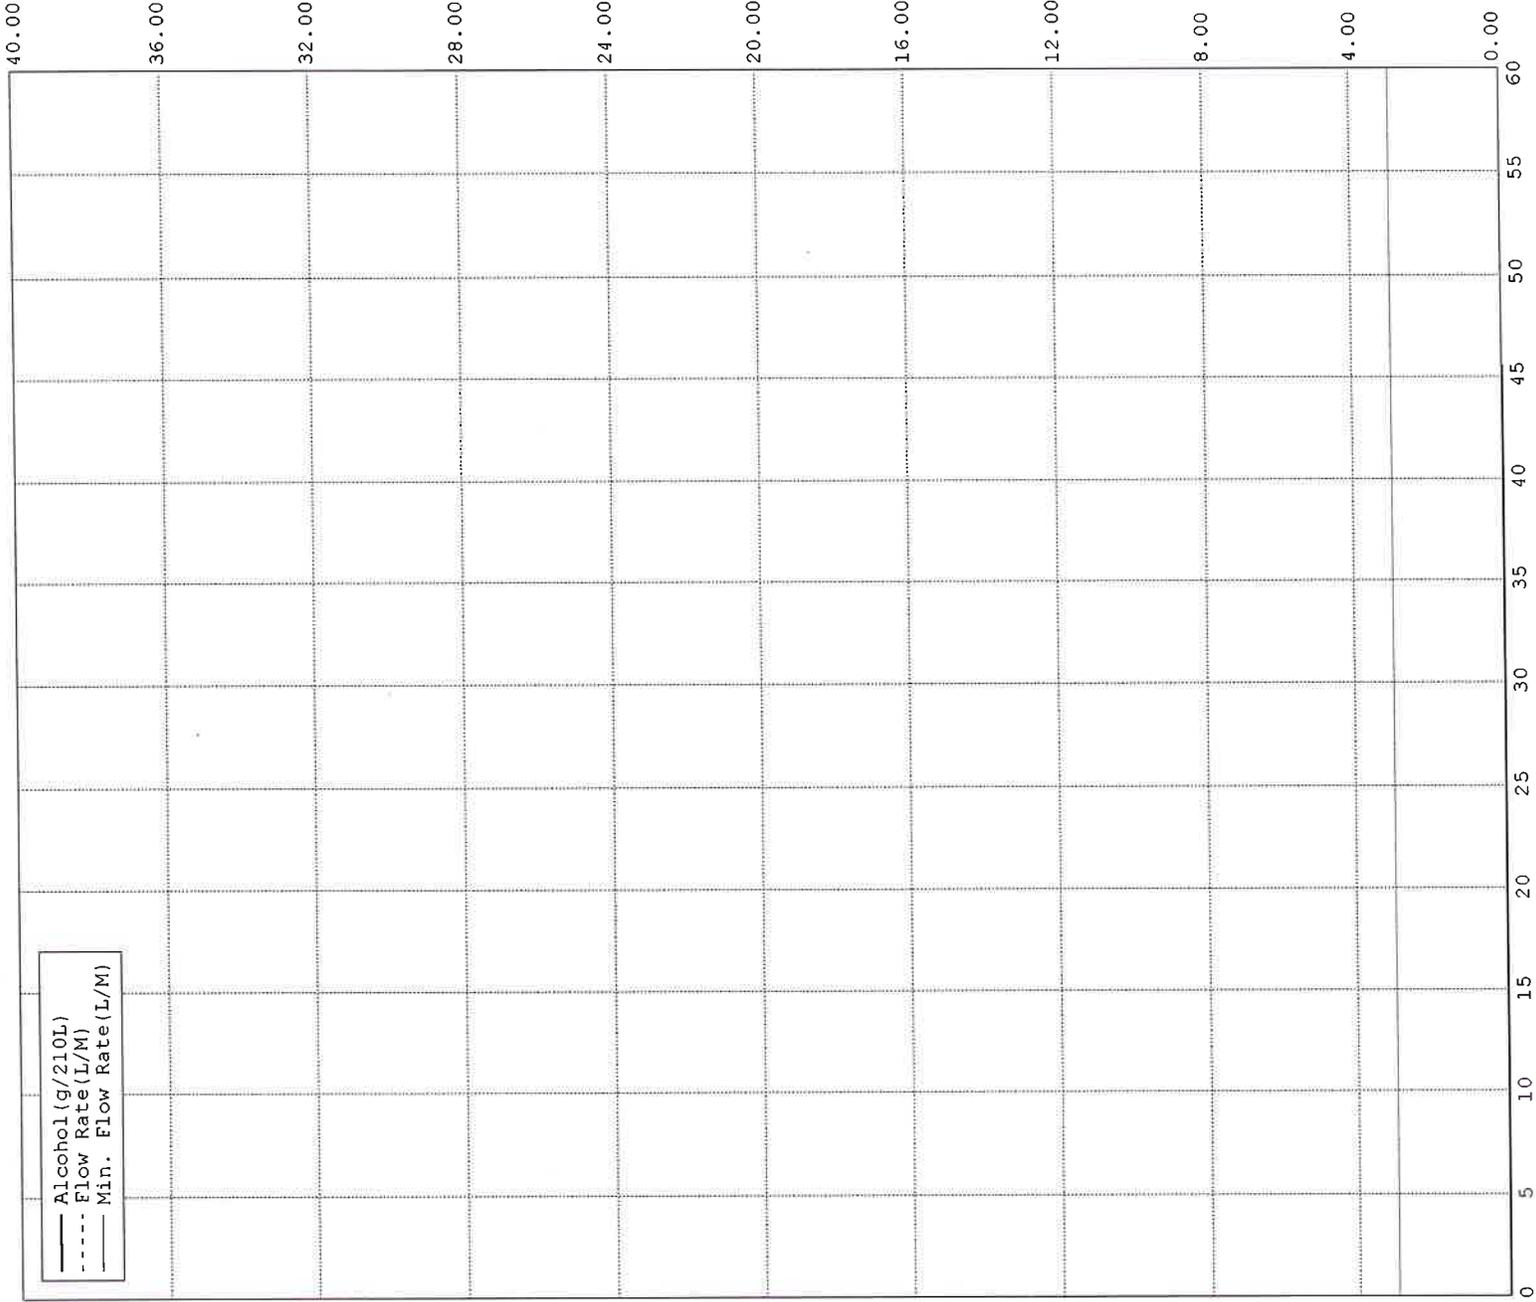

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 03/09/2026

Time: 13:27:47

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INTERFERENCE - ACETONE

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.62: 0.079

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK

PASSED 13:29

0.000 13:29

INTERNAL STANDARD

VERIFIED 13:29

Xq = 0.109 (1.90%)

0.078 13:29

EXTERNAL STANDARD

X[1] = 0.0782 (-0.0010) (0.0031)

0.000 13:30

BLANK TEST

XXX 13:31

SUBJECT SAMPLE

X[1] = 0.1068 (-0.0199) (0.0005)


Interference Detected

Filter 2 Avg: -0.0011

Filter 3 Avg: 0.0028

NW-39124

UNB

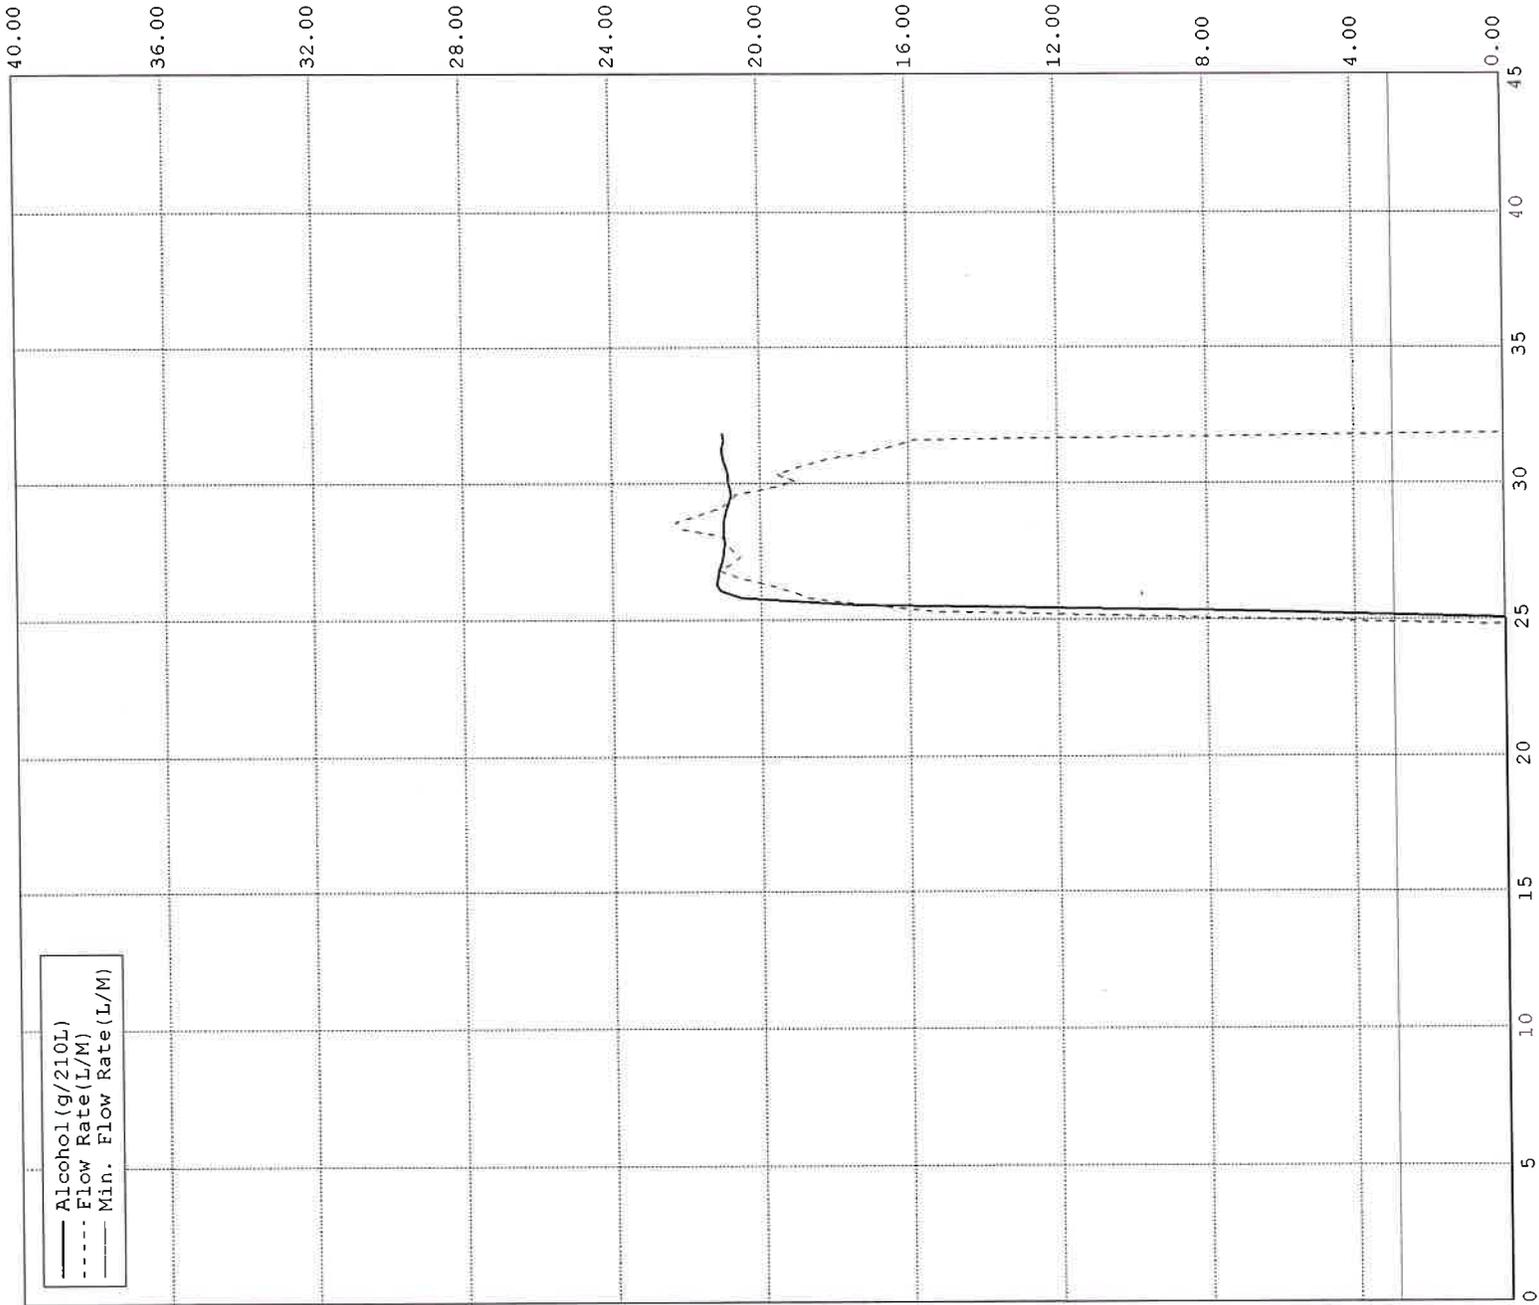

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100681

Date: 03/09/2026
Time: 13:17:27

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 13:19
BLANK TEST 0.000 13:19
INTERNAL STANDARD VERIFIED 13:19
Xq = 0.108 (1.65%) 0.078 13:19
EXTERNAL STANDARD X[1] = 0.0783 (-0.0009) (0.0030)
BLANK TEST 0.000 13:20
SUBJECT SAMPLE XXX 13:21
X[1] = 0.1147 (-0.0234) (0.0017)

Interference Detected

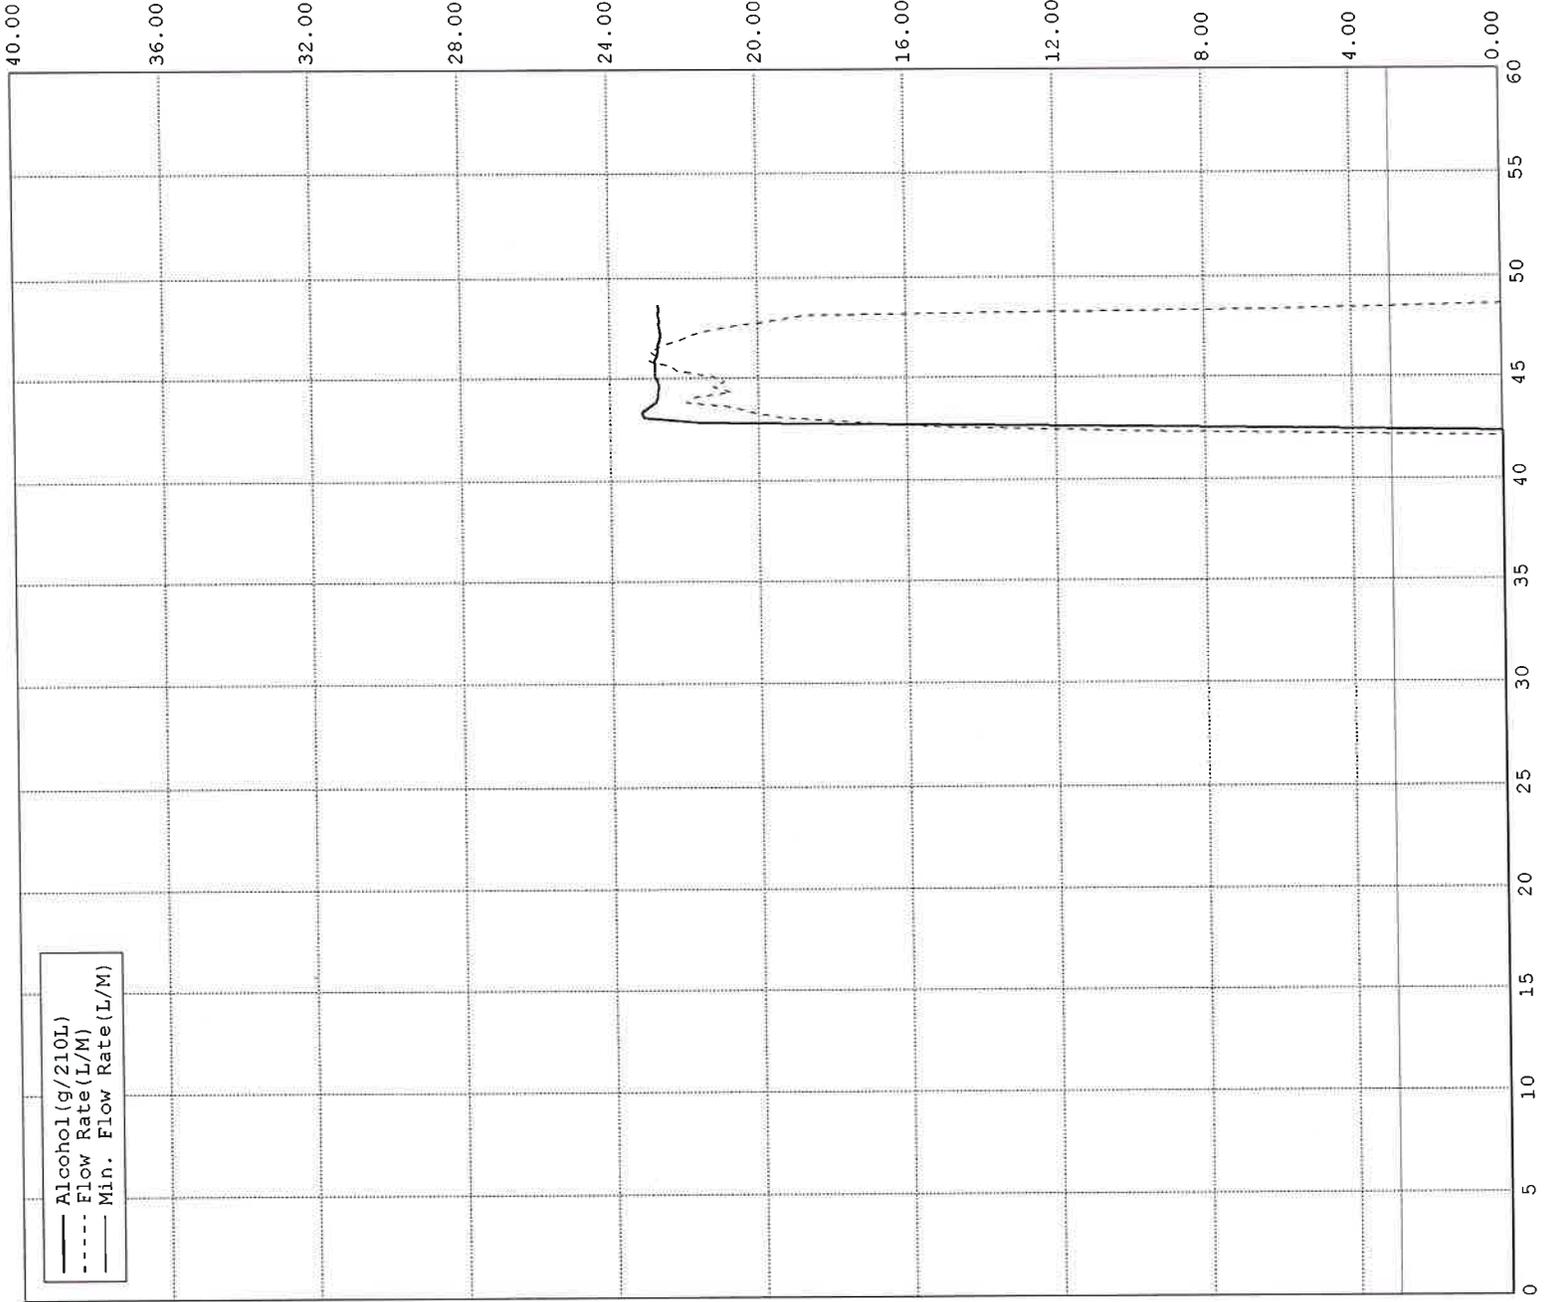

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100681

Date: 03/09/2026

Time: 13:41:27

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INTERFERENCE - NEGATIVE

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080

TARGET AT 29.62: 0.079

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	13:42
BLANK TEST	0.000	13:42
INTERNAL STANDARD	VERIFIED	13:43
Xq = 0.108 (1.49%)		
EXTERNAL STANDARD	0.078	13:43
X[1] = 0.0781 (-0.0013)	(0.0030)	
BLANK TEST	0.000	13:44
SUBJECT SAMPLE (Vol=2.05L)	0.092	13:44
X[1] = 0.0928 (-0.0010)	(0.0005)	
BLANK TEST	0.000	13:45
EXTERNAL STANDARD	0.078	13:45
X[1] = 0.0780 (-0.0012)	(0.0021)	
BLANK TEST	0.000	13:46

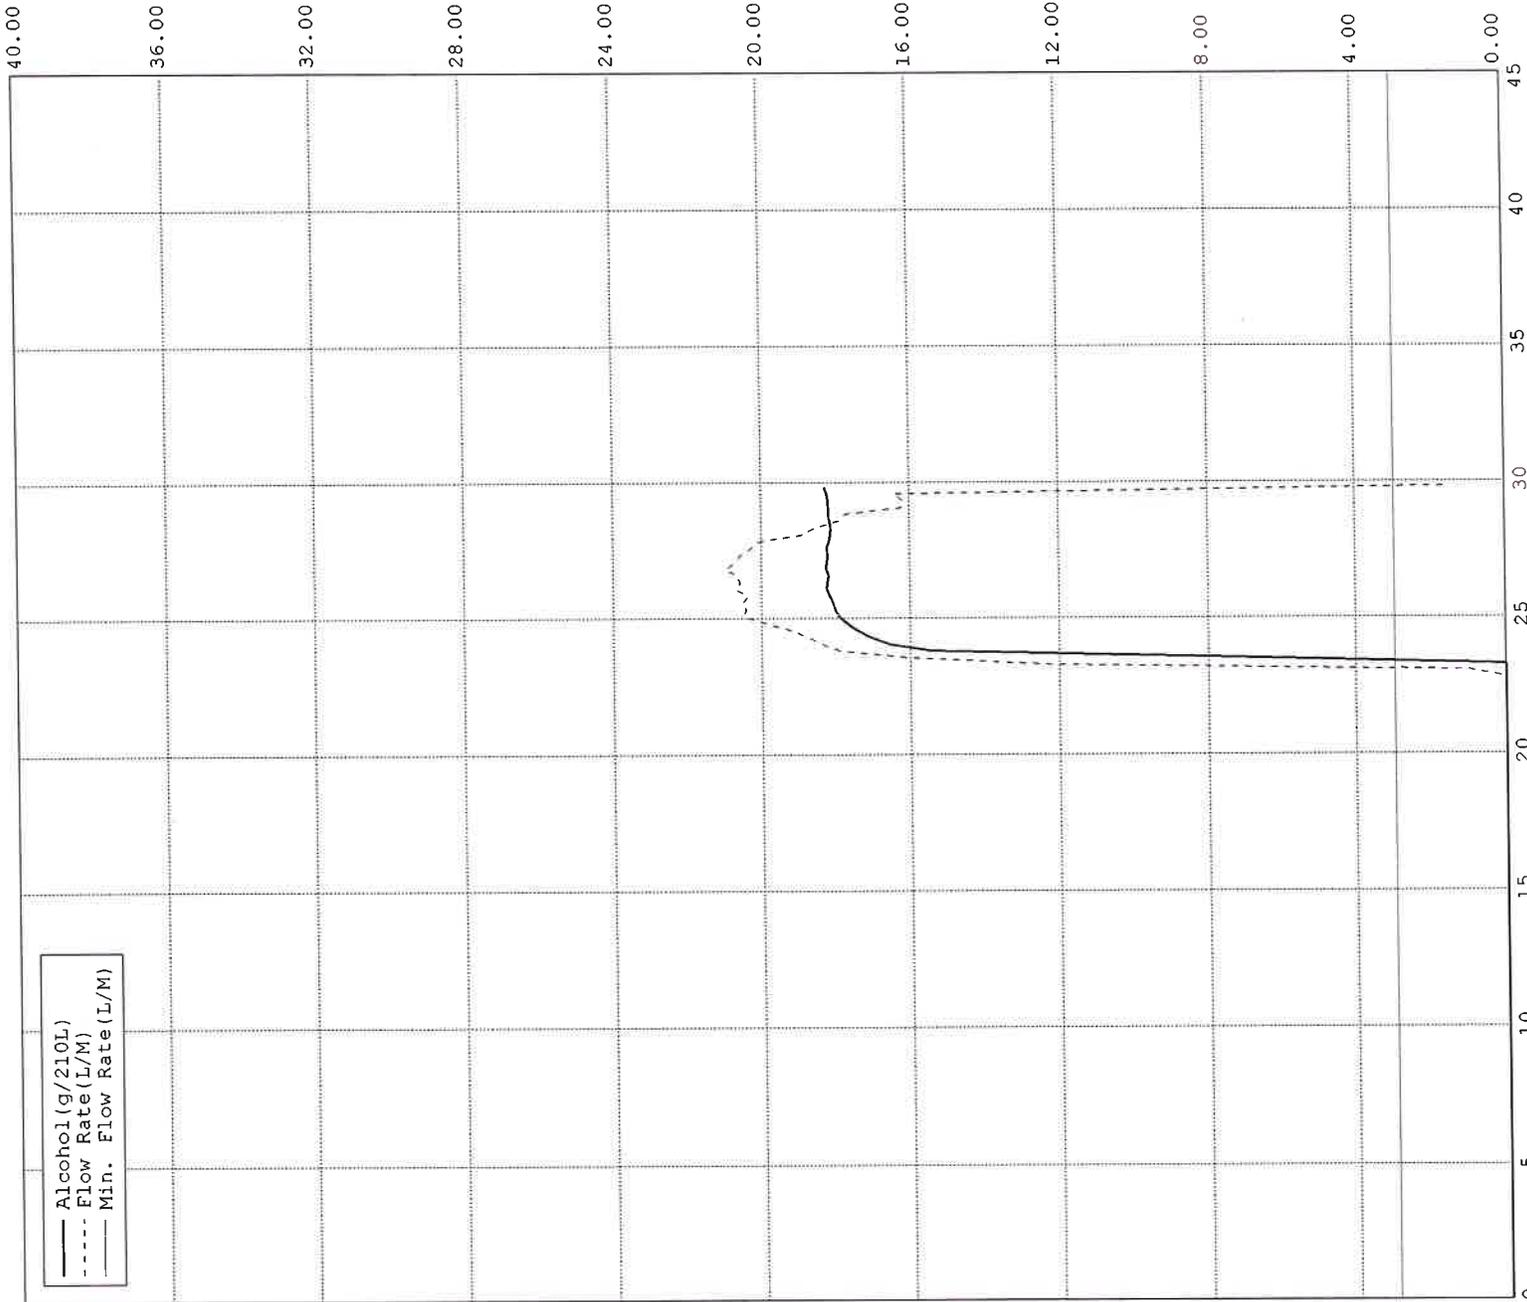

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100691

Date: 03/09/2026
Time: 15:28:43

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.59: 0.079
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	15:29
BLANK TEST	0.000	15:30
INTERNAL STANDARD	VERIFIED	15:30
EXTERNAL STANDARD	0.079	15:30
BLANK TEST	0.000	15:31
SUBJECT SAMPLE (Vol=1.60L)	0.000	15:32
BLANK TEST	0.000	15:33
EXTERNAL STANDARD	0.079	15:33
BLANK TEST	0.000	15:34

