



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100369

Report Issue Date: 11/19/2024
Date Received: 2024-08-01
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG408002	0.020	0.019	0.020	0.020	0.020	0.020	0.020
0.080	0.080	AG335202	0.079	0.078	0.079	0.079	0.079	0.080	0.079
0.300	0.300	AG327804	0.295	0.295	0.294	0.294	0.294	0.294	0.294

As Found - Evaluation Analyst: Megan Carlock
 As Found Conditions - Barometric Pressure (inHg): 29.66 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.5 Relative Humidity (%): 38
 As-Found Lab Activity Date Range: 08/01/2024 - 08/01/2024

Replaced O-ring and replaced missing plastic foot piece.

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG407908	0.040	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.080	AG335202	0.079	0.079	0.079	0.079	0.079	0.078	0.079	+/- 0.004
0.100	0.100	AG333401	0.099	0.099	0.099	0.099	0.099	0.100	0.099	+/- 0.004
0.150	0.150	AG332004	0.147	0.146	0.146	0.146	0.146	0.146	0.146	+/- 0.006
0.300	0.299	AG327804	0.296	0.296	0.296	0.295	0.295	0.296	0.296	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.88 Barometer Used: Fisher S/N 230307229 Temperature (C): 20.8 Relative Humidity (%): 17
 As-Left Lab Activity Date Range: 10/21/2024 - 10/21/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Colleen O'Bryant on 11/19/2024

colleen.obryant@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 11/19/2024

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100369 Analyst or Technician Name: C. O. Bryant

DataMaster DMT Calibration Start Date: 10/21/24

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 2 30307299
Calibration Due Date: 5/2/25
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.88 Temperature(C) 20.8 Relative Humidity(%) 17

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20240731MUC Expiration Date: 10/31/24

COB 2024.11.19 Simulator S/N: DR4178 Thermometer Verification Performed?

2. Isopropanol Reagent Lot Number: 20240501MUC Expiration Date: 10/31/24

Simulator S/N: DR6267 Thermometer Verification Performed?

3. Negative (Ethanol Only) Lot Number: 23IP41283 Expiration Date: 10/31/24

Simulator S/N: DR4163 Thermometer Verification Performed?

09/20/2025

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 9/19/25

COB 2024.10.21

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 10/21/24

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): C. O. Bryant 10/21/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100369

Date: 10/21/2024
Time: 09:08:31

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 45.4°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.58 V PASSED
(0.93 V - 2.17 V)
Cooler Voltage = 1.56 V PASSED
(1.00 V - 2.32 V)
Bias Voltage = 80 V PASSED
(47 V - 109 V)
Chopper Freq = 529 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.9 in

PUMP INFO

Flow Rate = 4.796 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.001 V <= 0.010 V)
PUMP OFF PASSED
(0.001 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.085 1.56% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100369

Date: 10/21/2024
Time: 10:01 AM

Temperatures (°C)

Sample Cell: 49.0°C
Breath Tube: 45.2°C

Current Barometer 29.9 in
Volume (Ltr) 1.54

Settings

Lamp: 1.66 V
Bias: 80 V
Cooler: 1.56 V
Chopper: 528 Hz

Voltages (V)

Flow: 1.04 V
Detector: -0.034 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100369

Date: 12/17/2019
Time: 13:08:22

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca = 0.1000
CAL = 0.971577 0.800 <= CAL < 1.200
b1 = 0.0006 0.0000 <= b1 < 0.0040
b2 = 0.0051 0.0010 <= b2 < 0.0100
b3 = 0.0004 0.0000 <= b3 < 0.0040
Xq = 0.0837 0.0500 <= Xq < 0.2000
a21 = 1.196816 1.050 <= a21 < 1.300
a31 = 0.486796 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
 DATA MASTER dmt: 100369

Date: 10/21/2024
 Time: 10:04:52

SUBJECT NAME:
 TEST TEST
 LICENSE #: VOLUME TEST


OPERATOR NAME:
 COLLEEN S O'BRYANT
 OPERATOR'S #: 6237

DEPT/AGENCY:
 AAA1
 CASE/REPORT: 24-1234
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.88: 0.080
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:06
BLANK TEST	0.000	10:06
INTERNAL STANDARD	VERIFIED	10:06
EXTERNAL STANDARD	0.079	10:06
BLANK TEST	0.000	10:07
SUBJECT SAMPLE (Vol=1.57L)	0.000	10:08
BLANK TEST	0.000	10:09
EXTERNAL STANDARD	0.079	10:10
BLANK TEST	0.000	10:10

COB

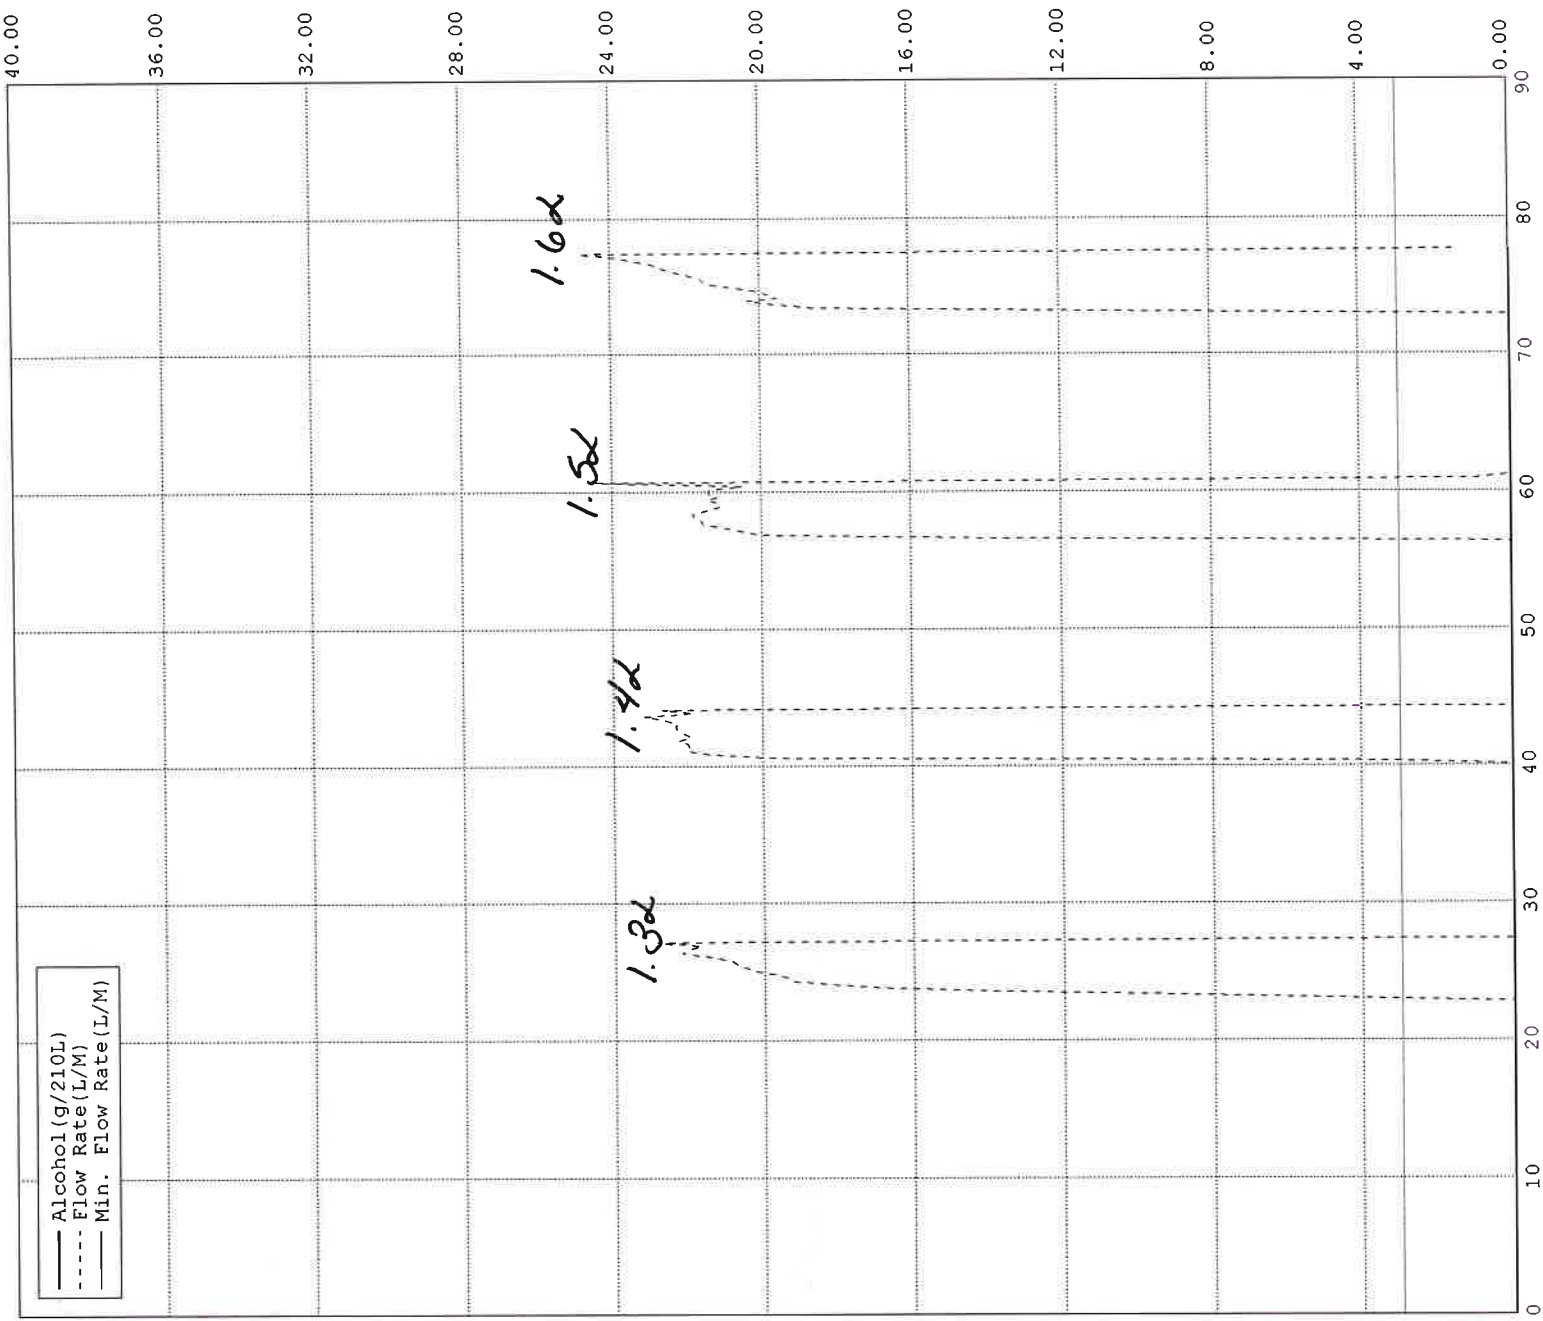

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100369

Date: 10/21/2024
 Time: 10:13:00

SUPERVISOR NAME:
 COLLEEN S OBRyant
 OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.040	0.0400	0.0000
0.080	0.0788	0.0004
0.100	0.0992	0.0004
0.150	0.1462	0.0004
0.299	0.2956	0.0005

SLOPE = 0.986203
 R² = 0.999915

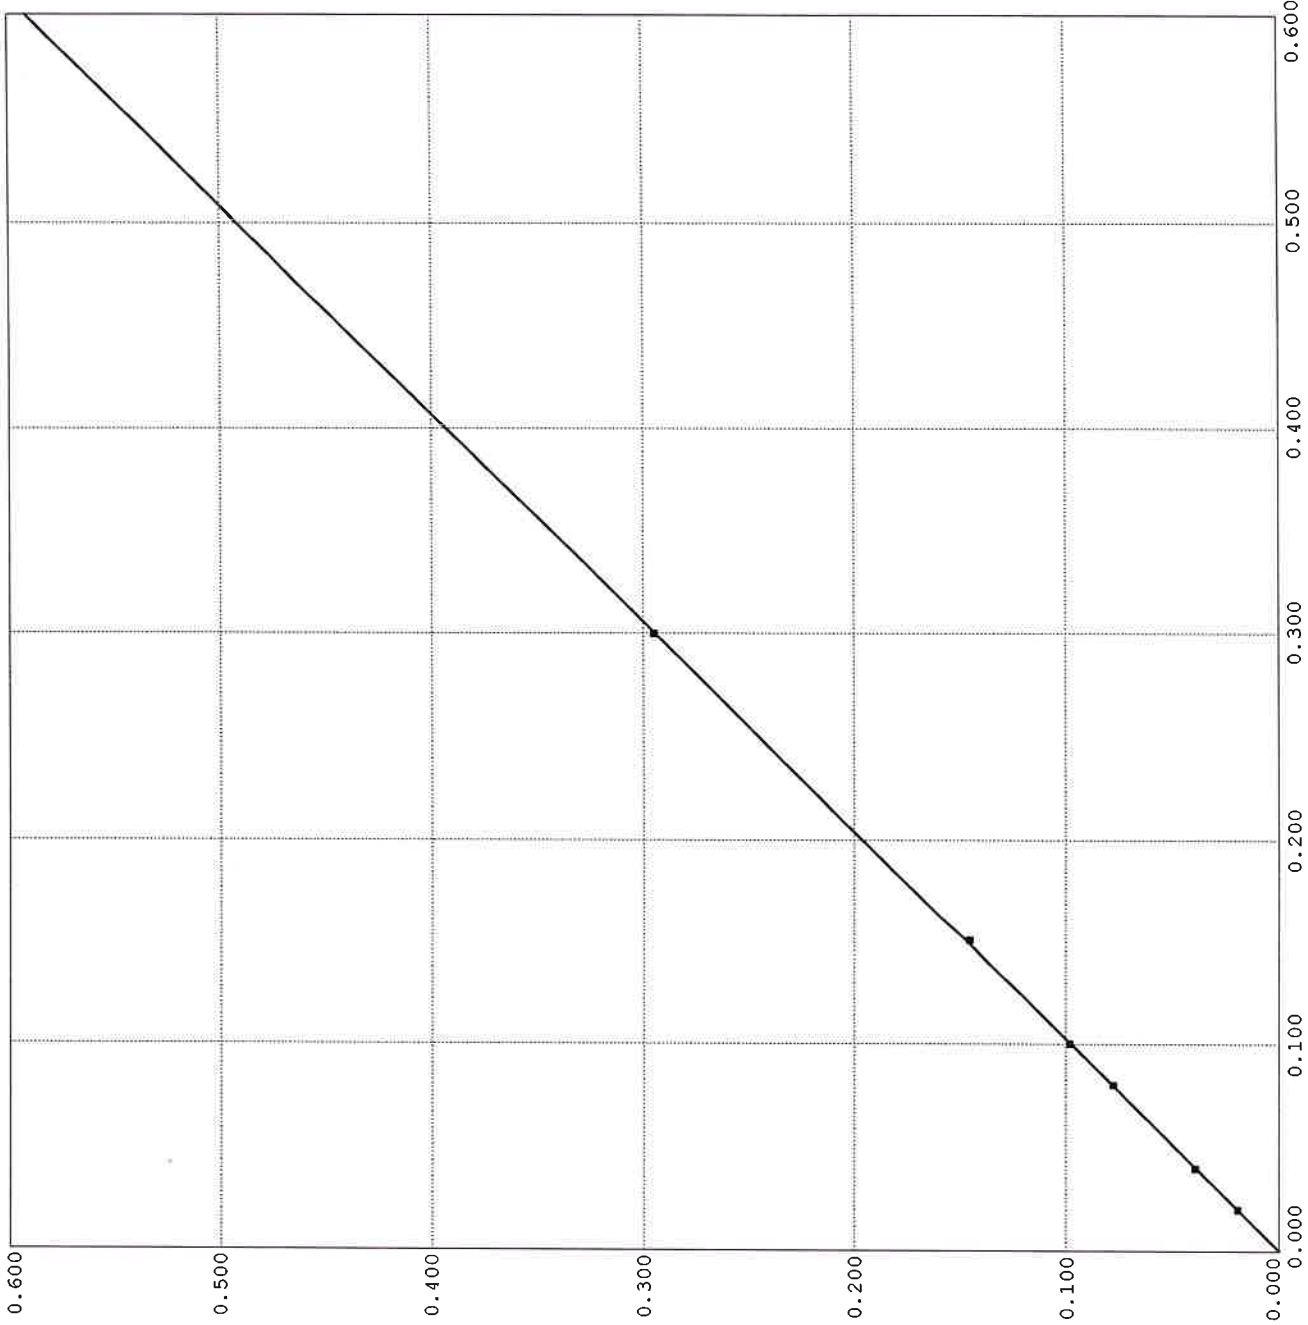

CSB

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100369






Date: 10/21/2024
Time: 10:13:02

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.87: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 864 psi

BLANK TEST	0.000	10:14
INTERNAL STANDARD	VERIFIED	10:14
EXTERNAL STANDARD	0.020	10:14
BLANK TEST	0.000	10:15
EXTERNAL STANDARD	0.020	10:15
BLANK TEST	0.000	10:16
EXTERNAL STANDARD	0.020	10:16
BLANK TEST	0.000	10:17
EXTERNAL STANDARD	0.020	10:17
BLANK TEST	0.000	10:18
EXTERNAL STANDARD	0.020	10:19
BLANK TEST	0.000	10:19

Average = 0.0200
Std Dev = 0.0000

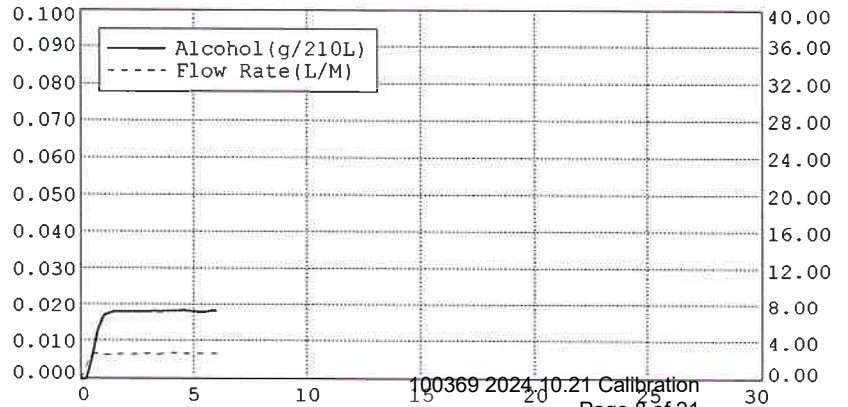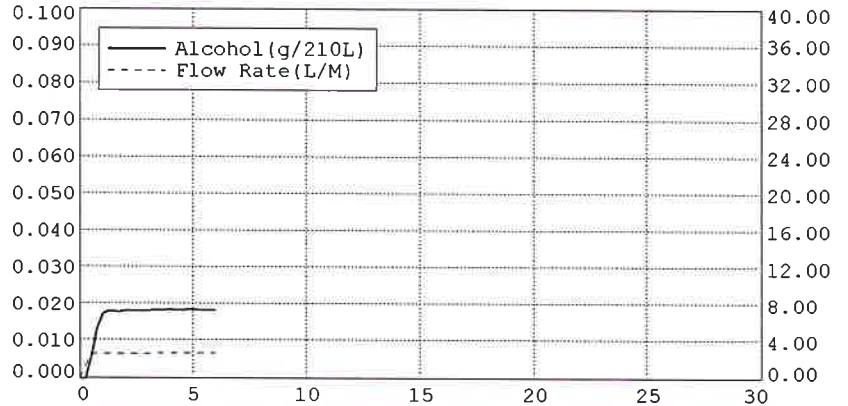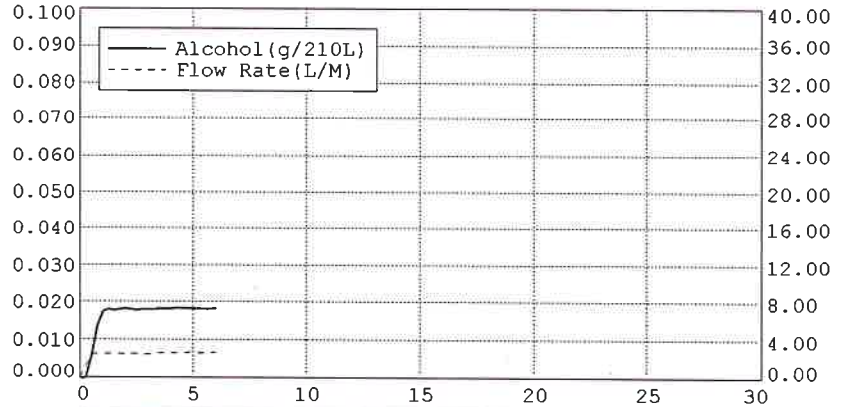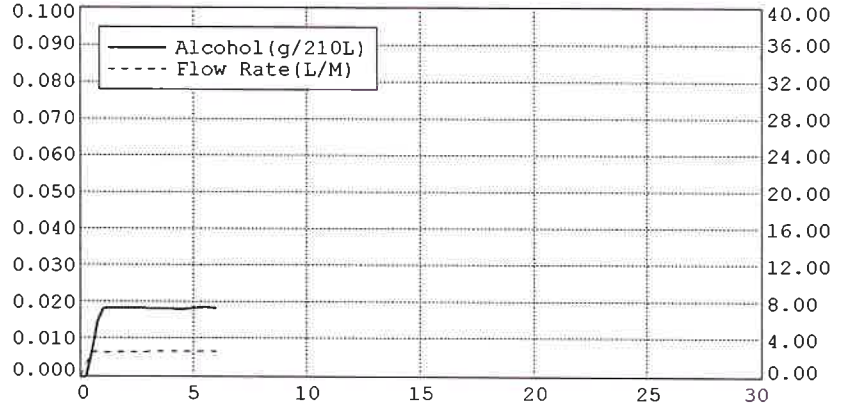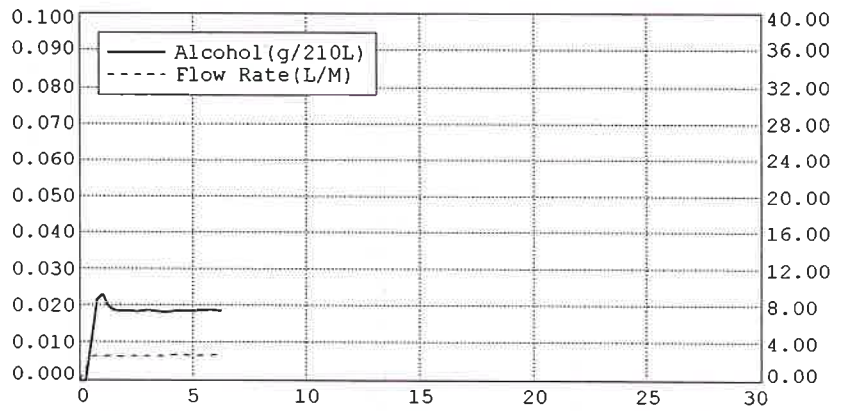

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100369






Date: 10/21/2024
Time: 10:21:28

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.87: 0.040
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 1057 psi

BLANK TEST	0.000	10:22
INTERNAL STANDARD	VERIFIED	10:22
EXTERNAL STANDARD	0.040	10:22
BLANK TEST	0.000	10:23
EXTERNAL STANDARD	0.040	10:24
BLANK TEST	0.000	10:25
EXTERNAL STANDARD	0.040	10:25
BLANK TEST	0.000	10:26
EXTERNAL STANDARD	0.040	10:26
BLANK TEST	0.000	10:27
EXTERNAL STANDARD	0.040	10:27
BLANK TEST	0.000	10:28

Average = 0.0400
Std Dev = 0.0000

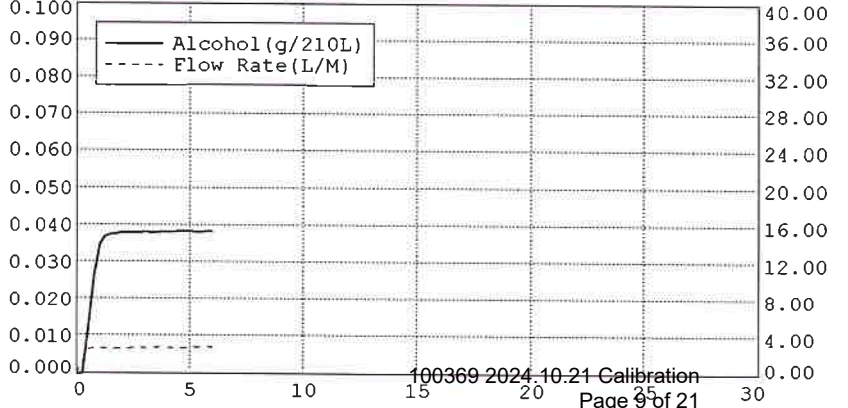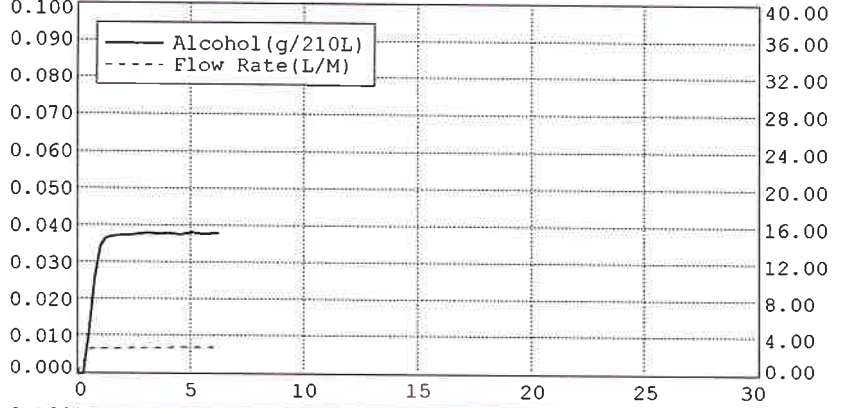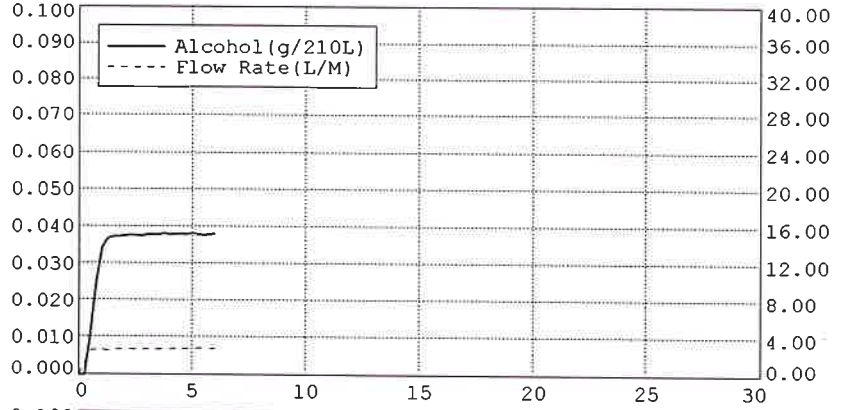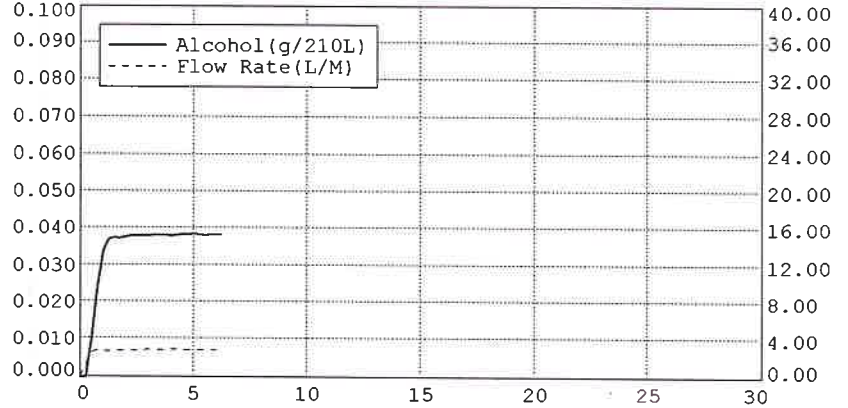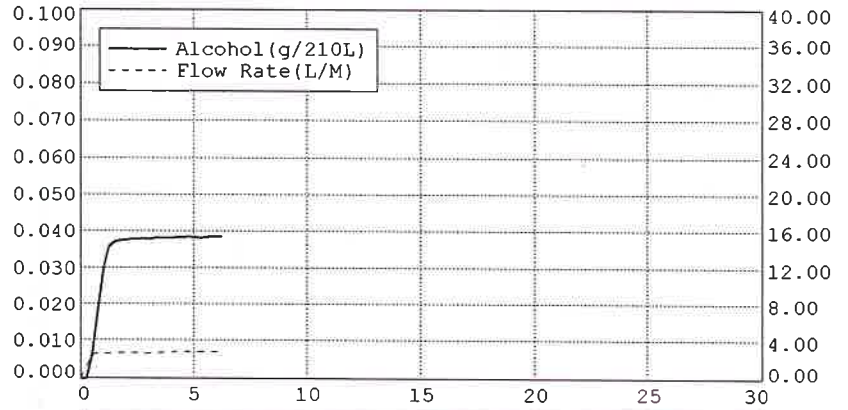

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100369






Date: 10/21/2024
 Time: 10:31:18

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.87: 0.080
 LOT #: AG335202
 EXPIRATION: 12/18/2025
 TANK PRESSURE: 710 psi

BLANK TEST	0.000	10:32
INTERNAL STANDARD	VERIFIED	10:32
EXTERNAL STANDARD	0.079	10:33
BLANK TEST	0.000	10:34
EXTERNAL STANDARD	0.079	10:34
BLANK TEST	0.000	10:35
EXTERNAL STANDARD	0.079	10:35
BLANK TEST	0.000	10:36
EXTERNAL STANDARD	0.079	10:36
BLANK TEST	0.000	10:37
EXTERNAL STANDARD	0.078	10:37
BLANK TEST	0.000	10:38

Average = 0.0788
 Std Dev = 0.0004

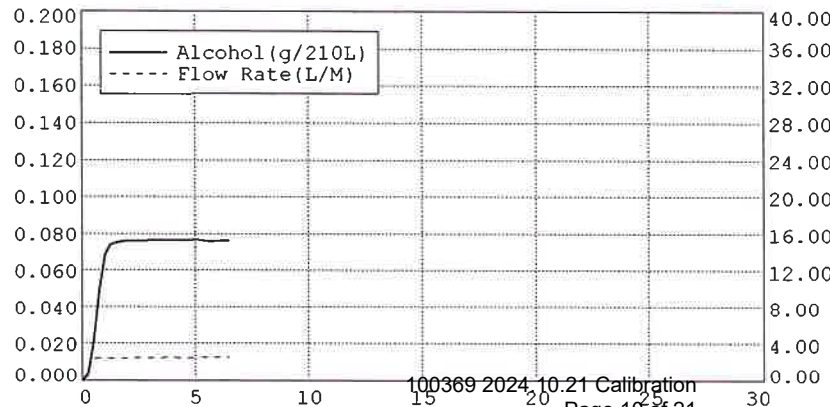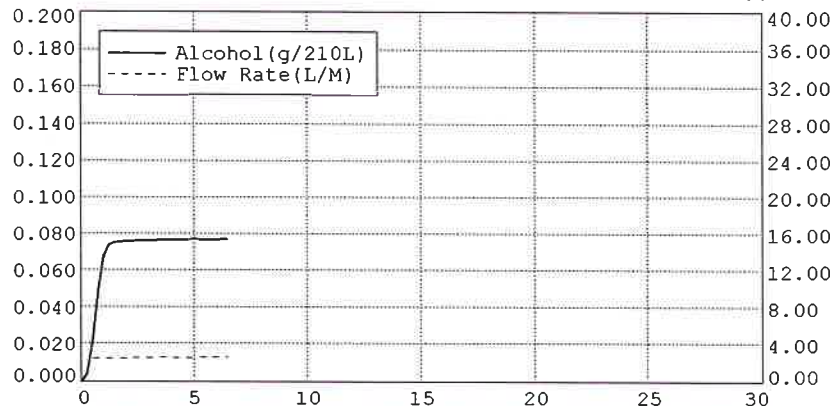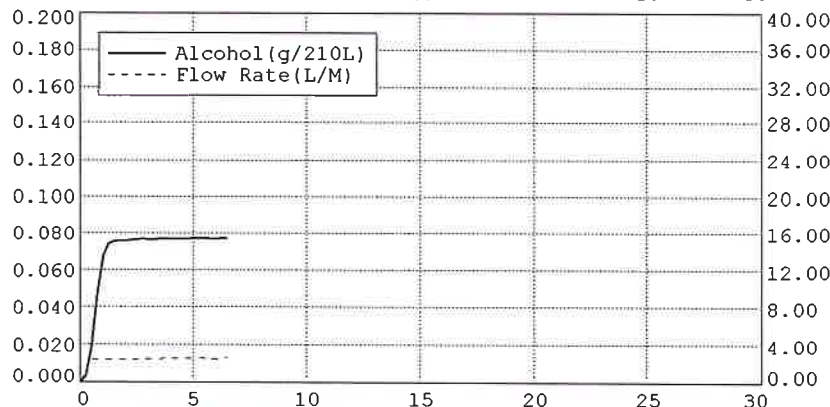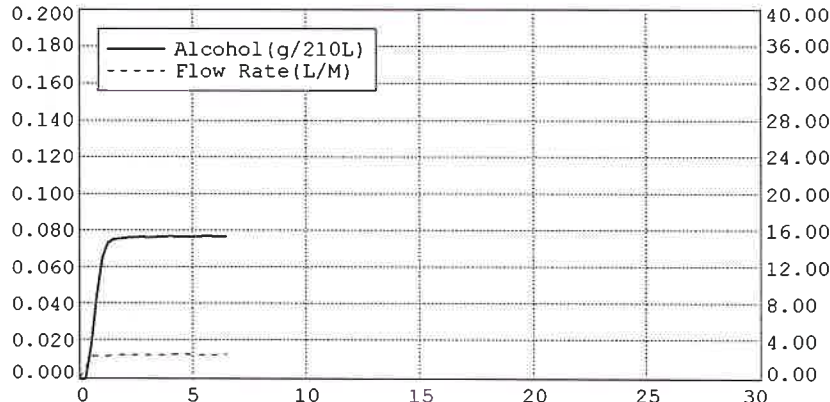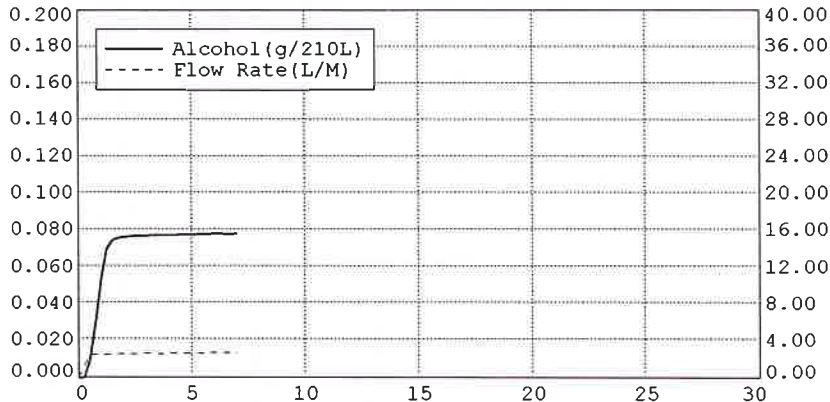

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100369






Date: 10/21/2024
 Time: 10:40:07

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.87: 0.100
 LOT #: AG333401
 EXPIRATION: 11/30/2025
 TANK PRESSURE: 765 psi

BLANK TEST	0.000	10:41
INTERNAL STANDARD	VERIFIED	10:41
EXTERNAL STANDARD	0.099	10:41
BLANK TEST	0.000	10:42
EXTERNAL STANDARD	0.099	10:42
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.099	10:43
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.099	10:45
BLANK TEST	0.000	10:45
EXTERNAL STANDARD	0.100	10:46
BLANK TEST	0.000	10:47

Average = 0.0992
 Std Dev = 0.0004

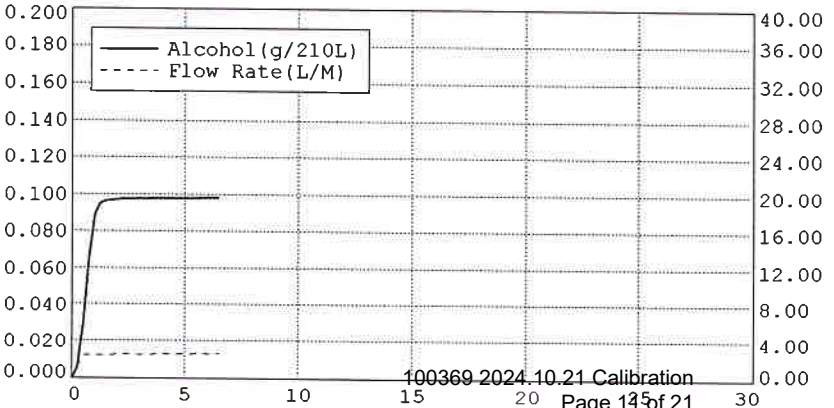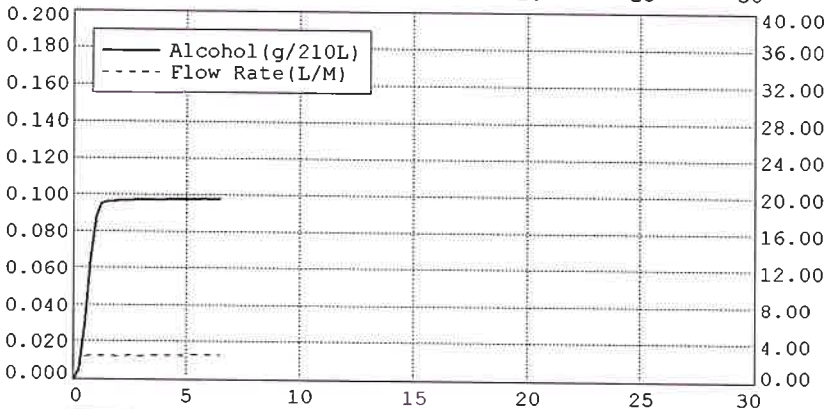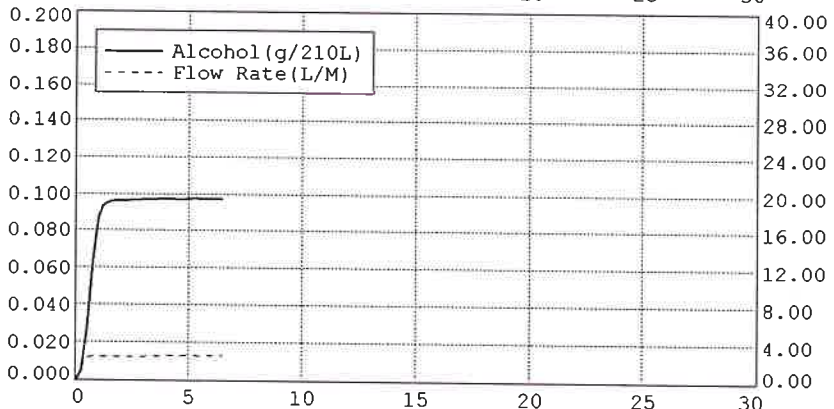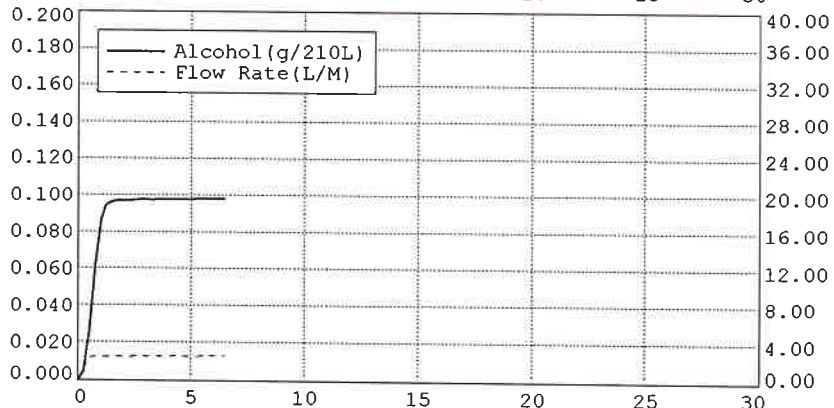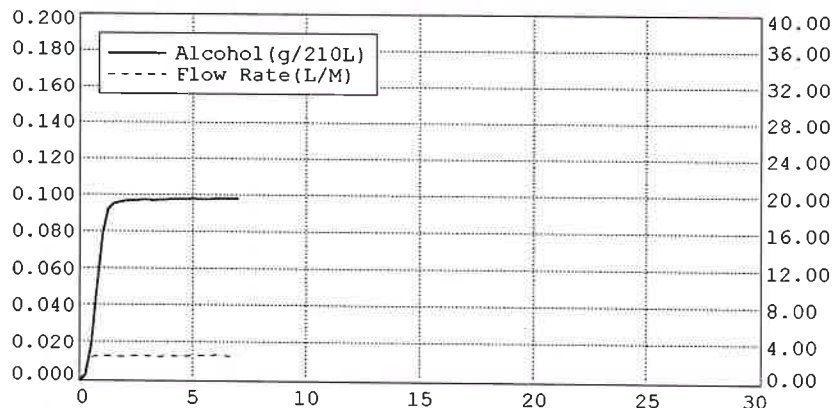

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100369






Date: 10/21/2024
 Time: 10:49:32

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.86: 0.150
 LOT #: AG332004
 EXPIRATION: 11/16/2025
 TANK PRESSURE: 396 psi

BLANK TEST	0.000	10:50
INTERNAL STANDARD	VERIFIED	10:50
EXTERNAL STANDARD	0.147	10:51
BLANK TEST	0.000	10:51
EXTERNAL STANDARD	0.146	10:52
BLANK TEST	0.000	10:53
EXTERNAL STANDARD	0.146	10:53
BLANK TEST	0.000	10:54
EXTERNAL STANDARD	0.146	10:54
BLANK TEST	0.000	10:55
EXTERNAL STANDARD	0.146	10:55
BLANK TEST	0.000	10:56

Average = 0.1462
 Std Dev = 0.0004

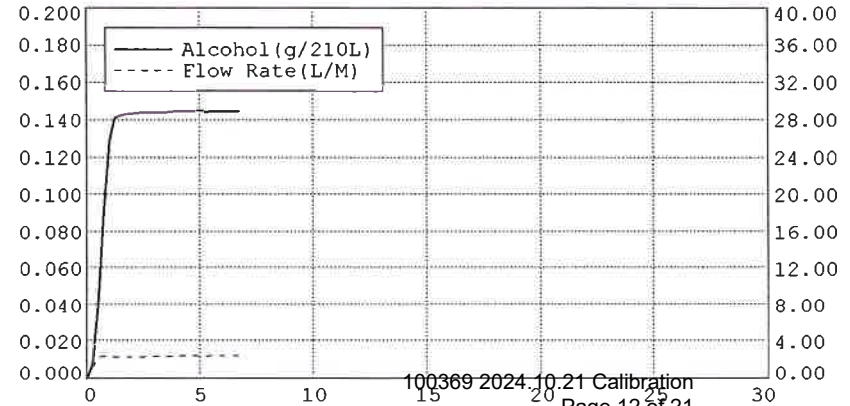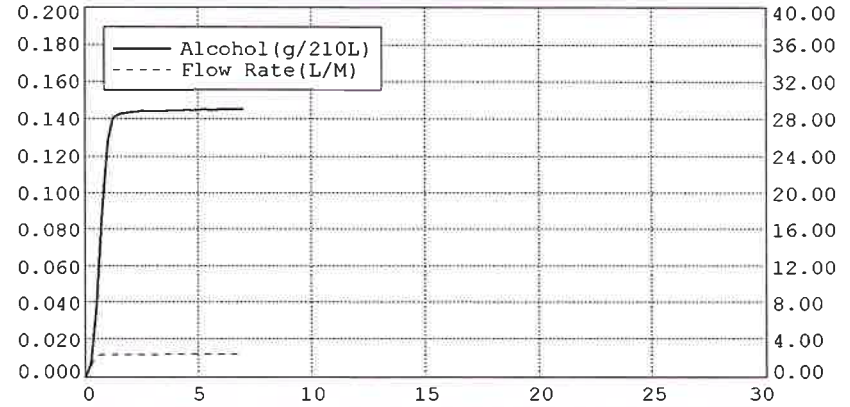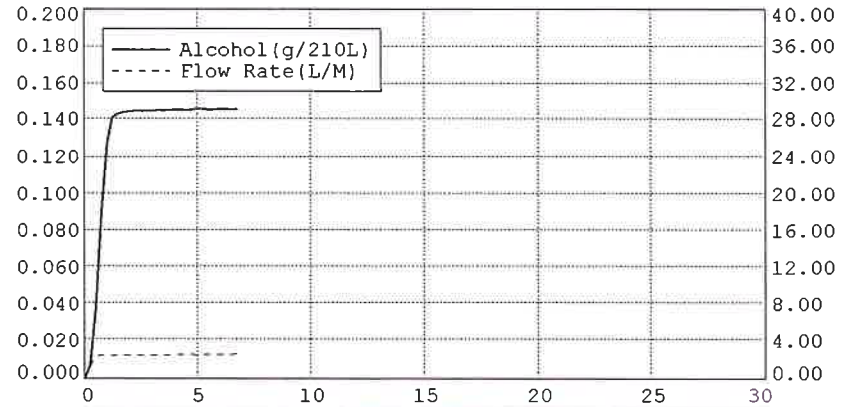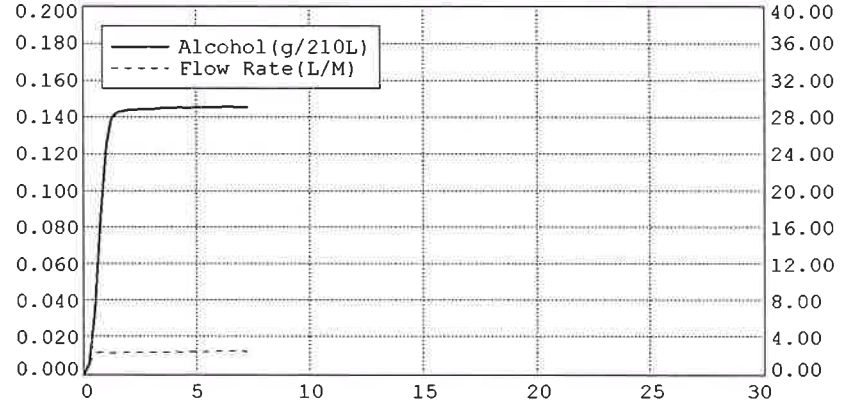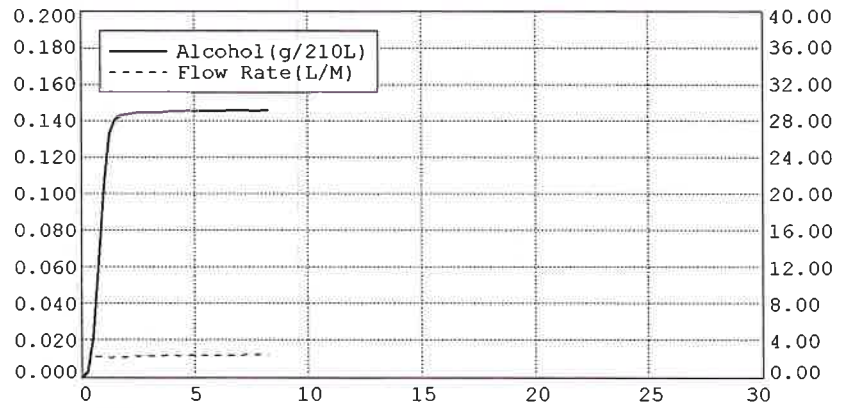

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100369






Date: 10/21/2024
 Time: 10:57:54

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.86: 0.299
 LOT #: AG327804
 EXPIRATION: 10/05/2025
 TANK PRESSURE: 205 psi

BLANK TEST	0.000	10:59
INTERNAL STANDARD	VERIFIED	10:59
EXTERNAL STANDARD	0.296	10:59
BLANK TEST	0.000	11:00
EXTERNAL STANDARD	0.296	11:00
BLANK TEST	0.000	11:01
EXTERNAL STANDARD	0.296	11:01
BLANK TEST	0.000	11:02
EXTERNAL STANDARD	0.295	11:03
BLANK TEST	0.000	11:03
EXTERNAL STANDARD	0.295	11:04
BLANK TEST	0.000	11:05

Average = 0.2956
 Std Dev = 0.0005

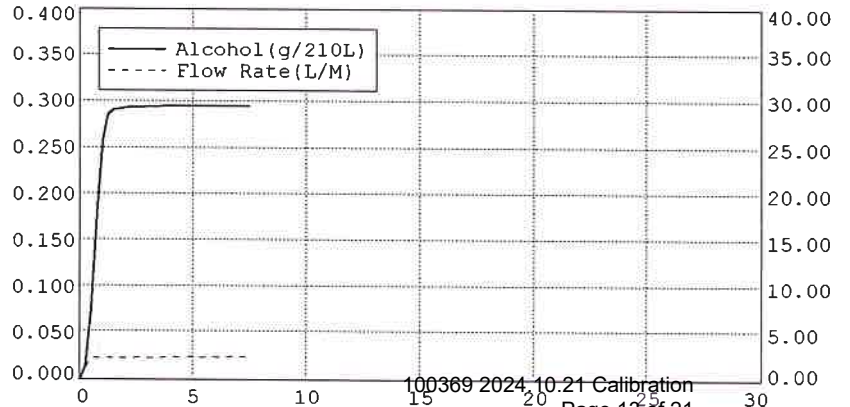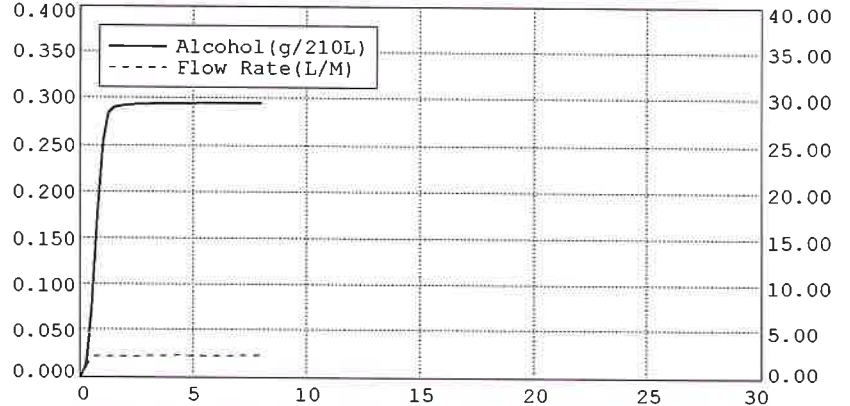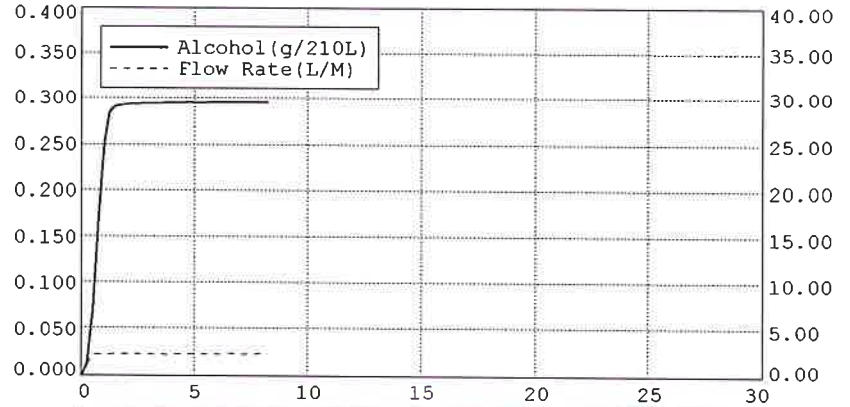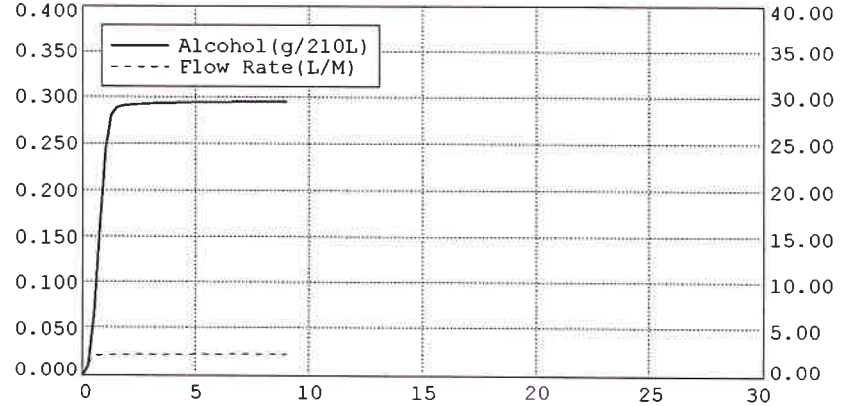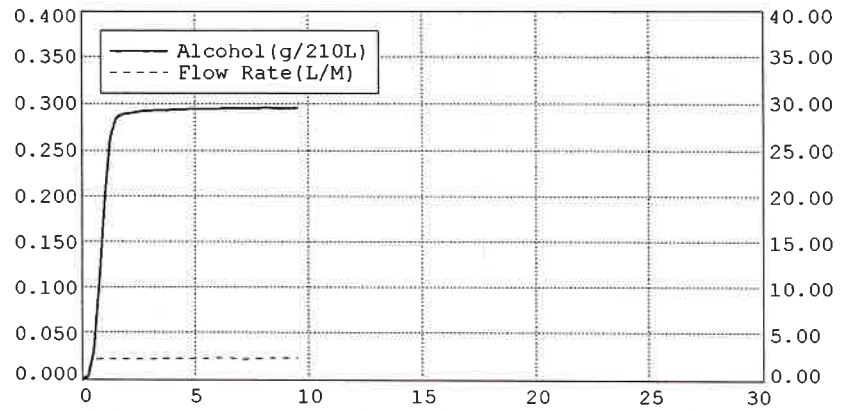

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100369

Date: 10/21/2024
Time: 11:39:34


SUBJECT NAME:
TEST TEST
LICENSE #: INCOMPLETE

OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 24-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.85: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:43
BLANK TEST 0.000 11:43
INTERNAL STANDARD VERIFIED 11:43
EXTERNAL STANDARD 0.079 11:43
BLANK TEST 0.000 11:44
SUBJECT SAMPLE INCOMPLETE 11:46

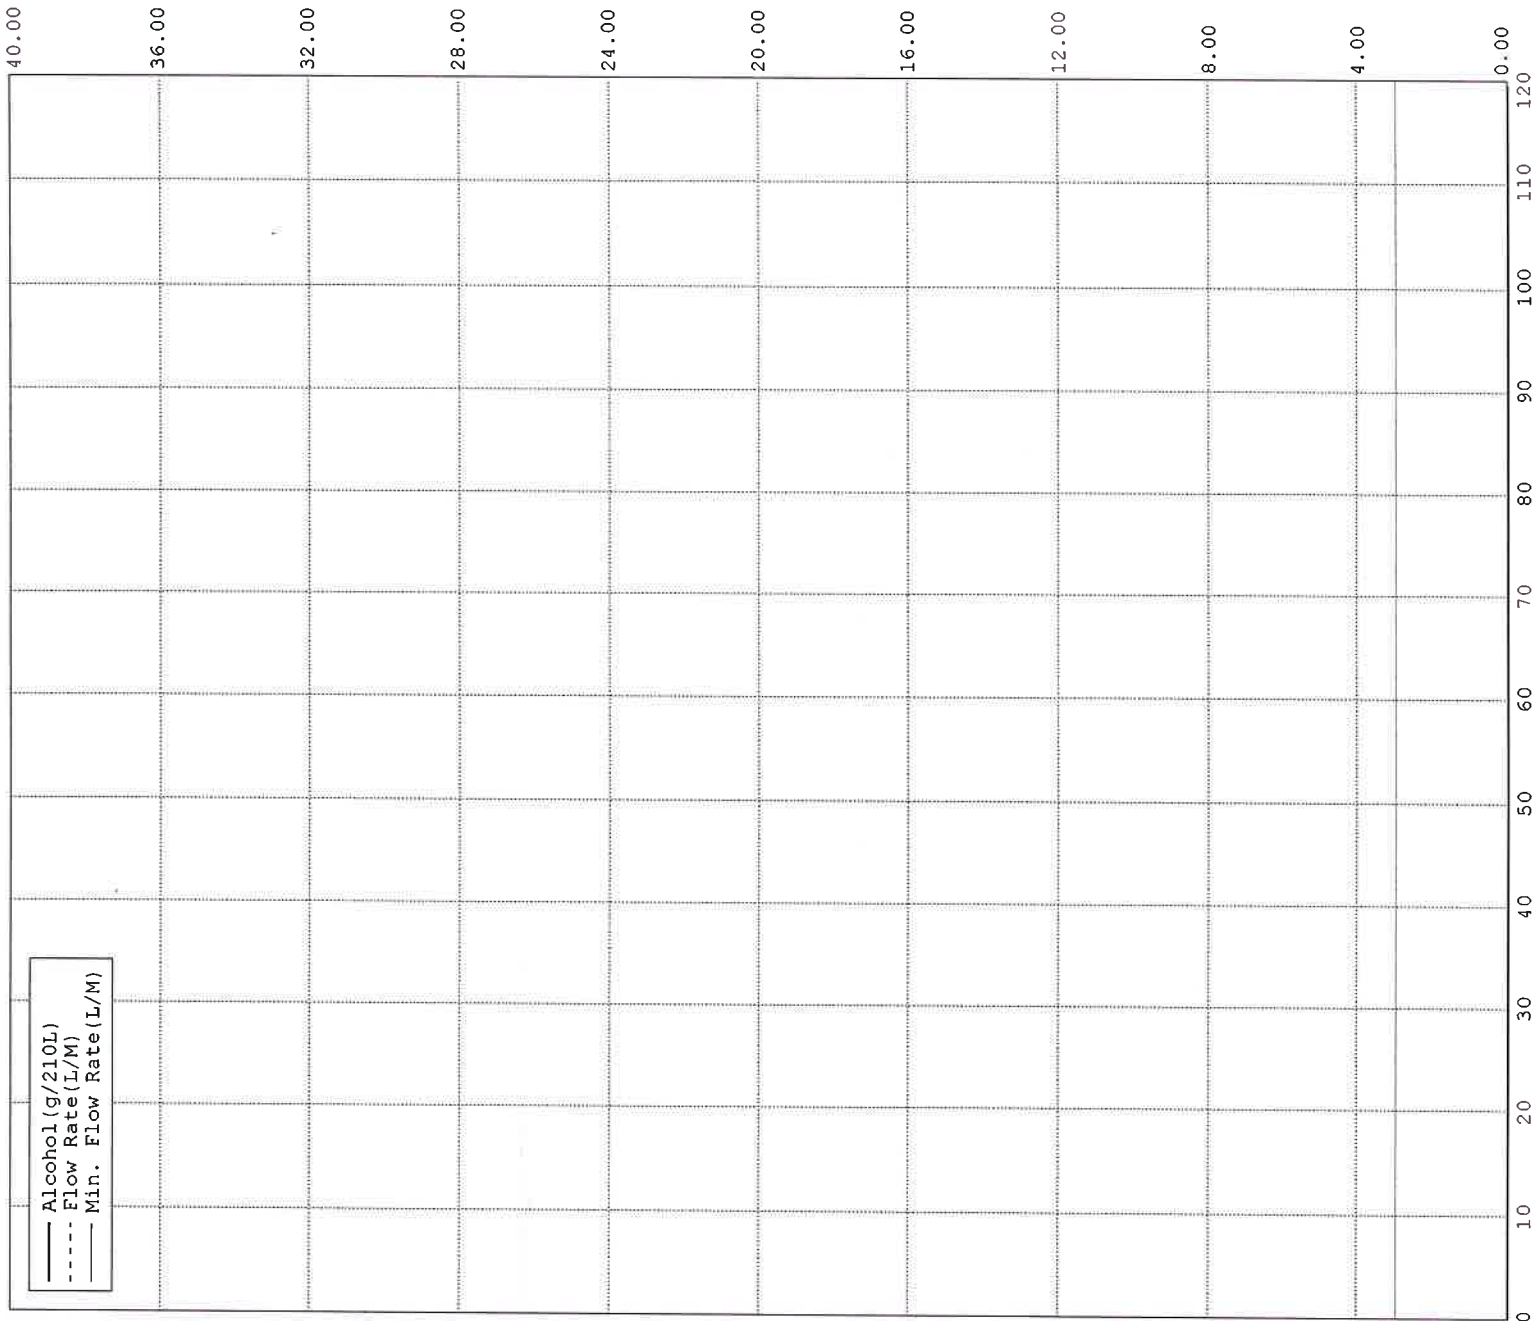

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100369

Date: 10/21/2024
Time: 11:49:07

SUBJECT NAME:
TEST TEST
LICENSE #: MAX ATTEMPTS


OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 24-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.85: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 11:50
BLANK TEST 0.000 11:50
INTERNAL STANDARD VERIFIED 11:50
EXTERNAL STANDARD 0.079 11:50
BLANK TEST 0.000 11:51
SUBJECT SAMPLE XXX 11:52

Maximum Attempts Exceeded

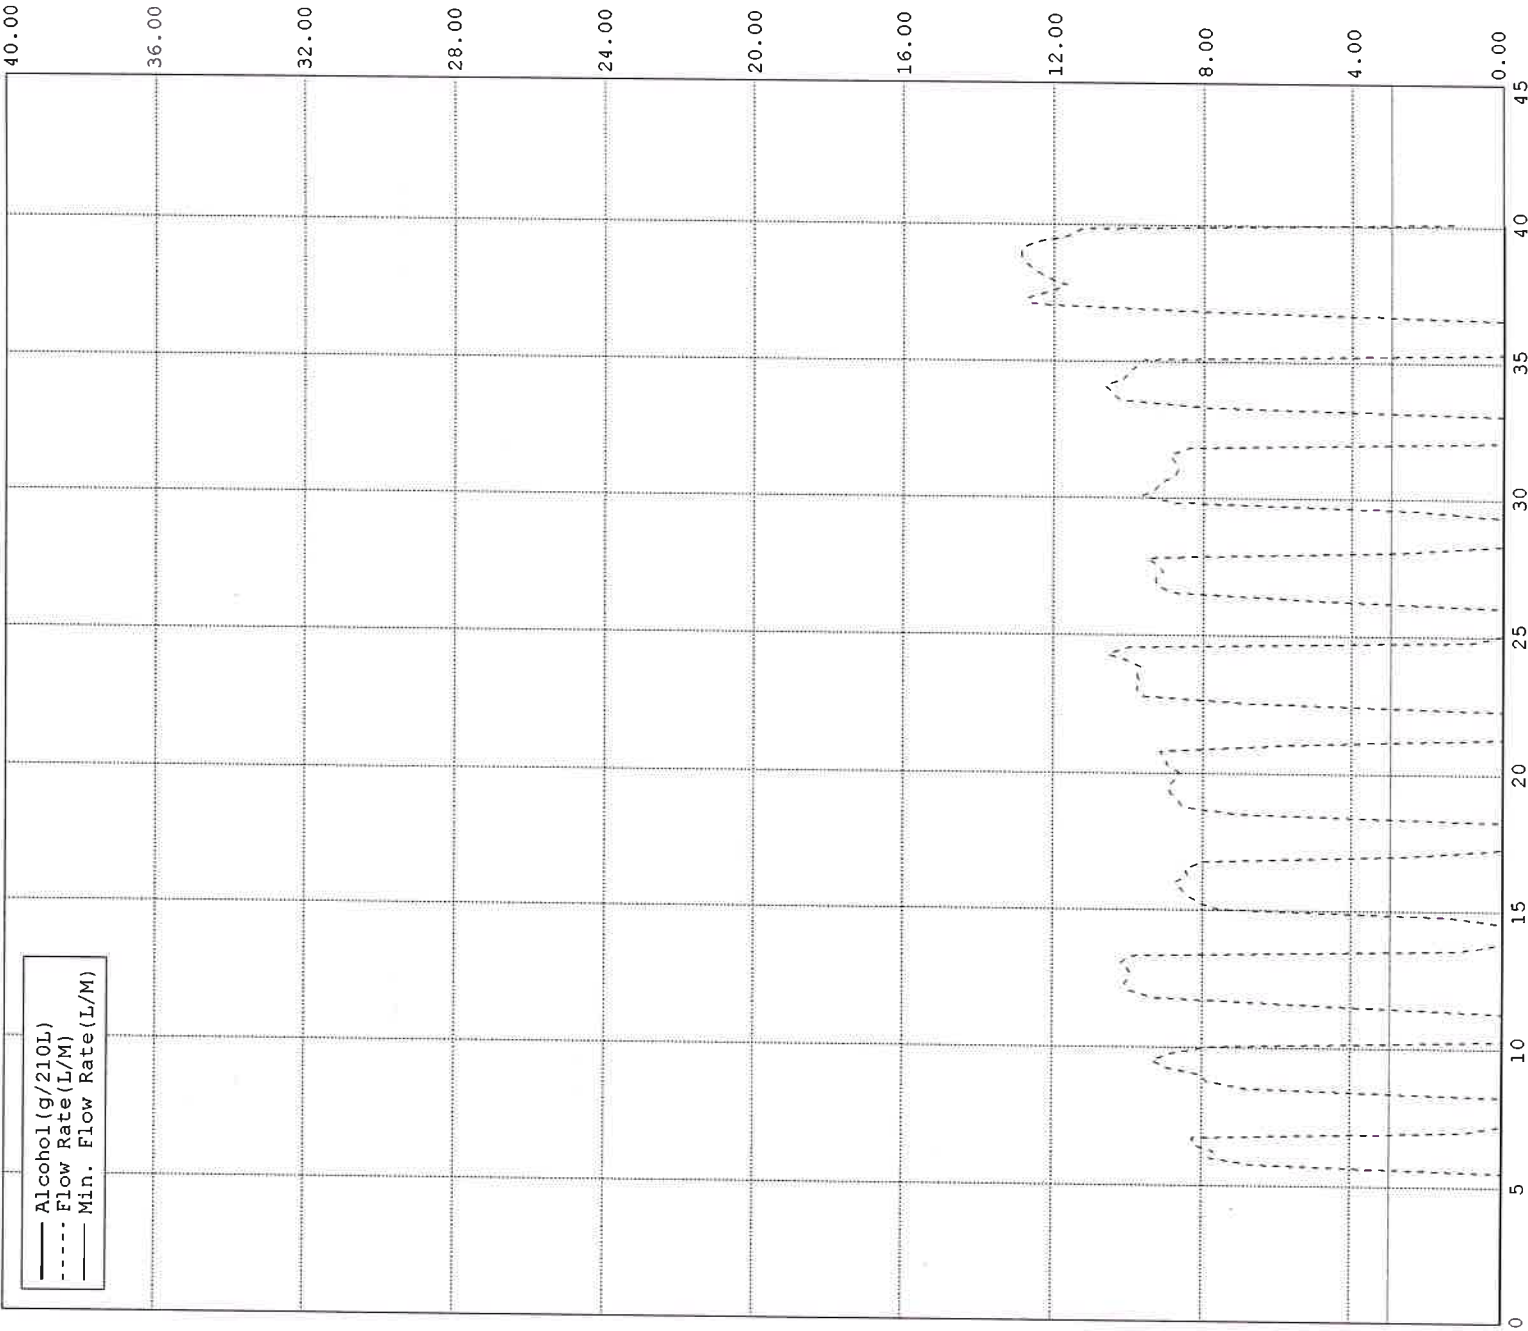

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100369

Date: 10/21/2024
Time: 11:53:57


SUBJECT NAME:
TEST TEST
LICENSE #: INVALID

OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 24-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.85: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:54
BLANK TEST	0.000	11:55
INTERNAL STANDARD	VERIFIED	11:55
EXTERNAL STANDARD	0.079	11:55
BLANK TEST	0.000	11:56
SUBJECT SAMPLE	INVALID	11:56

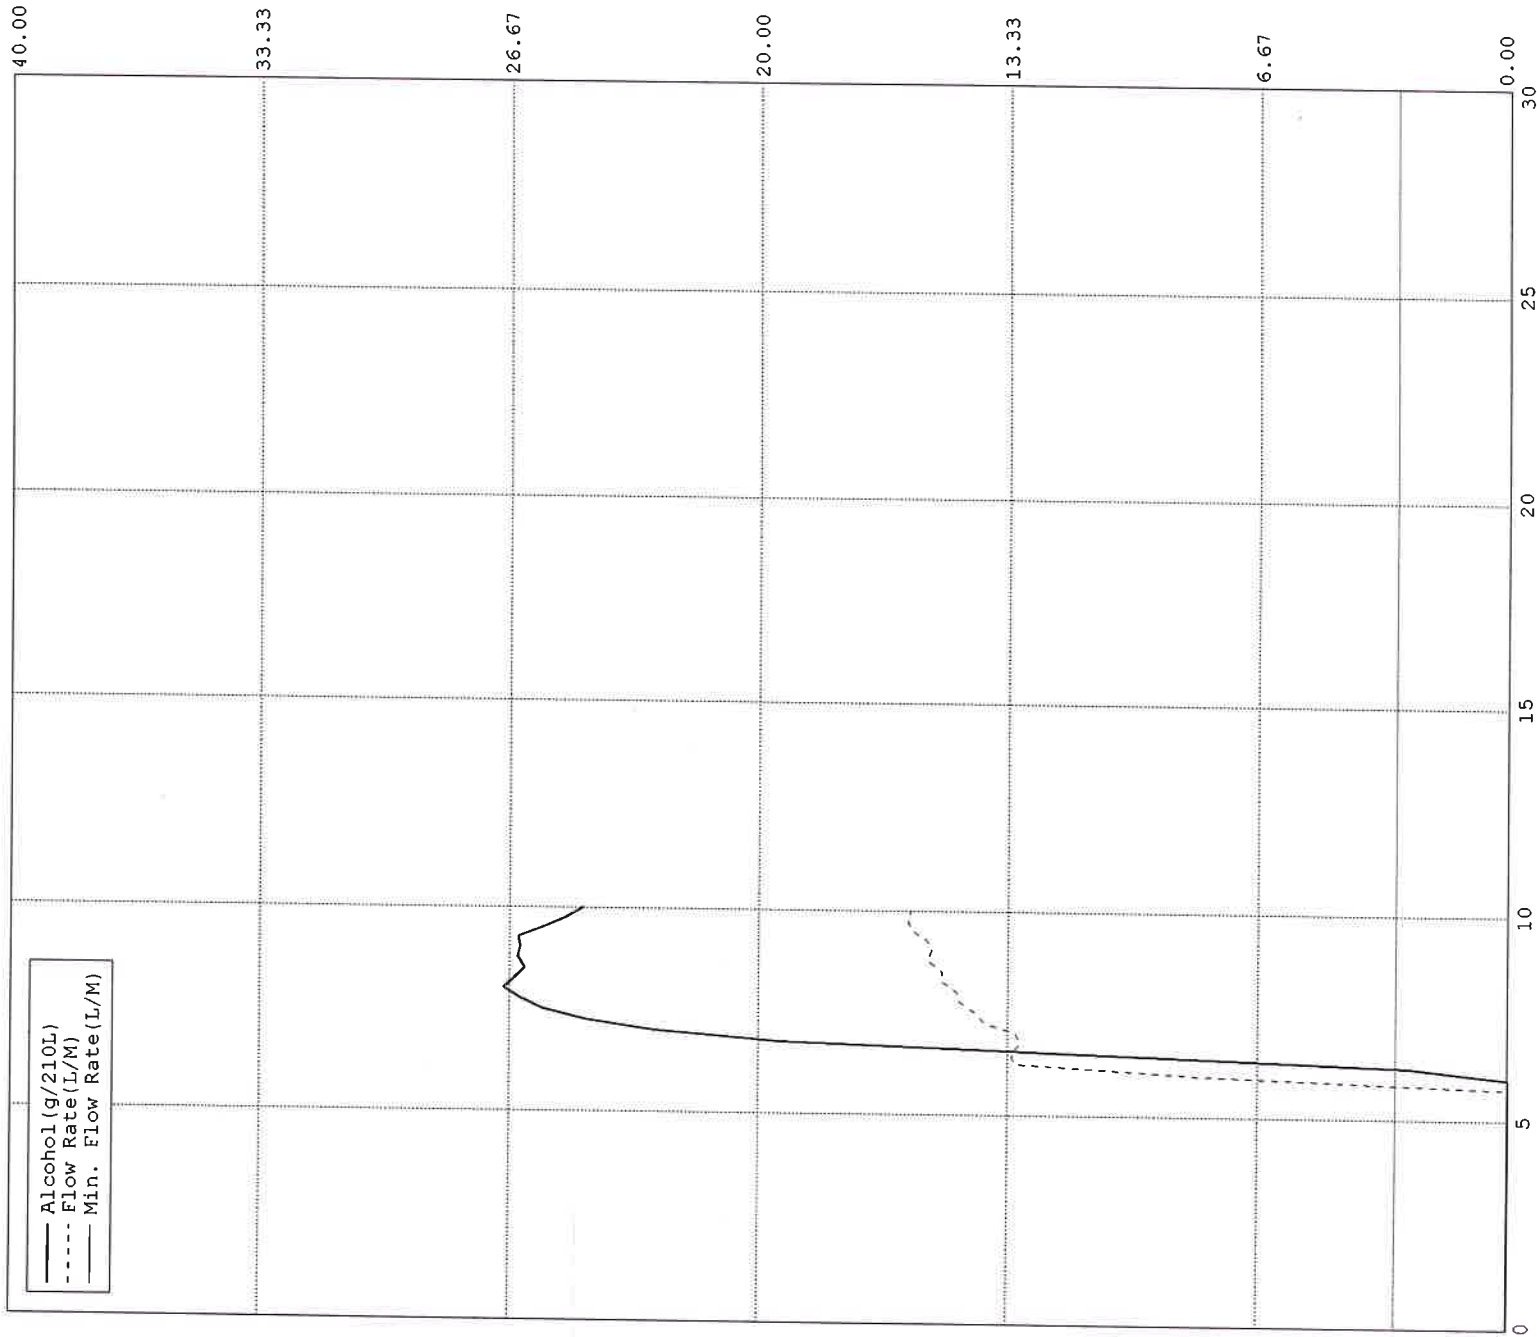

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100369

Date: 10/21/2024
Time: 11:58:45

SUBJECT NAME:
TEST TEST
LICENSE #: RFI


OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 24-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.84: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:59
BLANK TEST	0.000	12:00
INTERNAL STANDARD	VERIFIED	12:00
EXTERNAL STANDARD	0.079	12:00
BLANK TEST	0.000	12:01

RFI DETECTED

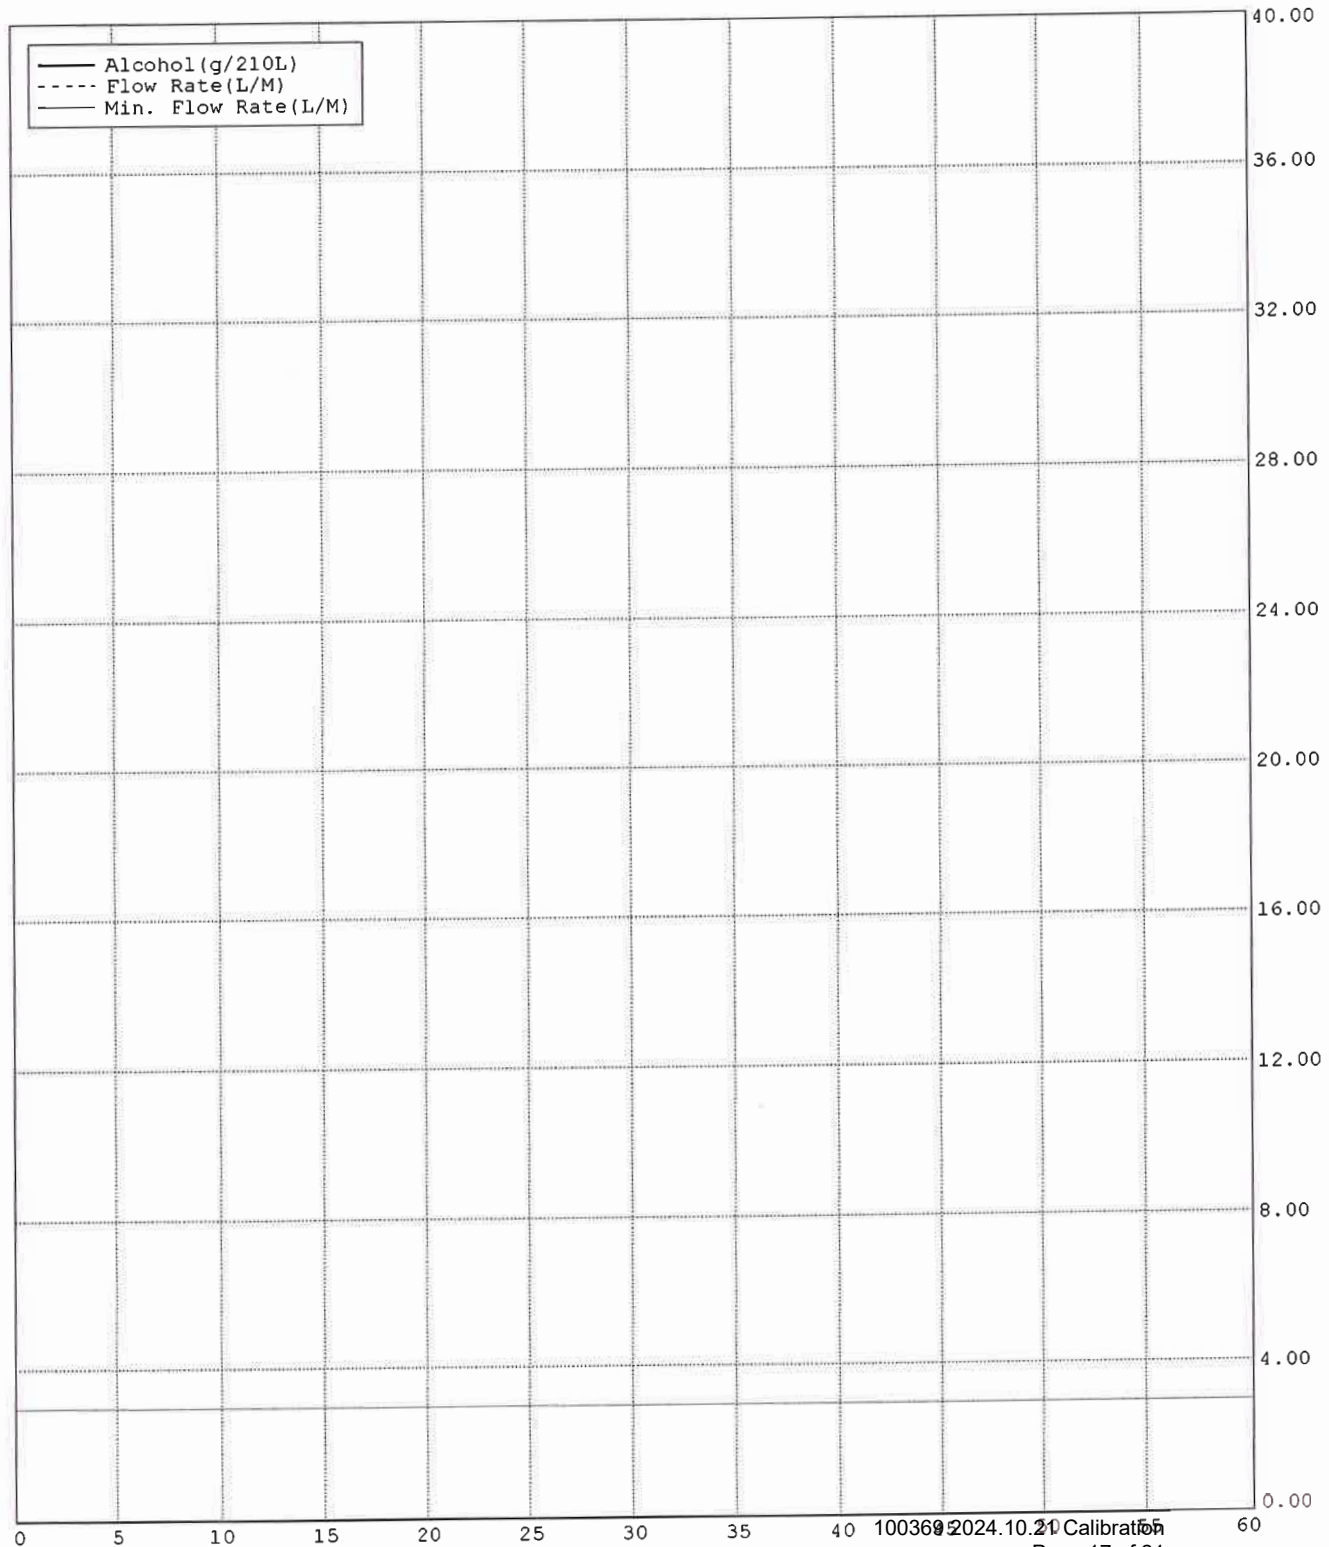

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100369

Date: 10/21/2024
Time: 12:10:14

SUBJECT NAME:
TEST TEST
LICENSE #: INT-ACETONE

OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 24-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.82: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:11
BLANK TEST	0.000	12:11
INTERNAL STANDARD	VERIFIED	12:11
Xq = 0.086 (2.29%)		
EXTERNAL STANDARD	0.079	12:11
X[1] = 0.0786 (0.0003) (0.0033)		
BLANK TEST	0.000	12:12
SUBJECT SAMPLE	XXX	12:13
X[1] = 0.1109 (-0.0159) (0.0031)		

Interference Detected

Filter 2 Avg = 0.0006

Filter 3 Avg = 0.0028

COB 2024.10.21



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100369

Date: 10/21/2024
Time: 12:14:54

SUBJECT NAME:
TEST TEST
LICENSE #: INT-IPA

OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237


DEPT/AGENCY:
AAA1
CASE/REPORT: 24-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.82: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:16
BLANK TEST	0.000	12:16
INTERNAL STANDARD	VERIFIED	12:16
Xq = 0.086 (2.50%)		
EXTERNAL STANDARD	0.079	12:16
X[1] = 0.0791 (0.0011) (0.0027)		
BLANK TEST	0.000	12:17
SUBJECT SAMPLE	XXX	12:17
X[1] = 0.1144 (-0.0292) (0.0020)		

Interference Detected

CB

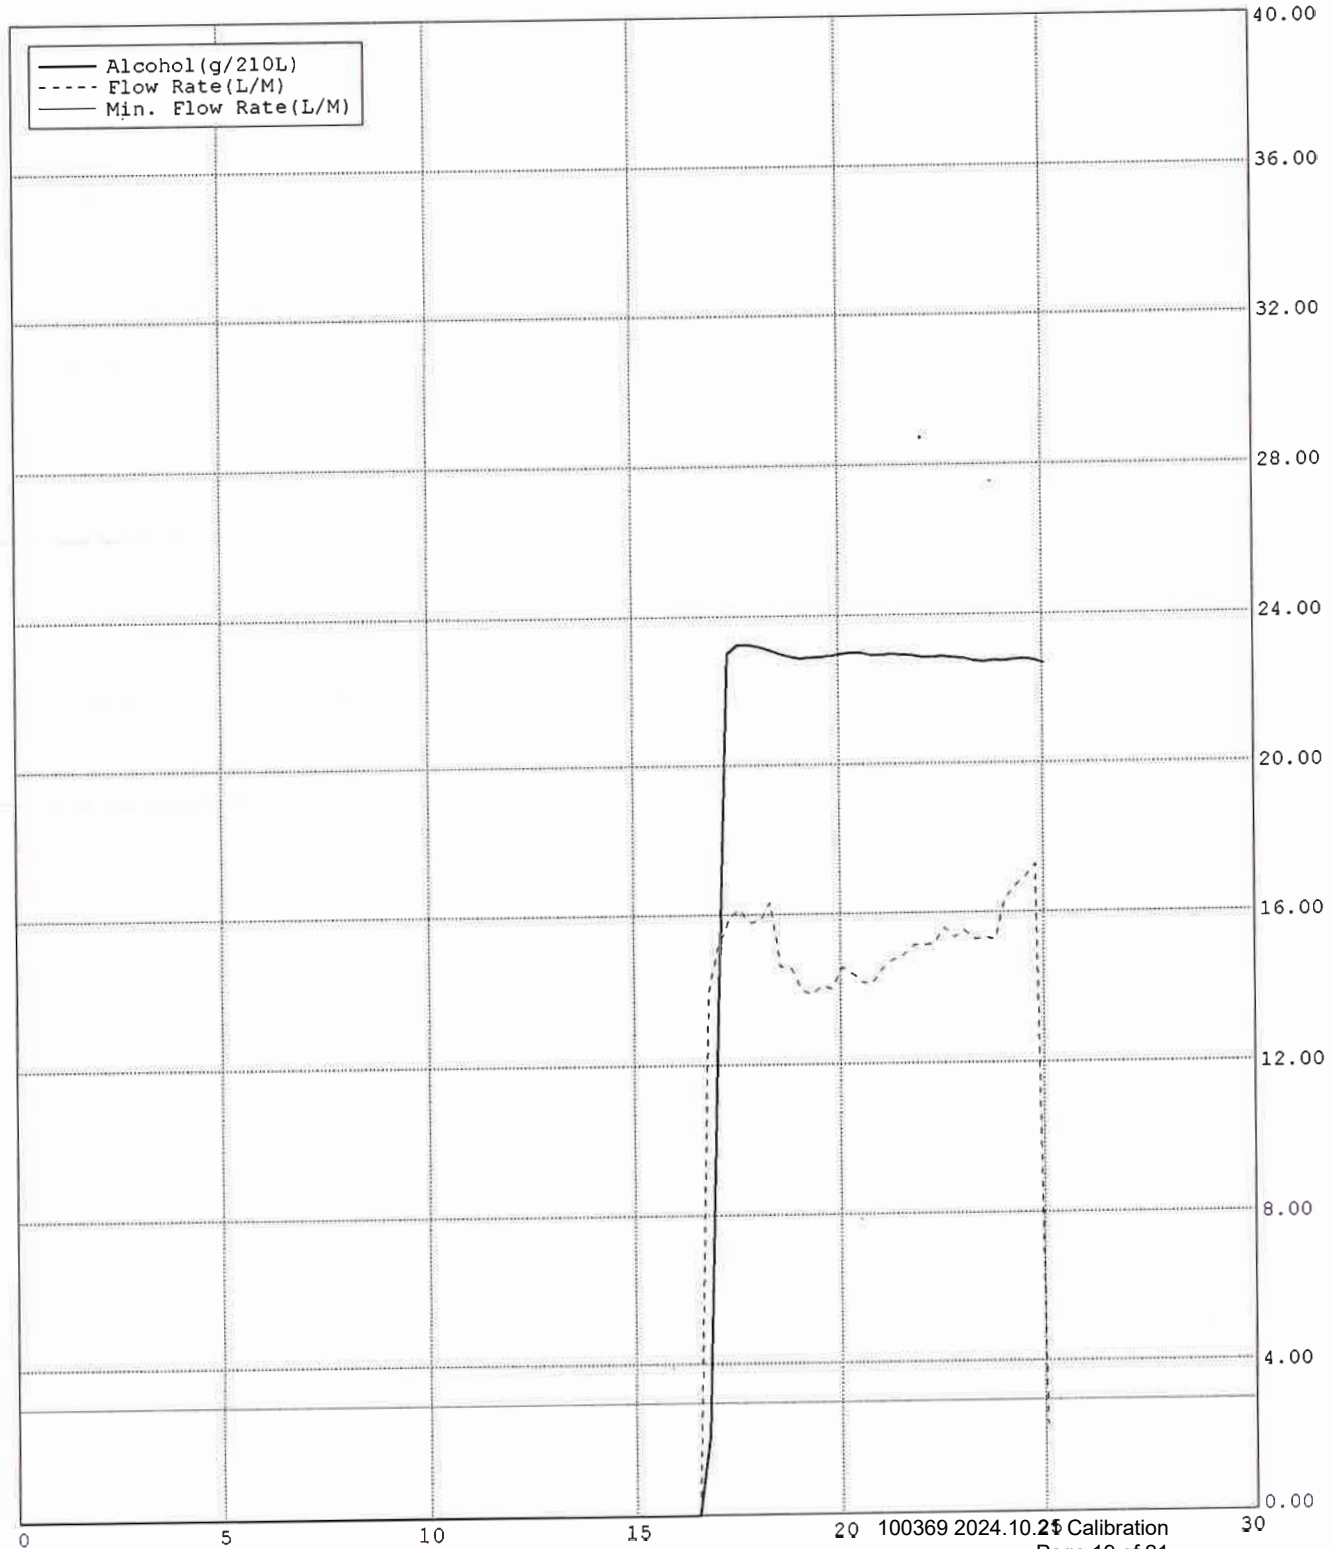

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100369

Date: 10/21/2024
Time: 12:19:35

SUBJECT NAME:
TEST TEST
LICENSE #: INT-NEGATIVE


OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 24-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.83: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:20
BLANK TEST	0.000	12:20
INTERNAL STANDARD	VERIFIED	12:20
Xq = 0.085 (2.08%)		
EXTERNAL STANDARD	0.079	12:21
X[1] = 0.0786 (0.0003) (0.0030)		
BLANK TEST	0.000	12:21
SUBJECT SAMPLE (Vol=1.99L)	0.093	12:22
X[1] = 0.0937 (0.0000) (0.0016)		
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.079	12:23
X[1] = 0.0787 (0.0005) (0.0023)		
BLANK TEST	0.000	12:24

CS

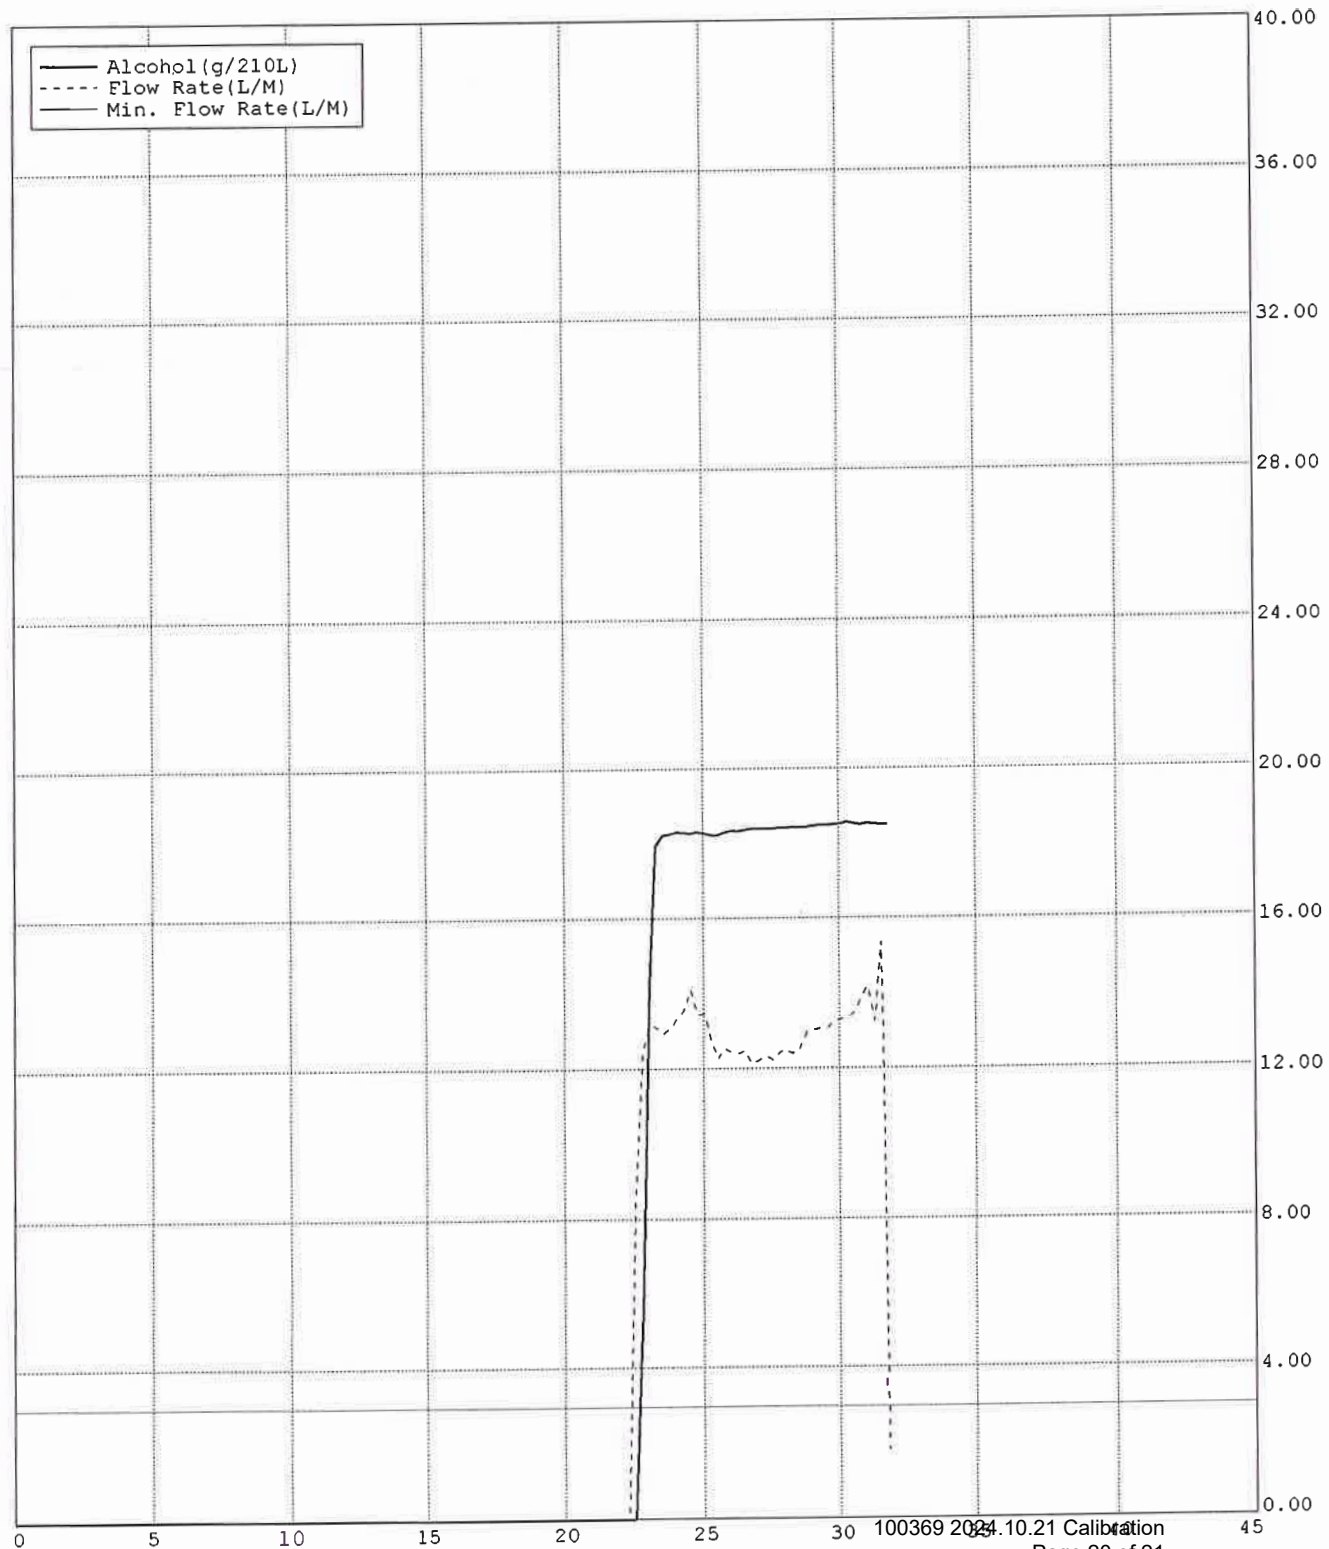

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100369

Date: 10/21/2024
Time: 12:50:50

SUBJECT NAME:
TEST TEST
LICENSE #: NONDRINKING

OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 24-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.81: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:51
BLANK TEST	0.000	12:51
INTERNAL STANDARD	VERIFIED	12:52
EXTERNAL STANDARD	0.079	12:52
BLANK TEST	0.000	12:53
SUBJECT SAMPLE (Vol=2.18L)	0.000	12:53
BLANK TEST	0.000	12:54
EXTERNAL STANDARD	0.079	12:55
BLANK TEST	0.000	12:55

OR

