

State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100381

Report Issue Date: 12/22/2025
Date Received: 2025-06-23
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.019	0.020	0.020	0.019	0.020	0.020
0.080	0.079	AG335202	0.077	0.076	0.077	0.077	0.077	0.077
0.300	0.297	AG427706	0.287	0.287	0.287	0.287	0.287	0.287

As Found - Evaluation Analyst: Colleen O'Bryant

As Found Conditions - Barometric Pressure (inHg): 29.64 Barometer Used: VWR S/N 240680771 Temperature (C): 21.9 Relative Humidity (%): 42

As-Found Lab Activity Date Range: 06/23/2025 - 06/24/2025

Unable to recreate drift during as found dry gas or non-drinking subject testing. Linearity slope - 0.965. Recommending repair to update controller board and continue trouble shooting.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.039	0.039	0.039	0.039	0.040	0.039	+/- 0.003
0.080	0.078	AG335202	0.078	0.078	0.078	0.078	0.078	0.078	+/- 0.004
0.100	0.098	AG516101	0.098	0.097	0.097	0.096	0.097	0.097	+/- 0.004
0.150	0.147	AG515604	0.146	0.146	0.145	0.145	0.145	0.145	+/- 0.006
0.300	0.294	AG427706	0.291	0.291	0.291	0.292	0.292	0.291	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.27 Barometer Used: VWR S/N 240680771 Temperature (C): 21.5 Relative Humidity (%): 4

As-Left Lab Activity Date Range: 12/08/2025 - 12/08/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Carlie Glaister on 12/19/2025

carlie.glaister@alaska.gov

Technically and administratively reviewed by Kaija Swisher on 12/22/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100381 Analyst or Technician Name: Carlie Glaister

DataMaster DMT Calibration Start Date: 12/8/25

Diagnostic Test

☒ Perform Diagnostic Test (View Details)

☒ Internal Standard Value $\leq$ 3.00%

Technician Screen and Calibration Factors

☒ Adjust Voltages (if needed)

- Lamp (2.60 V Maximum)
- Bias
- Cooler (2.00 V Maximum)
- Chopper Frequency
- Detector Voltage (-0.100V to 0.100V)

☒ Set RFI Sensitivity

☒ Adjust internal barometer reading to match NIST-traceable barometer

Barometer/Thermometer/Hygrometer S/N: 240680771

Calibration Due Date: 9/10/26

☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed

☒ Print Technician Screen

☒ Print "Cal Factors"

Minimum Volume Test

☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.27 Temperature(C) 21.5 Relative Humidity(%) 4

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

☒ Incomplete

☒ Maximum Attempts Exceeded

☒ Invalid

☒ Radio Frequency Interference (RFI)

☒ Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20250922KS Expiration Date: 12/22/25

Simulator S/N: DR4178 Thermometer Verification Performed? ☒

2. Isopropanol Reagent Lot Number: 20250922KS Expiration Date: 12/22/25

Simulator S/N: DR4177 Thermometer Verification Performed? ☒

3. Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 3/19/27 -> sln.

Simulator S/N: DR4163 Thermometer Verification Performed? ☒ 12/22/25 -> prep.

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 3/14/27

Administrative

☒ Verify Stylus Calibration

☒ Perform Non-Drinking Subject Test

☒ Reset Options

☒ Upload Instrument

☒ Clear Memory

☒ Remove Dry Gas Tank Before Shutdown

☒ Verification of Calibration (VOC)

☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: CMU-12/8/25

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): 12/8/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100381

Date: 12/08/2025
Time: 11:35:59

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C (44.0°C - 52.0°C)	PASSED
Breath Tube = 48.1°C (38.0°C - 50.0°C)	PASSED

SETTINGS

Lamp Voltage = 1.73 V (1.04 V - 2.42 V)	PASSED
Cooler Voltage = 1.63 V (0.98 V - 2.28 V)	PASSED
Bias Voltage = 80 V (48 V - 112 V)	PASSED
Chopper Freq = 526 Hz (475 Hz - 575 Hz)	PASSED
Barometer = 29.3 in	

PUMP INFO

Flow Rate = 4.673 L/M (3.500 L/M - 6.500 L/M)	PASSED
--	--------

DETECTOR INFO

PUMP ON (0.002 V <= 0.010 V)	PASSED
PUMP OFF (0.003 V <= 0.010 V)	PASSED

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
Xq = 0.092 0.19% (0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100381

Date: 12/08/2025

Time: 11:45 AM

Temperatures (°C)

Sample Cell: 48.8°C

Breath Tube: 47.9°C

Current Barometer 29.3 in

Volume (Ltr) 1.51

Settings

Lamp: 1.73 V

Bias: 80 V

Cooler: 1.63 V

Chopper: 526 Hz

Voltages (V)

Flow: 1.09 V

Detector: -0.078 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100381

Date: 12/08/2025
Time: 10:56:13

OPERATOR NAME:
CARLIE GLAISTER
CERTIFICATE #: 10436

Ca	=	0.1000		
CAL	=	0.983936	0.800	<= CAL < 1.200
b1	=	0.0003	0.0000	<= b1 < 0.0040
b2	=	0.0043	0.0010	<= b2 < 0.0100
b3	=	0.0002	0.0000	<= b3 < 0.0040
Xq	=	0.0922	0.0500	<= Xq < 0.2000
a21	=	1.102569	1.050	<= a21 < 1.300
a31	=	0.421738	0.300	<= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100381

Date: 12/08/2025

Time: 11:46:45

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.26: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:50
BLANK TEST	0.000	11:50
INTERNAL STANDARD	VERIFIED	11:50
EXTERNAL STANDARD	0.079	11:50
BLANK TEST	0.000	11:51
SUBJECT SAMPLE (Vol=1.53L)	0.000	11:52
BLANK TEST	0.000	11:53
EXTERNAL STANDARD	0.078	11:53
BLANK TEST	0.000	11:54

OK

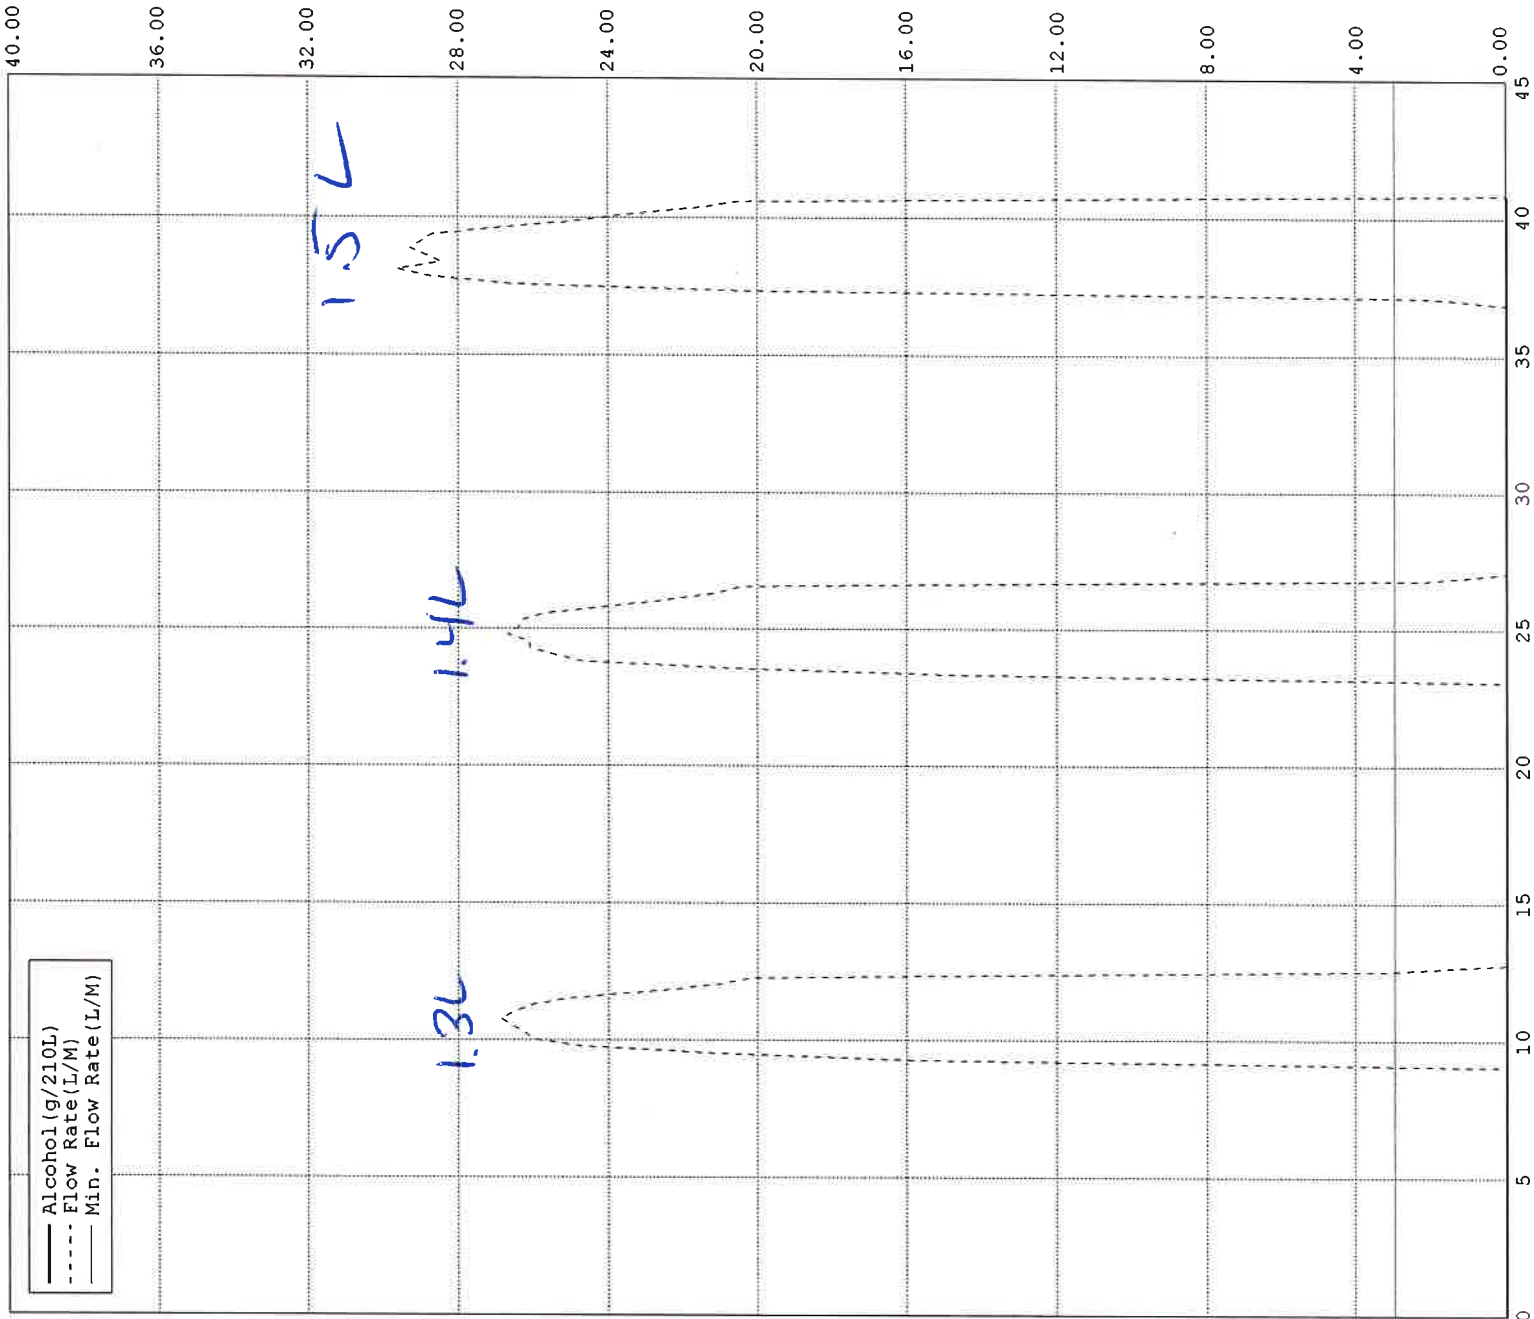

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100381

Date: 12/08/2025
 Time: 12:00:43

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.039	0.0392	0.0004
0.078	0.0780	0.0000
0.098	0.0970	0.0007
0.147	0.1454	0.0005
0.294	0.2914	0.0005

SLOPE = 0.989362
 R² = 0.999988

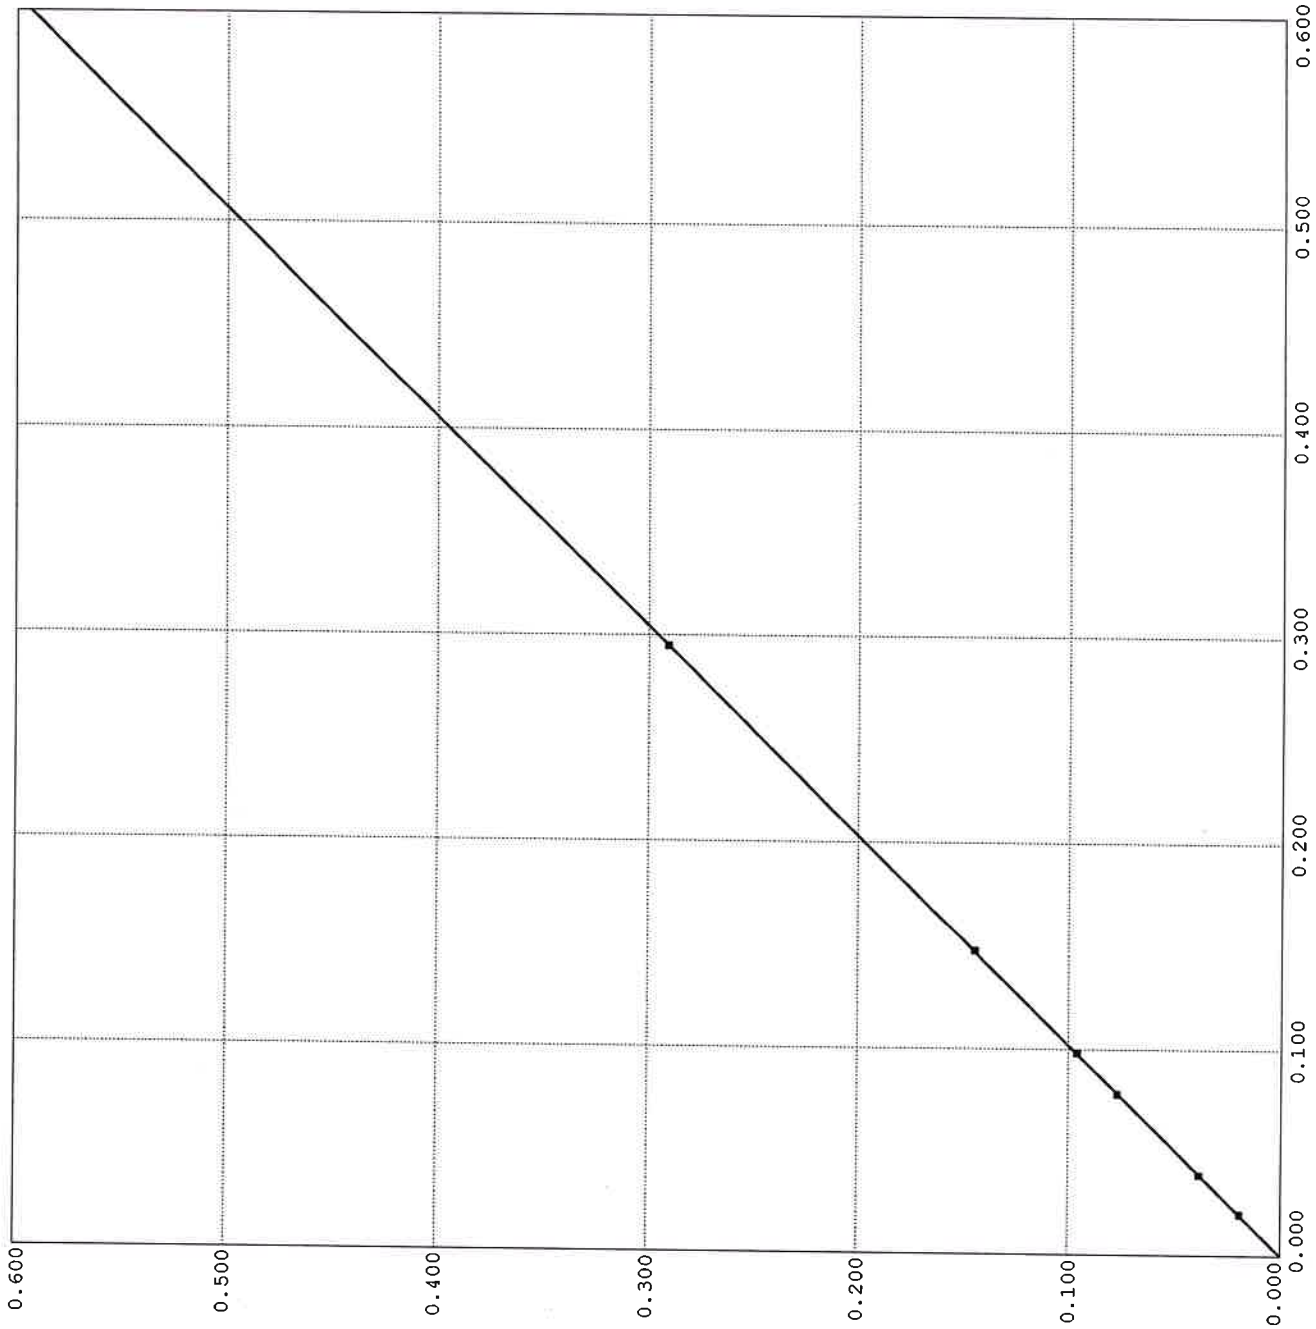

CLG

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100381






Date: 12/08/2025
Time: 12:00:46

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.28: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 798 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	12:01
INTERNAL STANDARD	VERIFIED	12:02
EXTERNAL STANDARD	0.020	12:02
BLANK TEST	0.000	12:03
EXTERNAL STANDARD	0.020	12:03
BLANK TEST	0.000	12:04
EXTERNAL STANDARD	0.020	12:04
BLANK TEST	0.000	12:05
EXTERNAL STANDARD	0.020	12:05
BLANK TEST	0.000	12:06
EXTERNAL STANDARD	0.020	12:06
BLANK TEST	0.000	12:07

Average = 0.0200
Std Dev = 0.0000

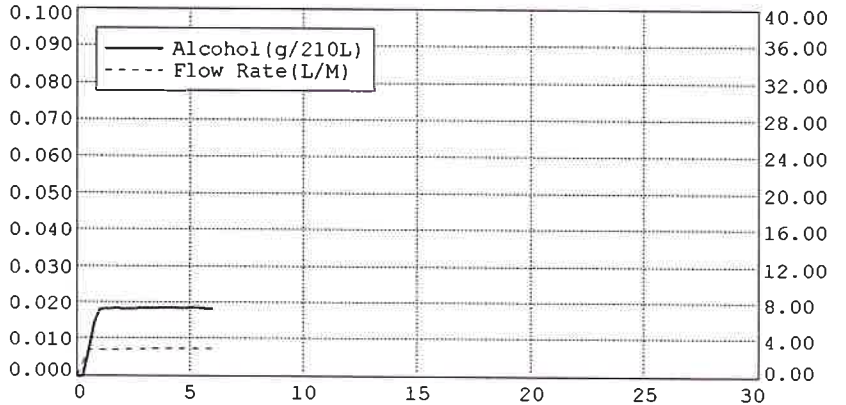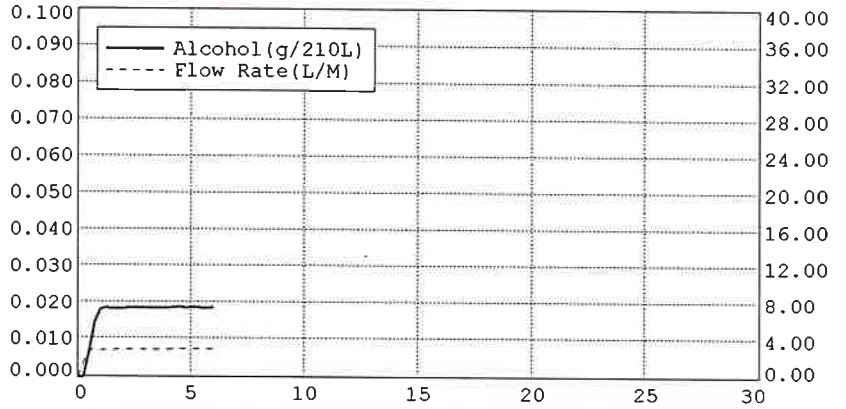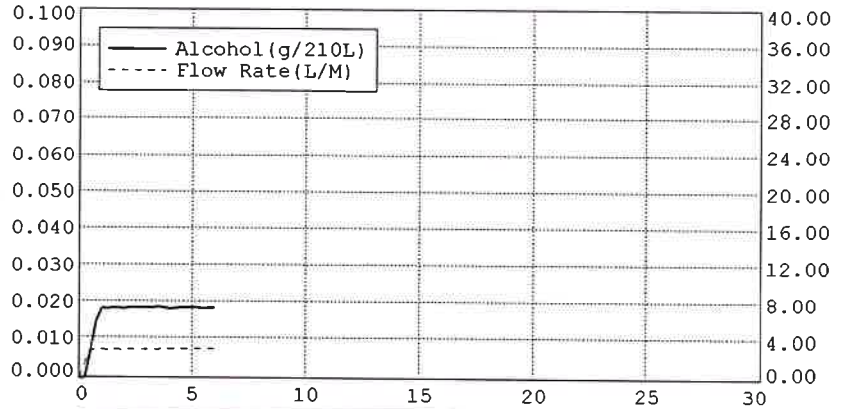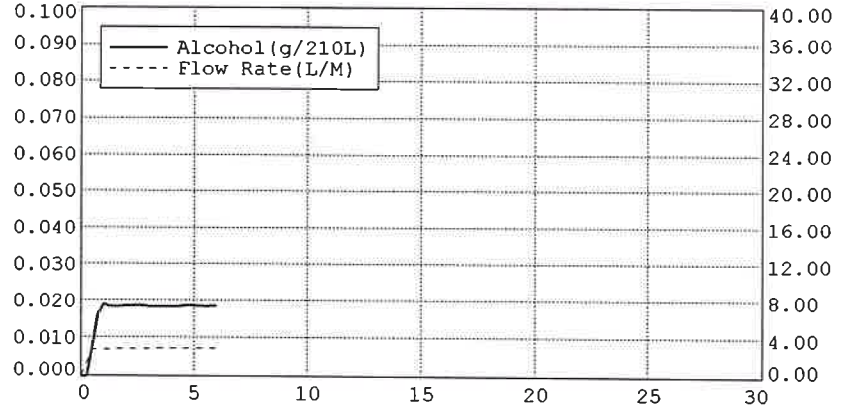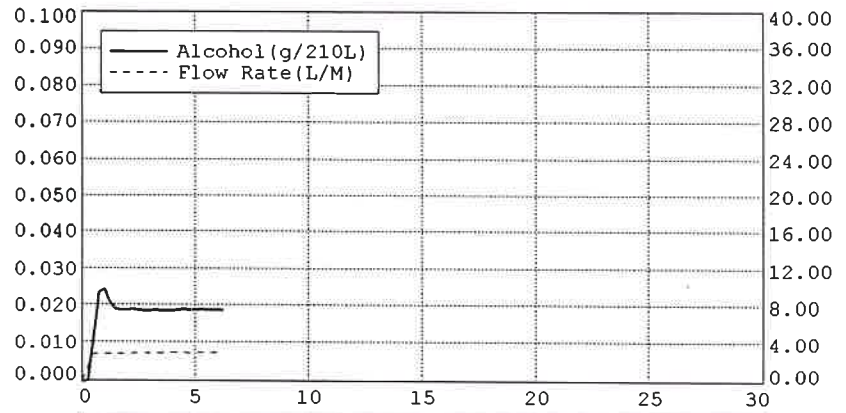

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100381

Date: 12/08/2025

Time: 12:10:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040

TARGET AT 29.28: 0.039

LOT #: AG407908






EXPIRATION: 03/19/2026

TANK PRESSURE: 715 psi

BLANK TEST	0.000	12:12
INTERNAL STANDARD	VERIFIED	12:12
EXTERNAL STANDARD	0.039	12:12
BLANK TEST	0.000	12:13
EXTERNAL STANDARD	0.039	12:13
BLANK TEST	0.000	12:14
EXTERNAL STANDARD	0.039	12:14
BLANK TEST	0.000	12:15
EXTERNAL STANDARD	0.039	12:15
BLANK TEST	0.000	12:16
EXTERNAL STANDARD	0.040	12:16
BLANK TEST	0.000	12:17

Average = 0.0392

Std Dev = 0.0004

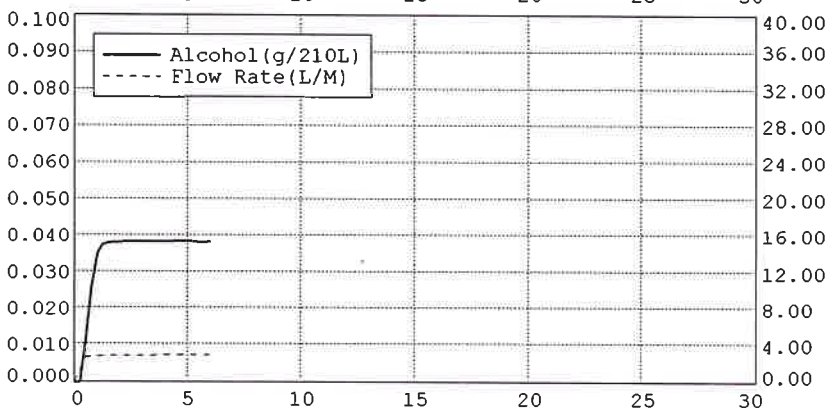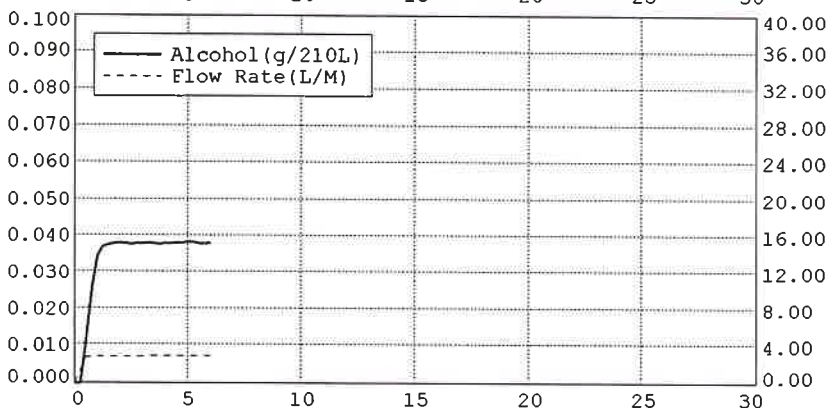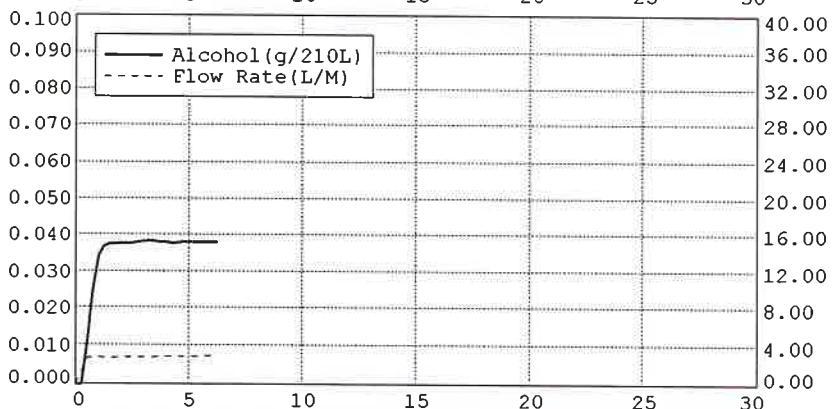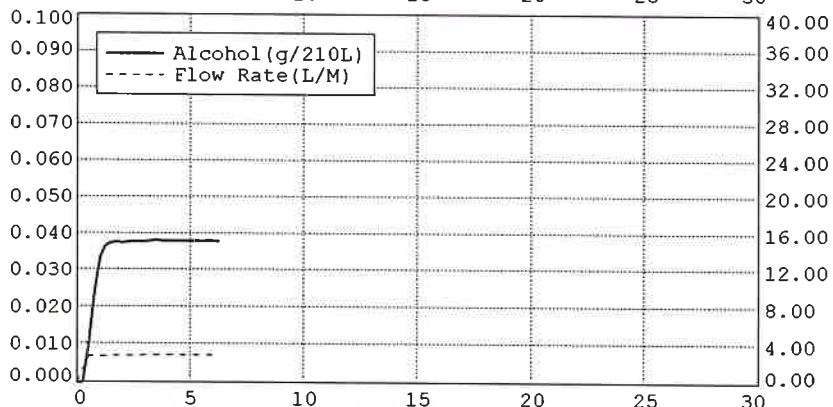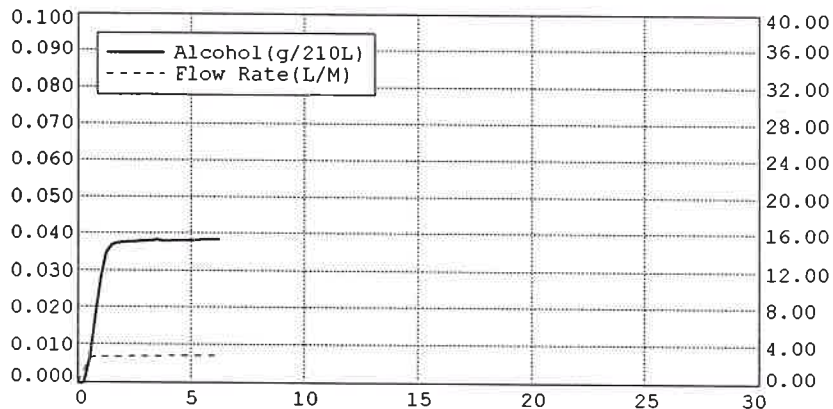

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100381






Date: 12/08/2025
Time: 12:18:30

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.28: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 237 psi

BLANK TEST	0.000	12:19
INTERNAL STANDARD	VERIFIED	12:19
EXTERNAL STANDARD	0.078	12:19
BLANK TEST	0.000	12:20
EXTERNAL STANDARD	0.078	12:21
BLANK TEST	0.000	12:21
EXTERNAL STANDARD	0.078	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.078	12:23
BLANK TEST	0.000	12:24
EXTERNAL STANDARD	0.078	12:24
BLANK TEST	0.000	12:25

Average = 0.0780
Std Dev = 0.0000

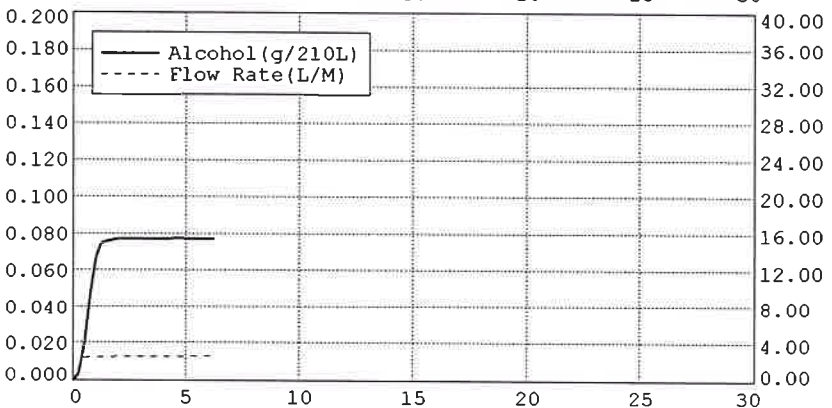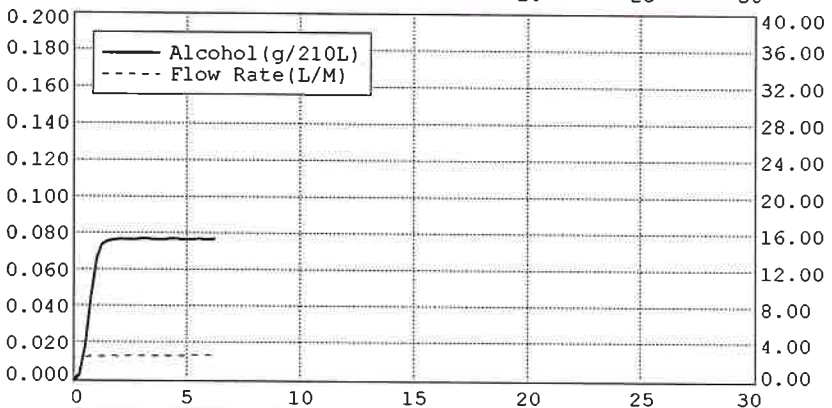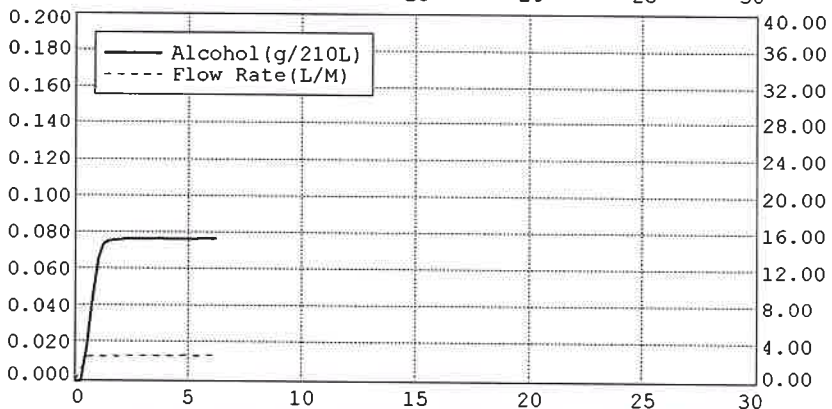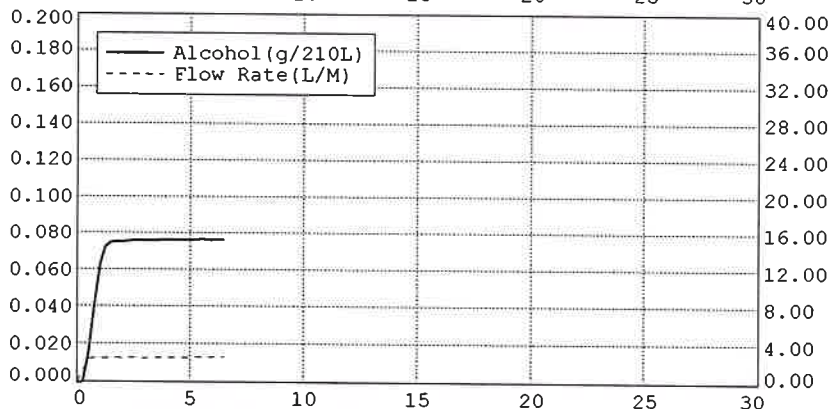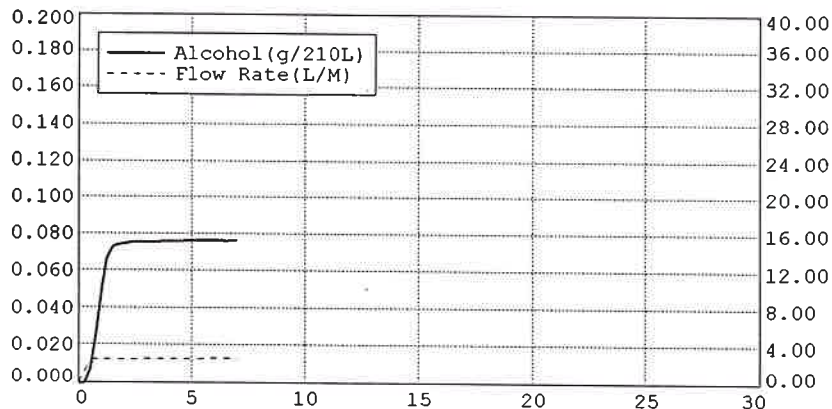

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100381

Date: 12/08/2025

Time: 12:26:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100

TARGET AT 29.28: 0.098

LOT #: AG516101






EXPIRATION: 06/10/2027

TANK PRESSURE: 1212 psi

BLANK TEST	0.000	12:27
INTERNAL STANDARD	VERIFIED	12:27
EXTERNAL STANDARD	0.098	12:27
BLANK TEST	0.000	12:28
EXTERNAL STANDARD	0.097	12:28
BLANK TEST	0.000	12:29
EXTERNAL STANDARD	0.097	12:29
BLANK TEST	0.000	12:30
EXTERNAL STANDARD	0.096	12:30
BLANK TEST	0.000	12:31
EXTERNAL STANDARD	0.097	12:32
BLANK TEST	0.000	12:32

Average = 0.0970

Std Dev = 0.0007

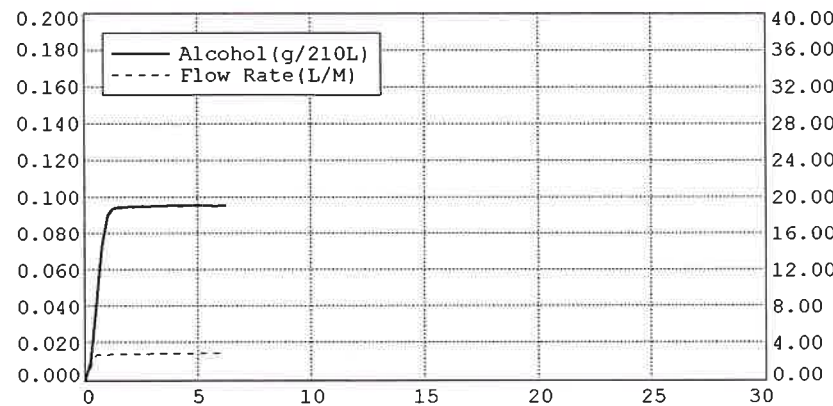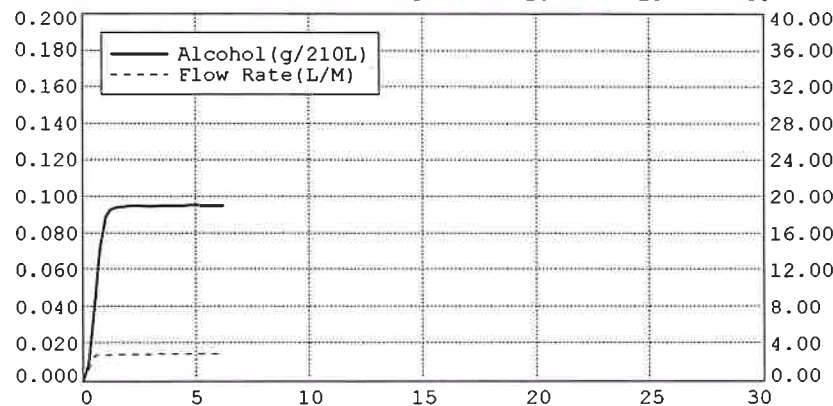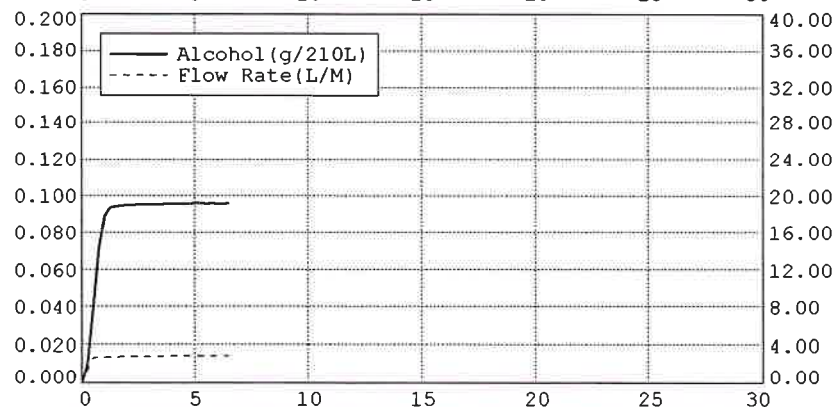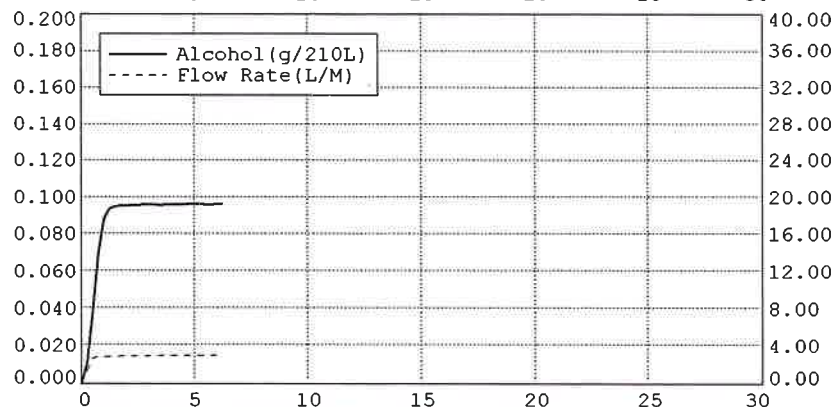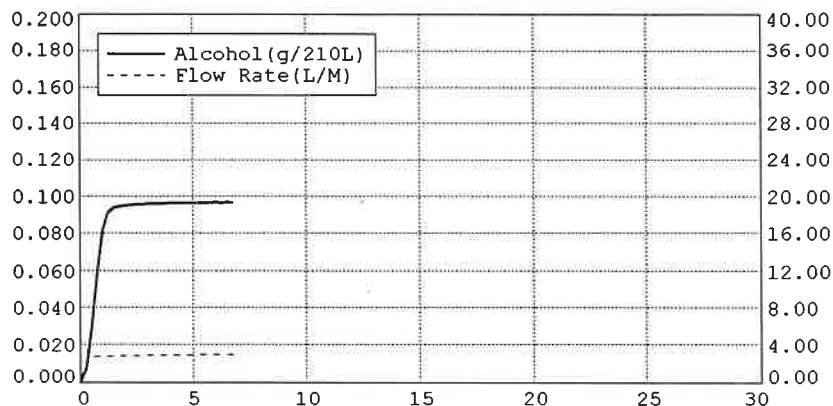

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100381






Date: 12/08/2025
Time: 12:33:22

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.28: 0.147
LOT #: AG515604
EXPIRATION: 06/05/2027
TANK PRESSURE: 721 psi

BLANK TEST	0.000	12:34
INTERNAL STANDARD	VERIFIED	12:34
EXTERNAL STANDARD	0.146	12:34
BLANK TEST	0.000	12:35
EXTERNAL STANDARD	0.146	12:36
BLANK TEST	0.000	12:36
EXTERNAL STANDARD	0.145	12:37
BLANK TEST	0.000	12:38
EXTERNAL STANDARD	0.145	12:38
BLANK TEST	0.000	12:39
EXTERNAL STANDARD	0.145	12:39
BLANK TEST	0.000	12:40

Average = 0.1454
Std Dev = 0.0005

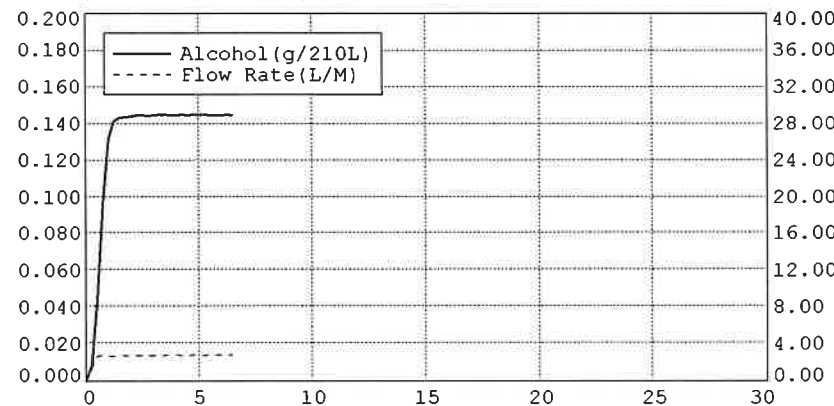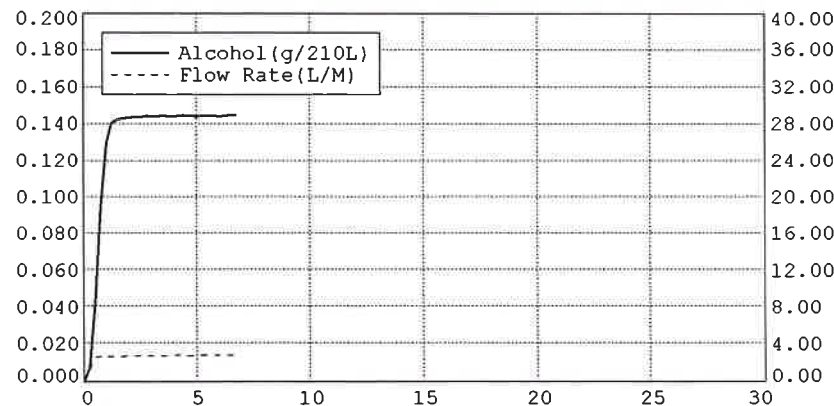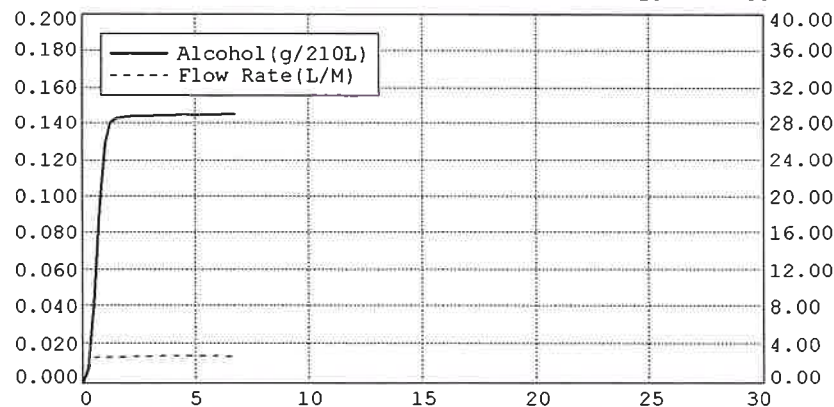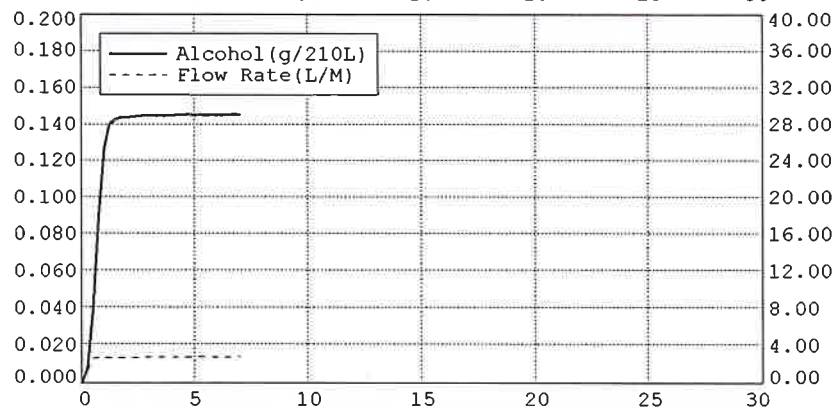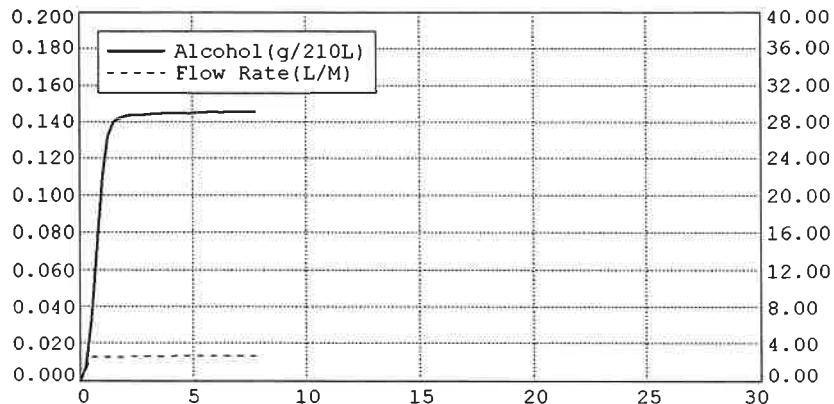

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100381

Date: 12/08/2025

Time: 12:43:03

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300

TARGET AT 29.28: 0.294

LOT #: AG427706






EXPIRATION: 10/03/2026


TANK PRESSURE: 222 psi

BLANK TEST	0.000	12:44
INTERNAL STANDARD	VERIFIED	12:44
EXTERNAL STANDARD	0.291	12:44
BLANK TEST	0.000	12:45
EXTERNAL STANDARD	0.291	12:45
BLANK TEST	0.000	12:46
EXTERNAL STANDARD	0.291	12:46
BLANK TEST	0.000	12:47
EXTERNAL STANDARD	0.292	12:48
BLANK TEST	0.000	12:49
EXTERNAL STANDARD	0.292	12:49
BLANK TEST	0.000	12:50

Average = 0.2914

Std Dev = 0.0005

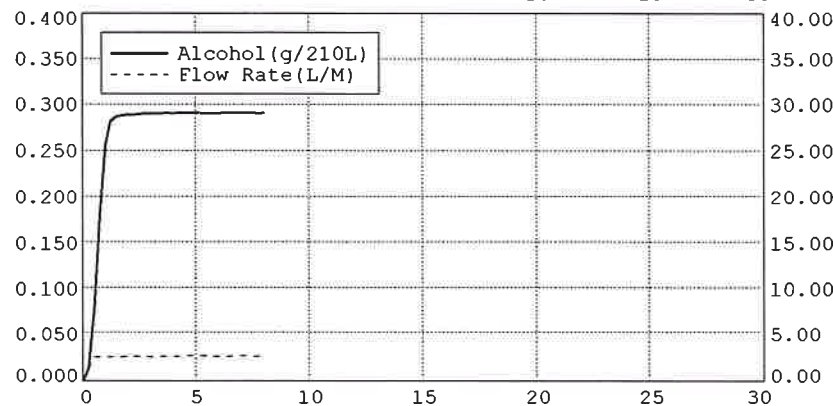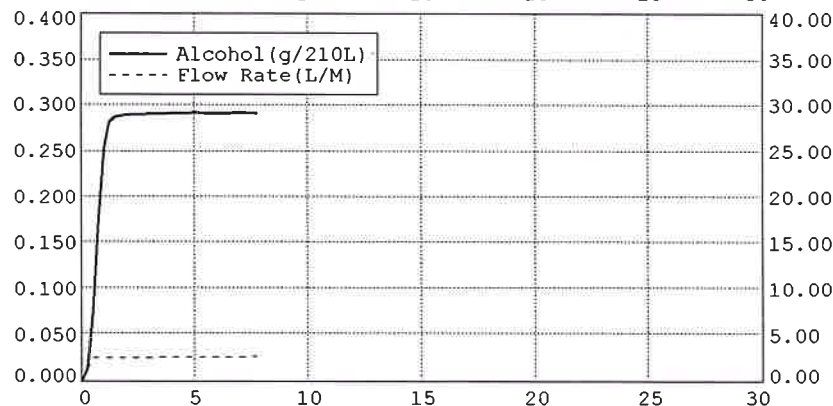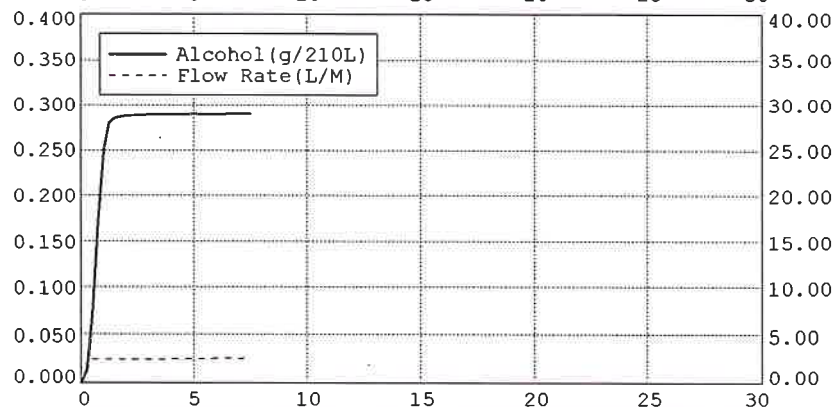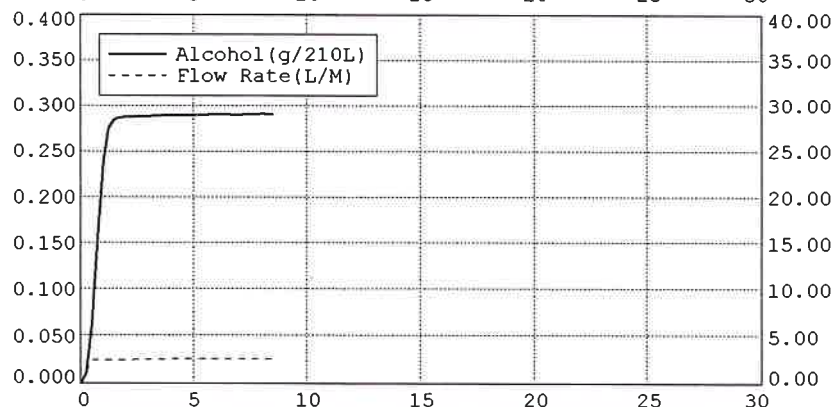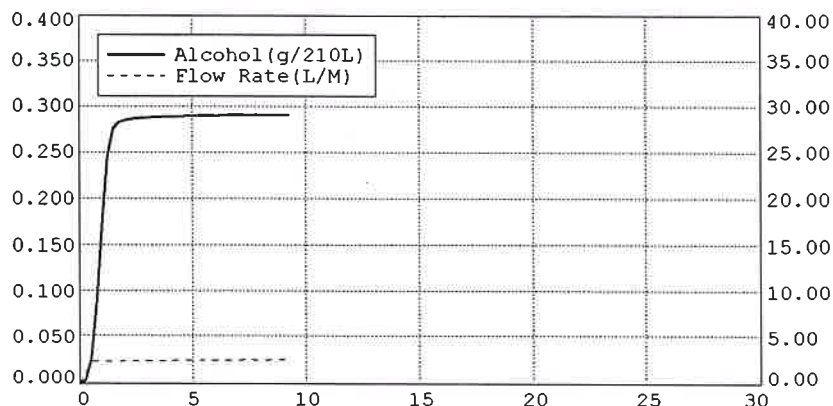

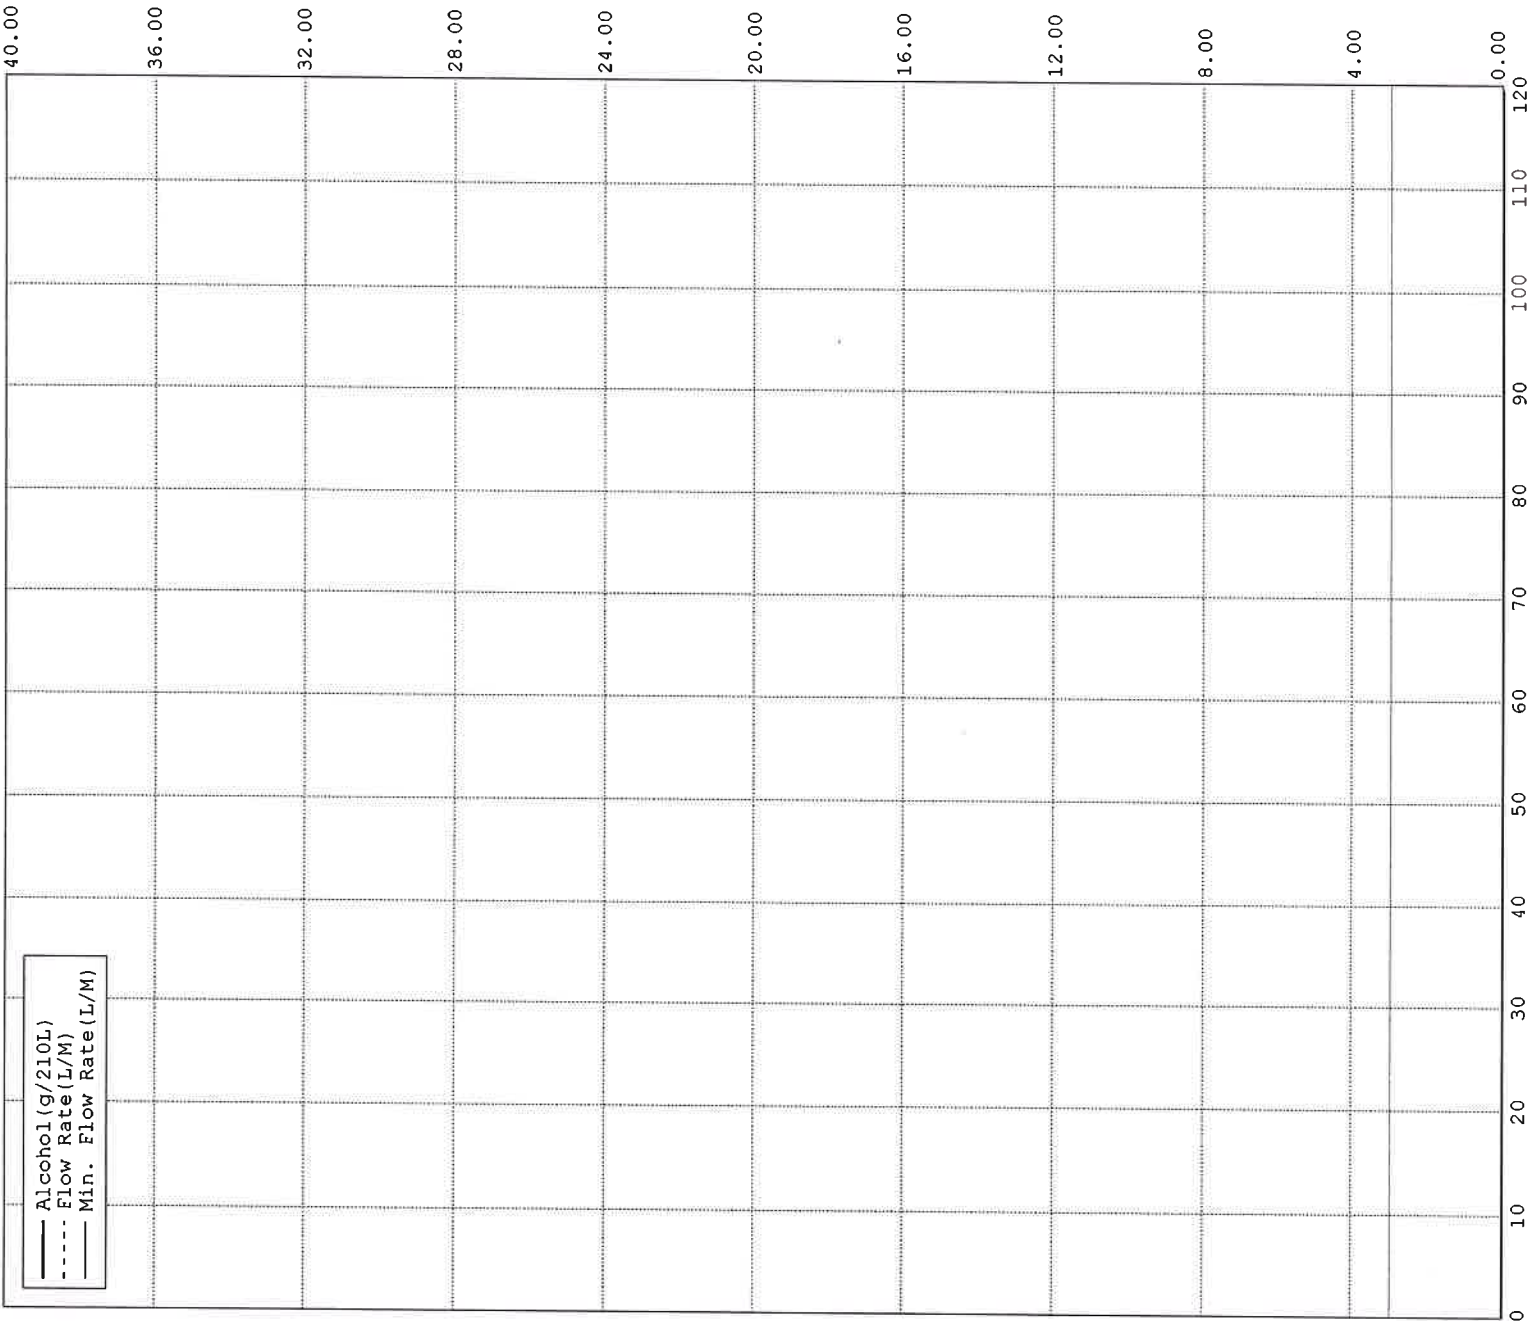

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100381

Date: 12/08/2025
Time: 12:56:56

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.29: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
PASSED 12:59
0.000 13:00
VERIFIED 13:00
INTERNAL STANDARD
0.079 13:00
EXTERNAL STANDARD
0.000 13:01
BLANK TEST
INCOMPLETE 13:03
SUBJECT SAMPLE

100381-2025-12-08-CALIBRATION Page 14 of 21

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100381

Date: 12/08/2025

Time: 13:07:23

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

MAX ATTEMPTS EXCEEDED

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.28: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

PASSED 13:08

BLANK TEST

0.000 13:08

INTERNAL STANDARD

VERIFIED 13:08

0.079 13:08

EXTERNAL STANDARD

0.000 13:09


BLANK TEST

XXX 13:10

SUBJECT SAMPLE

Maximum Attempts Exceeded

100381-2025-12-08-CALIBRATION Page 15 of 21

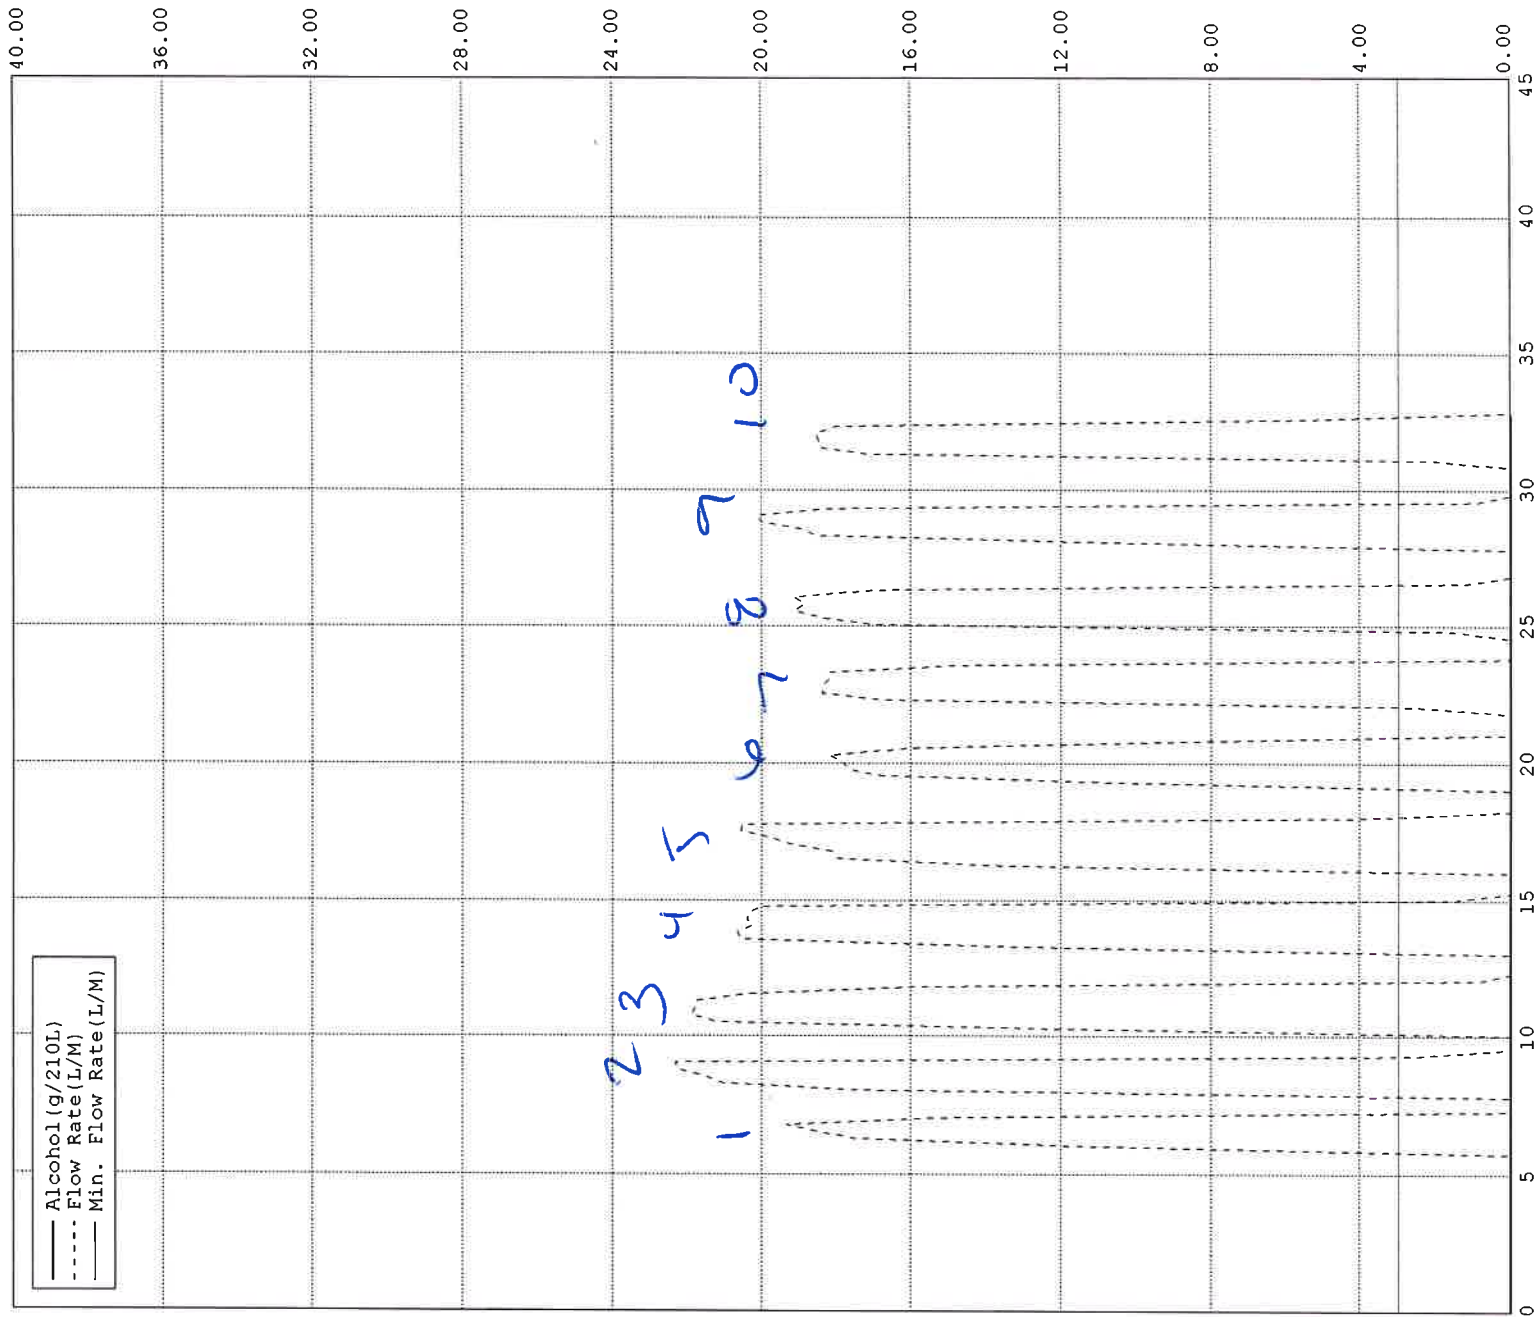

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100381

Date: 12/08/2025

Time: 14:10:30

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INVALID

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.26: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 14:11
0.000 14:11
VERIFIED 14:11
0.078 14:12
0.000 14:13
INVALID 14:13

OKG

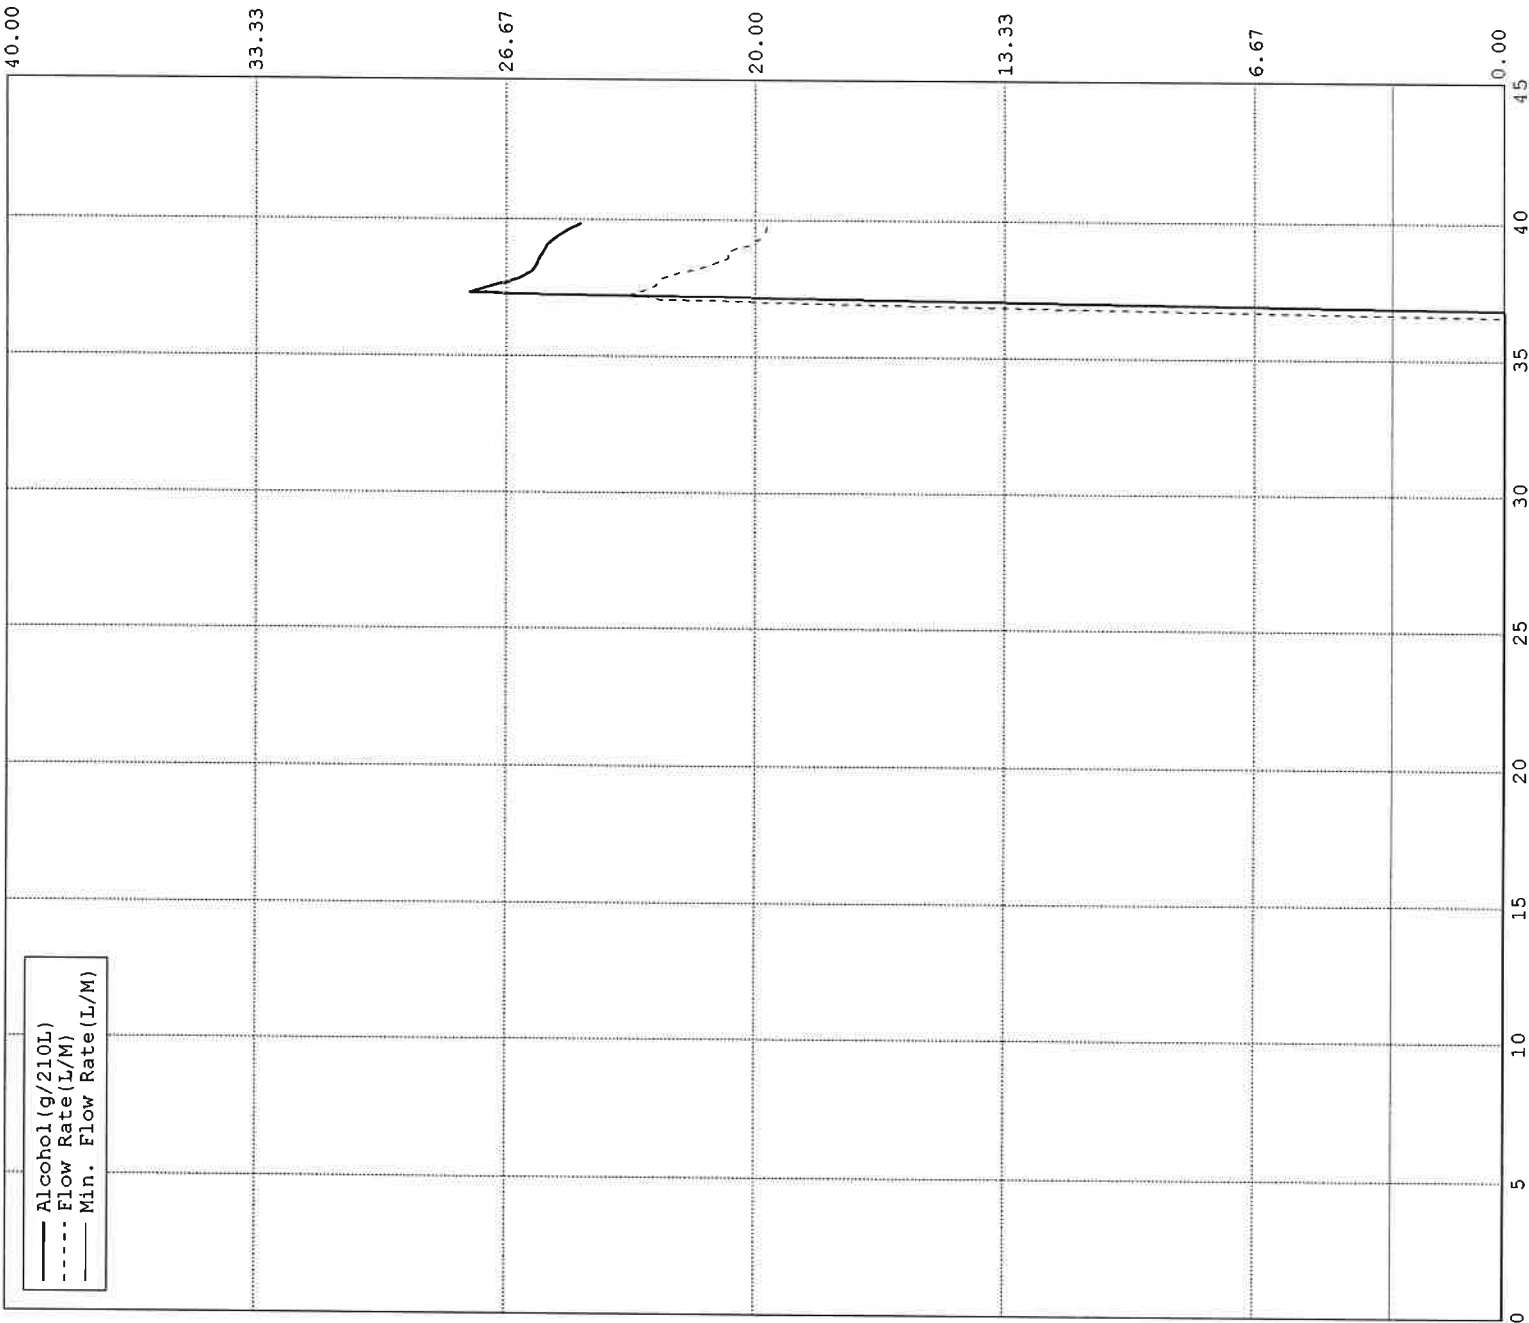

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100381

Date: 12/08/2025
Time: 14:16:09

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
RFI


CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
PASSED 14:17
BLANK TEST 0.000 14:17
INTERNAL STANDARD VERIFIED 14:18
EXTERNAL STANDARD 0.079 14:18
BLANK TEST 0.000 14:19

RFI DETECTED



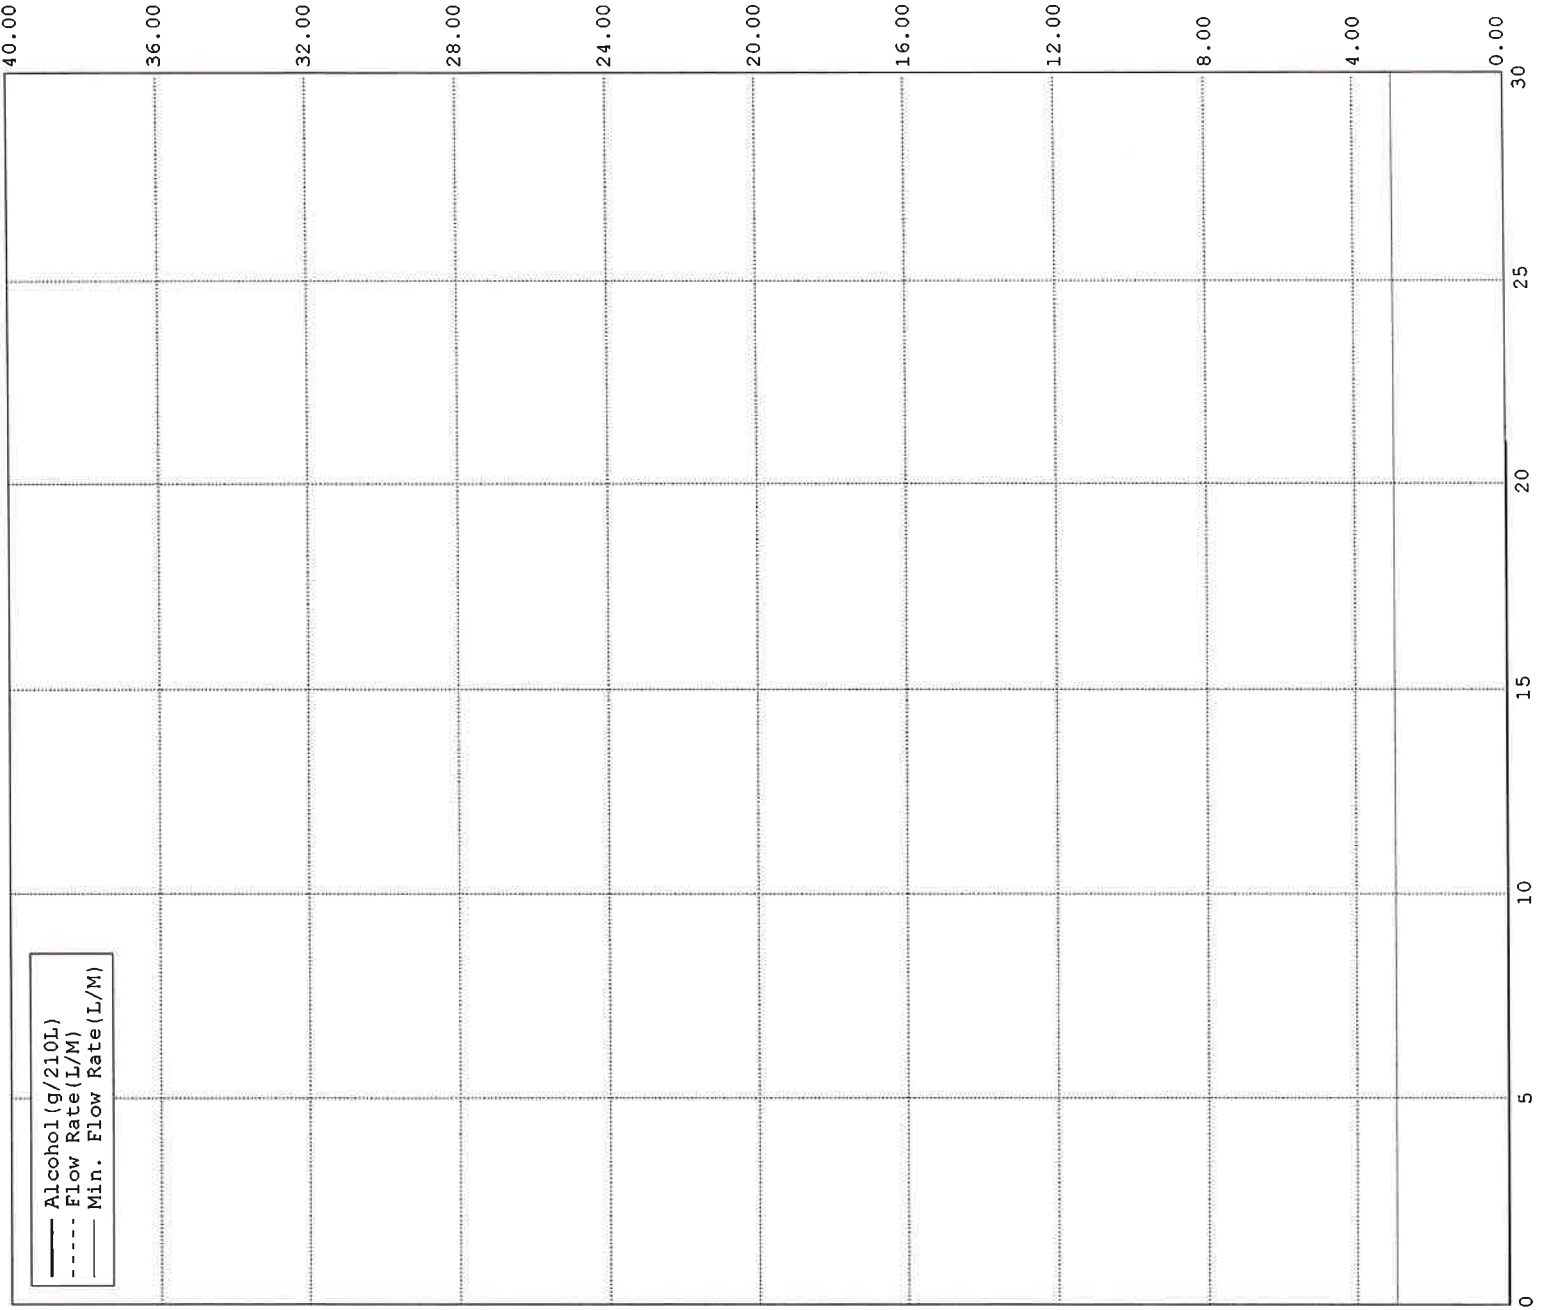

SUBJECT TEST

Alaska Department of Public Safety
 DATA MASTER dmt: 100381

Date: 12/08/2025
 Time: 13:13:20

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX

OPERATOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

DEPT/AGENCY:
 INTERFERENCE - ACETONE
 CASE/REPORT: XXXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.28: 0.078
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:14
BLANK TEST	0.000	13:14
INTERNAL STANDARD	VERIFIED	13:14
Xg = 0.092 (0.09%)		
EXTERNAL STANDARD	0.079	13:15
X[1] = 0.0790 (-0.0002)	(0.0028)	
BLANK TEST	0.000	13:15
SUBJECT SAMPLE	XXX	13:16
X[1] = 0.1091 (-0.0137)	(0.0026)	


Interference Detected

Filter 2 Avg: -0.0003

Filter 3 Avg: 0.0028

OWG 12/18/25

[Handwritten Signature]

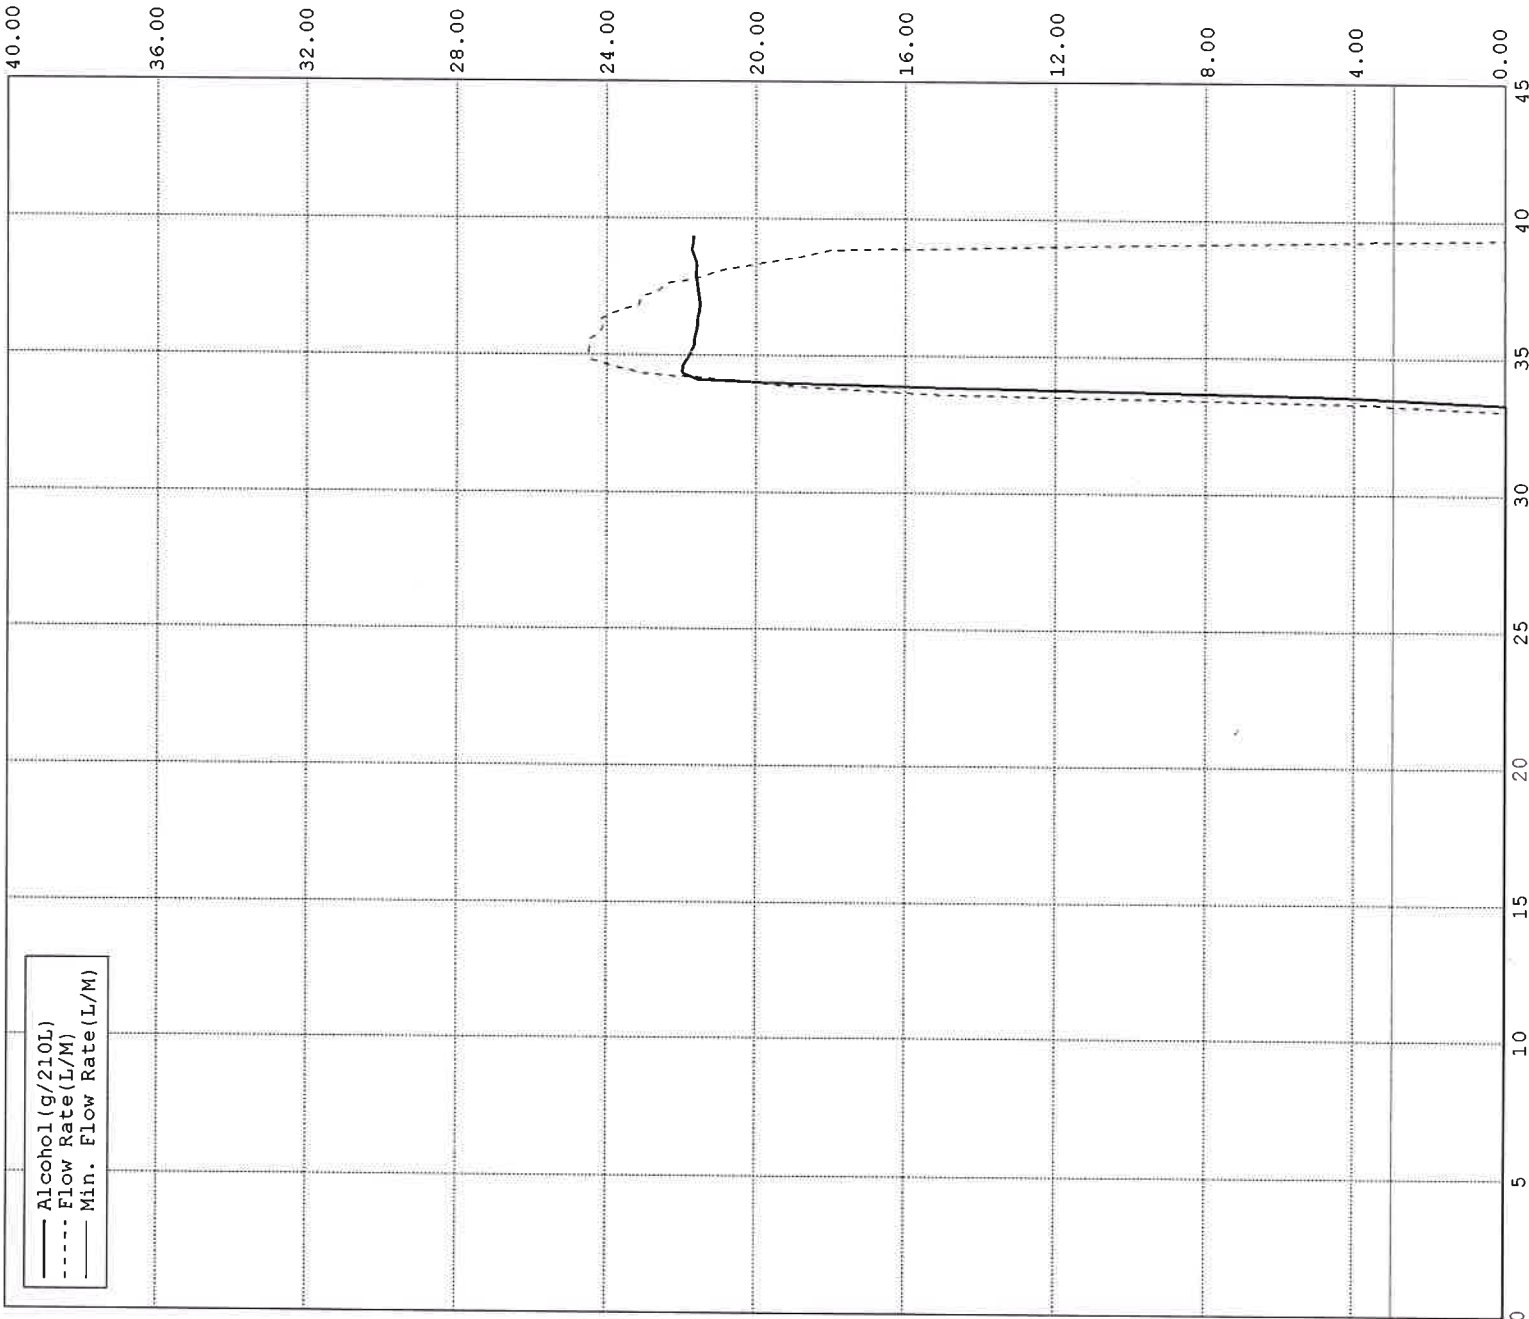

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100381

Date: 12/08/2025
Time: 13:19:29

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.28: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST
INTERNAL STANDARD
Xq = 0.092 (0.09%)
EXTERNAL STANDARD
X[1] = 0.0786 (-0.0005)
BLANK TEST
SUBJECT SAMPLE
X[1] = 0.1172 (-0.0181) (0.0026)

PASSED 13:20
0.000 13:21
VERIFIED 13:21

0.079 13:21
(0.0027)
0.000 13:22
XXX 13:22

Interference Detected

0005

Alcohol (g/210L)

Flow Rate (L/M)

Min. Flow Rate (L/M)

Time (min)

Time (min)	Alcohol (g/210L)	Flow Rate (L/M)	Min. Flow Rate (L/M)
0	0.00	0.00	0.00
5	0.00	0.00	0.00
10	0.00	0.00	0.00
15	0.00	0.00	0.00
20	24.00	24.00	24.00
20.5	28.00	28.00	28.00
21	24.00	24.00	24.00
25	0.00	0.00	0.00
30	0.00	0.00	0.00

100381-2025-12-08-CALIBRATION Page 19 of 21

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100381

Date: 12/08/2025
Time: 13:33:27

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.28: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:35
BLANK TEST	0.000	13:35
INTERNAL STANDARD	VERIFIED	13:35
Xq = 0.093 (0.57%)		
EXTERNAL STANDARD	0.079	13:36
X[1] = 0.0788 (-0.0003)	(0.0033)	
BLANK TEST	0.000	13:37
SUBJECT SAMPLE (Vol=2.03L)	0.092	13:37
X[1] = 0.0923 (0.0012)	(0.0012)	
BLANK TEST	0.000	13:38
EXTERNAL STANDARD	0.078	13:38
X[1] = 0.0782 (-0.0003)	(0.0024)	
BLANK TEST	0.000	13:39

Handwritten signature

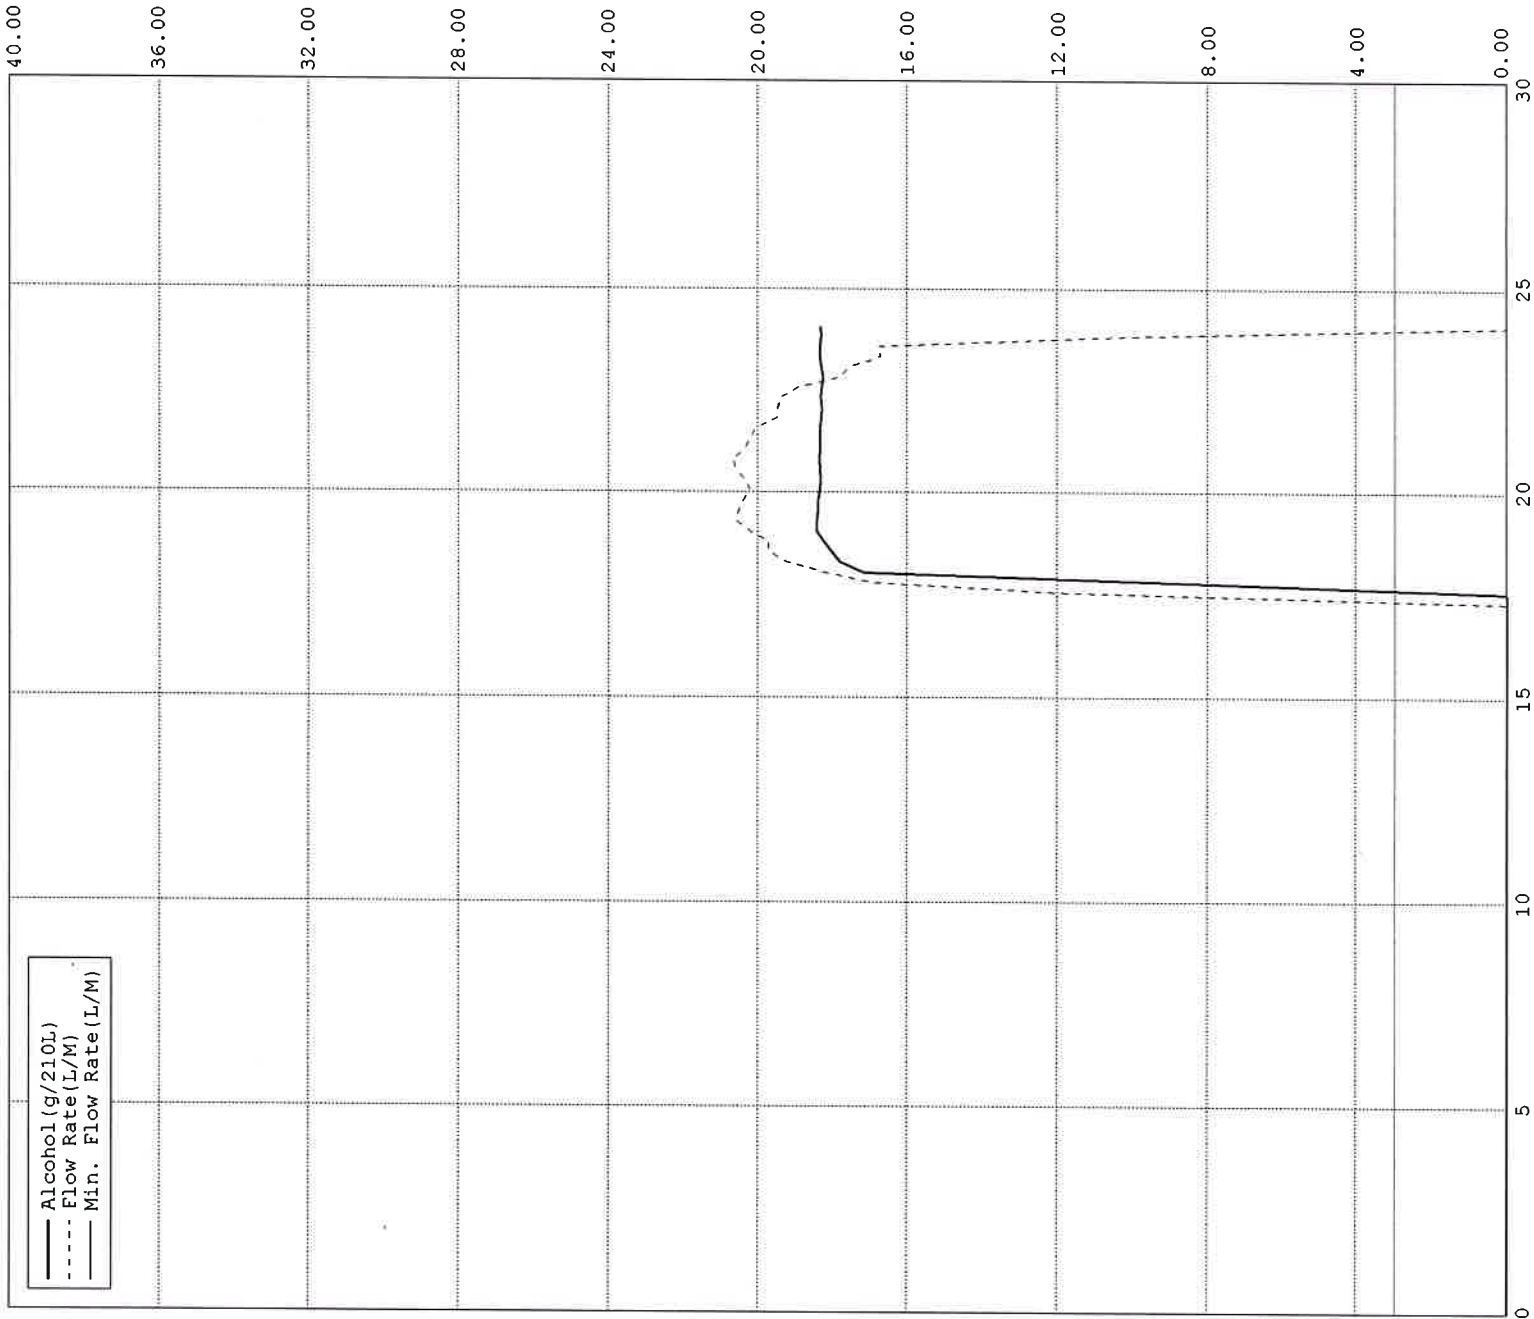

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100381

Date: 12/08/2025
Time: 14:46:23

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.26: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:49
BLANK TEST	0.000	14:50
INTERNAL STANDARD	VERIFIED	14:50
EXTERNAL STANDARD	0.078	14:50
BLANK TEST	0.000	14:51
SUBJECT SAMPLE (Vol=2.06L)	0.000	14:51
BLANK TEST	0.000	14:52
EXTERNAL STANDARD	0.079	14:52
BLANK TEST	0.000	14:53

Signature

