



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories

Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100668

Report Issue Date: 03/29/2023
Date Received: 2023-02-22
Condition of Item: Good

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

Start Date 02/22/2023 - As Found - **End Date 02/22/2023** As Found - Evaluation Analyst: Colleen O'Bryant
 As Found Conditions - Barometric Pressure (inHg): 30.23 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.2
 Relative Humidity (%): 12

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.022	0.022	0.022	0.022	0.021	0.022	
0.080	0.081	AG113402	0.080	0.079	0.081	0.081	0.081	0.080	
0.300	0.304	AG217903	0.303	0.303	0.303	0.304	0.304	0.303	

Completed a VOC + 5+ cycles of filter wheel tests without issue.

Start Date 03/14/2023 - As Left - **End Date 03/14/2023**

As Left Conditions - Barometric Pressure (inHg): 29.26 Barometer Used: Fisher S/N 221250180 Temperature (C): 21.6 Relative Humidity (%): 4

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG217902	0.021	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG217904	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.078	AG113402	0.078	0.078	0.078	0.078	0.078	0.078	+/- 0.003
0.100	0.098	AG211003	0.099	0.098	0.098	0.098	0.098	0.098	+/- 0.003
0.150	0.147	AG134205	0.148	0.148	0.147	0.147	0.148	0.148	+/- 0.004
0.300	0.293	AG217903	0.296	0.296	0.295	0.295	0.296	0.296	+/- 0.008

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Technically and administratively reviewed by Colleen O'Bryant on 03/29/2023

Results authorized by Derek Walton on 03/16/2023
derek.walton@alaska.gov

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100668 Analyst: Tatiana Malincke Start Date: 03-14-2023

- Diagnostic Test (attached)
- Adjust voltages, if needed
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
- Internal Standard value \leq 3.00%
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.6 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.26 Temperature (C): 21.6 Relative Humidity (%): 41

Linearity Test (attached)

0.020g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG217902</u>	Exp:	<u>06-28-2024</u>
0.040g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG217904</u>	Exp:	<u>06-28-2024</u>
0.080g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG113402</u>	Exp:	<u>05-14-2023</u>
0.100g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG211003</u>	Exp:	<u>04-20-2024</u>
0.150g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG134205</u>	Exp:	<u>12-08-2023</u>
0.300g/210L Mnf:	<u>Airgas</u>	Lot:	<u>AG217903</u>	Exp:	<u>06-28-2024</u>

Functional Tests (attached)

- Incomplete
- Maximum Attempts Exceeded
- Interference (Volatiles)
- Invalid
- Radio Frequency Interference (RFI)

Acetone Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11-09-2023

Simulator S/N: DK4161 Verification Performed?

Isopropanol Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11-09-2023

Simulator S/N: SD1088 Verification Performed?

Neg. Control Mnf: LIFELOC Lot: 21KP41172 Level: 0.100 Exp: 11-09-2023

Simulator S/N: SD1177 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11-09-2023

- Verify stylus is calibrated
 - Reset Options
 - Clear Memory
 - Verification of Calibration (VOC)
 - Non-Drinking Subject Test
 - Upload
 - Remove Tank Prior to Shutdown
- Calibration End Date: 03-14-2023

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 07:50:44

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 45.9°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.82 V PASSED
(0.97 V - 2.25 V)
Cooler Voltage = 1.79 V PASSED
(1.04 V - 2.44 V)
Bias Voltage = 79 V PASSED
(48 V - 112 V)
Chopper Freq = 533 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.3 in

PUMP INFO

Flow Rate = 4.756 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.090 0.58% (0.00% - 4.00%) PASSED

Technician Screen

DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 7:59 AM

Temperatures (°C)

Sample Cell: 48.6°C
Breath Tube: 45.3°C

Current Barometer 29.2 in
Volume (Ltr) 1.56

Settings

Lamp: 1.85 V
Bias: 79 V
Cooler: 1.79 V
Chopper: 532 Hz

Voltages (V)

Flow: 1.06 V
Detector: -0.082 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 07/31/2018
Time: 09:44:06

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca = 0.1000
CAL = 0.977818 0.800 <= CAL < 1.200
b1 = 0.0021 0.0000 <= b1 < 0.0040
b2 = 0.0063 0.0010 <= b2 < 0.0100
b3 = 0.0018 0.0000 <= b3 < 0.0040
Xq = 0.0899 0.0500 <= Xq < 0.2000
a21 = 1.160887 1.050 <= a21 < 1.300
a31 = 0.530987 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 08:17:55

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.26: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	08:18
BLANK TEST	0.000	08:19
INTERNAL STANDARD	VERIFIED	08:19
EXTERNAL STANDARD	0.078	08:19
BLANK TEST	0.000	08:20
SUBJECT SAMPLE (Vol=1.60L)	0.000	08:21
BLANK TEST	0.000	08:22
EXTERNAL STANDARD	0.077	08:22
BLANK TEST	0.000	08:23

TLM

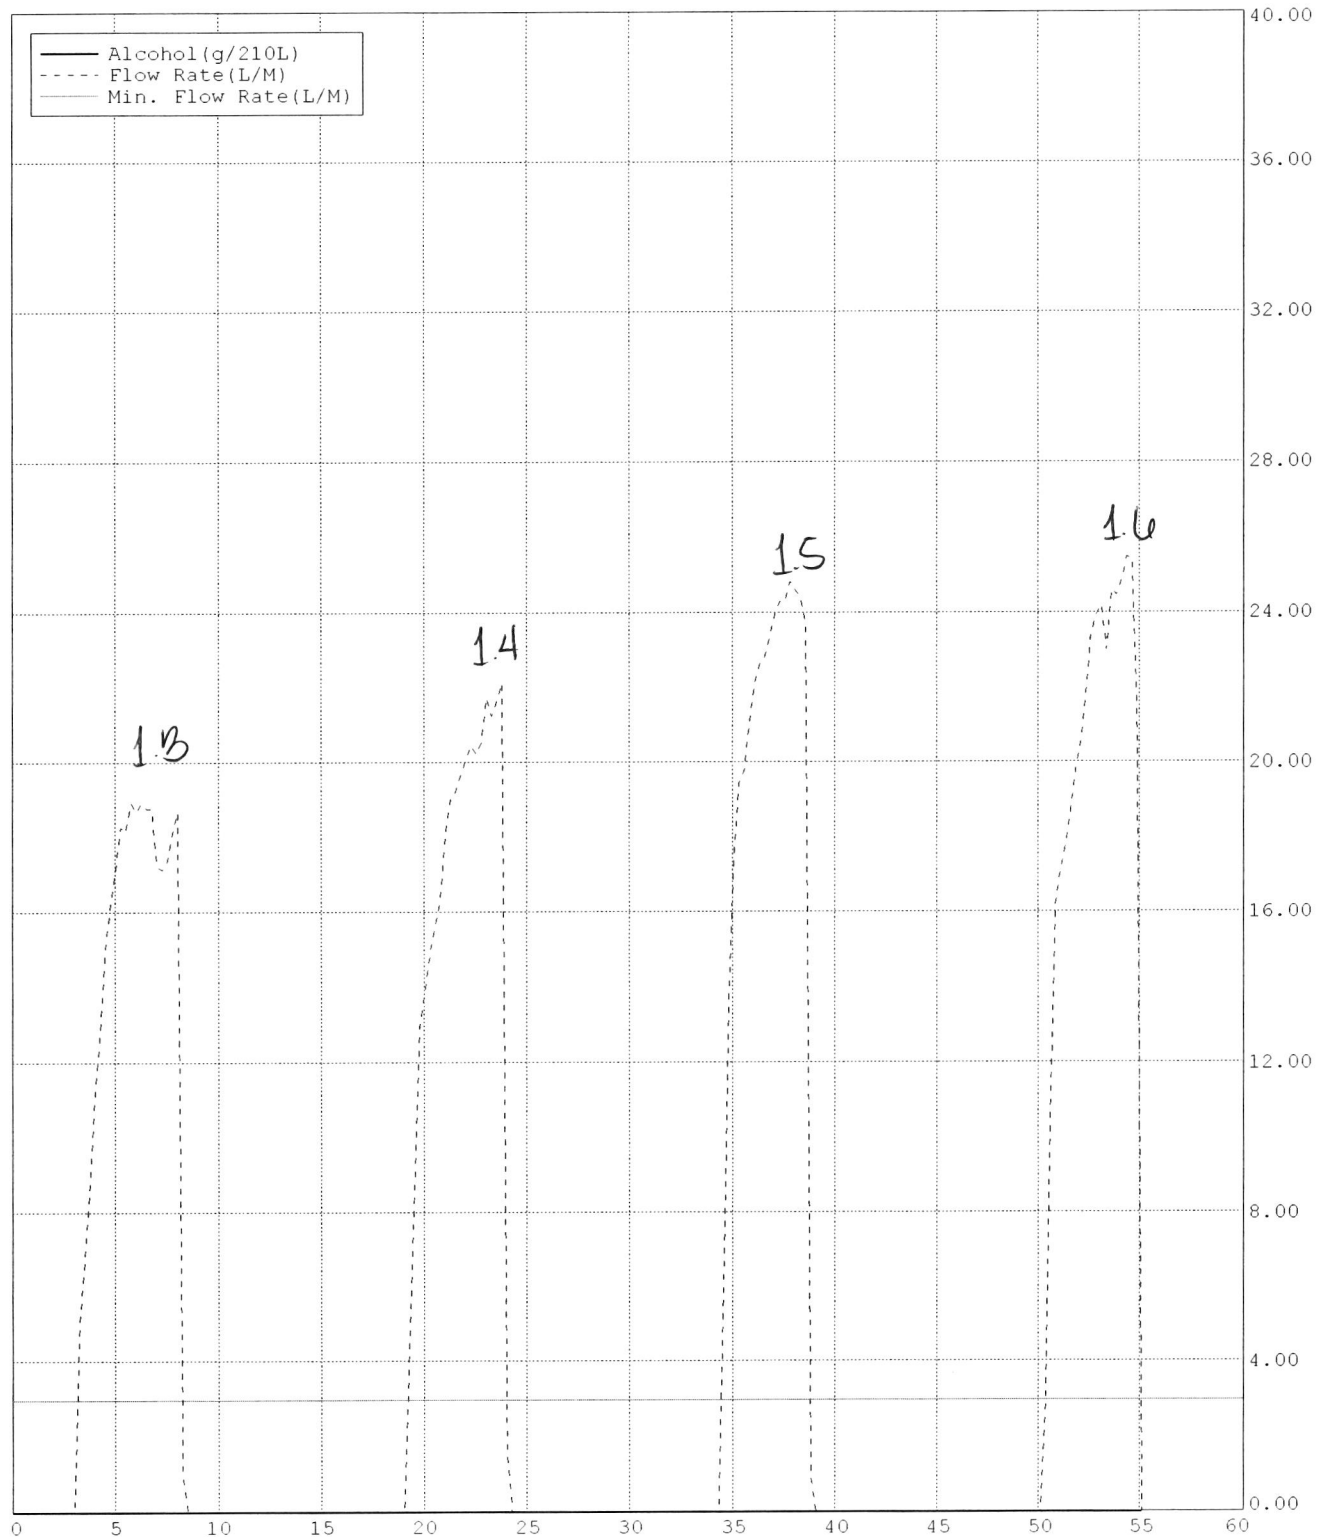

LINEARITY CHECK

Alaska Department of Public Safety
DATAMASTER dmt: 100668


Date: 03/14/2023
Time: 08:25:32

SUPERVISOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0004
0.039	0.0400	0.0000
0.078	0.0780	0.0000
0.098	0.0982	0.0004
0.147	0.1476	0.0005
0.293	0.2956	0.0005

SLOPE = 1.008042
R² = 0.999970

TLM

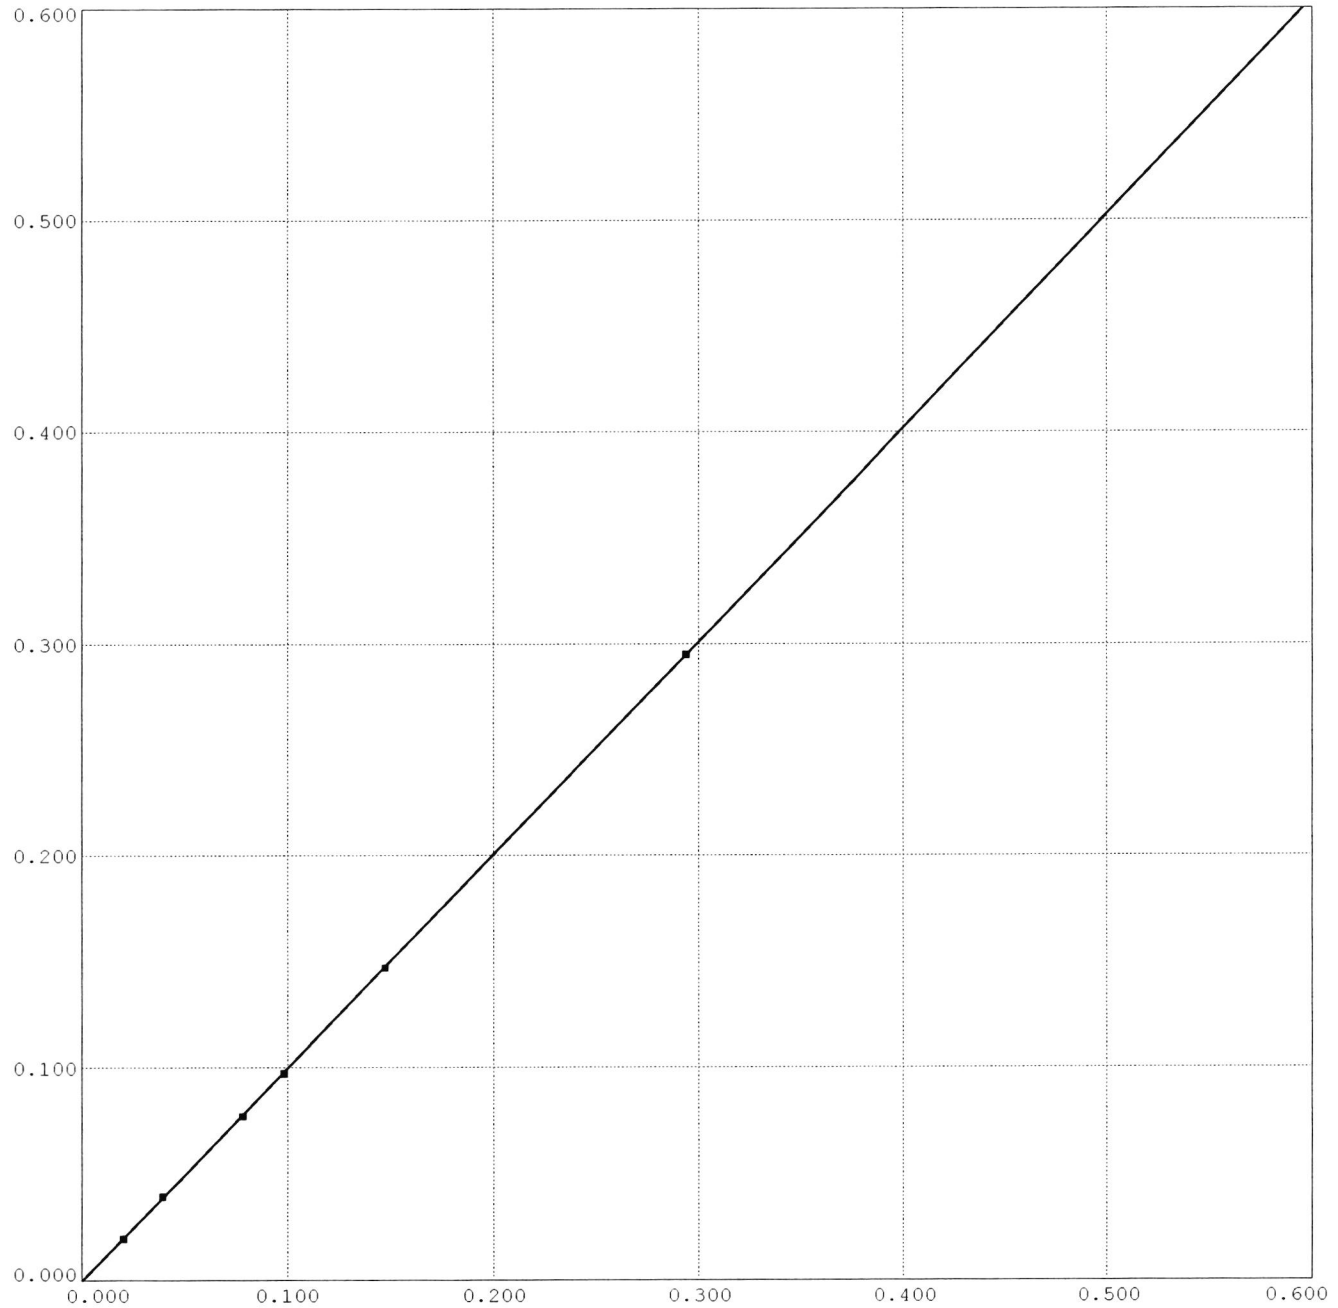

LINEARITY CHECK: Control Test 1

 Alaska Department of Public Safety
 DATAMASTER dmt: 100668






Date: 03/14/2023
 Time: 08:25:34

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.25: 0.020
 LOT #: AG217902
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 892 psi

BLANK TEST	0.000	08:26
INTERNAL STANDARD	VERIFIED	08:27
EXTERNAL STANDARD	0.021	08:27
BLANK TEST	0.000	08:28
EXTERNAL STANDARD	0.020	08:28
BLANK TEST	0.000	08:29
EXTERNAL STANDARD	0.020	08:29
BLANK TEST	0.000	08:30
EXTERNAL STANDARD	0.020	08:30
BLANK TEST	0.000	08:31
EXTERNAL STANDARD	0.020	08:31
BLANK TEST	0.000	08:32

Average = 0.0202
 Std Dev = 0.0004

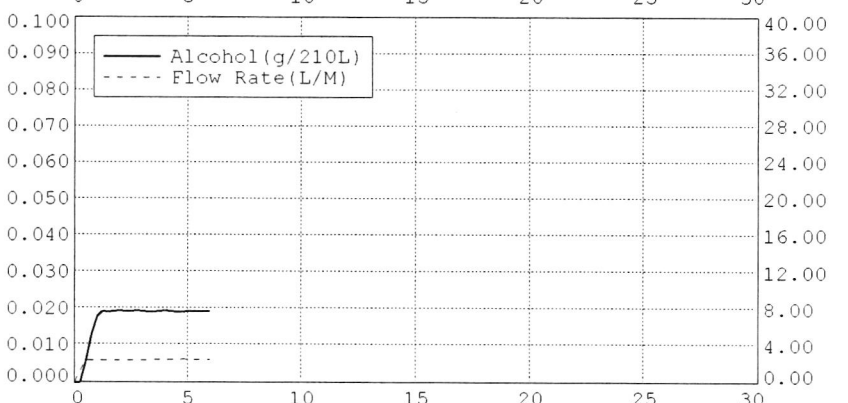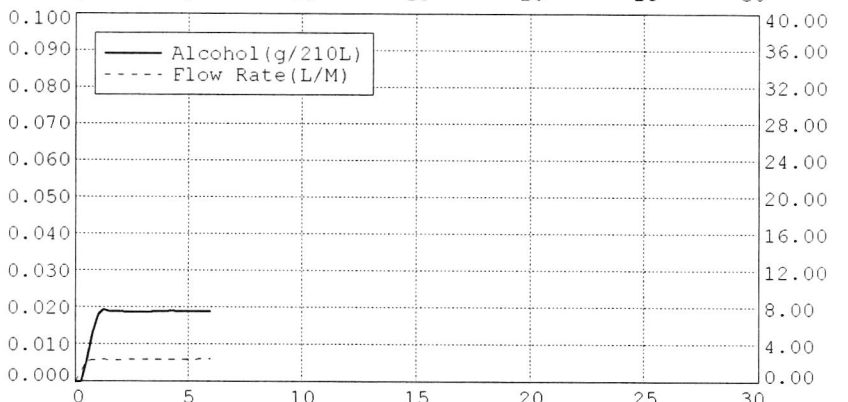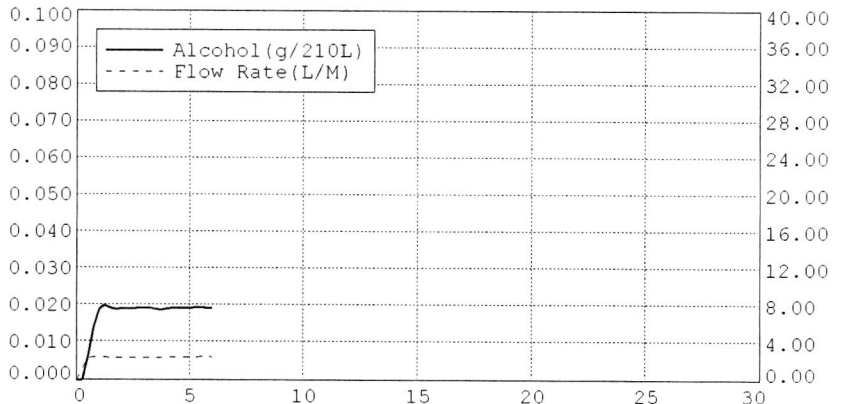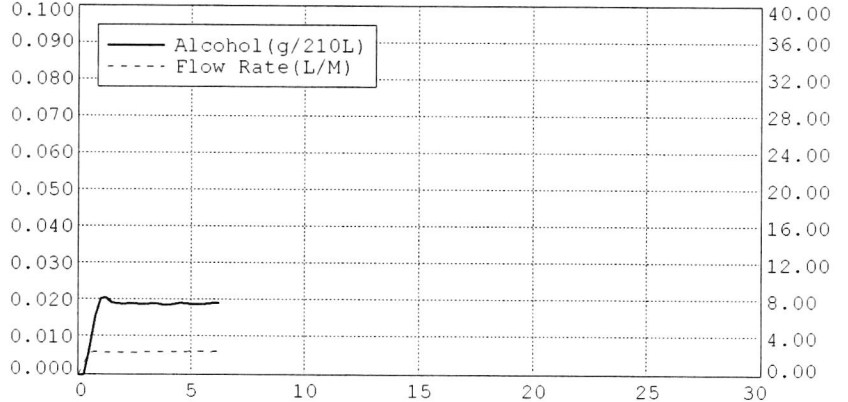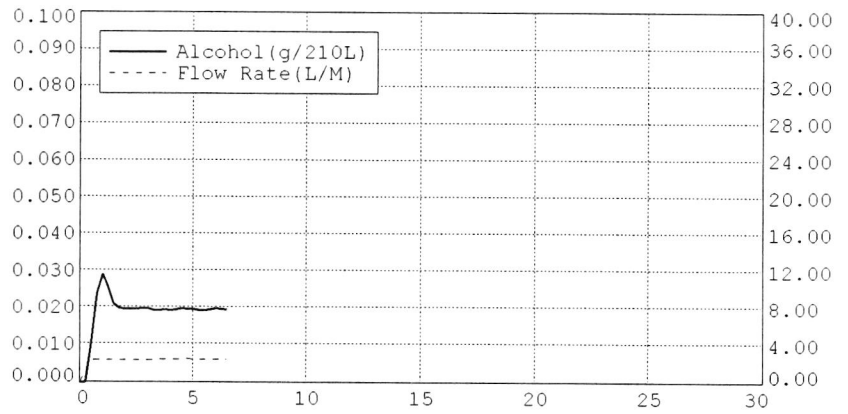

LINEARITY CHECK: Control Test 2

 Alaska Department of Public Safety
 DATAMASTER dmt: 100668






Date: 03/14/2023
 Time: 08:33:09

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.25: 0.039
 LOT #: AG217904
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 1114 psi

BLANK TEST	0.000	08:34
INTERNAL STANDARD	VERIFIED	08:34
EXTERNAL STANDARD	0.040	08:34
BLANK TEST	0.000	08:35
EXTERNAL STANDARD	0.040	08:35
BLANK TEST	0.000	08:36
EXTERNAL STANDARD	0.040	08:36
BLANK TEST	0.000	08:37
EXTERNAL STANDARD	0.040	08:38
BLANK TEST	0.000	08:38
EXTERNAL STANDARD	0.040	08:39
BLANK TEST	0.000	08:40

Average = 0.0400
 Std Dev = 0.0000

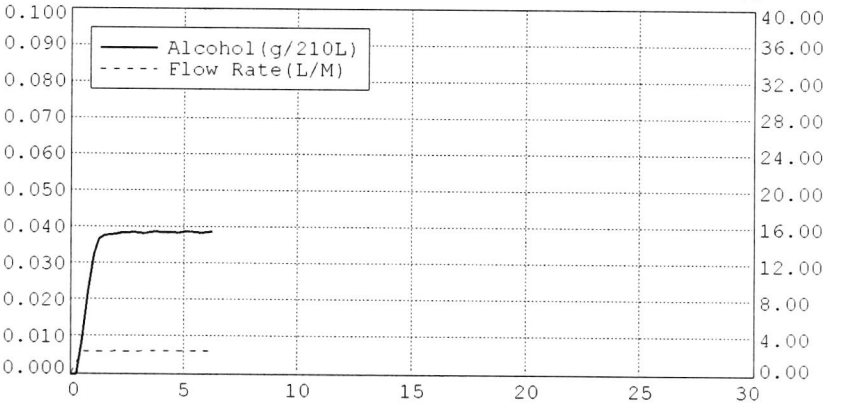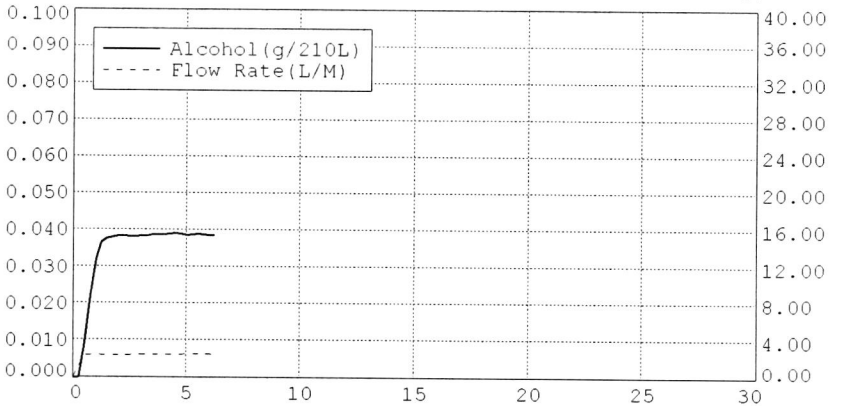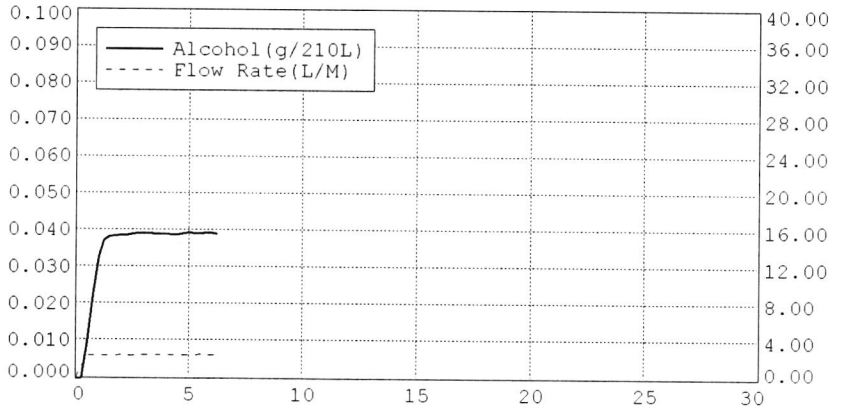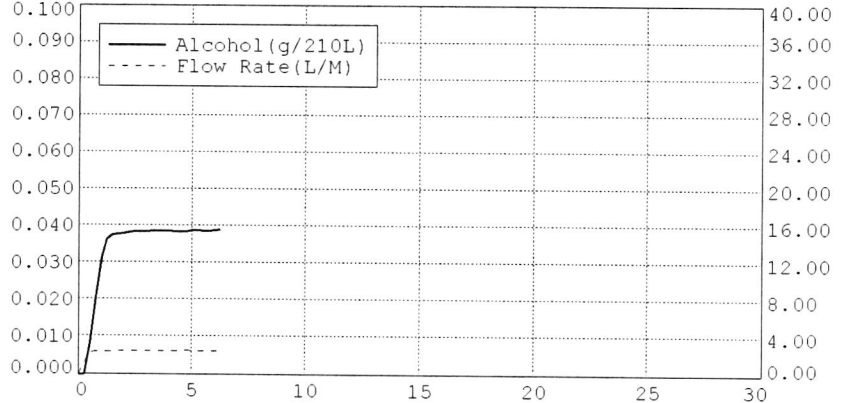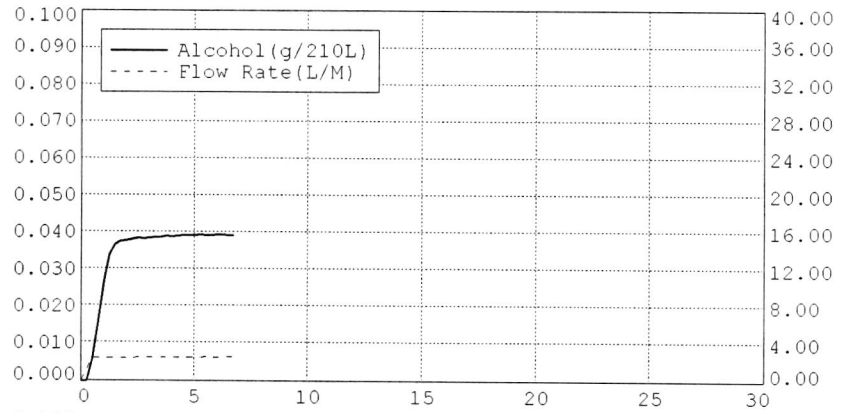

LINEARITY CHECK: Control Test 3

 Alaska Department of Public Safety
 DATAMASTER dmt: 100668






Date: 03/14/2023
 Time: 08:40:46

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.25: 0.078
 LOT #: AG113402
 EXPIRATION: 05/14/2023
 TANK PRESSURE: 378 psi

BLANK TEST	0.000	08:42
INTERNAL STANDARD	VERIFIED	08:42
EXTERNAL STANDARD	0.078	08:42
BLANK TEST	0.000	08:43
EXTERNAL STANDARD	0.078	08:43
BLANK TEST	0.000	08:44
EXTERNAL STANDARD	0.078	08:44
BLANK TEST	0.000	08:45
EXTERNAL STANDARD	0.078	08:45
BLANK TEST	0.000	08:46
EXTERNAL STANDARD	0.078	08:46
BLANK TEST	0.000	08:47

Average = 0.0780
 Std Dev = 0.0000

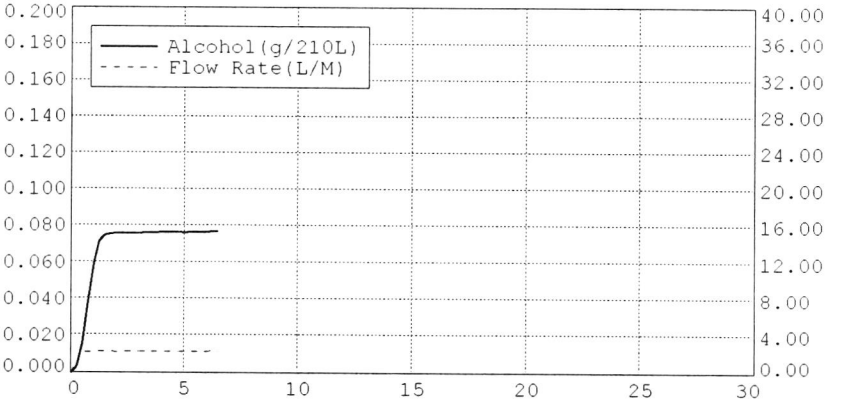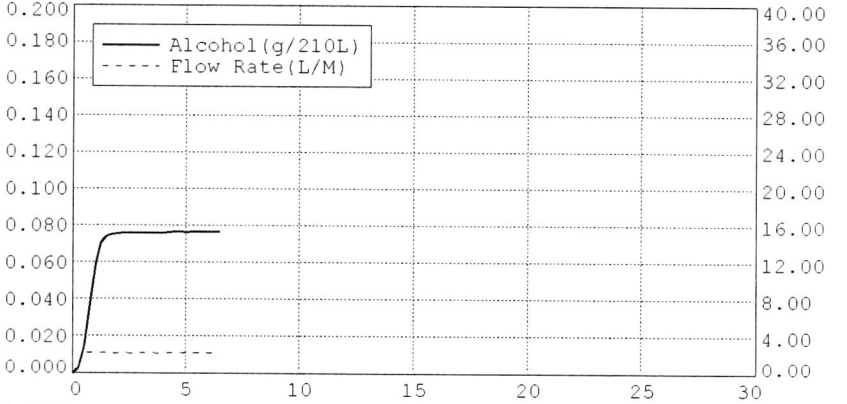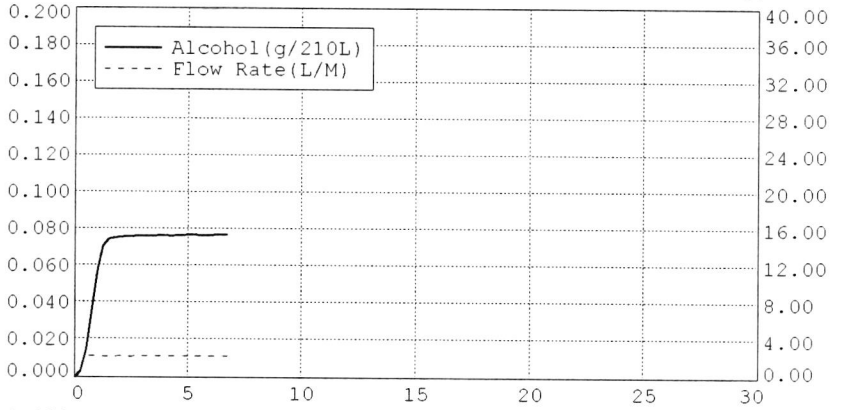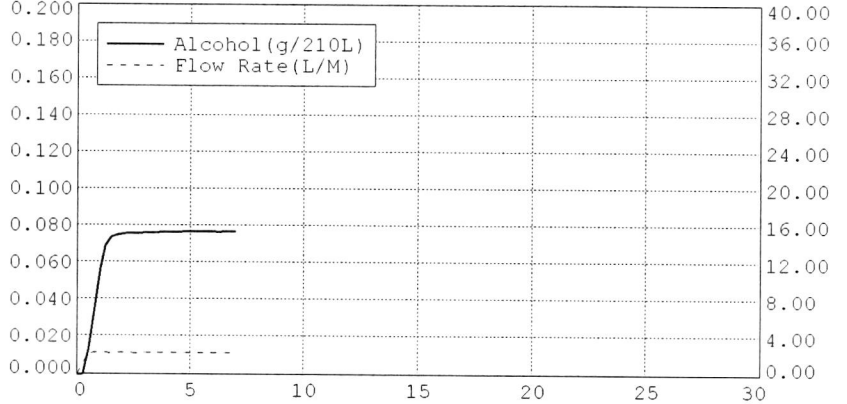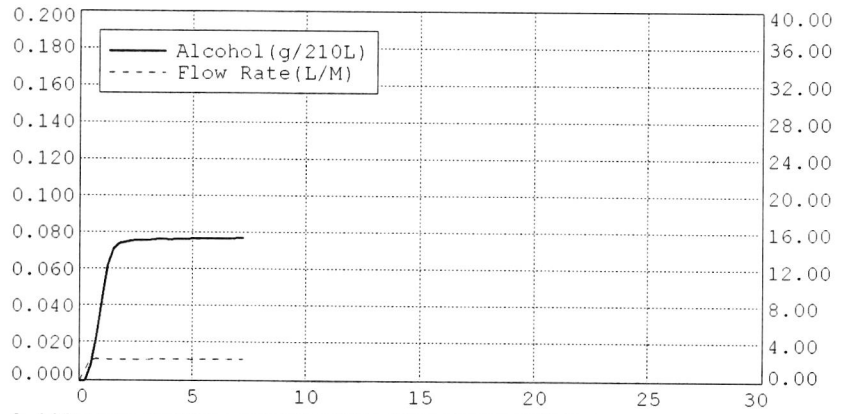

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100668






Date: 03/14/2023
 Time: 08:48:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.25: 0.098
 LOT #: AG211003
 EXPIRATION: 04/20/2024
 TANK PRESSURE: 831 psi

BLANK TEST	0.000	08:49
INTERNAL STANDARD	VERIFIED	08:49
EXTERNAL STANDARD	0.099	08:50
BLANK TEST	0.000	08:51
EXTERNAL STANDARD	0.098	08:51
BLANK TEST	0.000	08:52
EXTERNAL STANDARD	0.098	08:52
BLANK TEST	0.000	08:53
EXTERNAL STANDARD	0.098	08:53
BLANK TEST	0.000	08:54
EXTERNAL STANDARD	0.098	08:54
BLANK TEST	0.000	08:55

Average = 0.0982
 Std Dev = 0.0004

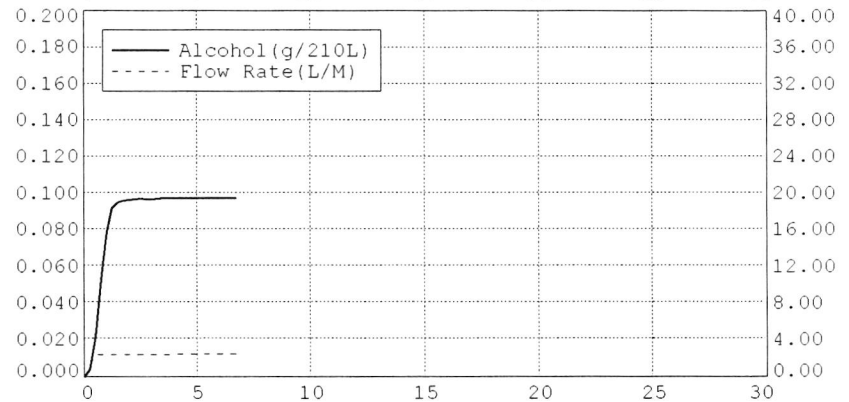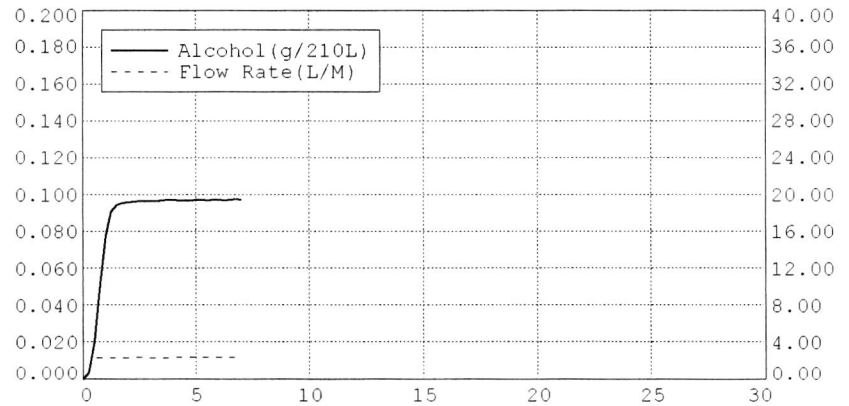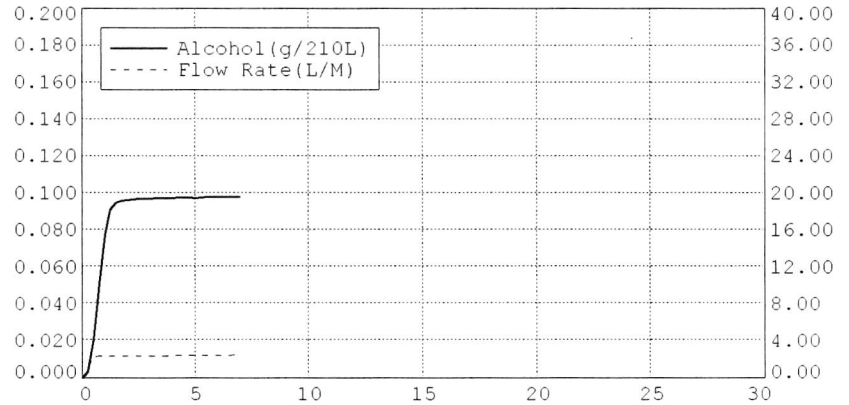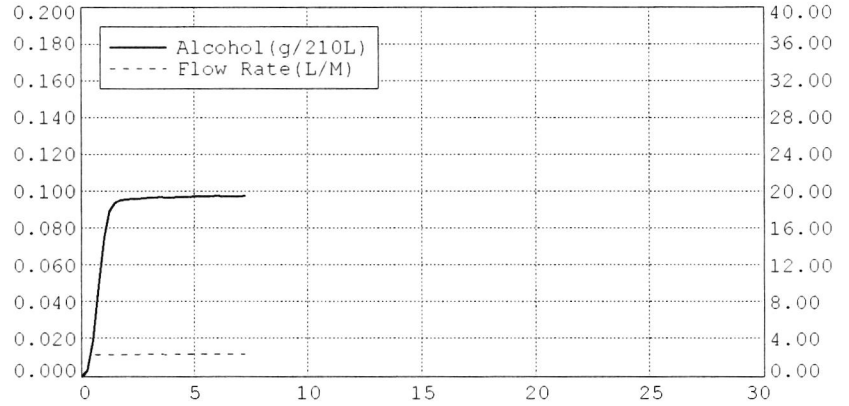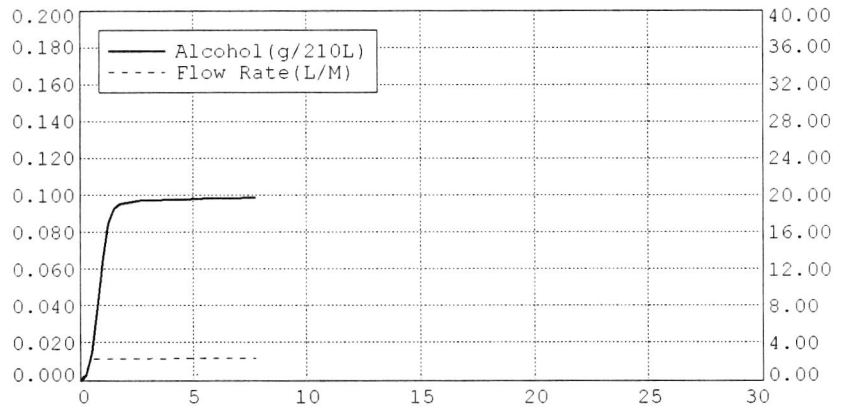

LINEARITY CHECK: Control Test 5

 Alaska Department of Public Safety
 DATAMASTER dmt: 100668






Date: 03/14/2023
 Time: 08:55:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.25: 0.147
 LOT #: AG134205
 EXPIRATION: 12/08/2023
 TANK PRESSURE: 1021 psi

BLANK TEST	0.000	08:57
INTERNAL STANDARD	VERIFIED	08:57
EXTERNAL STANDARD	0.148	08:57
BLANK TEST	0.000	08:58
EXTERNAL STANDARD	0.148	08:58
BLANK TEST	0.000	08:59
EXTERNAL STANDARD	0.147	08:59
BLANK TEST	0.000	09:00
EXTERNAL STANDARD	0.147	09:00
BLANK TEST	0.000	09:01
EXTERNAL STANDARD	0.148	09:01
BLANK TEST	0.000	09:02

Average = 0.1476
 Std Dev = 0.0005

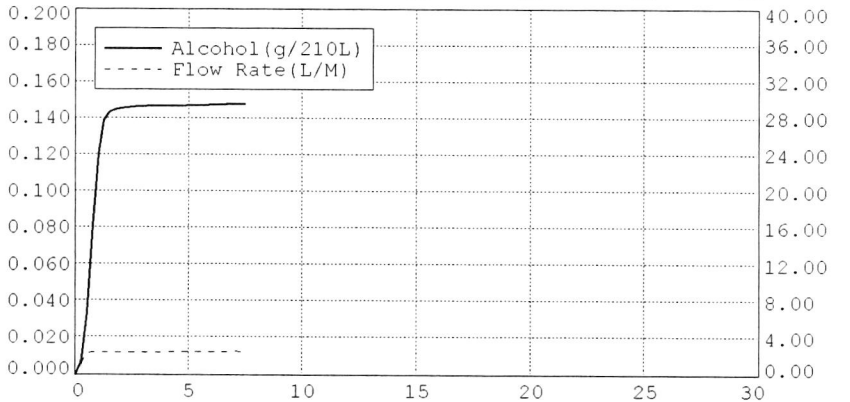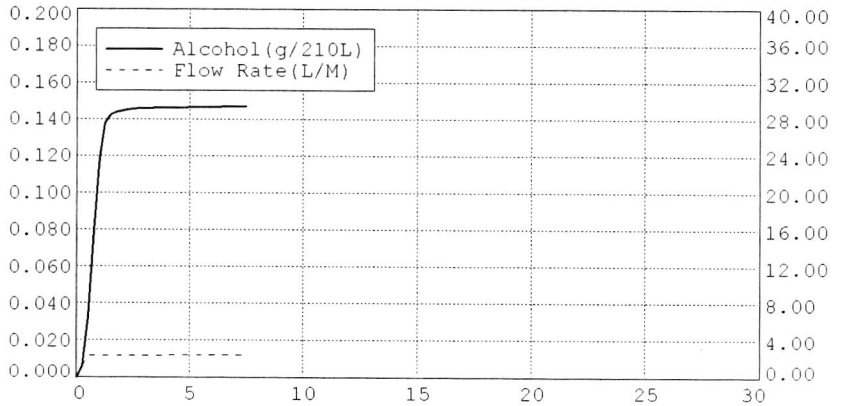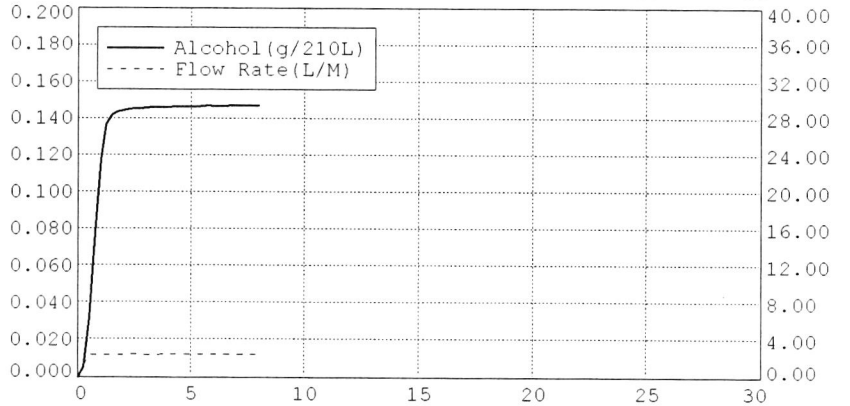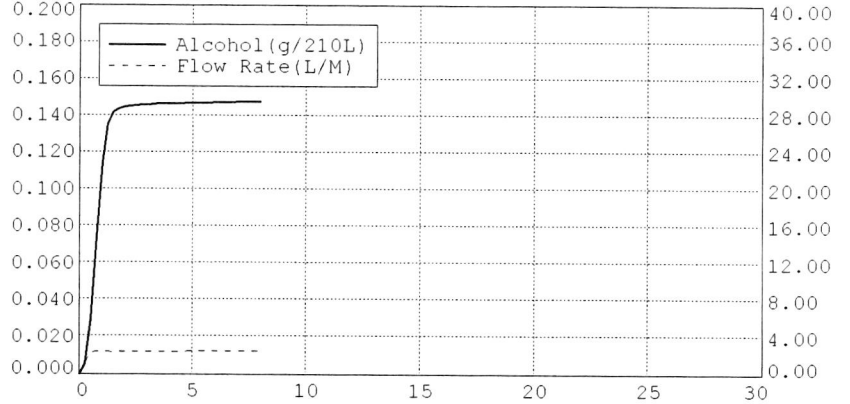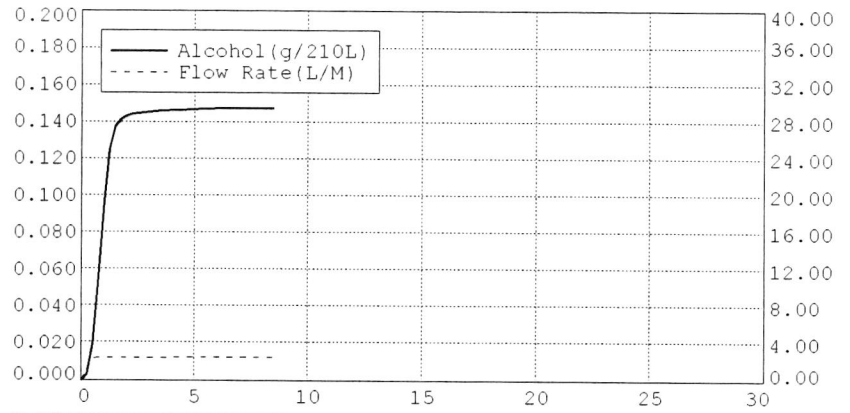

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100668






Date: 03/14/2023
 Time: 09:03:16

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.25: 0.293
 LOT #: AG217903
 EXPIRATION: 06/28/2024
 TANK PRESSURE: 415 psi

BLANK TEST	0.000	09:04
INTERNAL STANDARD	VERIFIED	09:04
EXTERNAL STANDARD	0.296	09:05
BLANK TEST	0.000	09:06
EXTERNAL STANDARD	0.296	09:06
BLANK TEST	0.000	09:07
EXTERNAL STANDARD	0.295	09:07
BLANK TEST	0.000	09:08
EXTERNAL STANDARD	0.295	09:08
BLANK TEST	0.000	09:09
EXTERNAL STANDARD	0.296	09:09
BLANK TEST	0.000	09:10

Average = 0.2956
 Std Dev = 0.0005

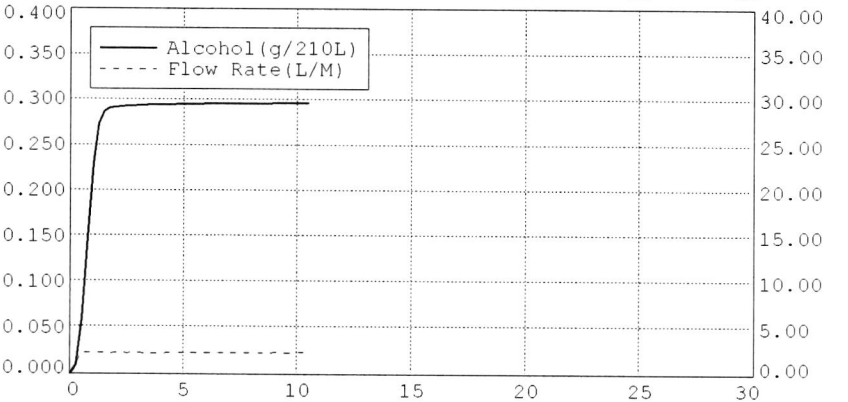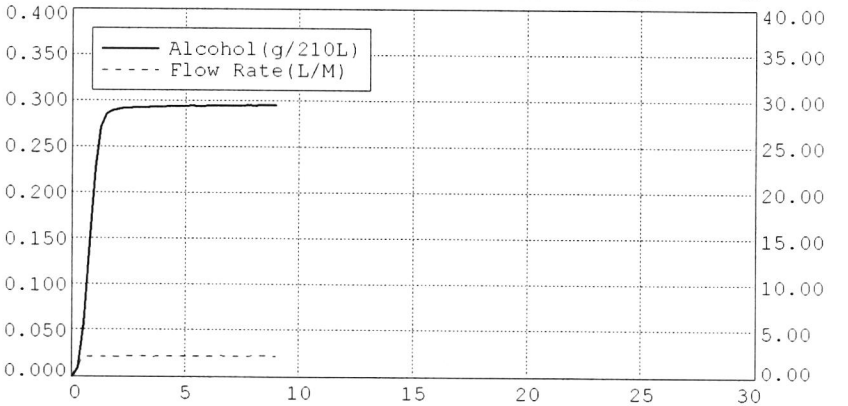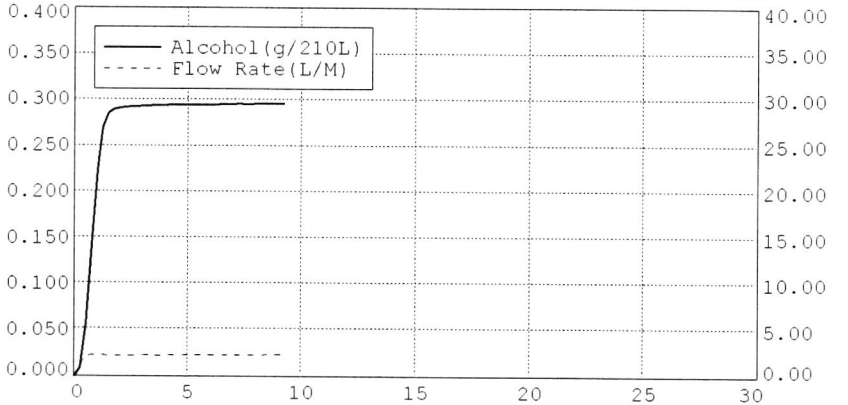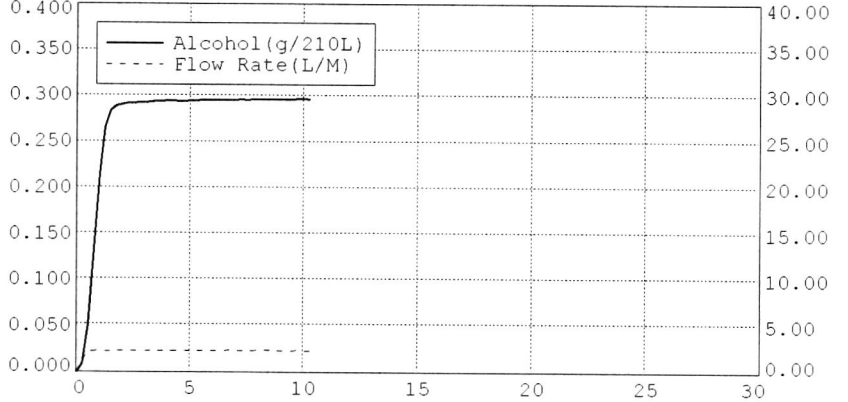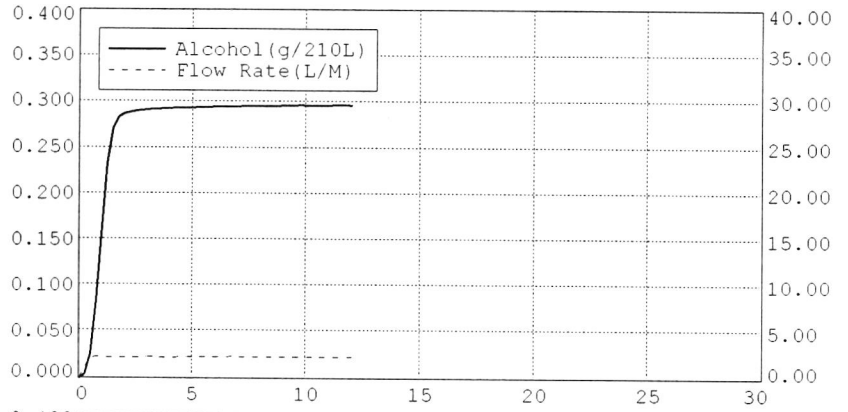

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 09:18:43

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.25: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:19
BLANK TEST	0.000	09:19
INTERNAL STANDARD	VERIFIED	09:20
EXTERNAL STANDARD	0.079	09:20
BLANK TEST	0.000	09:21
SUBJECT SAMPLE	INCOMPLETE	09:23

TLM

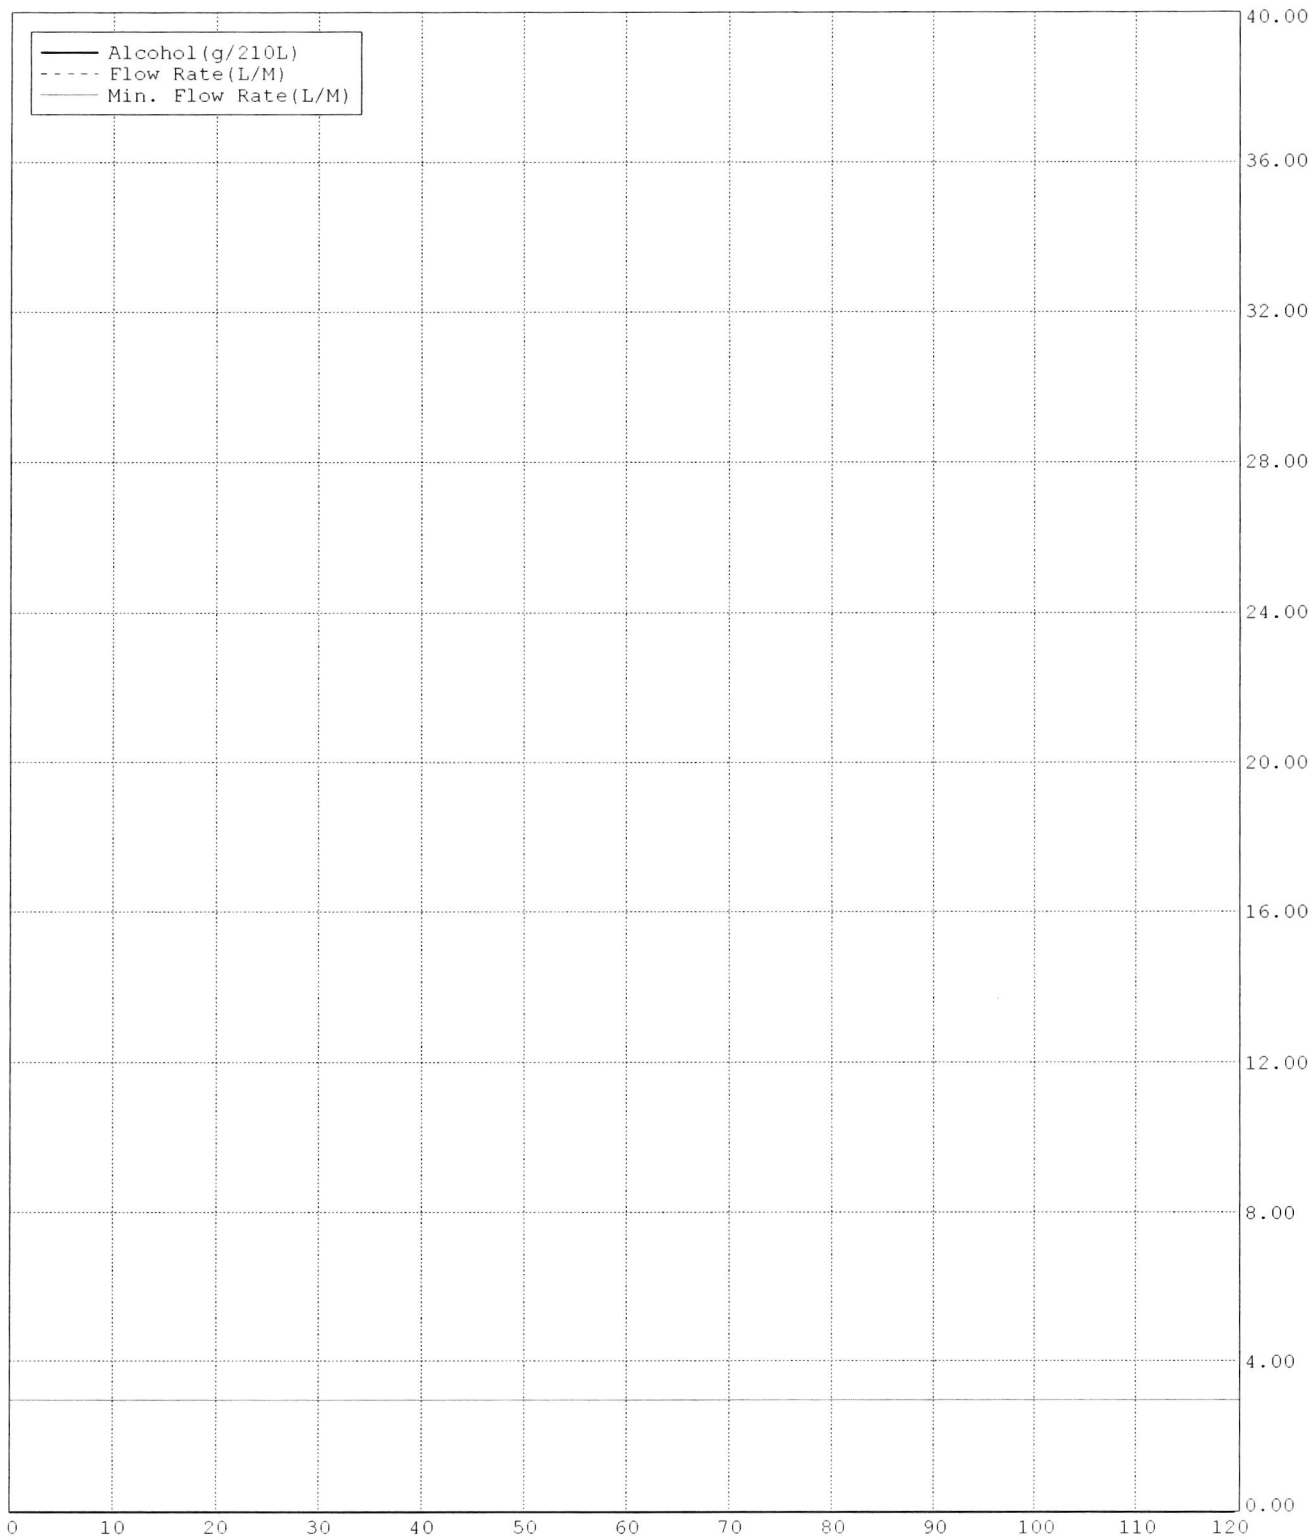

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 09:30:49

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437


DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.25: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	09:31
BLANK TEST	0.000	09:32
INTERNAL STANDARD	VERIFIED	09:32
EXTERNAL STANDARD	0.078	09:32
BLANK TEST	0.000	09:33
SUBJECT SAMPLE	XXX	09:33

Maximum Attempts Exceeded

TML

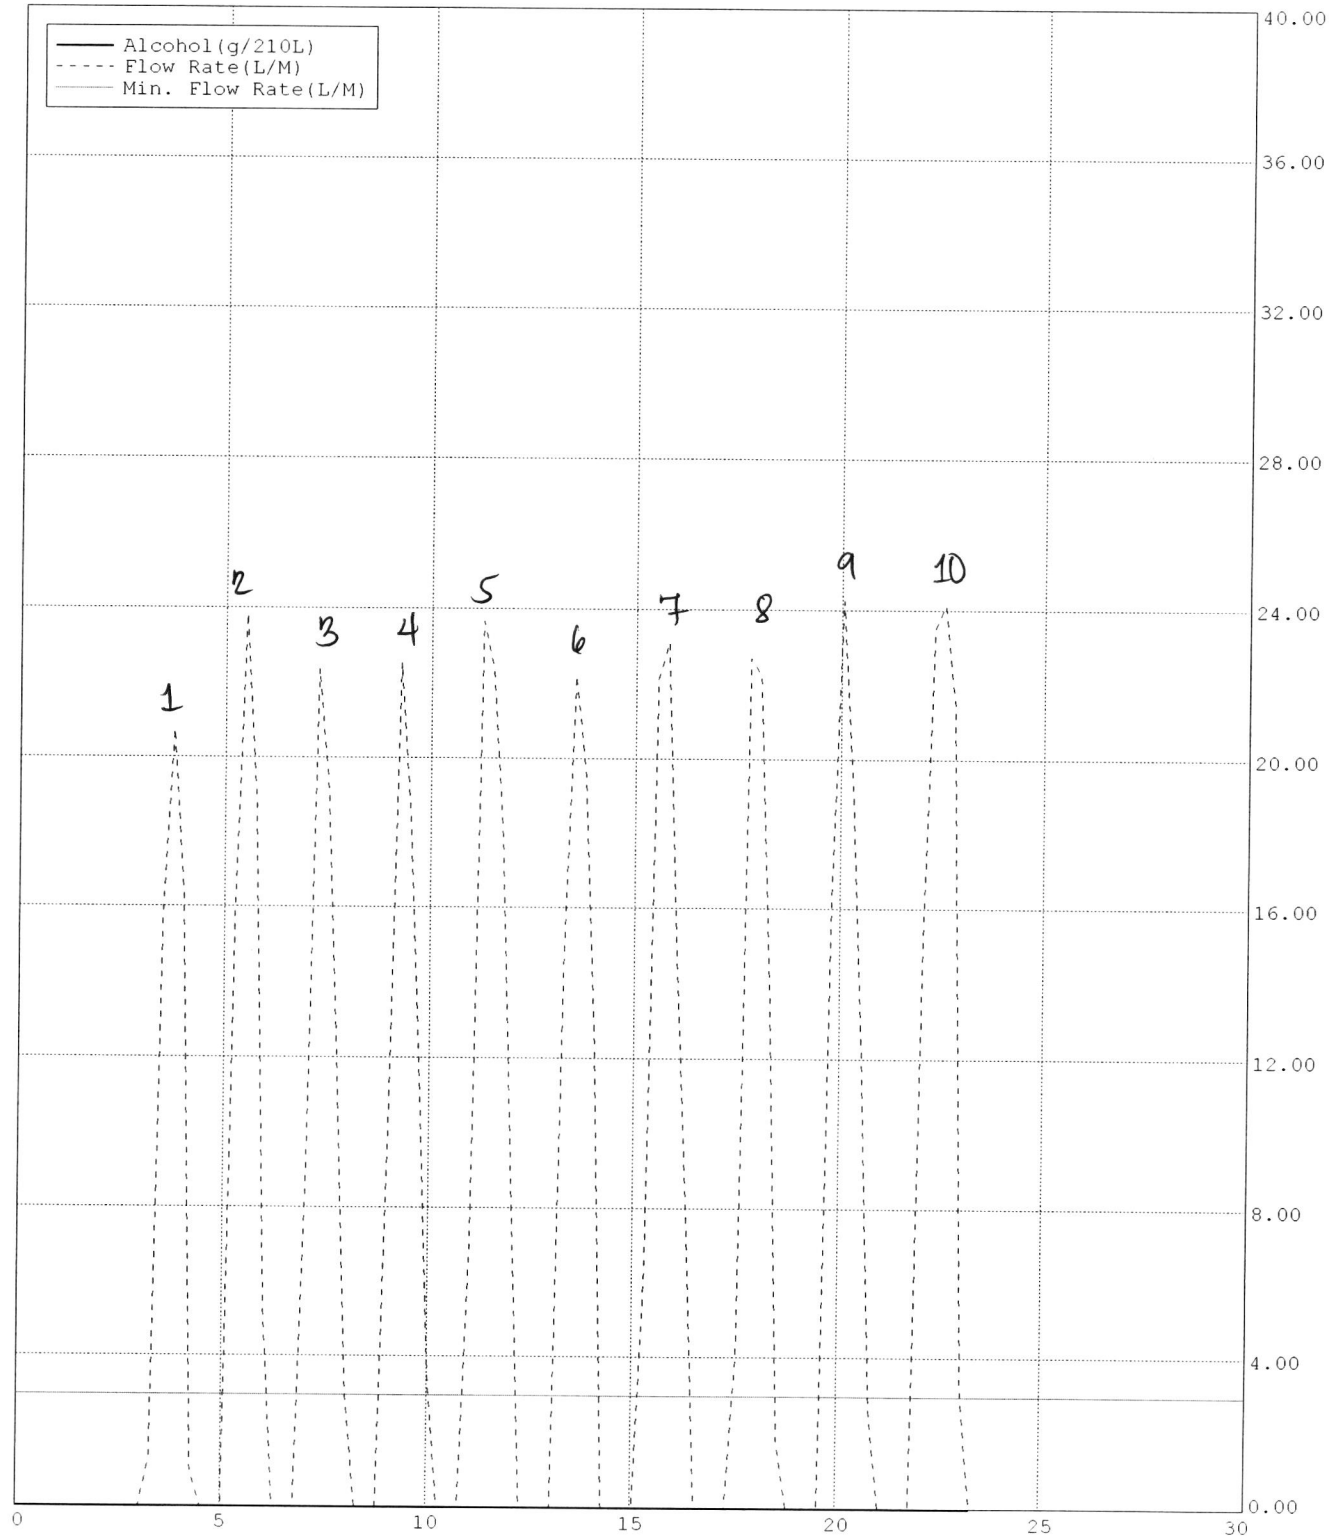

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 10:05:14

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.25: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:06
BLANK TEST	0.000	10:06
INTERNAL STANDARD	VERIFIED	10:06
EXTERNAL STANDARD	0.078	10:06
BLANK TEST	0.000	10:07
SUBJECT SAMPLE	INVALID	10:08

TM

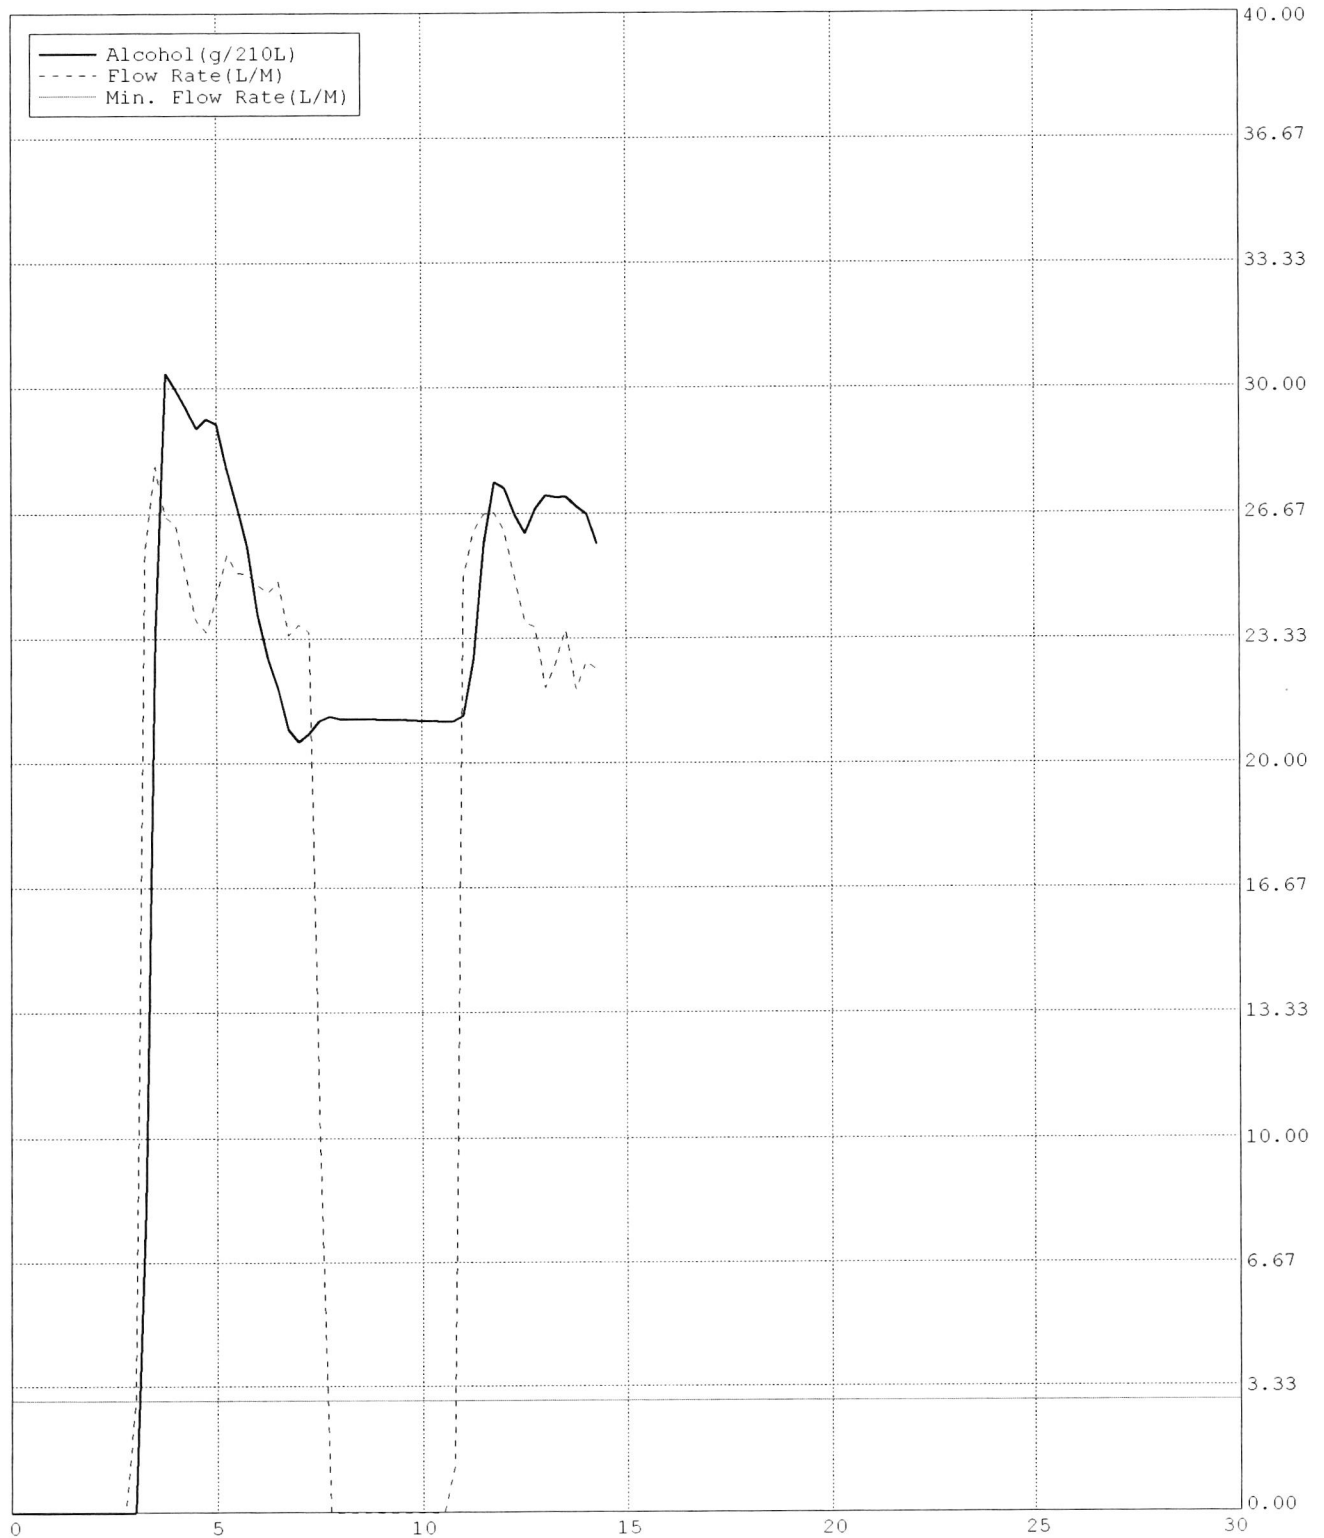

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 10:17:02

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437


DEPT/AGENCY:
RADIO FREQUENCY INTERFERENCE (RFI)
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.25: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:18
BLANK TEST	0.000	10:18
INTERNAL STANDARD	VERIFIED	10:18
EXTERNAL STANDARD	0.077	10:18
BLANK TEST	0.000	10:19

RFI DETECTED

TML

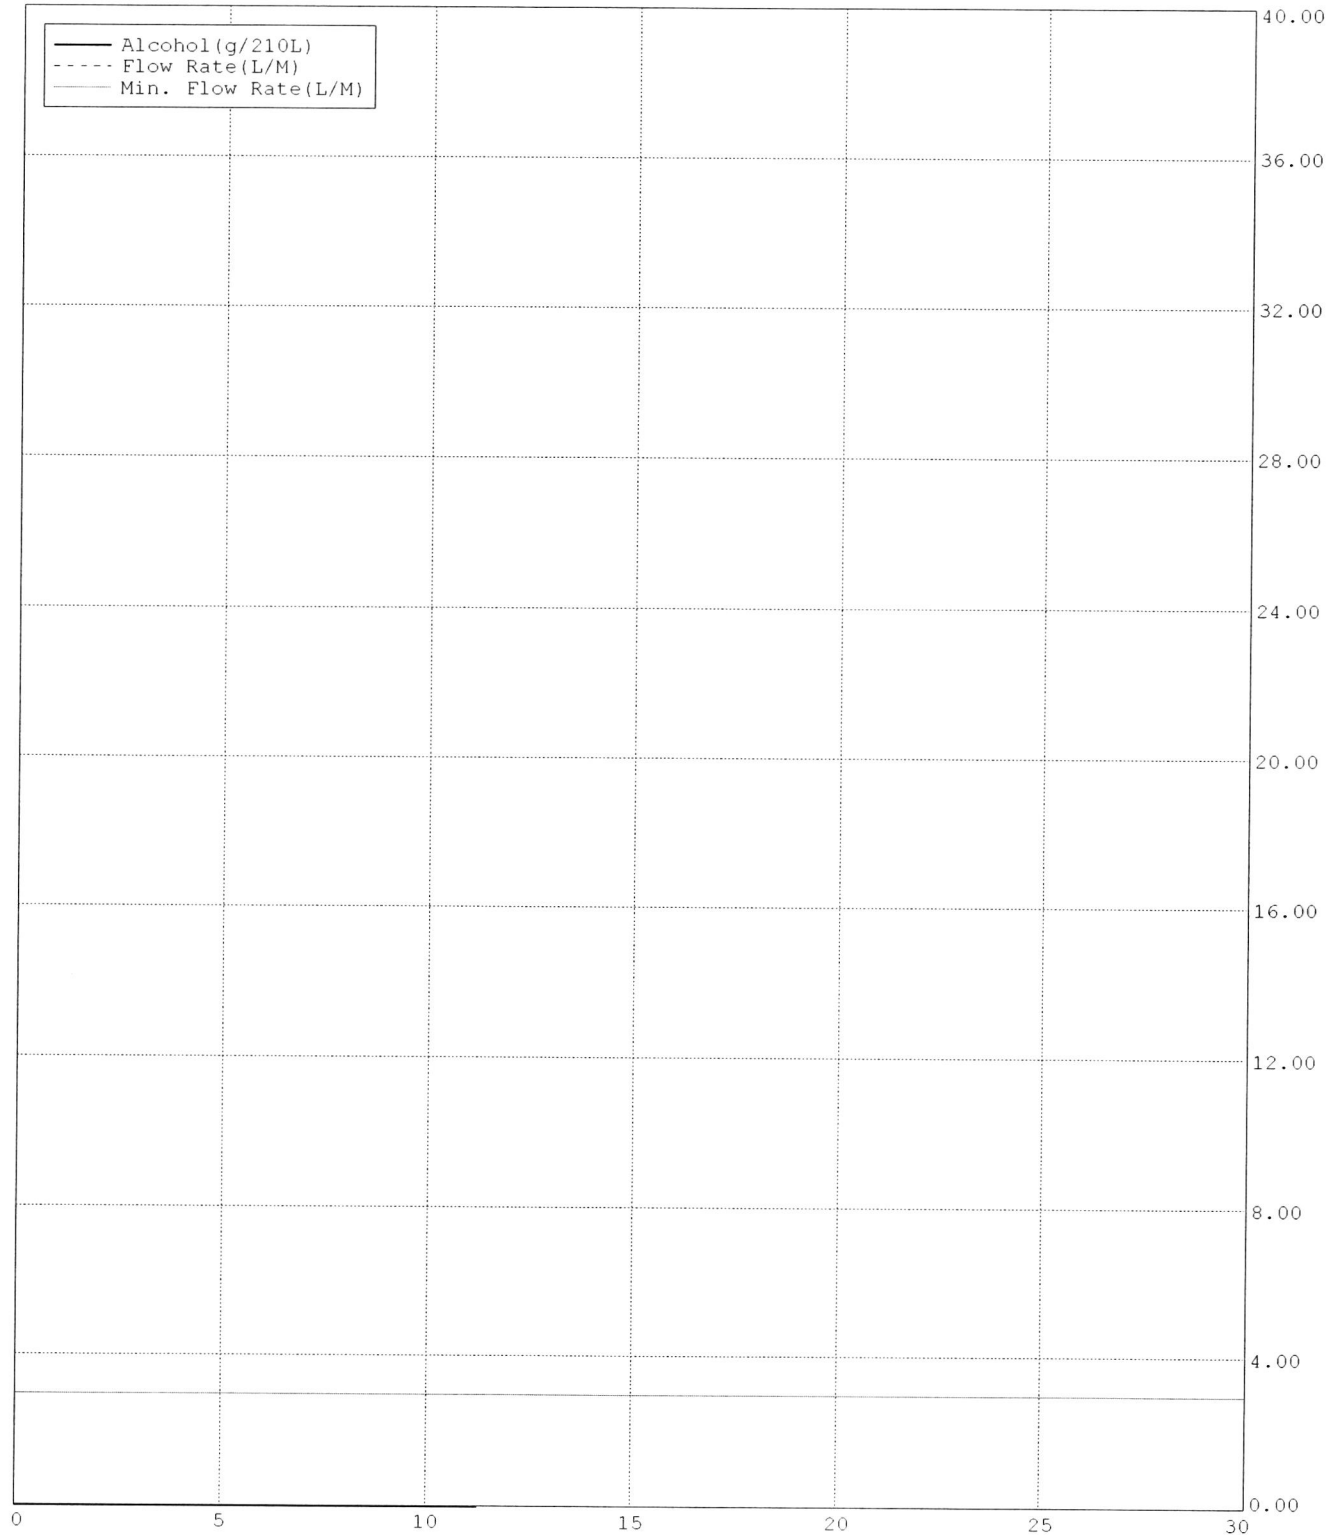

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 10:29:48

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.25: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:31
BLANK TEST	0.000	10:31
INTERNAL STANDARD	VERIFIED	10:31
Xq = 0.090 (0.58%)		
EXTERNAL STANDARD	0.078	10:31
X[1] = 0.0783 (-0.0008) (0.0012)		
BLANK TEST	0.000	10:32
SUBJECT SAMPLE	XXX	10:33
X[1] = 0.1091 (-0.0173) (0.0019)		

Interference Detected

Filter 2 Average: -0.0013
Filter 3 Average: 0.0009

TMM

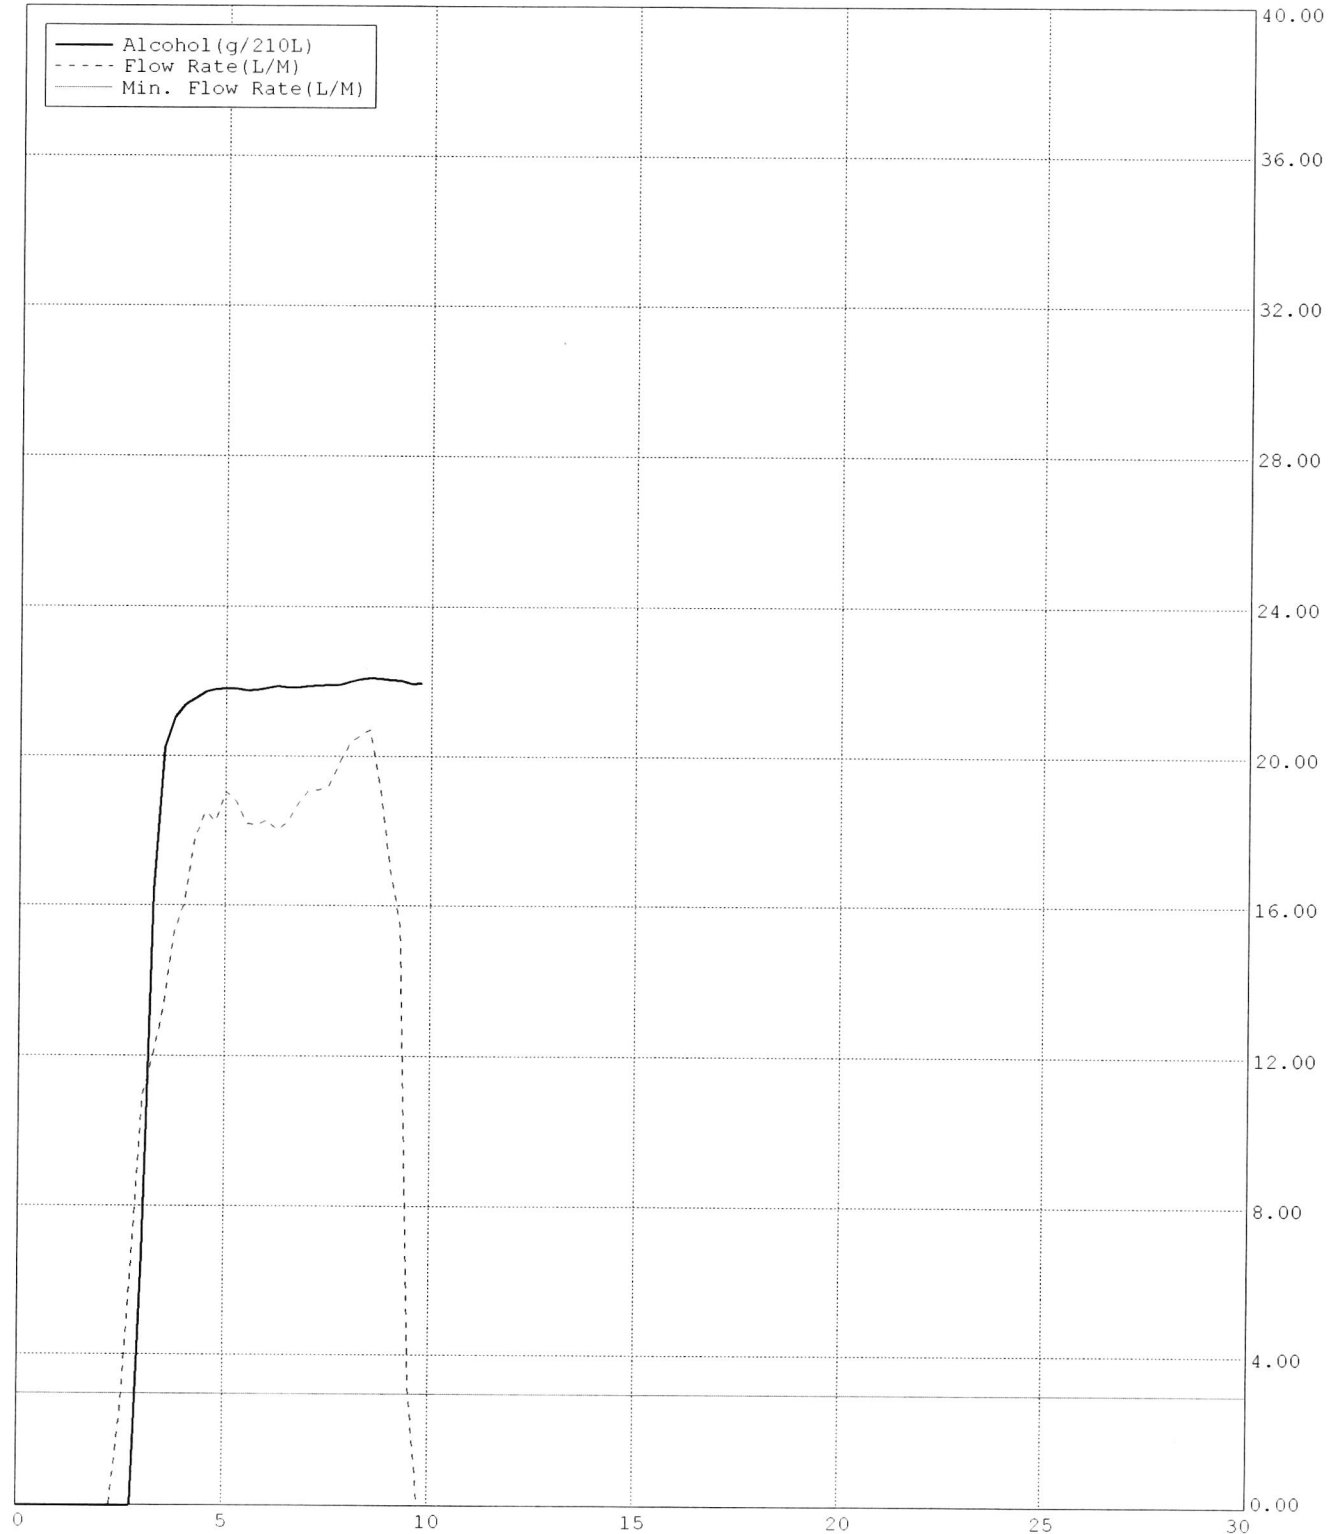

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 10:37:15

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437


DEPT/AGENCY:
INTERFERENCE - ISOPROPANOL
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.25: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:38
BLANK TEST	0.000	10:38
INTERNAL STANDARD	VERIFIED	10:38
Xq = 0.091 (0.87%)		
EXTERNAL STANDARD	0.078	10:38
X[1] = 0.0781 (-0.0007) (0.0012)		
BLANK TEST	0.000	10:39
SUBJECT SAMPLE	XXX	10:40
X[1] = 0.1165 (-0.0287) (0.0007)		

Interference Detected

TAM

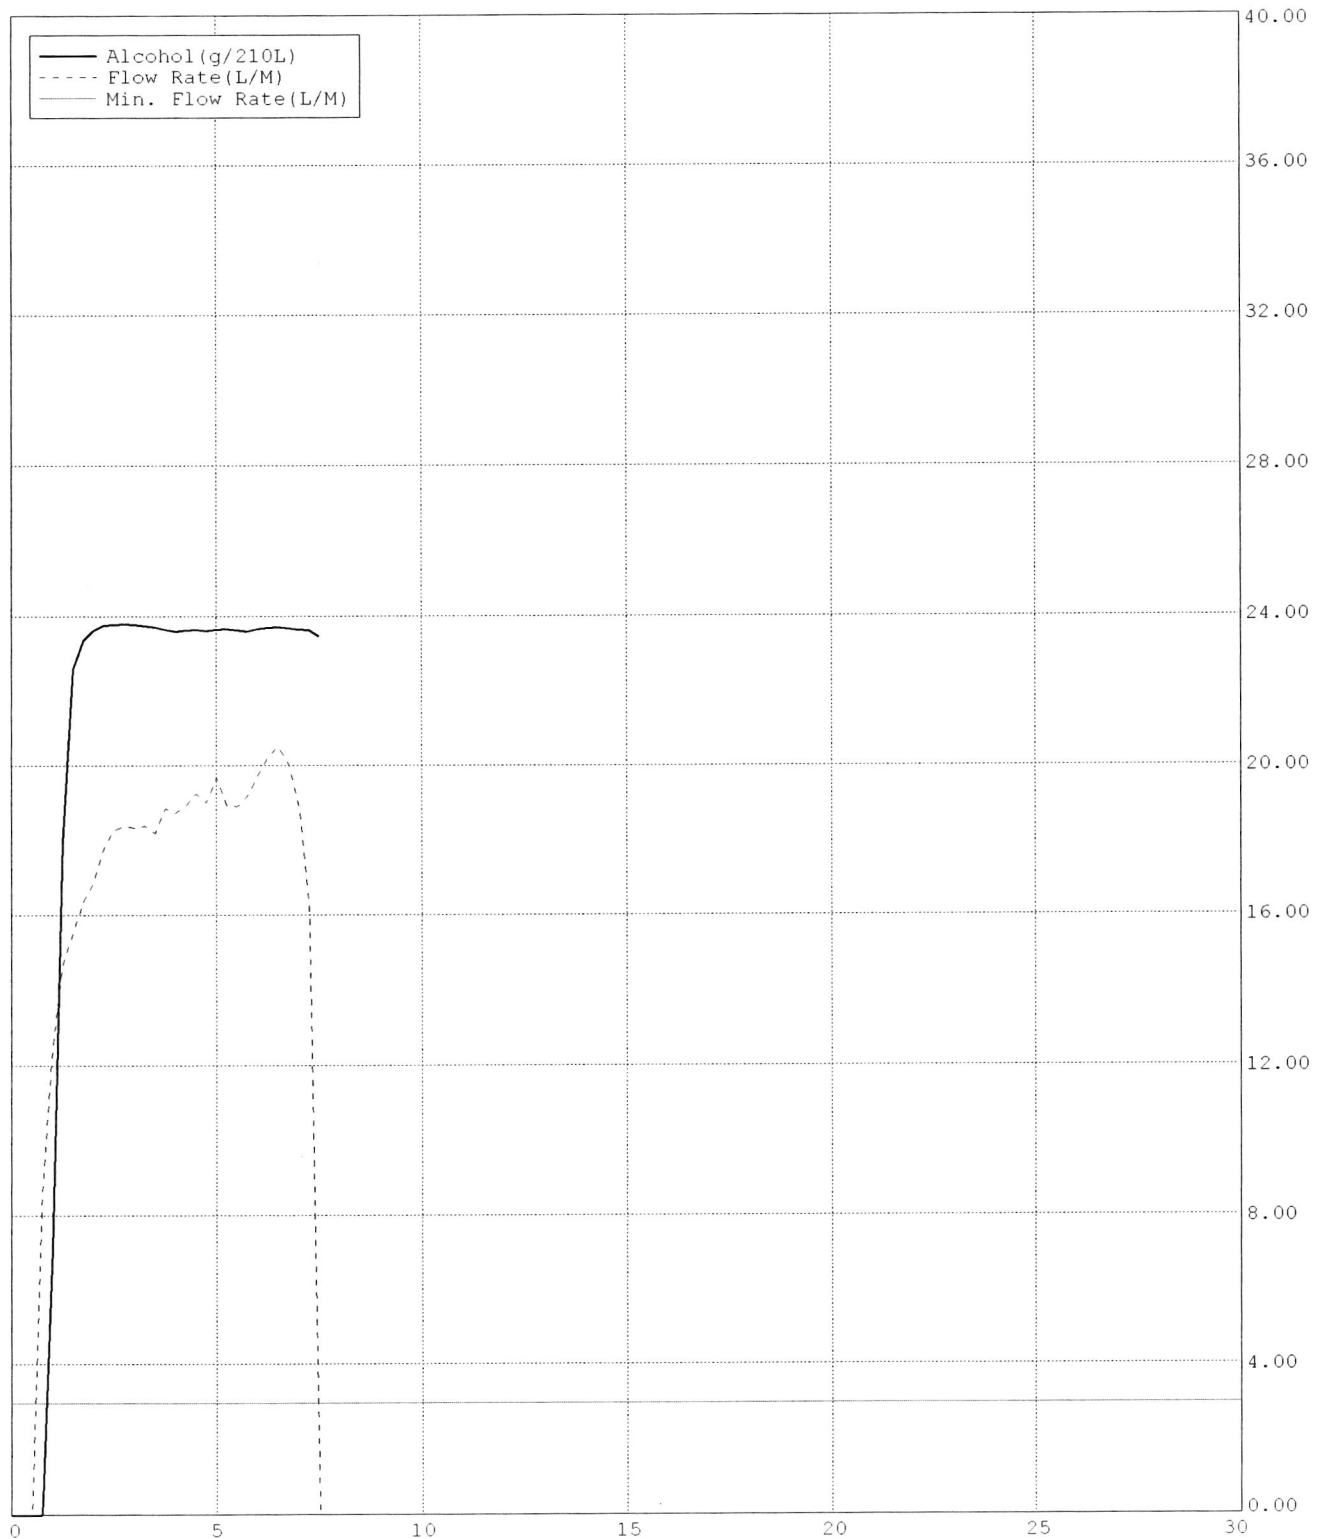

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 10:22:35

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
INTERFERENCE - NEGATIVE CONTROL
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.25: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	10:23
BLANK TEST	0.000	10:23
INTERNAL STANDARD	VERIFIED	10:23
Xq = 0.091 (1.17%)		
EXTERNAL STANDARD	0.078	10:24
X[1] = 0.0779 (-0.0017) (0.0004)		
BLANK TEST	0.000	10:24
SUBJECT SAMPLE (Vol=1.88L)	0.092	10:25
X[1] = 0.0922 (-0.0028) (-0.0010)		
BLANK TEST	0.000	10:26
EXTERNAL STANDARD	0.077	10:26
X[1] = 0.0767 (-0.0018) (0.0009)		
BLANK TEST	0.000	10:27

TJM

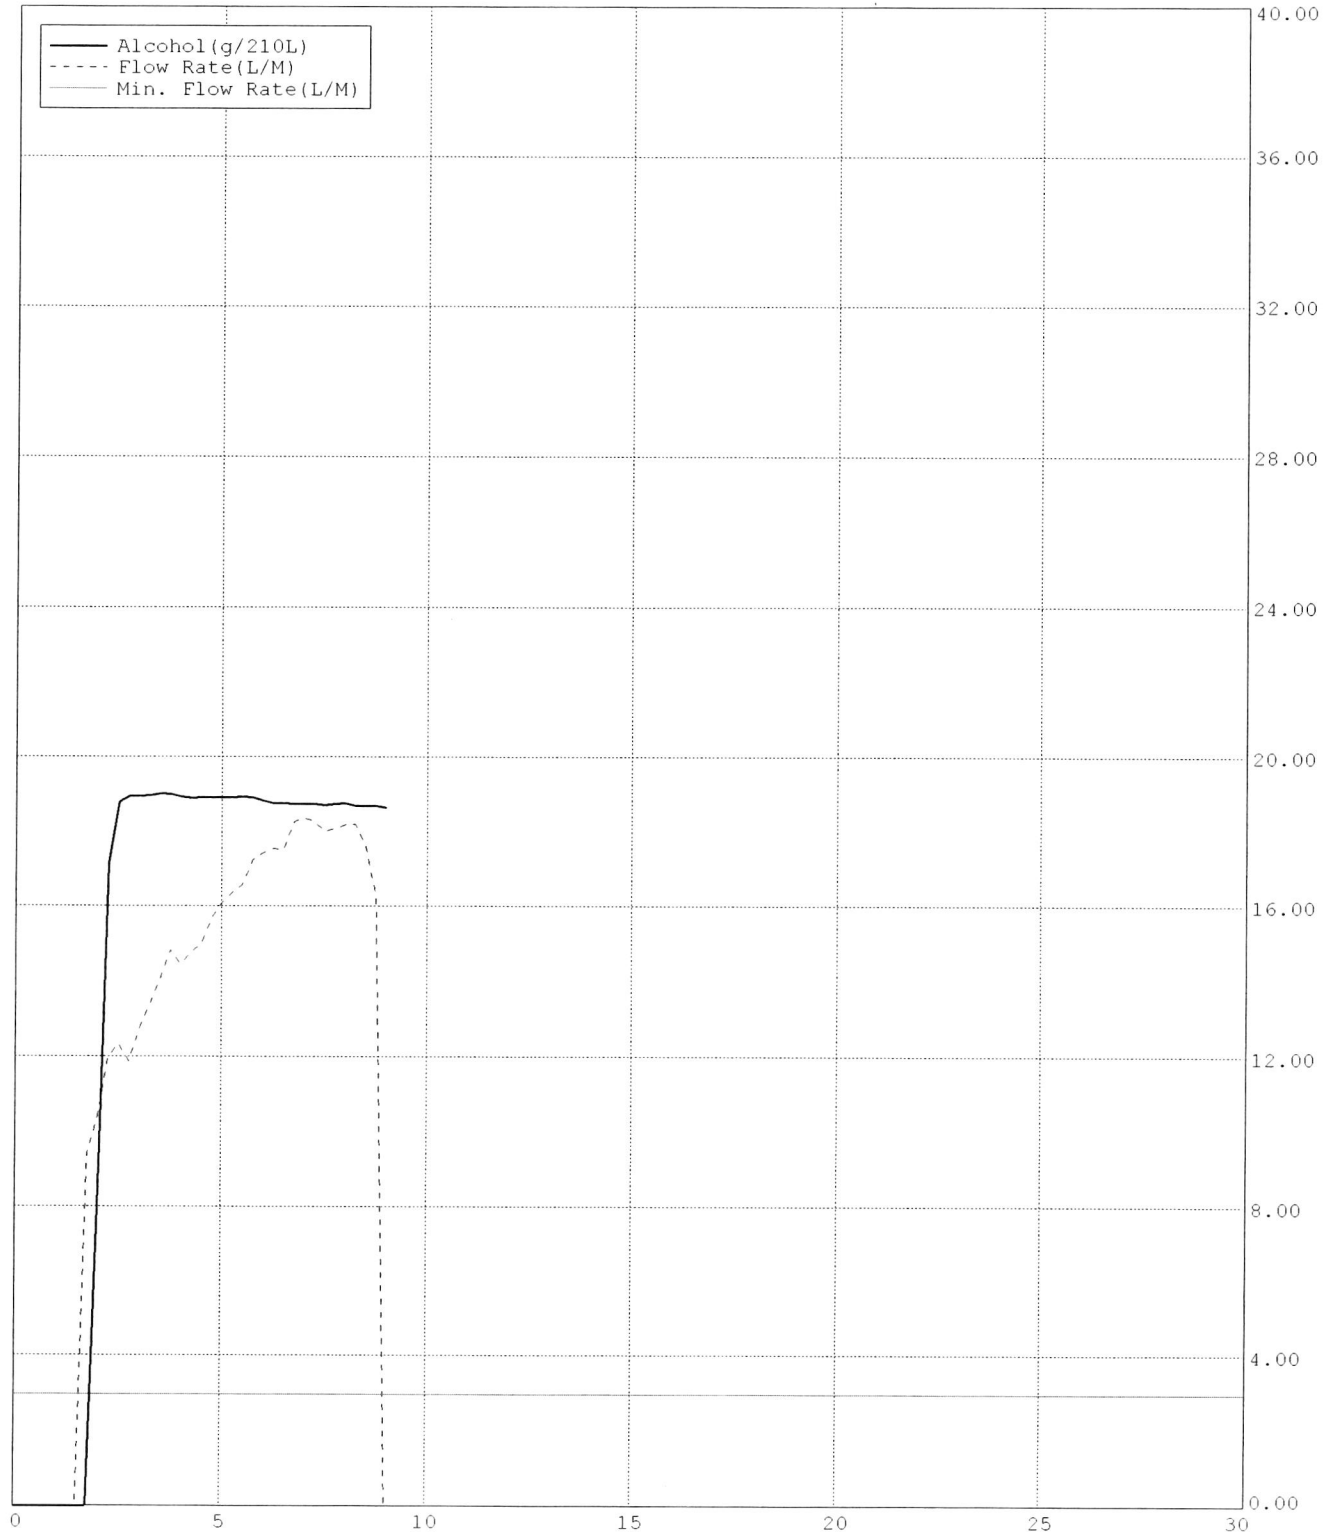

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100668

Date: 03/14/2023
Time: 11:05:17

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
TATIANA MALNOSKE
OPERATOR'S #: 10437

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.25: 0.078
LOT #: AG113402
EXPIRATION: 05/14/2023

DIAGNOSTIC CHECK	PASSED	11:06
BLANK TEST	0.000	11:06
INTERNAL STANDARD	VERIFIED	11:06
EXTERNAL STANDARD	0.079	11:07
BLANK TEST	0.000	11:08
SUBJECT SAMPLE (Vol=1.67L)	0.000	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.078	11:09
BLANK TEST	0.000	11:10

TUM

