

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100404

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 10/17/2017

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG634001
EXPIRATION: 12/05/2018
TANK PRESSURE: 552 psi

BLANK TEST	0.000	10:42
INTERNAL STANDARD	VERIFIED	10:42
EXTERNAL STANDARD	0.077	10:42
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.077	10:44
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.077	10:45
BLANK TEST	0.000	10:46
EXTERNAL STANDARD	0.077	10:46
BLANK TEST	0.000	10:47
EXTERNAL STANDARD	0.077	10:47
BLANK TEST	0.000	10:48

Average = 0.0770
Std Dev = 0.0000

Diagnostic Check

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
Breath Tube = 45.9°C PASSED

PUMP INFO

Flow Rate = 4.284 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED

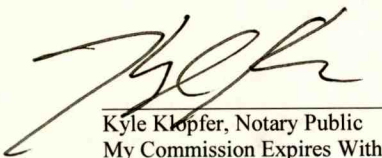
I, Charles R. Foster, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 11/9/17

Charles R. Foster
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 9 day of Nov, 20 17


Kyle Klopfer, Notary Public
My Commission Expires With Office




OMB
10/19/17