	State of Alaska Scientific Crime Detection Laboratory		
	DataMaster Acceptance Form - DMAF2011R0		
	Issuing Authority - Nita Bolz, Scientific Director		
	Approval date: 03/01/11	Effective date: 03/01/11	Archive date: Active


DataMaster DMT Acceptance Form

Instrument # 100421

Date: 7/20/11

Analyst: CRF / COB

1. Check in instrument in to JusticeTrax Breath Alcohol Database.
2. Visual Inspection
3. Update software
4. Print calibration factors (attached) ✓
5. NPAS calibration paperwork (attached) *Not submitted with instrument. Serial #*
6. Barcode Instrument
7. State of Alaska Property ID# JBER *changed. Will need to be recalibrated - CRF*

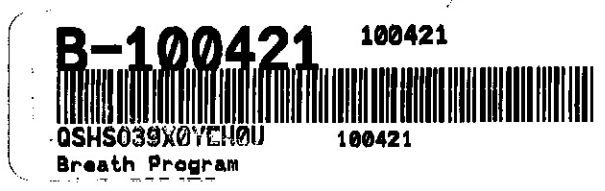

Replaced old sticker + updated SN COB 7/20/11



CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 300100

Date: 06/16/2011
Time: 07:16:56

Ca = 0.1000
CAL = 0.982489 0.800 <= CAL < 1.200
b1 = 0.0002 0.0000 <= b1 < 0.0040
b2 = 0.0029 0.0010 <= b2 < 0.0100
b3 = 0.0000 0.0000 <= b3 < 0.0040
Xq = 0.1012 0.0500 <= Xq < 0.2000
a21 = 1.126593 1.050 <= a21 < 1.300
a31 = 0.461525 0.300 <= a31 < 0.800

Final page for report

\

\\ANCSCLSAN01\JTRAX\CASEDOCS\B-100421\B-100421 ECF-20140

7/9/2014